



US00D820699S

(12) **United States Design Patent**  
**Bacon**

(10) **Patent No.:** **US D820,699 S**  
(45) **Date of Patent:** **\*\* Jun. 19, 2018**

(54) **HANDHELD ANALYZER**

- (71) Applicant: **Thermo Scientific Portable Analytical Instruments Inc.**, Tewksbury, MA (US)
- (72) Inventor: **Neil Bacon**, Milton, MA (US)
- (73) Assignee: **Thermo Scientific Portable Analytical Instruments Inc.**, Tewksbury, MA (US)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/564,400**
- (22) Filed: **May 12, 2016**

**Related U.S. Application Data**

- (63) Continuation of application No. 29/509,001, filed on Nov. 13, 2014, now Pat. No. Des. 760,101.
  - (51) **LOC (11) Cl.** ..... **10-04**
  - (52) **U.S. Cl.**  
USPC ..... **D10/78; D10/47**
  - (58) **Field of Classification Search**  
USPC ..... D10/47, 70, 78  
CPC ..... G01N 23/223; G01N 29/226; G01N 2223/0763; G01N 2223/076; G01N 2223/0766
- See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D264,191 S	5/1982	Jondrow	
D496,292 S	9/2004	Sowers	
6,909,770 B2	6/2005	Schramm et al.	
7,375,359 B1	5/2008	Grodzins	
8,759,791 B1	6/2014	Hug et al.	
8,909,770 B2 *	12/2014	Kulkarni	H04L 29/0899 709/224
D763,108 S *	8/2016	Hagerty	D10/78

(Continued)

**OTHER PUBLICATIONS**

Thermo Scientific Niton XRF Analyzers Datasheet, Jul. 2010, 12 pages.

*Primary Examiner* — Antoine Duval Davis

(74) *Attorney, Agent, or Firm* — William R. McCarthy, III

(57) **CLAIM**


The ornamental design for a handheld analyzer, substantially as shown and described.

**DESCRIPTION**

FIG. 1 is a left elevation view of an embodiment of the handheld analyzer;  
 FIG. 2 is a left elevation view of the embodiment of the handheld analyzer, wherein the screen is in the tilted position;  
 FIG. 3 is a front, left perspective view of the embodiment of the handheld analyzer;  
 FIG. 4 is a right elevation view of the embodiment of the handheld analyzer;  
 FIG. 5 is a front elevation view of the embodiment of the handheld analyzer, wherein the screen is in the tilted position;  
 FIG. 6 is a back elevation view of the embodiment of the handheld analyzer;  
 FIG. 7 is a back, left perspective view of the embodiment of the handheld analyzer;  
 FIG. 8 is a back, left perspective view of the embodiment of the handheld analyzer, wherein the screen is in the tilted position;  
 FIG. 9 is a top plan view of the embodiment of the handheld analyzer, wherein the screen is in the tilted position; and,  
 FIG. 10 is a bottom plan view of the embodiment of the handheld analyzer.

The broken lines in the figures form no part of the claimed design.

**1 Claim, 10 Drawing Sheets**

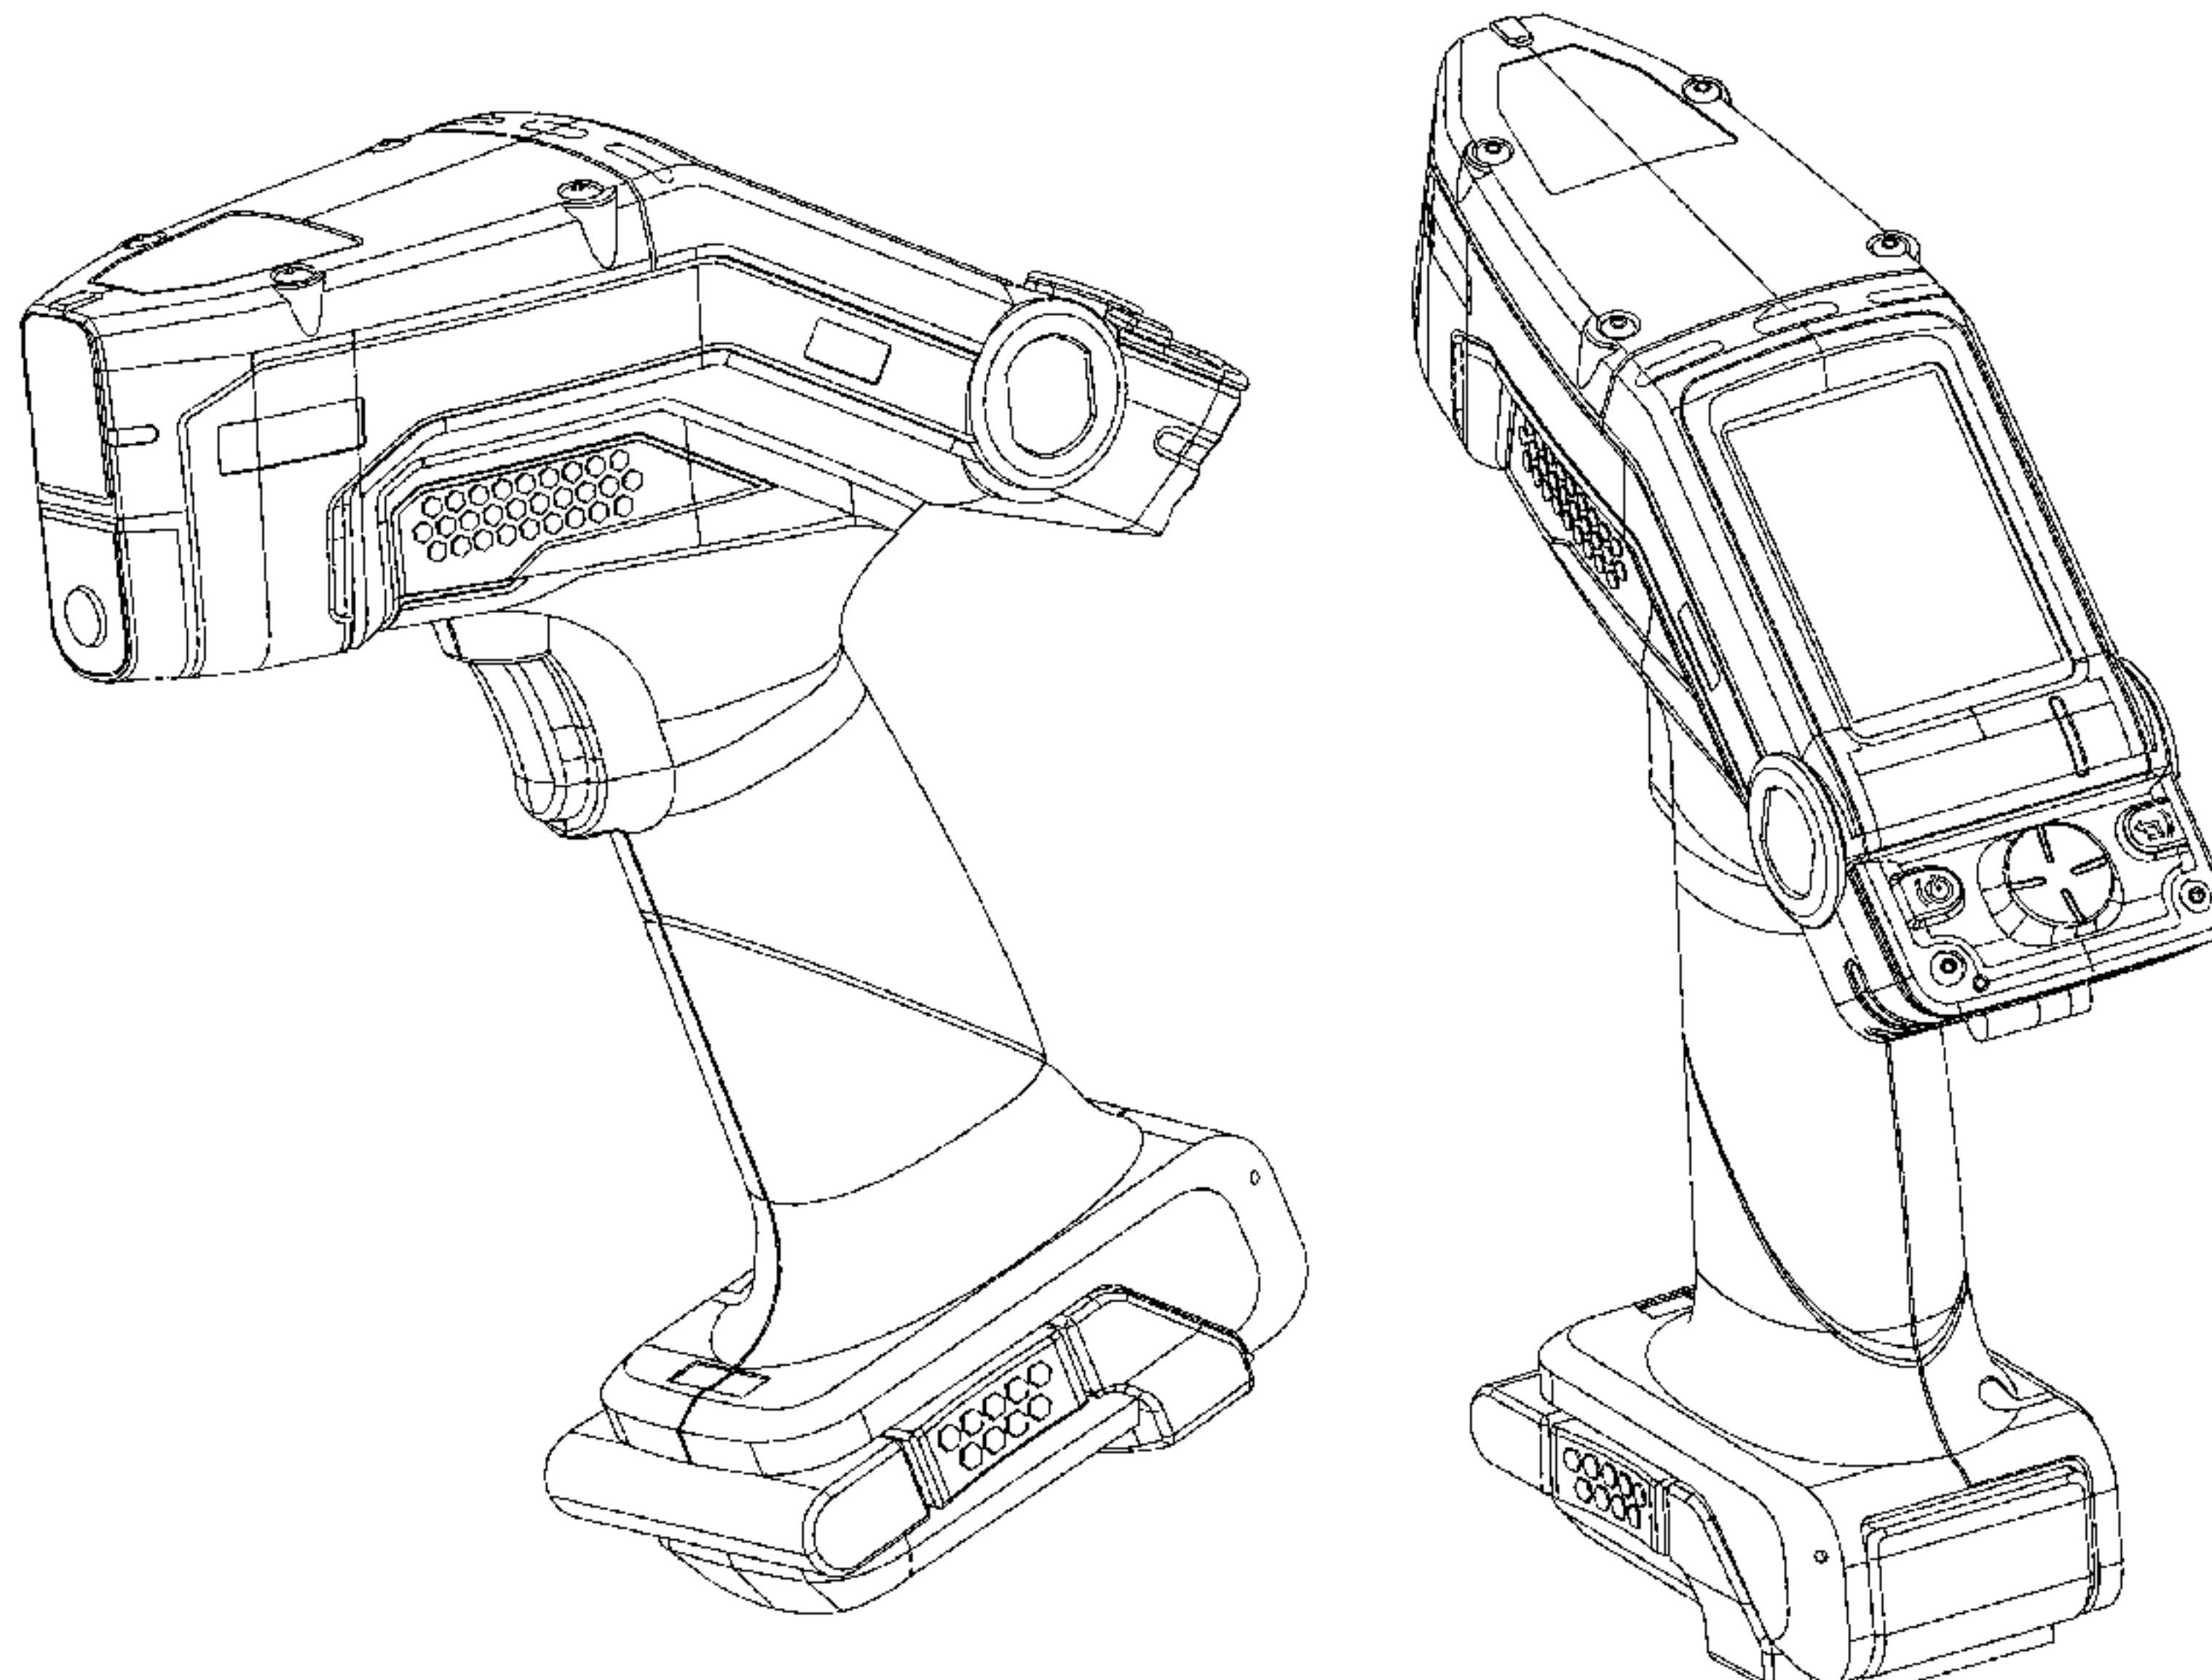

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2008/0205592	A1	8/2008	Connors et al.
2011/0079734	A1	4/2011	Grodzins et al.
2013/0022166	A1	1/2013	Drummy
2013/0136238	A1	5/2013	Laws et al.
2014/0301530	A1	10/2014	Faila, Jr. et al.
2014/0307849	A1	10/2014	Cancre et al.
2014/0328468	A1	11/2014	Pomerantz et al.
2015/0036804	A1	2/2015	Dunham et al.
2015/0212018	A1	7/2015	Shields et al.

\* cited by examiner

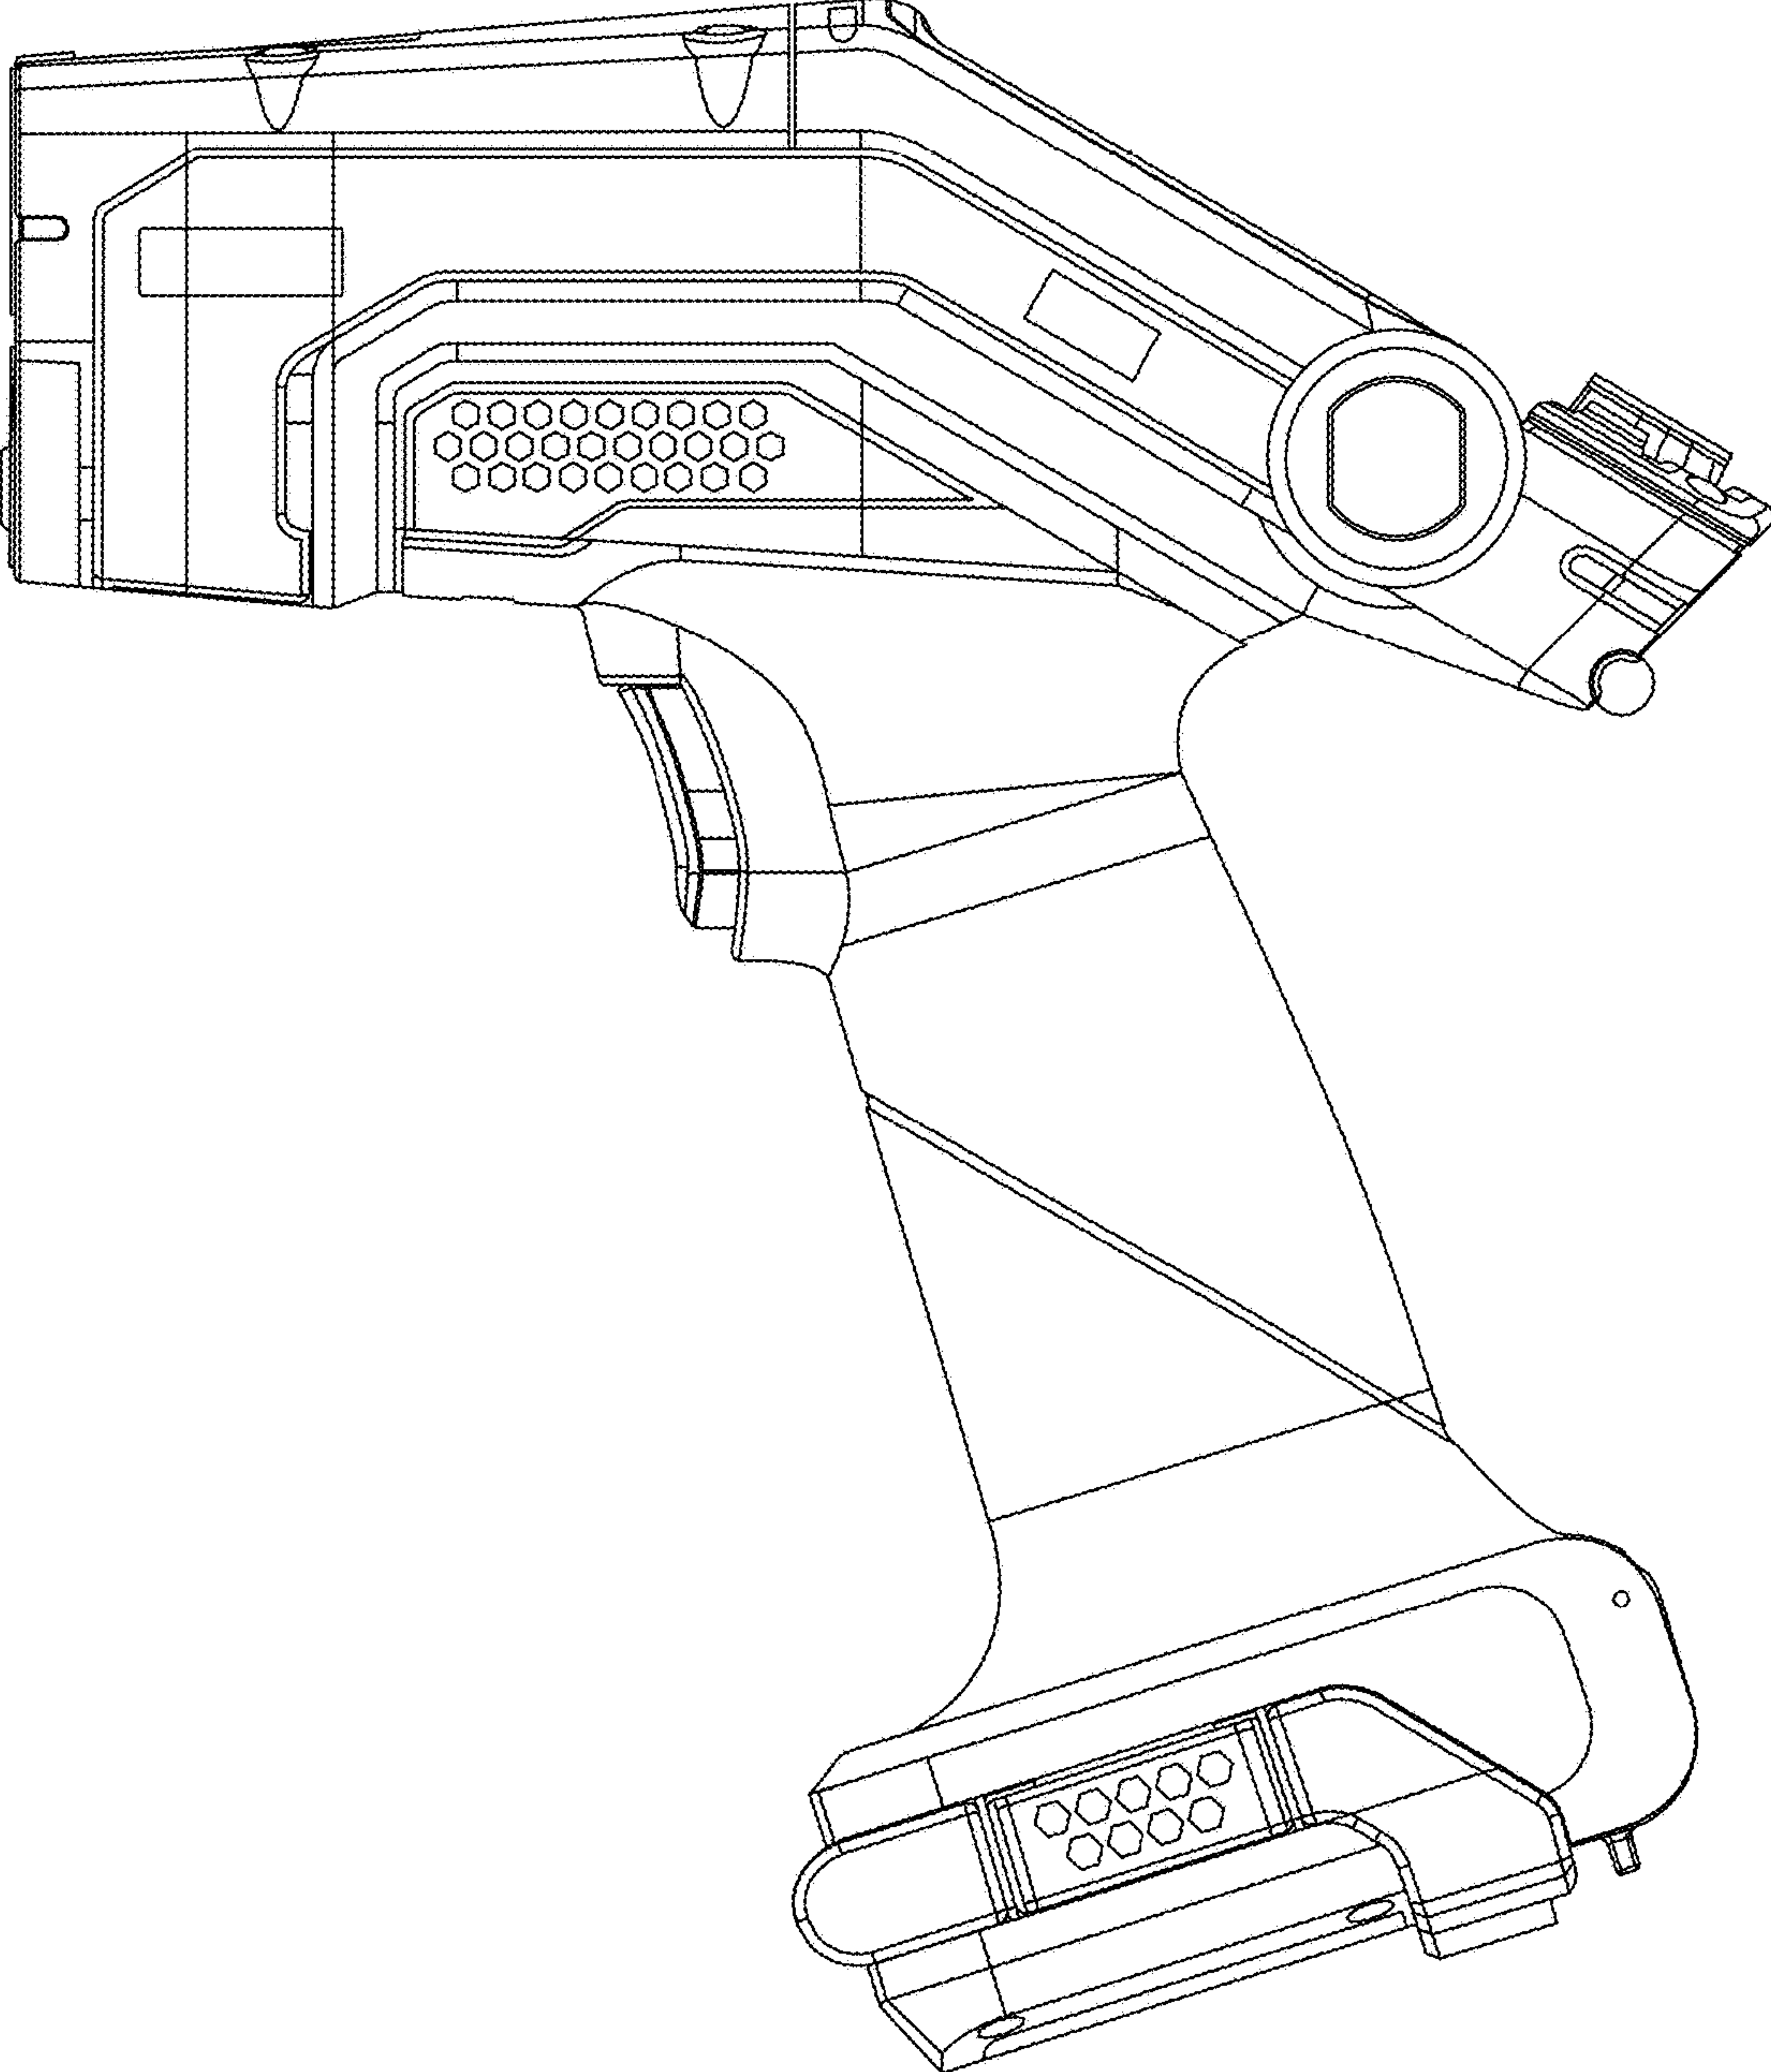


FIG. 1



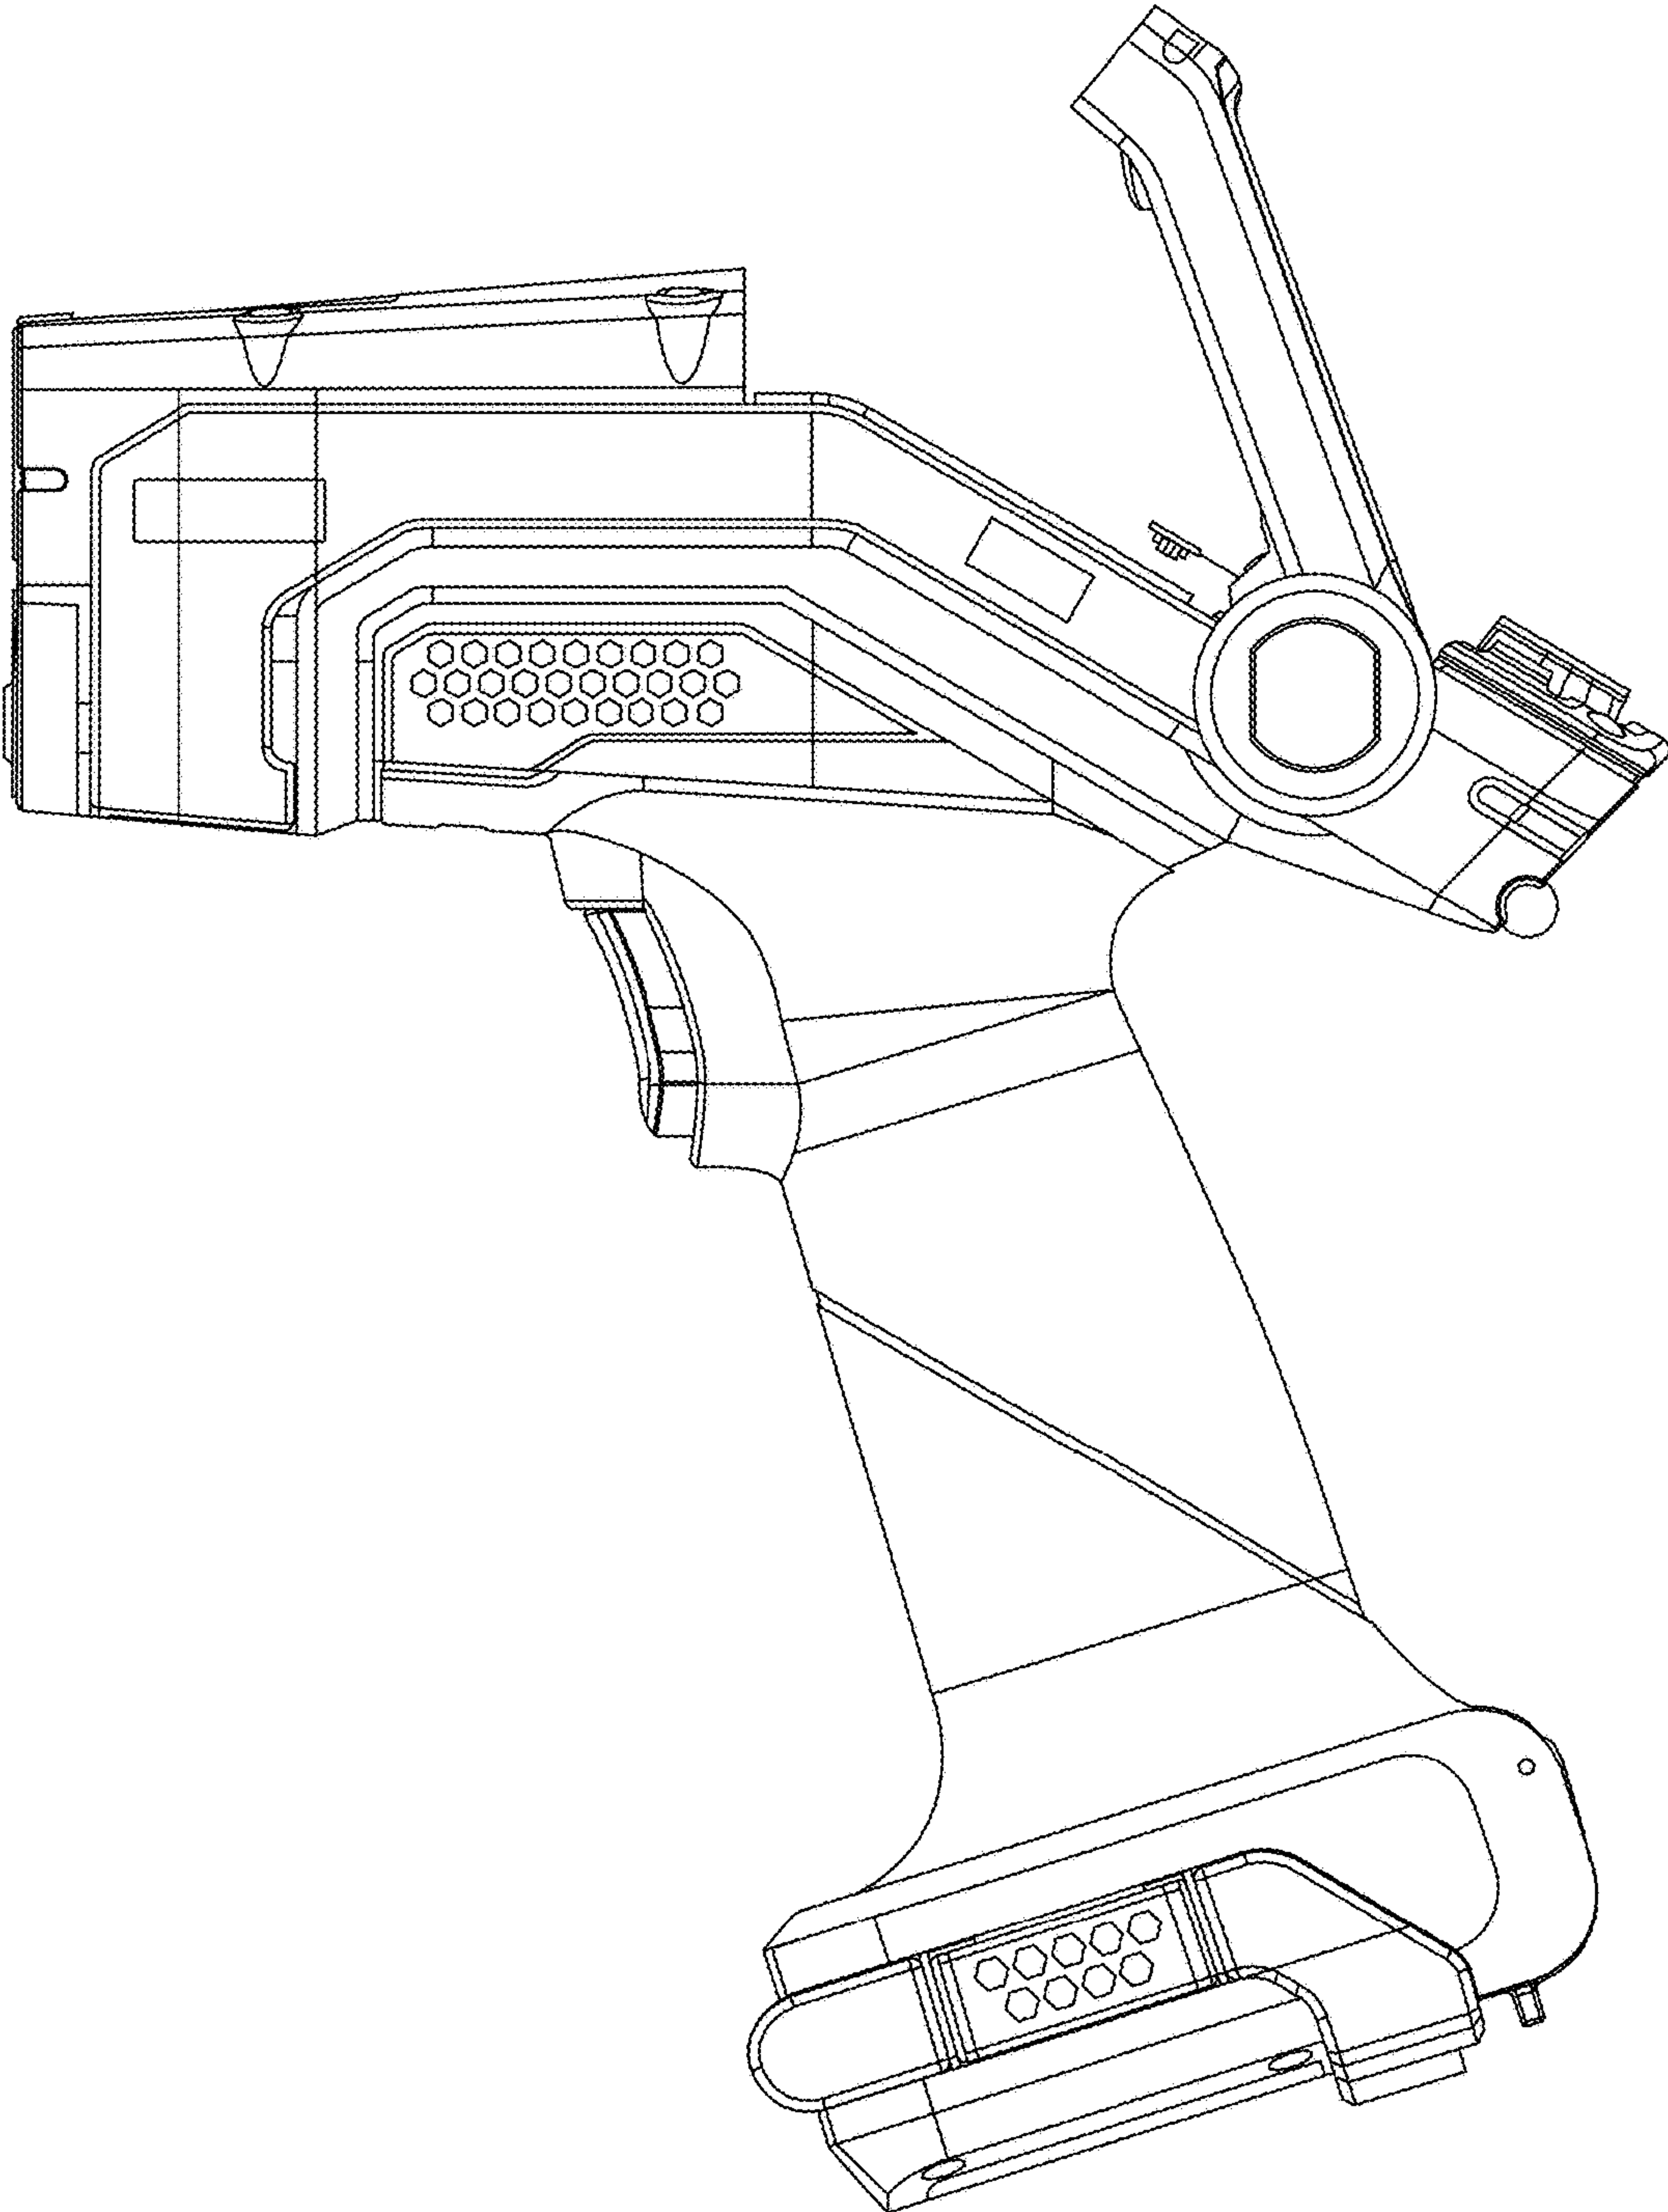


FIG. 2

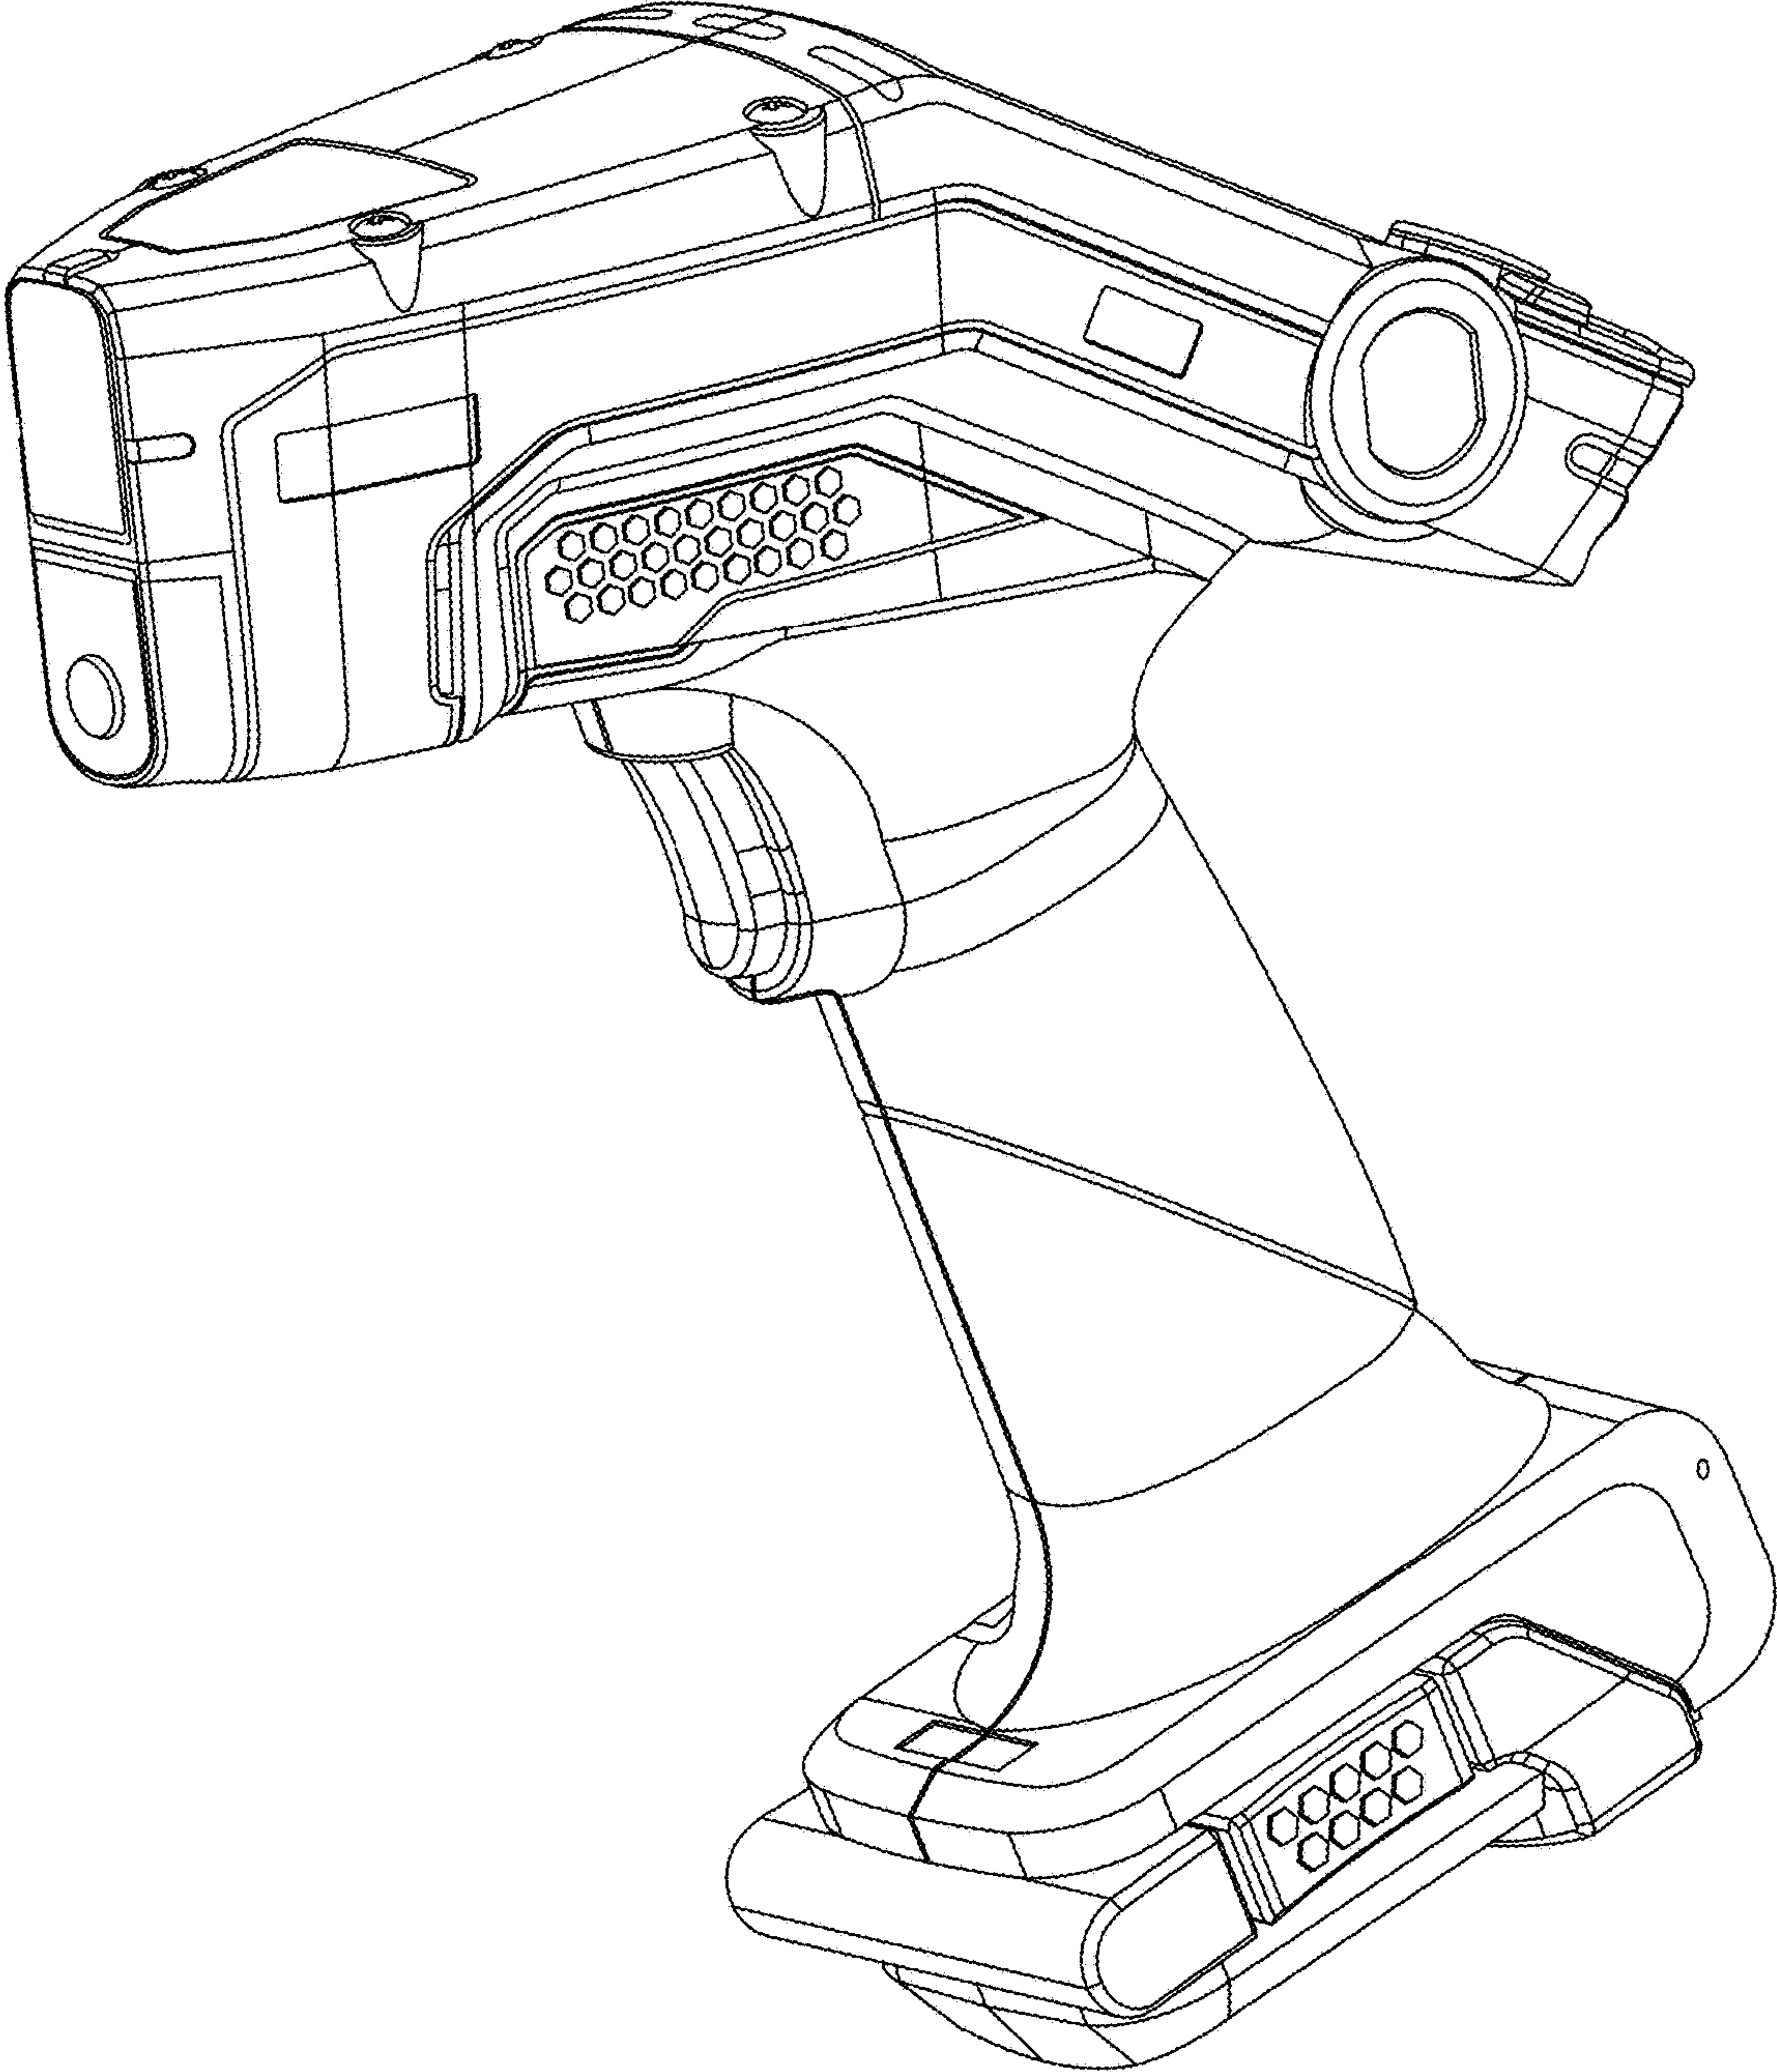


FIG. 3

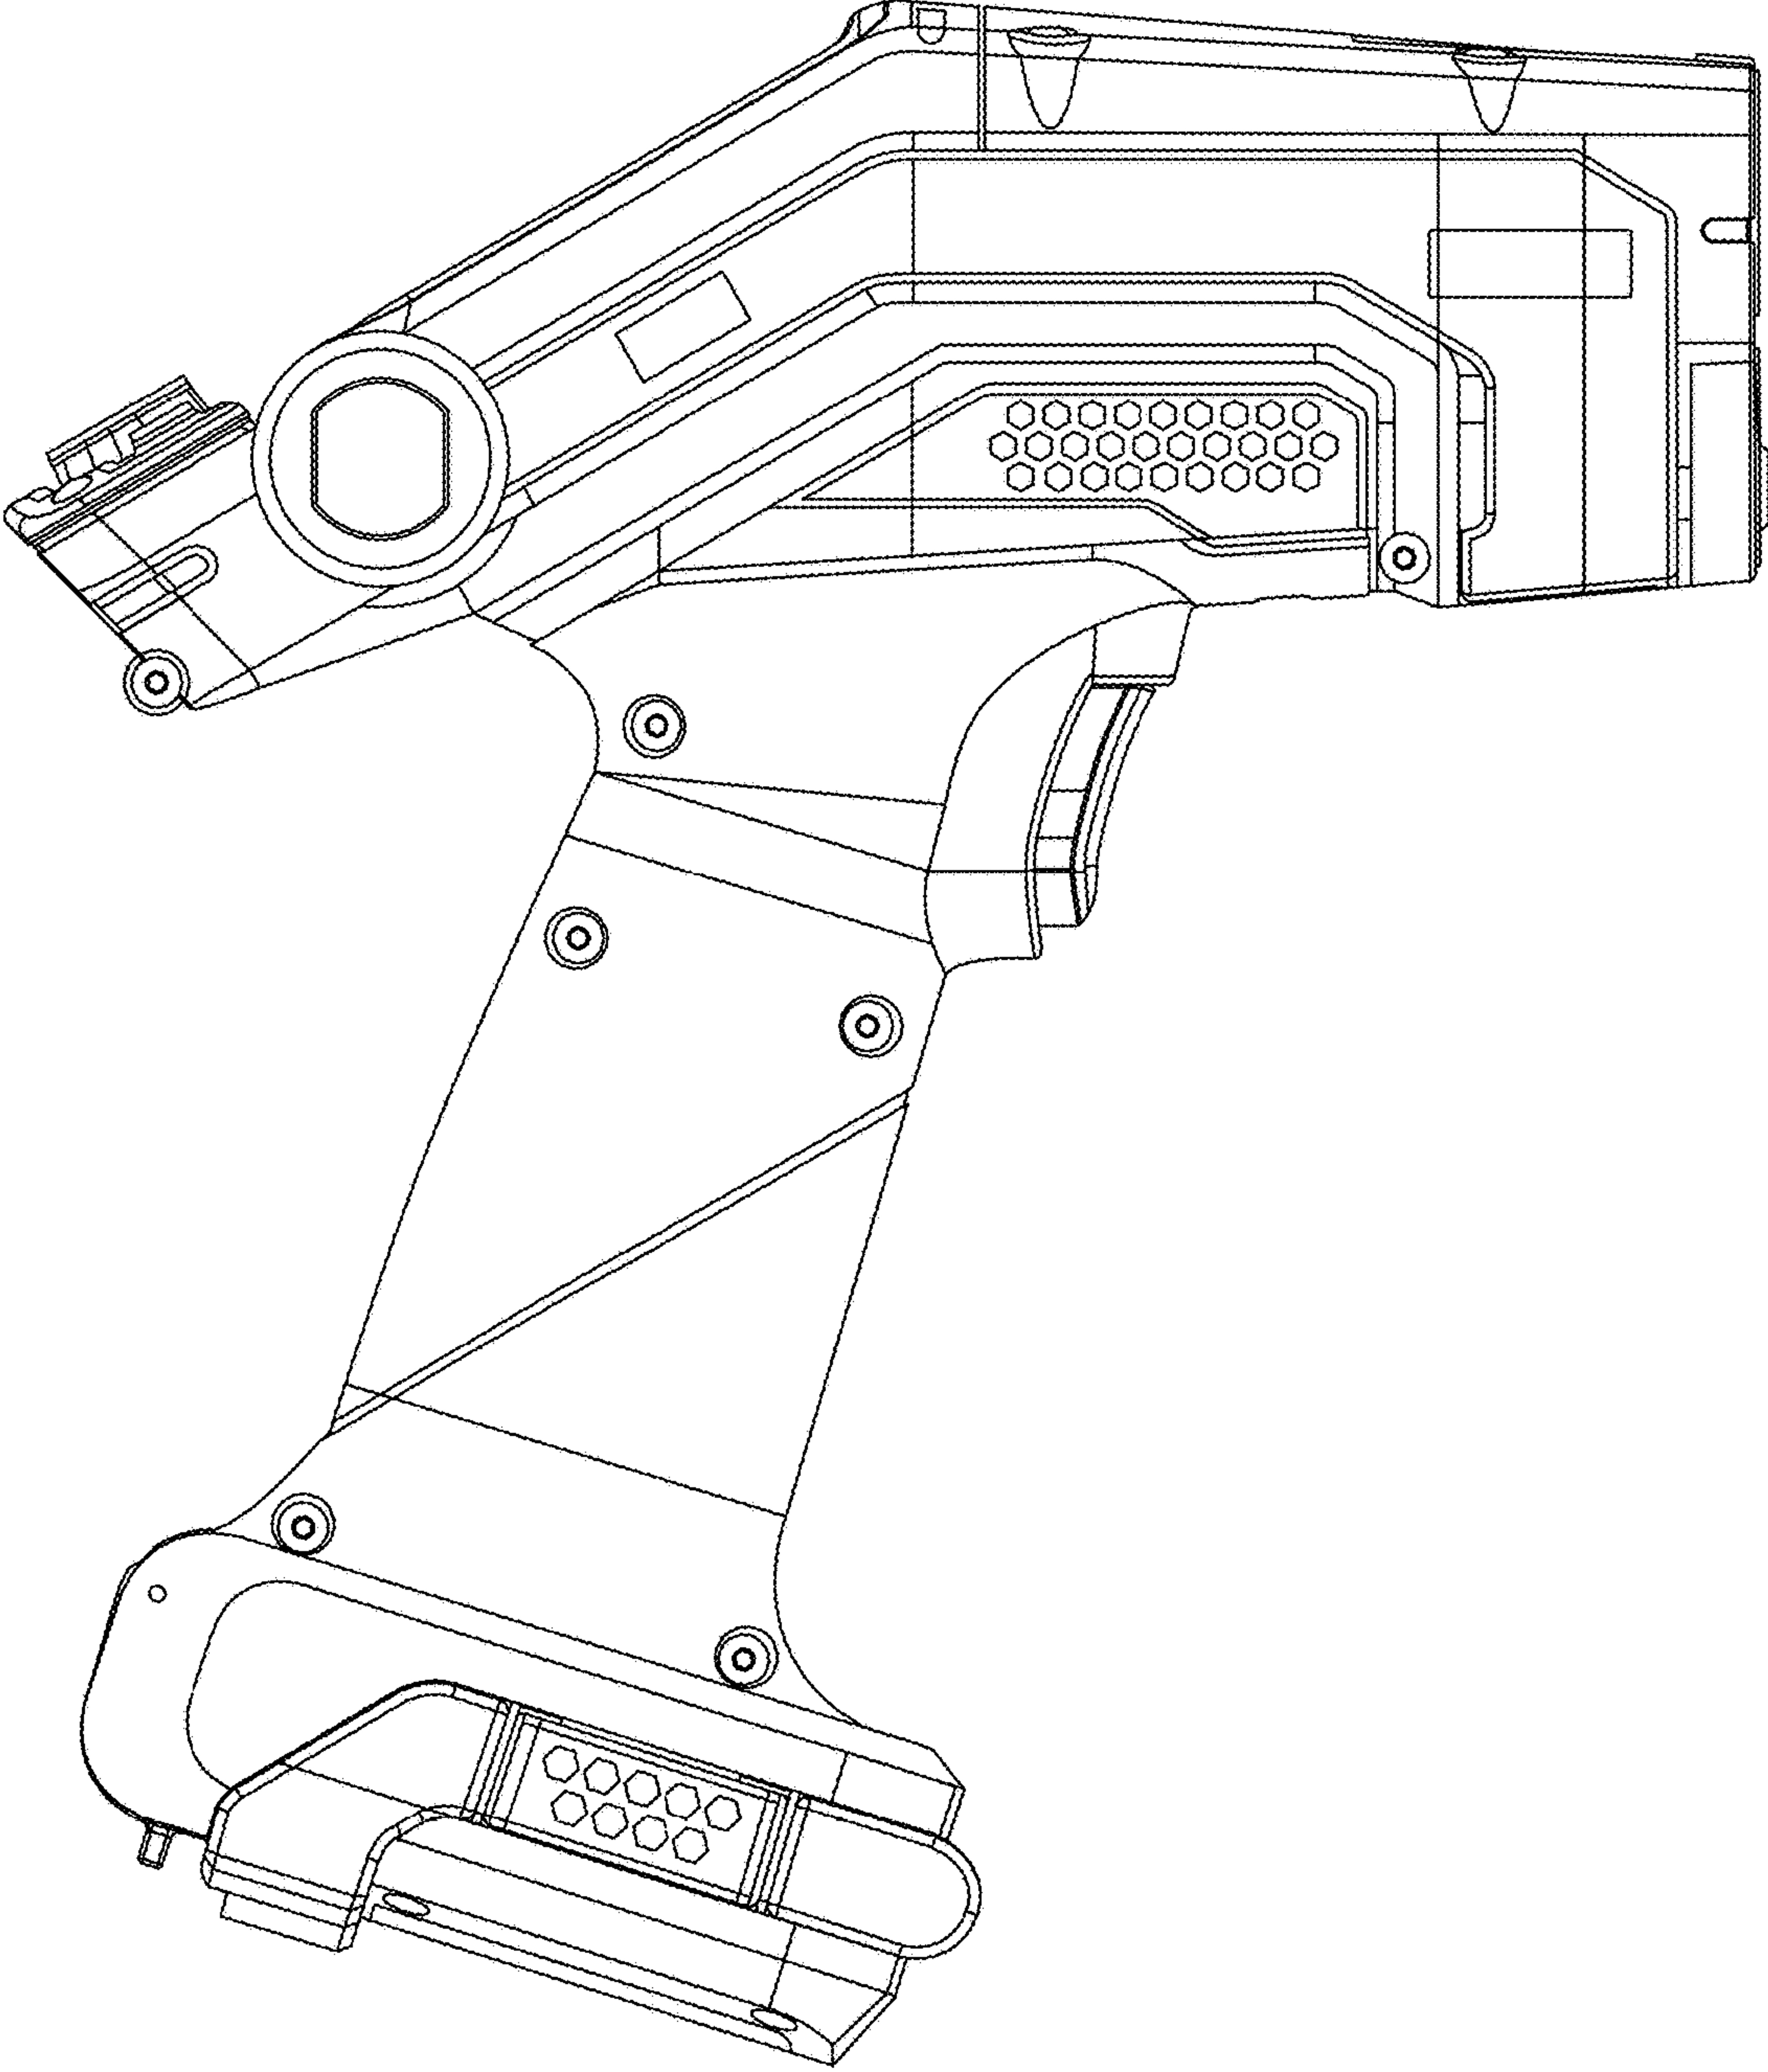


FIG. 4



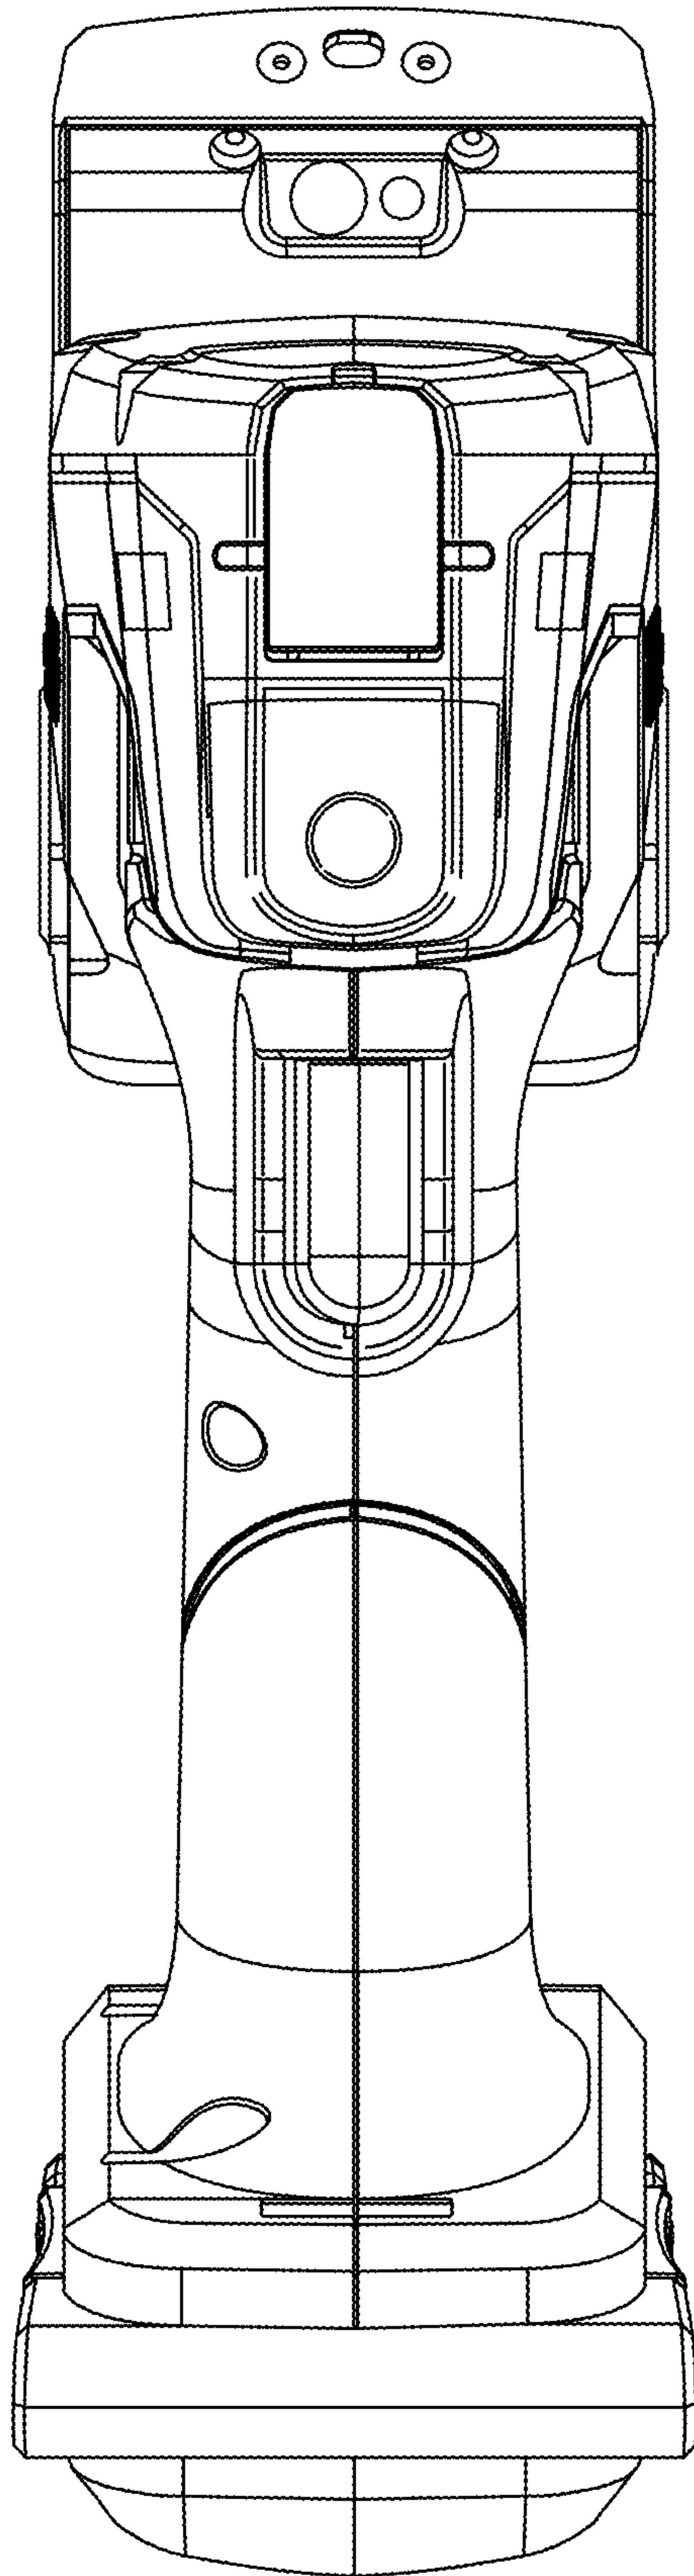


FIG. 5

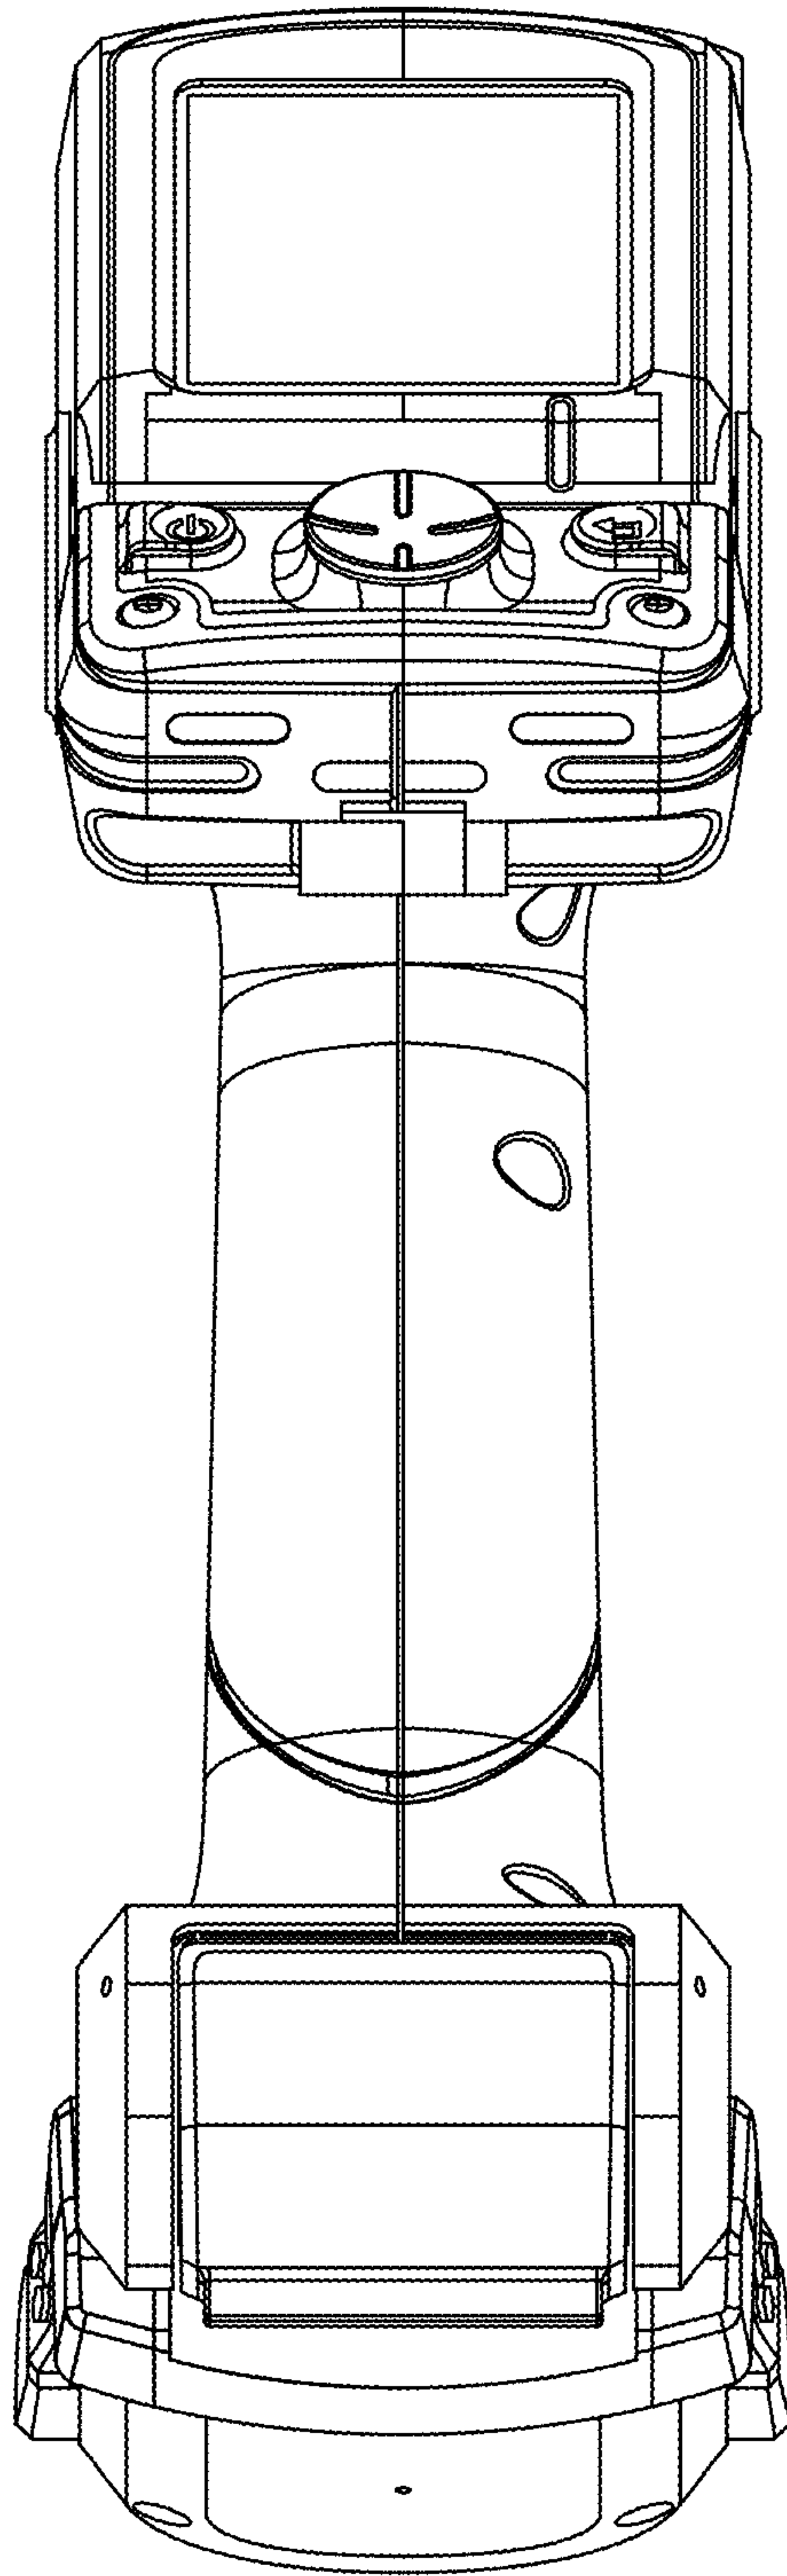


FIG. 6



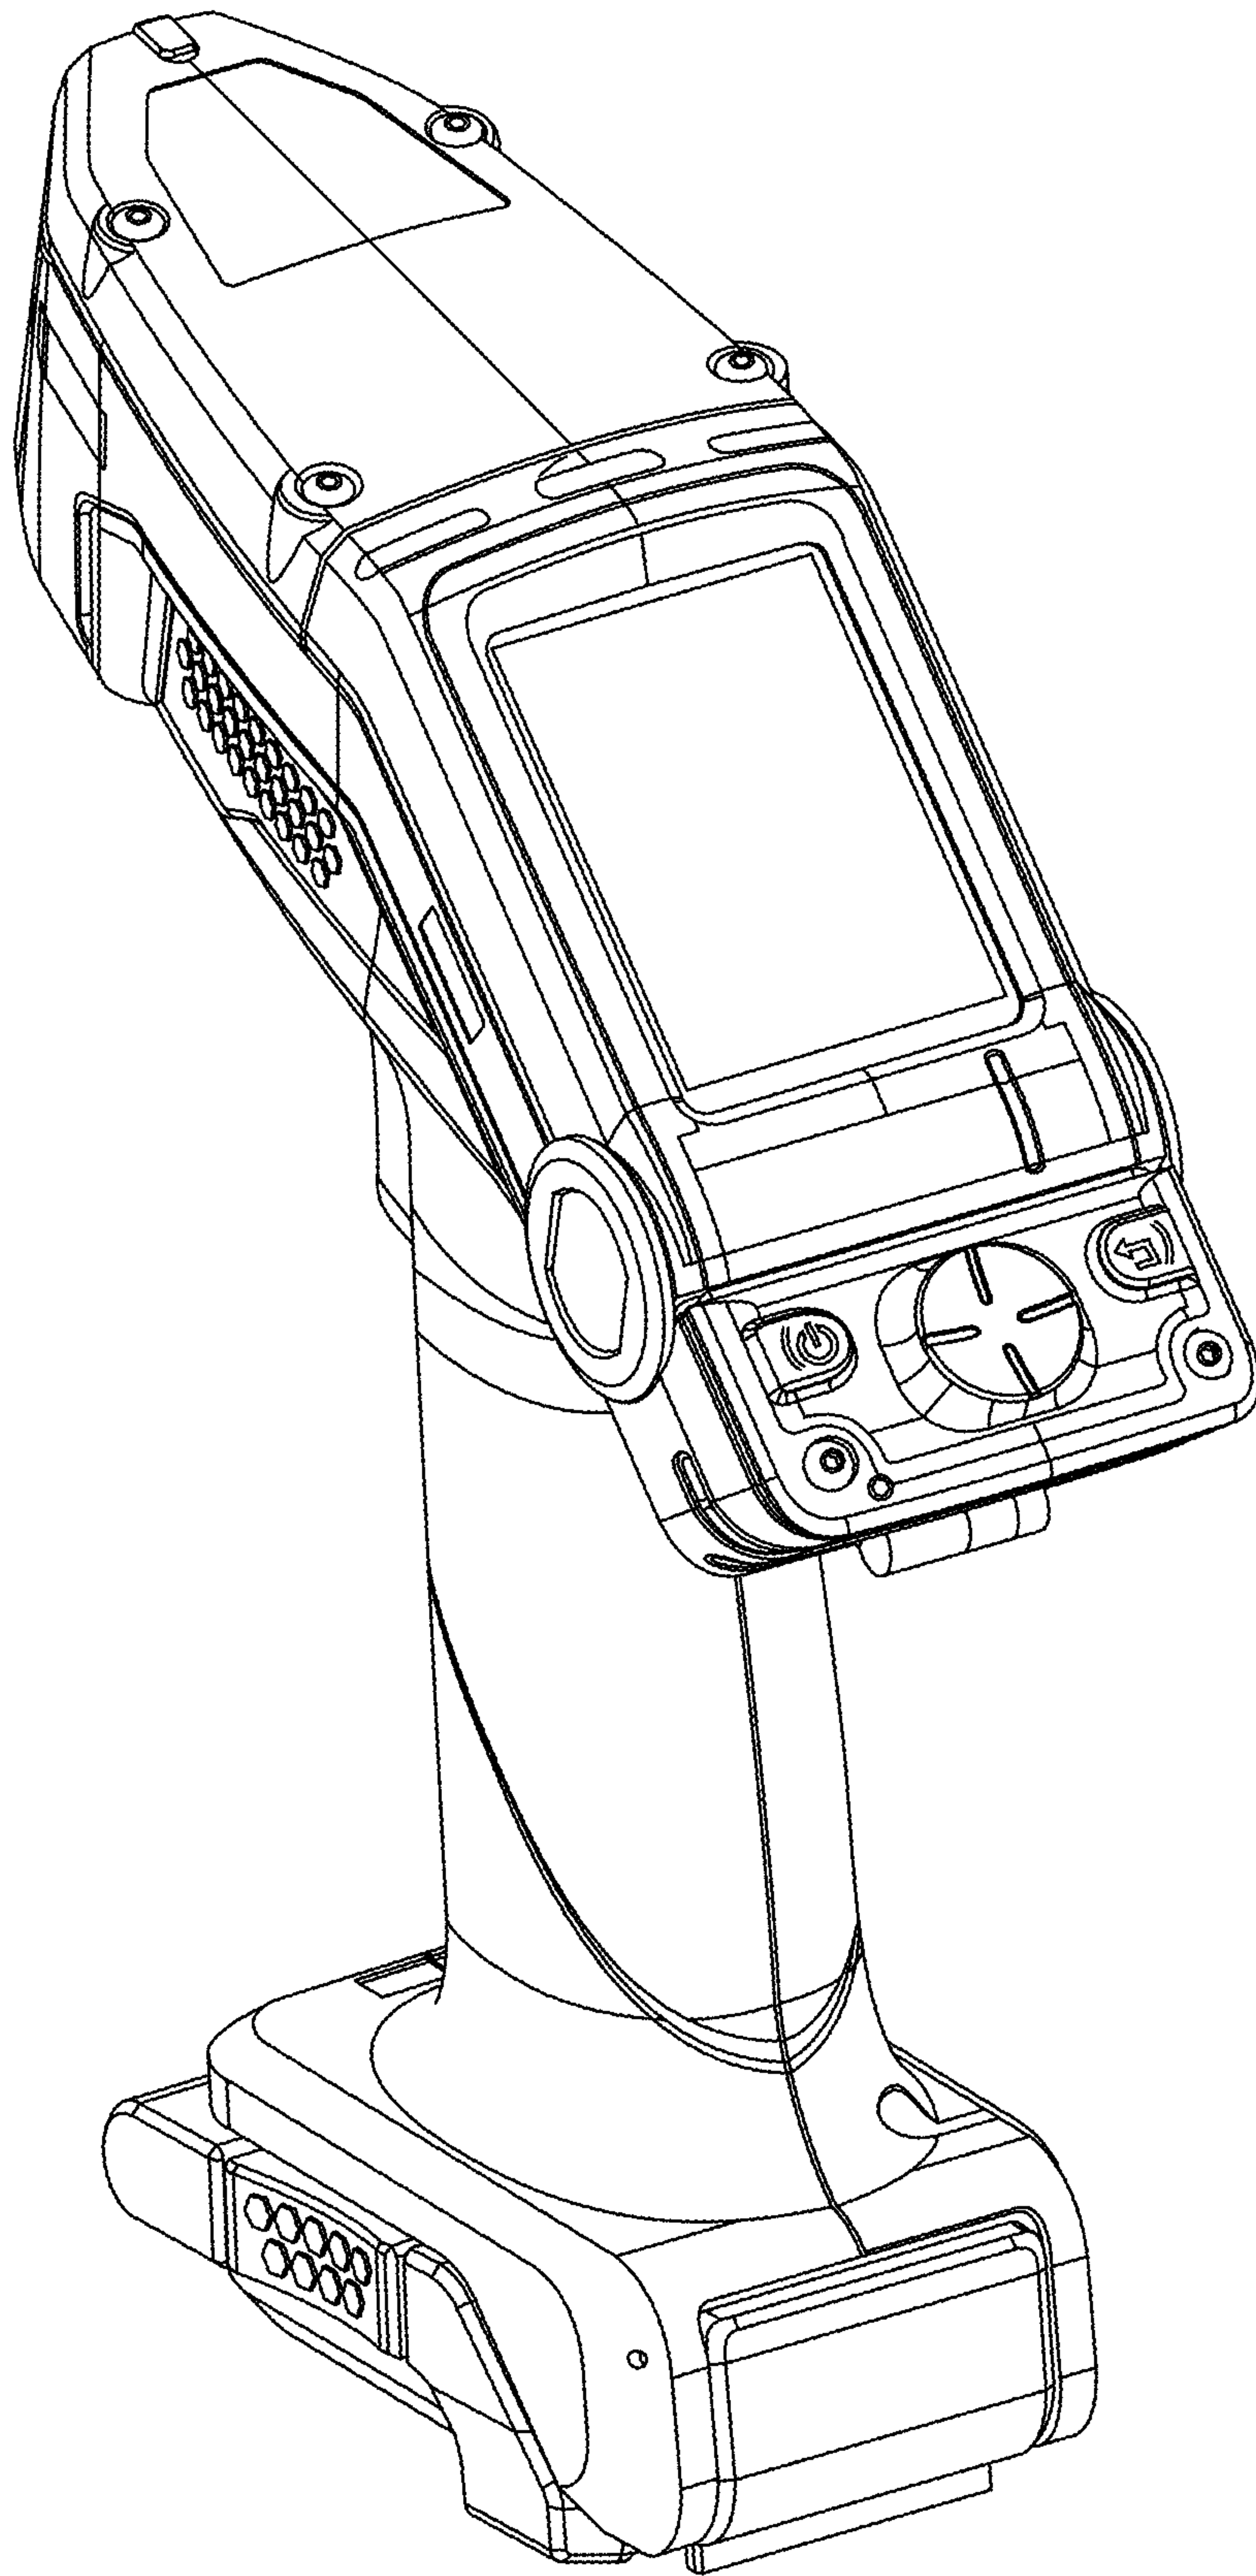


FIG. 7

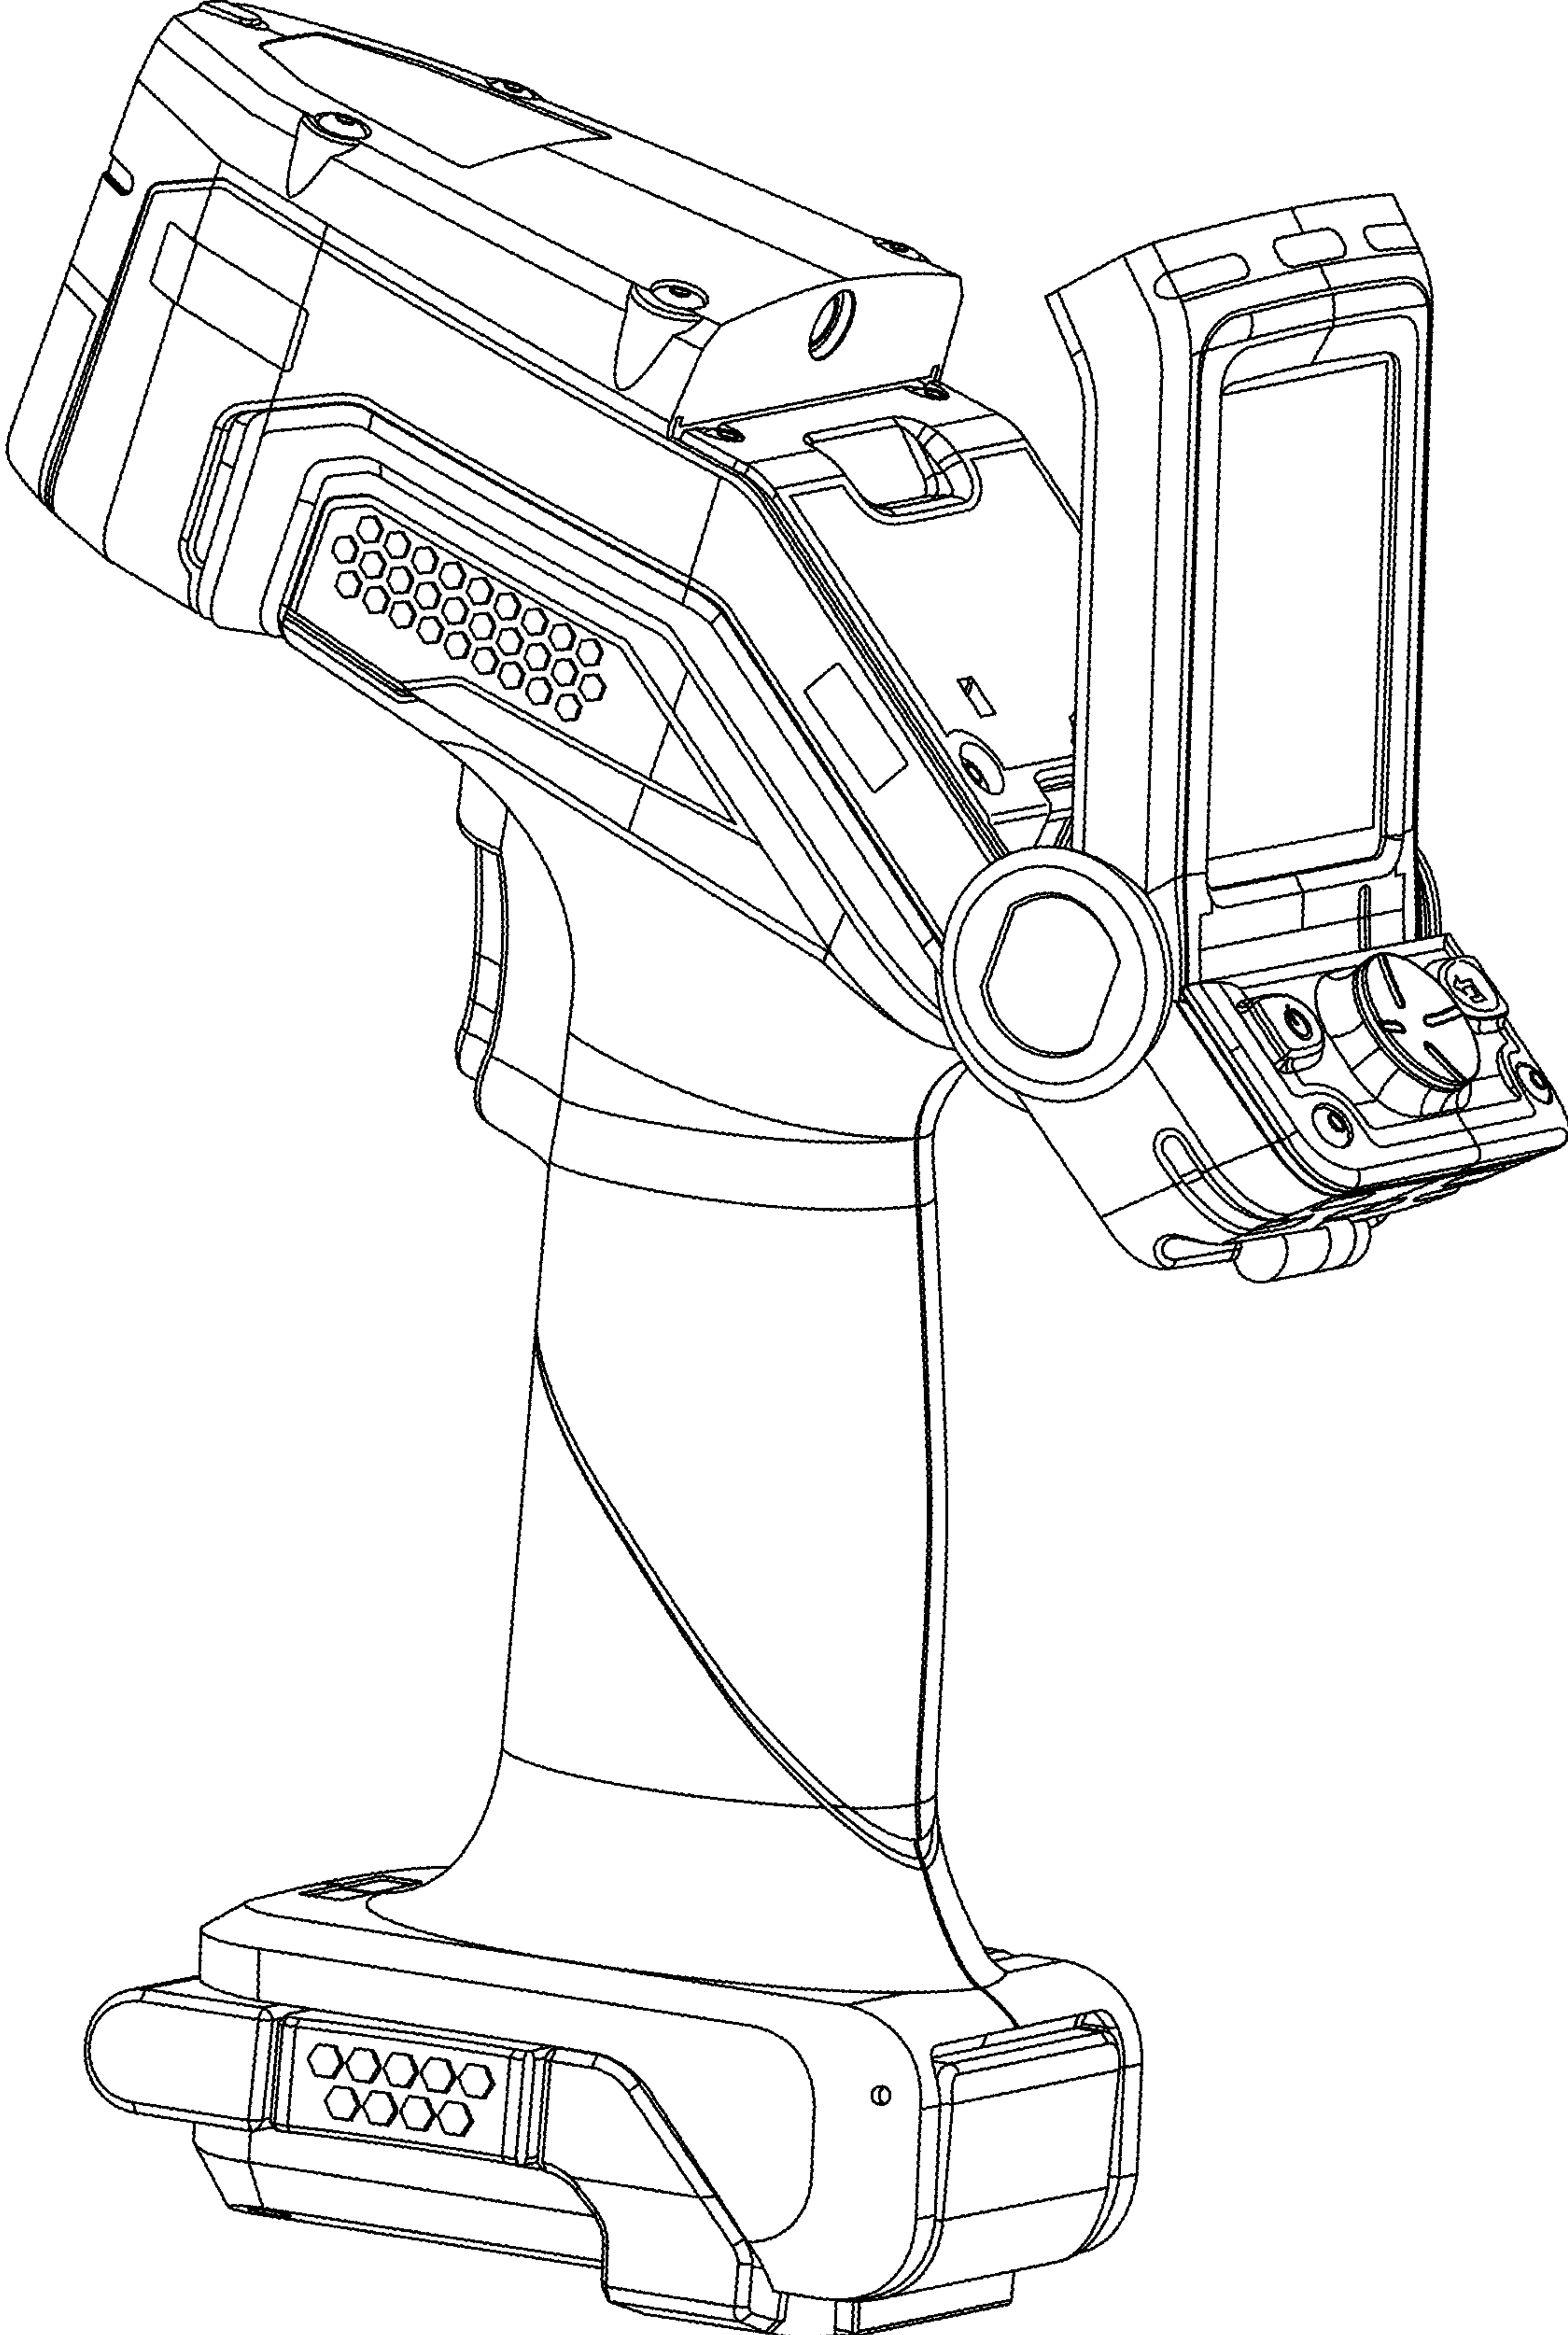


FIG. 8

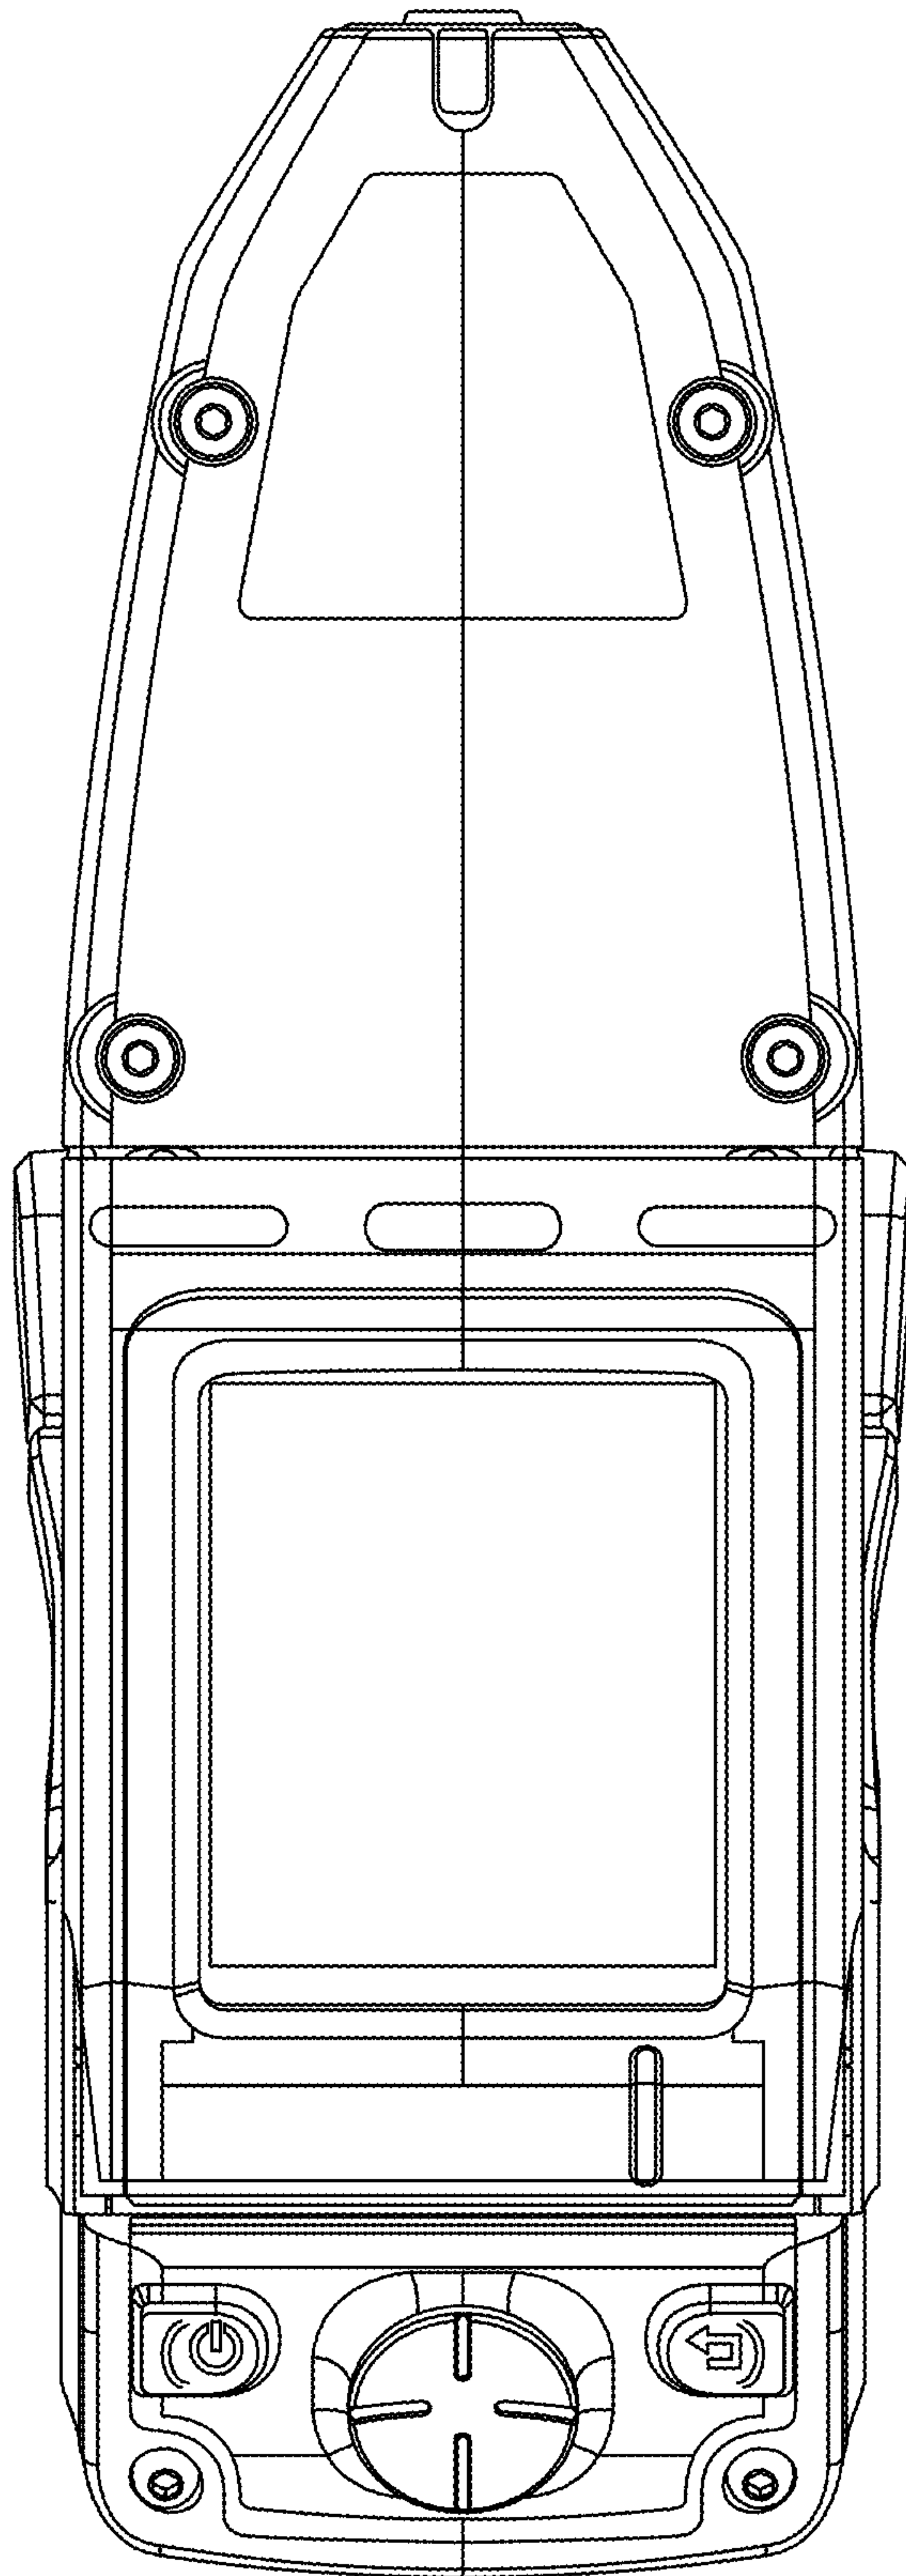


FIG. 9



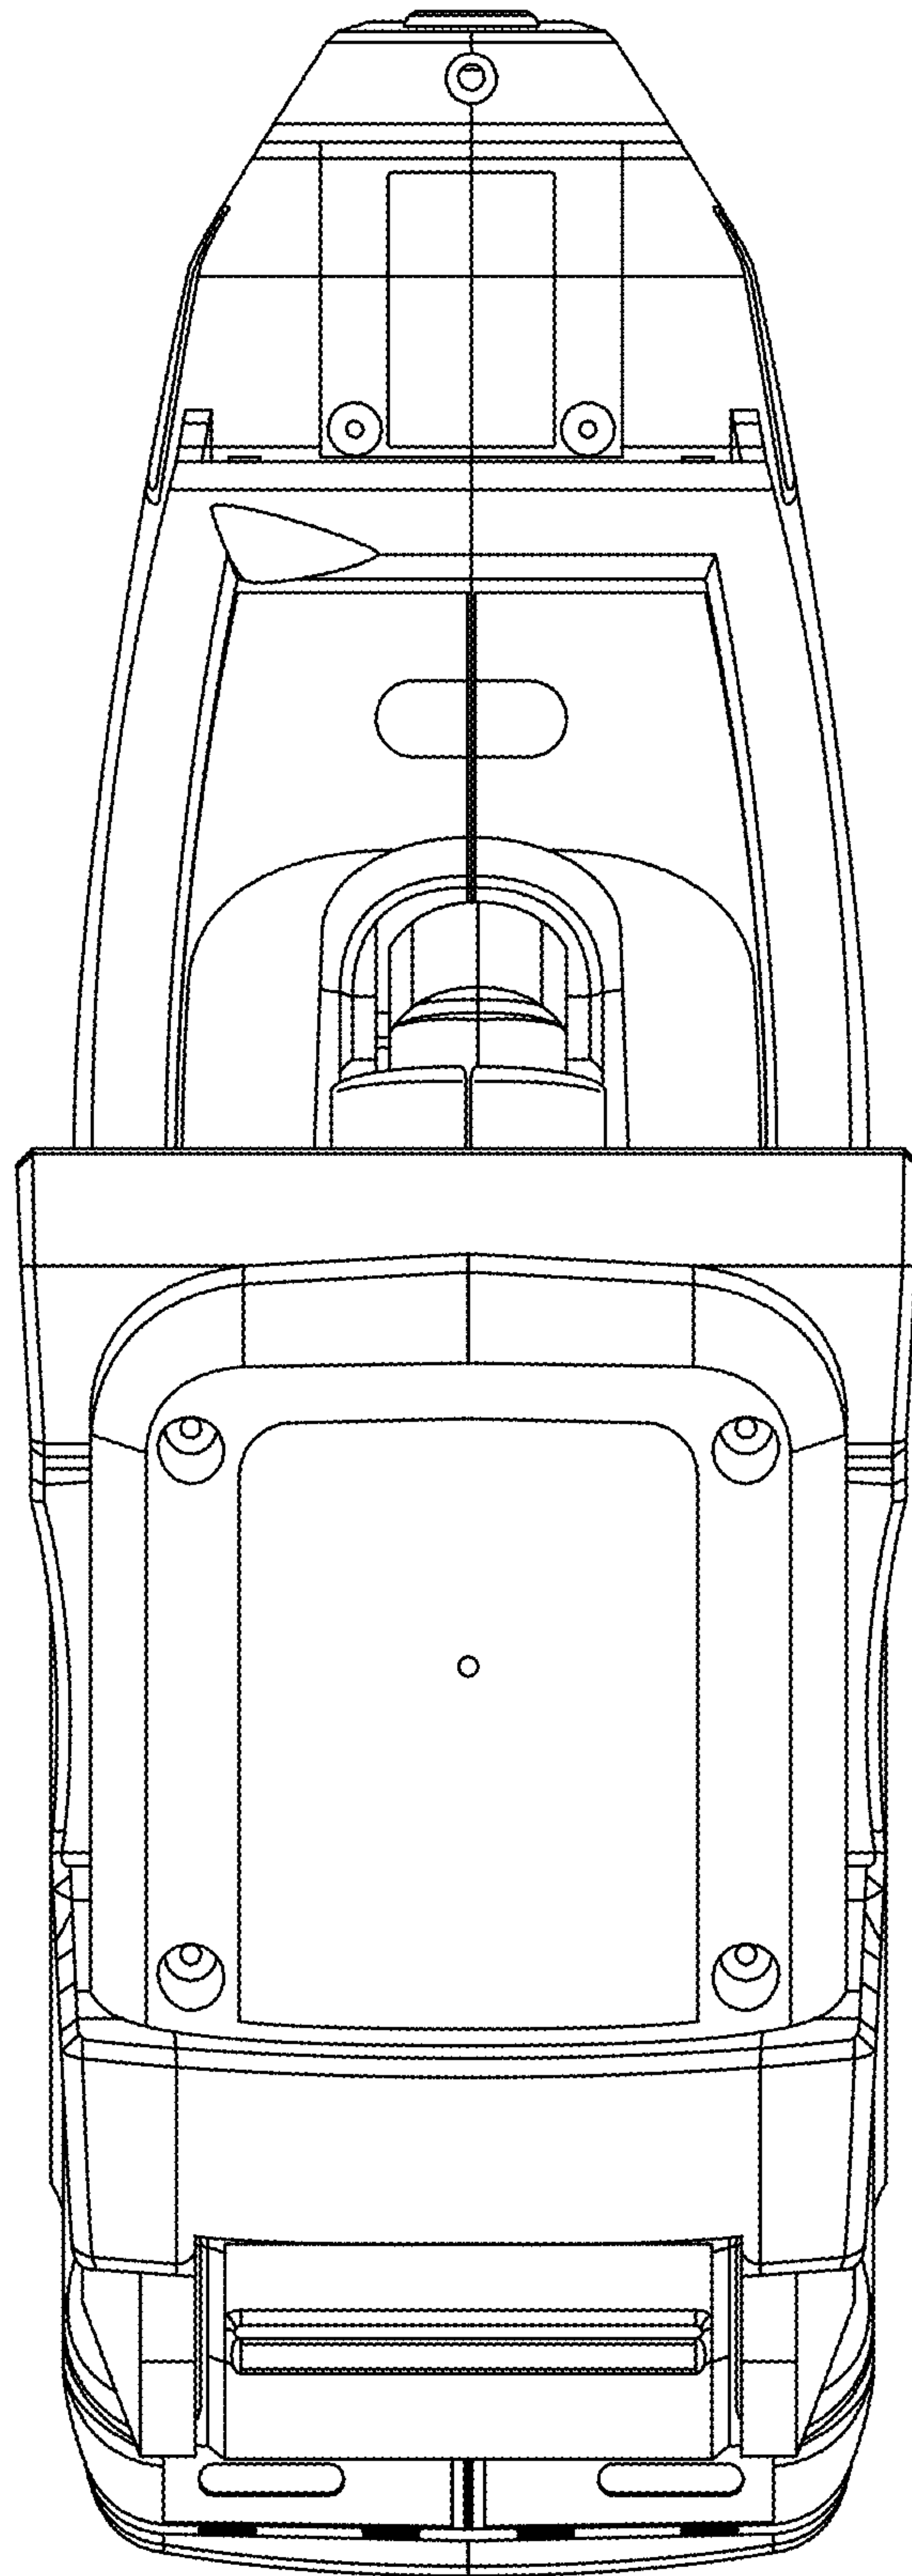


FIG. 10