



US00D820991S

(12) **United States Design Patent**  
**Hylton et al.**

(10) **Patent No.:** **US D820,991 S**  
(45) **Date of Patent:** **\*\* Jun. 19, 2018**

(54) **STIFFENER RECEIVER AND ATTACHMENT WRAP FOR ORTHOTIC DEVICE**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **CHILDREN'S THERAPY CENTER**,  
Burien, WA (US)

FR 2838957 A1 10/2003  
WO WO 2004/019812 A2 3/2004

(72) Inventors: **Nancy Hylton**, Burien, WA (US); **Brad Shatto**, Burien, WA (US); **Christie Skoorsmith**, Burien, WA (US)

*Primary Examiner* — Thomas Johannes

*Assistant Examiner* — Samantha Q. Lawrence

(74) *Attorney, Agent, or Firm* — R. Reams Goodloe, Jr.

(73) Assignee: **CHILDREN'S THERAPY CENTER**,  
Burien, WA (US)

(57) **CLAIM**

The ornamental design for a stiffener receiver and attachment wrap for orthotic device, as shown and described.

(\*\*) Term: **15 Years**

**DESCRIPTION**

(21) Appl. No.: **29/581,248**

(22) Filed: **Oct. 17, 2016**

(51) **LOC (11) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/190**

(58) **Field of Classification Search**  
USPC ..... D24/189, 190, 191, 192, 188, 206, 207;  
D29/101.1, 101.2, 122, 113, 117.1-119,  
D29/123; 602/7, 16, 20, 23, 27, 28, 56,  
602/60, 61, 62, 65, 66; D2/618, 619,  
D2/621, 610  
CPC .. A61F 5/028; A61F 5/02; A61F 5/022; A61F  
5/055; Y10S 128/23  
See application file for complete search history.

FIG. 1 is a perspective view of a stiffener receiver and attachment wrap for orthotic device in accordance with the invention comprising a stiffener receiver, and a body conforming attachment wrap.

FIG. 2 is a front view of a stiffener receiver and attachment wrap for orthotic device.

FIG. 3 is a back view of a stiffener receiver and attachment wrap.

FIG. 4 is a right side view of the stiffener receiver and attachment wrap for orthotic device.

FIG. 5 is a left side view of the stiffener receiver and attachment wrap for orthotic device.

FIG. 6 is a top plan view taken looking down at the top of the stiffener receiver and attachment wrap for orthotic device; and,

FIG. 7 is bottom plan view taken looking up at the underside of the stiffener receiver and attachment wrap for orthotic device.

In the drawing figures, surface shading is used to clearly show the character and contour of surfaces of the 3-dimensional aspects of the design, and form no part of the claimed design.

The broken lines in FIG. 1 that show a humanoid figure illustrate environment. All other broken lines illustrate stitching and form no part of the claimed design.


(56) **References Cited**

U.S. PATENT DOCUMENTS

89,018 A	4/1869	Brooks	
3,068,860 A	12/1962	Strazdas	
3,362,402 A	1/1968	Loeffel et al.	
4,143,654 A	3/1979	Sherman	
D267,976 S *	2/1983	Hammer et al.	D24/190
4,715,362 A	12/1987	Scott	
4,753,245 A	6/1988	Gedeon	
D300,475 S *	3/1989	Caulder	D29/101.1

(Continued)

**1 Claim, 4 Drawing Sheets**

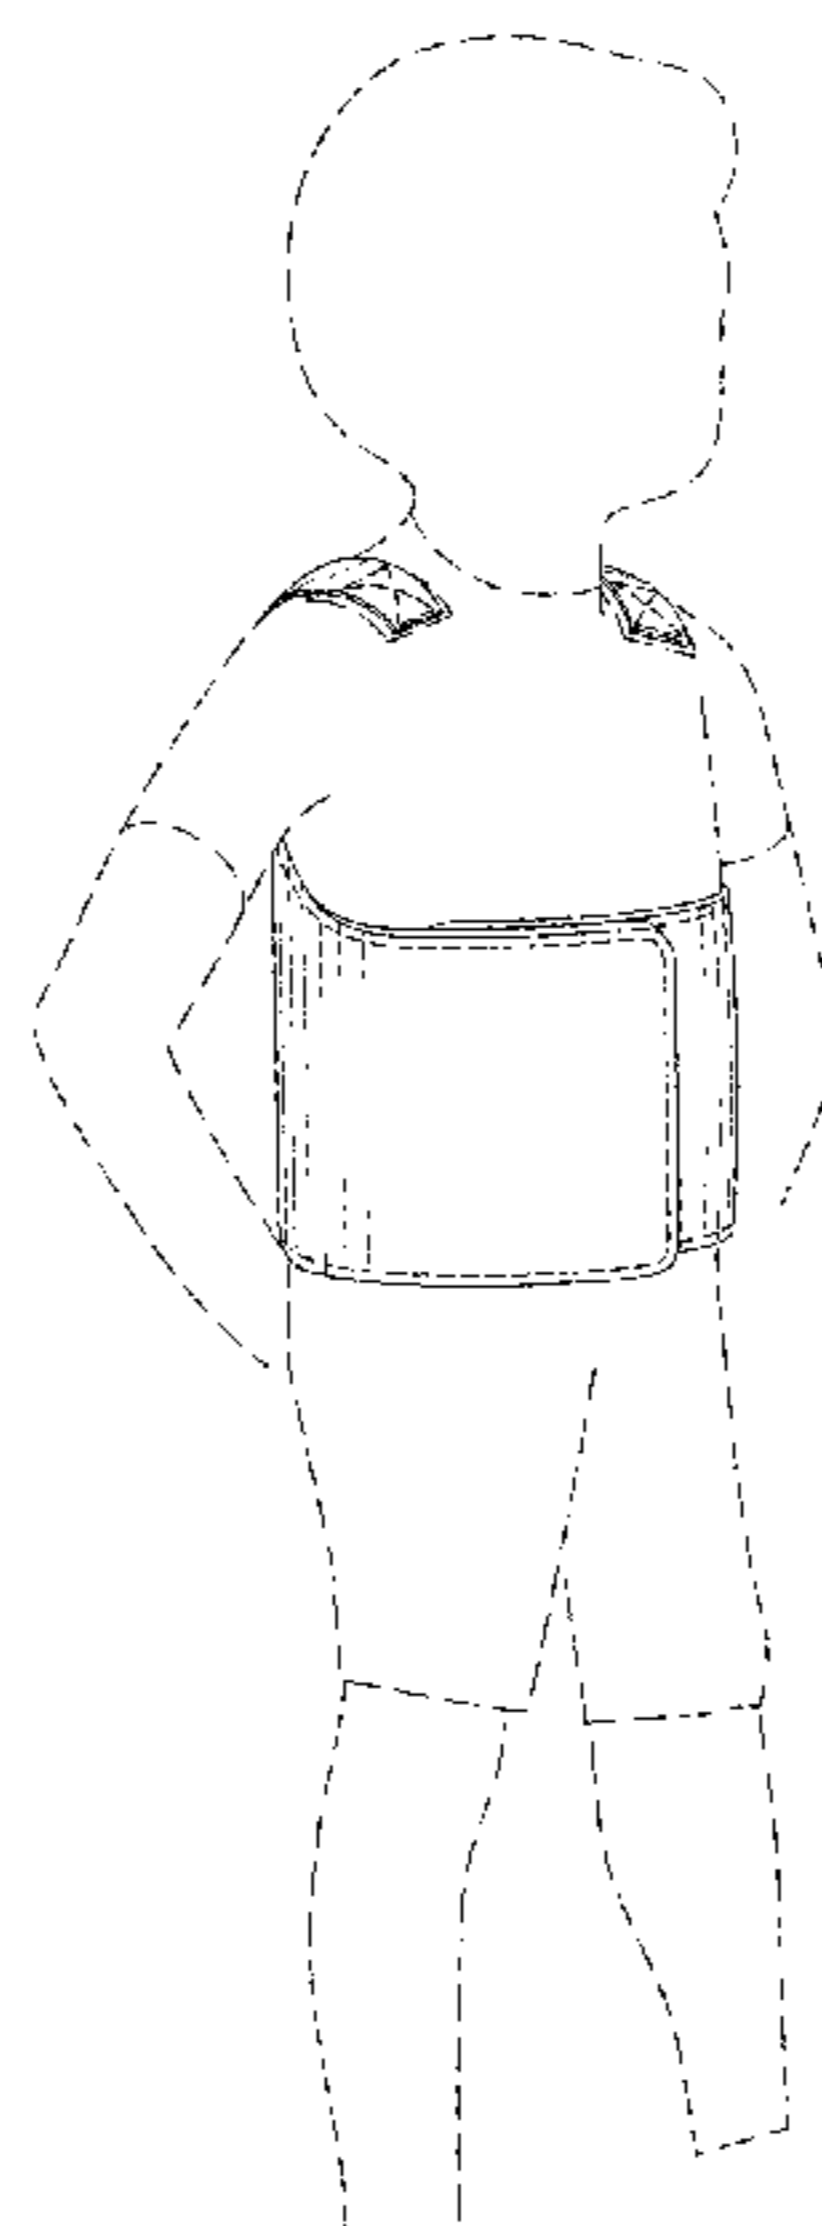

(56)

References Cited


U.S. PATENT DOCUMENTS



5,007,412 A 4/1991 DeWall  
 5,072,725 A 12/1991 Miller  
 D323,909 S 2/1992 DeWall  
 D326,492 S \* 5/1992 Leibowitz ..... D21/683  
 D334,063 S \* 3/1993 DeWall ..... D24/190  
 5,259,831 A 11/1993 Lebron  
 5,312,669 A 5/1994 Bedard  
 5,399,151 A \* 3/1995 Smith ..... A61F 5/028  
 2/44  
 D370,744 S \* 6/1996 Roberson ..... D2/829  
 D374,313 S \* 10/1996 Munoz ..... D24/190  
 D375,581 S \* 11/1996 Dyer ..... D29/101.1  
 5,709,648 A 1/1998 Webb  
 5,765,224 A \* 6/1998 Johnson ..... A41C 1/02  
 2/44  
 6,086,551 A 7/2000 Allen  
 6,213,968 B1 4/2001 Heinz et al.  
 6,364,851 B1 4/2002 Nafpliotis  
 D463,566 S \* 9/2002 Slautterback ..... D24/190  
 6,478,759 B1 11/2002 Modglin  
 6,533,358 B1 3/2003 Avihod  
 D480,145 S \* 9/2003 Slautterback ..... D24/190  
 6,932,780 B2 8/2005 Kozersky  
 7,025,737 B2 4/2006 Modglin  
 7,316,660 B1 1/2008 Modglin  
 7,322,950 B2 1/2008 Modglin  
 D608,008 S 1/2010 Jang  
 7,654,972 B2 2/2010 Alleyne  
 D612,507 S 3/2010 Arbesman et al.  
 D621,053 S 8/2010 Kase

D621,518 S 8/2010 Arbesman et al.  
 D636,964 S \* 4/2011 Thomas ..... D29/101.1  
 8,007,457 B2 8/2011 Taylor  
 D654,181 S 2/2012 Chiang  
 D663,432 S 7/2012 Nichols  
 D674,097 S 1/2013 Nichols  
 D674,098 S 1/2013 Nichols  
 D674,099 S 1/2013 Nichols  
 8,409,122 B2 4/2013 Cropper et al.  
 8,516,616 B2 8/2013 Nordstrom et al.  
 8,533,872 B1 9/2013 Rodriguez  
 8,657,769 B2 2/2014 Ingimundarson et al.  
 8,821,424 B2 9/2014 Alleyne  
 8,894,597 B2 11/2014 Newkirk  
 8,910,317 B2 12/2014 Decker  
 9,078,477 B2 7/2015 McAllister  
 9,205,015 B2 12/2015 Guillen  
 9,220,625 B2 12/2015 Ingimundarson et al.  
 D776,287 S \* 1/2017 Leonard ..... D24/190  
 D776,423 S \* 1/2017 Zhou ..... D24/190  
 D778,532 S \* 2/2017 Dorsey ..... D2/624  
 2005/0067861 A1 3/2005 Avihod  
 2006/0000478 A1 1/2006 Taylor  
 2008/0188785 A1 8/2008 Shutes et al.  
 2008/0295216 A1 12/2008 Nordstrom et al.  
 2008/0295230 A1 12/2008 Wright et al.  
 2008/0319365 A1 12/2008 Kendrick  
 2009/0133181 A1 5/2009 Nordstrom et al.  
 2011/0203030 A1 8/2011 Nordstrom et al.  
 2012/0150085 A1 6/2012 Kayser  
 2013/0053750 A1 2/2013 Taylor  
 2013/0086729 A1 4/2013 Carter et al.  
 2014/0249459 A1 9/2014 Dallison et al.

\* cited by examiner

FIG. 1

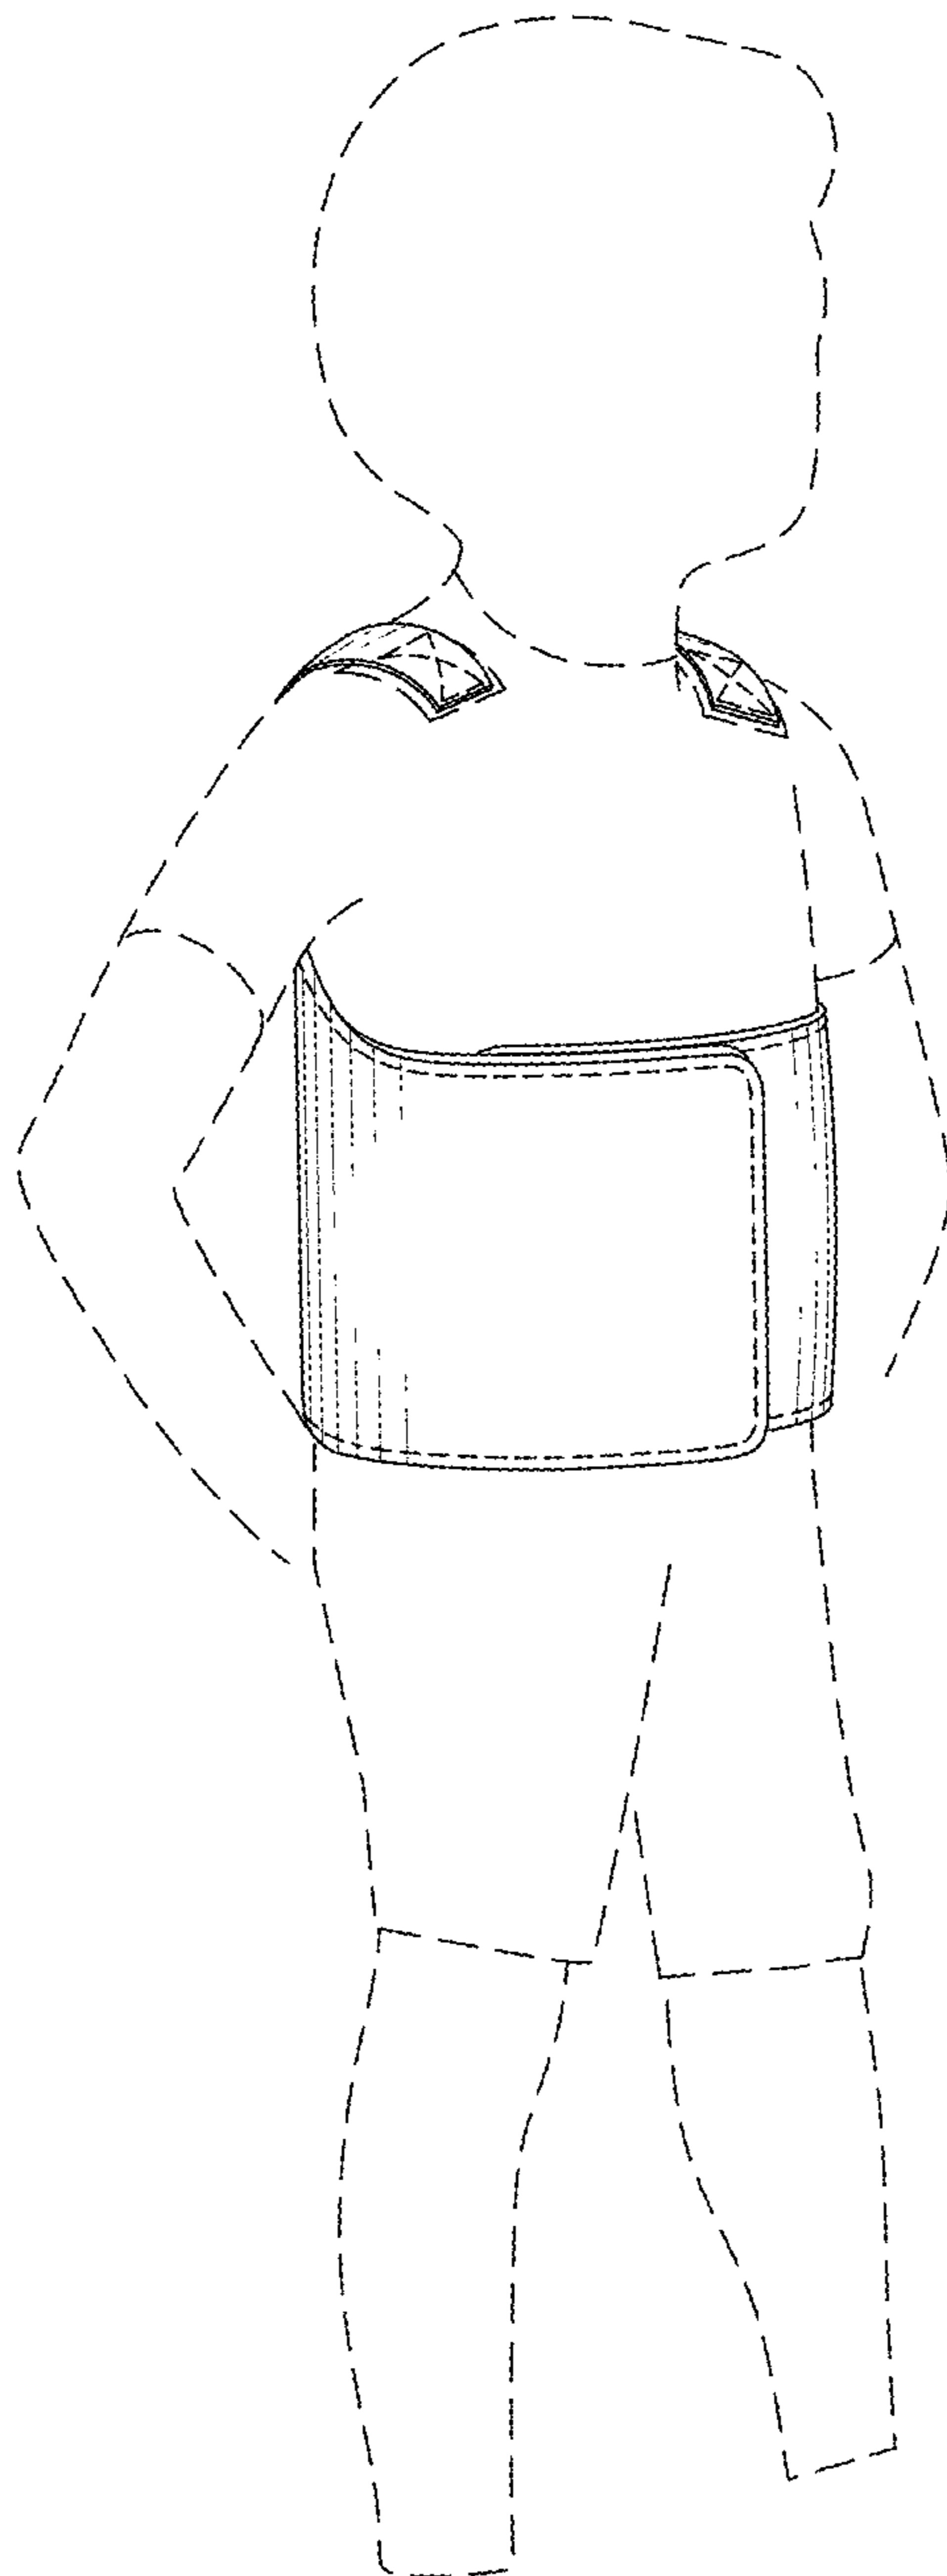

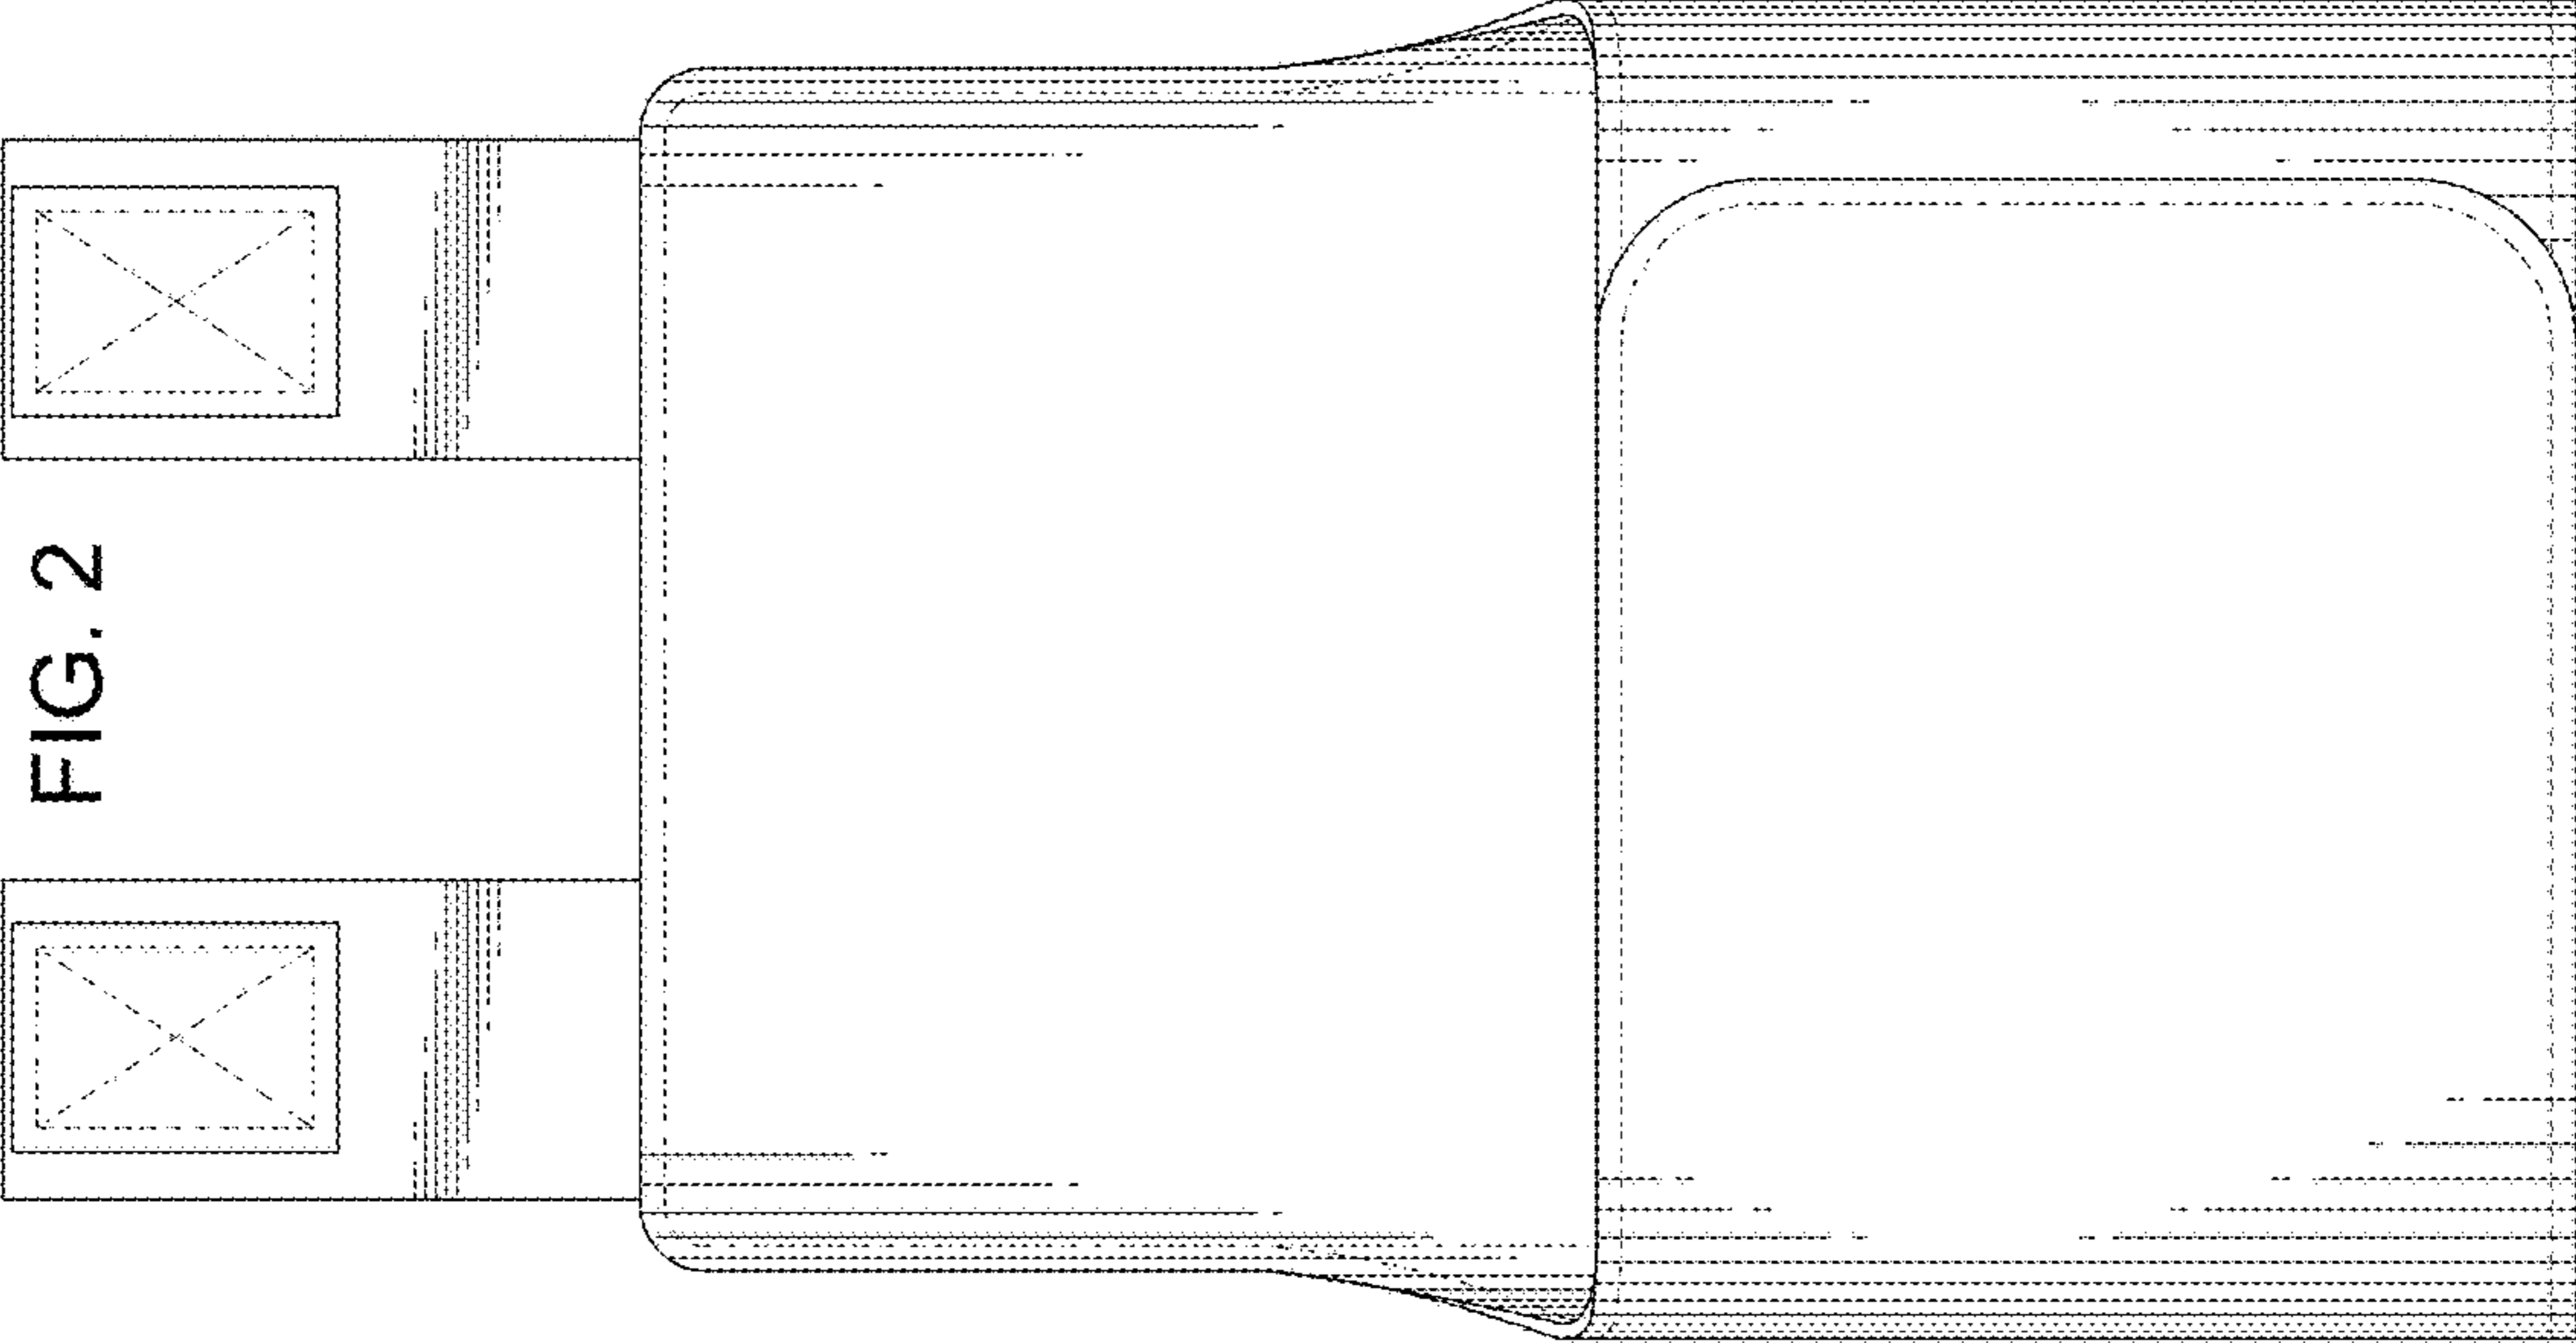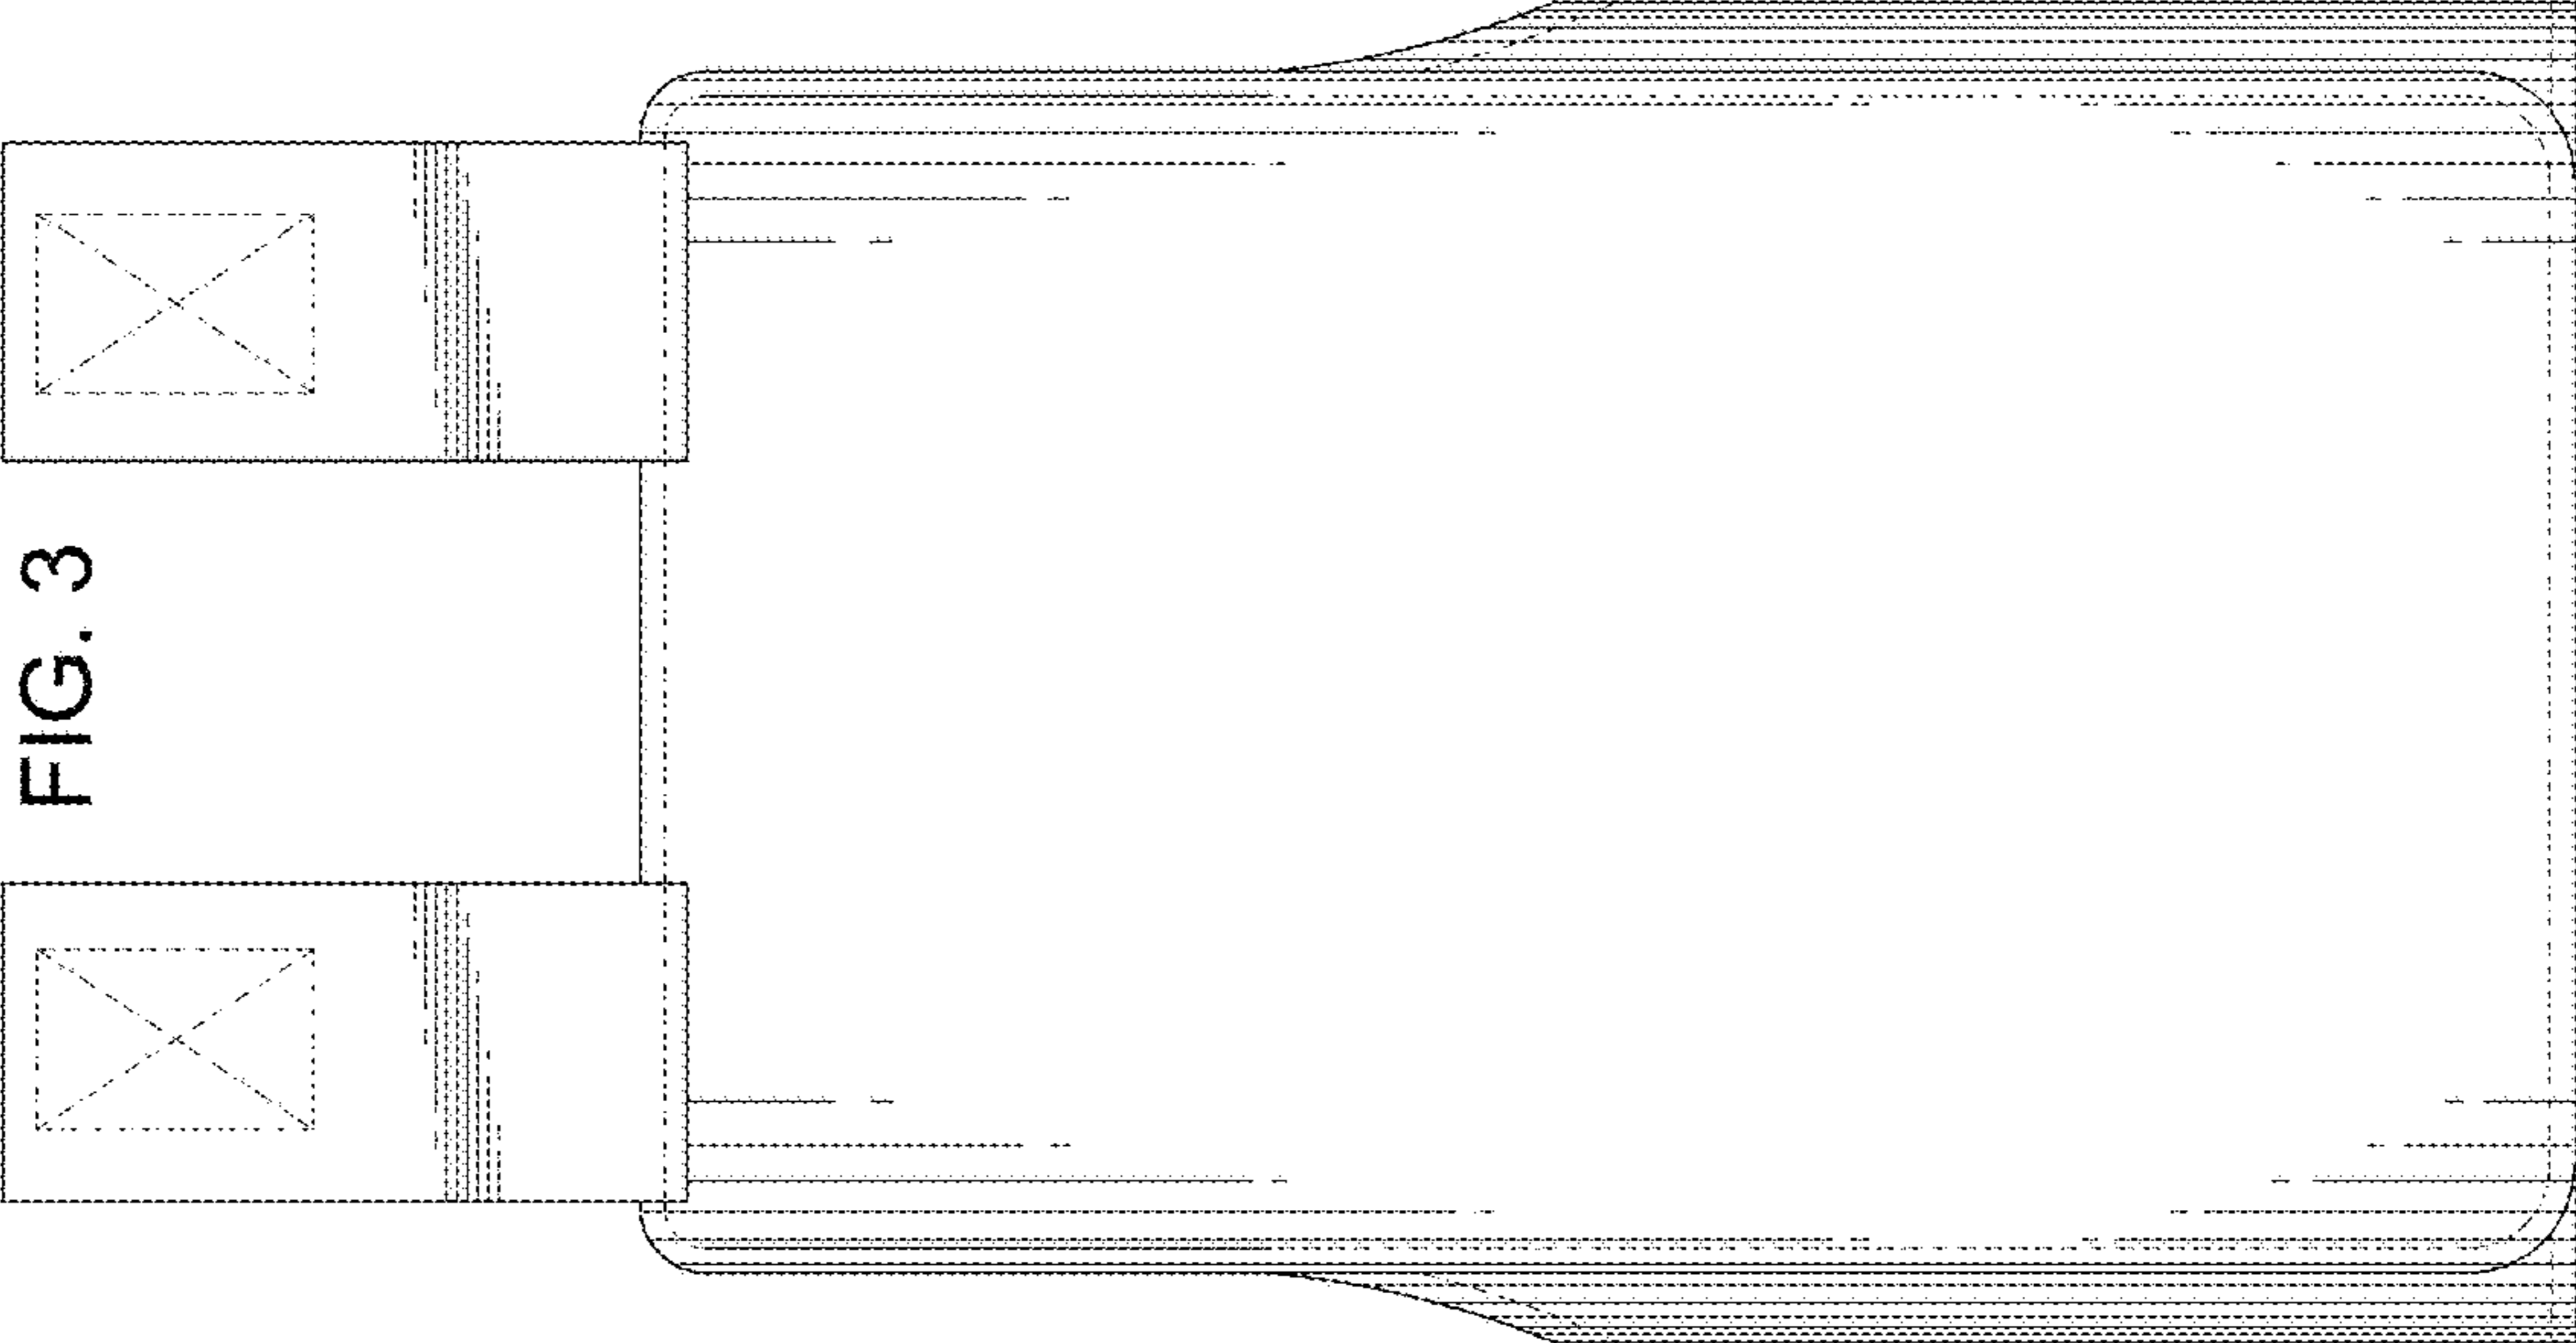

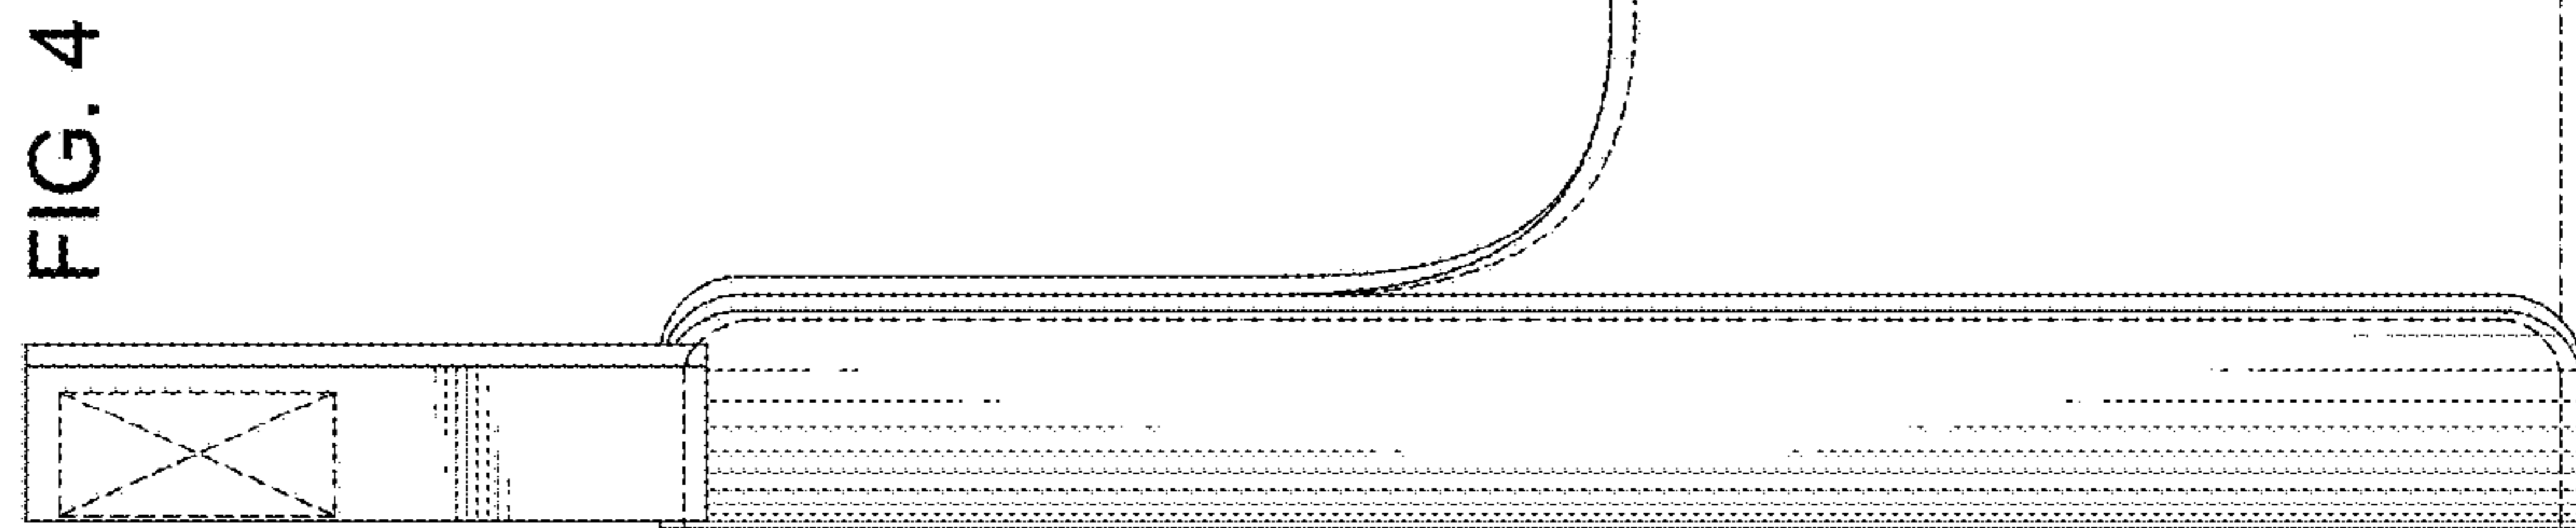
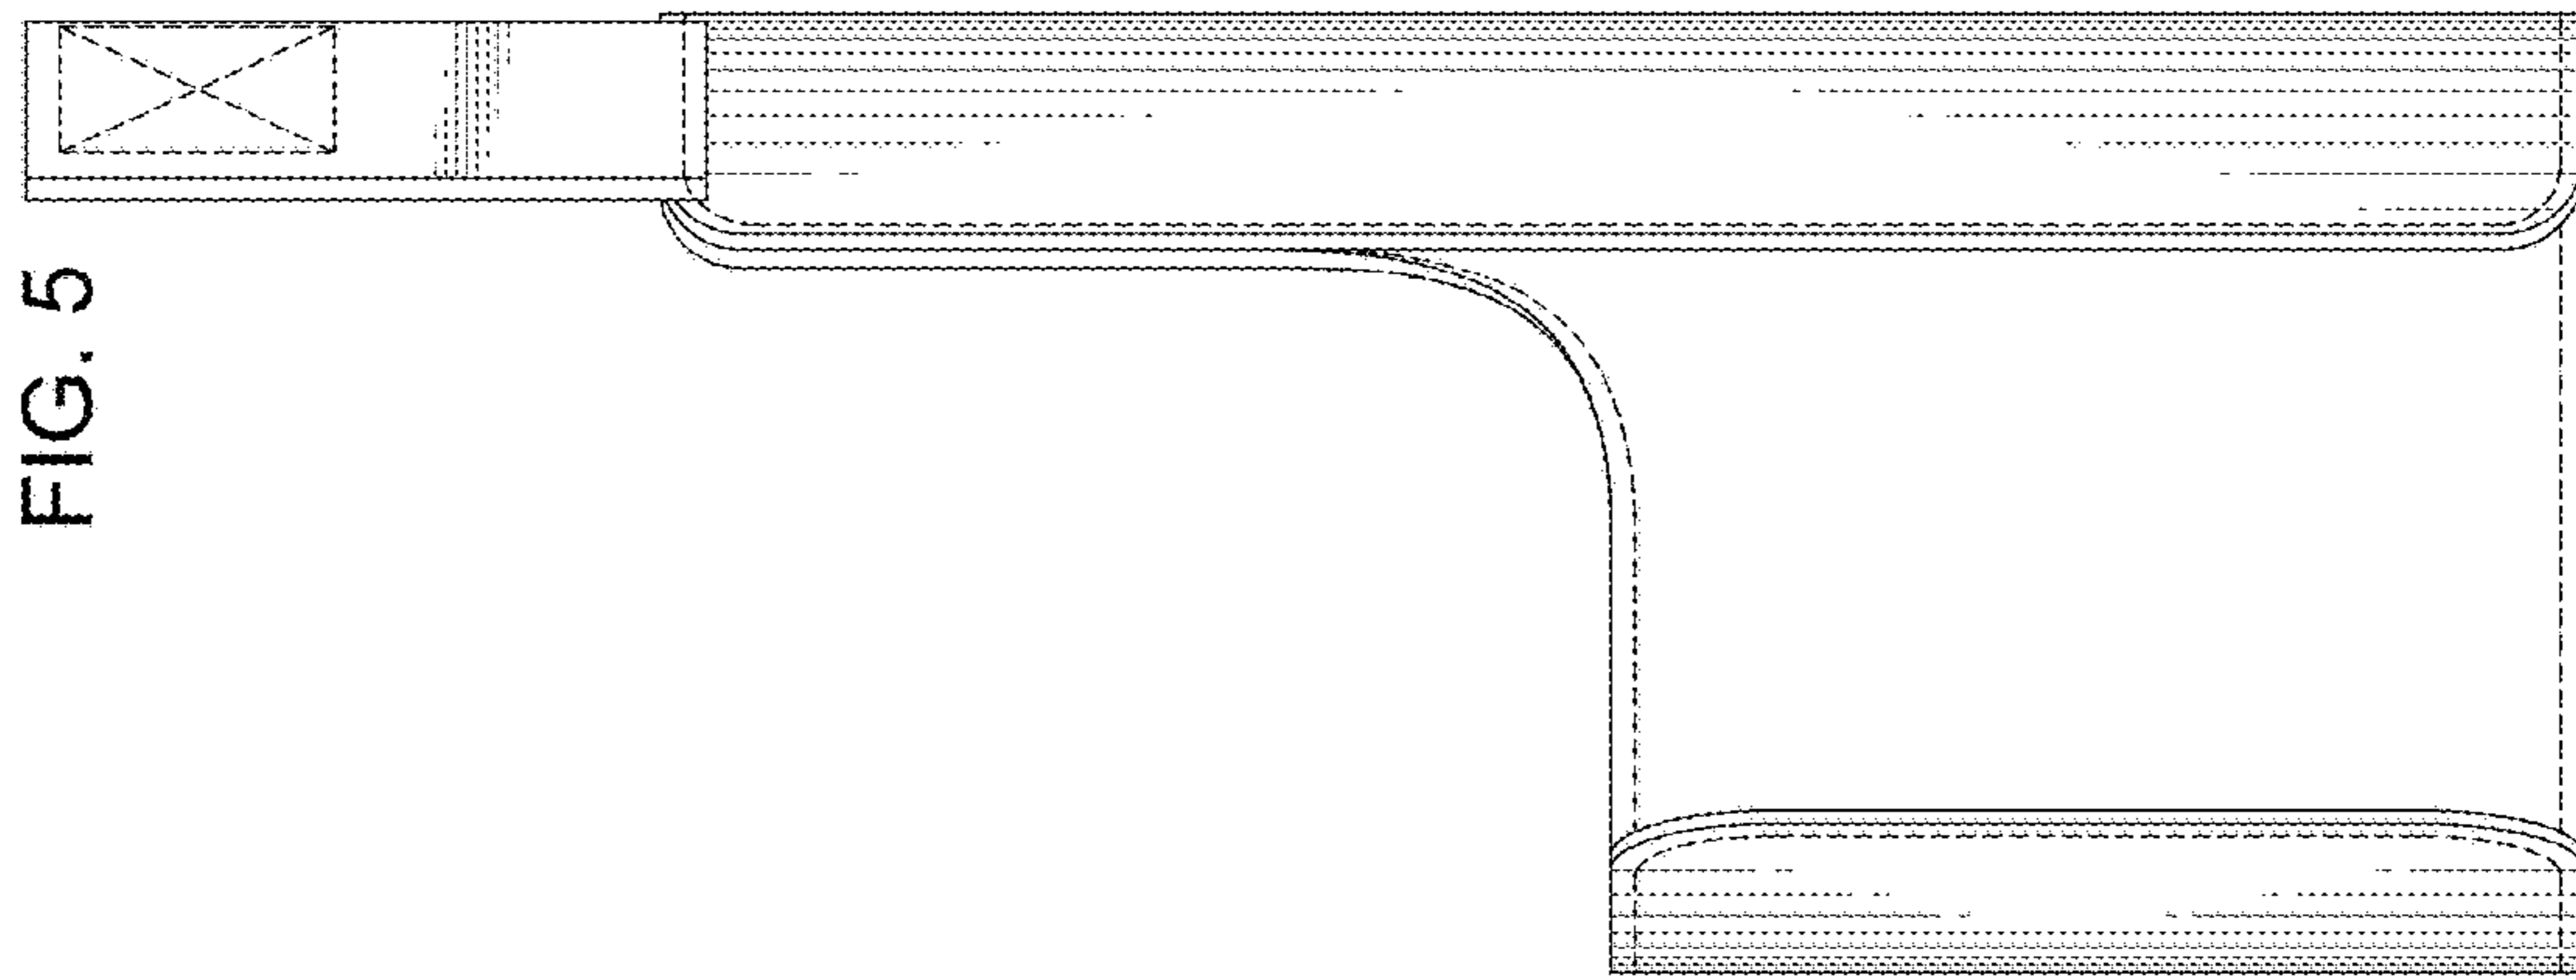


FIG. 6


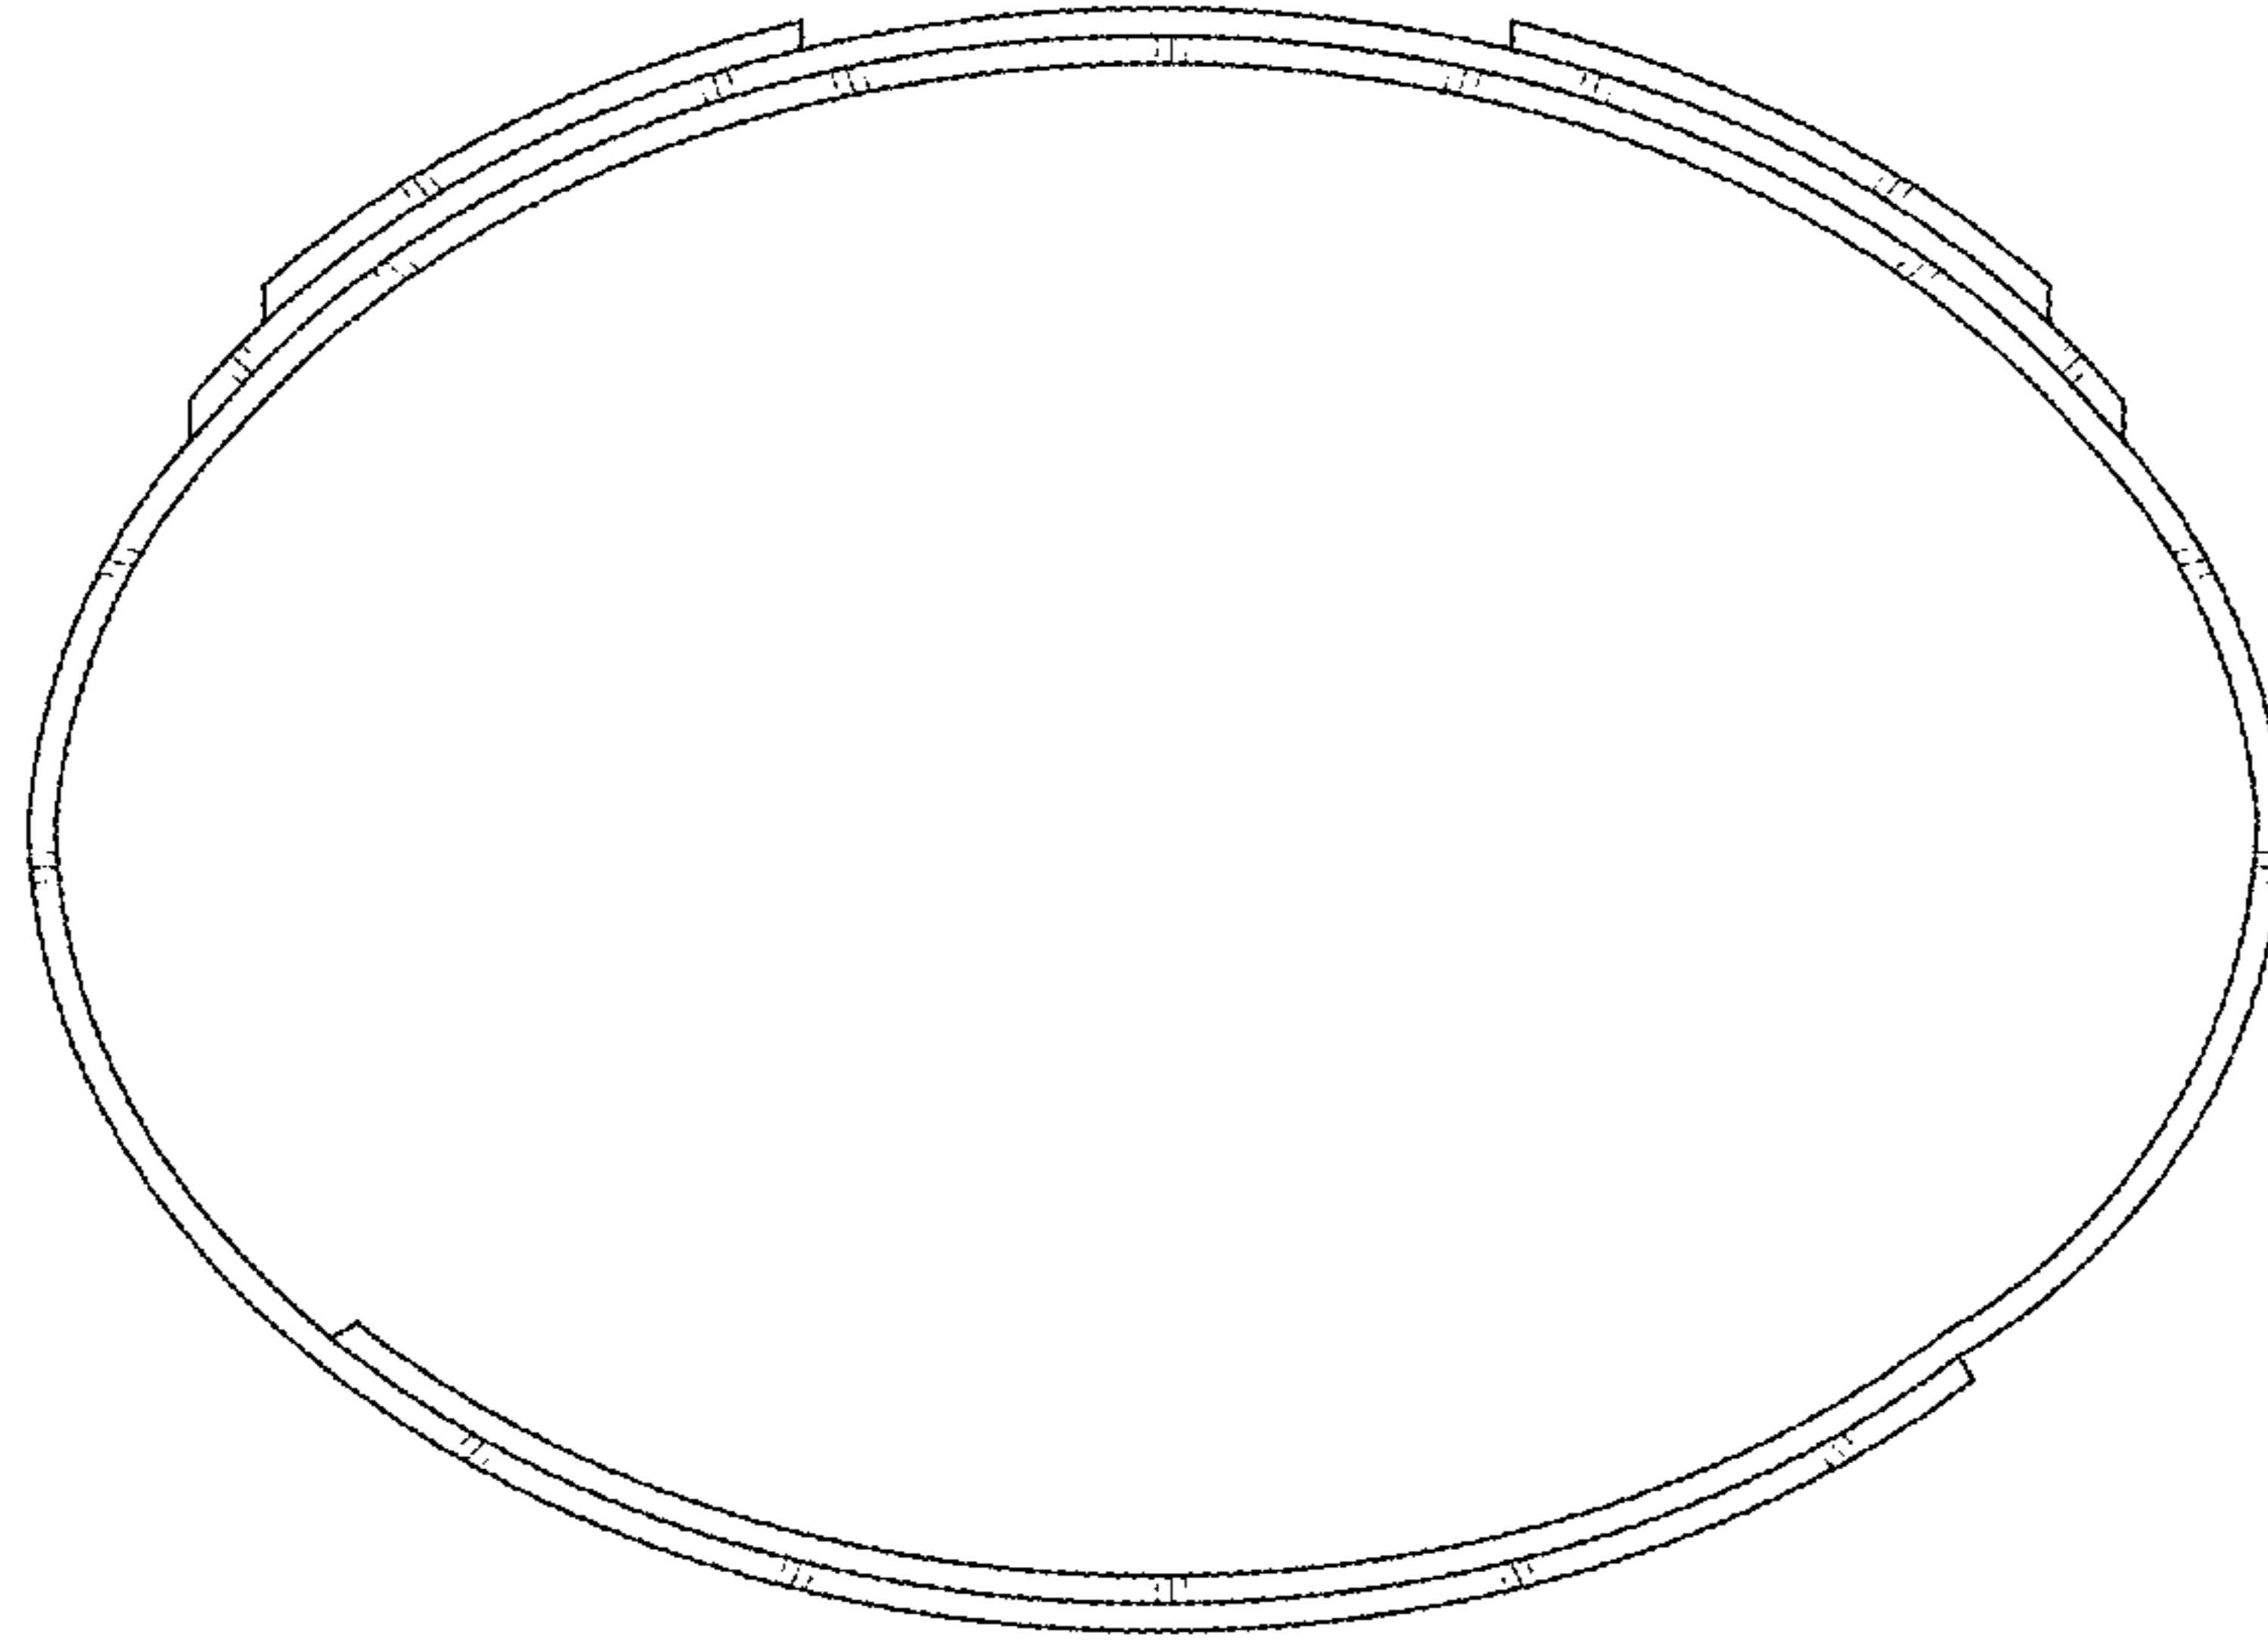


FIG. 7

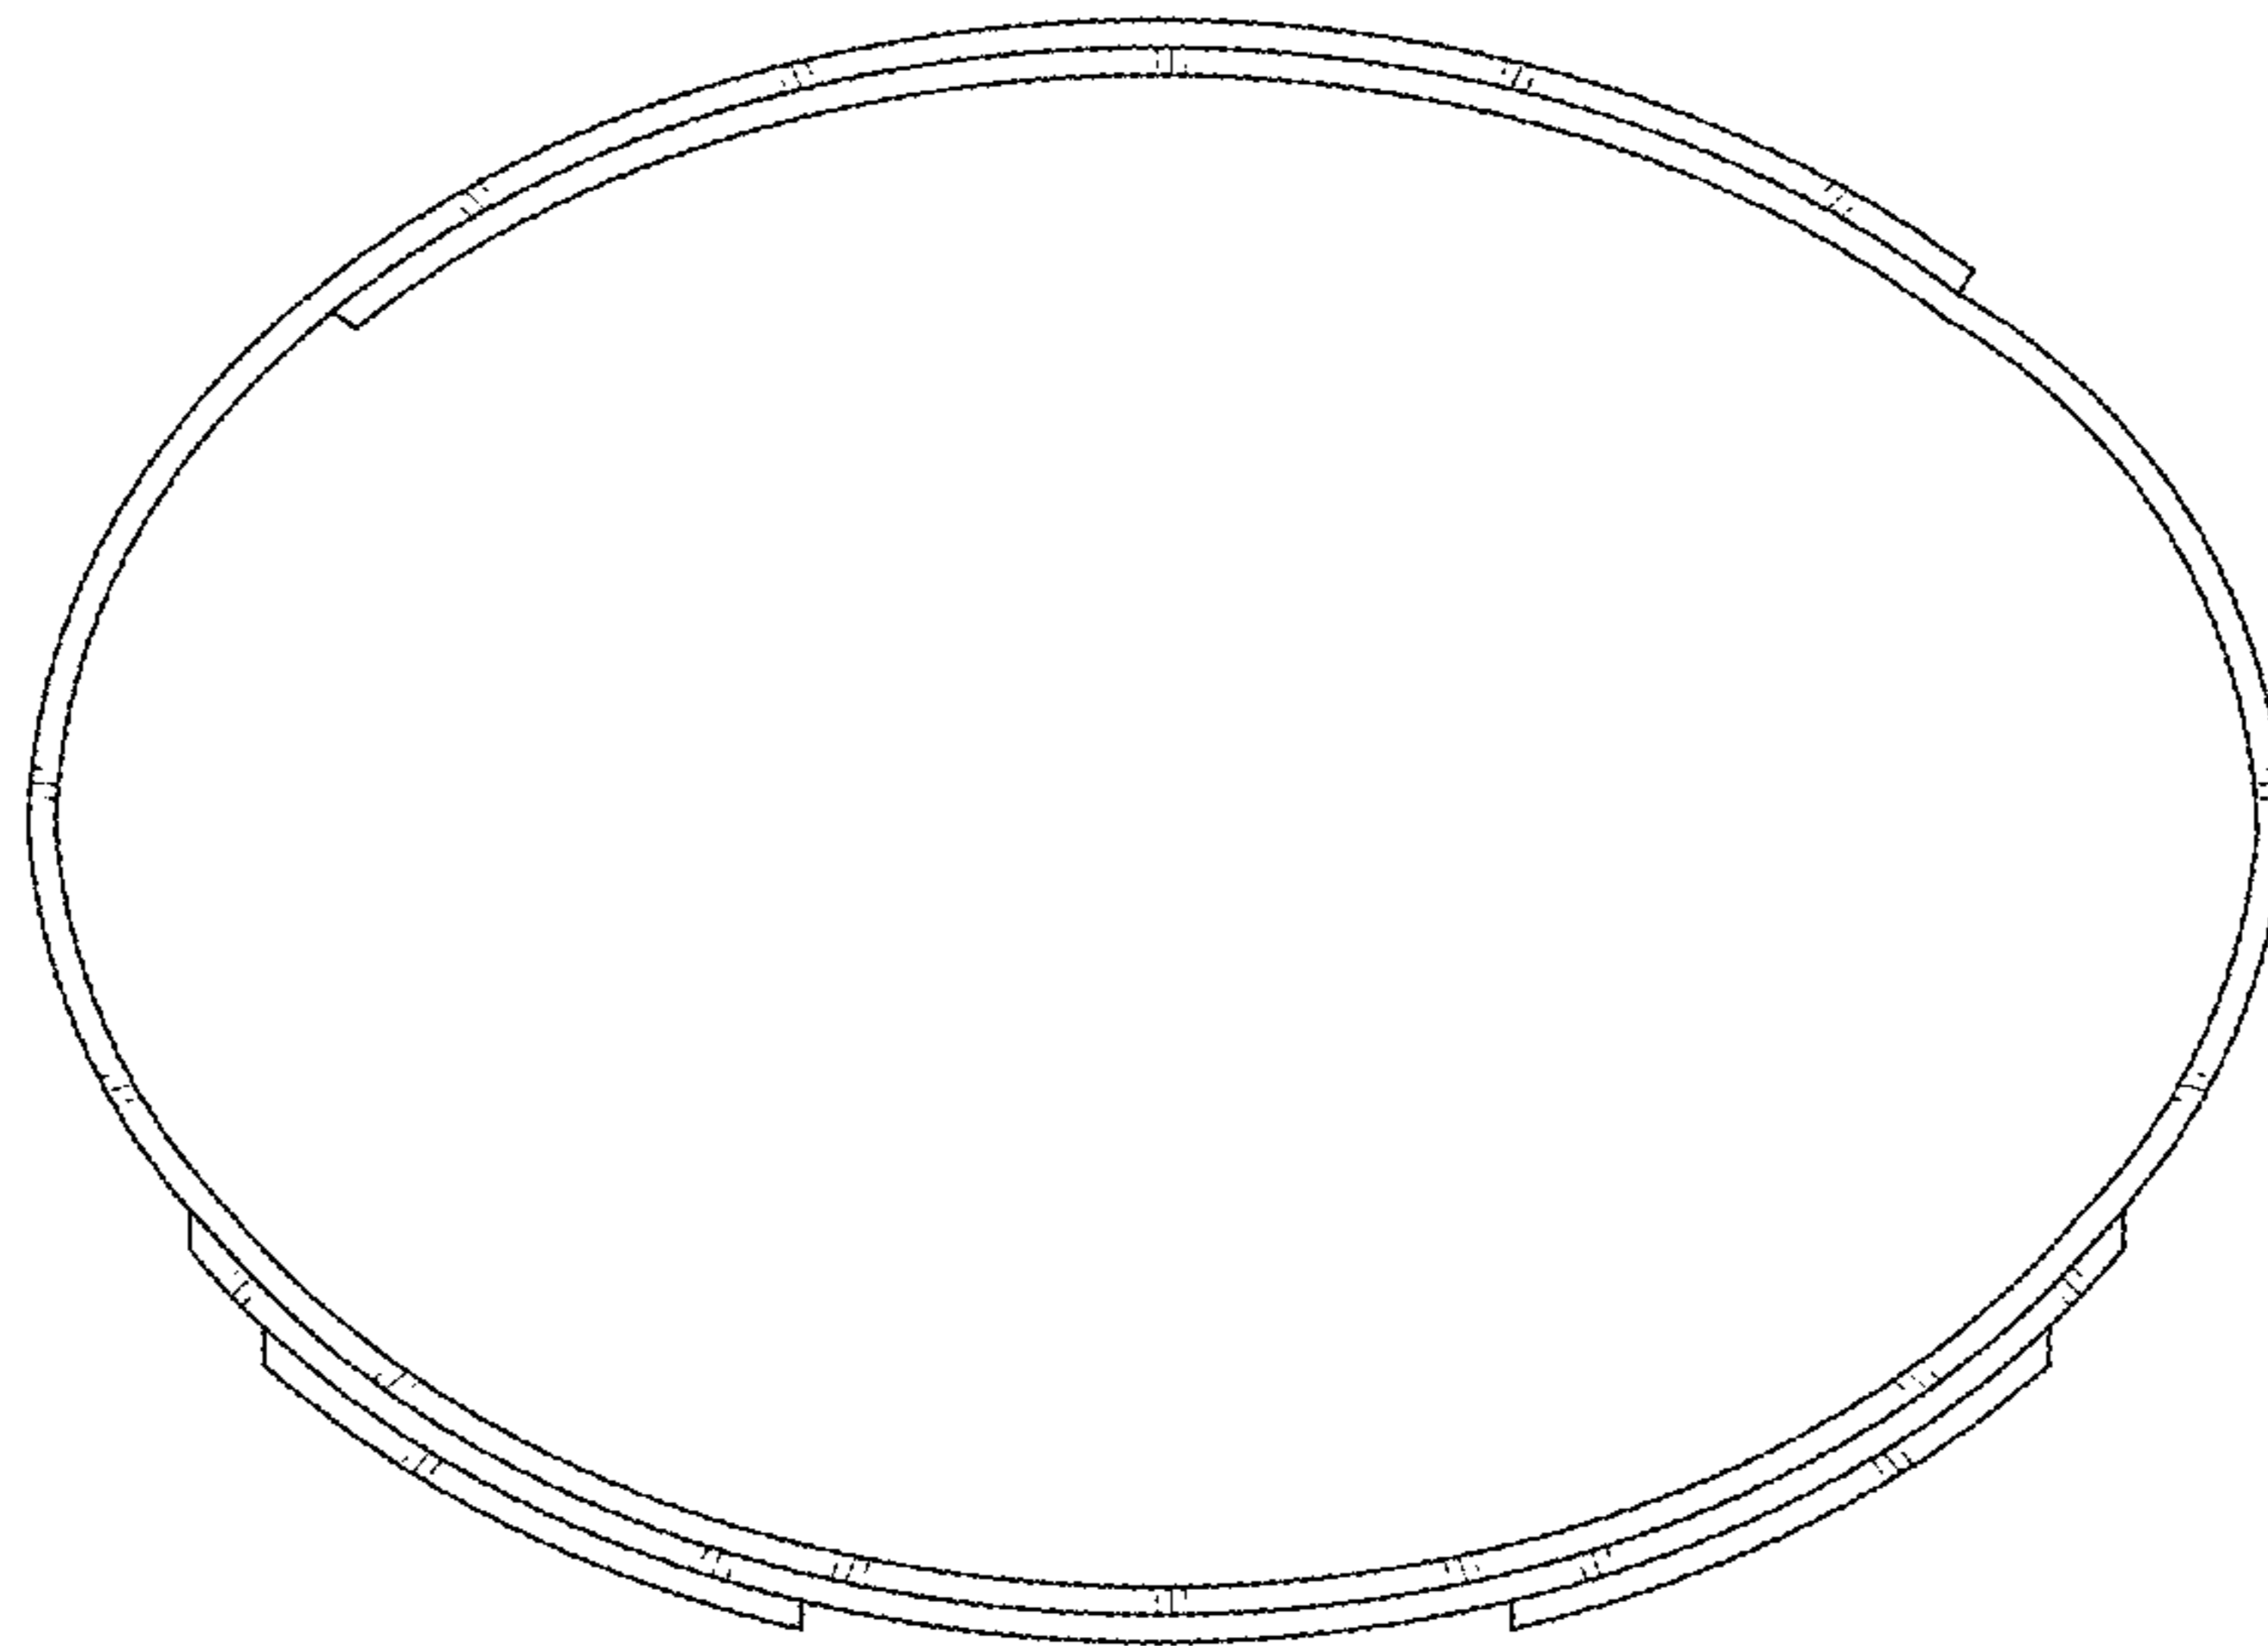

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : D820,991 S  
APPLICATION NO. : 29/581248  
DATED : June 19, 2018  
INVENTOR(S) : Nancy Hylton, Brad Shatto and Christie Skoorsmith

Page 1 of 1


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

IN THE DESCRIPTION

Column 2, Line 27 In the reference to “Fig. 6”, after the words “wrap for orthotic device”, delete “; and,” and insert --.--.

Signed and Sealed this  
Twentieth Day of August, 2019

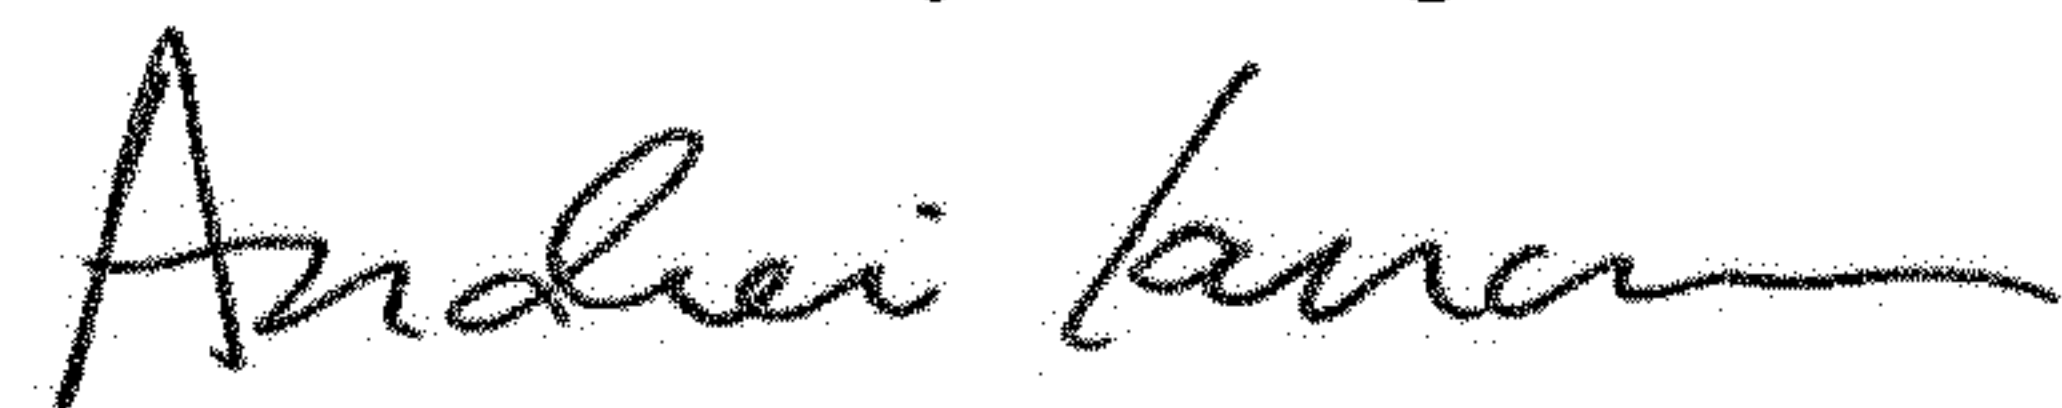

Andrei Iancu  
*Director of the United States Patent and Trademark Office*