



US00D822211S

(12) **United States Design Patent** (10) **Patent No.:** **US D822,211 S**
Davies et al. (45) **Date of Patent:** **** Jul. 3, 2018**

(54) **BLOOD GLUCOSE METER**
(71) Applicant: **Roche Diabetes Care, Inc.**,
Indianapolis, IN (US)
(72) Inventors: **Robert G. Davies**, Carmel, IN (US);
Sebastian Liedtke, Heidelberg (DE);
Dieter Loerwald, Hammah (DE);
Timothy L. Ranney, Lebanon, IN
(US); **Hendrik Edmund Steg**,
Wiswmar (DE)

D546,457 S 7/2007 Hannant et al.
D546,458 S 7/2007 Hannant
D611,853 S 3/2010 Salter et al.
D648,029 S * 11/2011 Presta D24/169
8,068,331 B2 11/2011 Sauers et al.
8,114,028 B2 2/2012 List et al.
D696,404 S 12/2013 Golnik et al.
D713,963 S 9/2014 Liedtke et al.
D723,404 S * 3/2015 Faulkner D10/78
2010/0113896 A1 5/2010 Cadio et al.
2010/0331650 A1 12/2010 Batman et al.
(Continued)

(73) Assignee: **Roche Diabetes Care, Inc.**,
Indianapolis, IN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/553,084**

(22) Filed: **Jan. 28, 2016**

Related U.S. Application Data

(62) Division of application No. 29/490,205, filed on May 7, 2014, now Pat. No. Des. 750,786.

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/169**

(58) **Field of Classification Search**
USPC D24/107, 147, 169, 186, 216, 223, 231;
D10/78, 81
CPC G01N 33/66; G01N 33/49; G01N 33/493;
A61B 5/14532; A61B 2560/0412; A61B
2560/0443; A61B 2560/0462
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D406,895 S 3/1999 Byrd et al.
D545,436 S 6/2007 Padain

OTHER PUBLICATIONS

Accu-Chek® Active Meter System, www.accu-chek.com/us/glucose-meters/active.html (printed therefrom on Apr. 15, 2014).

(Continued)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Harness Dickey


(57) **CLAIM**

The ornamental design for a blood glucose meter, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective of a blood glucose meter; FIG. 2 is a bottom perspective view of the blood glucose meter; FIG. 3 is a top view of the blood glucose meter; FIG. 4 is a bottom view of the blood glucose meter; FIG. 5 is an upper end view of the blood glucose meter; FIG. 6 is a lower end view of the blood glucose meter; FIG. 7 is a right side view of the blood glucose meter; and, FIG. 8 is a left side view of the blood glucose meter. The broken lines in the drawing views are included for the purpose of illustrating portions of the blood glucose meter that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

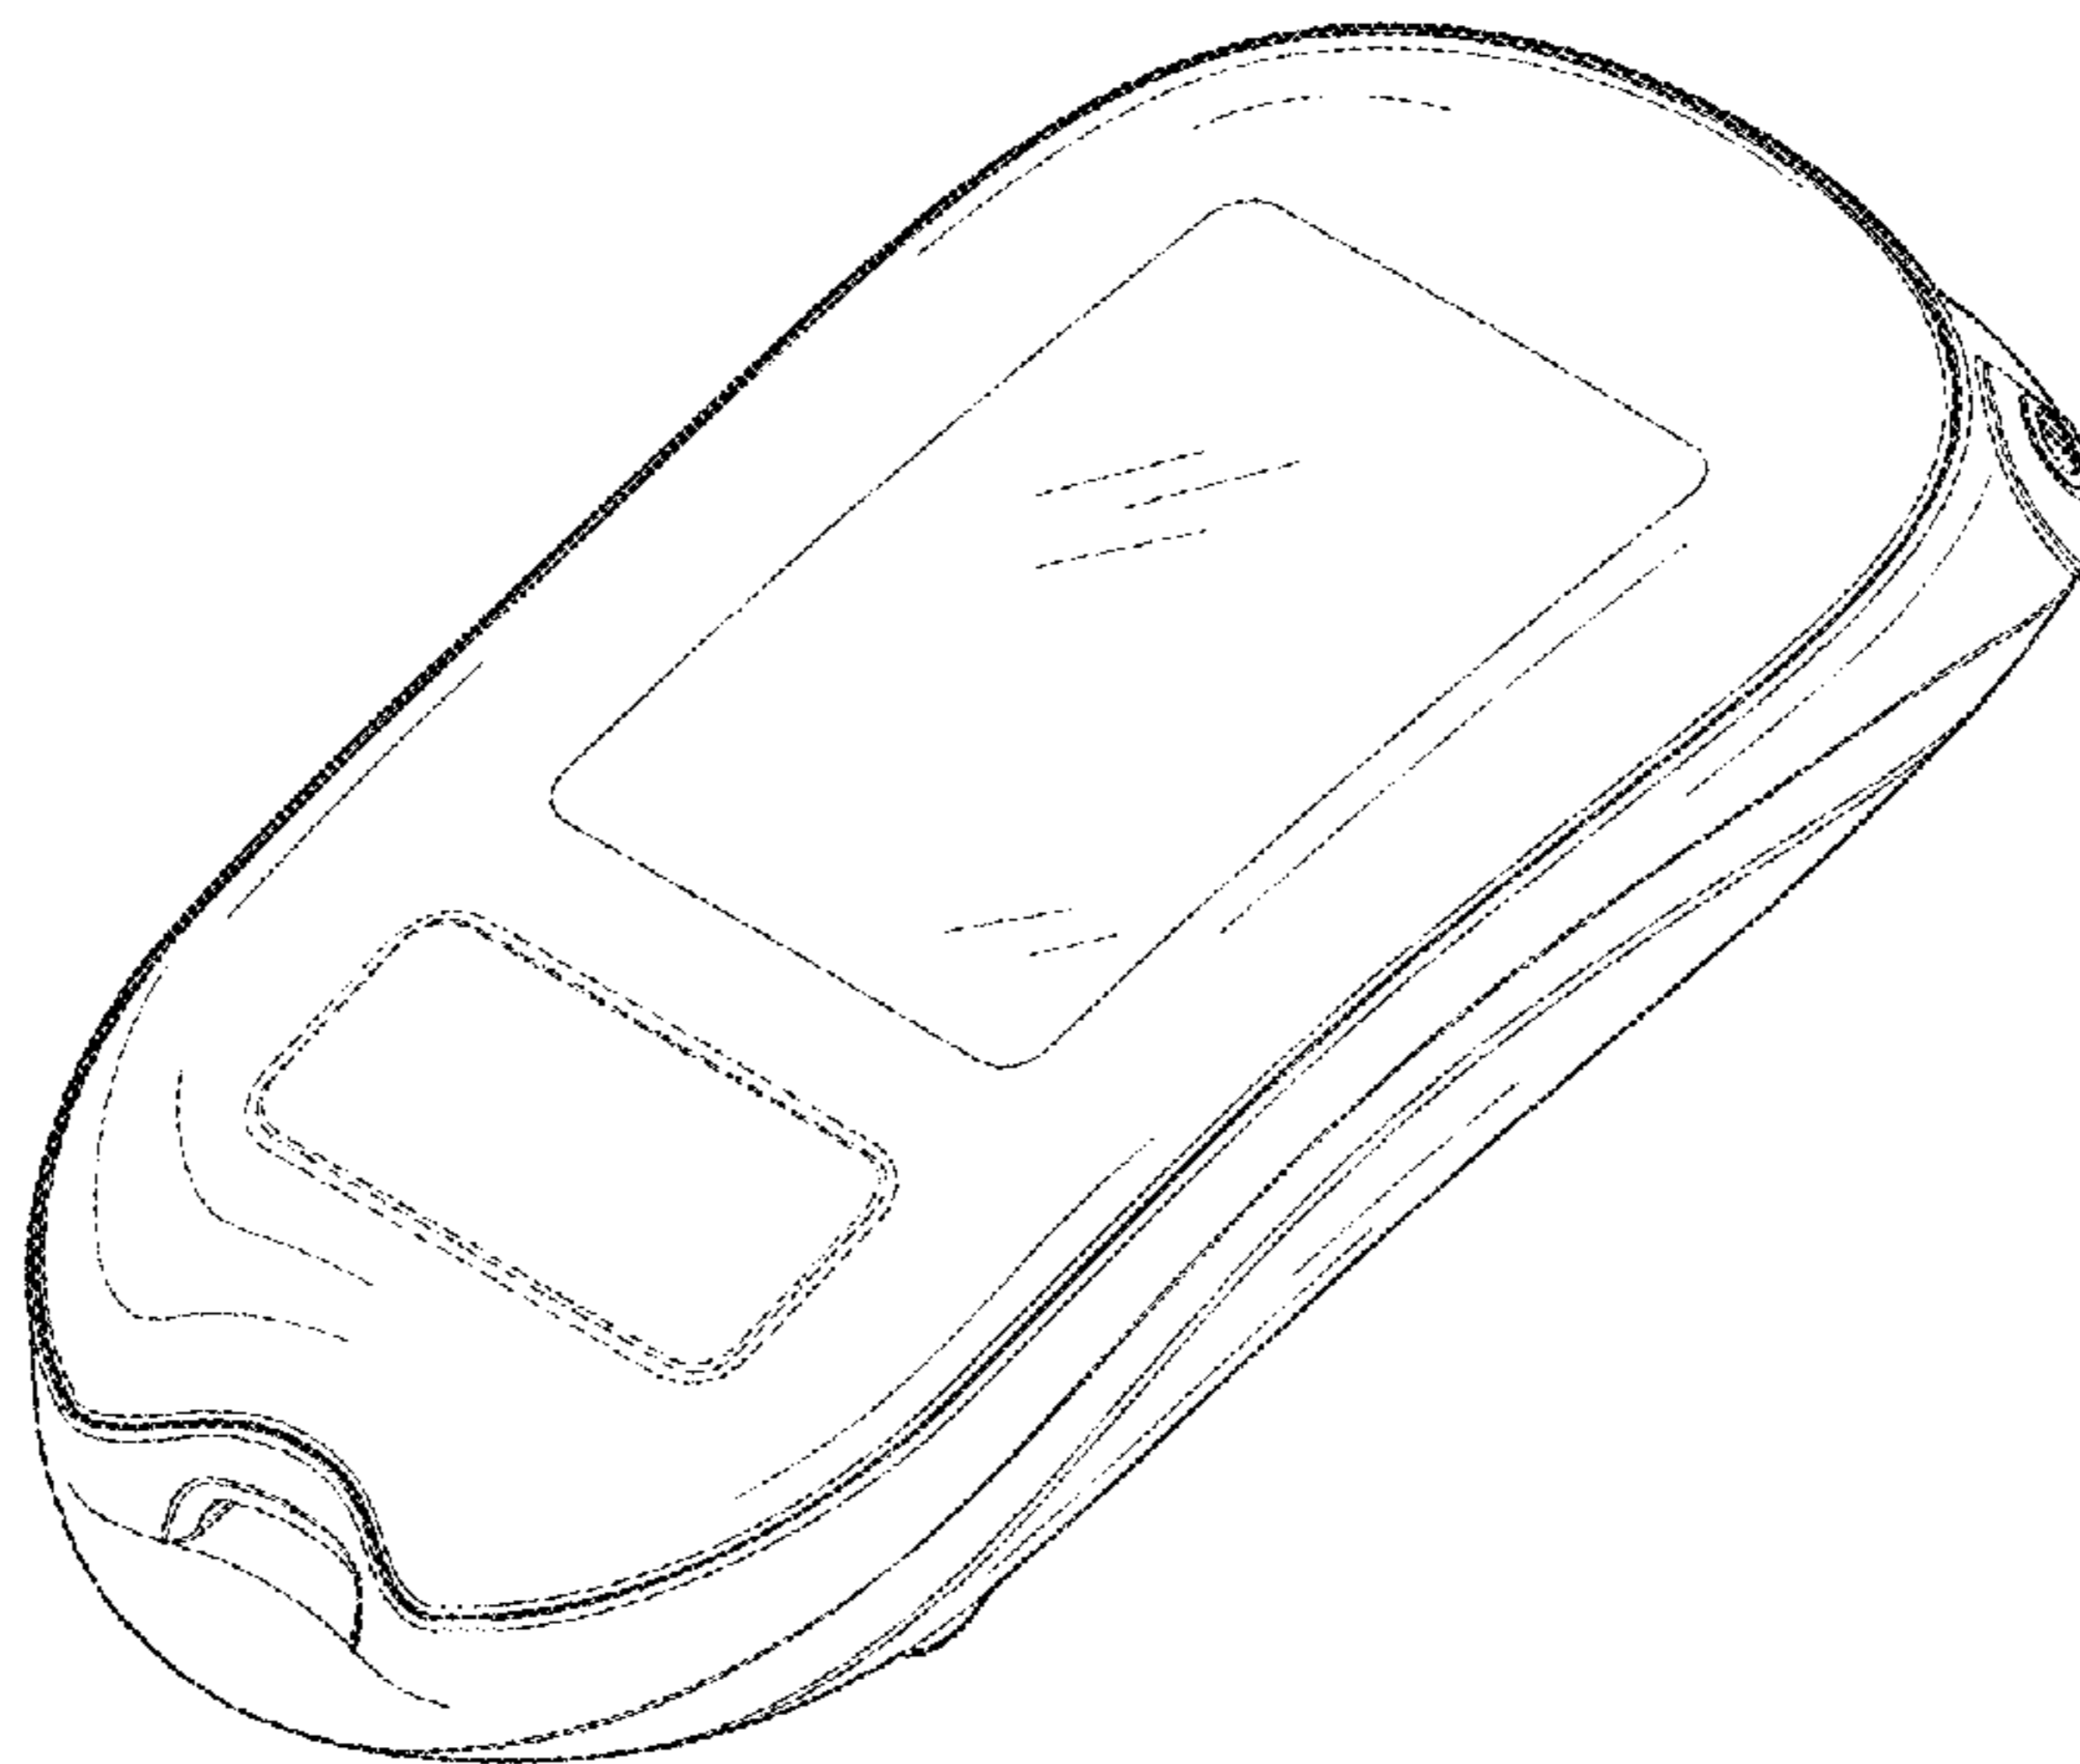

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0034786 A1 2/2011 Cadio et al.
2012/0221064 A1 8/2012 Wooldridge

OTHER PUBLICATIONS

Accu-Chek® Advantage Meter System, www.accu-chek.com/us/glucose-meters/advantage.html (printed therefrom on Apr. 15, 2014).

Accu-Chek® Aviva Plus System, www.accu-chek.com/us/glucose-meters/aviva.html (printed therefrom on Apr. 15, 2014).

Accu-Chek® Compact Plus Meter System, www.accu-chek.com/us/glucose-meters/compact-plus.html (printed therefrom on Apr. 15, 2014).

Accu-Chek® Nano Meter, www.accu-chek.com/us/glucose-meters/nano.html (printed therefrom on Apr. 15, 2014).

* cited by examiner

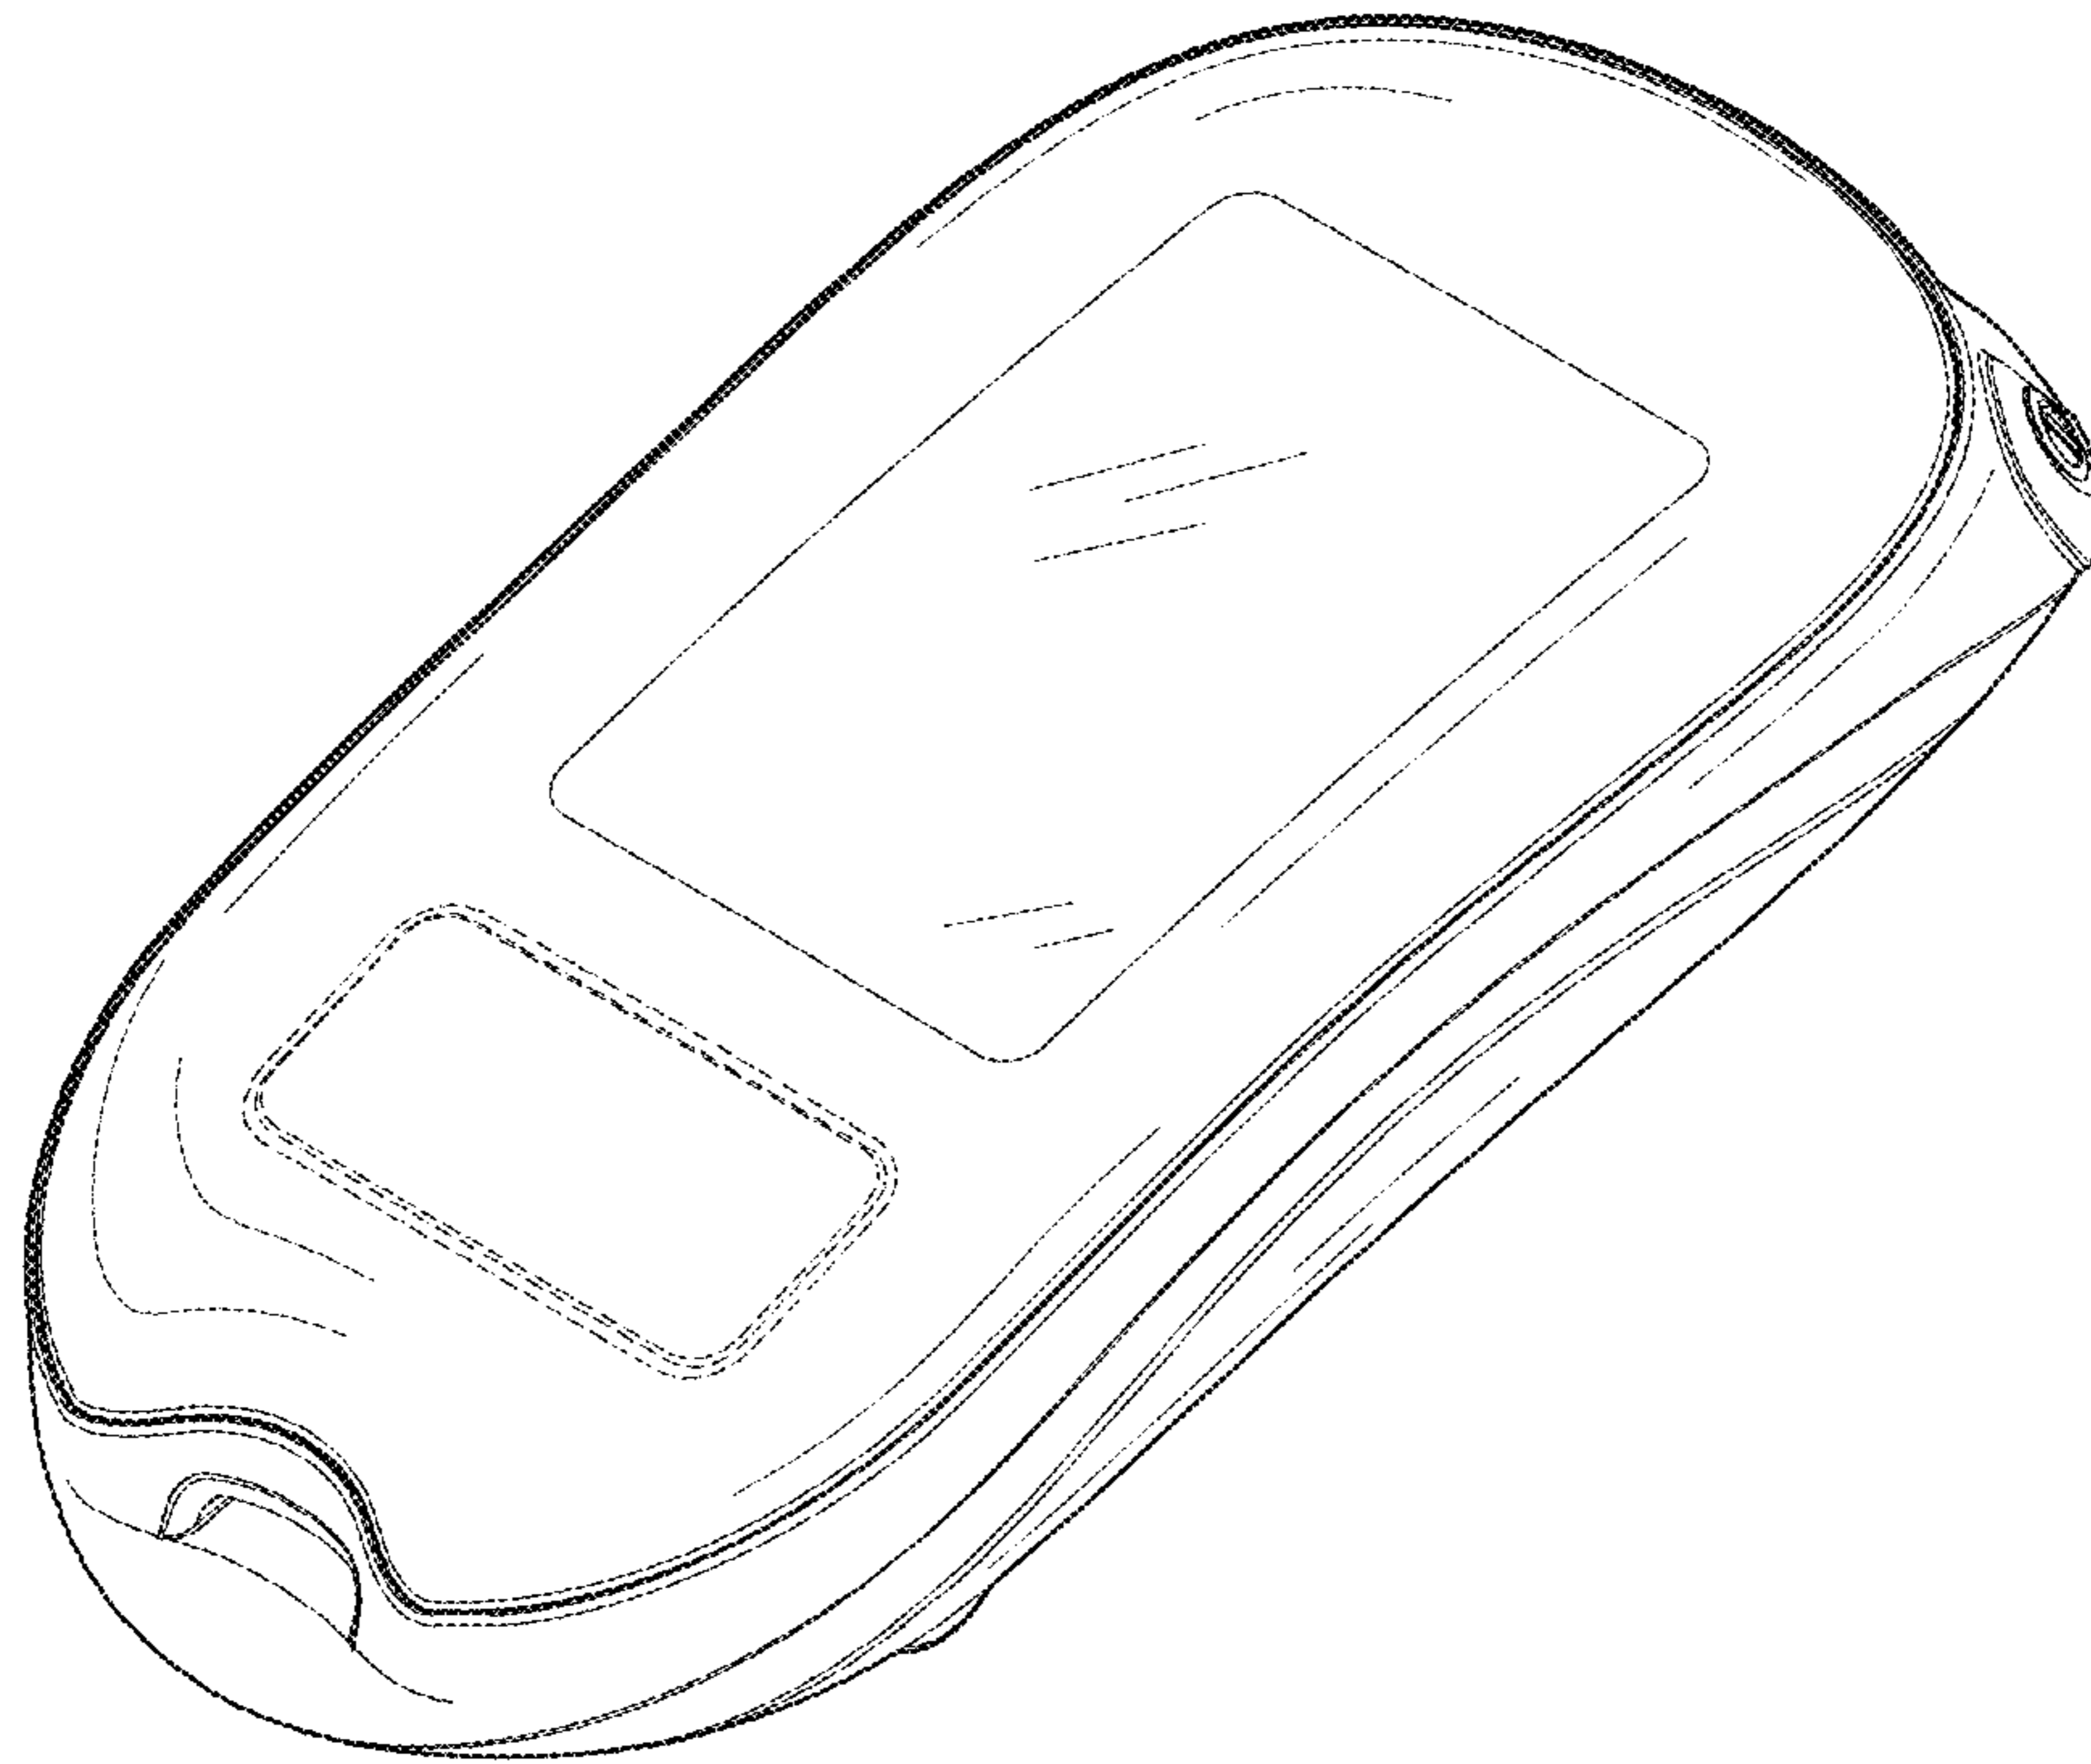


Fig. 1

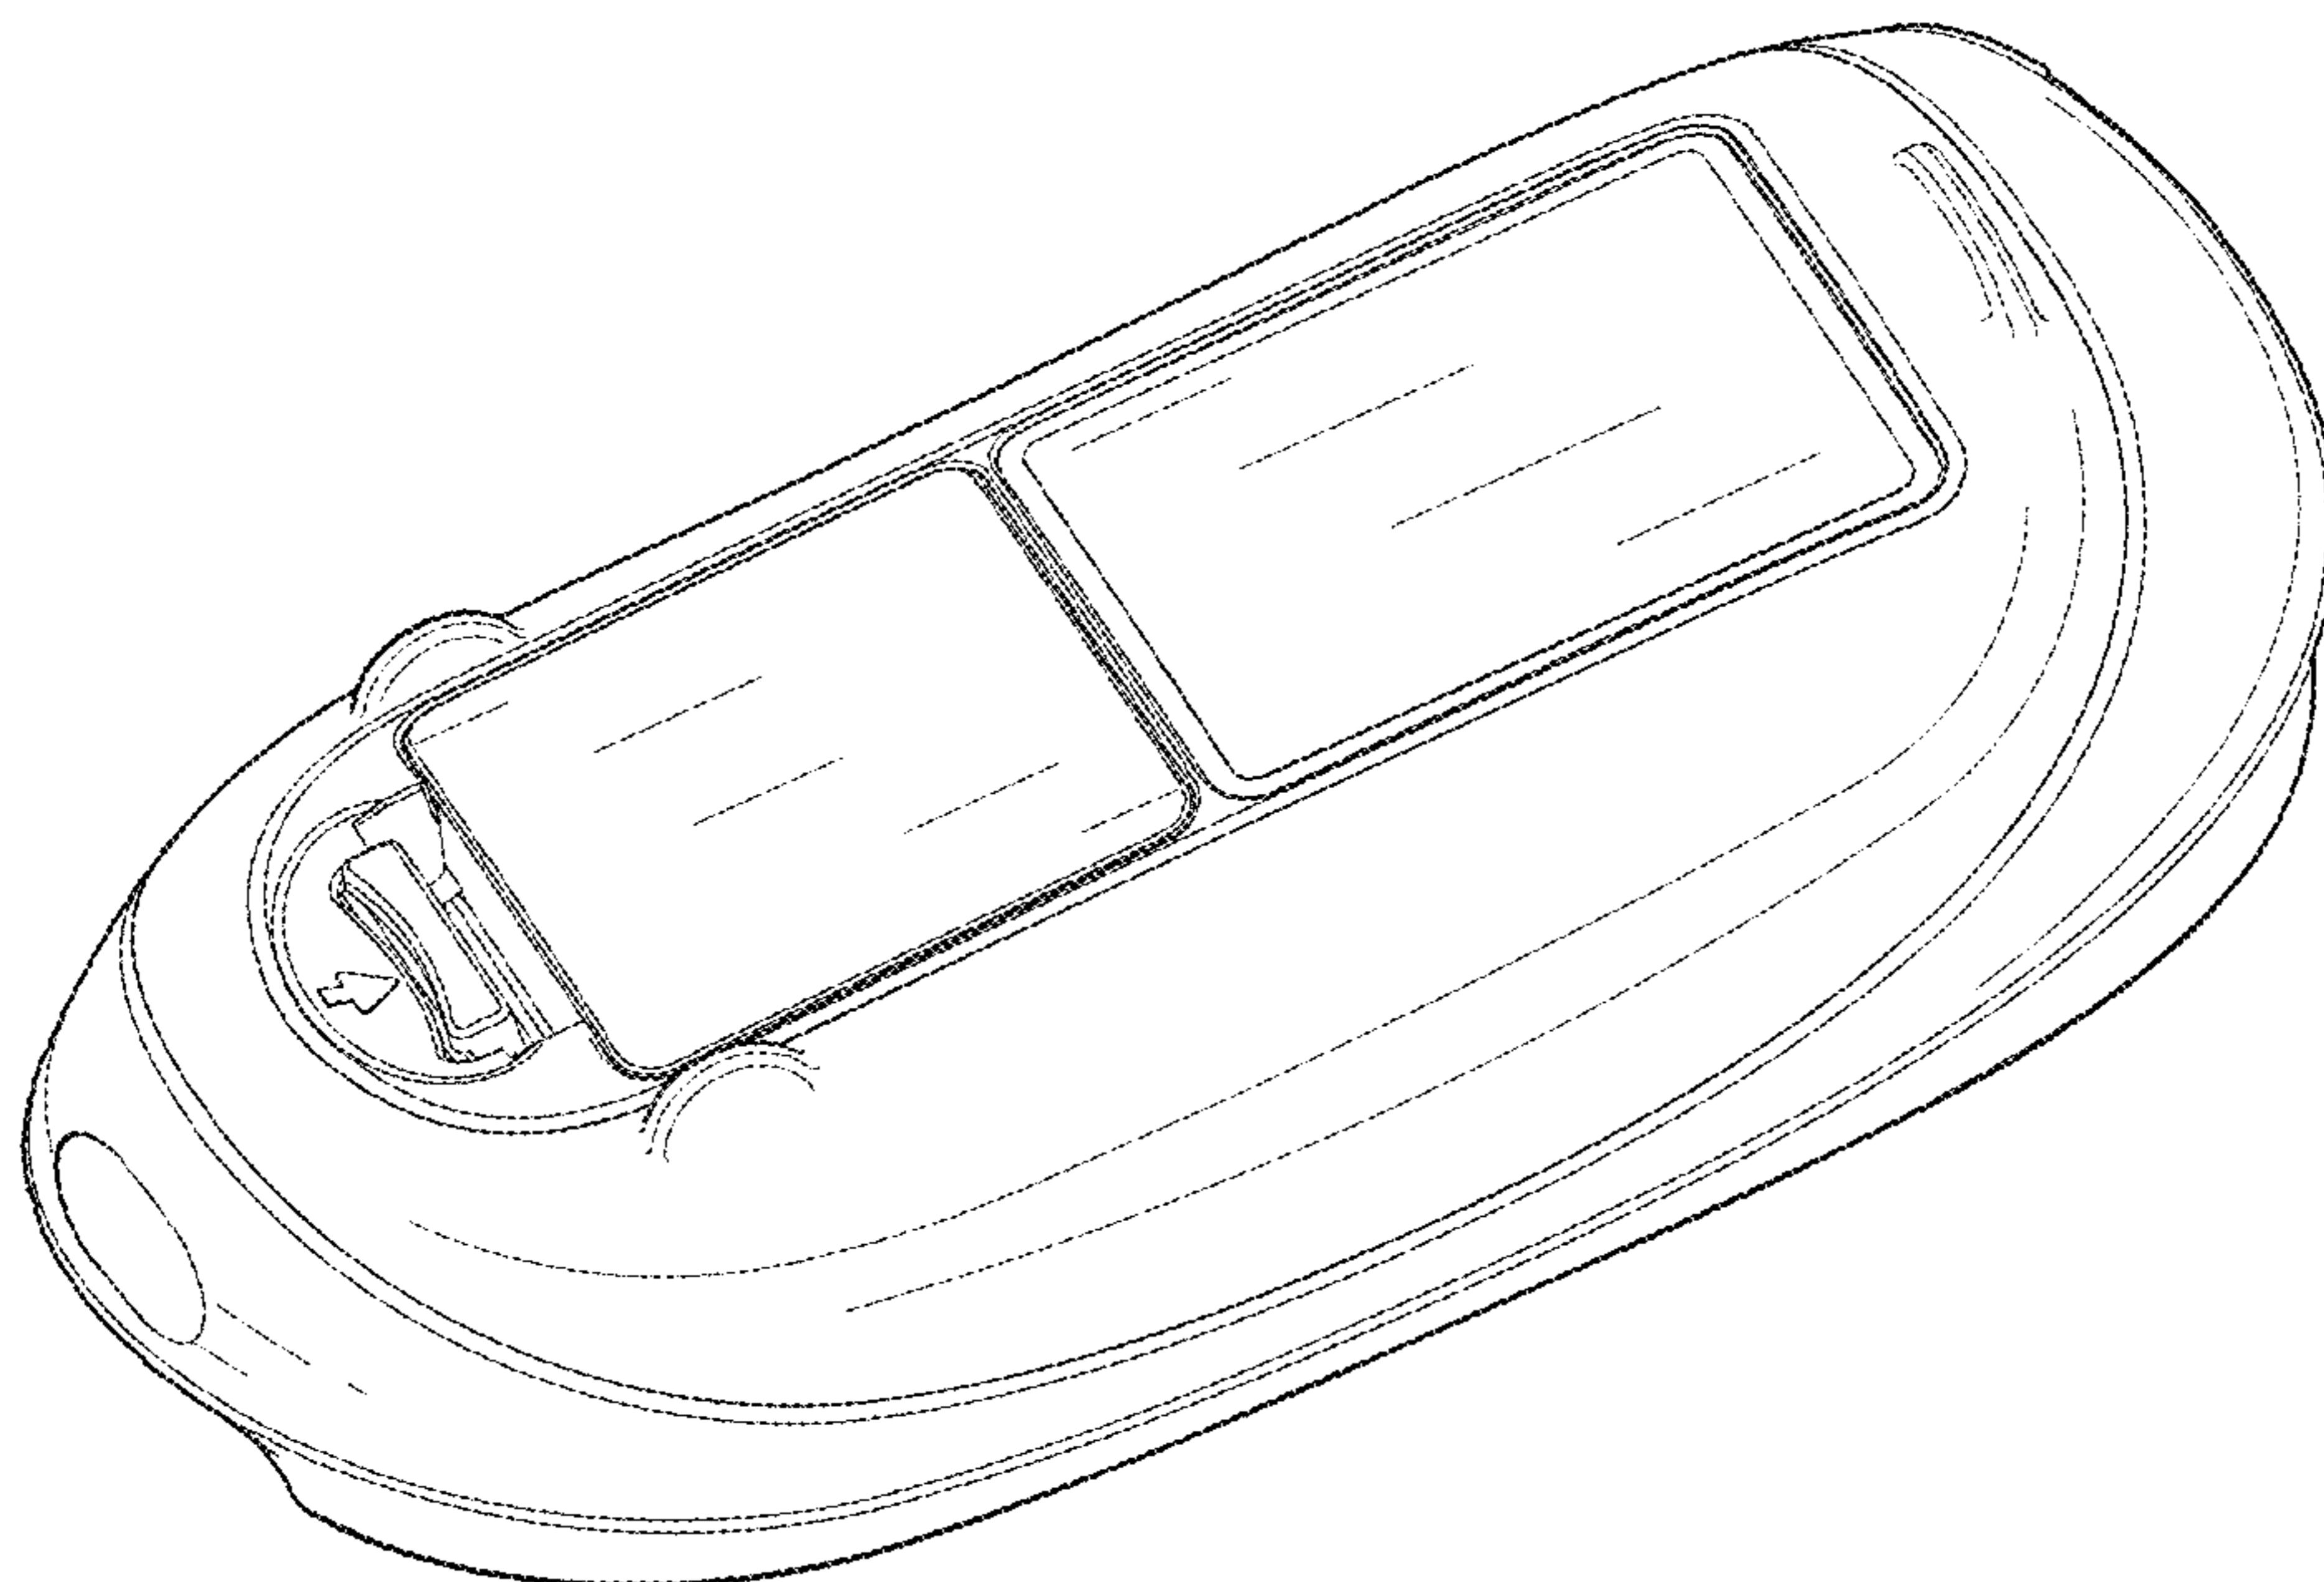


Fig. 2

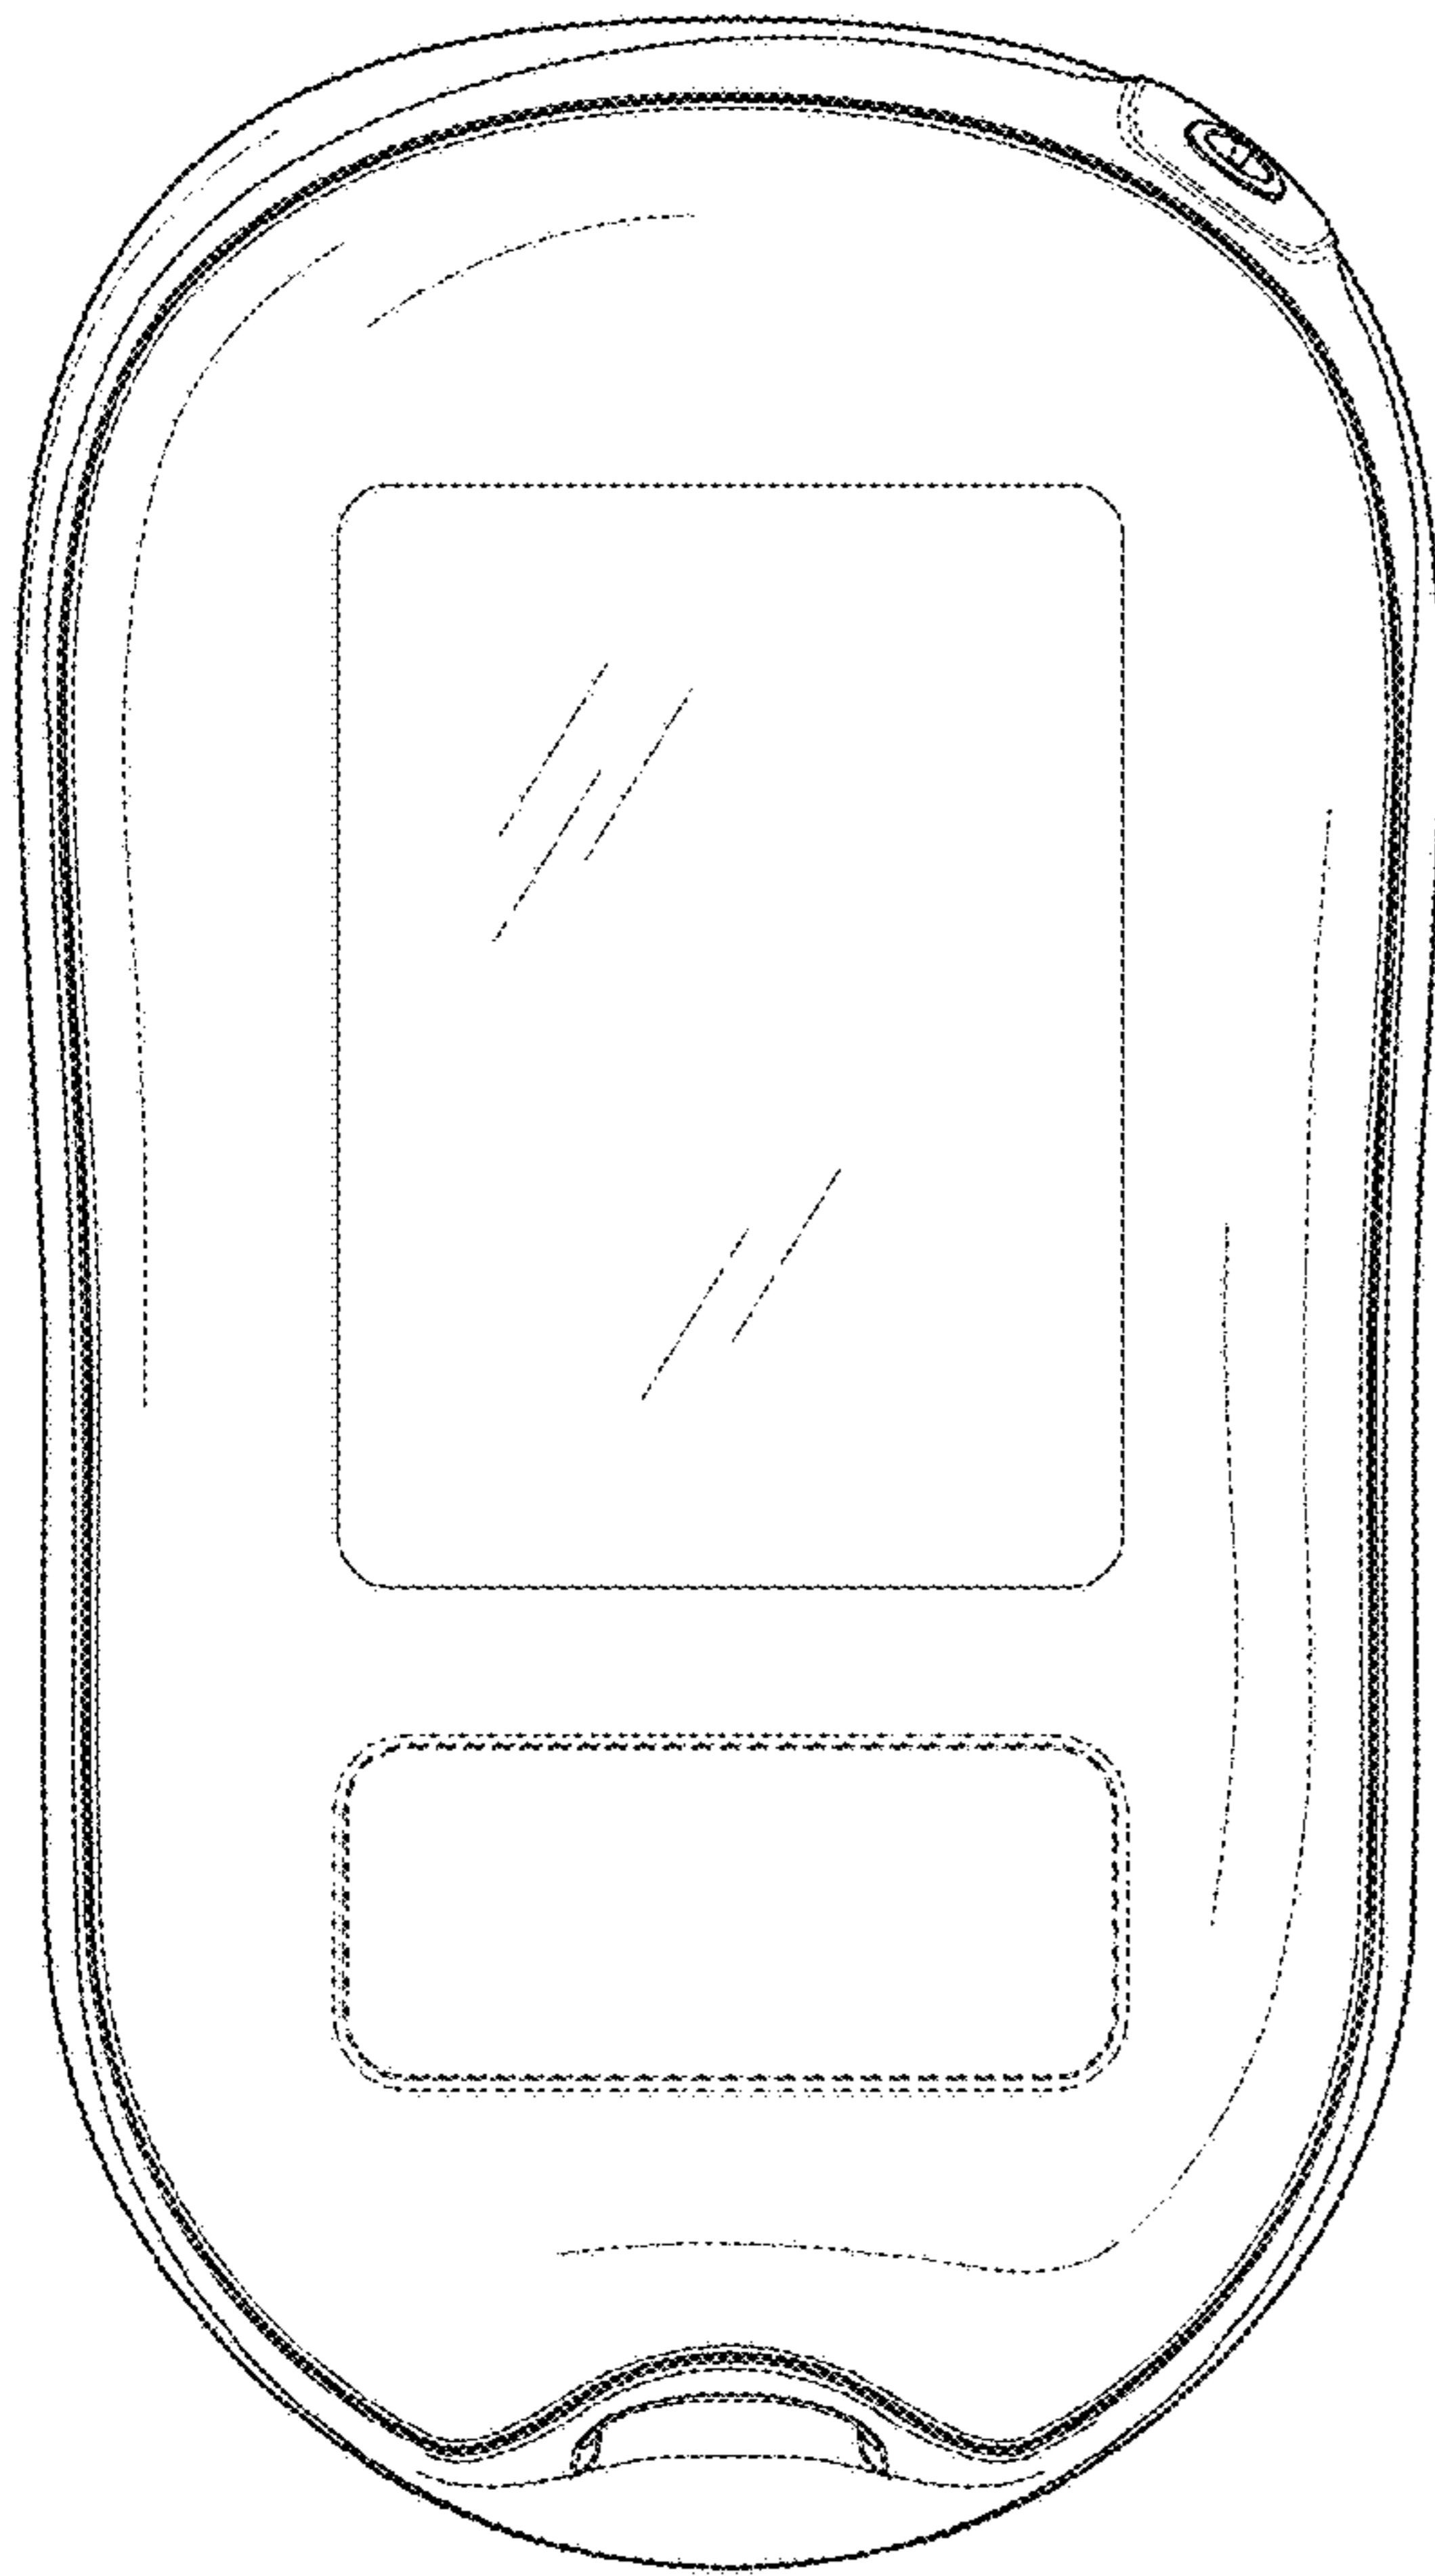


Fig. 3

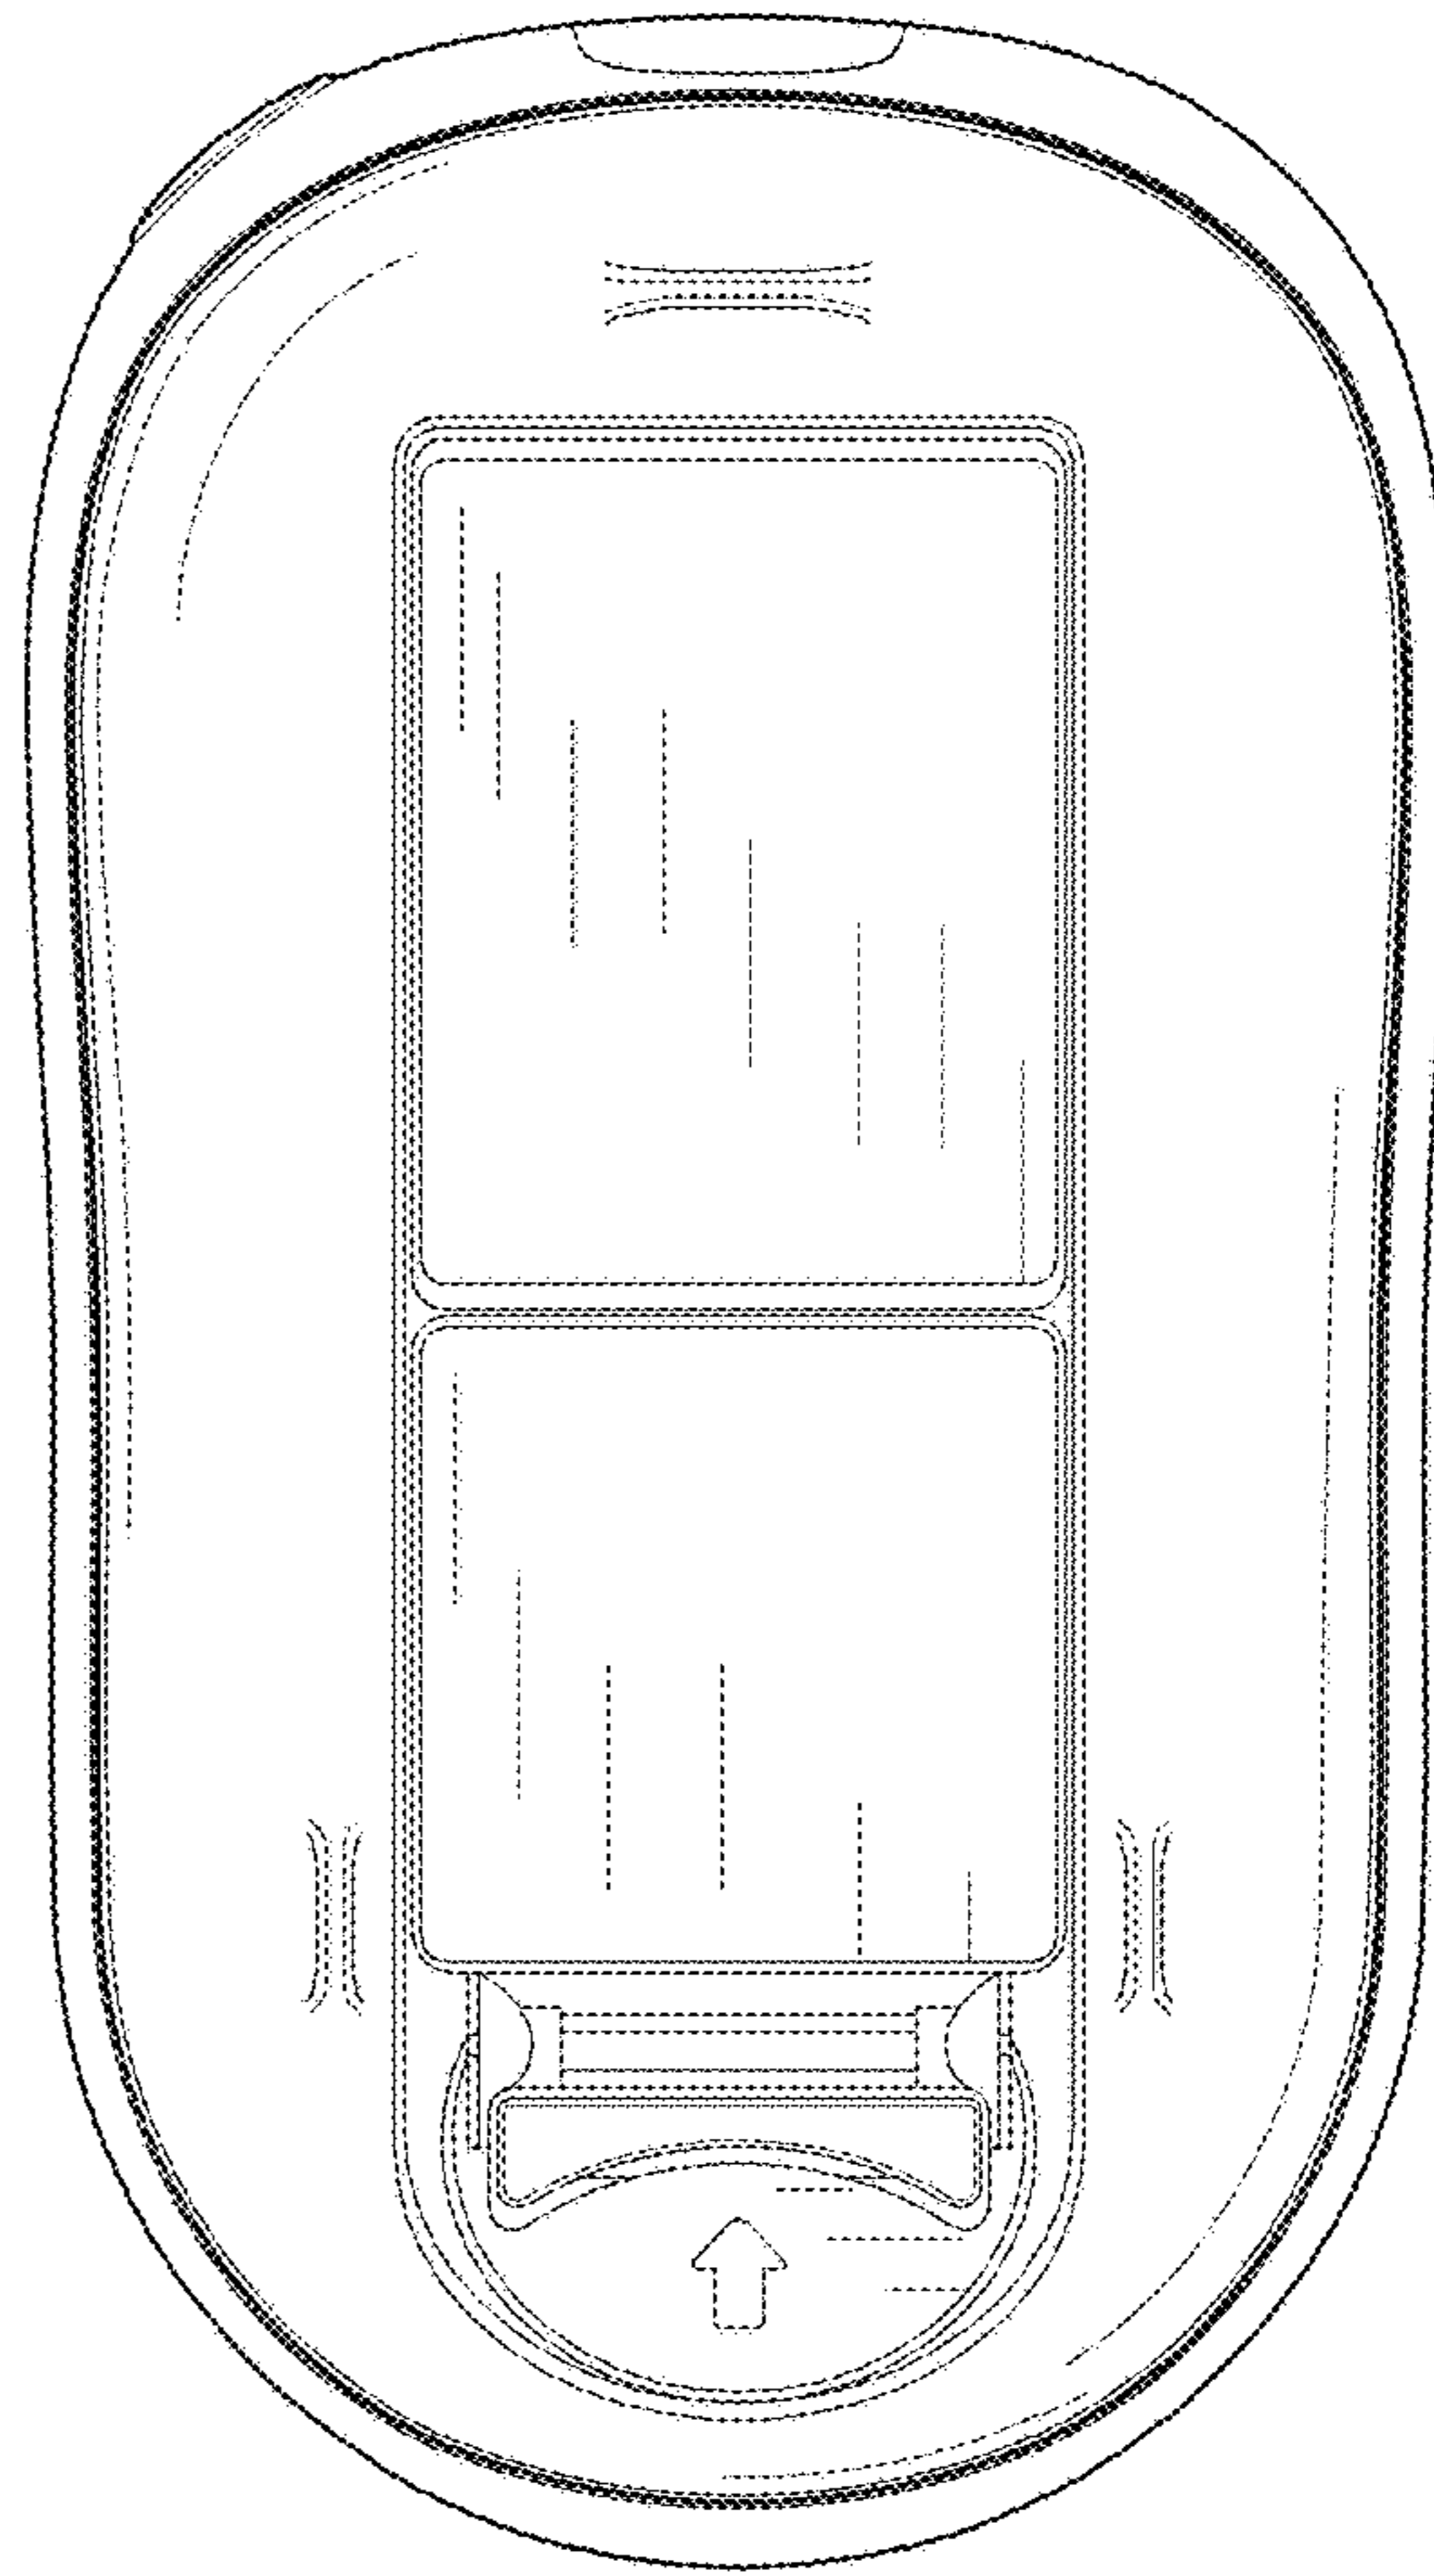


Fig. 4

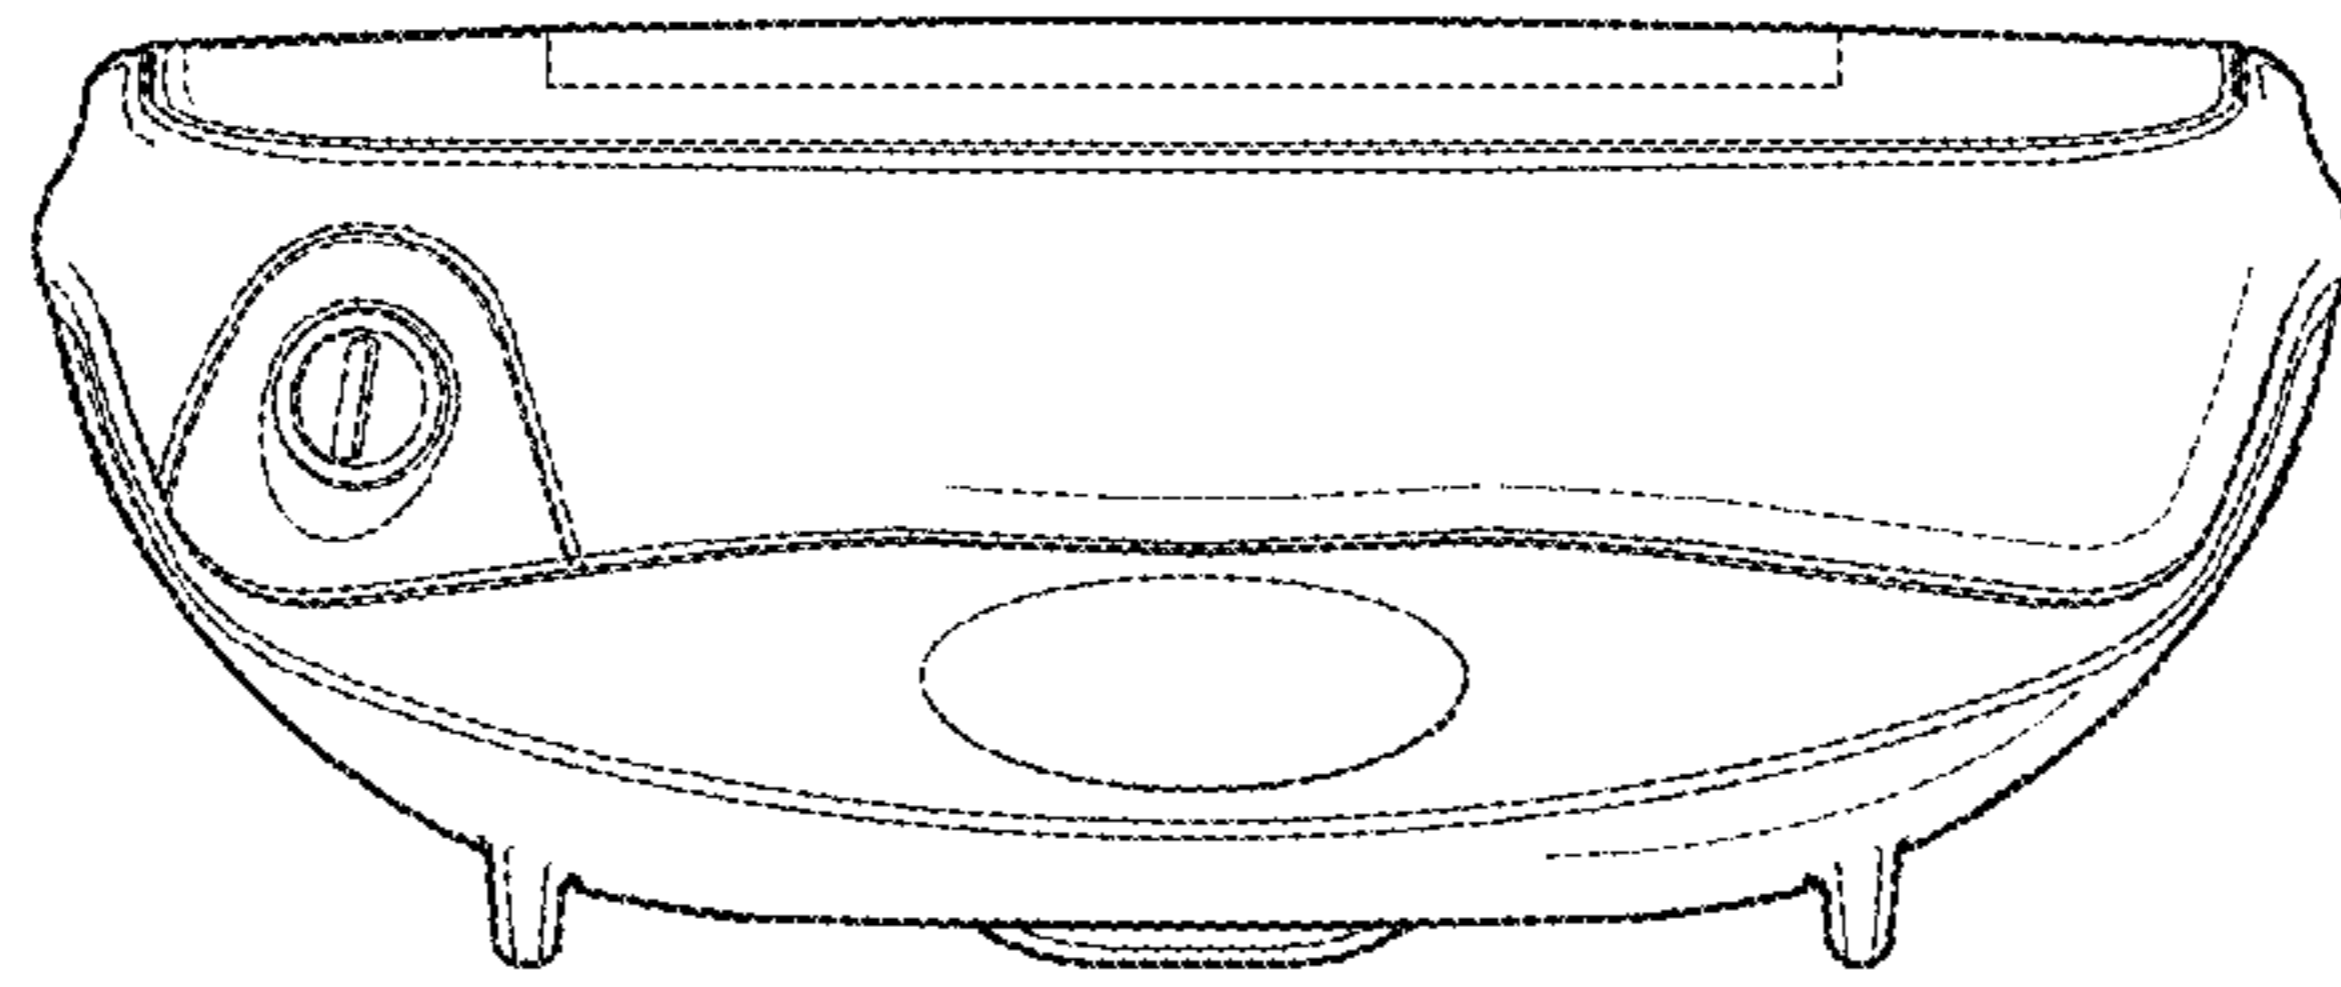


Fig.5

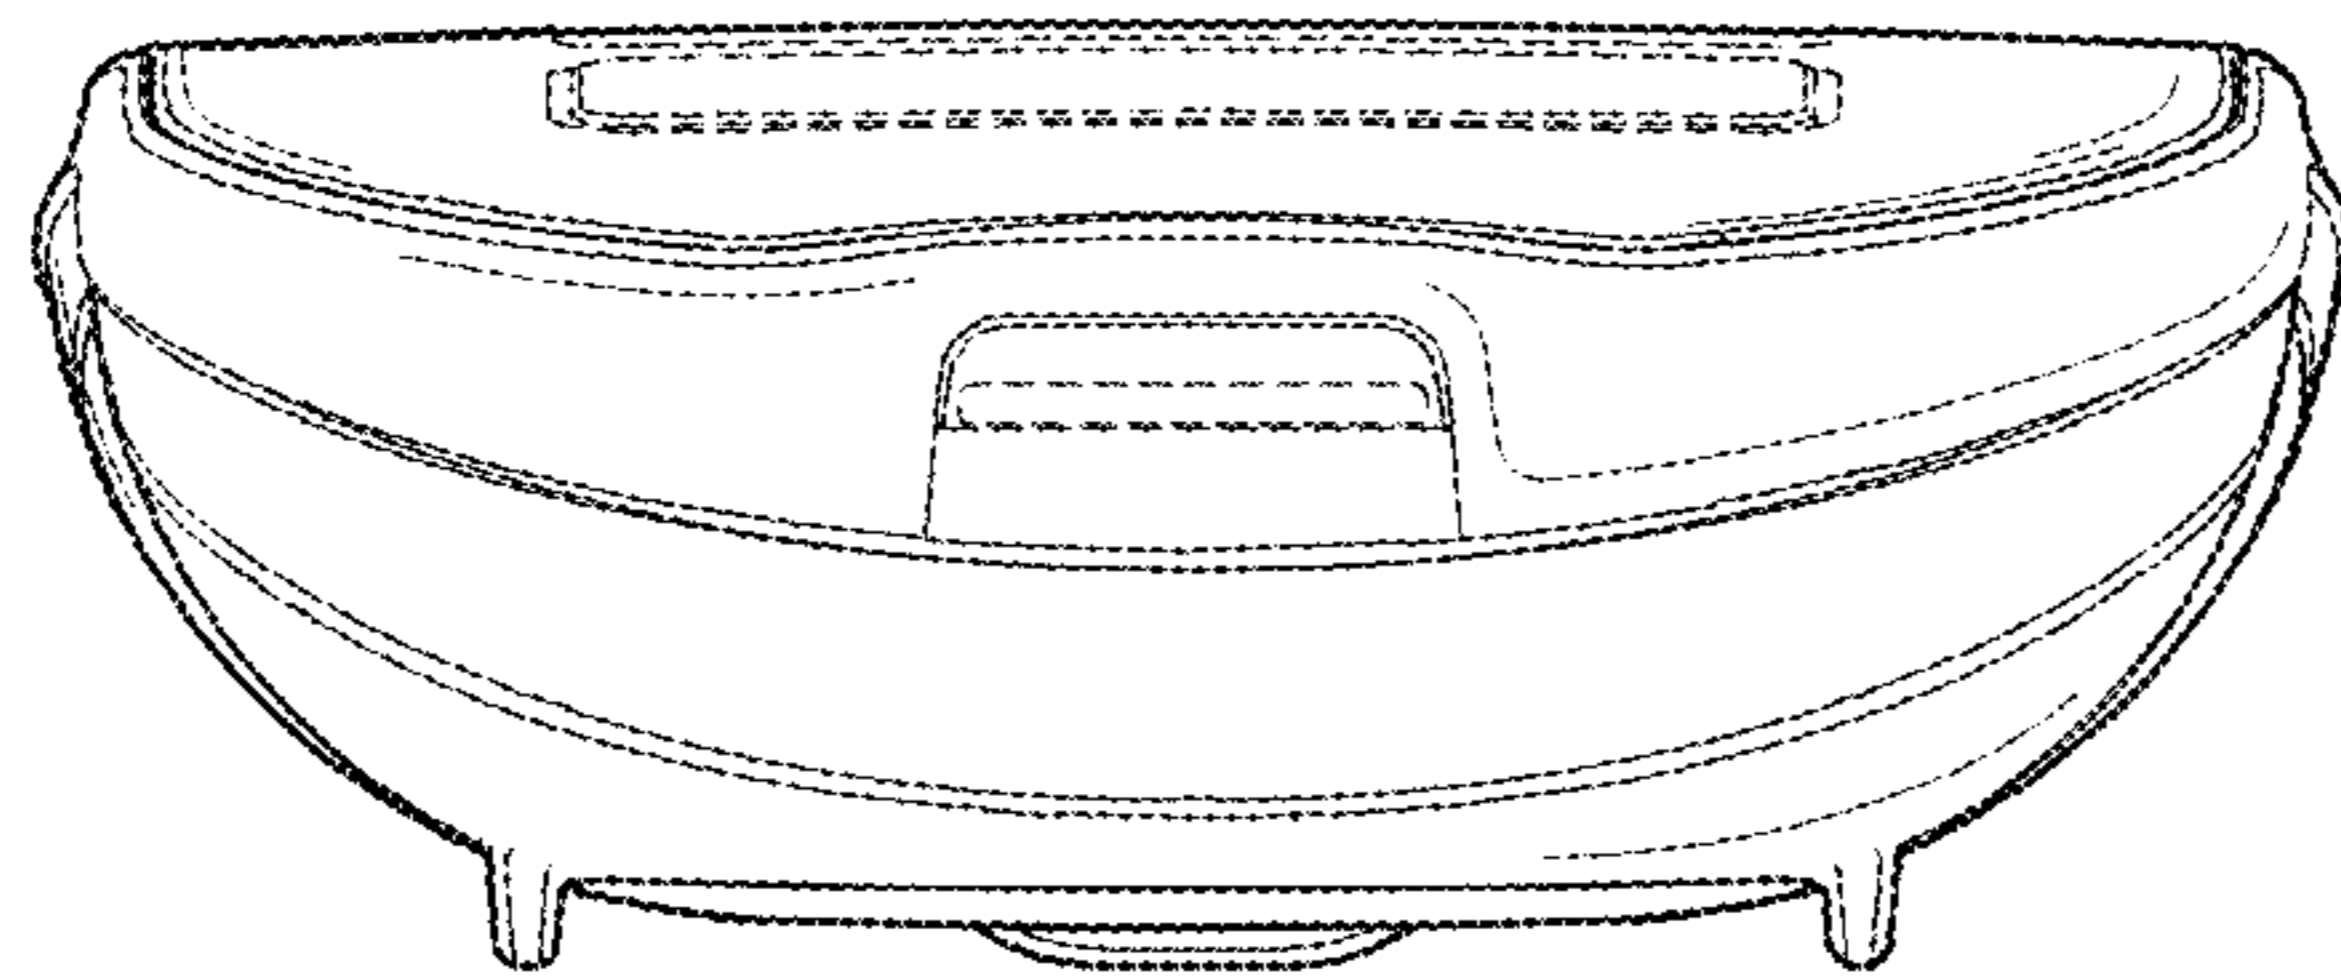


Fig.6

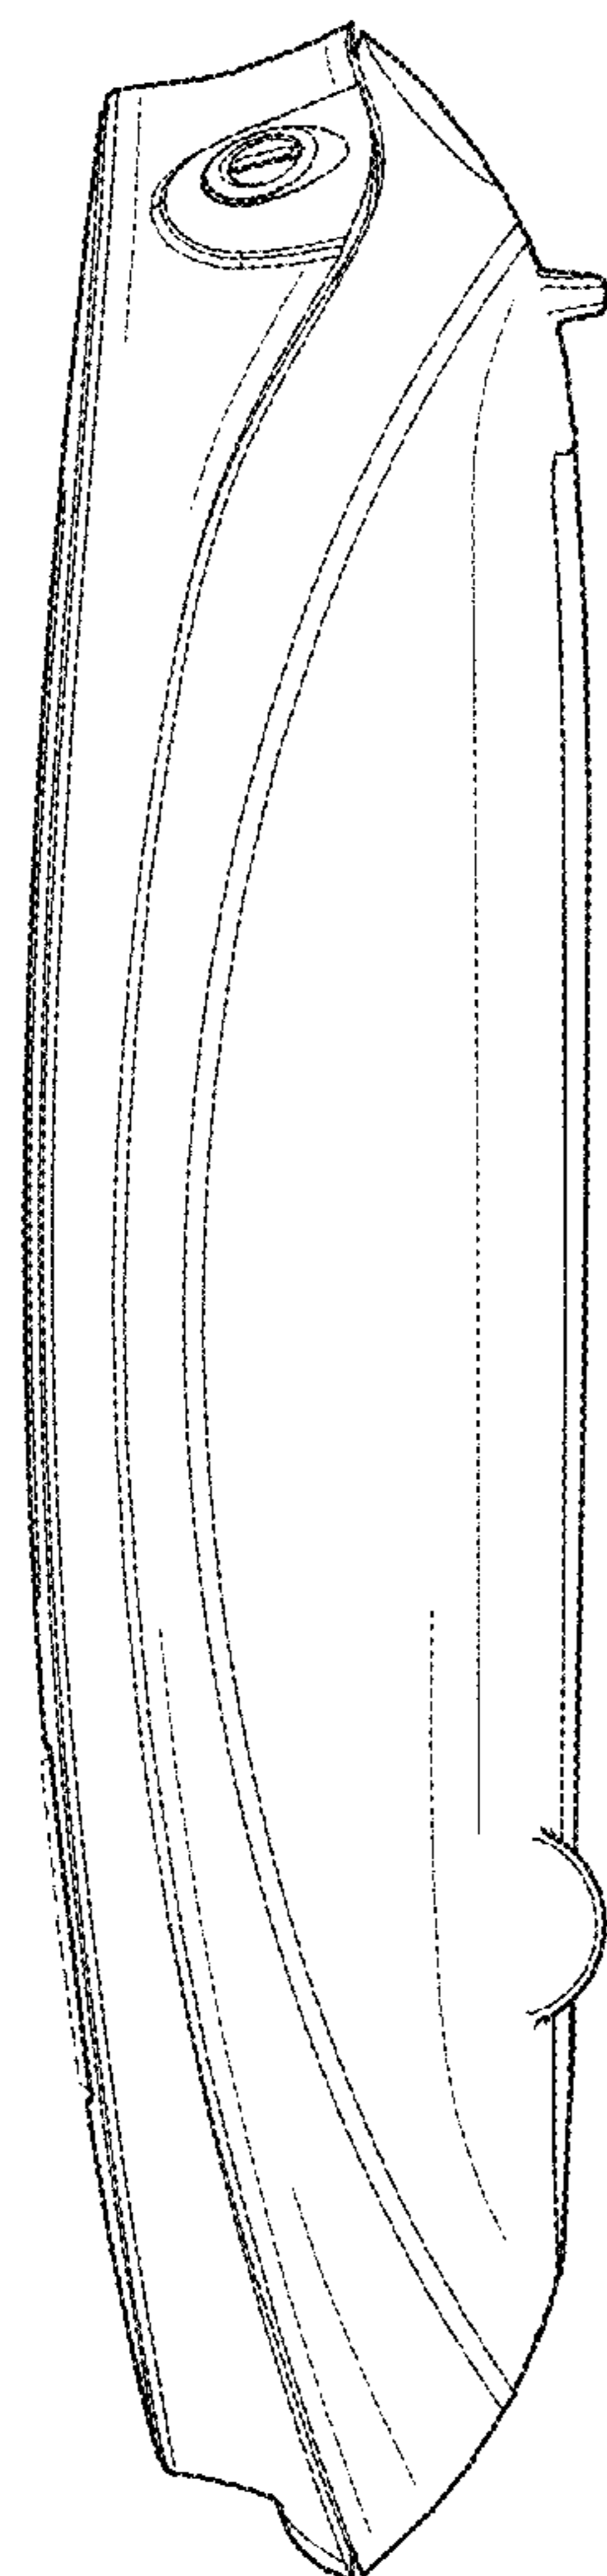


Fig. 7

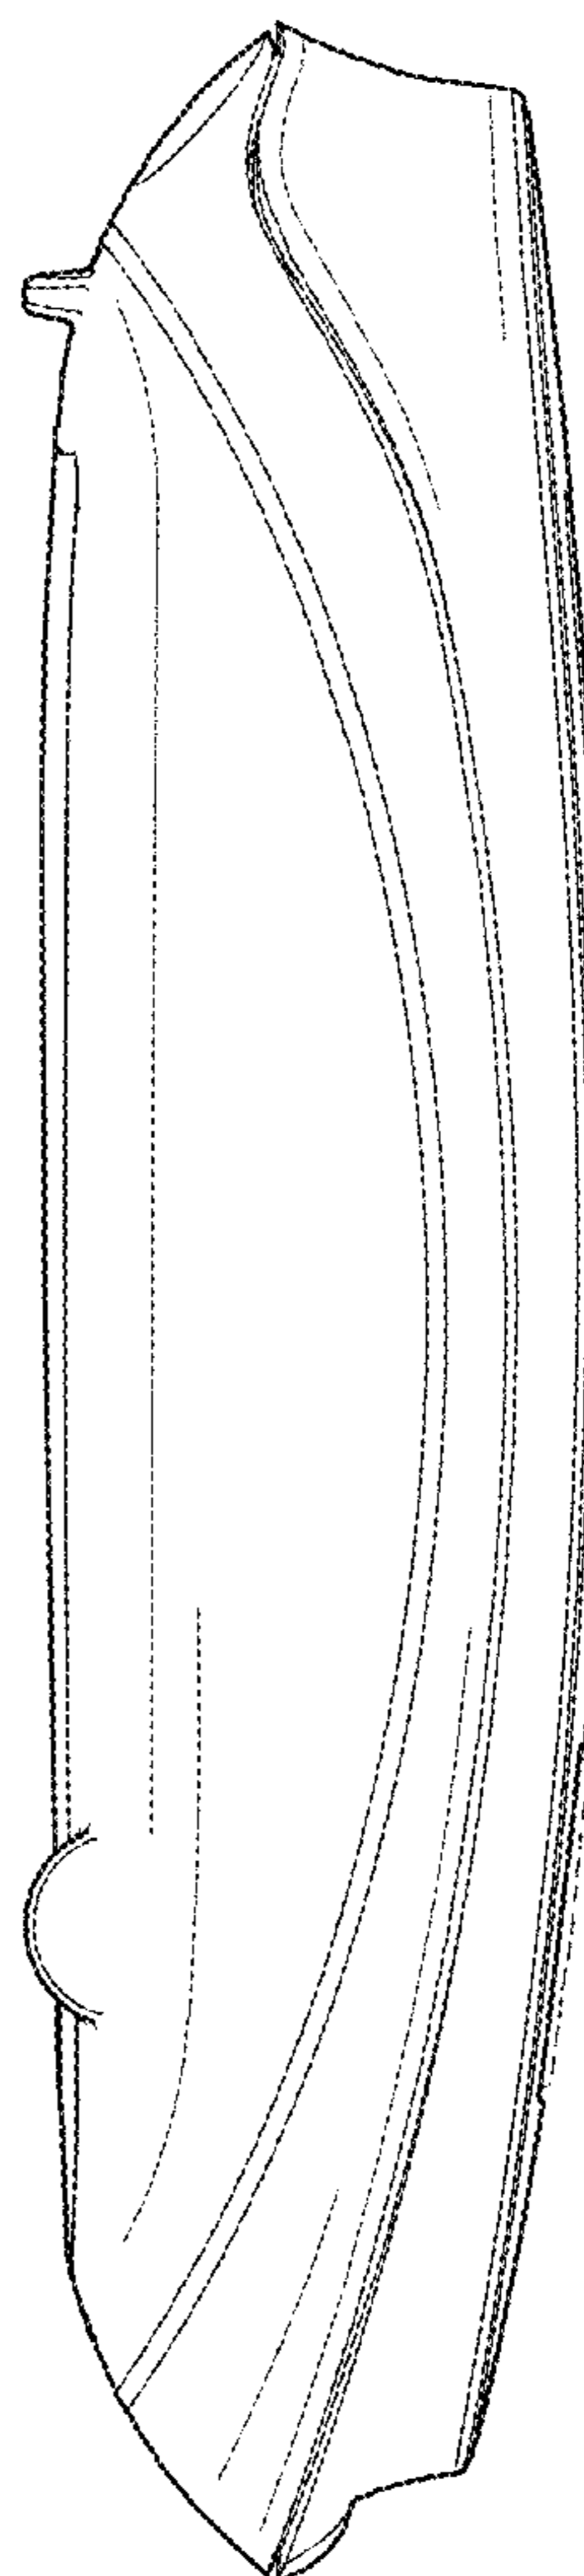


Fig. 8