



US00D822218S

(12) **United States Design Patent** (10) **Patent No.:** **US D822,218 S**
Asai et al. (45) **Date of Patent:** **** Jul. 3, 2018**

(54) **MEDICAL PROBE**

(71) Applicant: **KONICA MINOLTA, INC.**,
Chiyoda-ku, Tokyo (JP)

(72) Inventors: **Tomonari Asai**, Hachioji (JP);
Kenichiro Uchihara, Nagareyama (JP)

(73) Assignee: **Konica Minolta, Inc.**, Chiyoda-ku,
Tokyo (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/597,565**

(22) Filed: **Mar. 17, 2017**

(30) **Foreign Application Priority Data**

Oct. 18, 2016 (JP) D2016-022642

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**

USPC D24/107, 133, 137, 138, 141, 158–161,
D24/164, 165, 167, 170, 185–187;
D10/57, 60, 78, 80; 600/407, 439, 446,
600/459, 461; 378/98.7, 98.8, 189
CPC ... A61B 8/0437; A61B 8/0883; A61B 8/4405;
A61B 8/4411; A61B 8/4427; A61B
8/445; A61B 8/4455; A61B 8/4461; A61B
8/4483; A61B 8/46; A61B 8/462; A61B
5/0095

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D616,992 S * 6/2010 Kitayama D24/186
D697,627 S * 1/2014 Takano D24/187

D701,606 S * 3/2014 Ohmukai D24/187
D703,333 S * 4/2014 Saeki D24/187
D728,802 S * 5/2015 Matsumura D24/187
D748,808 S * 2/2016 Matsumura D24/187
2011/0251491 A1* 10/2011 Oonuki A61B 8/0841
600/461

FOREIGN PATENT DOCUMENTS

JP D1514542 1/2015

* cited by examiner

Primary Examiner — Anhdao Doan

Assistant Examiner — Mary Malley

(74) *Attorney, Agent, or Firm* — Buchanan Ingersoll &
Rooney PC


(57) **CLAIM**

The ornamental design for a medical probe, as shown and
described.

DESCRIPTION

FIG. 1 is a first perspective view of a medical probe;
FIG. 2 is a second perspective view thereof;
FIG. 3 is a front view thereof, the opposite side being a
mirror image of the side shown herein;
FIG. 4 is a left side view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a top view thereof;
FIG. 7 is a bottom view thereof; and,
FIG. 8 is a cross-sectional view taken along line 8-8 in FIG.
7 in which the internal mechanism is omitted thereof.
The broken lines show portions of the medical probe that
form no part of the claimed design.

1 Claim, 5 Drawing Sheets

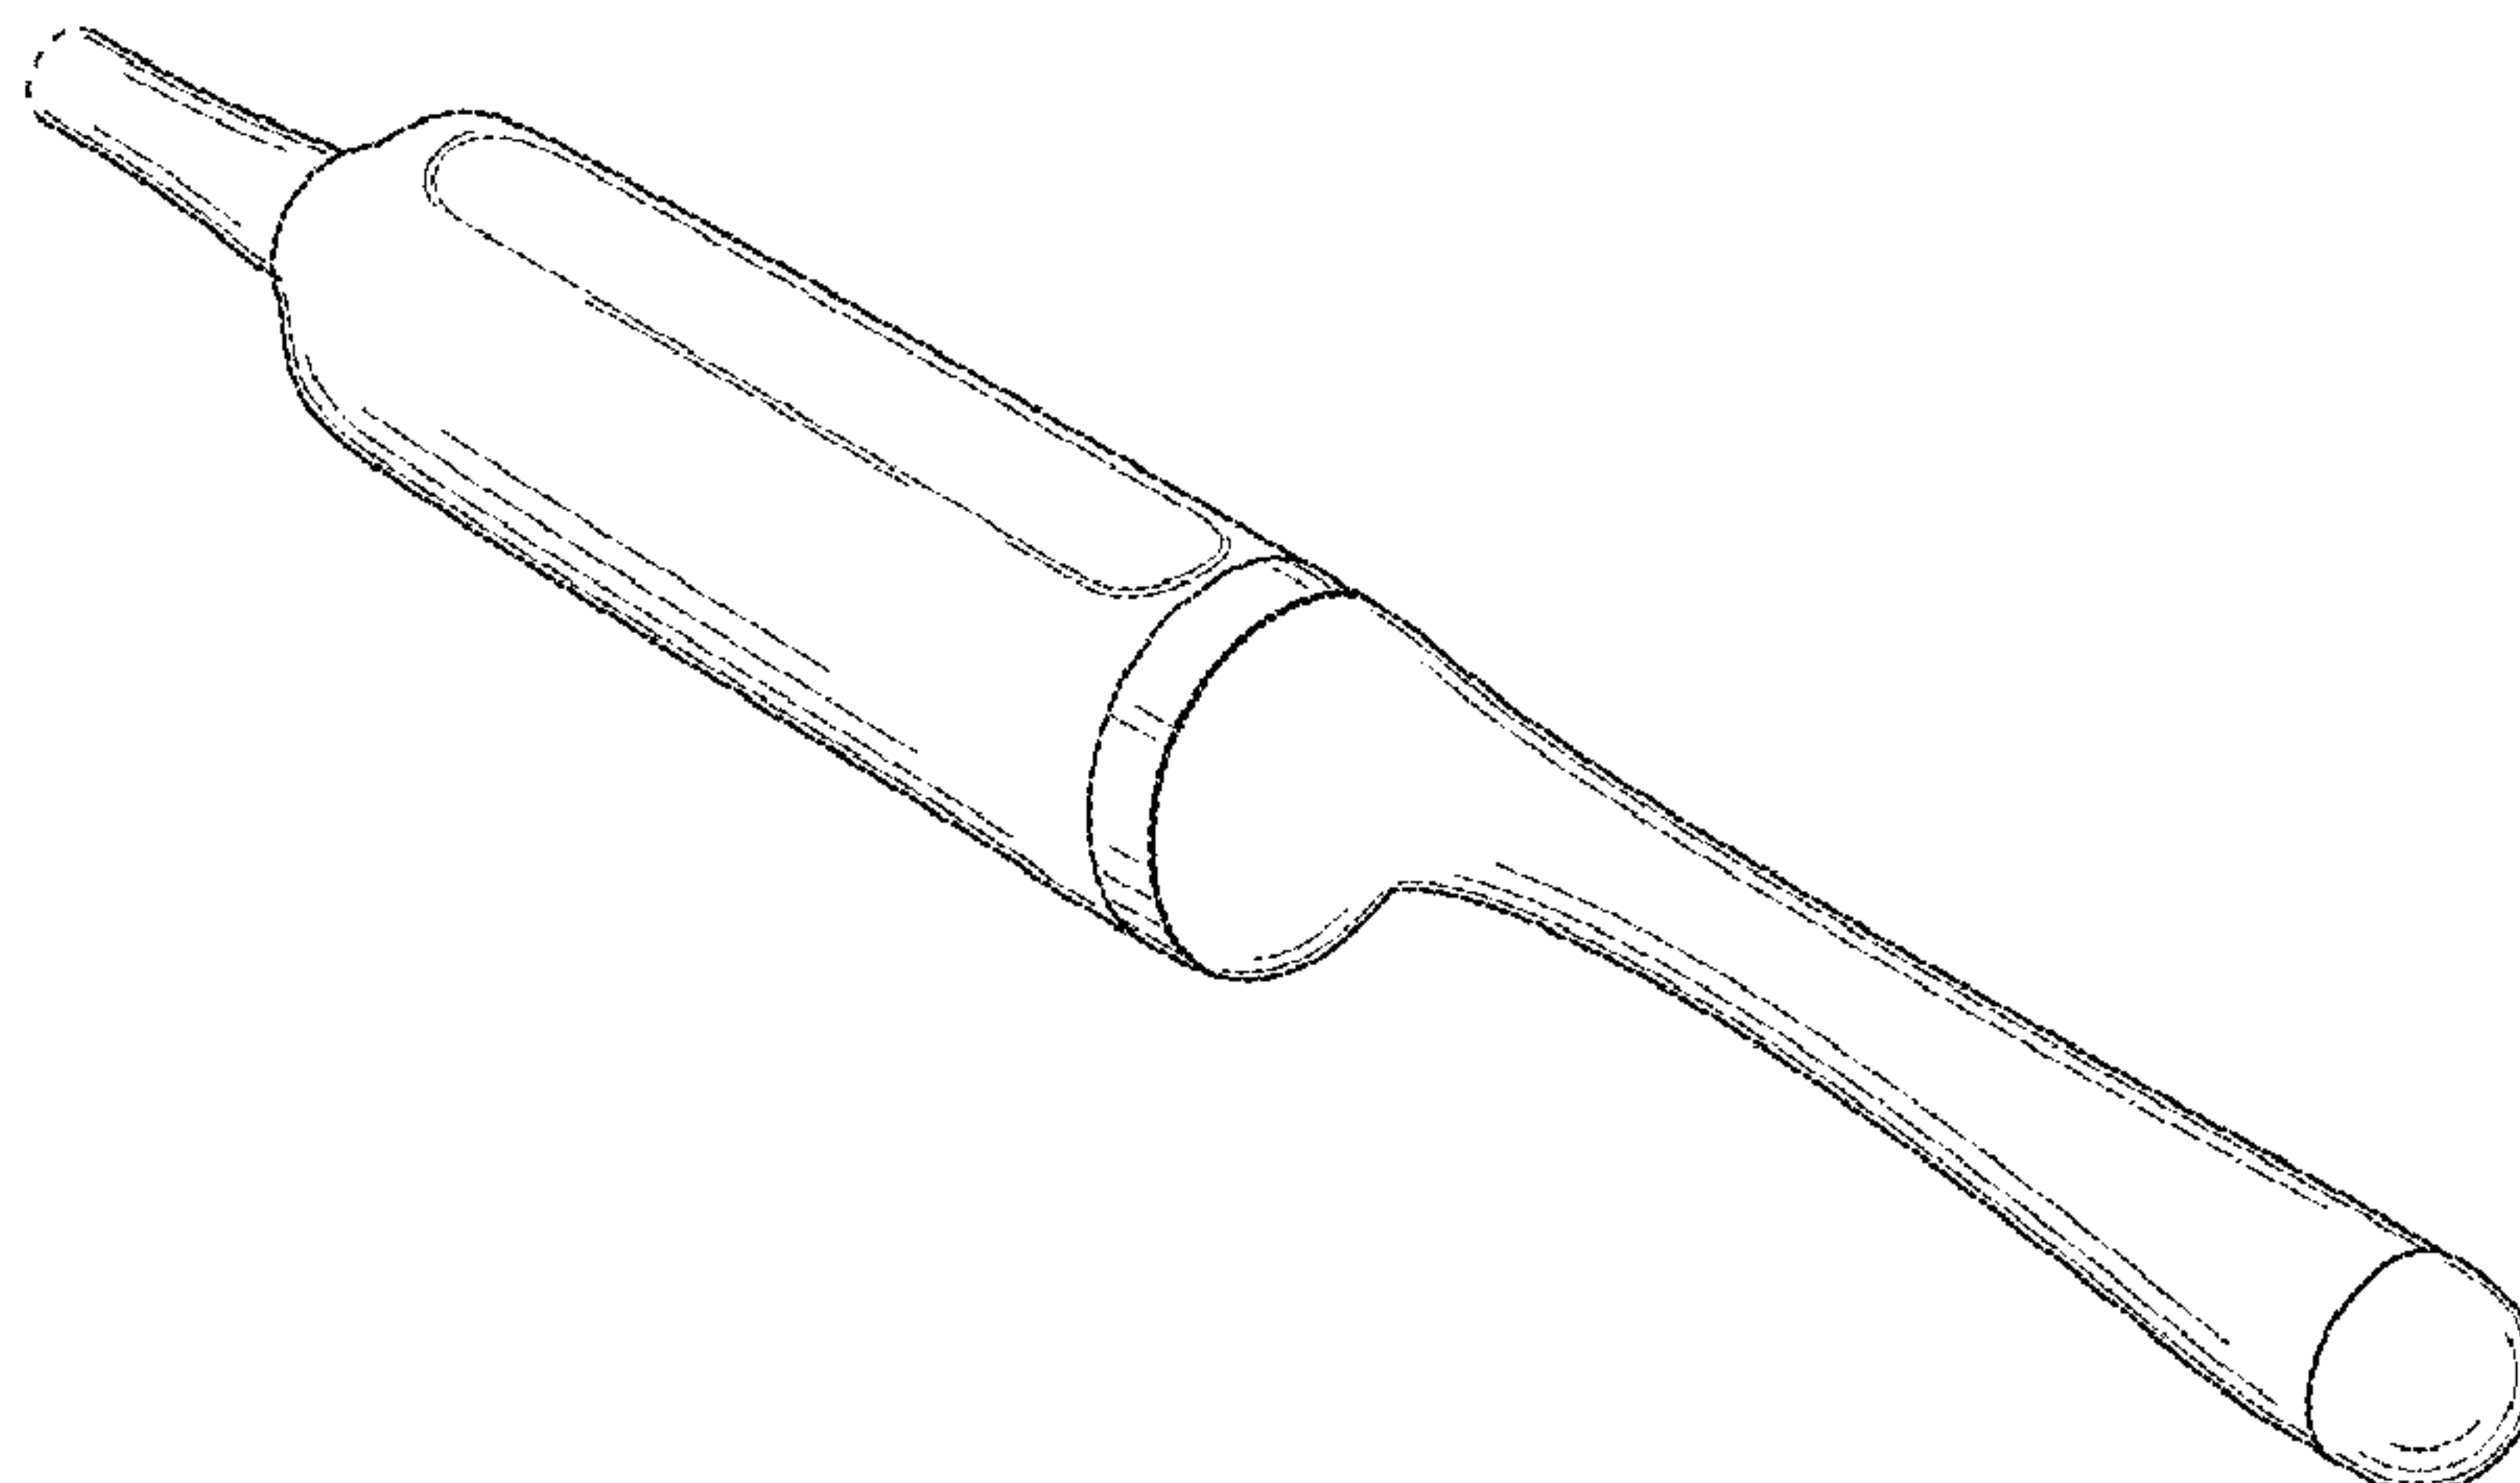

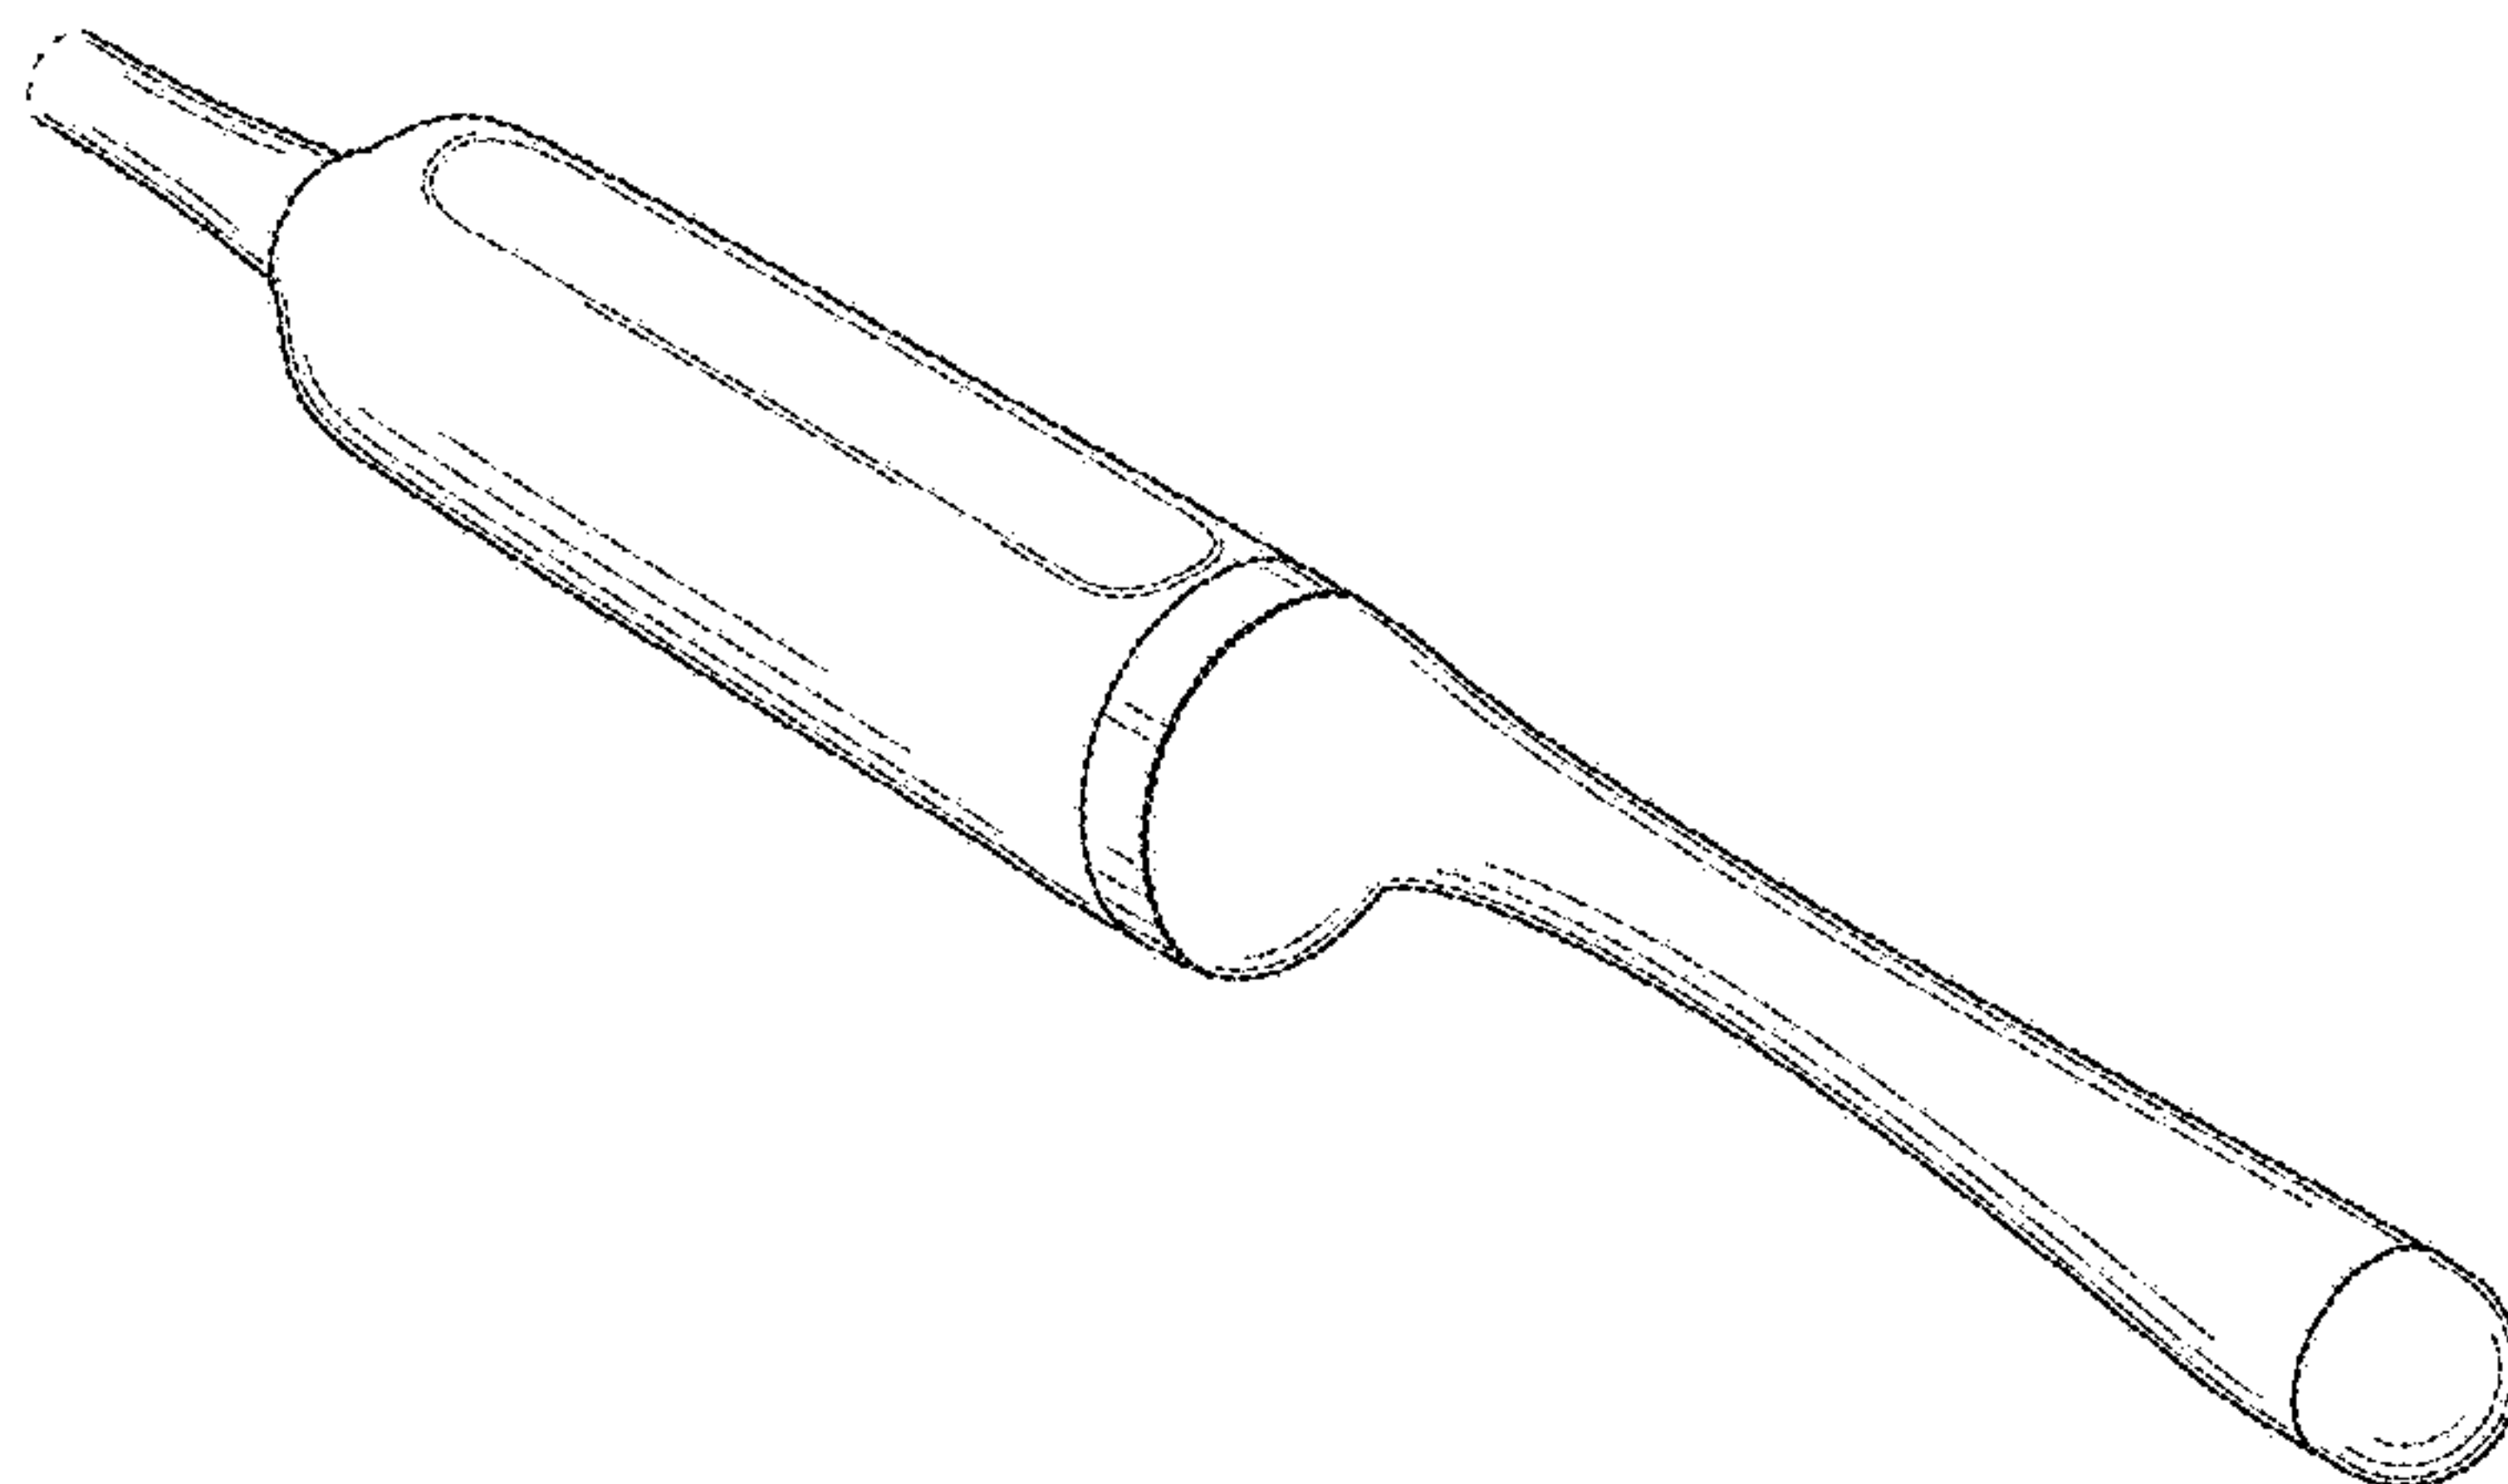


FIG.1

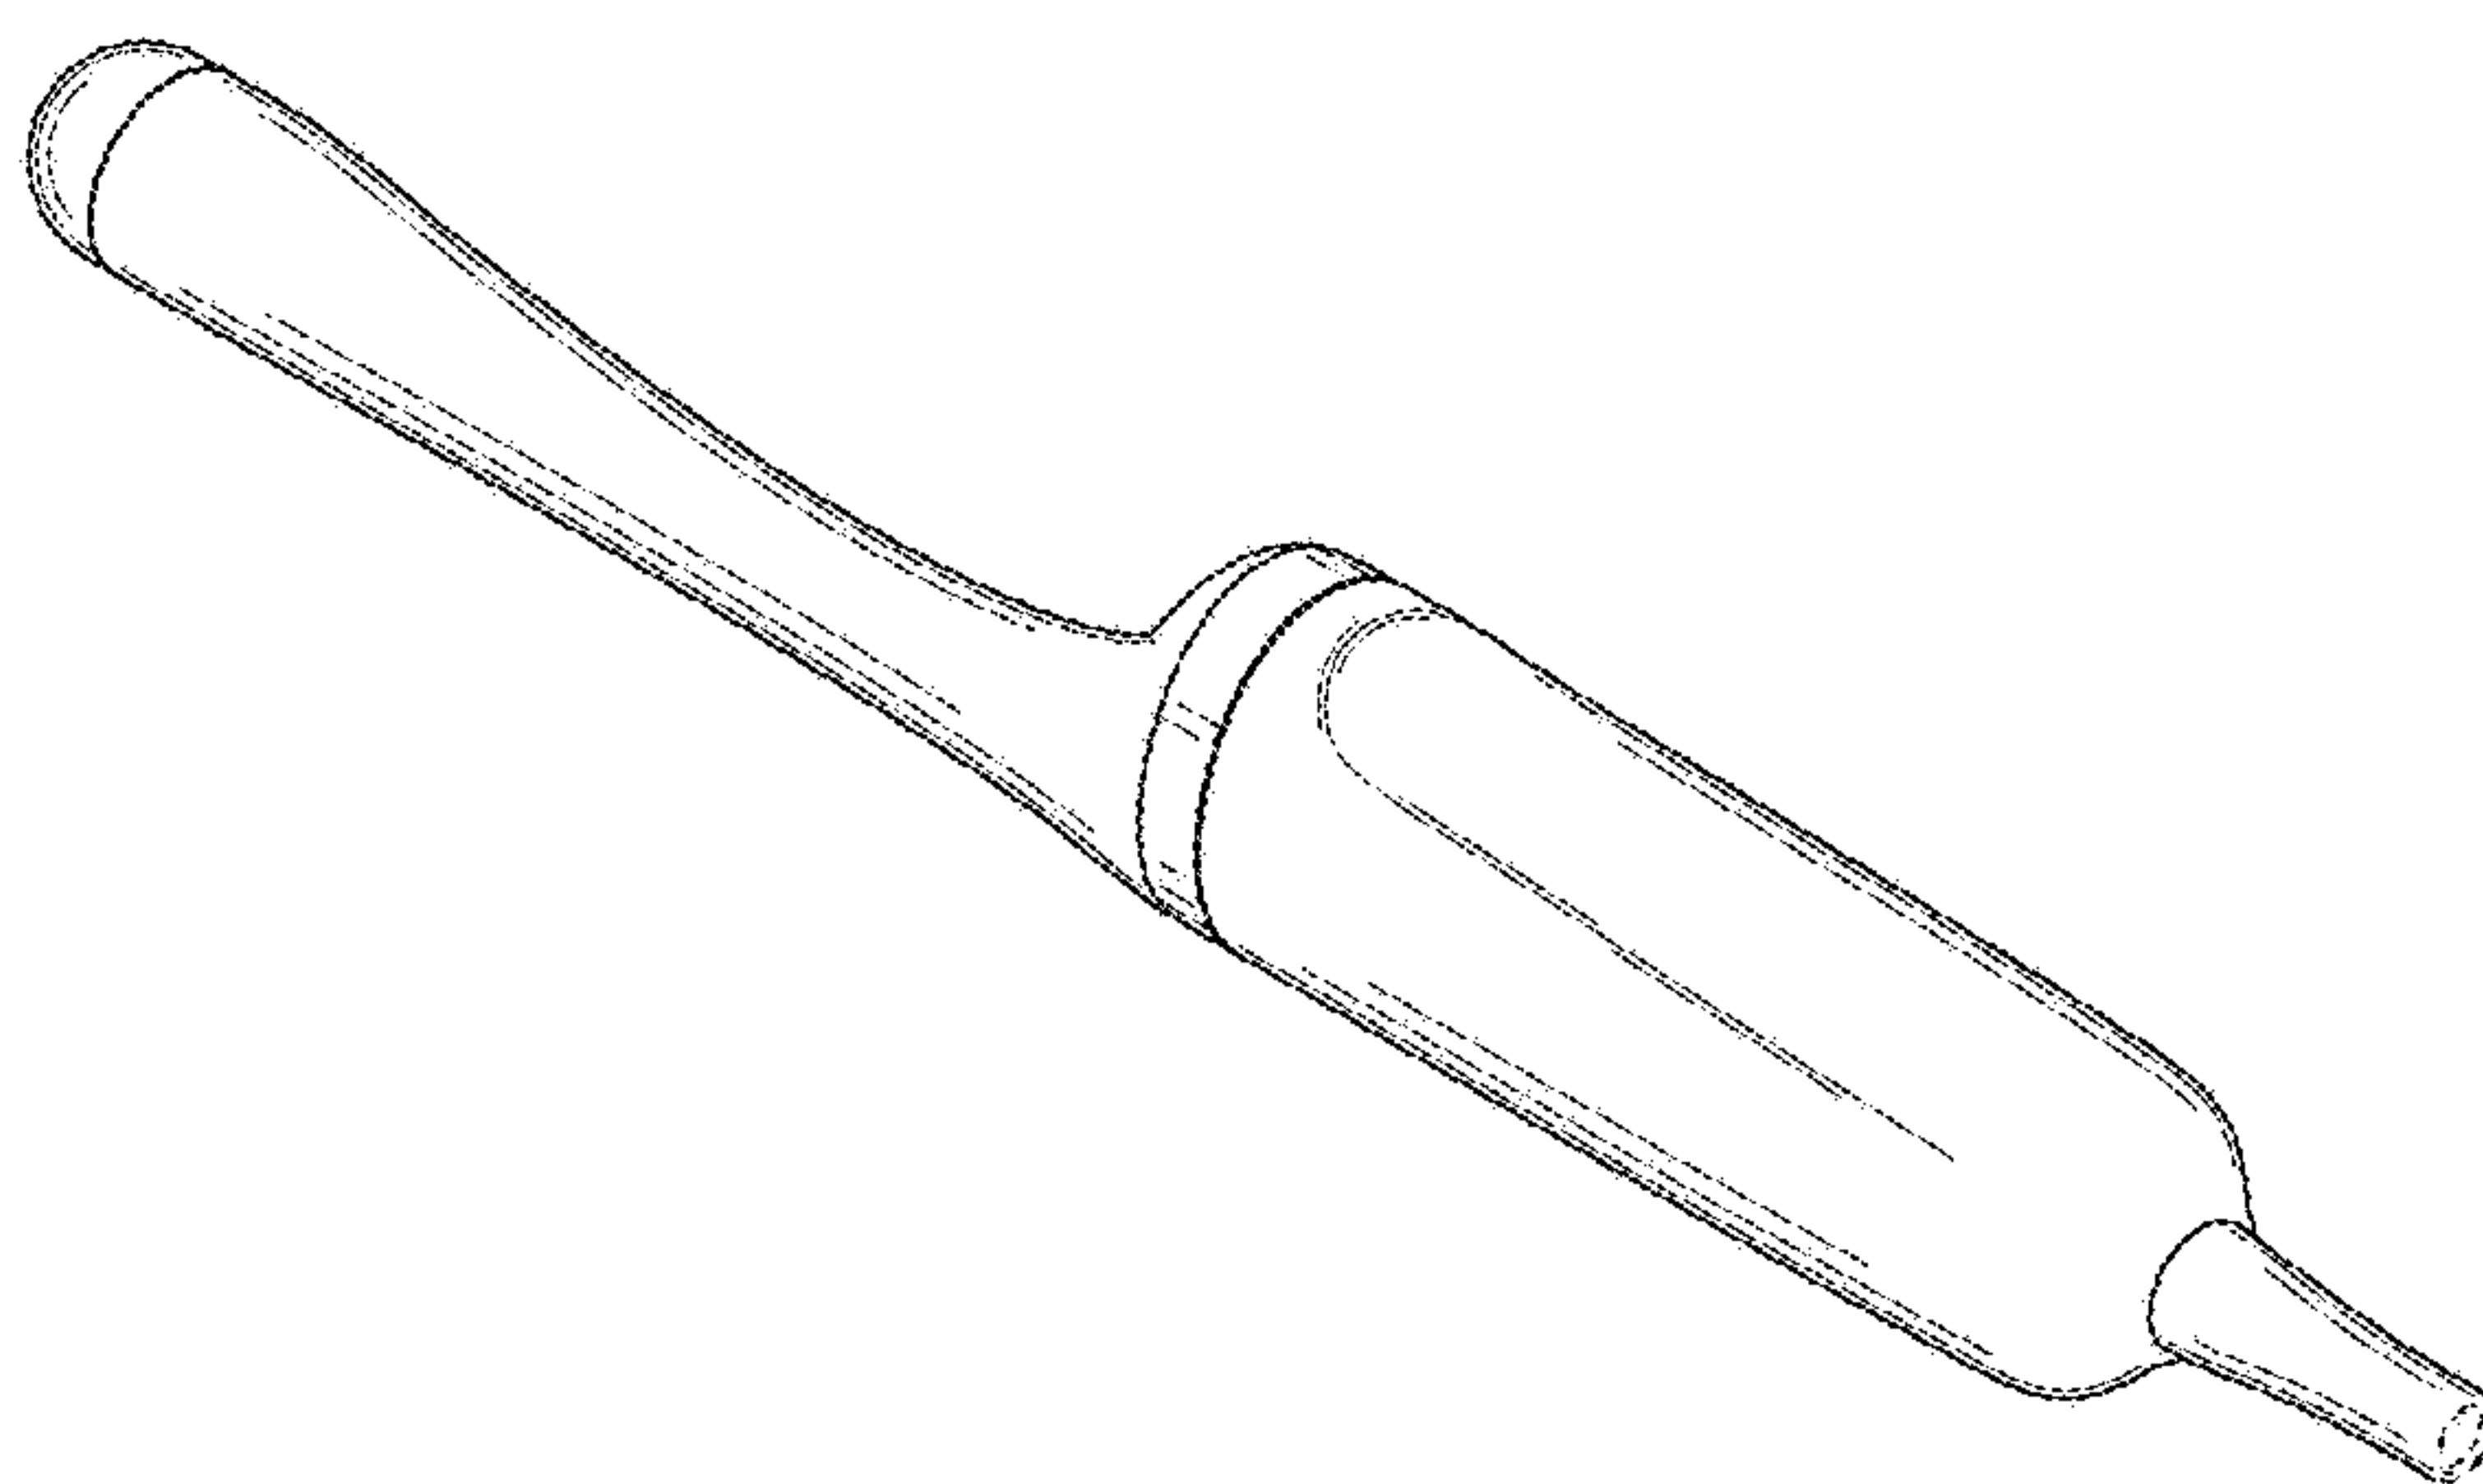


FIG.2

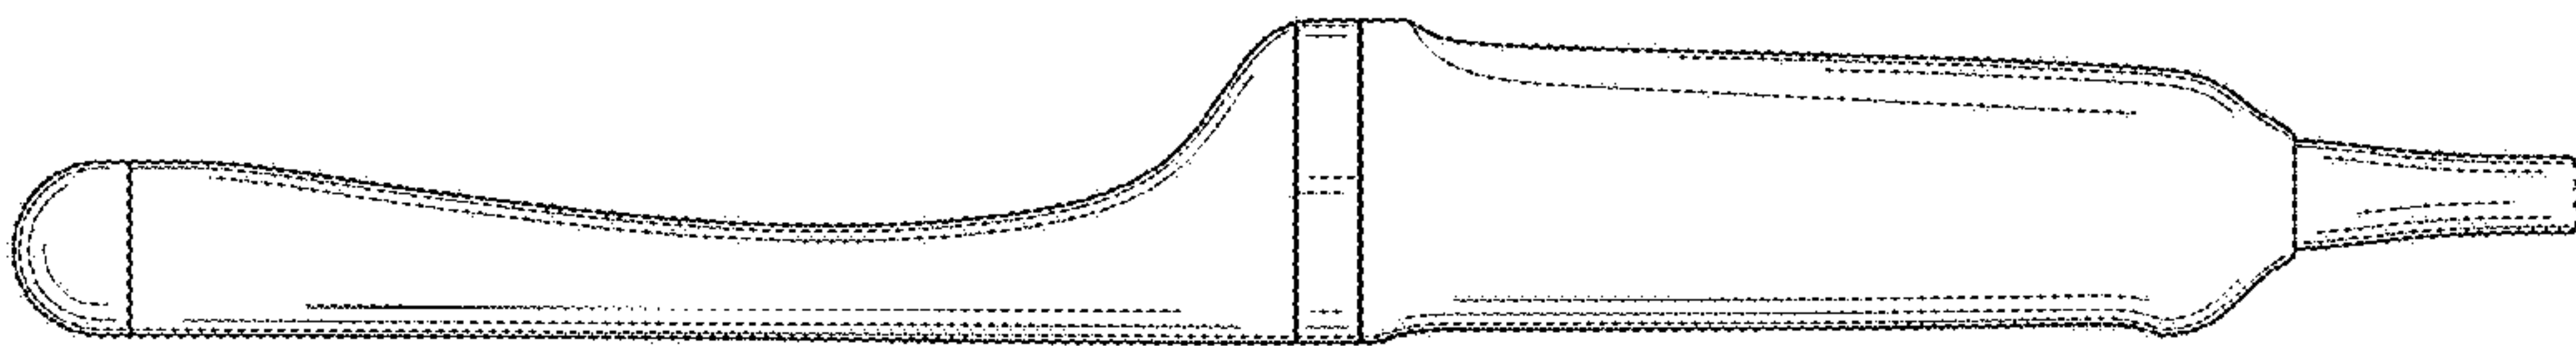


FIG.3

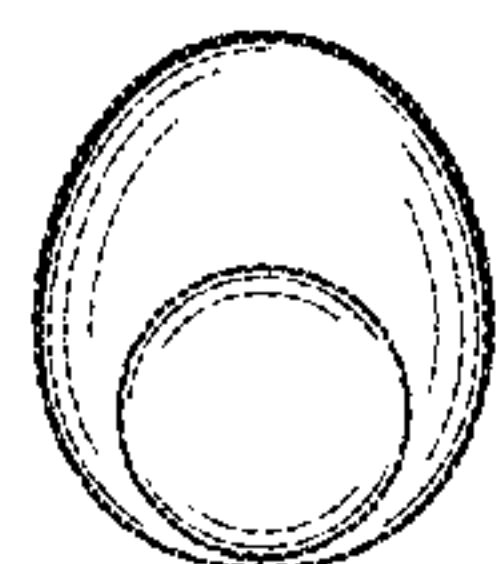


FIG.4

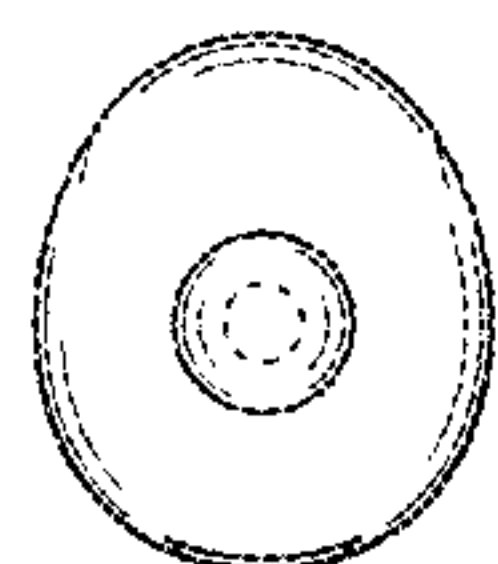


FIG.5

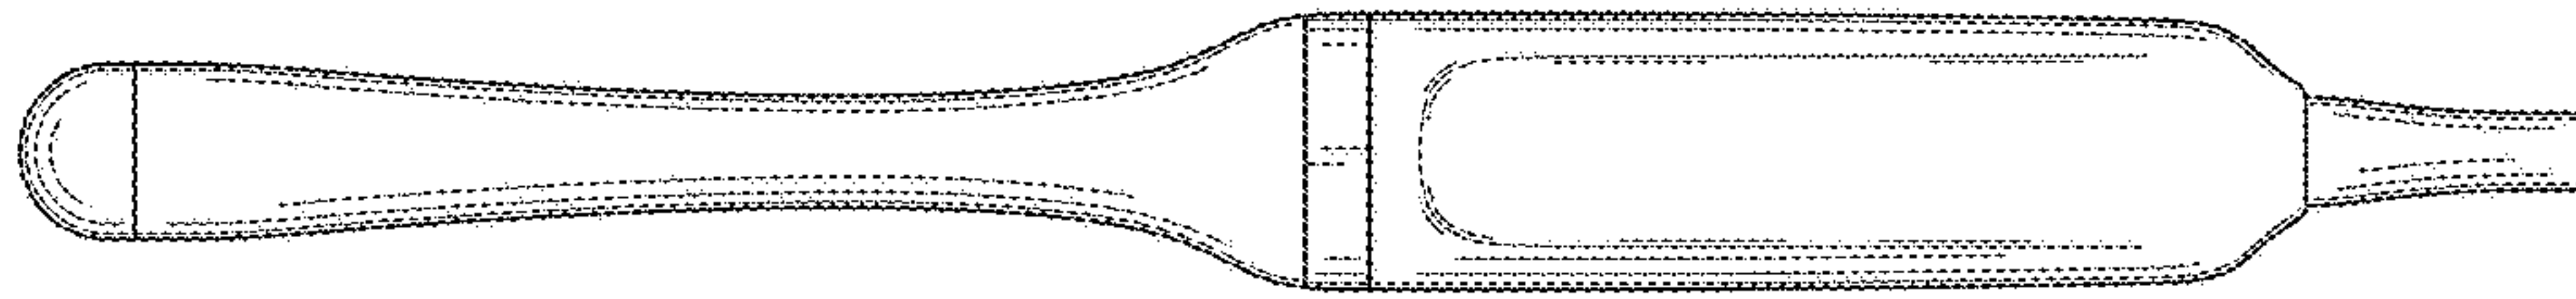


FIG. 6

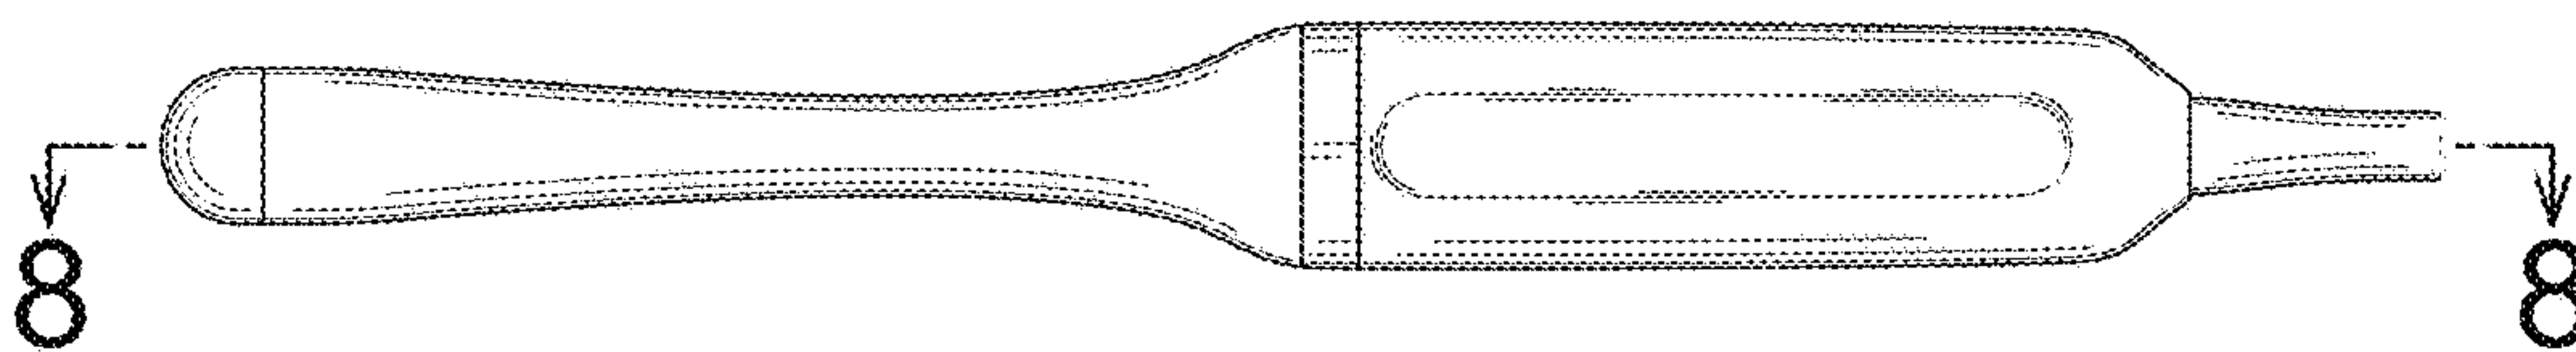


FIG. 7

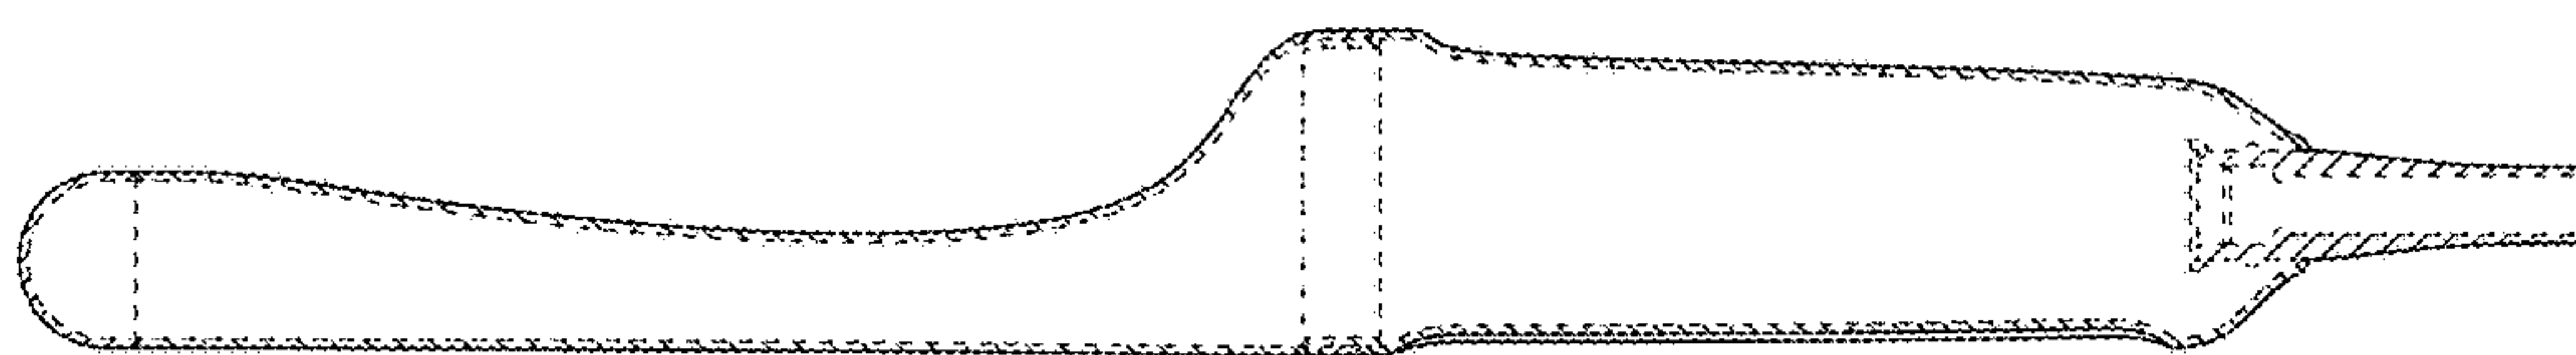


FIG.8