



US00D822225S

(12) **United States Design Patent** (10) **Patent No.:** **US D822,225 S**
Moon et al. (45) **Date of Patent:** **** Jul. 3, 2018**

(54) **DEVICE FOR ANALYSIS OF BIOLOGICAL SAMPLE**

D672,881 S * 12/2012 Kraihanzel D24/224
9,274,132 B2 * 3/2016 Wilson B01L 3/5085
2012/0115238 A1 * 5/2012 Akashi B01L 3/502

436/94

2013/0183769 A1 * 7/2013 Tajima G01N 35/00029
436/165

2014/0302611 A1 * 10/2014 Orning B01L 3/50855
436/71

2016/0291009 A1 * 10/2016 Kim B01L 3/5023

* cited by examiner

(71) Applicant: **Boditech Med Inc.**, Chuncheon-si, Gangwon-do (KR)

(72) Inventors: **Bong Suk Moon**, Chuncheon-si (KR); **Young Jin Oh**, Chuncheon-si (KR); **Yu Jin Park**, Chuncheon-si (KR)

(73) Assignee: **BODITECH MED INC.**, Chuncheon-si, Gangwon-Do (KR)

Primary Examiner — Anhdao Doan

(**) Term: **15 Years**

(74) *Attorney, Agent, or Firm* — Rabin & Berdo, P.C.

(21) Appl. No.: **29/604,703**

(57) **CLAIM**

(22) Filed: **May 19, 2017**

The ornamental design for a device for analysis of biological sample, as shown and described.

(30) **Foreign Application Priority Data**

DESCRIPTION

Nov. 24, 2016 (KR) 30-2016-0056501

FIG. 1 is a top perspective view of a device for analysis of biological sample;

(51) **LOC (11) Cl.** **24-01**

FIG. 2 is a front elevational view thereof;

(52) **U.S. Cl.**

FIG. 3 is a rear elevational view thereof;

USPC **D24/224**

FIG. 4 is a left side elevational view thereof;

(58) **Field of Classification Search**

FIG. 5 is a right side elevational view thereof;

USPC D24/121, 216, 219–221, 224–233;

FIG. 6 is a top plan view thereof;

D10/81

FIG. 7 is a bottom plan view thereof;

CPC .. B01L 3/502715; B01L 3/508; B01L 3/5085;

FIG. 8 is an exploded top perspective view thereof, showing reagent tubes are detached from the device for analysis of biological sample; and

B01L 3/50855; B01L 3/52; B01L 3/523;

FIG. 9 is a bottom perspective view of the device for analysis of biological sample; and,

B01L 3/527; B01L 2200/16; B01L

FIG. 10 is another bottom perspective view of the device for analysis of biological sample.


2200/18

In FIG. 8, the broken lines connecting the centers of the separated reagent tubes are included to show the order of assembly and form no part of the claimed design.

See application file for complete search history.

(56) **References Cited**

1 Claim, 9 Drawing Sheets

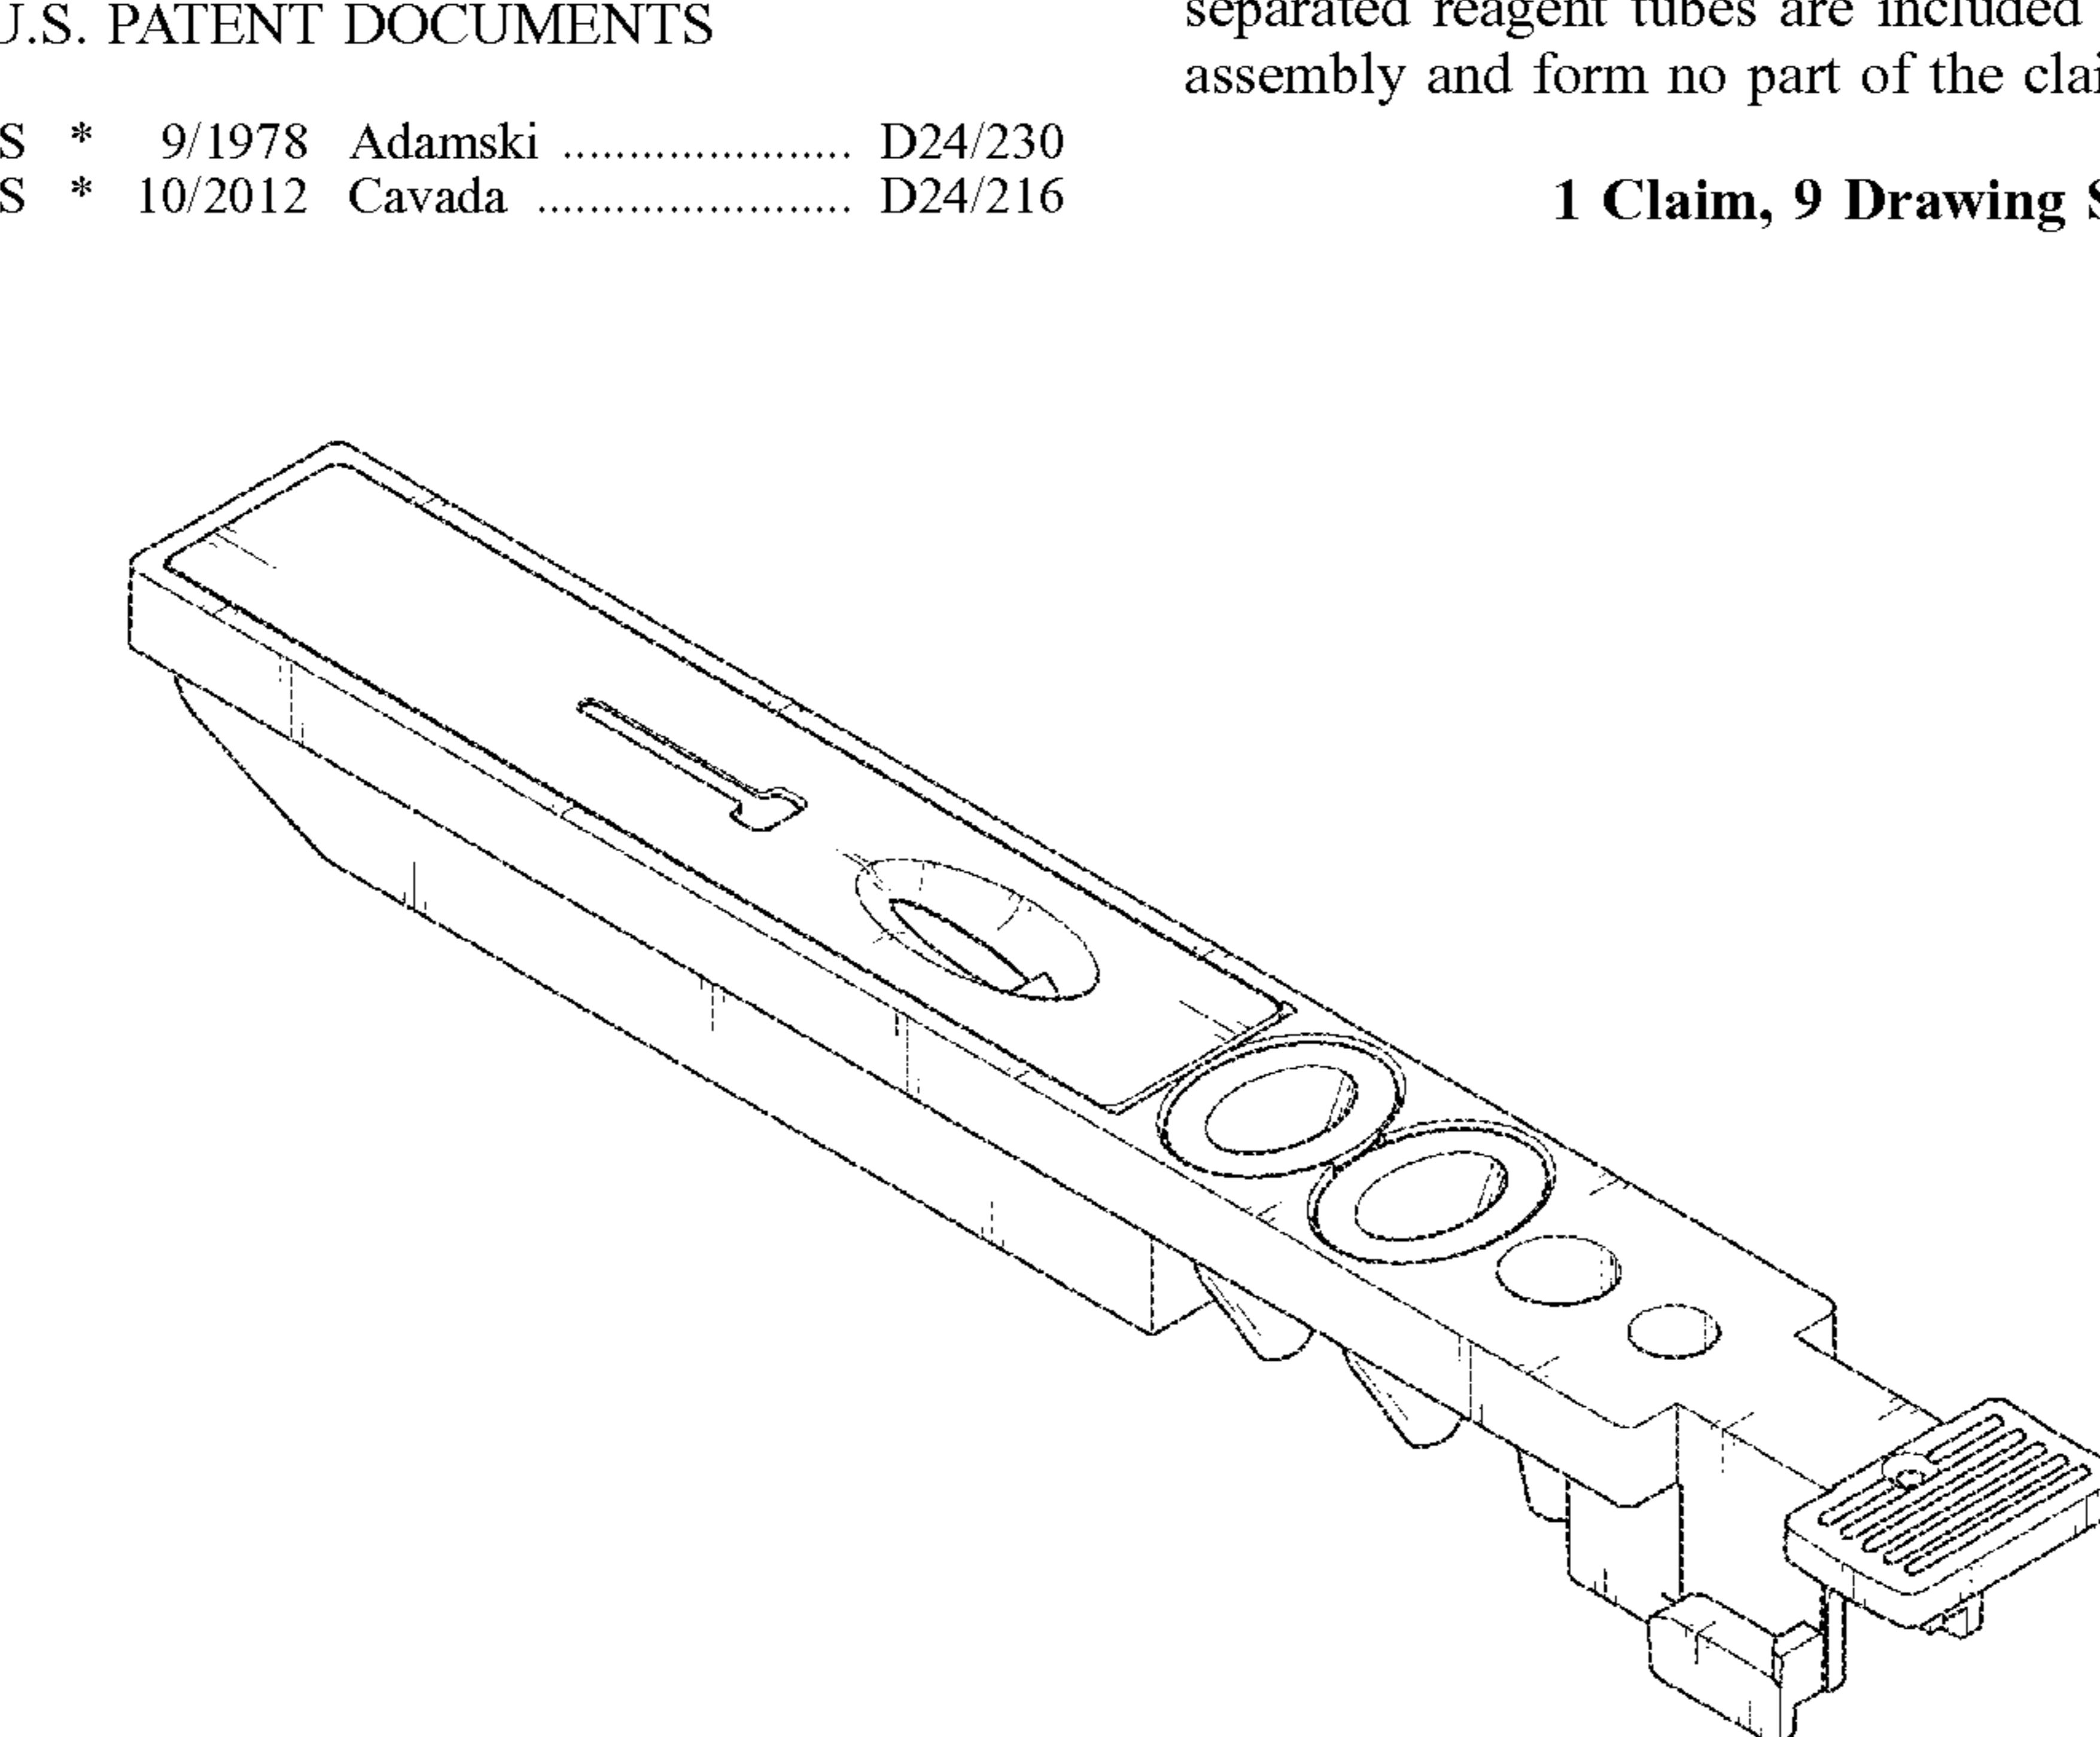

D249,706 S * 9/1978 Adamski D24/230
D669,597 S * 10/2012 Cavada D24/216

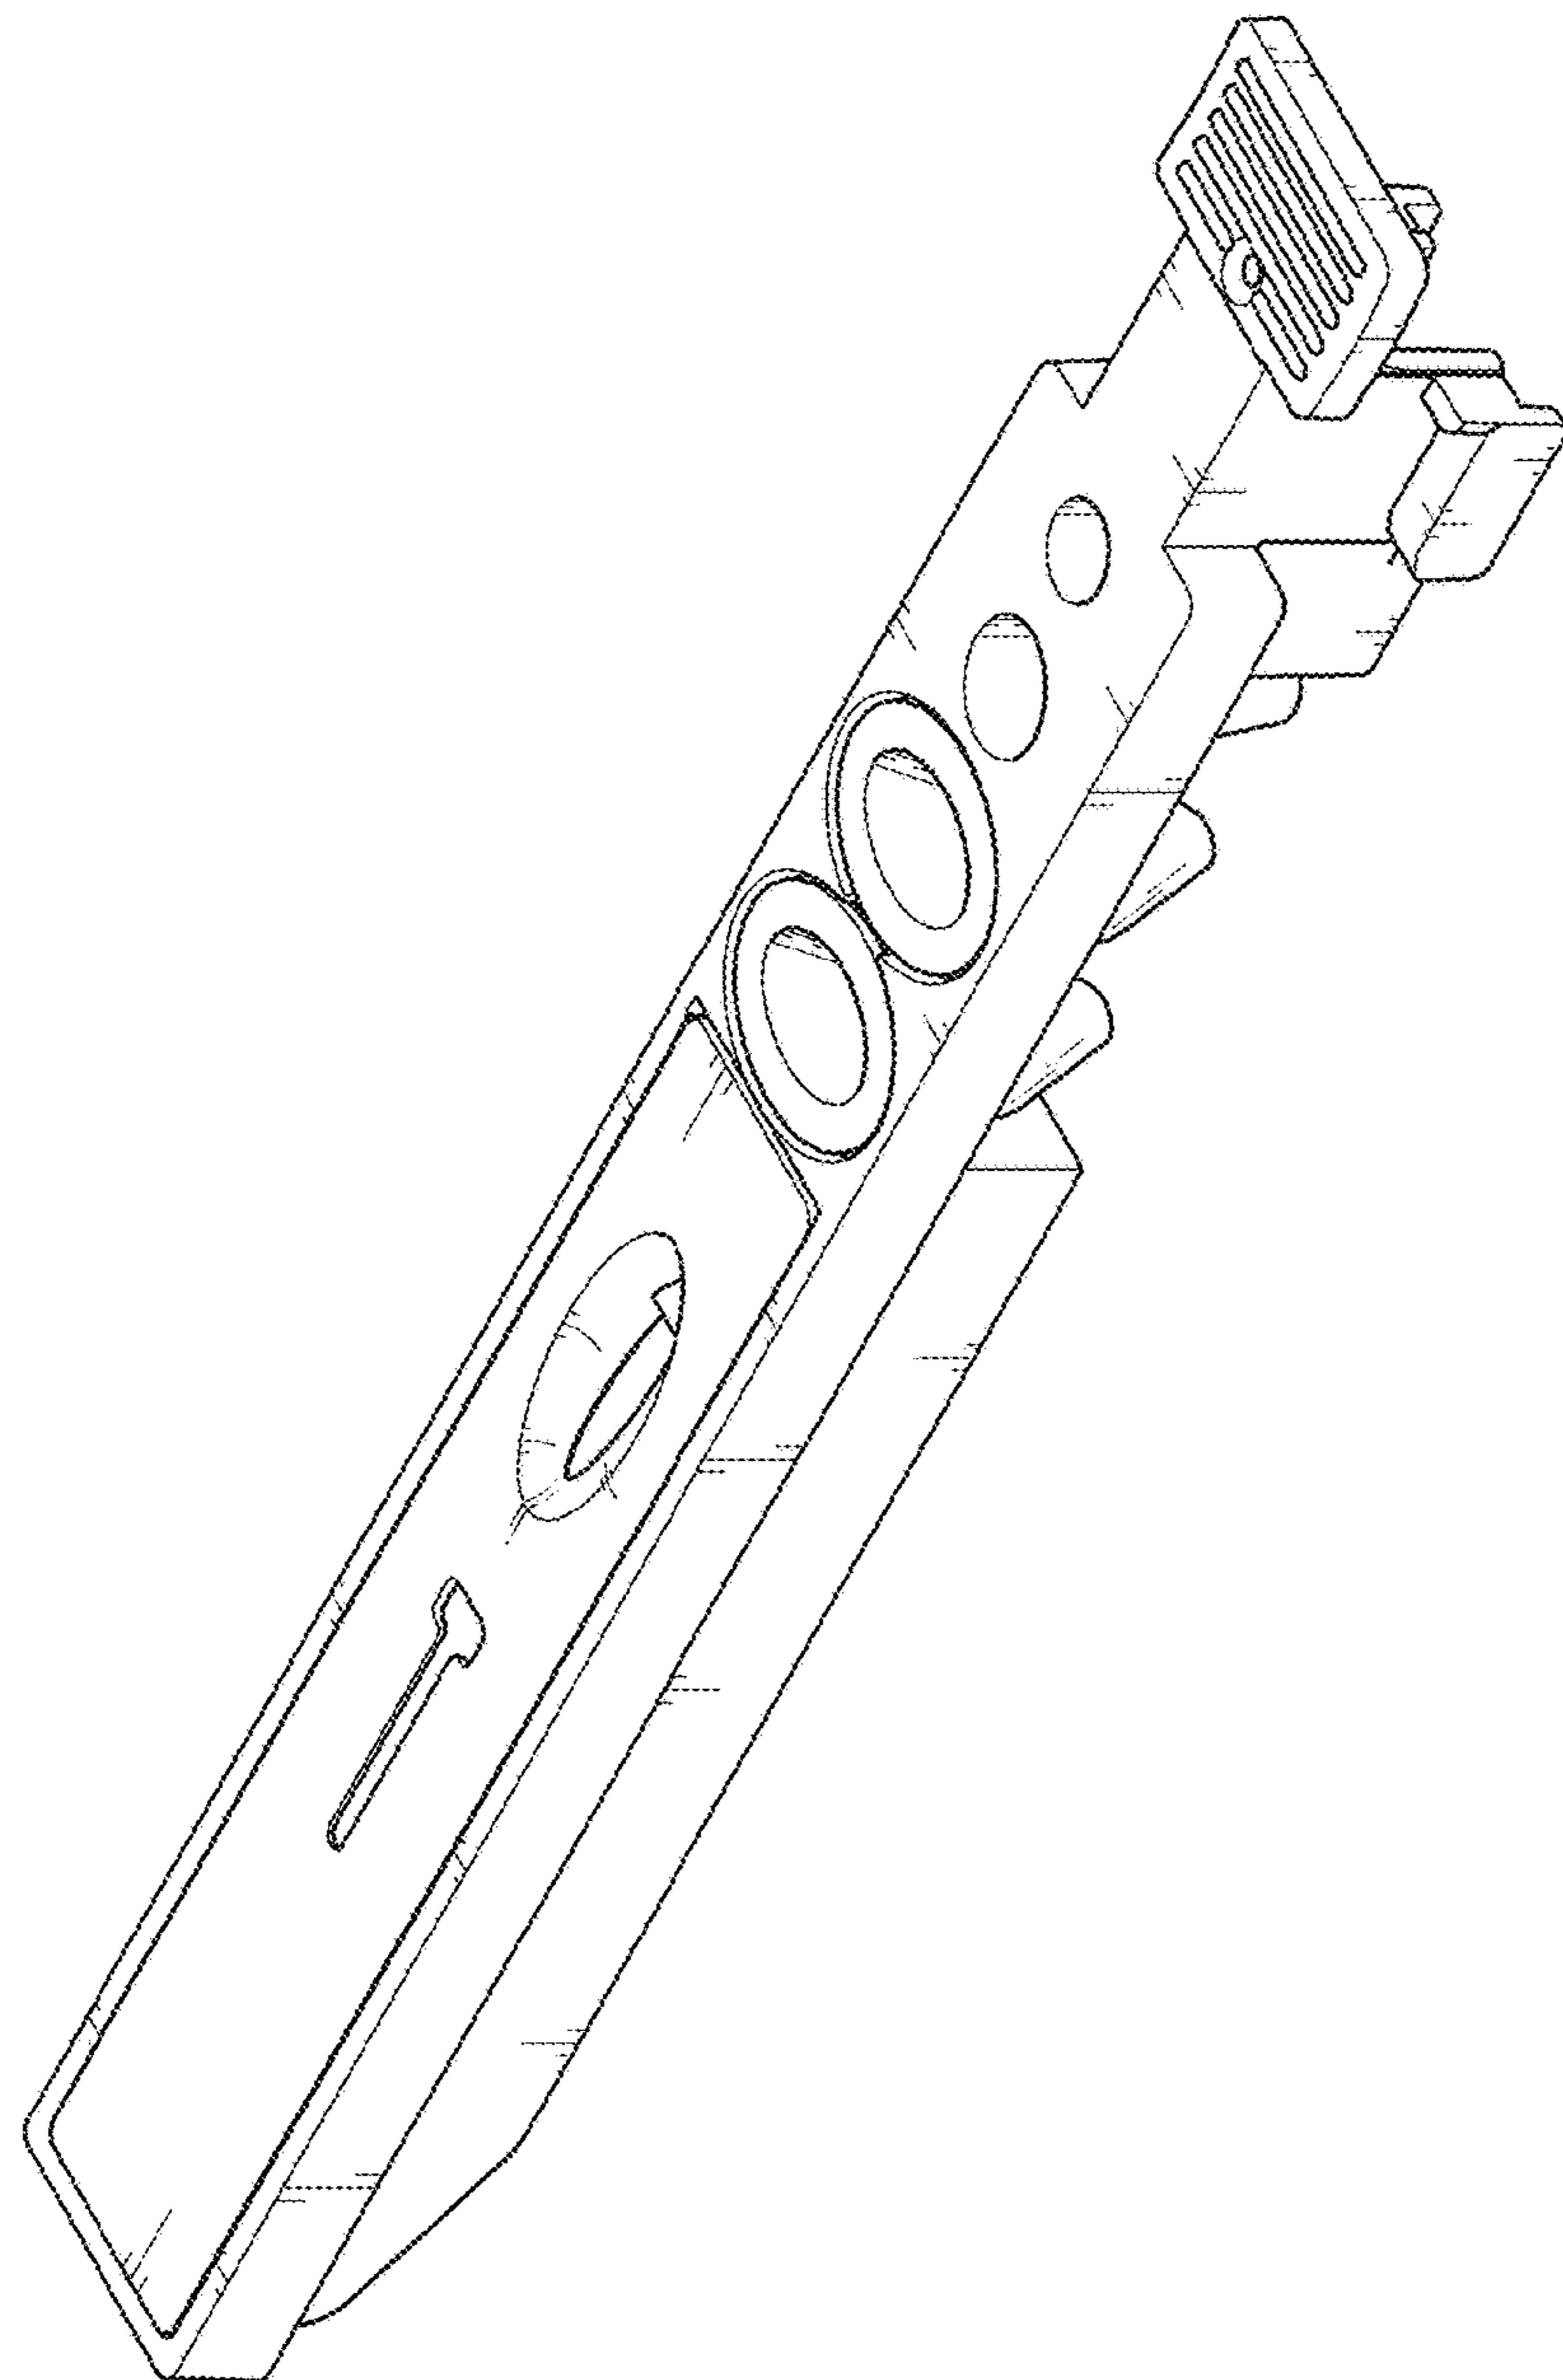


FIG. 1

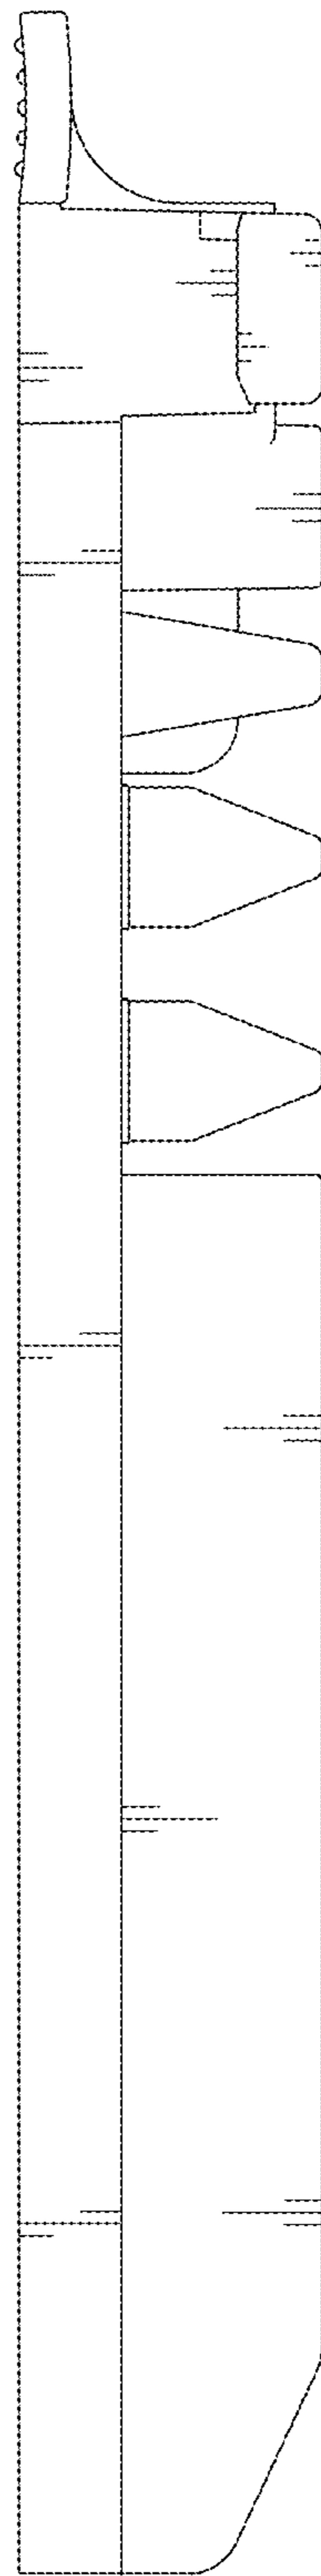


FIG. 2

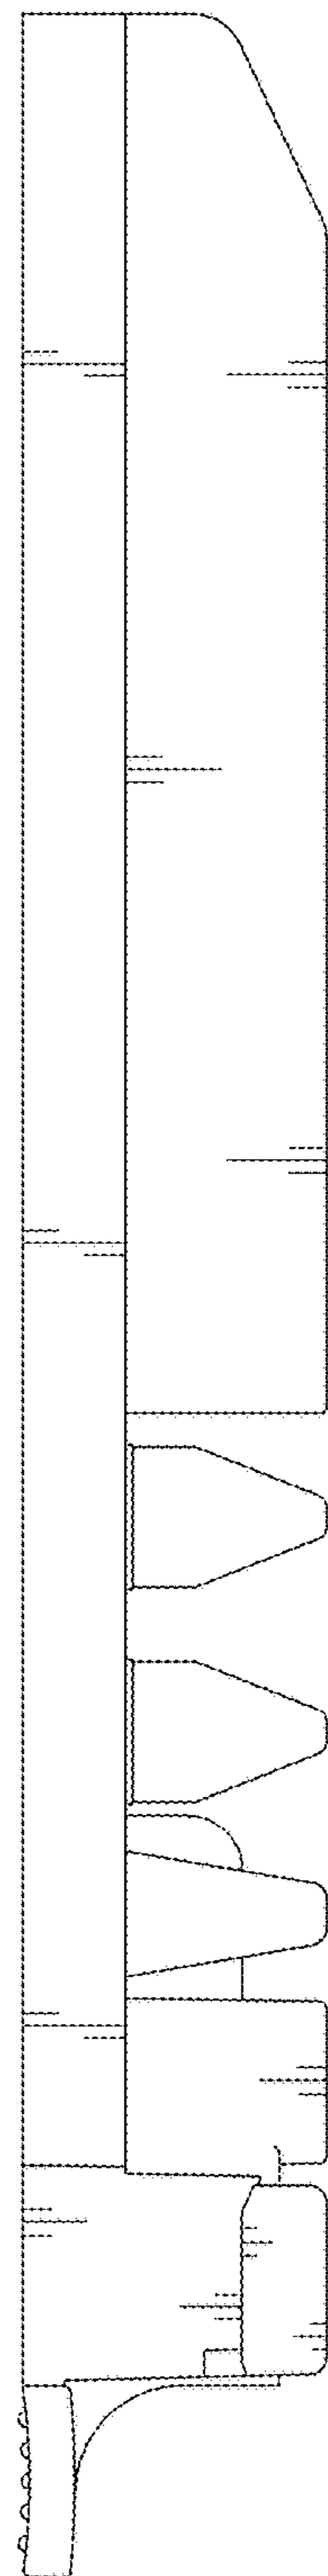


FIG. 3

FIG. 5

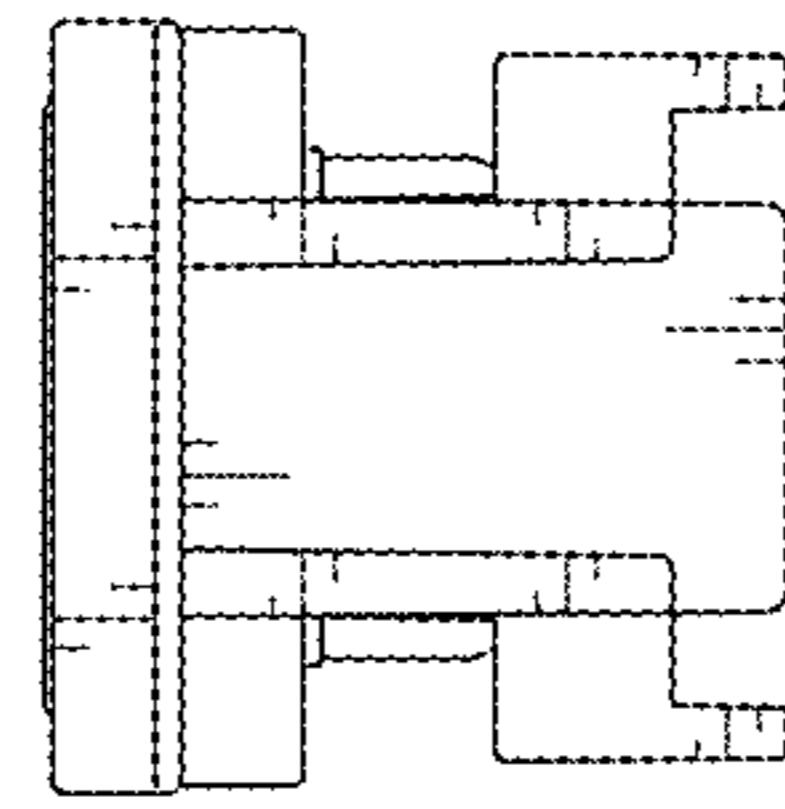
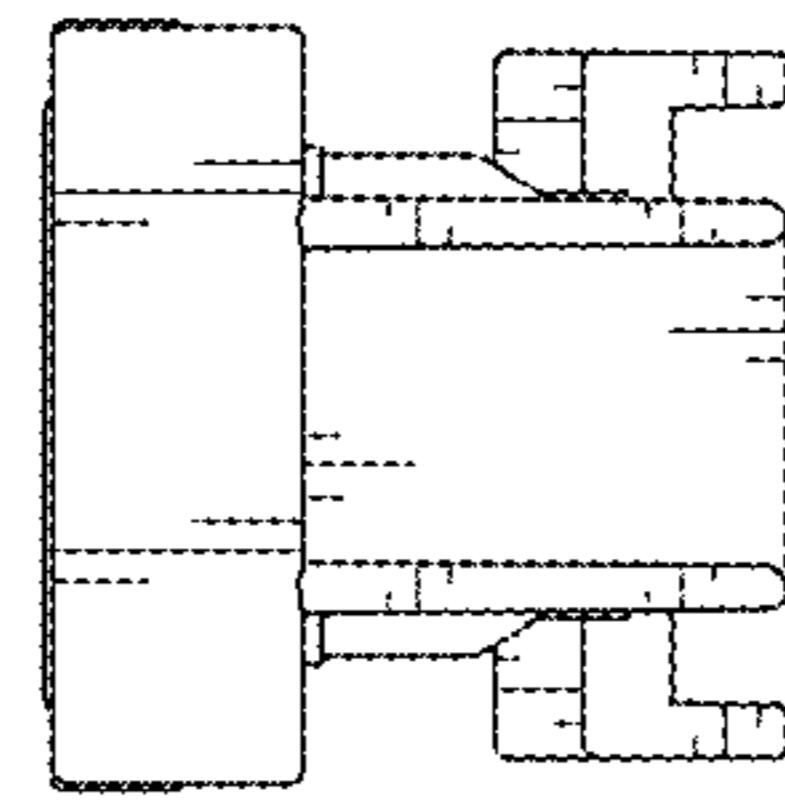


FIG. 4



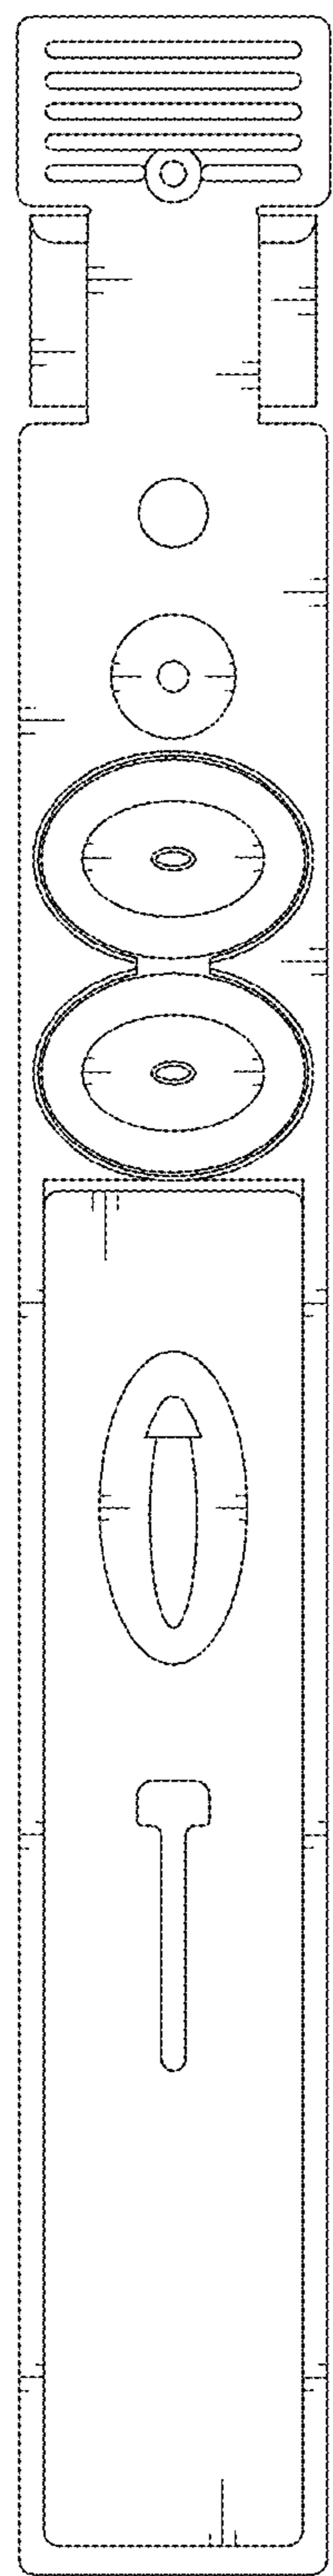


FIG. 6

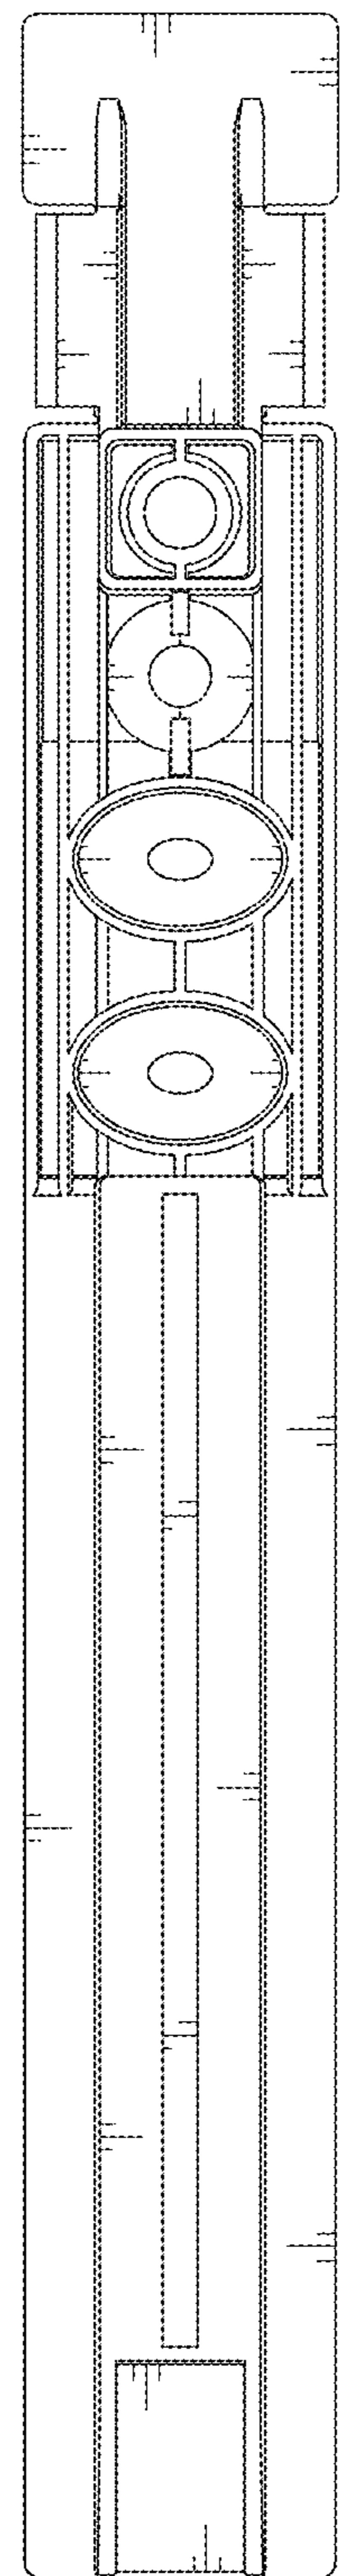


FIG. 7

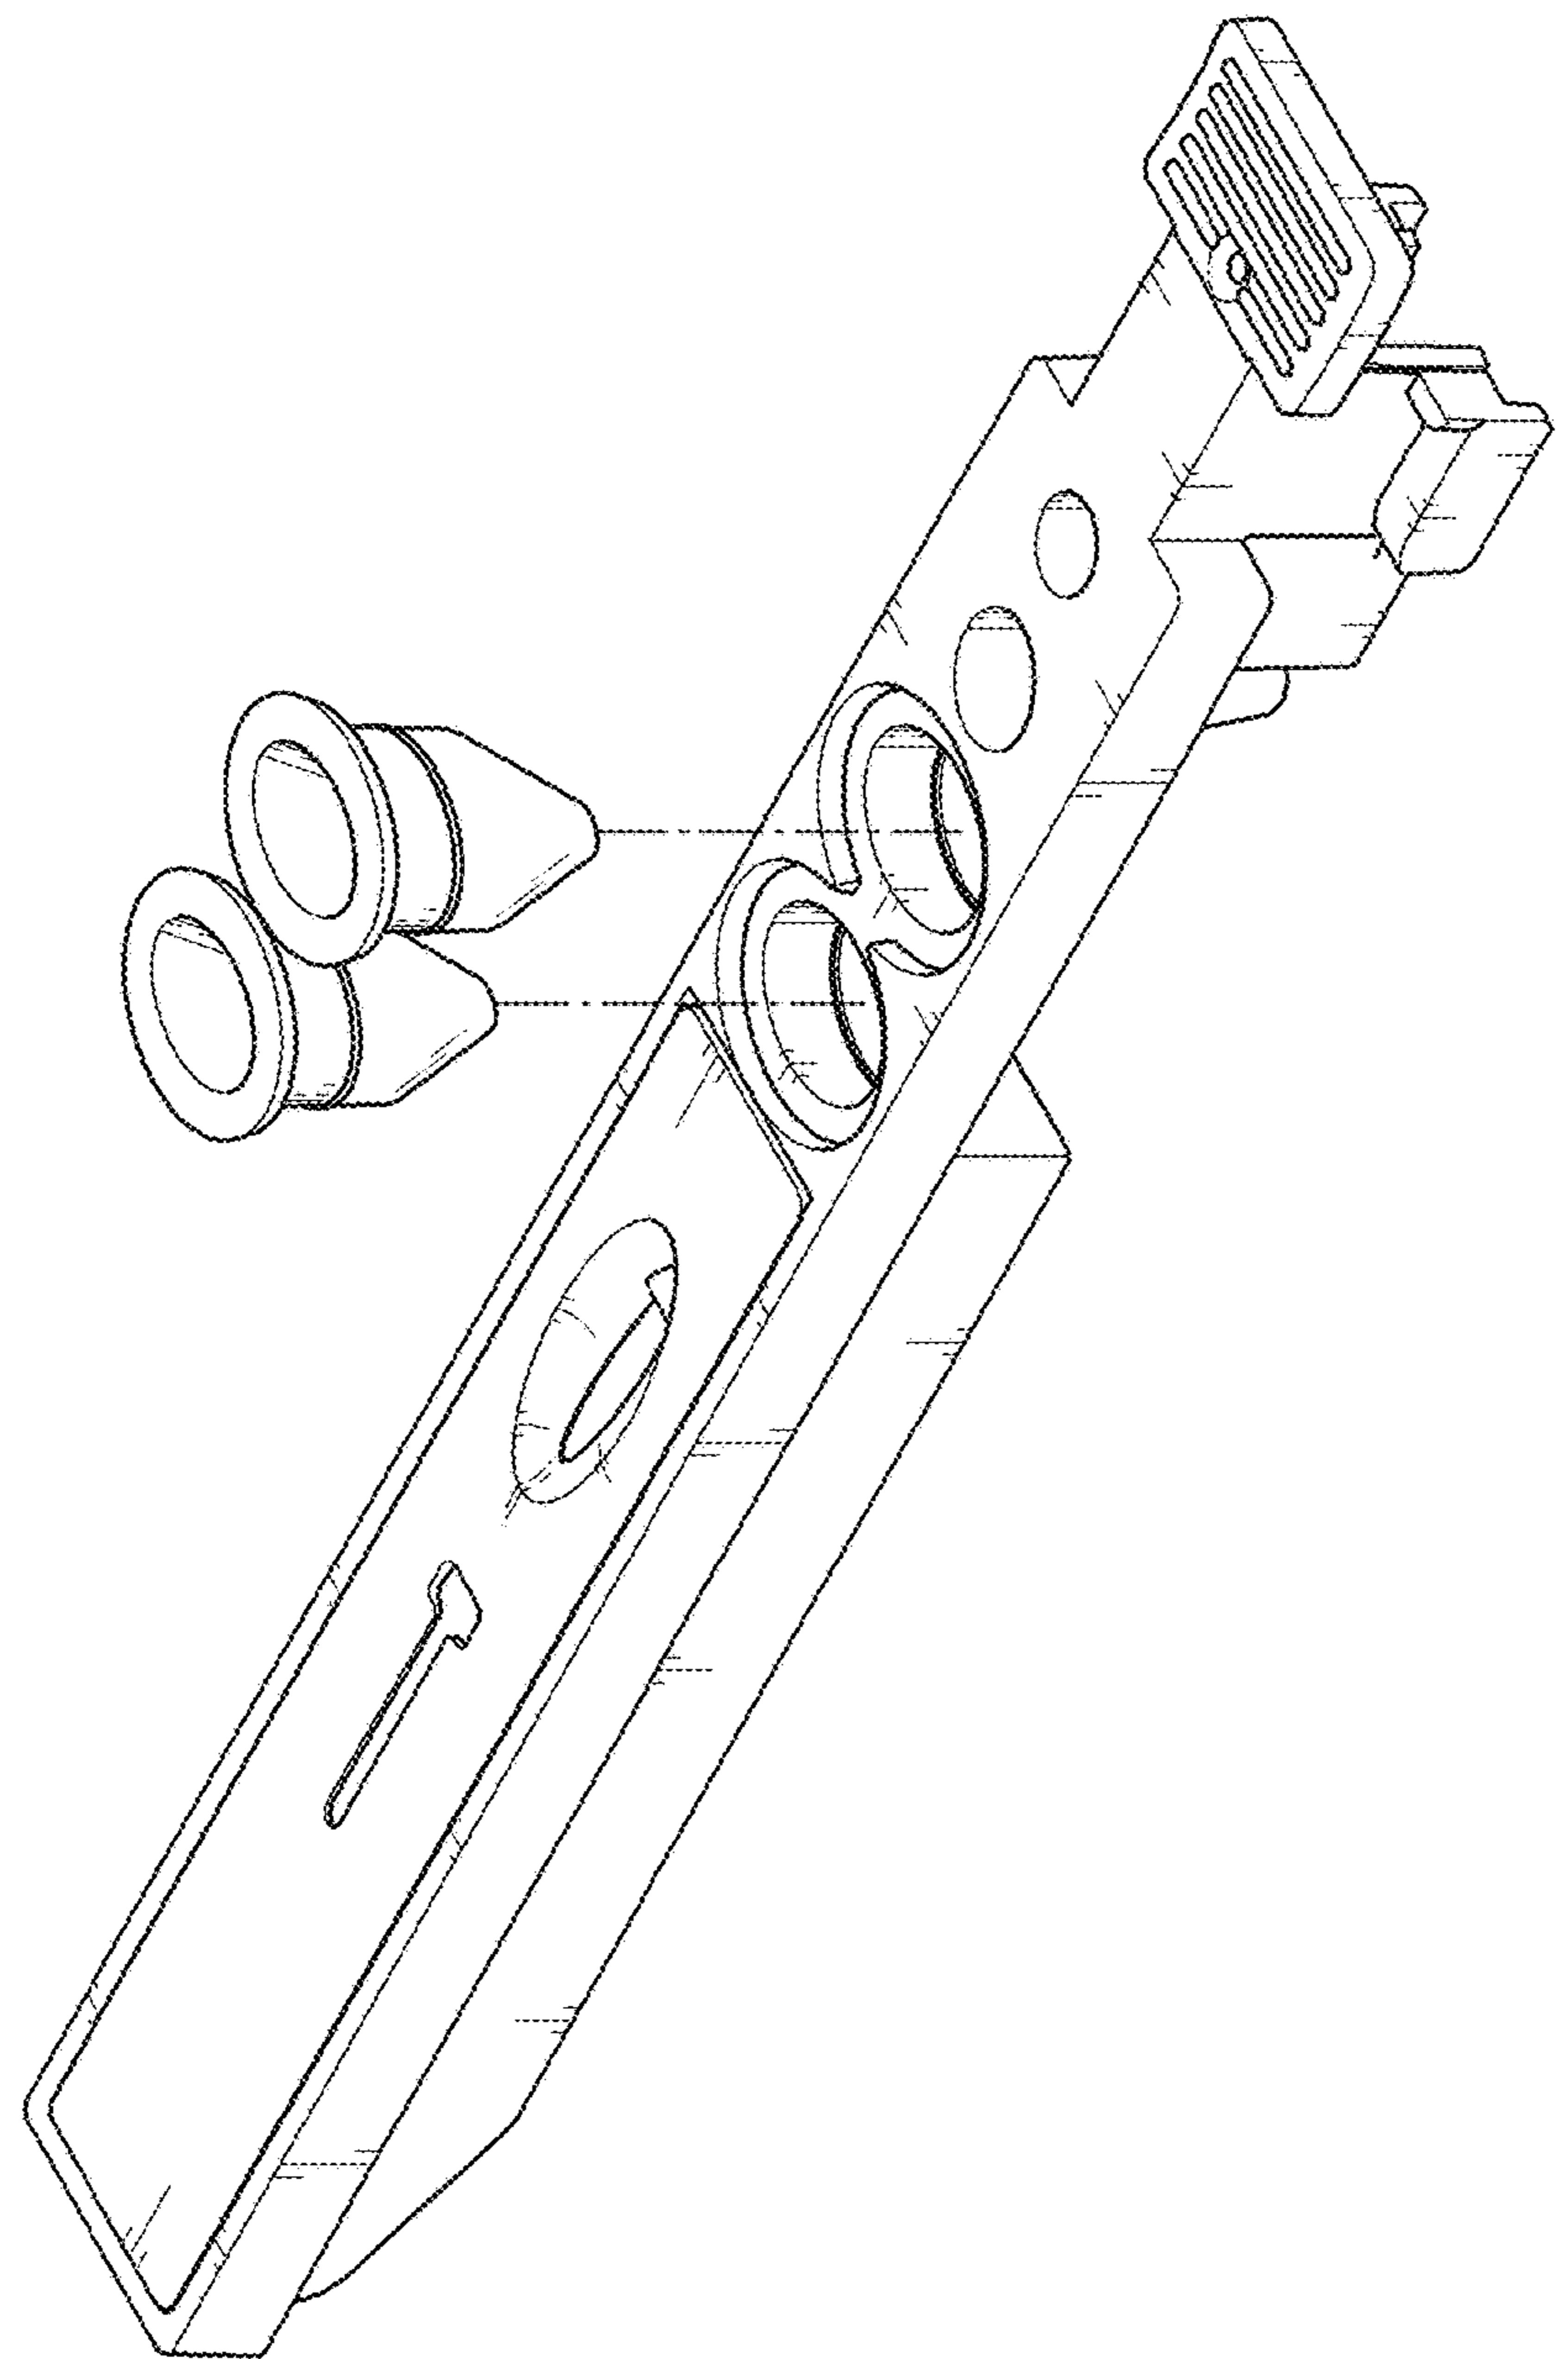


FIG. 8

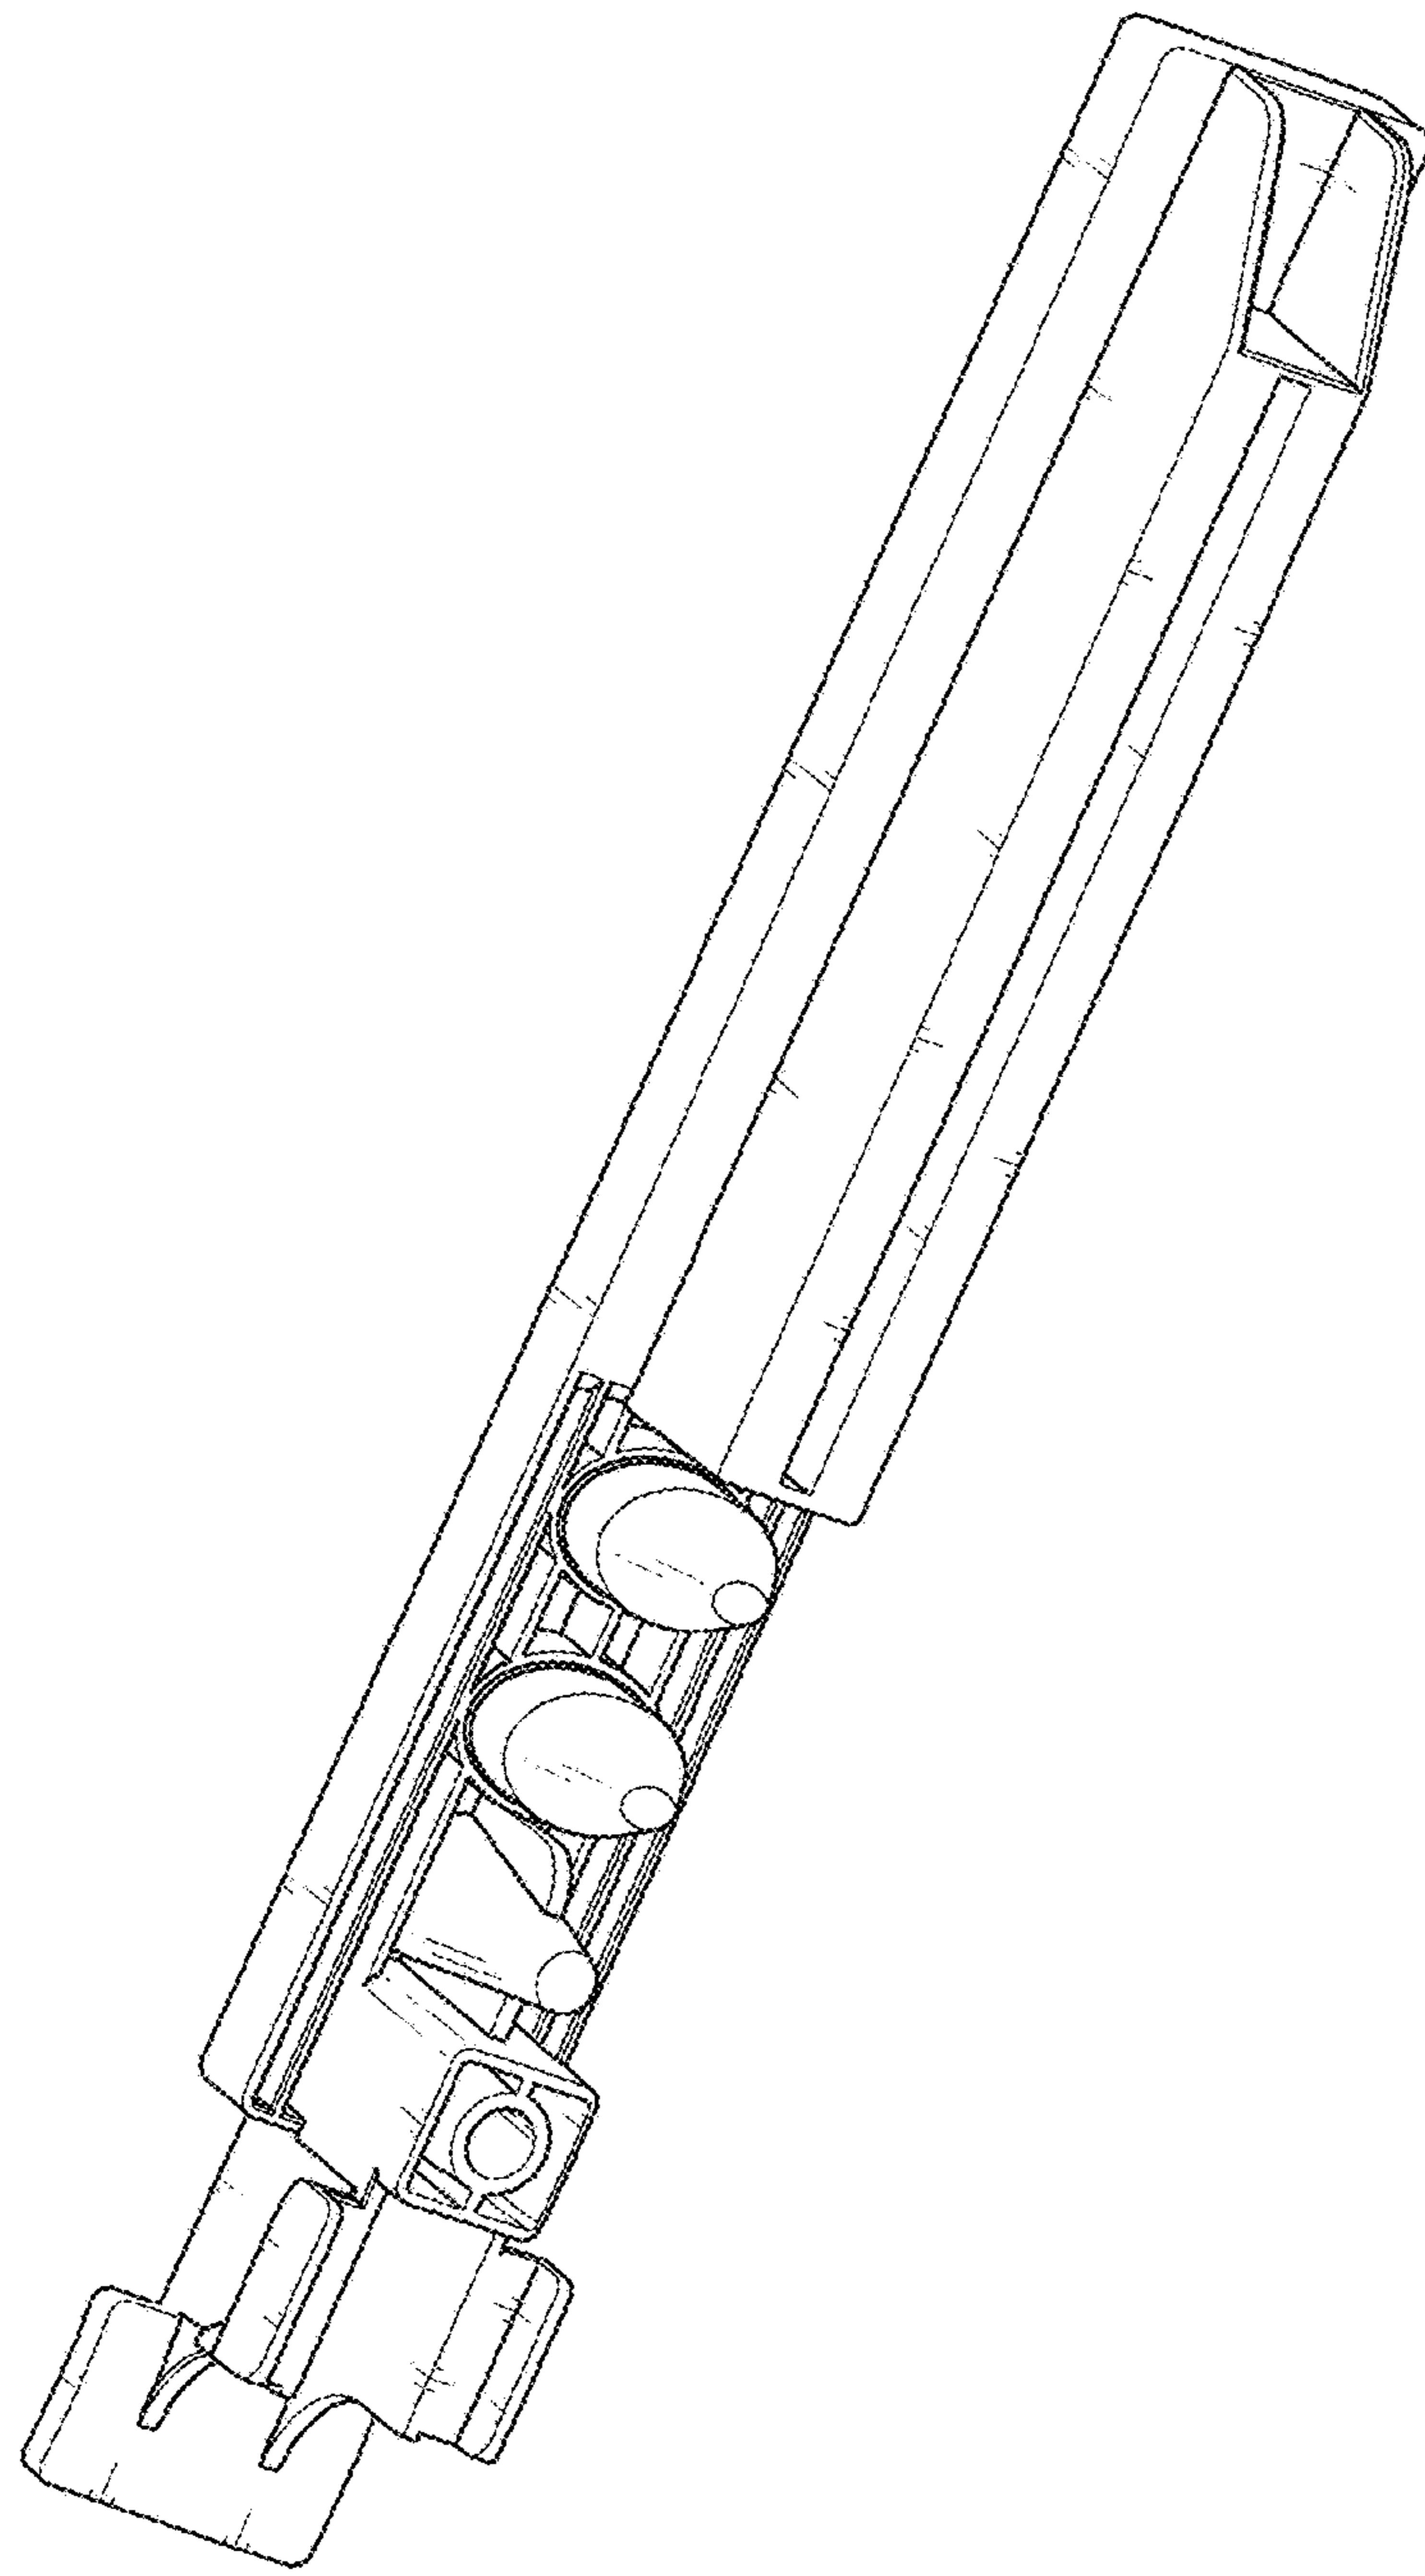


FIG. 9

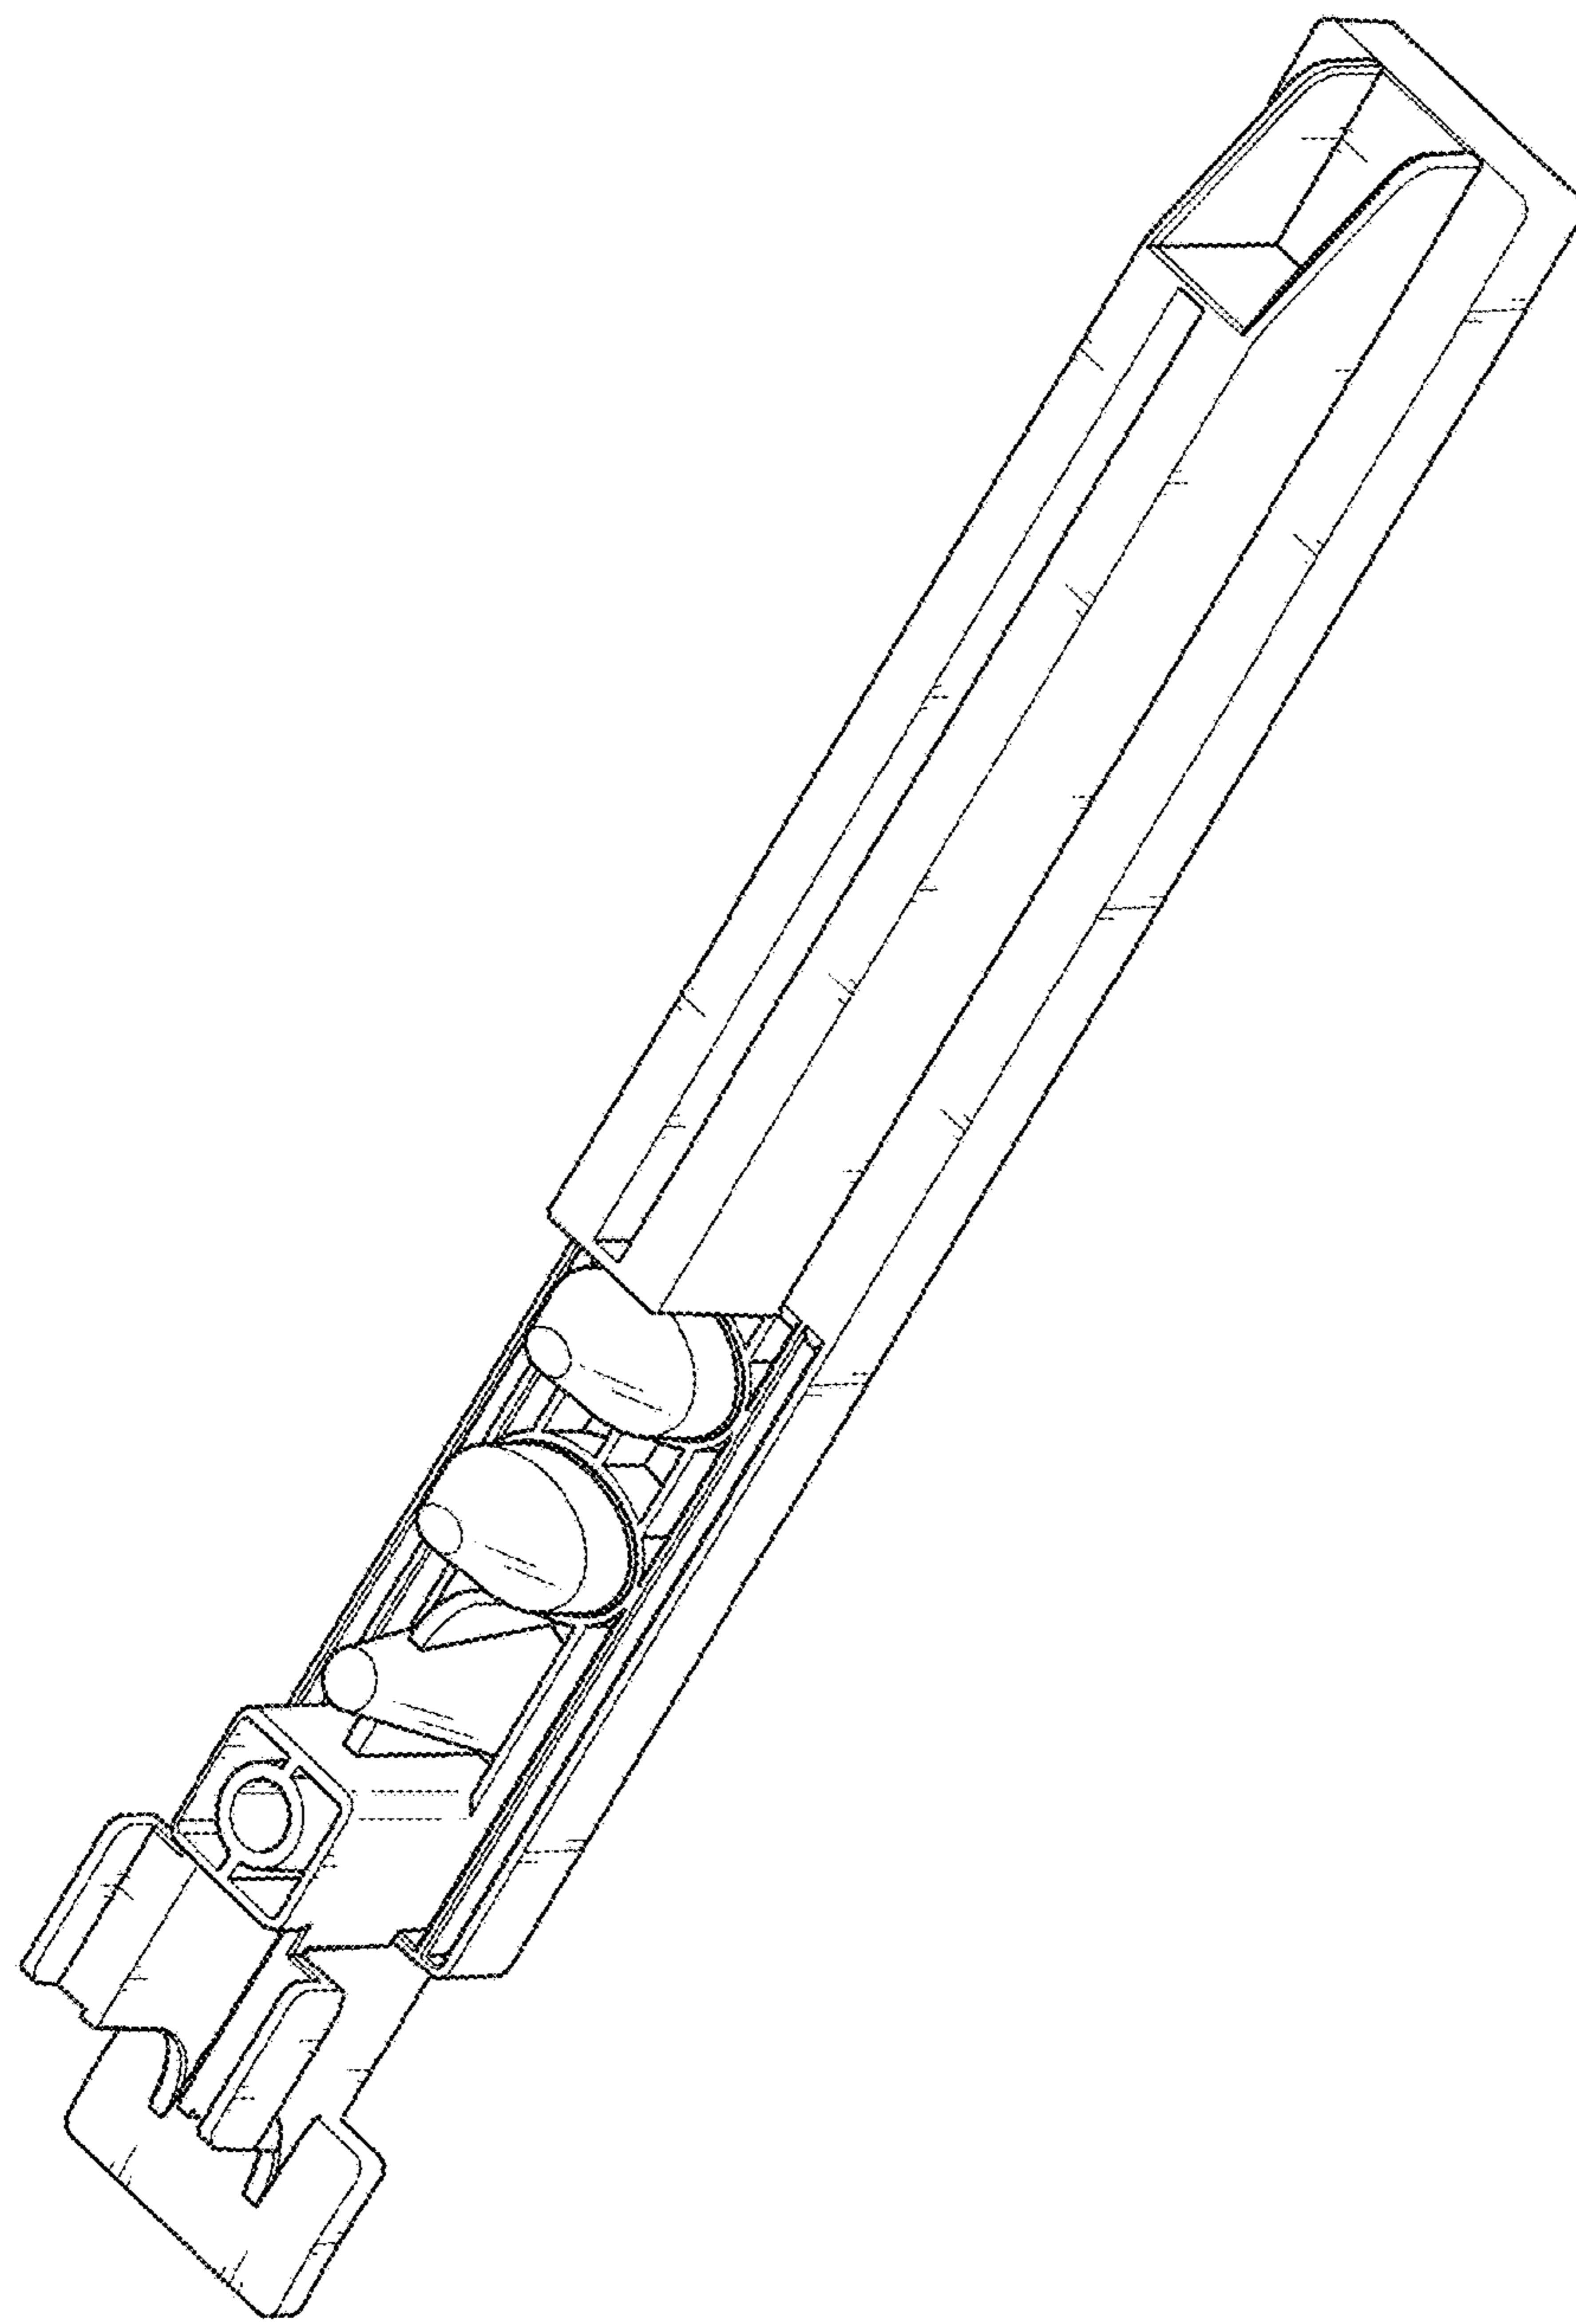


FIG. 10