



US00D822343S

(12) **United States Design Patent**
Nabbout

(10) **Patent No.:** **US D822,343 S**
(45) **Date of Patent:** **** Jul. 10, 2018**

- (54) **HOSPITAL GOWN**
- (71) Applicant: **Karine Nabbout**, Andover, MA (US)
- (72) Inventor: **Karine Nabbout**, Andover, MA (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/598,472**
- (22) Filed: **Mar. 27, 2017**
- (51) **LOC (11) Cl.** **02-01**
- (52) **U.S. Cl.**
USPC **D2/720**
- (58) **Field of Classification Search**
USPC D2/720, 718, 717, 739, 797, 840, 841,
D2/844, 847-850
CPC A41D 13/12; A41D 13/1209; A41D
13/1236; A41D 13/1245
See application file for complete search history.

- D622,479 S * 8/2010 Herzog D2/720
- D624,280 S * 9/2010 Halseth D2/720
- D636,558 S * 4/2011 Shelton D2/720
- 8,069,497 B2 12/2011 Sheward
- 8,286,263 B2 10/2012 Sampson-Howlett
- D687,209 S * 8/2013 Levine D2/720
- D688,847 S * 9/2013 Isaacs D2/720
- D707,919 S * 7/2014 Lockwood D2/720
- 8,821,461 B2 9/2014 Kovensky
- D721,869 S * 2/2015 Bernier D2/720
- D721,870 S * 2/2015 Levine D2/720
- 8,990,966 B2 3/2015 Von Furstenberg et al.
- D738,591 S * 9/2015 Criss D2/720
- D741,569 S * 10/2015 Fredrickson D2/720
- 9,179,716 B2 11/2015 Forbes et al.
- D752,318 S * 3/2016 Powell D2/720
- D760,474 S * 7/2016 Alonzo D2/720
- D767,252 S * 9/2016 Antons D2/720
- D788,403 S * 6/2017 Medeiros D2/720
- D802,884 S * 11/2017 Bennett D2/739
- 2014/0082823 A1 3/2014 Gordon et al.
- 2014/0123362 A1* 5/2014 Seitz A41D 7/008
2/69
- 2014/0189931 A1 7/2014 Fredrickson

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 1,877,697 A * 9/1932 Schlüsselberg A41F 9/007
2/312
- 1,905,685 A * 4/1933 Safir A41D 10/00
2/274
- 3,369,256 A * 2/1968 Kern A41D 13/1236
2/114
- 4,864,657 A * 9/1989 Lake A41D 13/1236
2/114
- D336,968 S * 7/1993 Russano D2/720
- D431,344 S * 10/2000 Briceno D2/720
- D463,093 S * 9/2002 Murray D2/720
- 6,484,321 B1 11/2002 Shamam
- D530,885 S * 10/2006 Barthel D2/720
- D547,927 S * 8/2007 Booth D2/720
- 7,305,716 B1 12/2007 Richards
- D574,126 S * 8/2008 McCray D2/720

* cited by examiner

Primary Examiner — George D. Kirschbaum

Assistant Examiner — Clese Moore, Jr.


(57) **CLAIM**

The ornamental design for the “hospital gown”, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of my “hospital gown”, thereof; and,
FIG. 2 is a rear elevational view of my “hospital gown”, thereof.

1 Claim, 2 Drawing Sheets

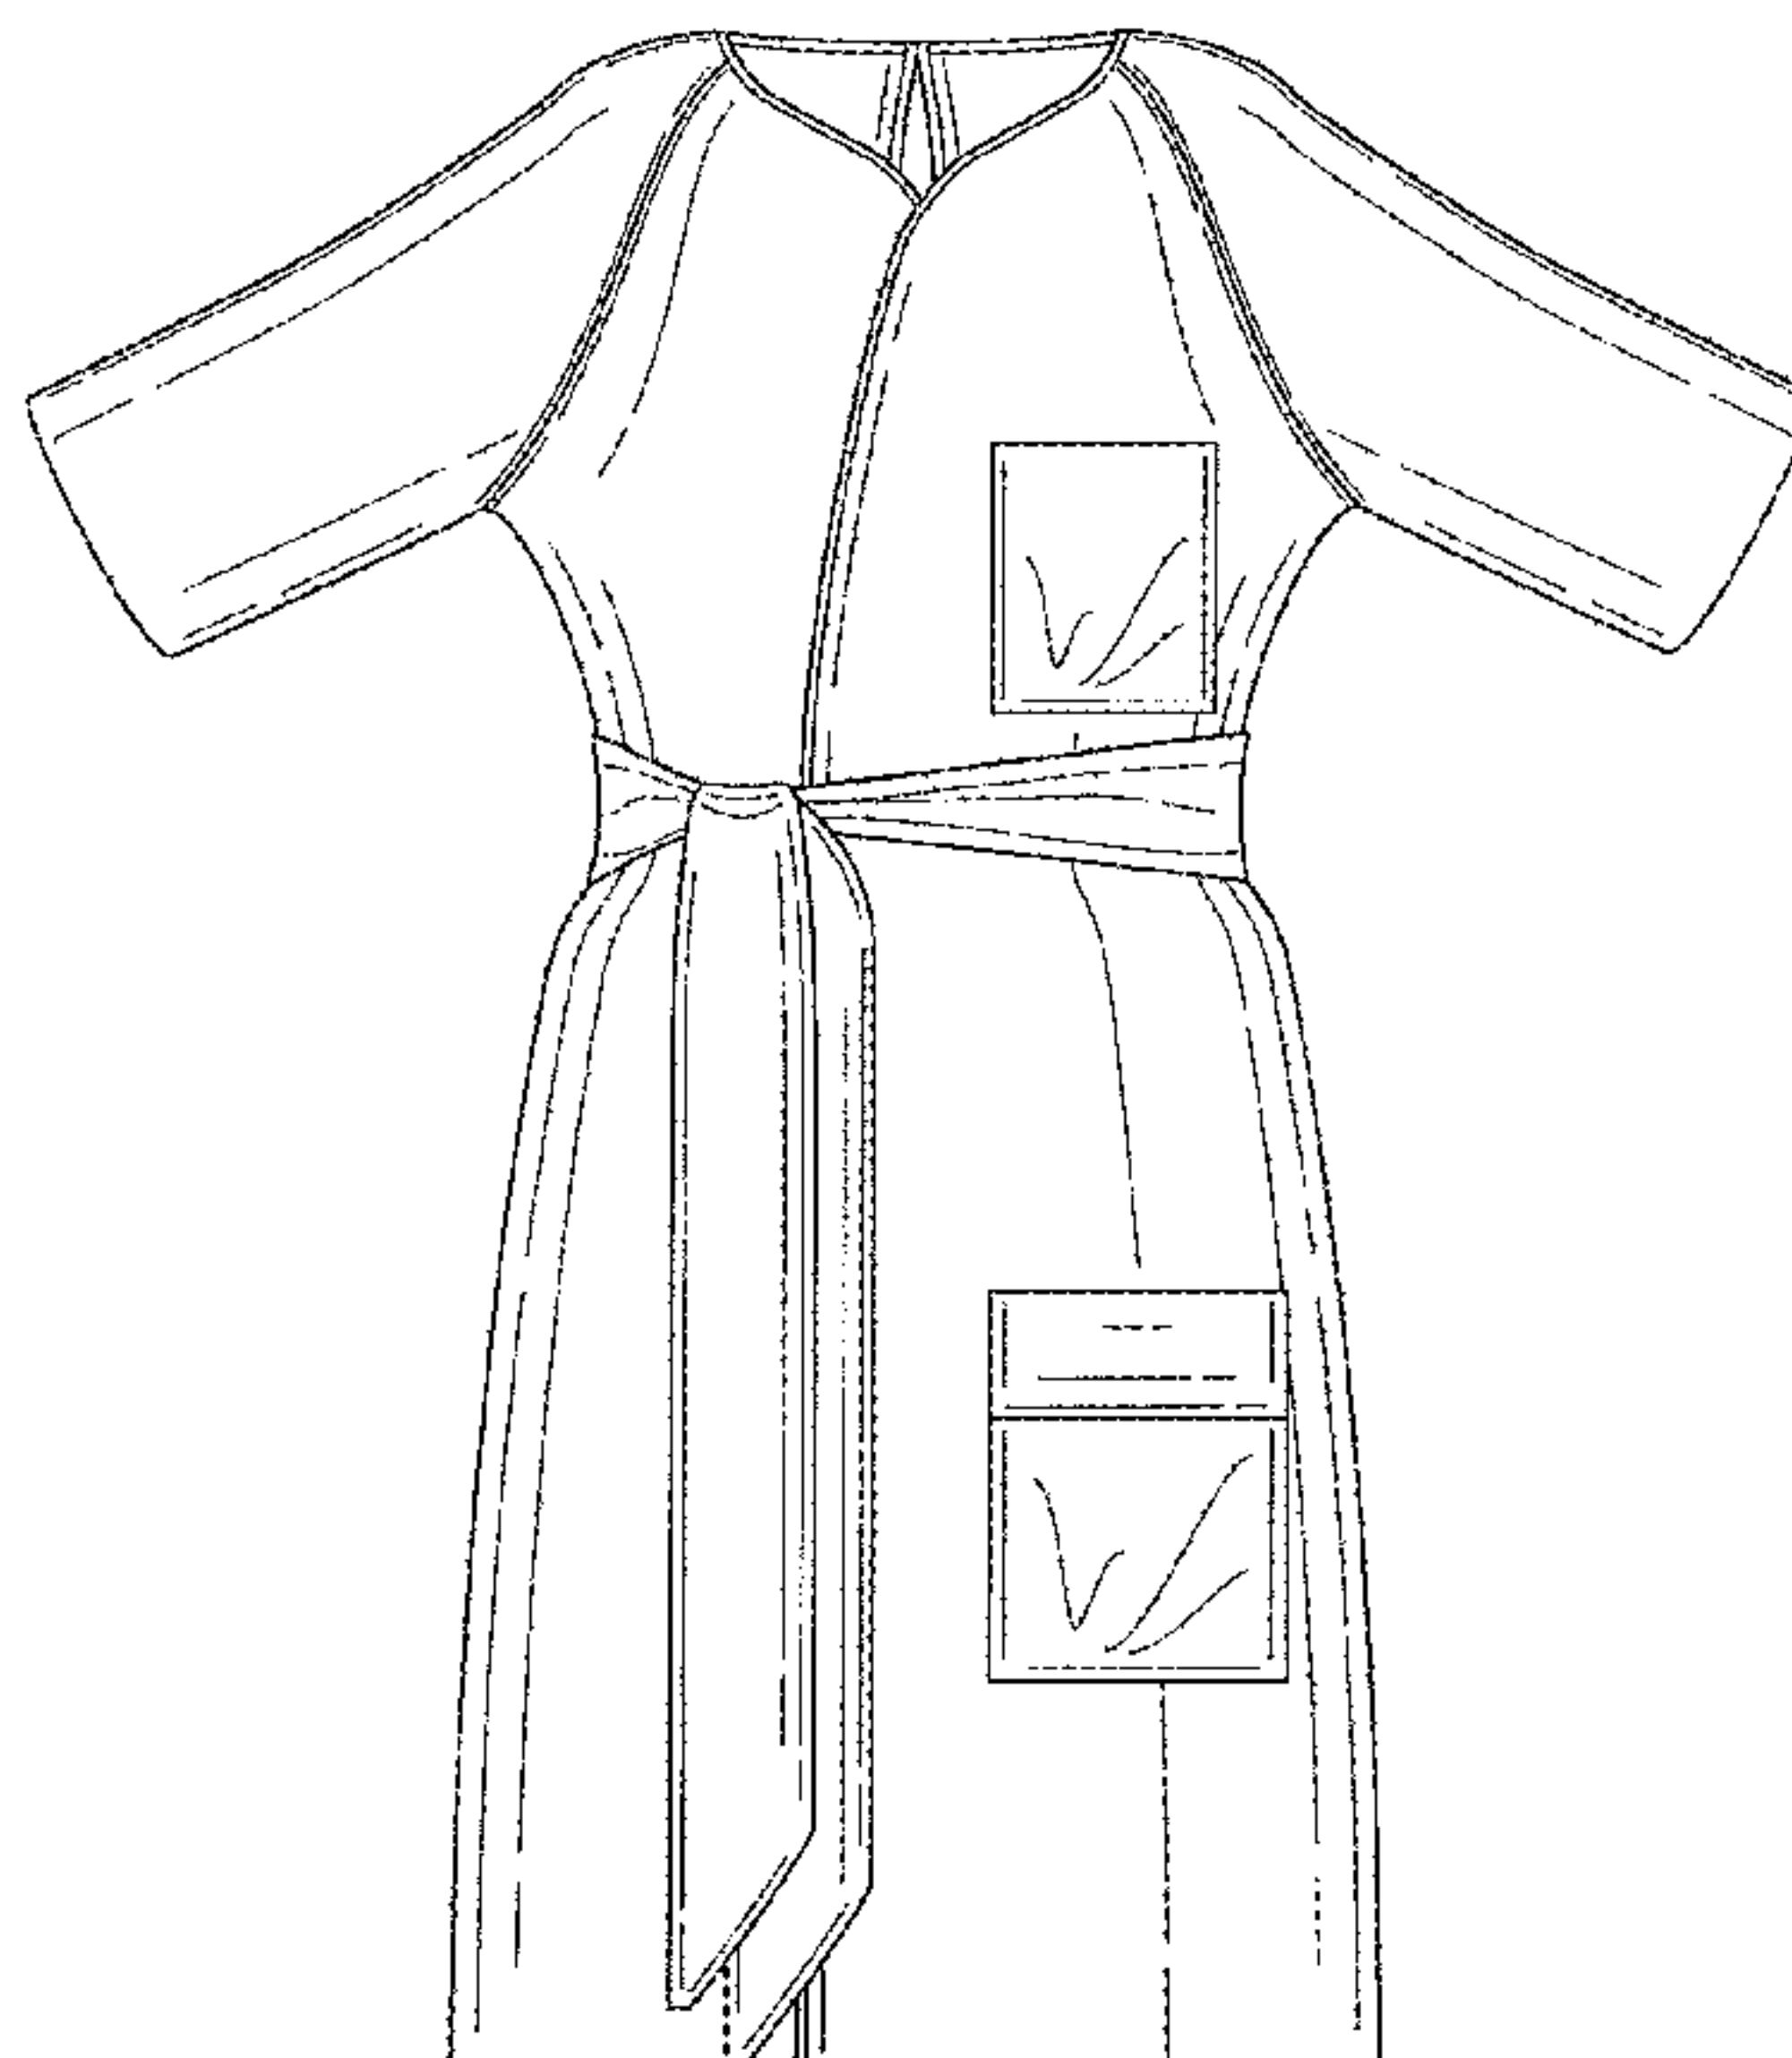

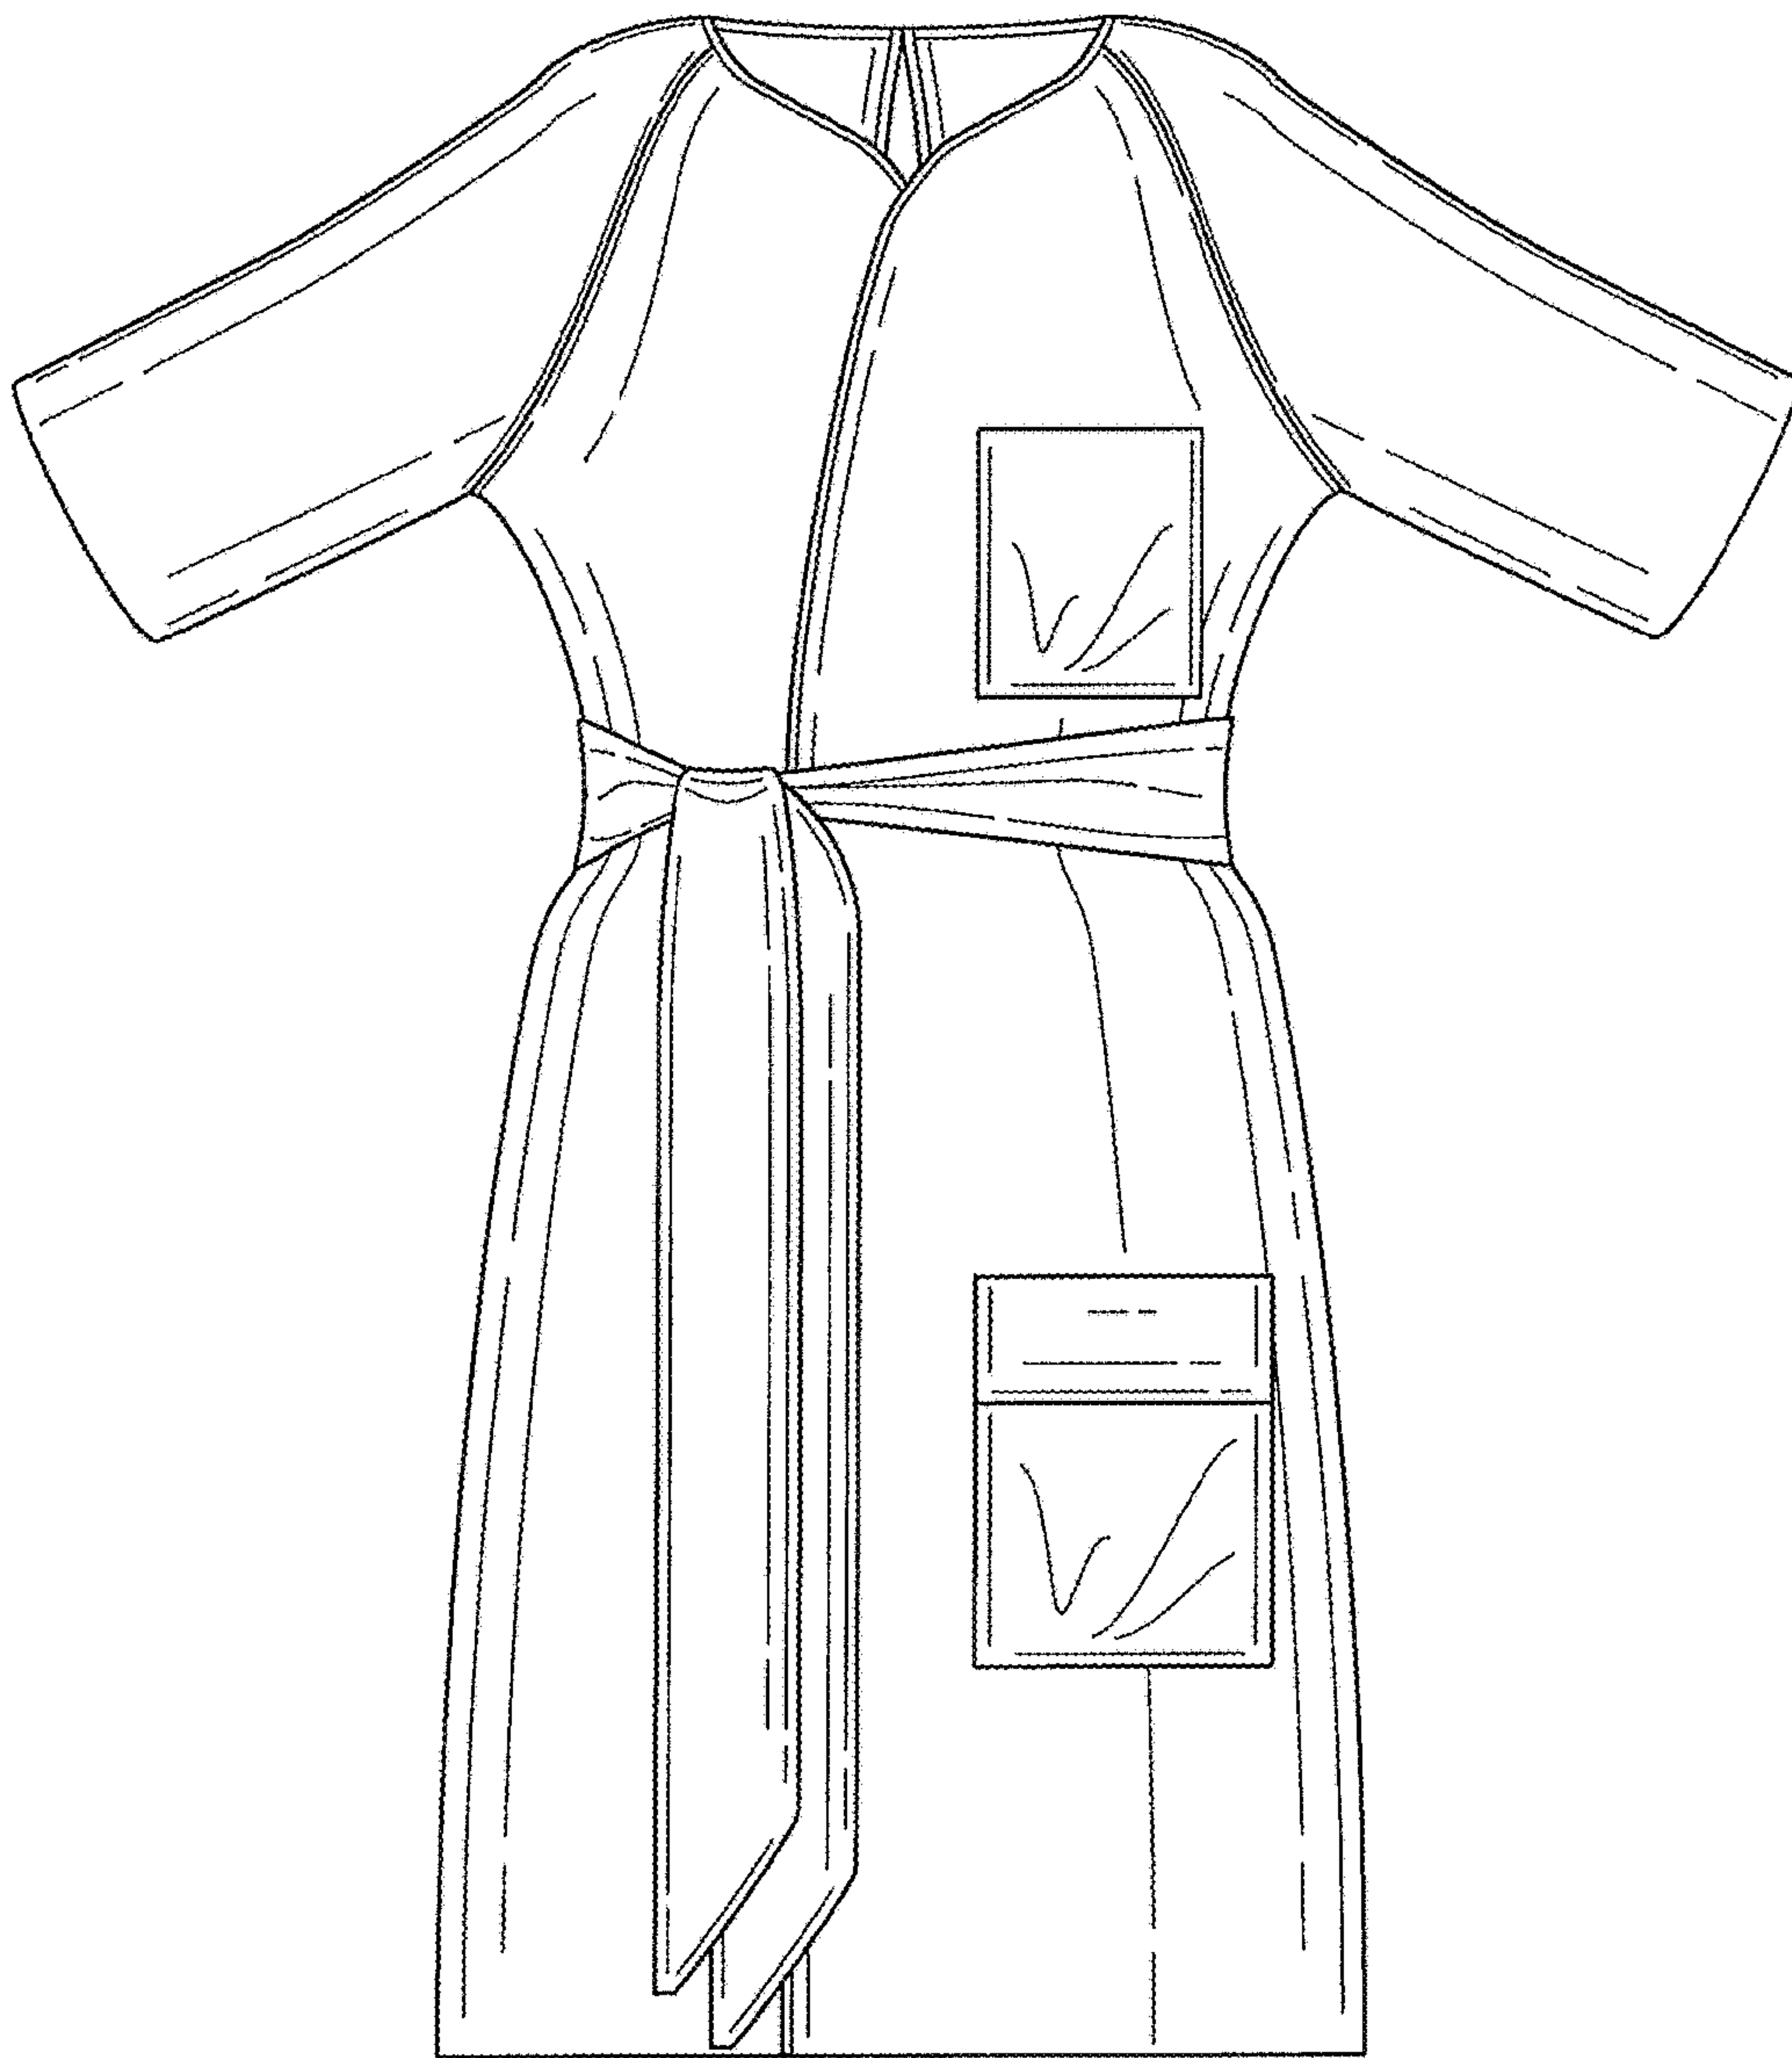


FIG. 1

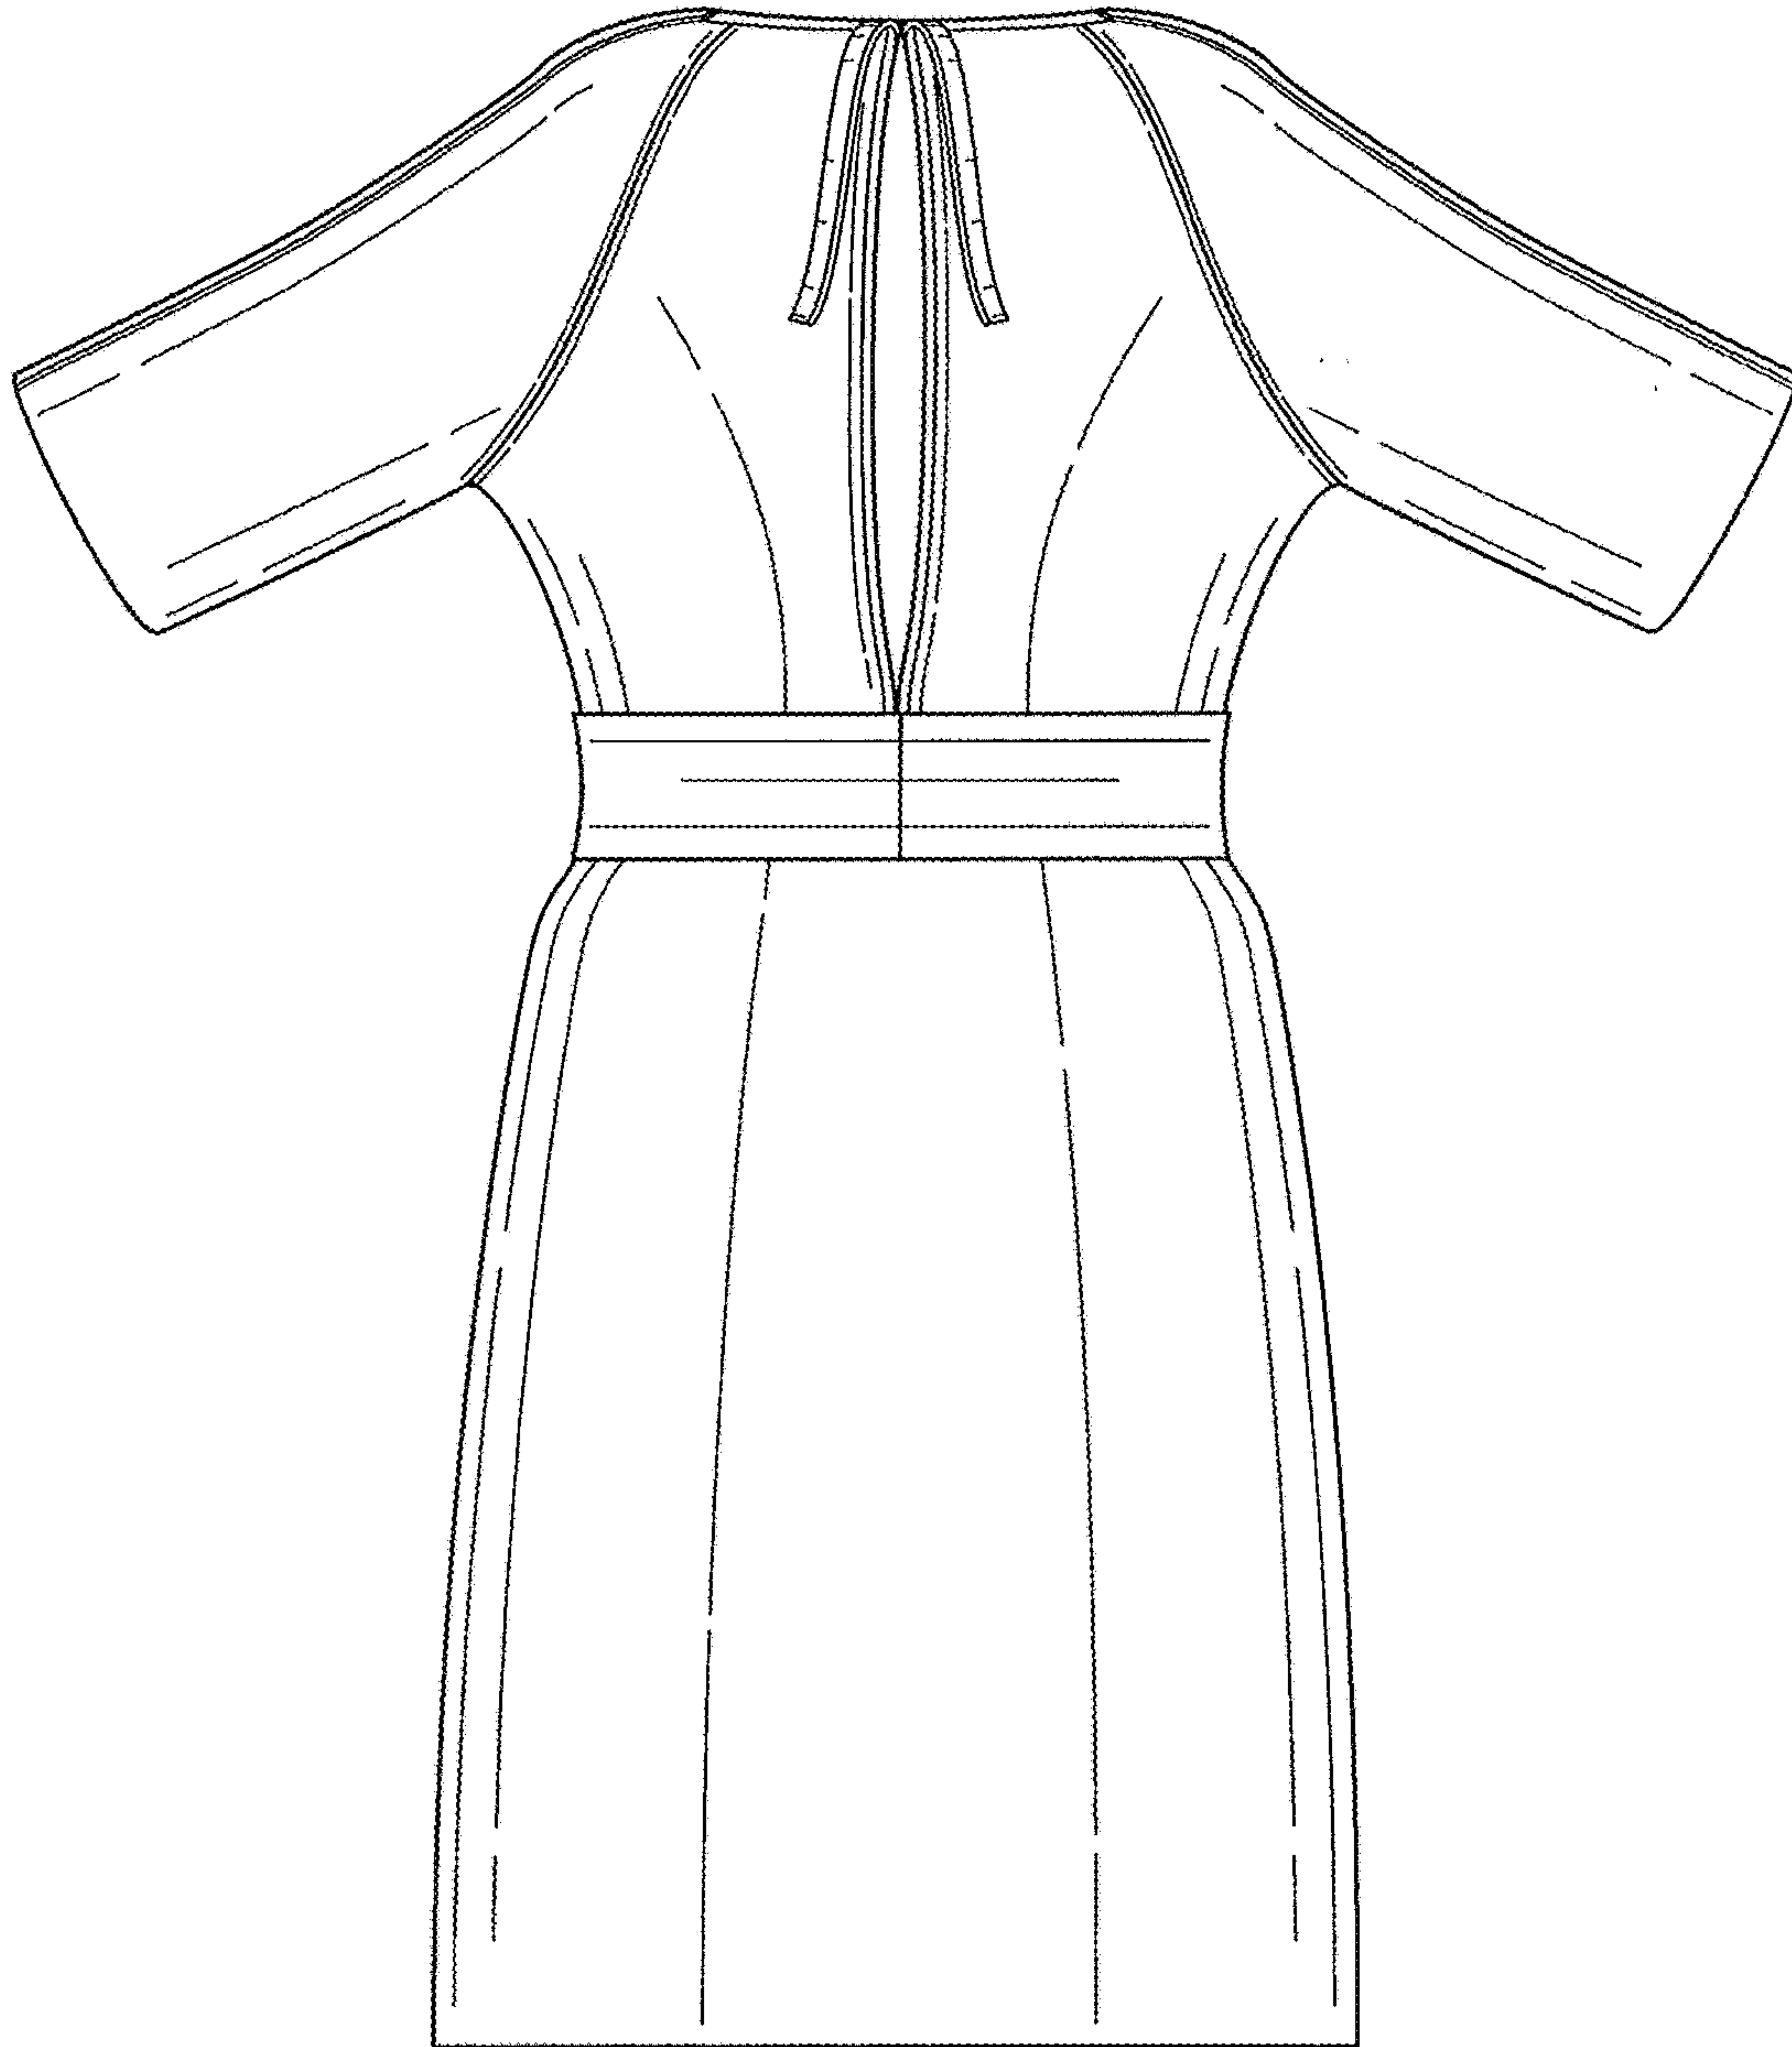


FIG. 2

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D822,343 S
APPLICATION NO. : 29/598472
DATED : June 7, 2016
INVENTOR(S) : Nabbout et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page


Item (72) Inventors, should read:

--Karln Nabbout, Andover, MA (US);

Michael E. Nabbout, Andover, MA (US);

Charles S. Nabbout, Andover, MA (US).--

Signed and Sealed this
Ninth Day of July, 2019

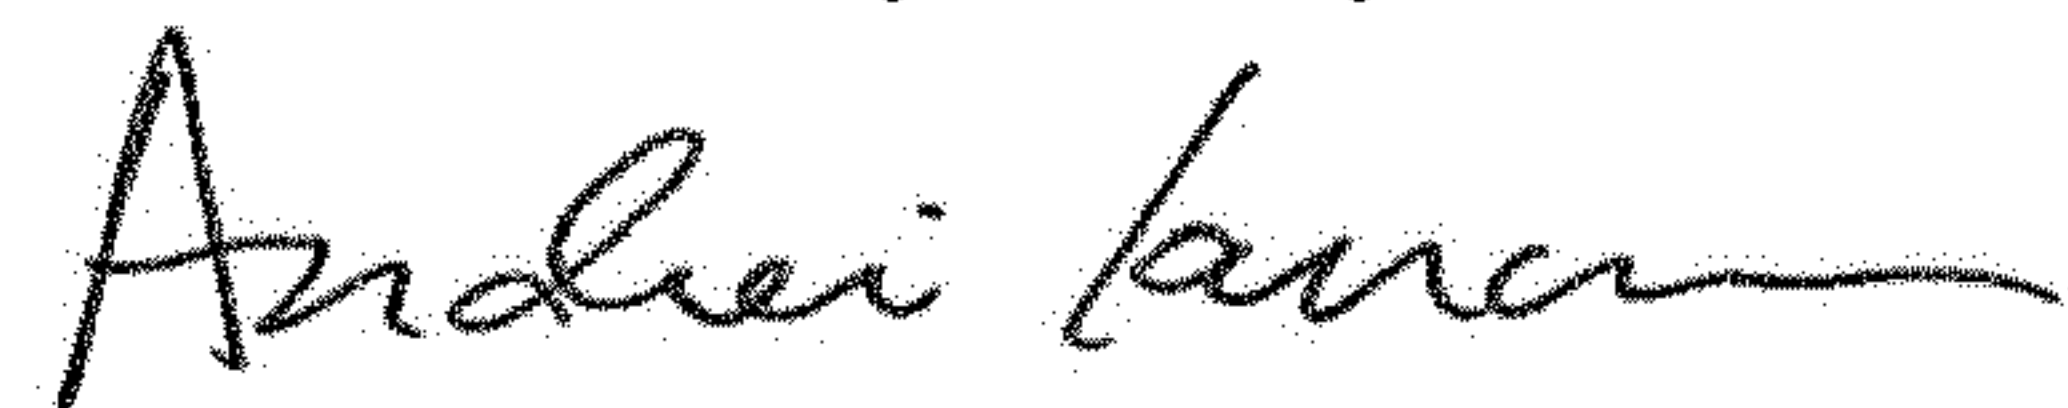

Andrei Iancu
Director of the United States Patent and Trademark Office