



US00D822830S

(12) **United States Design Patent** (10) **Patent No.:** **US D822,830 S**  
**Aten et al.** (45) **Date of Patent:** **\*\* Jul. 10, 2018**

(54) **CATHETER RETENTION DEVICE**  
(71) Applicant: **Arkis BioSciences Inc.**, Knoxville, TN (US)  
(72) Inventors: **Quentin T. Aten**, Knoxville, TN (US); **Ishan D. Gaud**, Knoxville, TN (US)  
(73) Assignee: **Arkis BioSciences Inc.**, Knoxville, TN (US)

D331,462 S \* 12/1992 Kraus ..... D24/143  
5,183,464 A 2/1993 Dubrul et al.  
5,356,390 A 10/1994 Erskine et al.  
(Continued)

**FOREIGN PATENT DOCUMENTS**

DE 69633411 T2 10/2005  
WO 1999052481 A1 10/1999  
(Continued)

**OTHER PUBLICATIONS**

Asico.com, Akahoshi Curved Ball I/A Tip, video dated Jun. 2013, online product page and demo video, retrieved Sep. 24, 2017 from <URL:http://www.asico.com/products/cannula/i-a/akahoshi-curved-ball-i-a-tip.html#.WceAU\_krlb9> (Year:2013).  
(Continued)

*Primary Examiner* — David Muller  
*Assistant Examiner* — Nathan Johnston  
(74) *Attorney, Agent, or Firm* — Meunier Carlin & Curfman LLC

(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/601,262**  
(22) Filed: **Apr. 20, 2017**  
(51) **LOC (11) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/128**  
(58) **Field of Classification Search**  
USPC ..... D24/128, 129, 112–114, 130, 127, 104, D24/133, 186, 108; 606/181, 185; 604/264, 272, 115, 164.01–164.09, 533, 604/232, 187, 168.01, 192, 19, 48, 93.01, 604/523, 524, 526; 600/101, 139, 143; 128/200.24, 207.14, 207.15; 601/67  
CPC ..... A61M 25/00; A61M 25/0014; A61M 25/0097; A61M 25/0026  
See application file for complete search history.


(57) **CLAIM**  
The ornamental design for a catheter retention device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a catheter retention device showing our new design.  
FIG. 2 is a rear perspective view thereof.  
FIG. 3 is a front view thereof.  
FIG. 4 is a rear view thereof.  
FIG. 5 is a left-side view thereof.  
FIG. 6 is a right-side view thereof.  
FIG. 7 is a rear view thereof; and,  
FIG. 8 is a top view thereof; and,  
FIG. 9 is a perspective view of our design in use.  
The broken lines are shown for environmental purposes only and form no part of the claimed design.

(56) **References Cited**  
U.S. PATENT DOCUMENTS  
4,149,535 A 4/1979 Volder et al.  
D257,567 S 11/1980 Peacock  
D263,445 S 3/1982 Gordin  
4,318,401 A 3/1982 Zimmerman  
4,464,178 A 8/1984 Dalton  
4,475,898 A 10/1984 Brodner et al.  
4,631,051 A 12/1986 Harris et al.  
4,846,186 A 7/1989 Box et al.  
4,950,232 A 8/1990 Ruzicka et al.

**1 Claim, 9 Drawing Sheets**

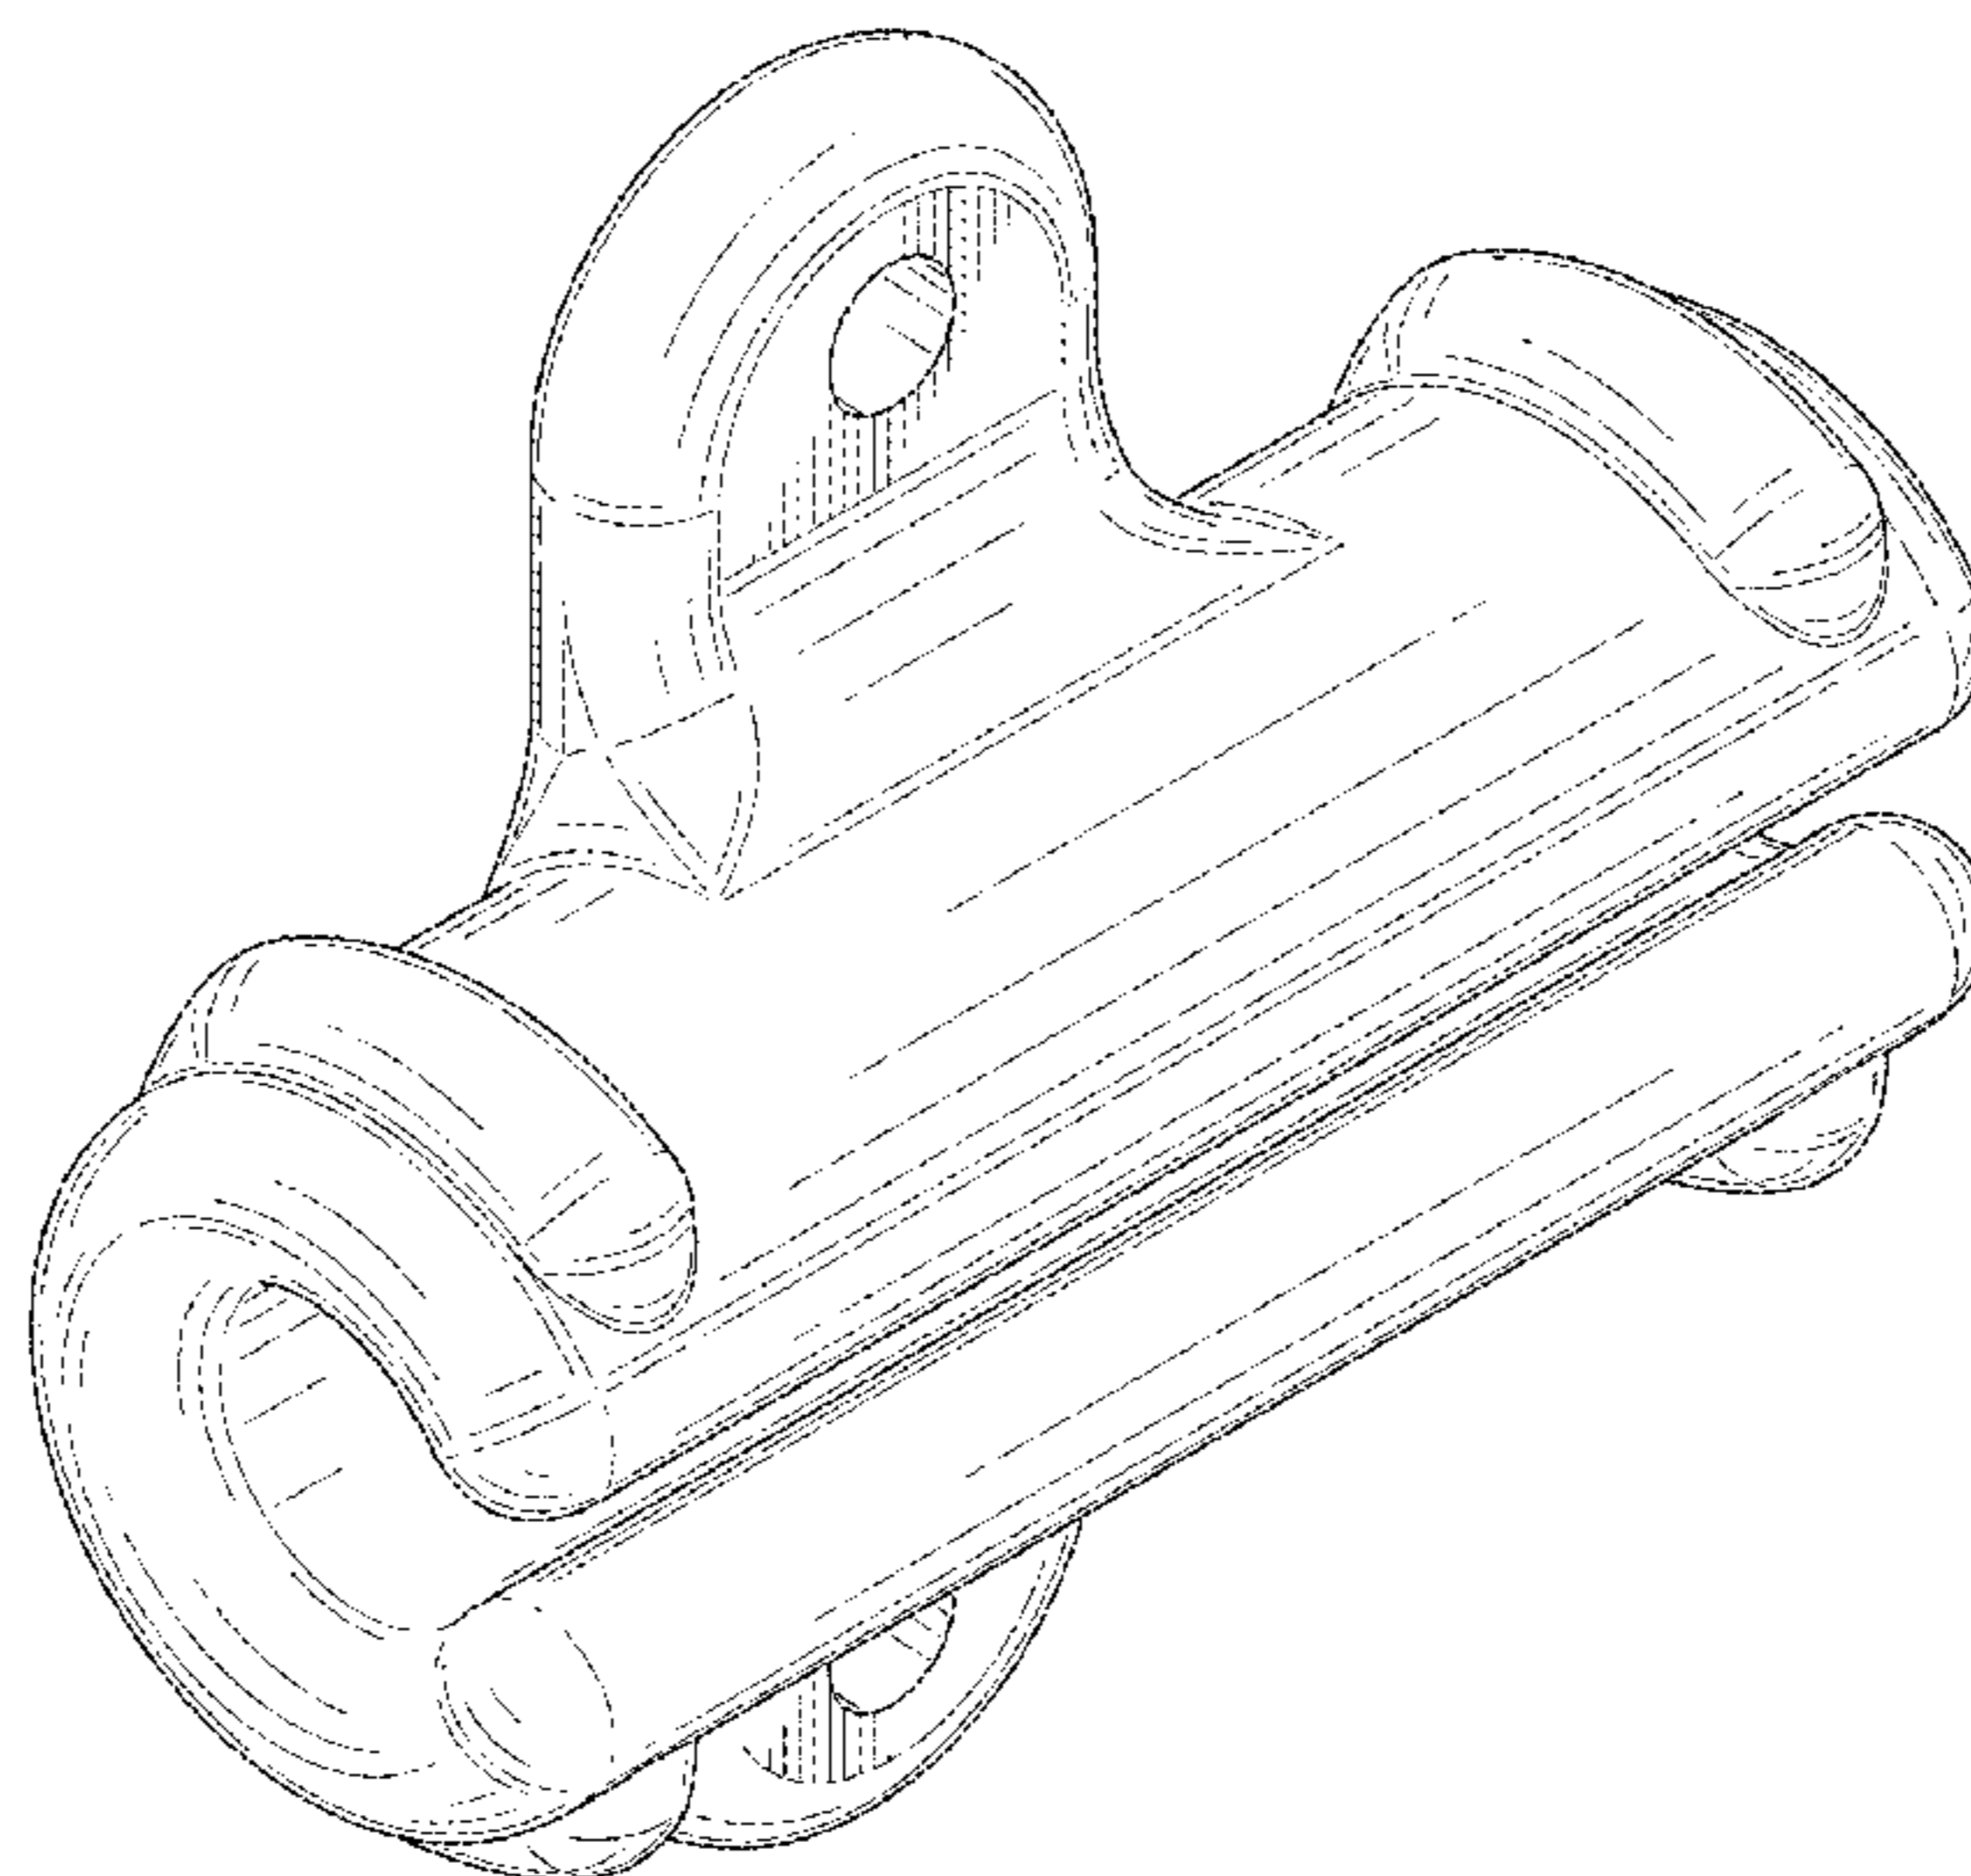

(56)

References Cited

U.S. PATENT DOCUMENTS

5,370,640 A 12/1994 Kolff  
 5,385,541 A 1/1995 Kirsch et al.  
 D356,161 S \* 3/1995 Peterson ..... D24/199  
 5,398,679 A \* 3/1995 Freed ..... A61M 16/0488  
 128/207.17  
 D383,968 S \* 9/1997 Bidwell ..... D8/356  
 5,704,352 A 1/1998 Buckles et al.  
 5,762,615 A 6/1998 Weier et al.  
 5,916,193 A 6/1999 Stevens et al.  
 5,944,732 A 8/1999 Raulerson et al.  
 5,980,504 A 11/1999 Sharkey et al.  
 6,007,510 A 12/1999 Nigam et al.  
 6,007,544 A 12/1999 Kim  
 6,197,041 B1 3/2001 Shichman et al.  
 6,267,769 B1 7/2001 Truwit et al.  
 6,655,386 B1 12/2003 Makower et al.  
 6,902,547 B2 6/2005 Aves et al.  
 7,134,438 B2 11/2006 Makower et al.  
 7,189,222 B2 3/2007 Elsberry et al.  
 D547,865 S \* 7/2007 Schoellhorn ..... D24/135  
 D557,410 S \* 12/2007 Guney ..... D24/110.1  
 D557,802 S \* 12/2007 Miceli, Jr. .... D24/110.6  
 7,678,100 B2 3/2010 Chin et al.  
 D614,289 S \* 4/2010 Veliss ..... D24/110.1  
 7,942,826 B1 5/2011 Scholl et al.  
 D640,788 S 6/2011 Appling  
 8,177,772 B2 5/2012 Christensen et al.  
 D672,004 S \* 12/2012 Stracener ..... D22/108  
 8,337,475 B2 12/2012 Smith et al.  
 D679,811 S 4/2013 Hahn  
 D692,133 S 10/2013 Steinwachs  
 D694,406 S 11/2013 Hahn  
 D700,318 S 2/2014 Amoah  
 D706,083 S \* 6/2014 Kyuba ..... D7/620  
 8,768,487 B2 7/2014 Farnan et al.  
 8,784,330 B1 7/2014 Scholl et al.  
 D733,880 S 7/2015 Mueller  
 D744,649 S 12/2015 Brannon  
 D747,636 S \* 1/2016 Maher ..... D8/72  
 D761,961 S 7/2016 Tan  
 D765,245 S 8/2016 Kamal  
 9,427,558 B2 8/2016 Arnott et al.  
 D767,127 S 9/2016 De Beer  
 D771,812 S 11/2016 Shayle  
 D772,411 S 11/2016 Heath  
 D773,664 S 12/2016 Deneui  
 D775,355 S 12/2016 Georgian  
 D775,723 S 1/2017 Rowe  
 D776,277 S 1/2017 Prendergast  
 D778,443 S 2/2017 Brannon  
 D786,433 S 5/2017 Seaver  
 9,682,221 B2 6/2017 Arnott et al.  
 D804,659 S \* 12/2017 Hood ..... D24/128  
 2002/0121282 A1 9/2002 McGuckin et al.  
 2005/0054948 A1 3/2005 Goldenberg  
 2005/0171452 A1 8/2005 Neff et al.  
 2007/0179426 A1 8/2007 Selden et al.

2008/0051721 A1 2/2008 Carter et al.  
 2008/0161843 A1 7/2008 Clague et al.  
 2008/0194993 A1 8/2008 McLaren et al.  
 2008/0262406 A1 10/2008 Wiener et al.  
 2009/0048537 A1 2/2009 Lydon et al.  
 2009/0171367 A1 7/2009 Hardin et al.  
 2010/0179483 A1 \* 7/2010 Wright ..... A61M 5/158  
 604/180  
 2010/0211048 A1 8/2010 Arai et al.  
 2010/0222732 A1 9/2010 Sevrain et al.  
 2013/0267982 A1 10/2013 Seaver et al.


FOREIGN PATENT DOCUMENTS

WO 2007089724 A2 8/2007  
 WO 2013147978 A2 10/2013

OTHER PUBLICATIONS

HomeDepot.com, Klein Tools 200 ft. Multi-Groove Non-Conduc-  
 tive Fiberglass Fish Tape, available on Archive.org Sep. 2015,  
 Retrieved Sep. 24, 2017 from <URL:http://www.homedepot.com/  
 p.Klein-Tools-200-ft-Multi-Groove-Non\_Conductive-Fiberglass-  
 Fish-Tape-560", 59/205595580> (Year: 2015).  
 Hull Anesthesia, CoPilot VL Reusable Stylet, Nov. 2016, online  
 product page, retrieved Sep. 24, 2017 from <URL:https://web.  
 archive.org/web/20160817114051/http://www.hullanesthesia.com/  
 p/982/copilot-vl-reusable-stylet> (Year: 2016).  
 Restriction Requirement issued in co-pending U.S. Appl. No.  
 29/582,461, dated Oct. 16, 2017.  
 Restriction Requirement issued in co-pending U.S. Appl. No.  
 29/582,463, dated Oct. 16, 2017  
 Harrison et al., "Guidewire Stiffness: What's in a Name?," J.  
 Endovasc. Ther., 2011, vol. 18, pp. 797-801.  
 European Supplementary Search Report conducted in European  
 Application No. 15765234.8, dated Nov. 3, 2017.  
 Ex Parte Quayle Action issued in co-pending U.S. Appl. No.  
 29/581,461, dated Feb. 22, 2018 (14 pages).  
 BassPro.com, Offshore Angler 3-1/2" Handy Hook, undated online  
 product page, retrieved Feb. 1, 2018 from <URL:https://www.  
 basspro.com/shop/en/offshore-angler-3-1-2-handly-hook?> (Year:  
 2018).  
 Sandquist, "A Single-Pass Tunneling Technique for CSF Shunting  
 Procedures", Pediatric Neurosurgery, 2003, 39: 254-257.  
 Office Action dated Dec. 31, 2015, issued in U.S. Appl. No.  
 14/660,616.  
 Office Action dated Sep. 27, 2016, issued in U.S. Appl. No.  
 15/237,024.  
 Restriction Requirement dated Jun. 29, 2017, issued in Design U.S.  
 Appl. No. 29/522,886.  
 International Search Report and Written Opinion issued in Interna-  
 tional Application No. PCT/US2015/020979, dated Jun. 26, 2015.  
 International Preliminary Report on Patentability issued in Interna-  
 tional Application No. PCT/US2015/020979, dated Sep. 20, 2016.  
 Notice of Allowance dated Mar. 28, 2017, issued in U.S. Appl. No.  
 29/553,272.

\* cited by examiner

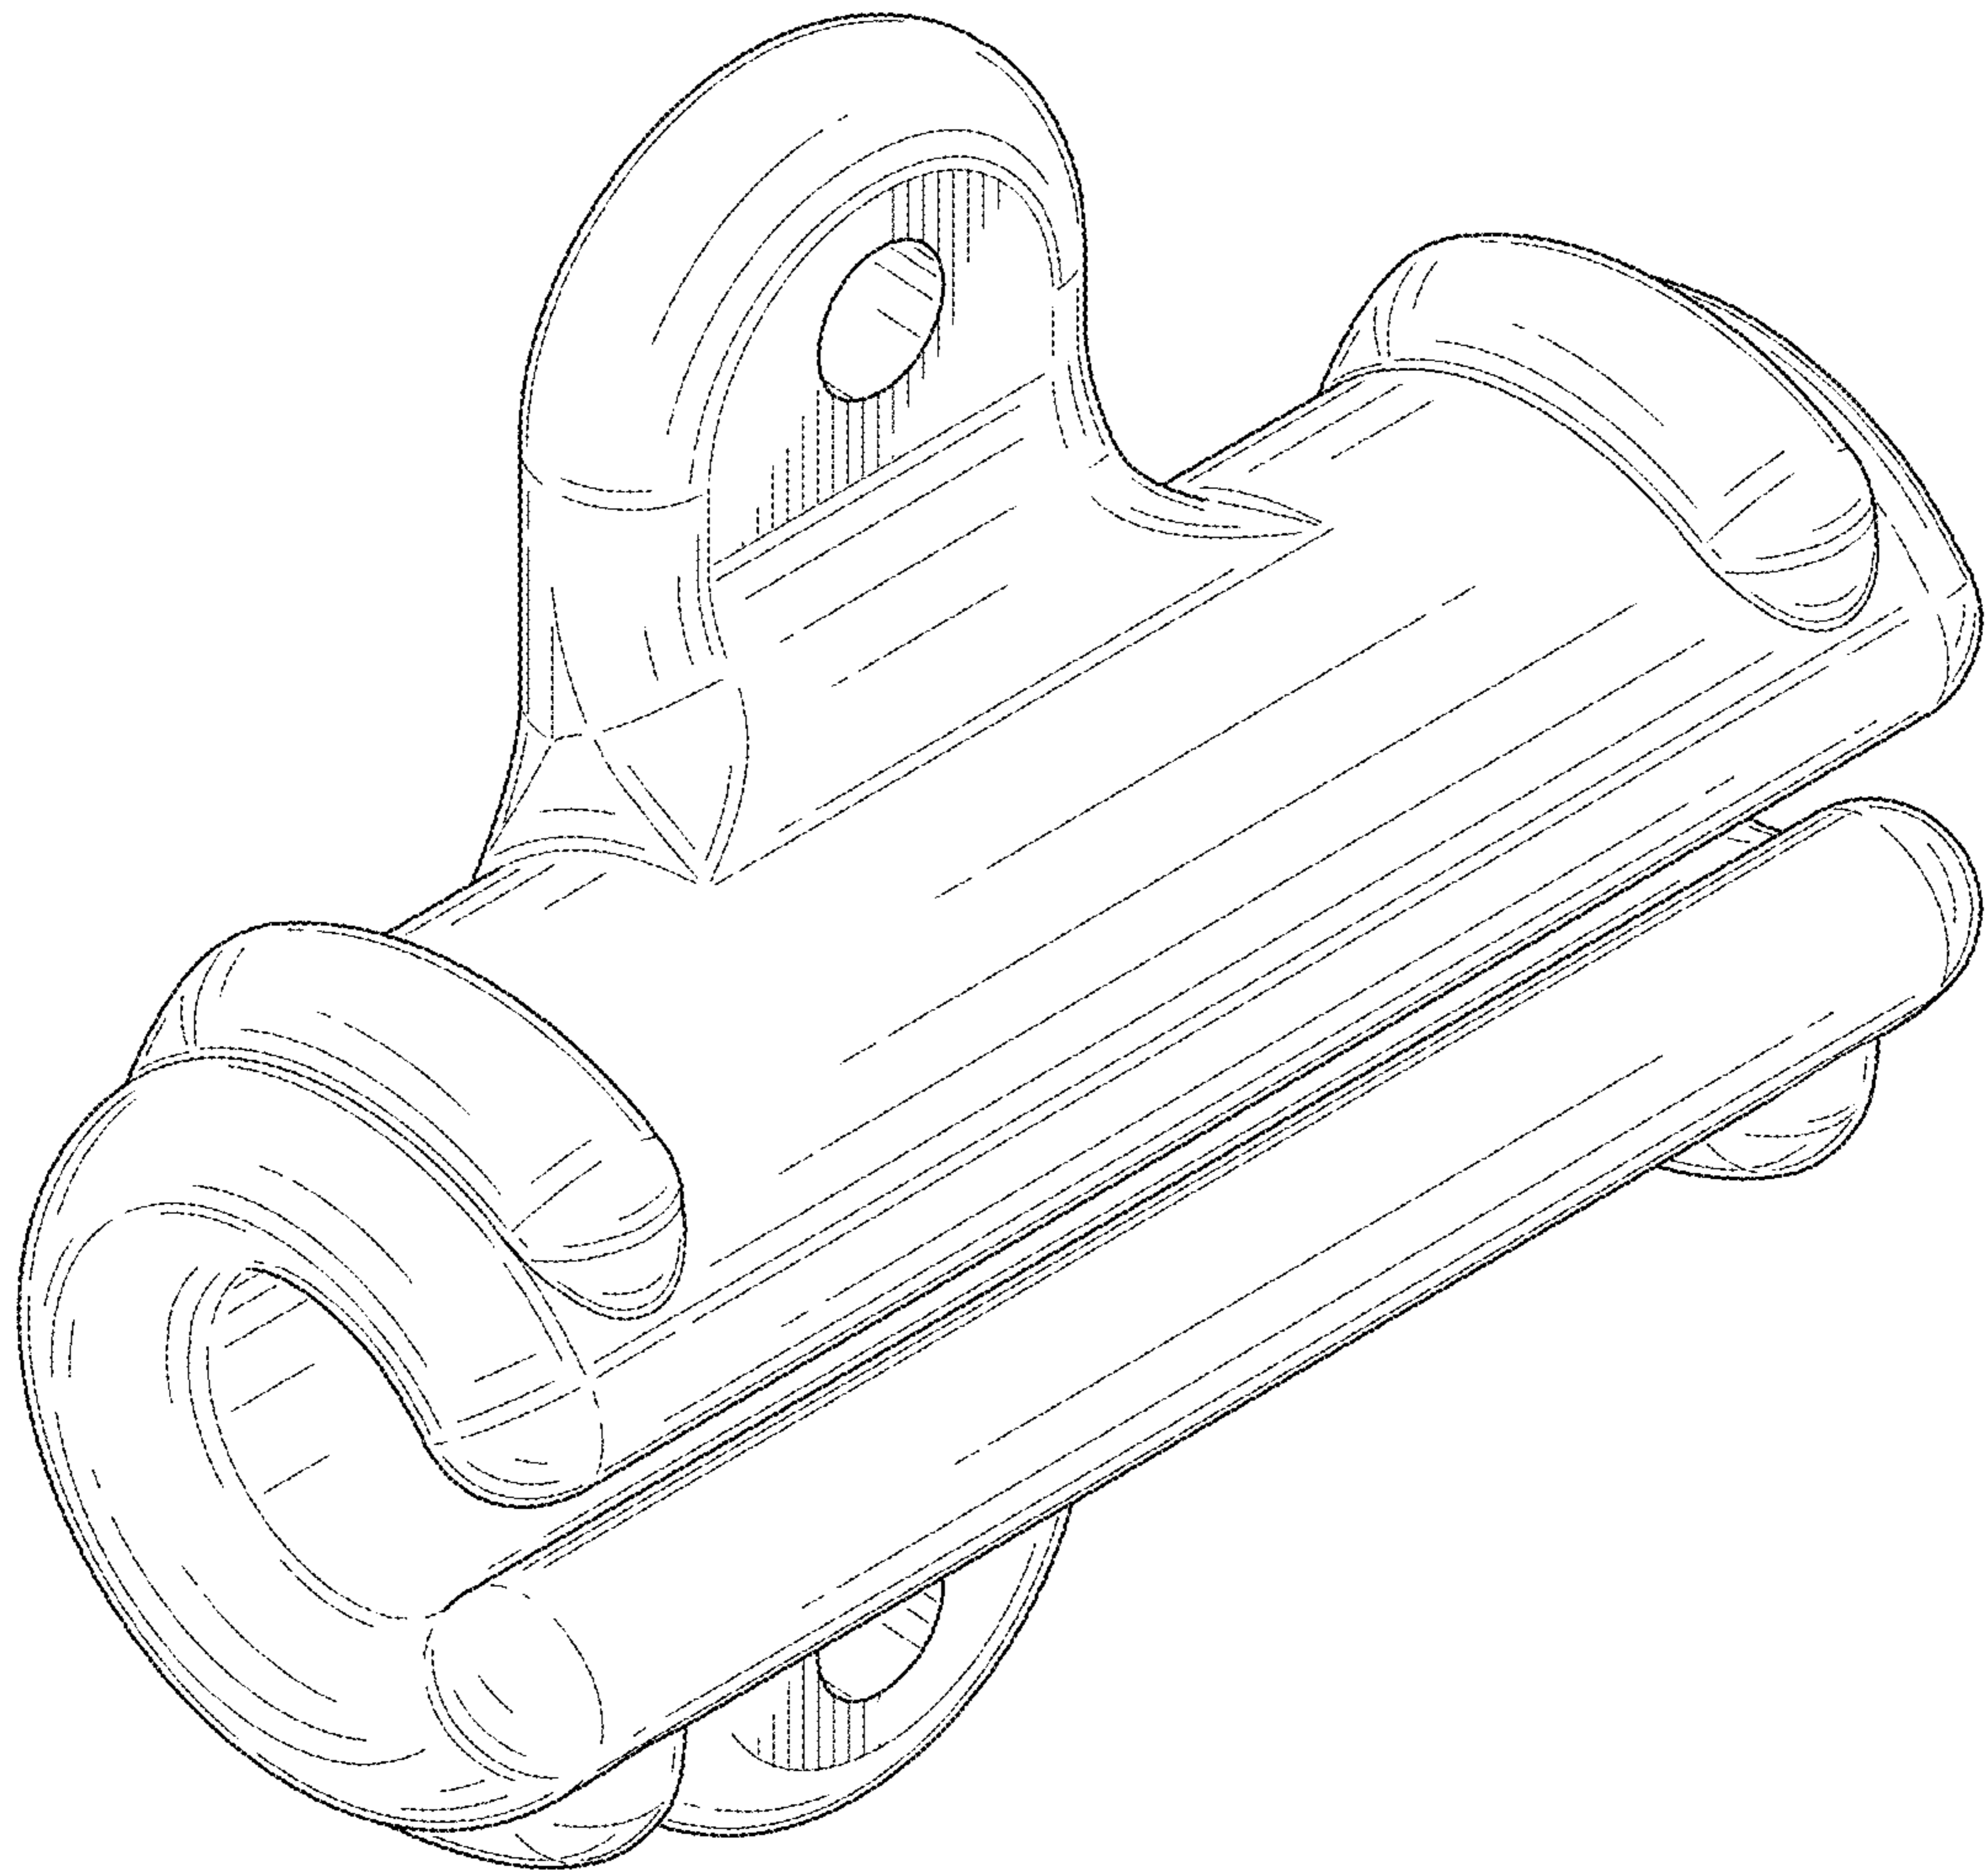

**FIG. 1**

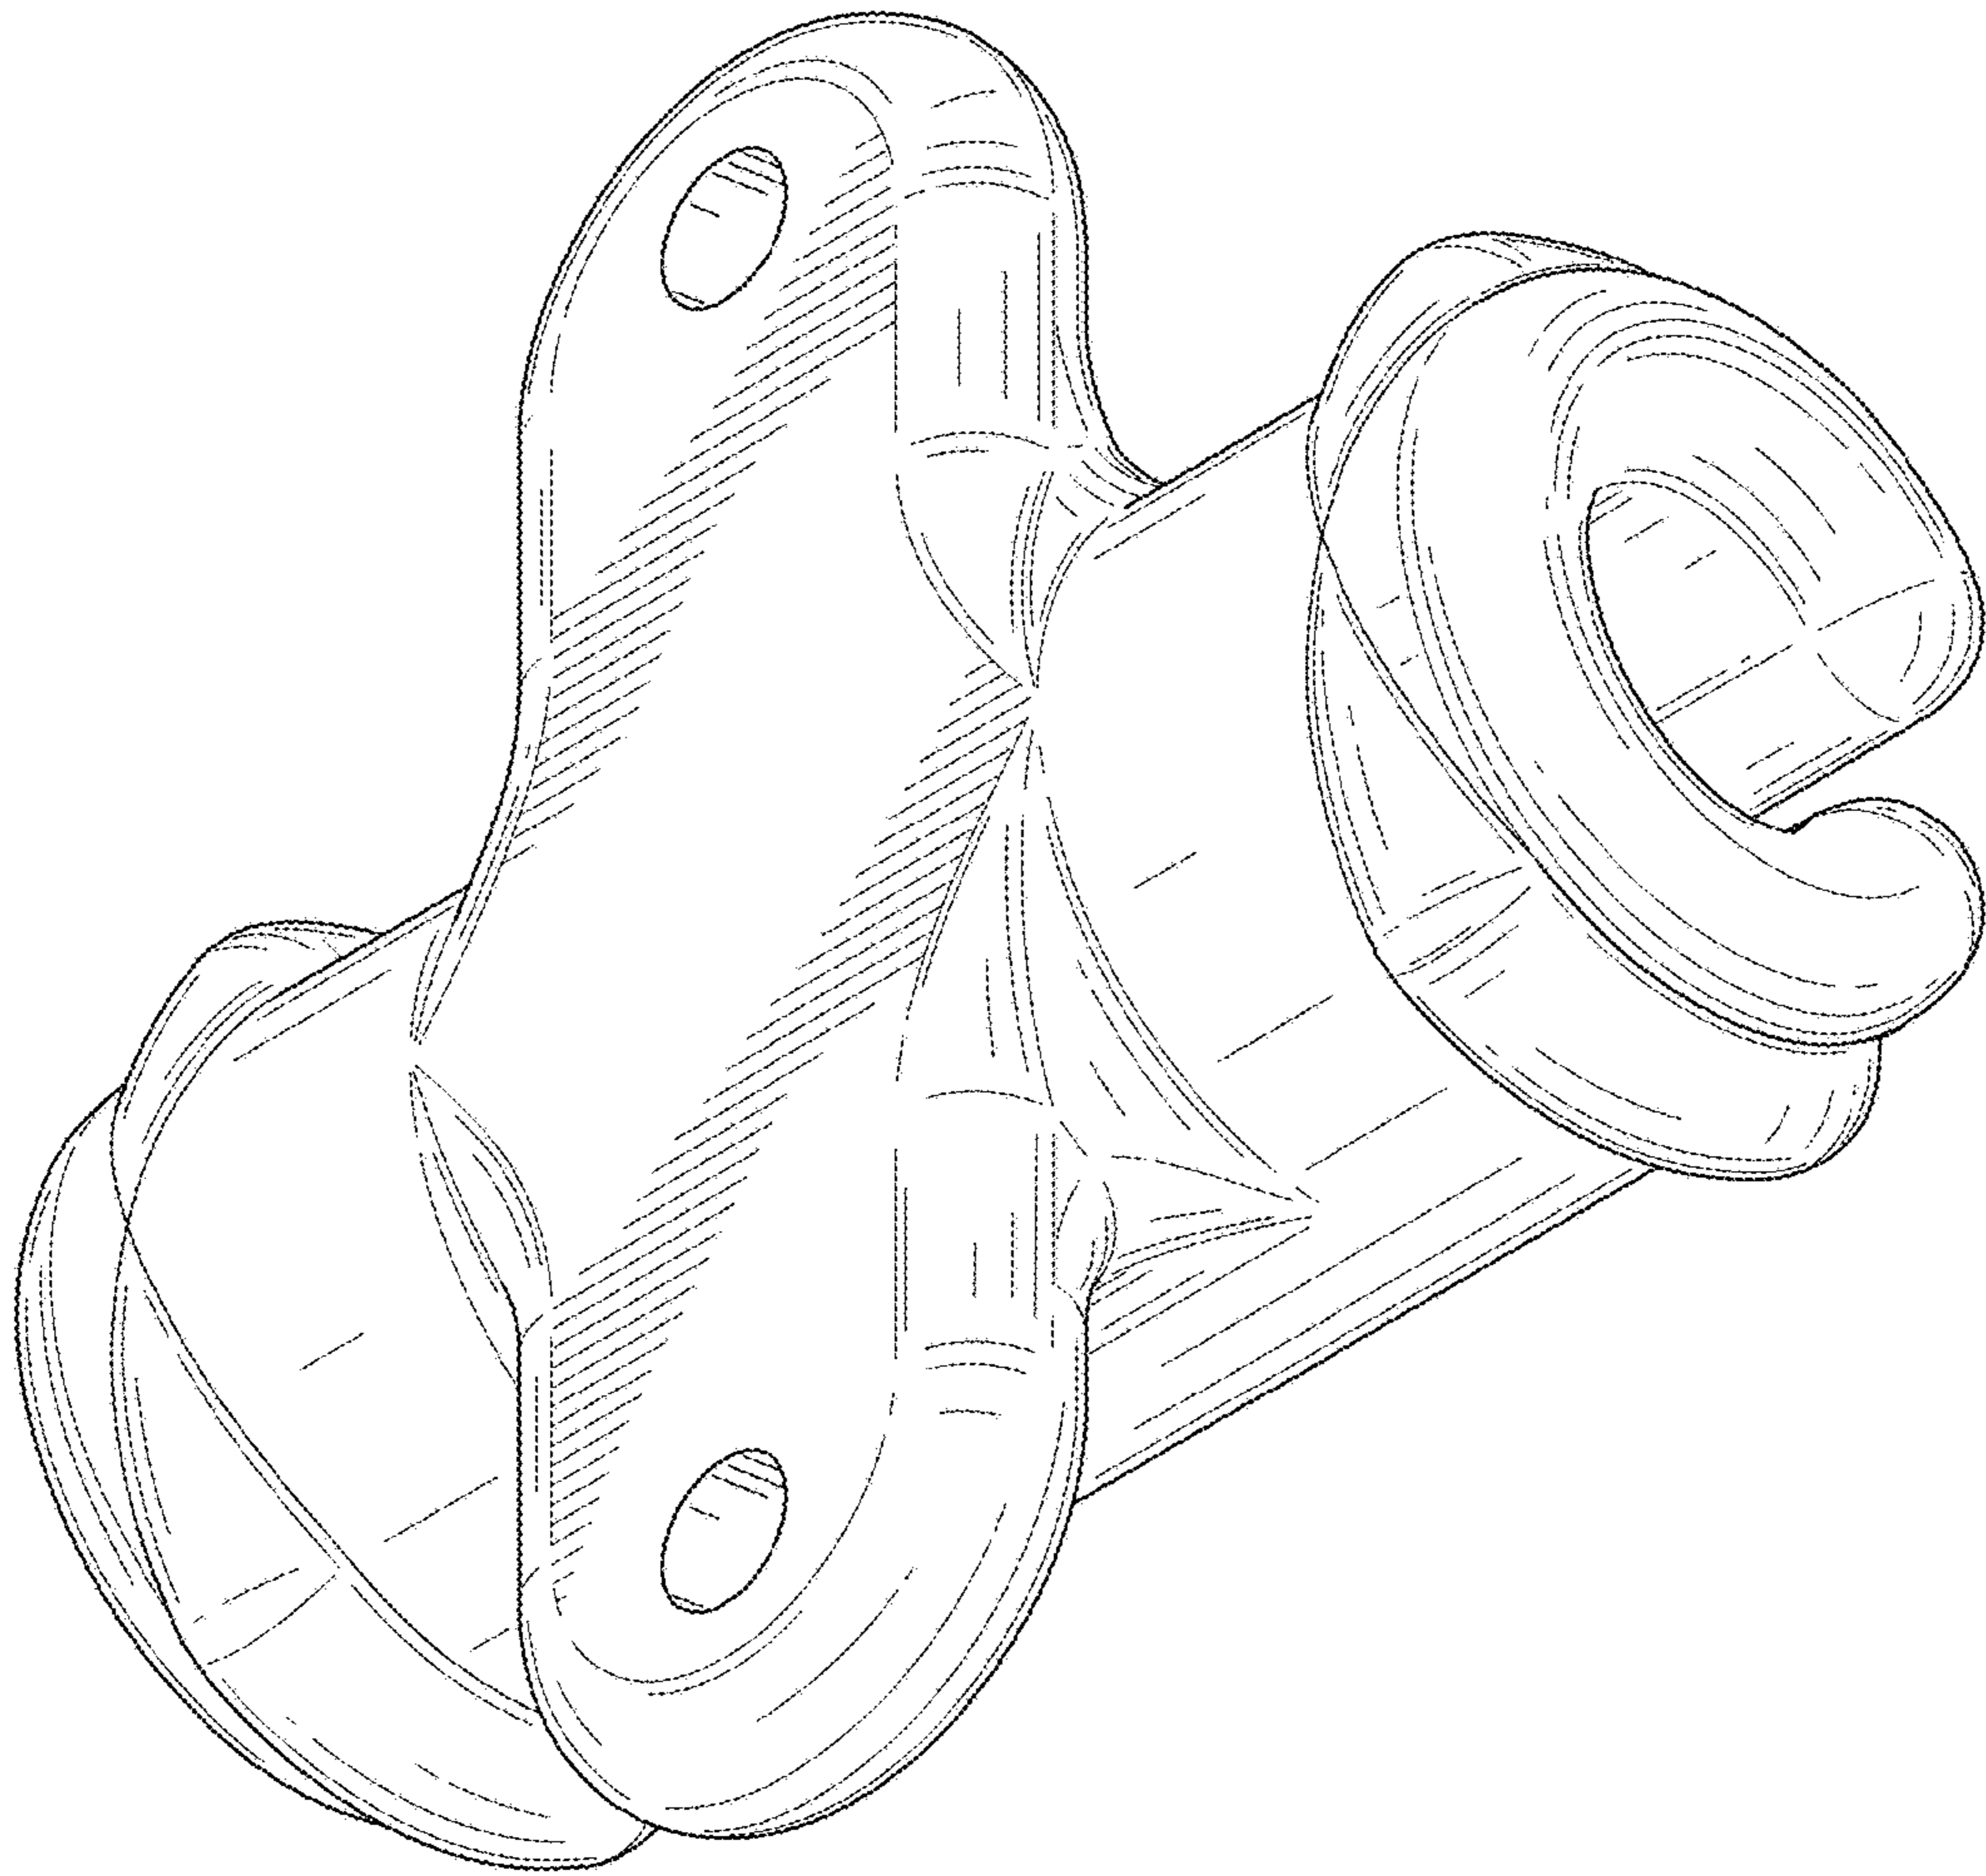


FIG. 2

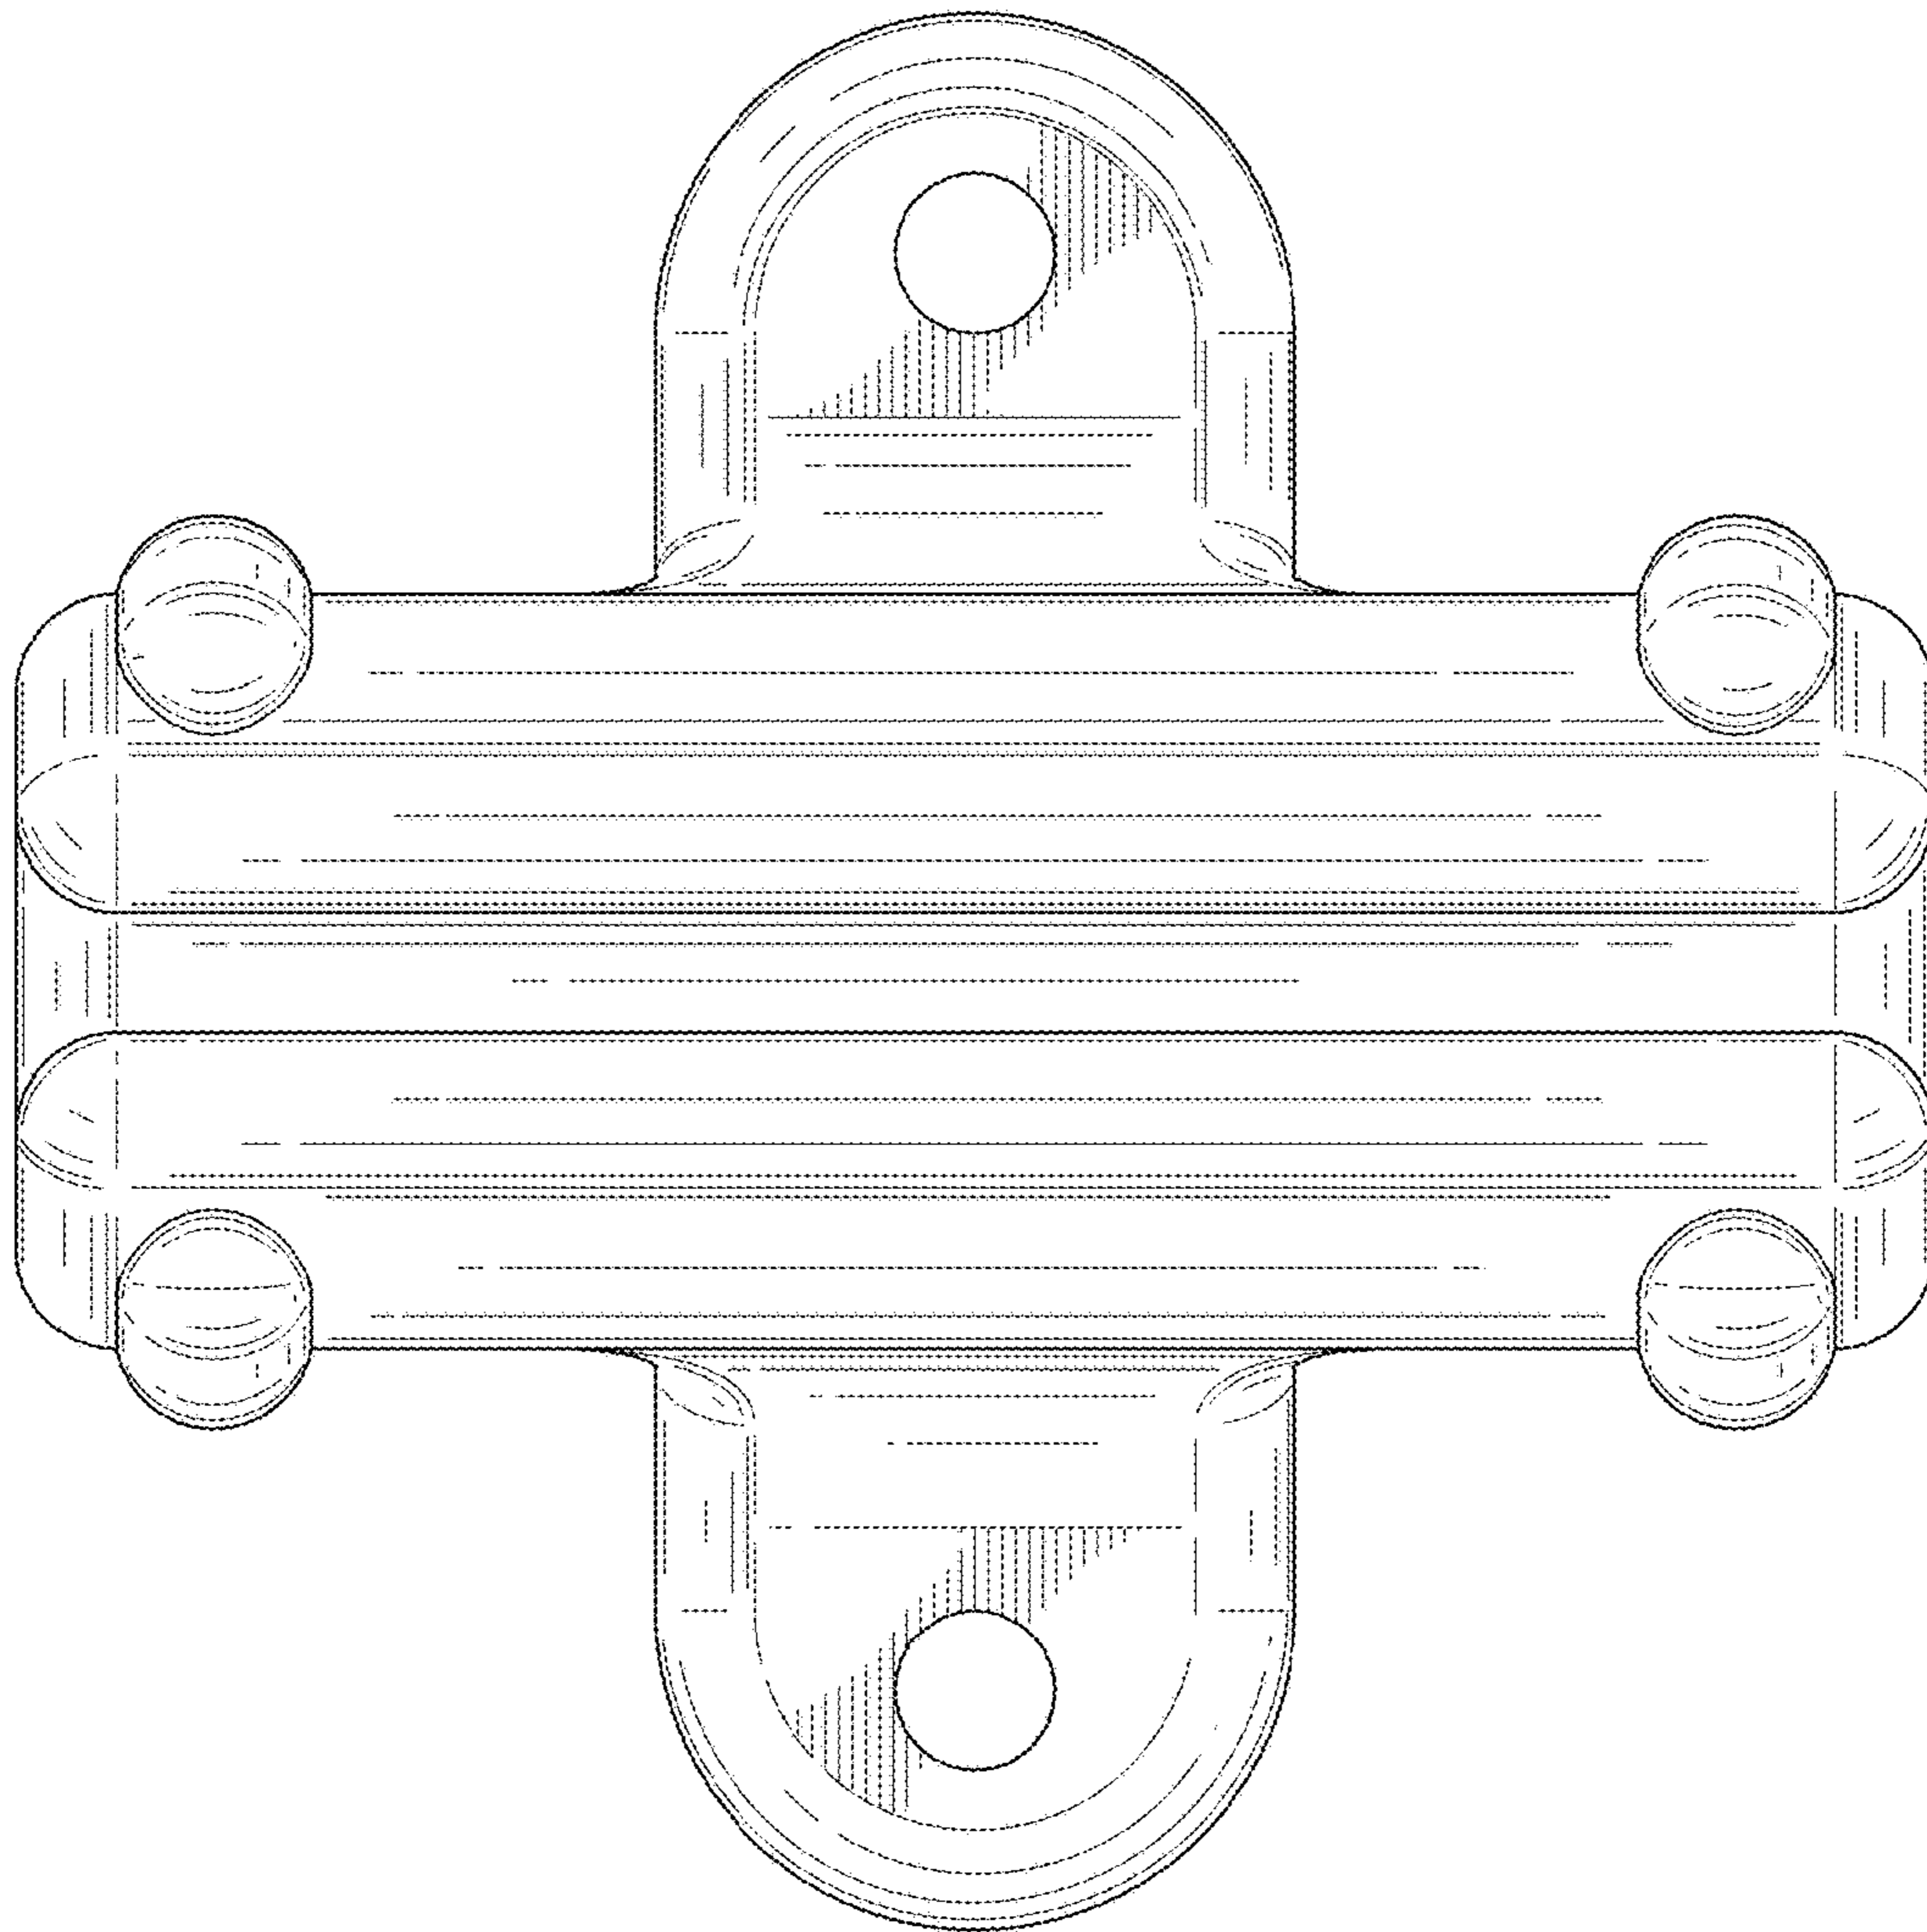


FIG. 3


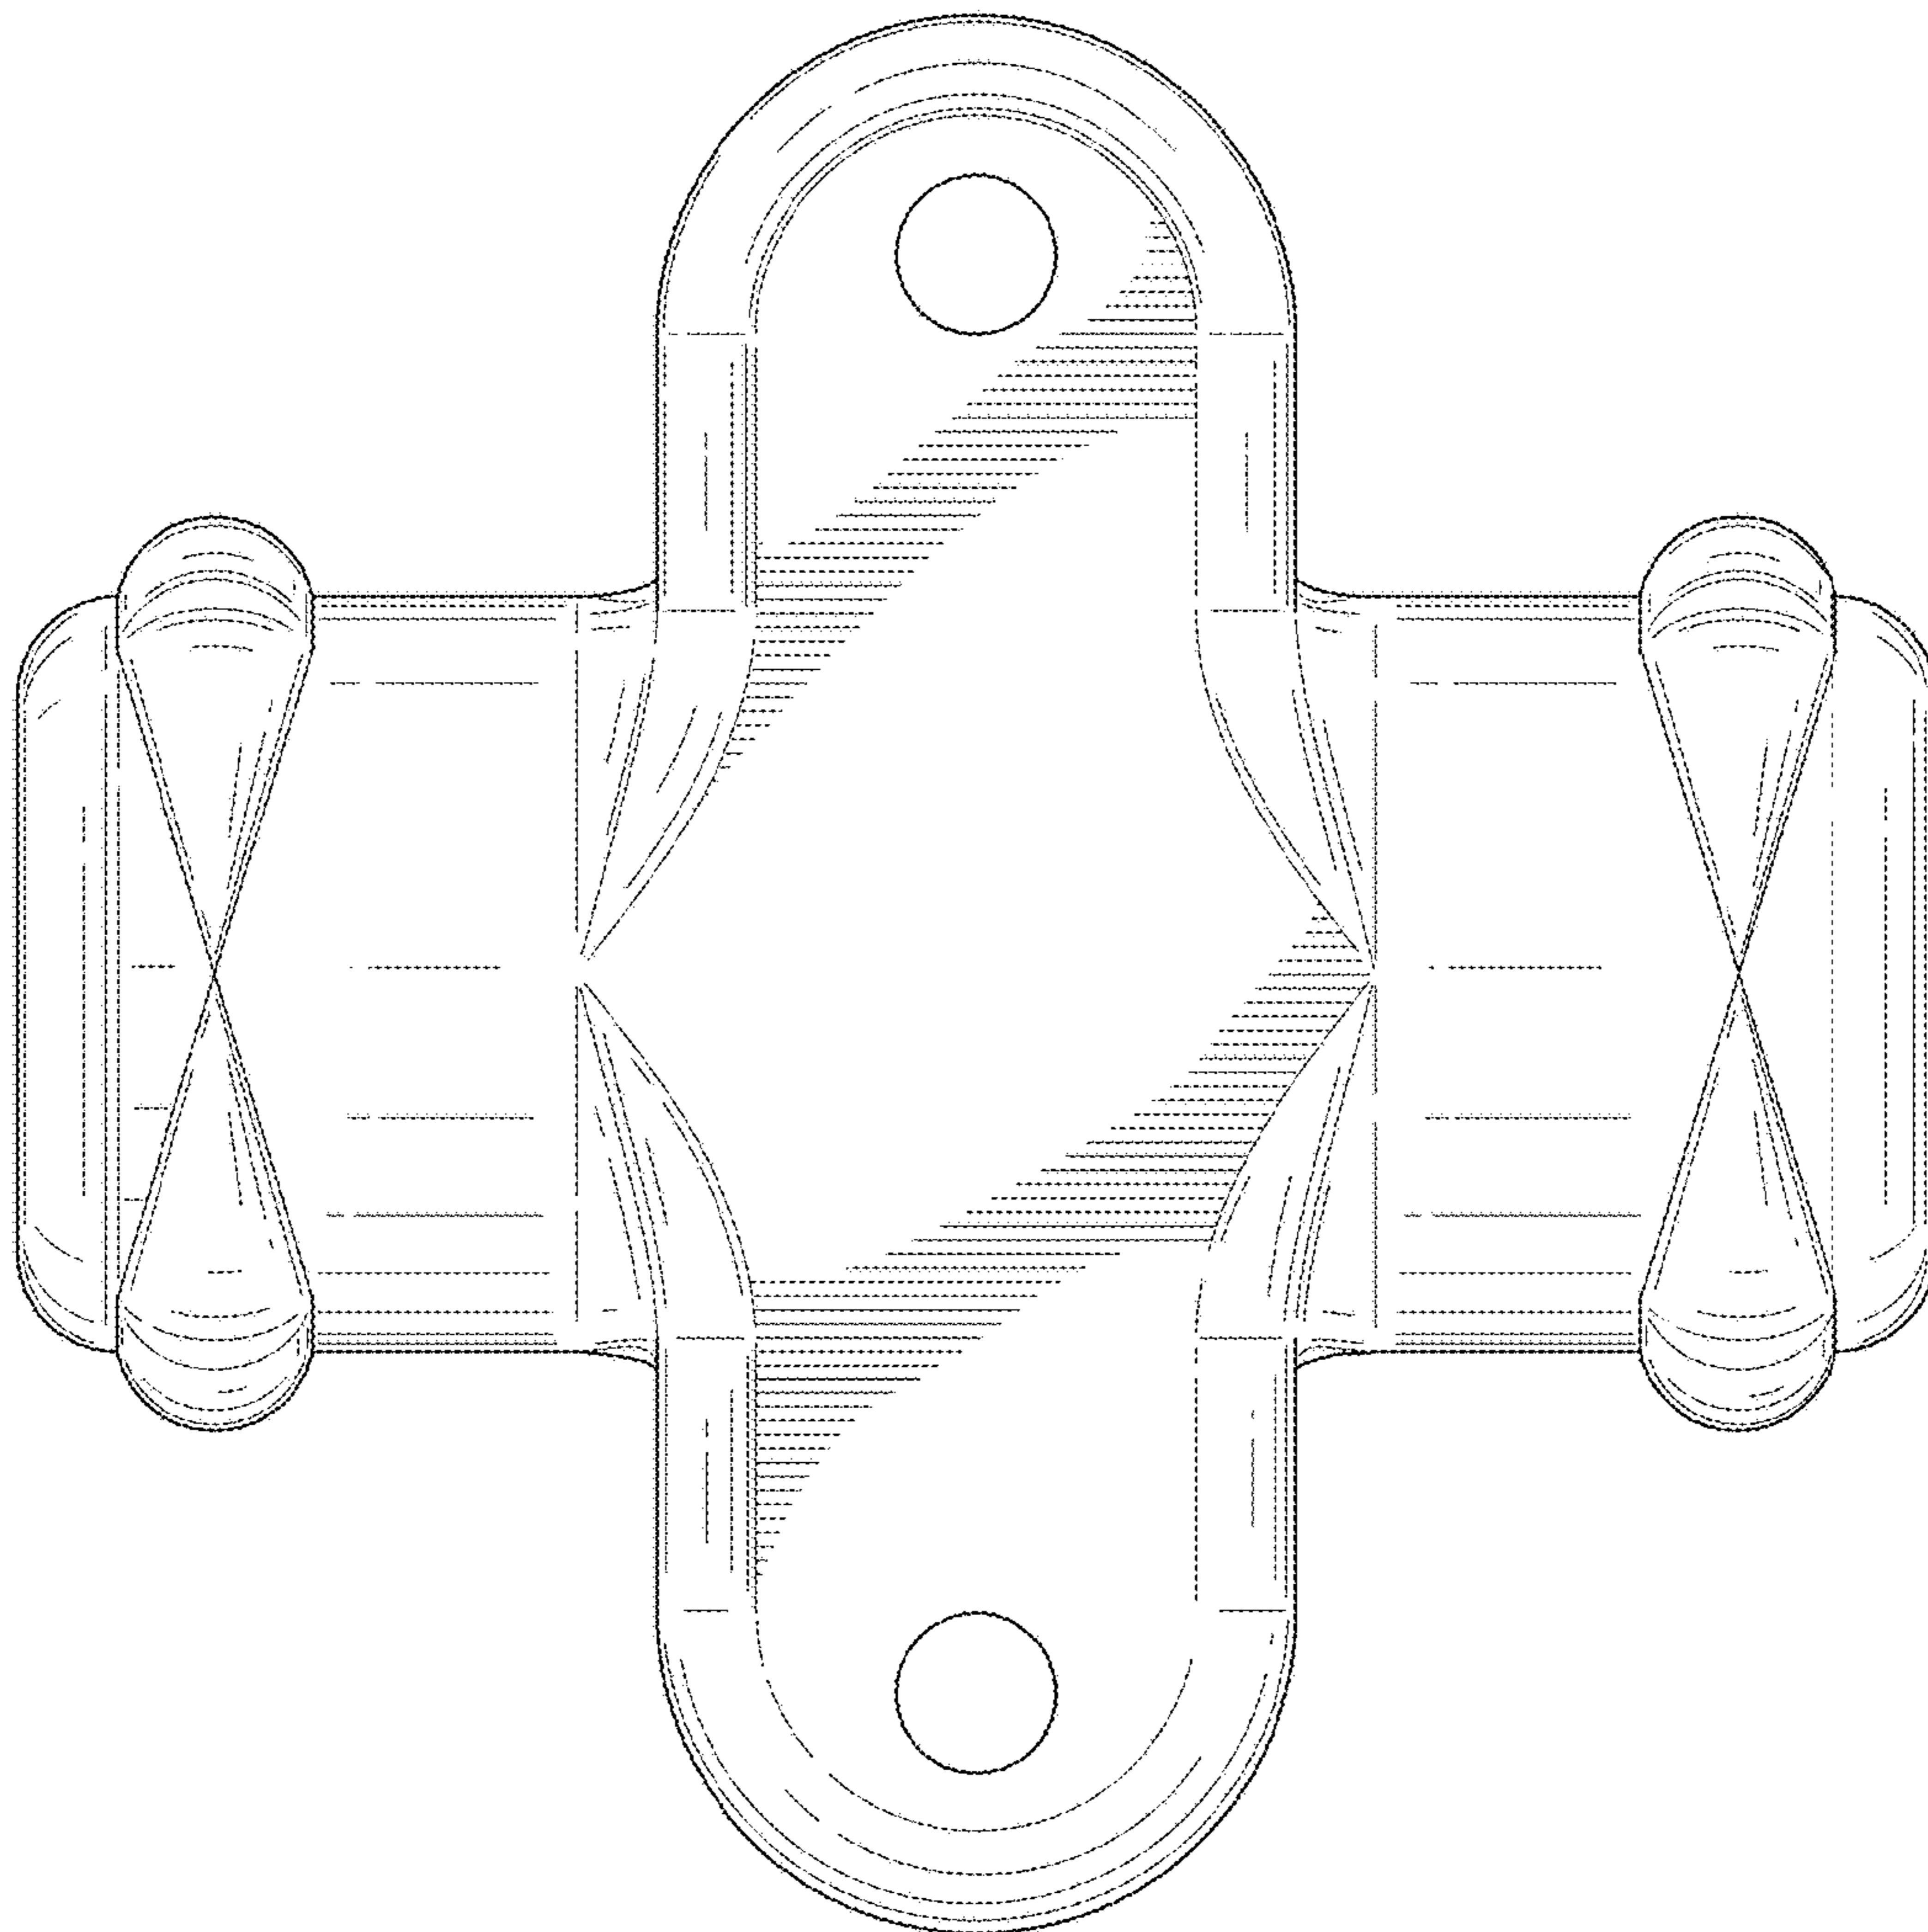


FIG. 4

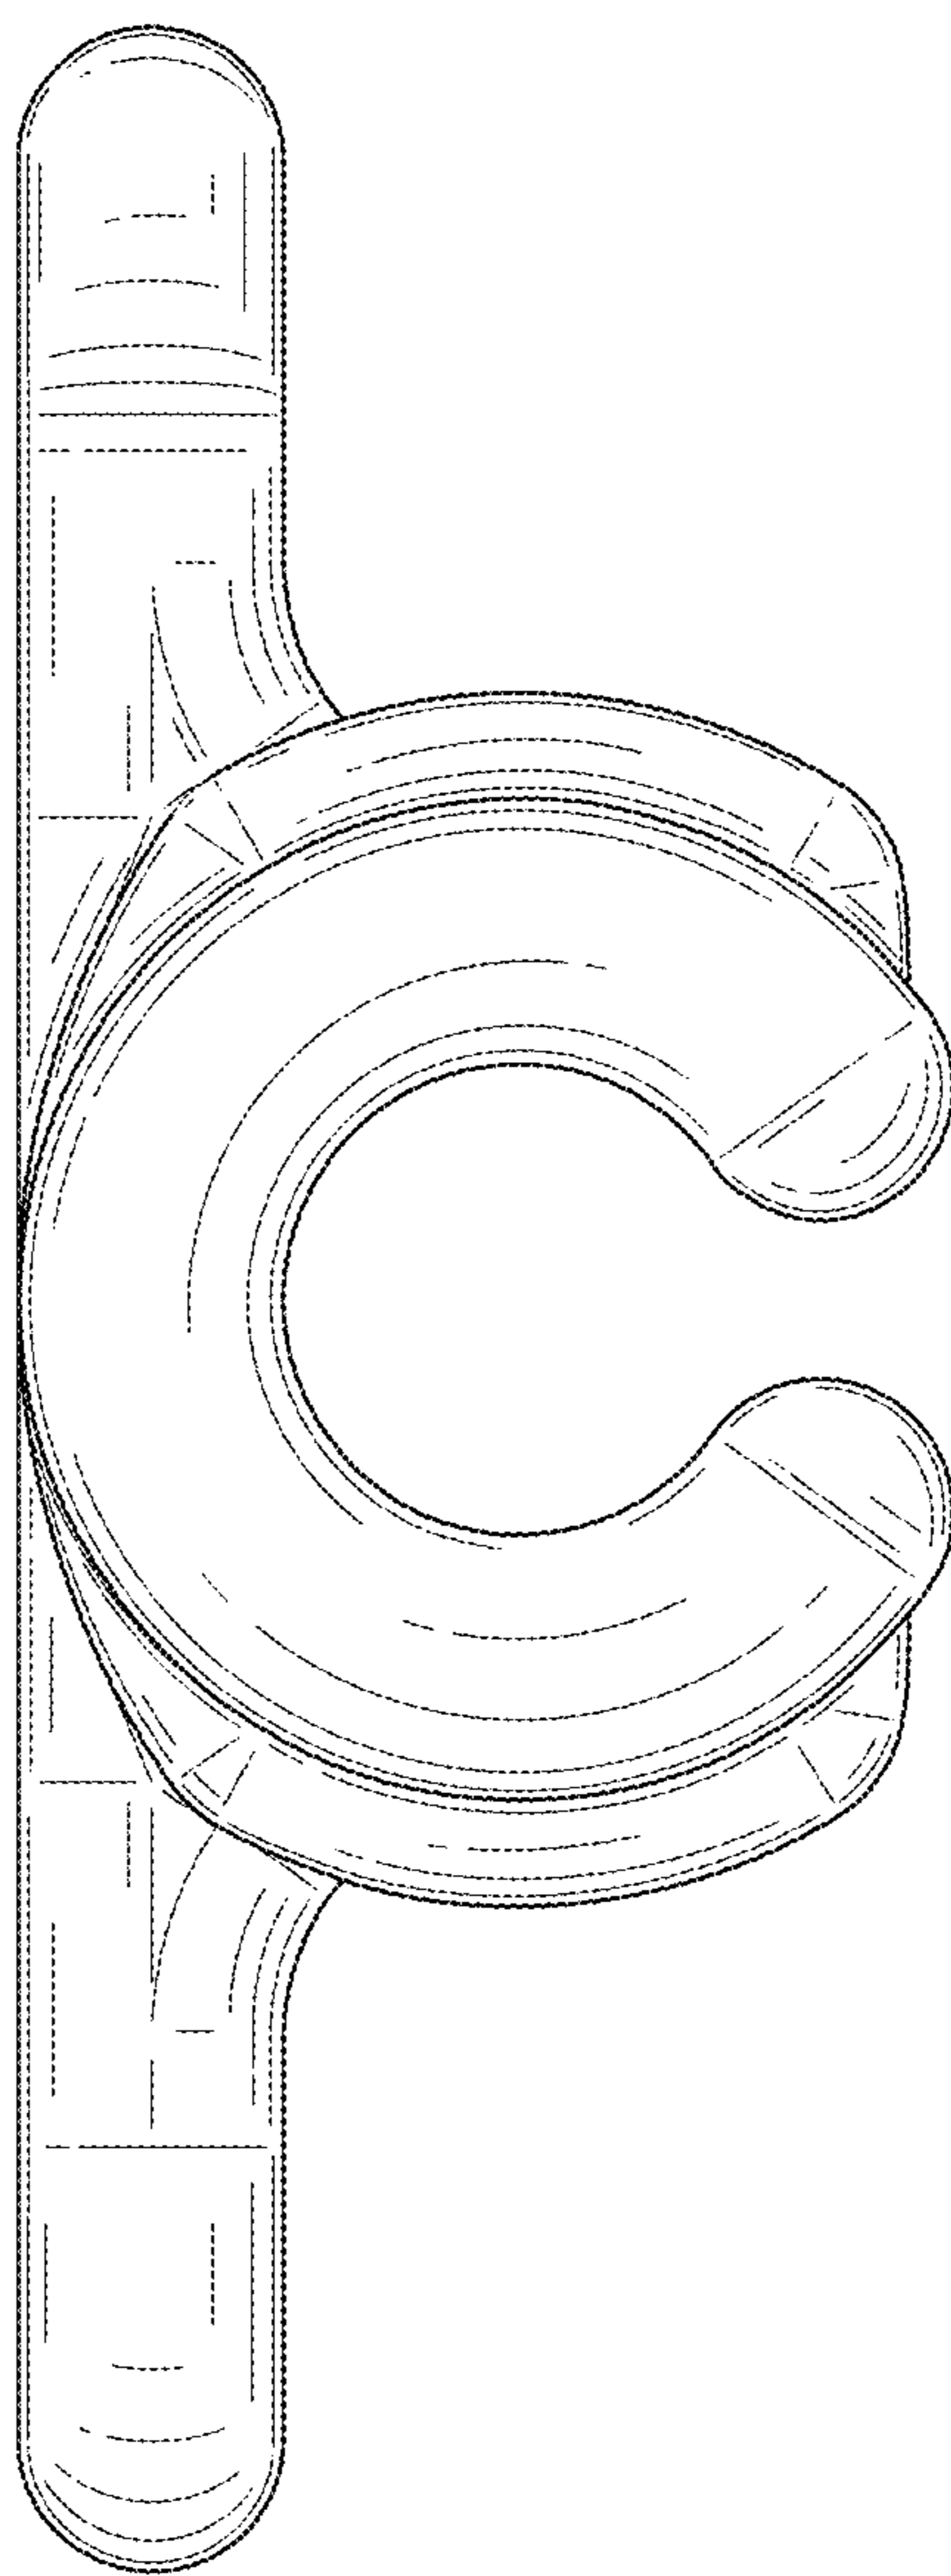

**FIG. 5**


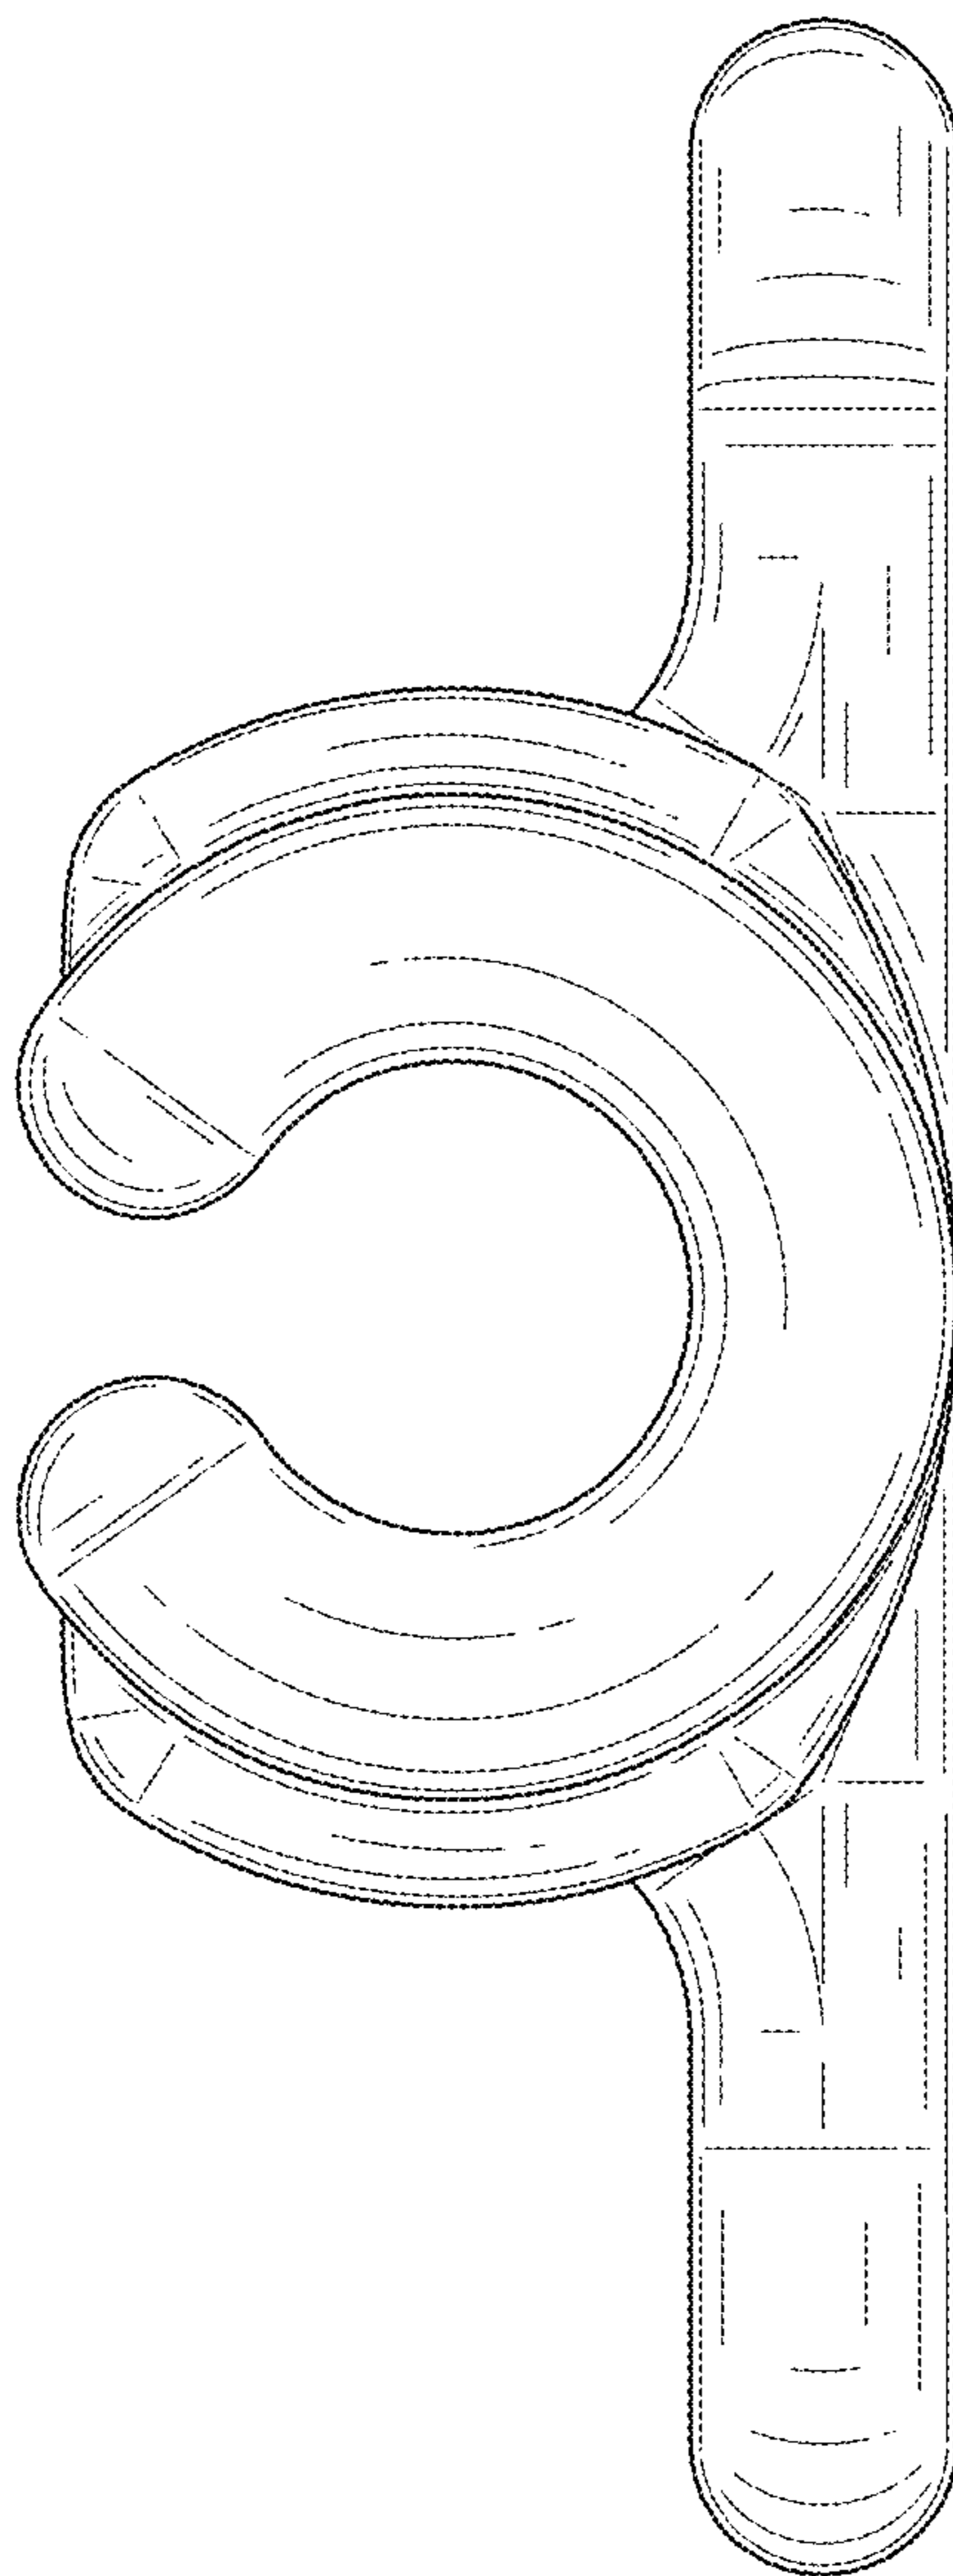


FIG. 6



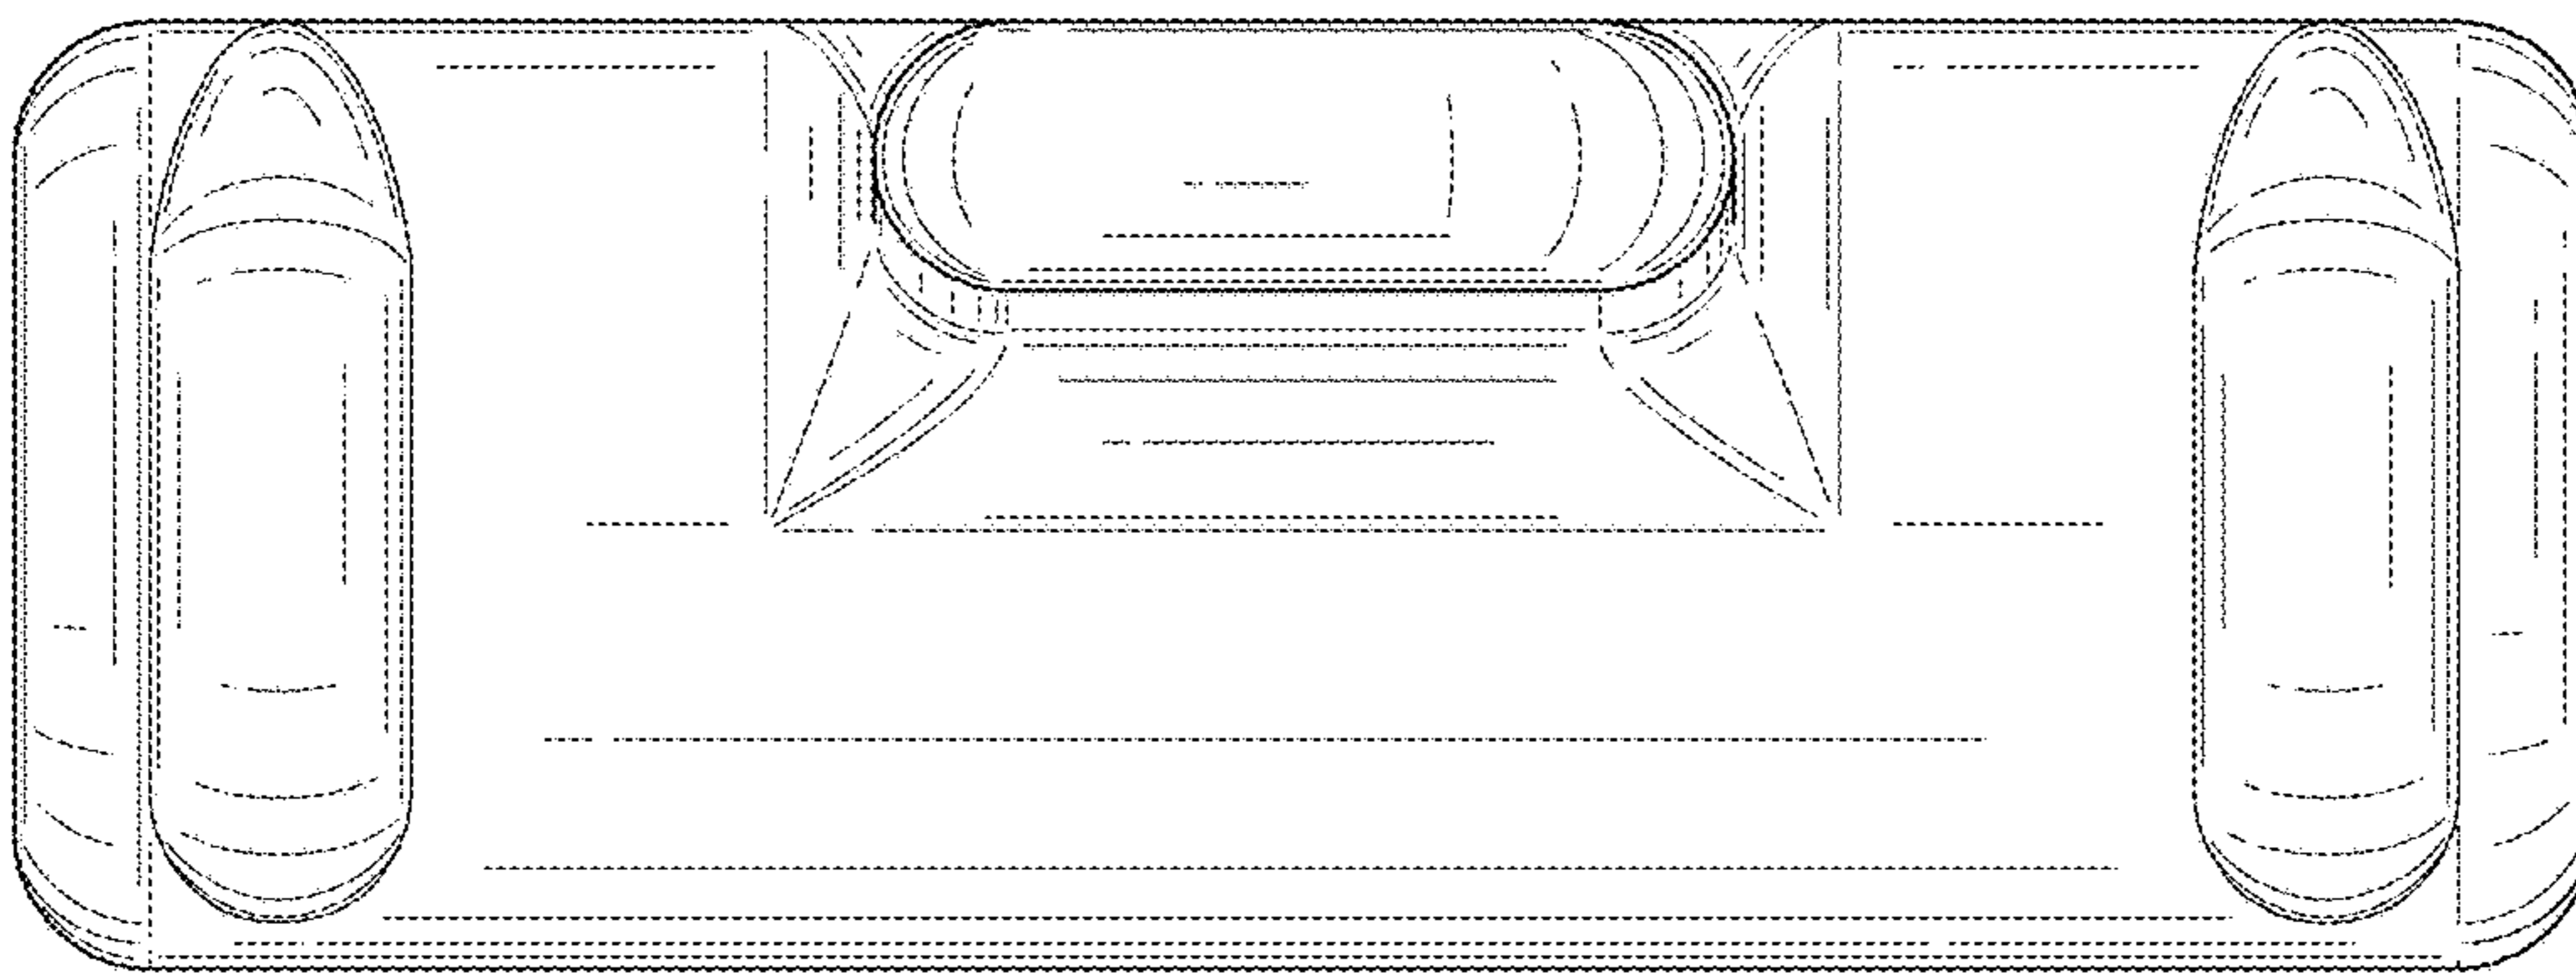

**FIG. 7**

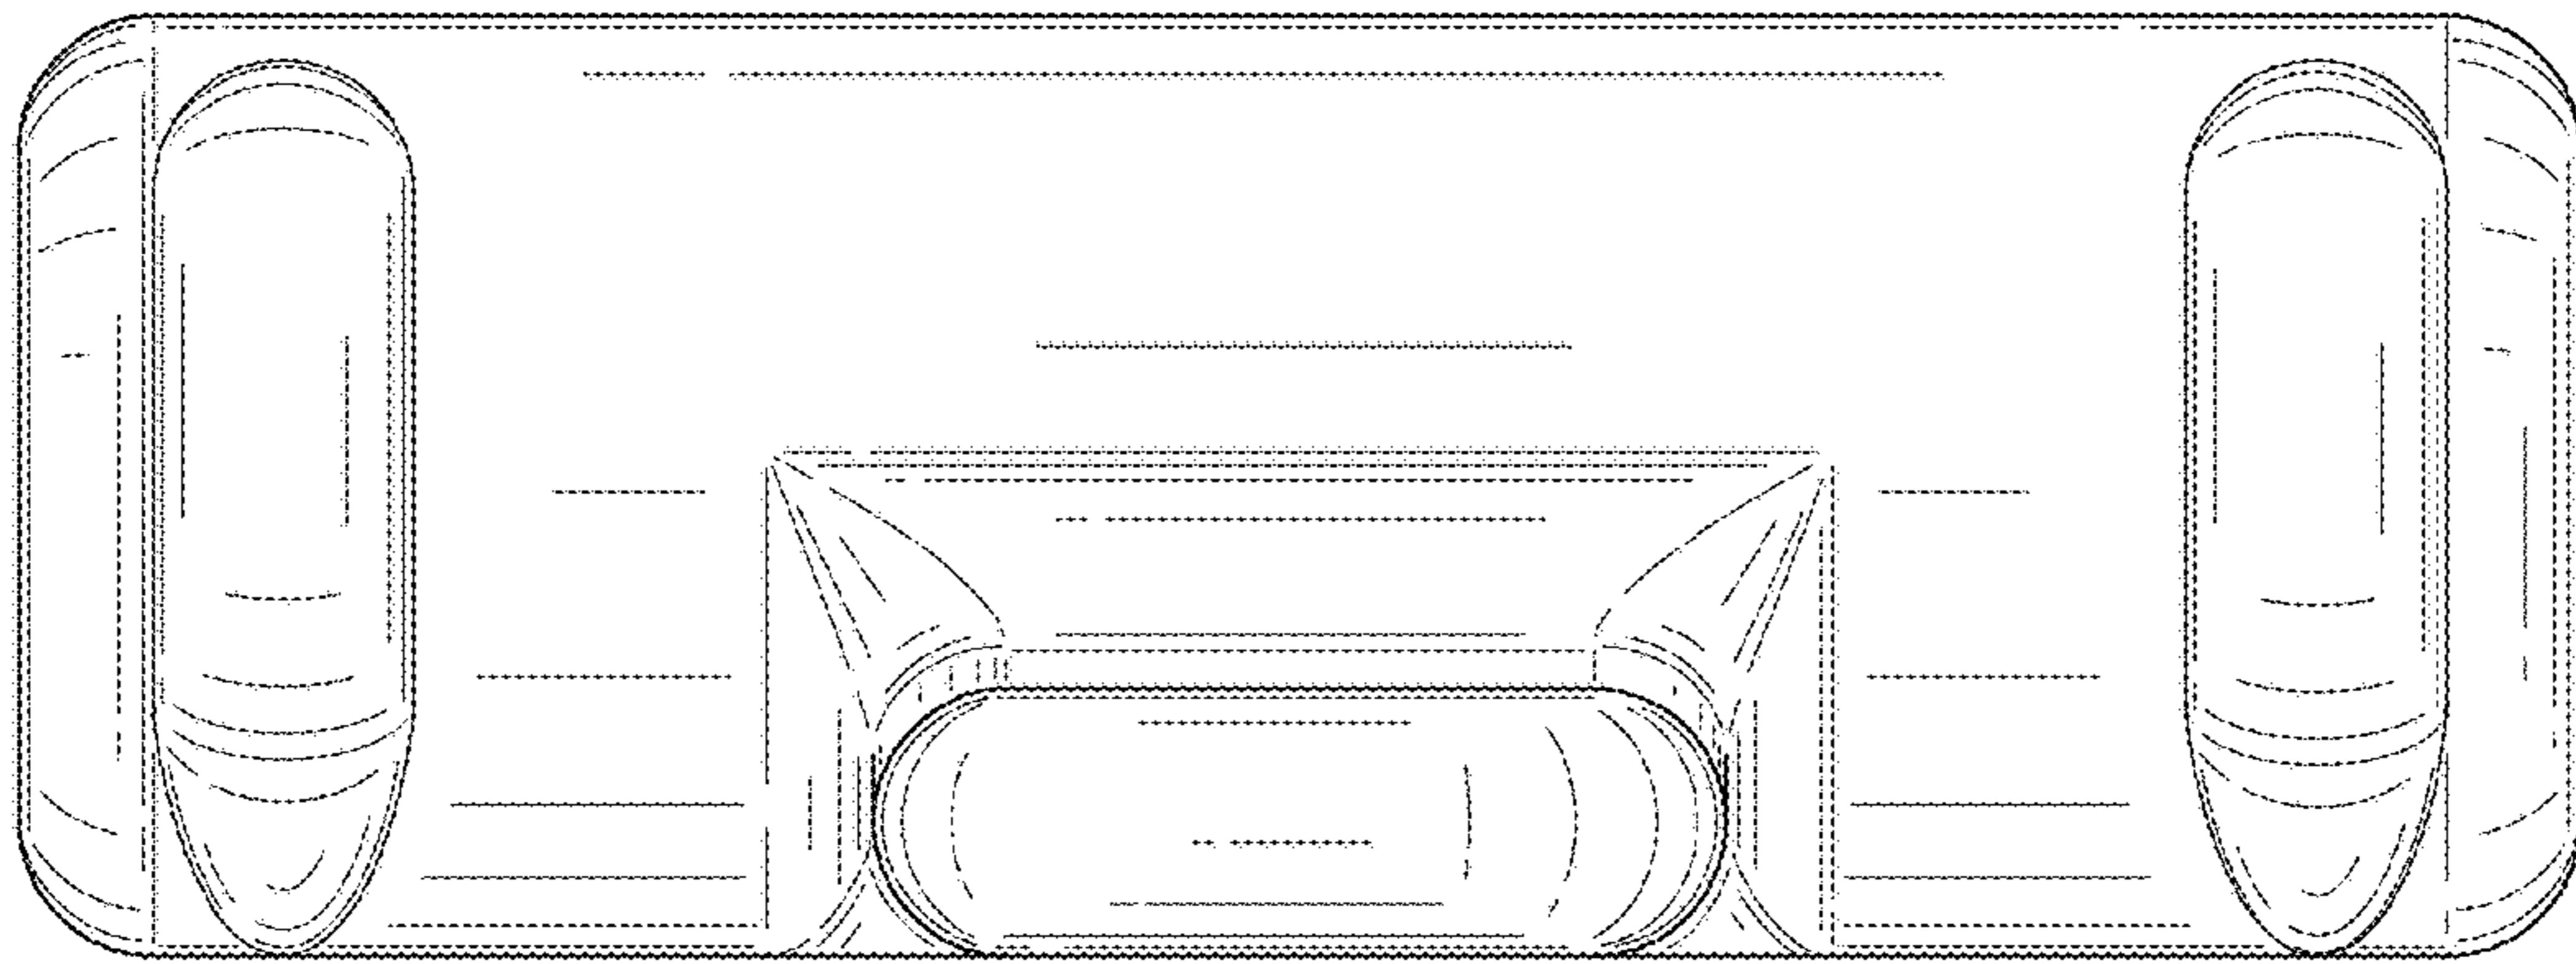


FIG. 8

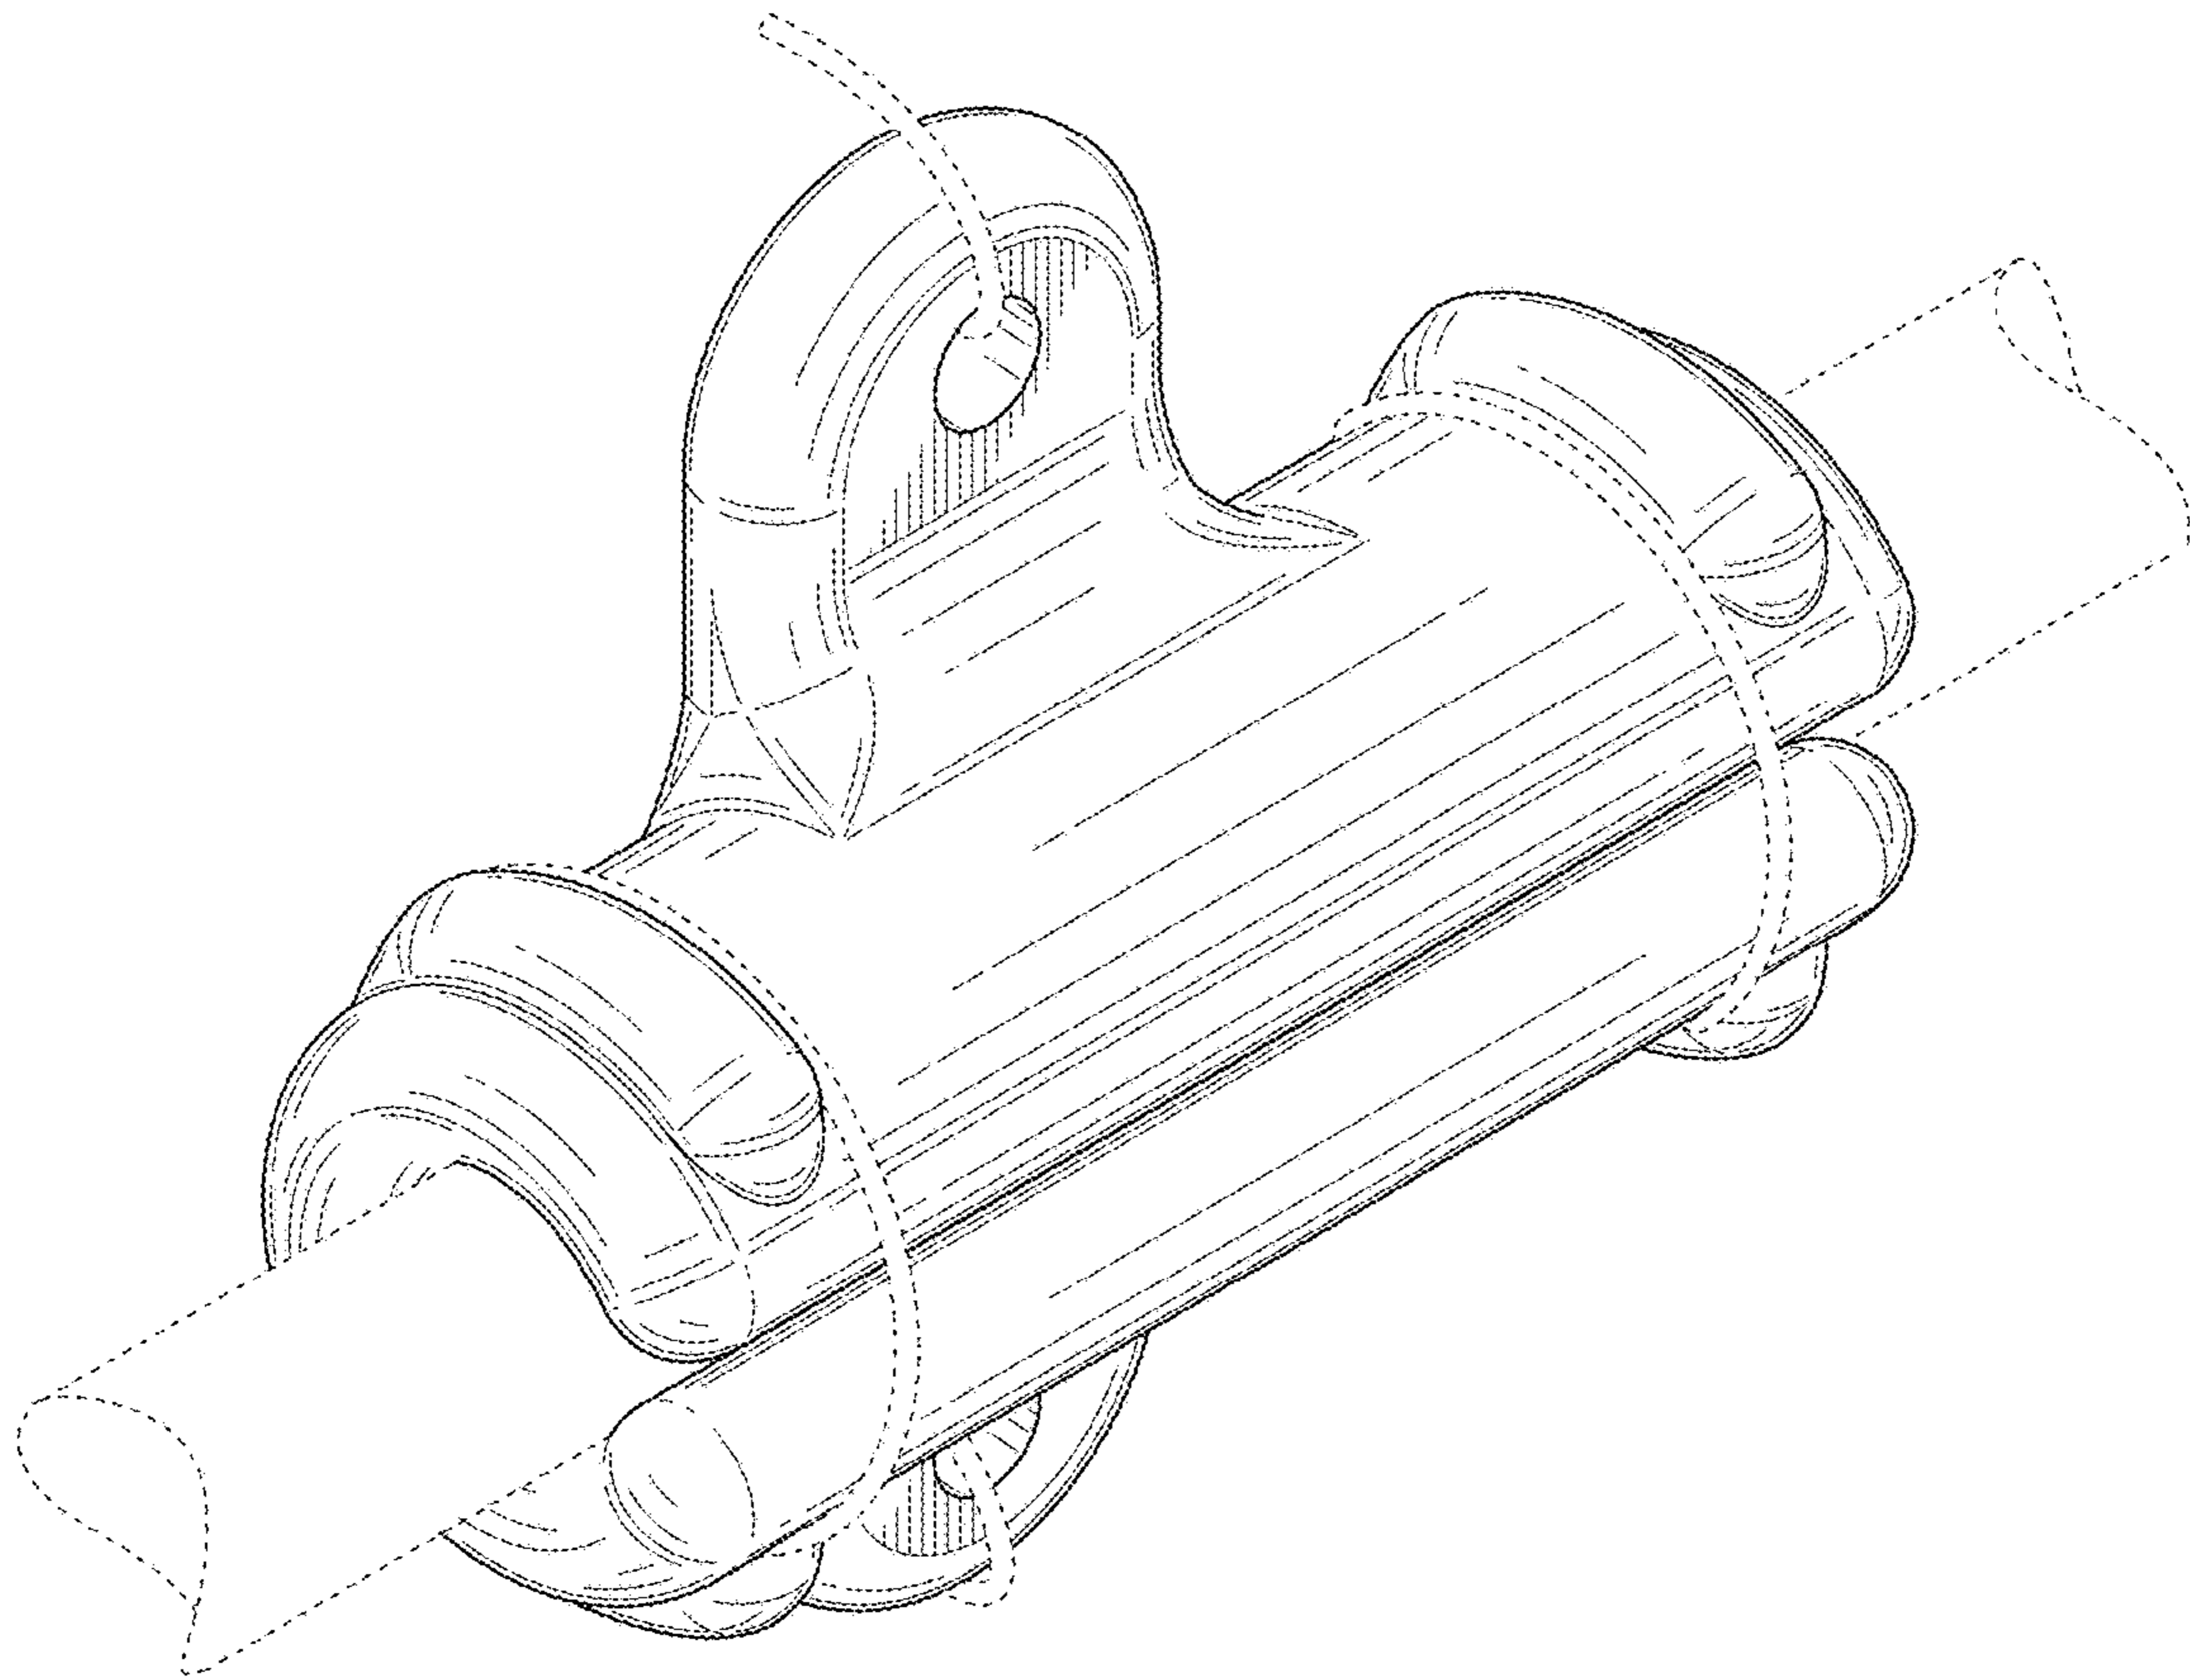


FIG. 9