



US00D823879S

(12) **United States Design Patent**  
**Brigham et al.**

(10) **Patent No.:** **US D823,879 S**  
(45) **Date of Patent:** **\*\* Jul. 24, 2018**

(54) **DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE FOR A SPHYGMOMANOMETER WITH WIRELESS COMMUNICATION DEVICE**

(71) Applicant: **OMRON HEALTHCARE Co., Ltd.**, Muko-shi, Kyoto (JP)

(72) Inventors: **Brian Brigham**, Muko (JP); **Shusuke Eshita**, Muko (JP)

(73) Assignee: **OMRON HEALTHCARE Co., Ltd.**, Kyoto (JP)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/608,357**

(22) Filed: **Jun. 21, 2017**

(30) **Foreign Application Priority Data**

Dec. 22, 2016 (JP) ..... 2016-027957  
Dec. 22, 2016 (JP) ..... 2016-027958  
Dec. 22, 2016 (JP) ..... 2016-027959

(51) **LOC (11) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/486**

(58) **Field of Classification Search**  
USPC ..... D14/485-495

(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D669,497 S \* 10/2012 Lee ..... D14/489  
D676,060 S \* 2/2013 Frost ..... D14/490

(Continued)

**OTHER PUBLICATIONS**

Dang!!! Motorola makes it so juicy that i am drawn back to electronic watches again!!, by Ed.Yang, dated Sep. 9, 2014, forums.

watchyouseek.com [online]. Retrieved Mar. 9, 2018 from internet. (Year: 2014).\*

(Continued)

*Primary Examiner* — Cathron C Brooks

*Assistant Examiner* — Andrew T Nemeth

(74) *Attorney, Agent, or Firm* — Capitol City TechLaw

(57) **CLAIM**

The ornamental design for a display screen with graphical user interface for a sphygmomanometer with wireless communication device, as shown and described.

**DESCRIPTION**

The file of this patent contains a least one drawing/photograph executed in color. Copies of this patent with color drawings/photographs will be provided by the united states Patent and Trademark office upon request and payment of the necessary fee.

FIG. 1 is a front view of a first embodiment of a display screen with graphical user interface for a sphygmomanometer with wireless communication device showing the first image of our new design;

FIG. 2 is a front view showing a second image thereof;

FIG. 3 is a front view showing a third image thereof;

FIG. 4 is a front view showing a fourth image thereof;

FIG. 5 is a front view showing a fifth image thereof; and

FIG. 6 is a front view showing a sixth image thereof.

FIG. 7 is a front view of a second embodiment of a display screen with graphical user interface for a sphygmomanometer with wireless communication device showing the first image of our new design;

FIG. 8 is a front view showing a second image thereof;

FIG. 9 is a front view showing a third image thereof;



FIG. 10 is a front view showing a fourth image thereof;

FIG. 11 is a front view showing a fifth image thereof; and,

FIG. 12 is a front view showing a sixth image thereof.

The appearance of the graphical user interface sequentially transitions between the images shown in FIGS. 1-6 and FIGS. 7-12. The process or period in which one image transitions into another image forms no part of the claimed design.

(Continued)

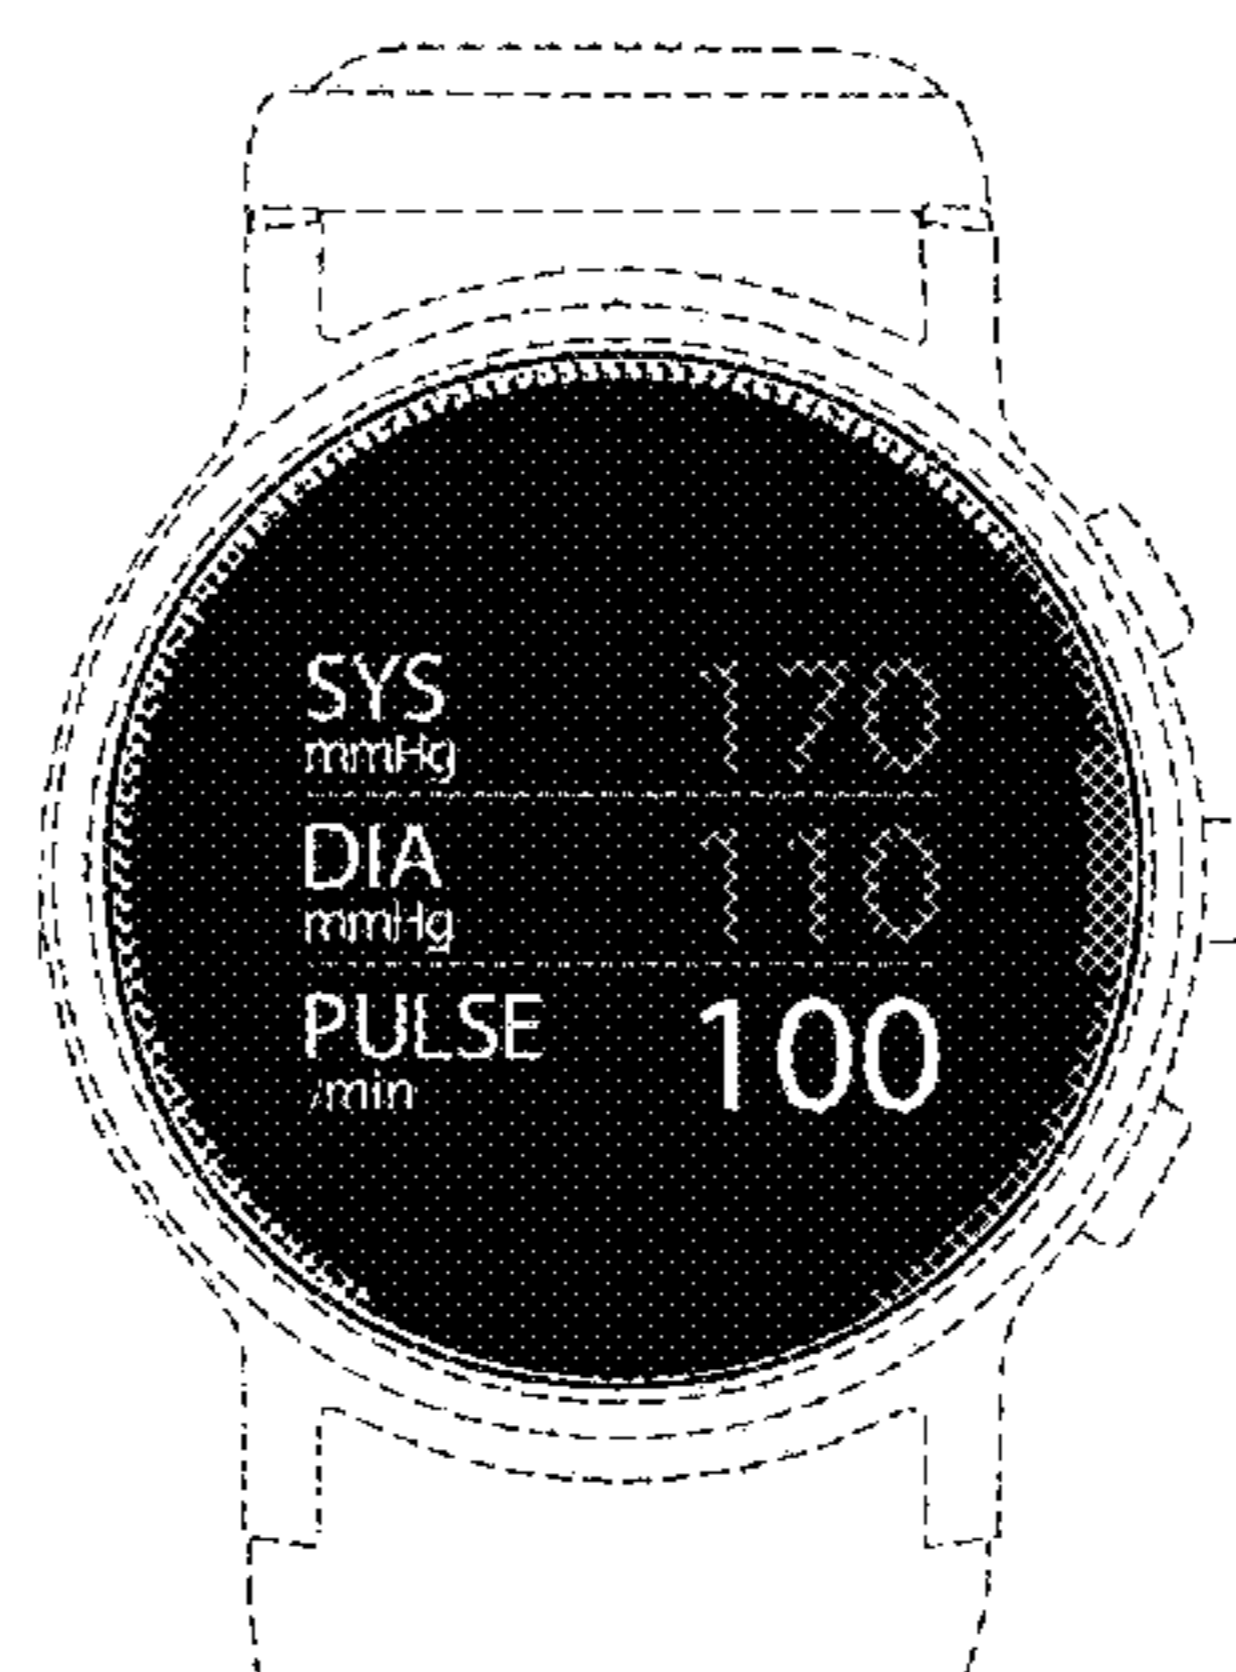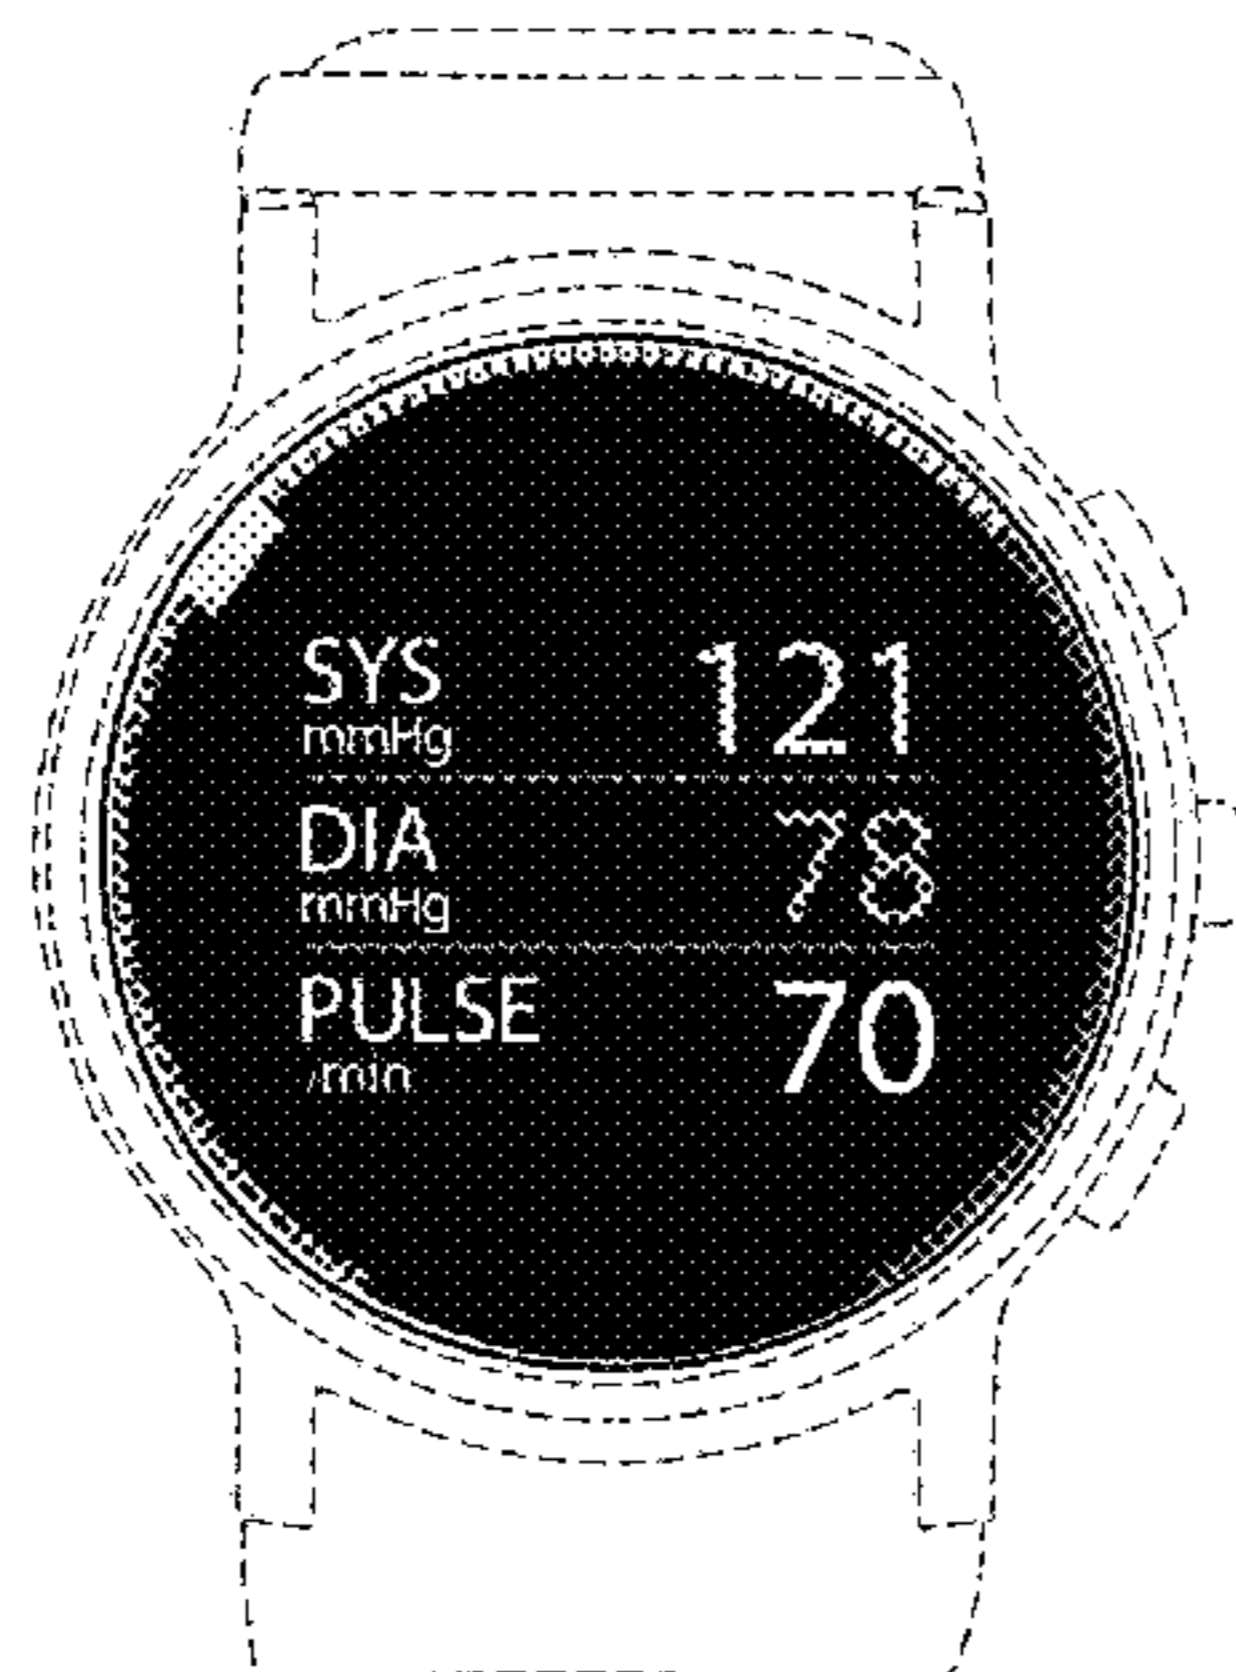

The dashed broken lines showing a sphygmomanometer with wireless communication device illustrate environmental structure that forms no part of the claimed design.

**1 Claim, 12 Drawing Sheets  
(12 of 12 Drawing Sheet(s) Filed in Color)**

(58) **Field of Classification Search**

CPC ..... G06F 3/0482; G06F 3/04847; G06F 3/04817; G06F 3/04842; G06F 3/04883; A63F 5/00

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D687,057 S *	7/2013	Plitkins .....	D14/488
D740,300 S *	10/2015	Lee .....	G06F 3/04817 D14/485
D741,898 S *	10/2015	Soegiono .....	D14/488
D750,125 S *	2/2016	Yang .....	D14/488
D752,062 S *	3/2016	Forsblom .....	D14/485
D761,277 S *	7/2016	Harvell .....	D14/485
D763,308 S *	8/2016	Wang .....	D14/486
D776,690 S *	1/2017	Tsujimoto .....	D14/486
D778,952 S *	2/2017	Kim .....	D14/489
D781,327 S *	3/2017	Conze .....	D14/486
D781,878 S *	3/2017	Butcher .....	D14/485
D783,630 S *	4/2017	Ahn .....	D14/485
D785,025 S *	4/2017	Zimmerman .....	D14/486
D786,278 S *	5/2017	Motamedi .....	D14/485
D787,533 S *	5/2017	Butcher .....	D14/485
D788,122 S *	5/2017	Tada .....	D14/485
D788,141 S *	5/2017	Kim .....	D14/486

D791,793 S *	7/2017	Aoki .....	D14/485
D791,806 S *	7/2017	Brewington .....	D14/486
D797,756 S *	9/2017	Meyer .....	D14/485
D798,315 S *	9/2017	Prophete .....	D14/485
9,804,610 B2 *	10/2017	Sloo .....	G05D 23/1902
D802,008 S *	11/2017	Zhang .....	D14/487
D803,233 S *	11/2017	Wilberding .....	D14/485
D803,247 S *	11/2017	Mistry .....	D14/486
D807,376 S *	1/2018	Mizono .....	D14/485
D808,402 S *	1/2018	Butcher .....	D14/485
D808,974 S *	1/2018	Chiappone .....	D14/485
D808,983 S *	1/2018	Narinedhat .....	D14/485
D808,984 S *	1/2018	Narinedhat .....	D14/485
D808,986 S *	1/2018	Dudey .....	D14/485
D809,535 S *	2/2018	Park .....	D14/485
D809,543 S *	2/2018	Broughton .....	D14/486
2015/0248235 A1 *	9/2015	Offenberg .....	G06F 3/04886 715/773

OTHER PUBLICATIONS


Fenix 3 HR, dated Dec. 12, 2016, buygarmin.com [online]. Retrieved Mar. 9, 2018 from internet <URL:https://web.archive.org/web/20161212235452/https://buy.garmin.com/en-US/US/p/545480> (Year: 2016).\*

Omron Project Zero 2.0—CES 2017, by Techy Agent, published Dec. 6, 2017, youtube.com [online]. Retrieved Mar. 9, 2018 from internet <URL:https://www.youtube.com/watch?v=3flnc1yBI8Q> (Year: 2017).\*


Omron Shows Off Project Zero 2.0 Wrist Blood Pressure Monitor, by Scott Jung, dated Dec. 13, 2017, medgadget.com [online]. Retrieved from internet <URL:https://www.medgadget.com/2017/01/omron-shows-off-project-zero-2-0-wrist-blood-pressure-monitor.html> (Year: 2017).\*

\* cited by examiner


**FIG. 1**

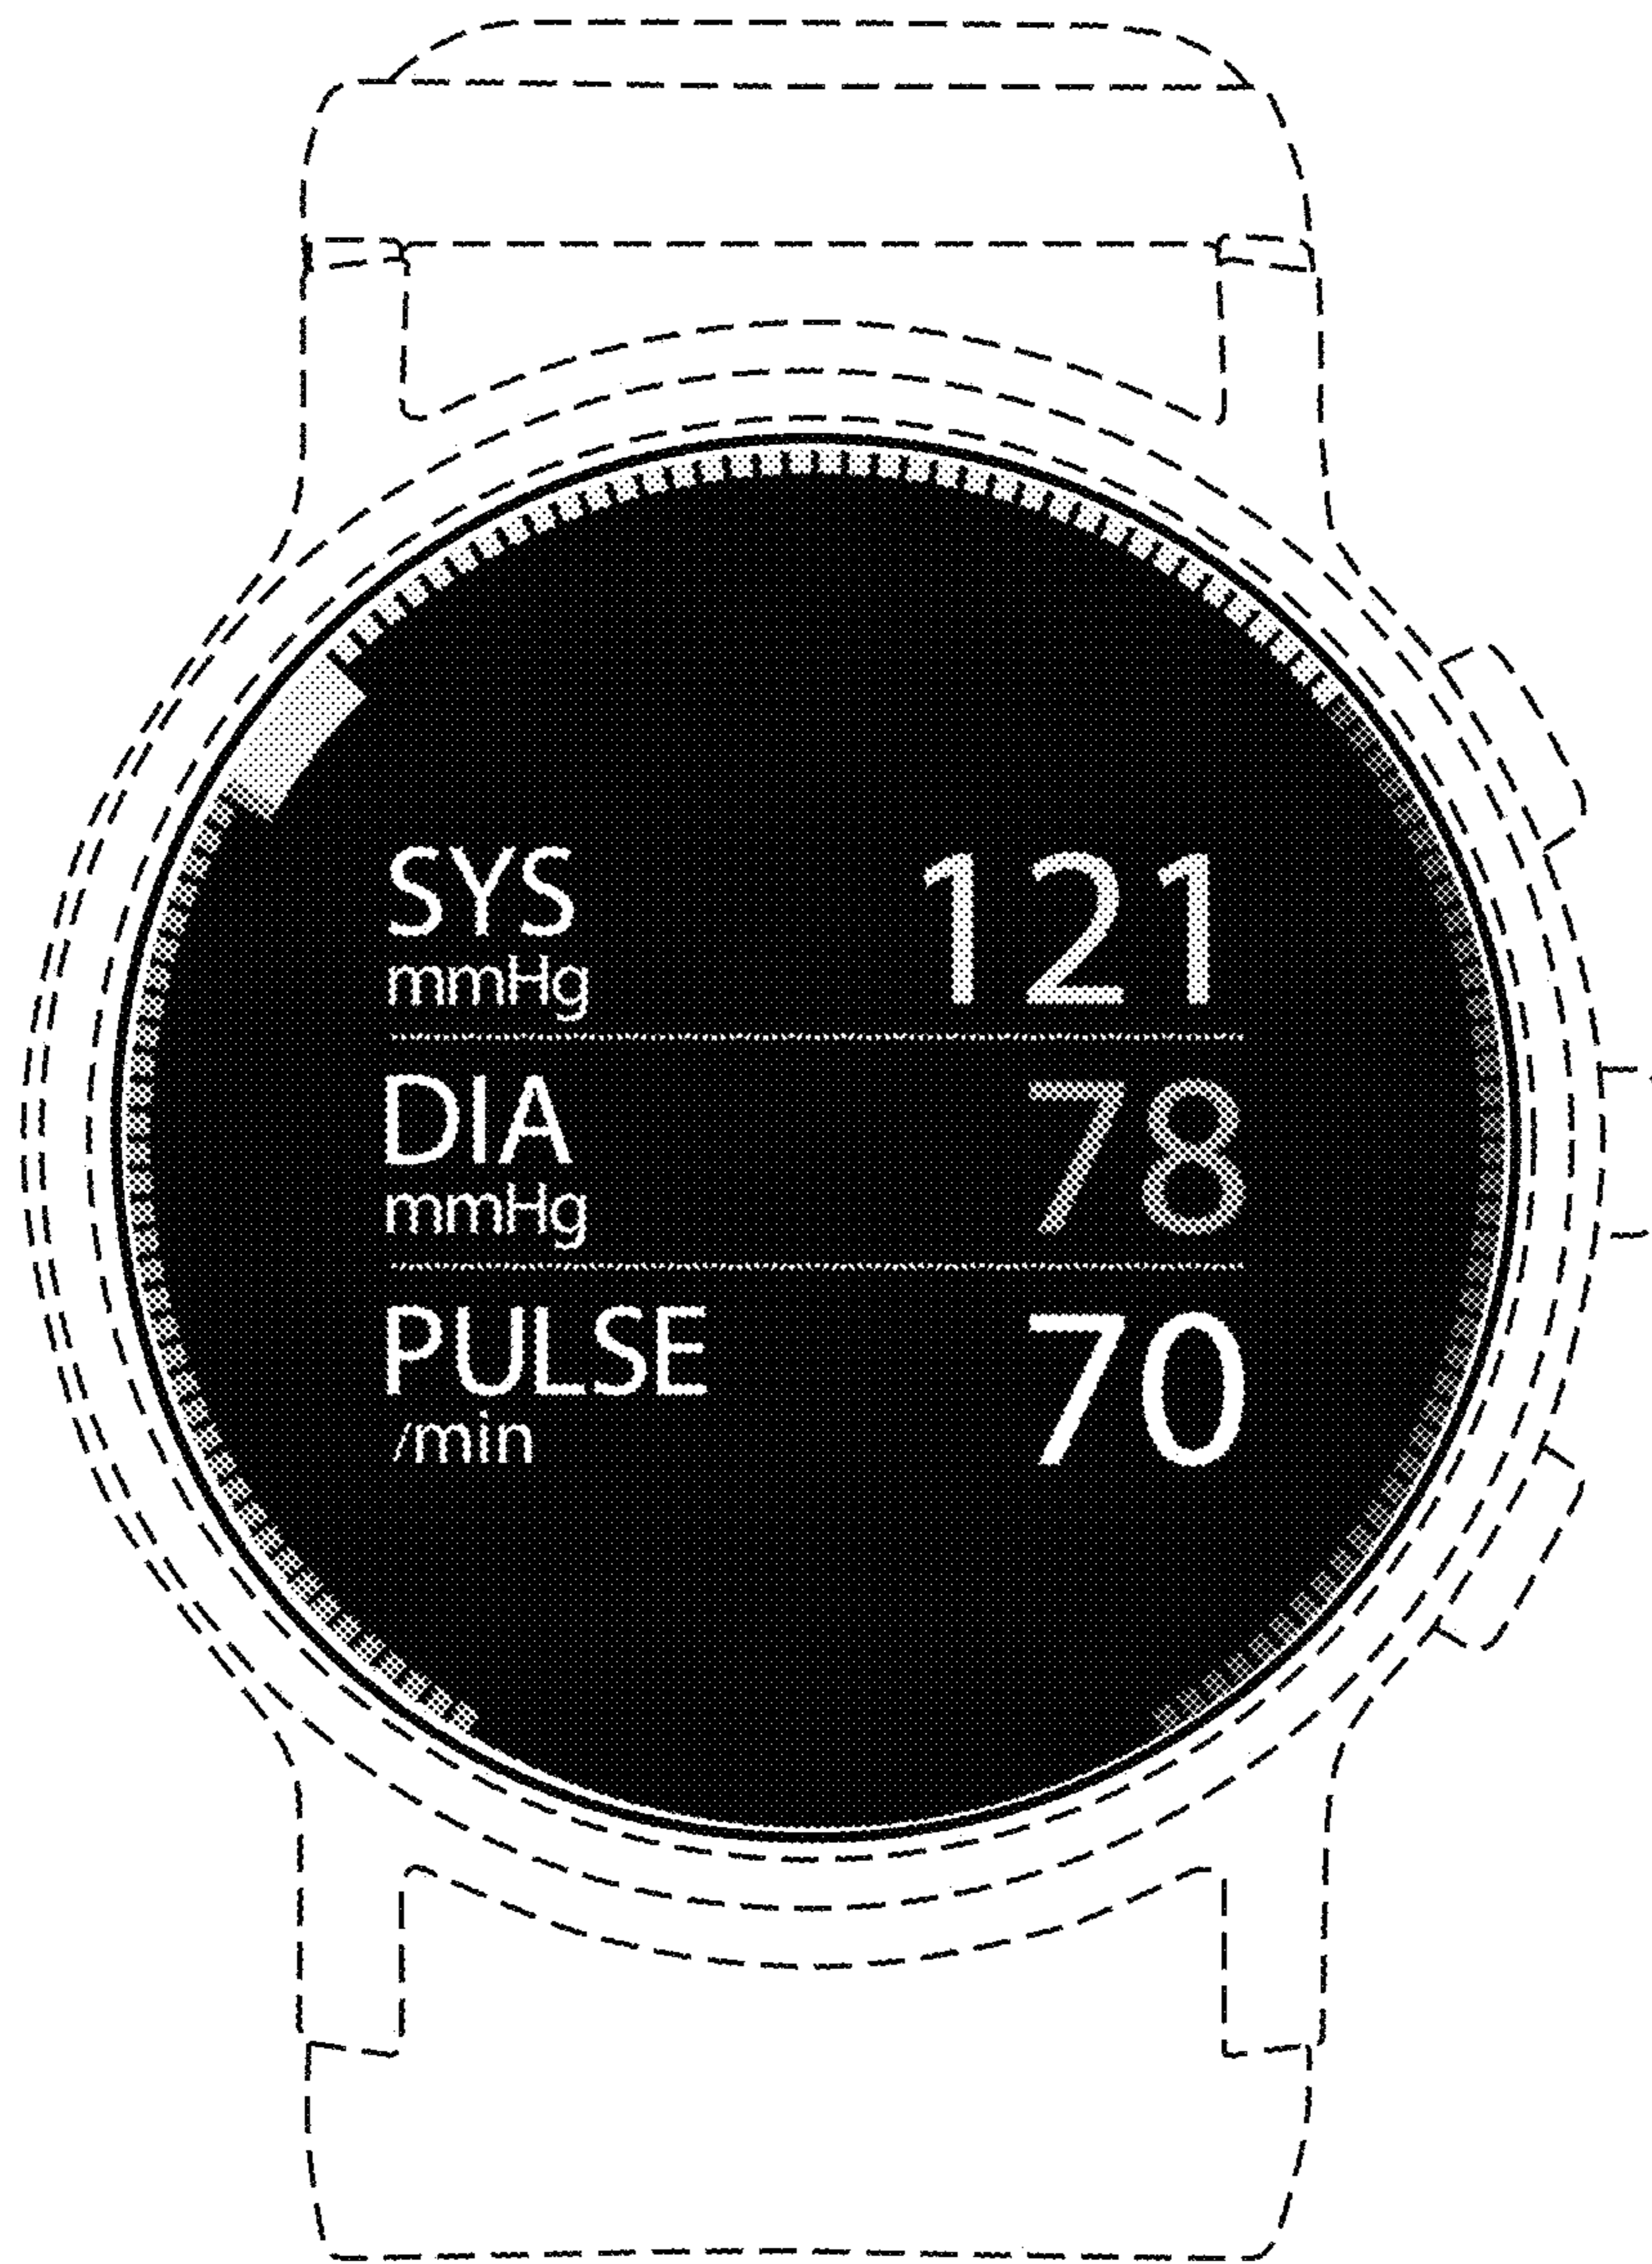

**FIG.2**

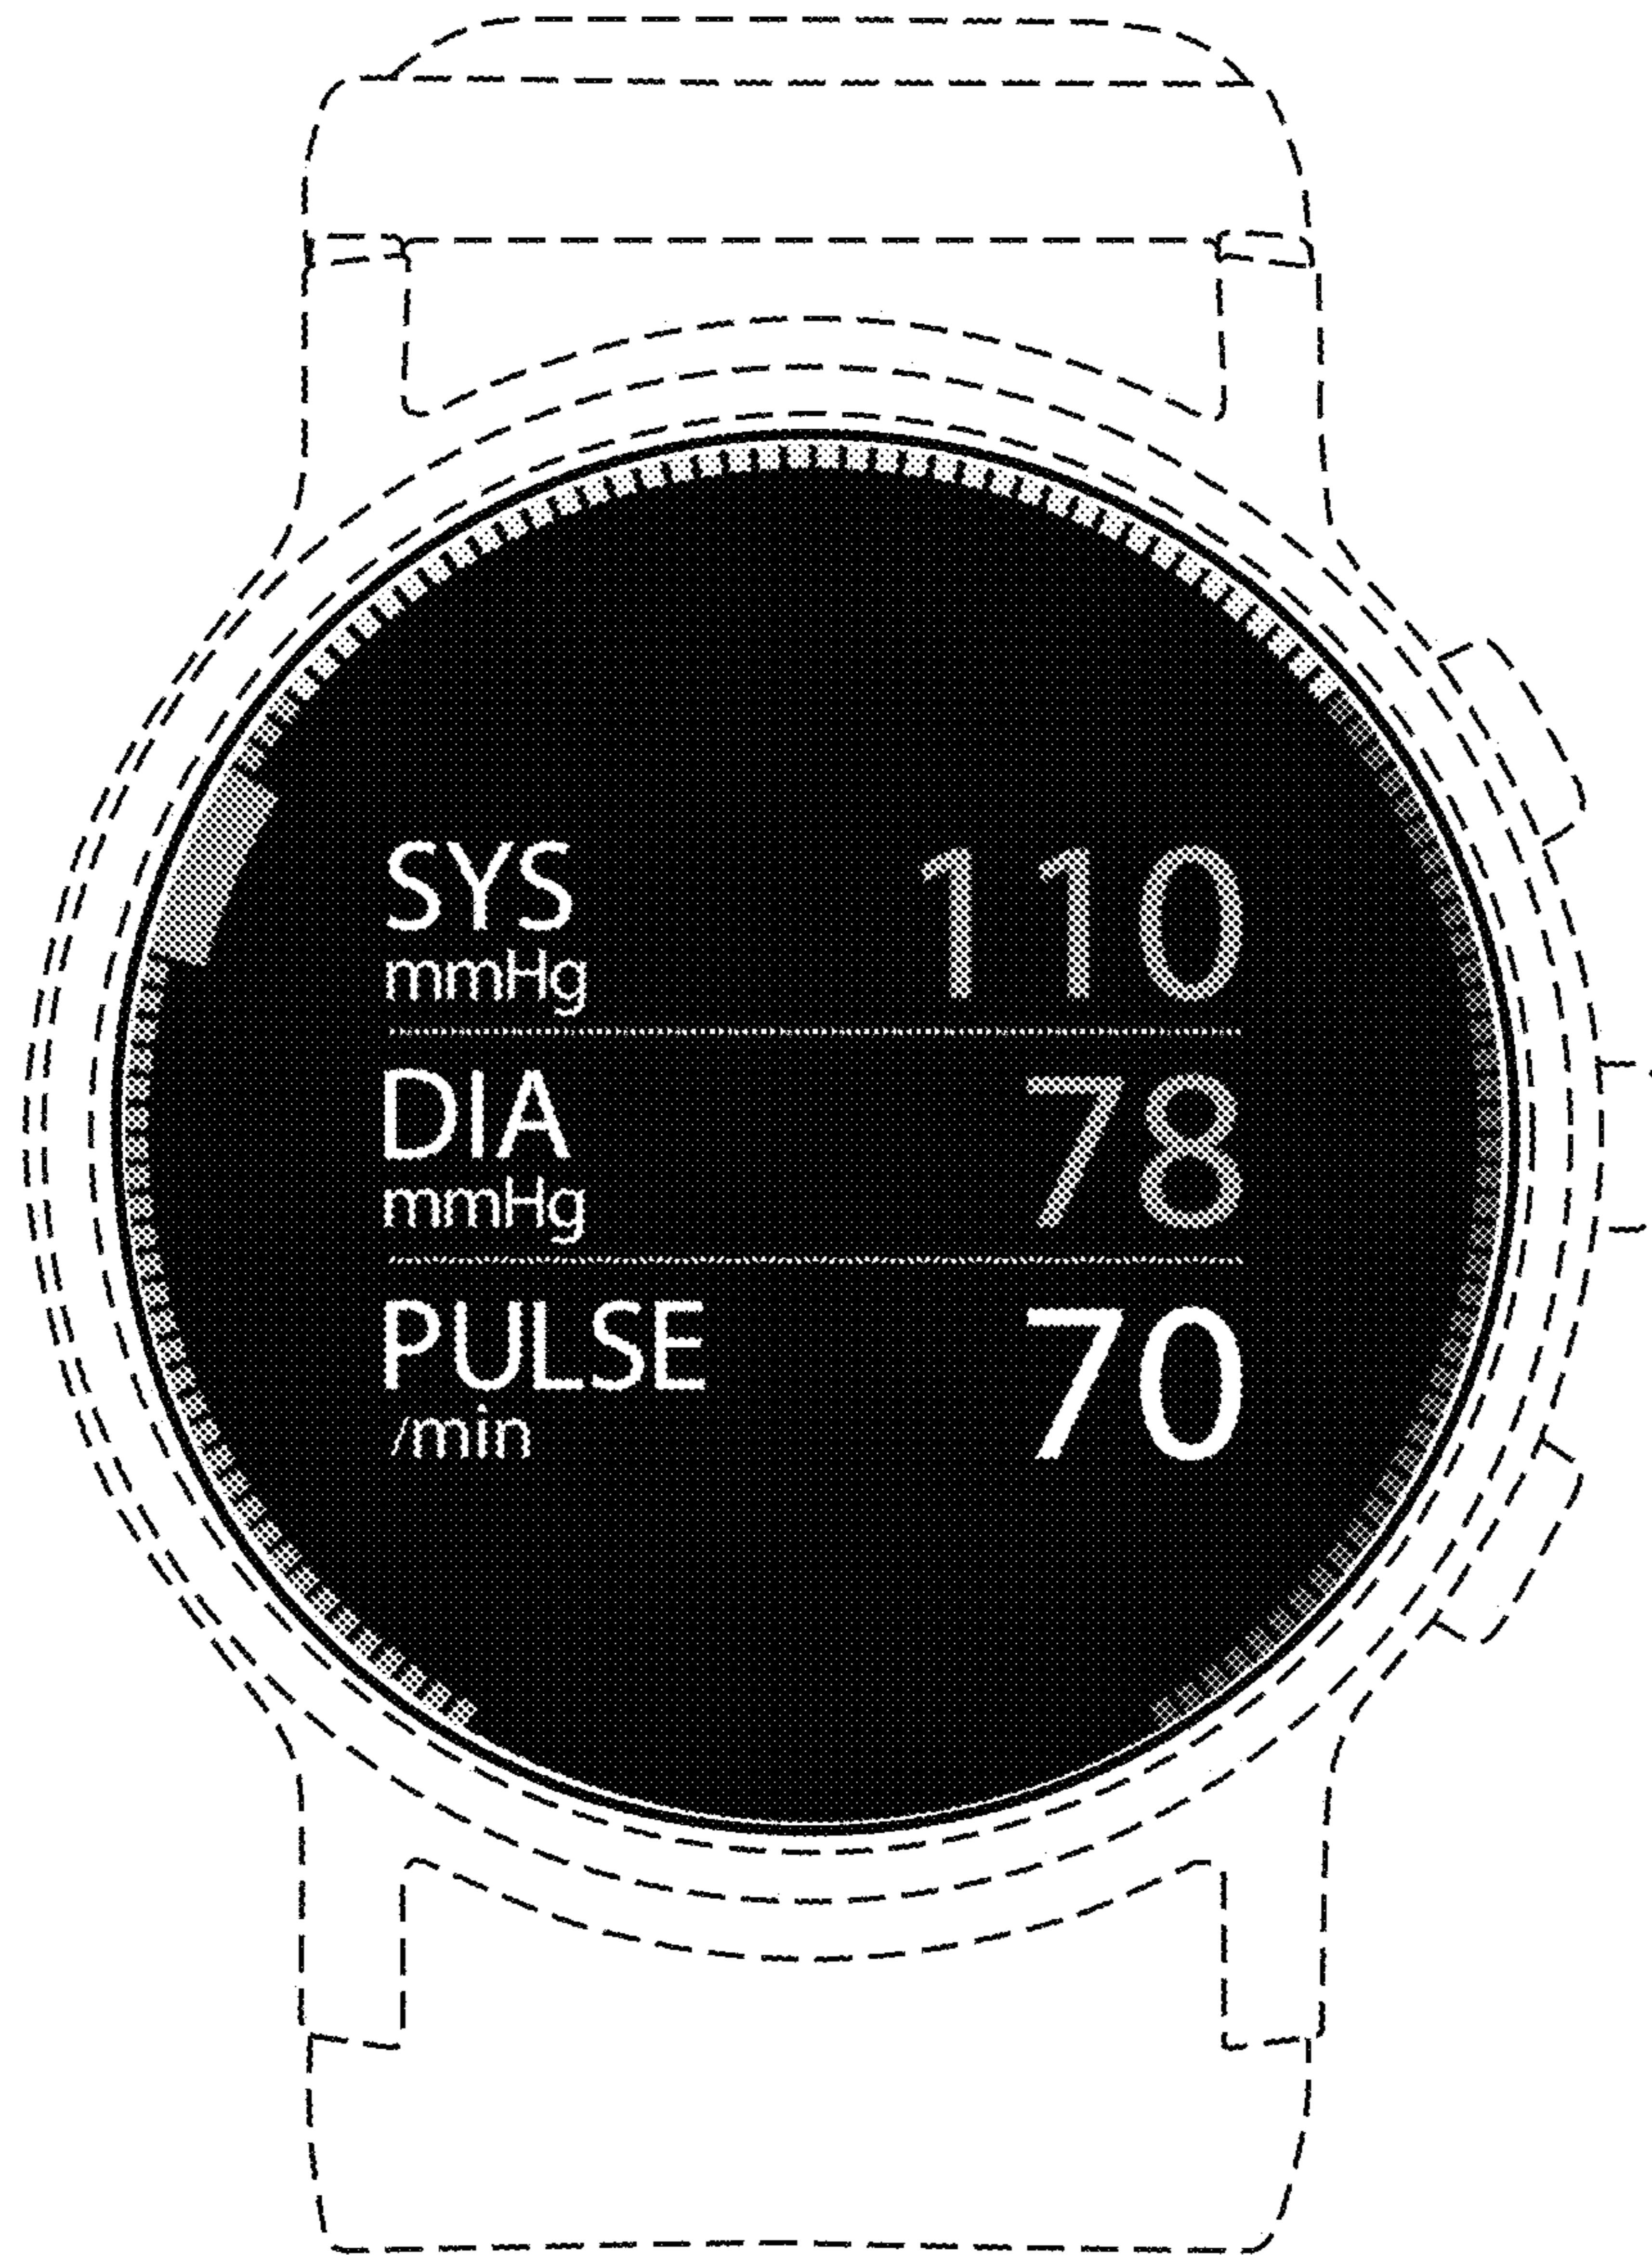

**FIG.3**

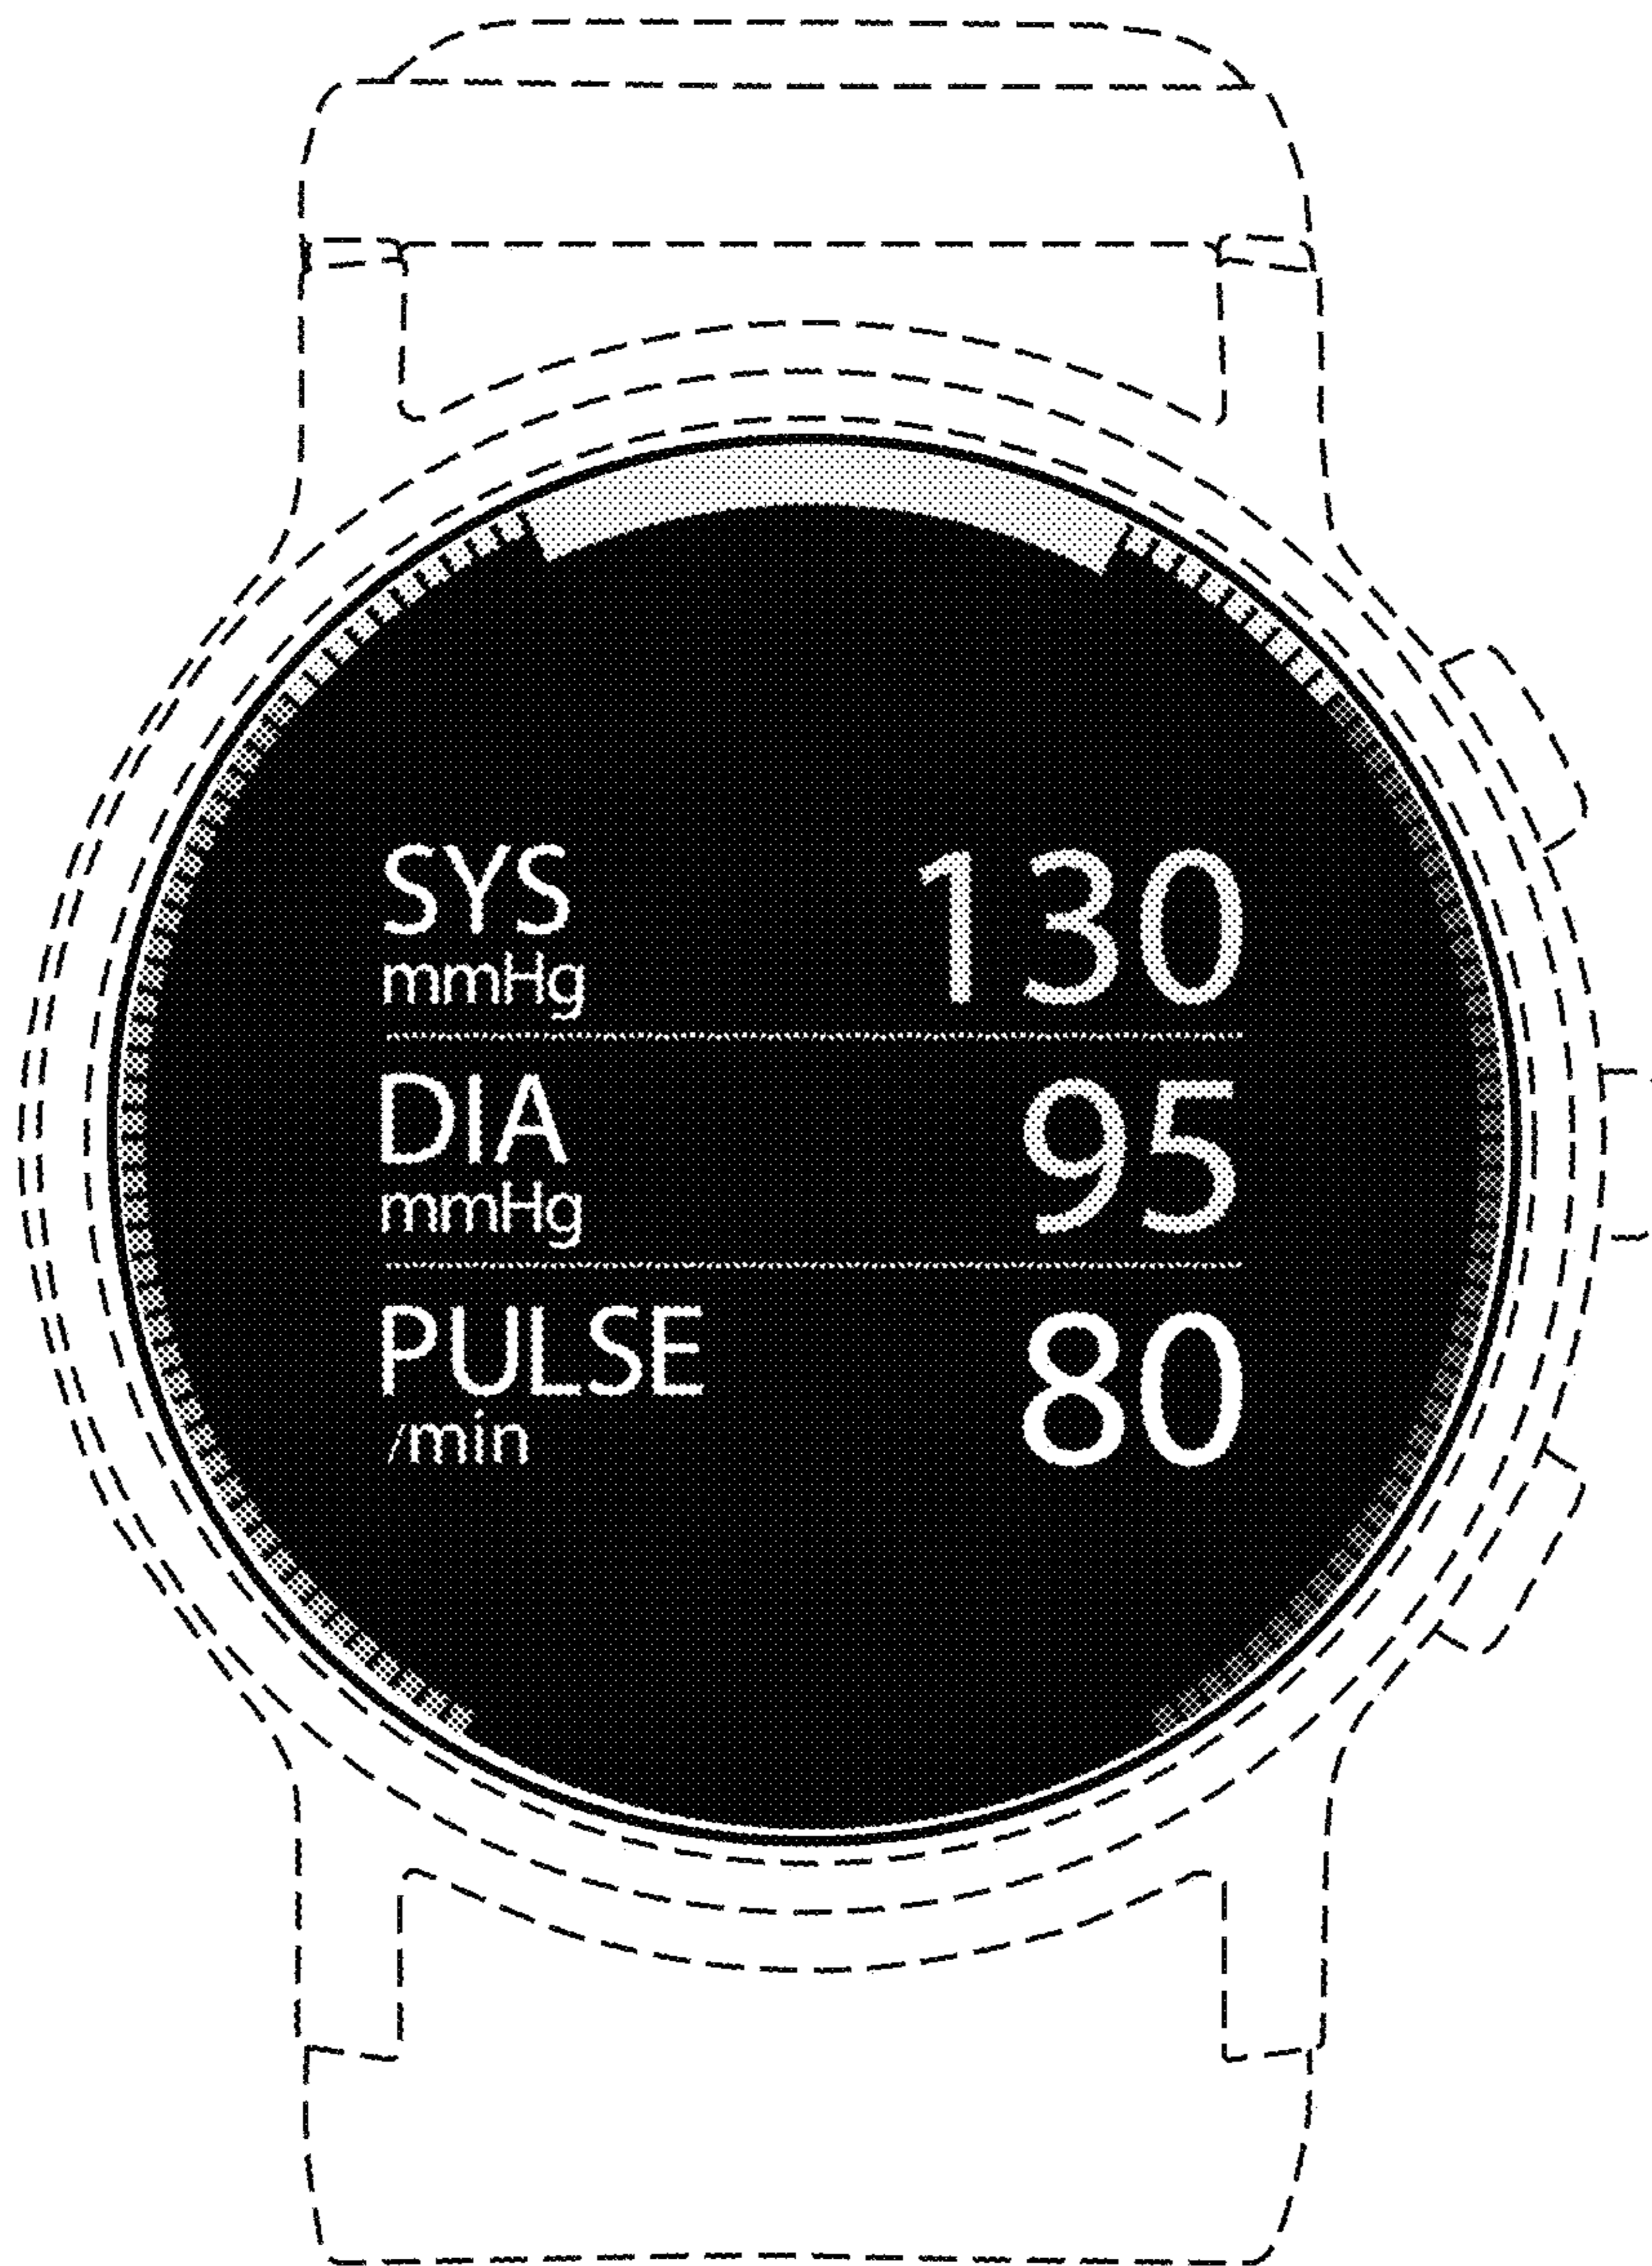

**FIG.4**



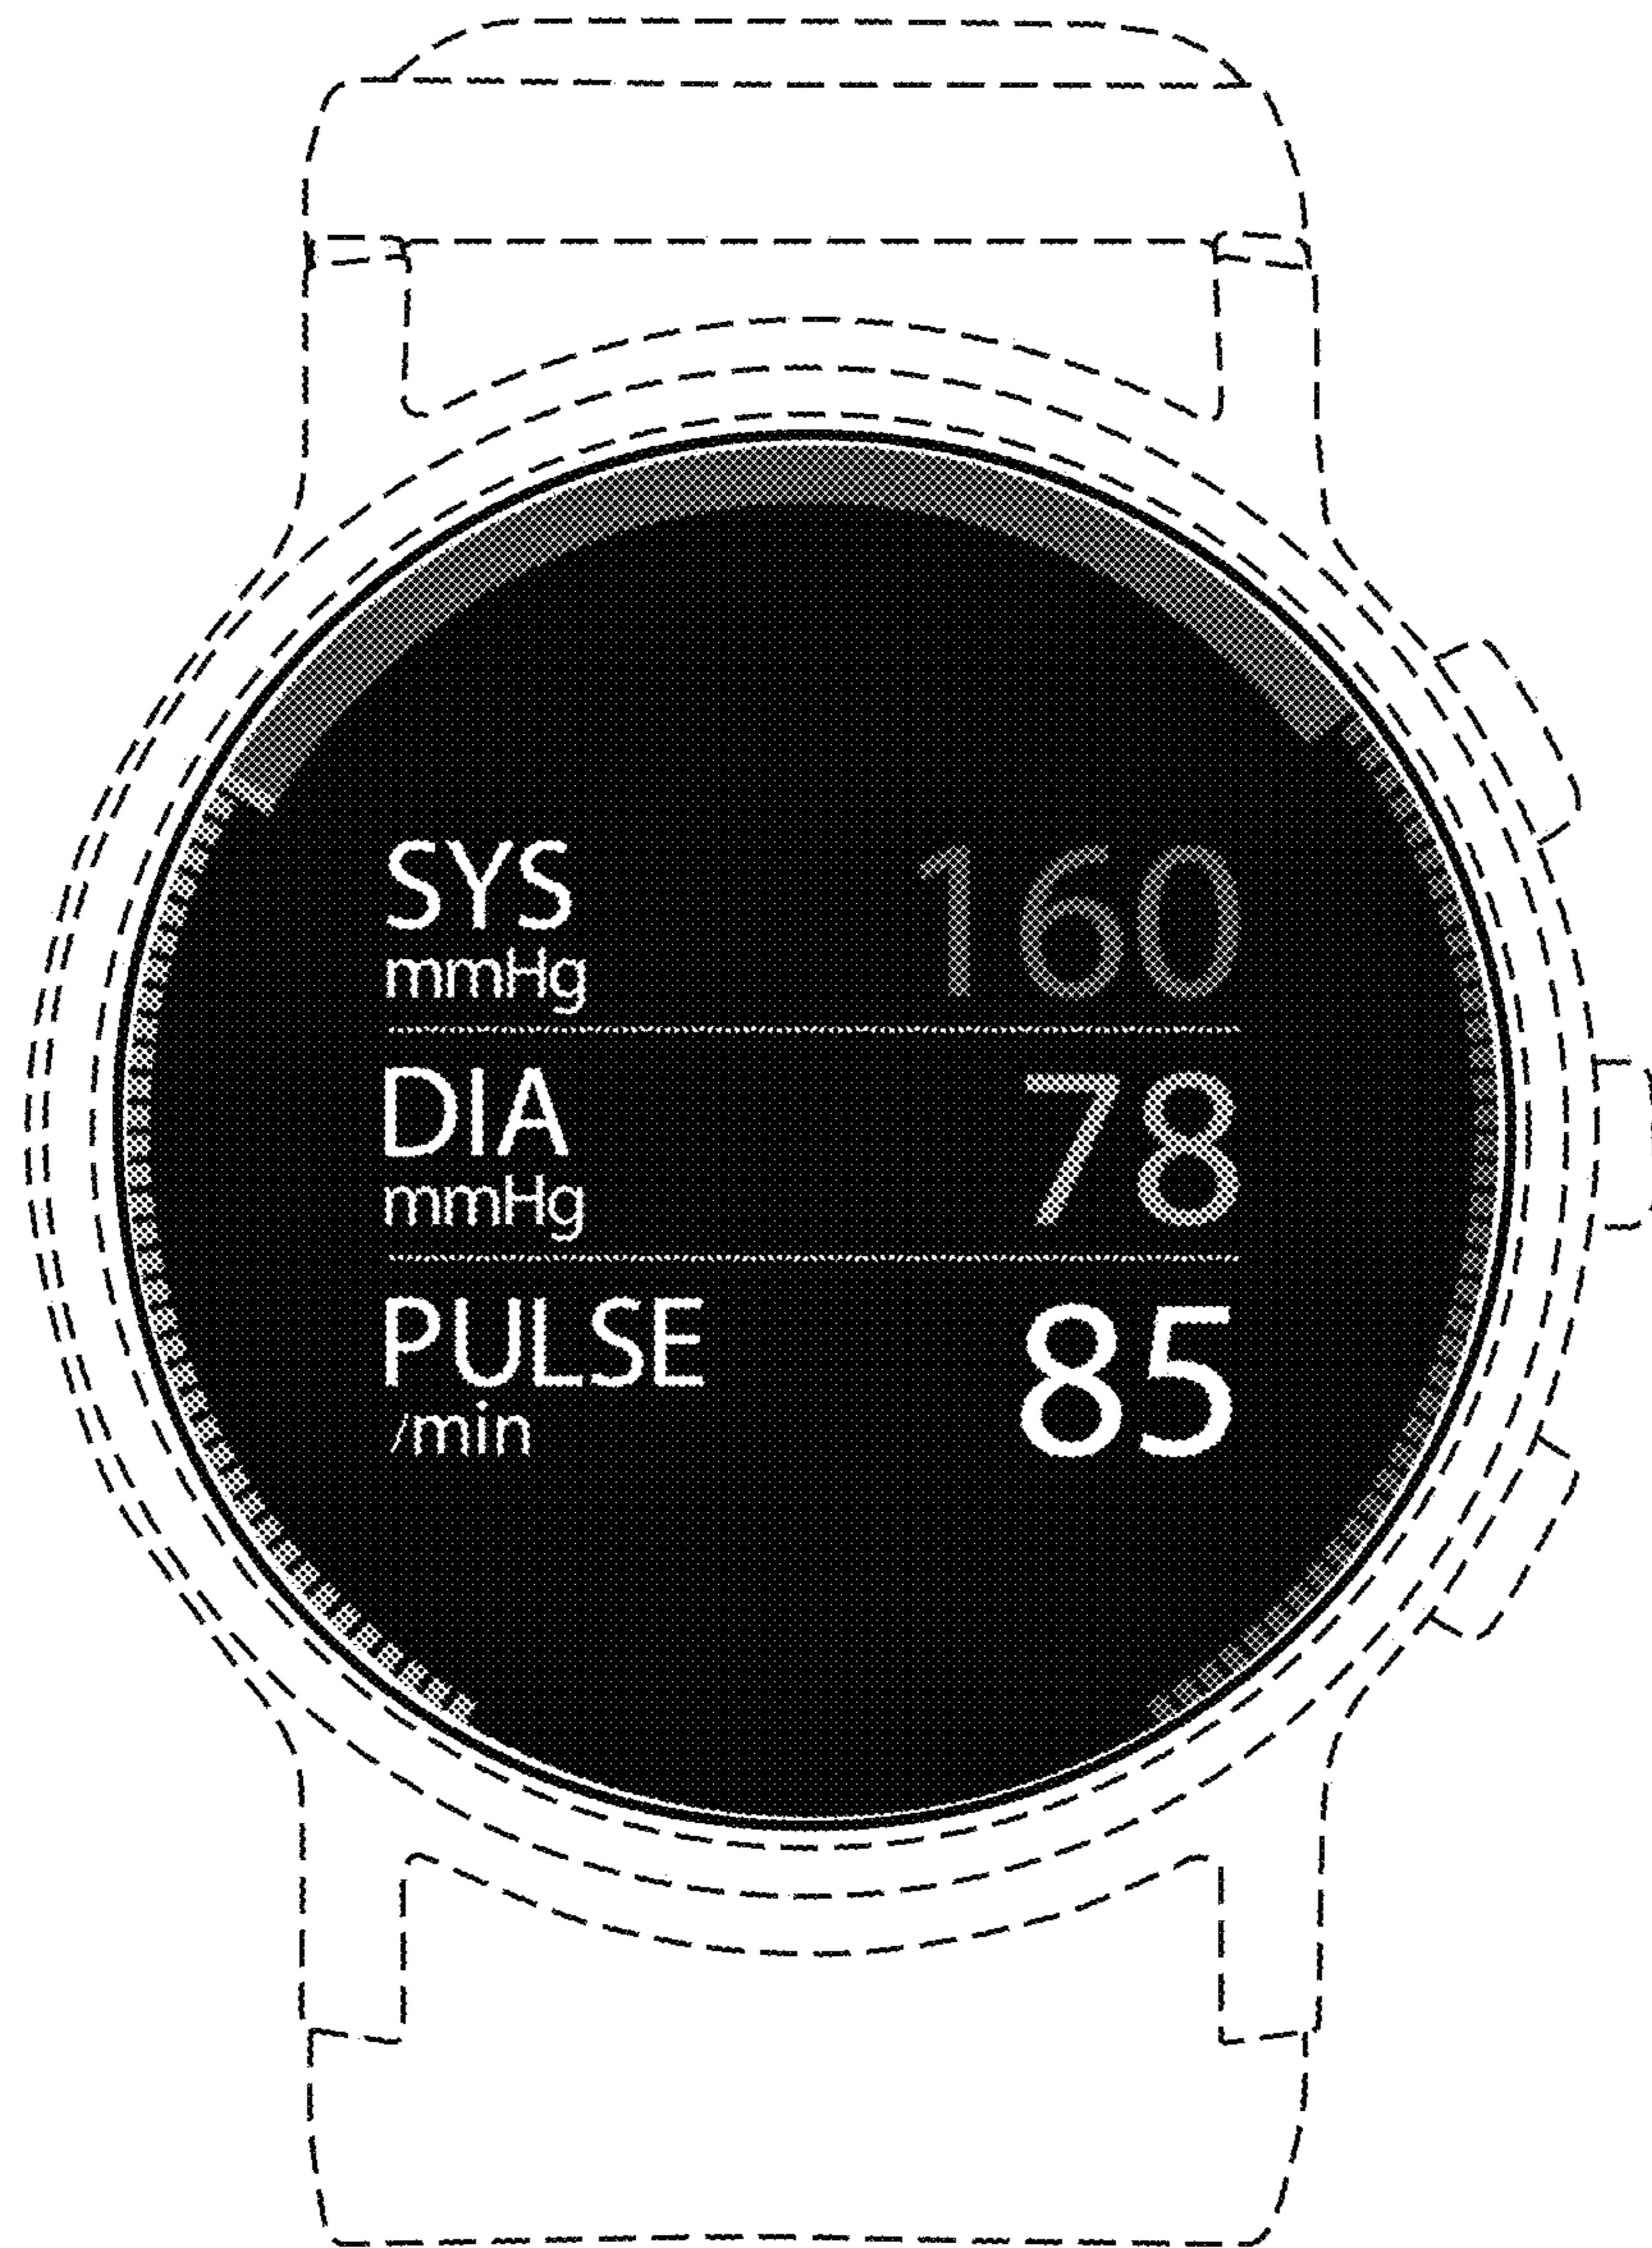


FIG. 5




**FIG.6**

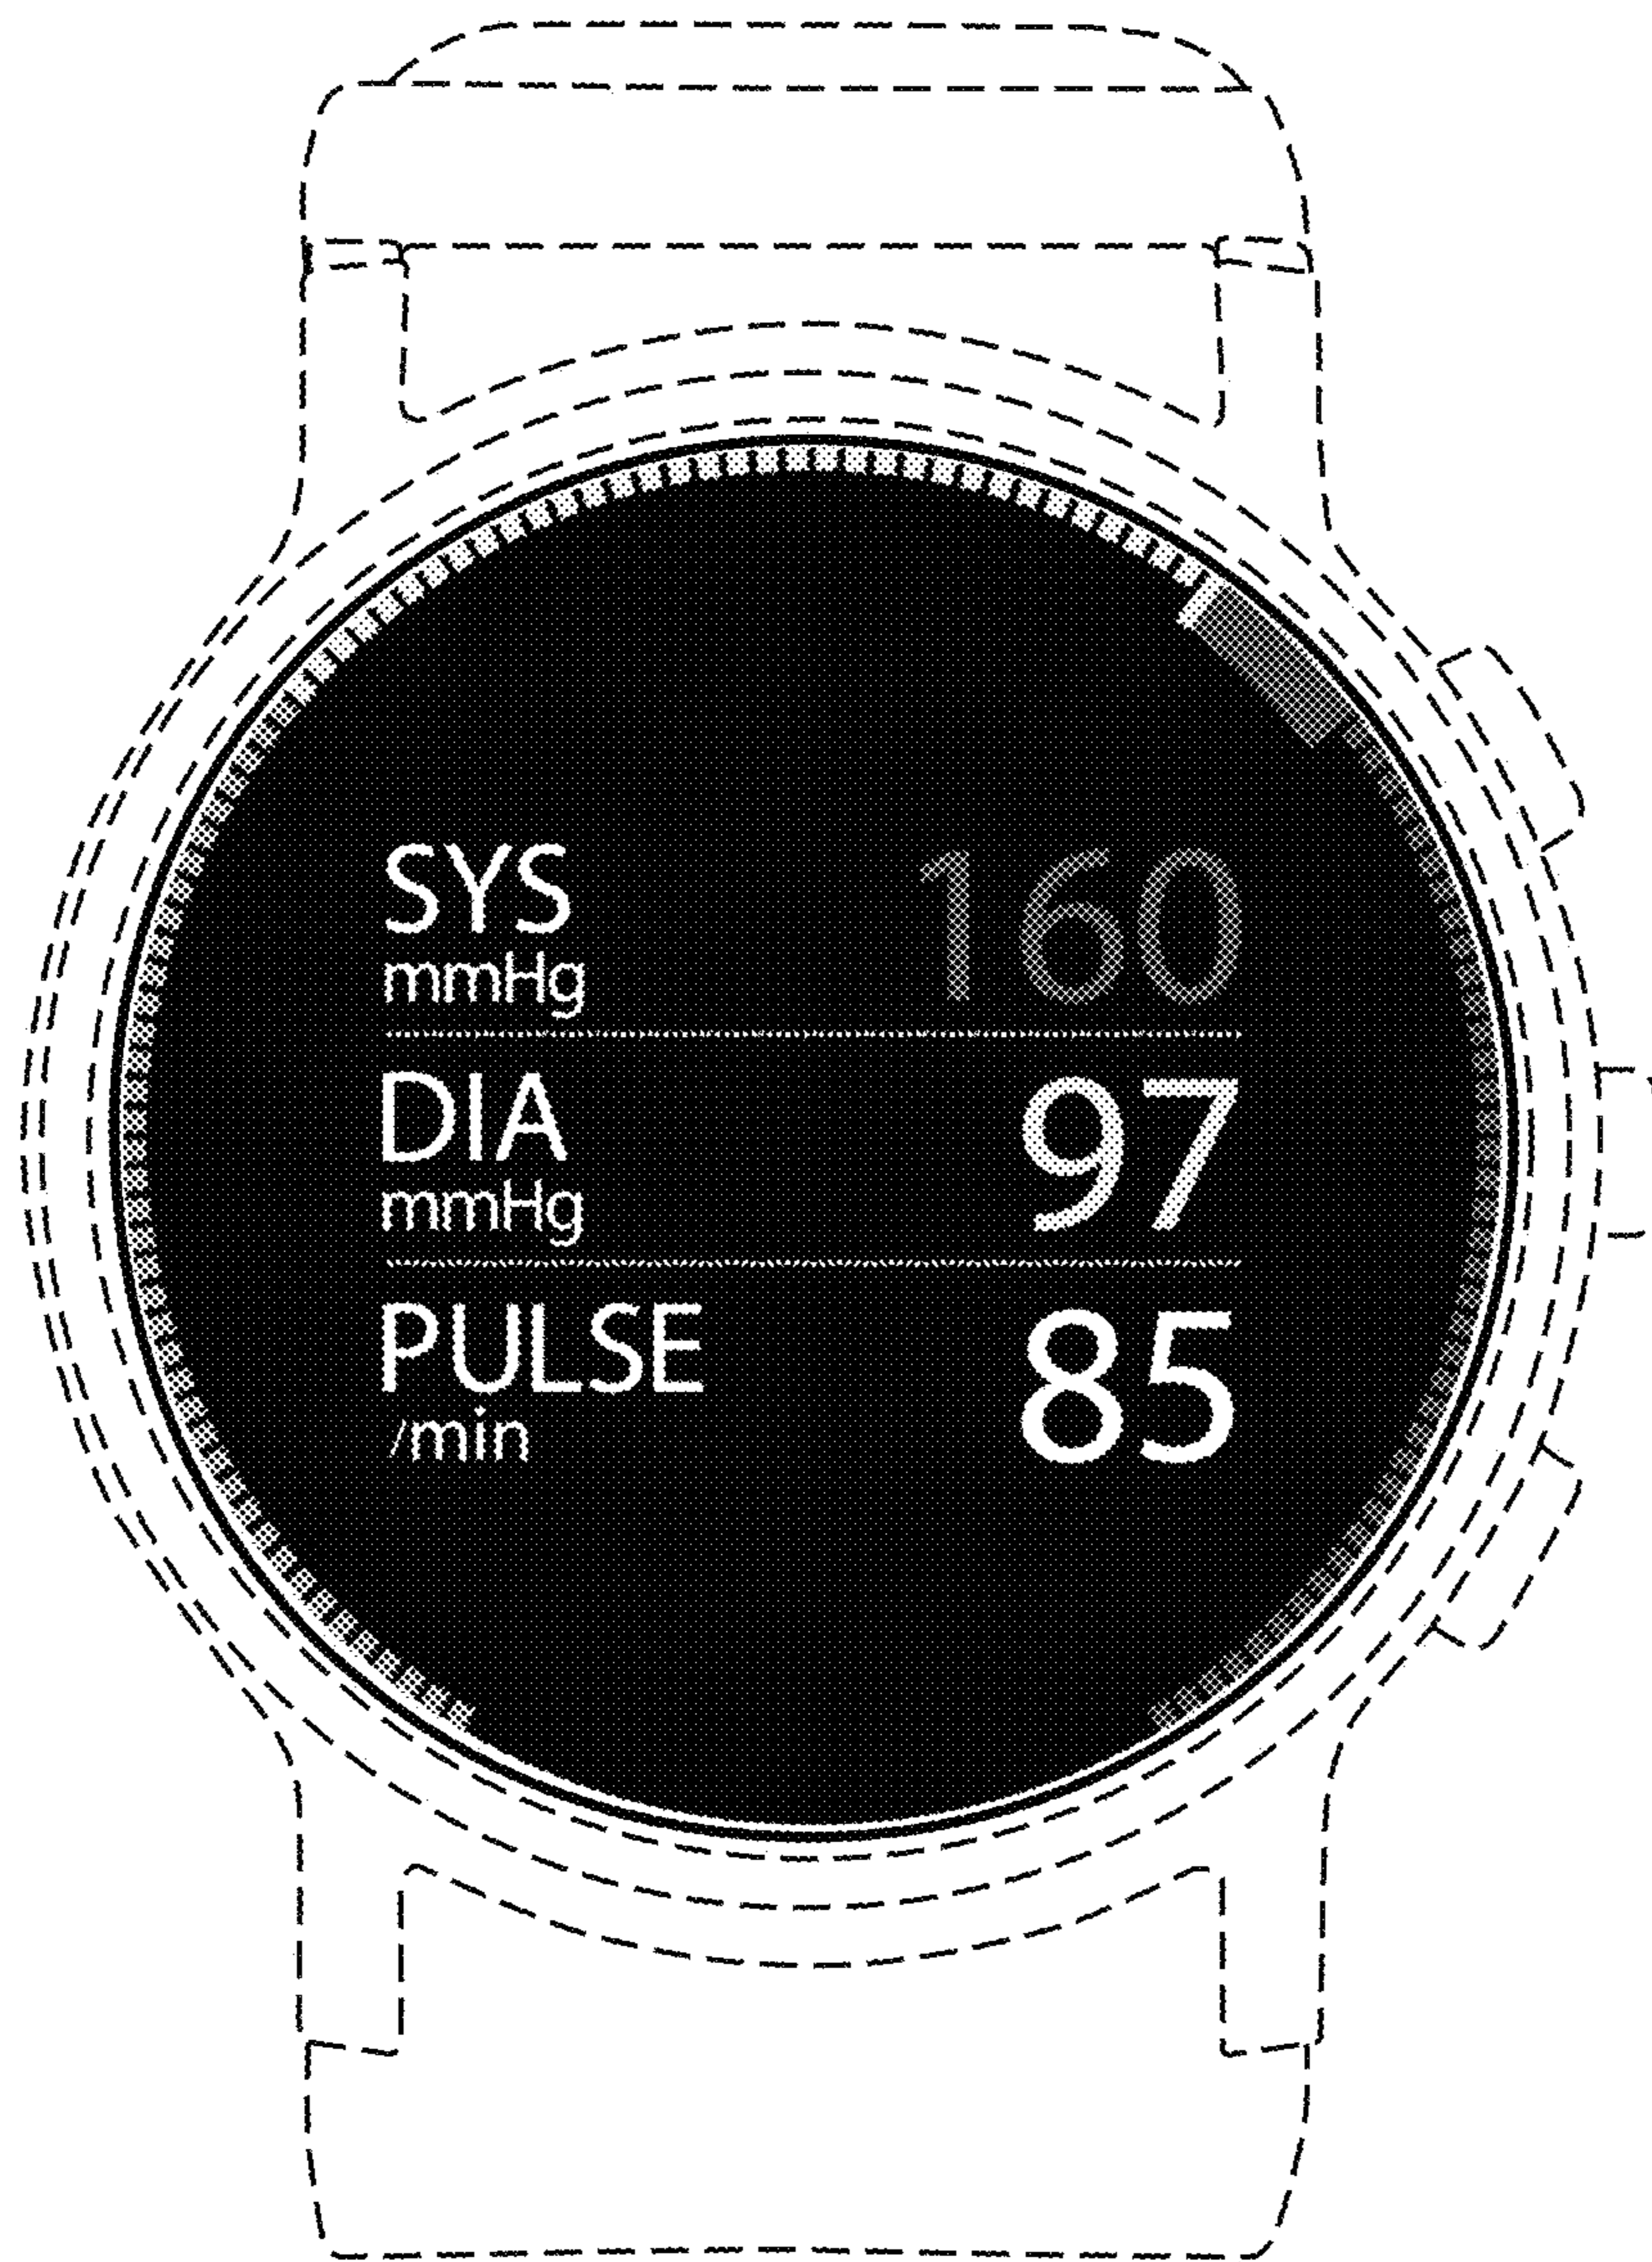


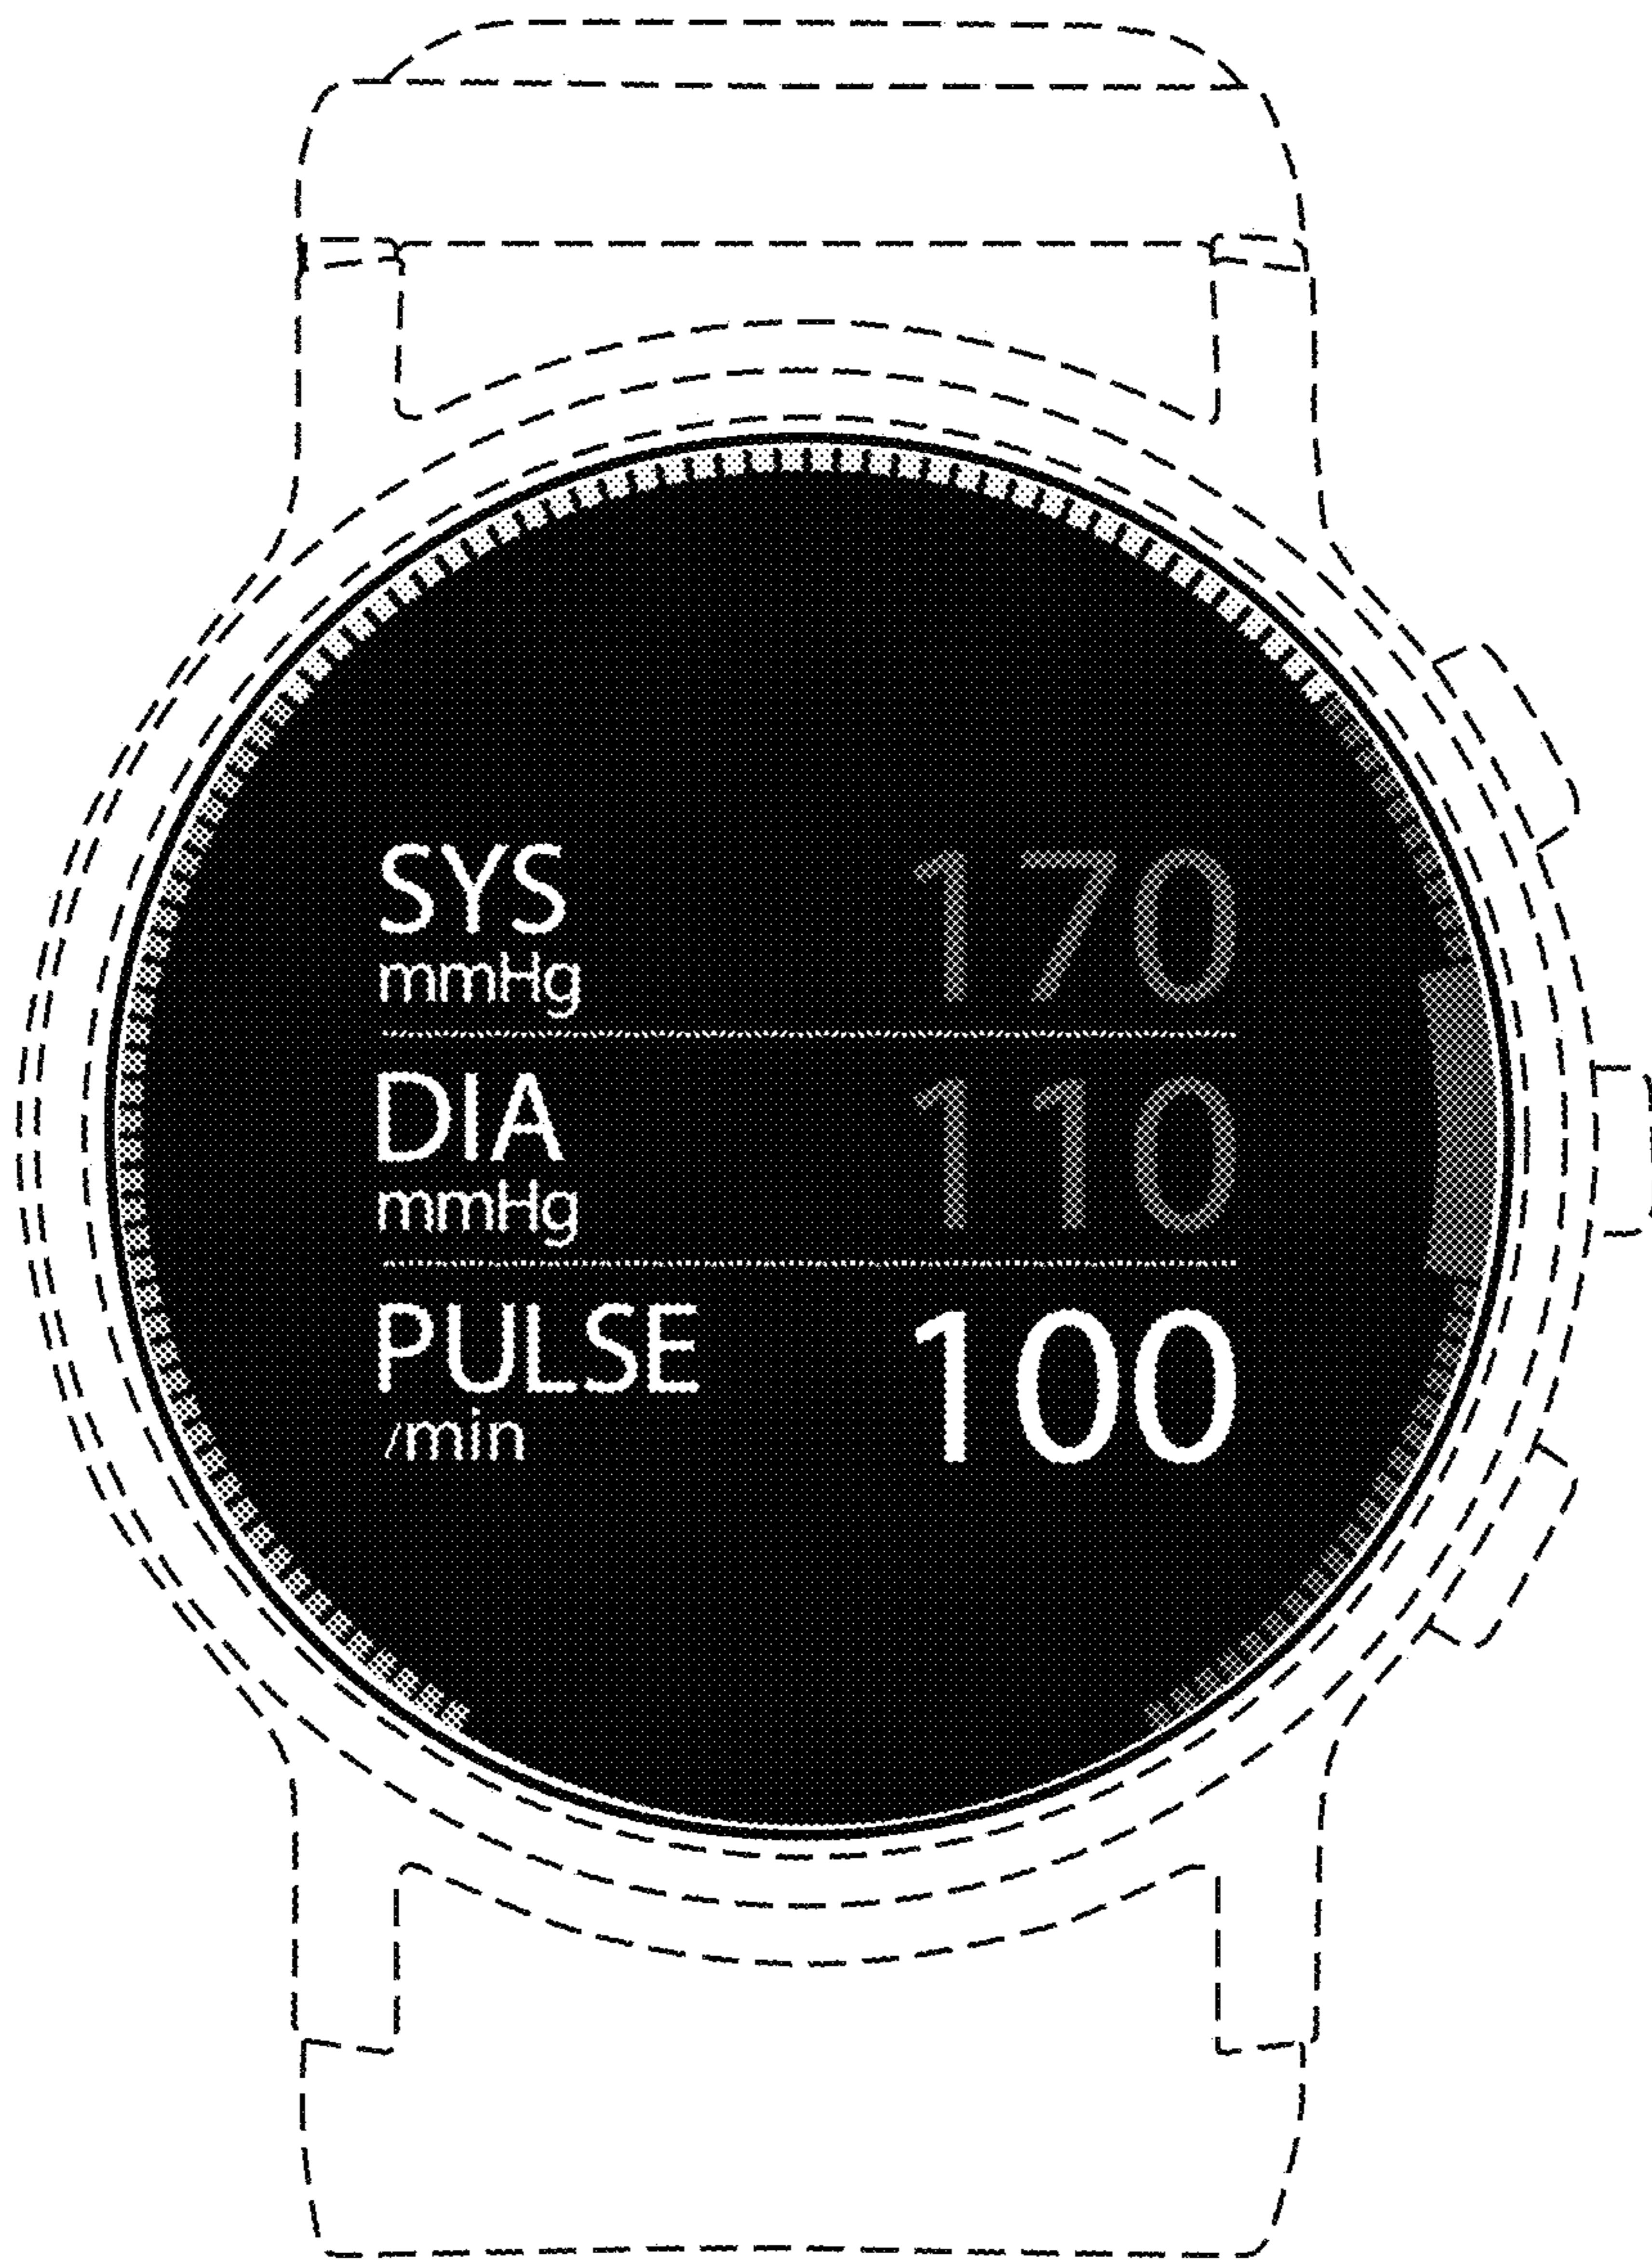


**FIG. 7**

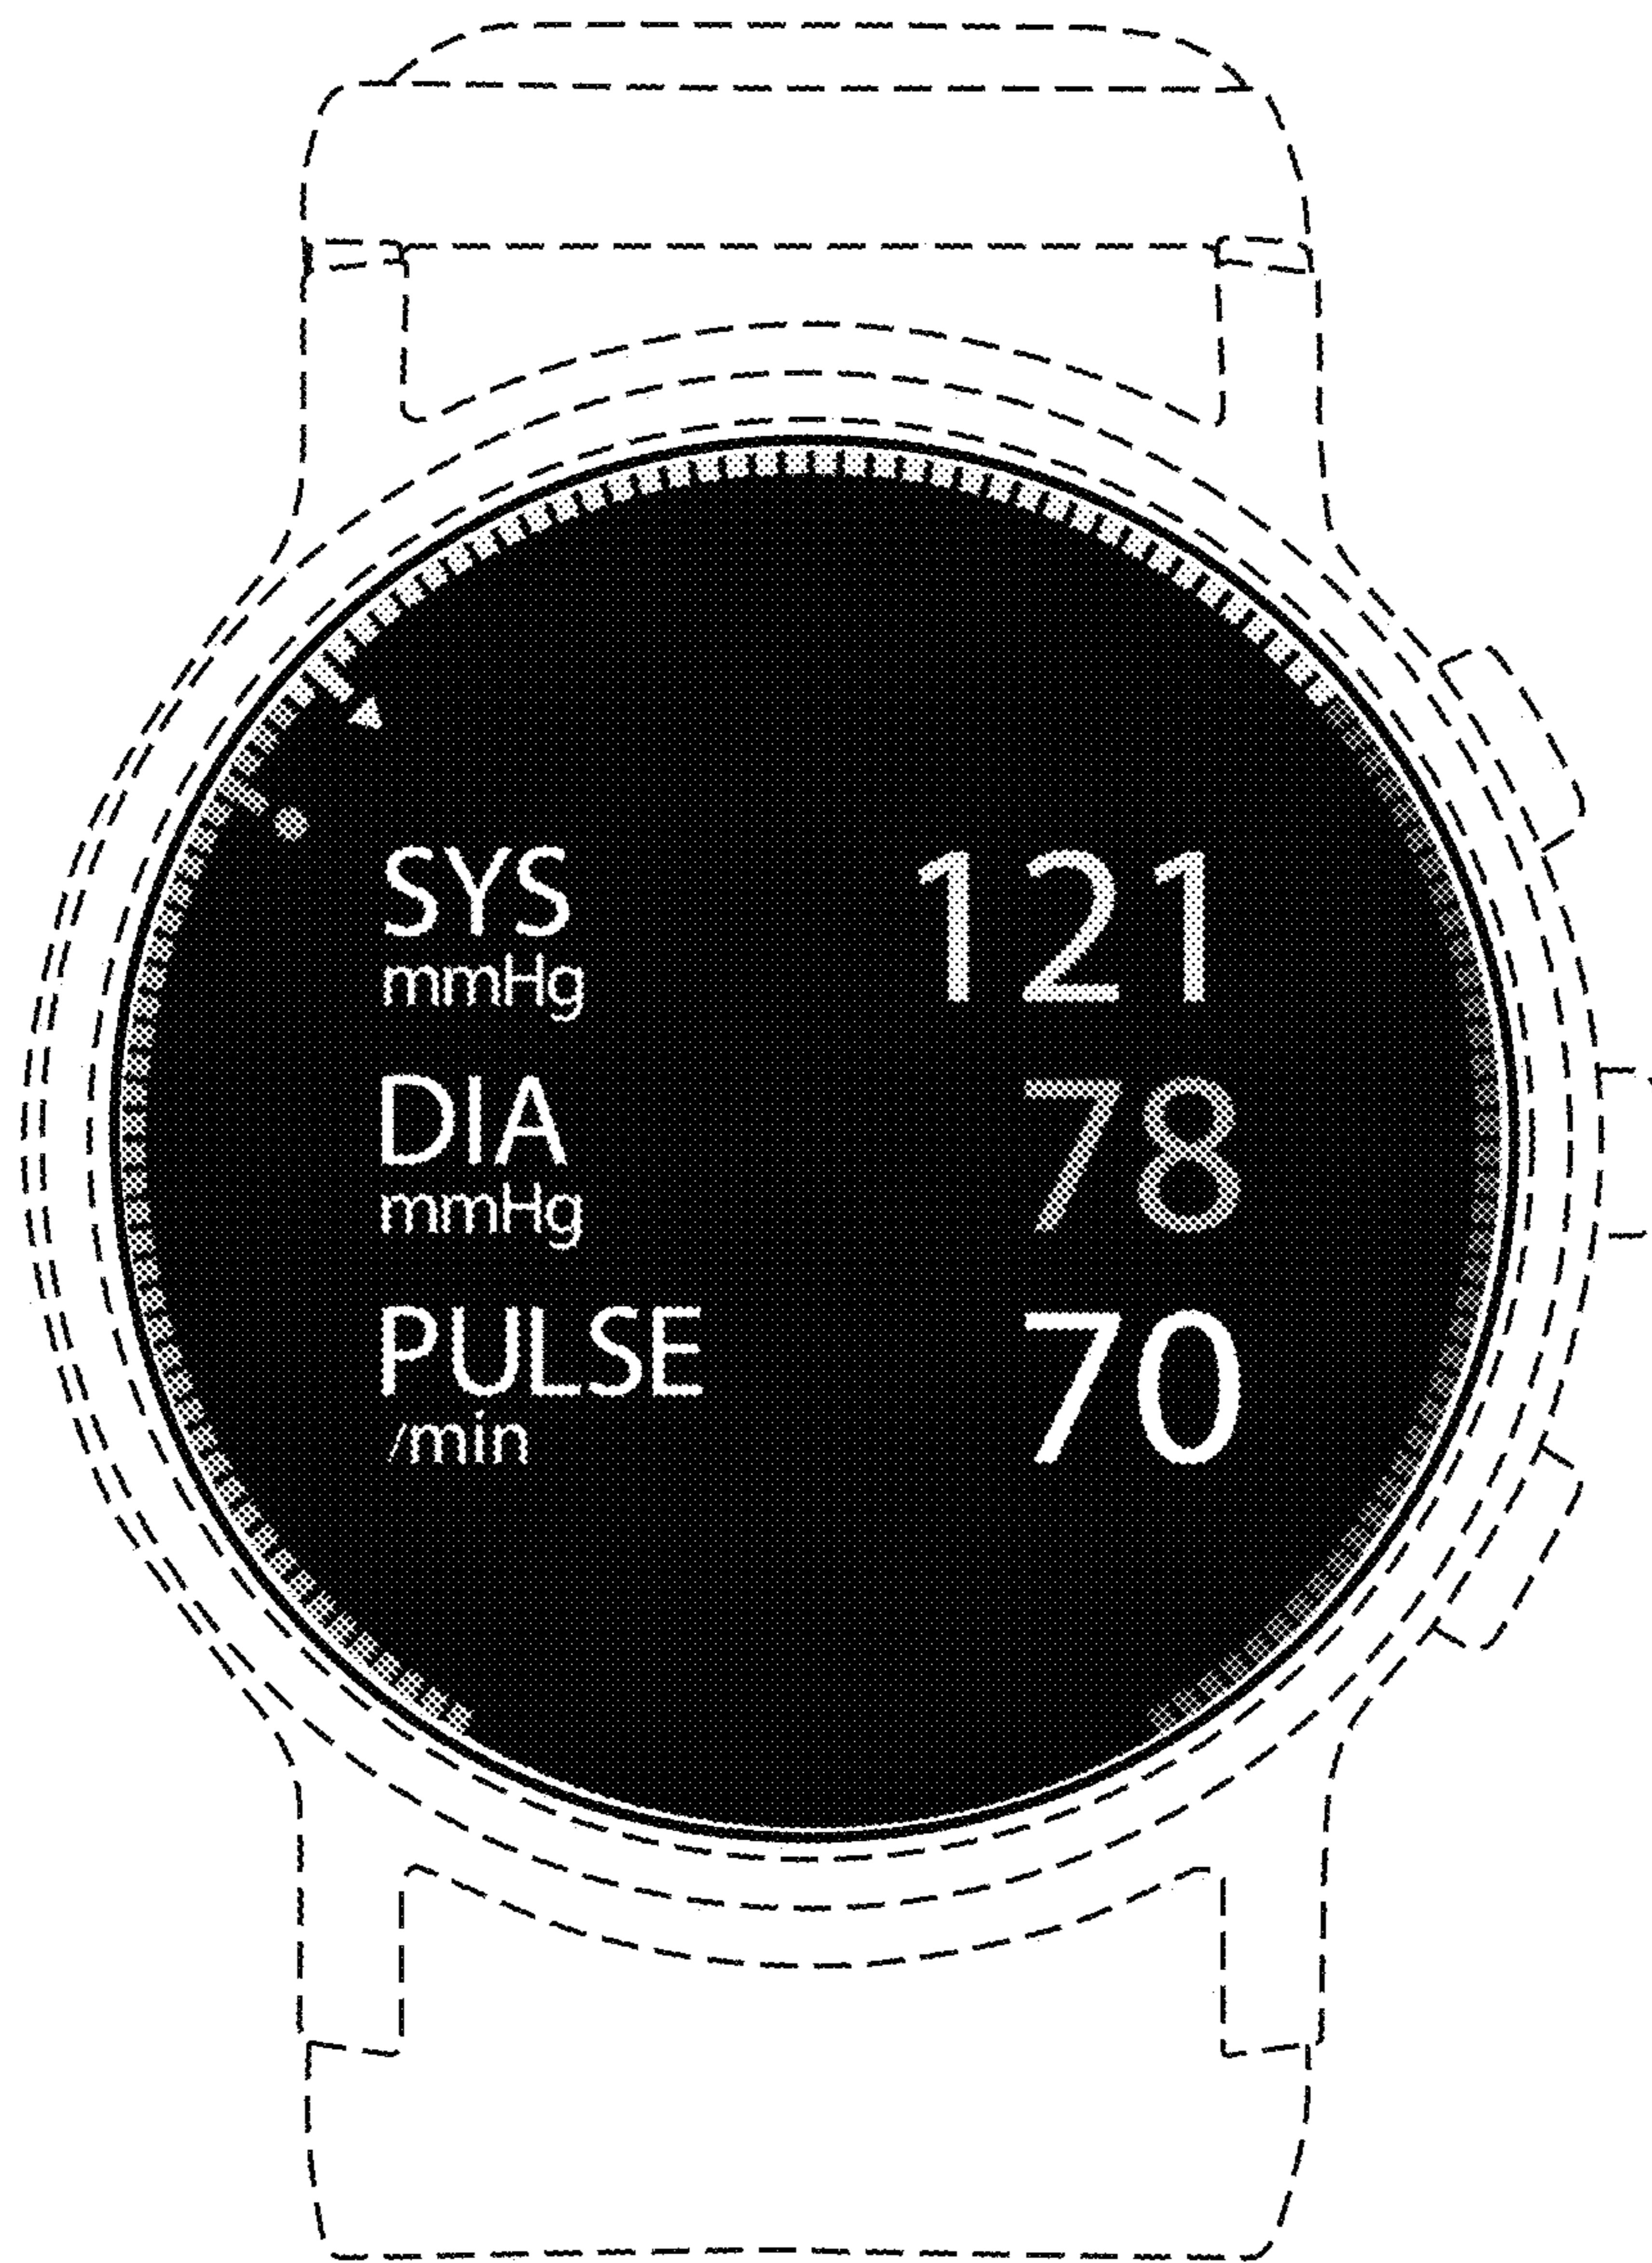


**FIG. 8**

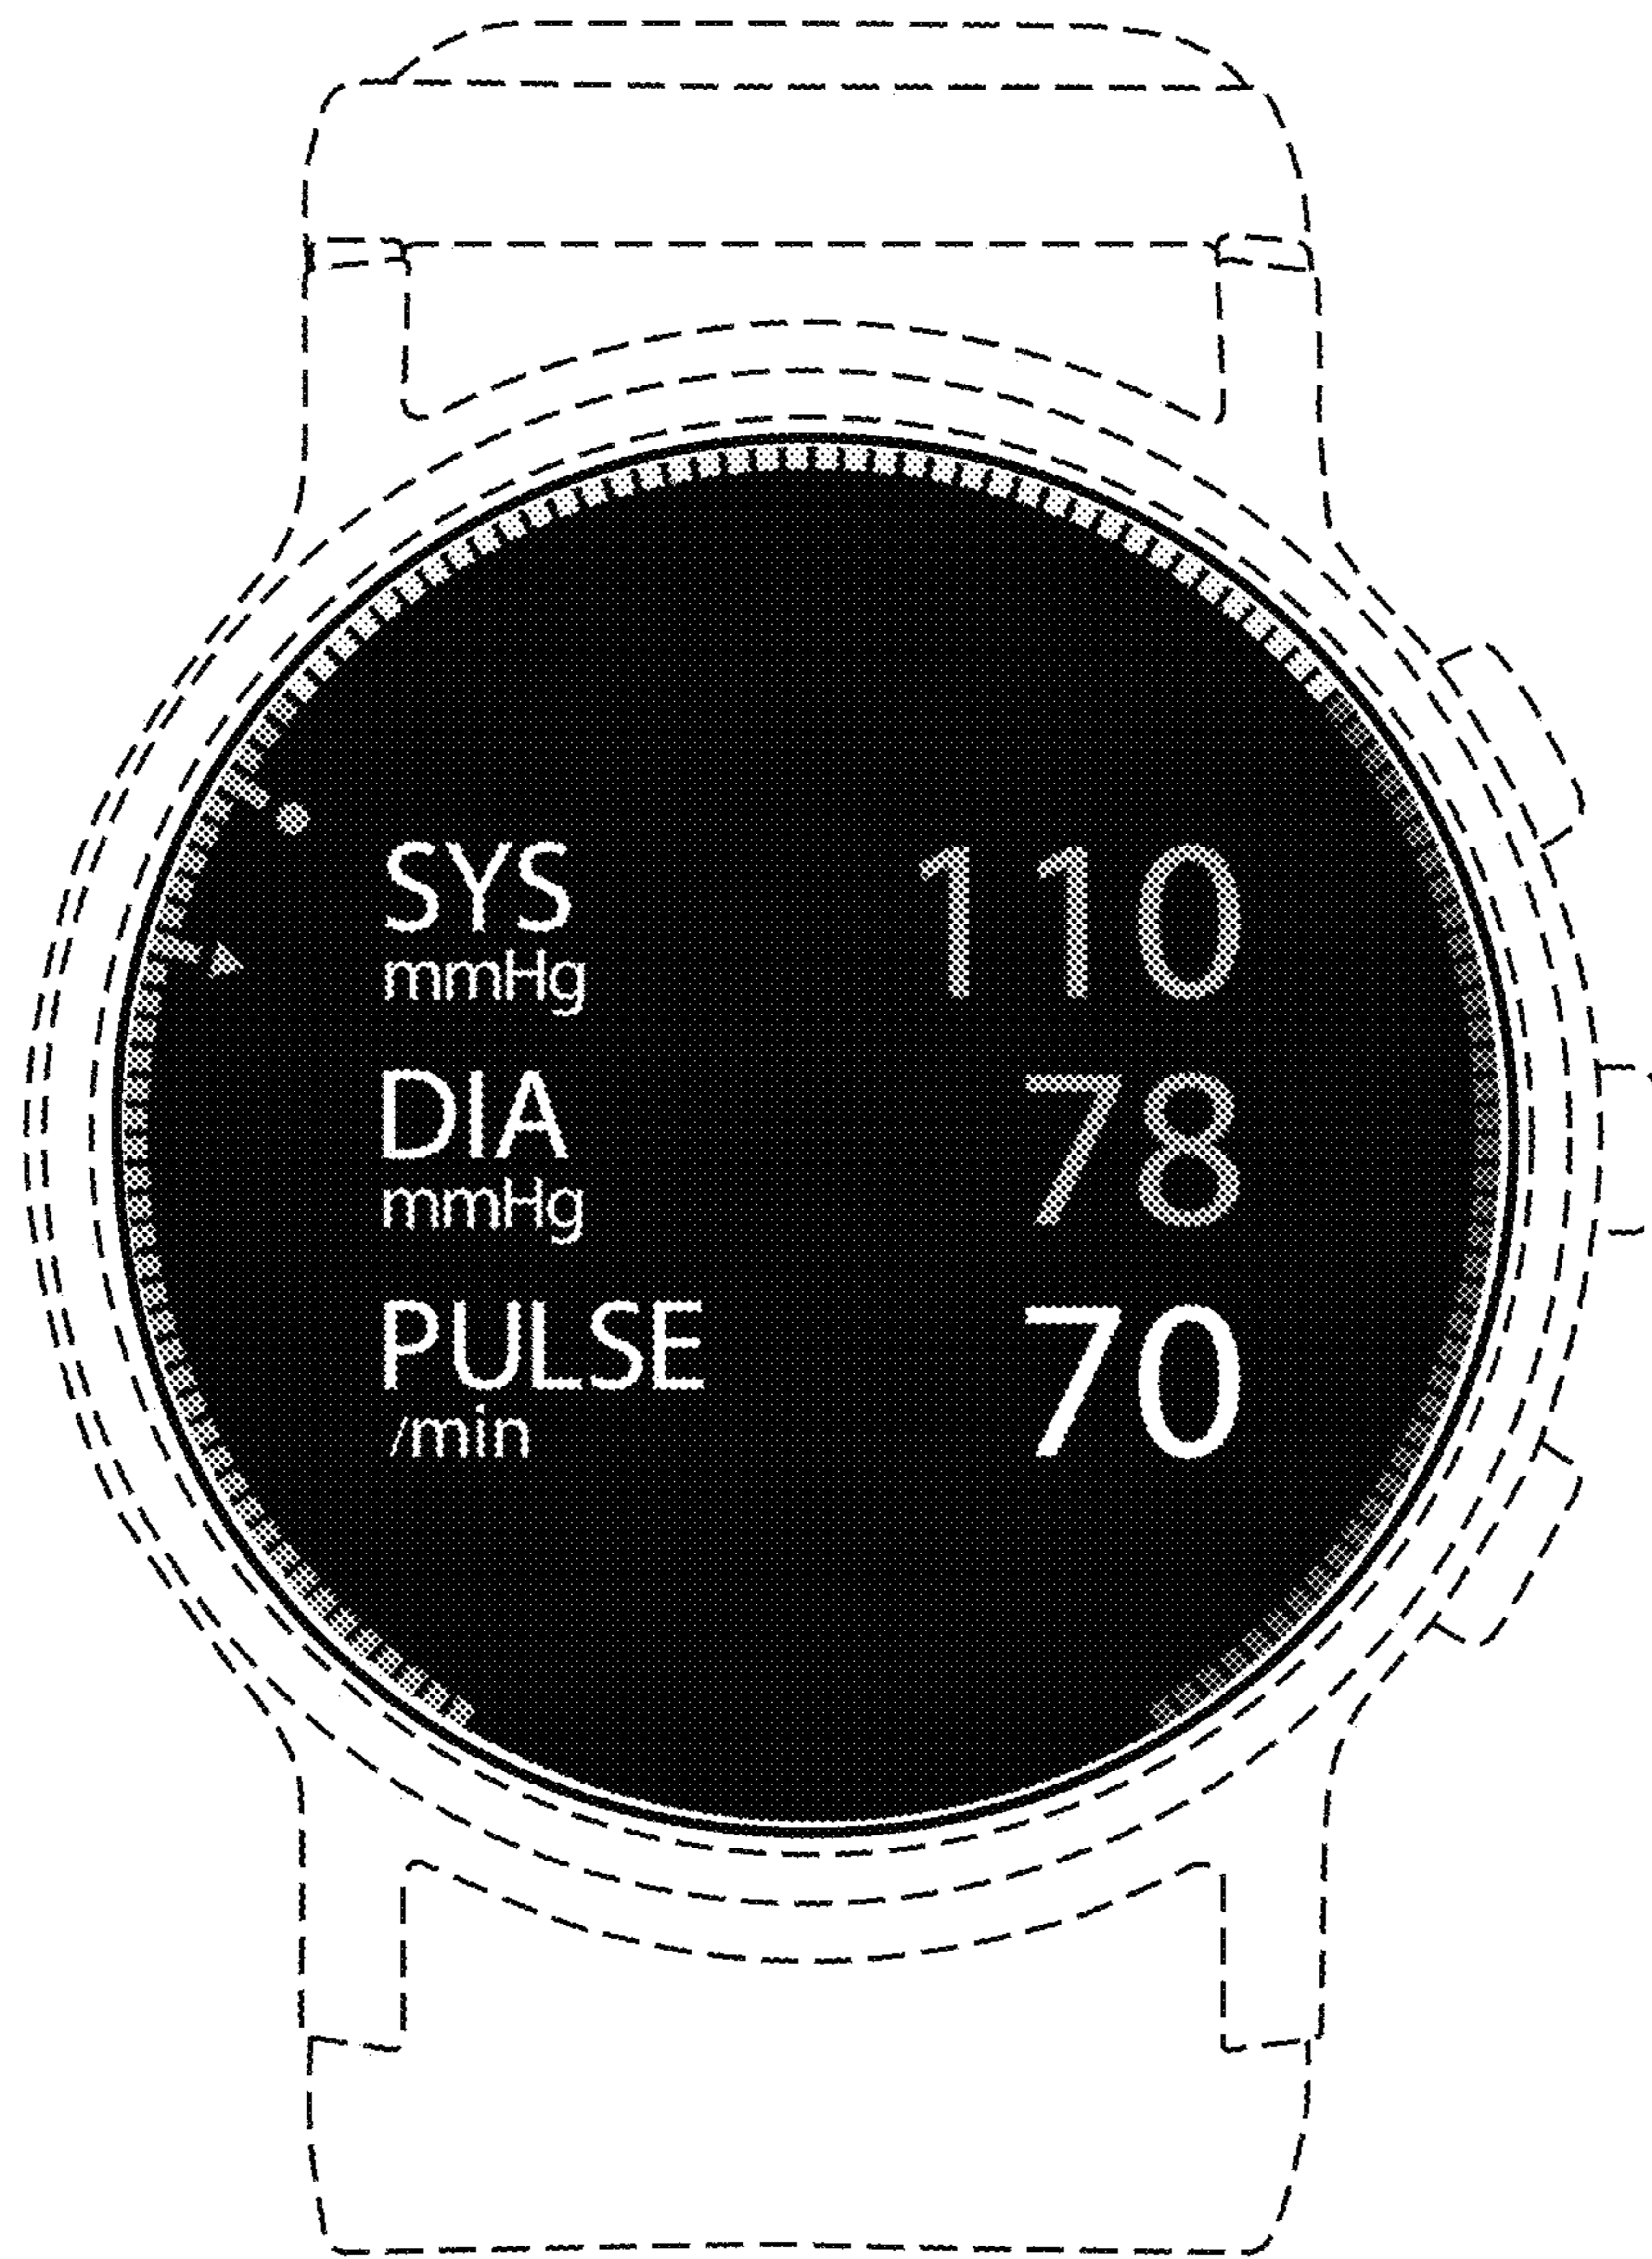


**FIG. 9**

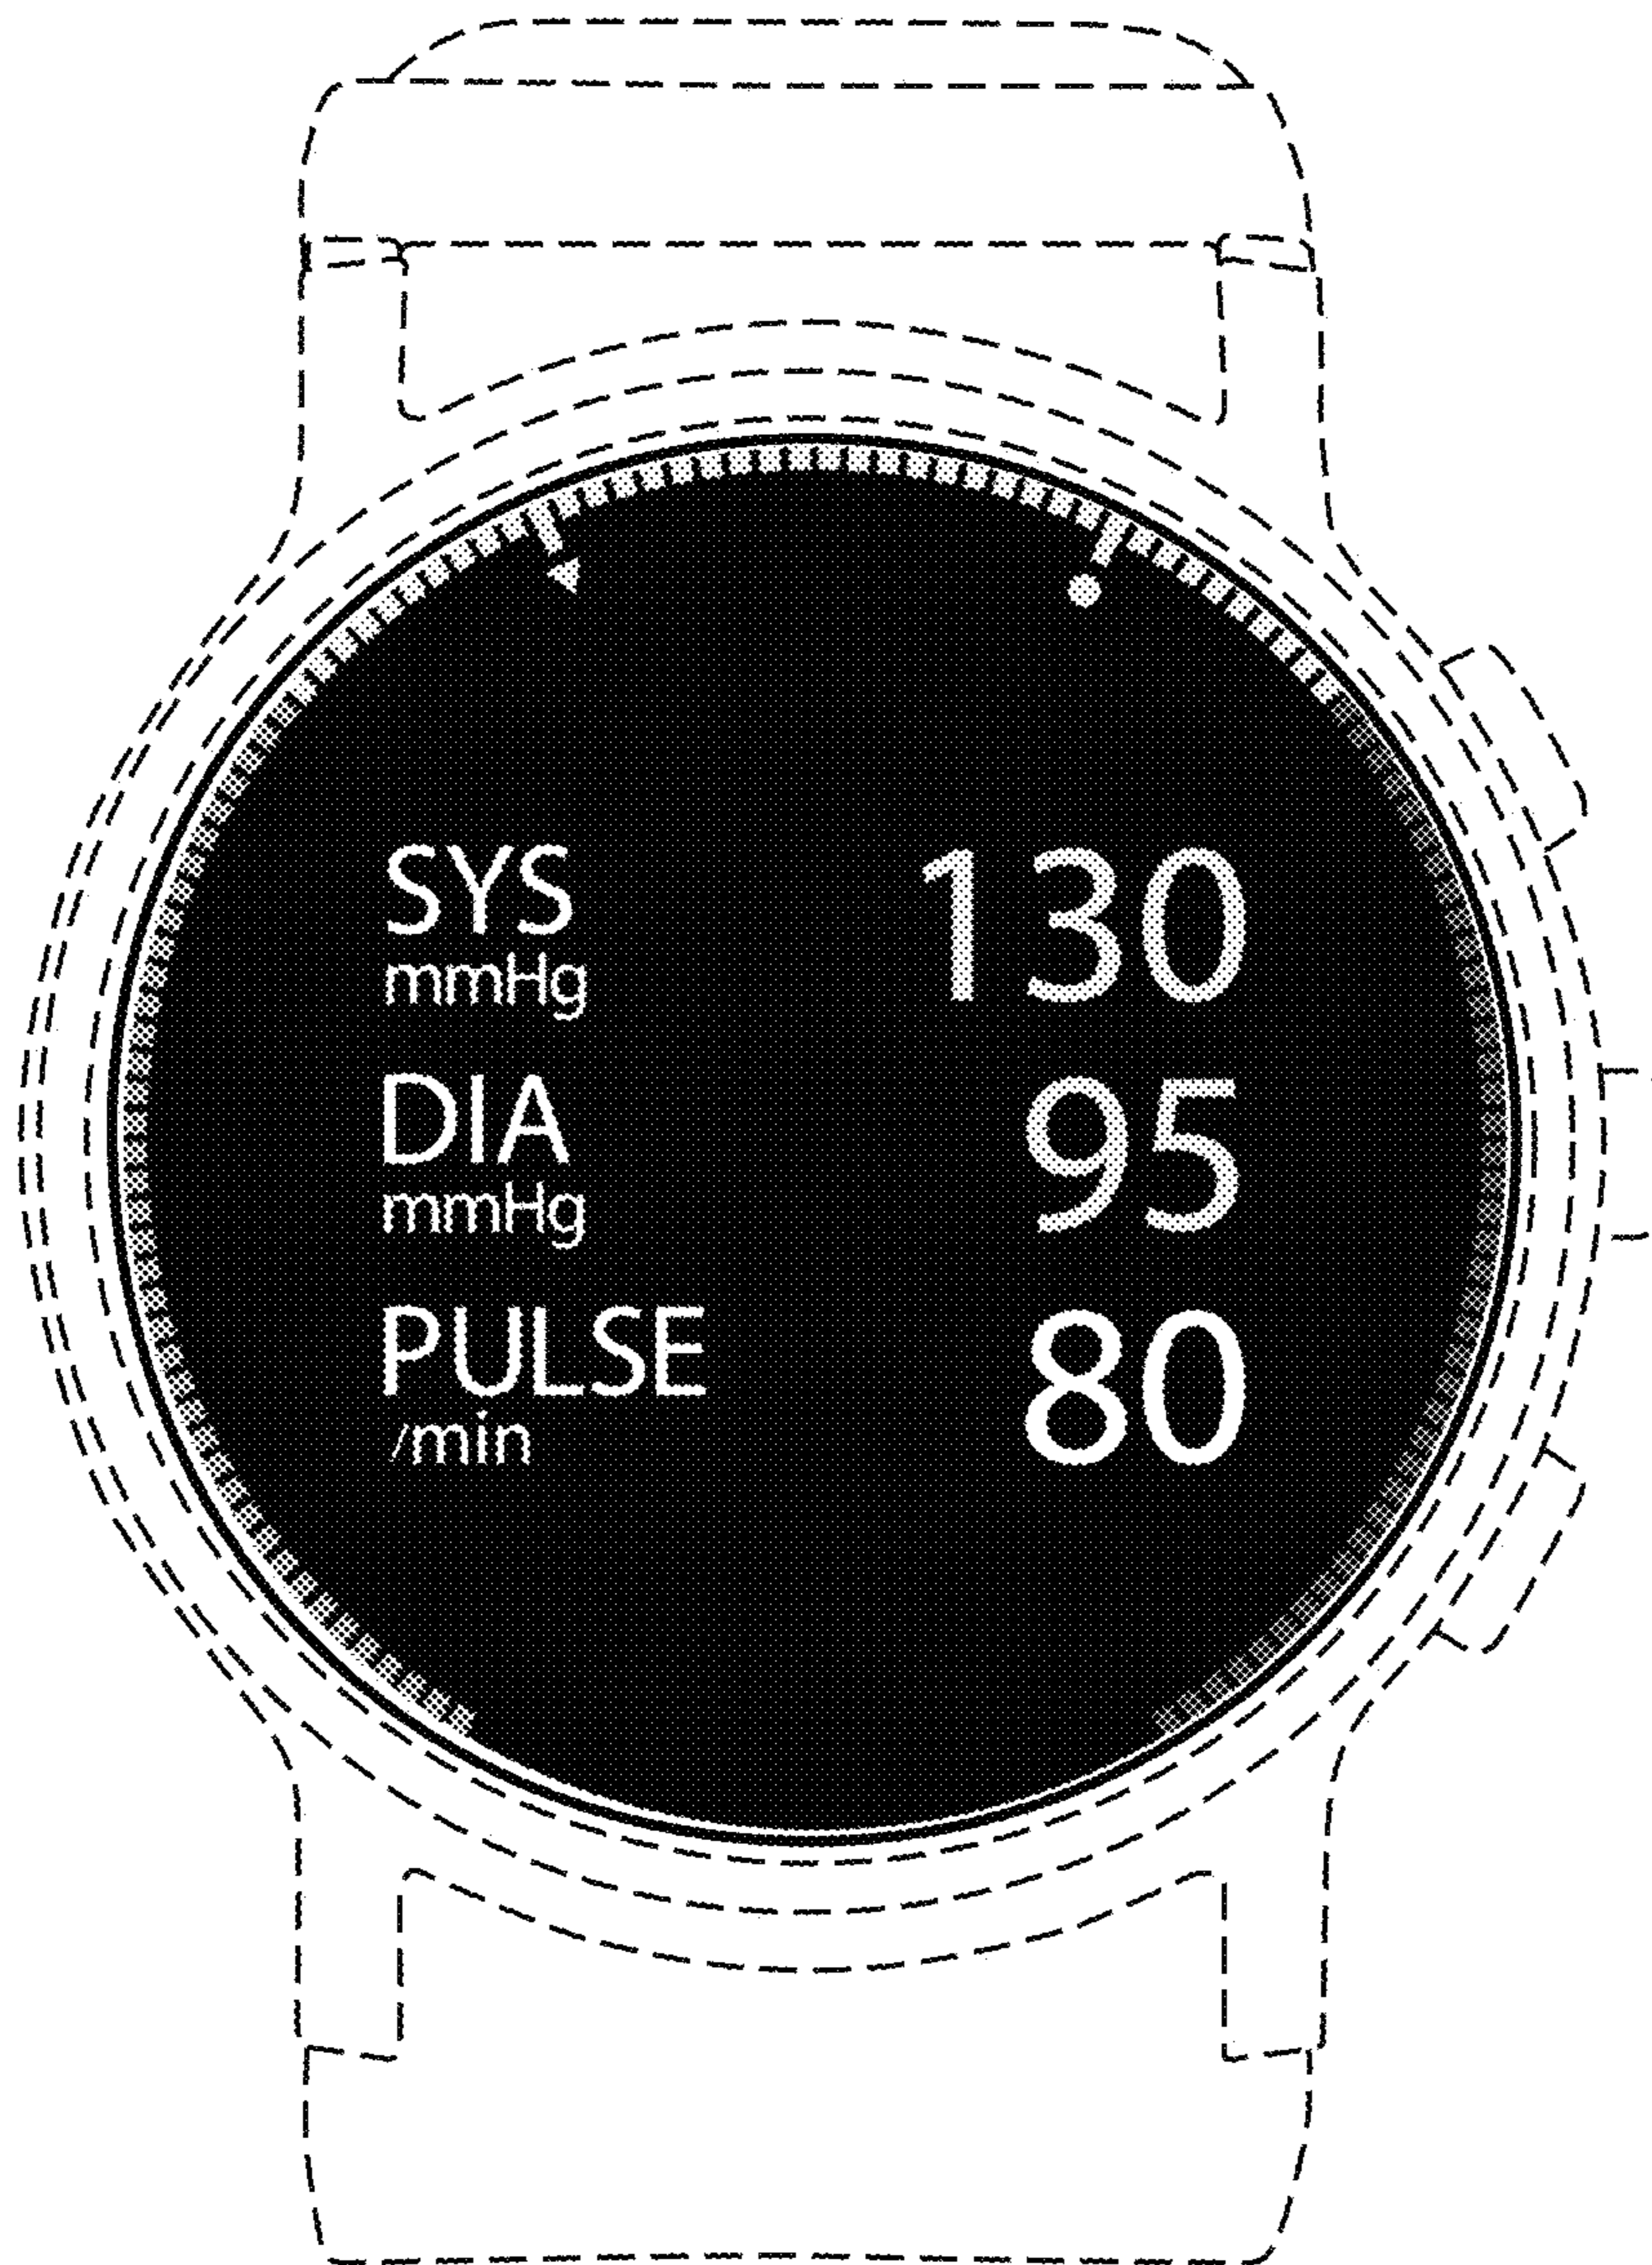

**FIG. 10**

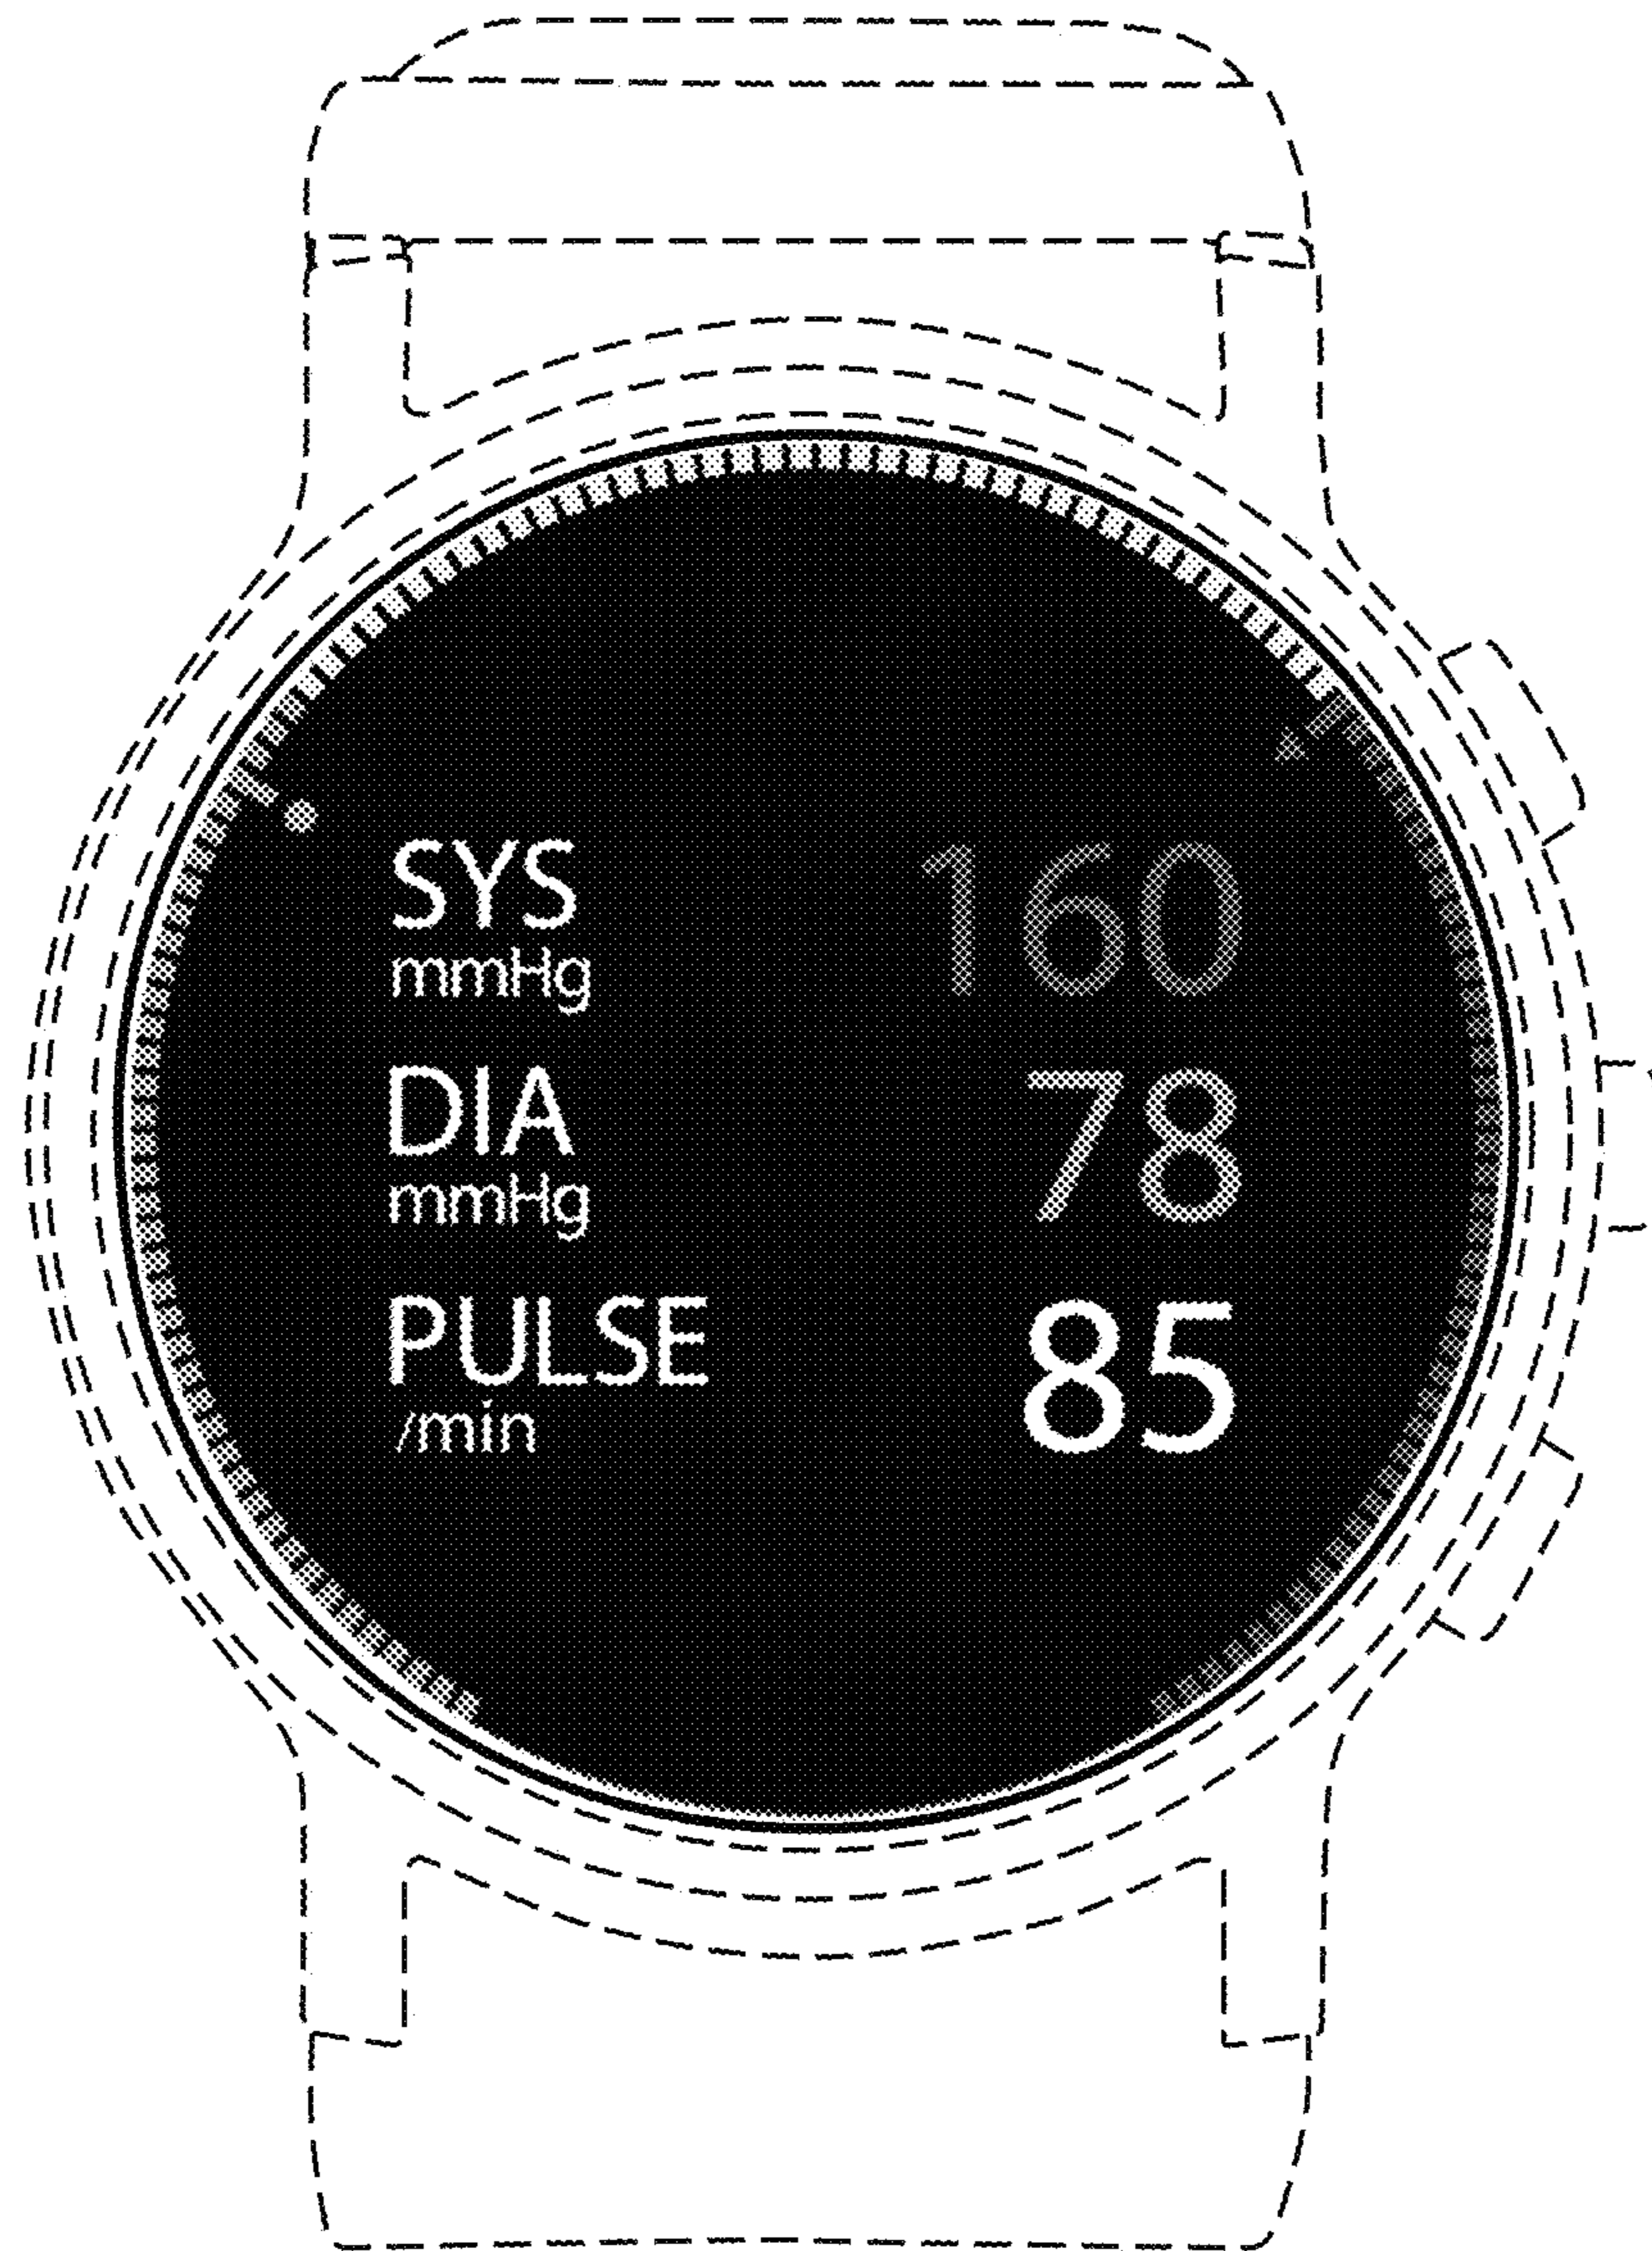

**FIG. 11**

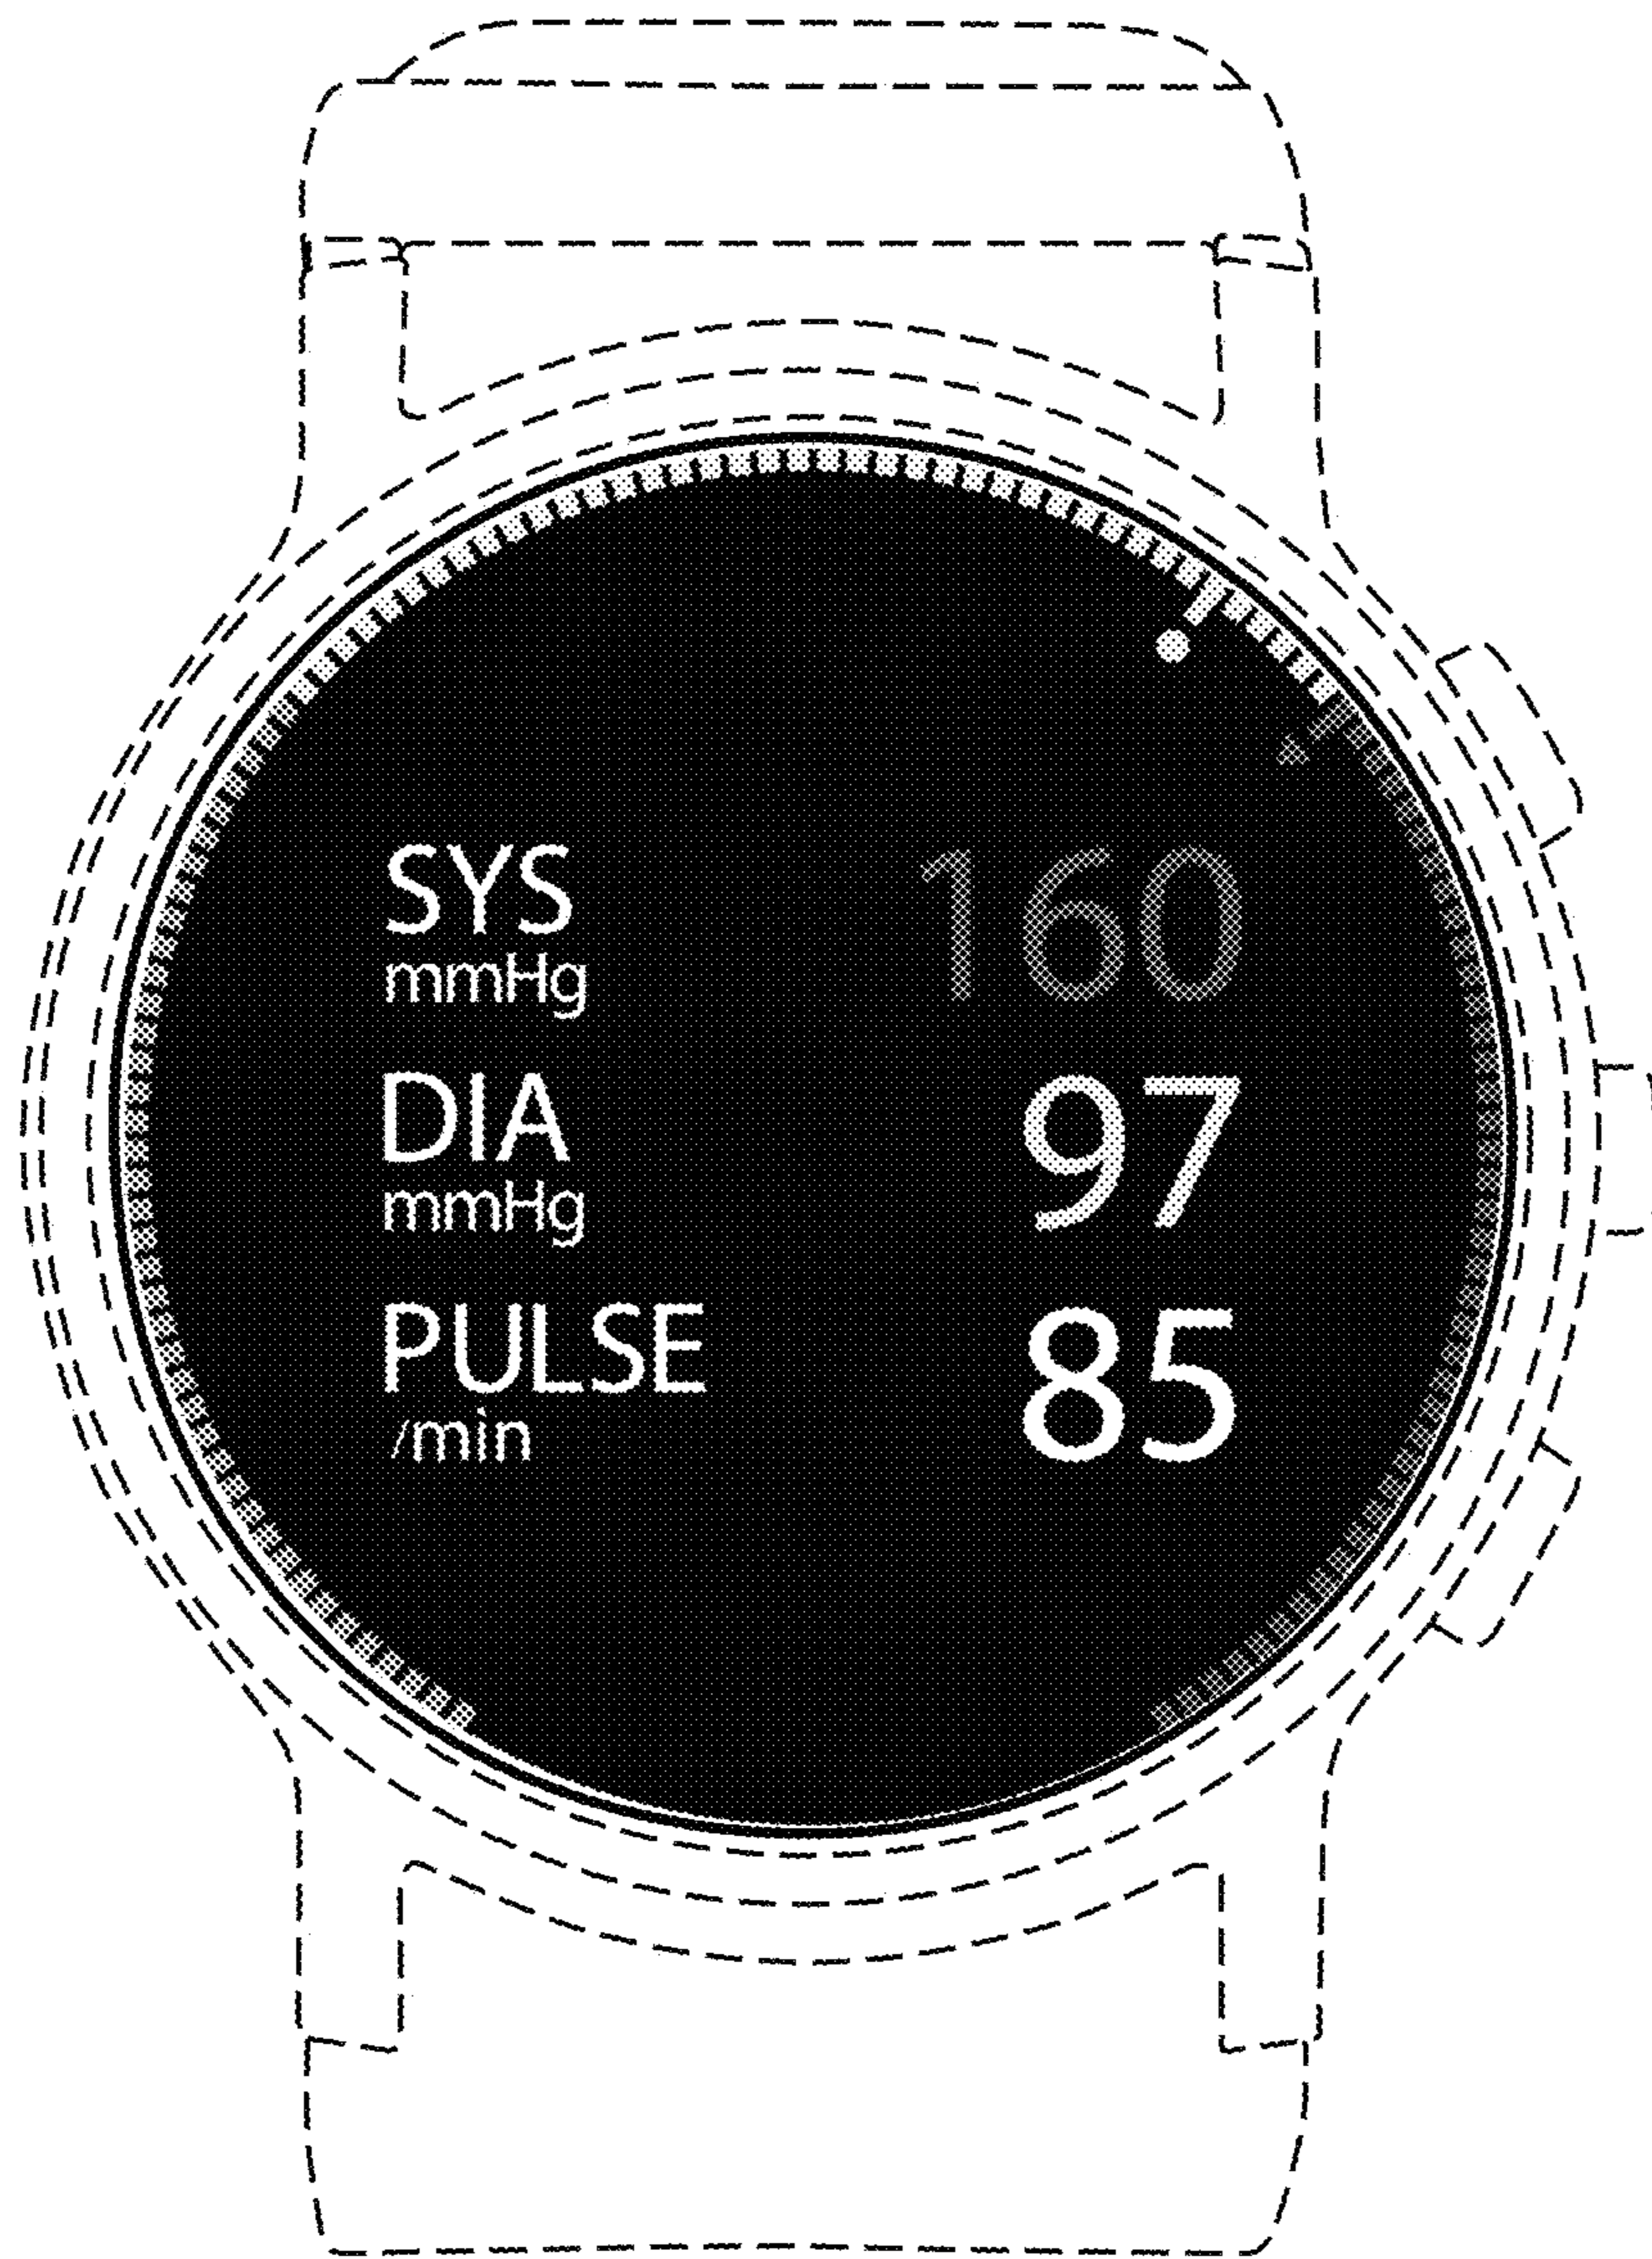

**FIG. 12**

