



US00D824536S

(12) **United States Design Patent** (10) **Patent No.:** **US D824,536 S**
Barton et al. (45) **Date of Patent:** **** Jul. 31, 2018**

(54) **DIAGNOSTIC ANALYZER**

(71) Applicant: **Abbott Laboratories**, Abbott Park, IL (US)
(72) Inventors: **Christina A. Barton**, Irving, TX (US); **Rachel Elizabeth Wallace**, Madison, WI (US); **Ami Marie Verhalen**, Sun Prairie, WI (US); **Daniel Roger Nett**, Sun Prairie, WI (US)
(73) Assignee: **Abbott Laboratories**, Abbott Park, IL (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/531,603**

(22) Filed: **Jun. 26, 2015**

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/232**

(58) **Field of Classification Search**
USPC D24/216–219, 231, 232, 233, 107, 169, D24/186; D10/81
CPC G01N 2035/00306; G01N 2035/00326; G01N 2035/00336; G01N 2030/027; G01N 21/76
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D319,307 S *	8/1991	Sakagami	D10/81
D346,027 S *	4/1994	Kobayashi	D24/232
D351,025 S *	9/1994	Yamashita	D24/216
D354,354 S *	1/1995	Yamashita	D24/232
6,521,183 B1 *	2/2003	Burri	G01N 35/026 422/65
D662,431 S *	6/2012	Kimura	D10/81
D672,471 S *	12/2012	Franco	D24/232
D676,568 S *	2/2013	Liu	D24/216
D715,456 S *	10/2014	Oonuma	D24/216

(Continued)

OTHER PUBLICATIONS

Notification of the Registration of the Community Designs, issued by the Office for Harmonization in The Internal Market, in connection with European Community Design Nos. 002930230-0001 through 002930230-0029, dated Mar. 17, 2016, 6 pages.

(Continued)

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Hanley, Flight & Zimmerman, LLC


(57) **CLAIM**

The ornamental design for a “diagnostic analyzer,” as shown and described.

DESCRIPTION

FIG. 1 is a front left perspective view of a diagnostic analyzer.
FIG. 2 is a front view of the diagnostic analyzer of FIG. 1.
FIG. 3 is a rear view of the diagnostic analyzer of FIGS. 1 or 8.
FIG. 4 is a right side view of the diagnostic analyzer of FIGS. 1 or 8.
FIG. 5 is a left side view of the diagnostic analyzer of FIGS. 1 or 8.
FIG. 6 is a top view of the diagnostic analyzer of FIG. 1.
FIG. 7 is a bottom view of the diagnostic analyzer of FIGS. 1 or 8.
FIG. 8 is a front left perspective view of a diagnostic analyzer.
FIG. 9 is a front view of the diagnostic analyzer of FIG. 8; and,
FIG. 10 is a top view of the diagnostic analyzer of FIG. 8.
The features shown in broken lines form no part of the claimed design.

1 Claim, 10 Drawing Sheets

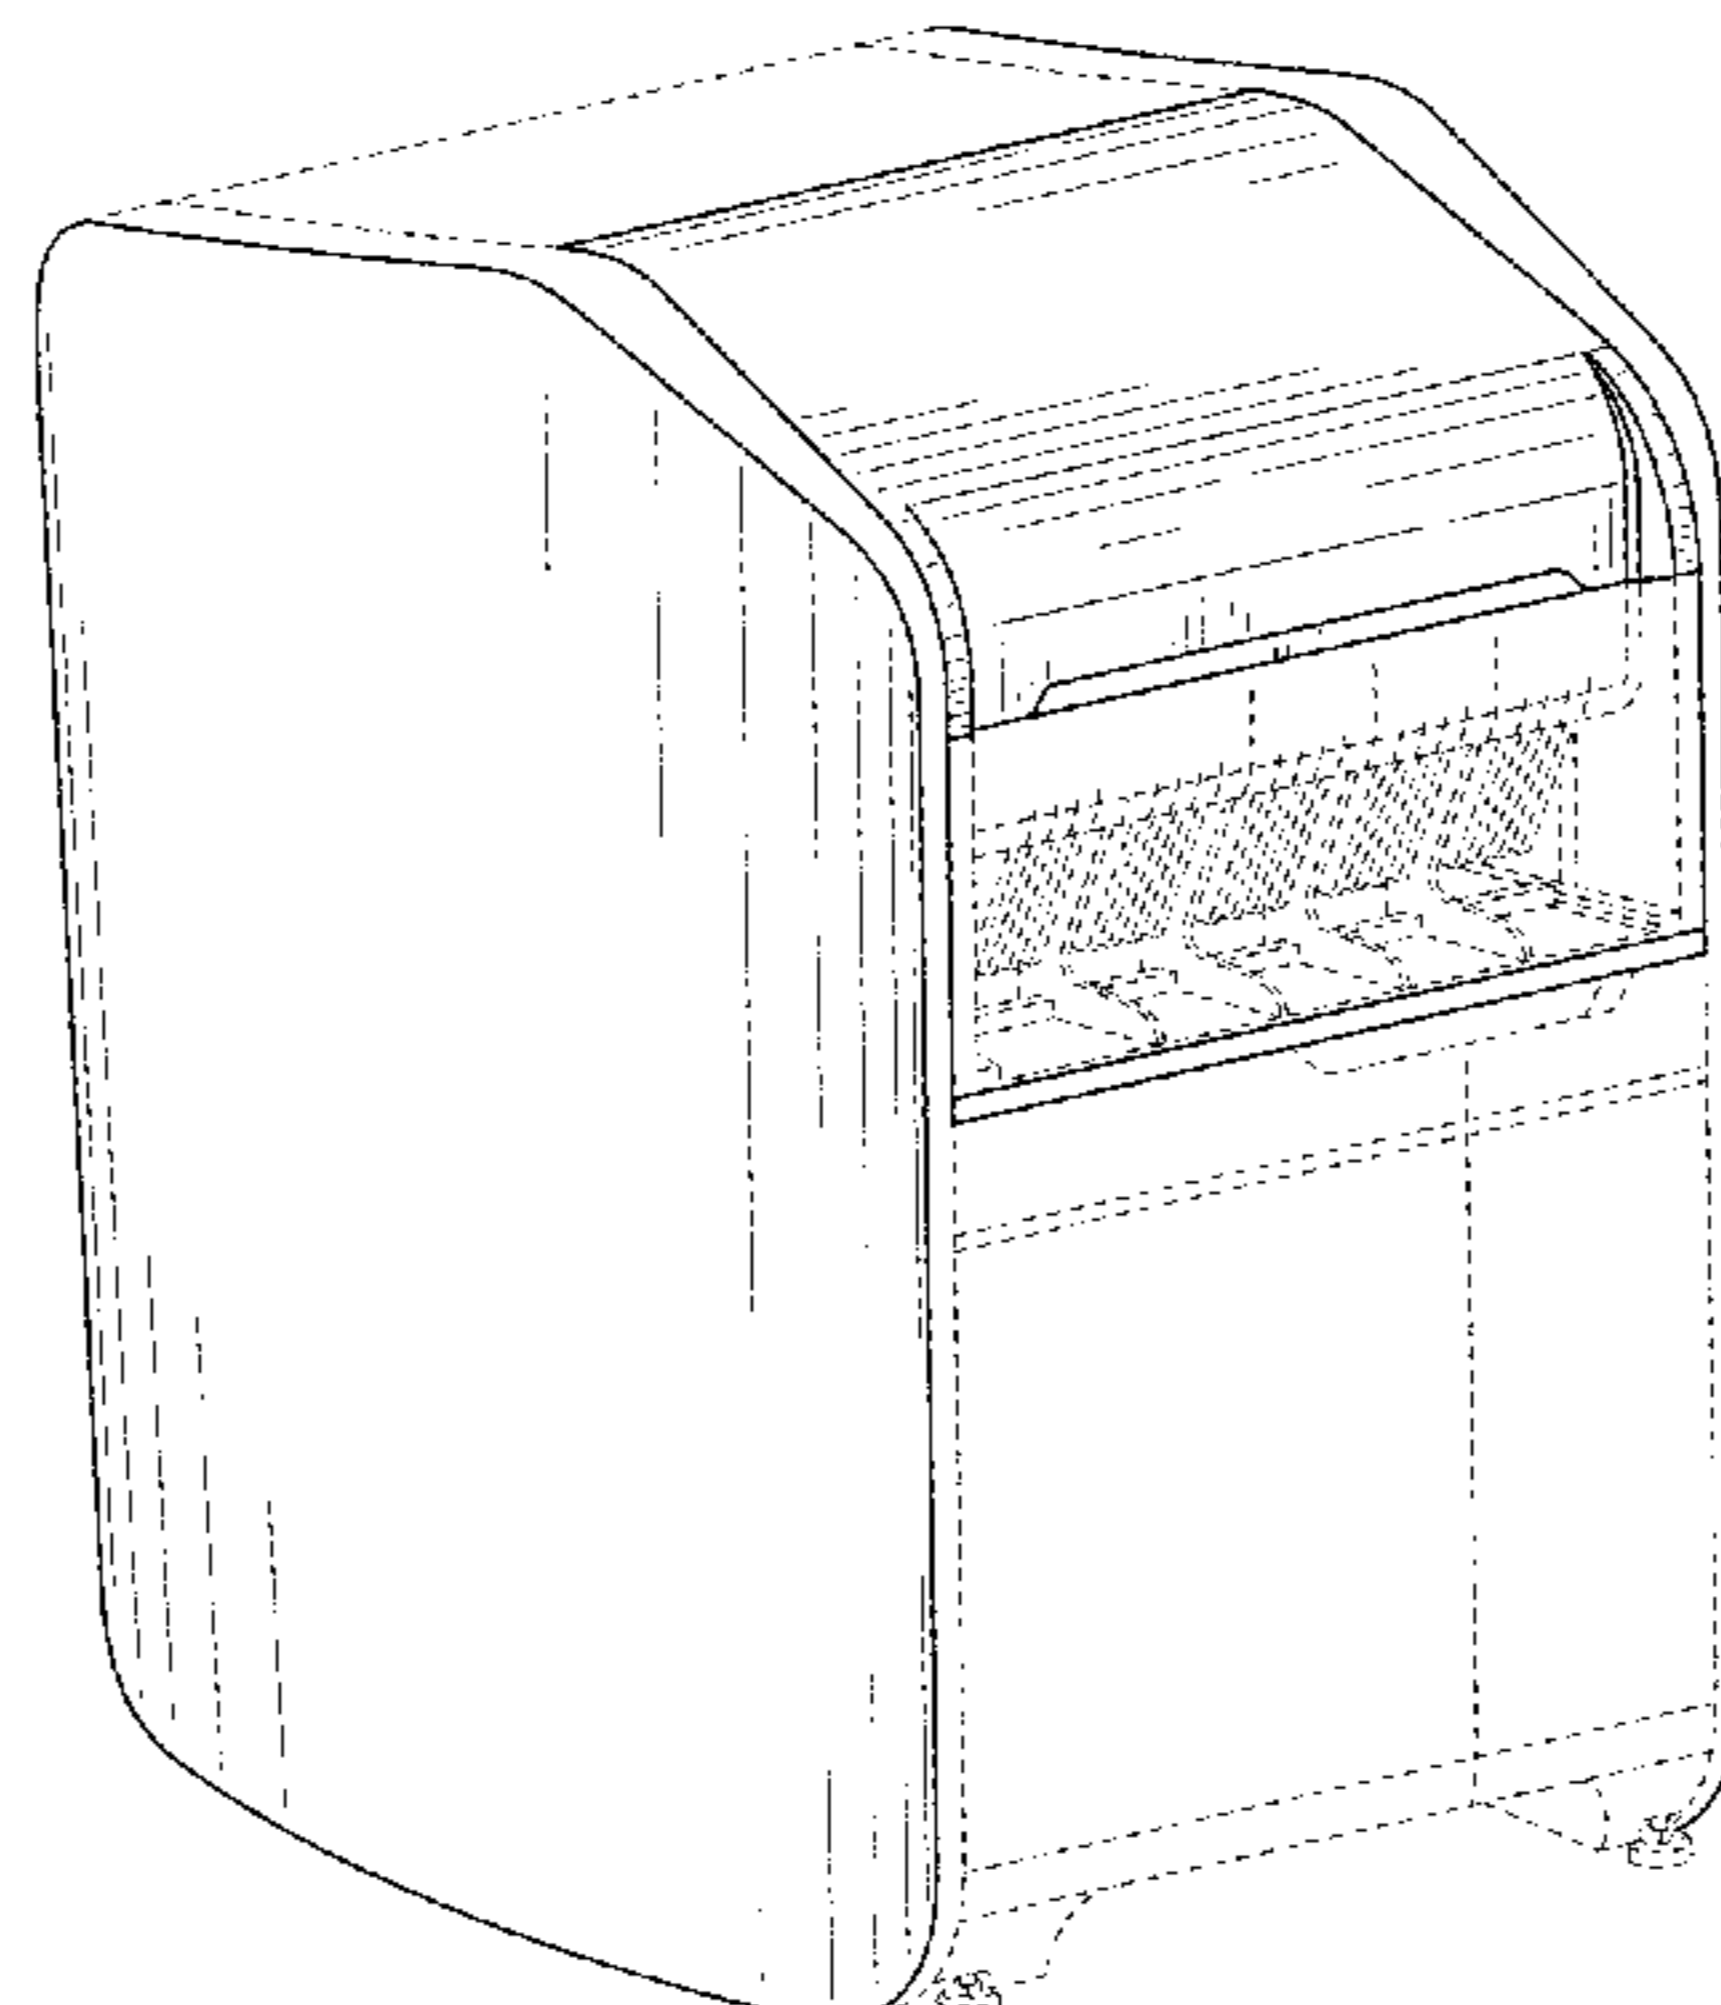

(56)

References Cited

U.S. PATENT DOCUMENTS

D716,966	S	*	11/2014	Lizari Illarramendi	D24/232
D721,820	S		1/2015	Oonuma et al.		
D724,753	S	*	3/2015	Gutmann	D24/216
D728,124	S	*	4/2015	Oonuma	D24/216
D729,399	S		5/2015	Oonuma et al.		
D736,402	S	*	8/2015	Gutmann	D24/216
D777,049	S		1/2017	Barton et al.		
D800,000	S		10/2017	Barton et al.		
D802,785	S		11/2017	Barton et al.		
2002/0169518	A1	*	11/2002	Luoma, II	B01L 9/00 700/218
2013/0034466	A1	*	2/2013	Wakamiya	G01N 35/00584 422/64
2013/0288355	A1	*	10/2013	DeWitte	G01N 30/06 435/288.6
2015/0140577	A1	*	5/2015	Li	G01N 33/56972 435/7.24
2015/0276566	A1	*	10/2015	Berntsen	G01N 1/312 435/309.1

OTHER PUBLICATIONS

Notification of the Registration of the Community Designs, issued by the European Union Intellectual Property Office, in connection

with European Community Design Nos. 003003631-0001 through 003003631-0014, dated Apr. 28, 2016, 5 pages.

Notice for Reasons for Rejection, English Language, issued by the Intellectual Property Office of Japan, in connection with Japanese application No. 2015-28871, dated Jun. 14, 2016, 5 pages.

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2016-1034, dated Sep. 6, 2016, 5 pages.

State Intellectual Property Office of China, "First Office Action," issued in connection with Chinese Application No. 201530555269.1, dated Oct. 9, 2016, 3 pages.

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2016-22301, dated Nov. 8, 2016, 4 pages.

United States Patent and Trademark Office, "Restriction and/or Election Requirement," issued in connection with U.S. Appl. No. 29/505,590, dated Oct. 13, 2016, 27 pages.

United States Patent and Trademark Office, "Restriction Requirement," issued in connection with U.S. Appl. No. 29/505,590, dated Oct. 13, 2016, 27 pages.

Notification of First Corrections, issued by the State Intellectual Property Office of the P.R. China, in connection with Chinese Patent Application No. 201530555269.1, dated Apr. 25, 2016, 4 pages.

United States Patent and Trademark Office, "Non-Final Office Action," issued in connection with U.S. Appl. No. 29/602,019, dated Jan. 17, 2018, 15 pages.

* cited by examiner

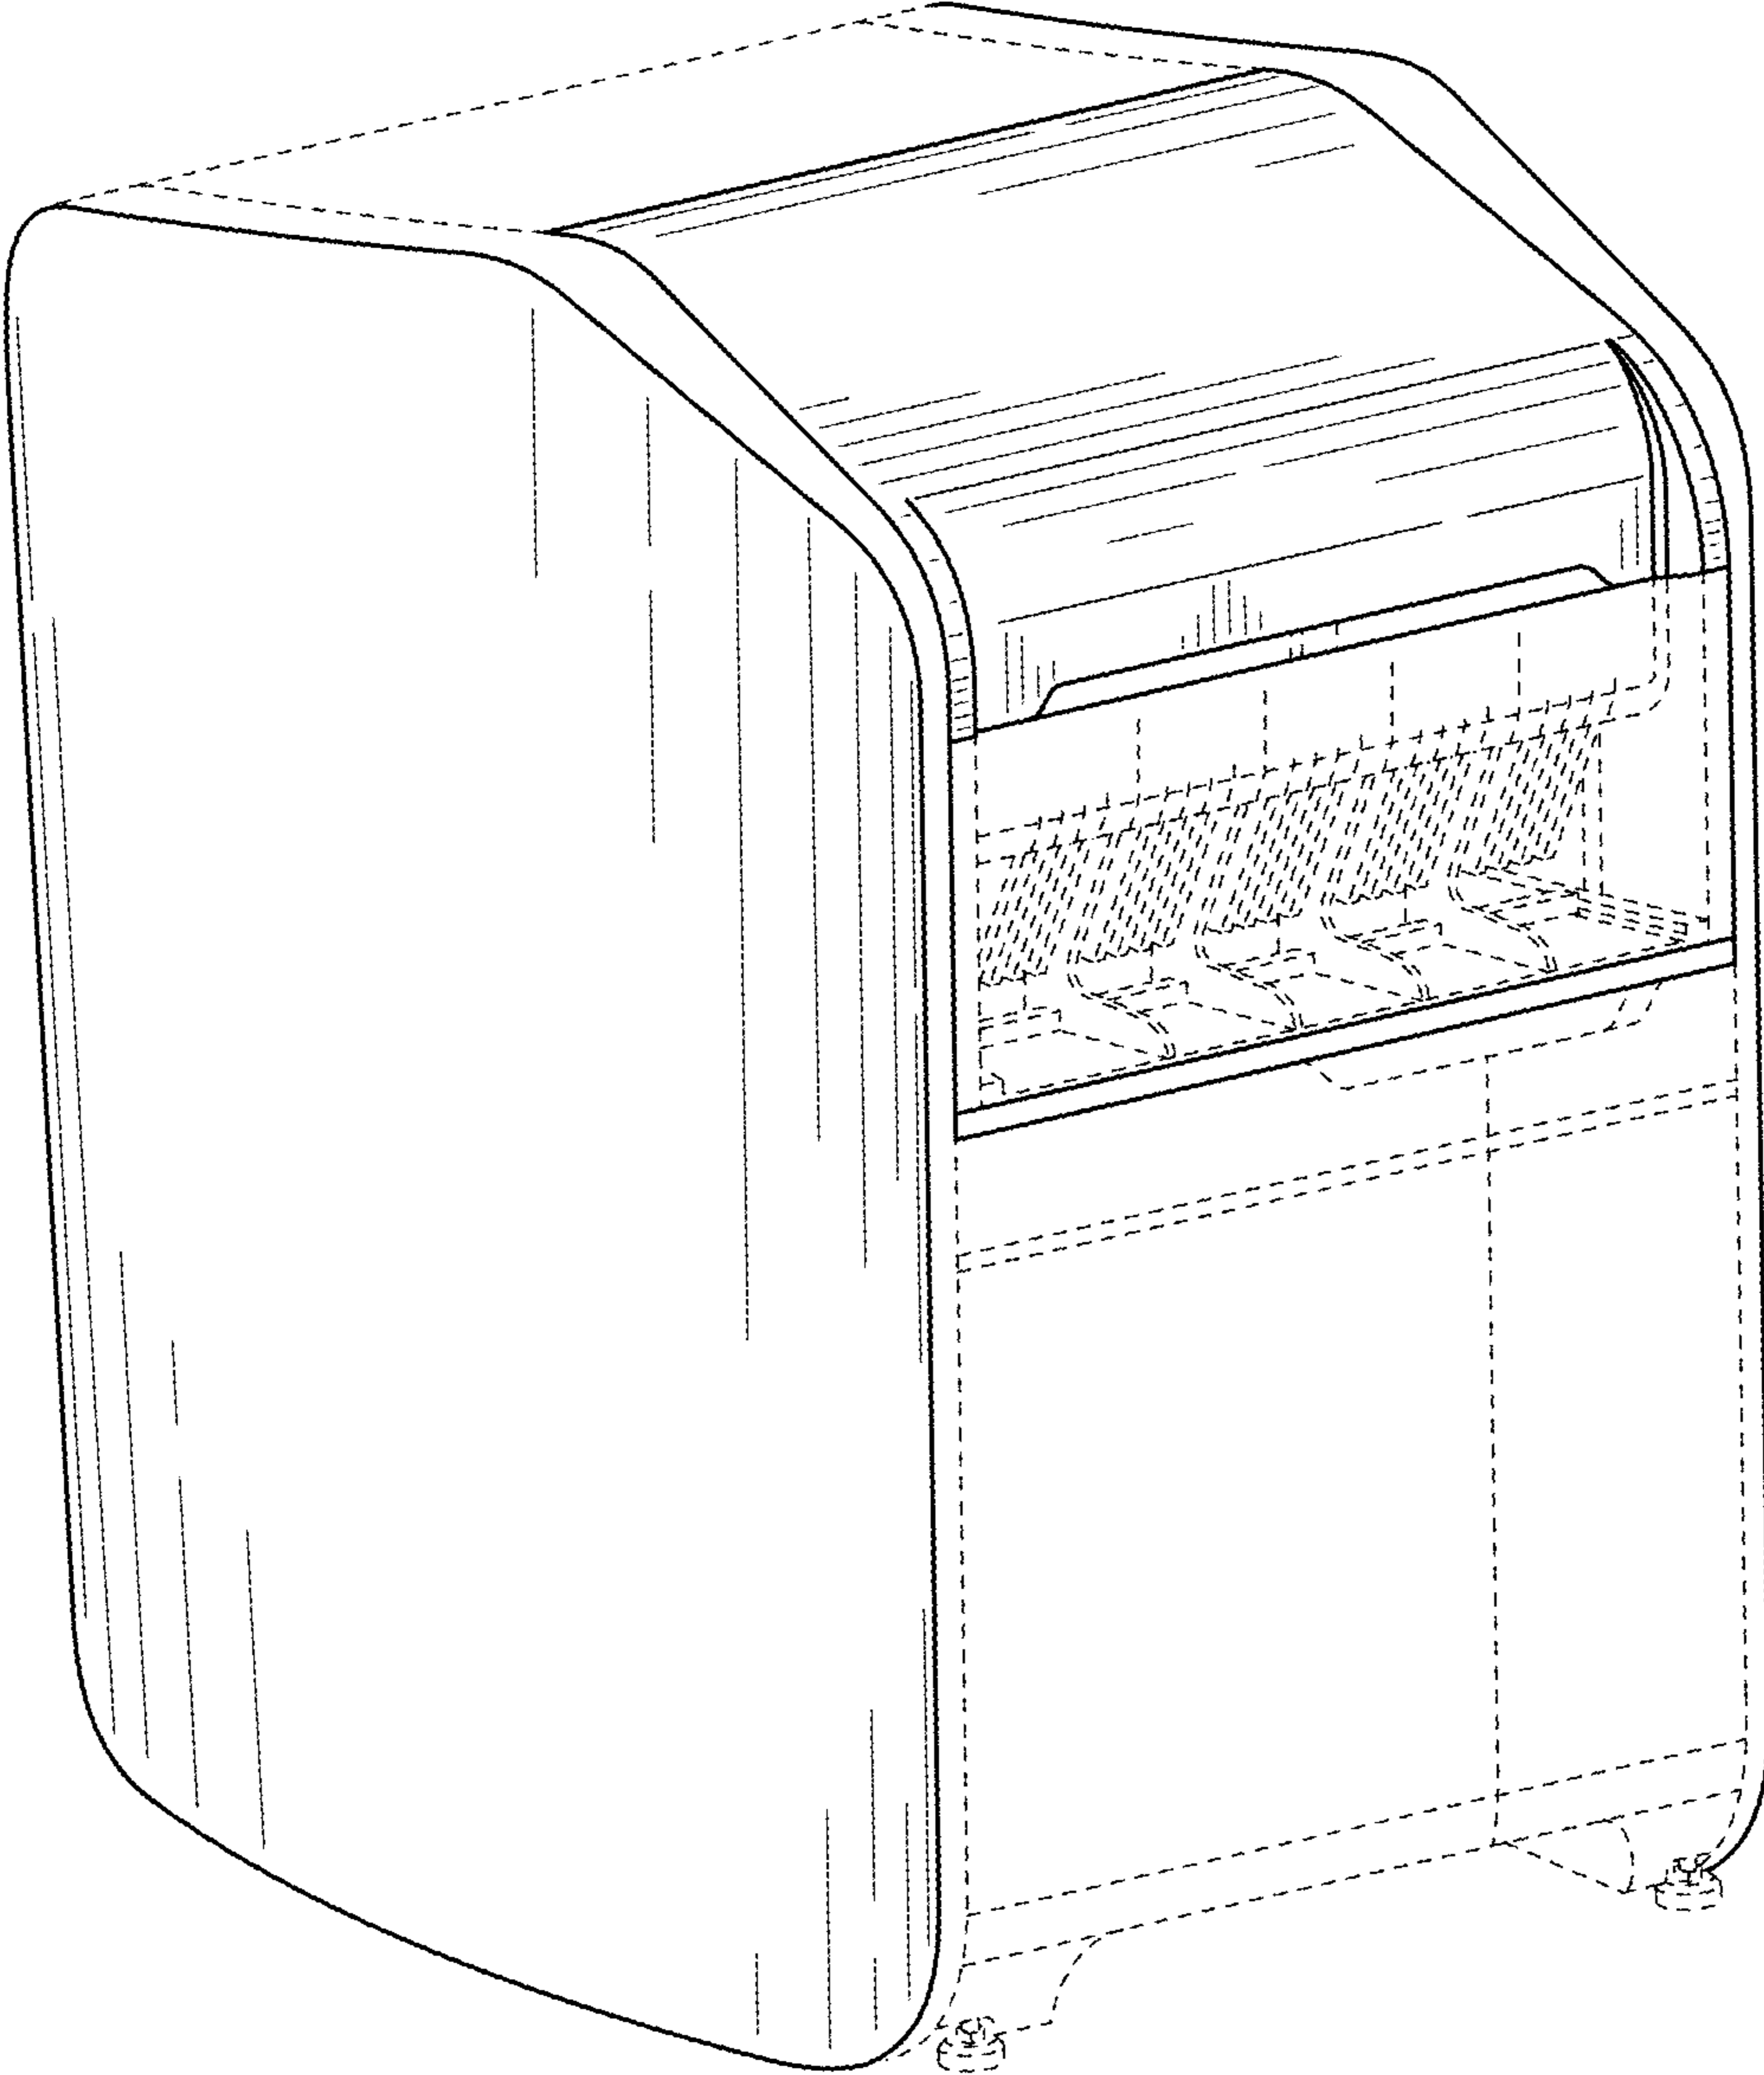


FIG. 1

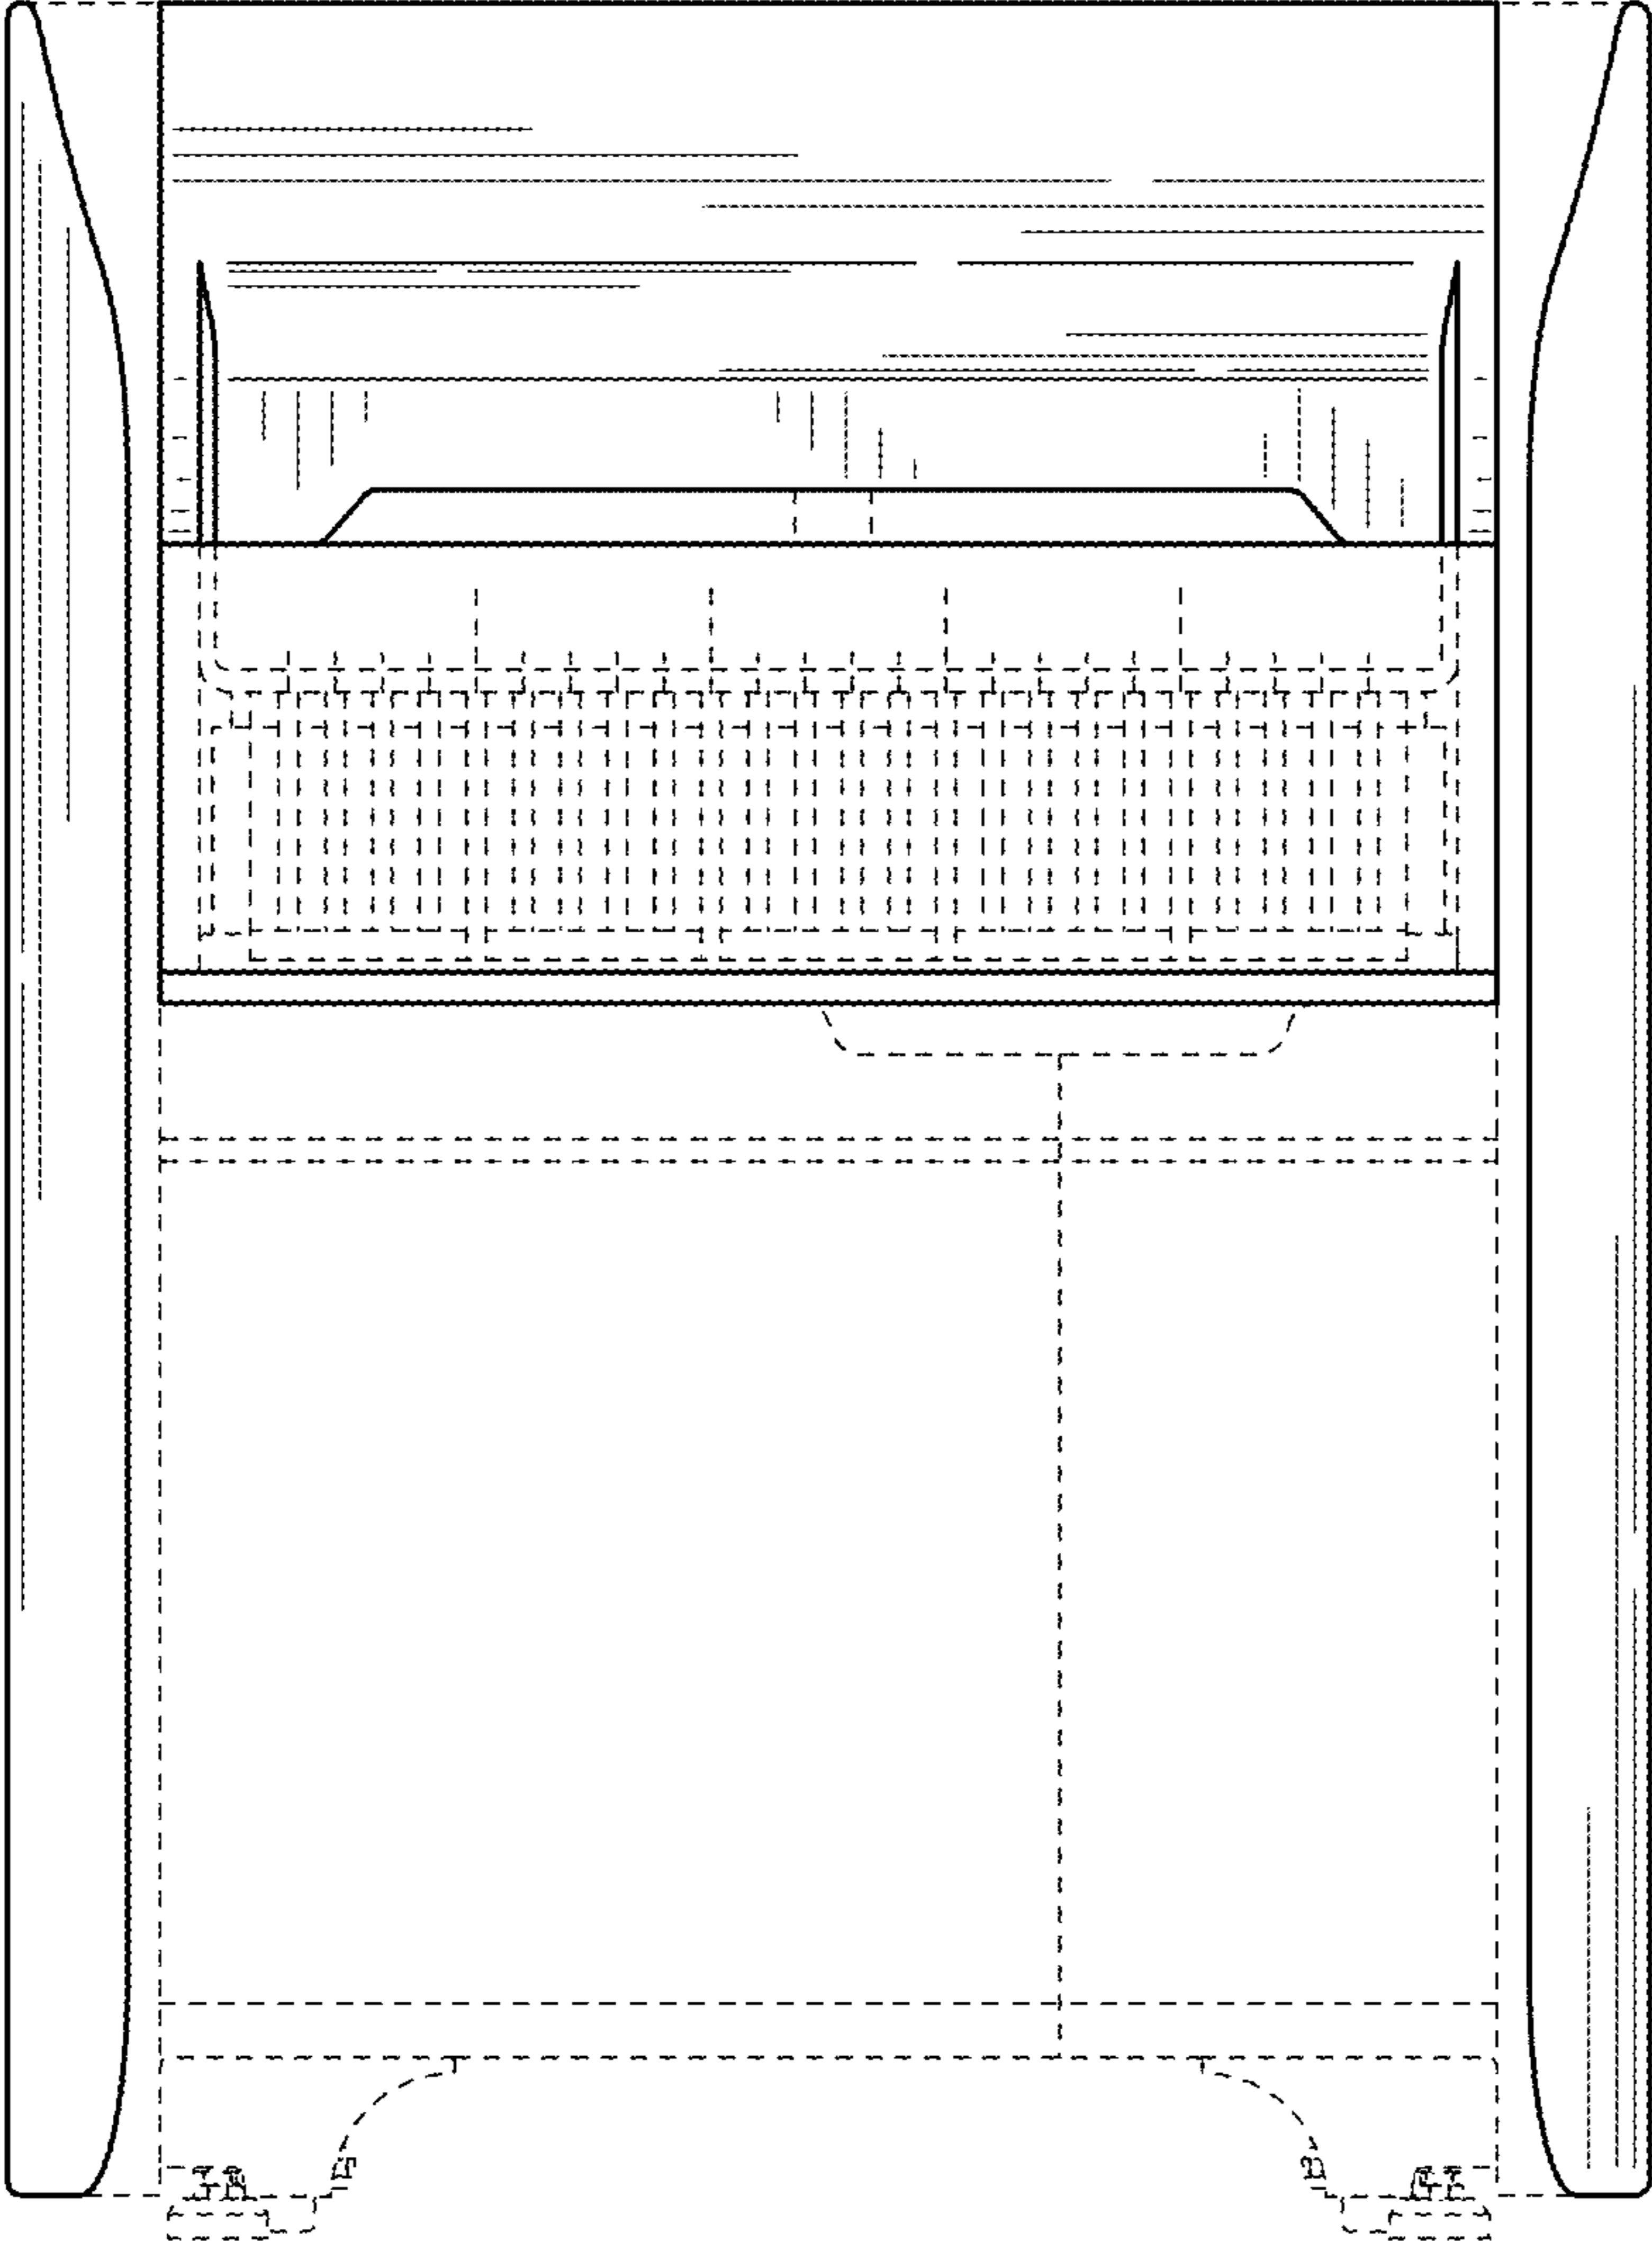


FIG. 2

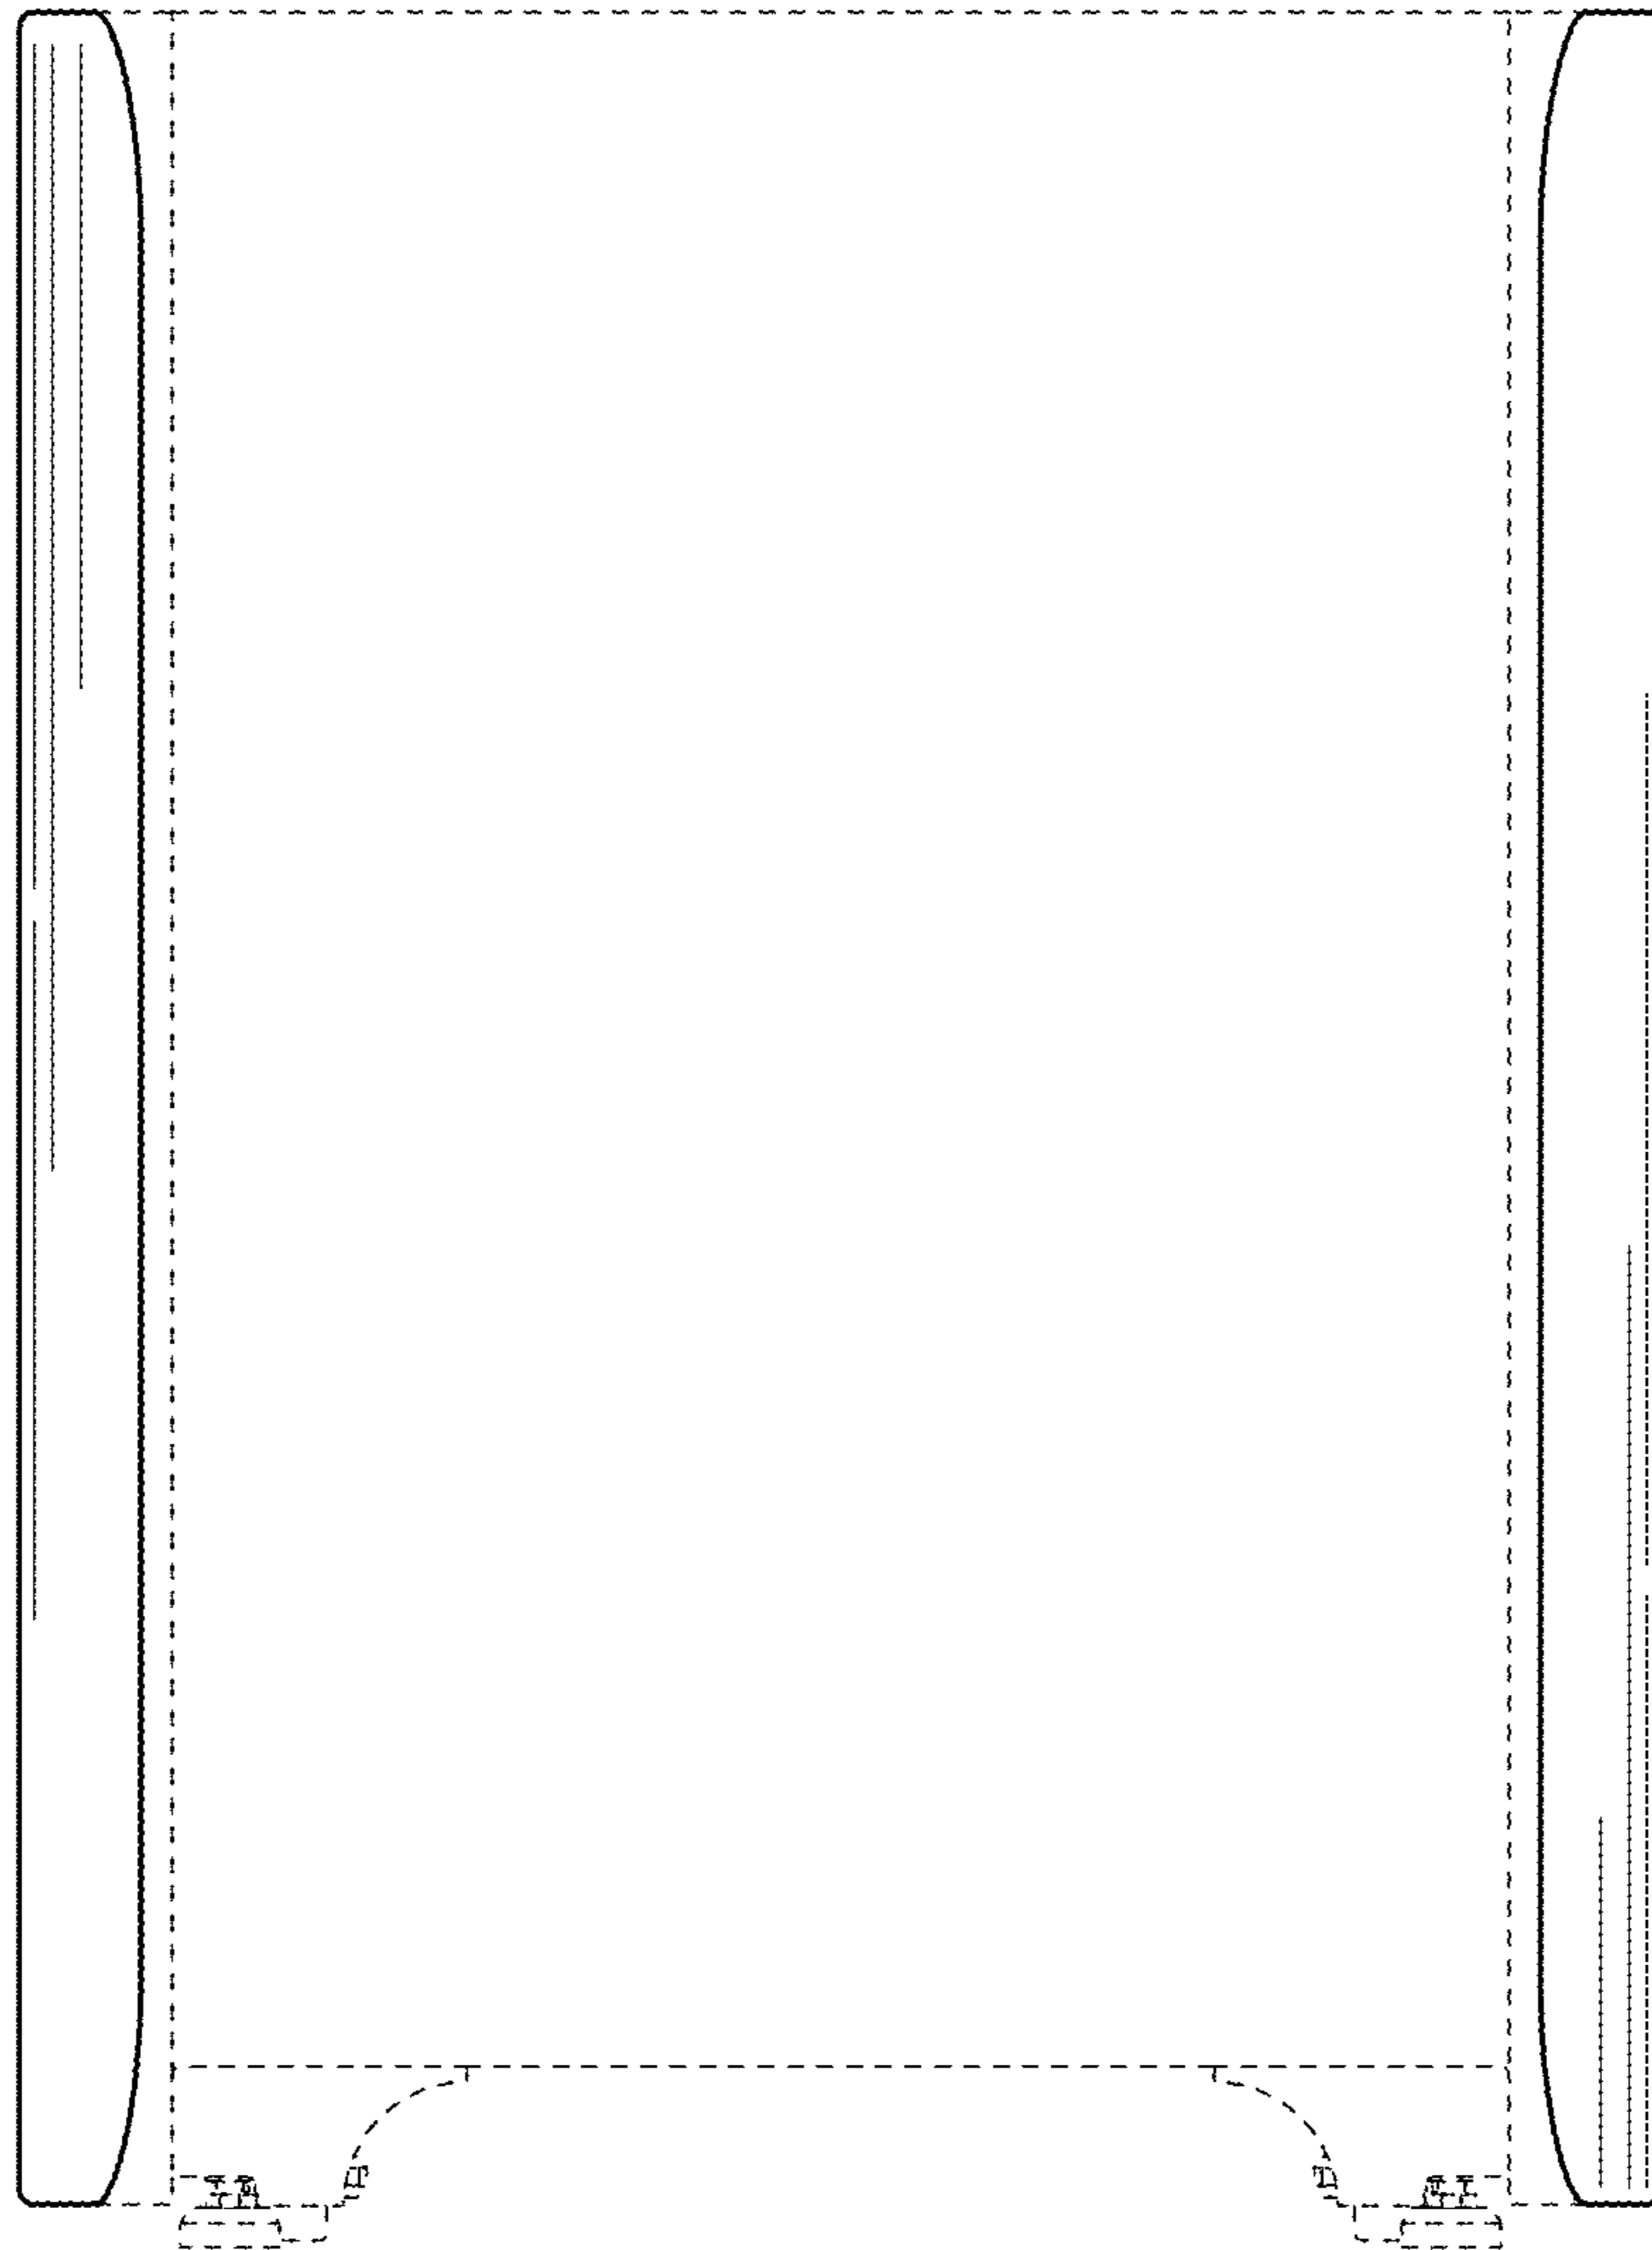


FIG. 3

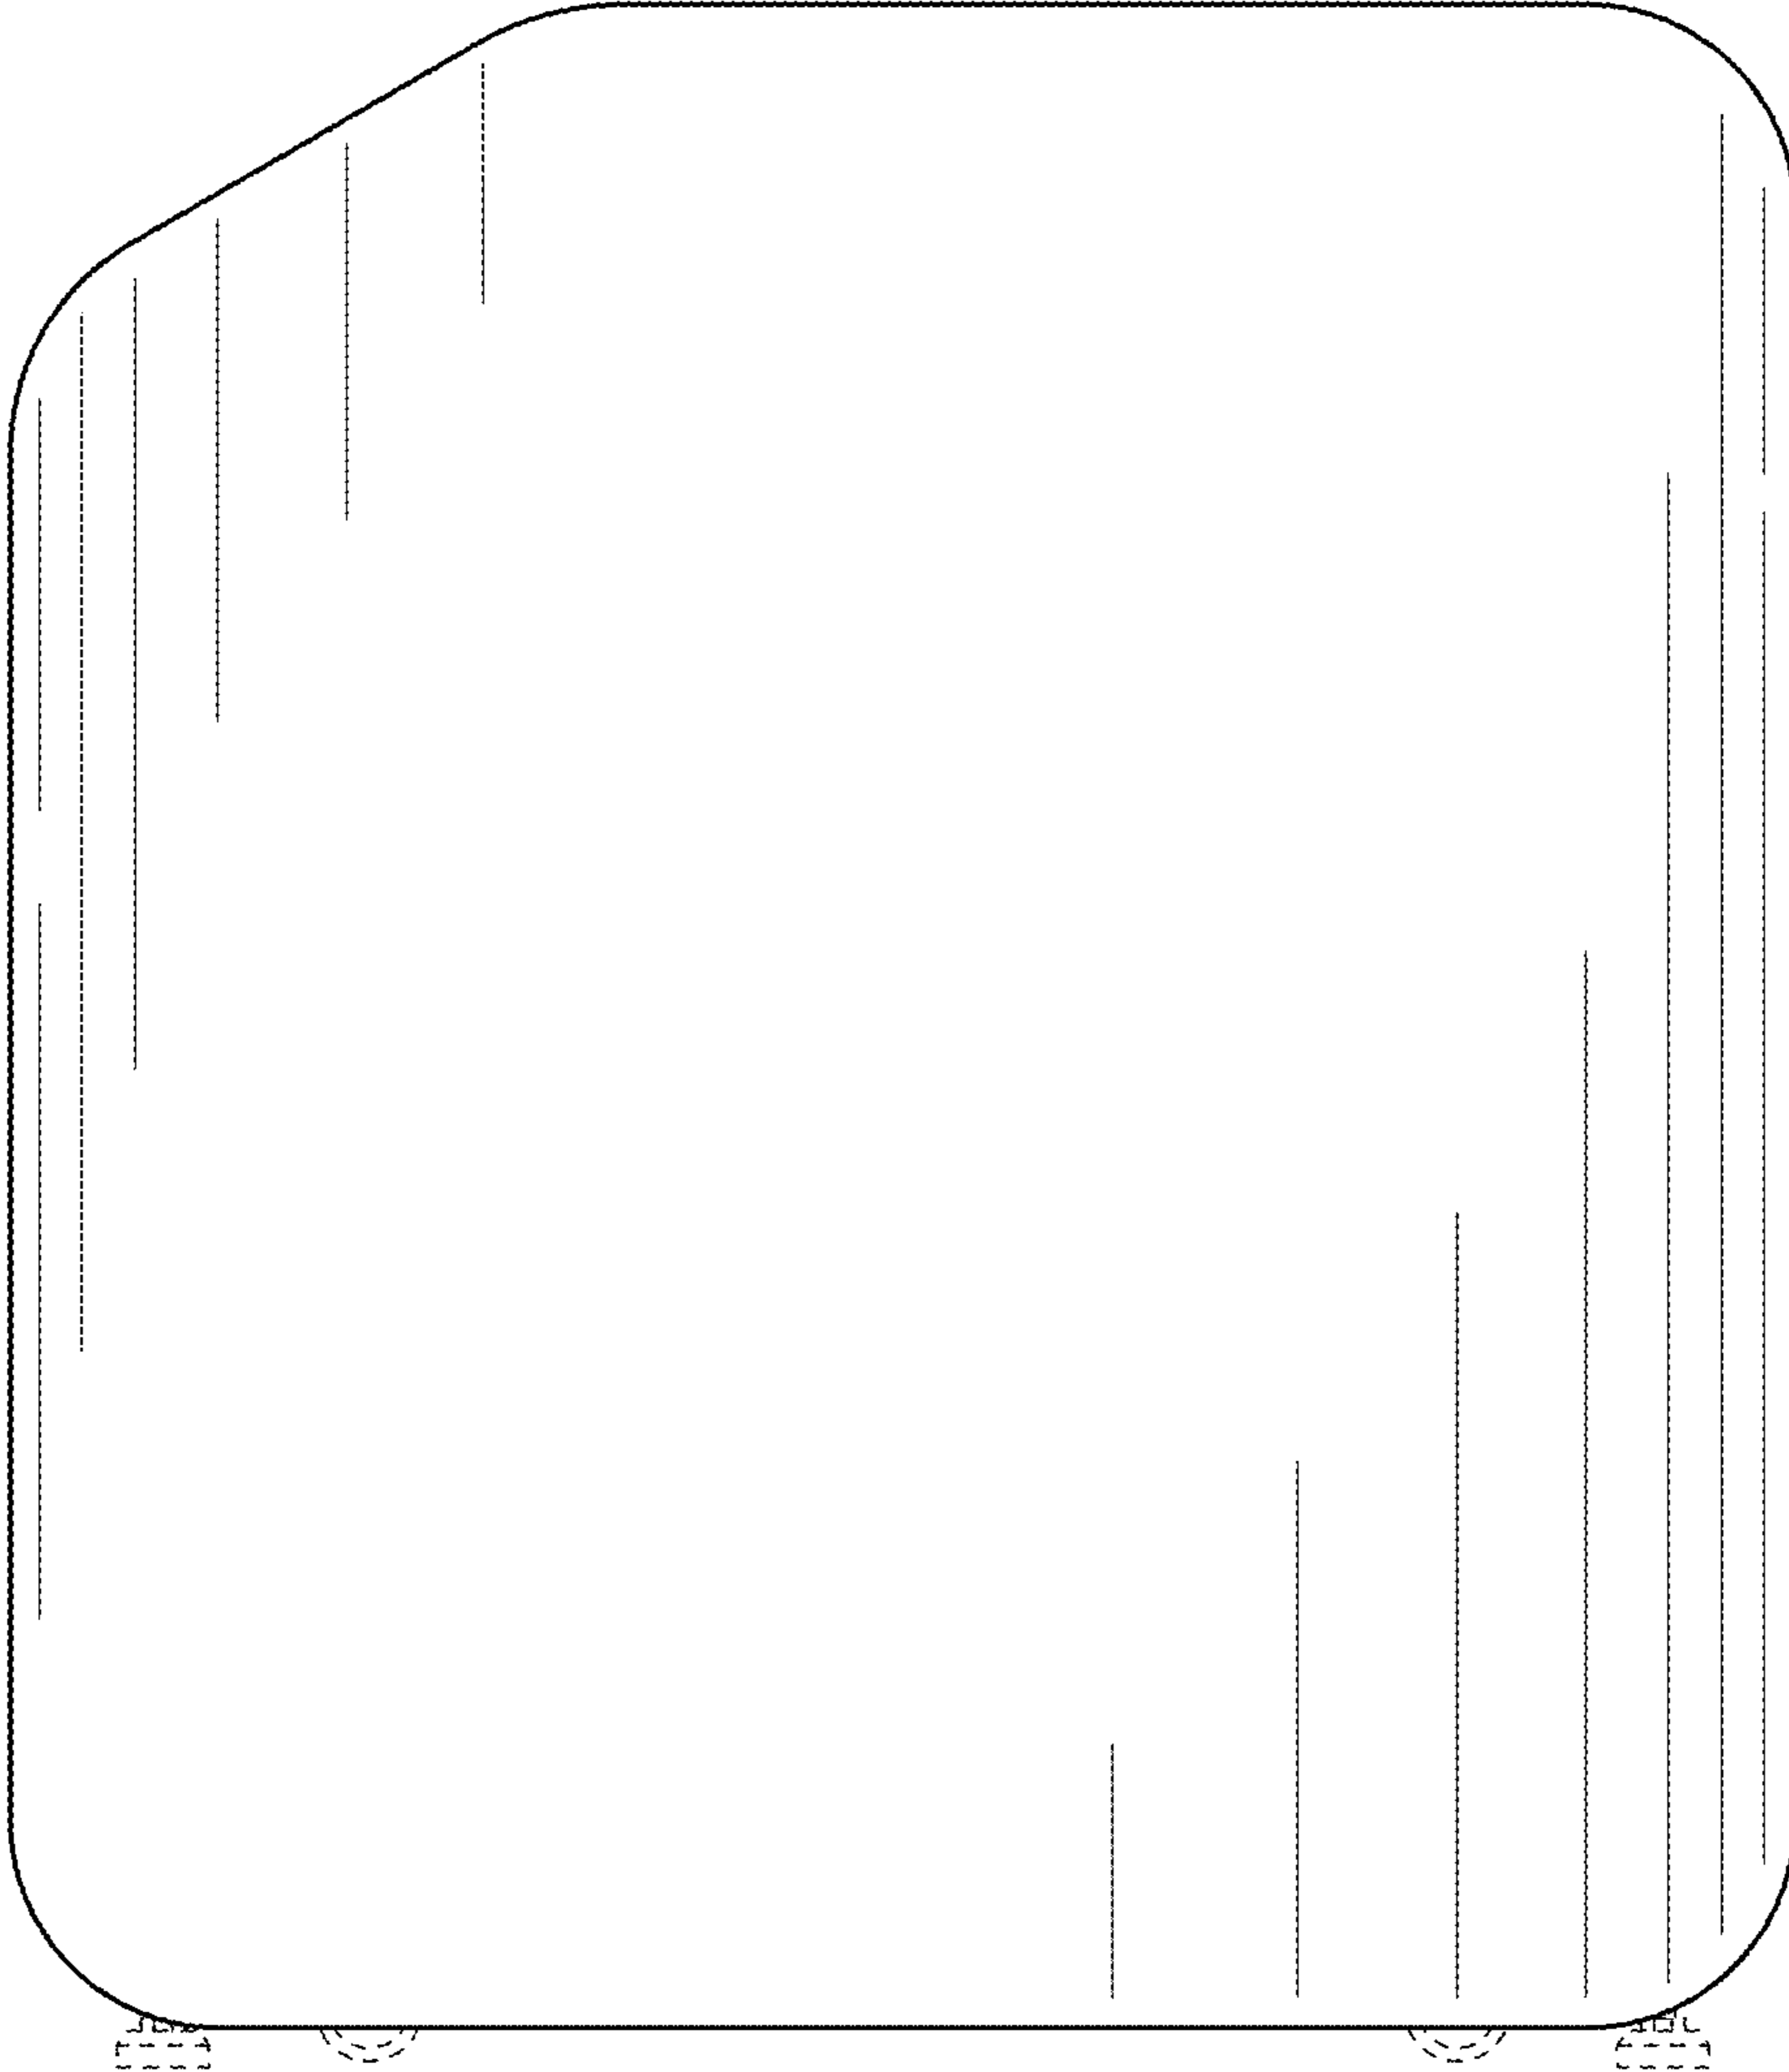


FIG. 4

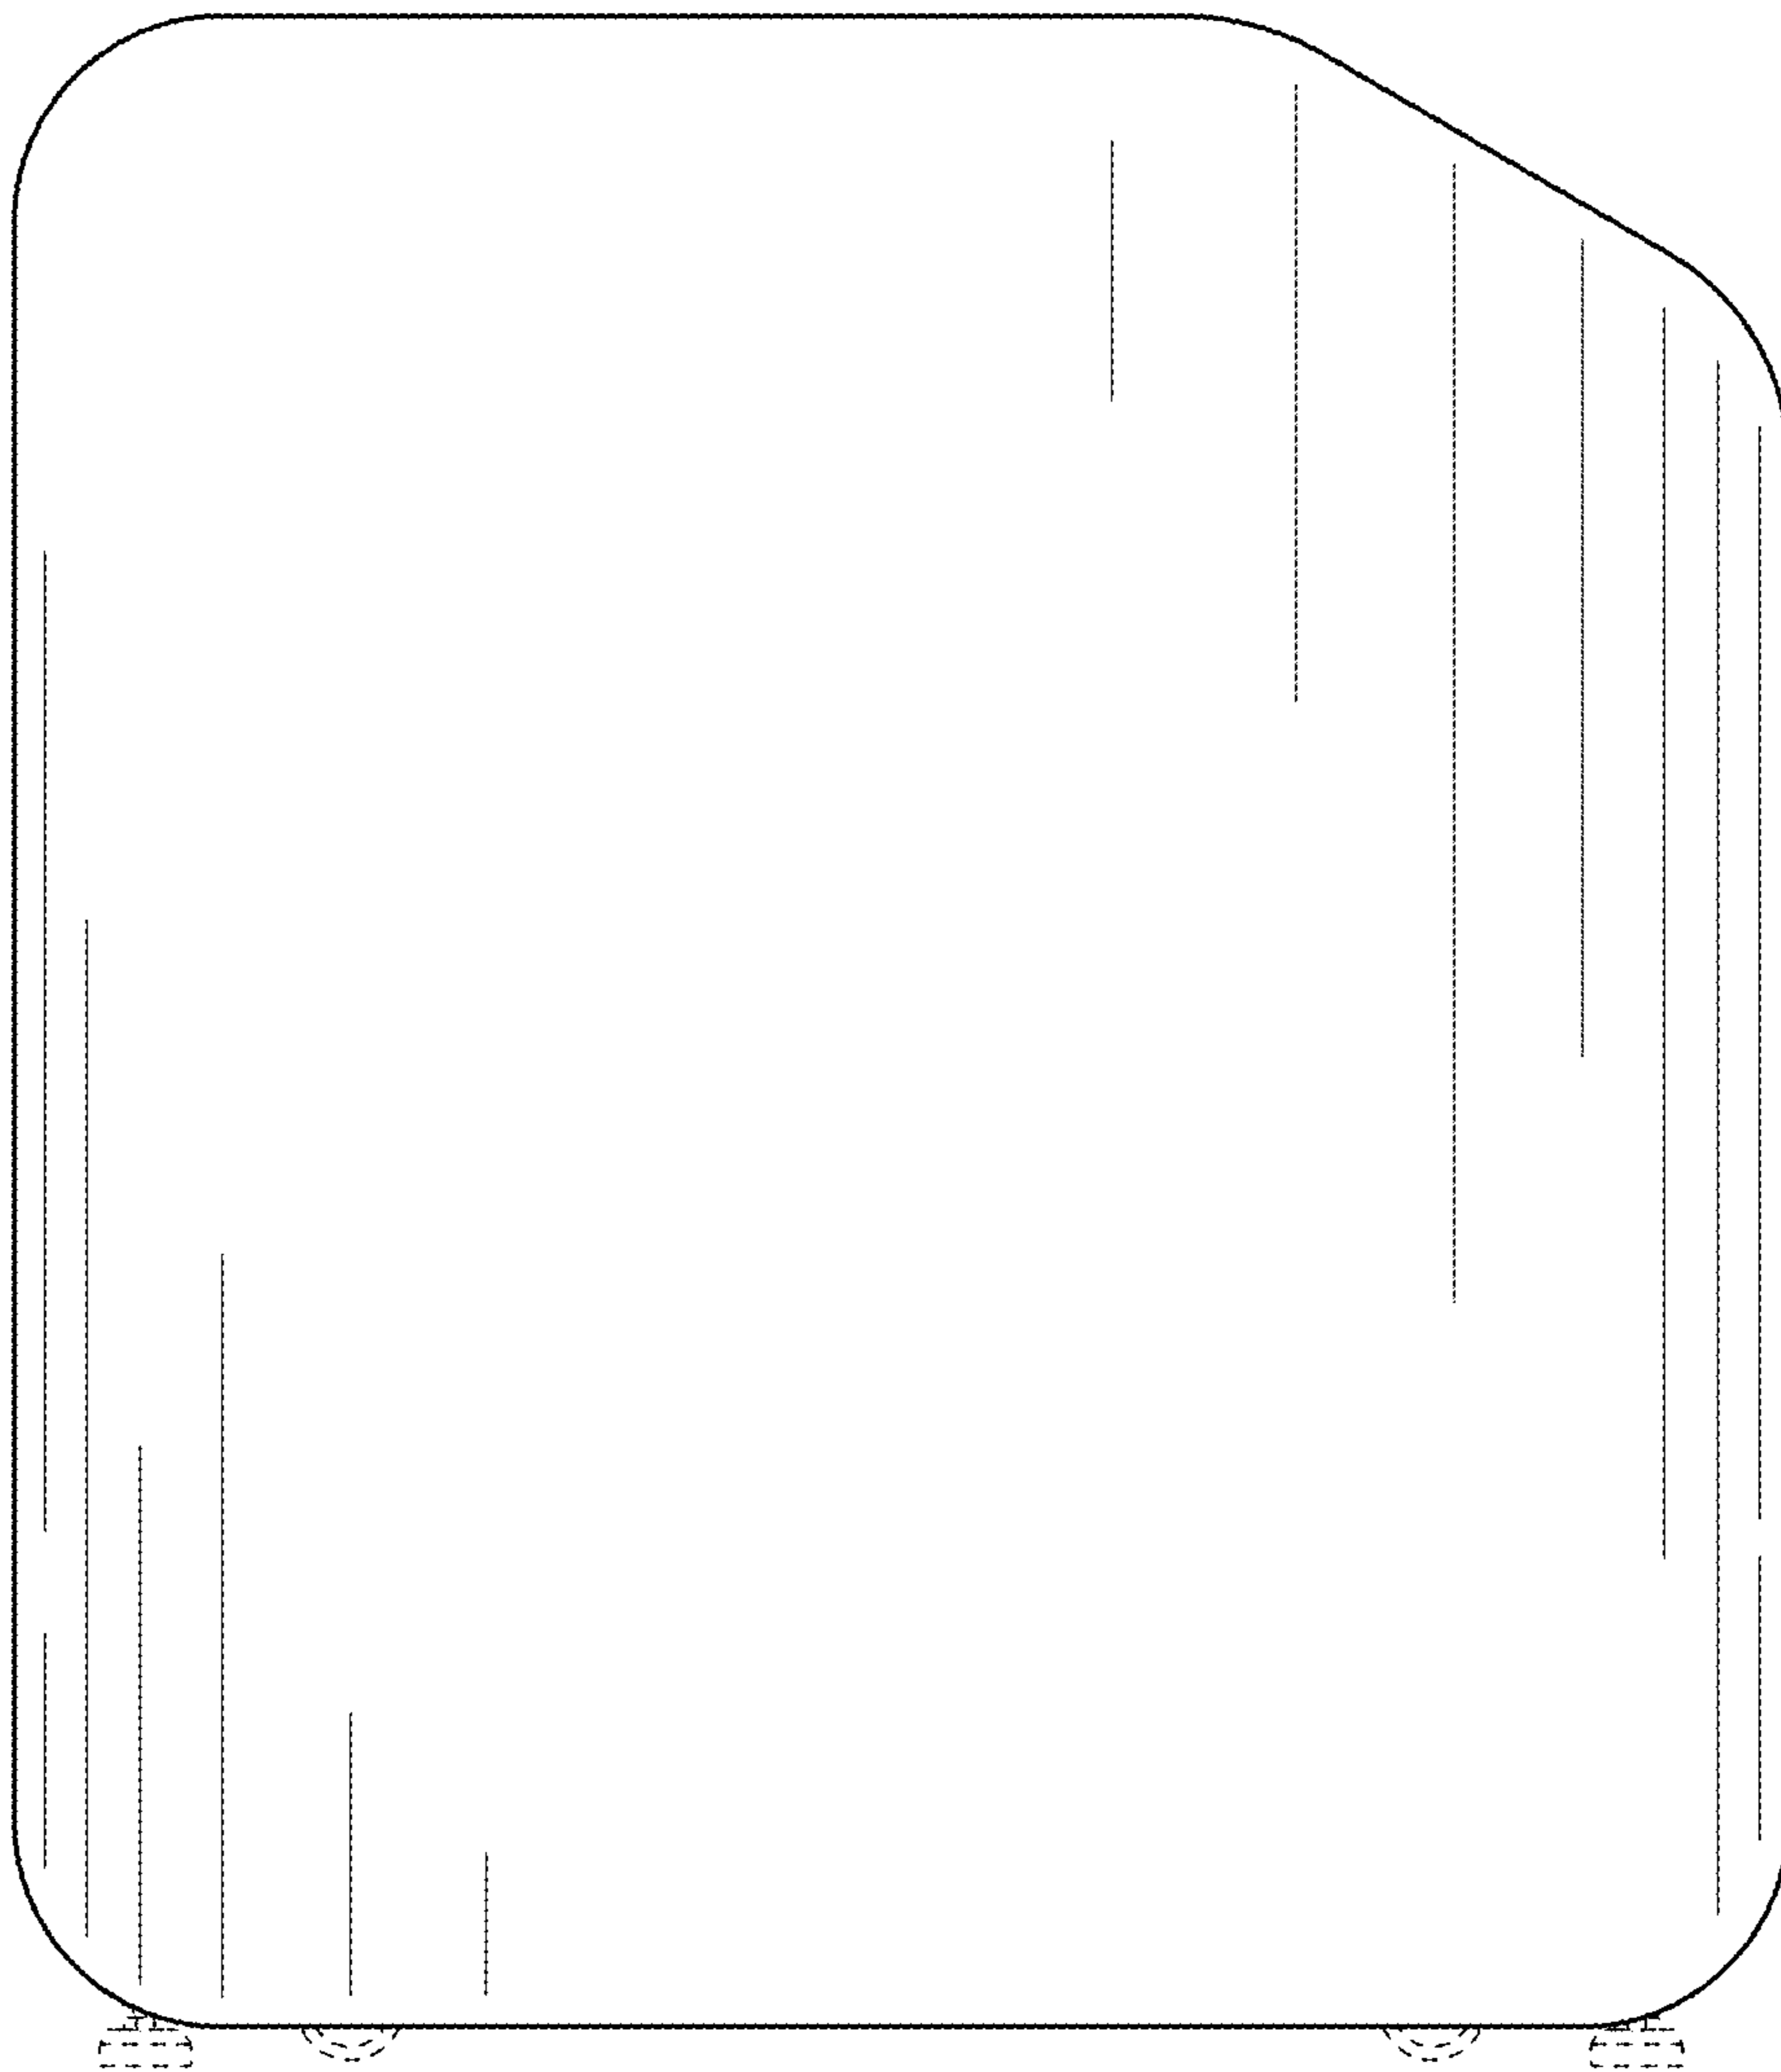


FIG. 5

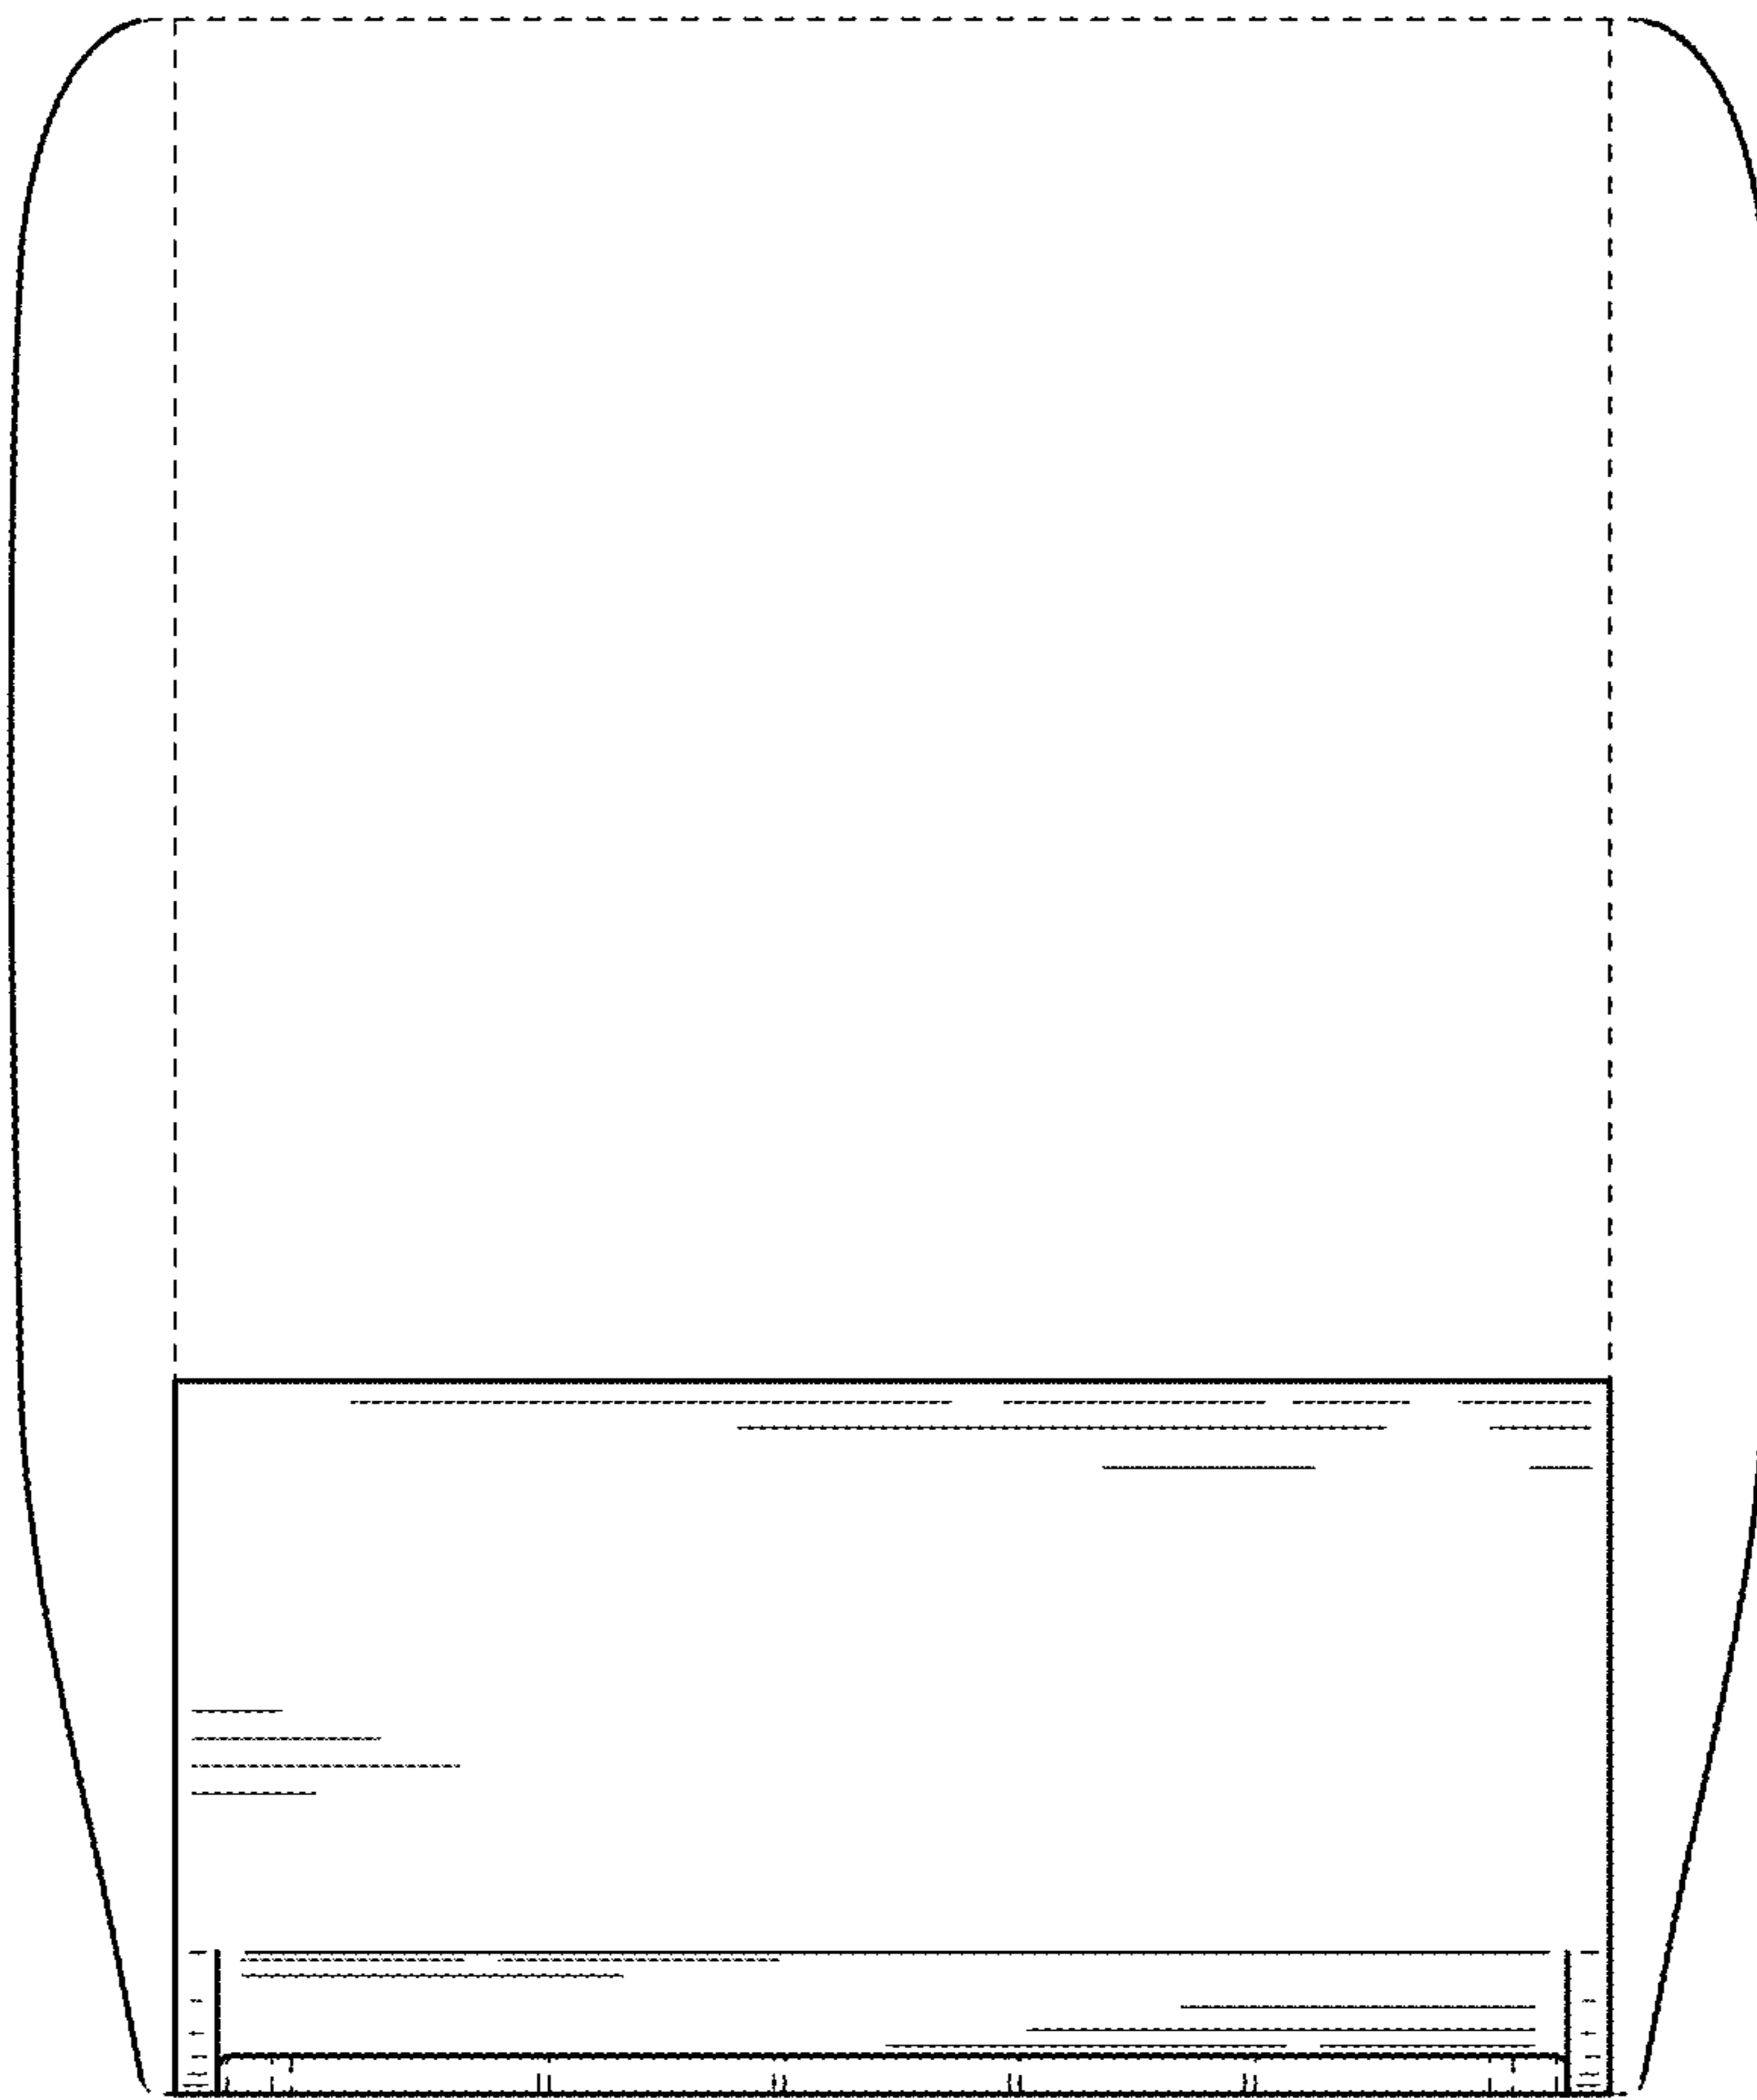


FIG. 6

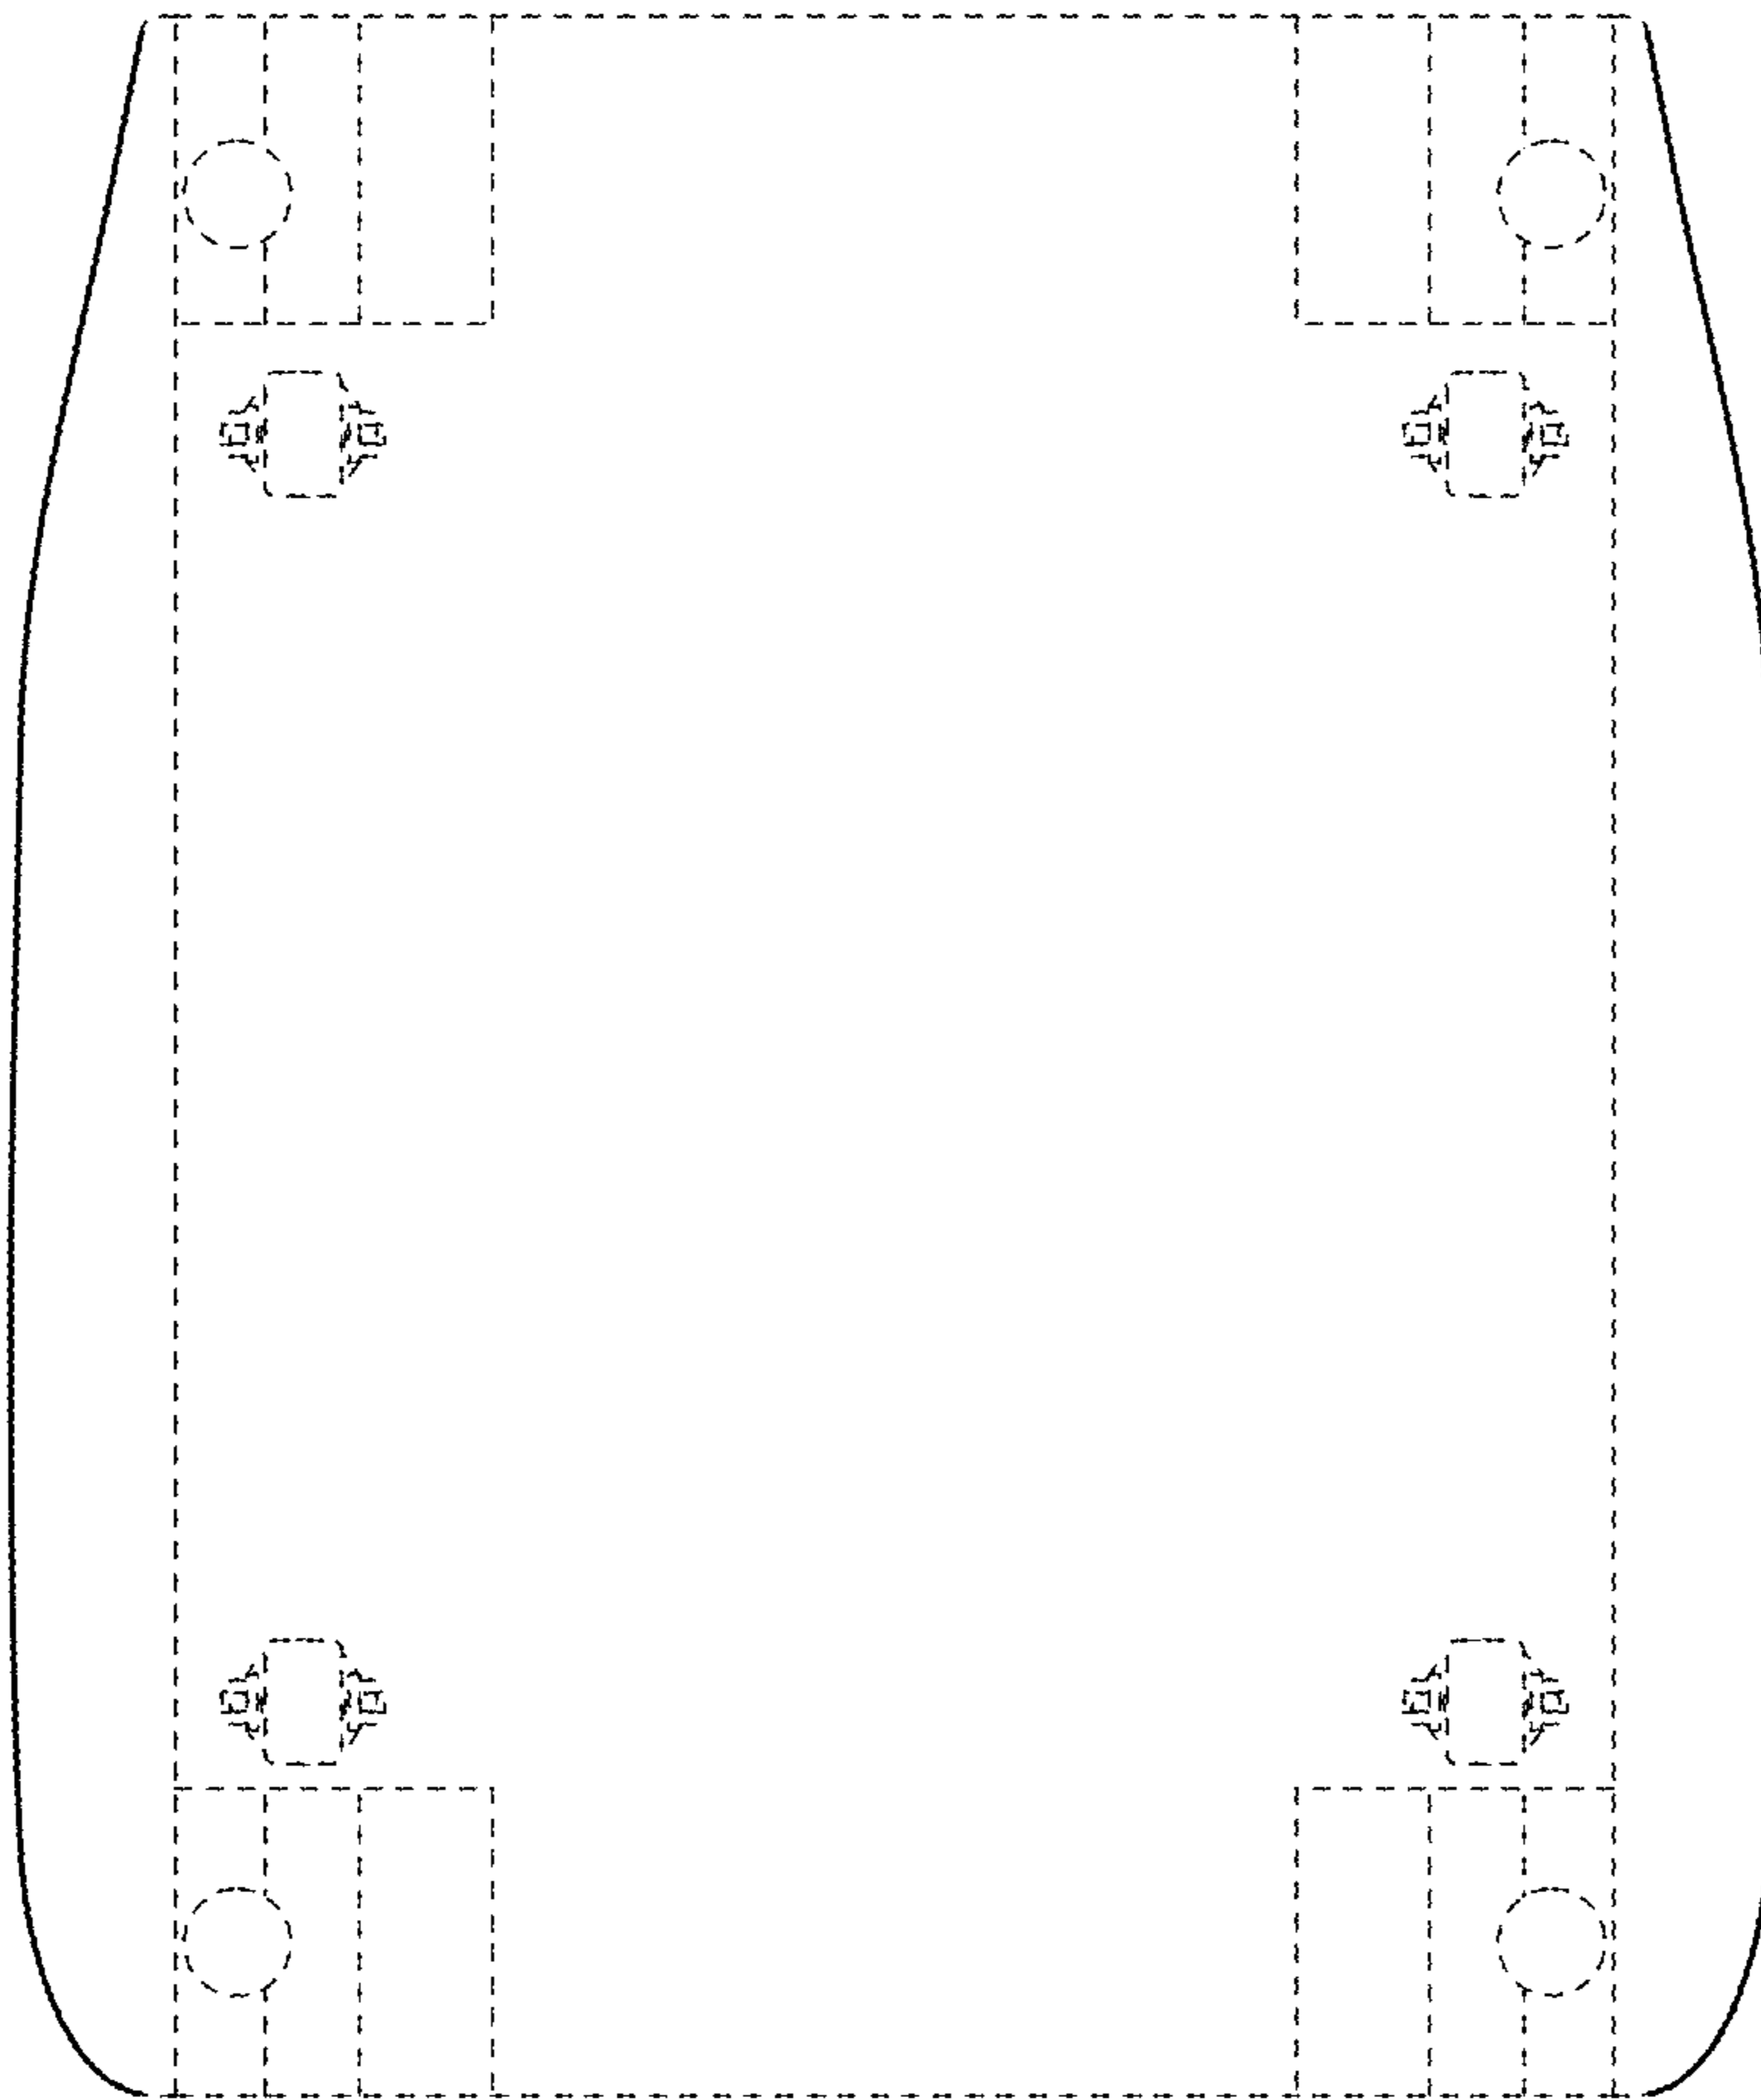


FIG. 7

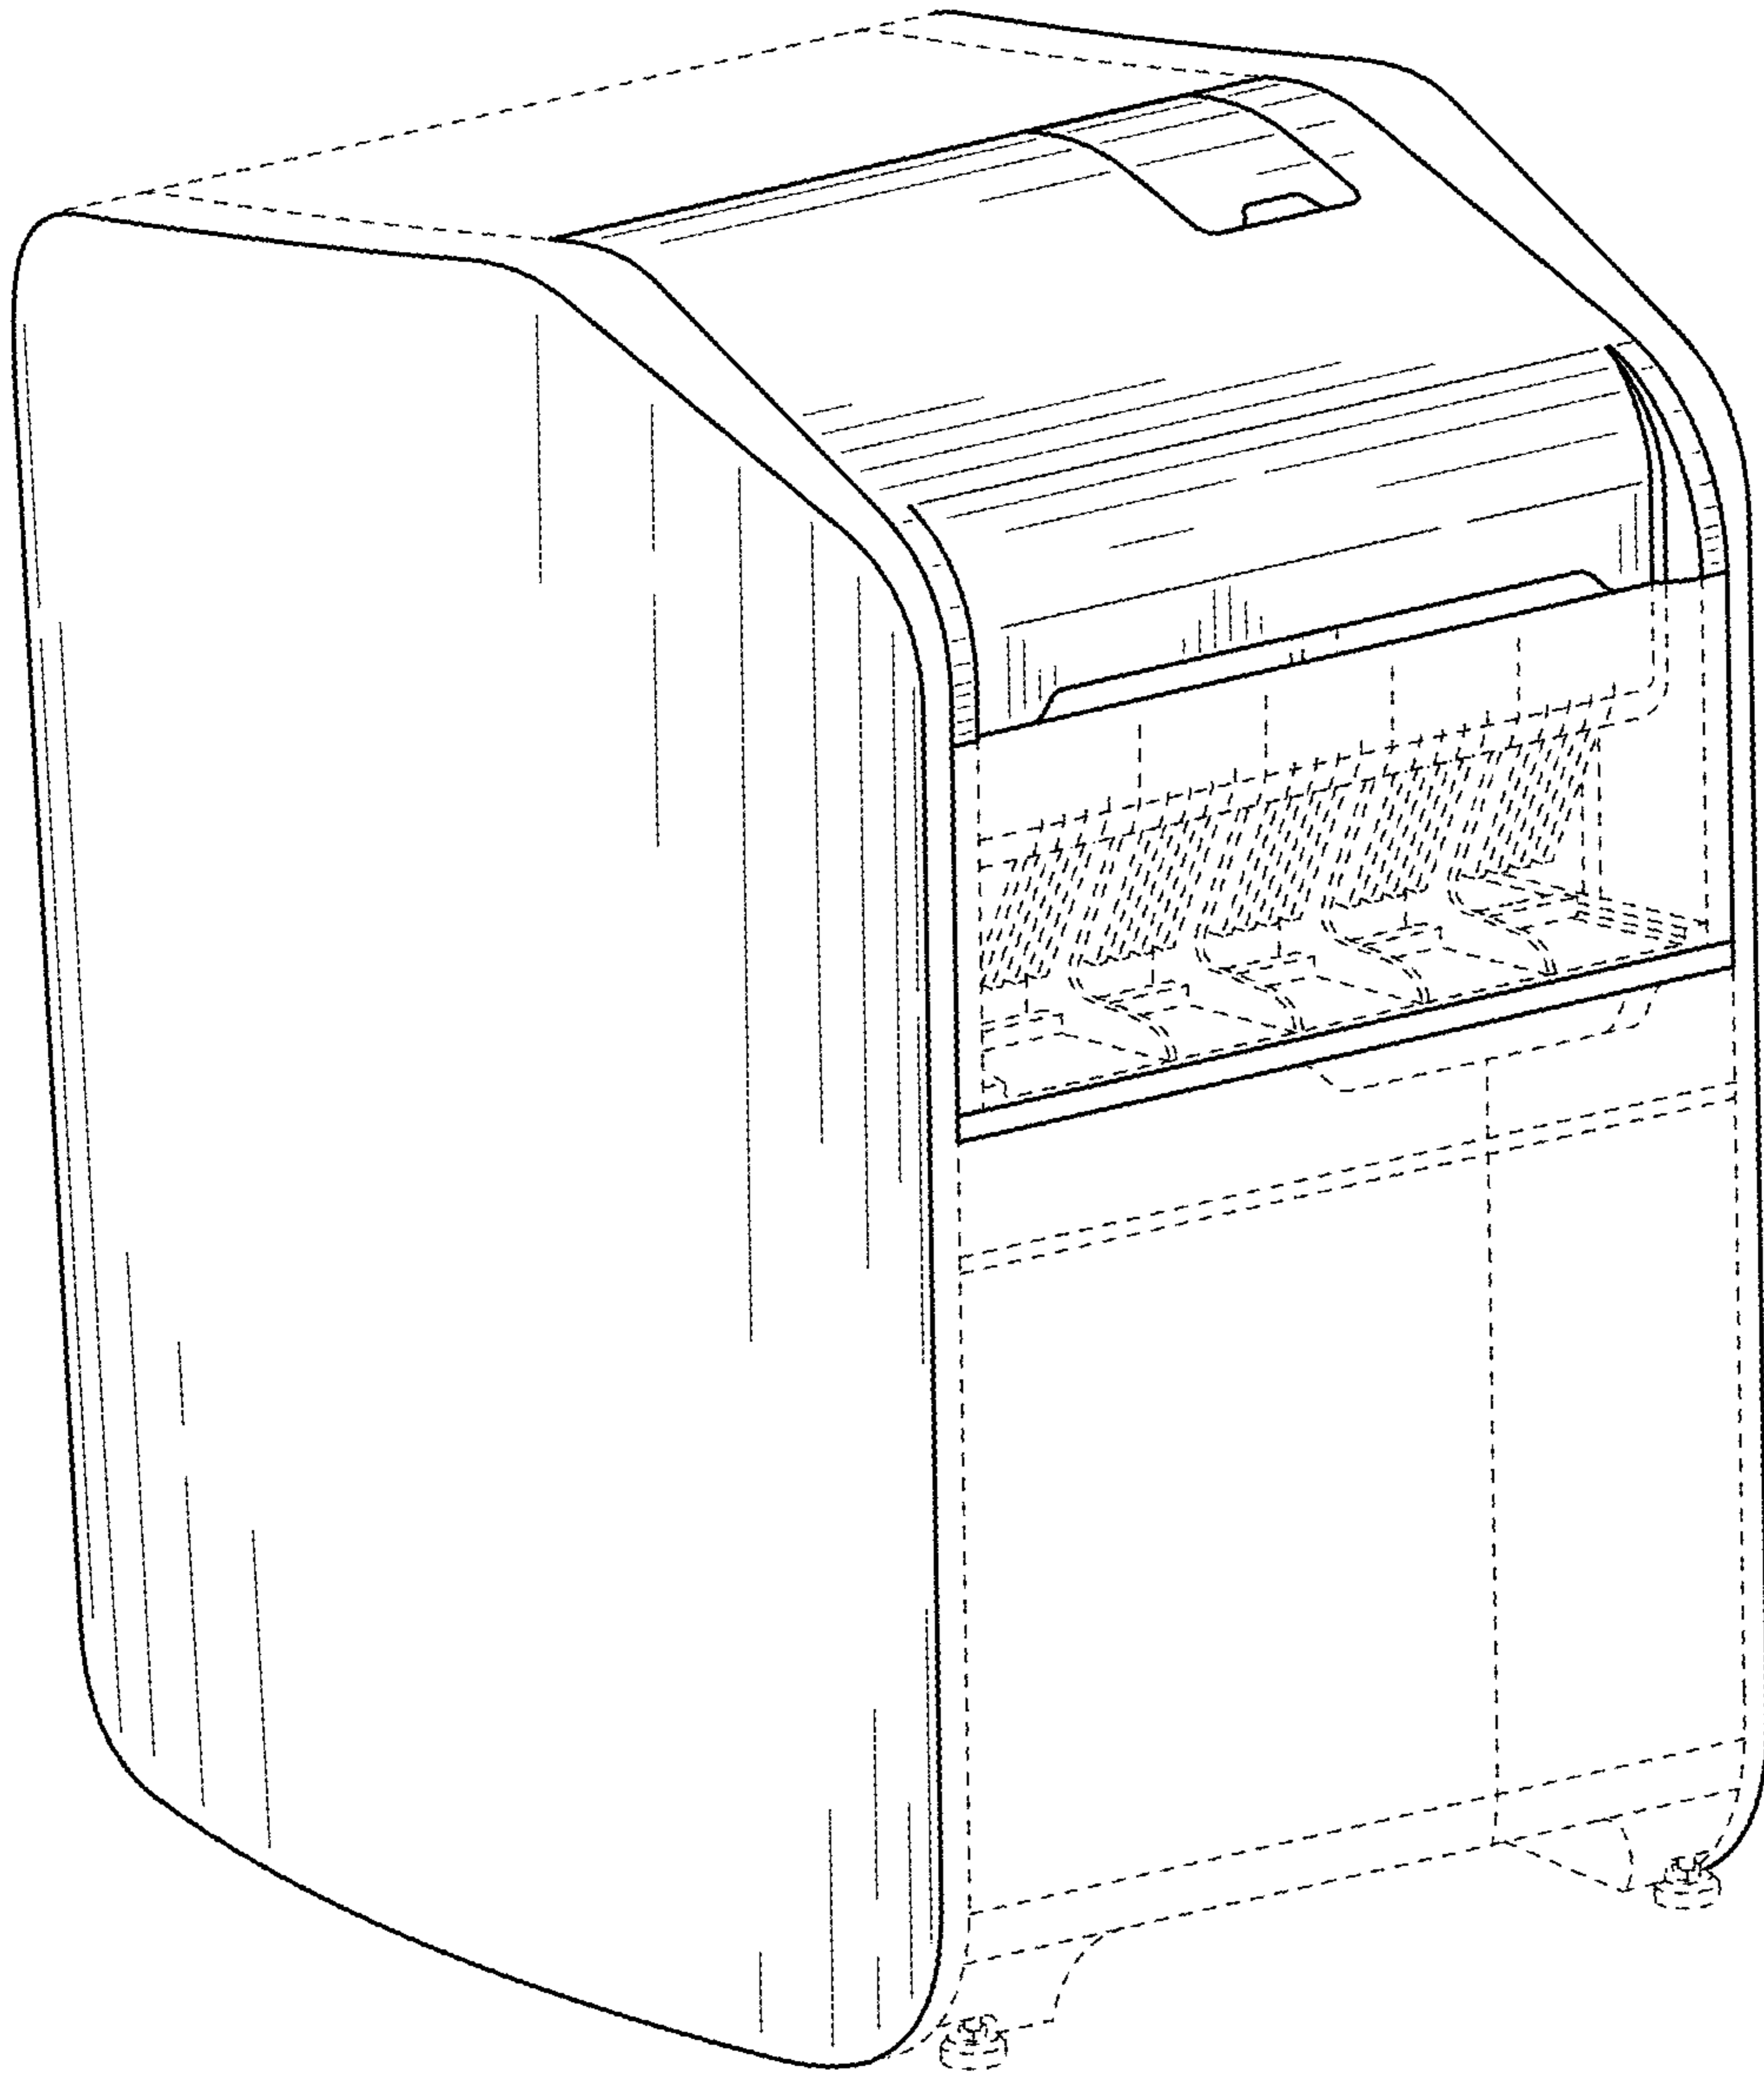


FIG. 8

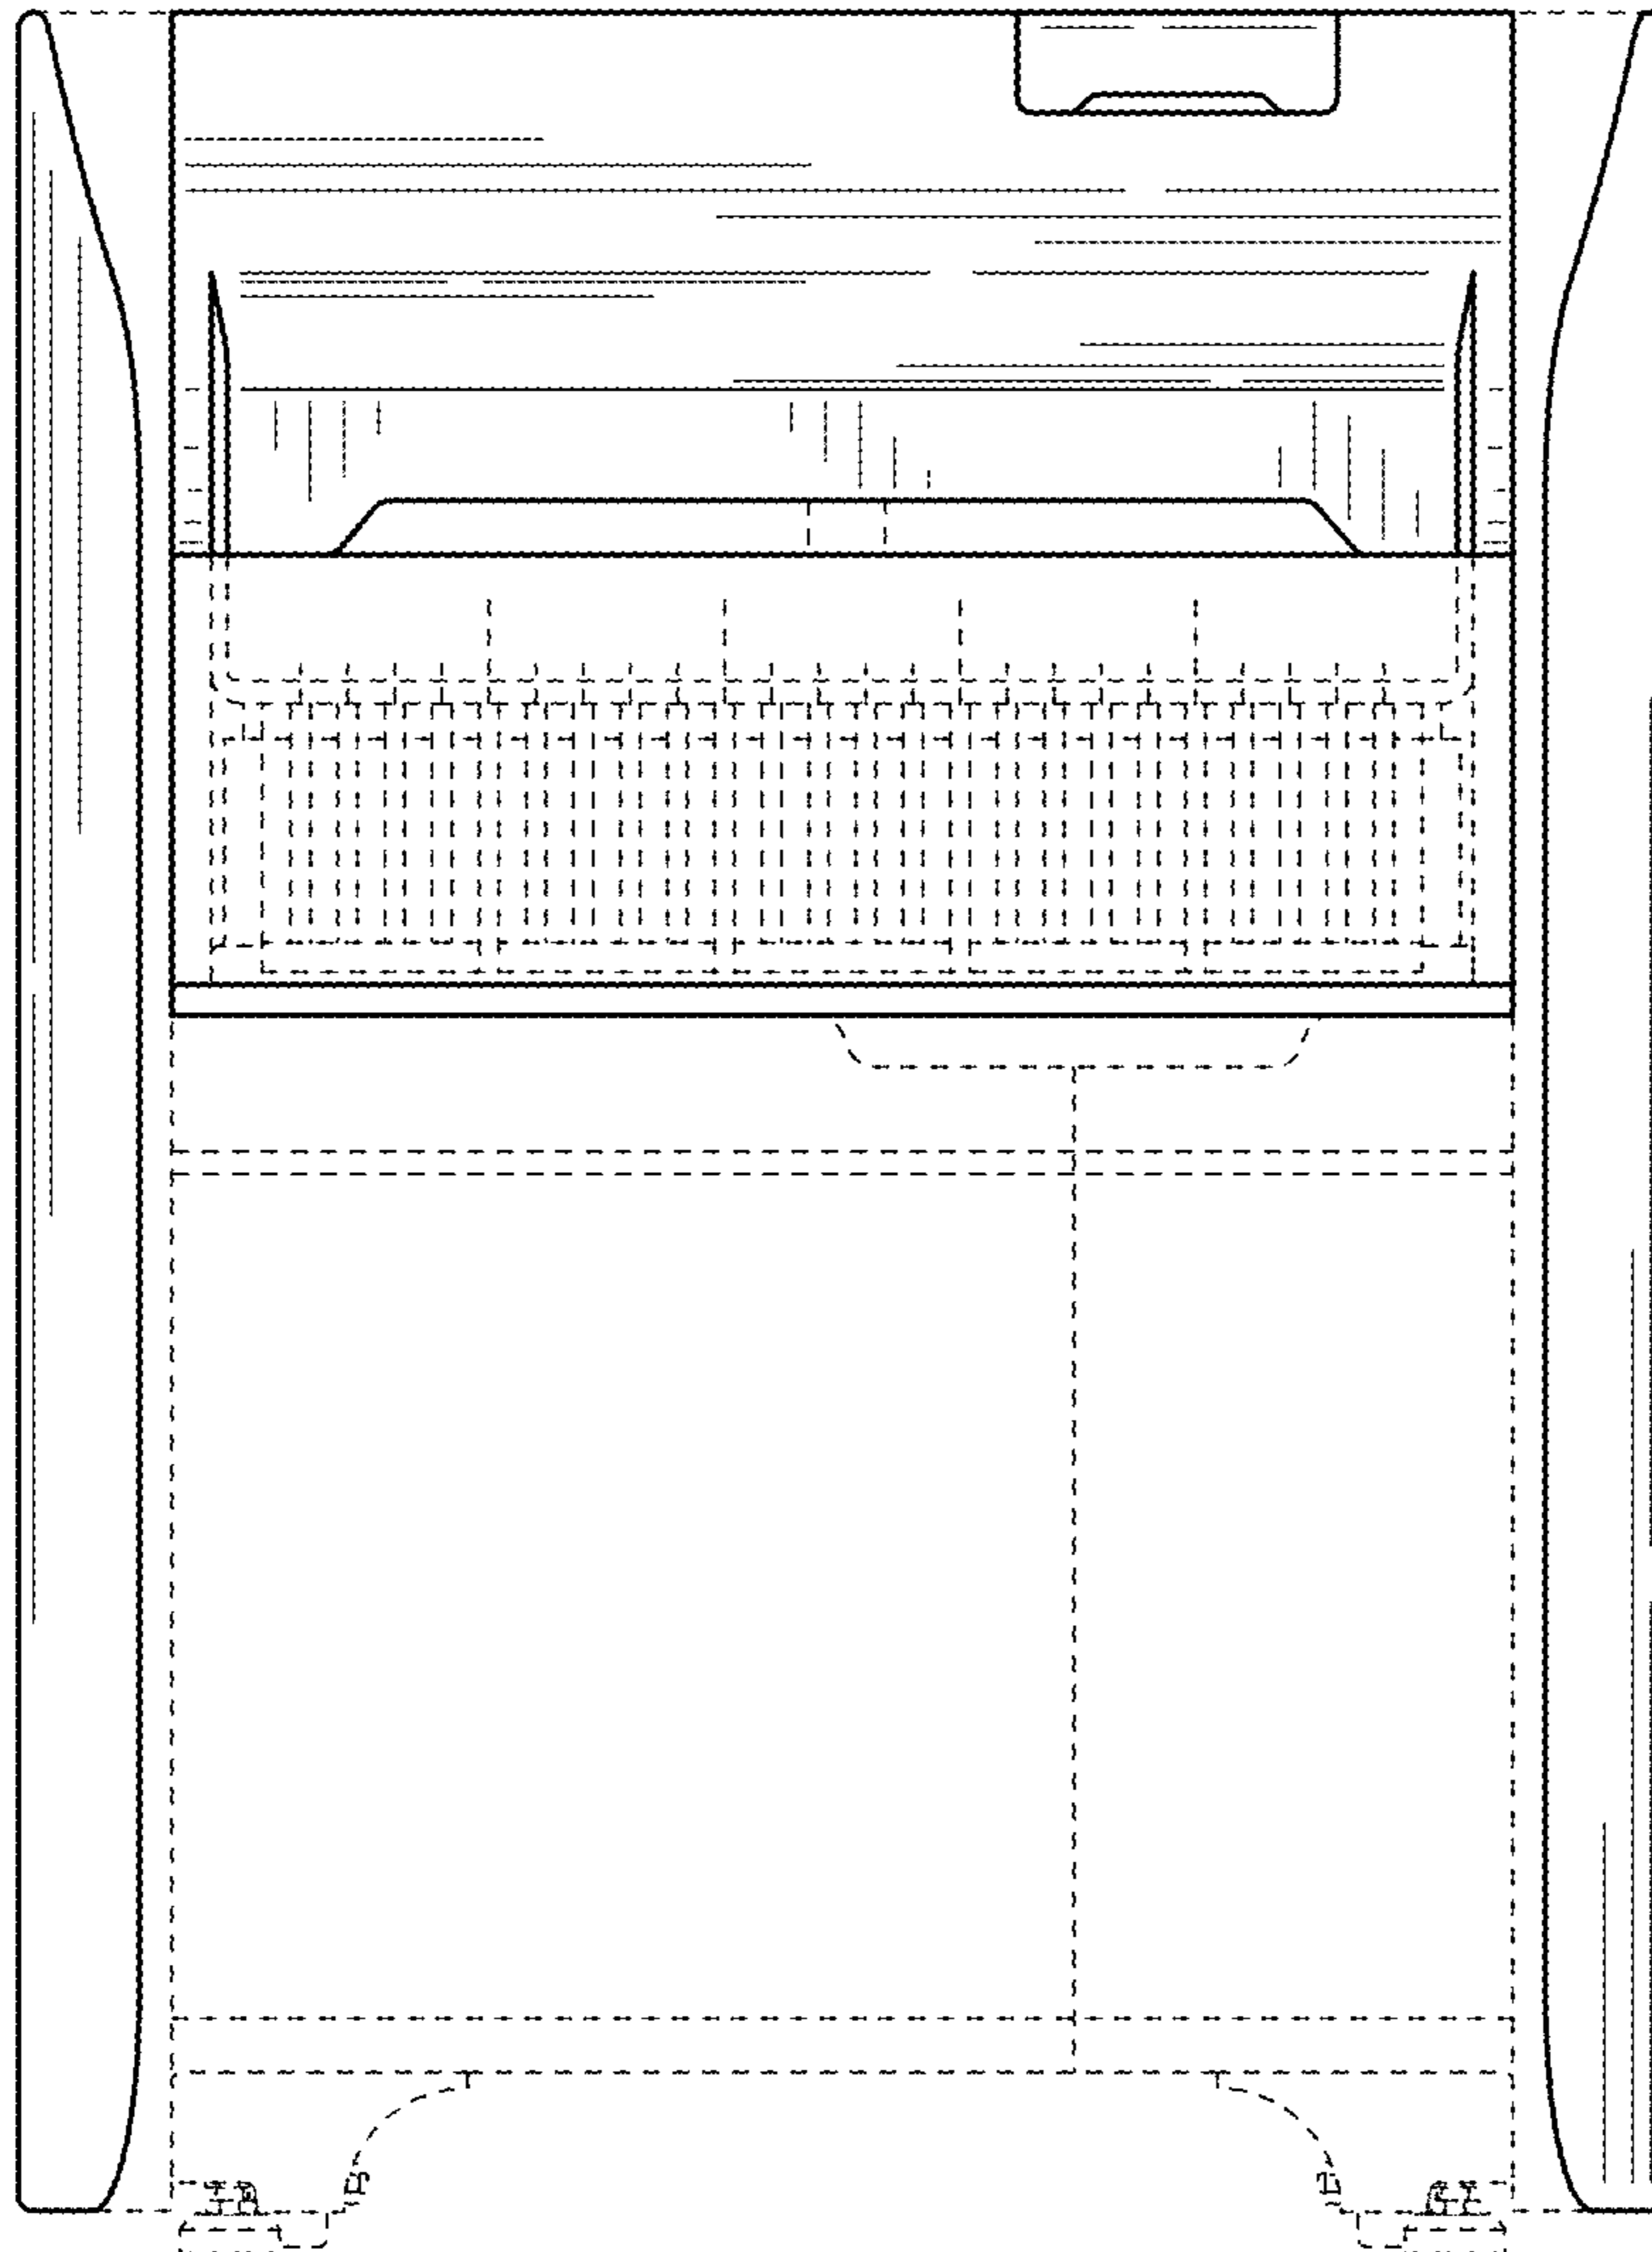


FIG. 9

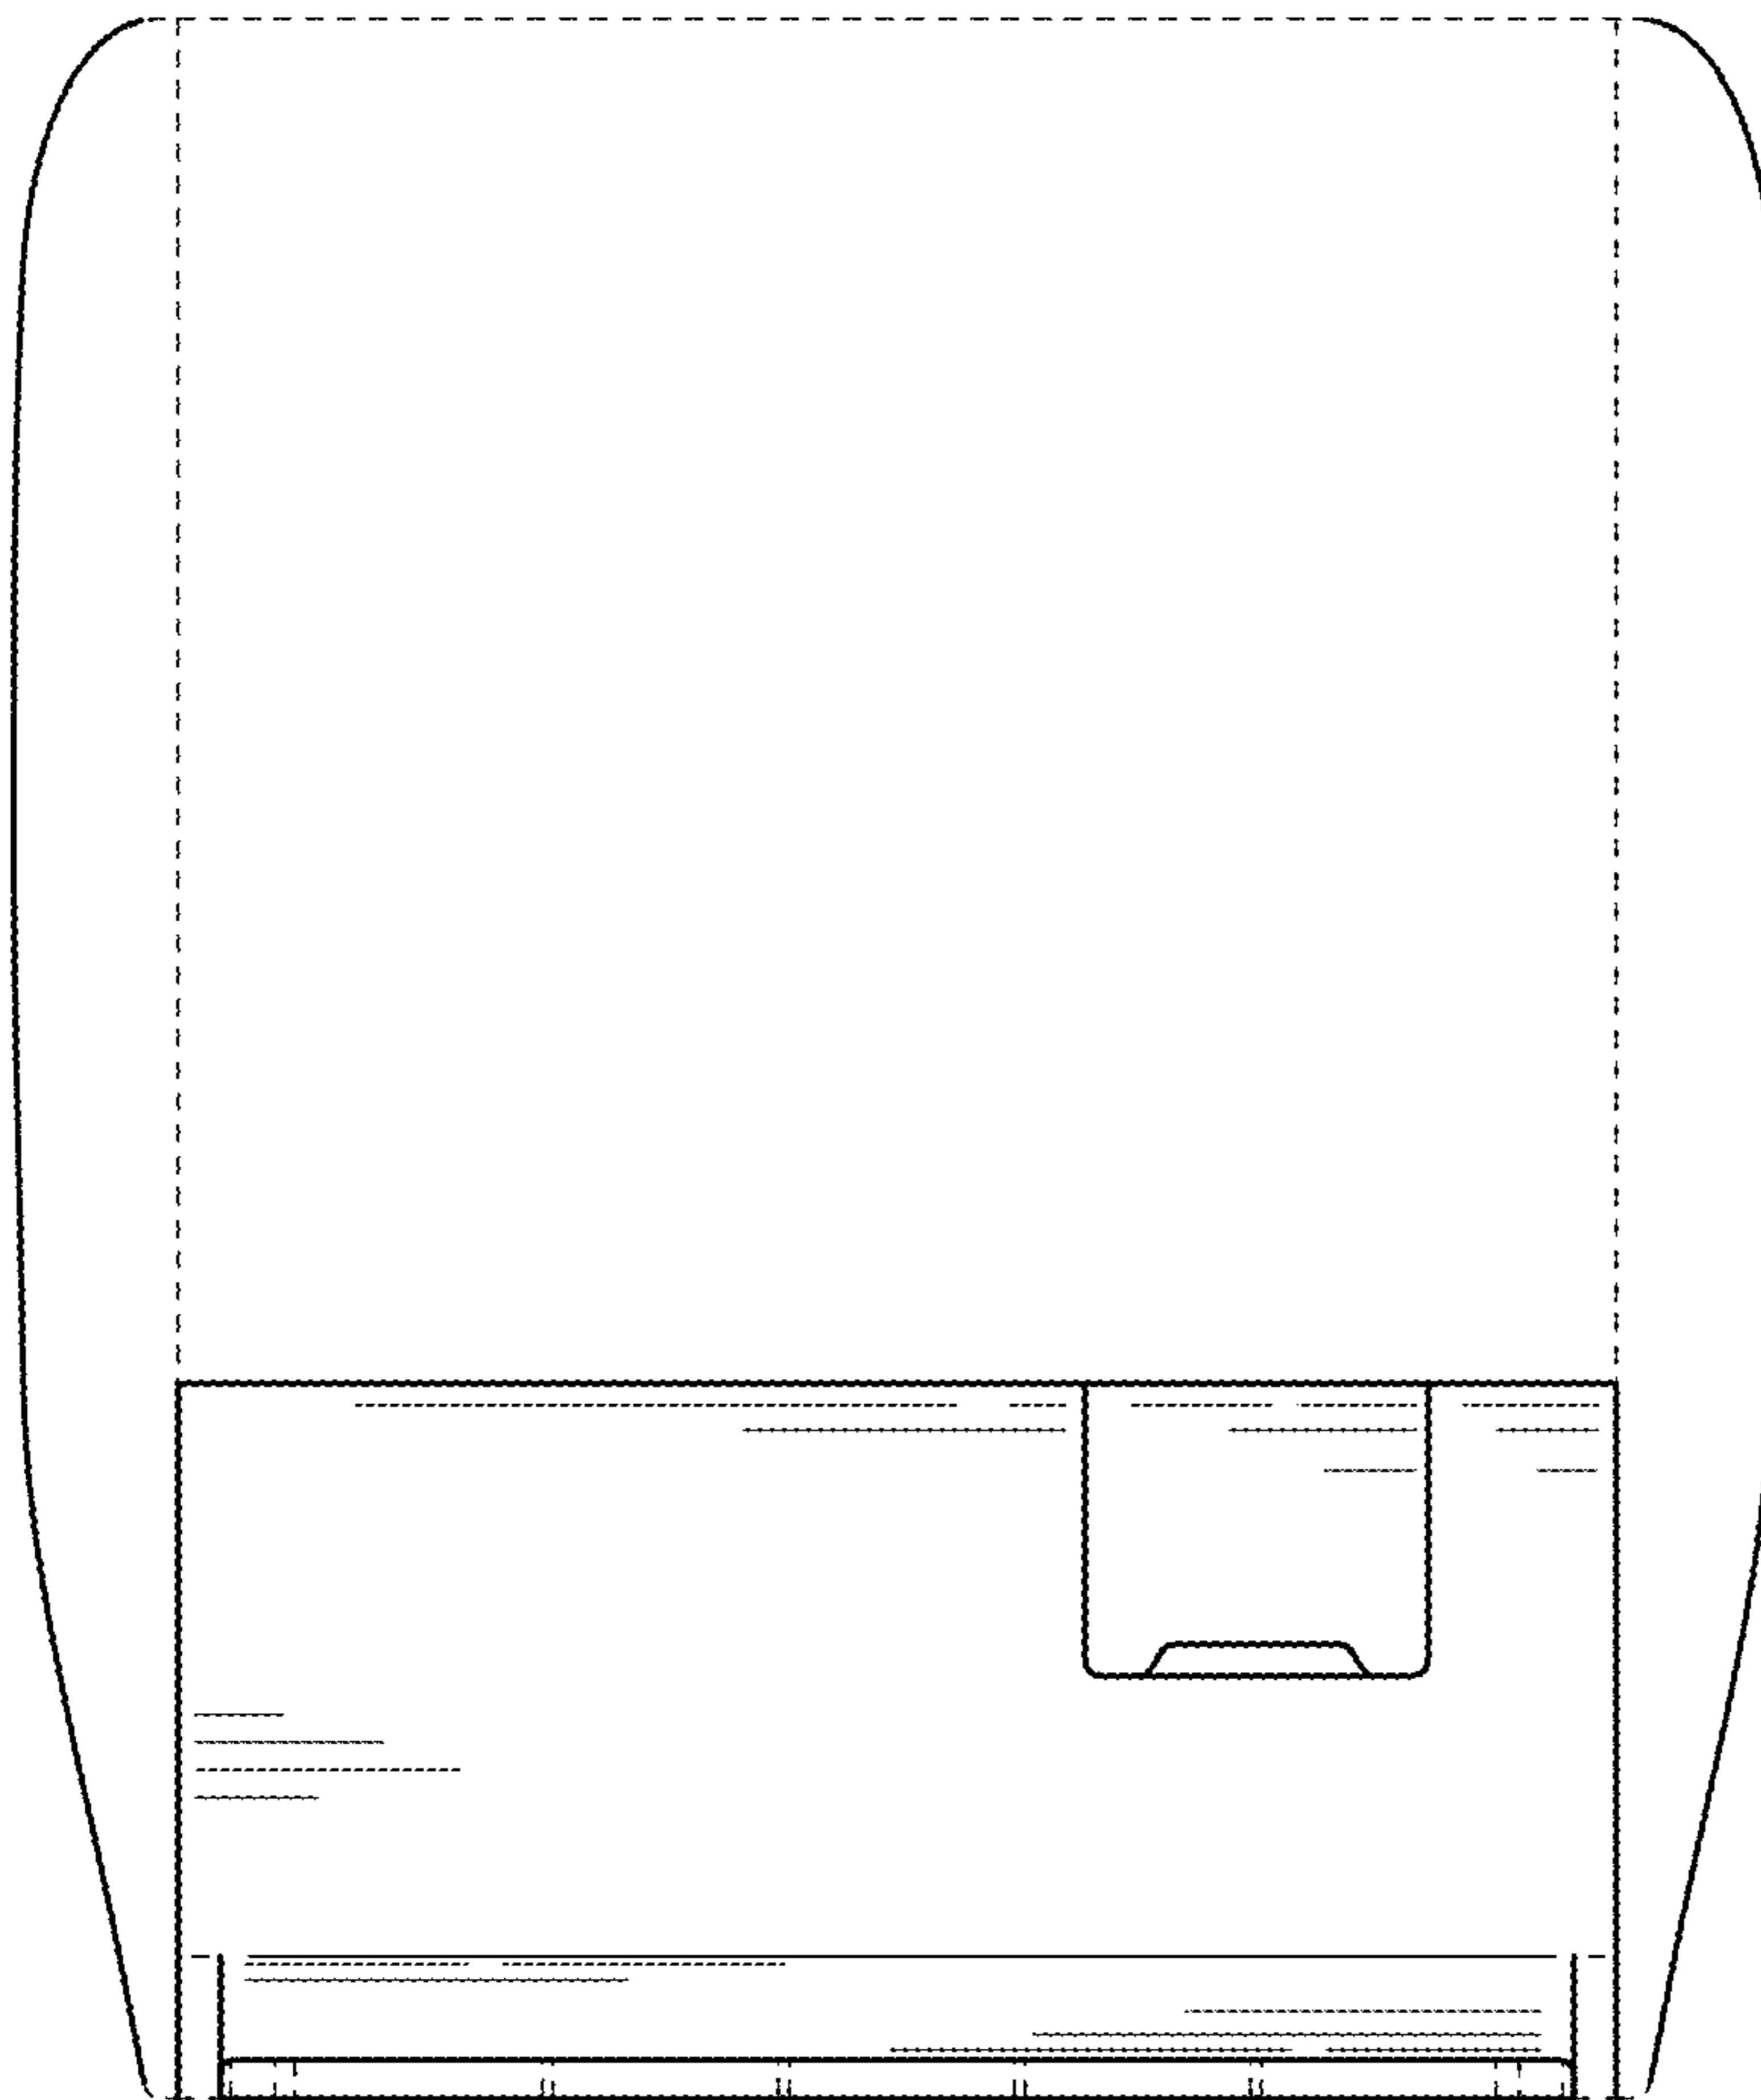


FIG. 10