



US00D825746S

(12) **United States Design Patent** (10) **Patent No.:** **US D825,746 S**  
**Davis et al.** (45) **Date of Patent:** **\*\* Aug. 14, 2018**

(54) **SYRINGE-TO-SYRINGE COUPLER**  
(71) Applicant: **NEOMED, INC.**, Woodstock, GA (US)  
(72) Inventors: **Benjamin Martin Davis**, Woodstock, GA (US); **Aaron N. Ingram**, Canton, GA (US); **Mark M. Costello**, Co. Mayo (IE); **John Burke**, County Roscommon (IE)

4,842,592 A 6/1989 Caggiani et al.  
D303,710 S \* 9/1989 Neill ..... D23/262  
D327,318 S \* 6/1992 Dudar ..... D24/112  
(Continued)

**FOREIGN PATENT DOCUMENTS**

DE 7740288 U1 5/1978  
DE 8613738 U1 7/1986  
(Continued)

(73) Assignee: **NEOMED, INC.**, Woodstock, GA (US)  
(\*\*) Term: **15 Years**

**OTHER PUBLICATIONS**

Covidien ENFit Coupling; Mar. 2014; 1 pg.  
(Continued)

(21) Appl. No.: **29/530,722**  
(22) Filed: **Jun. 18, 2015**  
(51) **LOC (11) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/129**  
(58) **Field of Classification Search**  
USPC ..... D24/127-131, 112-114, 133, 186;  
606/181, 185; 604/264, 523-528, 272,  
604/187, 158, 164.01-164.11, 181, 184,  
604/227; 600/101, 139, 143;  
128/200.24, 207.14, 207.15  
CPC ..... A61M 25/00; A61M 39/00; A61M 27/00;  
A61M 25/0043; A61M 25/0067; A61M  
25/0097; A61F 2/958  
See application file for complete search history.

*Primary Examiner* — David Muller  
(74) *Attorney, Agent, or Firm* — Gardner Groff  
Greenwald & Villanueva, PC

(57) **CLAIM**

The ornamental design for a syringe-to-syringe coupler, substantially as shown and described.


**DESCRIPTION**

FIG. 1 is a perspective view of a syringe-to-syringe coupler according to an embodiment of the design.  
FIG. 2 is a front view of the syringe-to-syringe coupler shown in FIG. 1, the rear view being substantially identical to the front view.  
FIG. 3 is a top view of the syringe-to-syringe coupler shown in FIG. 1, the bottom view being substantially identical to the front view.  
FIG. 4 is a first (left or right) side view of the syringe-to-syringe coupler shown in FIG. 1, the opposite side view being substantially identical to the front view; and,  
FIG. 5 is a perspective view showing the environment of a syringe-to-syringe coupler according to the design in use coupling two syringes.  
Portions shown in broken lines are for illustrative purposes only and form no part of the claimed design.

(56) **References Cited**  
**U.S. PATENT DOCUMENTS**

2,477,598 A 8/1949 Hain  
3,473,833 A 10/1969 Bremer  
3,572,337 A 3/1971 Schunk  
4,046,145 A 9/1977 Choksi et al.  
4,685,173 A 8/1987 Pavur  
4,743,229 A 5/1988 Chu

**1 Claim, 3 Drawing Sheets**

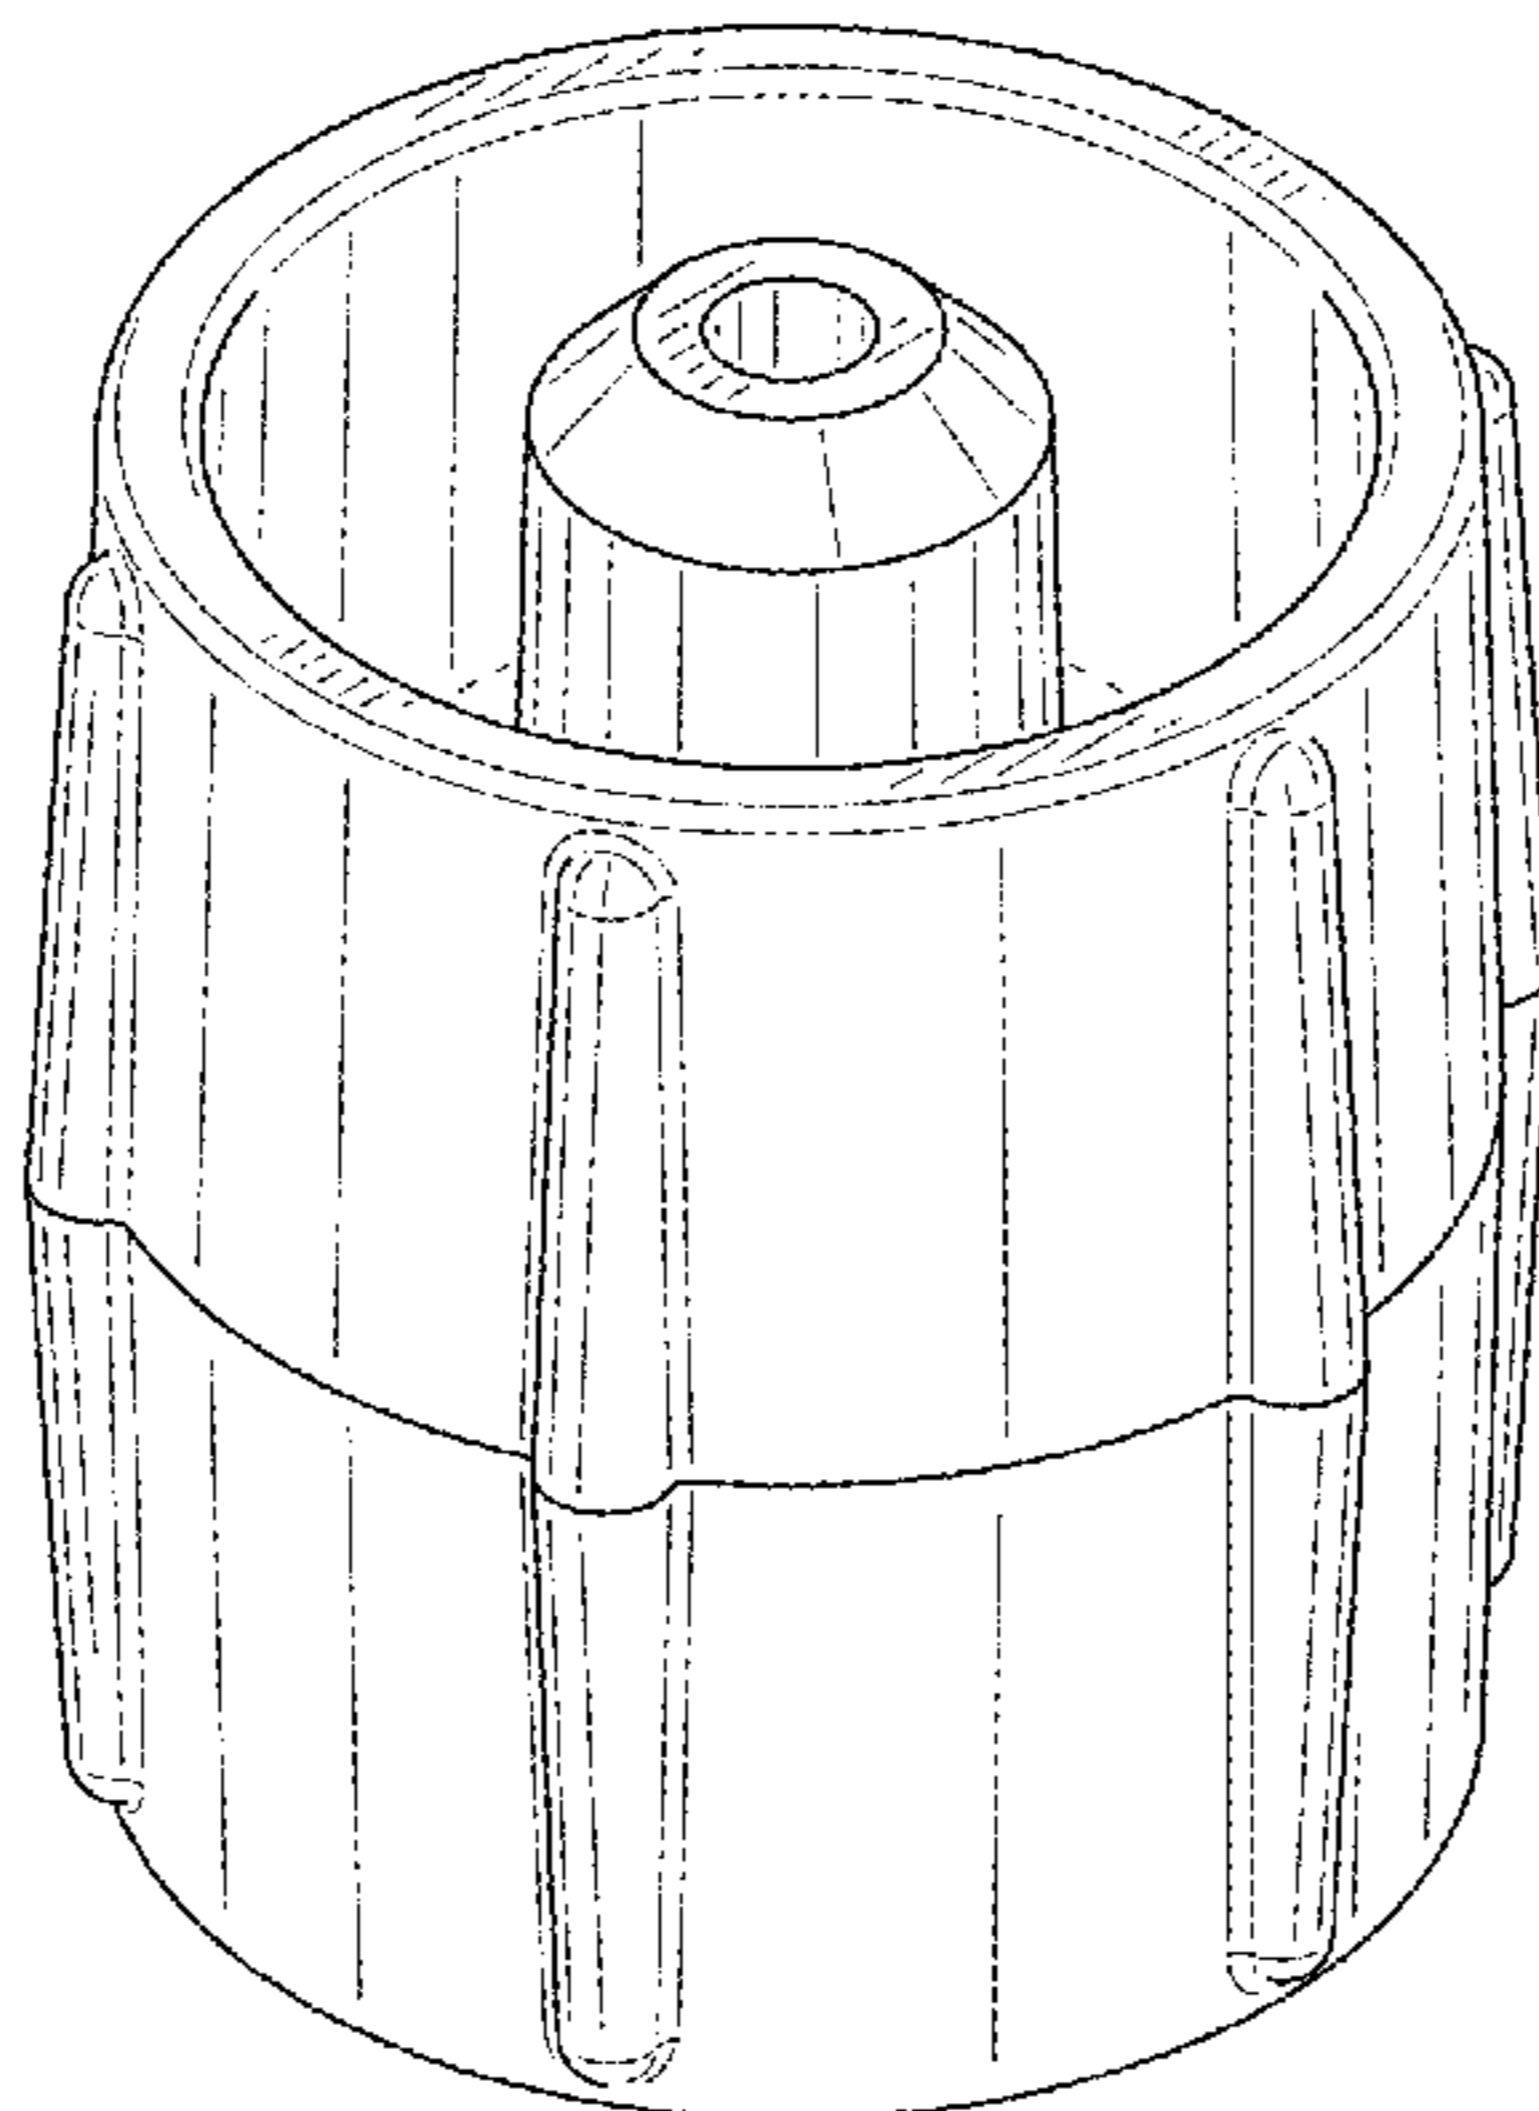

(56)

References Cited

U.S. PATENT DOCUMENTS

5,224,937 A 7/1993 van der Heiden et al.  
 5,405,339 A 4/1995 Kohnen et al.  
 D395,502 S \* 6/1998 Deily ..... D24/112  
 D398,060 S 9/1998 Brown  
 5,957,166 A 9/1999 Safabash  
 D435,652 S \* 12/2000 Nazarifar ..... D23/262  
 6,270,519 B1 8/2001 Botts  
 D473,647 S \* 4/2003 Francavilla ..... D24/129  
 6,592,251 B2 7/2003 Edwards et al.  
 6,726,672 B1 4/2004 Hanly et al.  
 D534,796 S \* 1/2007 Falkenburg ..... D23/262  
 7,503,905 B2 3/2009 Jessop et al.  
 7,523,967 B2 4/2009 Steppe  
 7,594,681 B2 9/2009 DeCarlo  
 7,666,170 B2 2/2010 Guala  
 7,740,288 B2 6/2010 Mantell  
 7,766,919 B2 8/2010 Delmotte  
 7,811,278 B2 10/2010 Knipple, Jr. et al.  
 7,857,284 B2 12/2010 Kimball et al.  
 7,985,205 B2 7/2011 Adams  
 D644,618 S 9/2011 Morihira  
 8,016,795 B2 9/2011 Barrelle et al.  
 8,109,902 B2 2/2012 Middleton et al.  
 8,152,790 B2 4/2012 Lopez et al.  
 8,303,571 B2 11/2012 Kraushaar et al.  
 8,328,768 B2 12/2012 Quigley et al.  
 8,398,607 B2 3/2013 Fangrow, Jr.  
 8,479,370 B2 7/2013 Grant  
 8,529,524 B2 9/2013 Newton et al.  
 D691,261 S \* 10/2013 Kawamura ..... D24/130  
 8,551,068 B2 10/2013 Kyle et al.  
 8,613,738 B2 12/2013 Mantell  
 8,641,685 B2 2/2014 Mansour et al.  
 8,679,090 B2 3/2014 Anderson et al.  
 D712,025 S \* 8/2014 Kawamura ..... D24/112  
 D714,935 S \* 10/2014 Nishioka ..... D24/130  
 8,852,167 B2 10/2014 Trombley, III et al.  
 8,870,834 B2 10/2014 Milijasevic  
 D716,636 S 11/2014 McDonald  
 D717,948 S \* 11/2014 Strong ..... D24/130  
 9,017,295 B2 4/2015 Pan  
 9,033,938 B2 5/2015 Milijasevic  
 9,073,021 B2 7/2015 Nakamura et al.  
 D736,914 S \* 8/2015 Schultz ..... D24/129  
 D736,915 S \* 8/2015 Schultz ..... D24/129  
 D737,962 S \* 9/2015 Schultz ..... D24/129  
 9,126,029 B2 9/2015 Fangrow et al.  
 9,149,623 B1 10/2015 Colman  
 9,289,587 B2 3/2016 Colman  
 D756,200 S 5/2016 McDonald  
 9,427,715 B2 8/2016 Palazzolo et al.  
 9,433,562 B2 9/2016 Ingram et al.  
 2005/0209555 A1 9/2005 Middleton et al.  
 2006/0217679 A1 9/2006 Hanly et al.  
 2007/0076401 A1 4/2007 Carrez et al.  
 2008/0183153 A1 7/2008 Enns

2008/0312640 A1 12/2008 Grant  
 2010/0022951 A1 1/2010 Ferrera et al.  
 2011/0112543 A1 5/2011 Palazzolo et al.  
 2014/0020788 A1 1/2014 Kyle et al.  
 2014/0246616 A1 9/2014 Fangrow  
 2014/0276466 A1 9/2014 Yeh et al.  
 2014/0276651 A1 9/2014 Schultz  
 2014/0323995 A1 10/2014 Clauson et al.  
 2016/0001056 A1 1/2016 Nelson et al.  
 2016/0030293 A1 2/2016 Dorsey et al.  
 2016/0067422 A1 3/2016 Davis et al.  
 2016/0067471 A1 3/2016 Ingram et al.  
 2016/0143815 A1 5/2016 Koelper et al.  
 2016/0159635 A1 6/2016 Davis et al.  
 2016/0206845 A1 7/2016 Colman et al.  
 2016/0367439 A1 12/2016 Davis et al.  
 2017/0239141 A1 8/2017 Davis et al.

FOREIGN PATENT DOCUMENTS


DE 20302788 U1 6/2004  
 DE 102005030510 A1 1/2007  
 EP 0960616 A2 12/1999  
 EP 2269685 A2 1/2011  
 EP 3042691 A1 7/2016  
 FR 2930428 A1 10/2009  
 JP 4743229 B2 8/2011  
 WO 9200717 A1 1/1992  
 WO 9932155 A2 7/1999  
 WO 2005065767 A2 7/2005  
 WO 2009090627 A1 7/2009  
 WO 2013081699 A2 6/2013  
 WO 2015034045 A1 3/2015  
 WO 2016089869 A1 6/2016

OTHER PUBLICATIONS


Specialty Medical Products Coupling (Item Code SMP-SCFF); Apr. 10, 2014; 1 pg.  
 Alternative Syringes Low Displacement Option PowerPoint Presentation; Presented by Rork Swisher of Covidien; ISO 80369 Series Meeting; Berlin Germany; 11 pgs; Mar. 19, 2014.pgs.  
 International Search Report & Written Opinion for PCT/US2016/023771; dated Jun. 27, 2016; 17 pgs.  
 International Search Report & Written Opinion for PCT/US2016/038051; dated Sep. 2, 2016; 13 pgs.  
 International Search Report & Written Opinion for PCT/US2016/042514; Nov. 10, 2016; 12 pgs.  
 International Search Report & Written Opinion for PCT/US2017/019021; dated Sep. 22, 2017; 20 pgs.  
 Invitation to Pay Additional Fees for PCT/US2017/019021; Jun. 6, 2017; 12 pgs.  
 New ISO Tubing Connector Standards: A Follow-Up to the Sentinel Event Alert Webinar PowerPoint Presentation; www.jointcommission.org; 50 pgs; Dec. 3, 2014.  
 New Tube Feeding Connectors Webinar PowerPoint Presentation; www.oley.org; 24 pgs; Jun. 24, 2014.

\* cited by examiner




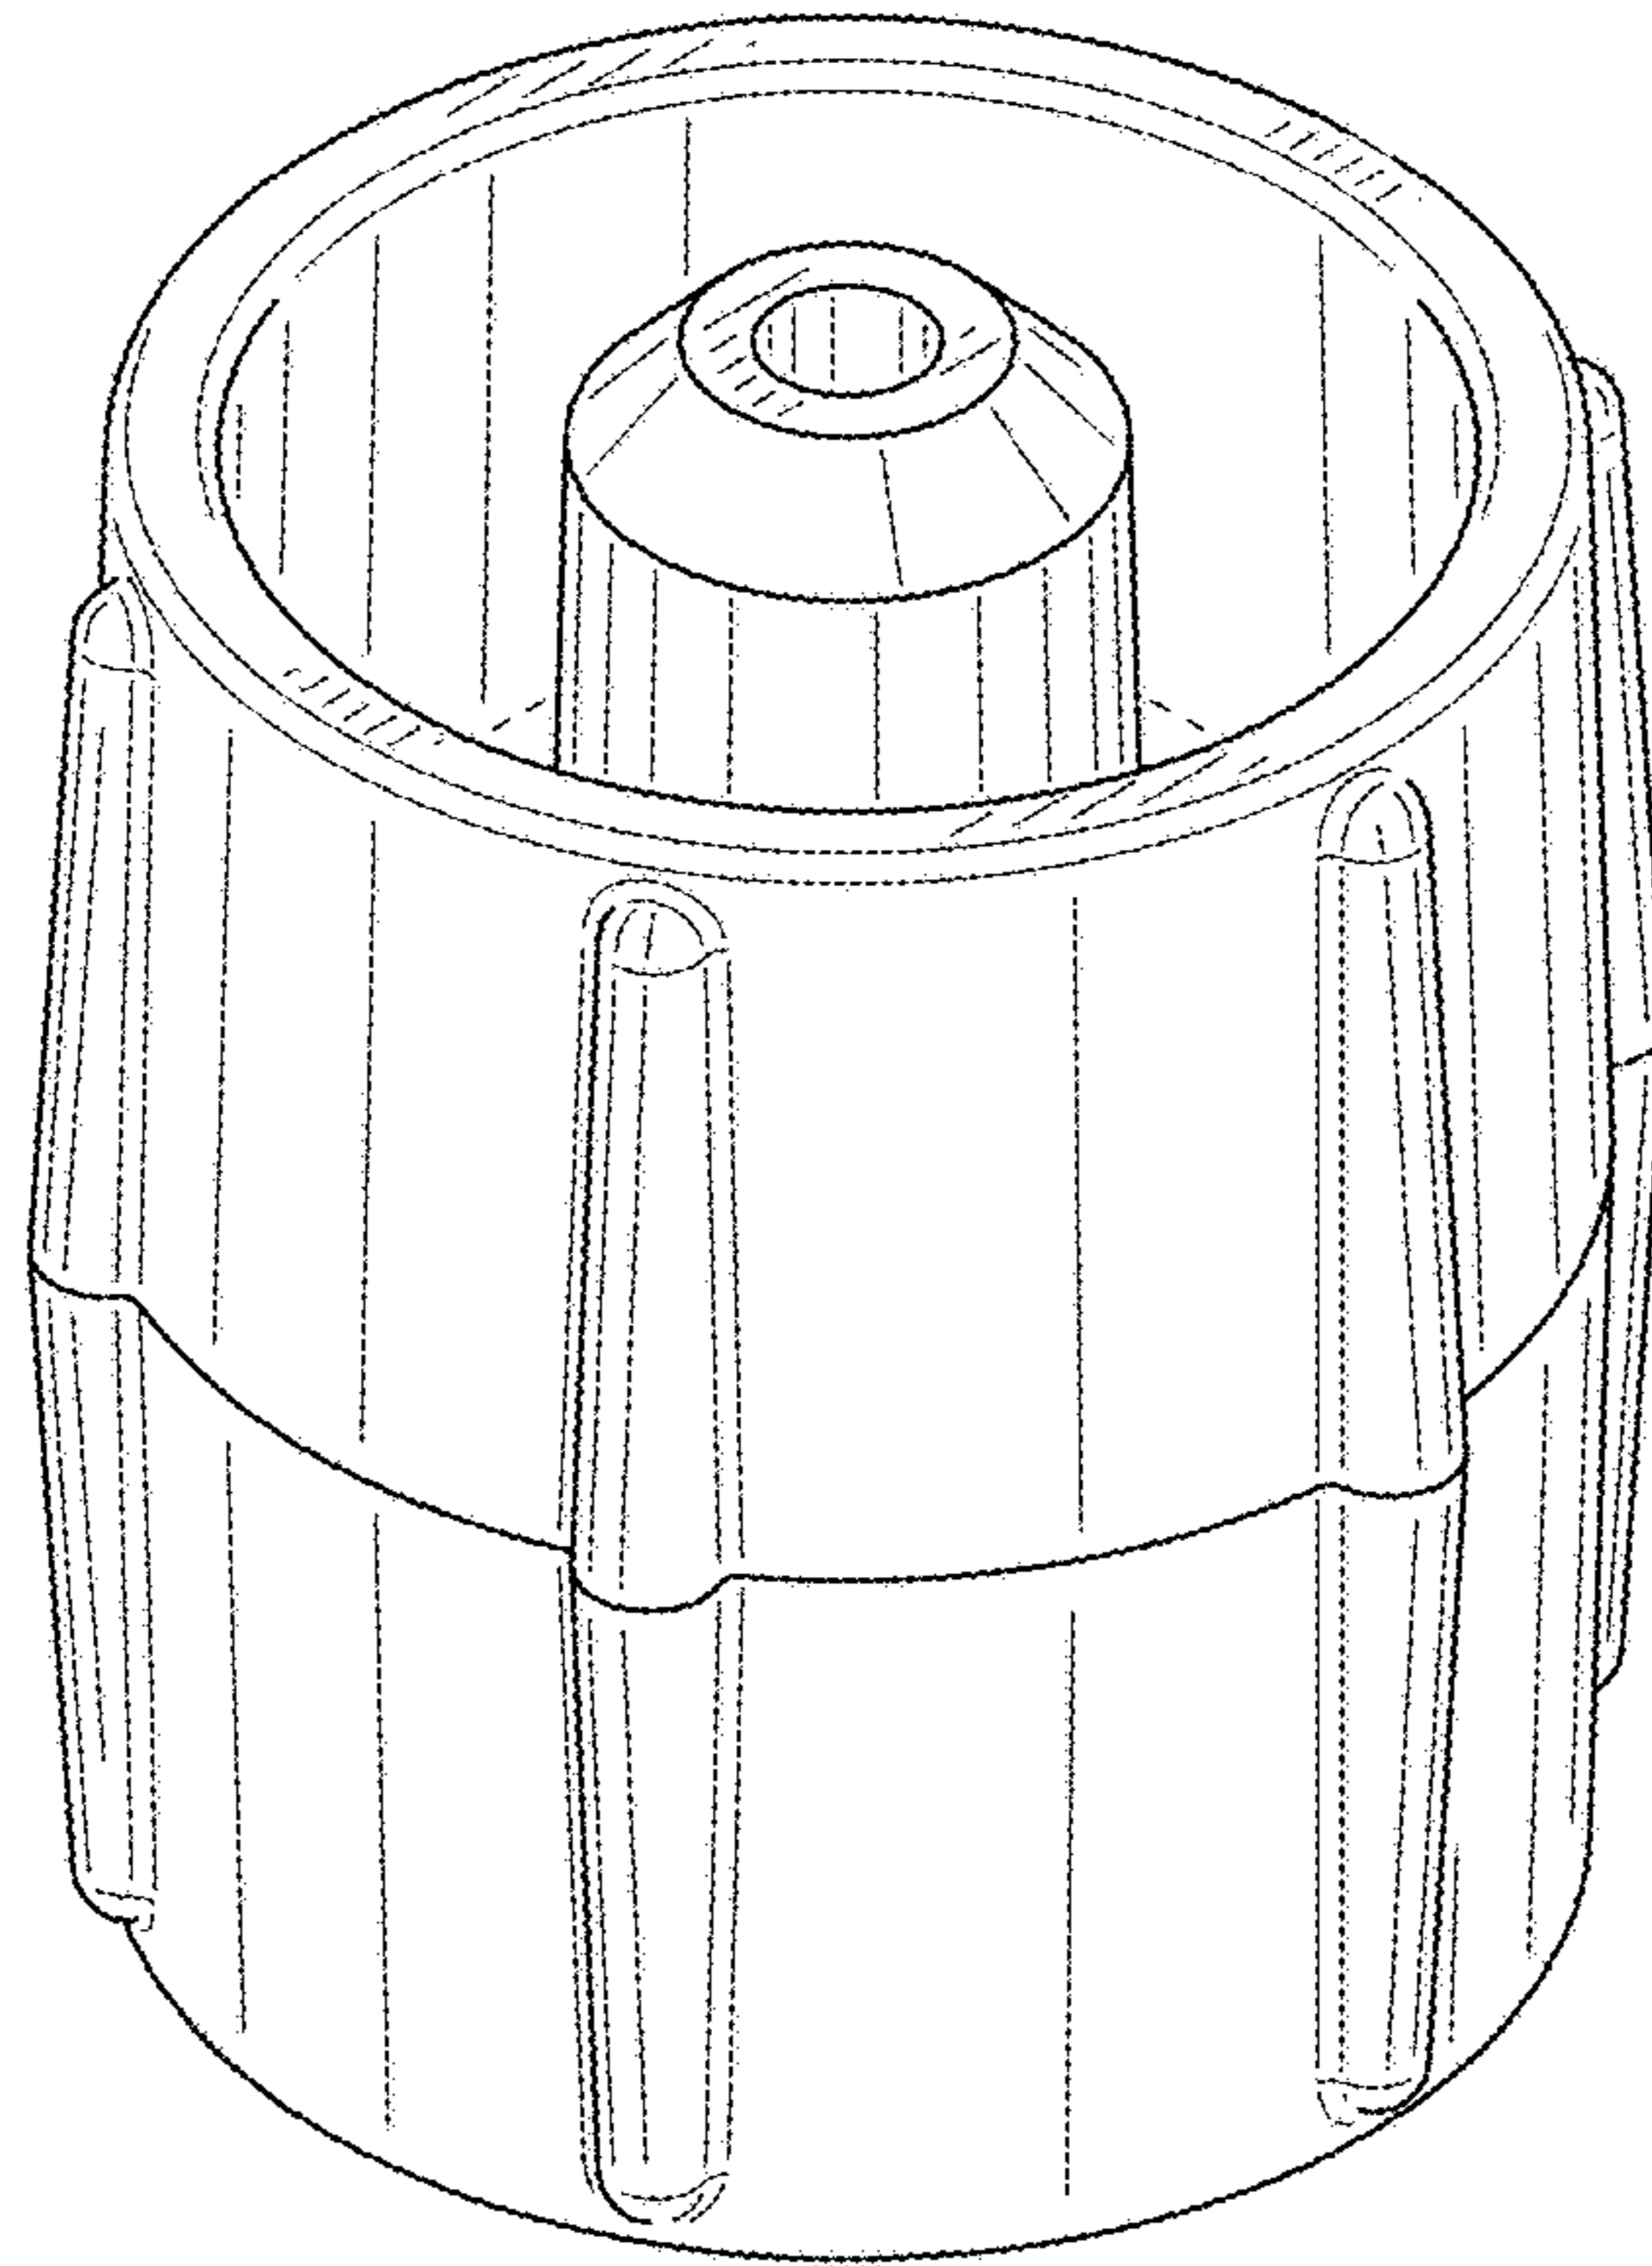


*FIG. 1*

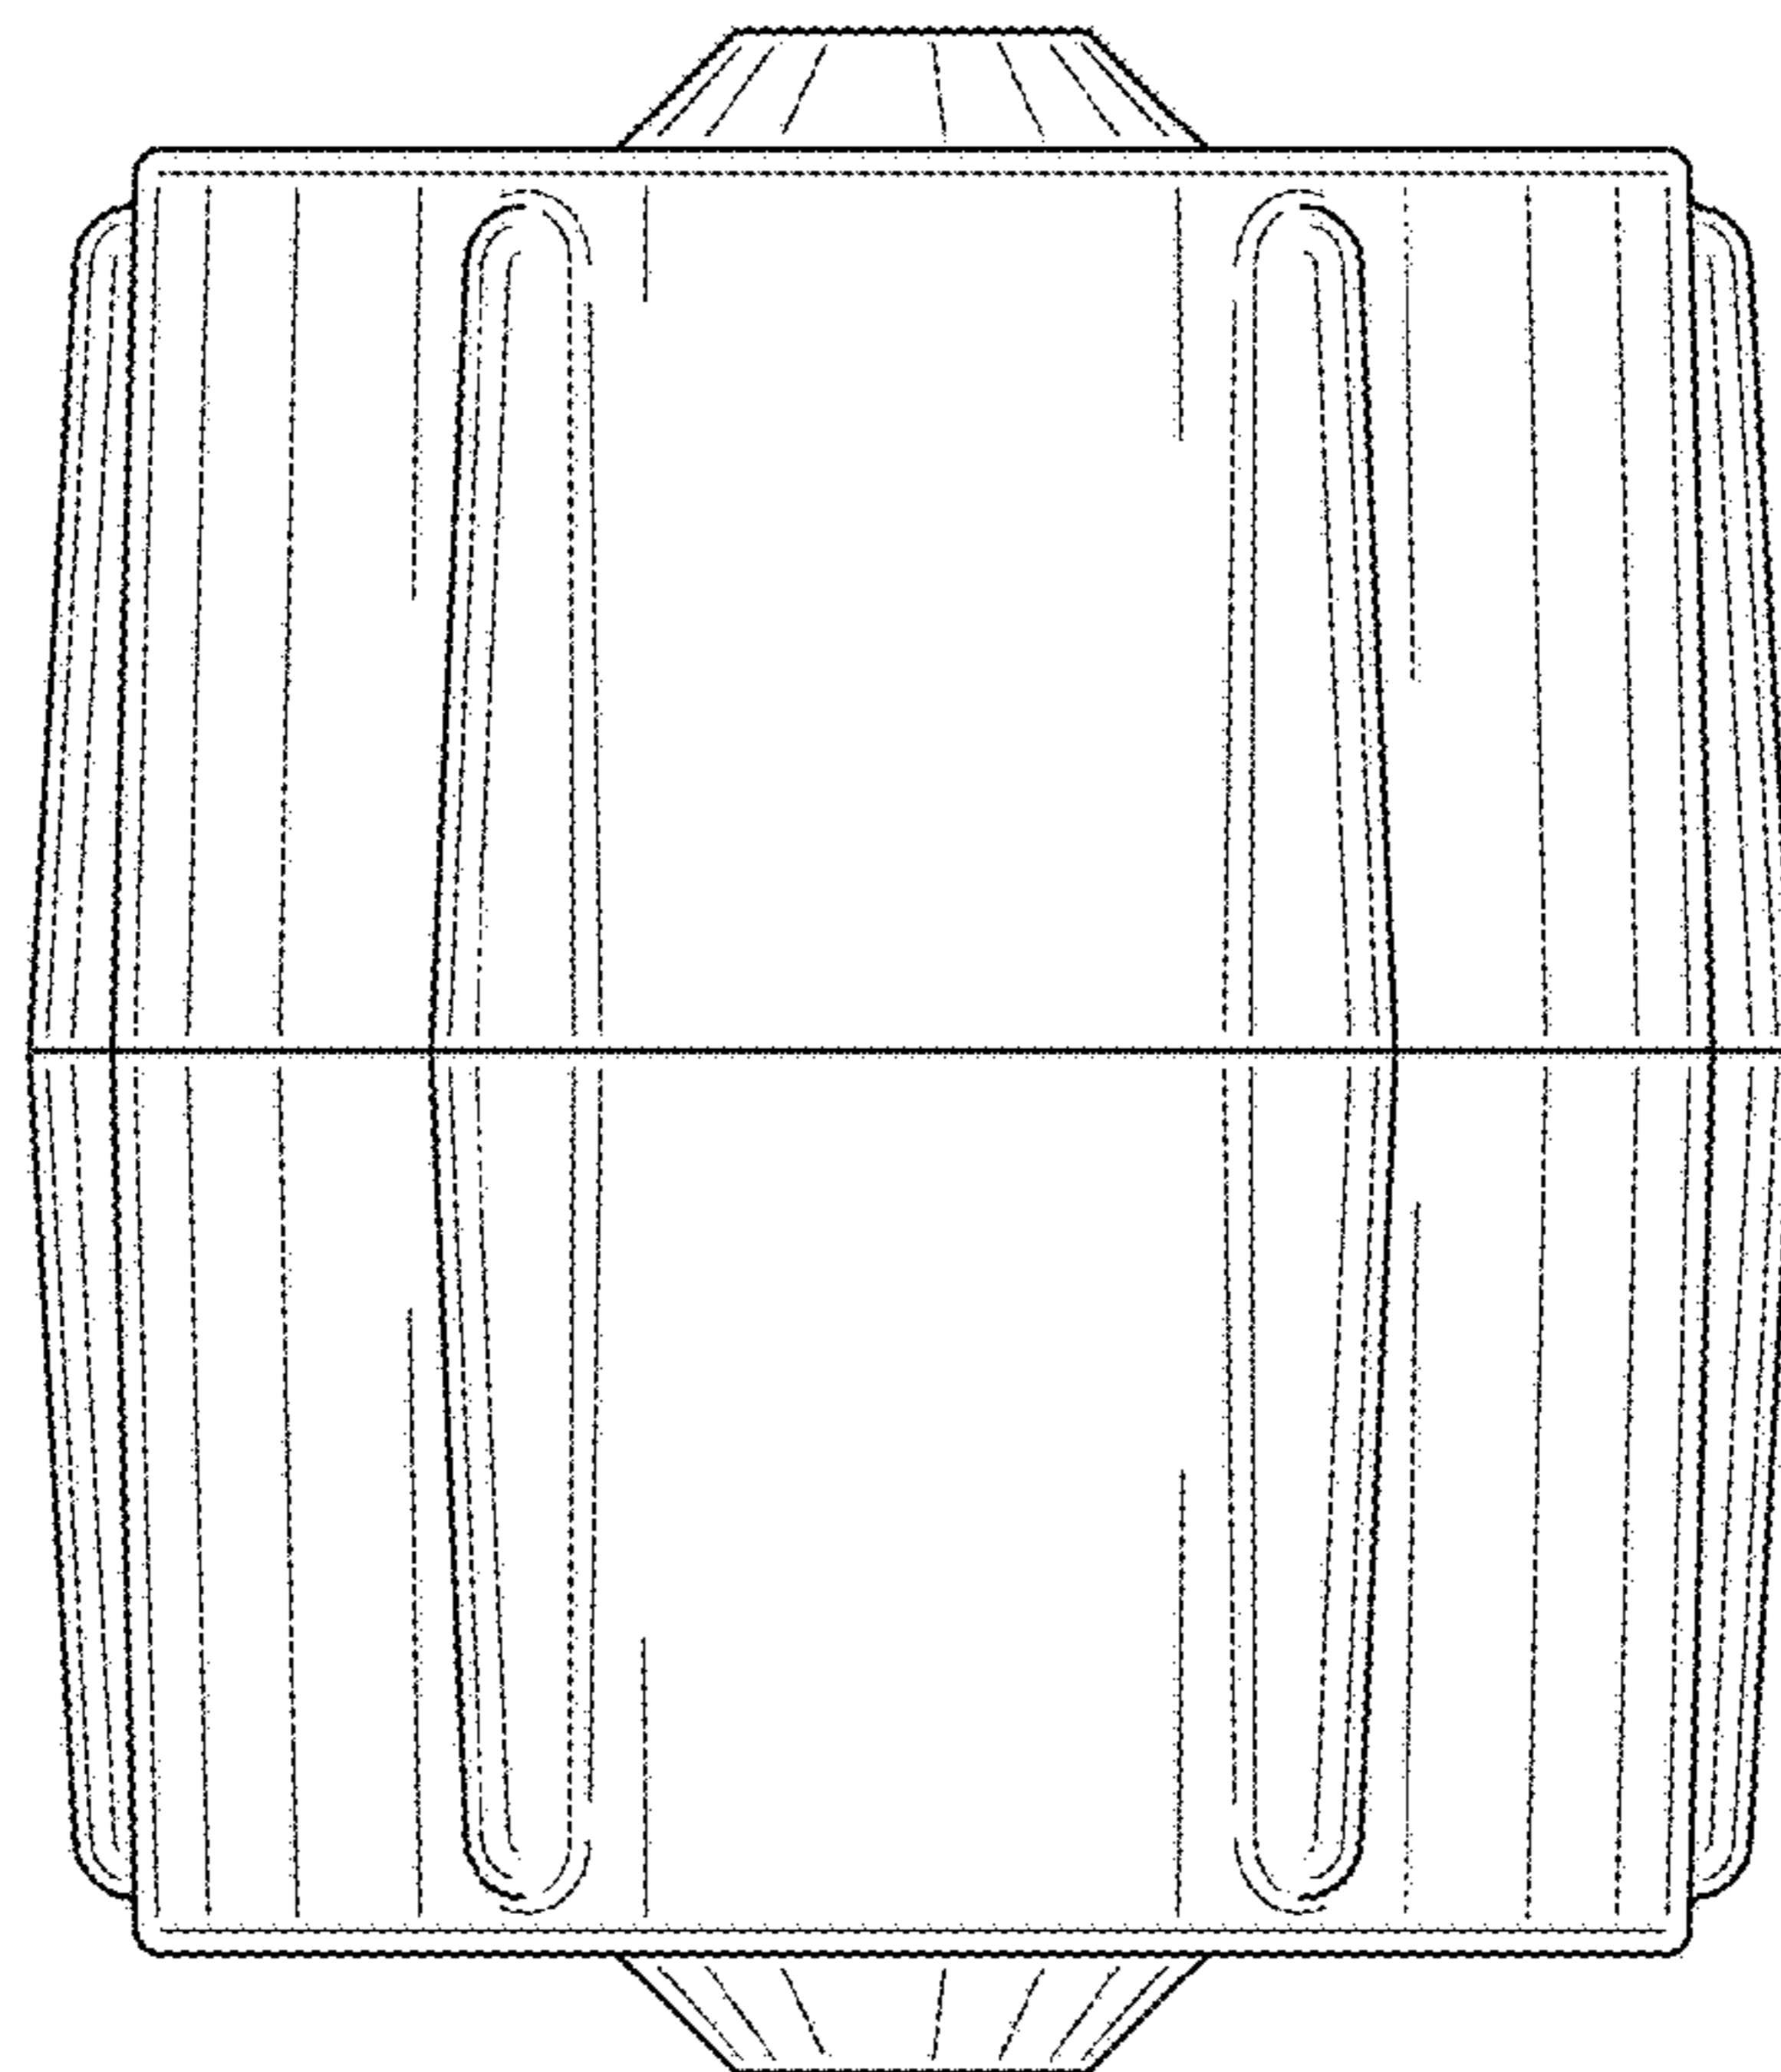

*FIG. 2*

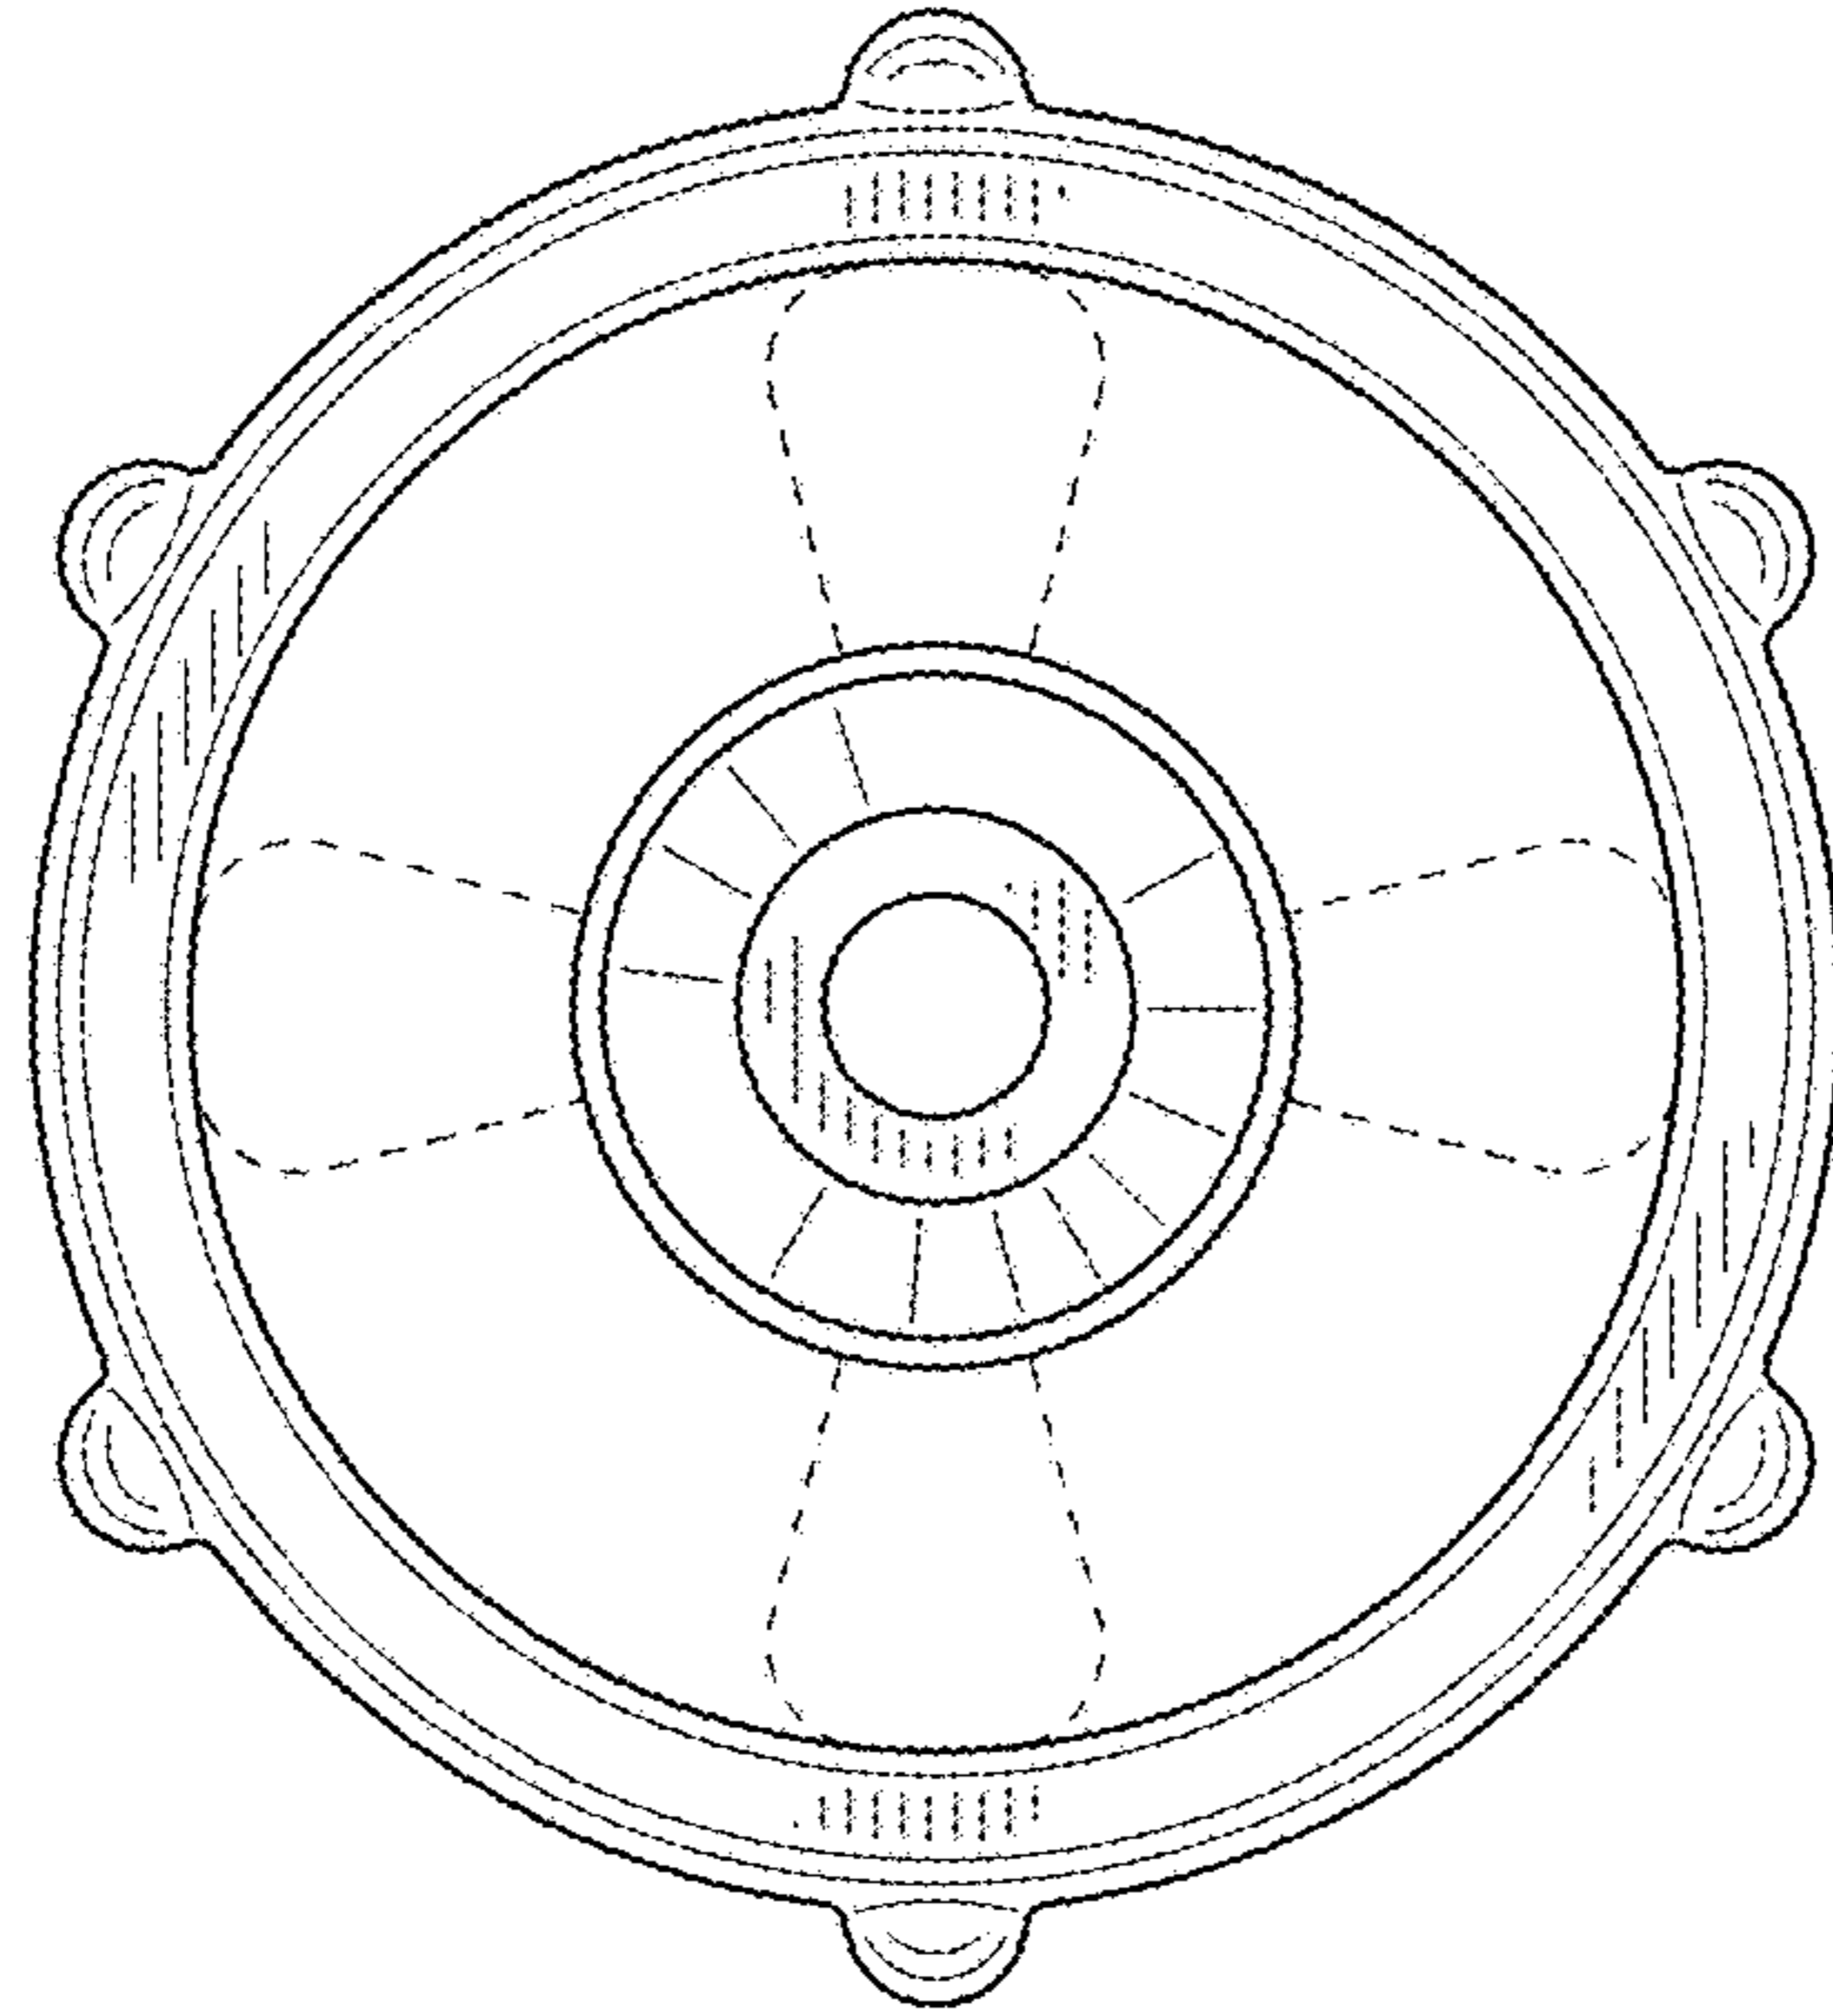

*FIG. 3*

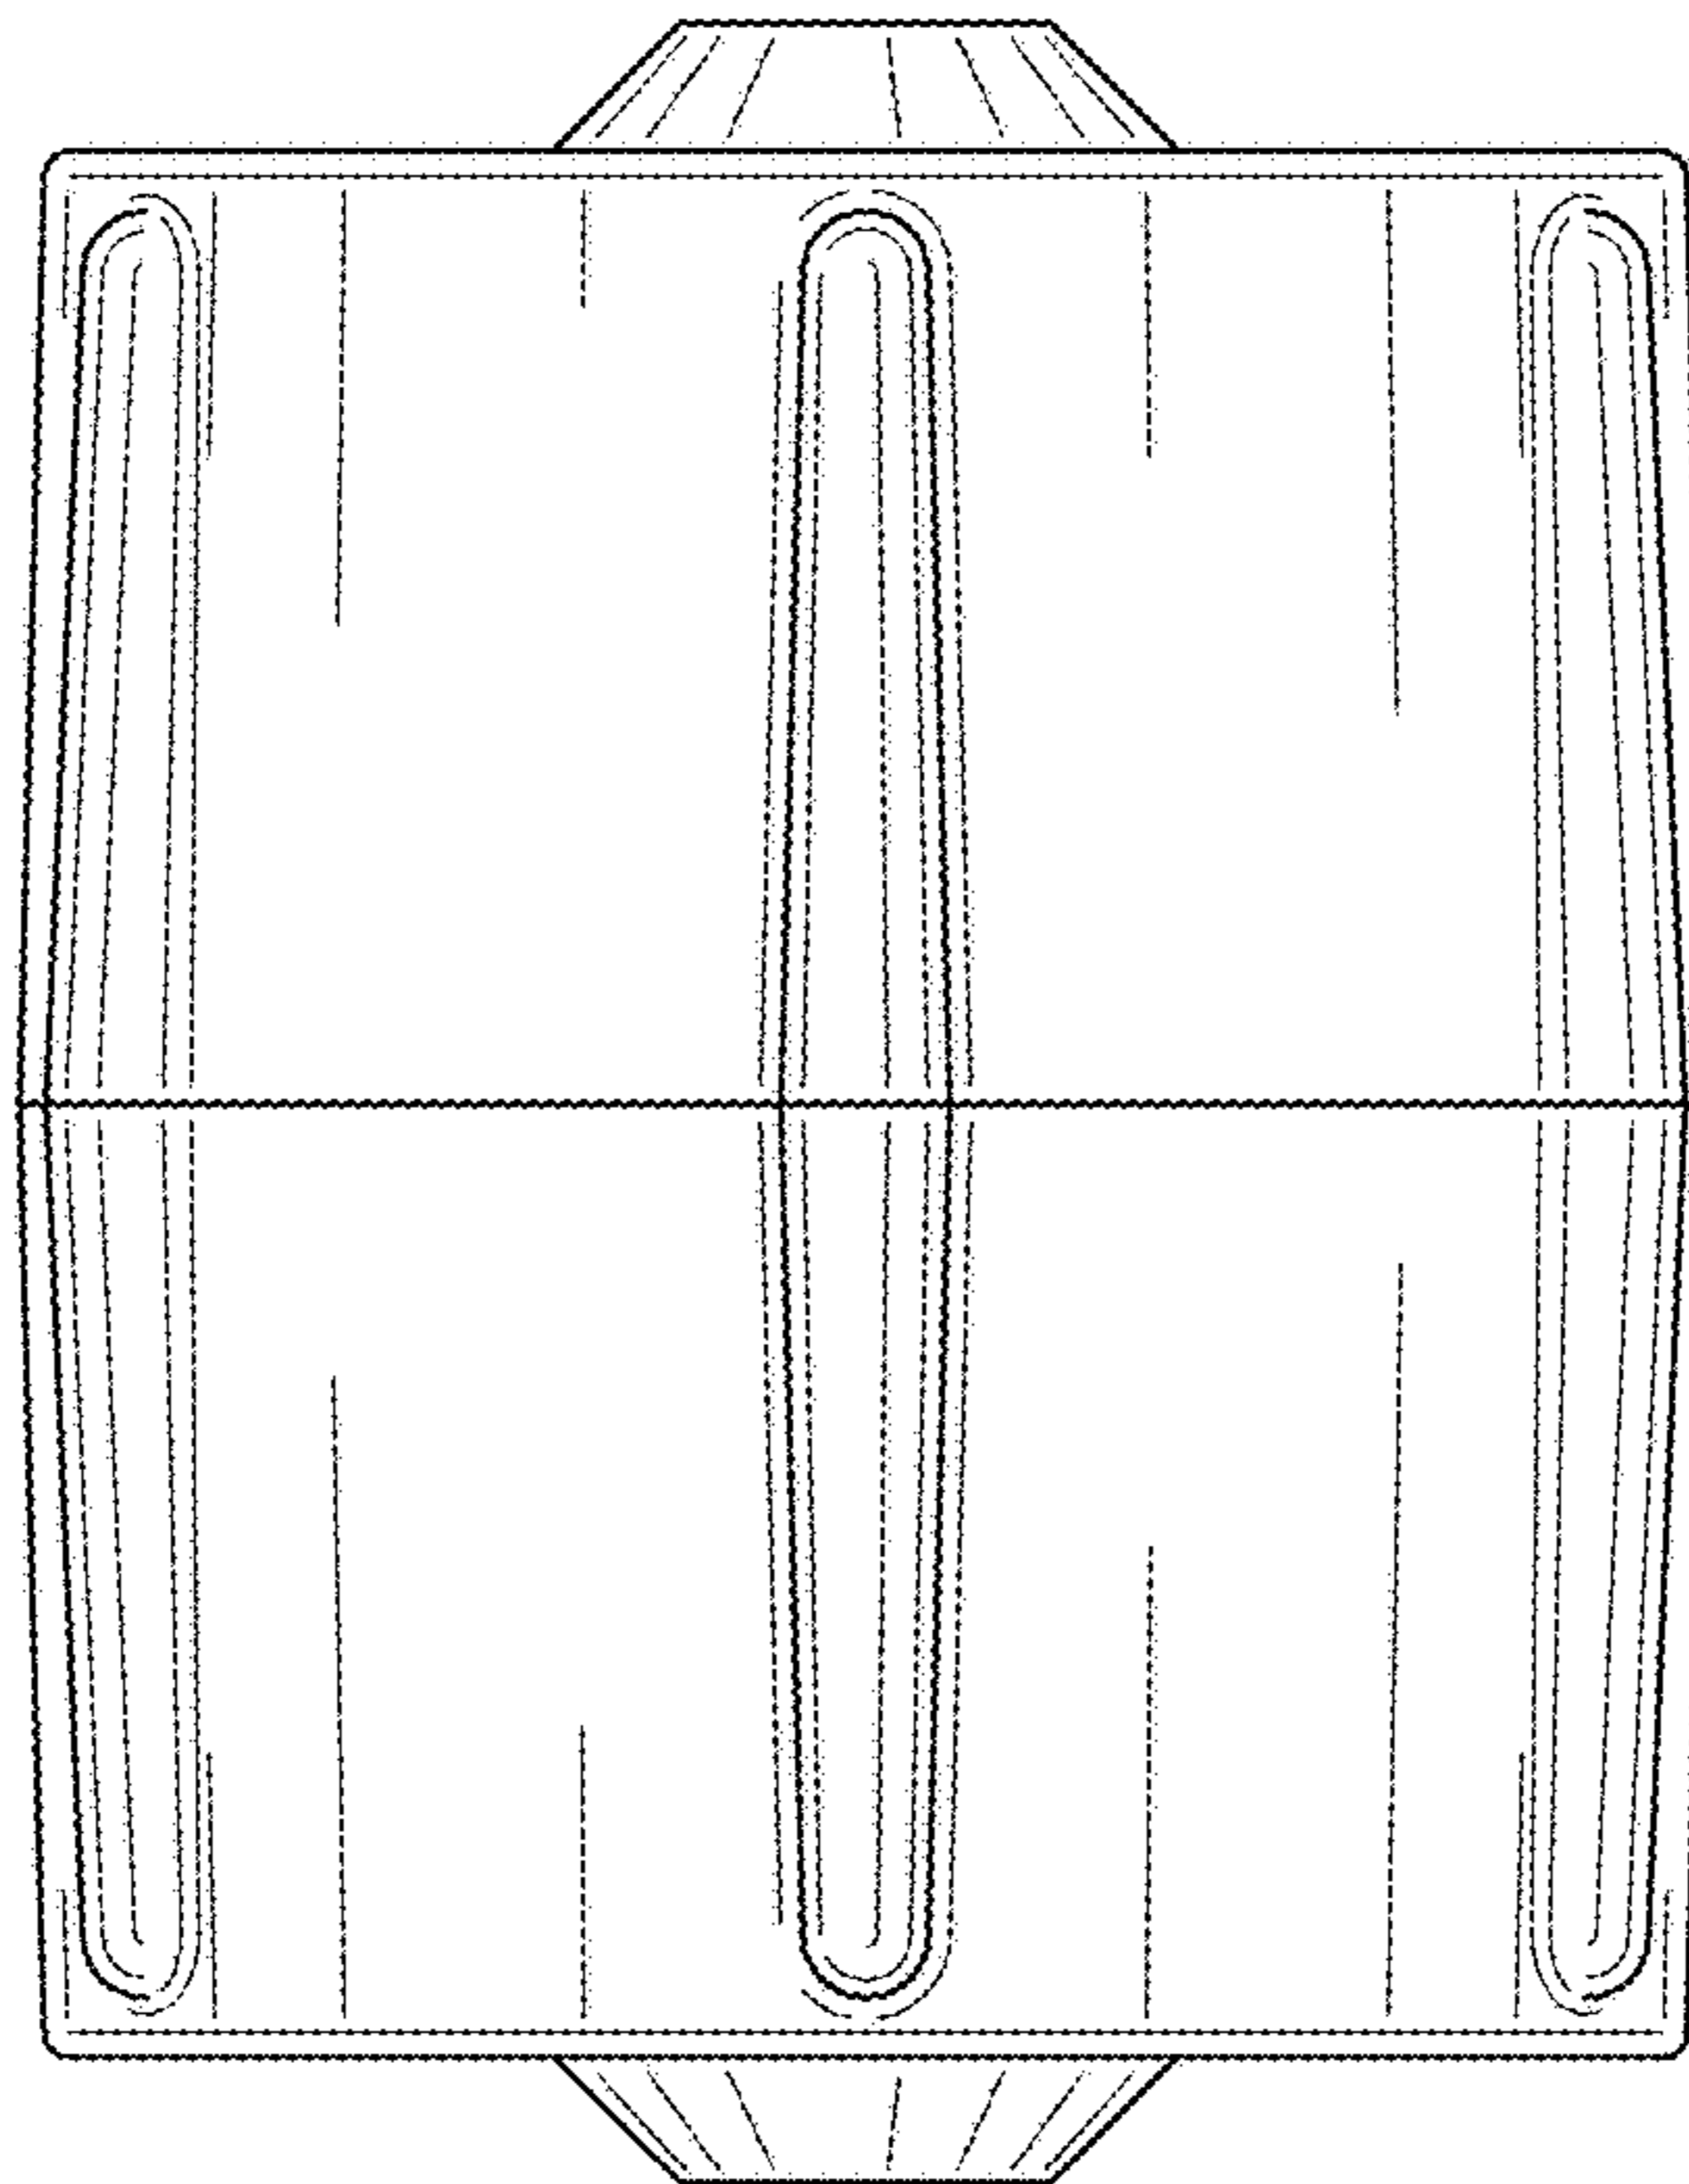

*FIG. 4*

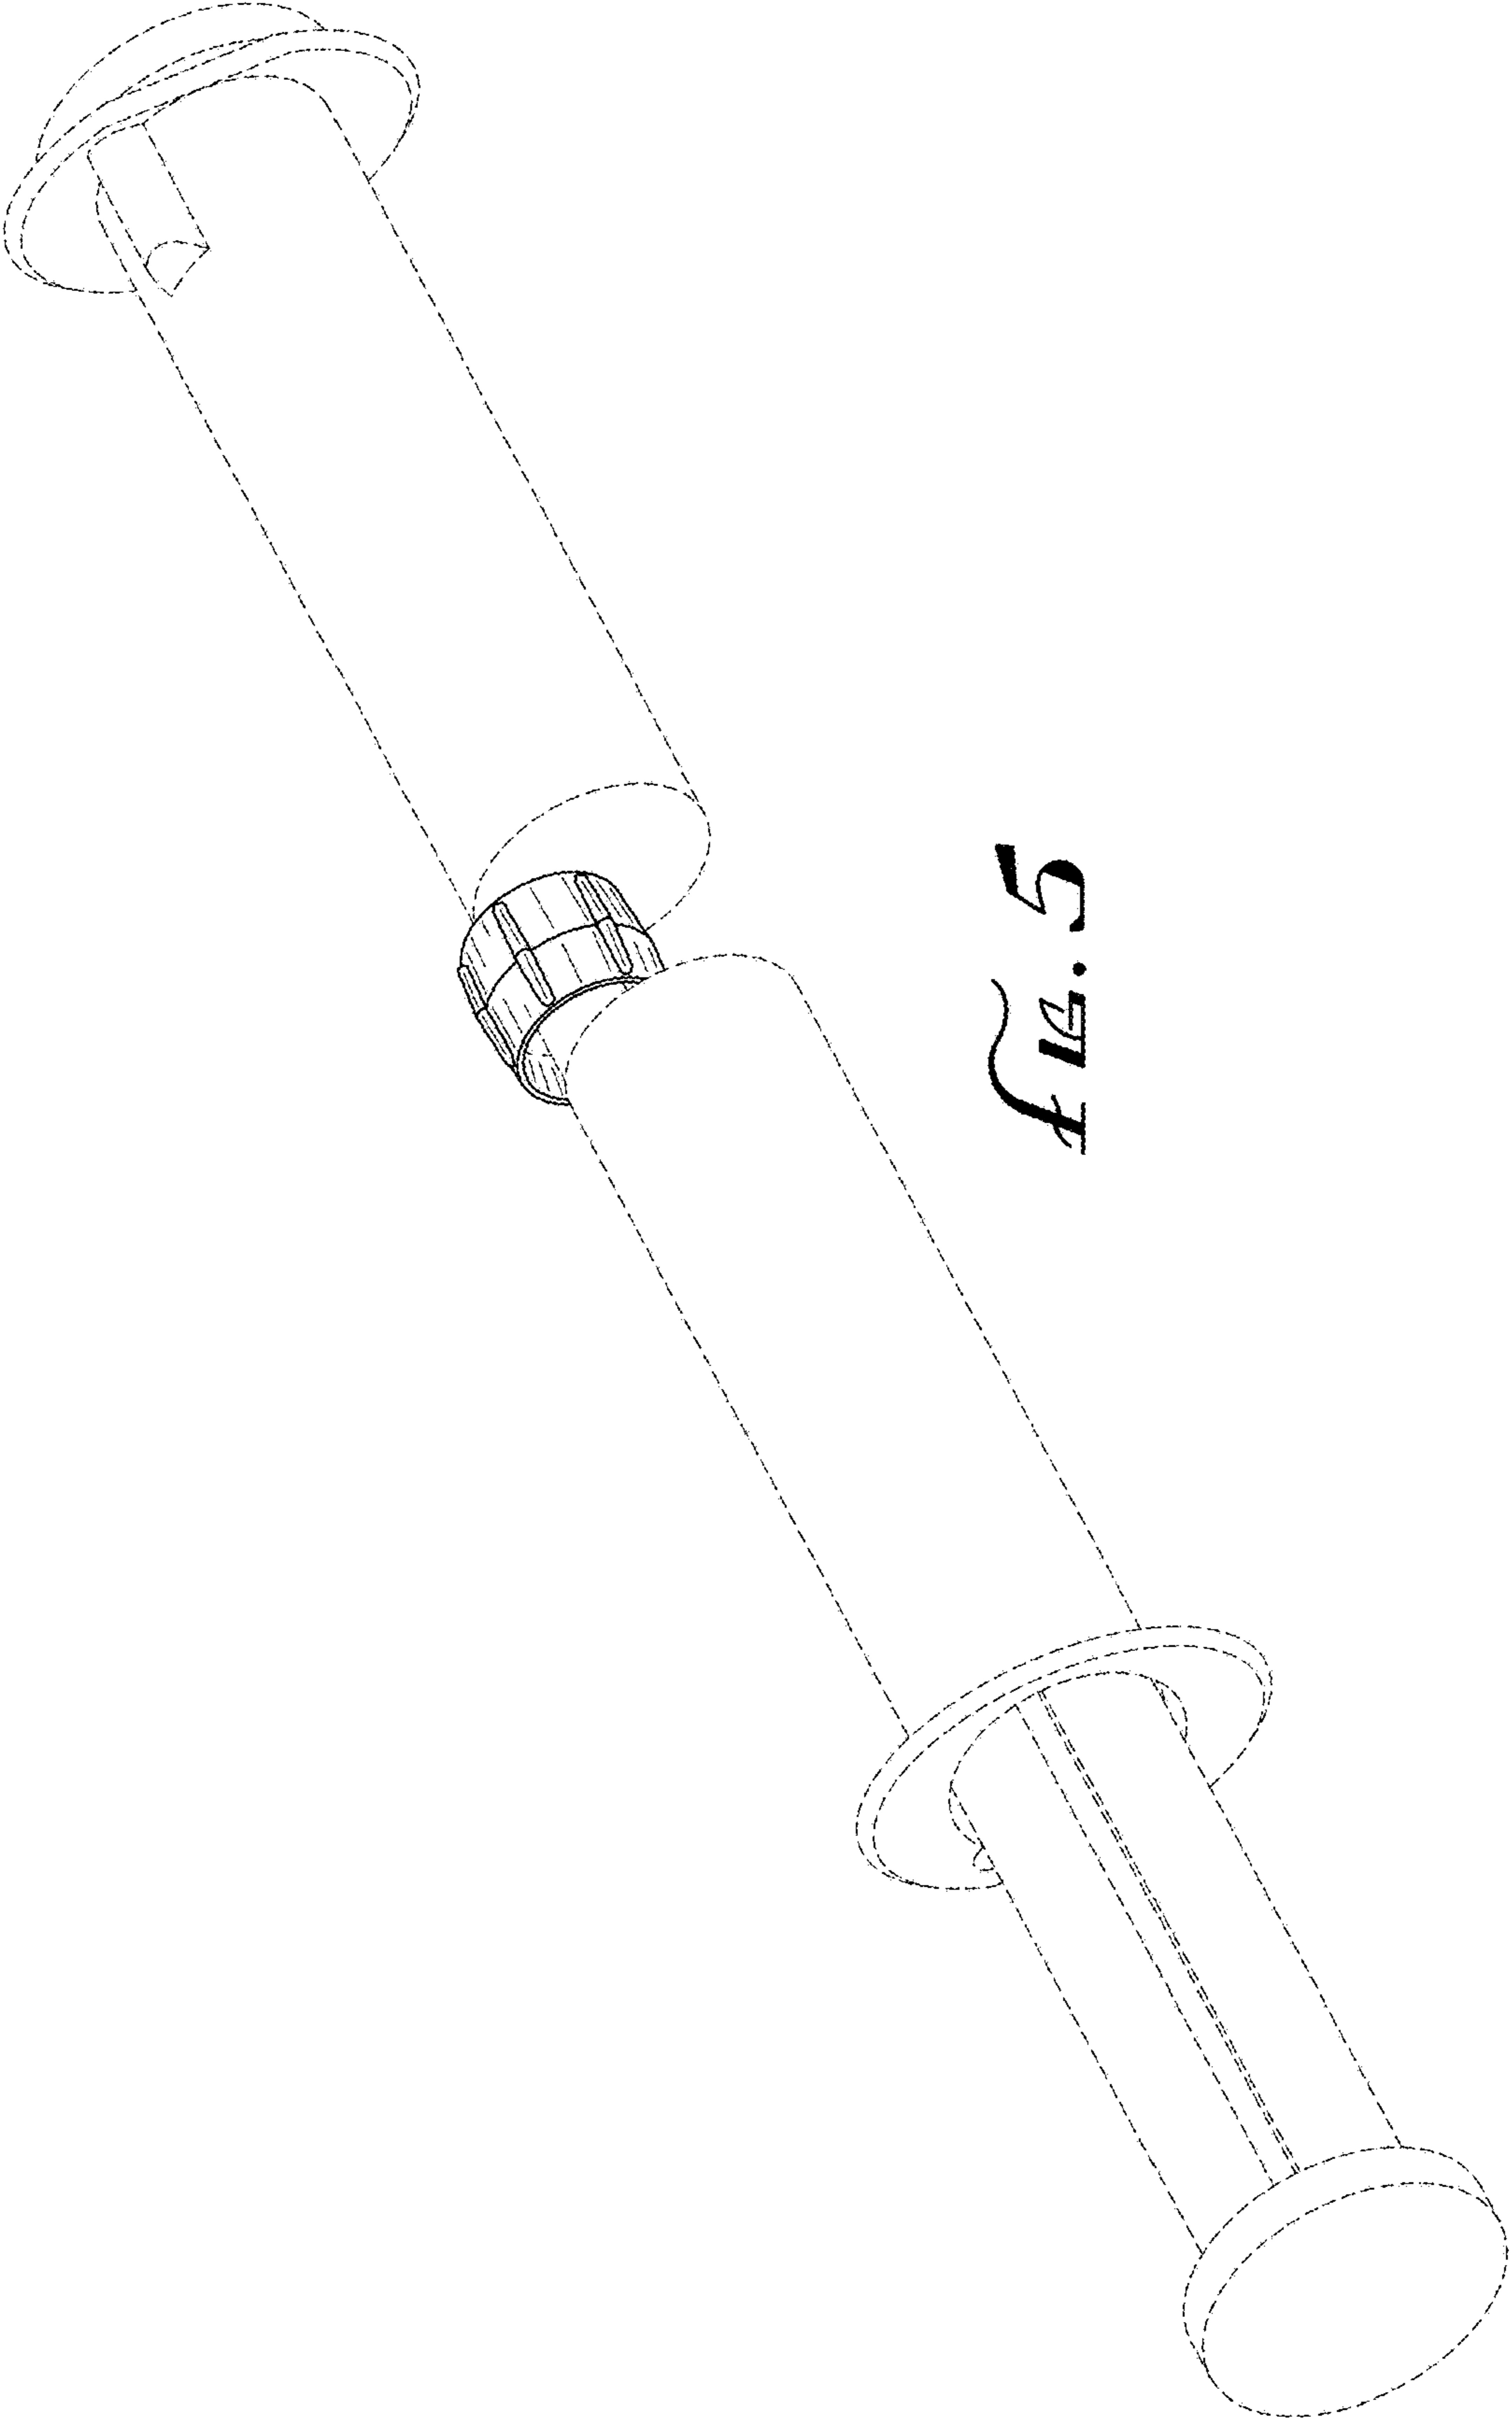


FIG. 5