



US00D827141S

(12) **United States Design Patent** (10) **Patent No.:** **US D827,141 S**
Pichette (45) **Date of Patent:** **** Aug. 28, 2018**

- (54) **ORTHOPEdic POST PAD**
- (71) Applicant: **Timothy Kelley Pichette**, Nashville, TN (US)
- (72) Inventor: **Timothy Kelley Pichette**, Nashville, TN (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/599,399**
- (22) Filed: **Apr. 3, 2017**
- (51) **LOC (11) Cl.** **24-04**
- (52) **U.S. Cl.**
USPC **D24/184**
- (58) **Field of Classification Search**
USPC D24/183, 184, 190, 191, 192;
D29/101.3, 120.1, 121.1, 121.2, 122;
D6/382, 383, 384, 406.1-406.6, 596, 601,
D6/604, 610, 611, 710, 712, 716.2, 716.4,
D6/716.6, 718, 718.3; D2/720, 826, 860,
D2/861
CPC A61G 1/003-1/013; A61G 1/04-1/052;
A61G 7/1036; A61G 7/1053-7/1057;
A61G 13/00; A47C 20/021-20/027; A47C
7/18; A47C 7/50
See application file for complete search history.

- 2009/0151076 A1* 6/2009 Cararra A47G 9/10
5/636
- 2010/0043147 A1* 2/2010 Popp A47D 13/083
5/636
- 2010/0275378 A1* 11/2010 Xiao A47G 9/1045
5/639

OTHER PUBLICATIONS

OR Specialty Products American Surgical Specialties Company.
[online] Retrieved Jun. 11, 2018 from URL: <http://www.americansurg.com/or-specialty-products.html>.*

Carson Perineal Post Pad—Patient Positioning Solutions, Inc.
[online] Retrieved Jun. 11, 2018 from URL: <https://pps-products.com/orthopedic-surgery-disposables/carson-perineal-post-pad/>.*

* cited by examiner

Primary Examiner — Vy N Koenig
(74) *Attorney, Agent, or Firm* — Michael A. Blake

(57) **CLAIM**

The ornamental design for an orthopedic post pad, as shown and described.

DESCRIPTION


FIG. 1 is a perspective view of an orthopedic post pad showing my new design;
FIG. 2 is a front elevation view of the orthopedic post pad;
FIG. 3 is a rear elevation view of the orthopedic post pad;
FIG. 4 is a top view of the orthopedic post pad; and,
FIG. 5 is a perspective view of the orthopedic post pad in a configuration of use, inserted between the legs of a patient about to have an arthroscopic procedure.
The broken lines in FIG. 5 represent environmental subject matter, specifically the patient and distraction and positioning system in a configuration of use, and form no part of the claimed design.

1 Claim, 5 Drawing Sheets

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D456,516 S * 4/2002 Chshaek 5/638
- D469,541 S * 1/2003 Cheatham D24/191
- 7,100,641 B2 * 9/2006 Tyrer F16L 1/123
138/110
- D641,859 S * 7/2011 van Walraven D23/393
- D675,881 S * 2/2013 Wamack, Jr. D7/608
- D743,557 S * 11/2015 Pichette D24/184
- D769,079 S * 10/2016 Kotani D7/608
- D815,460 S * 4/2018 Beyda D6/601

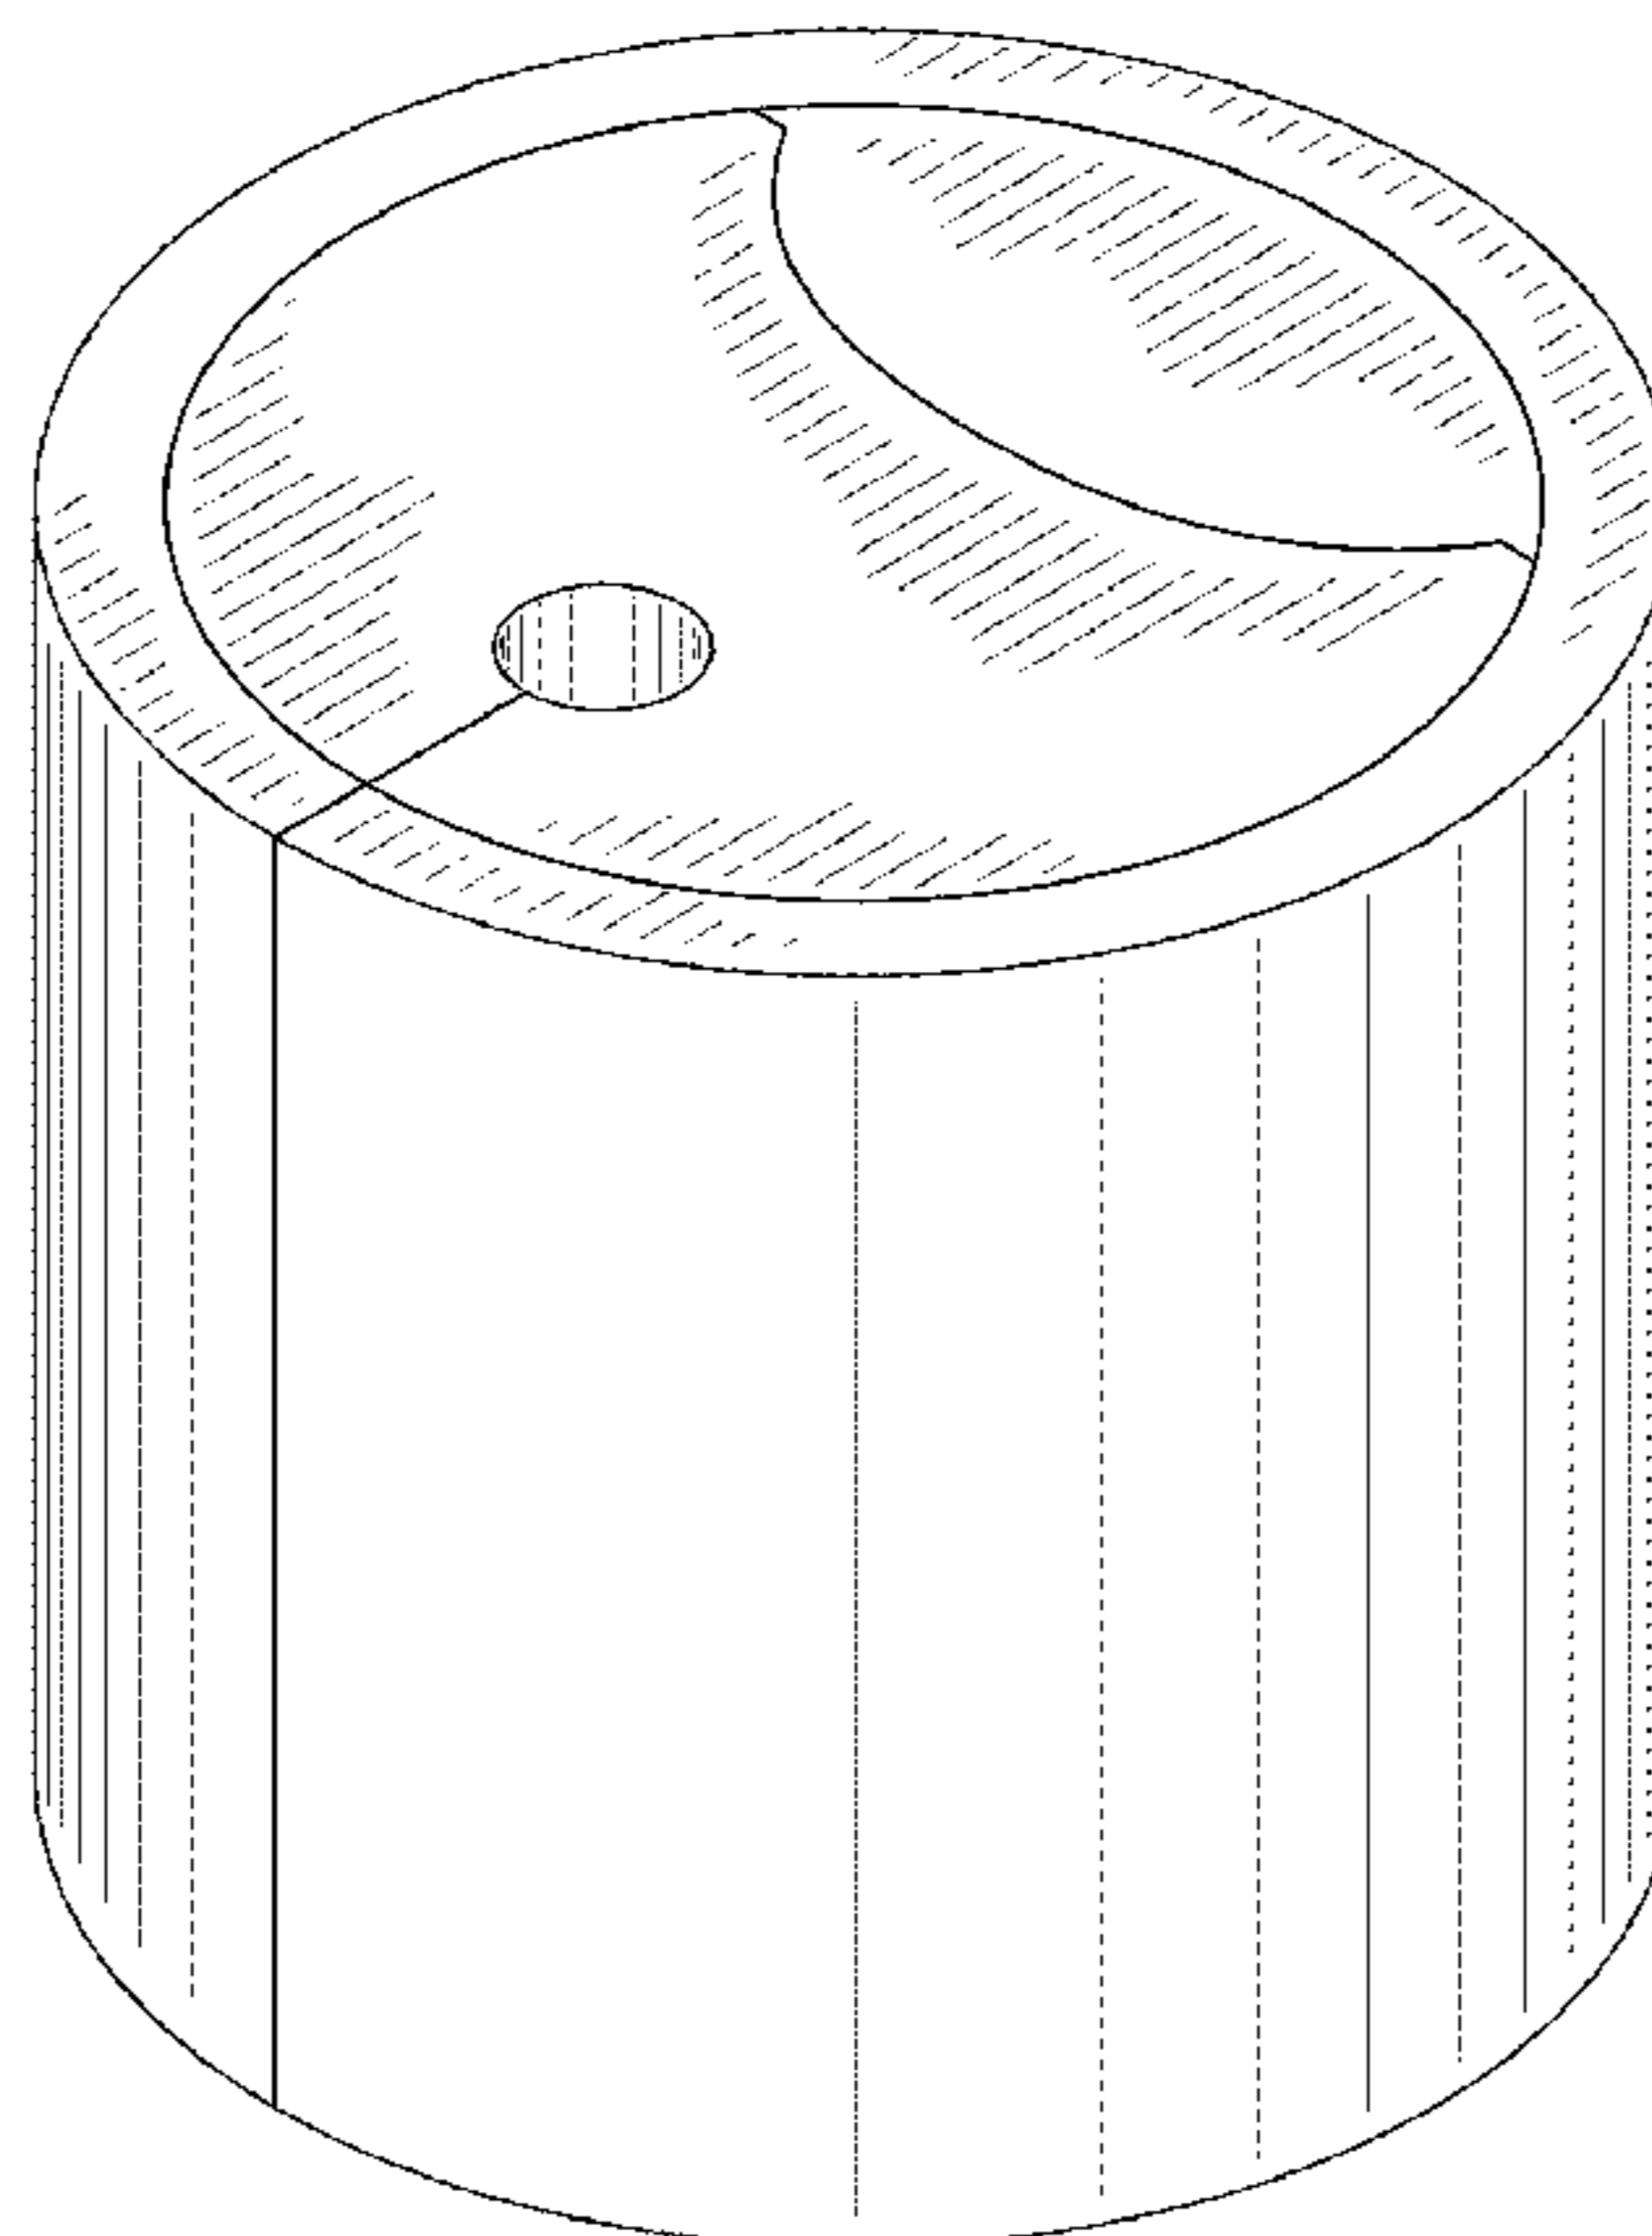

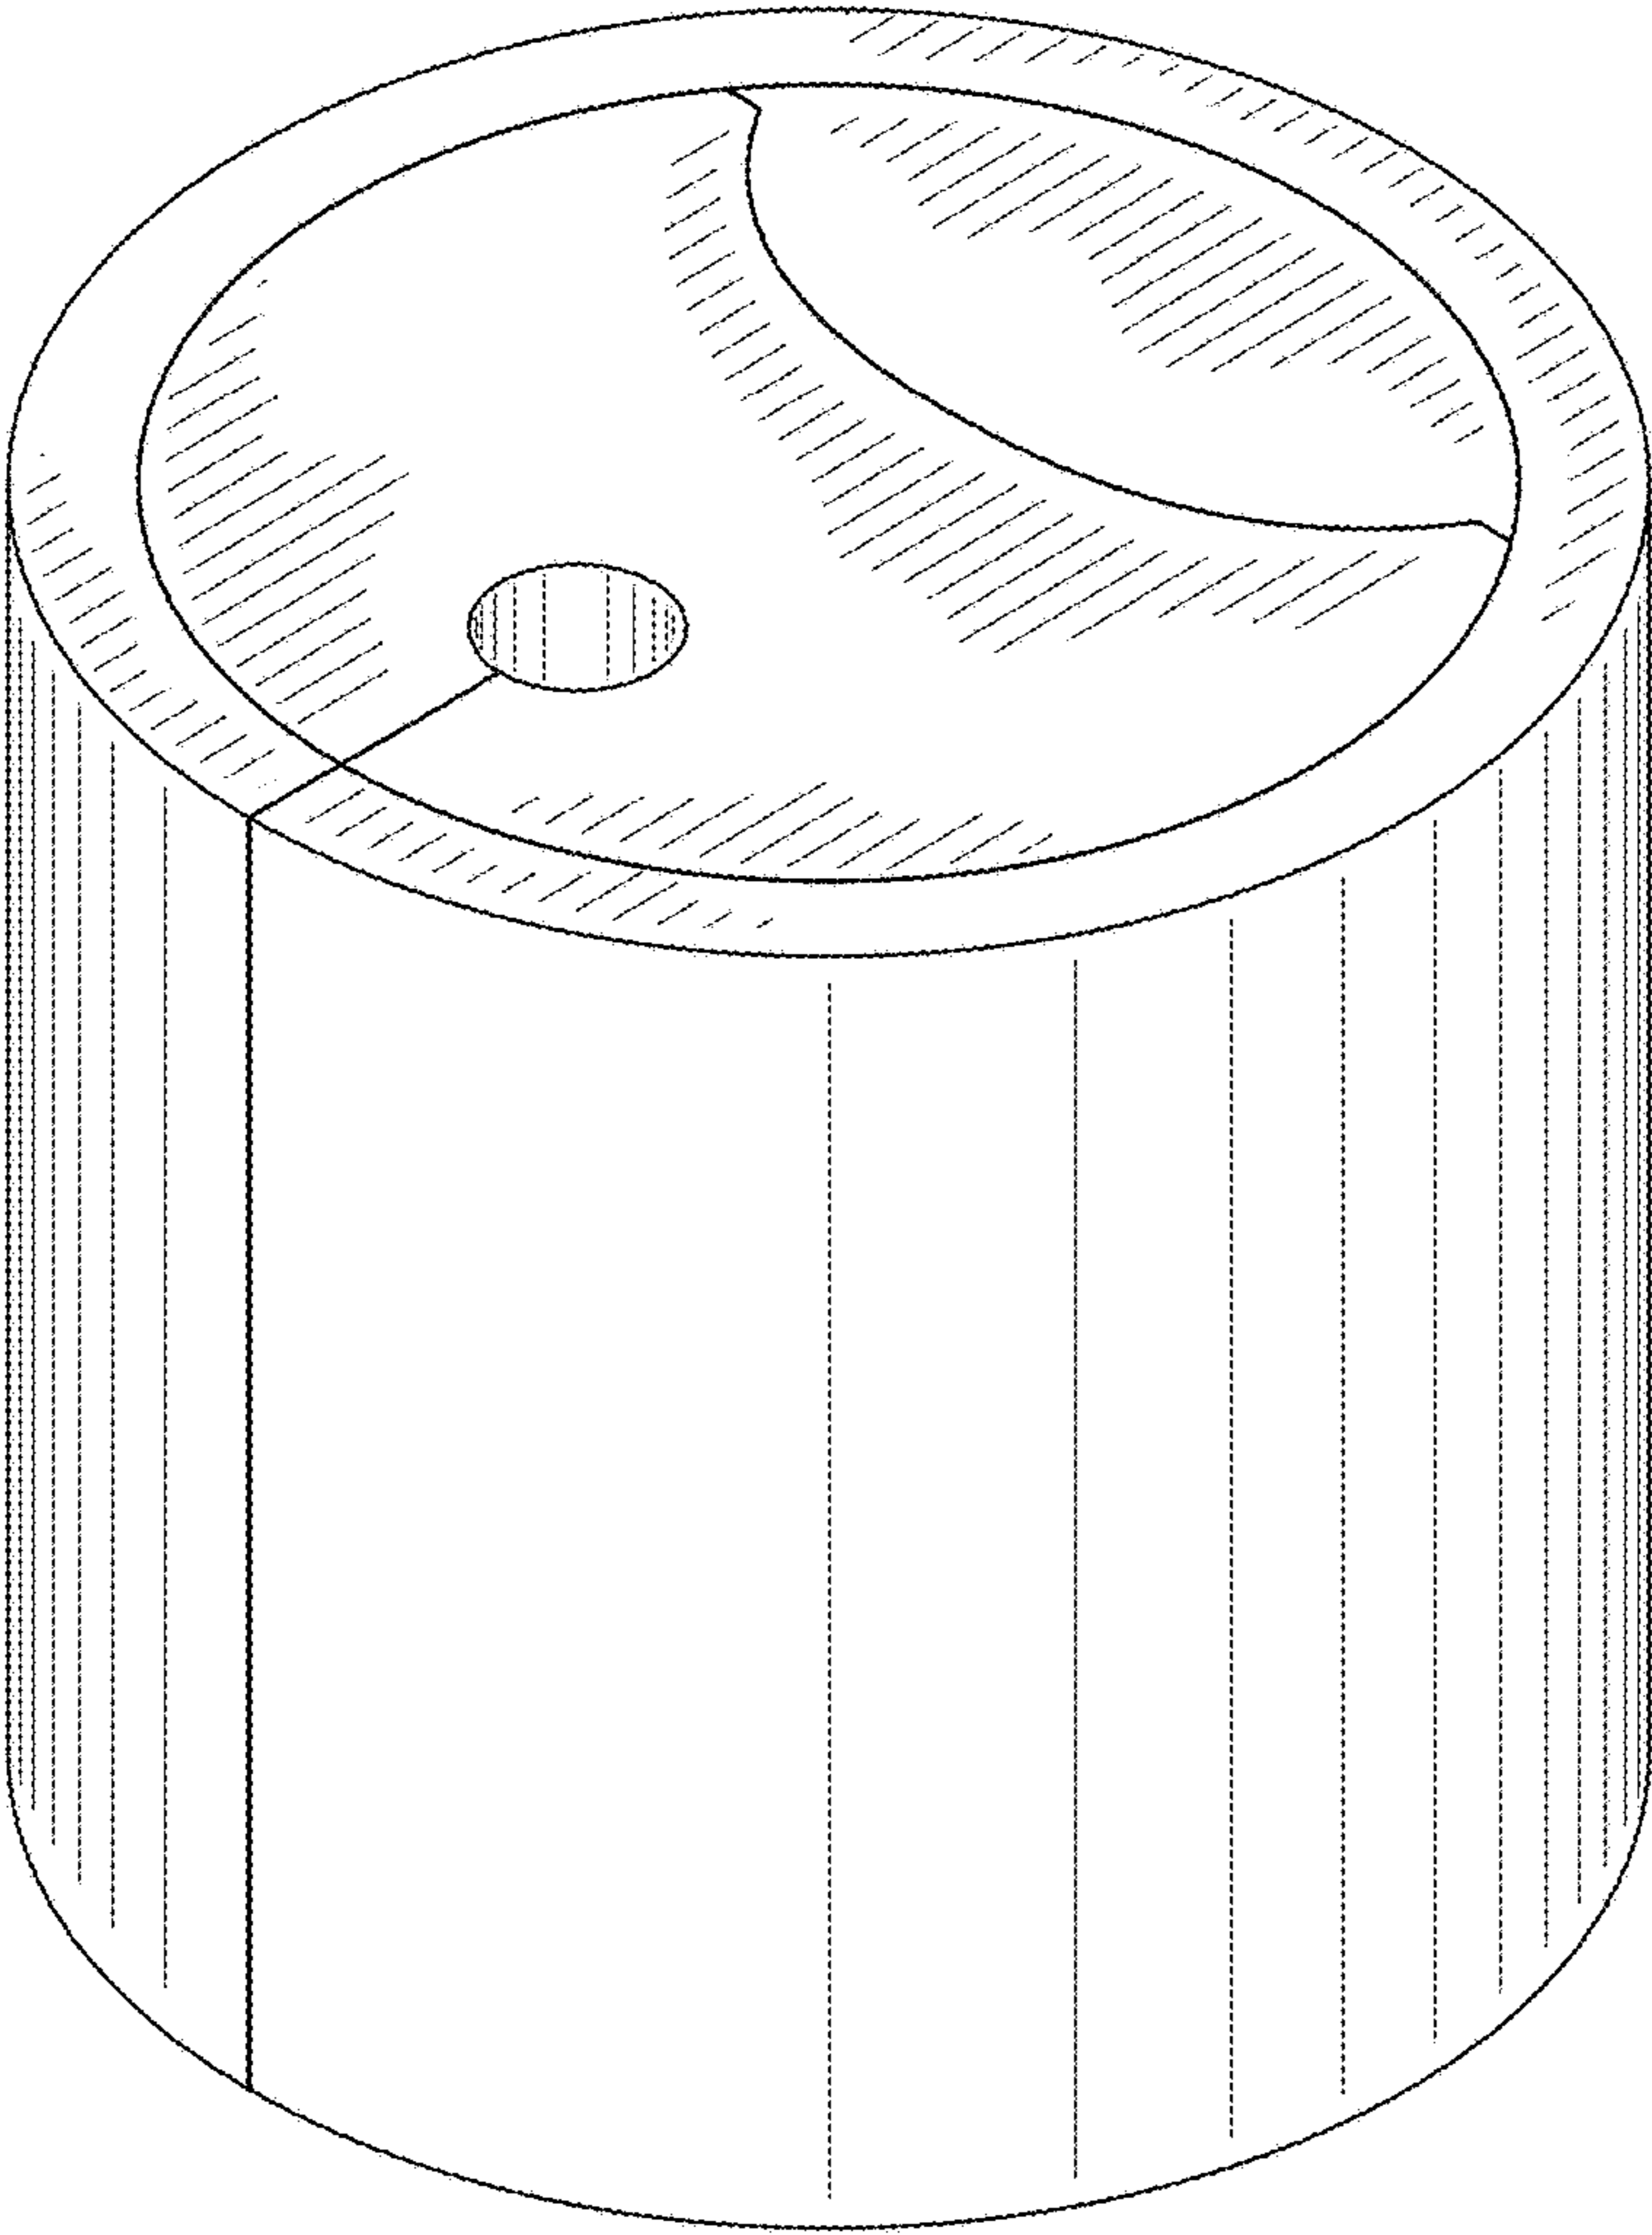


FIG. 1

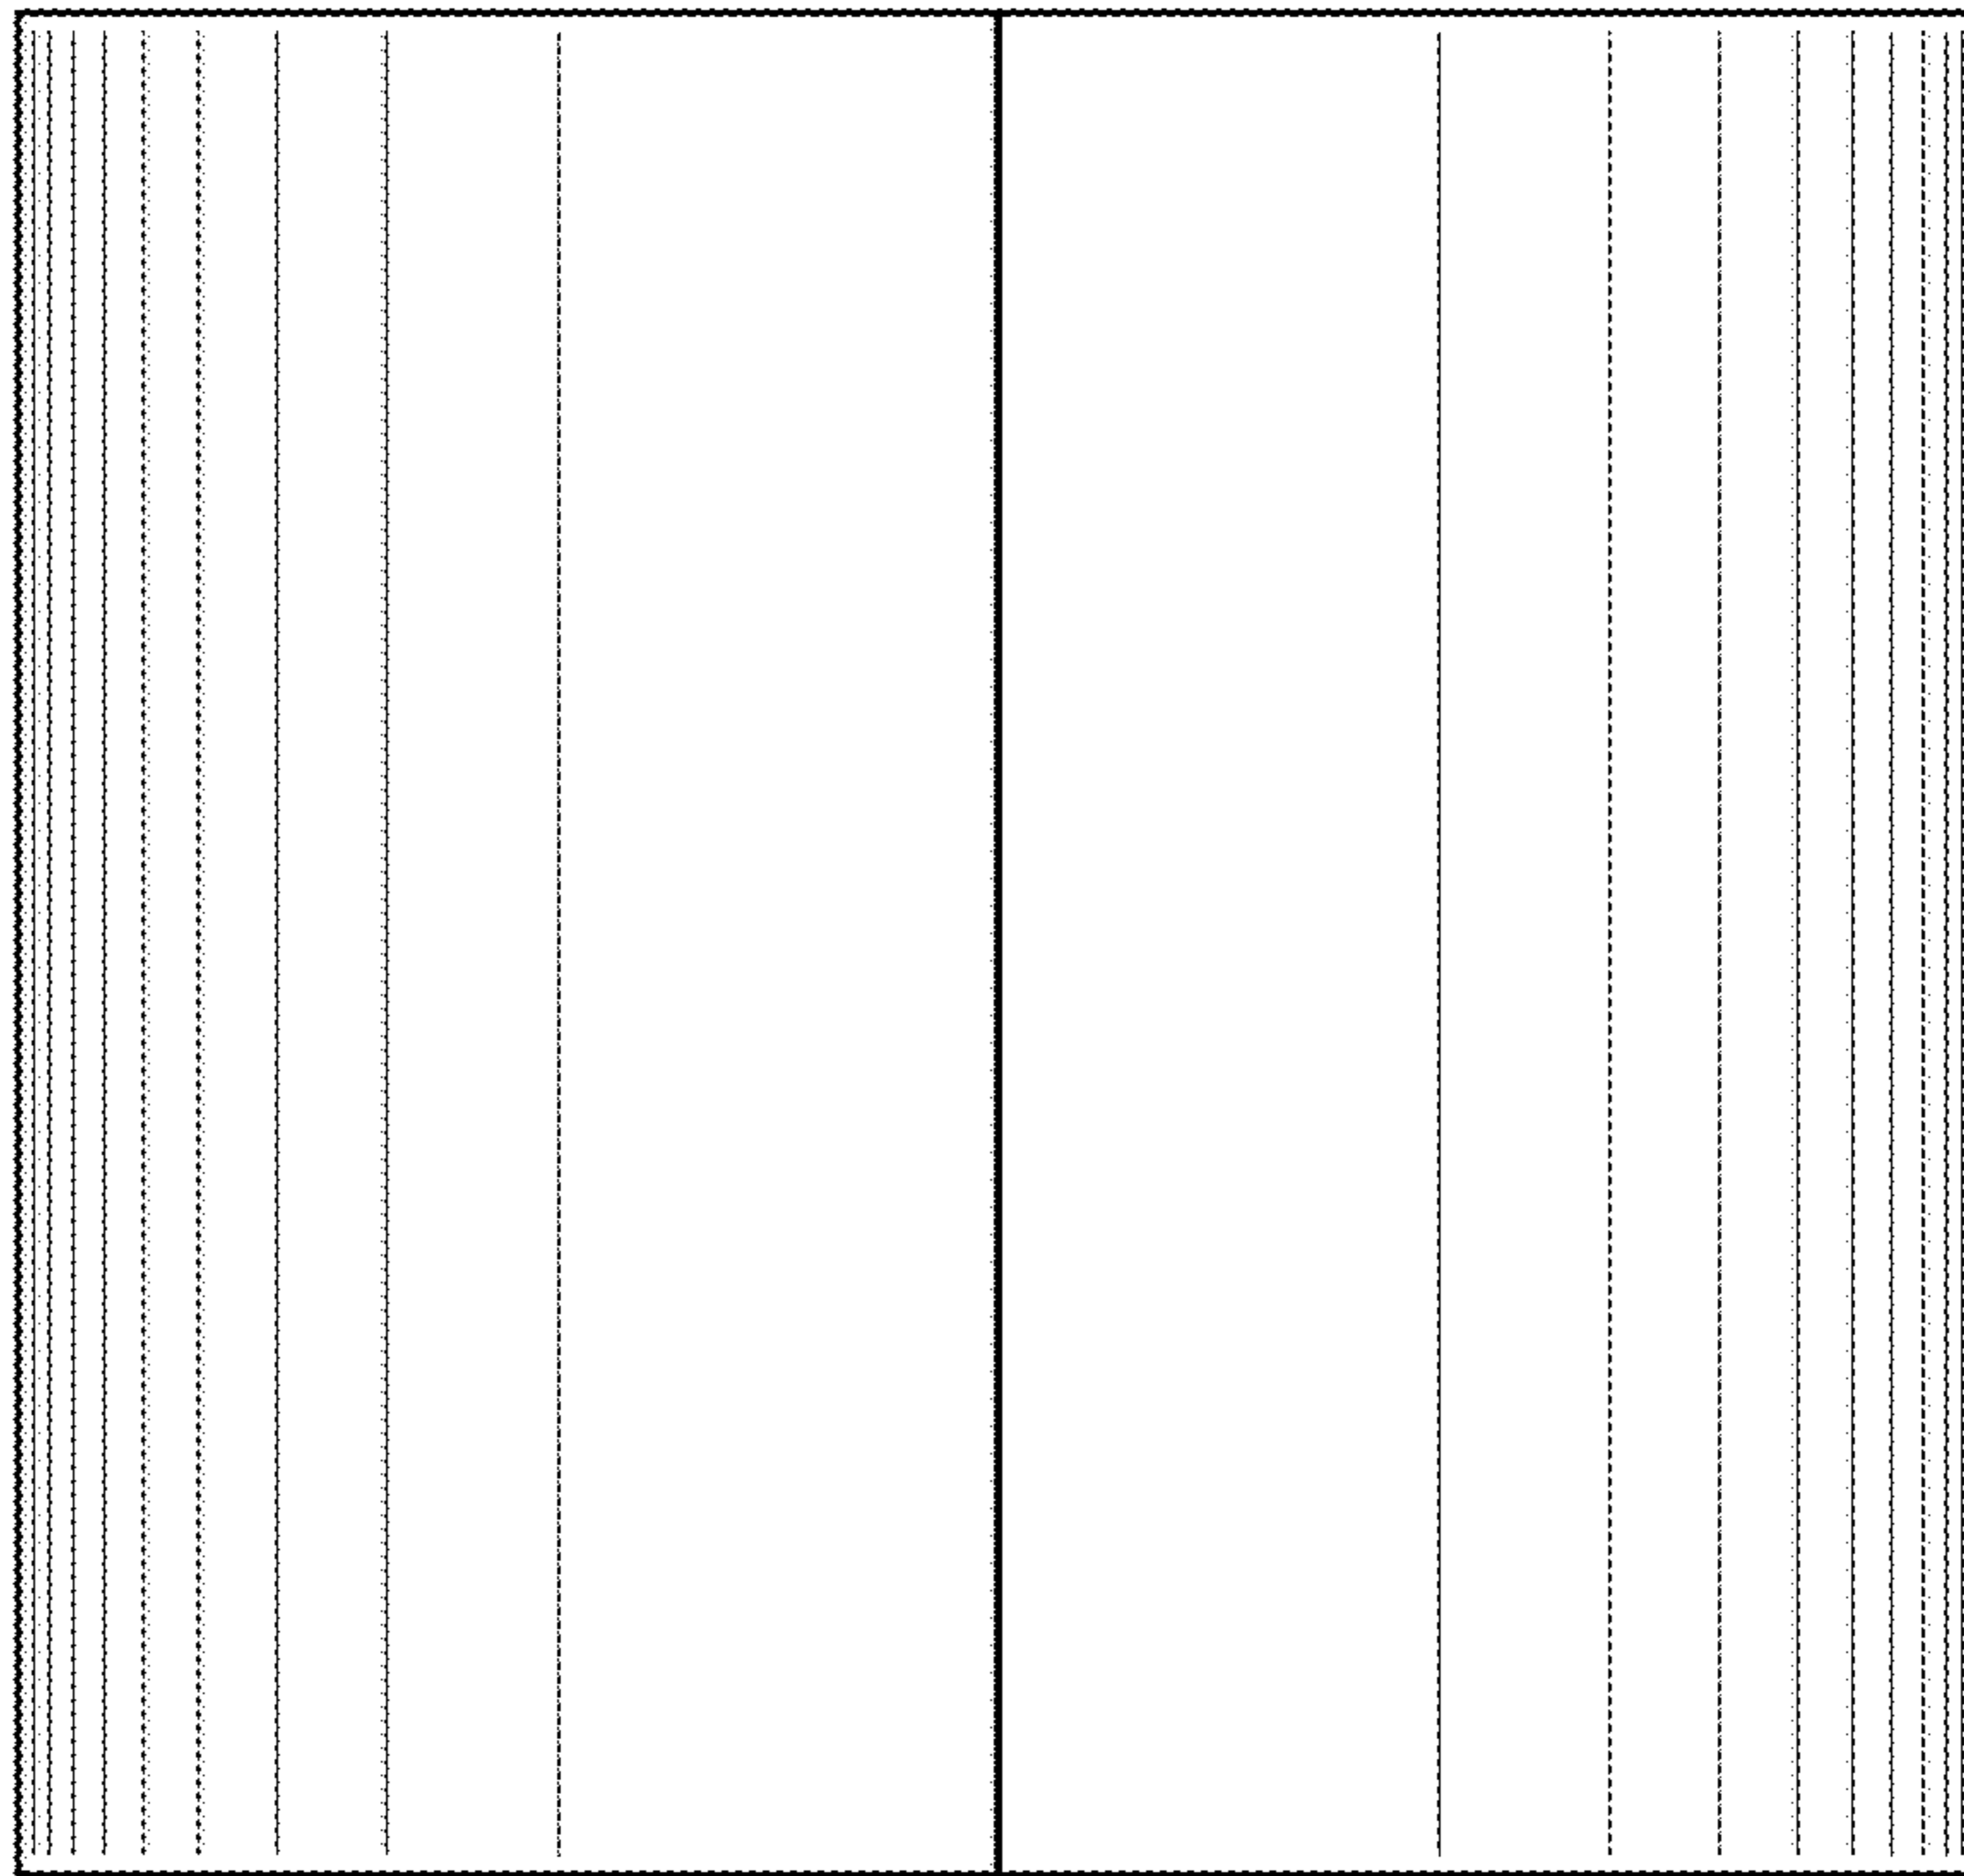


FIG. 2

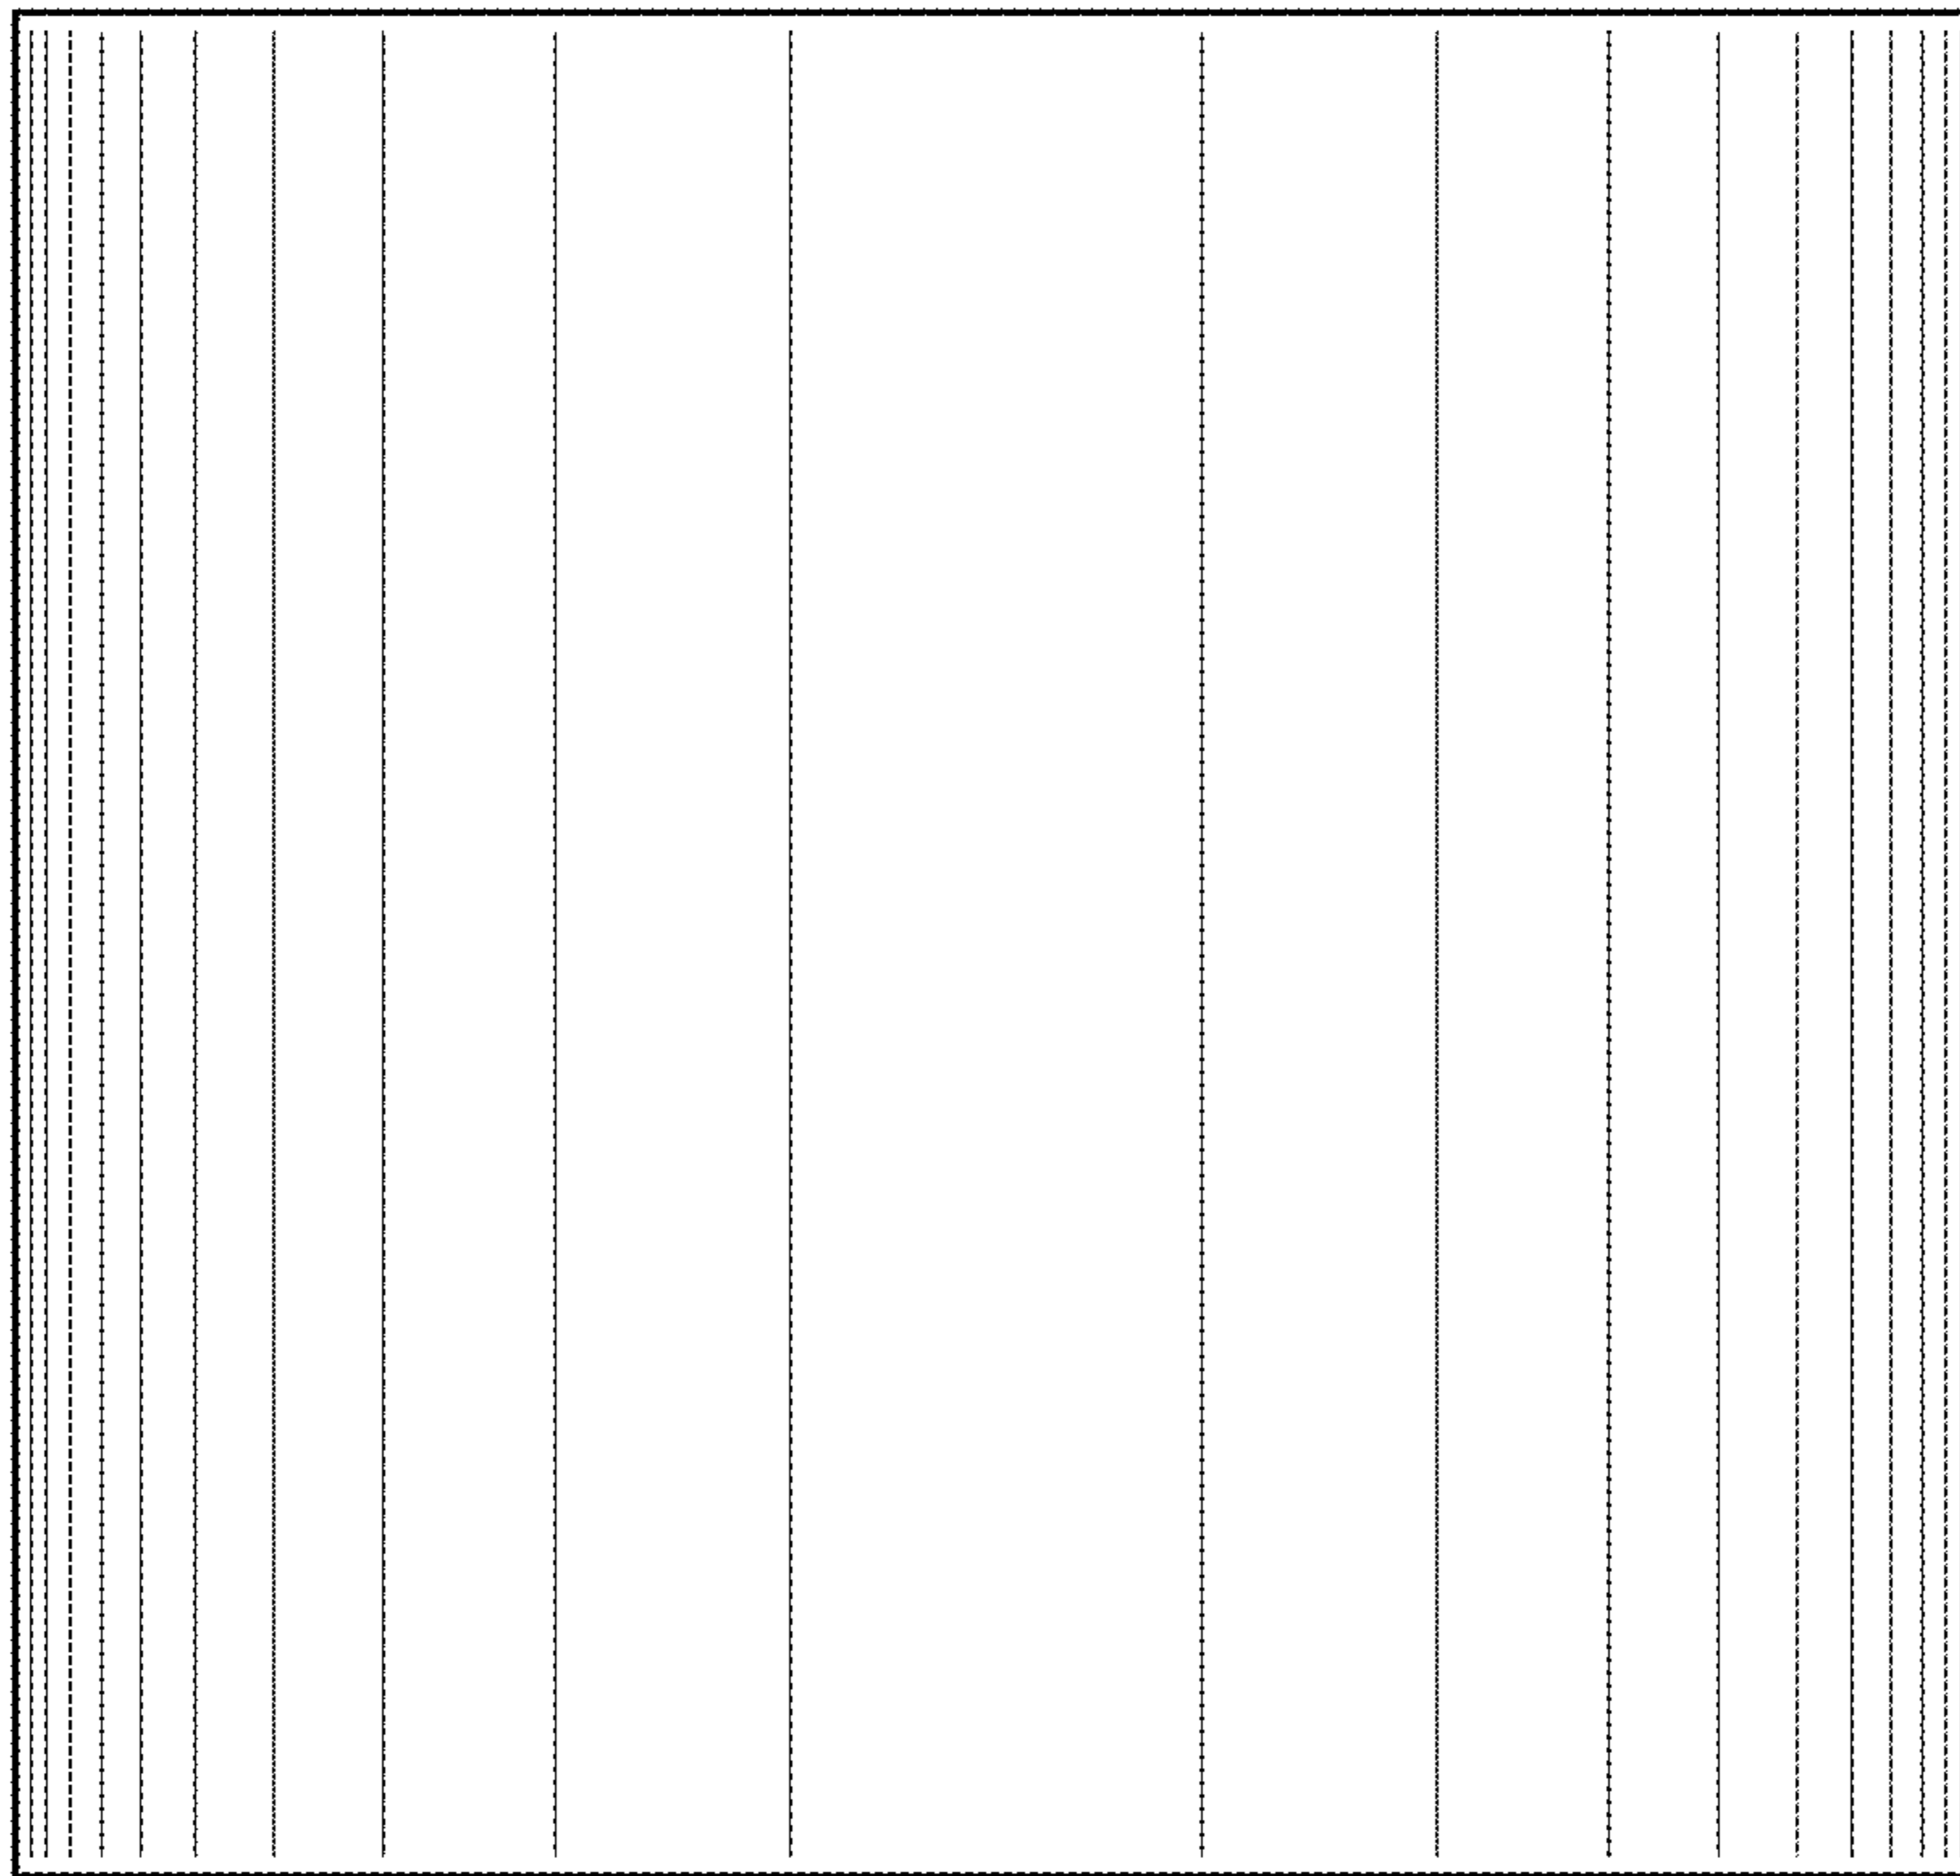


FIG. 3

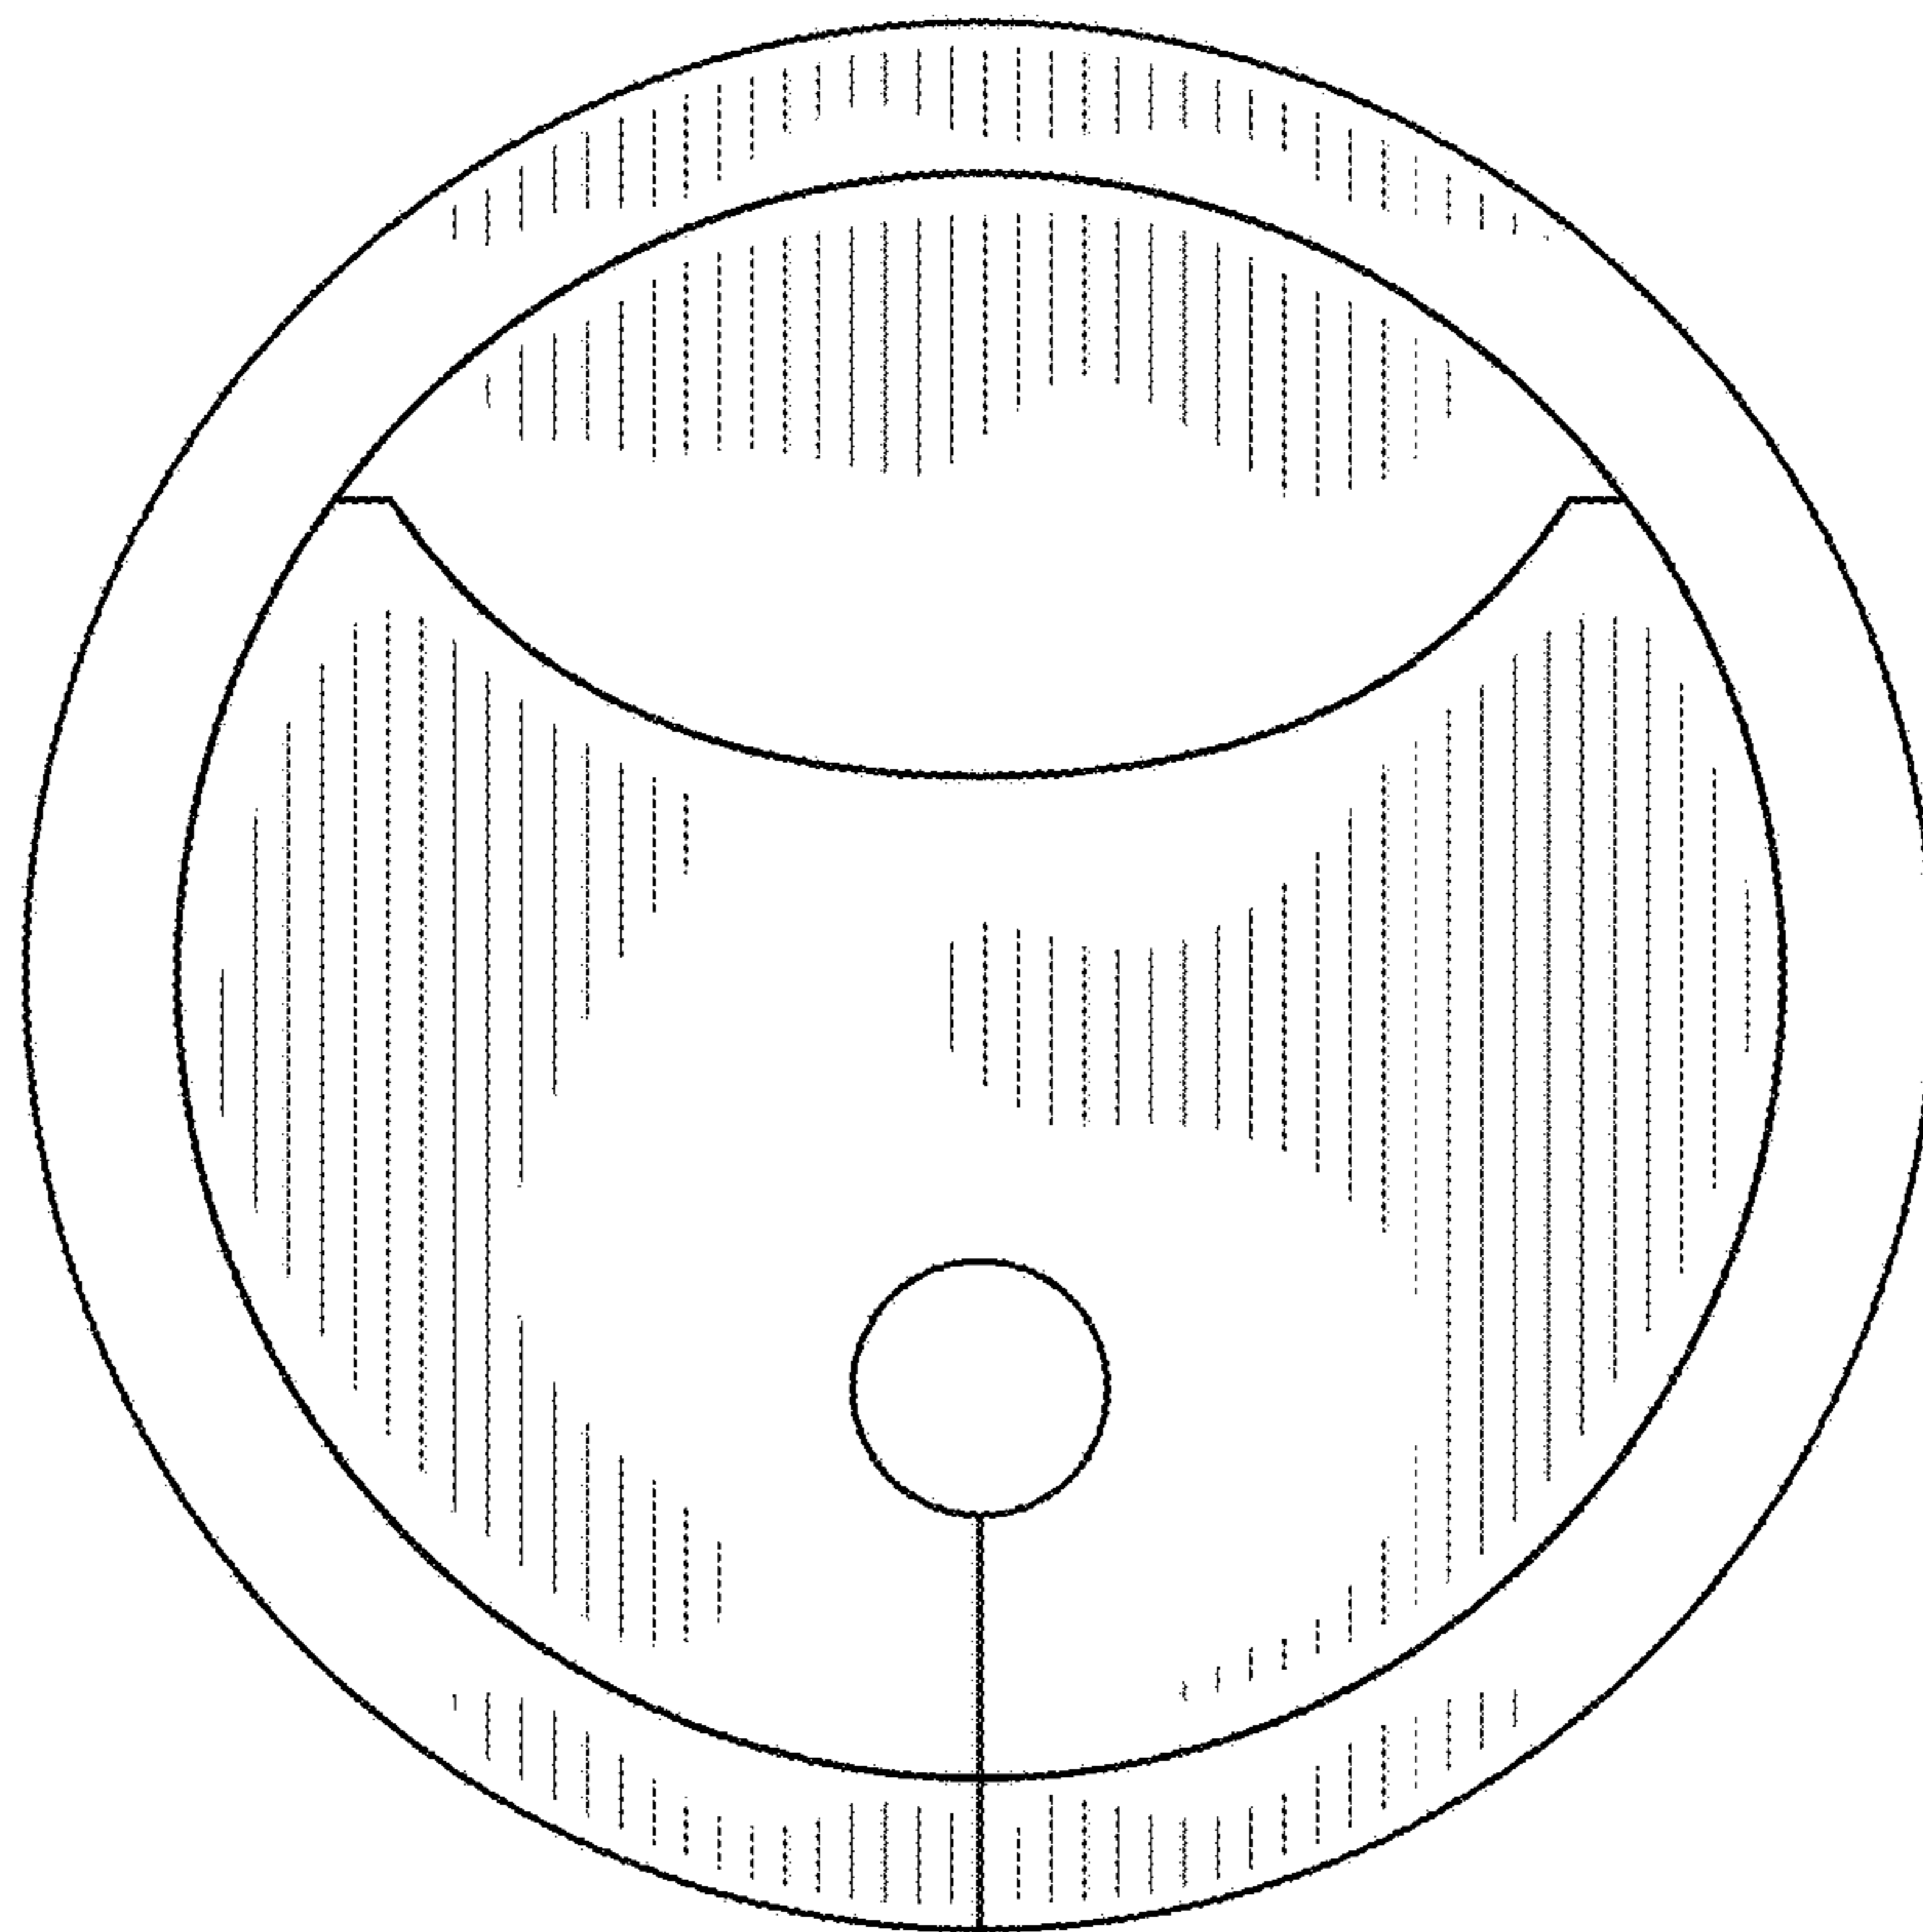


FIG. 4

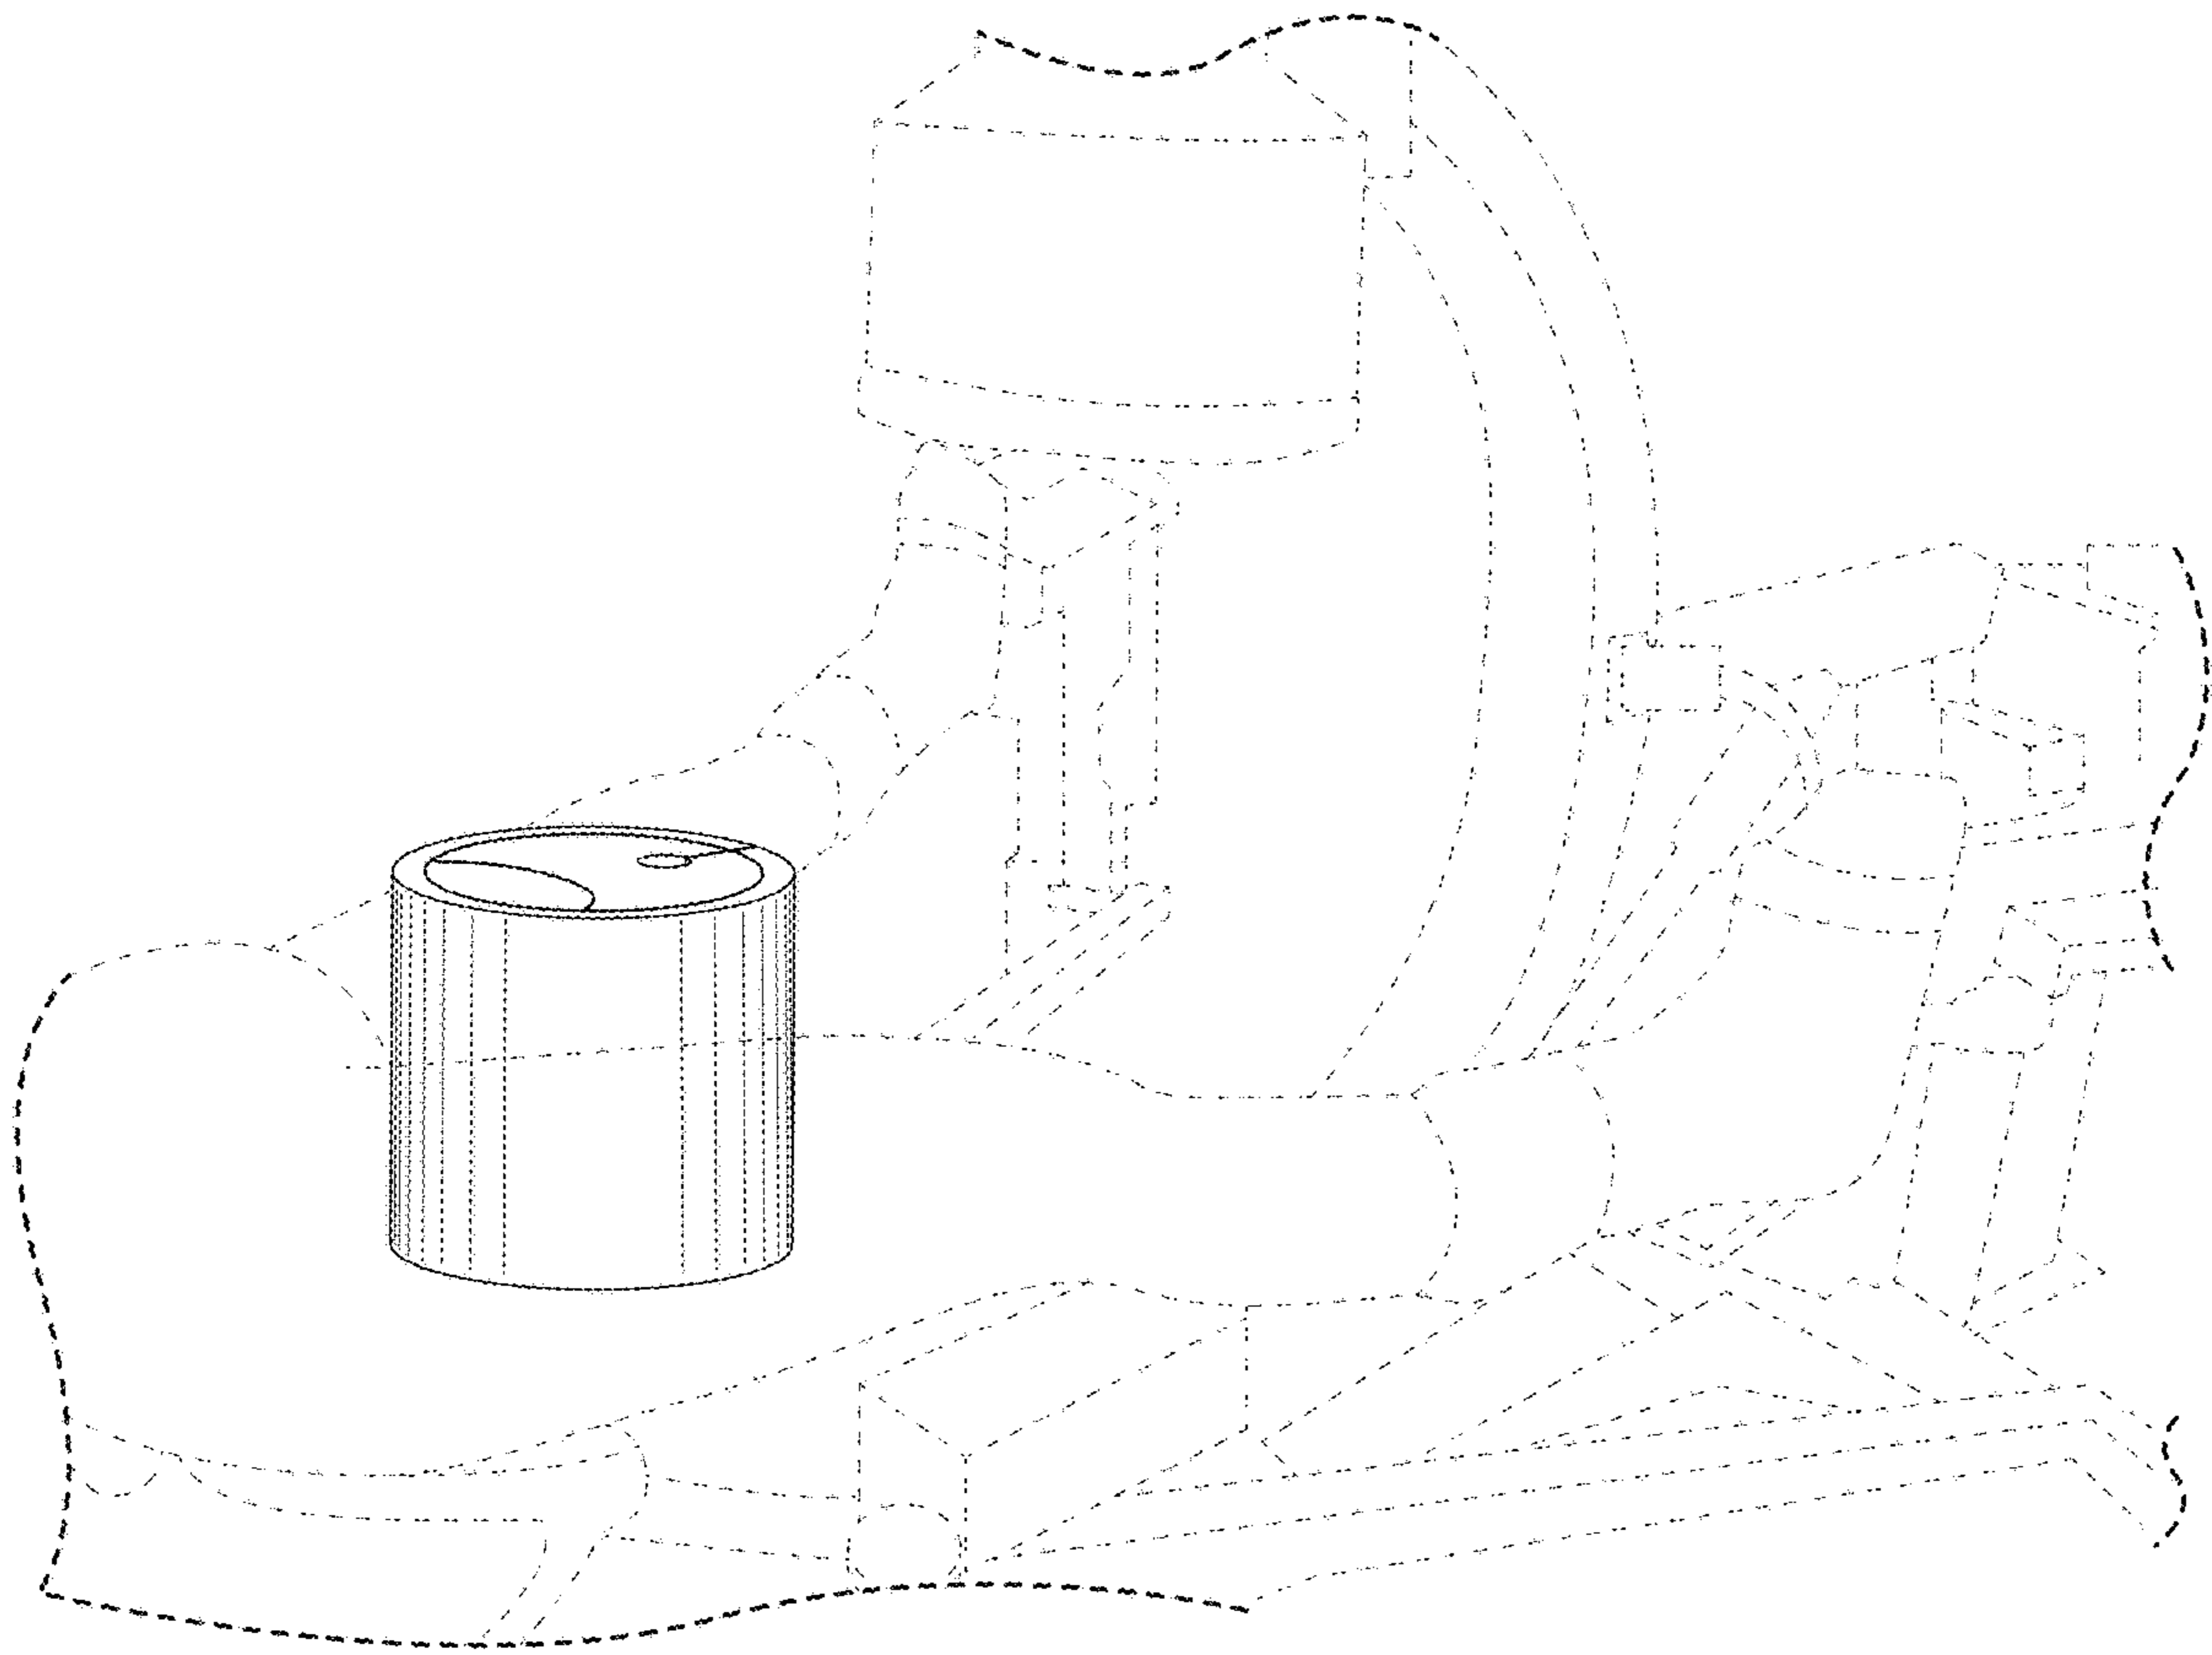


FIG. 5