



US00D828575S

(12) **United States Design Patent** (10) **Patent No.:** **US D828,575 S**
Ohno (45) **Date of Patent:** **** Sep. 11, 2018**

(54) **MEDICAL IMMUNOASSAY DEVICE**

(71) Applicant: **FUJIFILM Corporation**, Tokyo (JP)

(72) Inventor: **Hirotohi Ohno**, Ashigarakami-gun (JP)

(73) Assignee: **FUJIFILM Corporation**, Minato-ku, Tokyo (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/593,934**

(22) Filed: **Feb. 14, 2017**

(30) **Foreign Application Priority Data**

Aug. 15, 2016 (JP) 2016-017380

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**

USPC D24/186, 107-108, 169, 216-219,
D24/223-225, 229-233; D10/81;
422/63-64, 68.1, 85.05, 82.05, 554, 561,
422/565, 420; 435/287.2

CPC Y10S 436/806; Y10S 436/809; Y10S
977/918; B01D 15/3804; B01D 15/10;
B01D 15/3809; B01D 15/3857; B01L
2300/0867; B01L 7/52; G06K 9/00127;
G01N 33/53; G01N 2035/00306; G01N
2035/00326; G01N 2035/00336; G01N
2035/00366

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D718,462 S * 11/2014 Cook D24/216
D728,121 S * 4/2015 Cook D24/216
D730,535 S * 5/2015 Gutmann D24/216

D734,484 S * 7/2015 Nishikawa D24/216
9,205,379 B2 * 12/2015 Latham G01N 27/44739
D772,086 S * 11/2016 Schueren D10/81
D774,205 S * 12/2016 Grace D24/169
D775,365 S * 12/2016 Mathers D24/232
2003/0180815 A1 * 9/2003 Rawson G01N 33/558
435/7.9
2004/0101952 A1 * 5/2004 Vent G01N 15/1463
435/287.3
2012/0227471 A1 * 9/2012 Smith G01N 35/1011
73/61.59

(Continued)

FOREIGN PATENT DOCUMENTS

KR 300917916.0000 * 8/2017

Primary Examiner — Anhdao Doan

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(57) **CLAIM**


The ornamental design for a medical immunoassay device, as shown and described.

DESCRIPTION

FIG. 1 is a top, front and right side perspective view of a medical immunoassay device showing my new design; FIG. 2 is a top, rear and left side perspective view thereof; FIG. 3 is a front elevational view thereof; FIG. 4 is a rear elevational view thereof; FIG. 5 is a top plan view thereof; FIG. 6 is a bottom plan view thereof; FIG. 7 is a left side elevational view thereof; and, FIG. 8 is a top, front and right side perspective view thereof, in a state where the lid is opened.

The broken lines depict portions of a medical immunoassay device in which the design is embodied that form no part of the claimed design. The broken line areas show a boundary of the medical immunoassay device that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

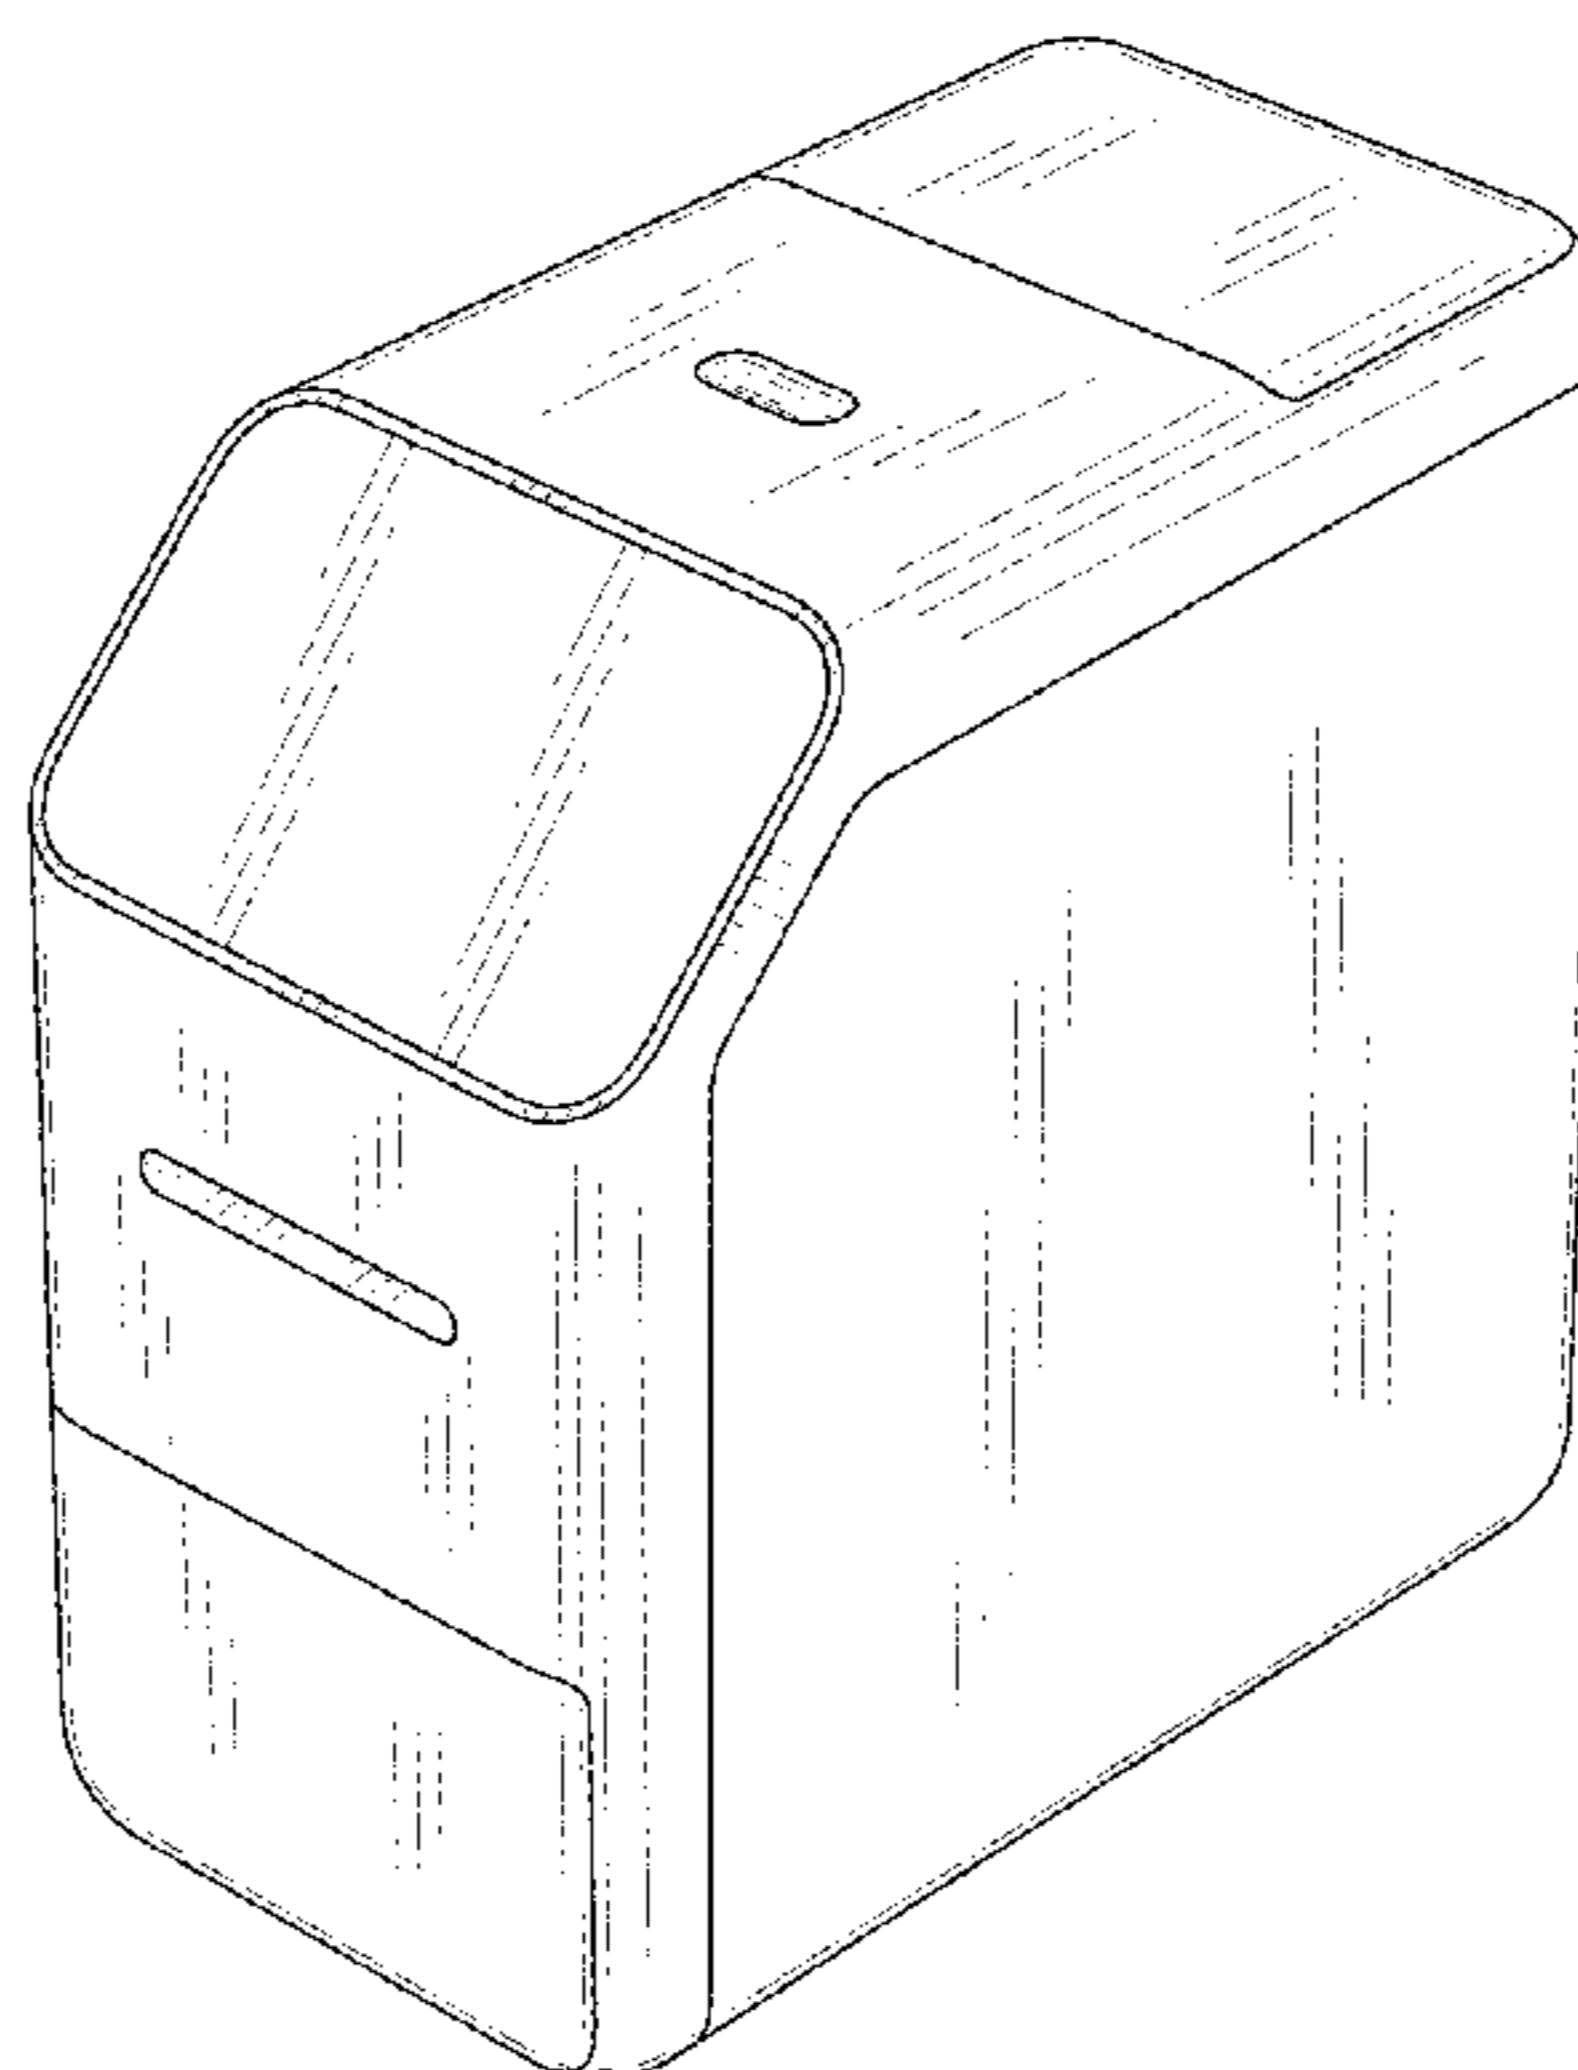

(56)

References Cited

U.S. PATENT DOCUMENTS

2016/0228876 A1* 8/2016 Chu C12Q 1/6806

* cited by examiner

FIG. 1

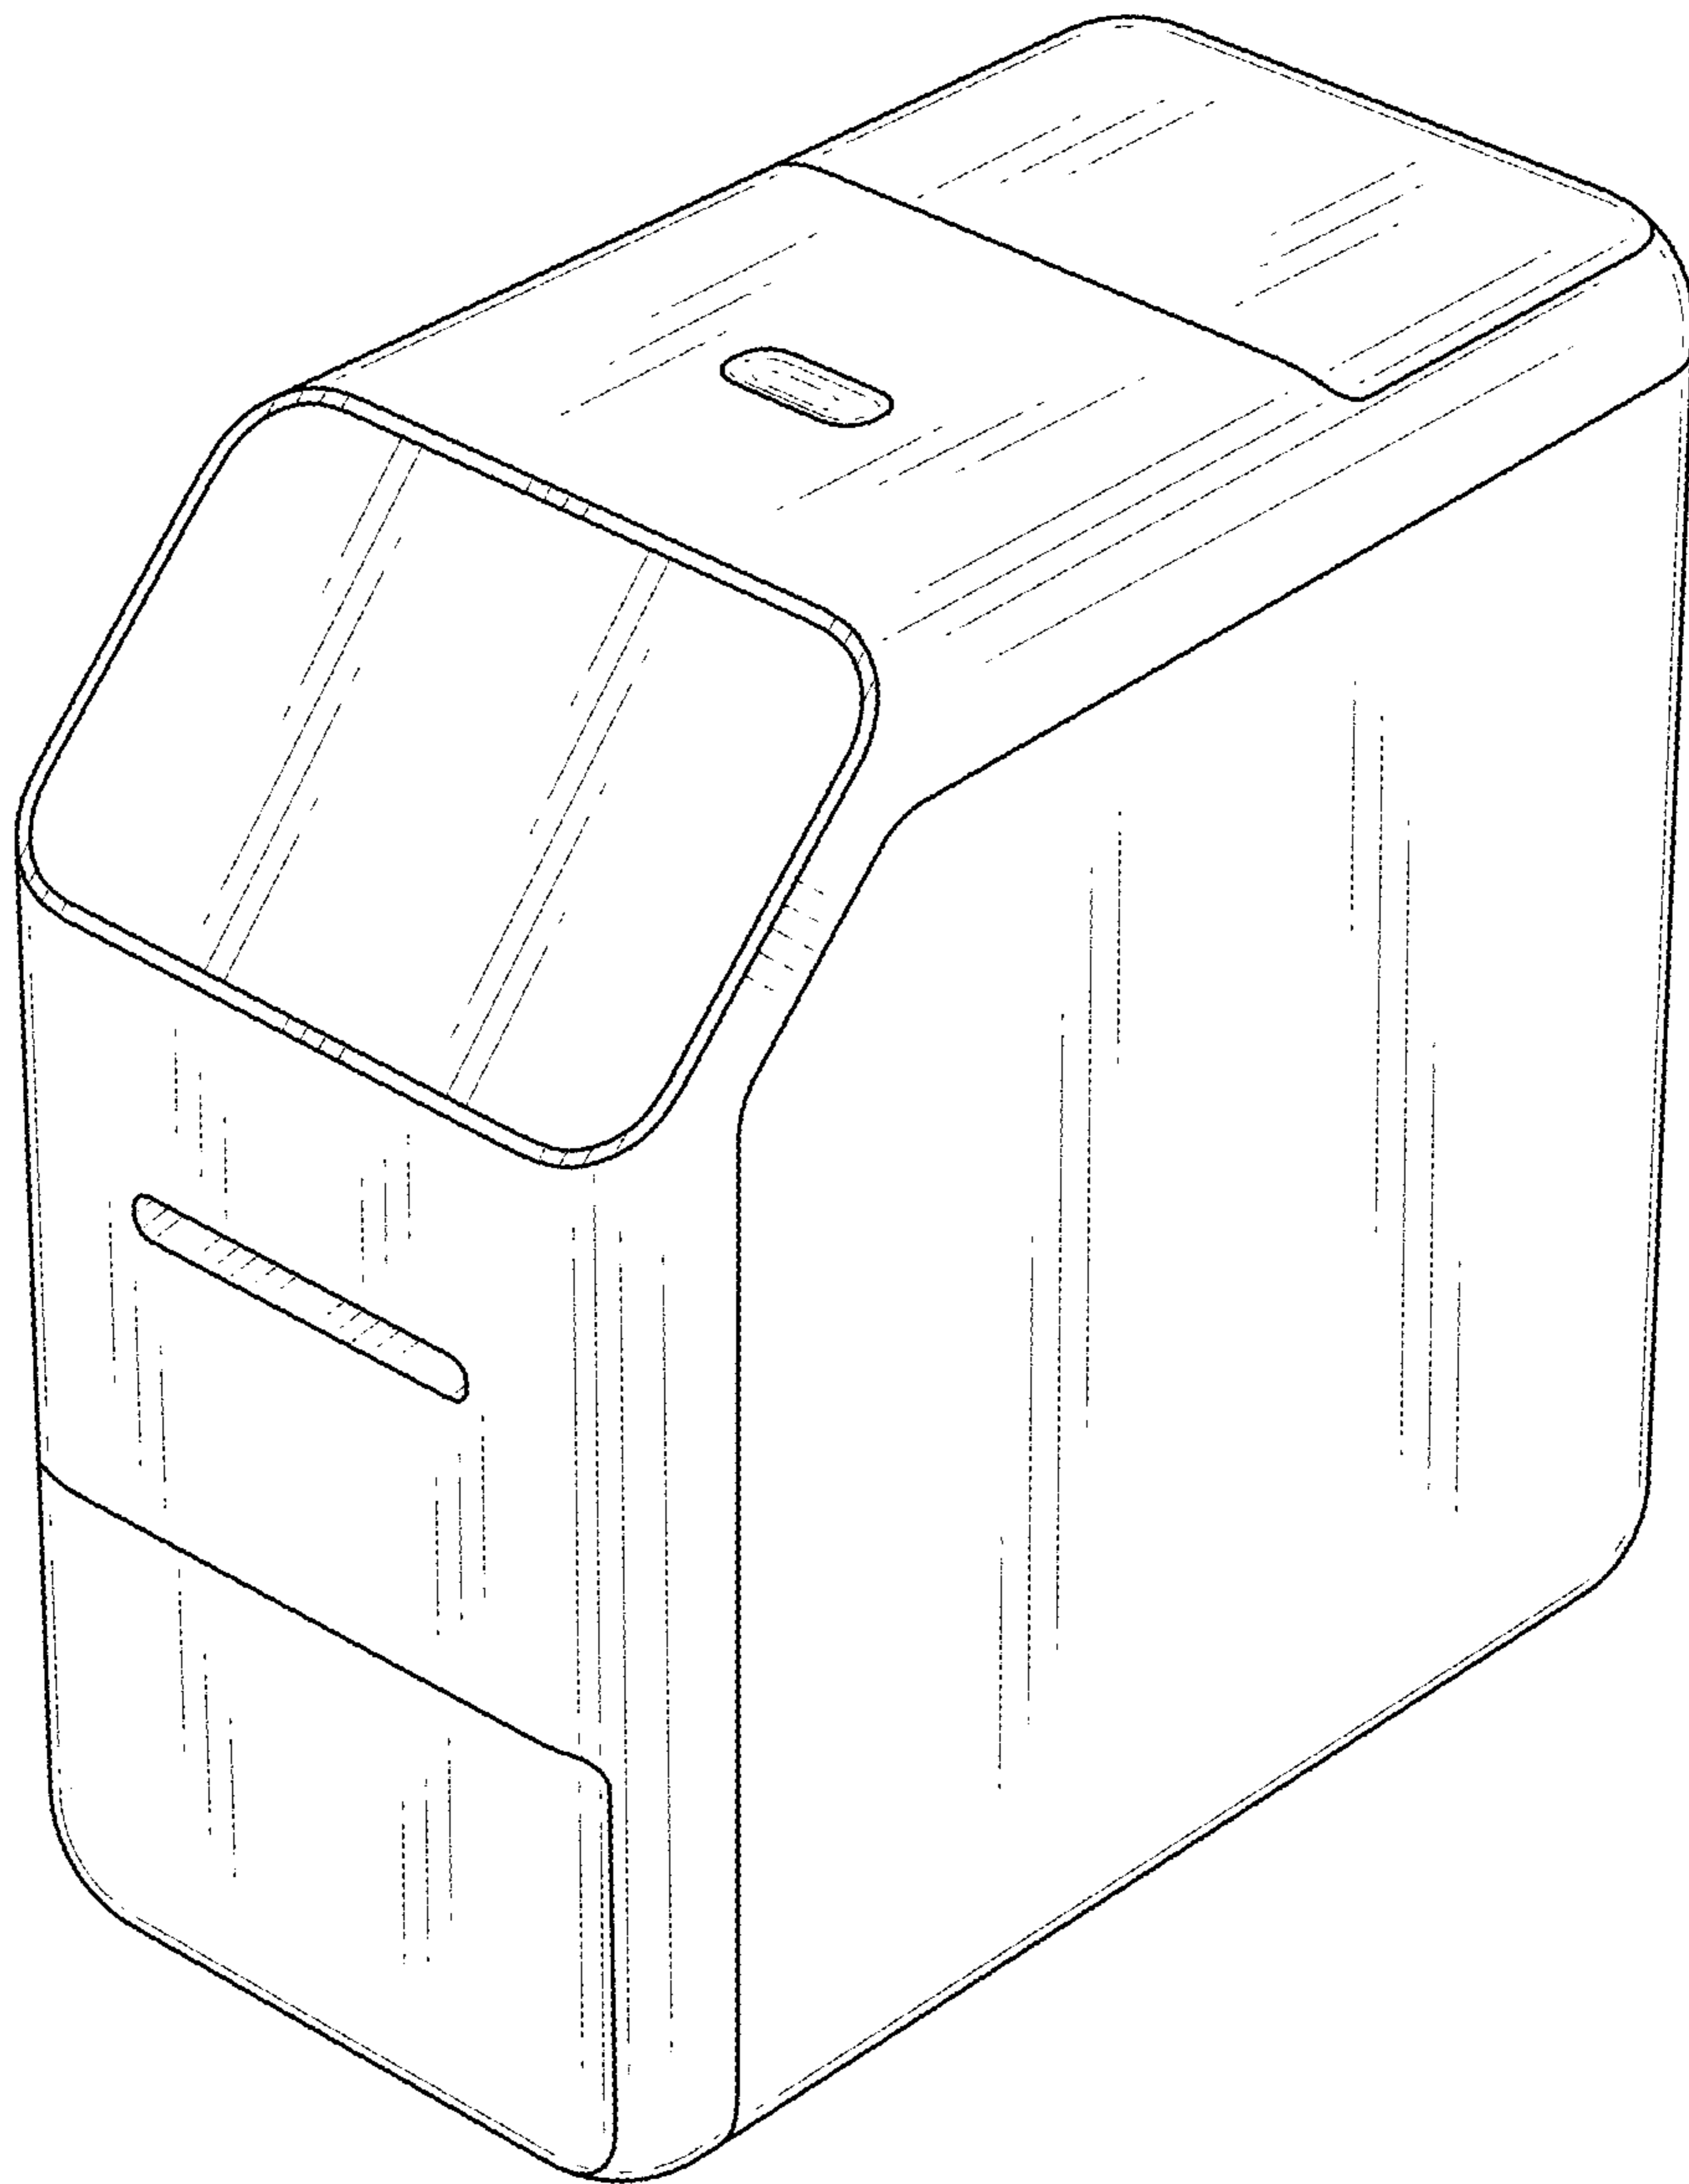


FIG. 2

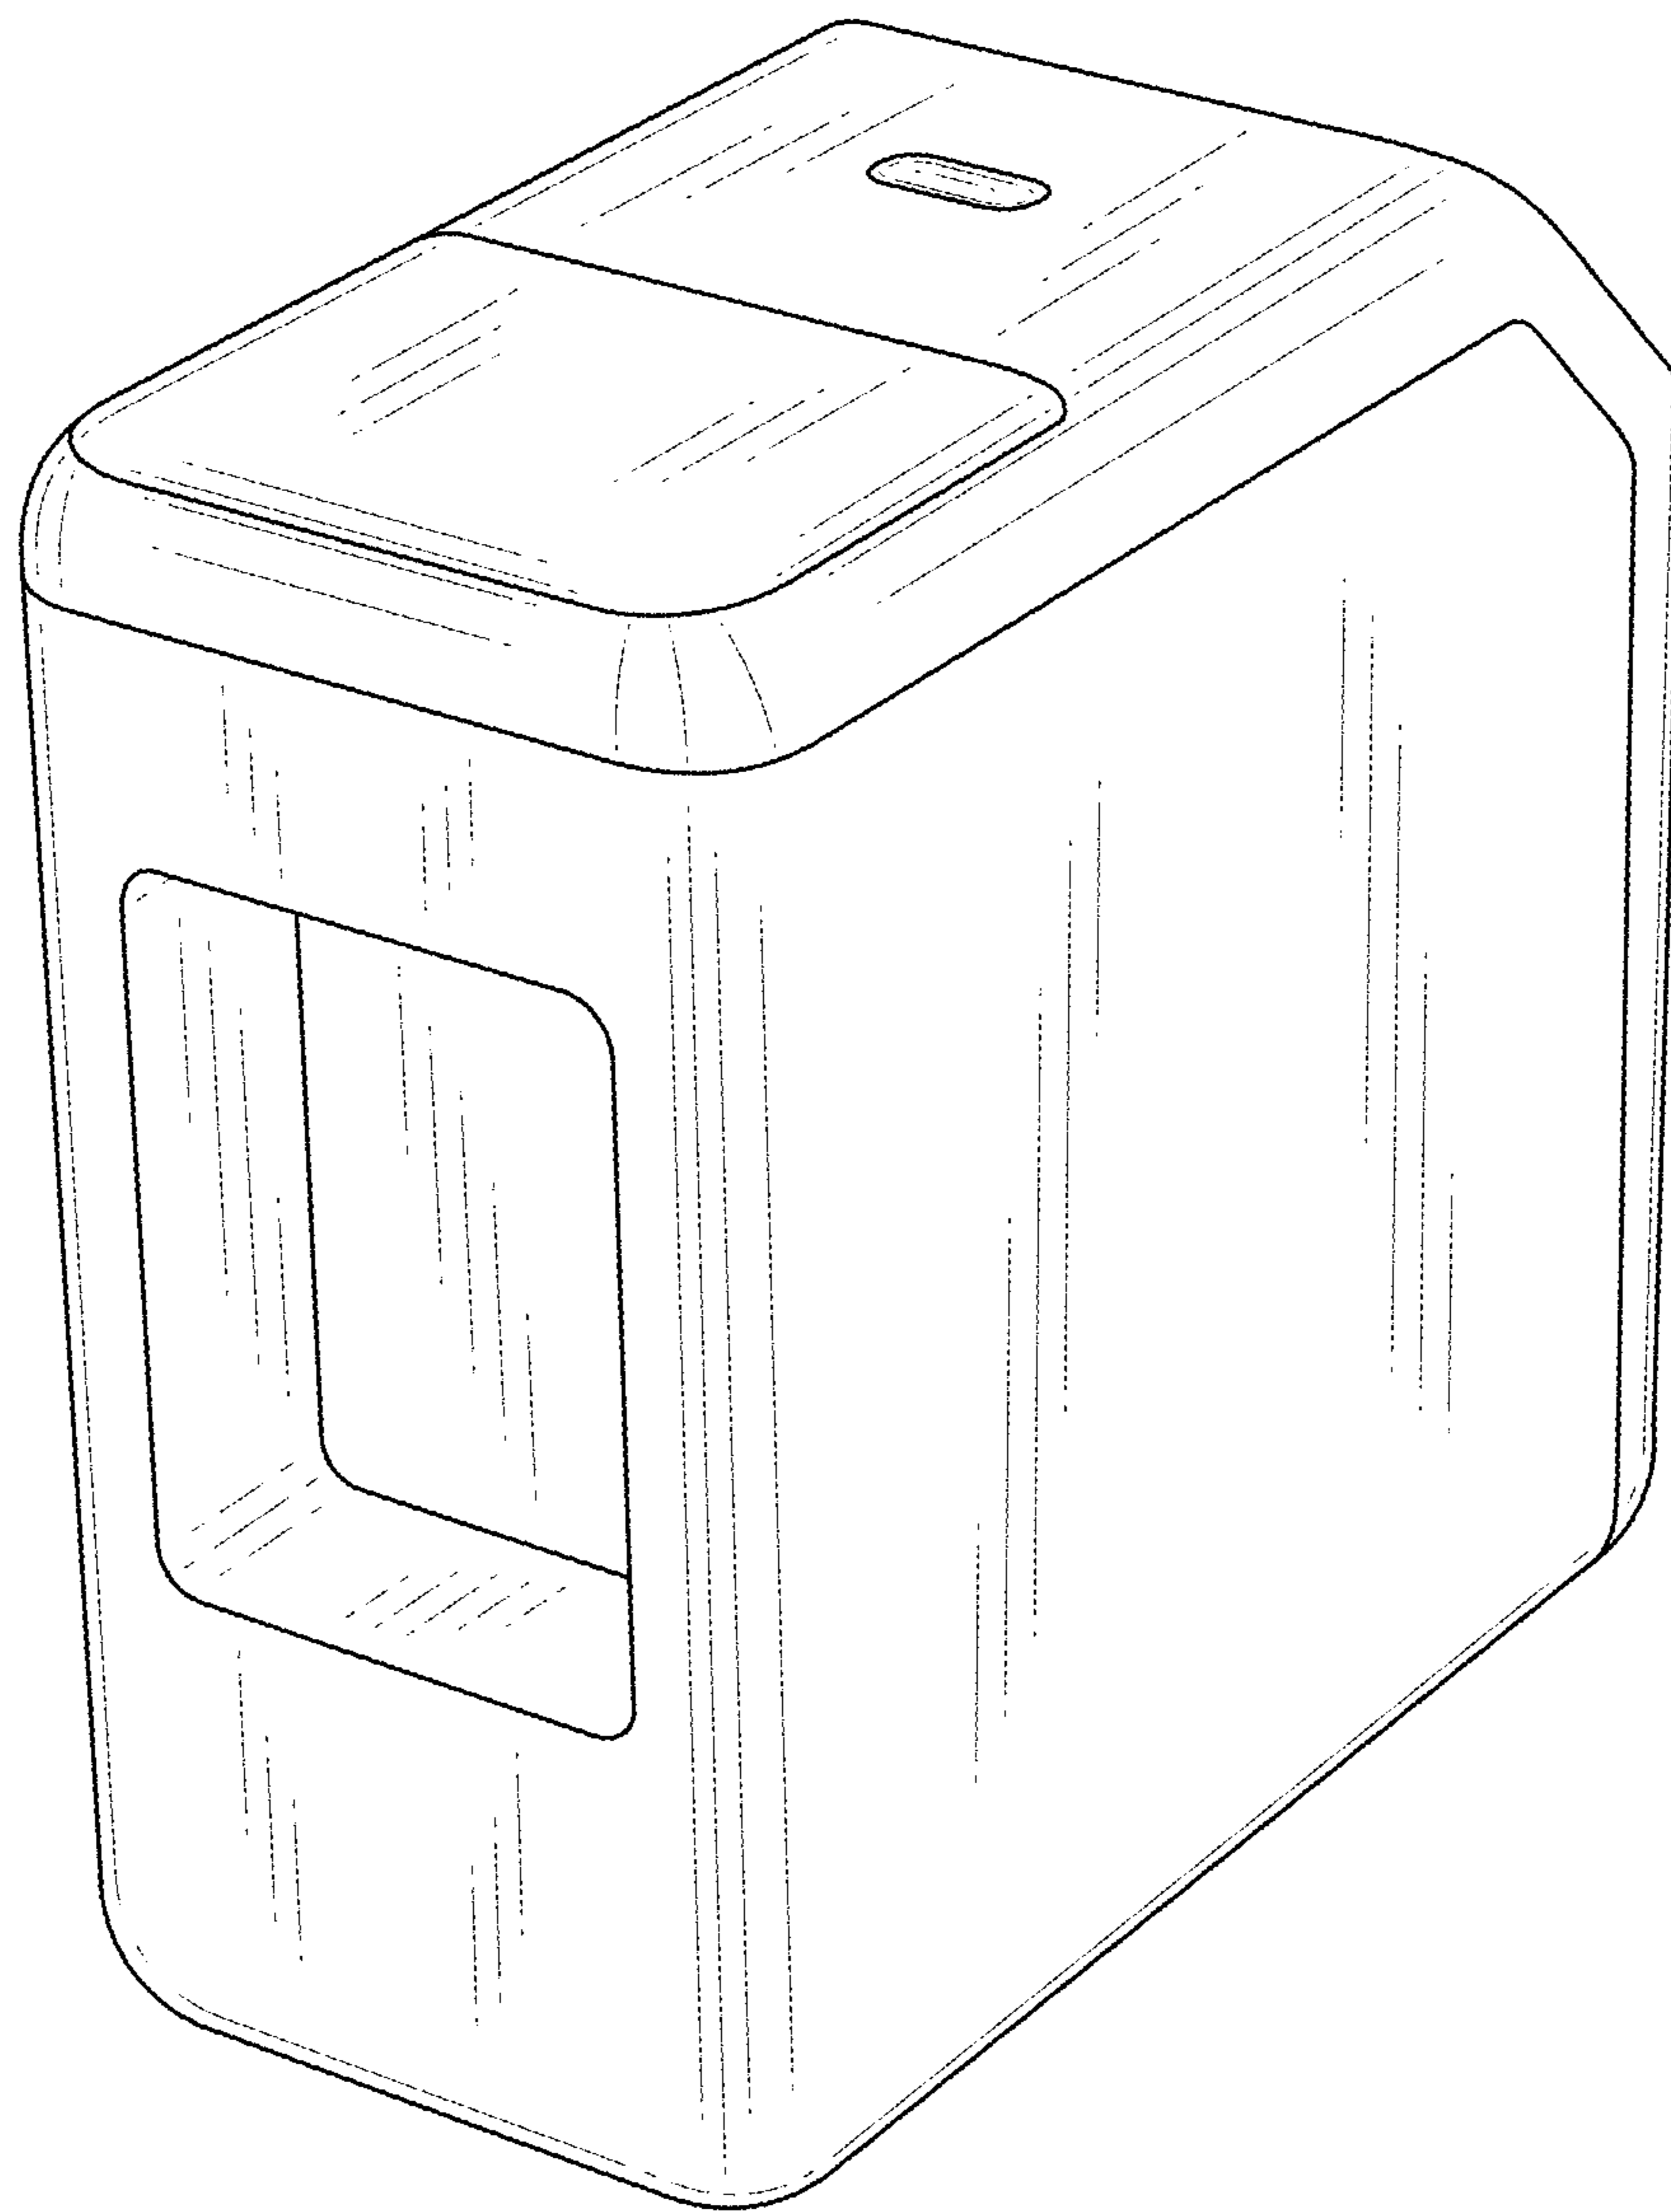


FIG. 3

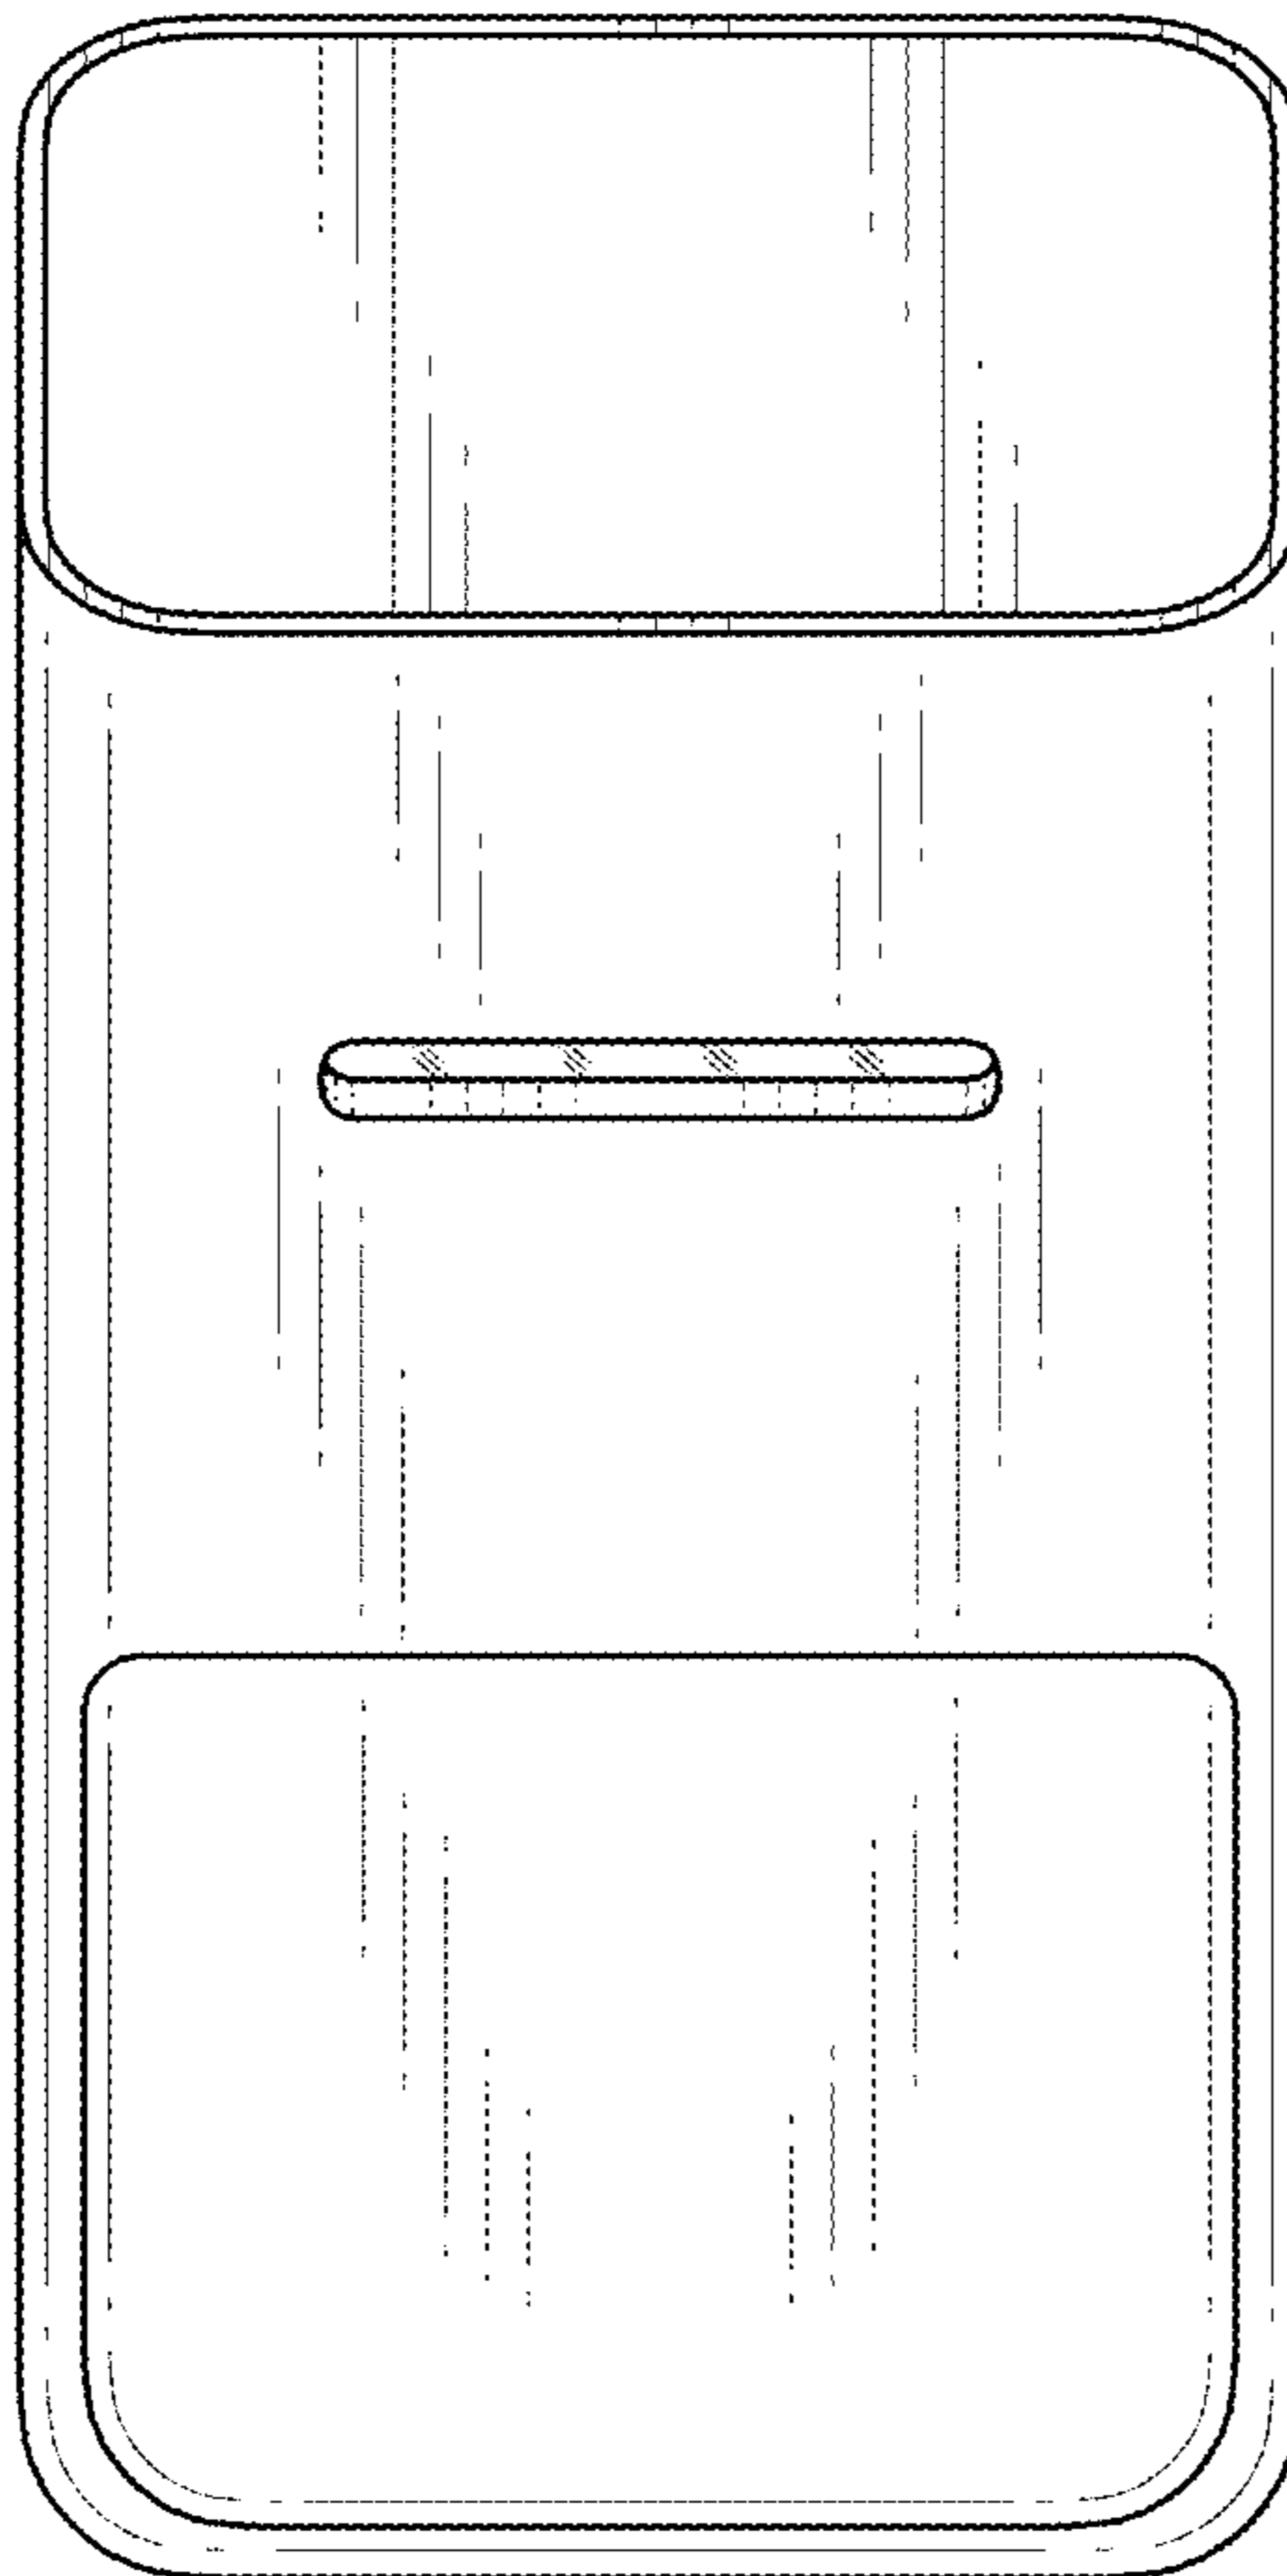


FIG. 4

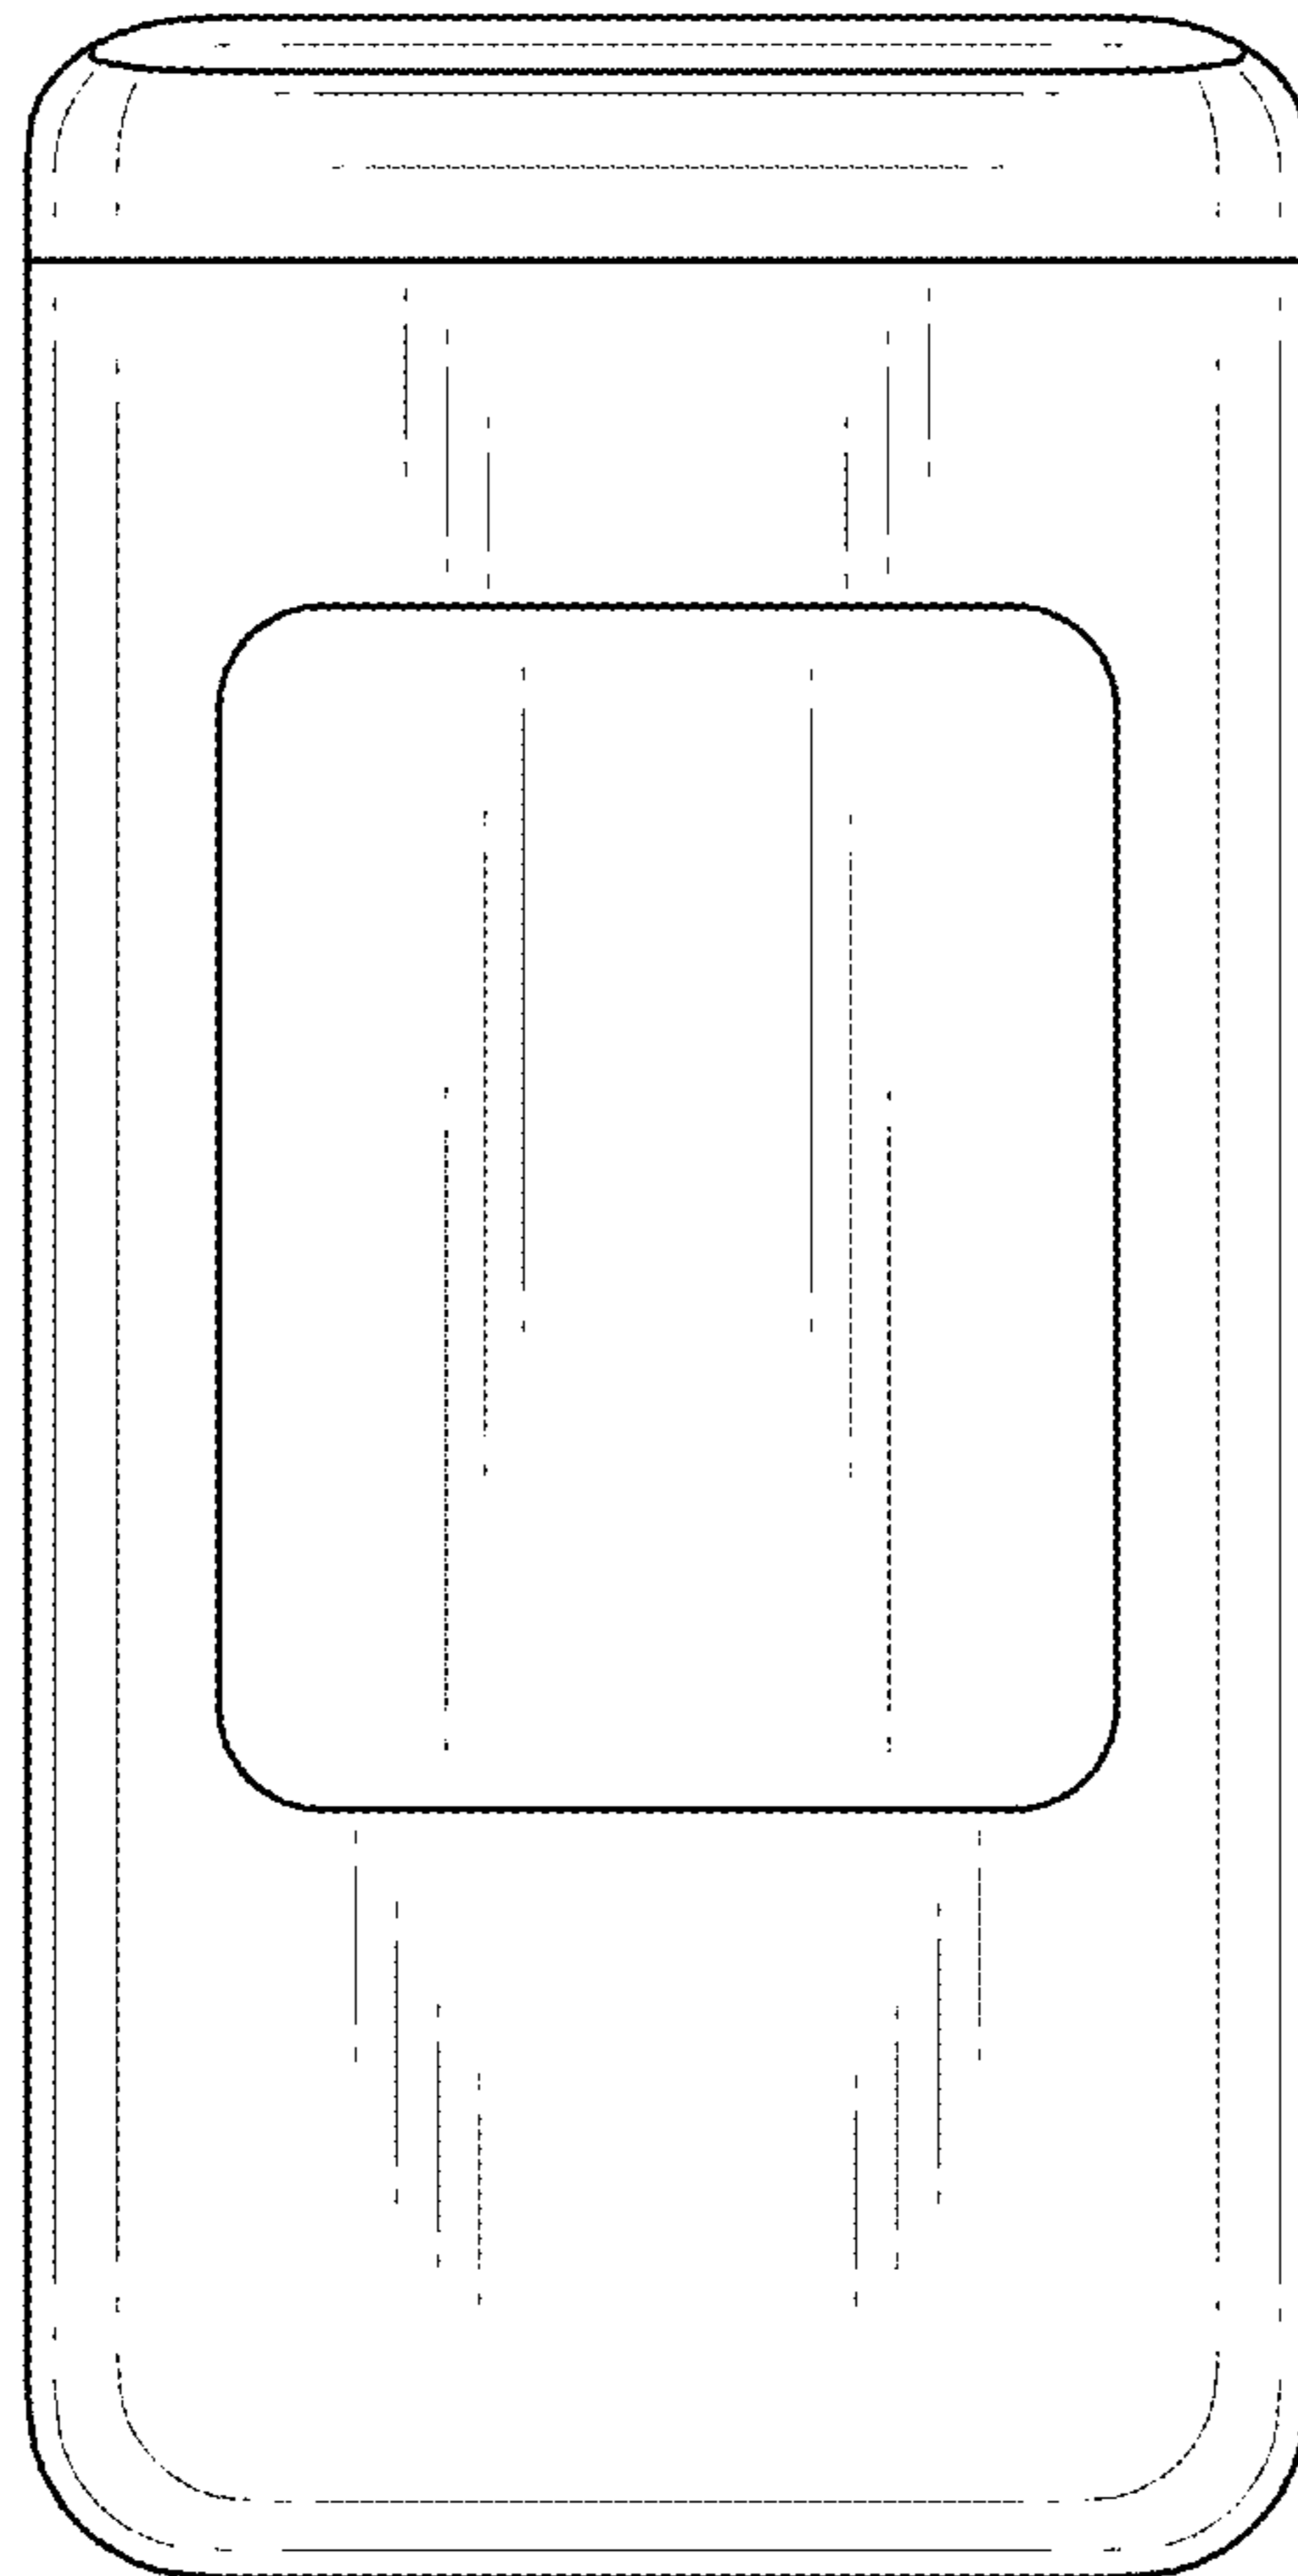


FIG. 5

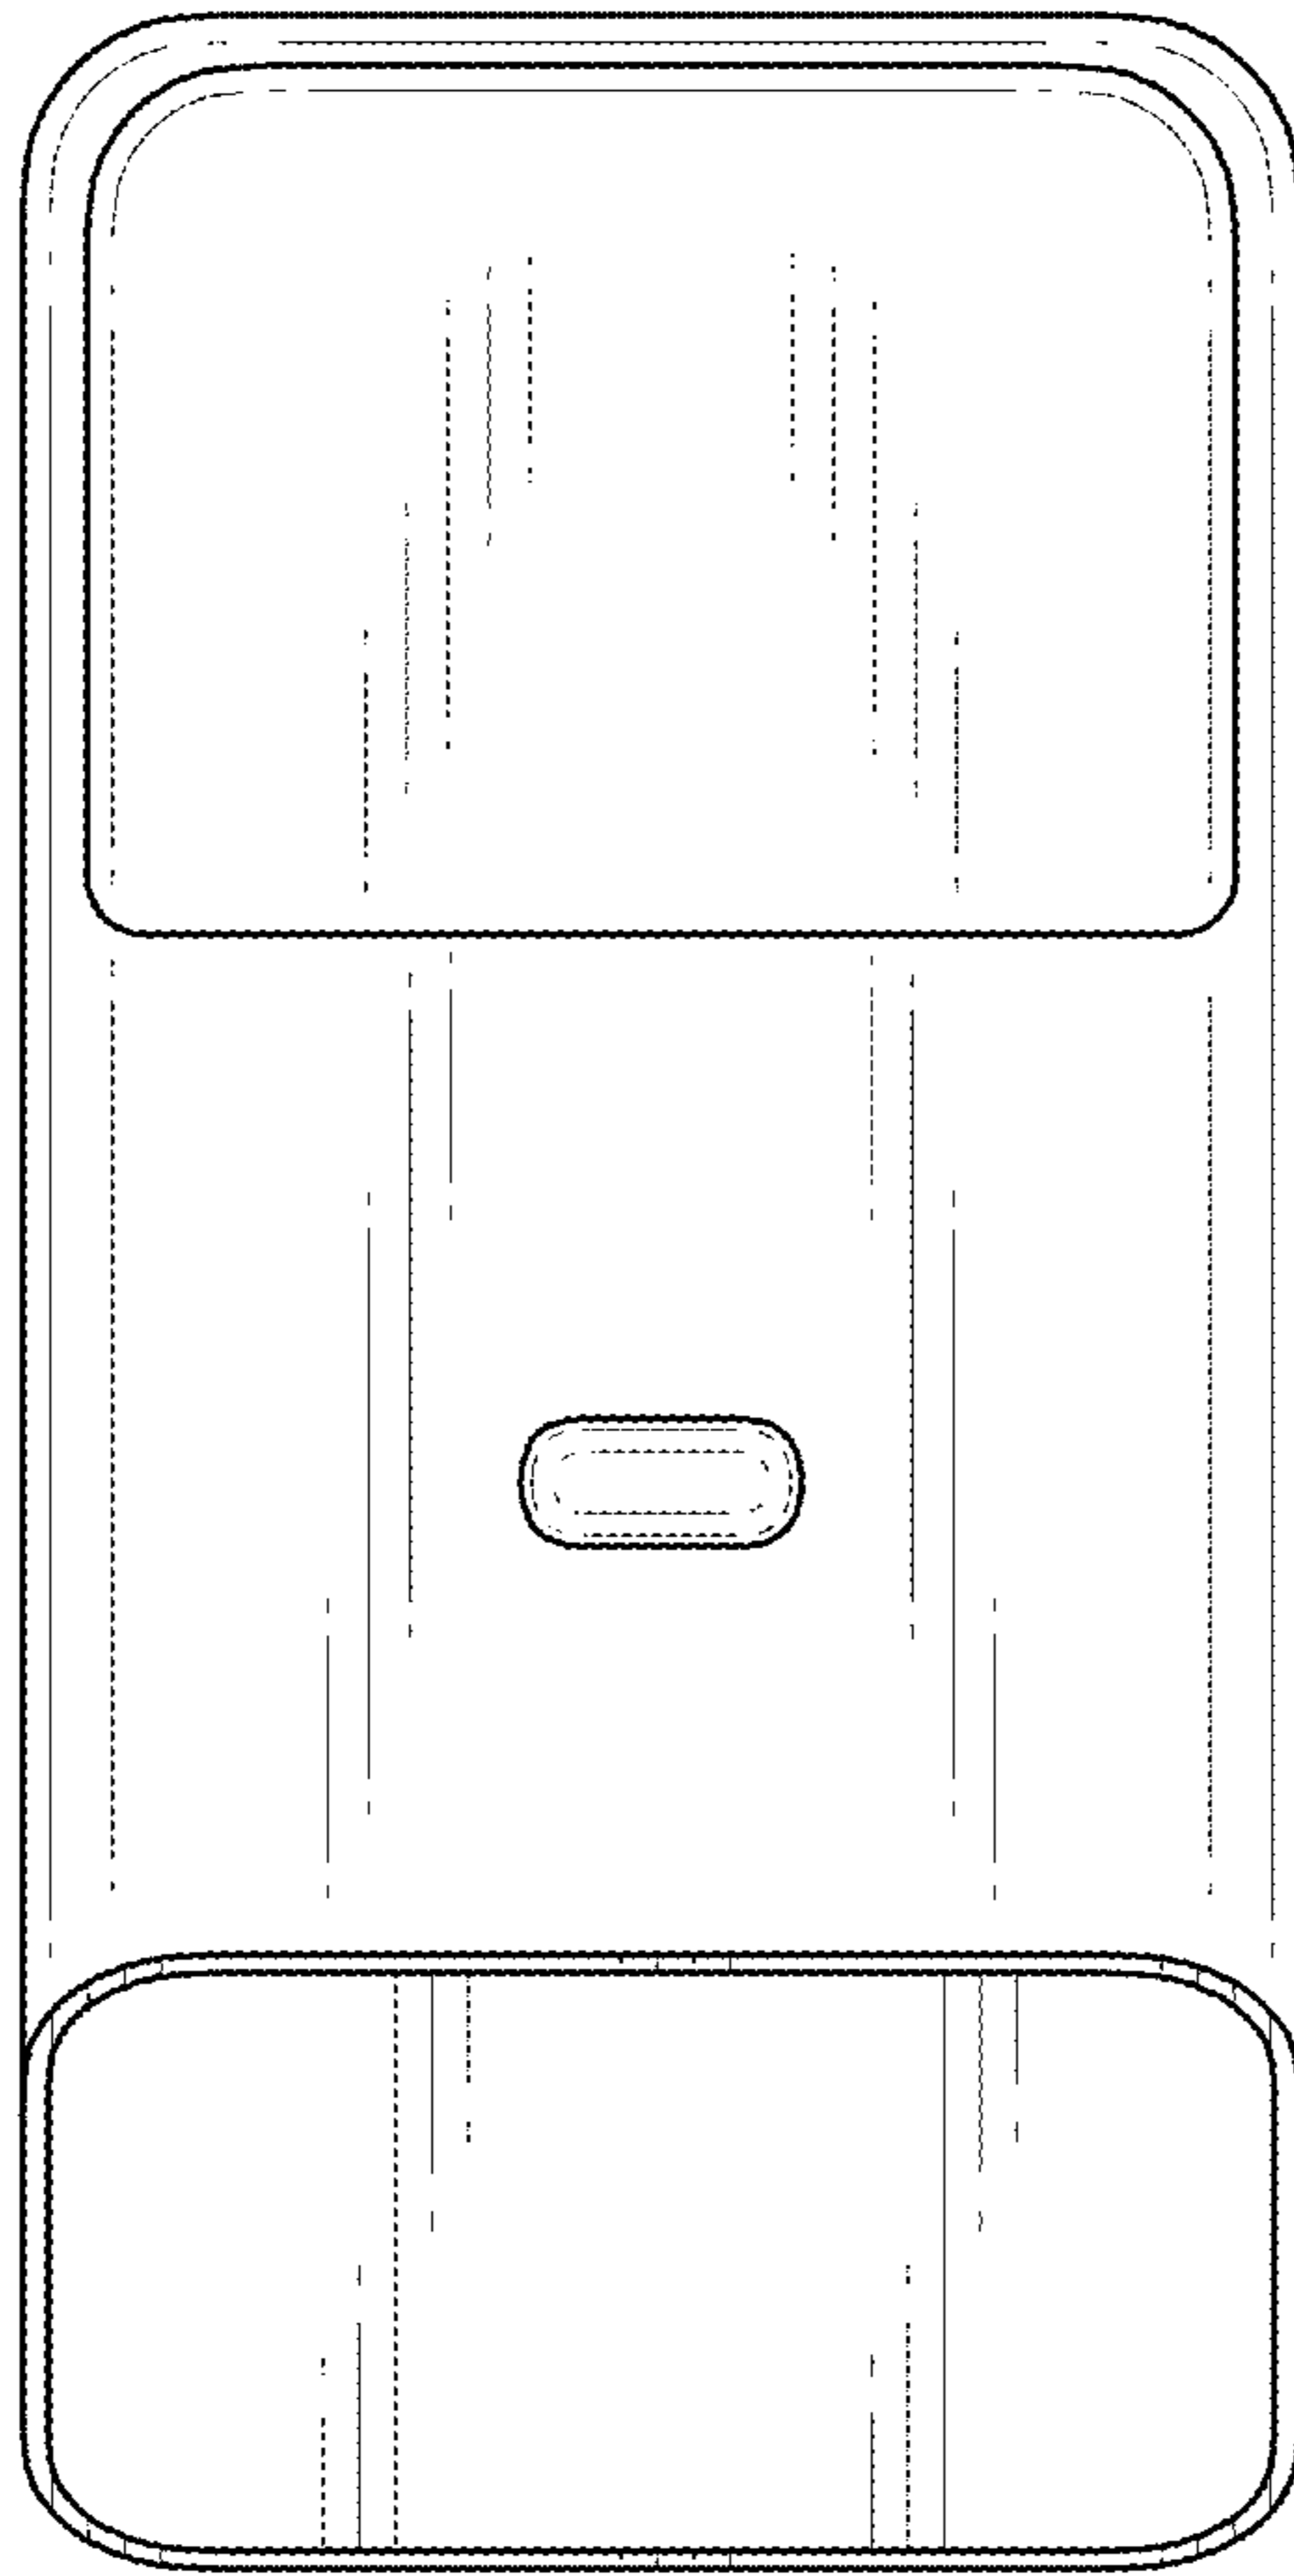


FIG. 6

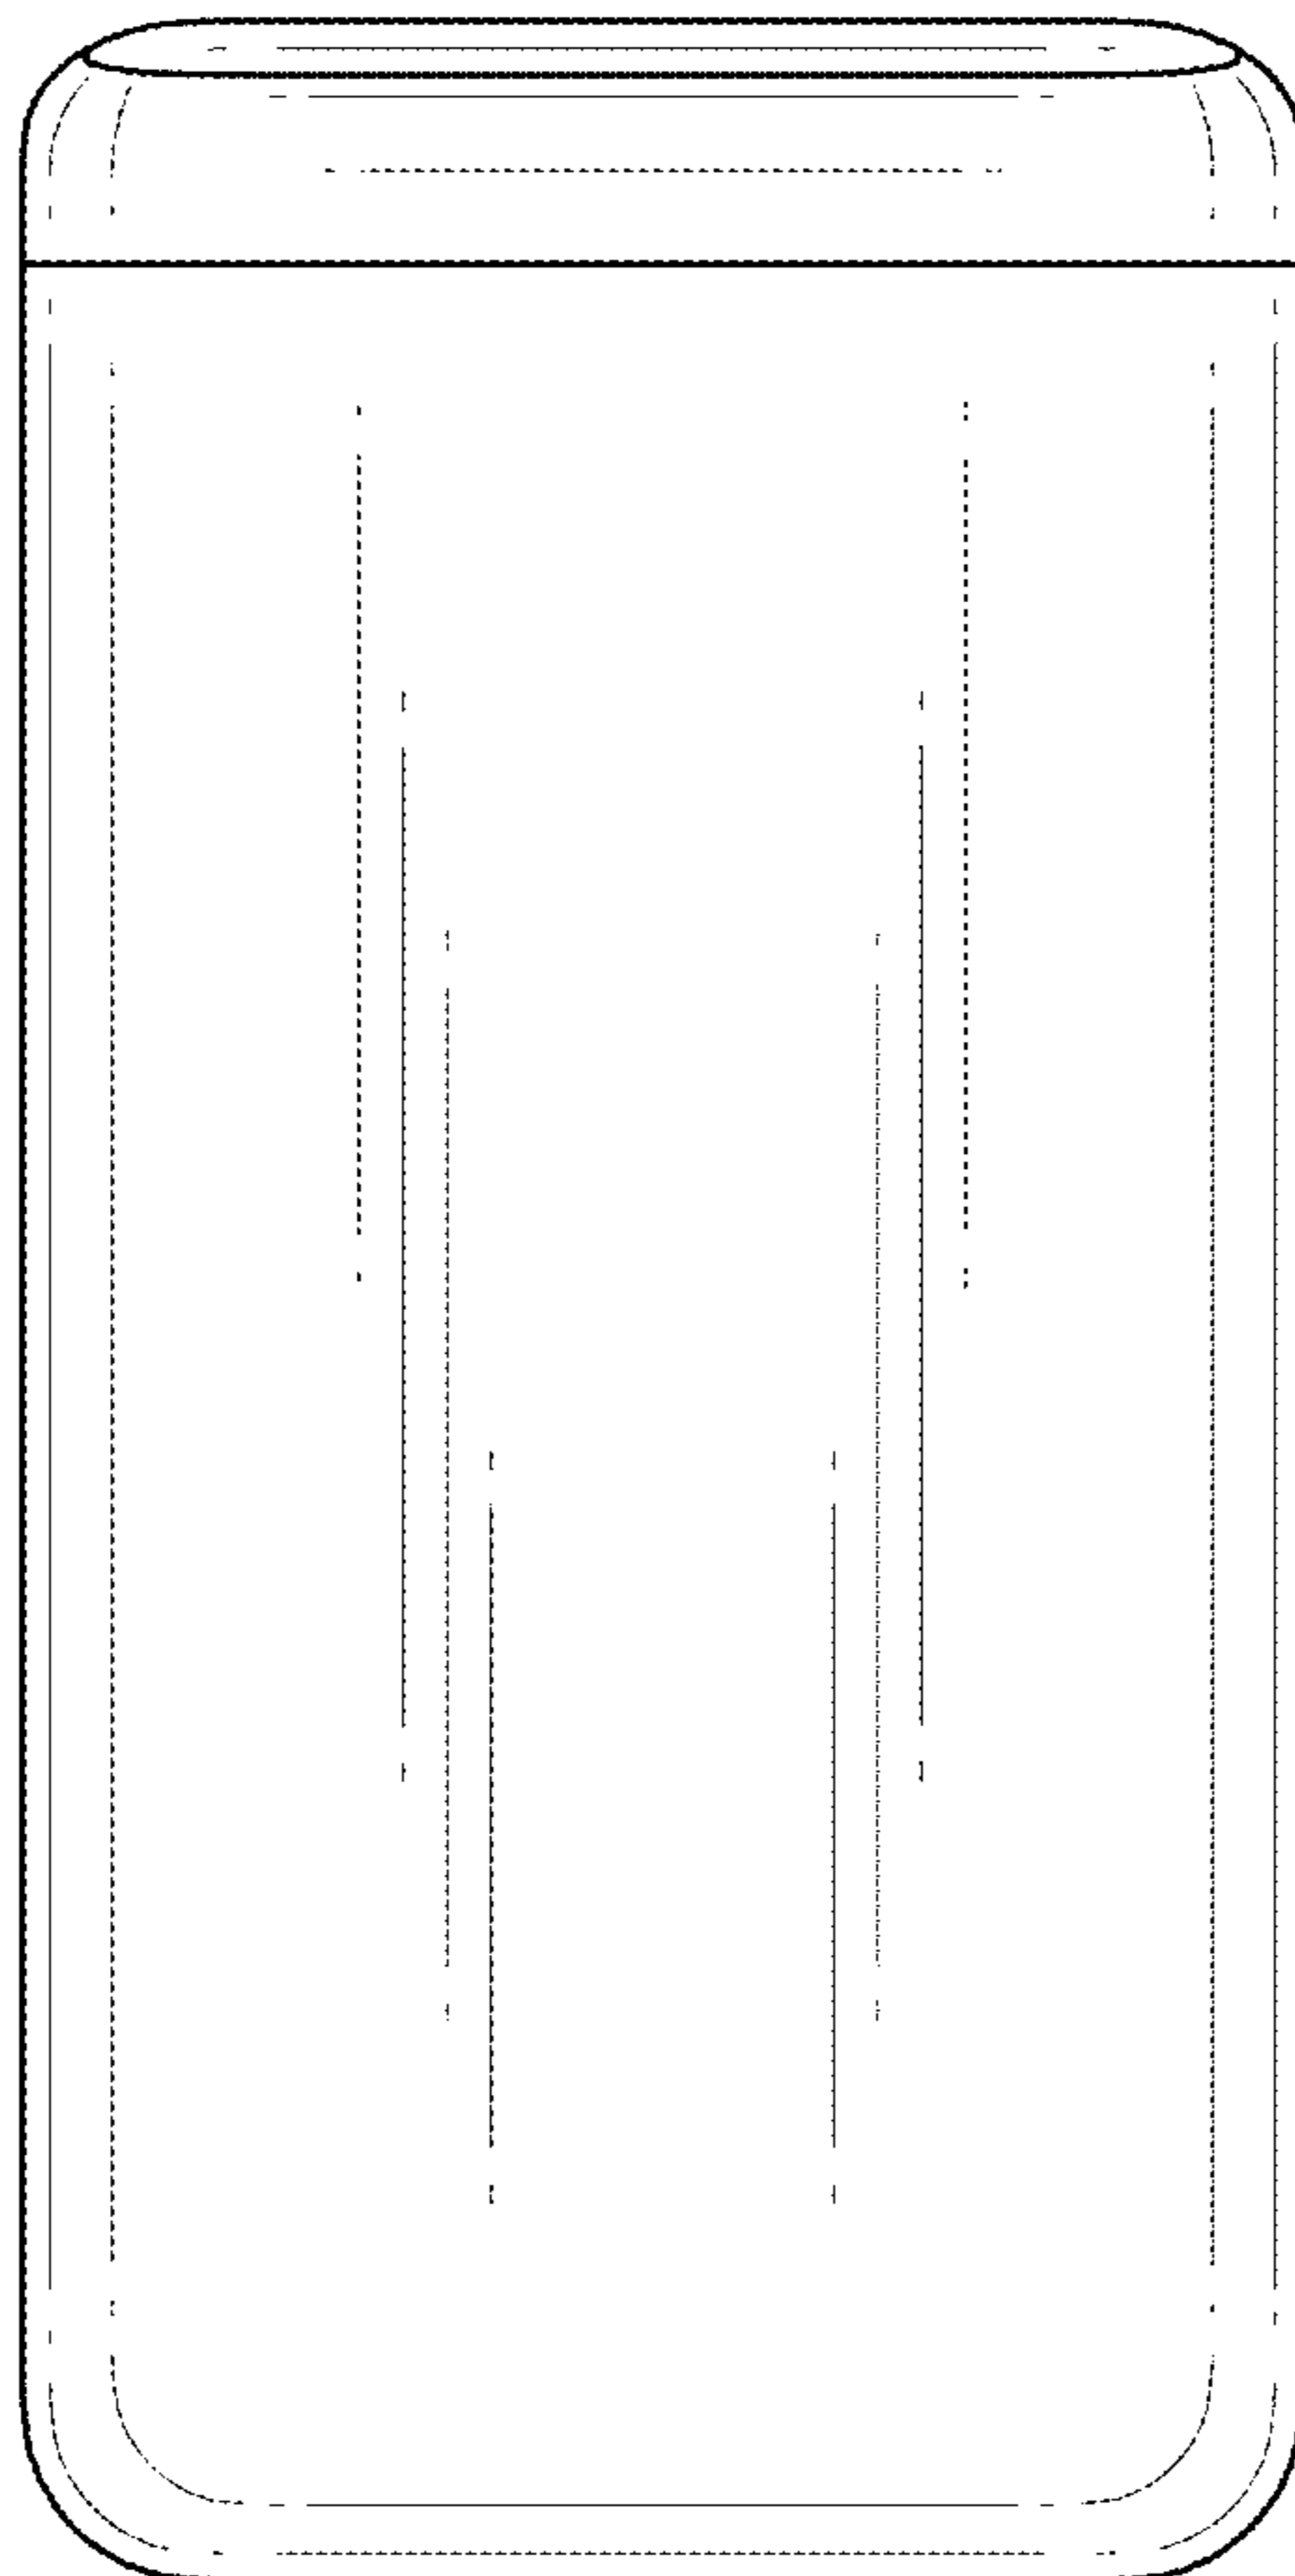


FIG. 7

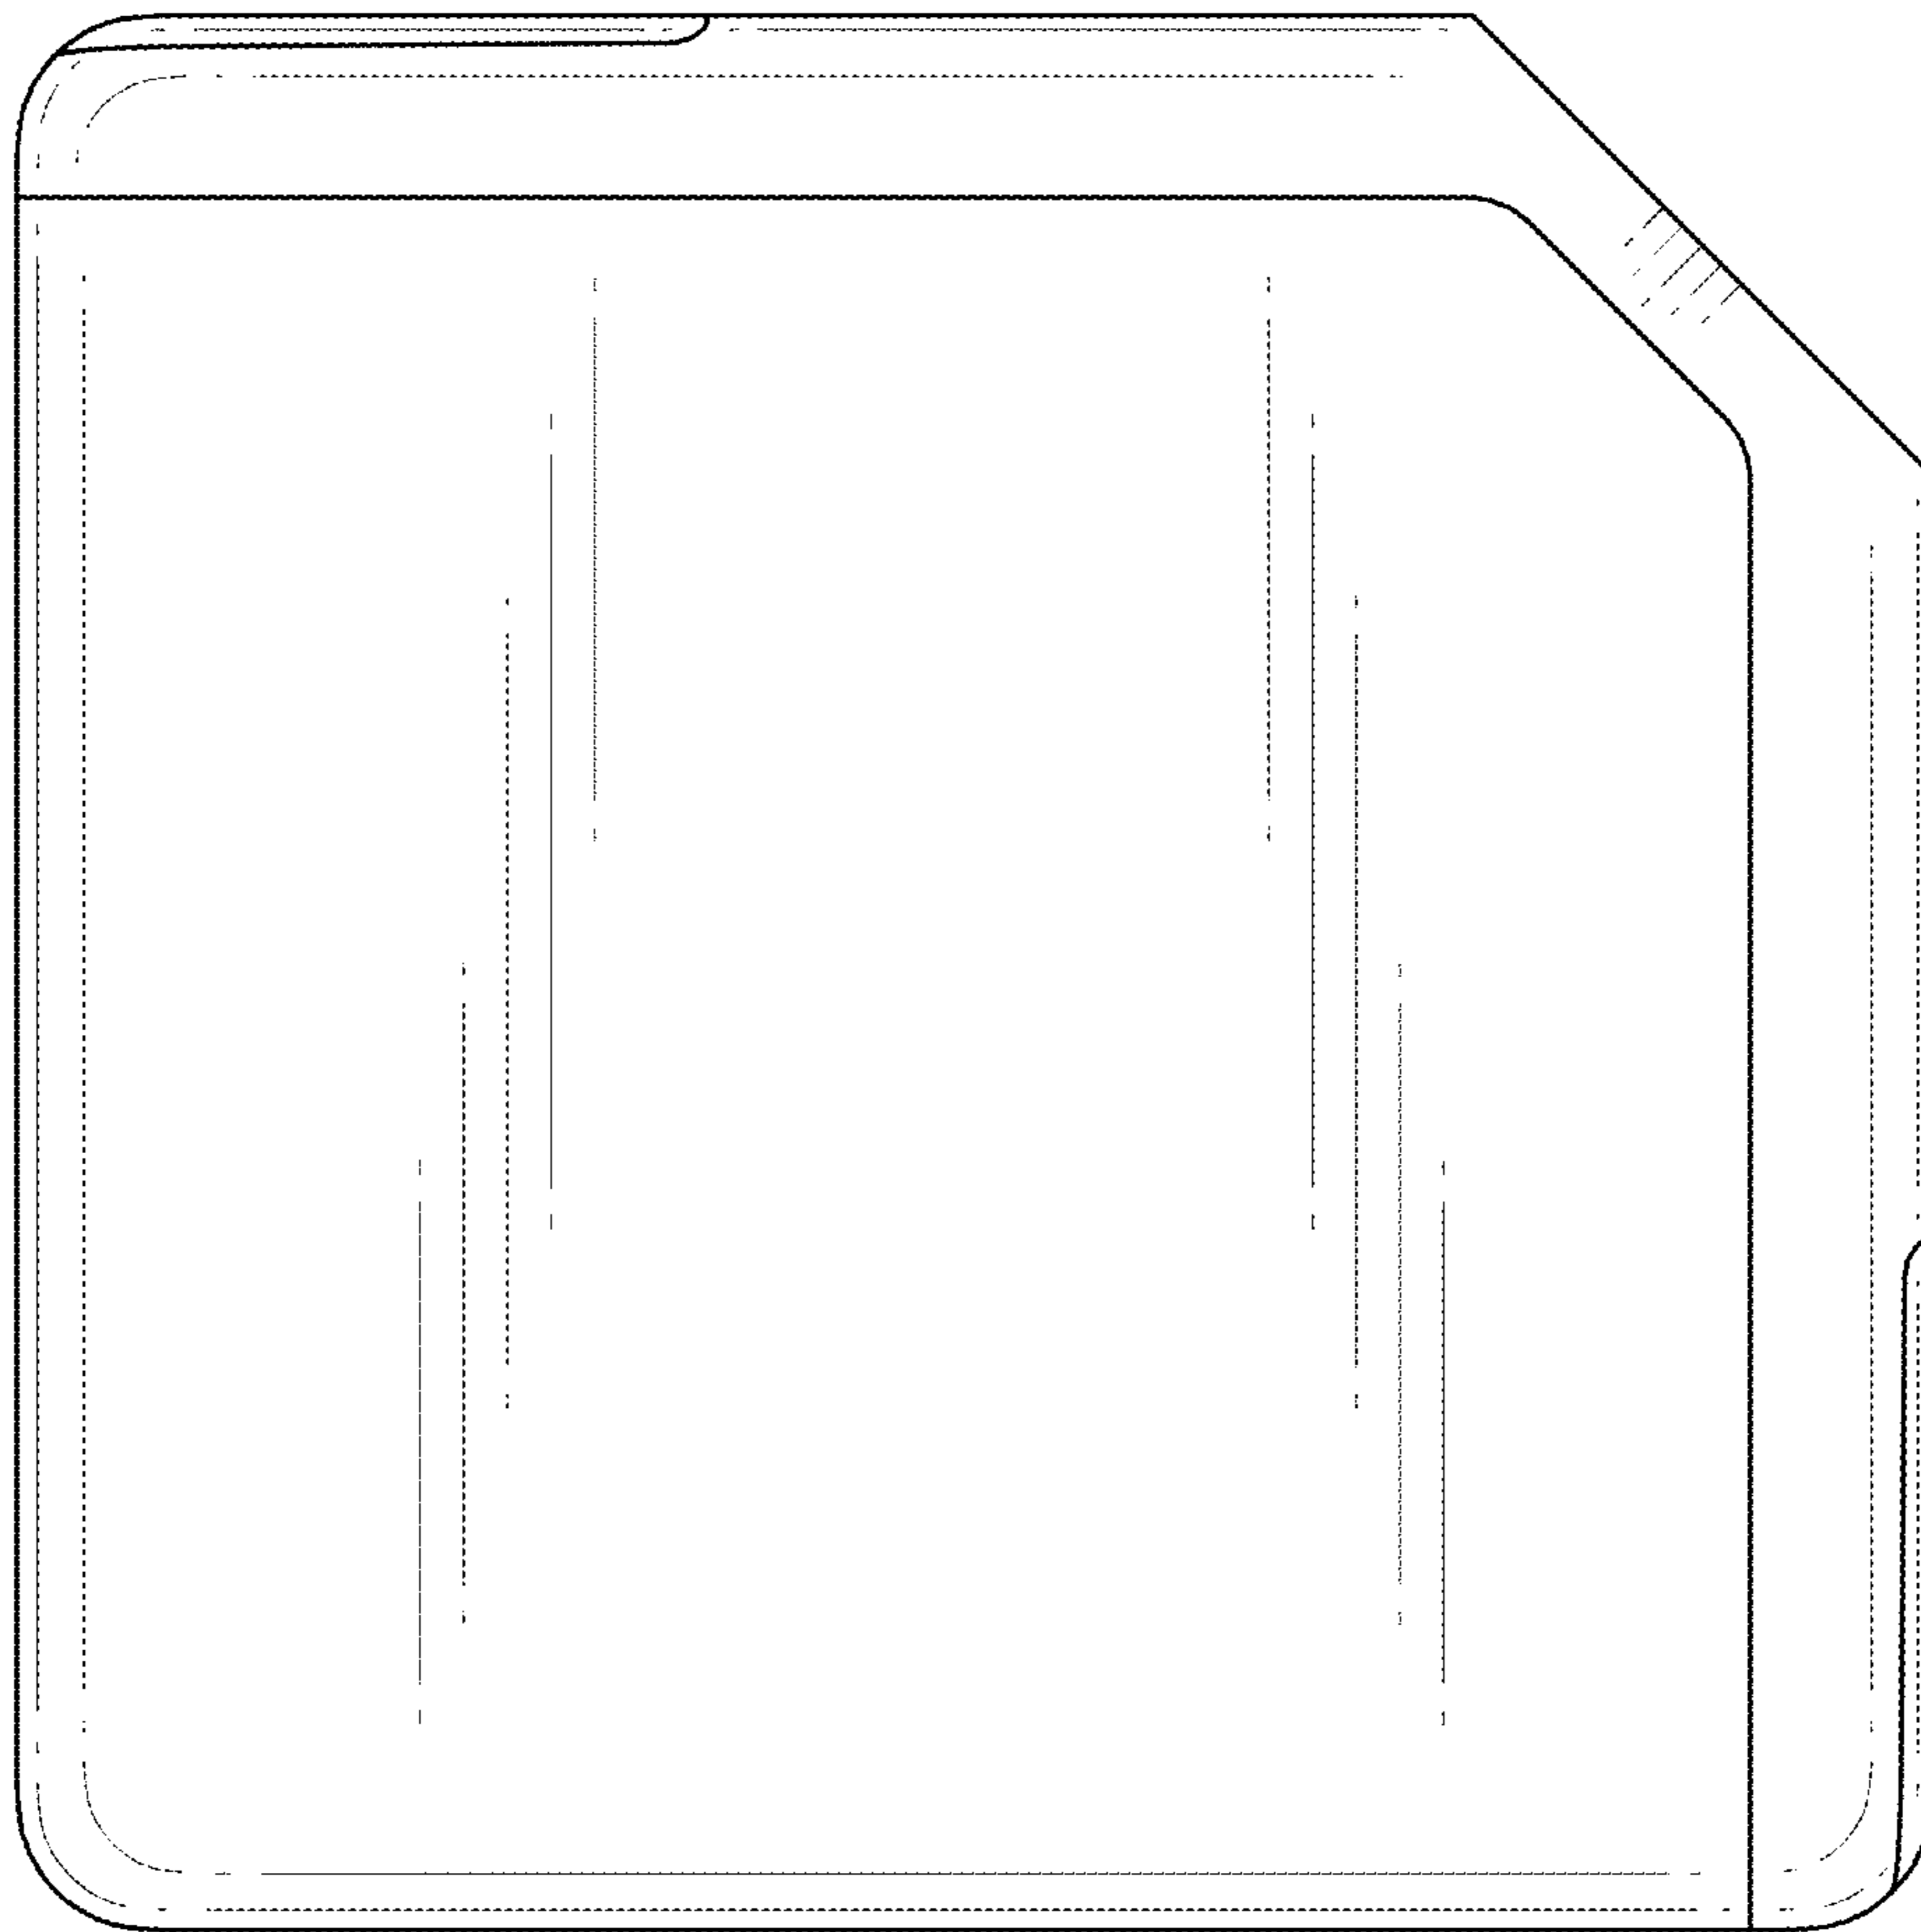


FIG. 8

