



US00D831217S

(12) **United States Design Patent**  
**Geissen**

(10) **Patent No.:** **US D831,217 S**  
(45) **Date of Patent:** **\*\* Oct. 16, 2018**

(54) **ELECTRICAL STIMULATION DEVICE**

(71) Applicant: **Sanofi**, Paris (FR)

(72) Inventor: **Julia Geissen**, Paris (FR)

(73) Assignee: **Sanofi** (FR)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/633,242**

(22) Filed: **Jan. 12, 2018**

**Related U.S. Application Data**

(62) Division of application No. 29/579,018, filed on Sep. 27, 2016, now Pat. No. Des. 816,227.

(30) **Foreign Application Priority Data**

Mar. 29, 2016 (EM) ..... 003046028-0002  
Mar. 29, 2016 (EM) ..... 003046028-0004  
Mar. 29, 2016 (EM) ..... 003046028-0006

(51) **LOC (11) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/168; D24/200**

(58) **Field of Classification Search**  
USPC ..... D24/165-168, 186, 187, 107, 200, 214;  
D10/75; D3/203.1  
CPC ..... A61N 1/39; A61N 1/3925; A61N 1/3968;  
A61N 1/3987; A61N 1/3993; A61N  
1/046; A61N 1/0484; A61N 1/0492  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D409,752 S 5/1999 Bishay et al.  
D414,266 S \* 9/1999 Pastrick ..... D24/168  
D467,661 S \* 12/2002 Buckley ..... D24/187  
6,782,293 B2 8/2004 Dupelle et al.  
D498,848 S 11/2004 Vaisnys et al.

D615,209 S 5/2010 Minogue et al.  
D639,437 S 6/2011 Bishay et al.  
D670,396 S \* 11/2012 Doogan ..... D24/200  
8,463,388 B2 6/2013 Wei  
9,211,399 B2 12/2015 Tsumura et al.  
9,439,599 B2 9/2016 Thompson et al.  
(Continued)

**FOREIGN PATENT DOCUMENTS**

BR MU8901002 2/2011  
CN 101648051 2/2010  
(Continued)

**OTHER PUBLICATIONS**

Painmaster, Micro Current Therapy Unit, available at least as early as Mar. 9, 2016, 2 pages.  
(Continued)

*Primary Examiner* — Anhdao Doan  
*Assistant Examiner* — Mary Shannon Malley  
(74) *Attorney, Agent, or Firm* — Saidman DesignLaw Group, LLC


(57) **CLAIM**

The ornamental design for an electrical stimulation device, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of an electrical stimulation device showing my new design;  
FIG. 2 is a front view thereof;  
FIG. 3 is a rear view thereof;  
FIG. 4 is a left side view thereof;  
FIG. 5 is a right side view thereof;  
FIG. 6 is a top view thereof; and,  
FIG. 7 is a bottom view thereof.  
The broken lines show portions of the electrical stimulation device that form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

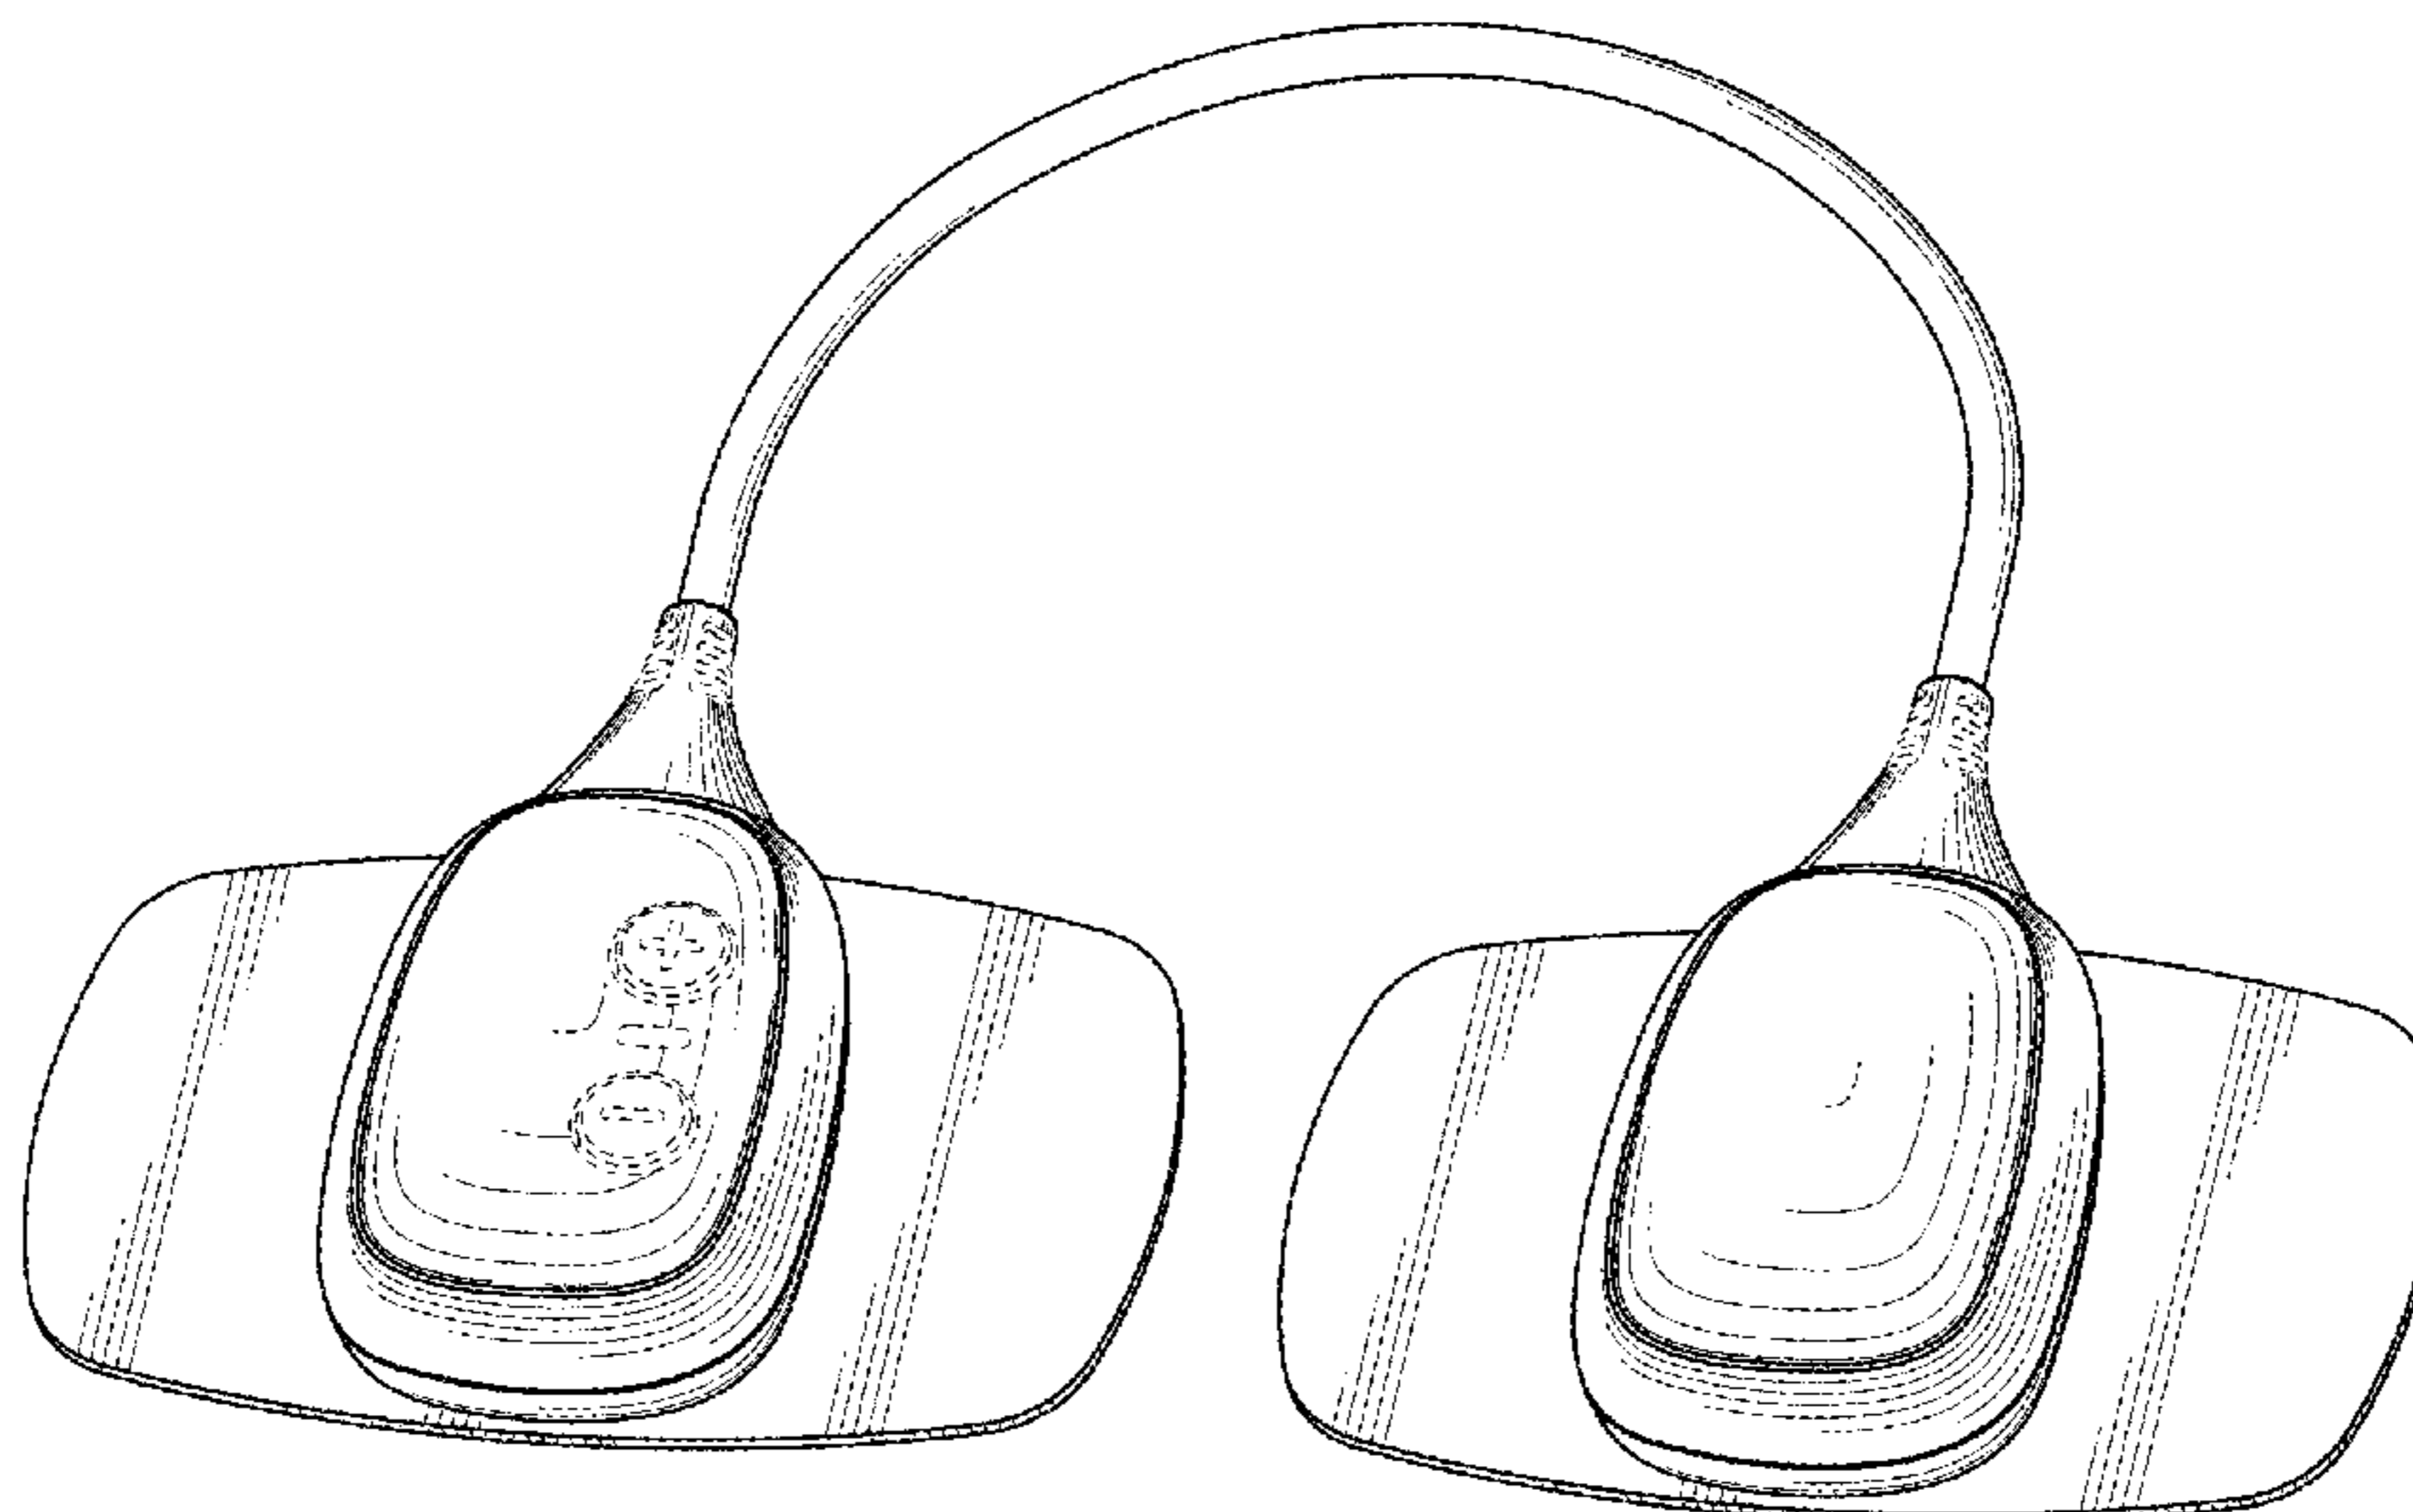

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D783,832 S 4/2017 Dascoli et al.  
D787,684 S 5/2017 Vezina  
D805,209 S \* 12/2017 Moon ..... D24/200  
D812,229 S \* 3/2018 Al-Siddiq ..... D24/167  
9,955,887 B2 \* 5/2018 Hughes ..... A61B 5/6832  
2003/0181950 A1 9/2003 Powers et al.  
2013/0226275 A1 8/2013 Duncan  
2014/0128757 A1 5/2014 Ballet et al.  
2014/0170622 A1 6/2014 Pastrick et al.

FOREIGN PATENT DOCUMENTS

CN 102198309 9/2011  
CN 202605531 12/2012  
CN 203183518 9/2013  
DE 202010008165 10/2010  
EP 2263744 12/2010  
EP 2392381 12/2011  
GB 2478787 9/2011  
RU 124157 1/2013  
TW M263115 5/2005  
TW 201002380 1/2010  
TW 201117850 6/2011  
WO 2006/113801 10/2006  
WO 2010/144982 12/2010

OTHER PUBLICATIONS

Beurer, EM10 Back Tens to-go Mini-Pad, available at least as early as Mar. 9, 2016, 2 pages.

Sanitas, SEM05 Mini-Pad Tens, available at least as early as Mar. 9, 2016, 2 pages.

\* cited by examiner

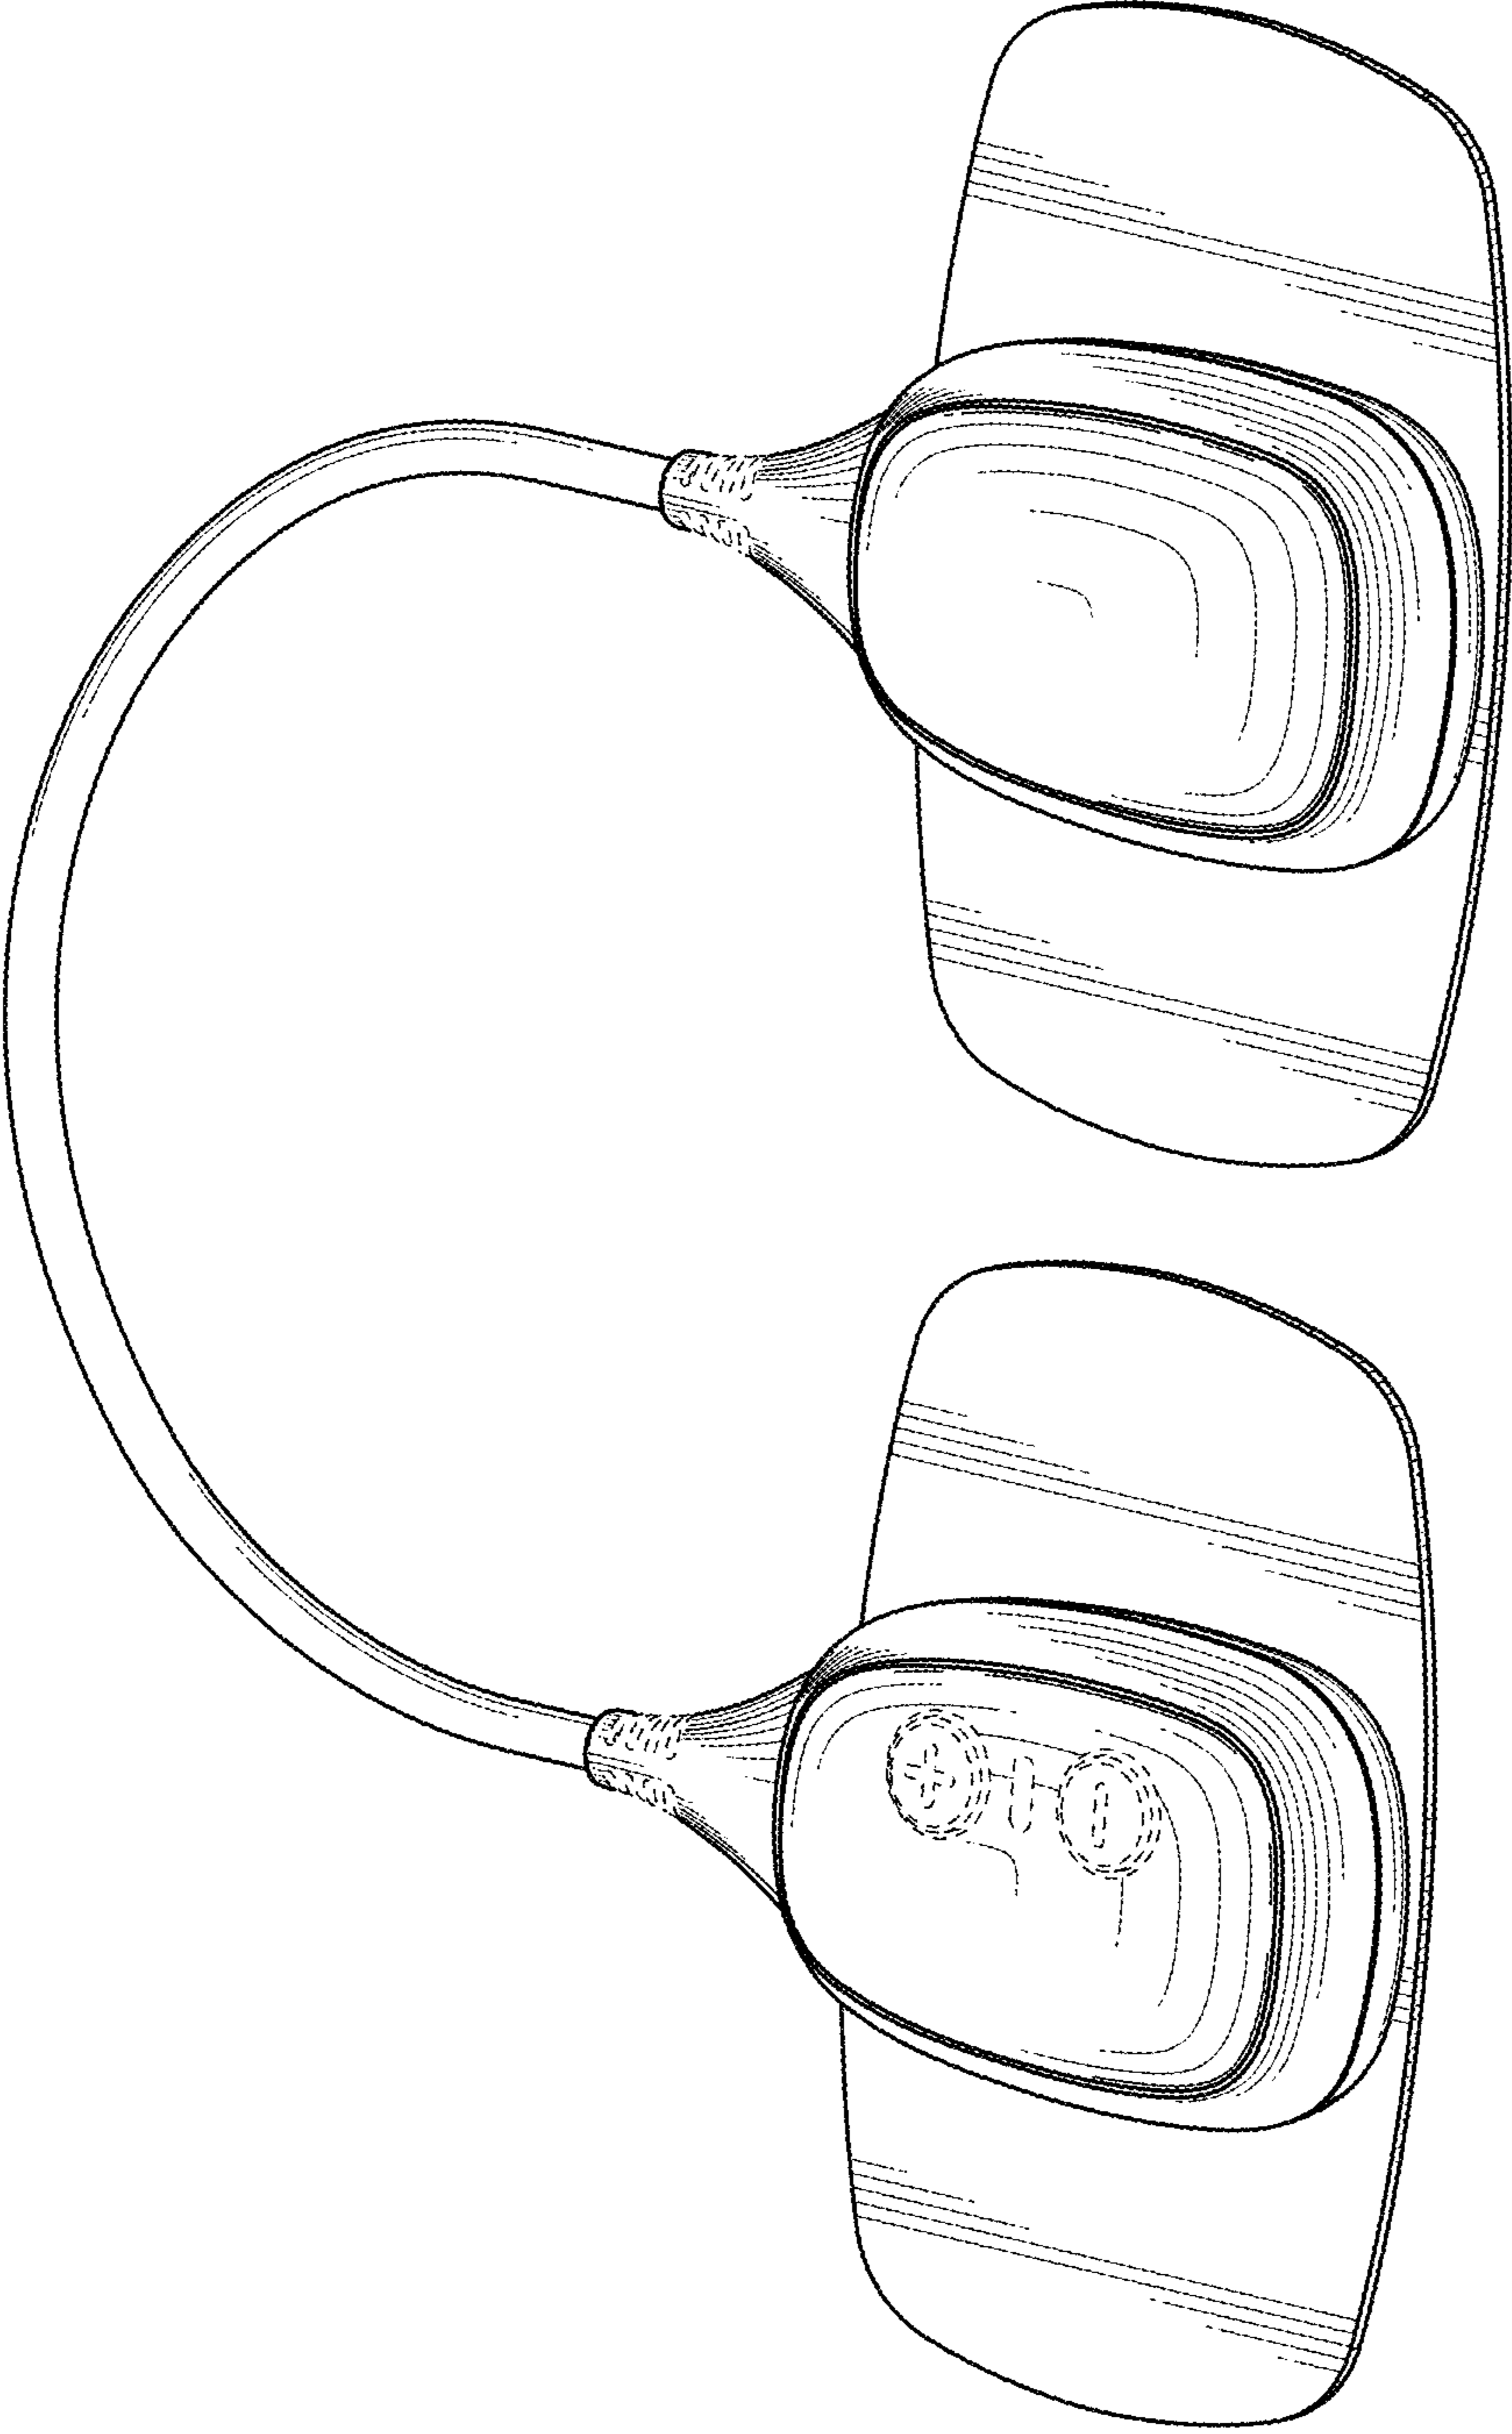


FIG. 1

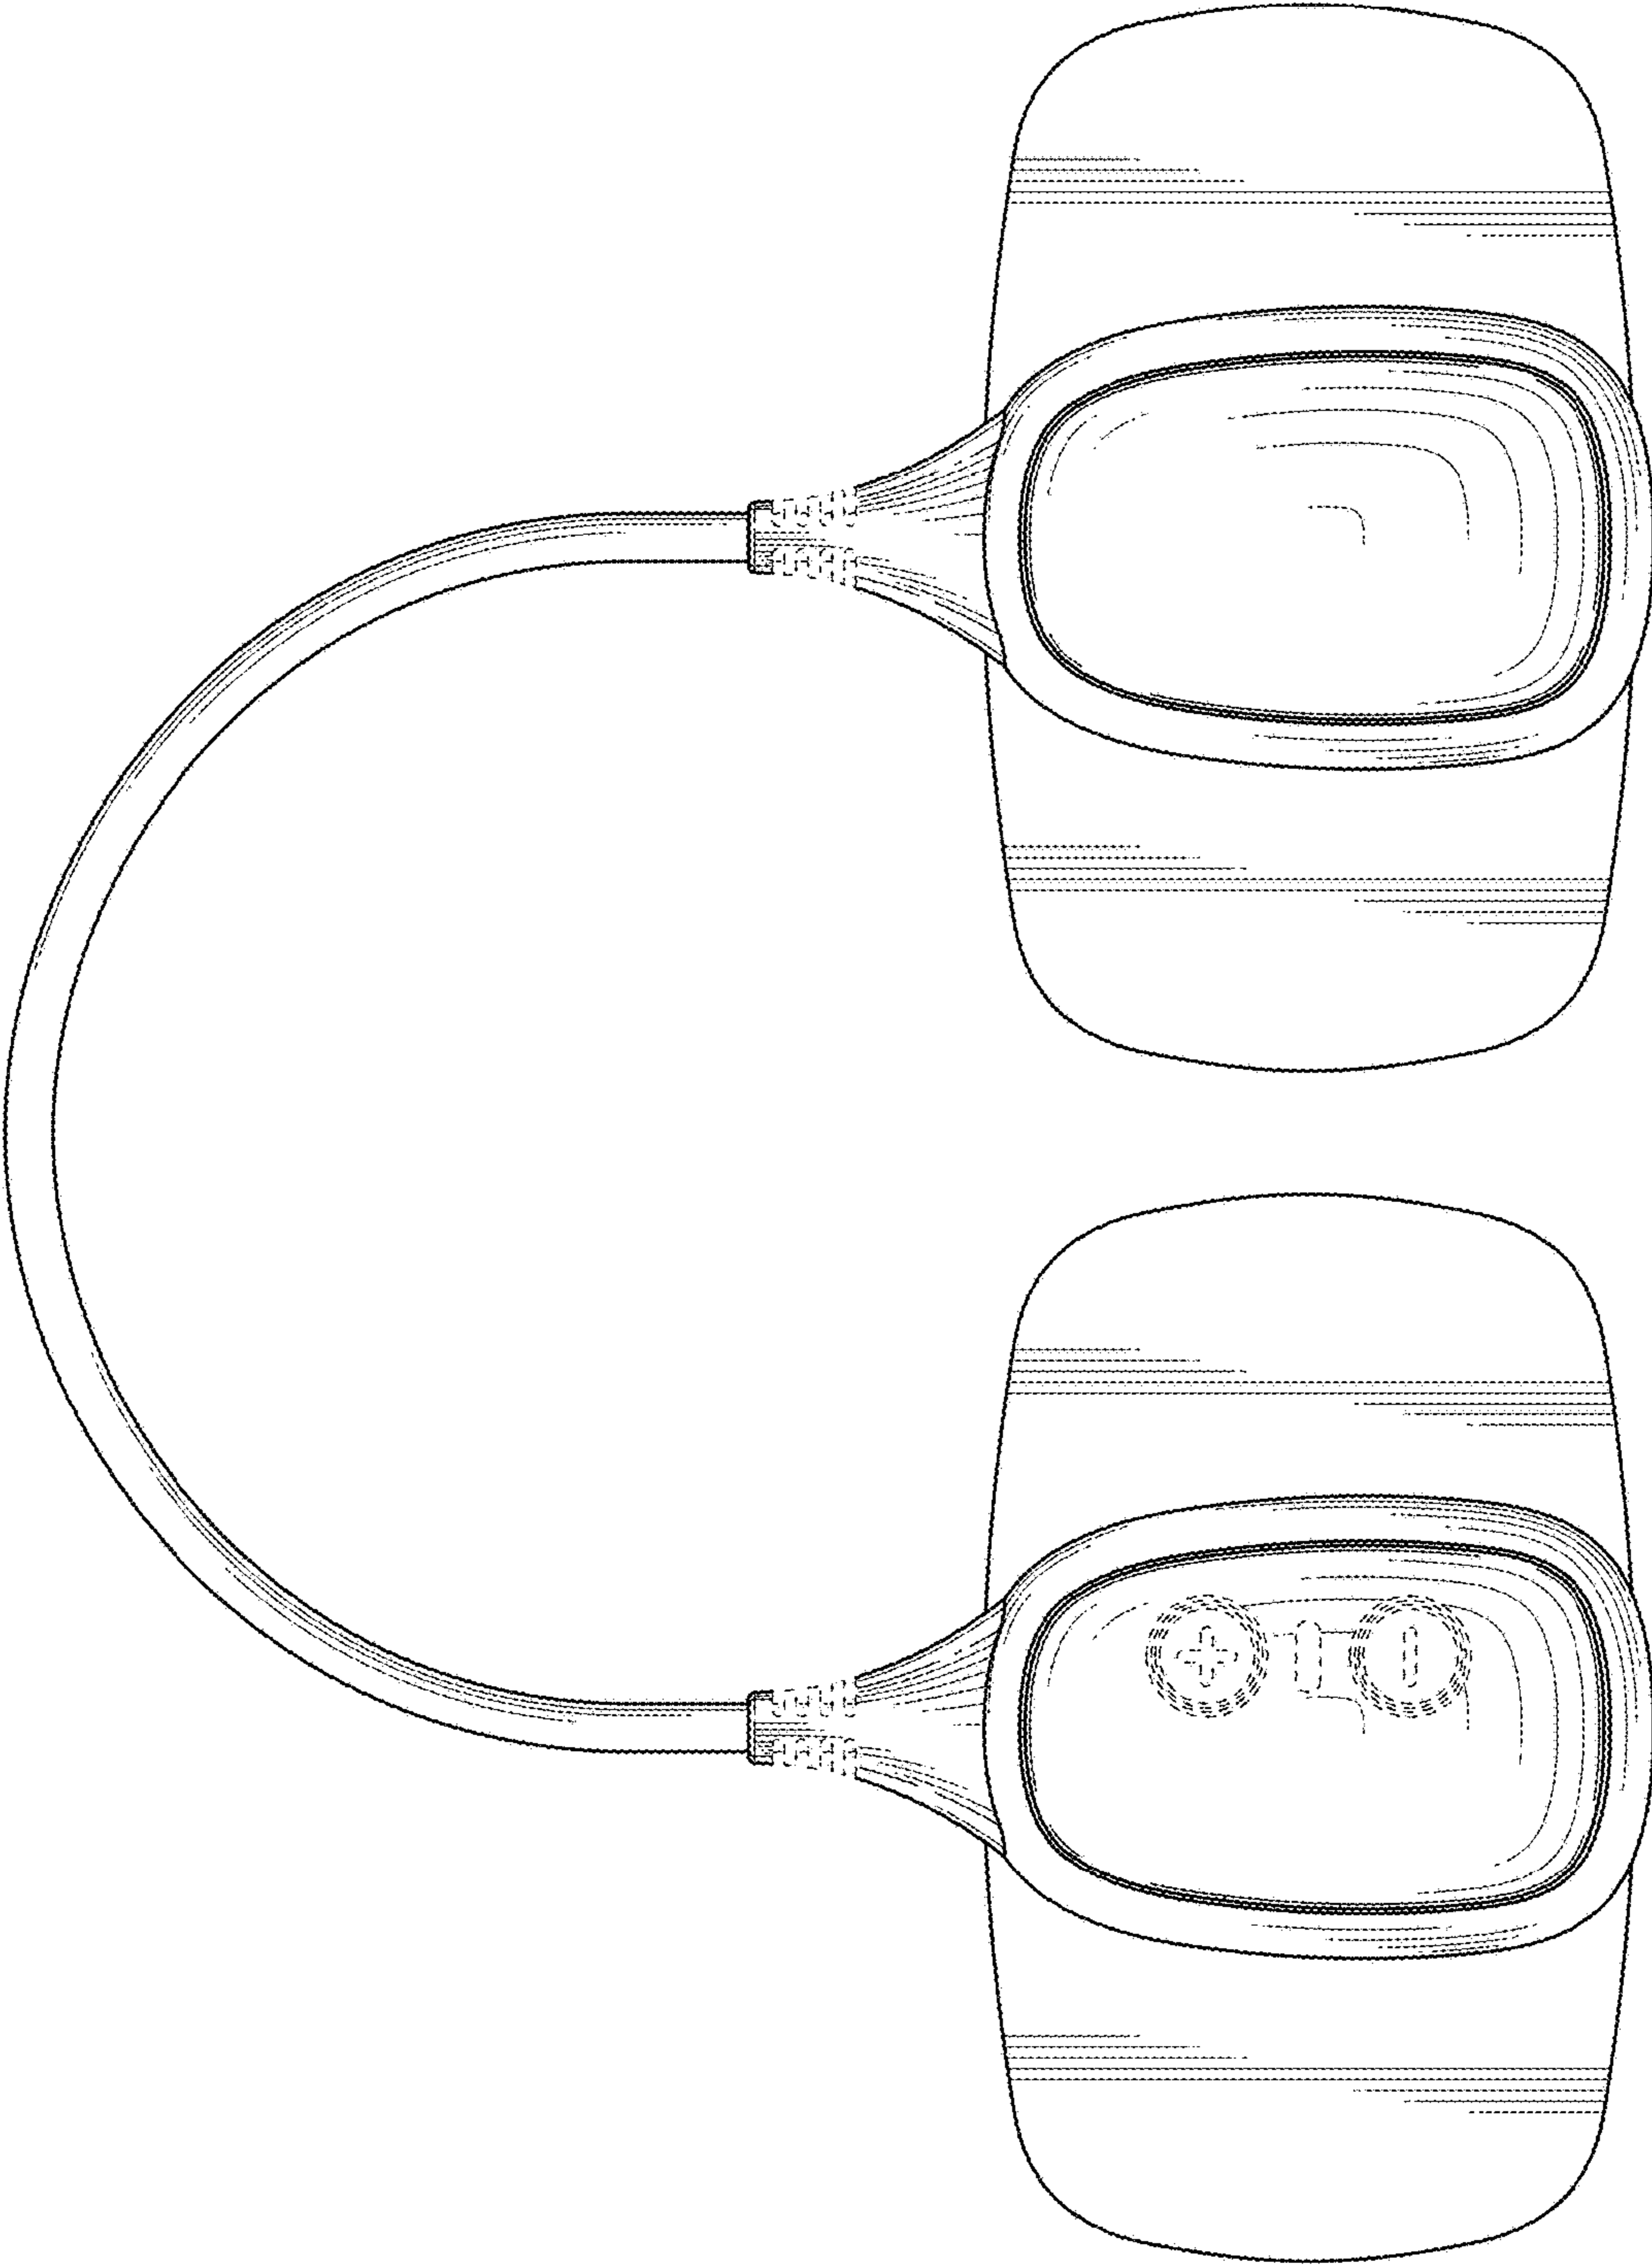


FIG. 2

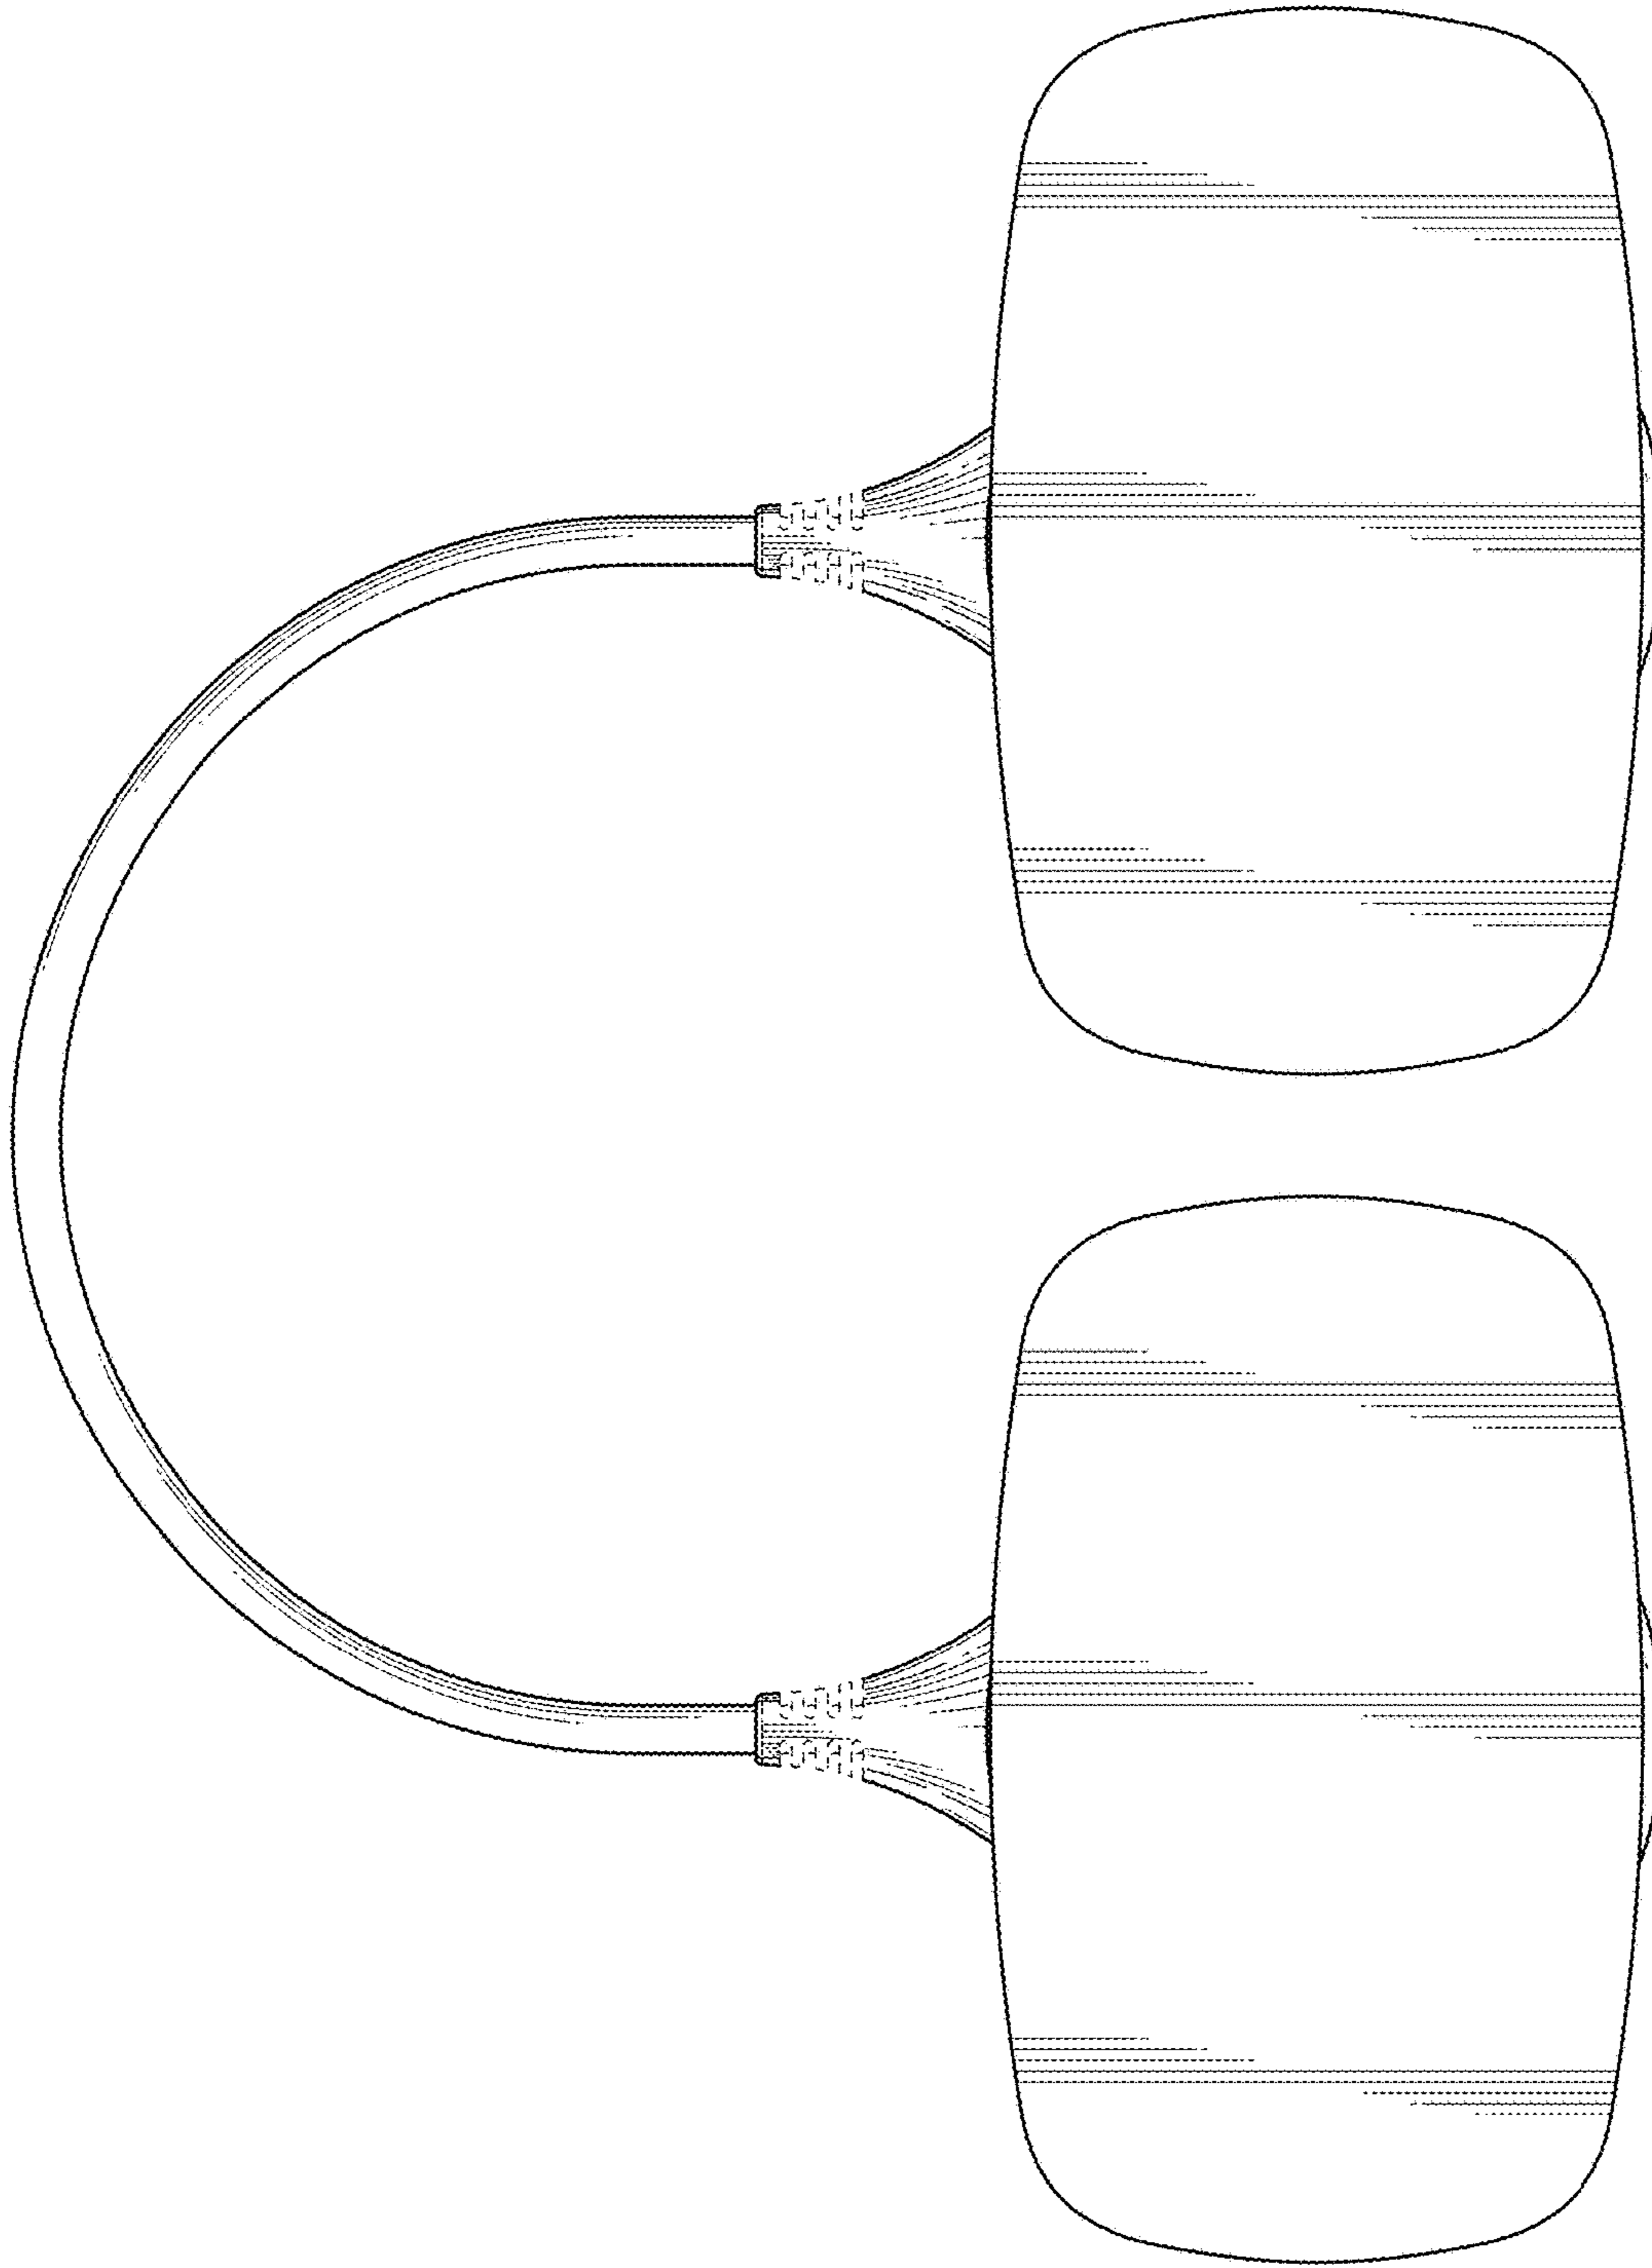


FIG. 3

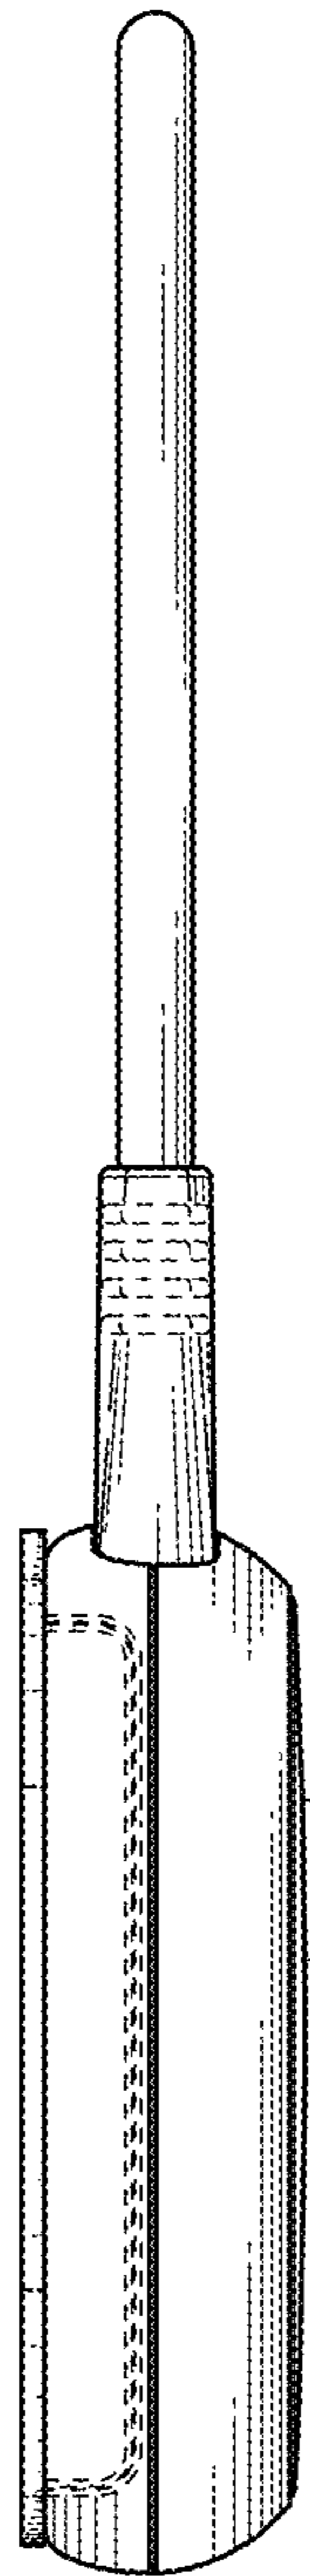


FIG. 4

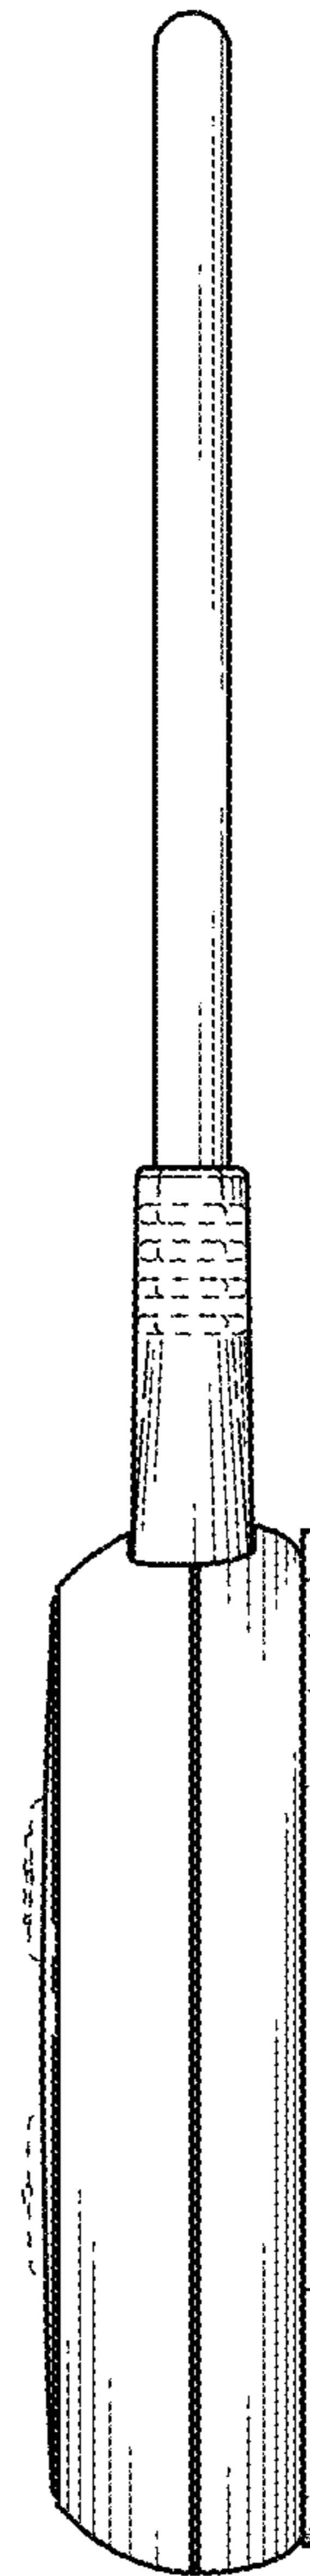


FIG. 5

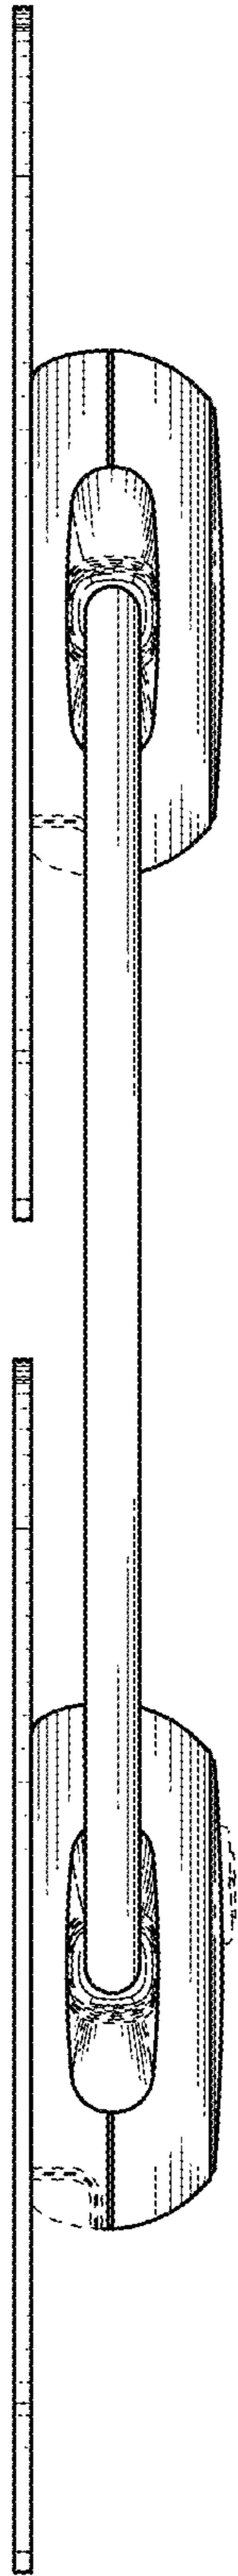


FIG. 6

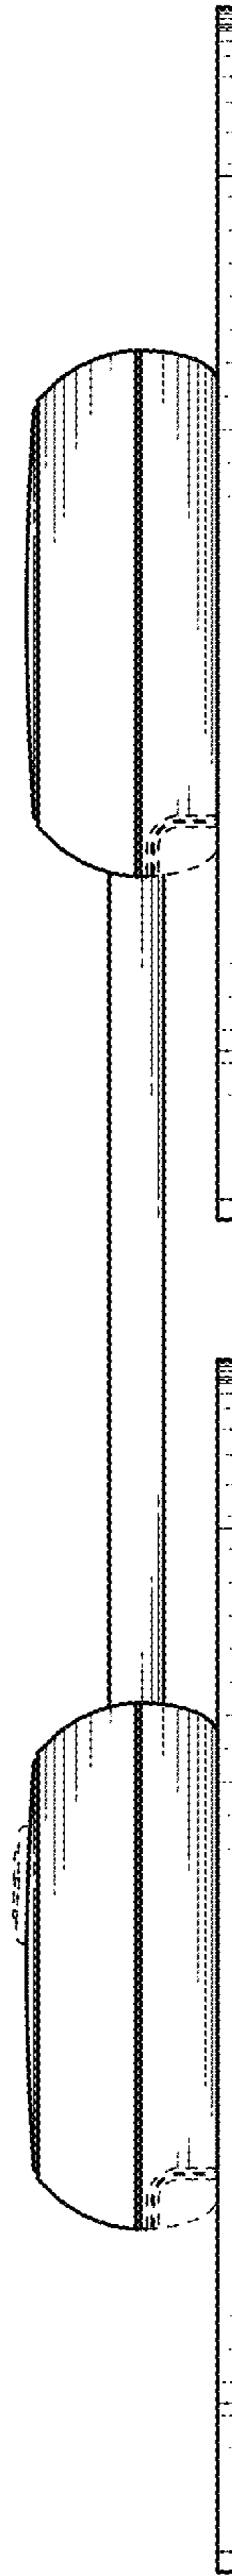


FIG. 7