



US00D834184S

(12) **United States Design Patent** (10) **Patent No.:** **US D834,184 S**
Anderson (45) **Date of Patent:** **** Nov. 20, 2018**

(54) **INSERTION DEVICE WITHOUT A DISTAL OPENING**

(71) Applicant: **Robert G. Anderson**, Aledo, TX (US)

(72) Inventor: **Robert G. Anderson**, Aledo, TX (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/573,482**

(22) Filed: **Aug. 5, 2016**

(51) **LOC (11) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/115**

(58) **Field of Classification Search**
USPC D24/121, 123, 224; 604/317-325; 623/8
CPC A61F 2/12; B65D 41/04; B65D 2251/023;
B65D 41/0485; B65D 41/3428
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,641,648	A	2/1987	Shapiro	
4,990,145	A *	2/1991	Fleury	A61G 9/006 604/317
4,995,906	A	2/1991	Iwasaki et al.	
5,322,071	A *	6/1994	Ambrose	A61B 46/00 128/849
5,571,178	A	11/1996	Ledergerber	
5,584,884	A *	12/1996	Pignataro	A61F 2/12 606/151
5,723,006	A	3/1998	Ledergerber	
5,782,913	A	7/1998	Schindler et al.	
5,897,590	A *	4/1999	Donovan	A61F 13/36 606/190
8,136,175	B1 *	3/2012	Fagundes	A61B 10/0038 4/479
8,206,443	B2	6/2012	Preissman	
8,211,173	B2 *	7/2012	Keller	A61F 2/12 600/185
8,313,760	B2	11/2012	Hunter	
D672,051	S *	12/2012	Rannikko	D24/224

8,550,090	B2	10/2013	Keller et al.	
8,555,893	B2	10/2013	Keller et al.	
8,641,758	B1	2/2014	Anderson	
D707,353	S *	6/2014	Carr	D24/123
D726,309	S *	4/2015	Wood	D24/121
D731,052	S *	6/2015	Doerr	D24/121
D736,372	S	8/2015	Anderson	
D738,490	S	9/2015	Anderson	
D742,509	S	11/2015	Anderson	

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO/2013/122568 A1 8/2013

OTHER PUBLICATIONS

Richard A. Mladick, M.D., F.A.C.S. "No-Touch" Submuscular Saline Breast Augmentation Technique, *Aesthetic Plastic Surgery*, 17:183-192, 1993, New York, NY.

(Continued)

Primary Examiner — David Muller

(74) *Attorney, Agent, or Firm* — Kirby Drake


(57) **CLAIM**

The ornamental design of an insertion device, without a distal opening.

DESCRIPTION

FIG. 1: Top side perspective view of an ornamental design for an insertion device without a distal opening;
FIG. 2: Top view of an ornamental design for an insertion device without a distal opening;
FIG. 3: Bottom view of an ornamental design for an insertion device without a distal opening;
FIG. 4: Right side view thereof;
FIG. 5: Left side view thereof;
FIG. 6: First end view thereof; and,
FIG. 7: Second end view thereof.

1 Claim, 3 Drawing Sheets

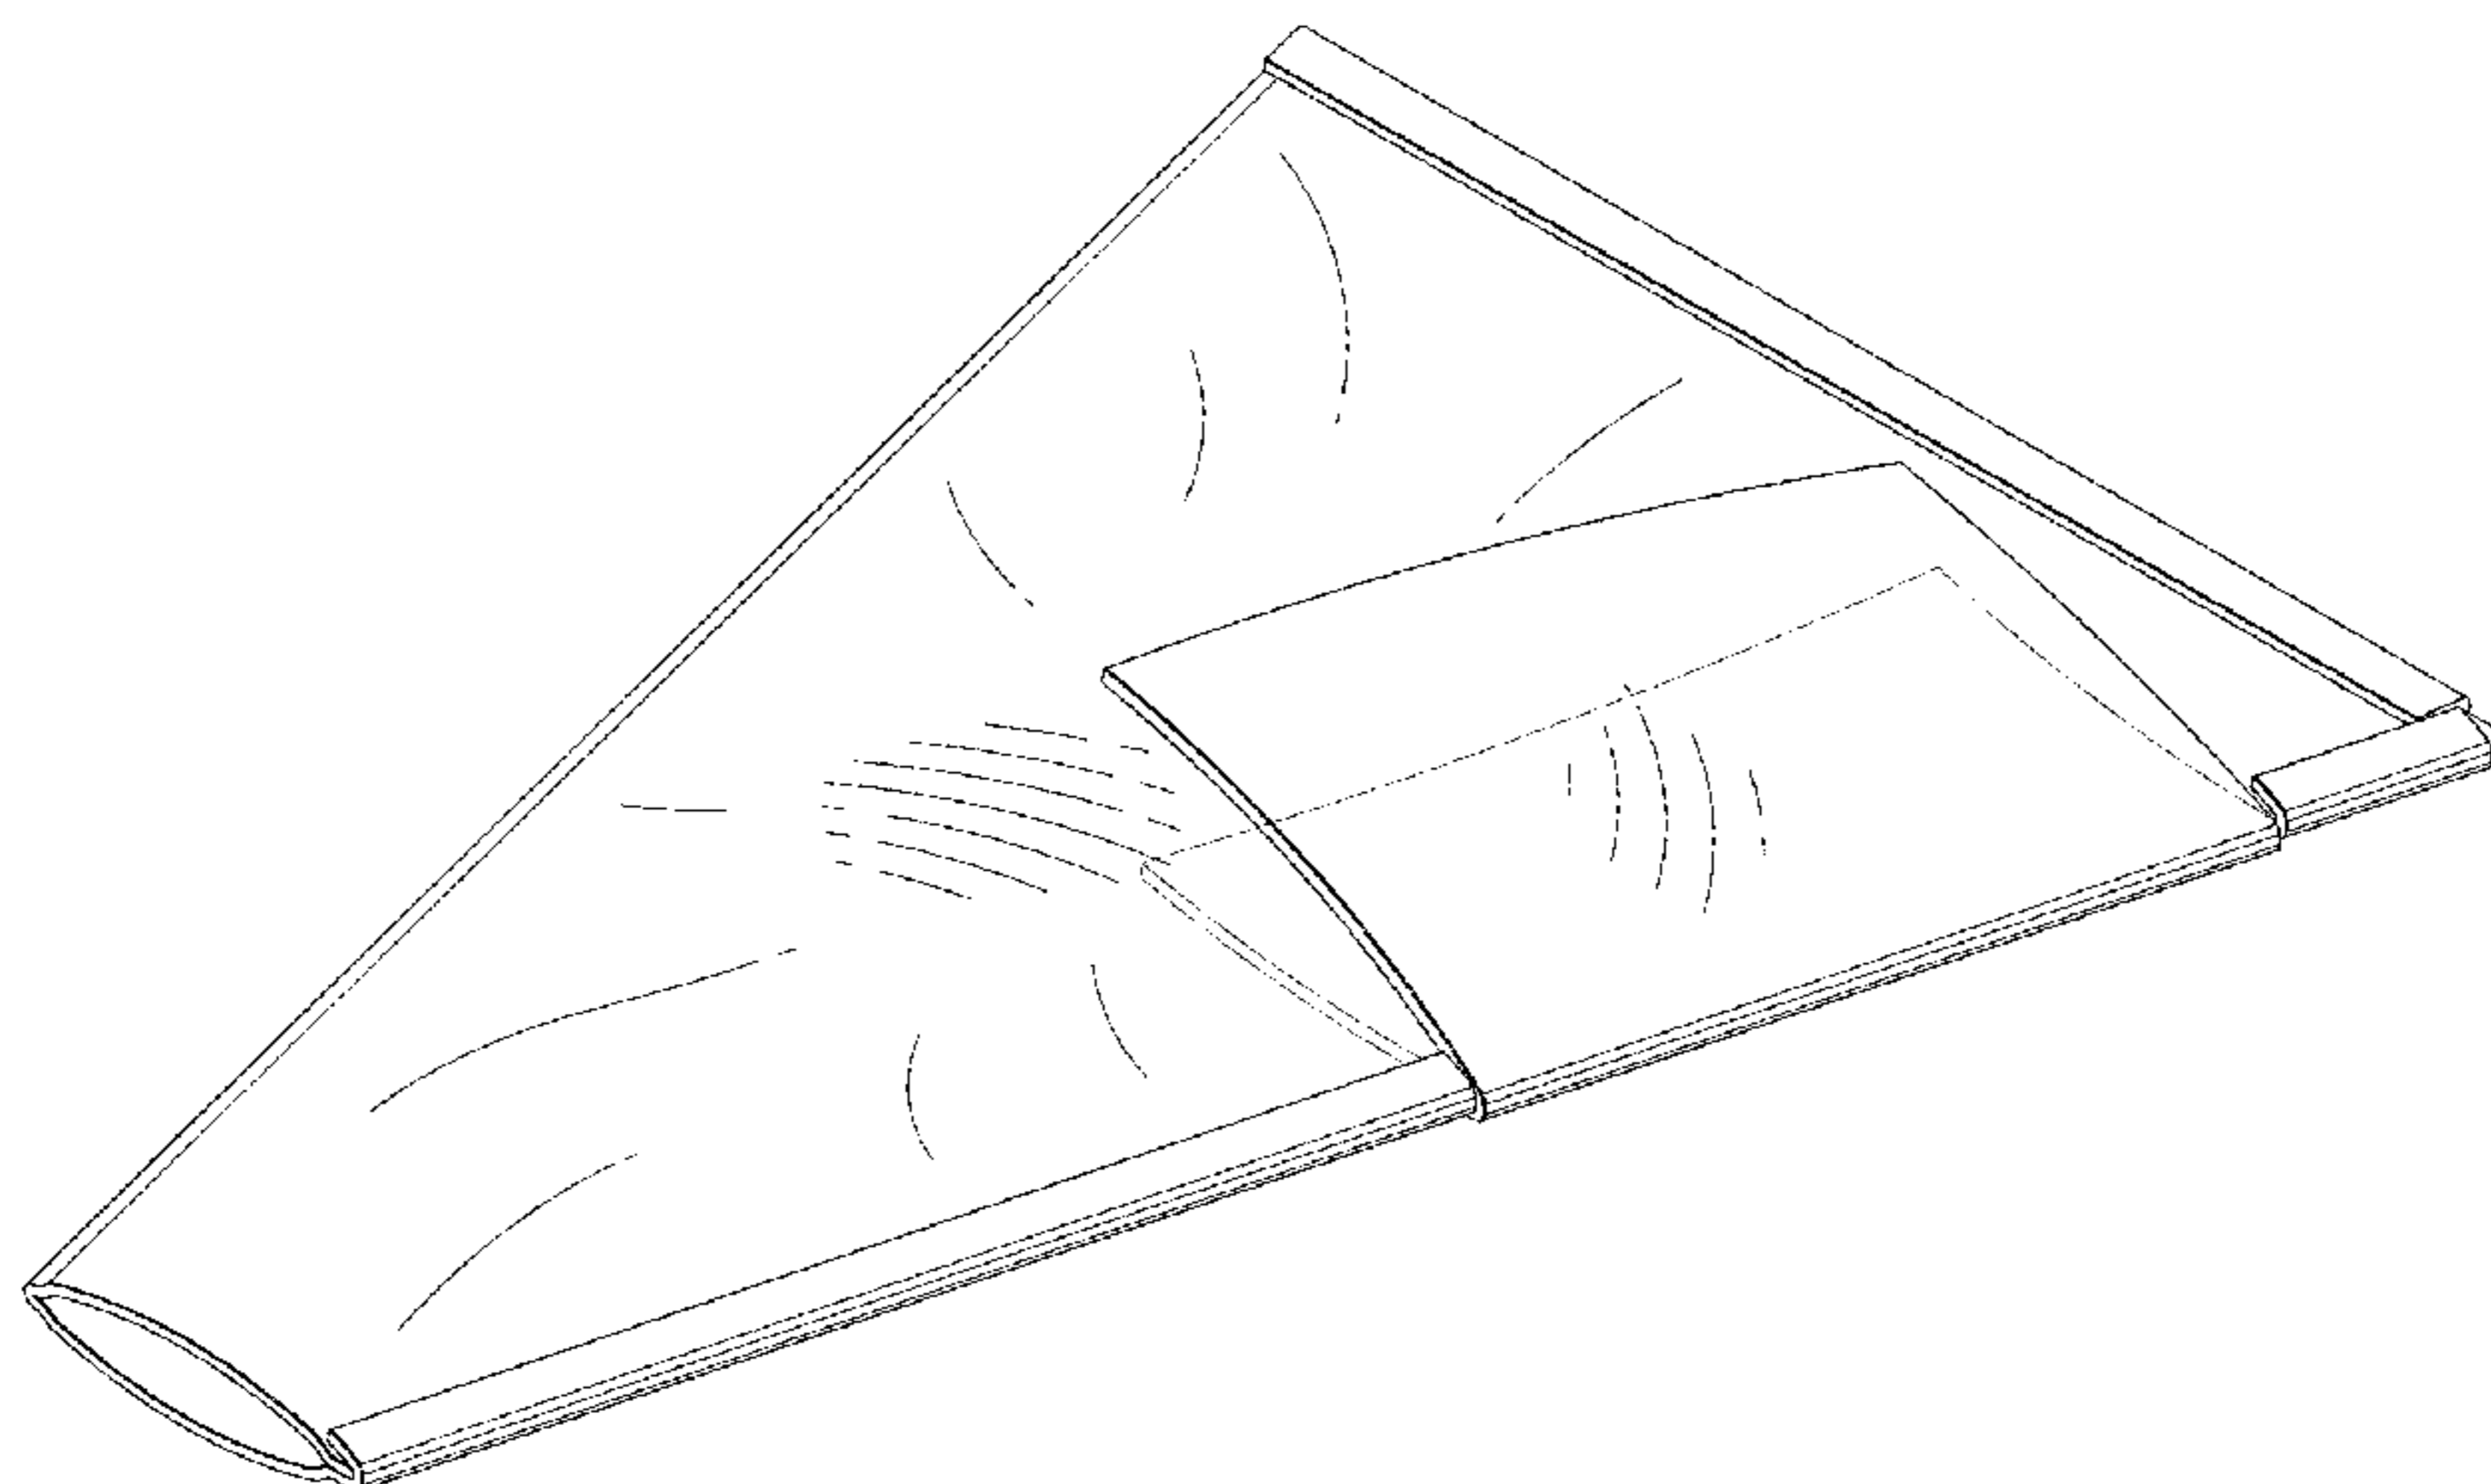

(56)

References Cited

U.S. PATENT DOCUMENTS

D752,739	S	3/2016	Anderson	
D773,652	S *	12/2016	Anderson D24/115
D775,725	S *	1/2017	Anderson D24/115
D776,806	S *	1/2017	Anderson D24/115
2007/0276484	A1	11/2007	Abell et al.	
2009/0204107	A1	8/2009	Keller et al.	
2010/0280610	A1	11/2010	Preissman	
2011/0035003	A1	2/2011	Preissman	
2011/0218624	A1	9/2011	Preissman	
2012/0185042	A1	7/2012	Preissman	
2012/0259414	A1	10/2012	Preissman	
2013/0073040	A1	3/2013	Preissman	
2014/0074235	A1	3/2014	Keller et al.	
2014/0074236	A1	3/2014	Keller et al.	
2014/0148901	A1	5/2014	Anderson	
2015/0126812	A1	5/2015	Anderson	
2015/0374478	A1	12/2015	Anderson	
2016/0038275	A1	2/2016	Preissman	
2016/0095697	A1	4/2016	Anderson	

OTHER PUBLICATIONS


Richard A. Mladick, M.D., F.A.C.S. Significance of *Staphylococcus* epidermidis Causing Subclinical Infection, *Plastic & Reconstructive Surgery*: Apr. 15, 2005—vol. 115—Issue 5—pp. 1426-1427, Virginia Beach, VA.

Richard A. Mladick, M.D., F.A.C.S. Prevention of Capsular Contracture, *Plastic & Reconstructive Surgery*: May 1999—vol. 103—Issue 6—pp. 1773-1774, Virginia Beach, VA.

Thomas M. Biggs, M.D. Prefilled Saline Breast Implants Offer Significant Advantages, *Aesthetic Surgery Journal* Sep. 1999 vol. 19 No. 5 424, St Louis, MO.

“Mitchel H. Brown, M.D., M.Ed. Cohesive Silicone Gel Breast Implants in Aesthetic and Reconstructive Breast Surgery, *Plastic & Reconstructive Surgery*: Sep. 1, 2005—vol. 116—Issue 3—pp. 768-779”.

* cited by examiner

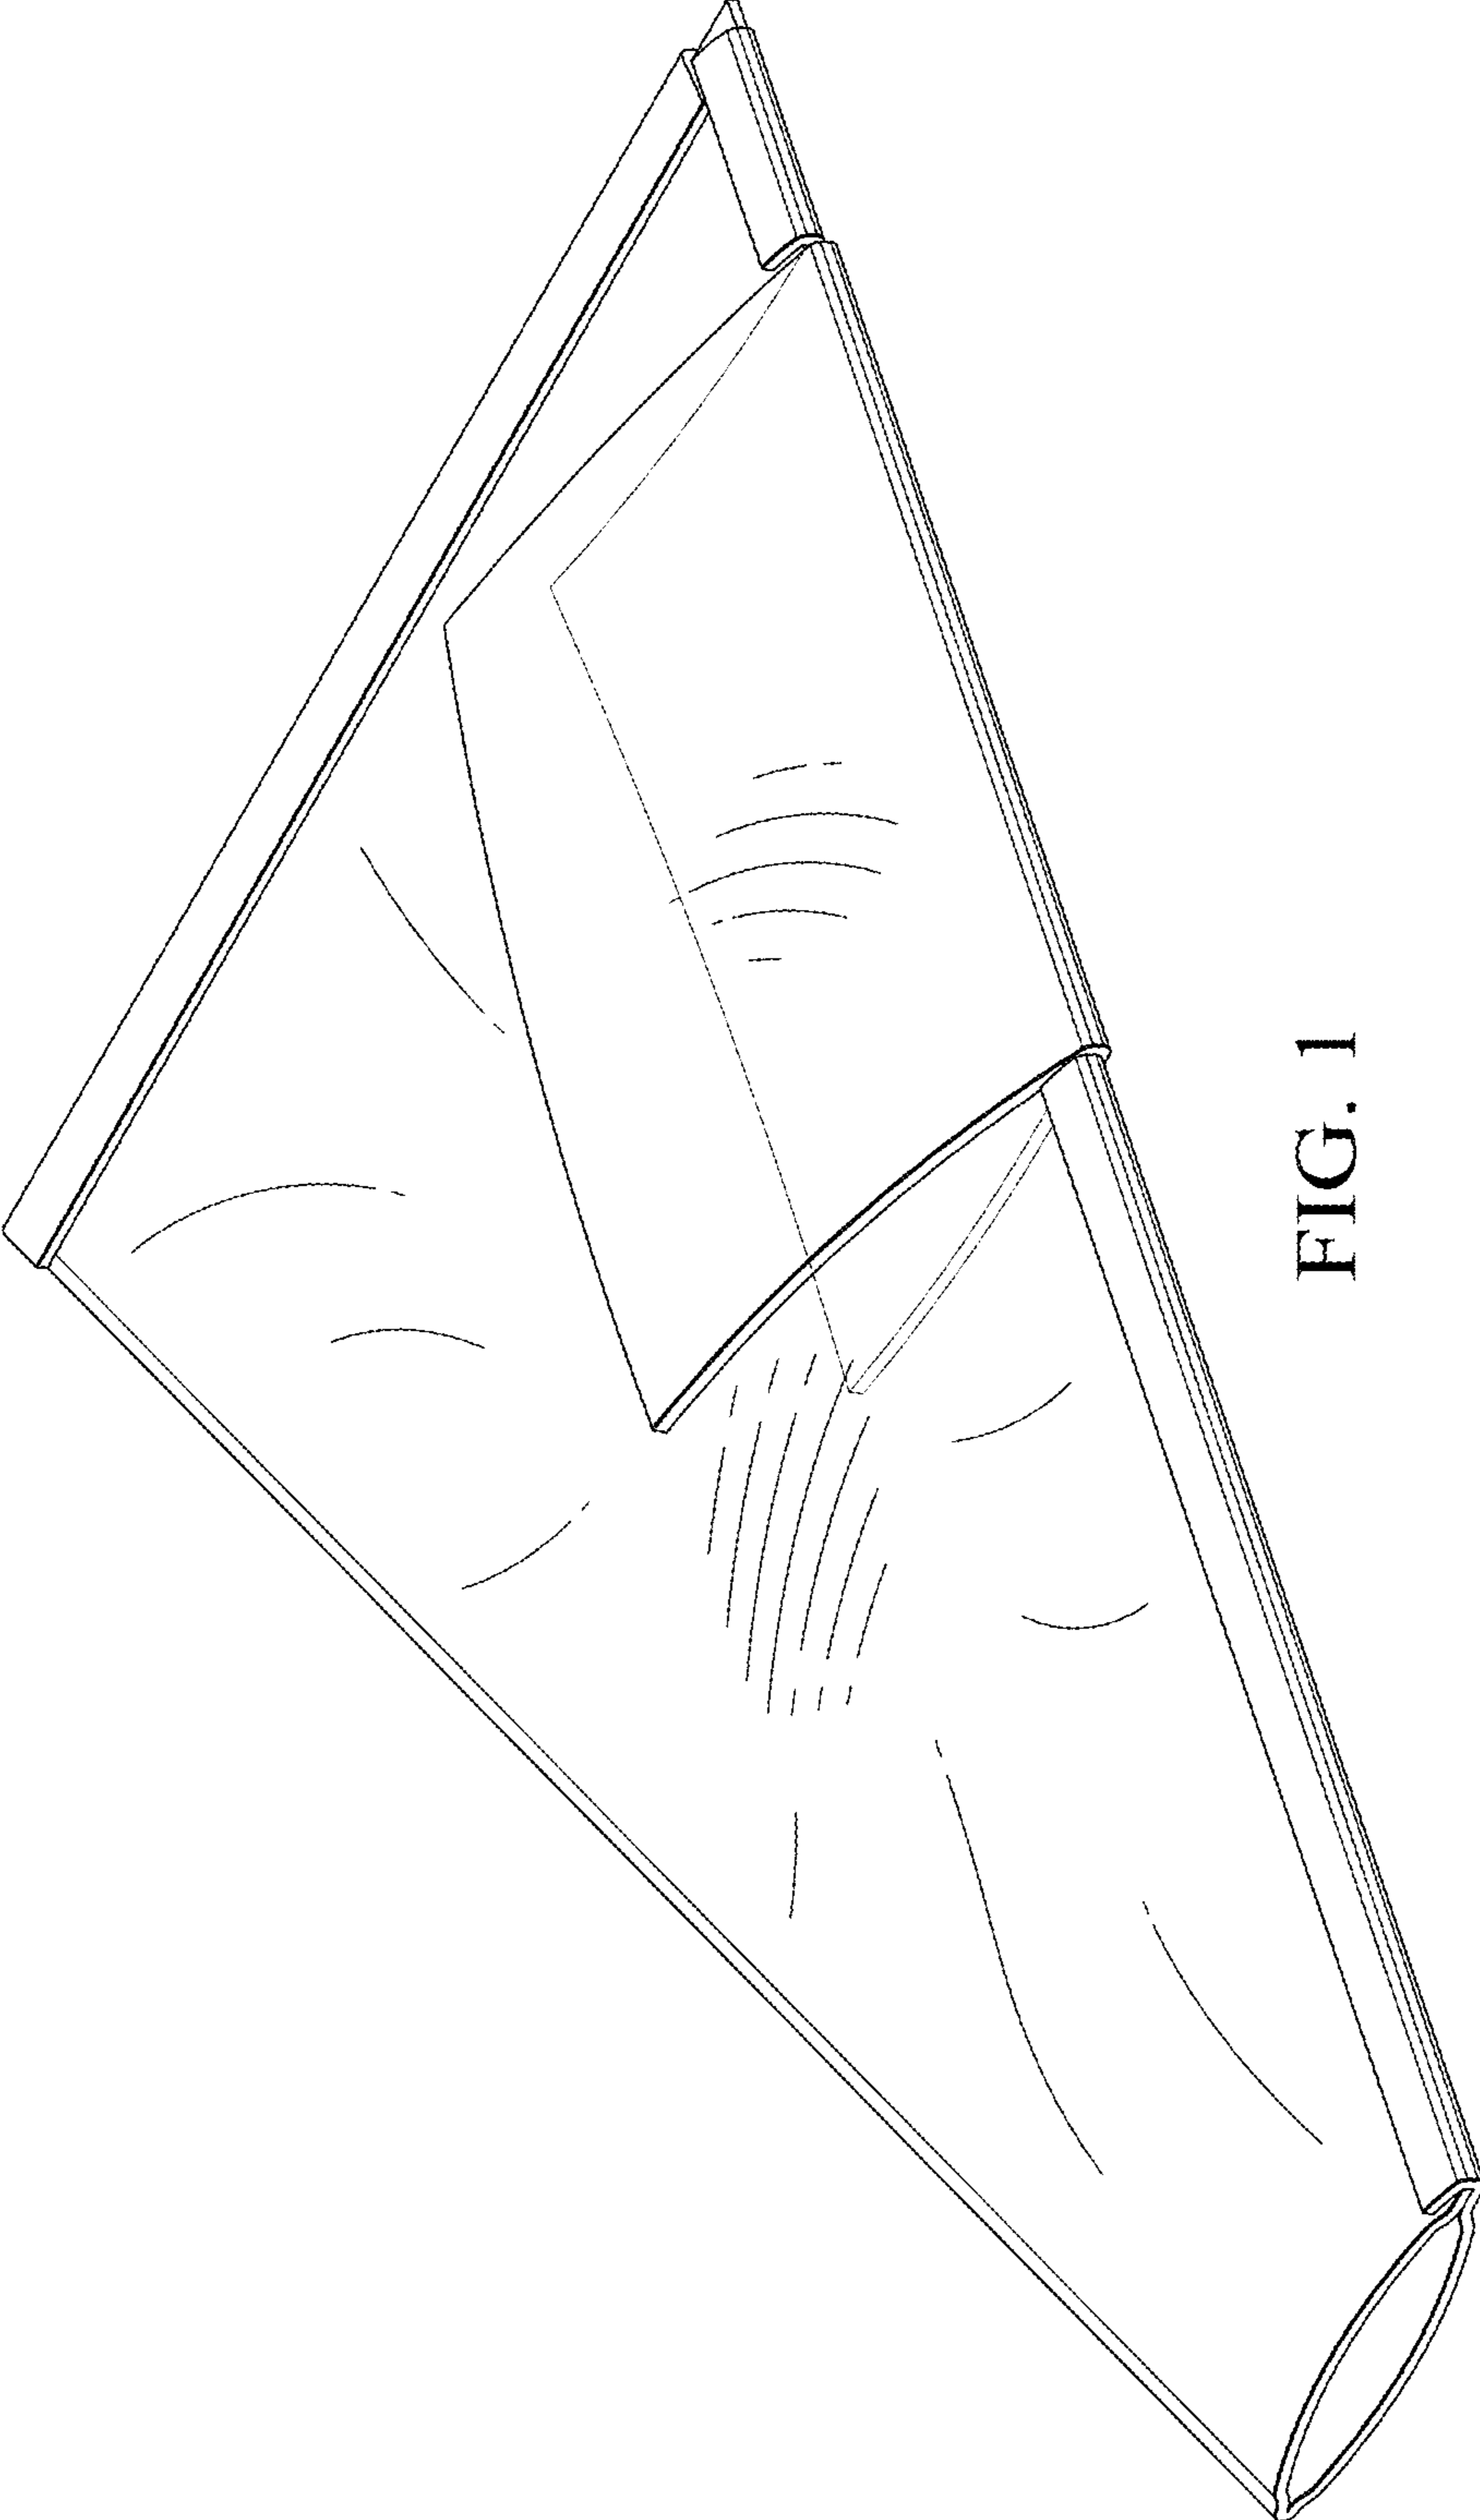

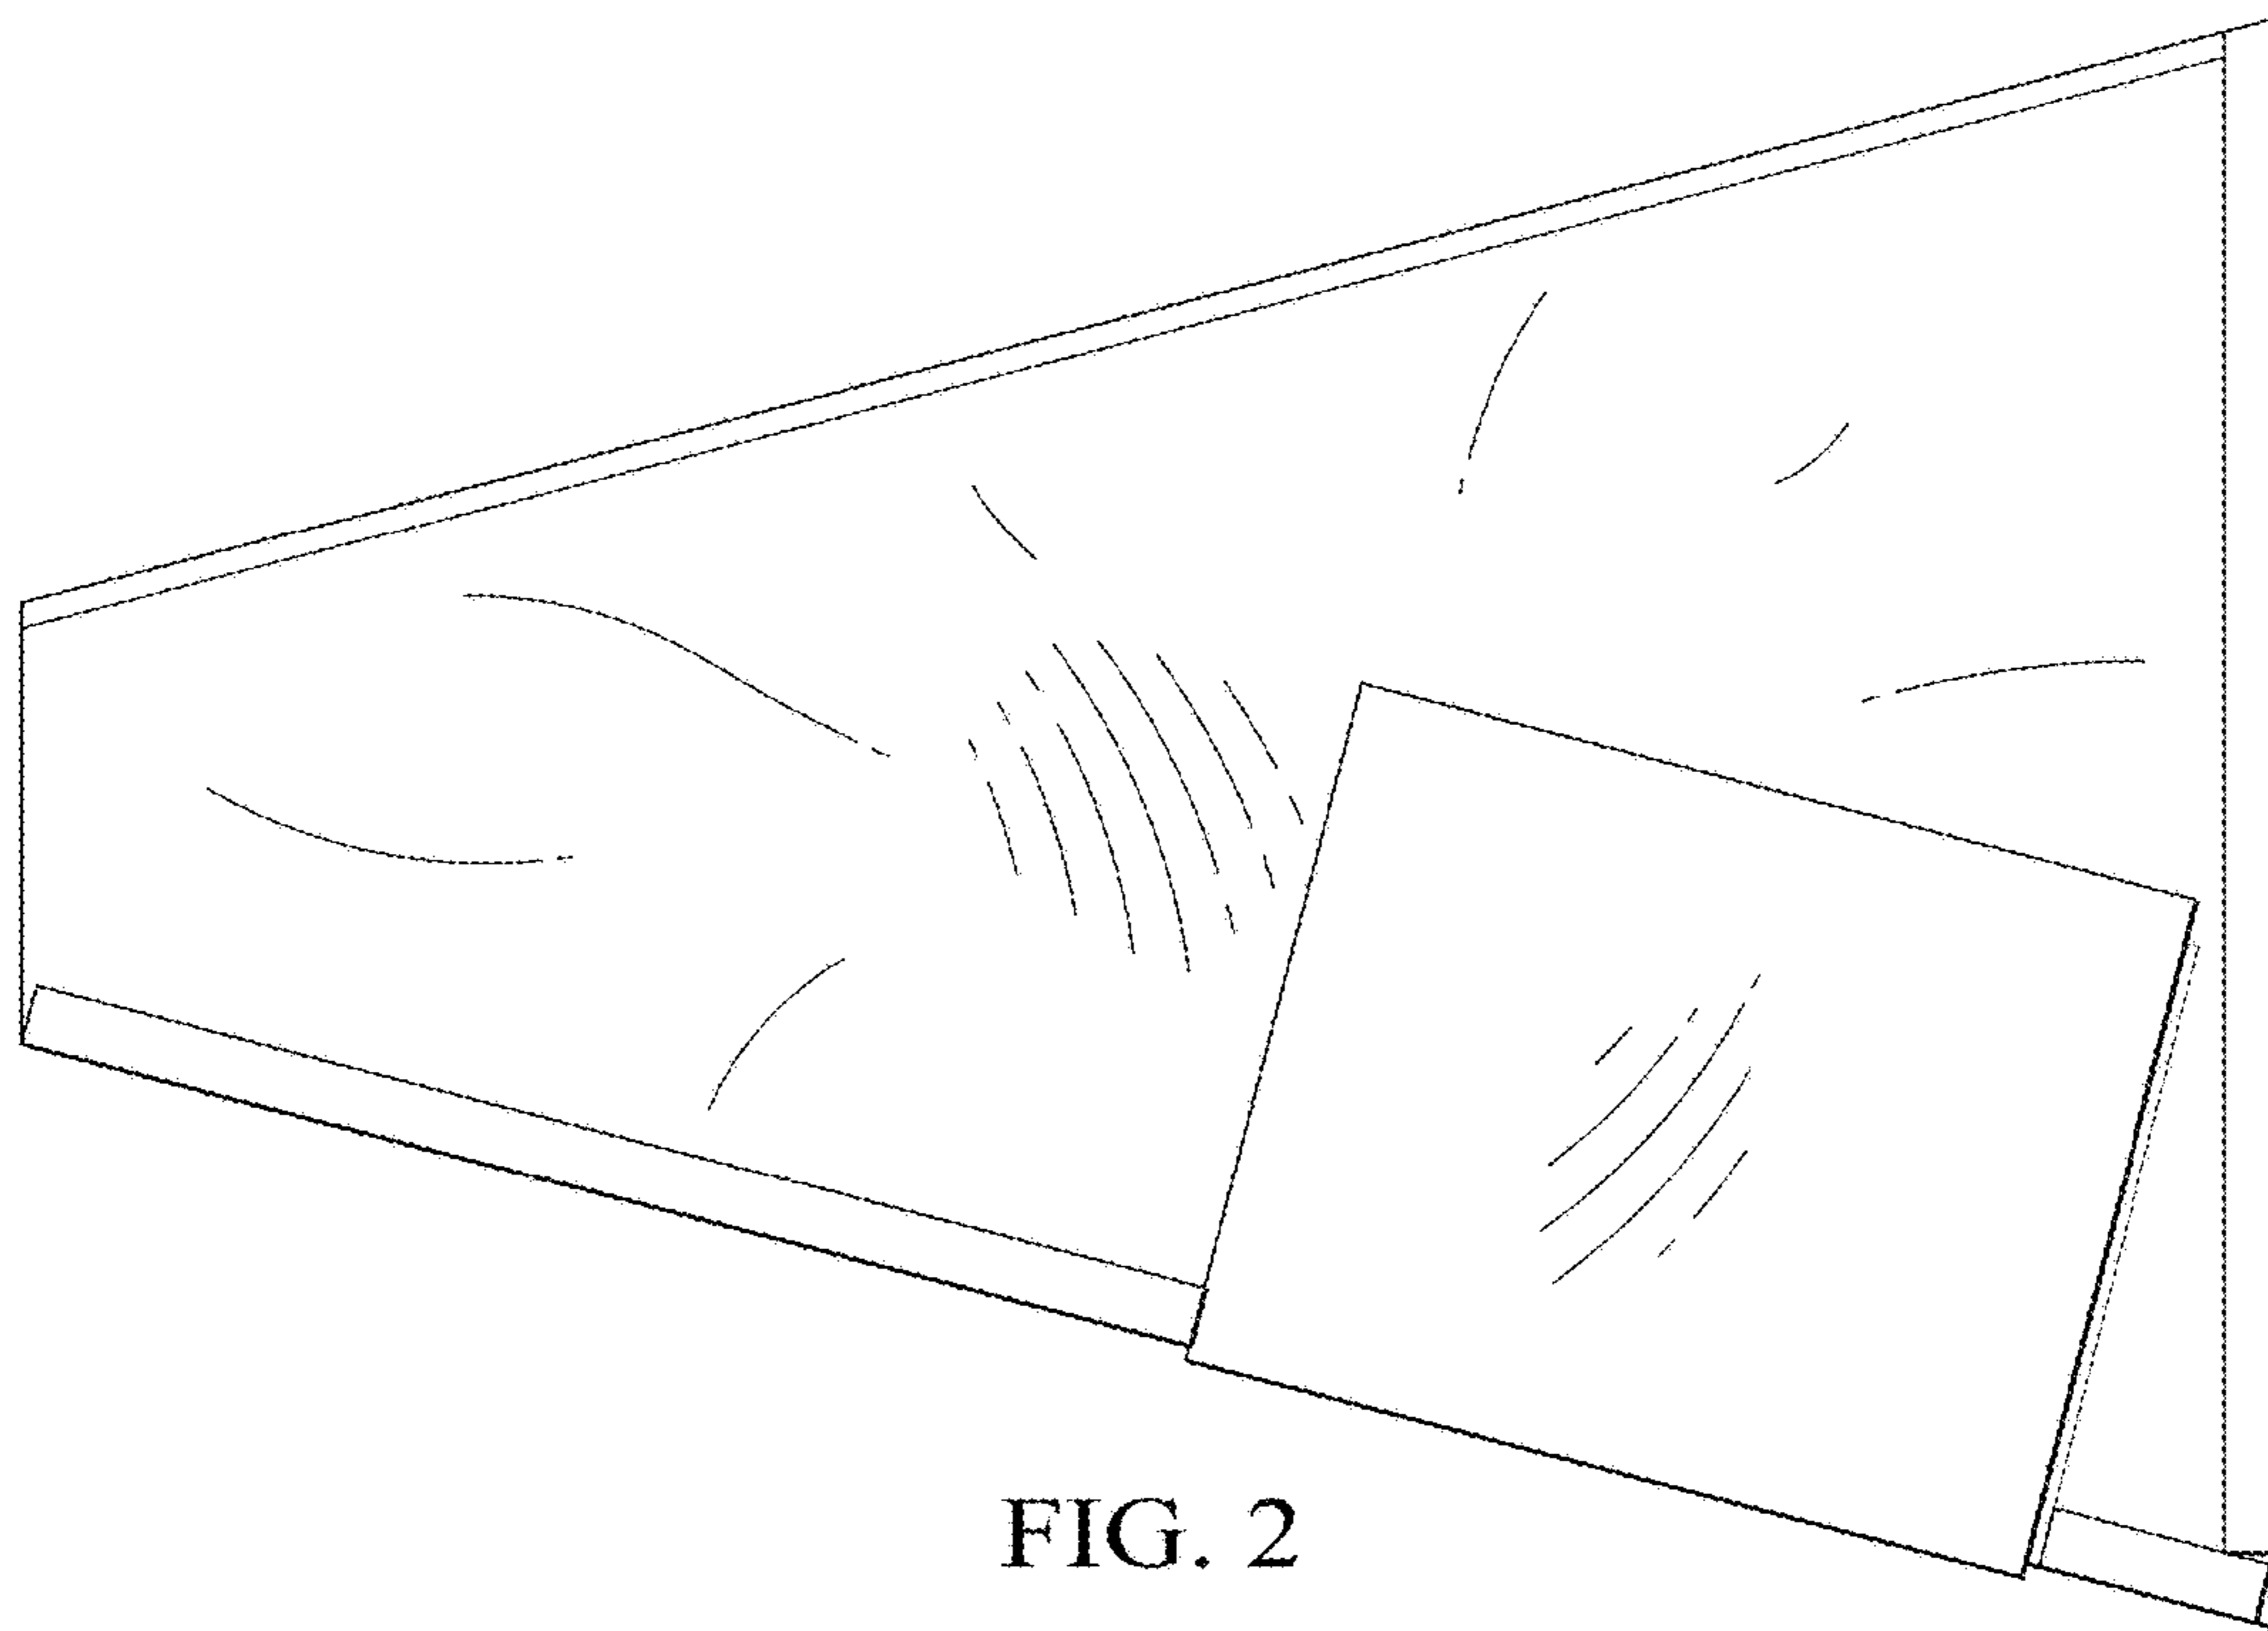


FIG. 2

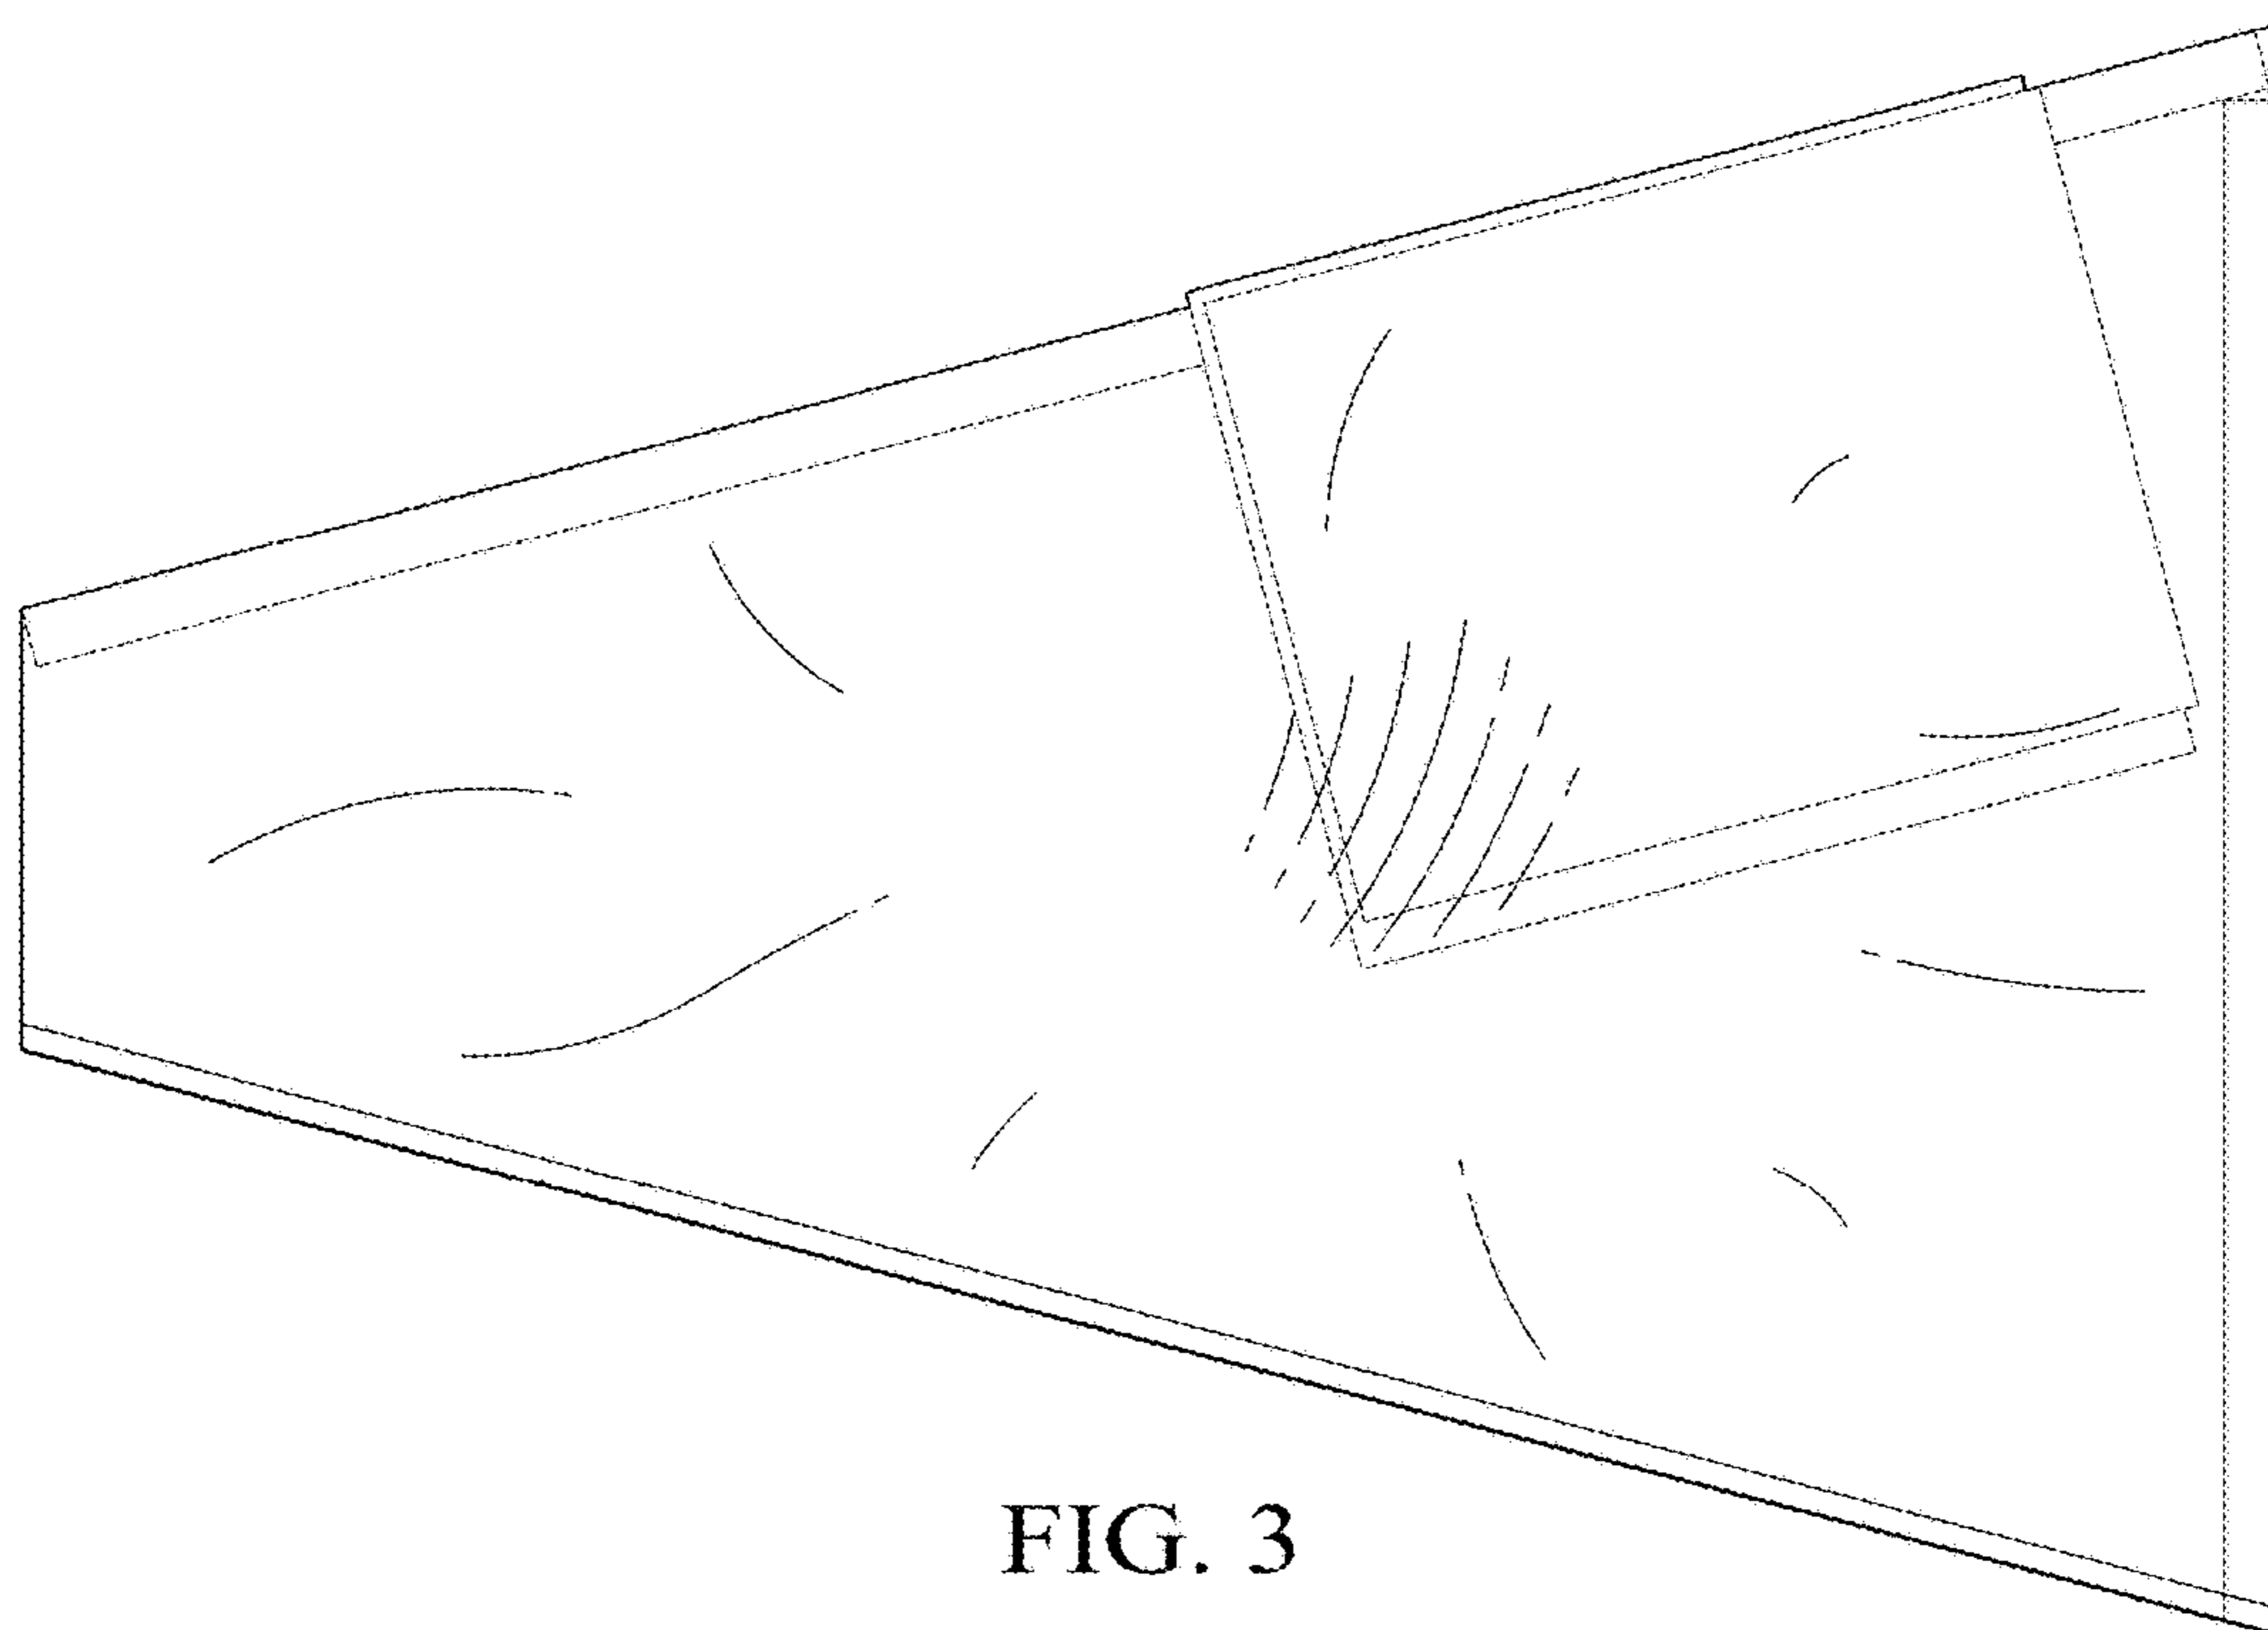


FIG. 3

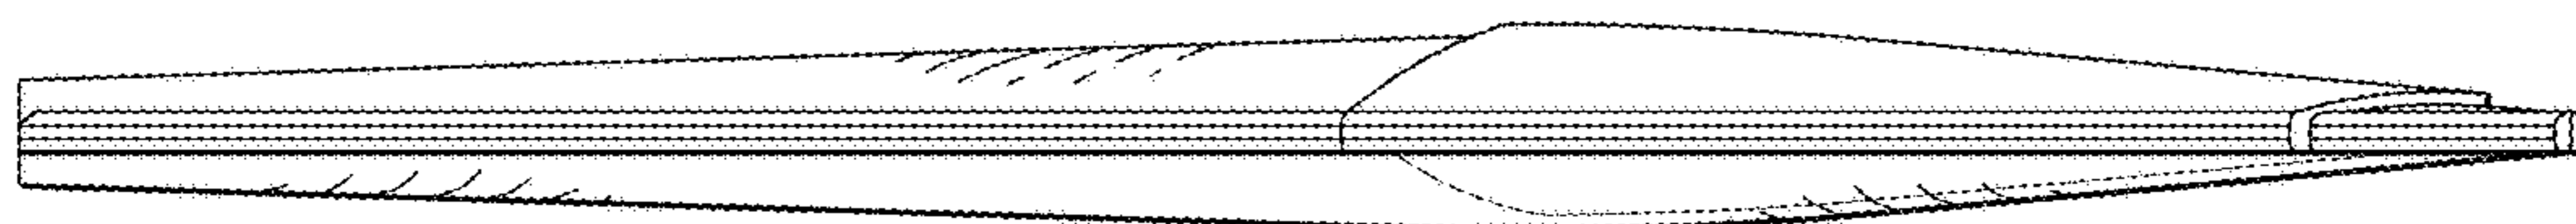


FIG. 4

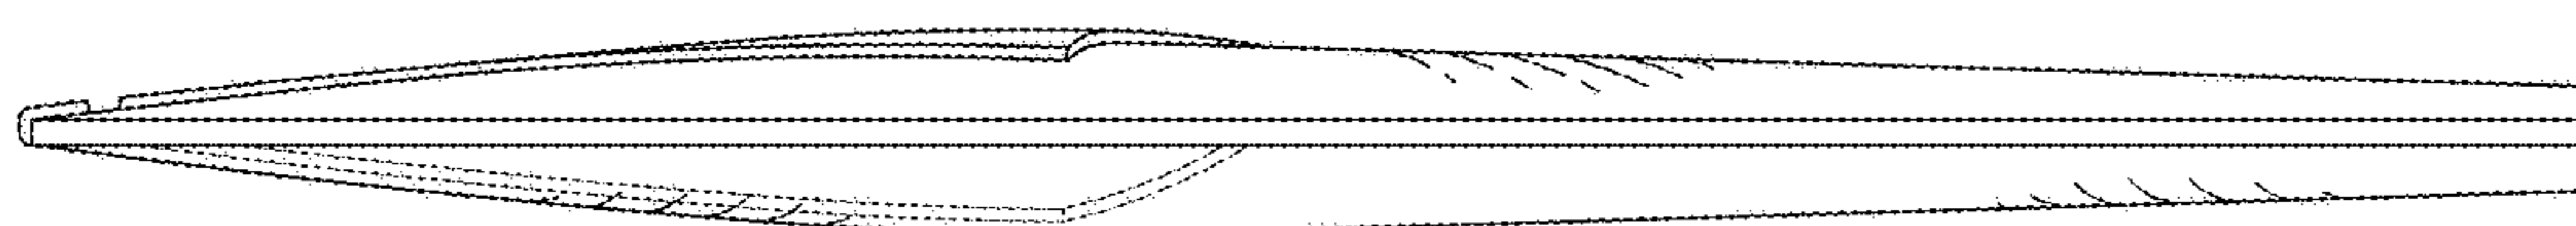


FIG. 5

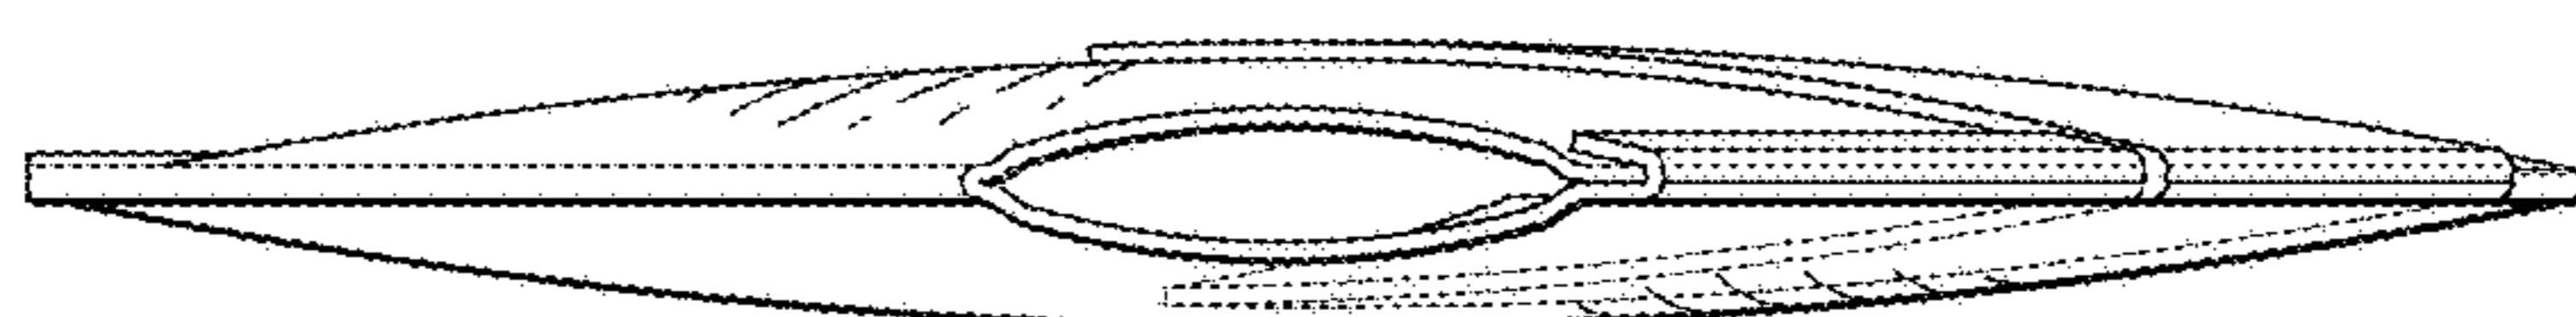


FIG. 6

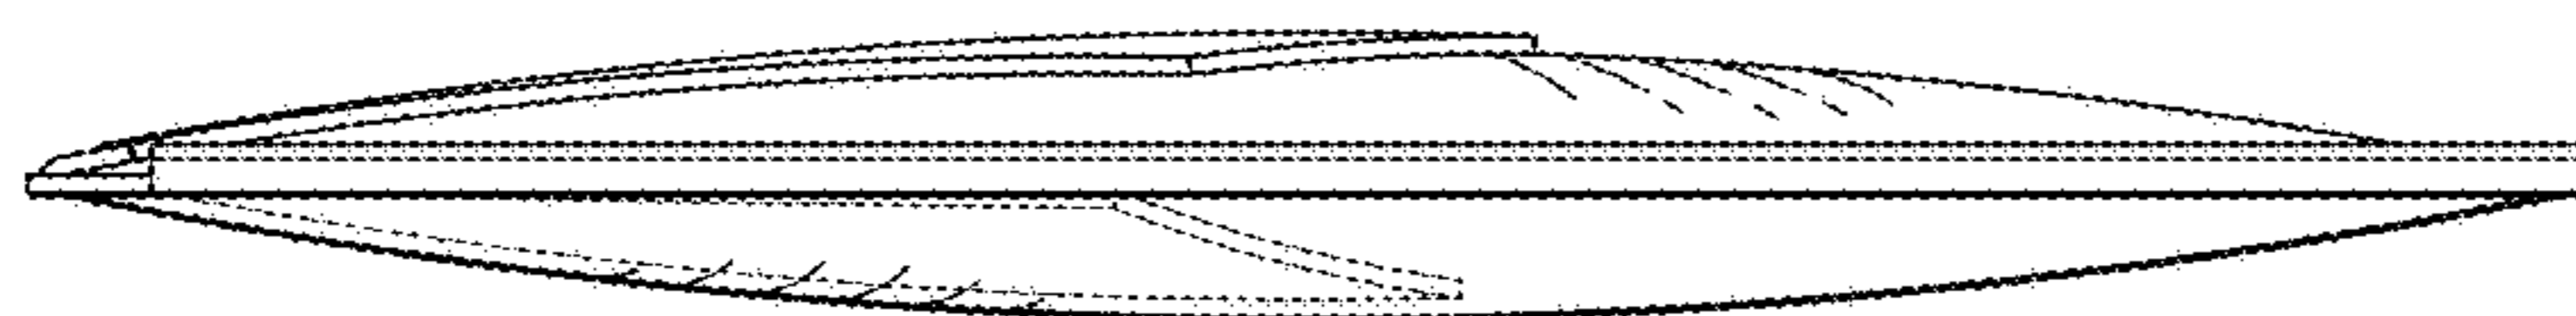


FIG. 7