



US00D834184S

(12) **United States Design Patent** (10) **Patent No.:** **US D834,184 S**
Anderson (45) **Date of Patent:** **** Nov. 20, 2018**

(54) **INSERTION DEVICE WITHOUT A DISTAL OPENING**

(71) Applicant: **Robert G. Anderson**, Aledo, TX (US)

(72) Inventor: **Robert G. Anderson**, Aledo, TX (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/573,482**

(22) Filed: **Aug. 5, 2016**

(51) **LOC (11) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/115**

(58) **Field of Classification Search**
USPC D24/121, 123, 224; 604/317-325; 623/8
CPC A61F 2/12; B65D 41/04; B65D 2251/023;
B65D 41/0485; B65D 41/3428
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|-----------|------|---------|------------------|-----------------------|
| 4,641,648 | A | 2/1987 | Shapiro | |
| 4,990,145 | A * | 2/1991 | Fleury | A61G 9/006 604/317 |
| 4,995,906 | A | 2/1991 | Iwasaki et al. | |
| 5,322,071 | A * | 6/1994 | Ambrose | A61B 46/00 128/849 |
| 5,571,178 | A | 11/1996 | Ledergerber | |
| 5,584,884 | A * | 12/1996 | Pignataro | A61F 2/12 606/151 |
| 5,723,006 | A | 3/1998 | Ledergerber | |
| 5,782,913 | A | 7/1998 | Schindler et al. | |
| 5,897,590 | A * | 4/1999 | Donovan | A61F 13/36 606/190 |
| 8,136,175 | B1 * | 3/2012 | Fagundes | A61B 10/0038 4/479 |
| 8,206,443 | B2 | 6/2012 | Preissman | |
| 8,211,173 | B2 * | 7/2012 | Keller | A61F 2/12 600/185 |
| 8,313,760 | B2 | 11/2012 | Hunter | |
| D672,051 | S * | 12/2012 | Rannikko | D24/224 |

| | | | | |
|-----------|-----|---------|---------------|---------|
| 8,550,090 | B2 | 10/2013 | Keller et al. | |
| 8,555,893 | B2 | 10/2013 | Keller et al. | |
| 8,641,758 | B1 | 2/2014 | Anderson | |
| D707,353 | S * | 6/2014 | Carr | D24/123 |
| D726,309 | S * | 4/2015 | Wood | D24/121 |
| D731,052 | S * | 6/2015 | Doerr | D24/121 |
| D736,372 | S | 8/2015 | Anderson | |
| D738,490 | S | 9/2015 | Anderson | |
| D742,509 | S | 11/2015 | Anderson | |

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO/2013/122568 A1 8/2013

OTHER PUBLICATIONS

Richard A. Mladick, M.D., F.A.C.S. "No-Touch" Submuscular Saline Breast Augmentation Technique, *Aesthetic Plastic Surgery*, 17:183-192, 1993, New York, NY.

(Continued)

Primary Examiner — David Muller

(74) *Attorney, Agent, or Firm* — Kirby Drake


(57) **CLAIM**

The ornamental design of an insertion device, without a distal opening.

DESCRIPTION

FIG. 1: Top side perspective view of an ornamental design for an insertion device without a distal opening;
FIG. 2: Top view of an ornamental design for an insertion device without a distal opening;
FIG. 3: Bottom view of an ornamental design for an insertion device without a distal opening;
FIG. 4: Right side view thereof;
FIG. 5: Left side view thereof;
FIG. 6: First end view thereof; and,
FIG. 7: Second end view thereof.

1 Claim, 3 Drawing Sheets

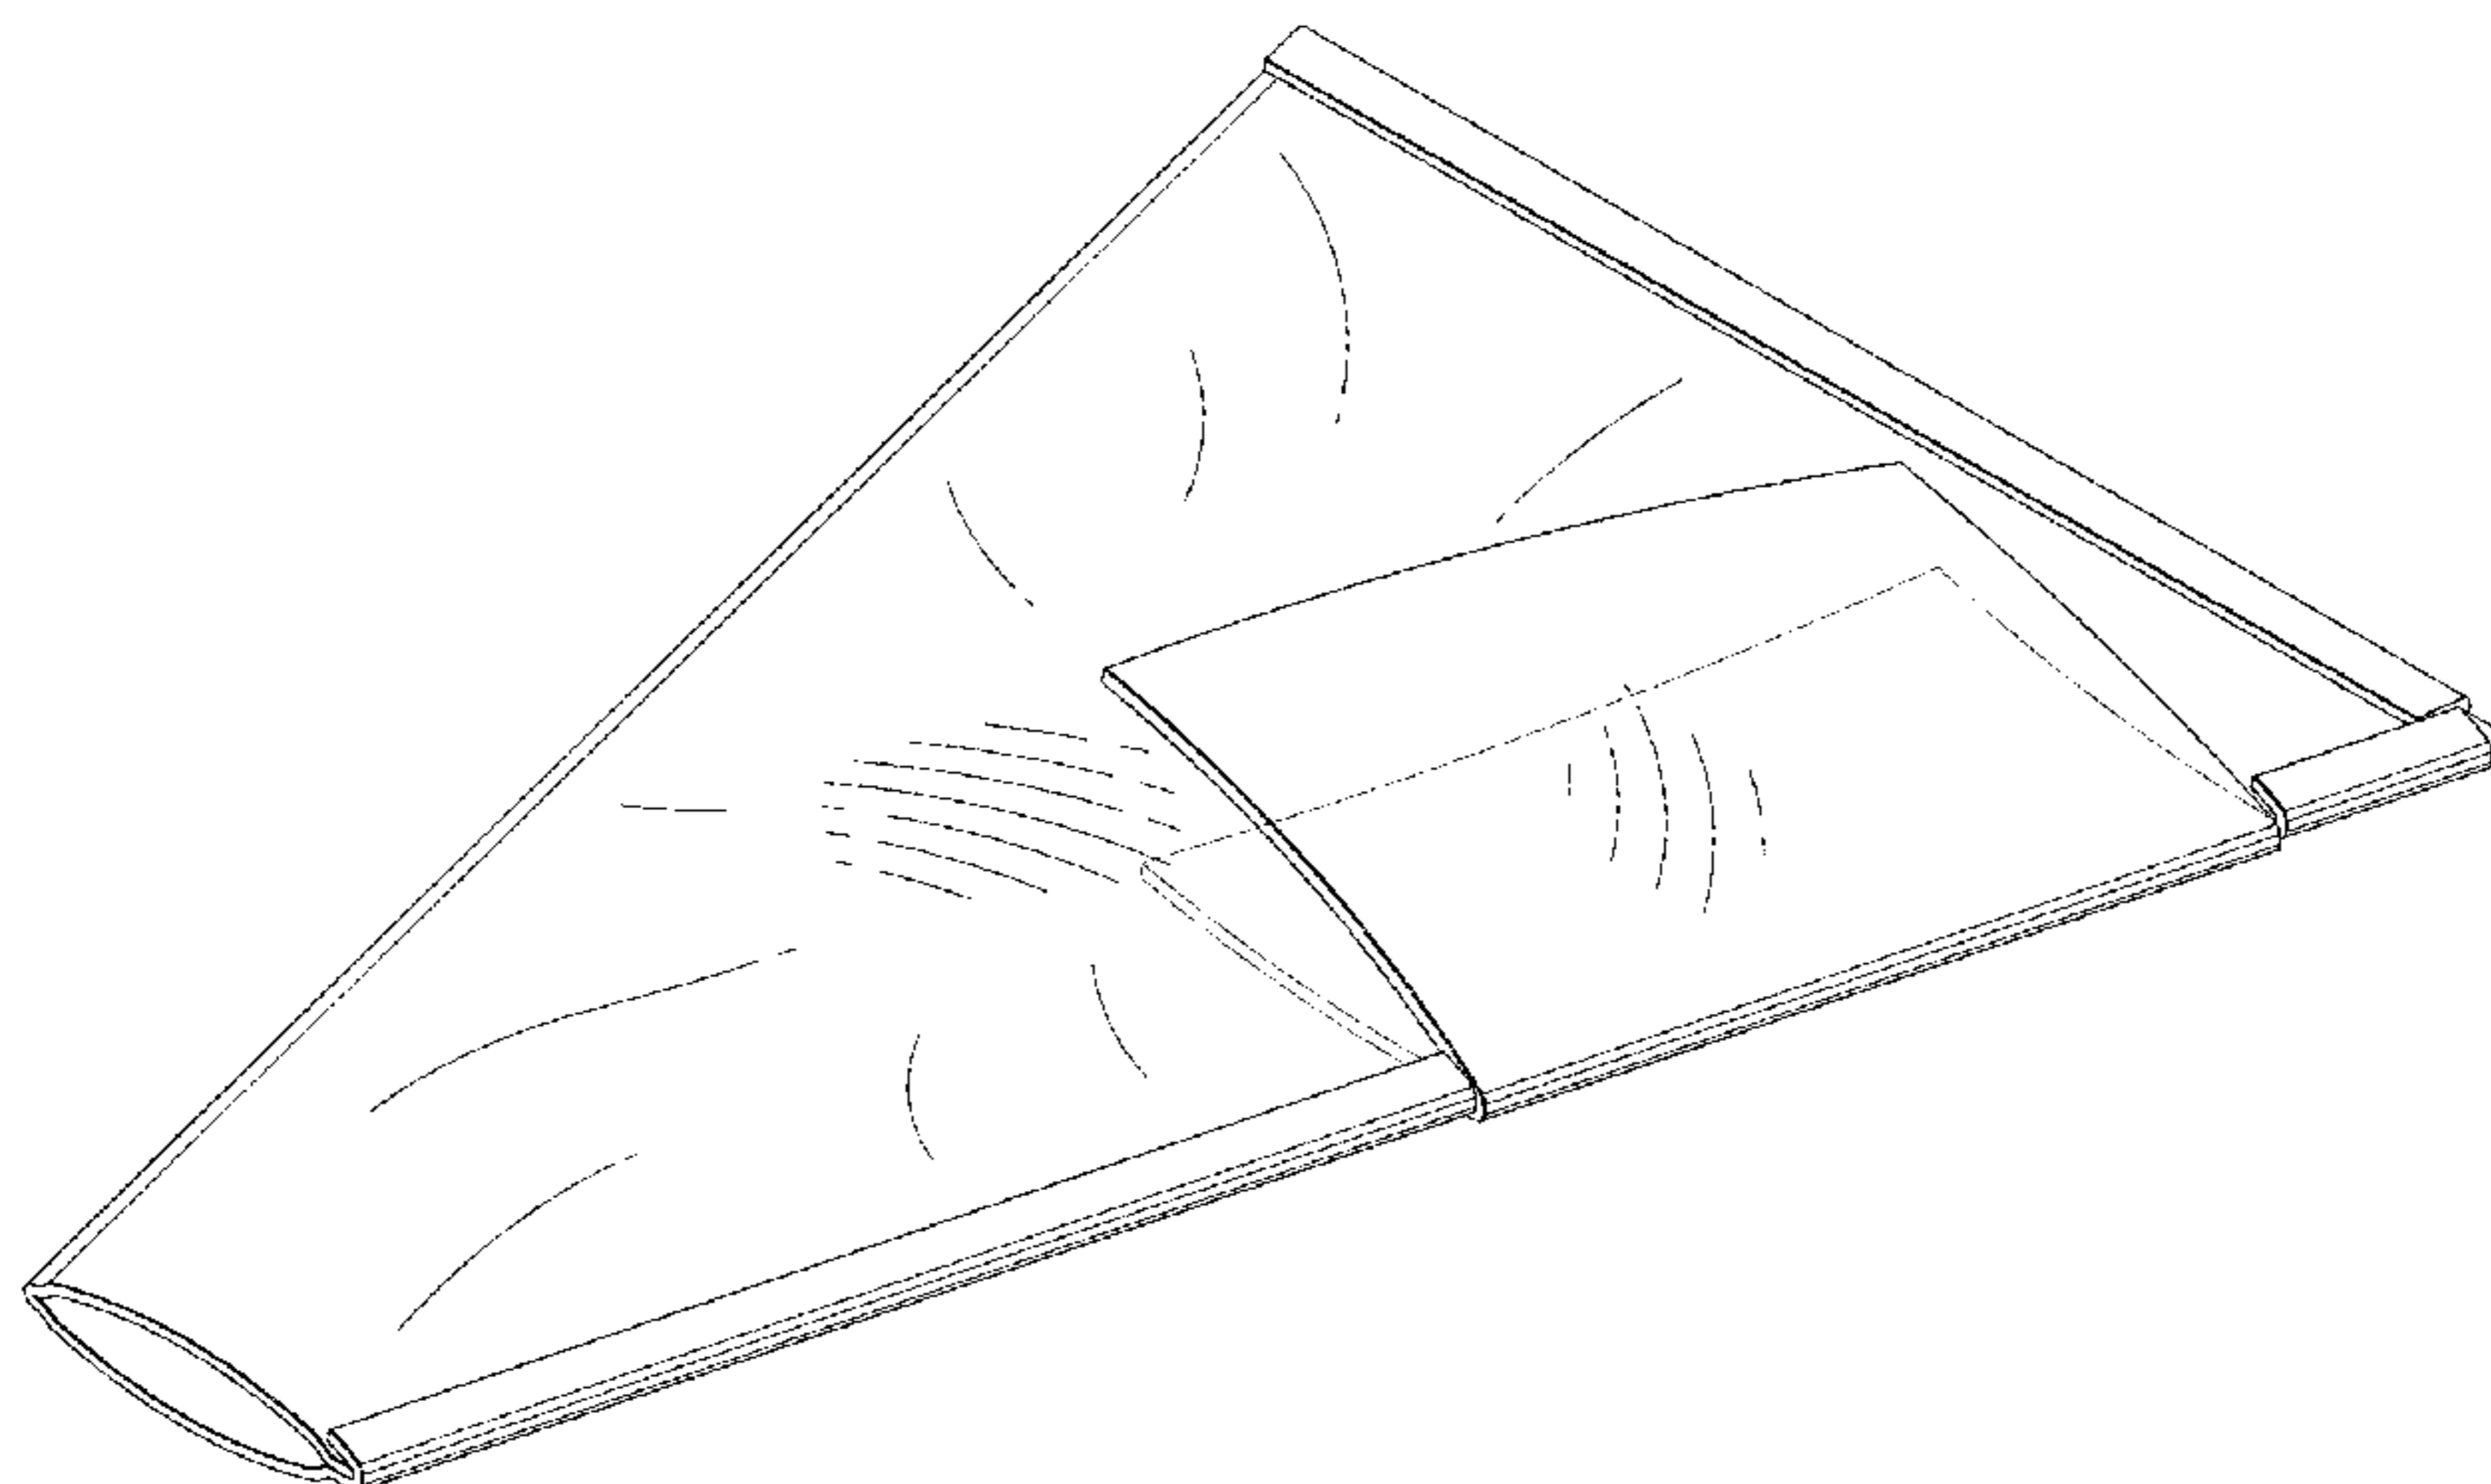

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | |
|--------------|-----|---------|---------------|---------------|
| D752,739 | S | 3/2016 | Anderson | |
| D773,652 | S * | 12/2016 | Anderson | D24/115 |
| D775,725 | S * | 1/2017 | Anderson | D24/115 |
| D776,806 | S * | 1/2017 | Anderson | D24/115 |
| 2007/0276484 | A1 | 11/2007 | Abell et al. | |
| 2009/0204107 | A1 | 8/2009 | Keller et al. | |
| 2010/0280610 | A1 | 11/2010 | Preissman | |
| 2011/0035003 | A1 | 2/2011 | Preissman | |
| 2011/0218624 | A1 | 9/2011 | Preissman | |
| 2012/0185042 | A1 | 7/2012 | Preissman | |
| 2012/0259414 | A1 | 10/2012 | Preissman | |
| 2013/0073040 | A1 | 3/2013 | Preissman | |
| 2014/0074235 | A1 | 3/2014 | Keller et al. | |
| 2014/0074236 | A1 | 3/2014 | Keller et al. | |
| 2014/0148901 | A1 | 5/2014 | Anderson | |
| 2015/0126812 | A1 | 5/2015 | Anderson | |
| 2015/0374478 | A1 | 12/2015 | Anderson | |
| 2016/0038275 | A1 | 2/2016 | Preissman | |
| 2016/0095697 | A1 | 4/2016 | Anderson | |

OTHER PUBLICATIONS


Richard A. Mladick, M.D., F.A.C.S. Significance of *Staphylococcus* epidermidis Causing Subclinical Infection, *Plastic & Reconstructive Surgery*: Apr. 15, 2005—vol. 115—Issue 5—pp. 1426-1427, Virginia Beach, VA.

Richard A. Mladick, M.D., F.A.C.S. Prevention of Capsular Contracture, *Plastic & Reconstructive Surgery*: May 1999—vol. 103—Issue 6—pp. 1773-1774, Virginia Beach, VA.

Thomas M. Biggs, M.D. Prefilled Saline Breast Implants Offer Significant Advantages, *Aesthetic Surgery Journal* Sep. 1999 vol. 19 No. 5 424, St Louis, MO.

“Mitchel H. Brown, M.D., M.Ed. Cohesive Silicone Gel Breast Implants in Aesthetic and Reconstructive Breast Surgery, *Plastic & Reconstructive Surgery*: Sep. 1, 2005—vol. 116—Issue 3—pp. 768-779”.

* cited by examiner

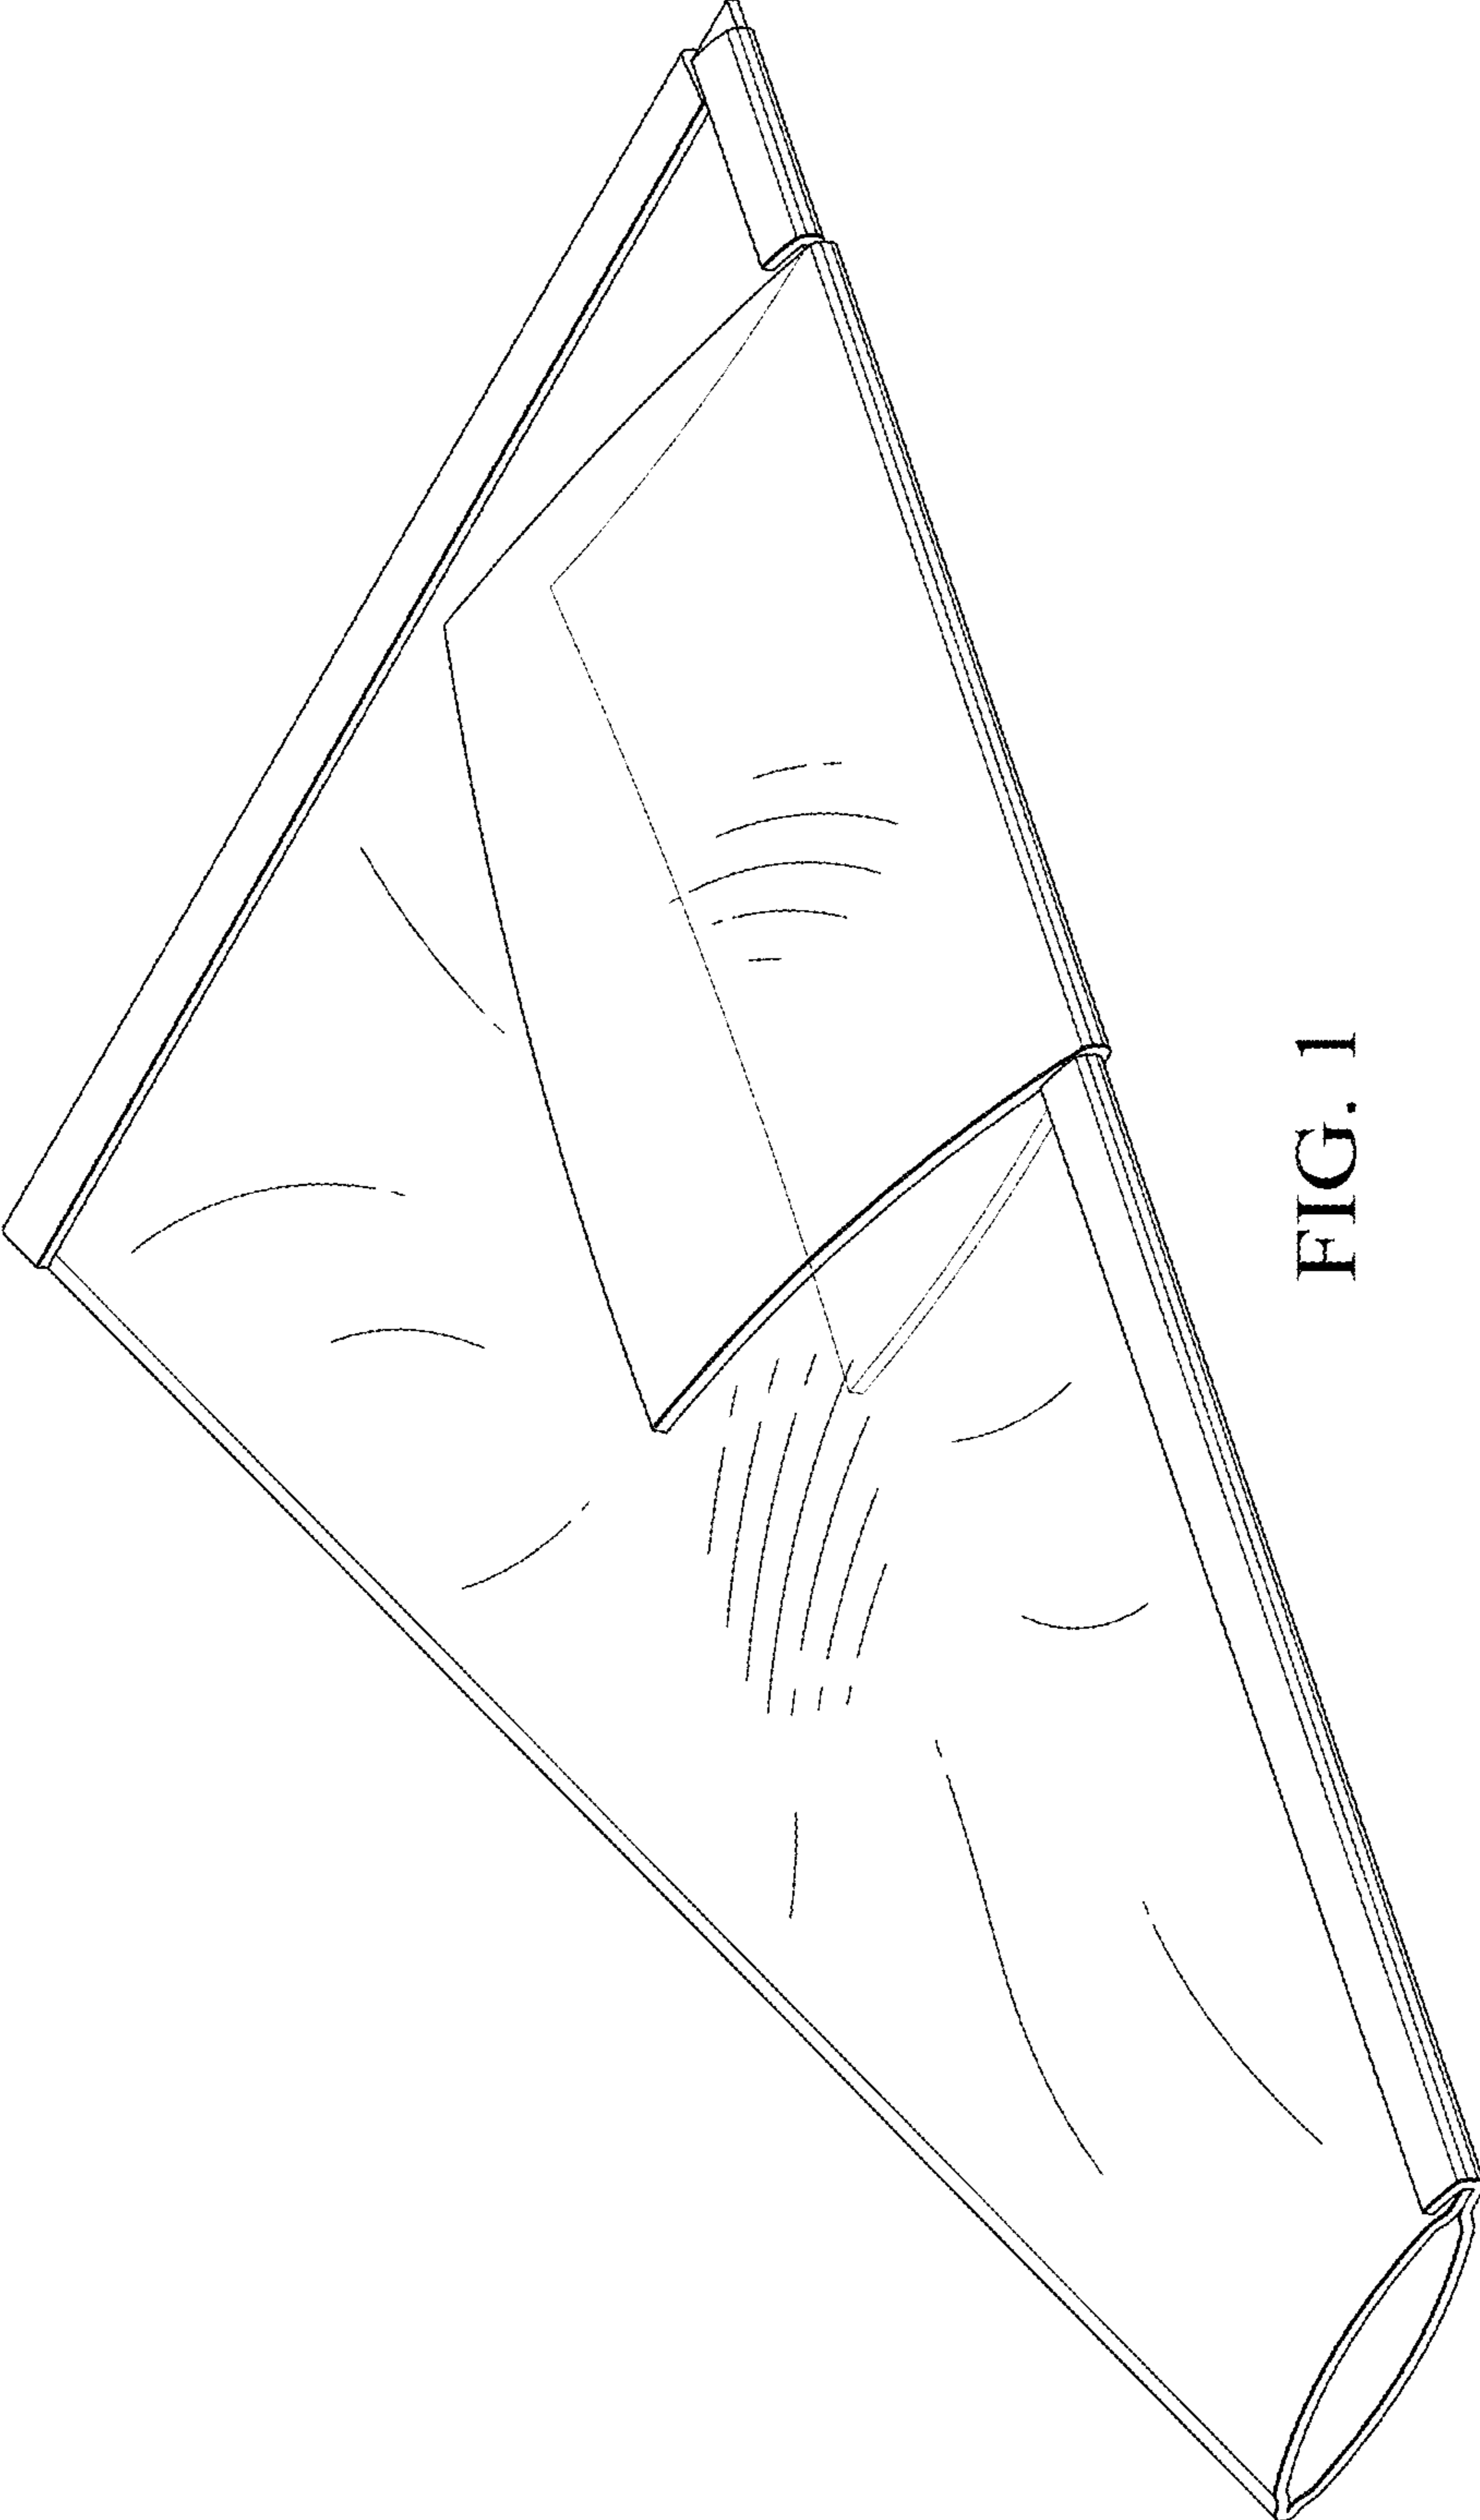

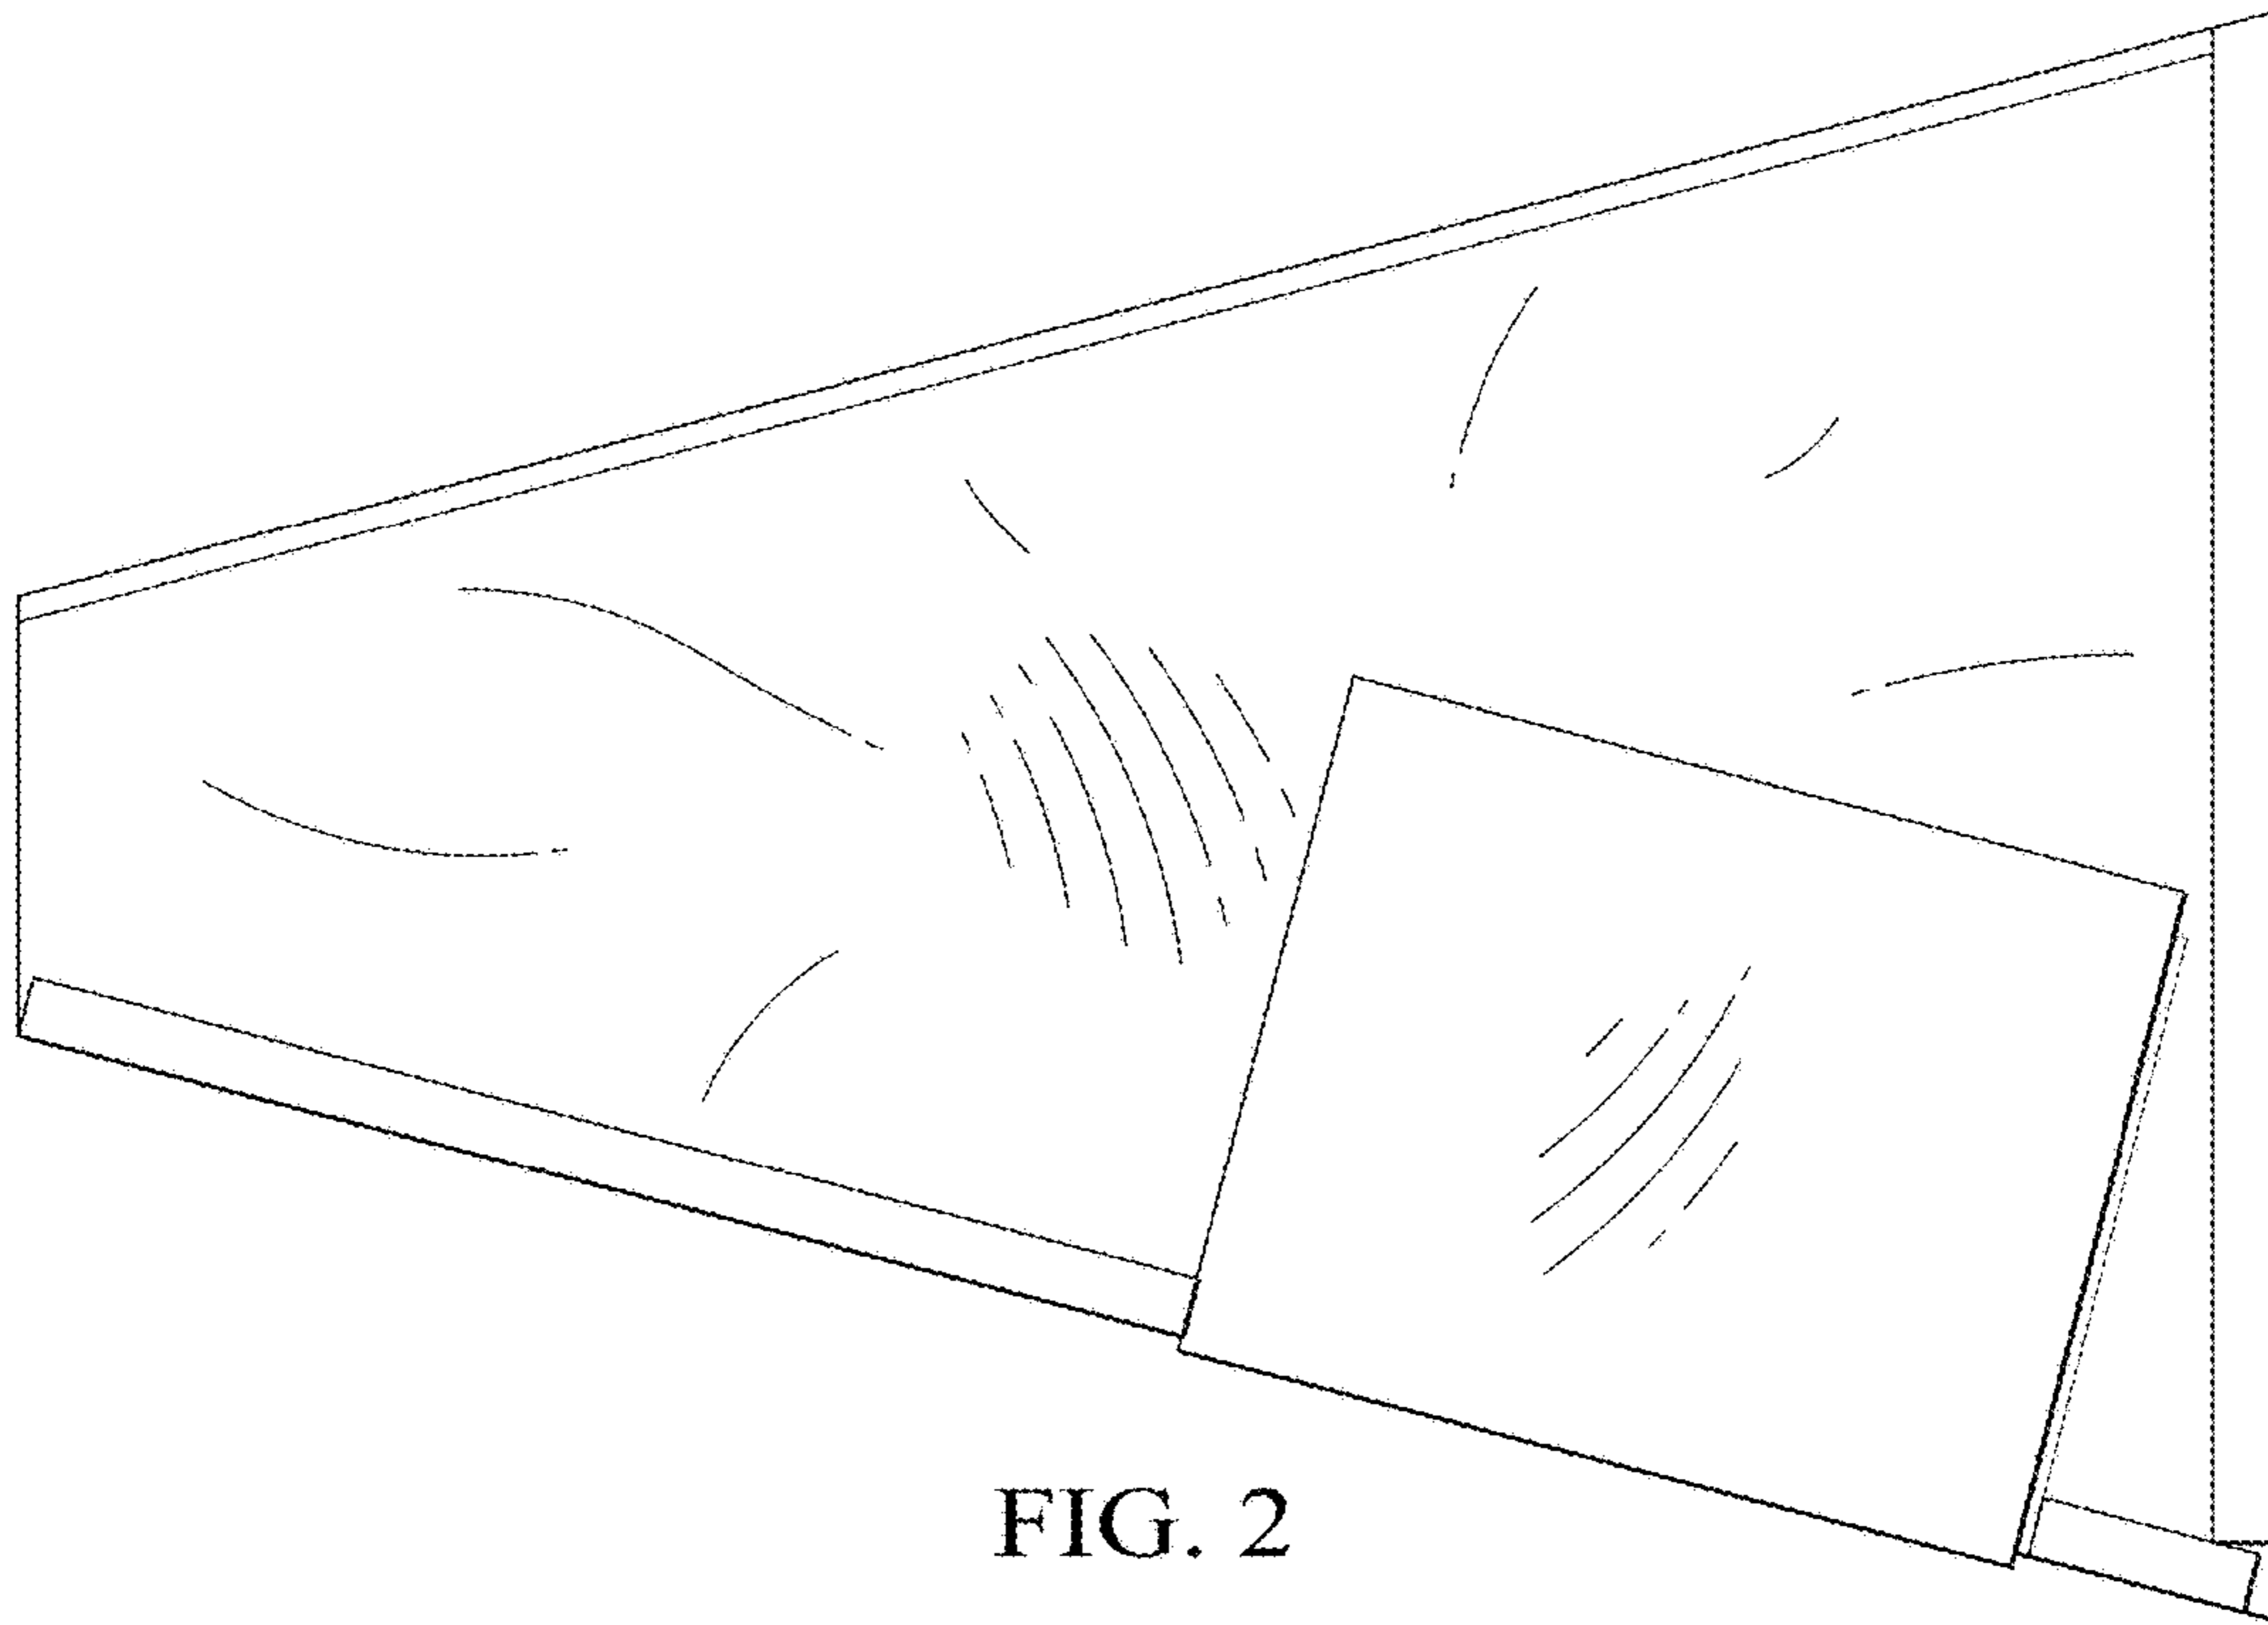


FIG. 2

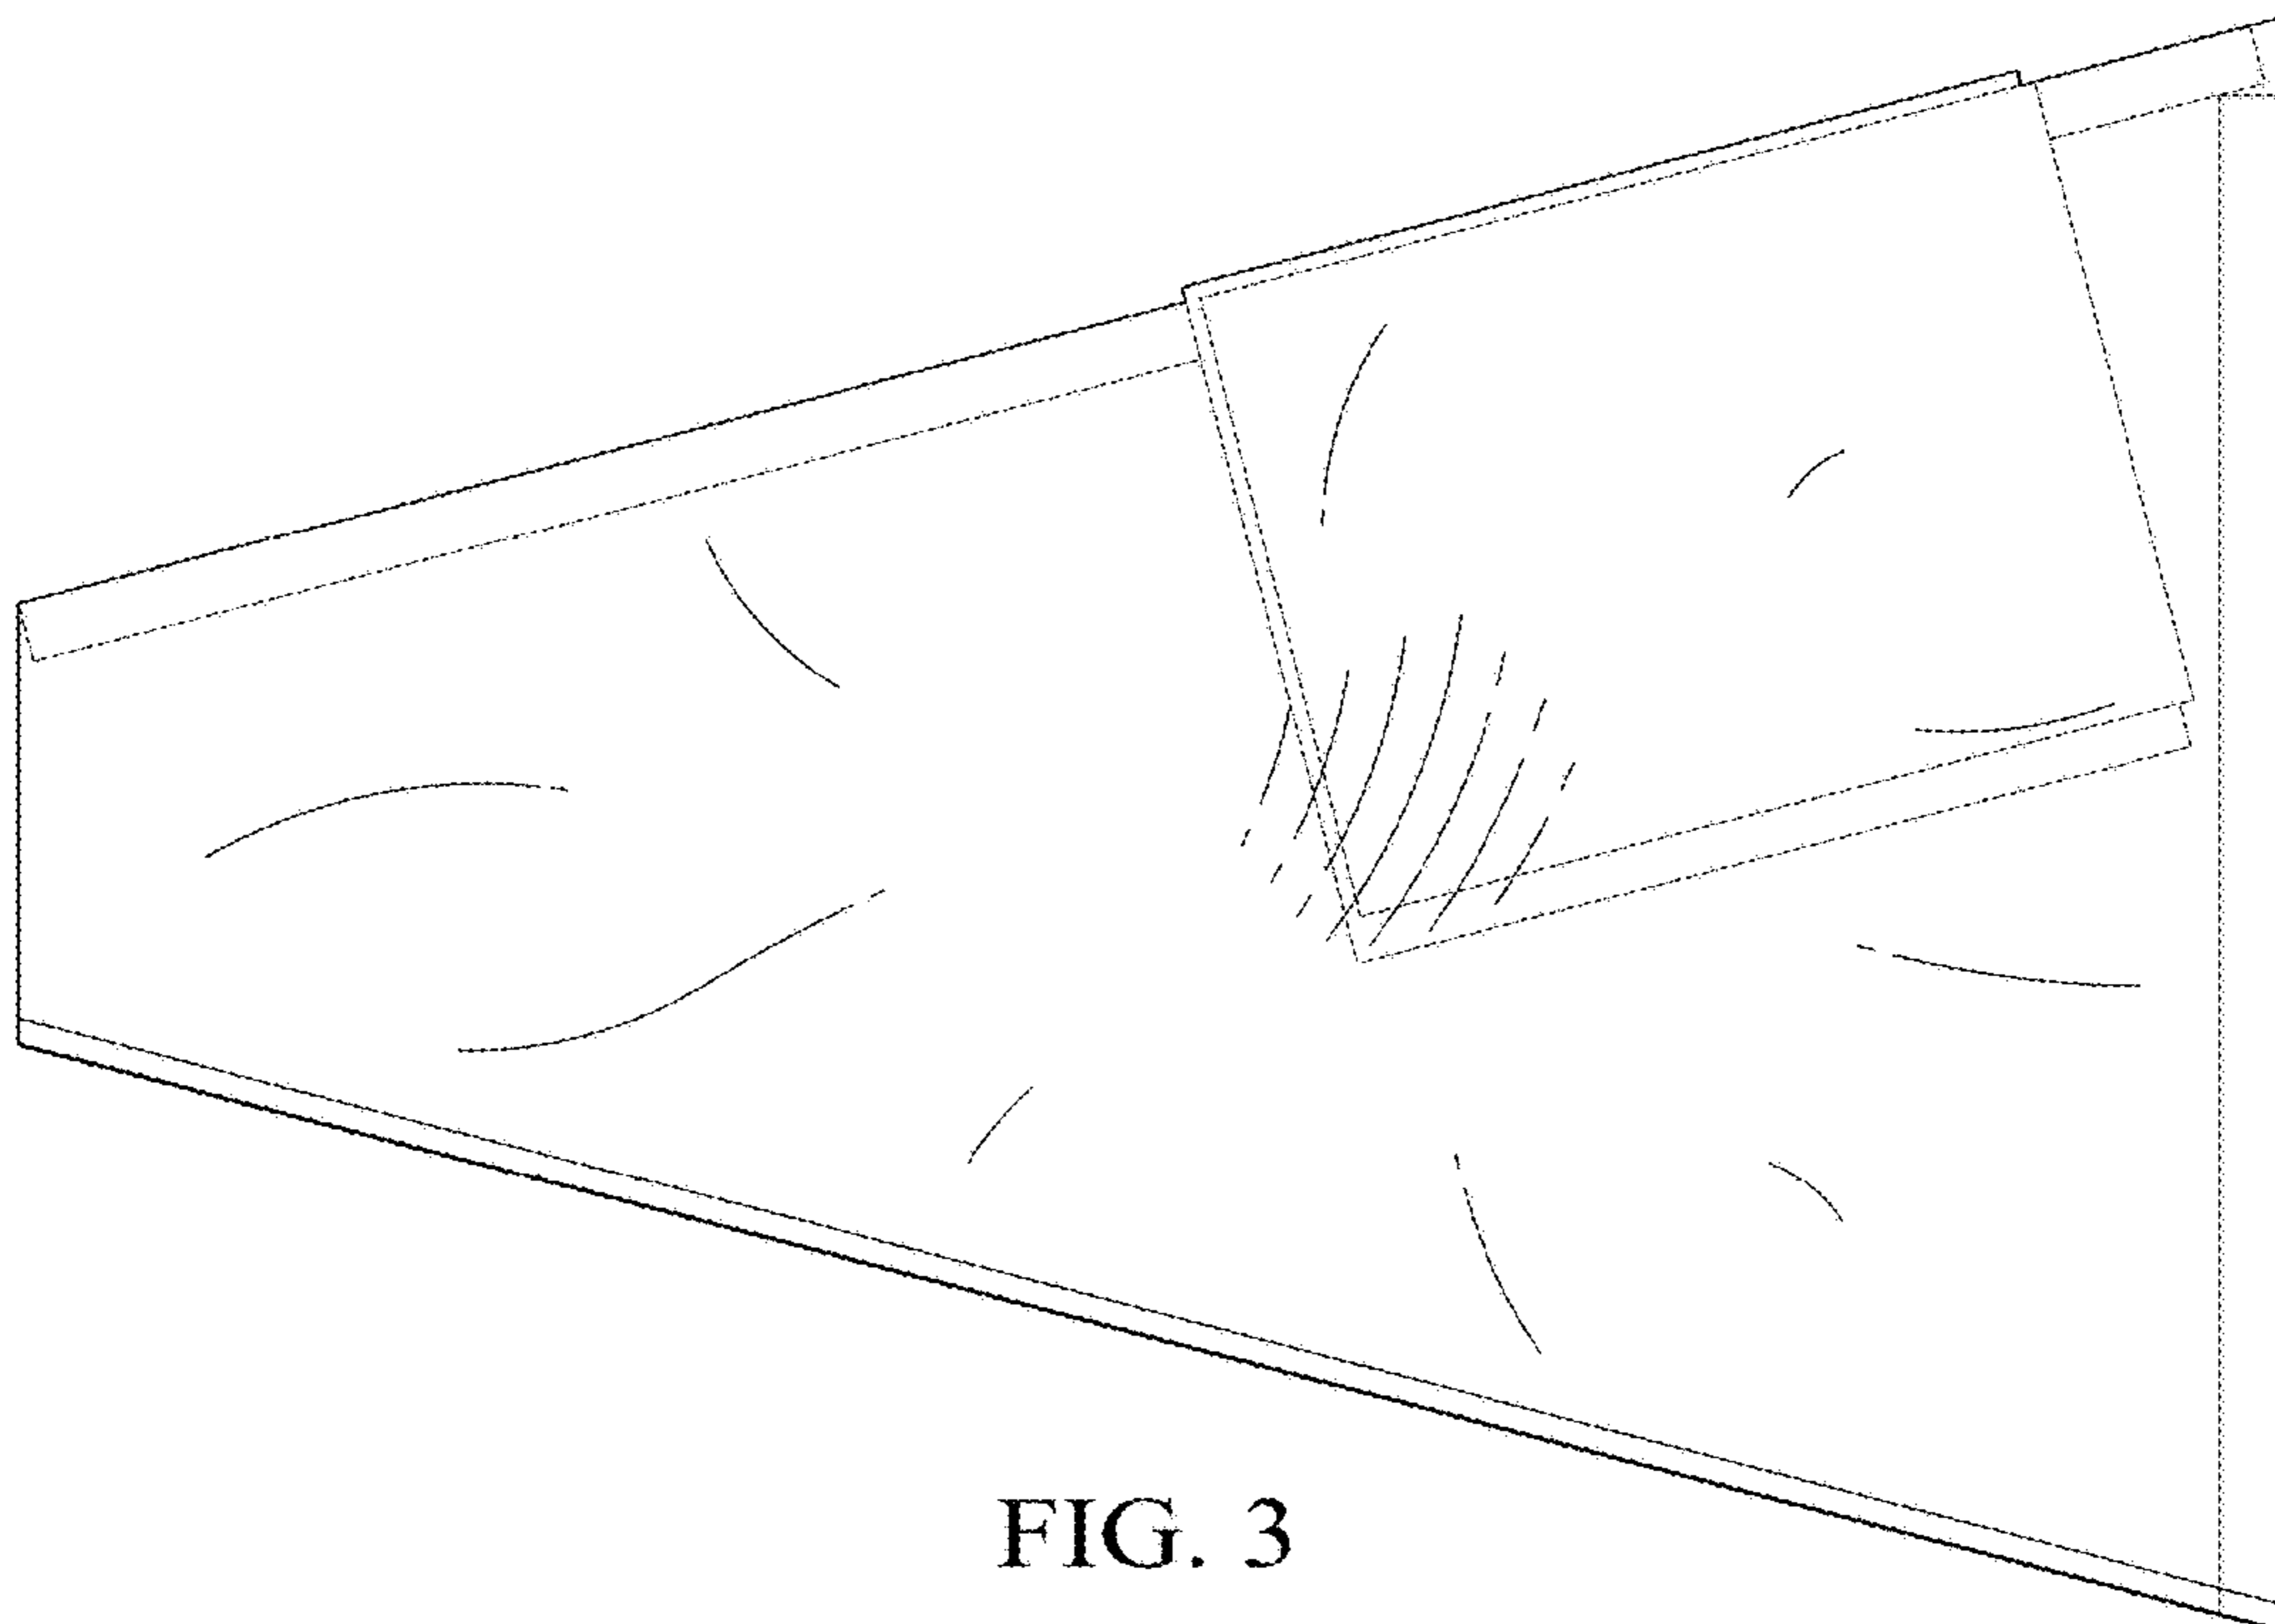


FIG. 3

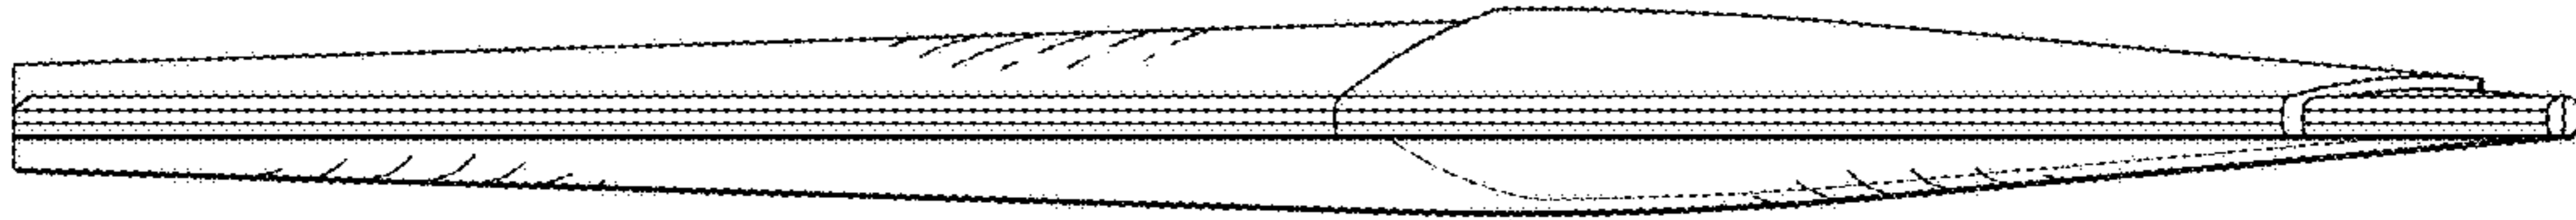


FIG. 4

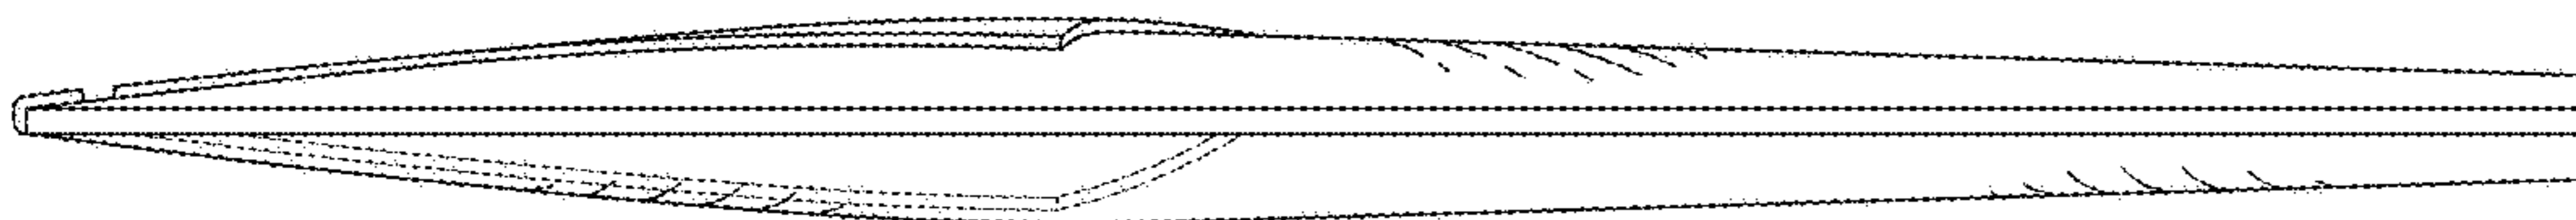


FIG. 5

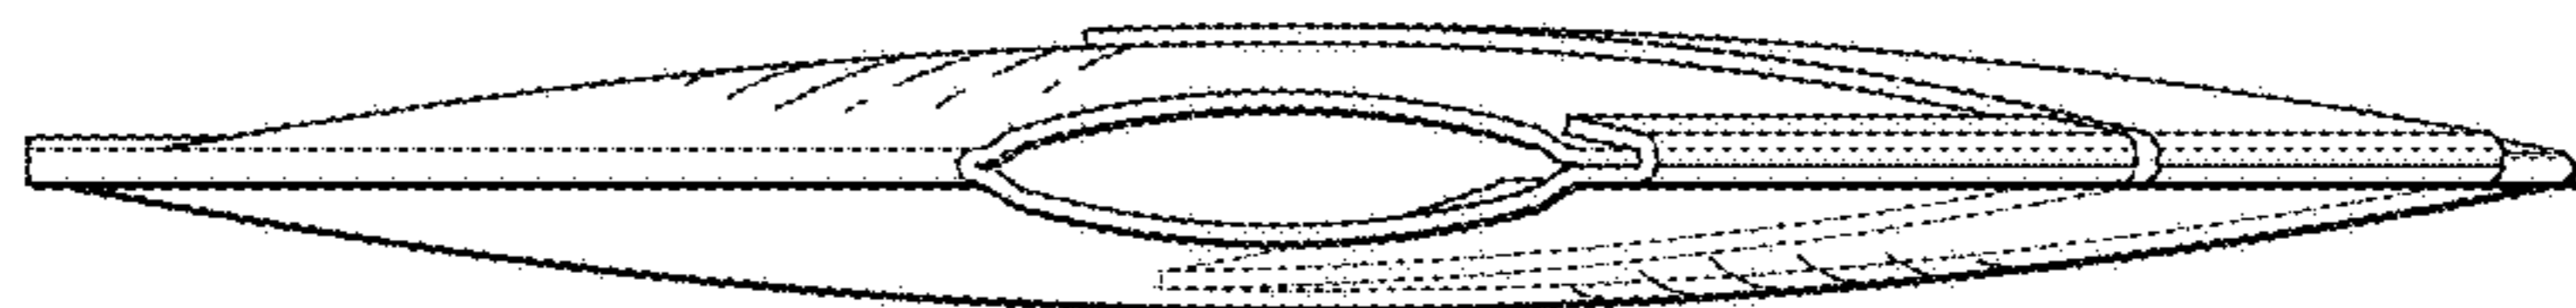


FIG. 6

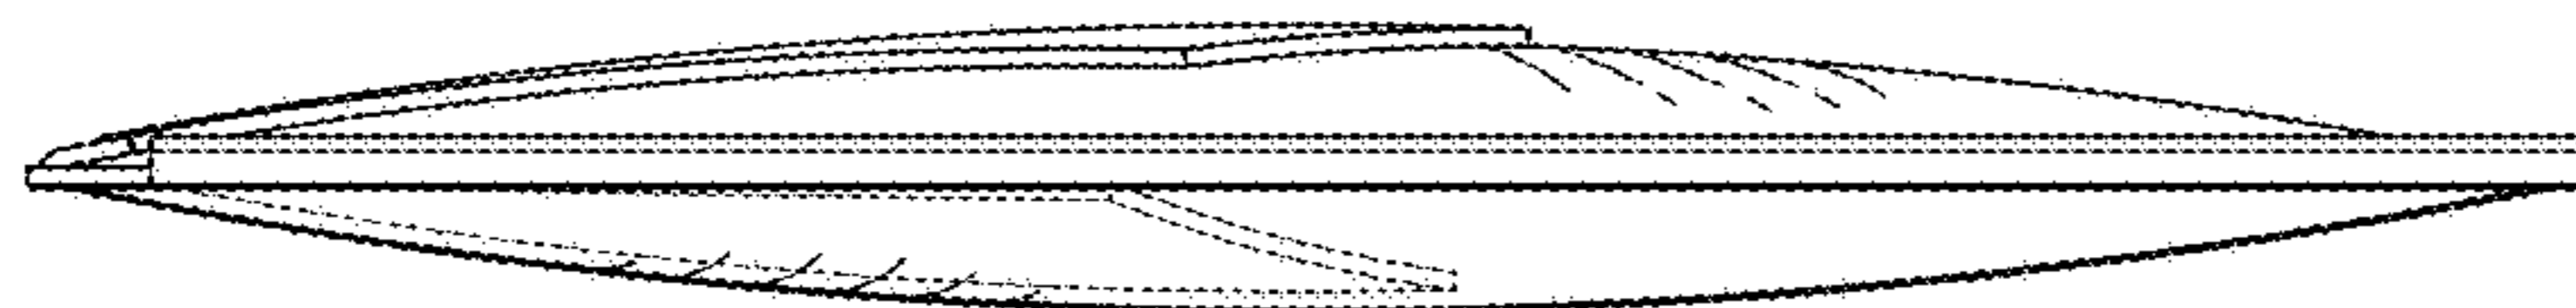


FIG. 7