



US00D834718S

(12) **United States Design Patent** (10) **Patent No.:** **US D834,718 S**
Bobey et al. (45) **Date of Patent:** **** Nov. 27, 2018**

(54) **OUTER COVERING FOR A PERCUSSIVE HIGH FREQUENCY CHEST WALL OSCILLATION SYSTEM**

5,235,967 A 8/1993 Arbisi et al.
D456,591 S 5/2002 Hansen
D461,897 S 8/2002 Hansen
D469,876 S 2/2003 Hansen et al.
D478,989 S 8/2003 Hansen et al.

(71) Applicant: **HILL-ROM SERVICES PTE. LTD.**,
Singapore (SG)

(Continued)

(72) Inventors: **John A. Bobey**, Daniel Island, SC (US); **Deny D. Barilea**, Singapore (SG); **Suresha Ventakaraya**, Singapore (SG); **Wei T. Tan**, Singapore (SG); **Clementine Pirio**, Nantes (FR); **Bryan Chng**, Singapore (SG); **Scott Saunders**, Portland, OR (US); **Damon Clegg**, Portland, OR (US)

OTHER PUBLICATIONS

Hodsden, Suzanne, "Hill-Rom Unveils Mobile, Connected Airway Clearance System for Patients on the Move" May 2, 2017, [online], [site visited Jun. 14, 2018]. Retrieved from Internet: <URL: https://www.meddeviceonline.com/doc/hill-rom-unveils-mobile-connected-airway-clearance-system-for-patients-on-the-move-0001>.*

(Continued)

(73) Assignee: **HILL-ROM SERVICES PTE. LTD.**,
Singapore (SG)

Primary Examiner — Wan Laymon

(74) *Attorney, Agent, or Firm* — Barnes & Thornburg LLP

(**) Term: **15 Years**

(21) Appl. No.: **29/594,780**

(22) Filed: **Feb. 22, 2017**

(51) **LOC (11) Cl.** **28-03**

(52) **U.S. Cl.**
USPC **D24/200**

(58) **Field of Classification Search**
USPC D24/200, 107, 164; D2/828-829
CPC A61H 9/00; A61H 9/005; A61H 9/0071;
A61H 9/0007; A61H 9/0078; A61H
7/004; A61H 23/00; A61H 23/006; A61H
23/02; A61H 23/0218; A61H 23/04;
A61H 2023/045; A41D 13/0518

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,869,537 A * 1/1959 Chu A61H 9/0078
482/112
3,053,250 A * 9/1962 Stubbs A61H 23/0218
601/79

(57) **CLAIM**

The ornamental design for an outer covering for a percussive high frequency chest wall oscillation system, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of an outer covering for a percussive high frequency chest wall oscillation system in accordance with the present design, as viewed from a top right corner thereof;

FIG. 2 is front elevation view thereof;

FIG. 3 is a rear elevation view thereof;

FIG. 4 is a right side elevation view thereof;


FIG. 5 is a left side elevation view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines showing the remainder of the outer covering for a percussive high frequency chest wall oscillation system are directed to environment. None of the broken lines form a part of the claimed design.

1 Claim, 7 Drawing Sheets

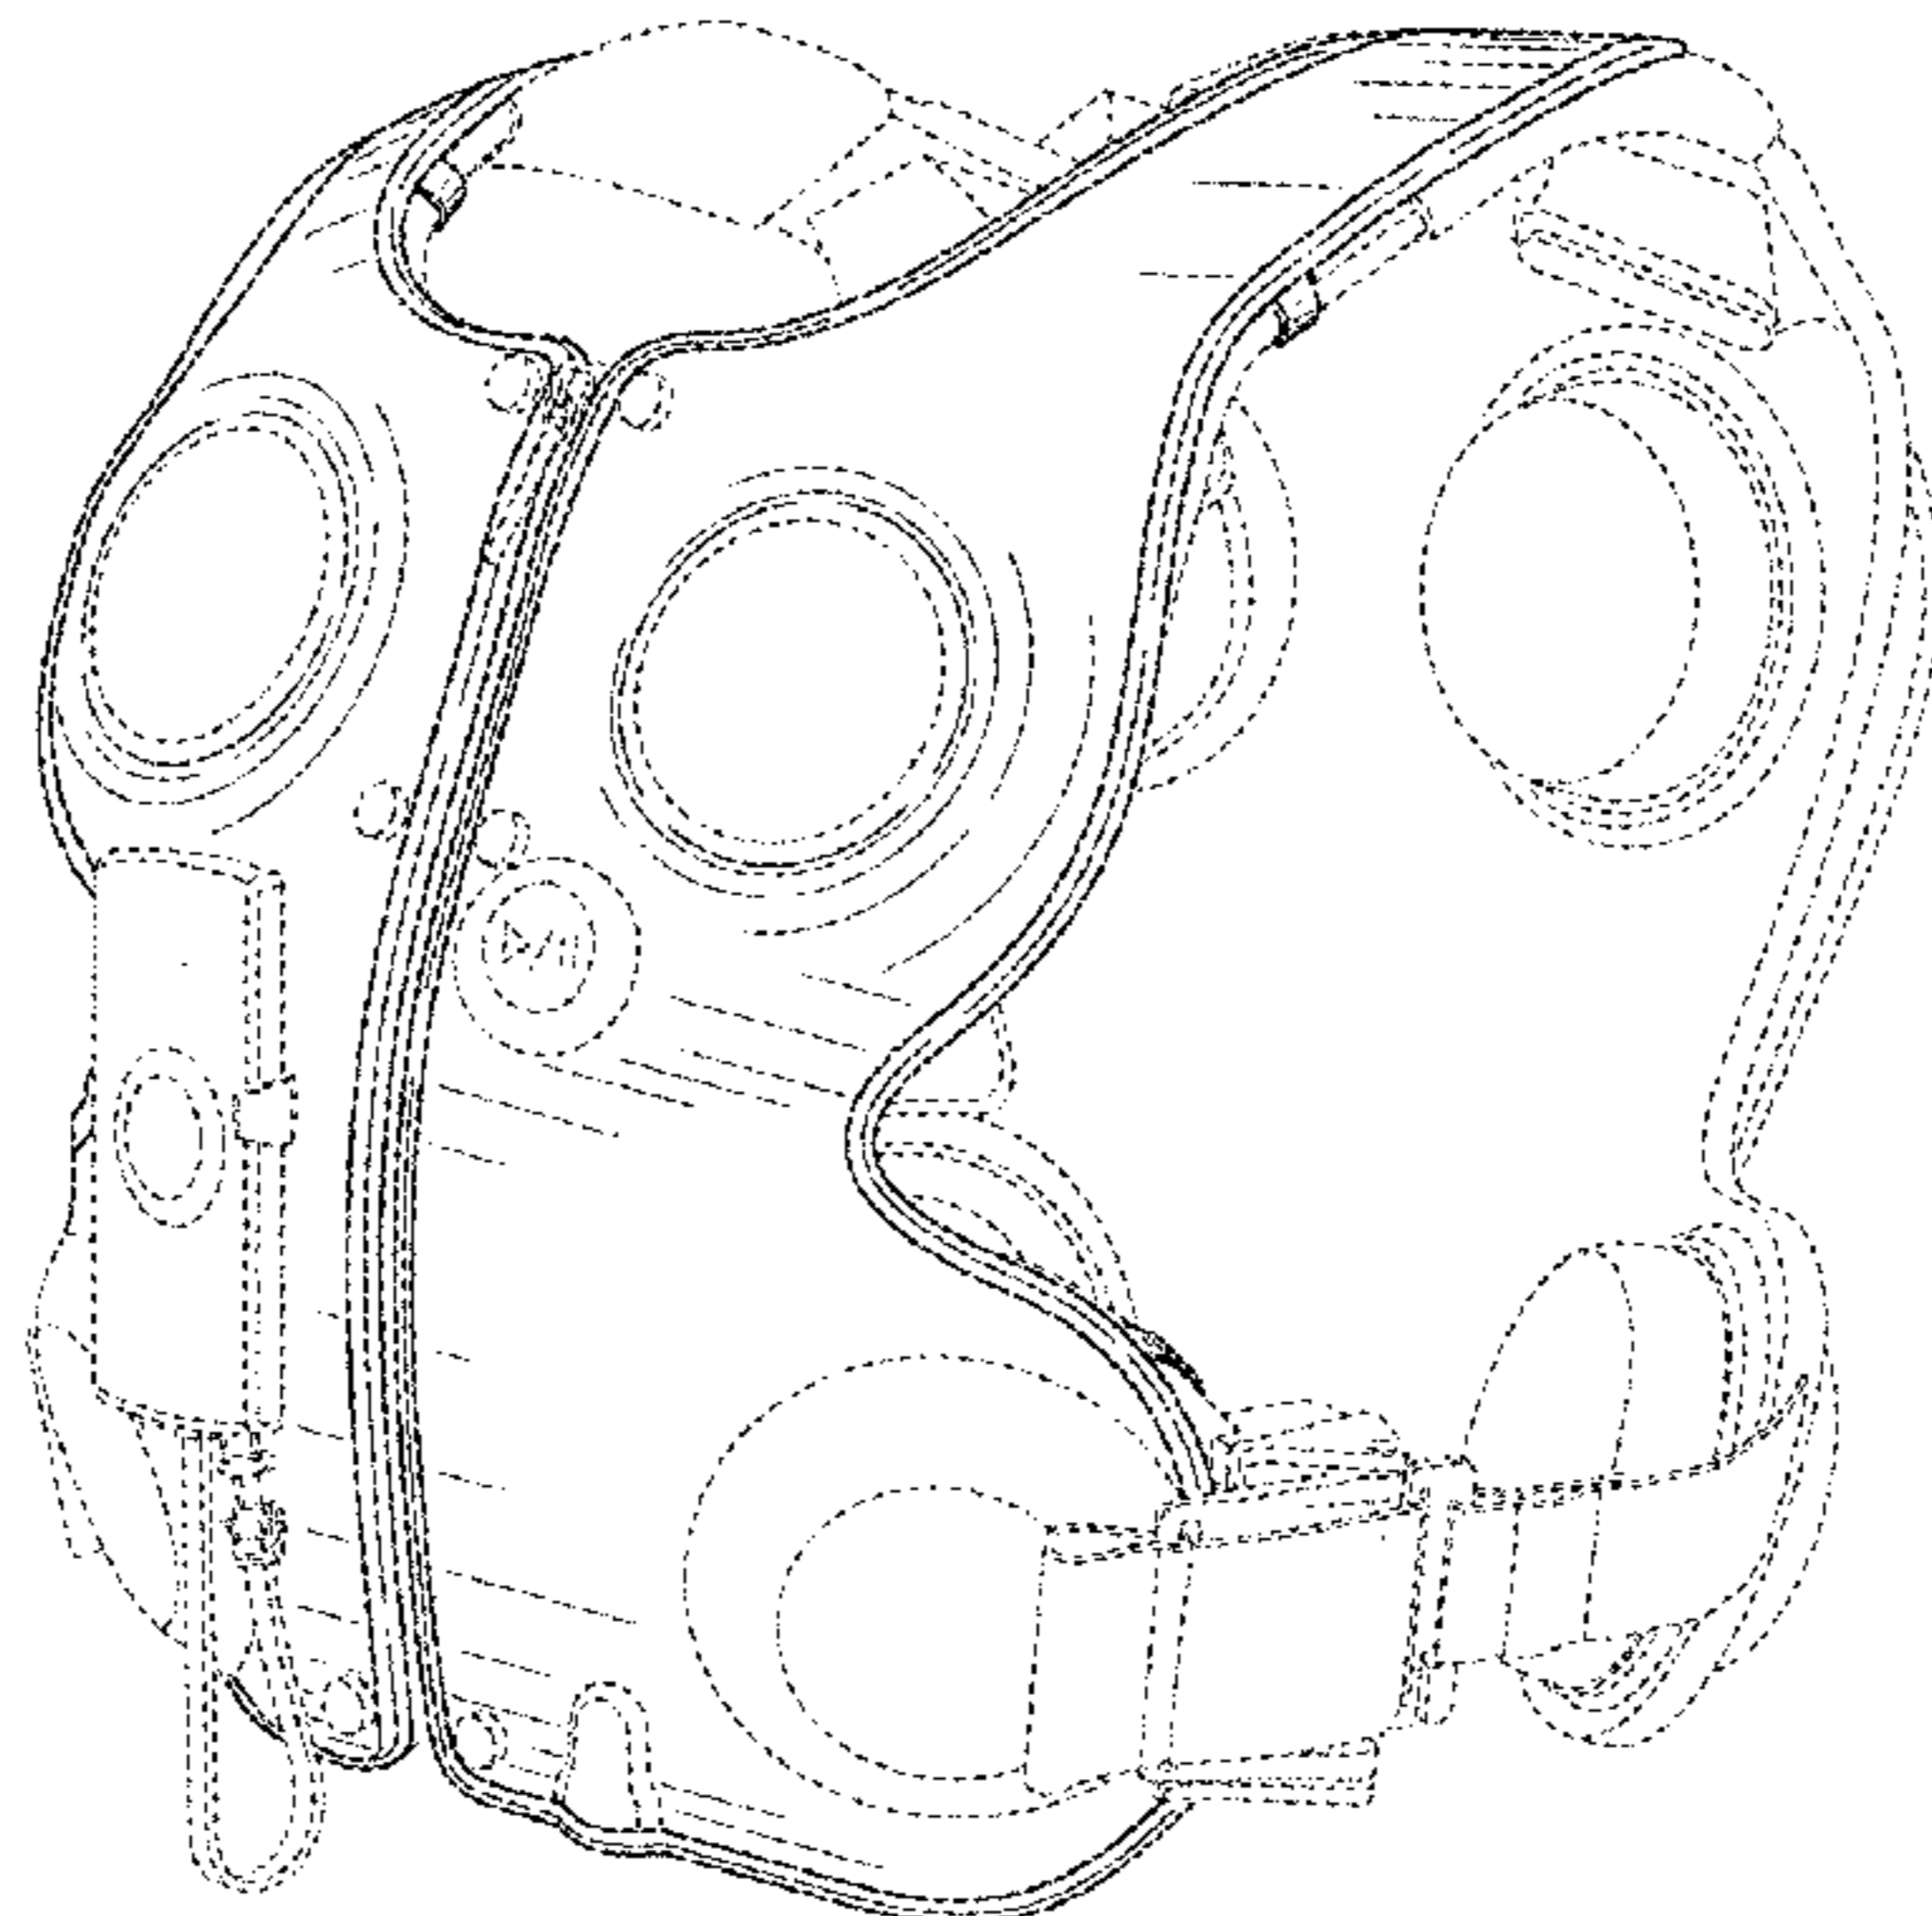

(56)

References Cited

U.S. PATENT DOCUMENTS

7,115,104 B2 * 10/2006 Van Brunt A61H 9/0078
601/41
7,931,607 B2 4/2011 Biondo et al.
D639,954 S 6/2011 Helgeson et al.
8,460,223 B2 6/2013 Huster et al.
D704,849 S * 5/2014 Hunter D24/200
9,237,982 B2 1/2016 Van Brunt
9,549,869 B2 1/2017 DeVlieger et al.
9,968,511 B2 * 5/2018 Huster A61H 9/005
2004/0133133 A1 7/2004 Dreimann et al.
2006/0005306 A1 1/2006 Call et al.
2008/0108914 A1 5/2008 Brouqueyre et al.
2009/0192421 A1 * 7/2009 Huster A61H 9/0078
601/44
2011/0087143 A1 4/2011 Bobey et al.
2012/0291798 A1 11/2012 Park et al.
2014/0005579 A1 1/2014 Drlik et al.
2014/0276271 A1 * 9/2014 Stryker A61H 23/04
601/46
2016/0095790 A1 4/2016 Shockley, Jr. et al.
2018/0049939 A1 * 2/2018 Bobey A61H 9/005

OTHER PUBLICATIONS

Hill-Rom | Respiratory Care | Monarch™ Airway Clearance System 3D Animation Video, published on Jun. 26, 2017, [online], [site visited Jun. 14, 2018]. Retrieved from Internet: <URL: https://www.youtube.com/results?search_query=monarch+airway+clearance+system>.*

* cited by examiner

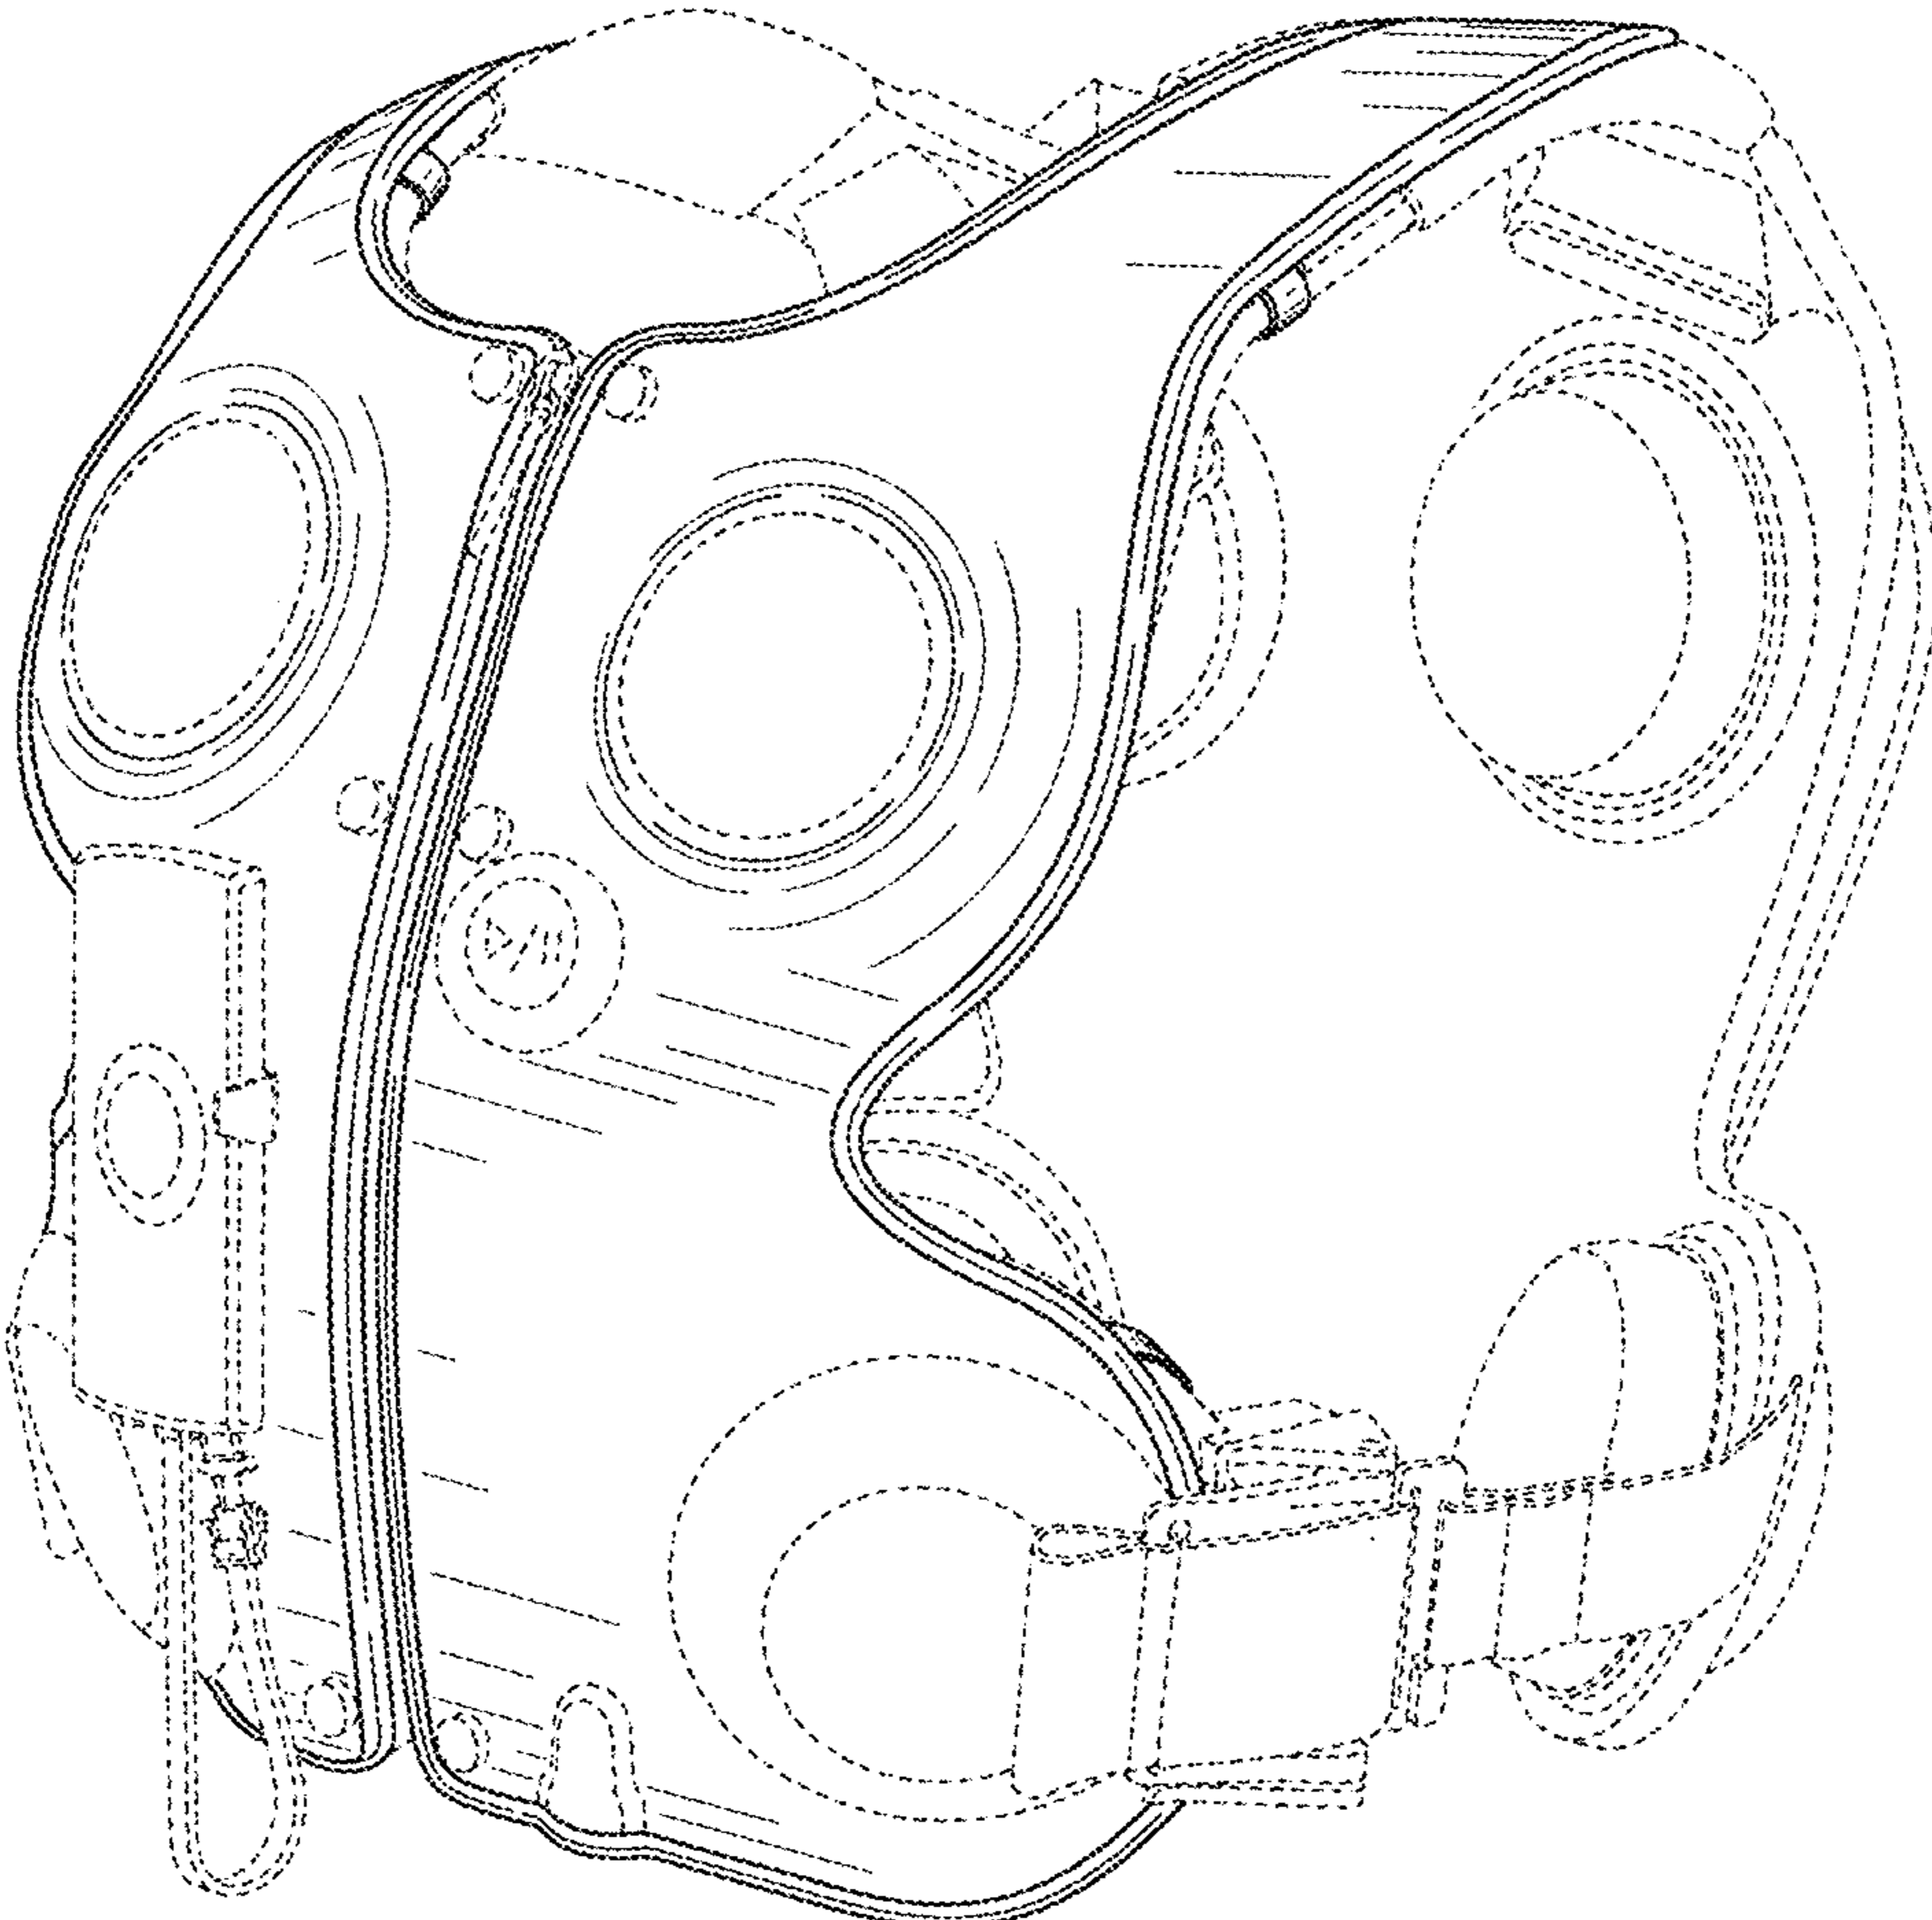


FIG. 1

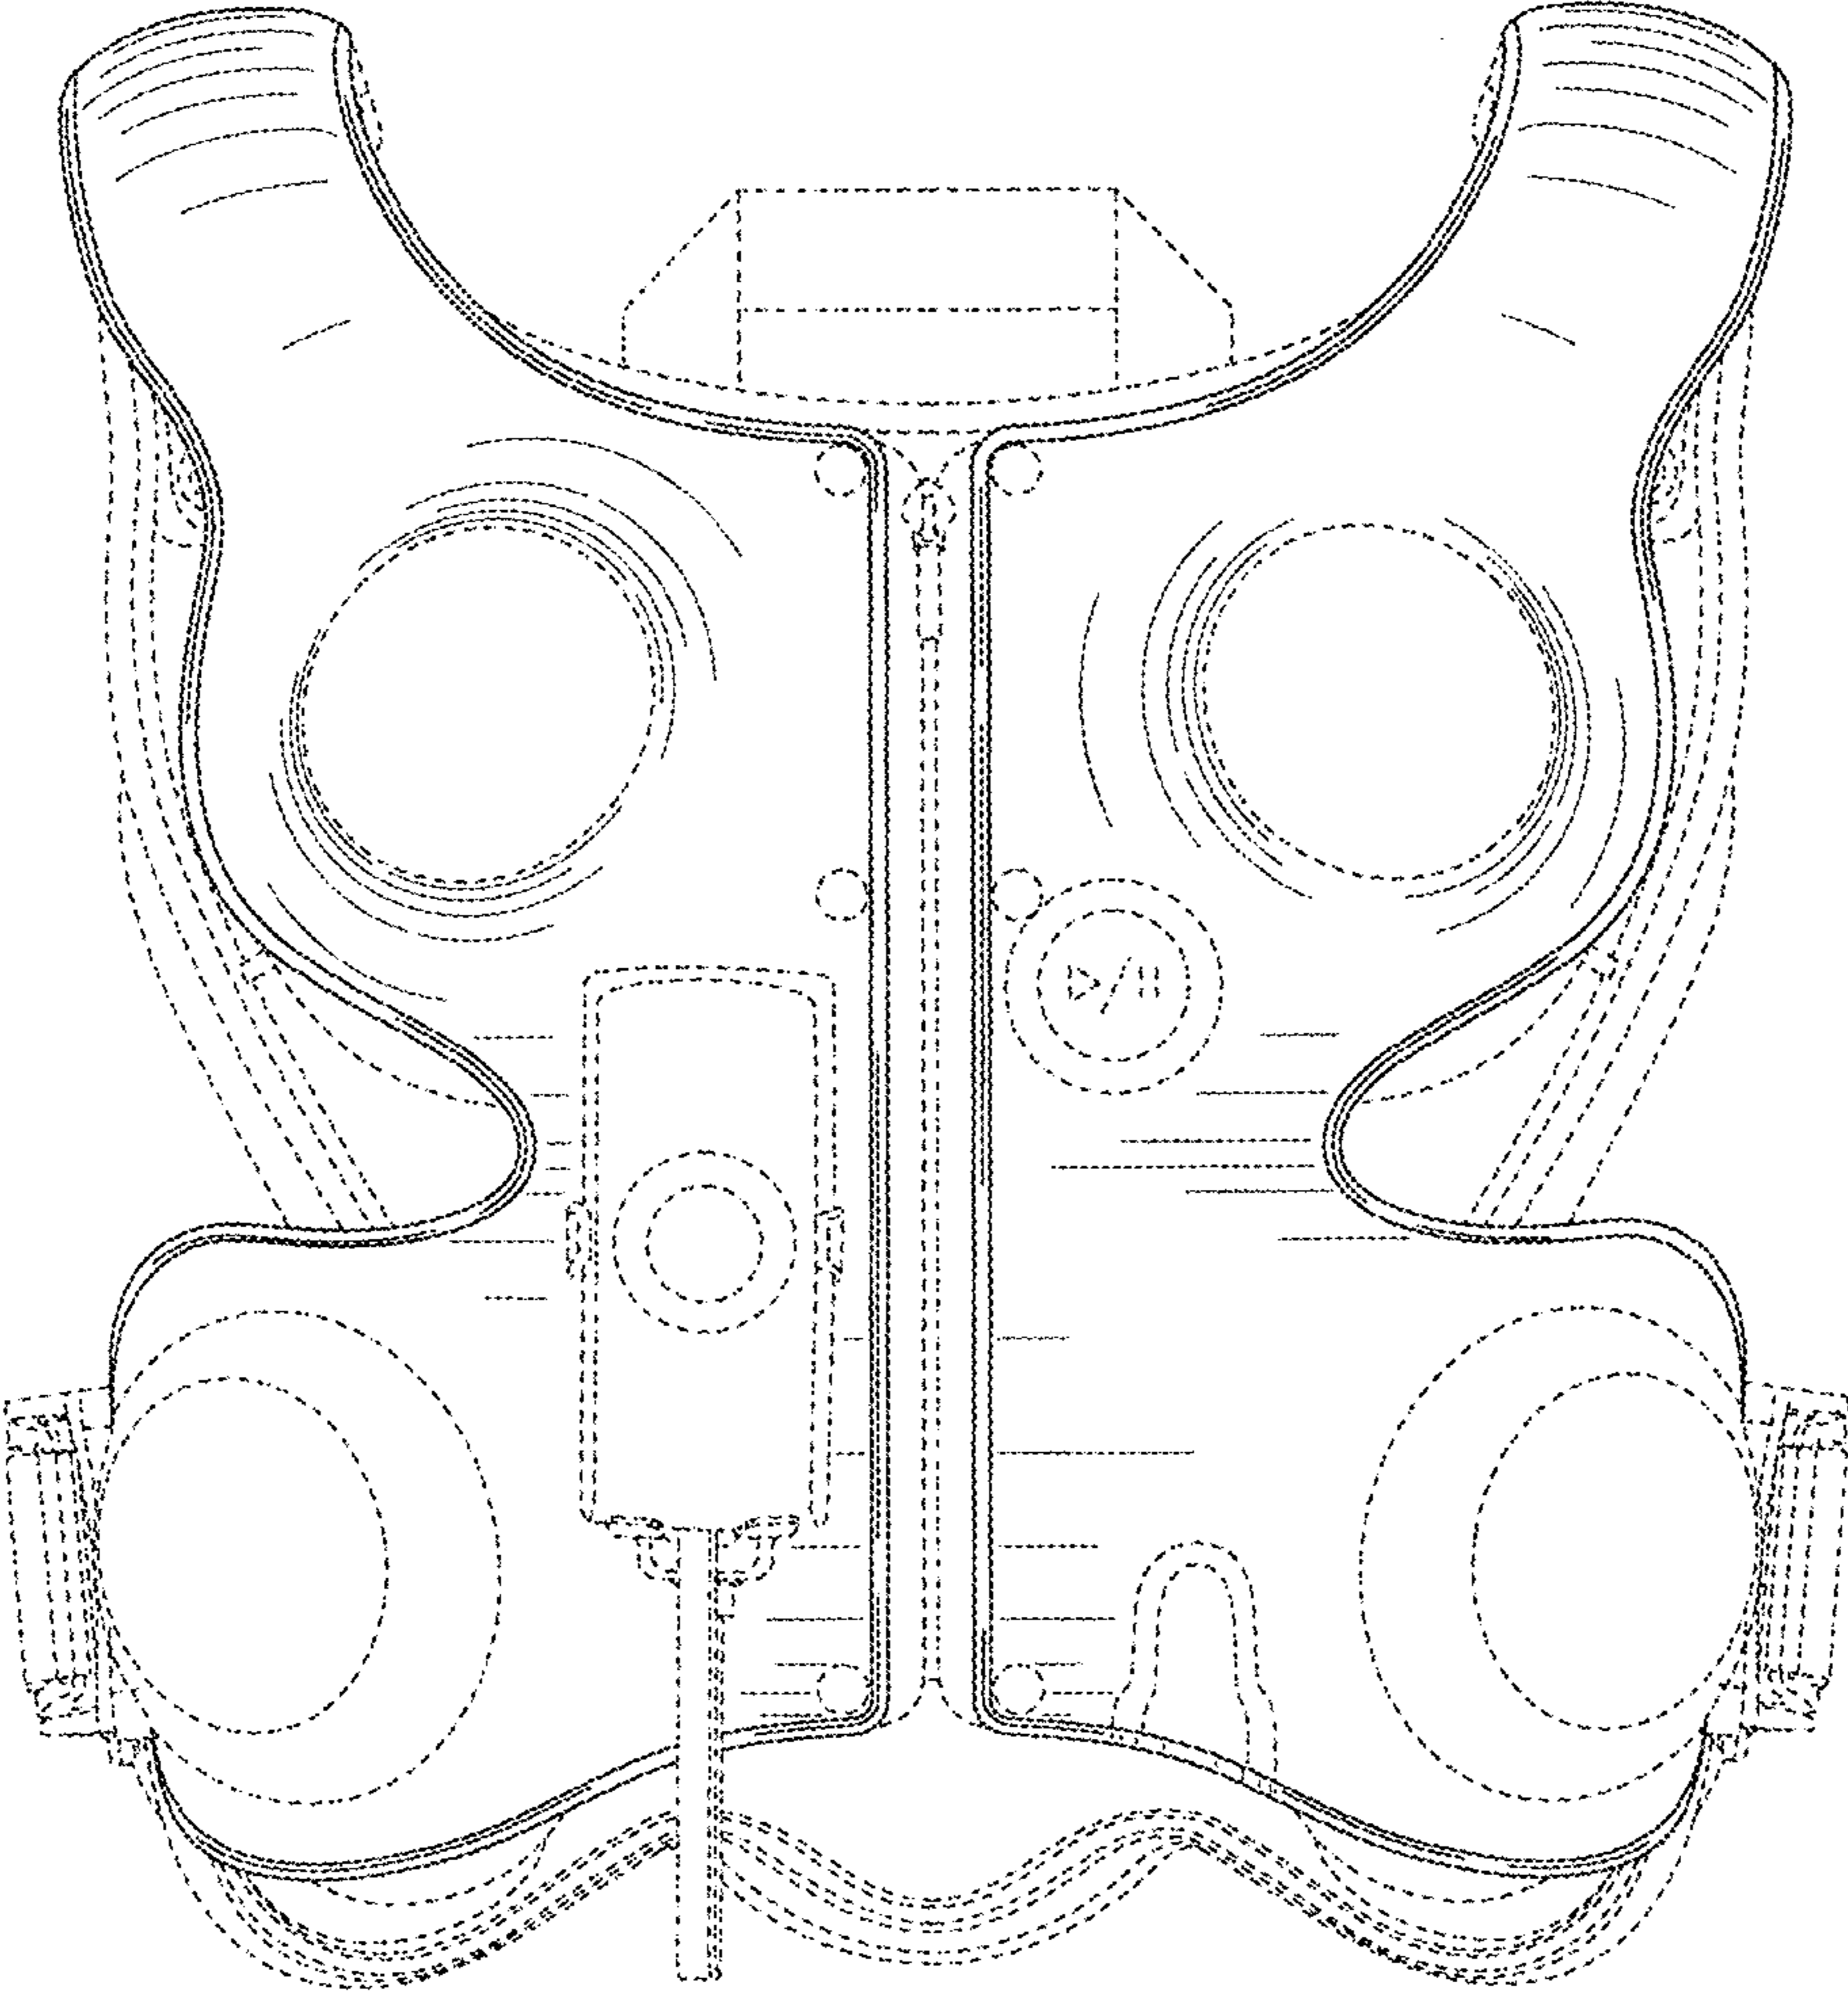


FIG. 2

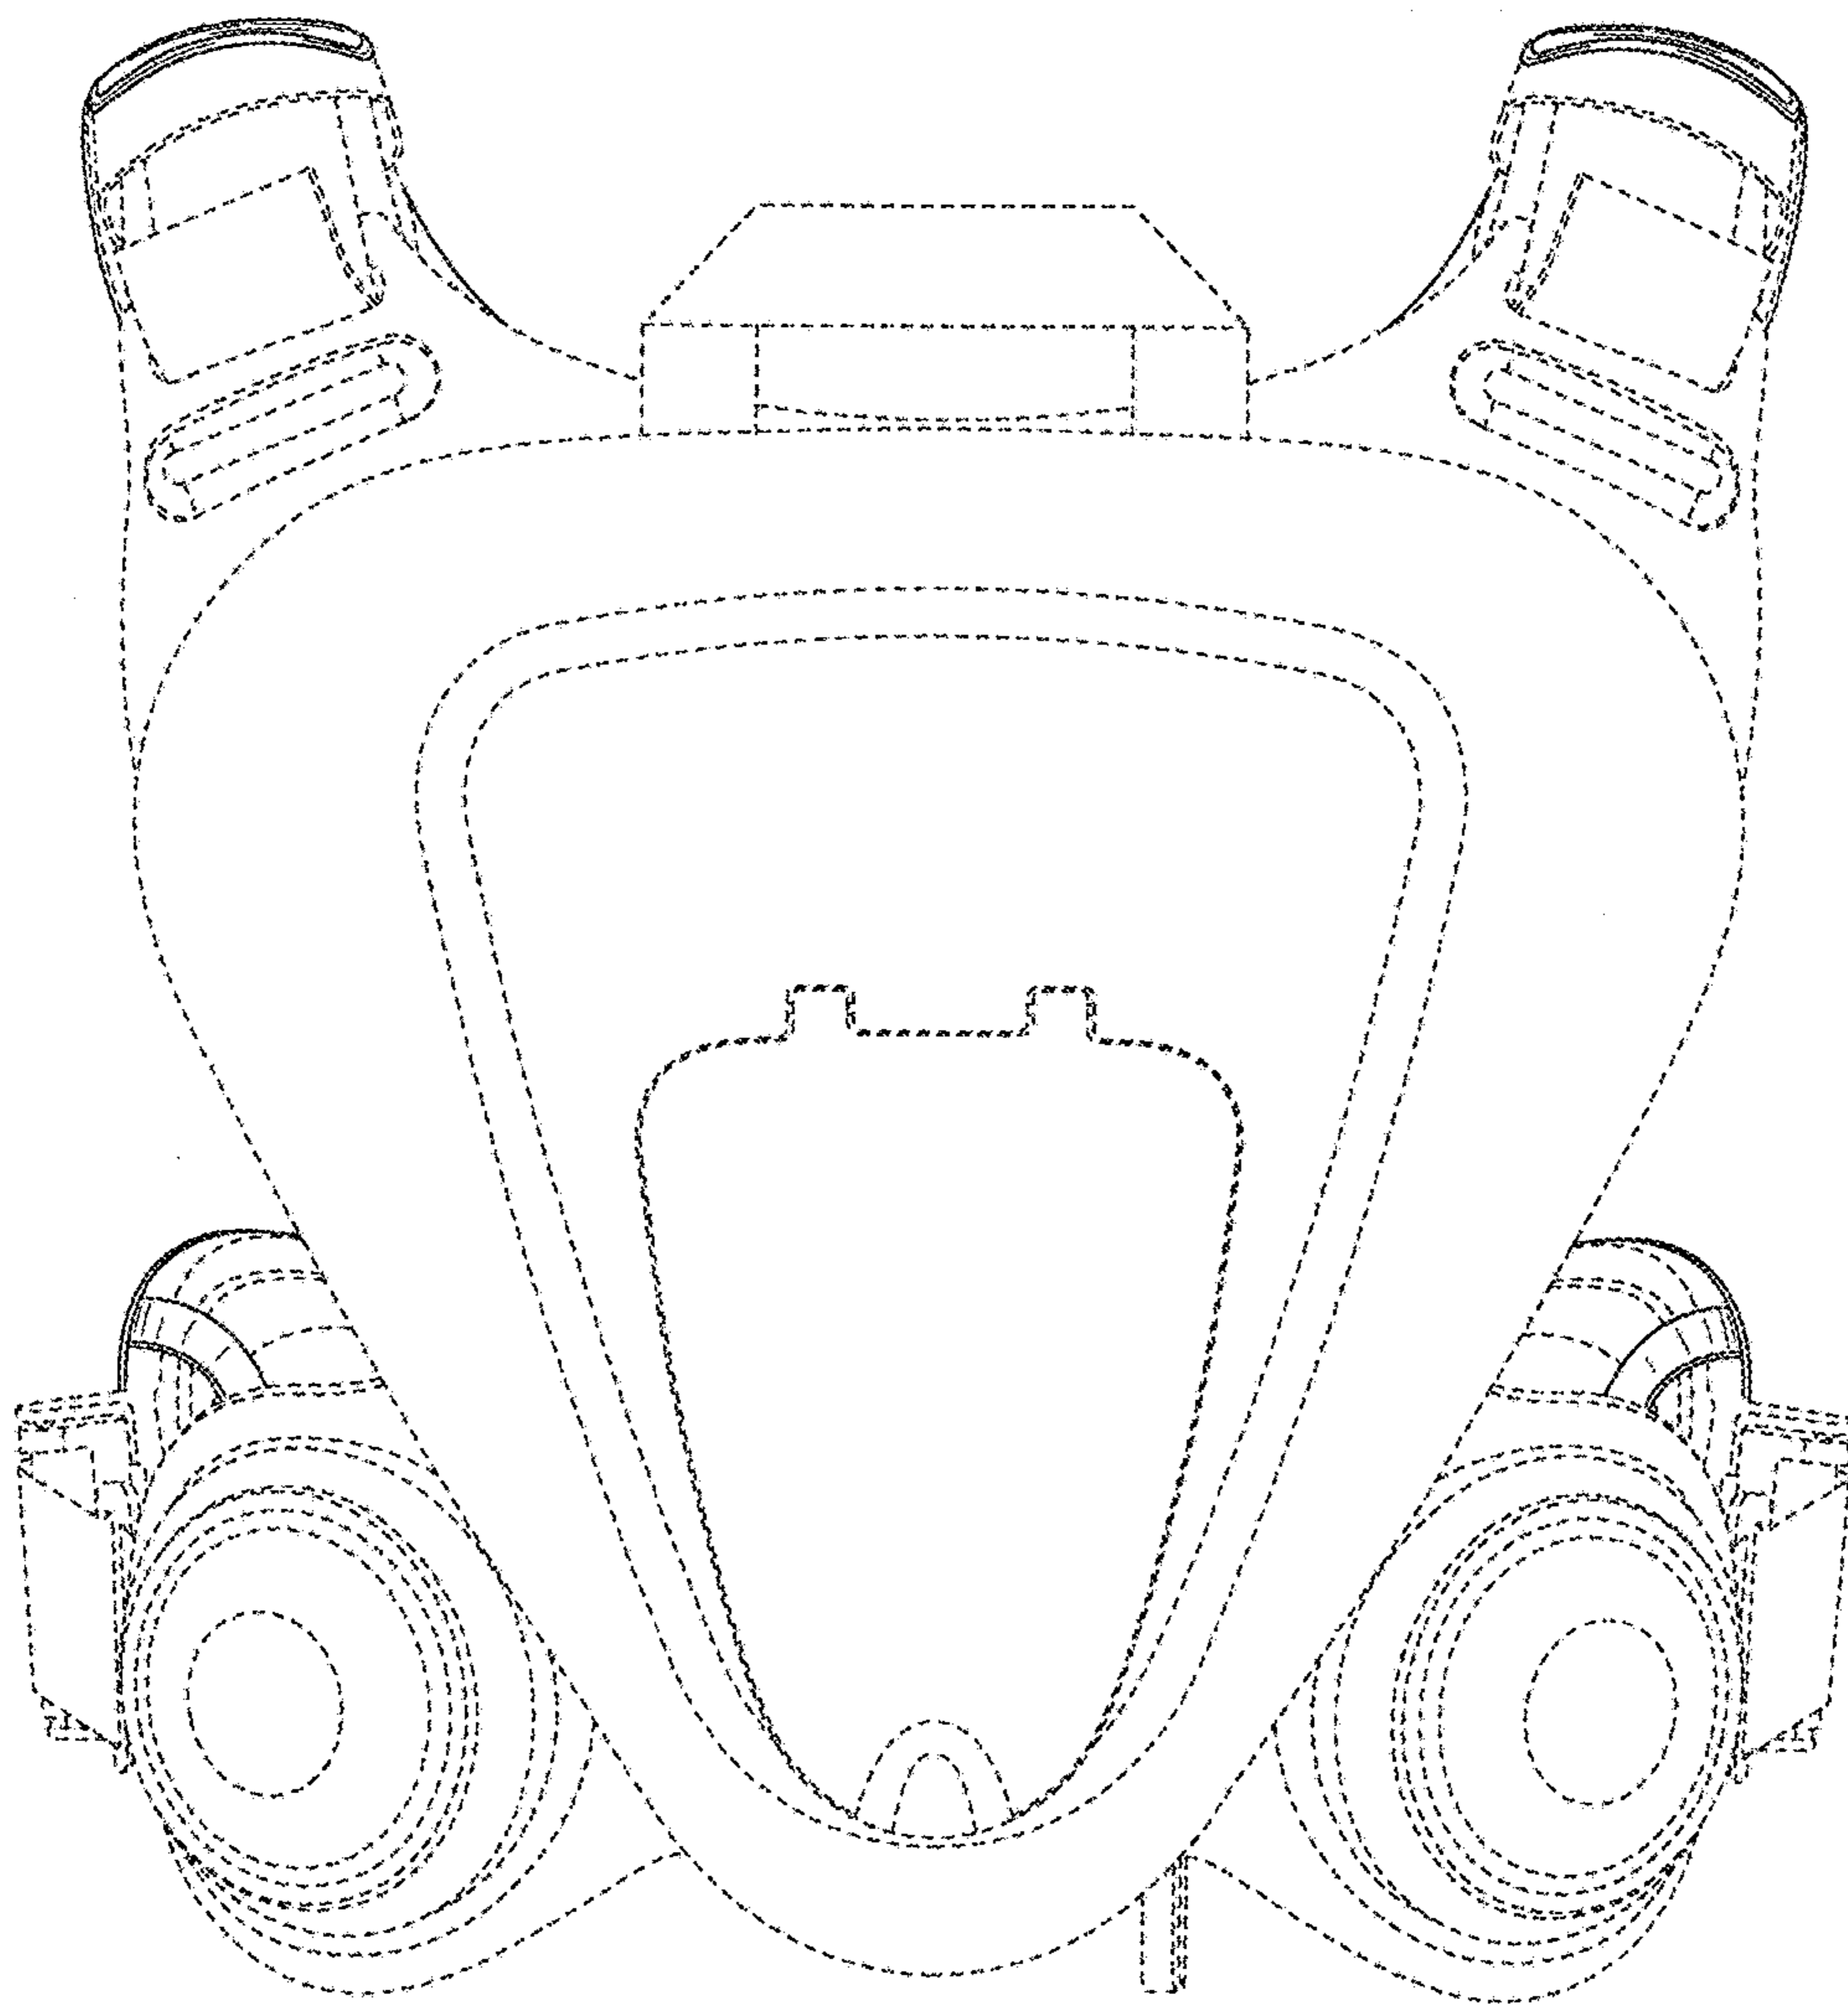


FIG. 3

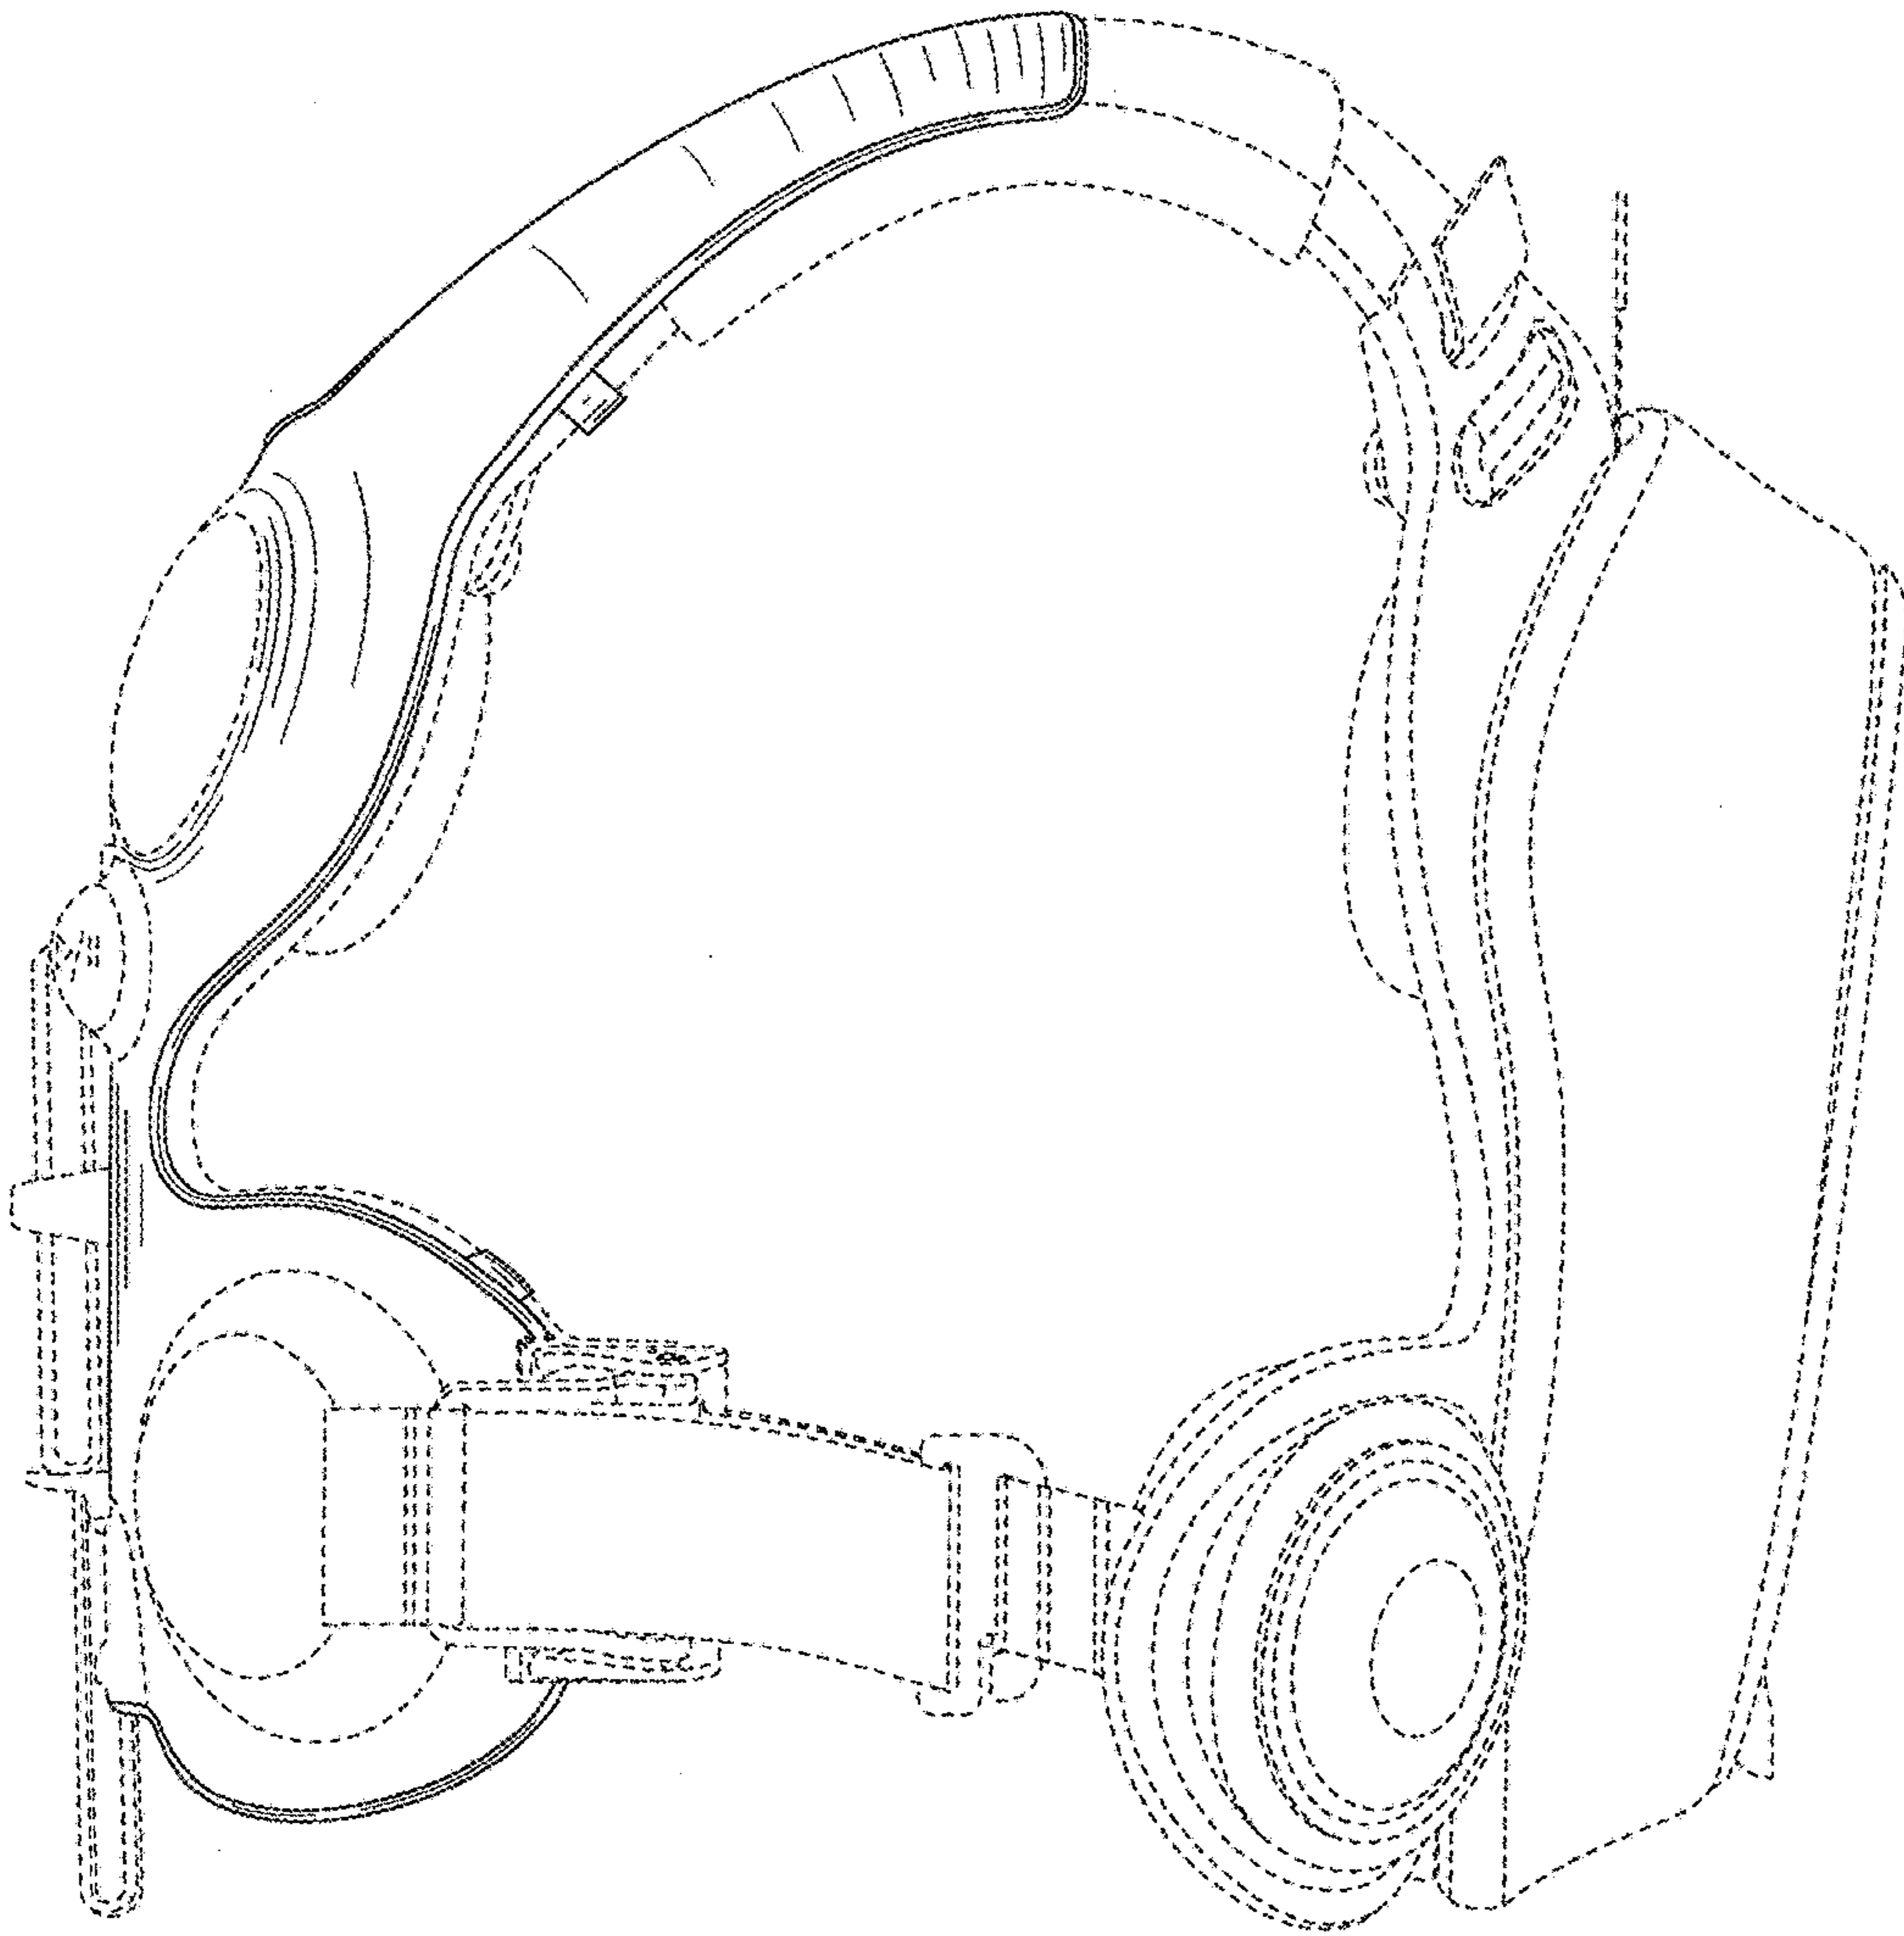


FIG. 4

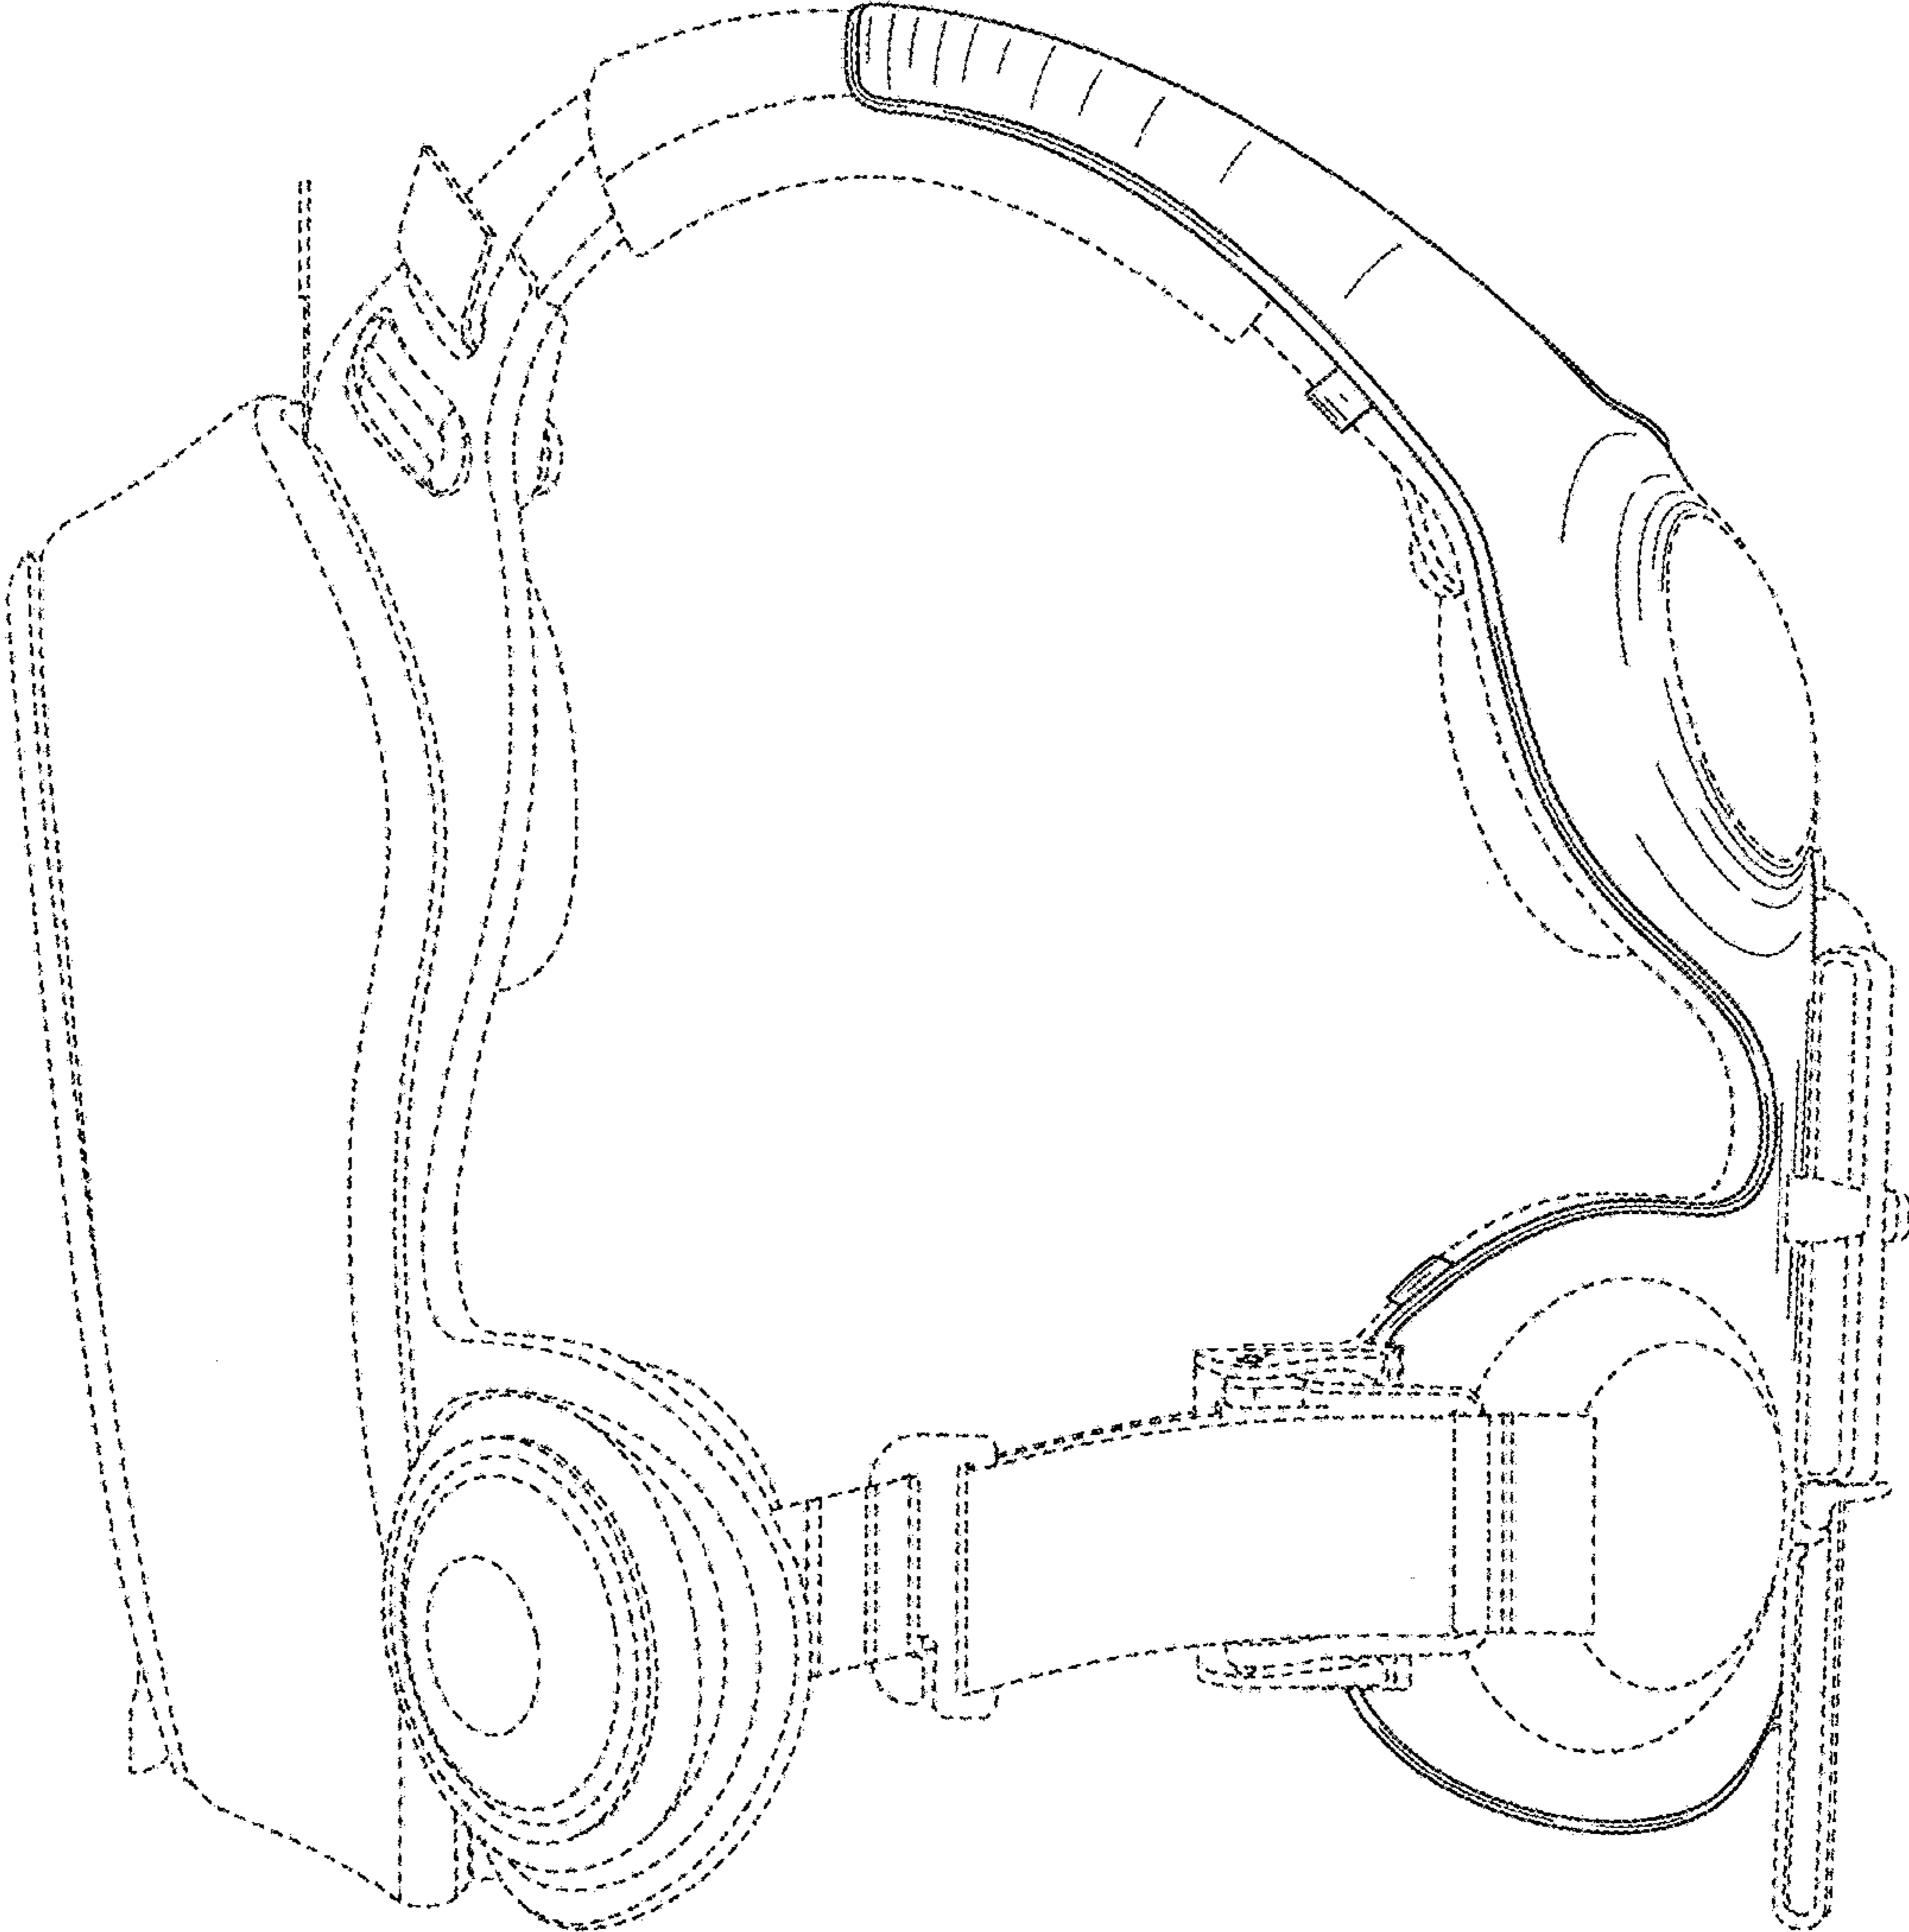


FIG. 5

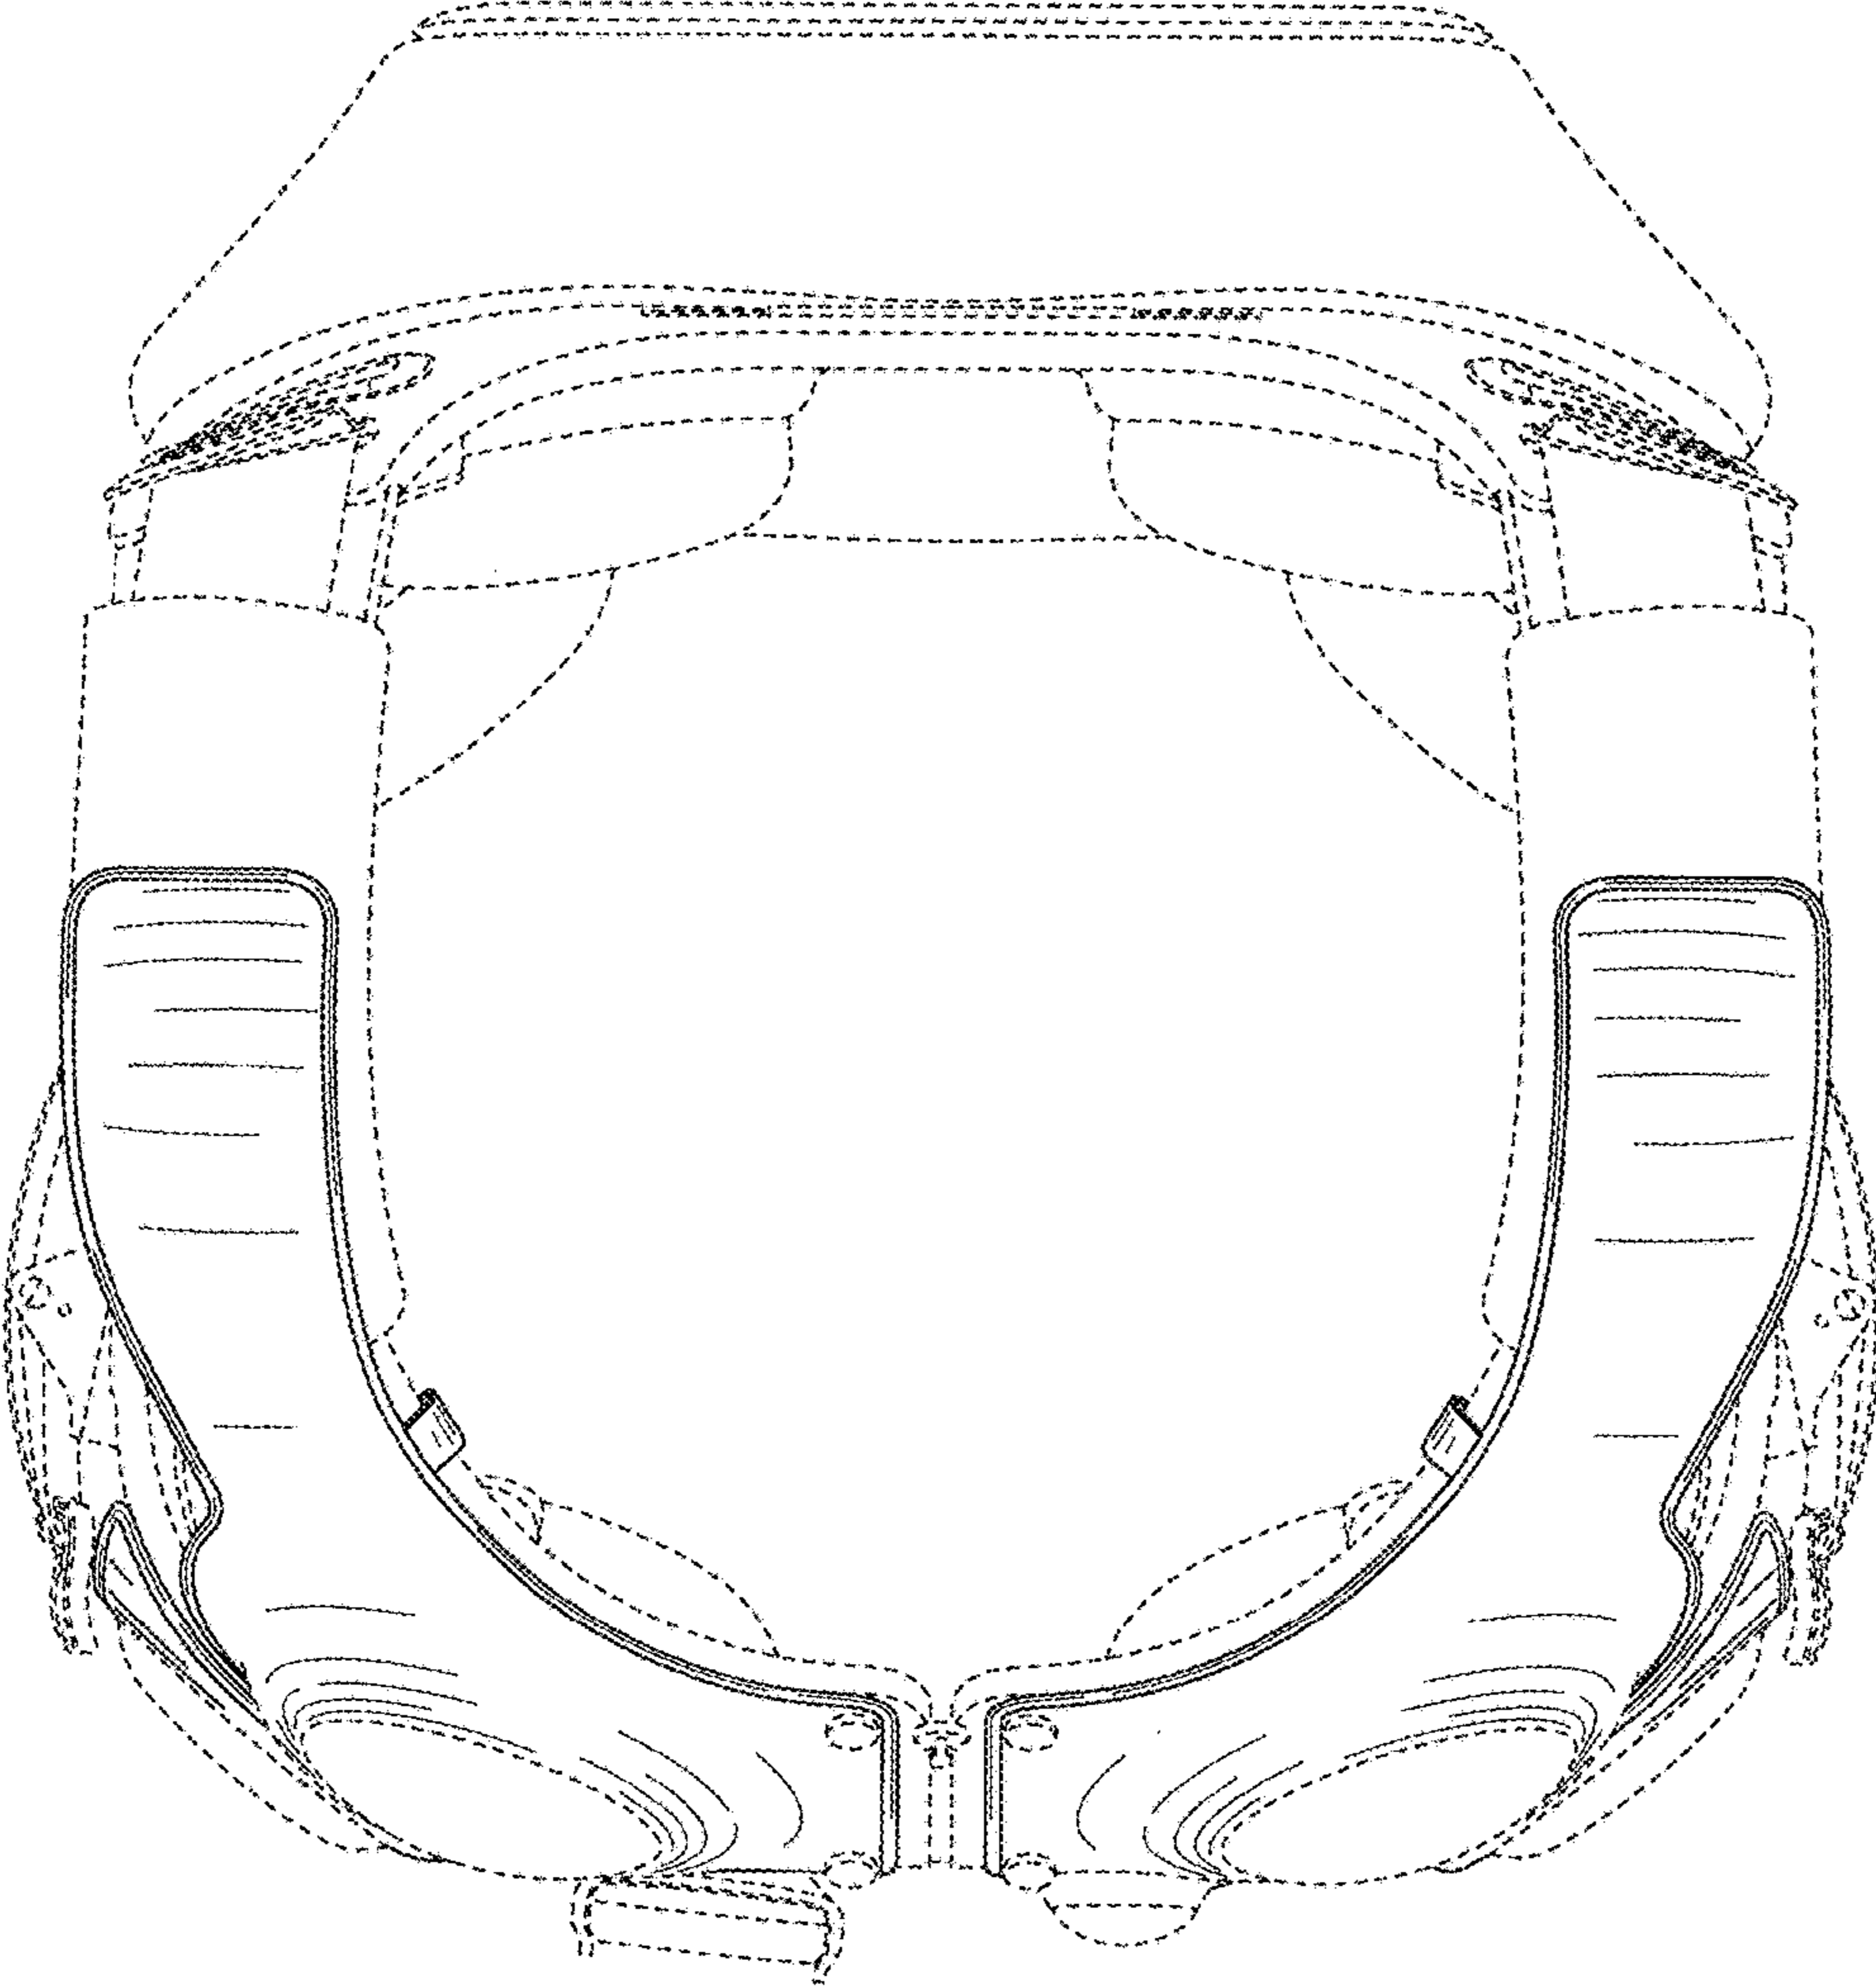


FIG. 6

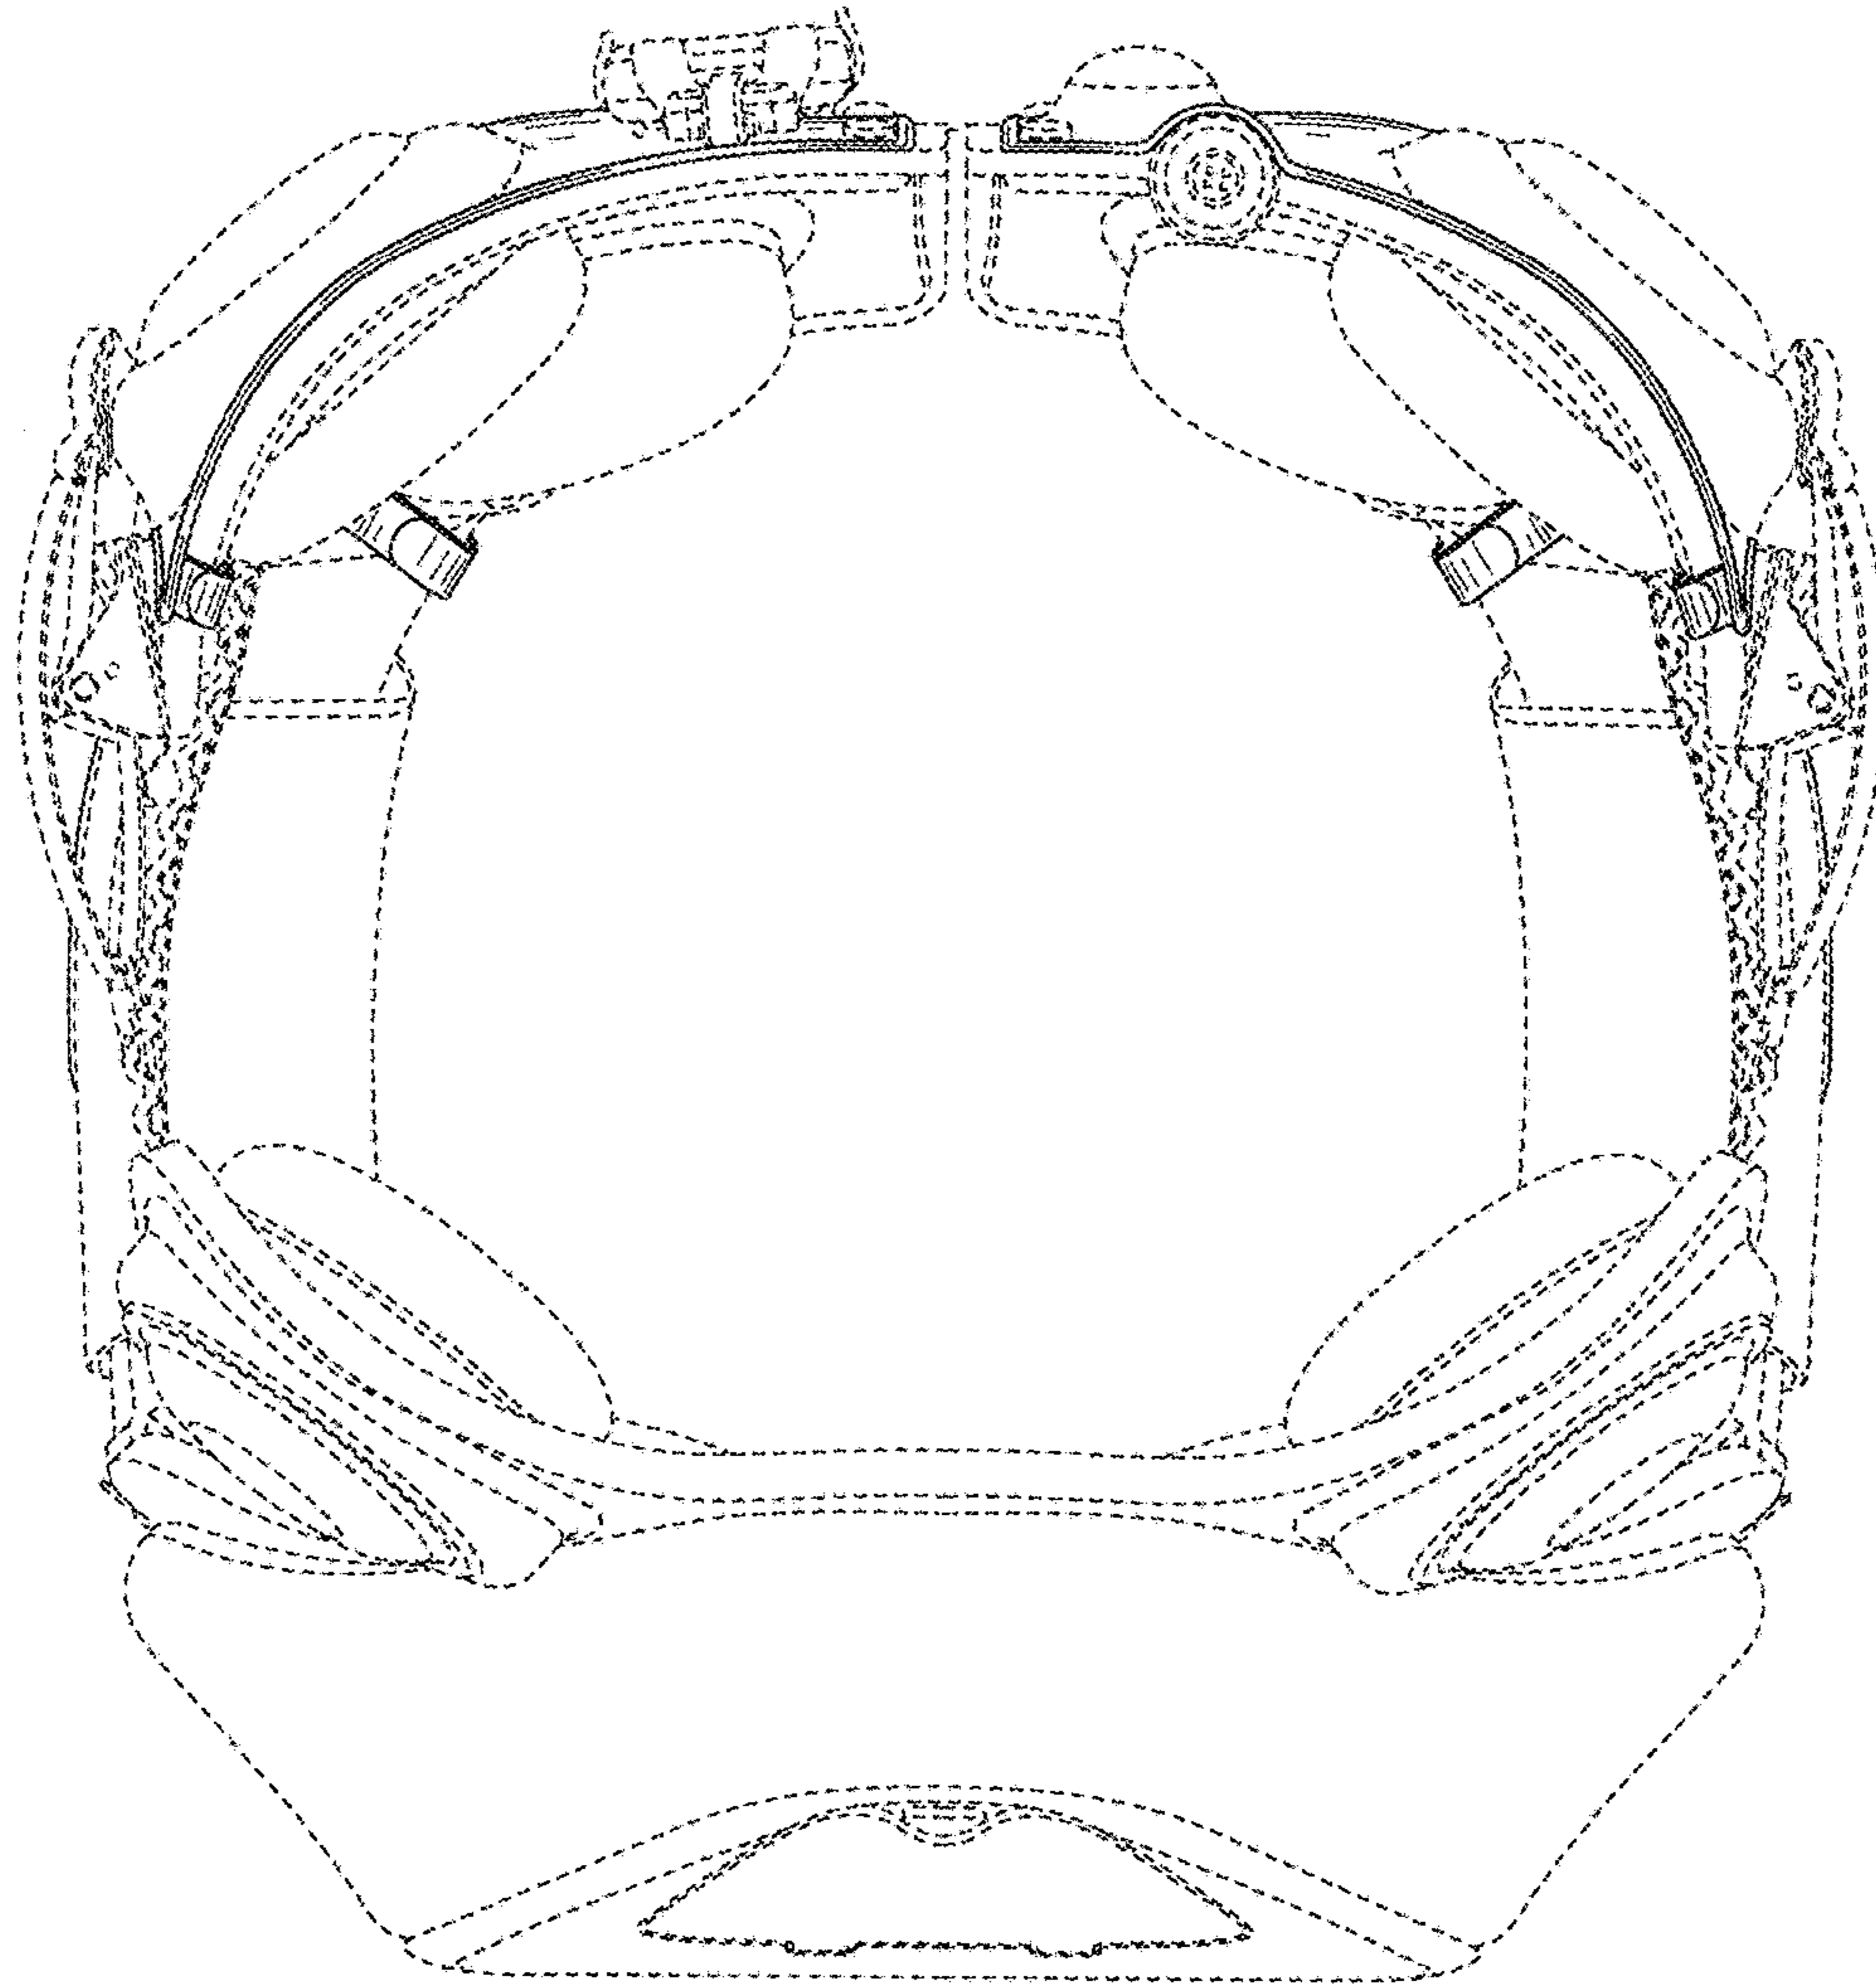


FIG. 7

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D834,718 S
APPLICATION NO. : 29/594780
DATED : November 27, 2018
INVENTOR(S) : John A. Bobey et al.


Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

The last name of the third inventor in item (72), replace "Ventakaraya" with --Venkataraya--.

Signed and Sealed this
Nineteenth Day of February, 2019

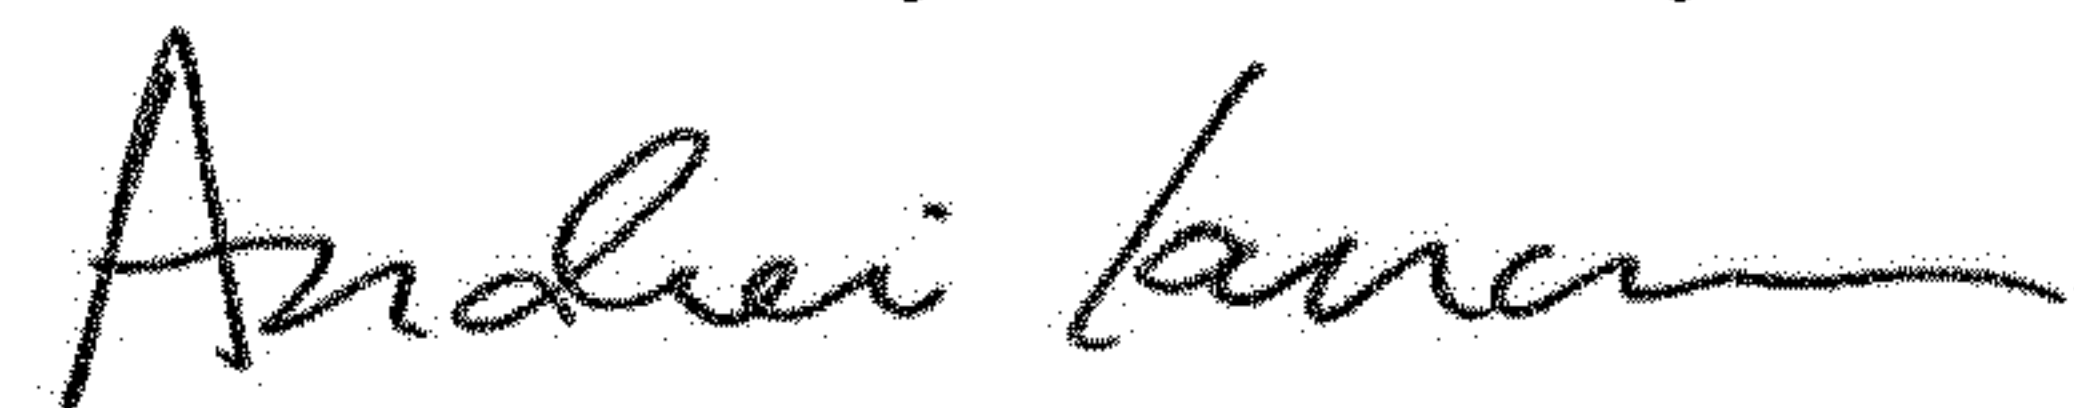

Andrei Iancu
Director of the United States Patent and Trademark Office