



US00D836116S

(12) **United States Design Patent**  
**Fecteau et al.**

(10) **Patent No.:** **US D836,116 S**

(45) **Date of Patent:** **\*\* Dec. 18, 2018**

(54) **DISPLAY SCREEN PORTION WITH GRAPHICAL USER INTERFACE**

(71) Applicant: **ICENTIA INC.**, Québec (CA)

(72) Inventors: **Pierre Fecteau**,  
St-Augustin-de-Desmaures (CA);  
**Germain Éthier**, Québec (CA)

(73) Assignee: **ICENTIA INC.**, Quebec (CA)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/583,407**

(22) Filed: **Nov. 4, 2016**

(51) **LOC (11) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/485**

(58) **Field of Classification Search**  
USPC ..... D14/485-495  
CPC ..... A61B 5/02; A61B 5/044  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

6,370,423	B1 *	4/2002	Guerrero	.....	A61B 5/044 600/509
6,409,659	B1	6/2002	Warner et al.		
D652,048	S *	1/2012	Joseph	.....	D14/485
D677,274	S *	3/2013	Phelan	.....	D14/492
D734,773	S *	7/2015	Barbato	.....	D14/486
2003/0142142	A1 *	7/2003	Jaffe	.....	G01R 13/02 715/810
2008/0097226	A1 *	4/2008	McConnell	.....	A61B 5/0215 600/485
2009/0070054	A1 *	3/2009	Zeng	.....	A61B 5/044 702/67
2013/0096394	A1 *	4/2013	Gupta	.....	A61B 5/04012 600/301
2014/0107541	A1 *	4/2014	Sullivan	.....	A61B 5/7217 601/41
2015/0297104	A1 *	10/2015	Chen	.....	A61B 5/04001 600/377

(Continued)

**OTHER PUBLICATIONS**

P. Kathirvel et al., "An Efficient R-peak Detection Based on New Nonlinear Transformation and First-Order Gaussian Differentiator", Cardiovascular Engineering and Technology, vol. 2, No. 4, Dec. 2011, pp. 408-425, India.

(Continued)

*Primary Examiner* — Richelle G Shelton

(74) *Attorney, Agent, or Firm* — Norton Rose Fulbright Canada LLP; Alexandre Daoust

(57) **CLAIM**

The ornamental design for a display screen portion with graphical user interface, as shown and described.

**DESCRIPTION**

The file of this patent contains at least one drawing/photograph executed in color. Copies of this patent with color drawing(s)/photograph(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a first view of a display screen portion with graphical user interface showing our new design, in accordance with a first embodiment;



FIG. 2 is a second view in accordance with a second embodiment;

FIG. 3 is a third view in accordance with a third embodiment; and,

FIG. 4 is a fourth view in accordance with a fourth embodiment.

The dashed line showing is included for the purpose of illustrating a display screen portion and forms no part of the claimed design.

**1 Claim, 4 Drawing Sheets**  
**(4 of 4 Drawing Sheet(s) Filed in Color)**

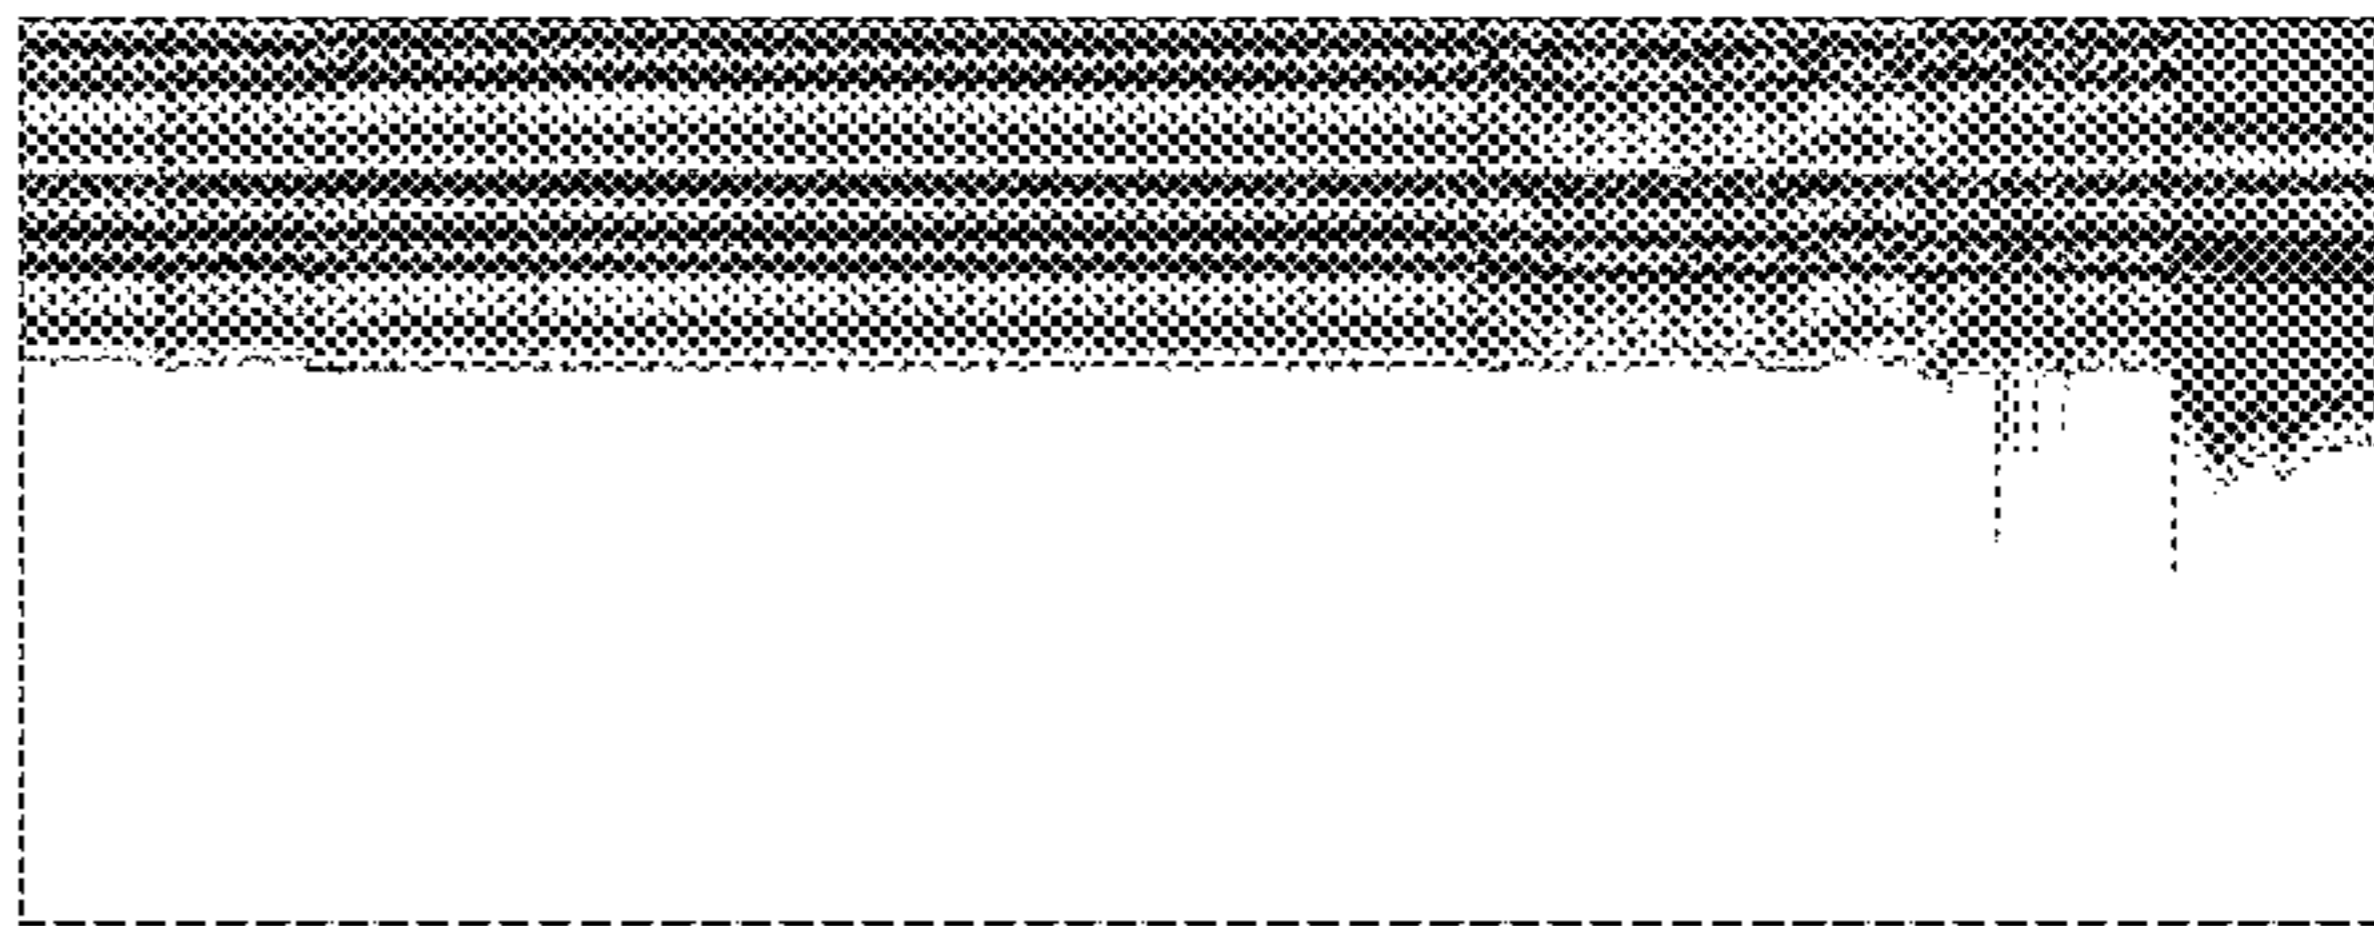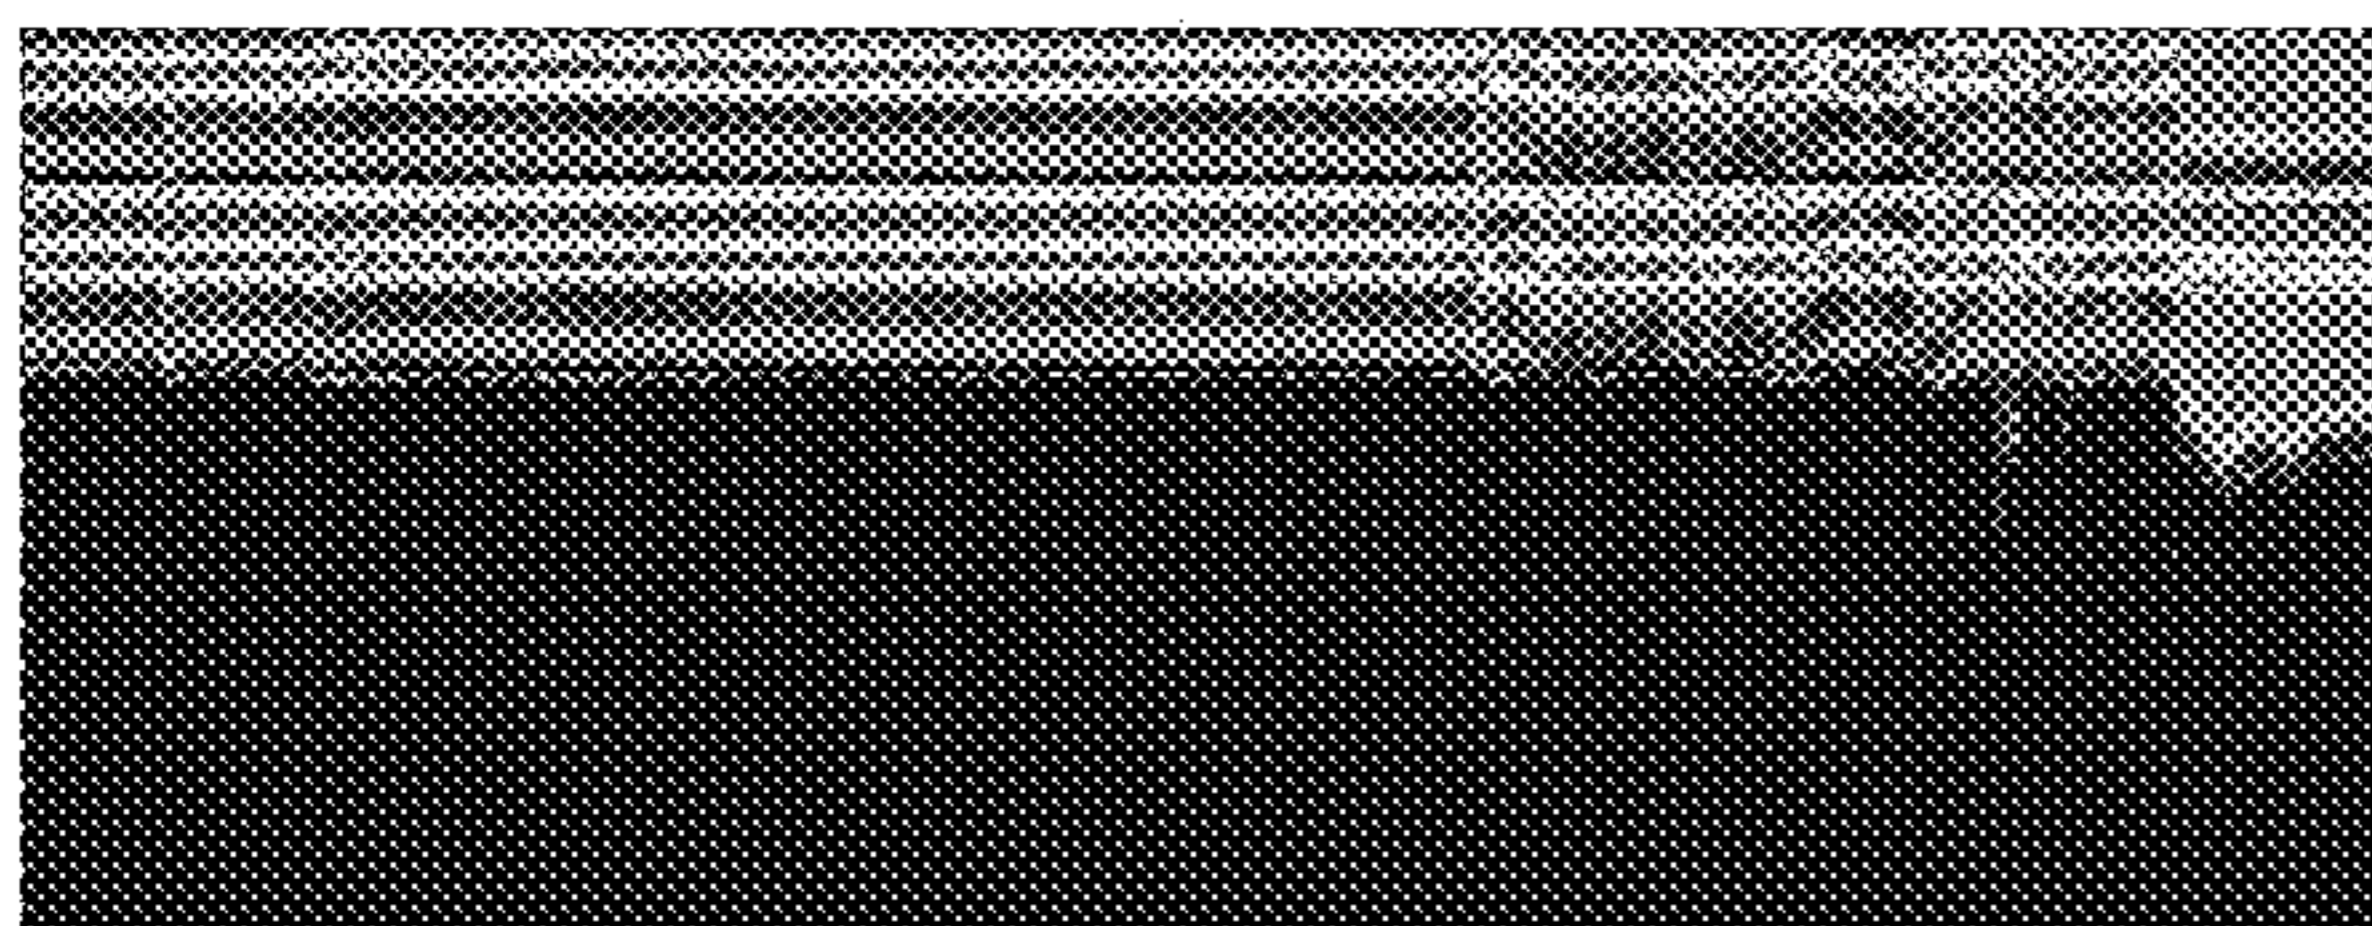

(56)

**References Cited**

U.S. PATENT DOCUMENTS


2016/0058318 A1\* 3/2016 Borjigin ..... A61B 5/04015  
600/516  
2016/0143594 A1\* 5/2016 Moorman ..... A61B 5/02405  
705/2  
2016/0192853 A1\* 7/2016 Bardy ..... A61B 5/02405  
600/382  
2016/0206921 A1\* 7/2016 Szabados ..... A61B 5/0024  
2016/0292894 A1\* 10/2016 Huang ..... G06T 11/206  
2016/0331258 A1\* 11/2016 Du ..... A61B 5/04012  
2017/0196472 A1\* 7/2017 Felix ..... A61B 5/0402

OTHER PUBLICATIONS

Warner, R.A. et al, "Marquette Waterfall Display", GE Healthcare,  
Apr. 2002, General Electric Company, U.S.A.  
"Schiller's Medilog Holter system", Schiller The Art of Diagnos-  
tics, 2013, Switzerland.

\* cited by examiner



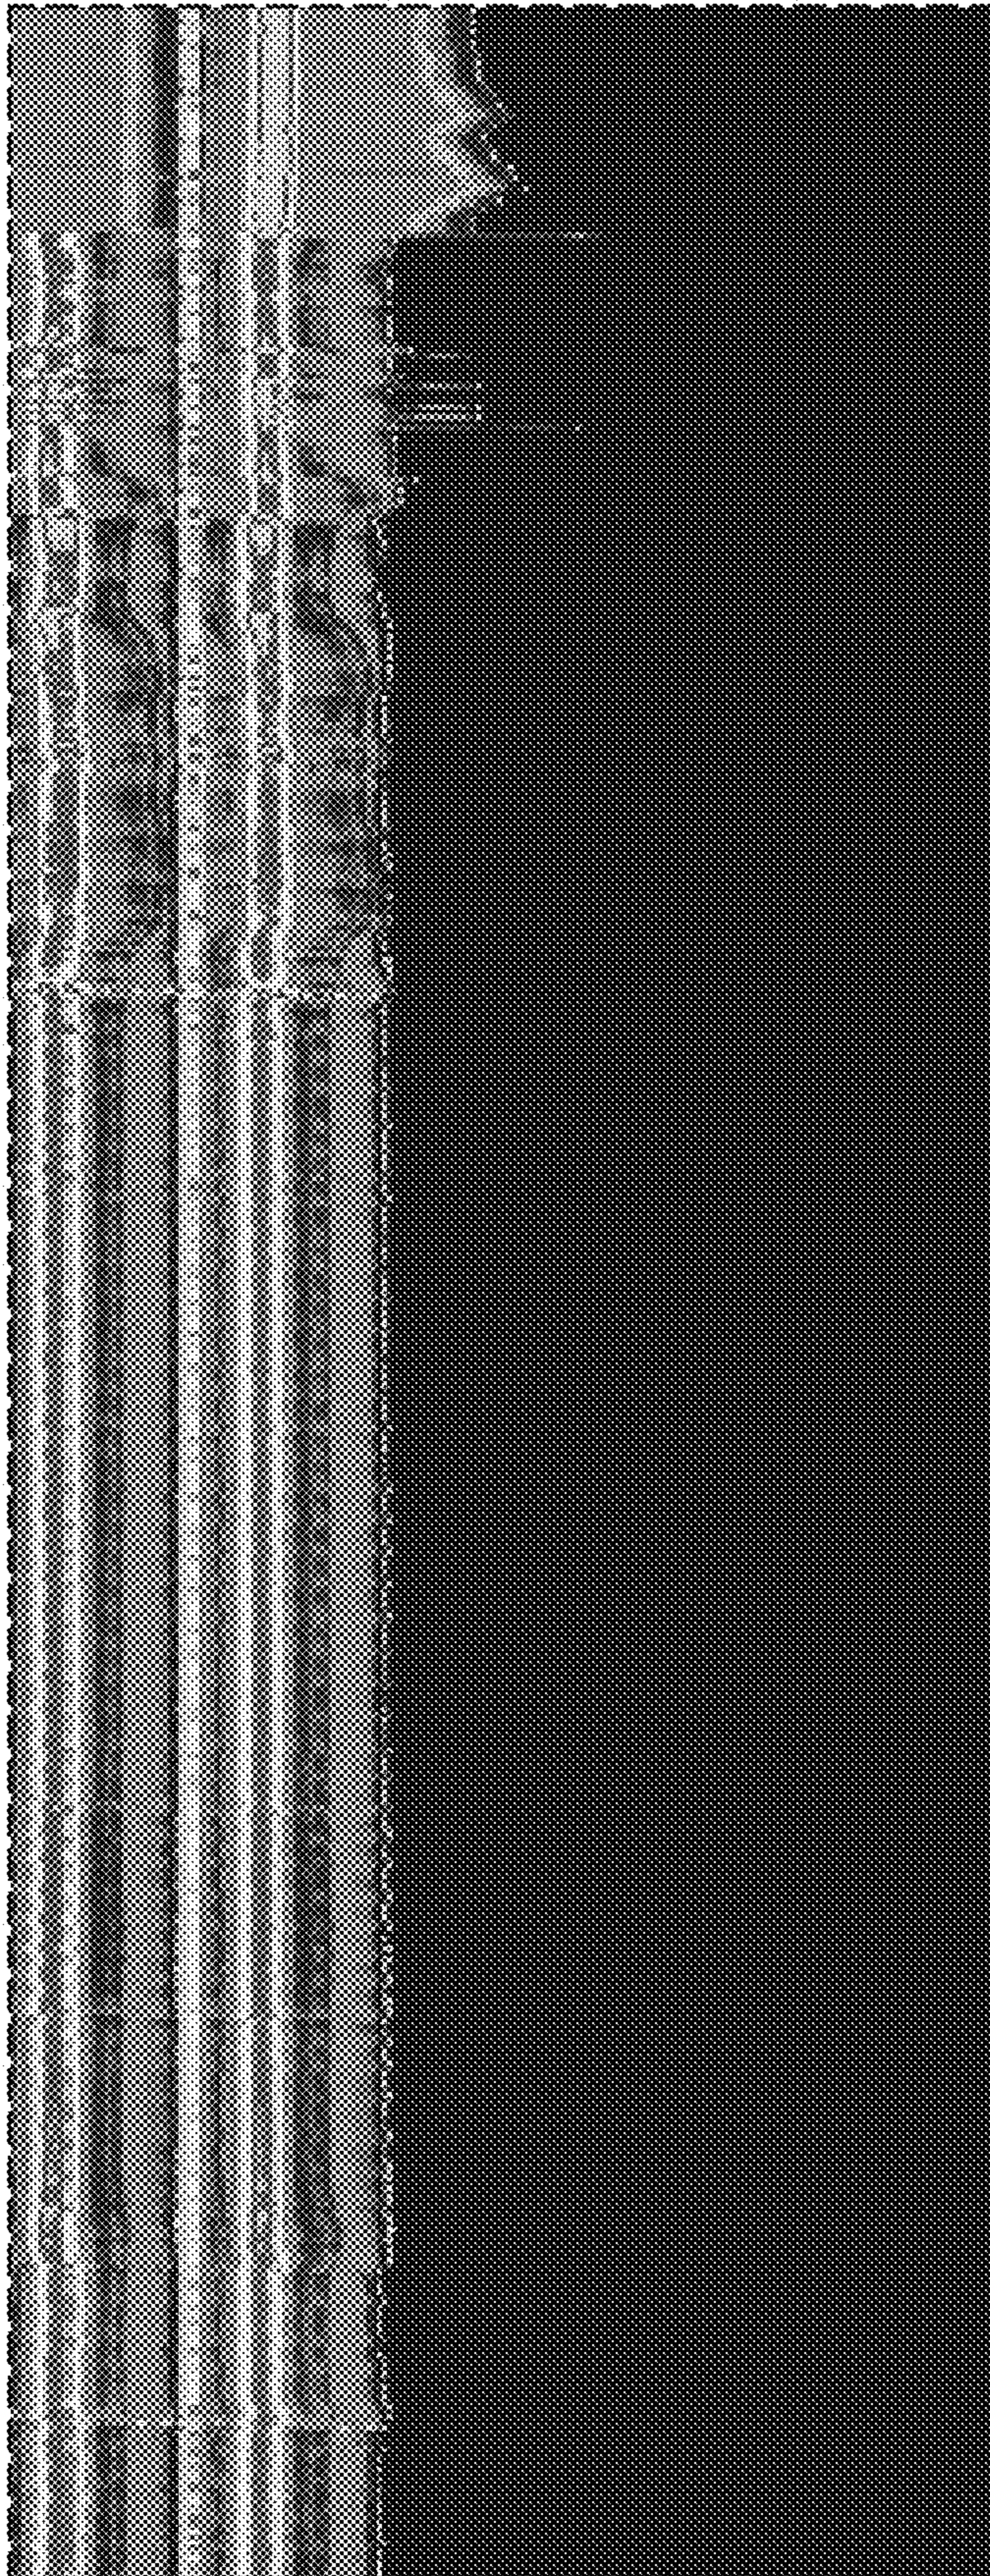

*FIG. 1*



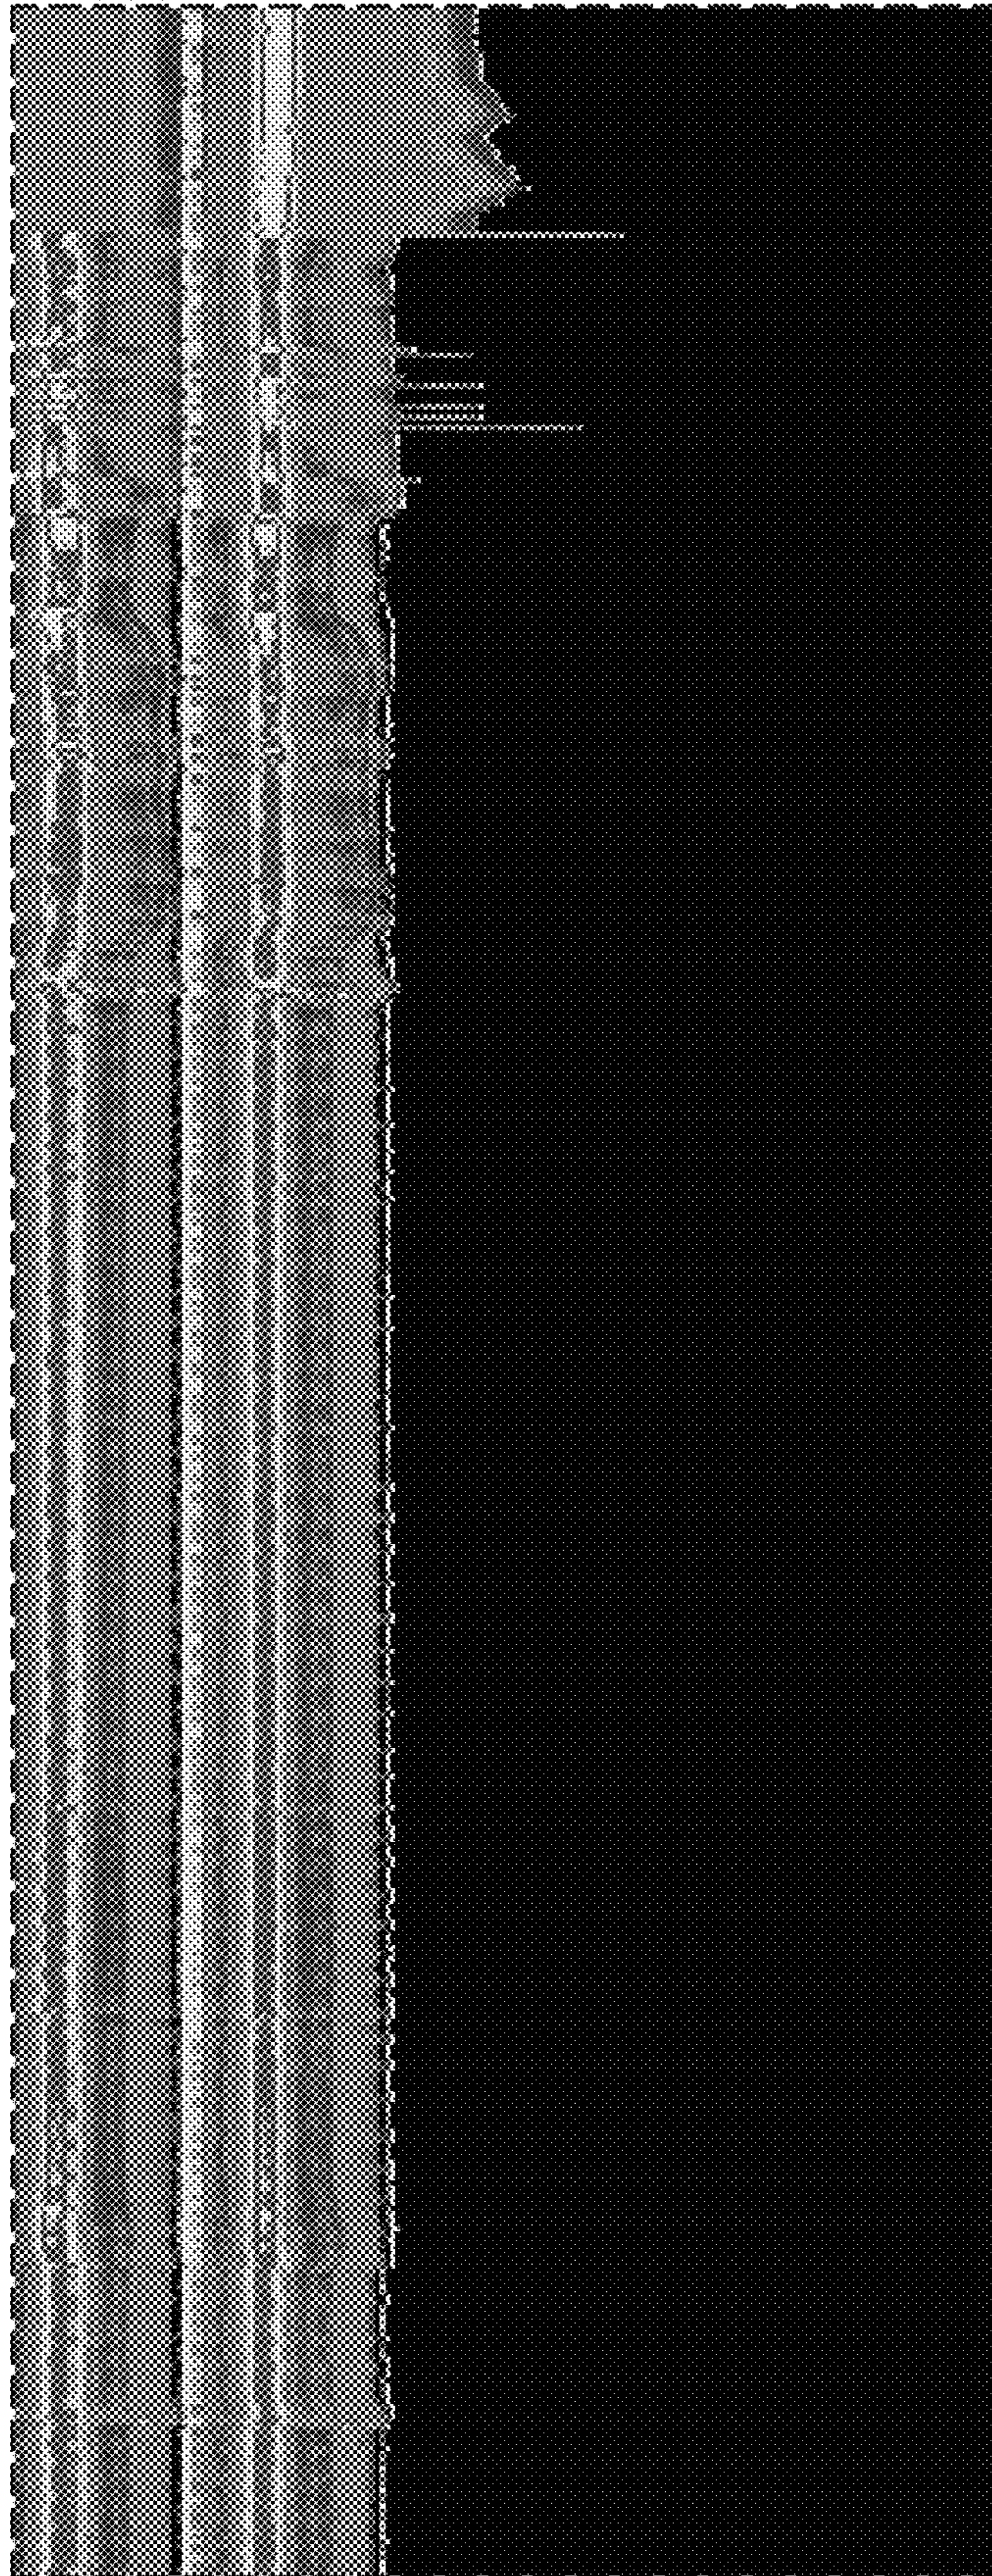


FIG. 2



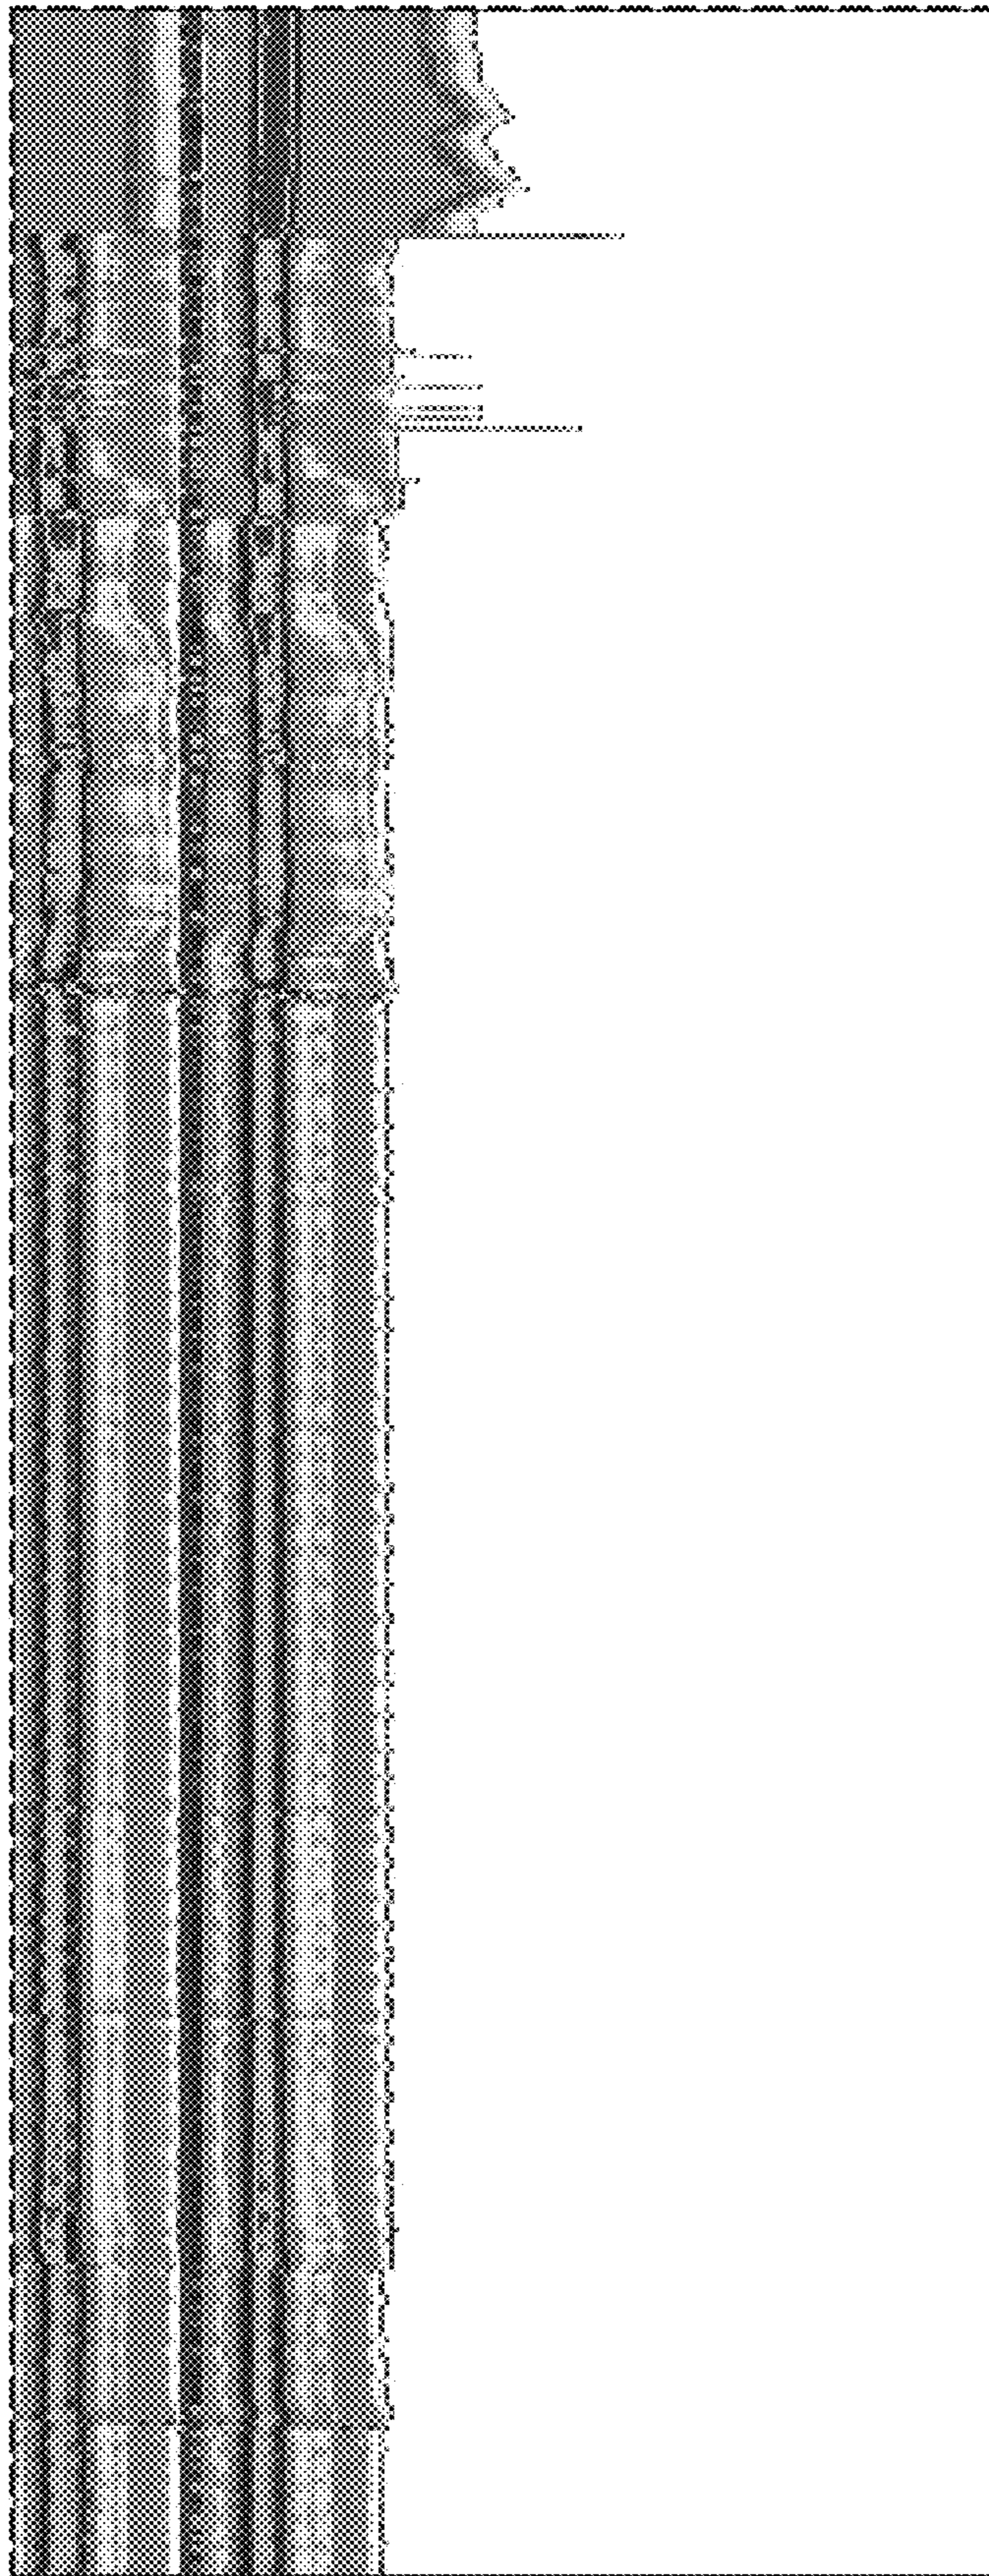


FIG. 3



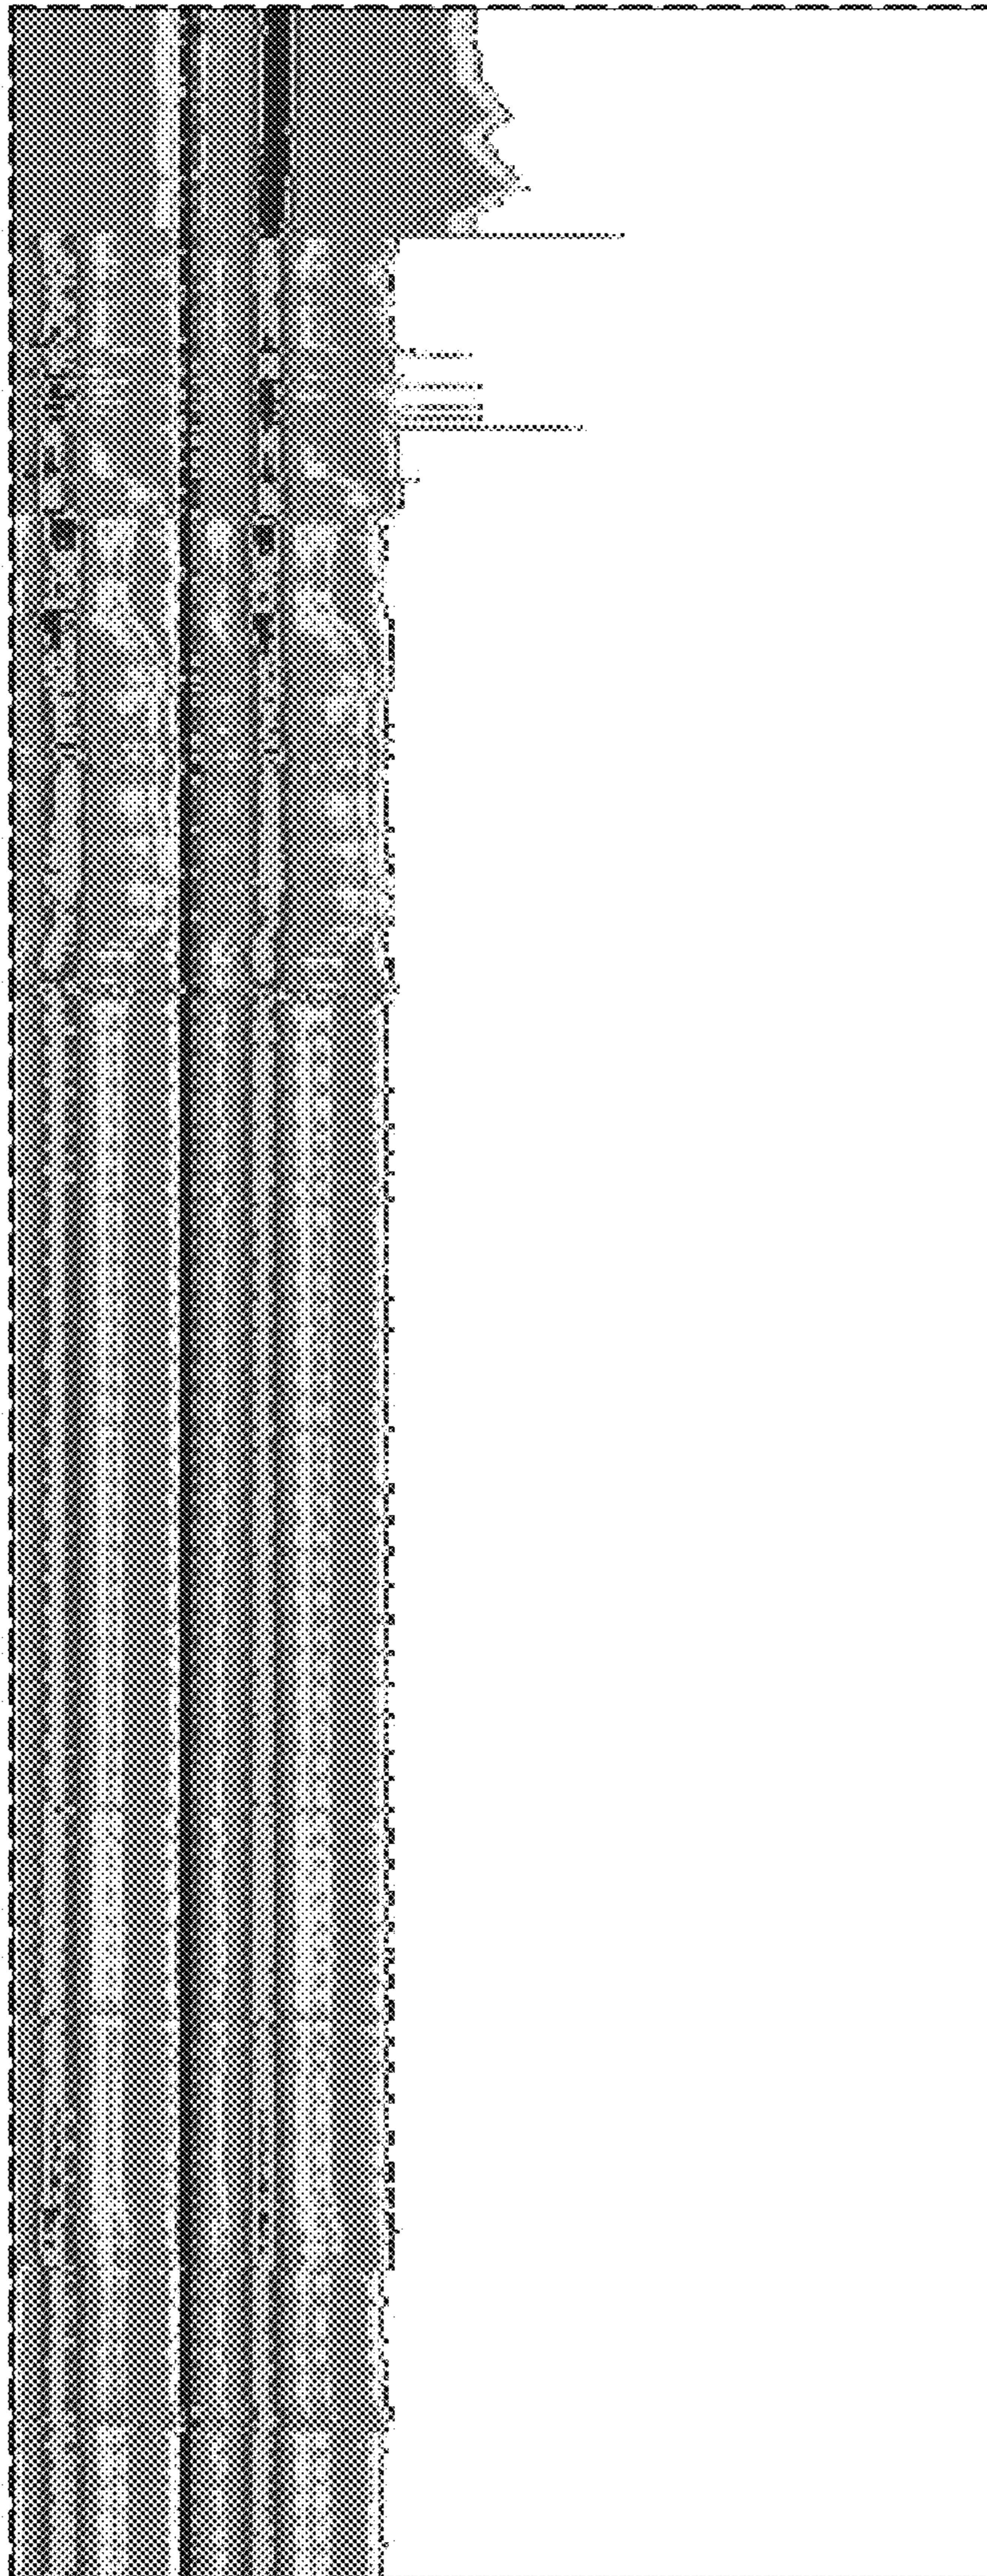


FIG. 4