

US00D837375S

(12) **United States Design Patent** (10) **Patent No.:** **US D837,375 S**
Park et al. (45) **Date of Patent:** **** Jan. 1, 2019**

(54) **BIOPSY DEVICE HANDLE**

(71) Applicant: **Argon Medical Devices, Inc.**, Plano, TX (US)

(72) Inventors: **Jae Park**, Seattle, WA (US); **Matthew Mobley**, Athens, TX (US); **Sophie Marcoux**, Gainesville, FL (US); **Stephen Choi**, Seattle, WA (US); **Scott P Jarnagin**, Seattle, WA (US)

(73) Assignee: **Argon Medical Devices, Inc.**, Plano, TX (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/586,577**

(22) Filed: **Dec. 5, 2016**

(51) **LOC (11) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/146**

(58) **Field of Classification Search**

USPC D7/649; D24/130, 133, 146, 147, 150, D24/151

CPC A61B 2010/0208; A61B 10/0275; A61B 10/0266; A61B 10/0233; A61B 2017/00367; A61B 10/025; A61B 10/04; A61B 17/34; A61F 2002/011; A61M 2005/1585

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,842,999 A 12/1998 Pruitt et al.
5,993,399 A 11/1999 Pruitt et al.
8,192,369 B2 6/2012 Bacon et al.

8,197,419 B2 6/2012 Field et al.
8,506,504 B2 8/2013 Field et al.
8,734,363 B2 5/2014 Bacon
9,072,508 B2 7/2015 Calledé et al.
D736,923 S 8/2015 Snow
D737,440 S 8/2015 Shabaz
9,113,856 B2 8/2015 Calledé et al.
9,392,998 B2 7/2016 Snow
2014/0207021 A1 7/2014 Snow
2015/0201917 A1 7/2015 Snow
2015/0238171 A1 8/2015 Shabaz

FOREIGN PATENT DOCUMENTS

WO 2014081812 5/2014
WO 2014113665 7/2014

Primary Examiner — Cathron C Brooks

Assistant Examiner — Samantha Q. Lawrence

(74) *Attorney, Agent, or Firm* — IpHorgan Ltd.

(57) **CLAIM**

The ornamental design for a biopsy device handle, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a biopsy device handle, showing the new design;

FIG. 2 is a top view thereof;

FIG. 3 is a bottom view thereof;

FIG. 4 is a left side view thereof;


FIG. 5 is a right side view thereof;

FIG. 6 is a front view thereof; and,

FIG. 7 is a rear view thereof.

The broken lines shown in FIGS. 1-7 illustrate portions of the biopsy device handle that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

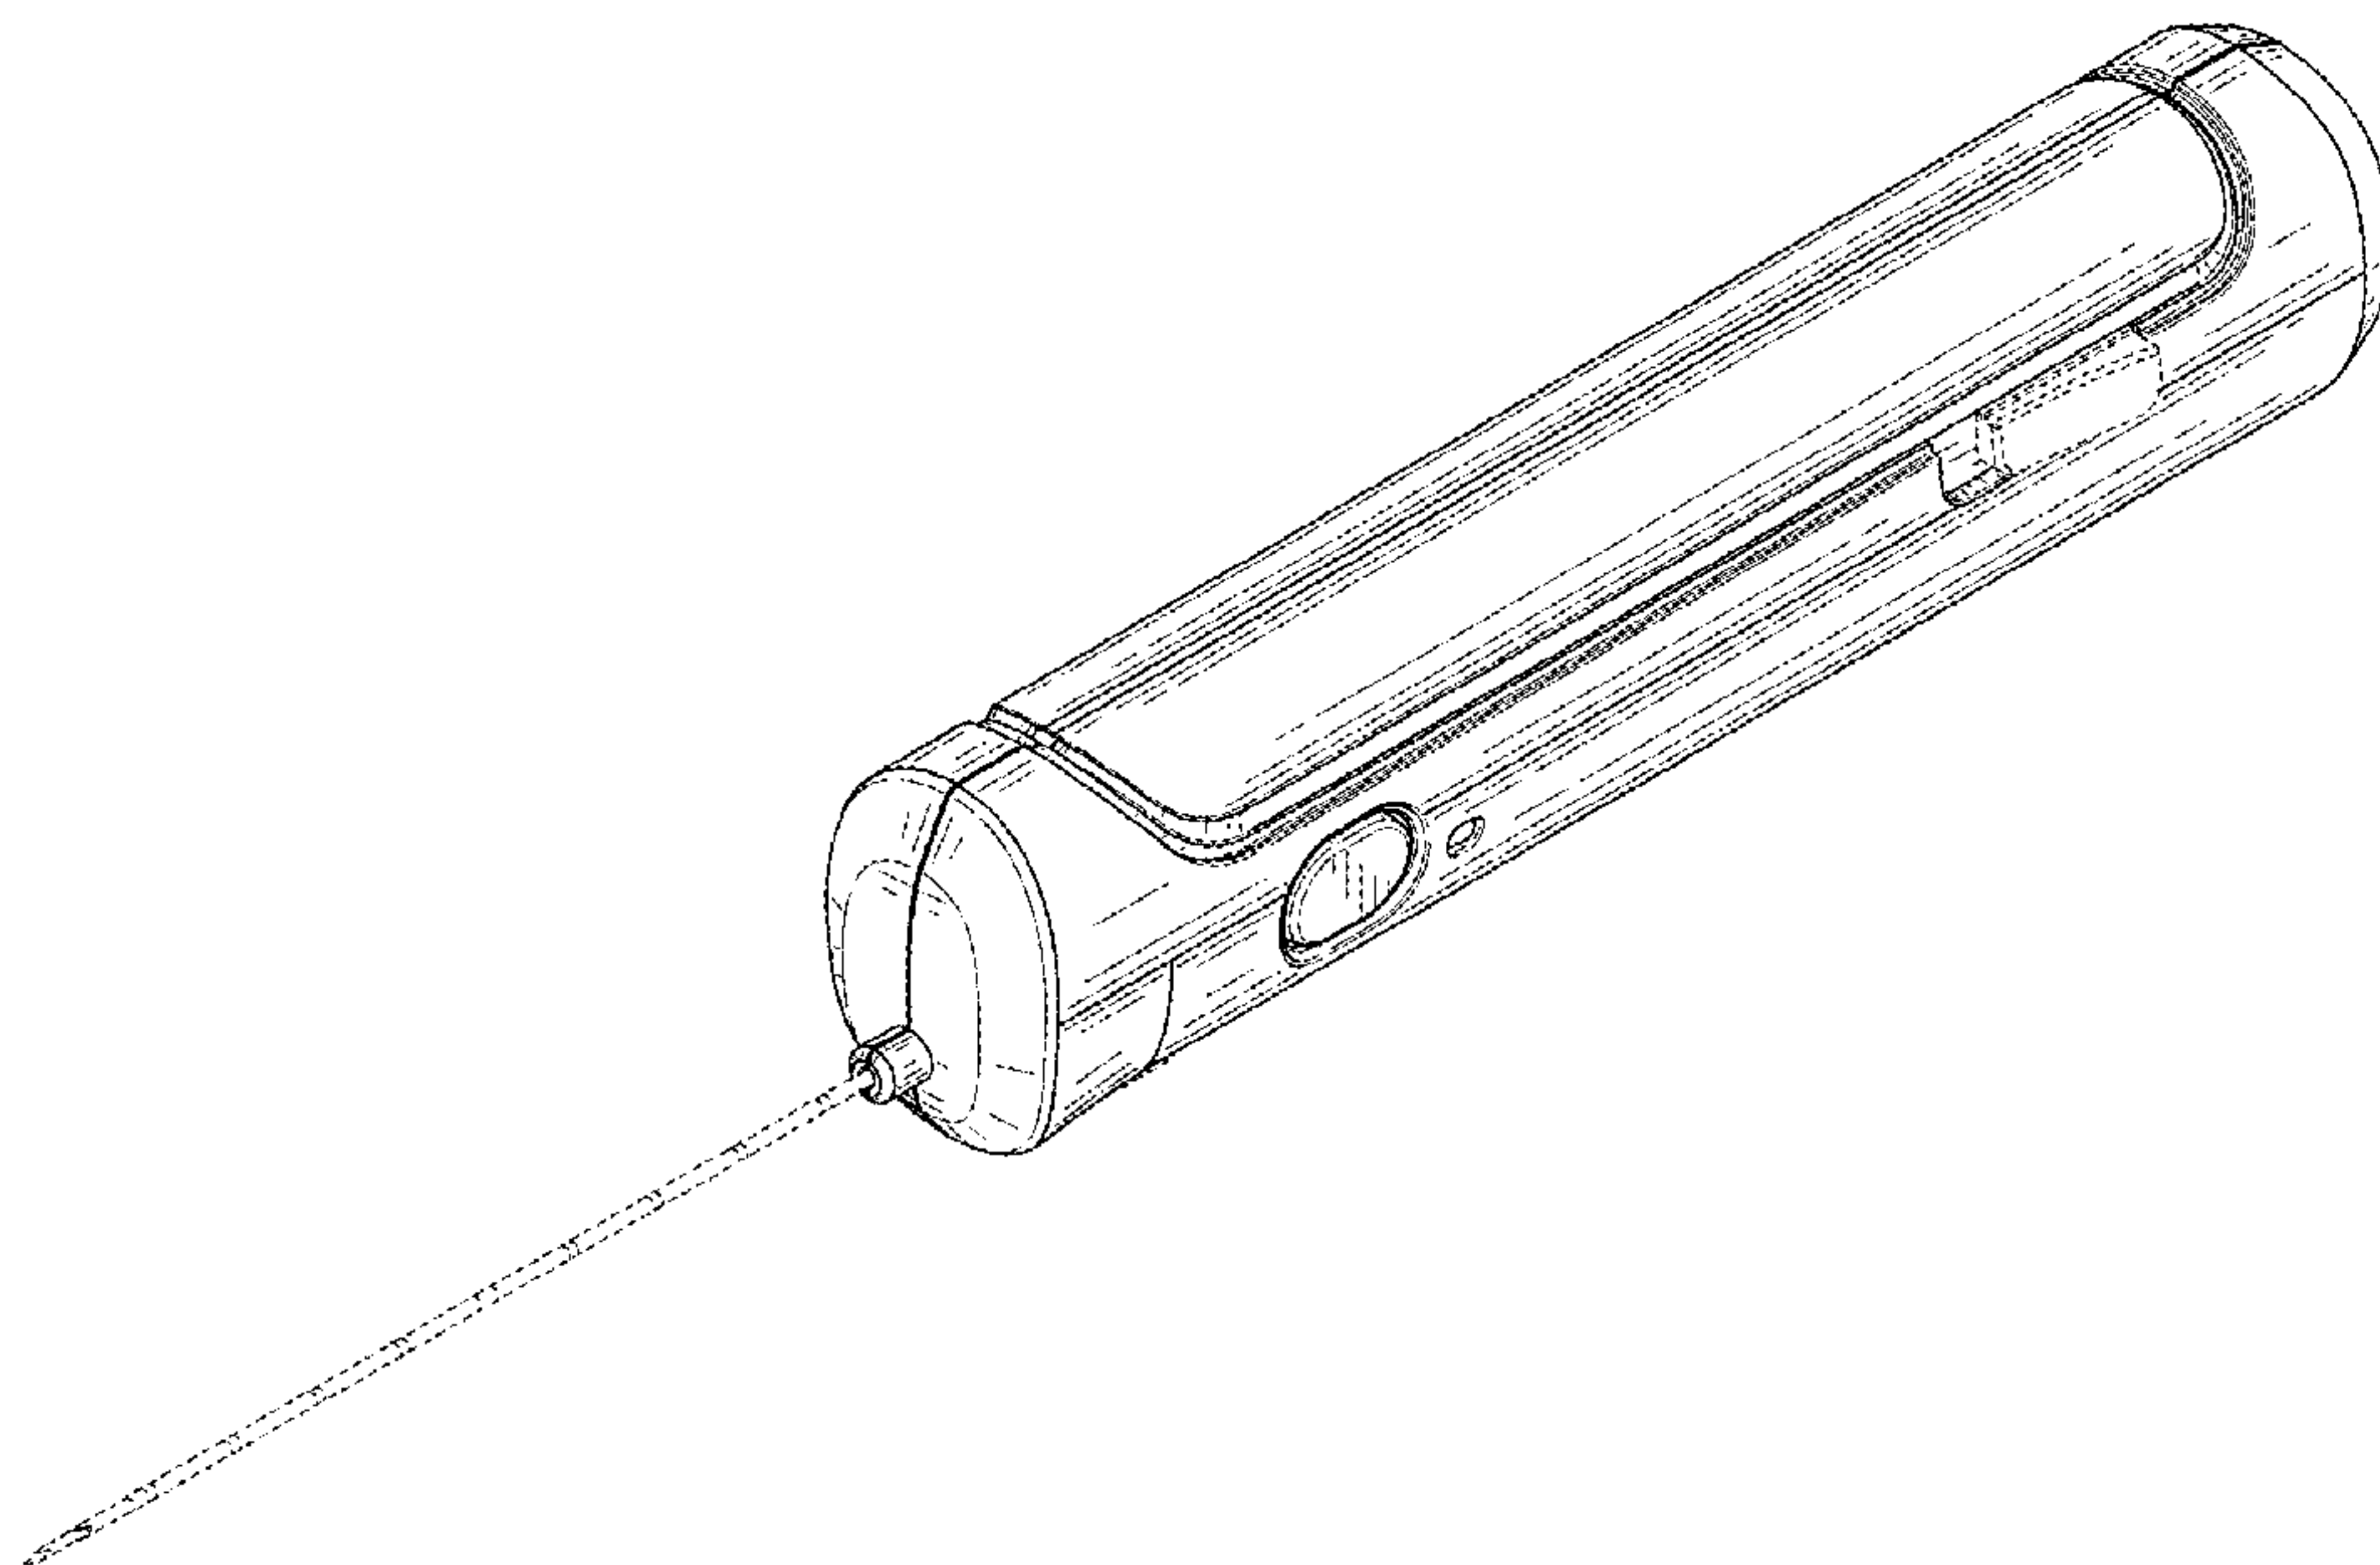

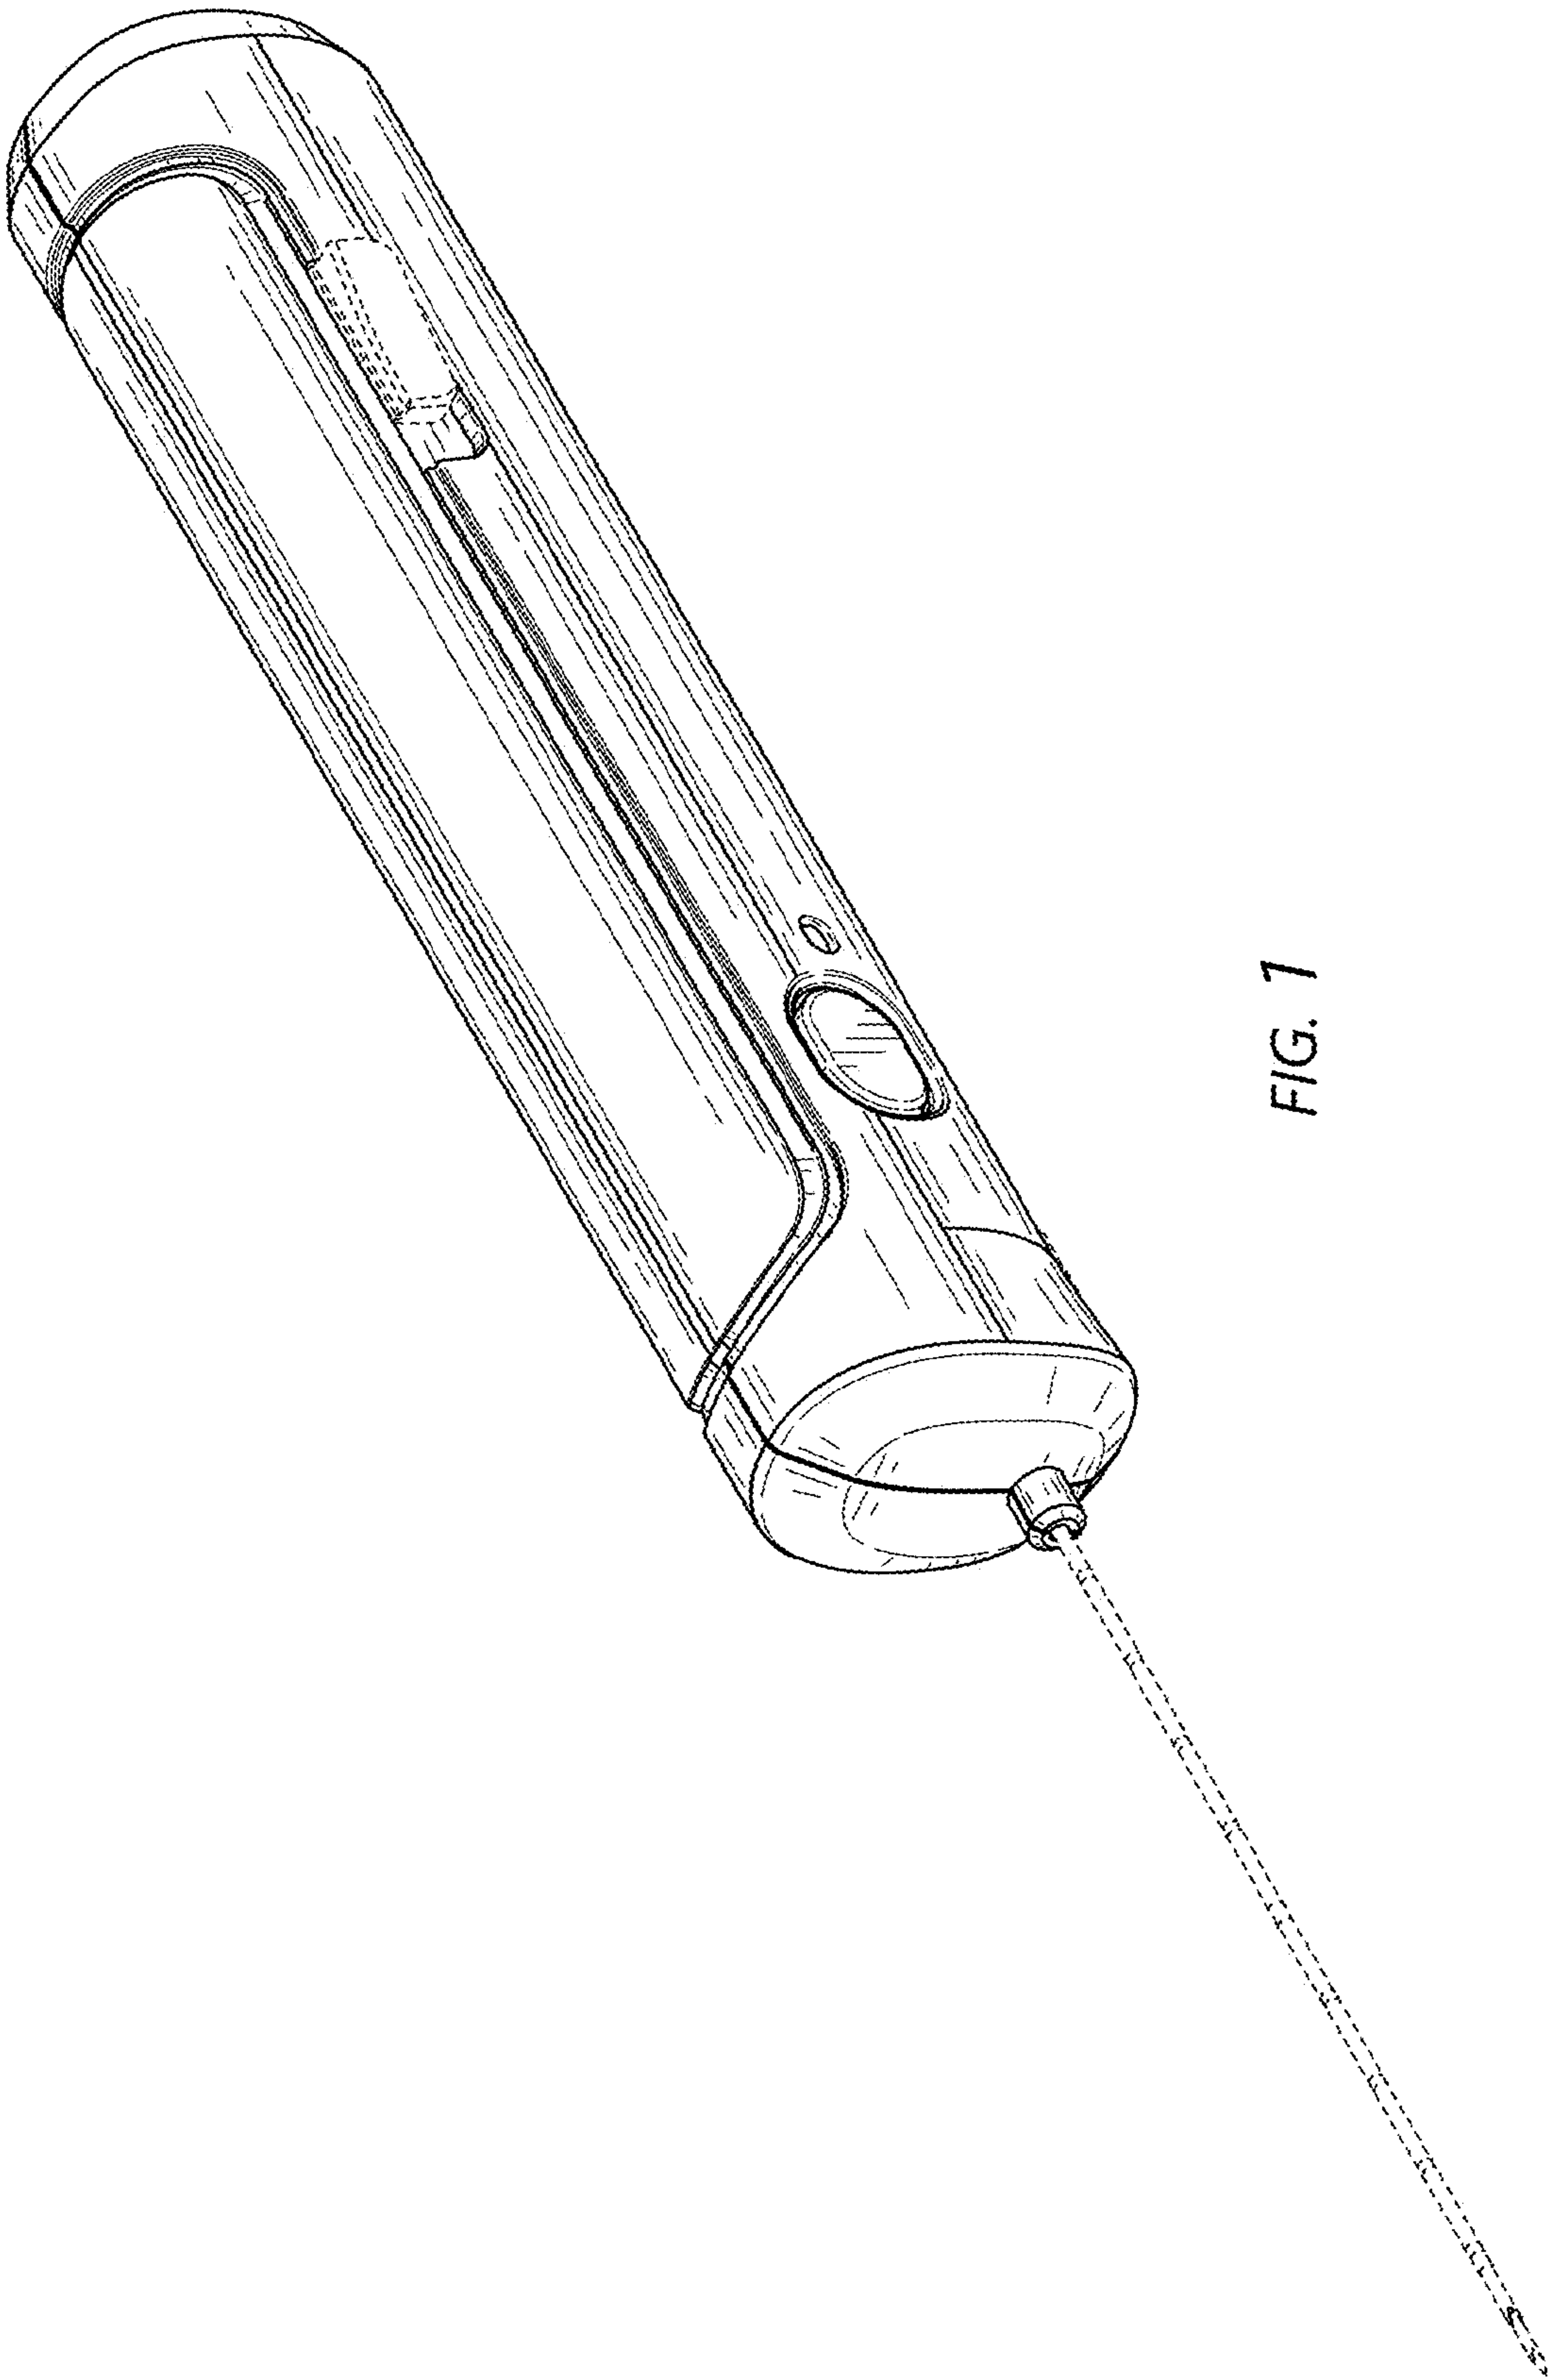


FIG. 1

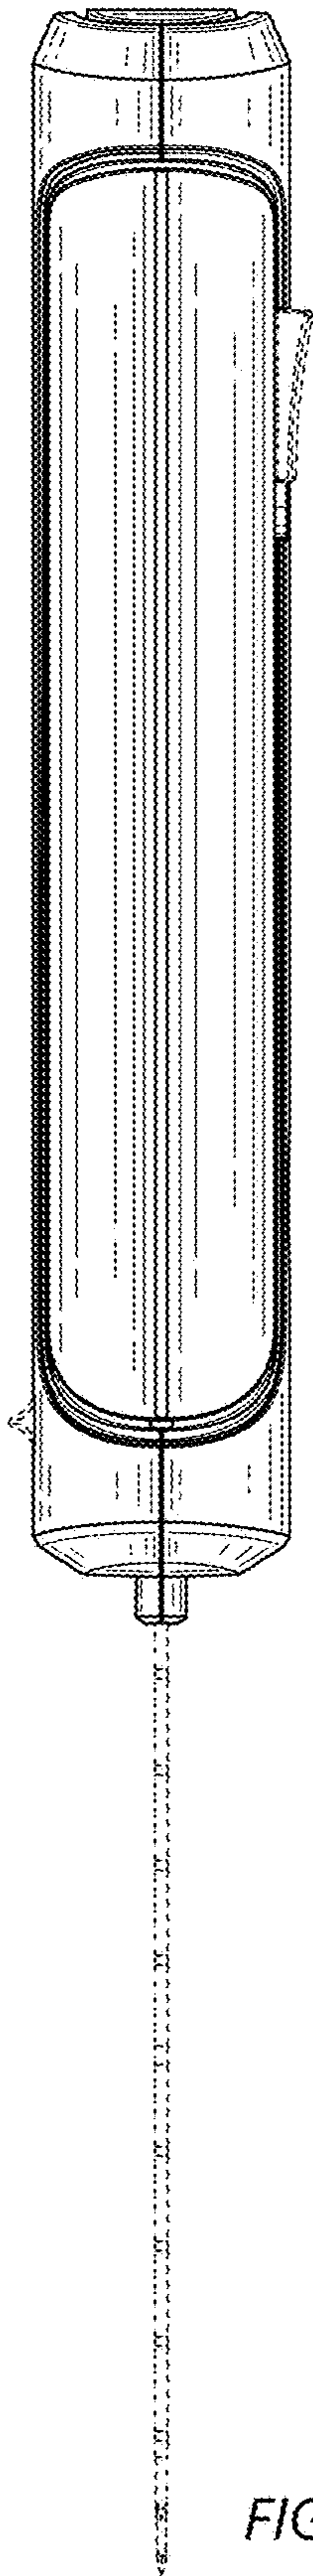


FIG. 2

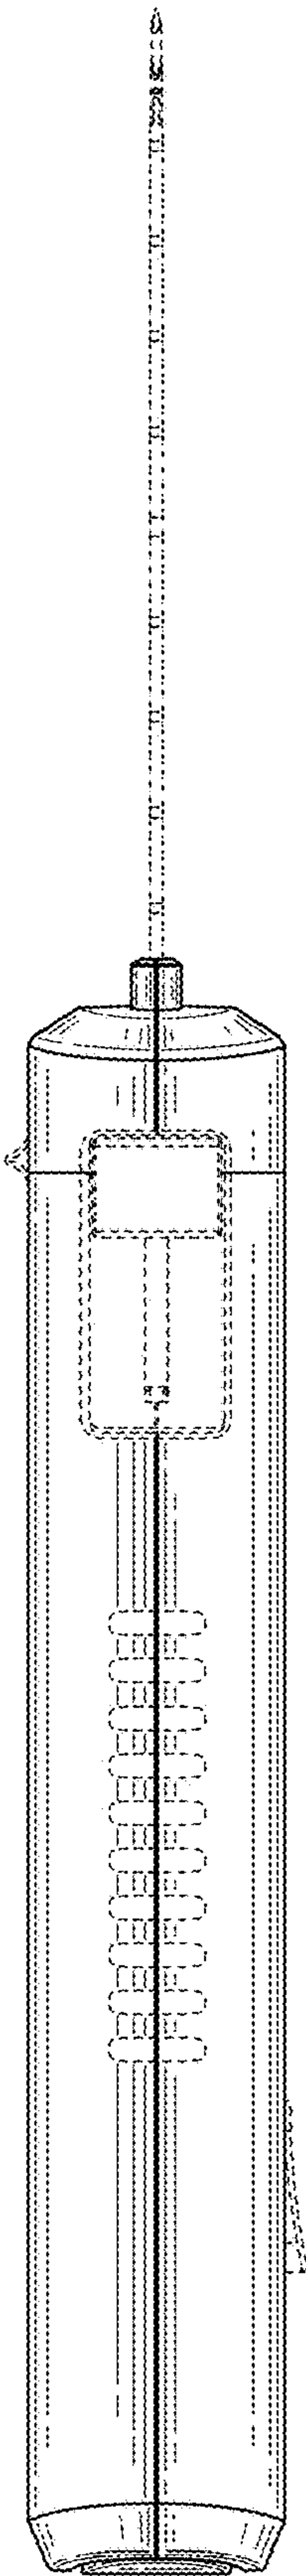


FIG. 3

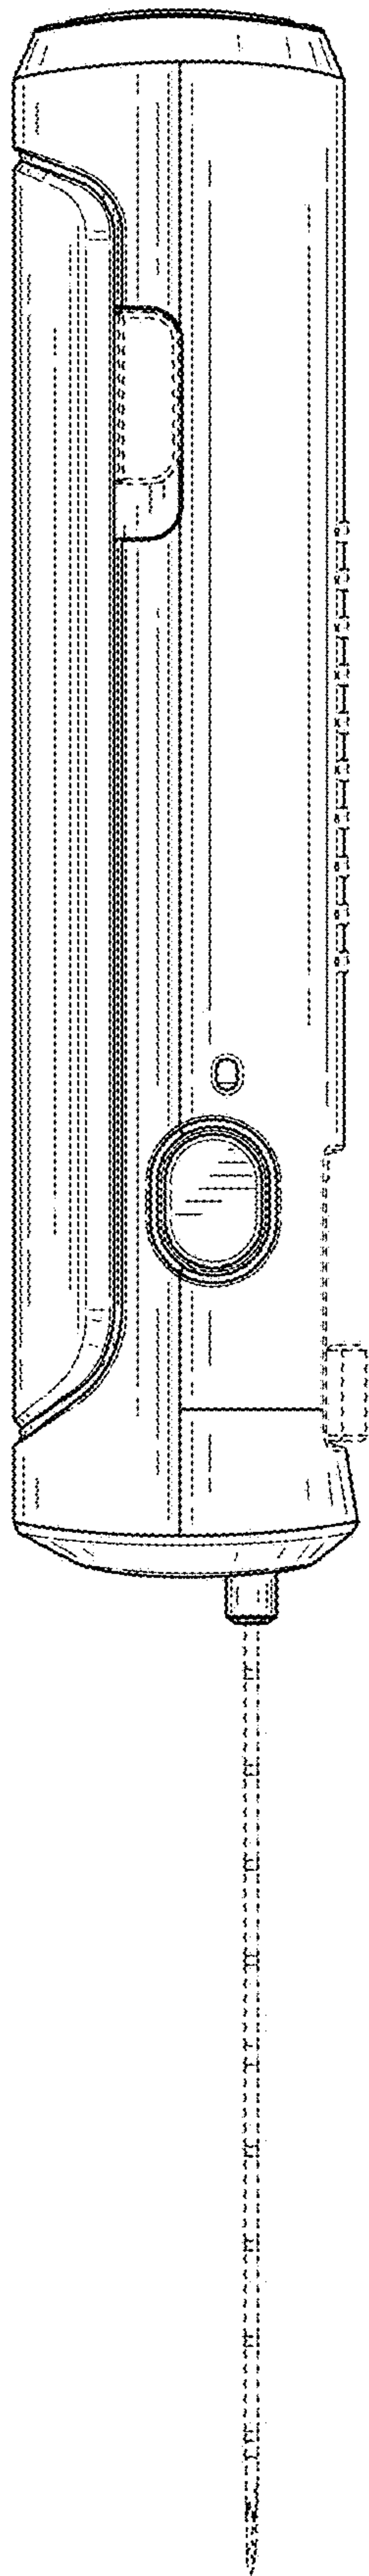


FIG. 4

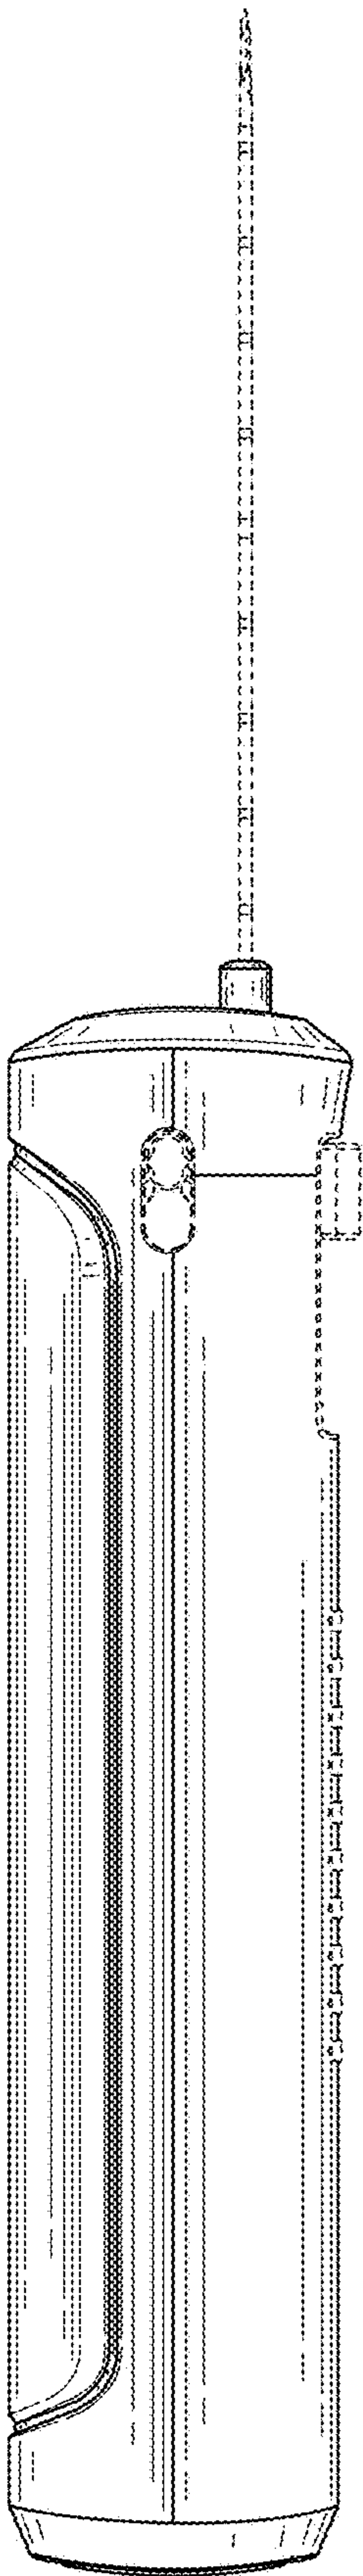


FIG. 5

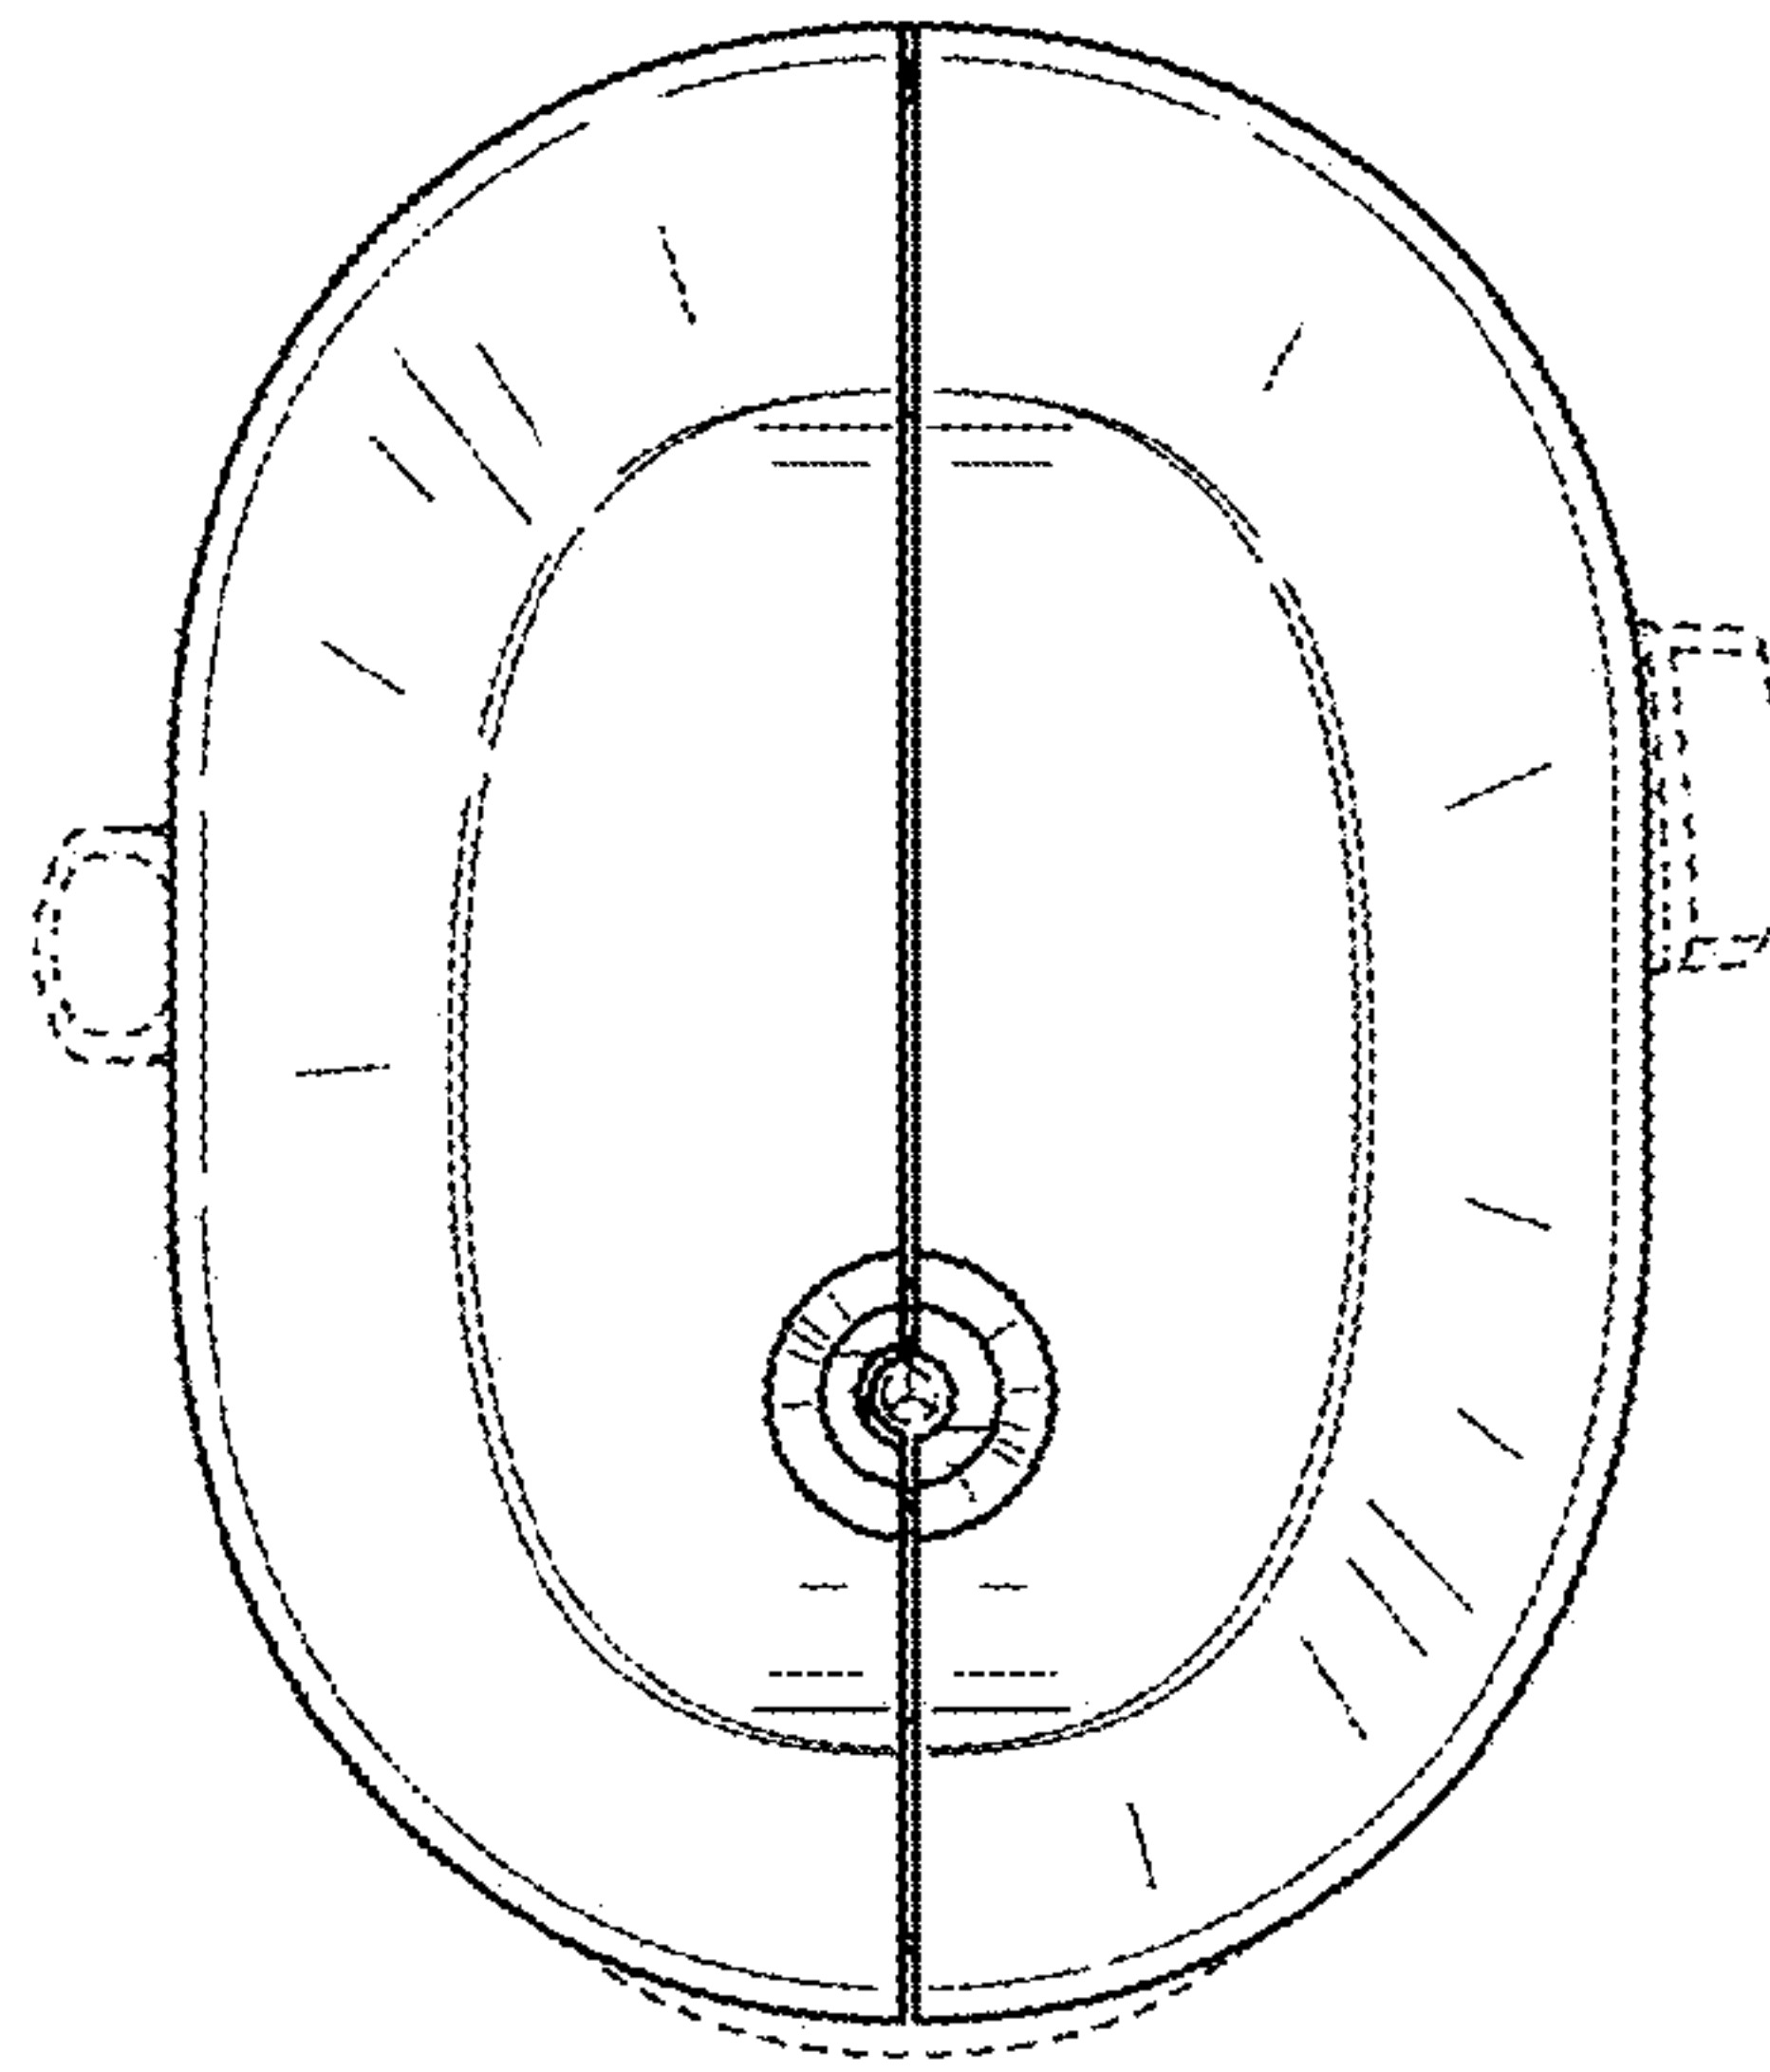


FIG. 6

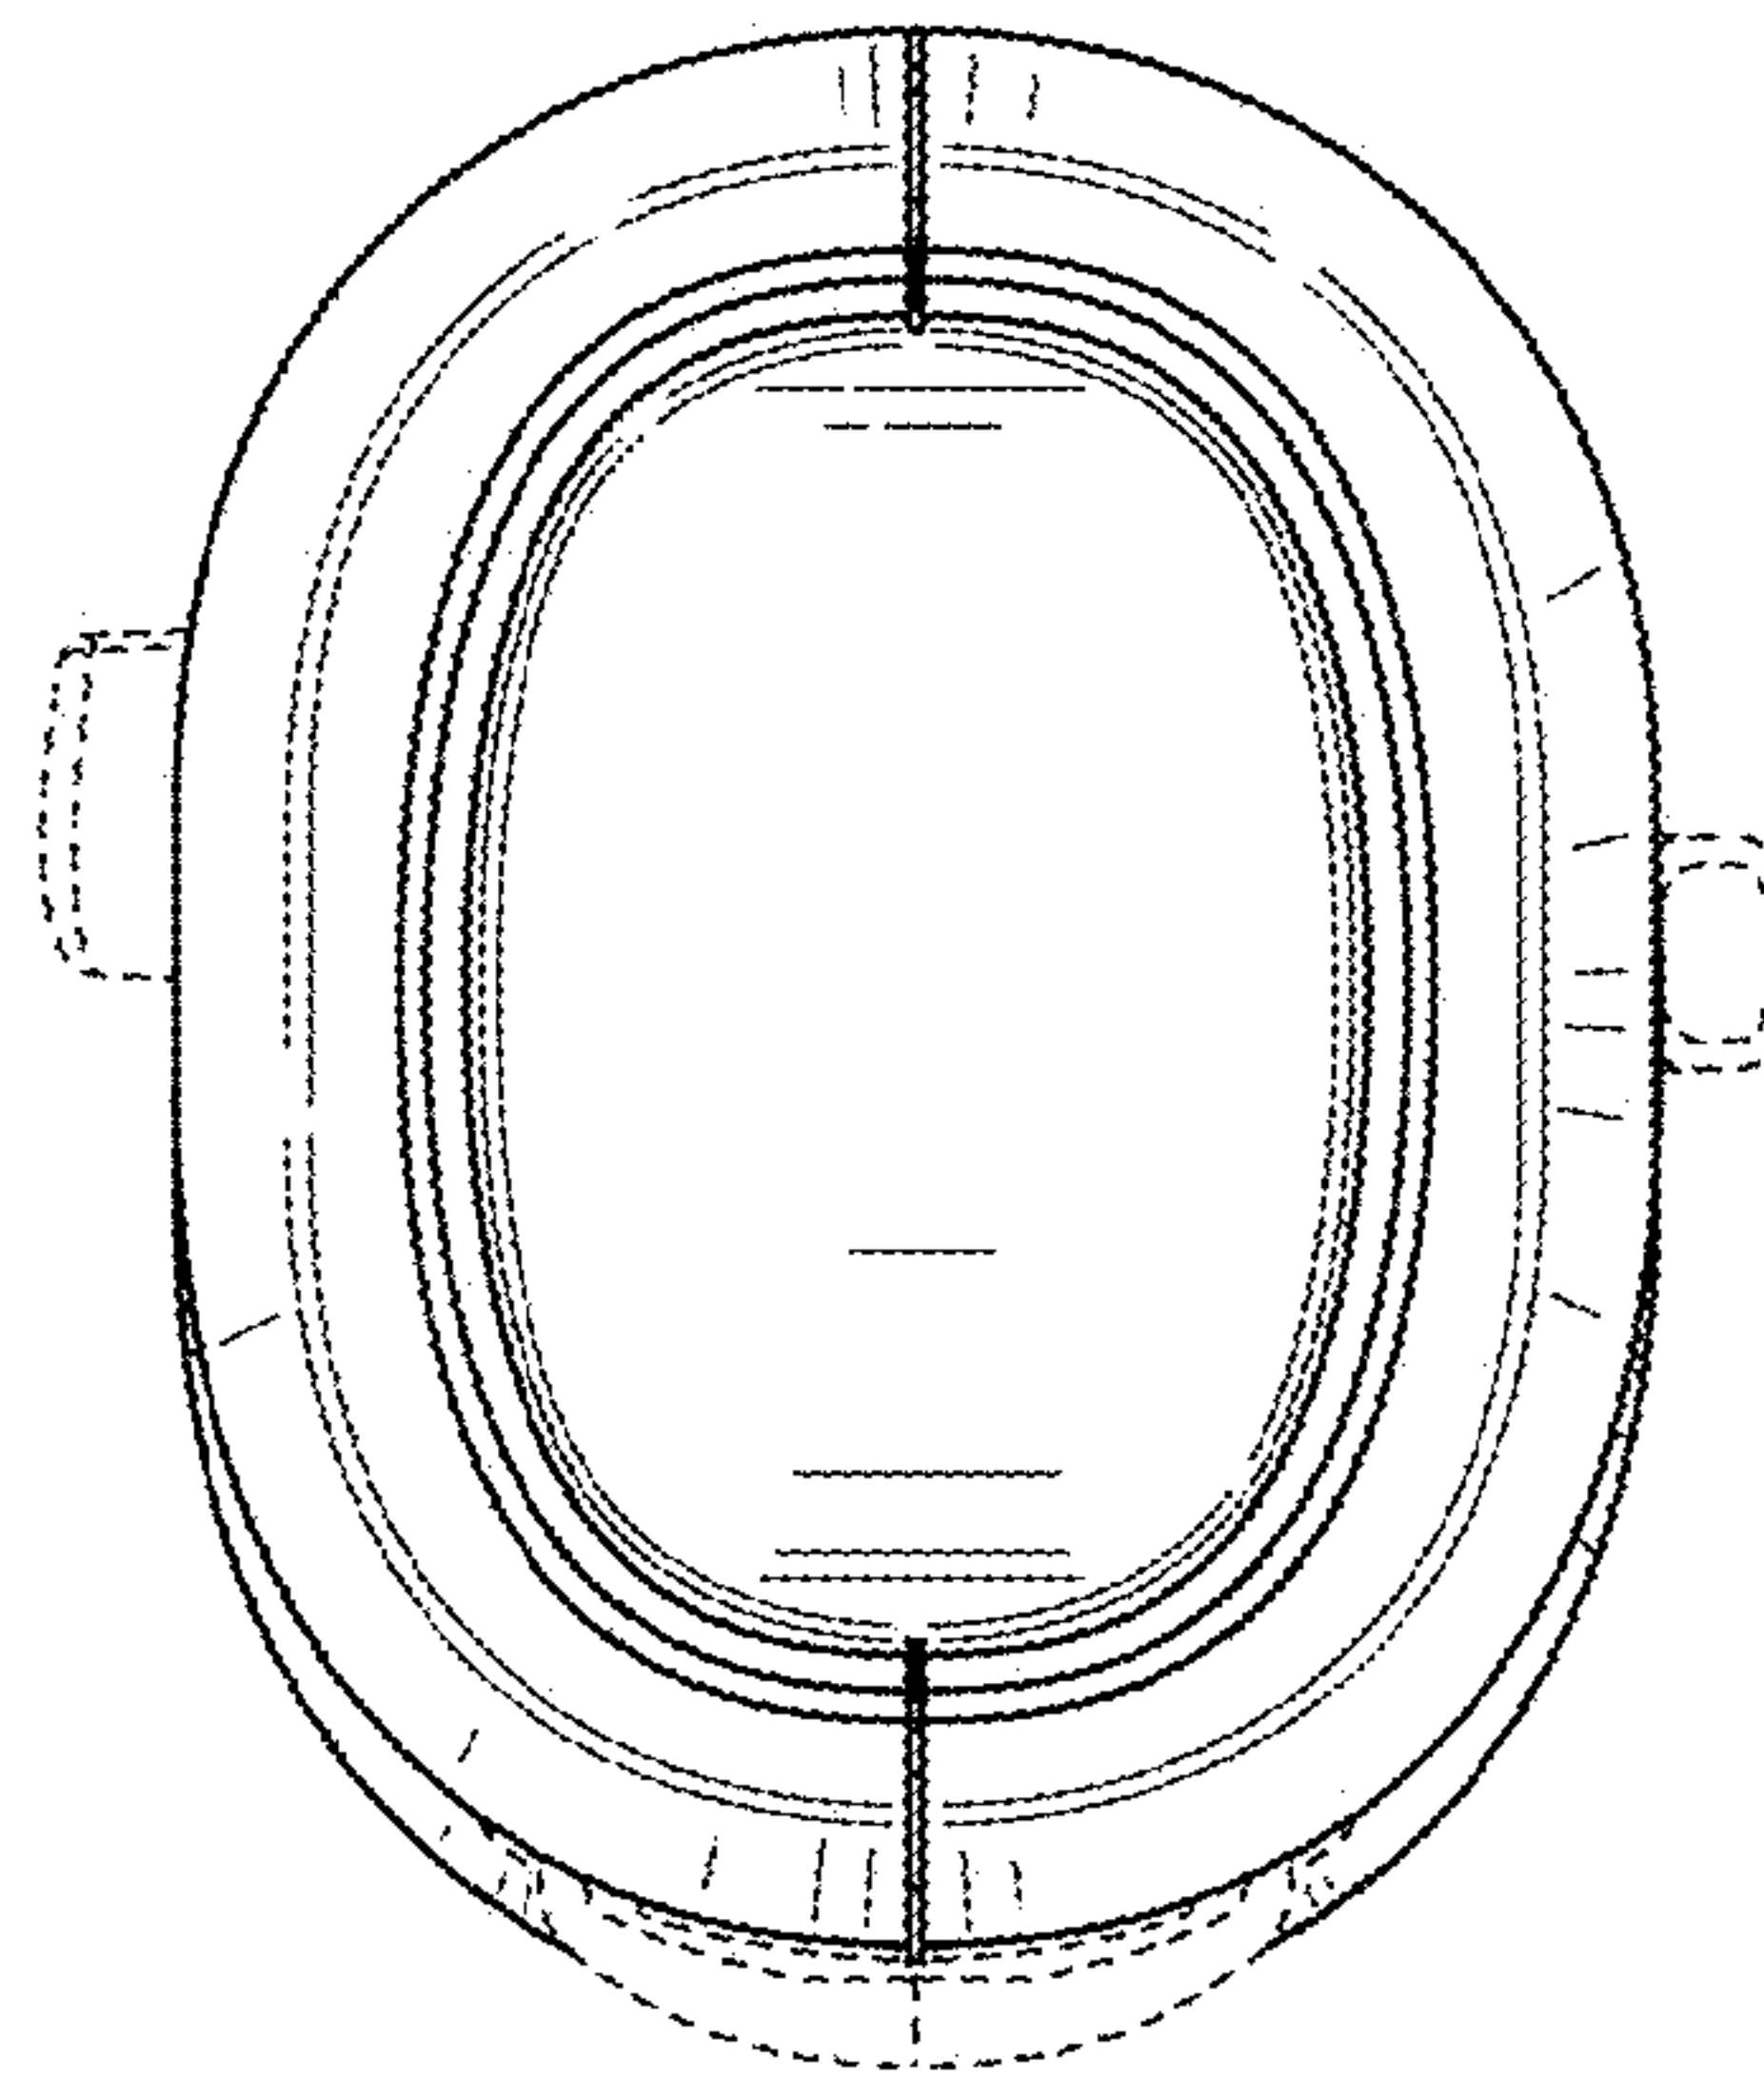


FIG. 7