

US00D840537S

(12) United States Design Patent (10) Patent No.:

Wong et al.

(45) Patent Pro.: (45) Date of Patent:

US D840,537 S

nt: ** Feb. 12, 2019

(54) TWO-POINT DISCRIMINATOR

- (71) Applicants: Julielynn Yee-Ching Wong, Toronto (CA); Jody Mou, North York (CA)
- (72) Inventors: Julielynn Yee-Ching Wong, Toronto (CA); Jody Mou, North York (CA)
- (73) Assignee: **3D4MD Inc.**, Toronto, Ontario (CA)
- (**) Term: 15 Years
- (21) Appl. No.: 29/559,426
- (22) Filed: Mar. 28, 2016
- (52) U.S. Cl.

(56) References Cited

U.S. PATENT DOCUMENTS

4,823,806 A	*	4/1989	Bajada	A61B 5/441
				600/556
5,222,504 A	*	6/1993	Solomon	A61B 5/4824
				600/557

FOREIGN PATENT DOCUMENTS

(Continued)

CA 1282660 C 4/1991 A61B 5/00

OTHER PUBLICATIONS

AxoGen, Inc., AxoTouchTM, Two-Point Discriminator, http://www.axogeninc.com/products/4154/index.html, 1 page, Jan. 2017.

(Continued)

Primary Examiner — Wan Laymon (74) Attorney, Agent, or Firm — Sunstein Kann Murphy & Timbers LLP


(57) CLAIM


The ornamental design for a two-point discriminator, as shown and described.

DESCRIPTION

- FIG. 1 shows a top perspective view of a first embodiment of a two-point discriminator in accordance with the present invention;
- FIG. 2 shows a top view of the first embodiment;
- FIG. 3 shows a bottom view of the first embodiment;
- FIG. 4 shows a right side view of the first embodiment;
- FIG. 5 shows a left side view of the first embodiment;
- FIG. 6 shows a front view of the first embodiment;
- FIG. 7 shows a rear view of the first embodiment;
- FIG. 8 shows a top perspective view of a second embodiment of a two-point discriminator in accordance with the present invention;
- FIG. 9 shows a top view of the second embodiment;
- FIG. 10 shows a bottom view of the second embodiment;
- FIG. 11 shows a right side view of the second embodiment;
- FIG. 12 shows a left side view of the second embodiment;
- FIG. 13 shows a front view of the second embodiment;
- FIG. 14 shows a rear view of the second embodiment;
- FIG. 15 shows a top perspective view of a third embodiment of a two-point discriminator in accordance with the present invention;
- FIG. 16 shows a top view of the third embodiment;
- FIG. 17 shows a bottom view of the third embodiment;
- FIG. 18 shows a right side view of the third embodiment;
- FIG. 19 shows a left side view of the third embodiment;
- FIG. 20 shows a front view of the third embodiment;
- FIG. 21 shows a rear view of the third embodiment;
- FIG. 22 shows a top perspective view of a fourth embodiment of a two-point discriminator in accordance with the present invention;
- FIG. 23 shows a top view of the fourth embodiment;
- FIG. 24 shows a bottom view of the fourth embodiment;
- FIG. 25 shows a right side view of the fourth embodiment;
- FIG. 26 shows a left side view of the fourth embodiment;
- FIG. 27 shows a front view of the fourth embodiment; and, FIG. 28 shows a rear view of the fourth embodiment.
- The broken lines depict portions of the two-point discriminator that form no part of the claimed design.

(Continued)

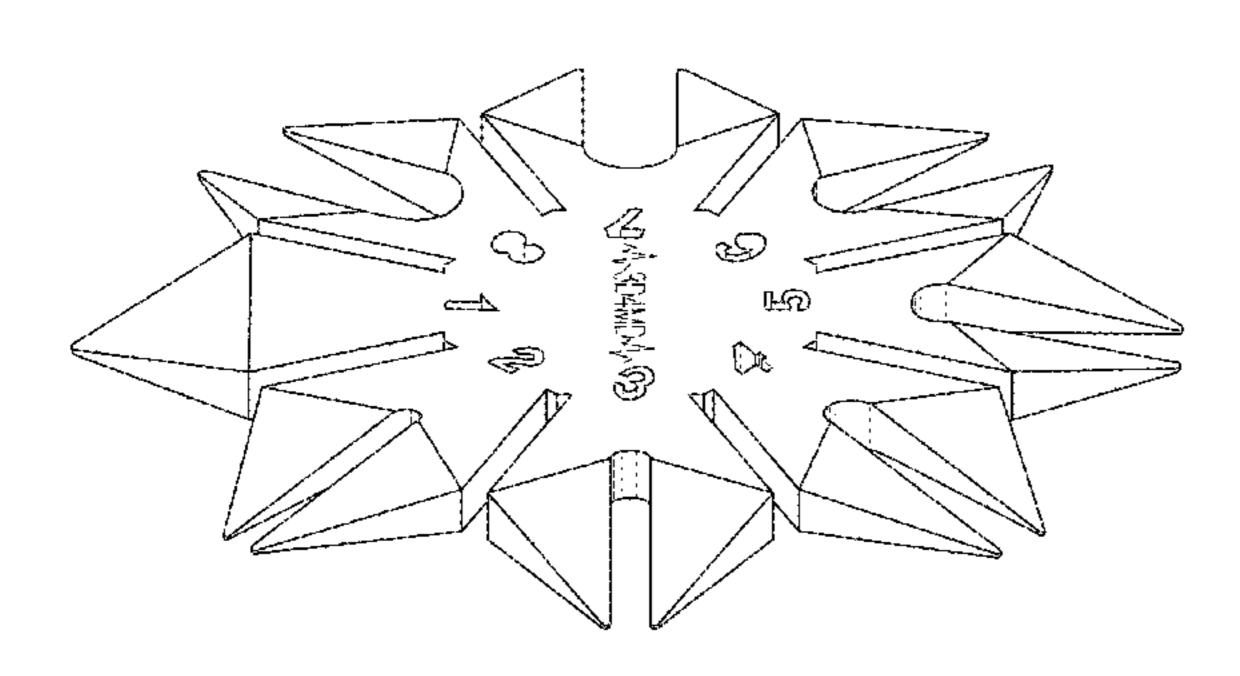

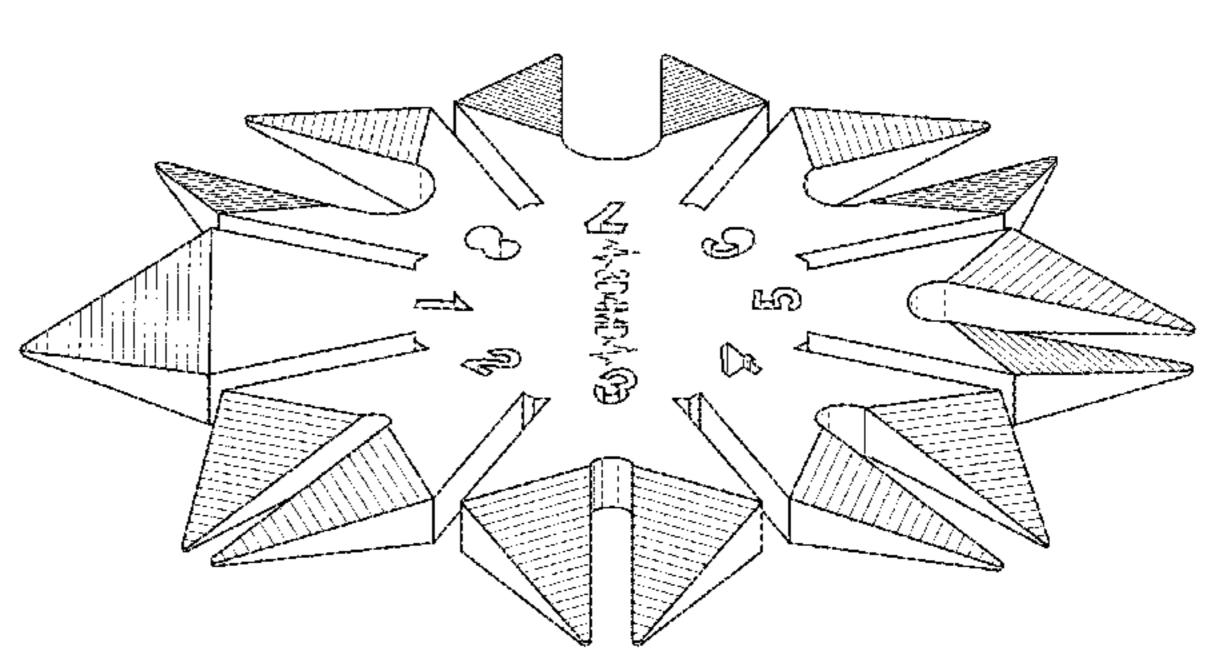

The broken line perimeters seen on the surface of the two-point discriminator are boundaries of the claimed design. These broken lines and the areas within them also form no part of the claimed design.

1 Claim, 16 Drawing Sheets

(58) Field of Classification Search

CPC A61B 5/4827; A61B 5/4824; A61B 5/483; A61B 5/44; A61B 5/441; A61B 5/0048; A61B 5/0051

See application file for complete search history.

(56) References Cited


U.S. PATENT DOCUMENTS

5,529,074	A	*	6/1996	Greenfield A61B 5/4824
				600/557
6,387,055	B1	*	5/2002	Christy A61B 5/4827
				600/557
D669,985	S	*	10/2012	Cheney D24/140
				Freudenthal D24/140
D777,917	S	*	1/2017	Kabra D24/144

OTHER PUBLICATIONS

NexGen Medical Systems, Baseline, DISCRIM-A-GONTM, http://www.nexgenergo.com/medical/baseline9.html, 1 page, Jan. 2017. North Coast Medical, Inc., Disk-CriminatorTM, https://ssl.cdn.ncmedical.com/item_1283.html, 1 page, Jan. 2017. North Coast Medical, Inc., Touch-Test®, Two-Point Discriminator, https://ssl.cdn.ncmedical.com/item_705.html,1 page, Jan. 2017.

^{*} cited by examiner

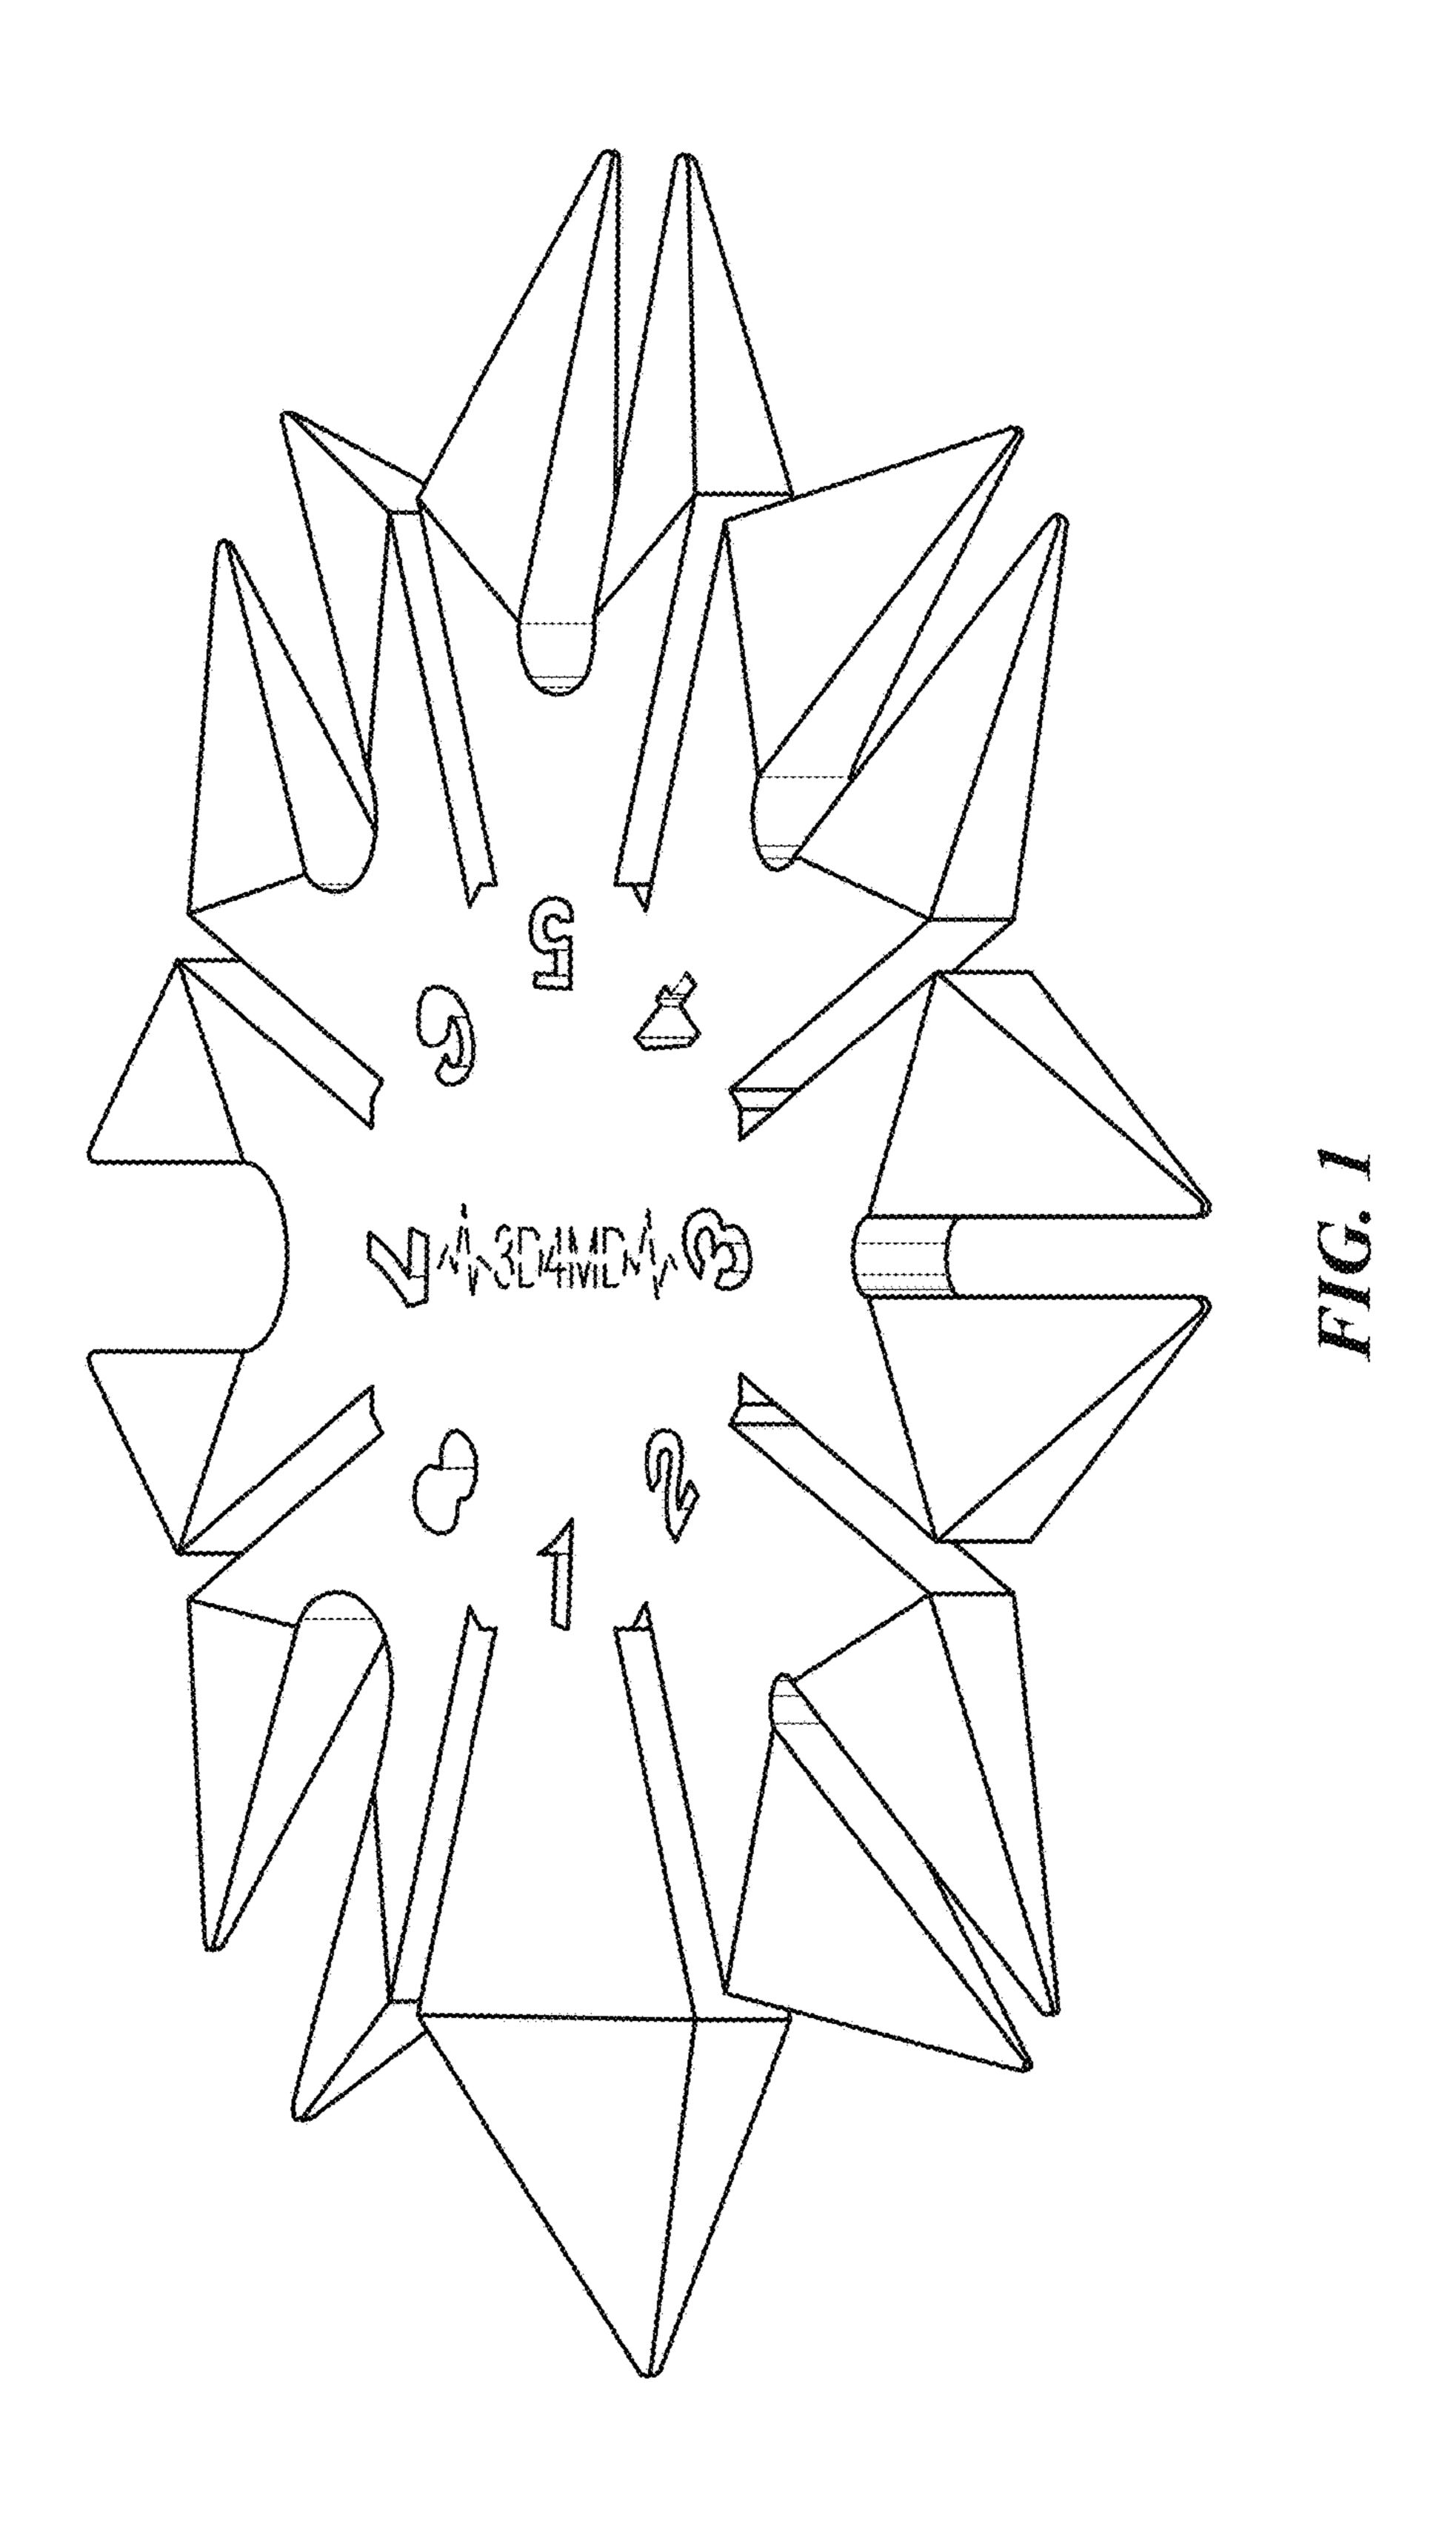

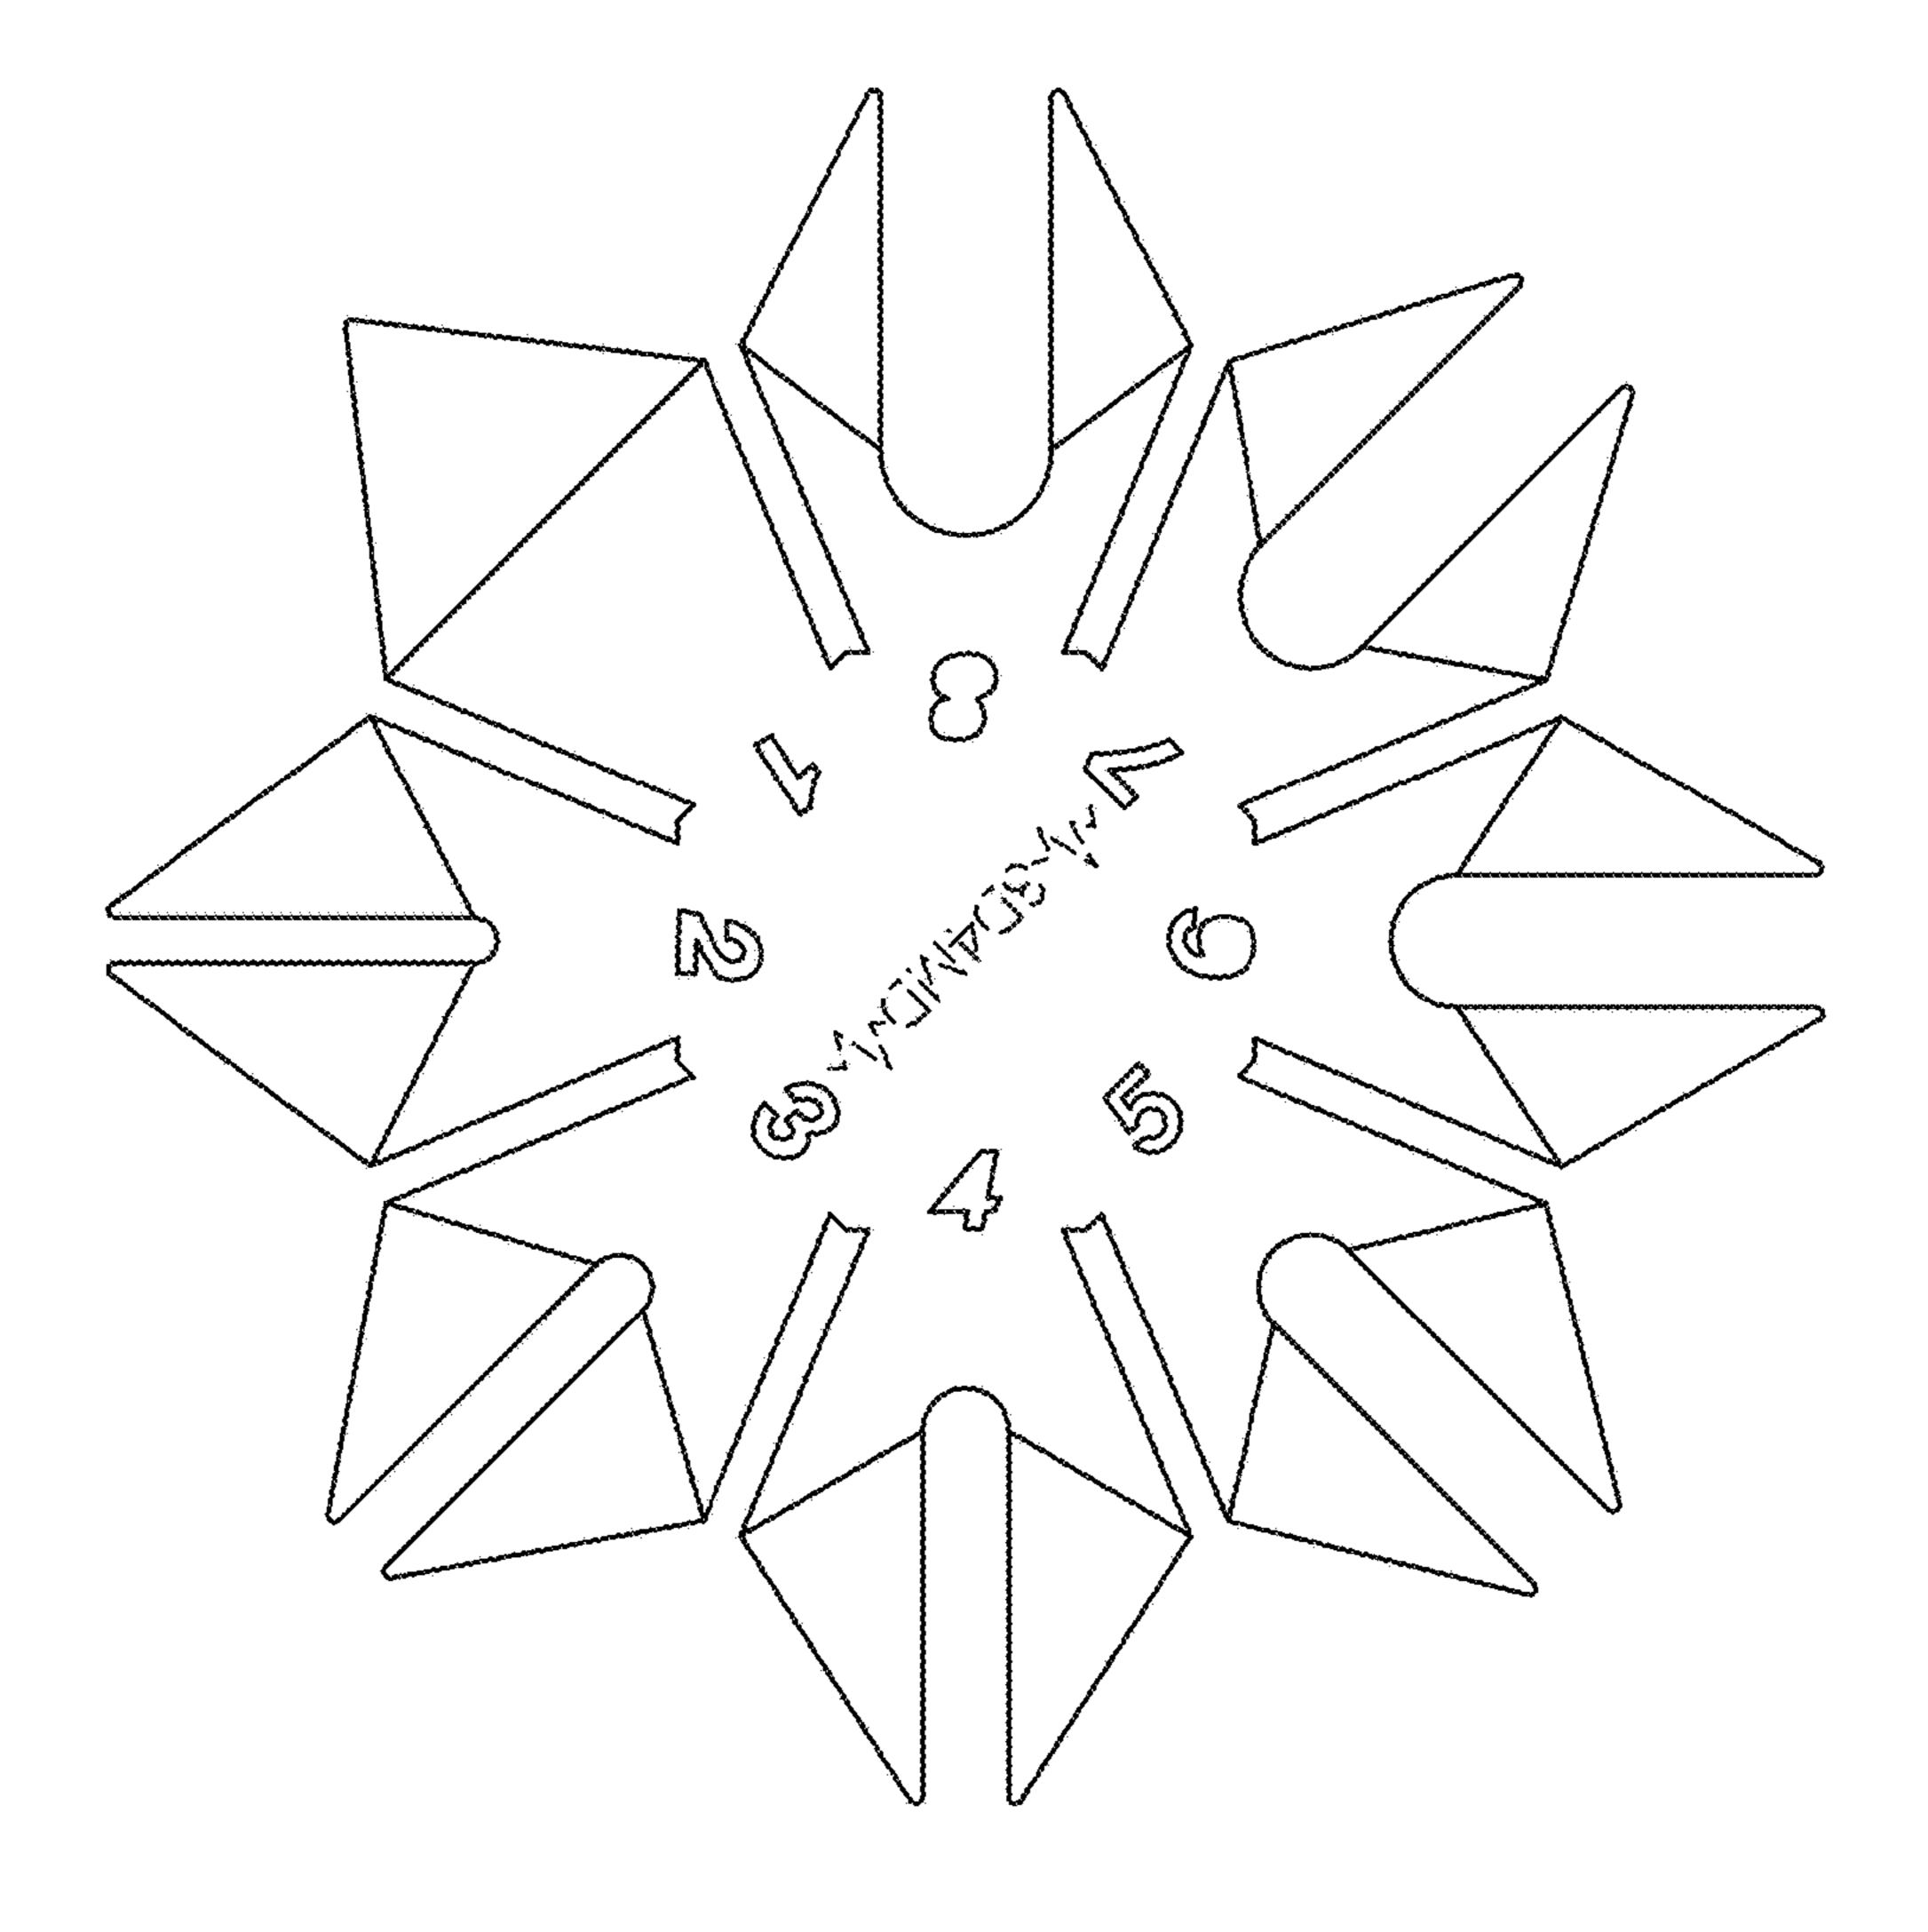


FIG. 2

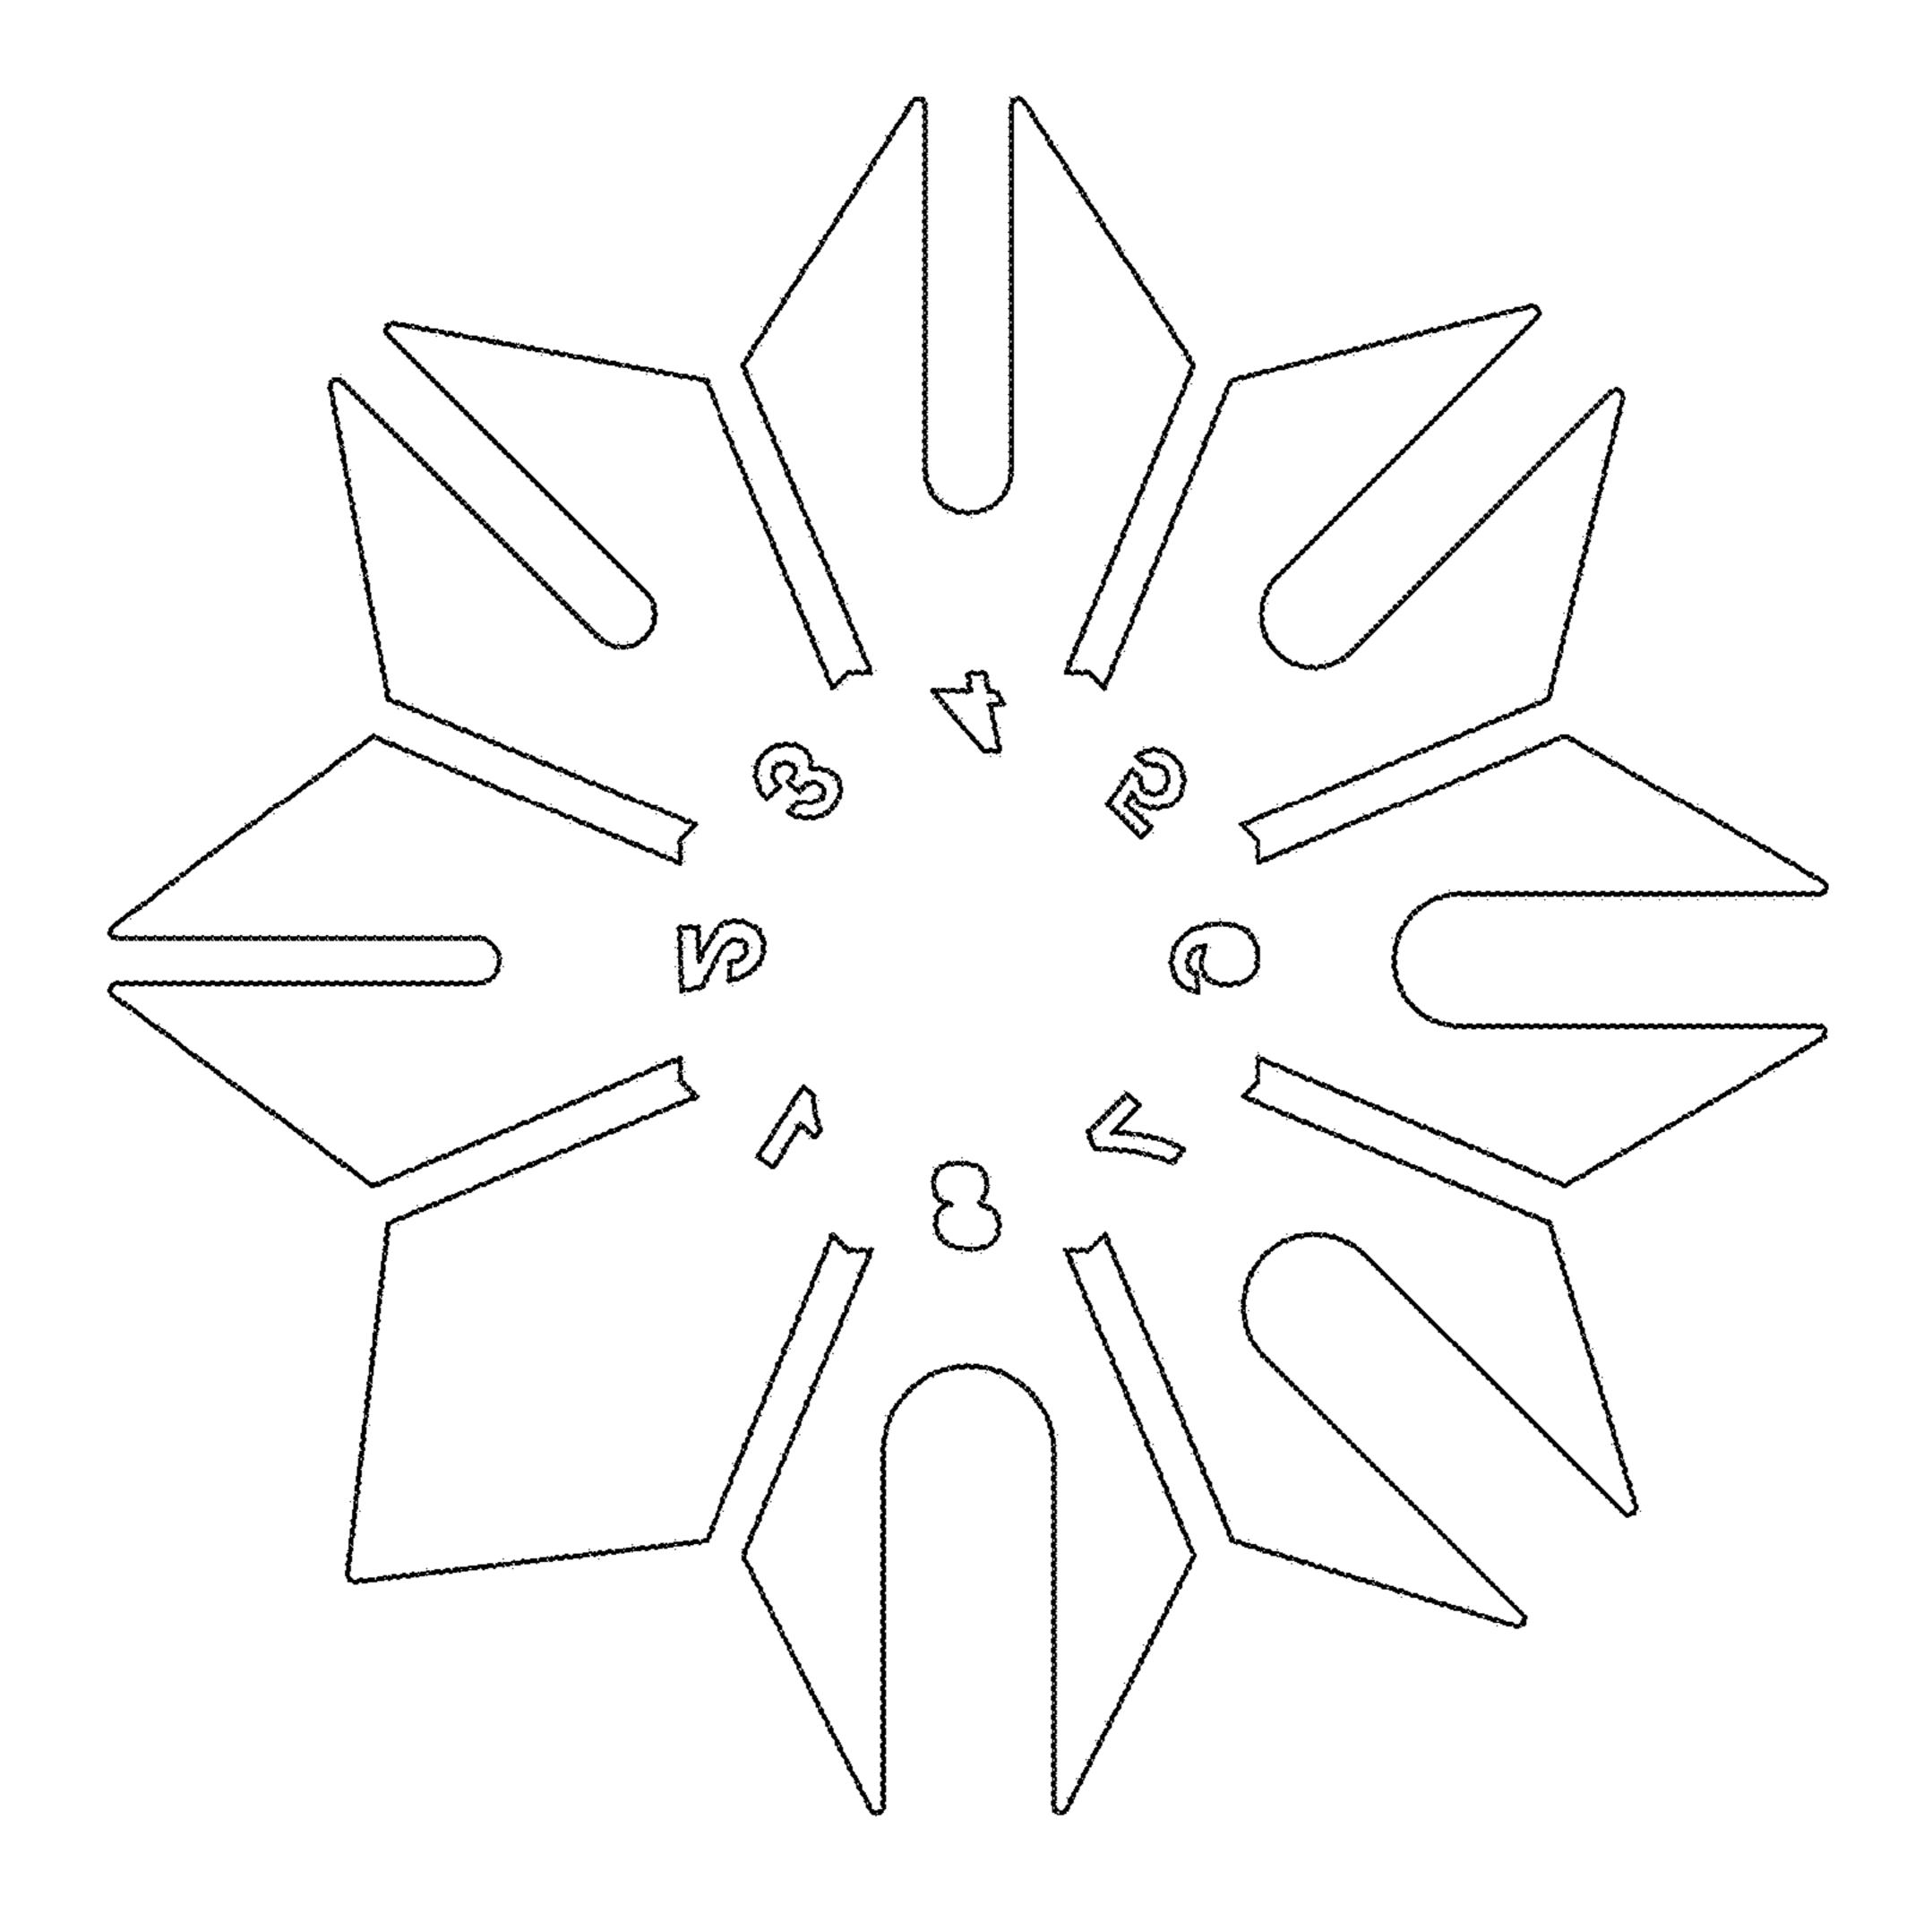
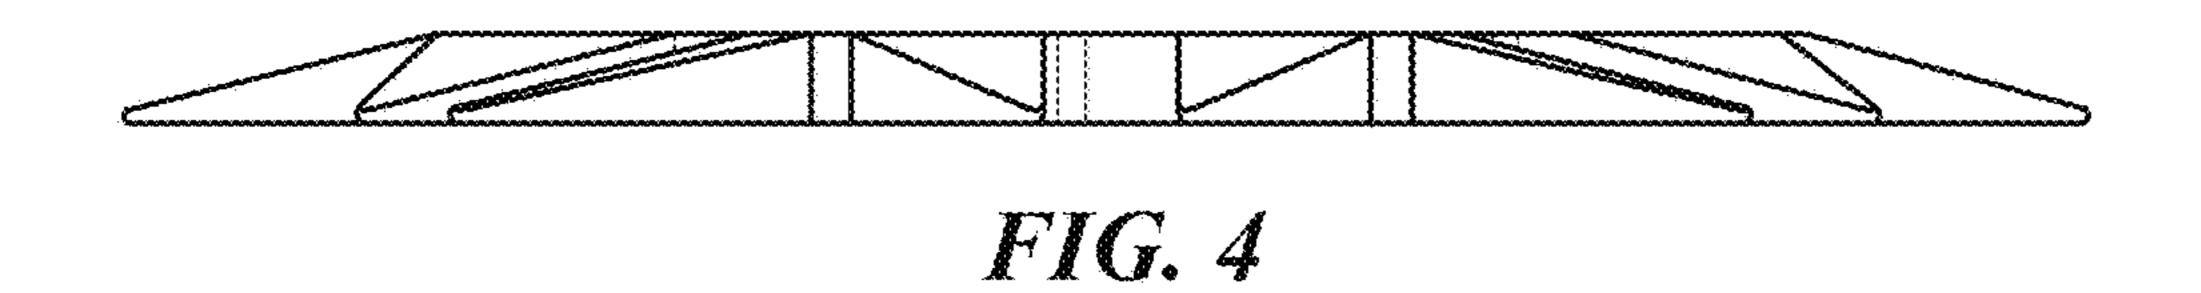


FIG. 3



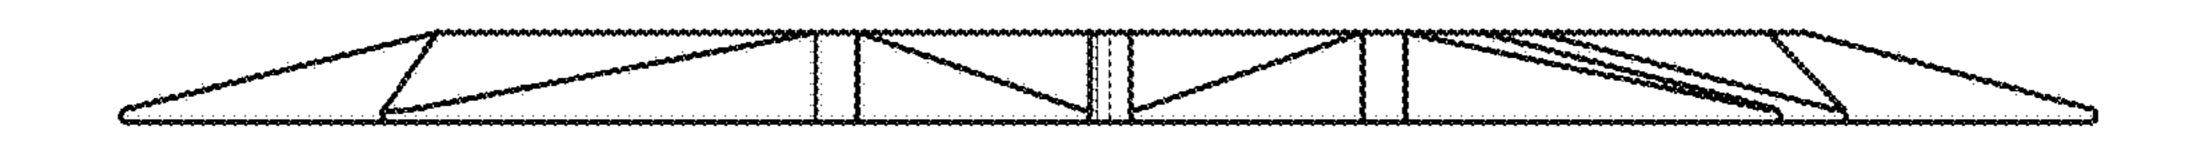


FIG. 5

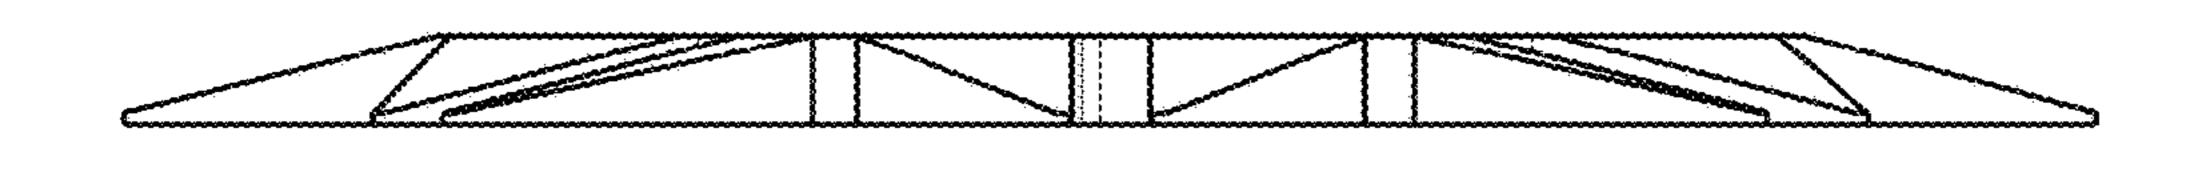


FIG. 6

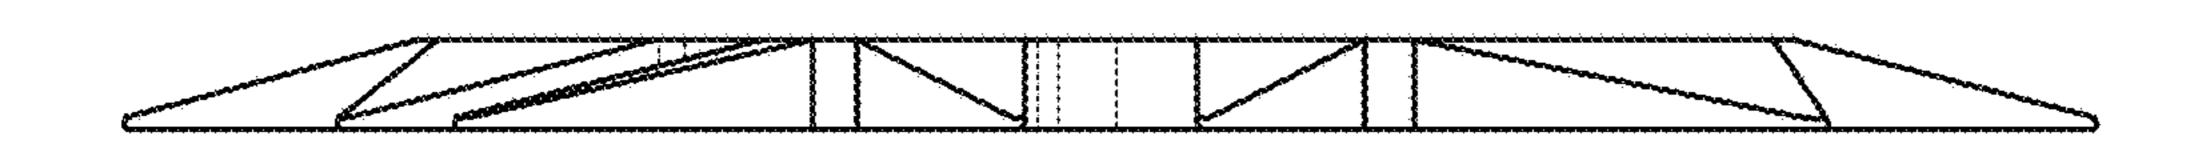
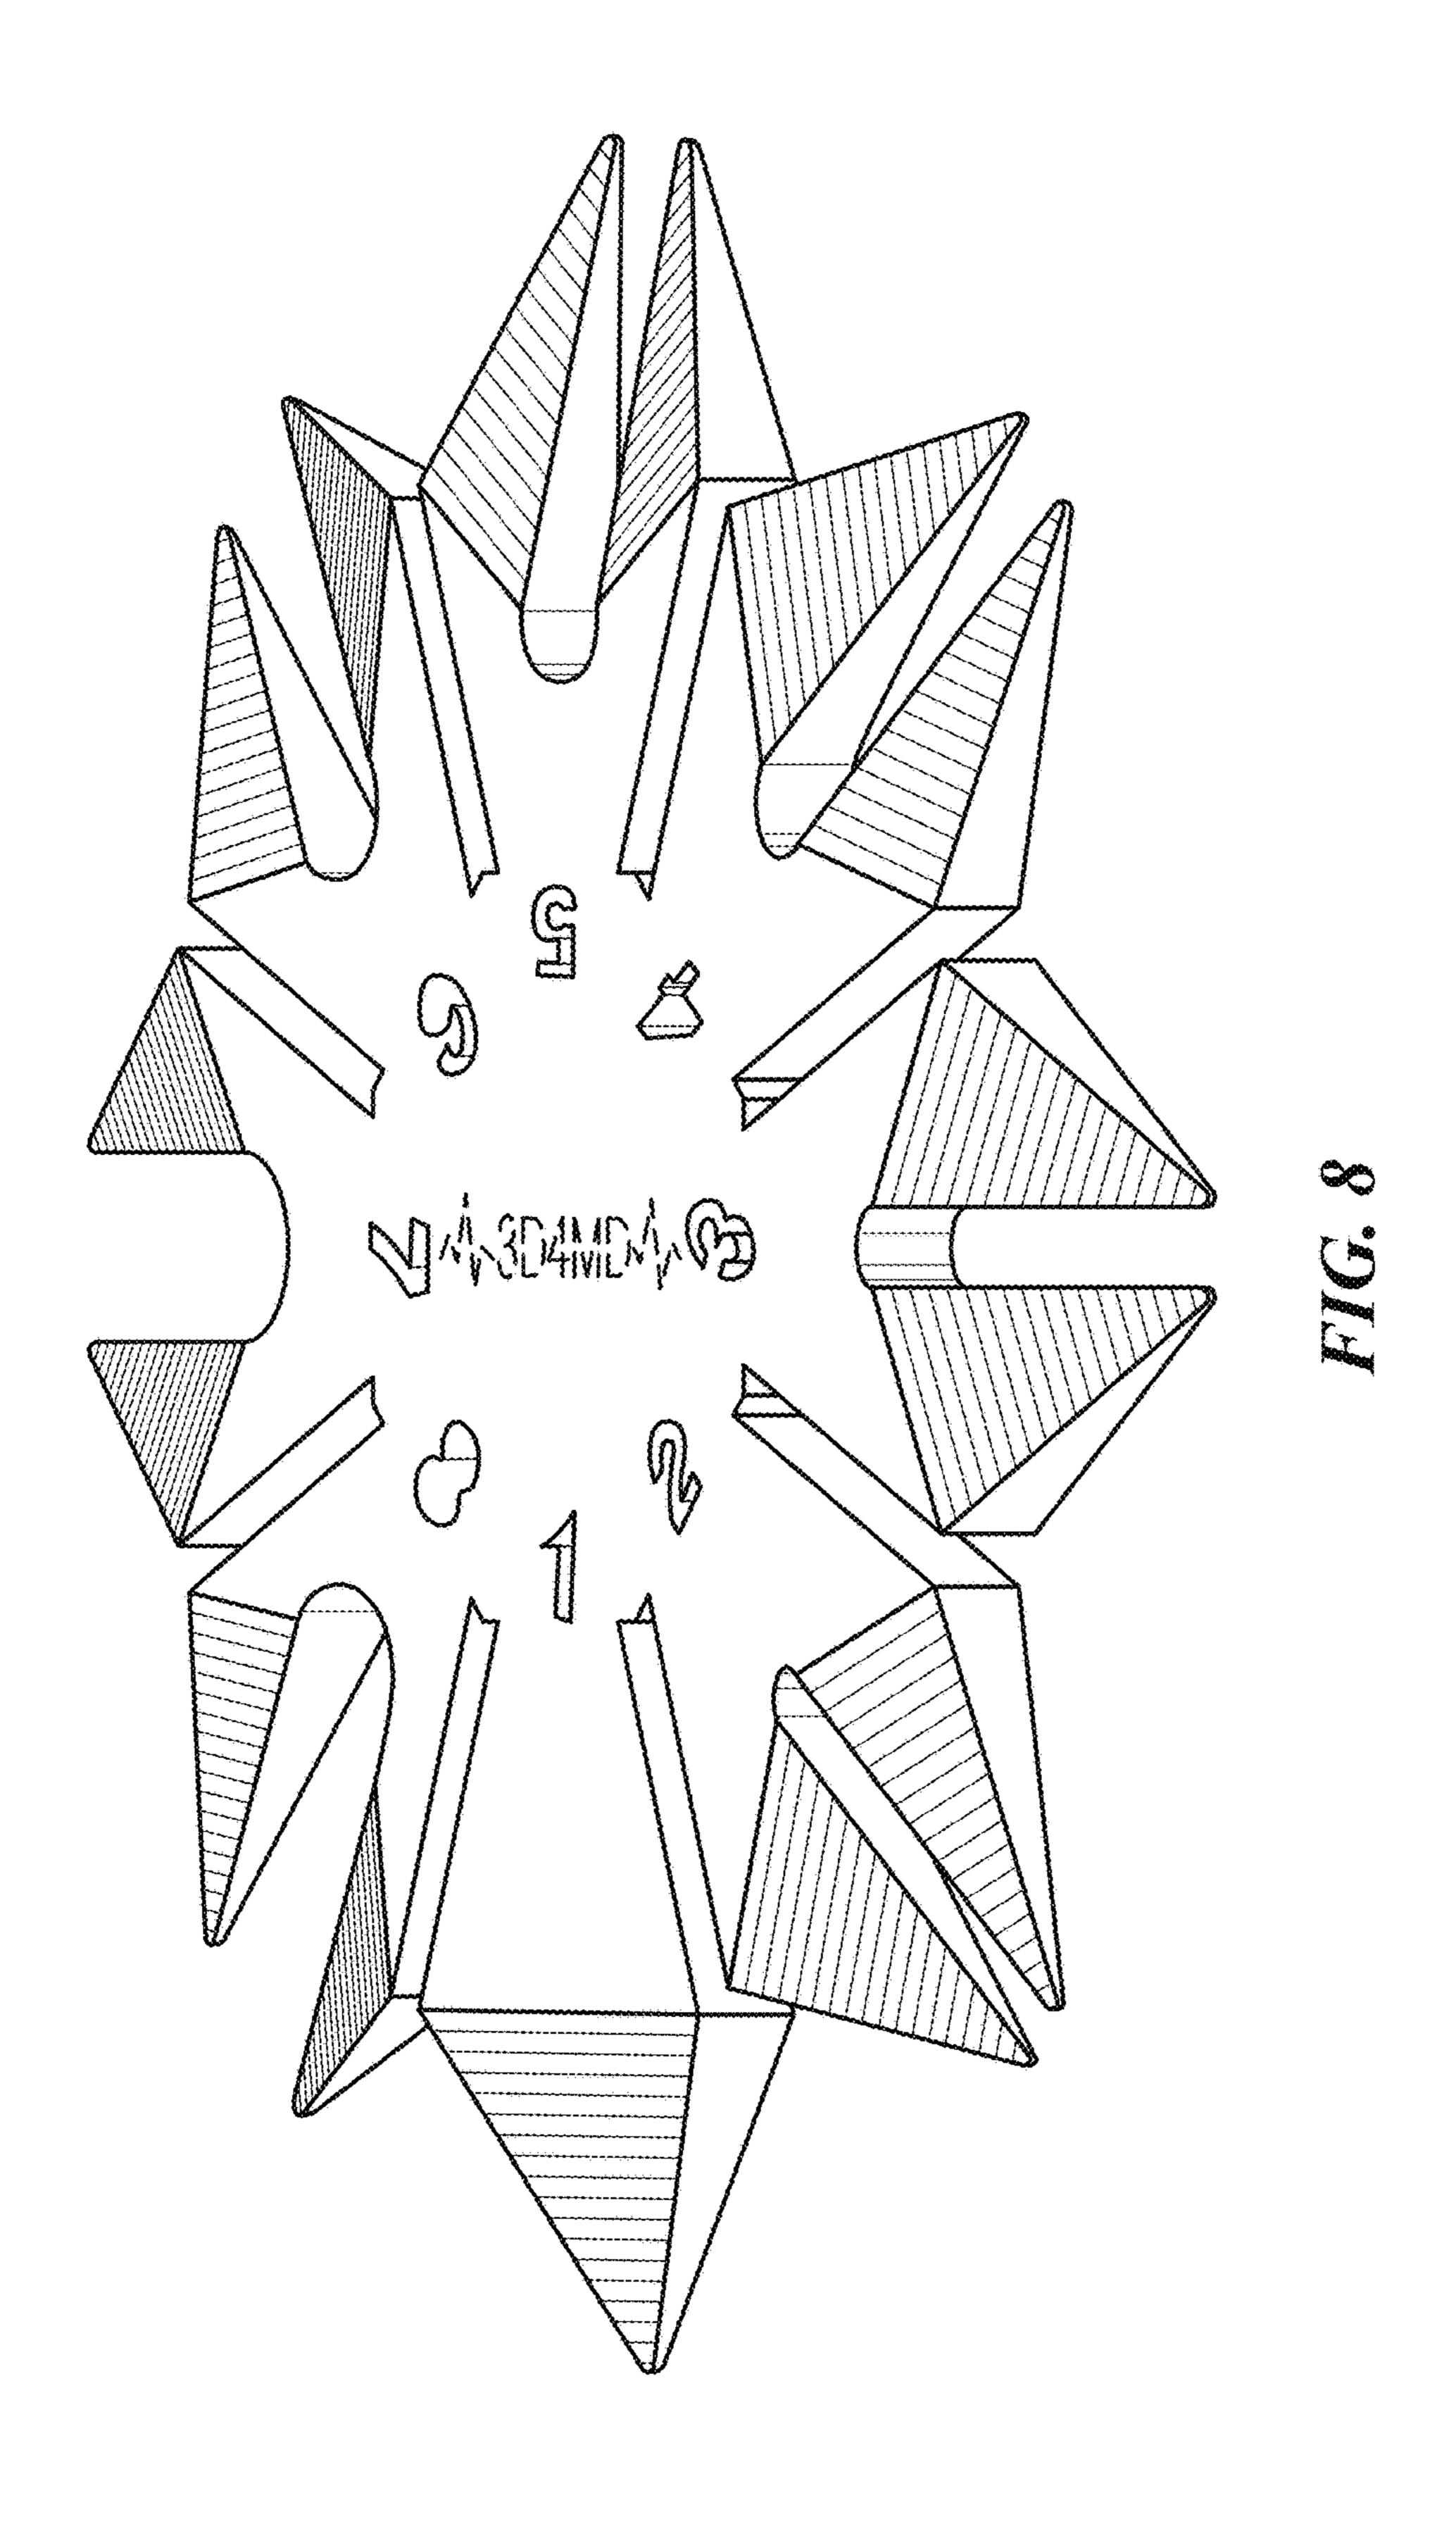


FIG. 7



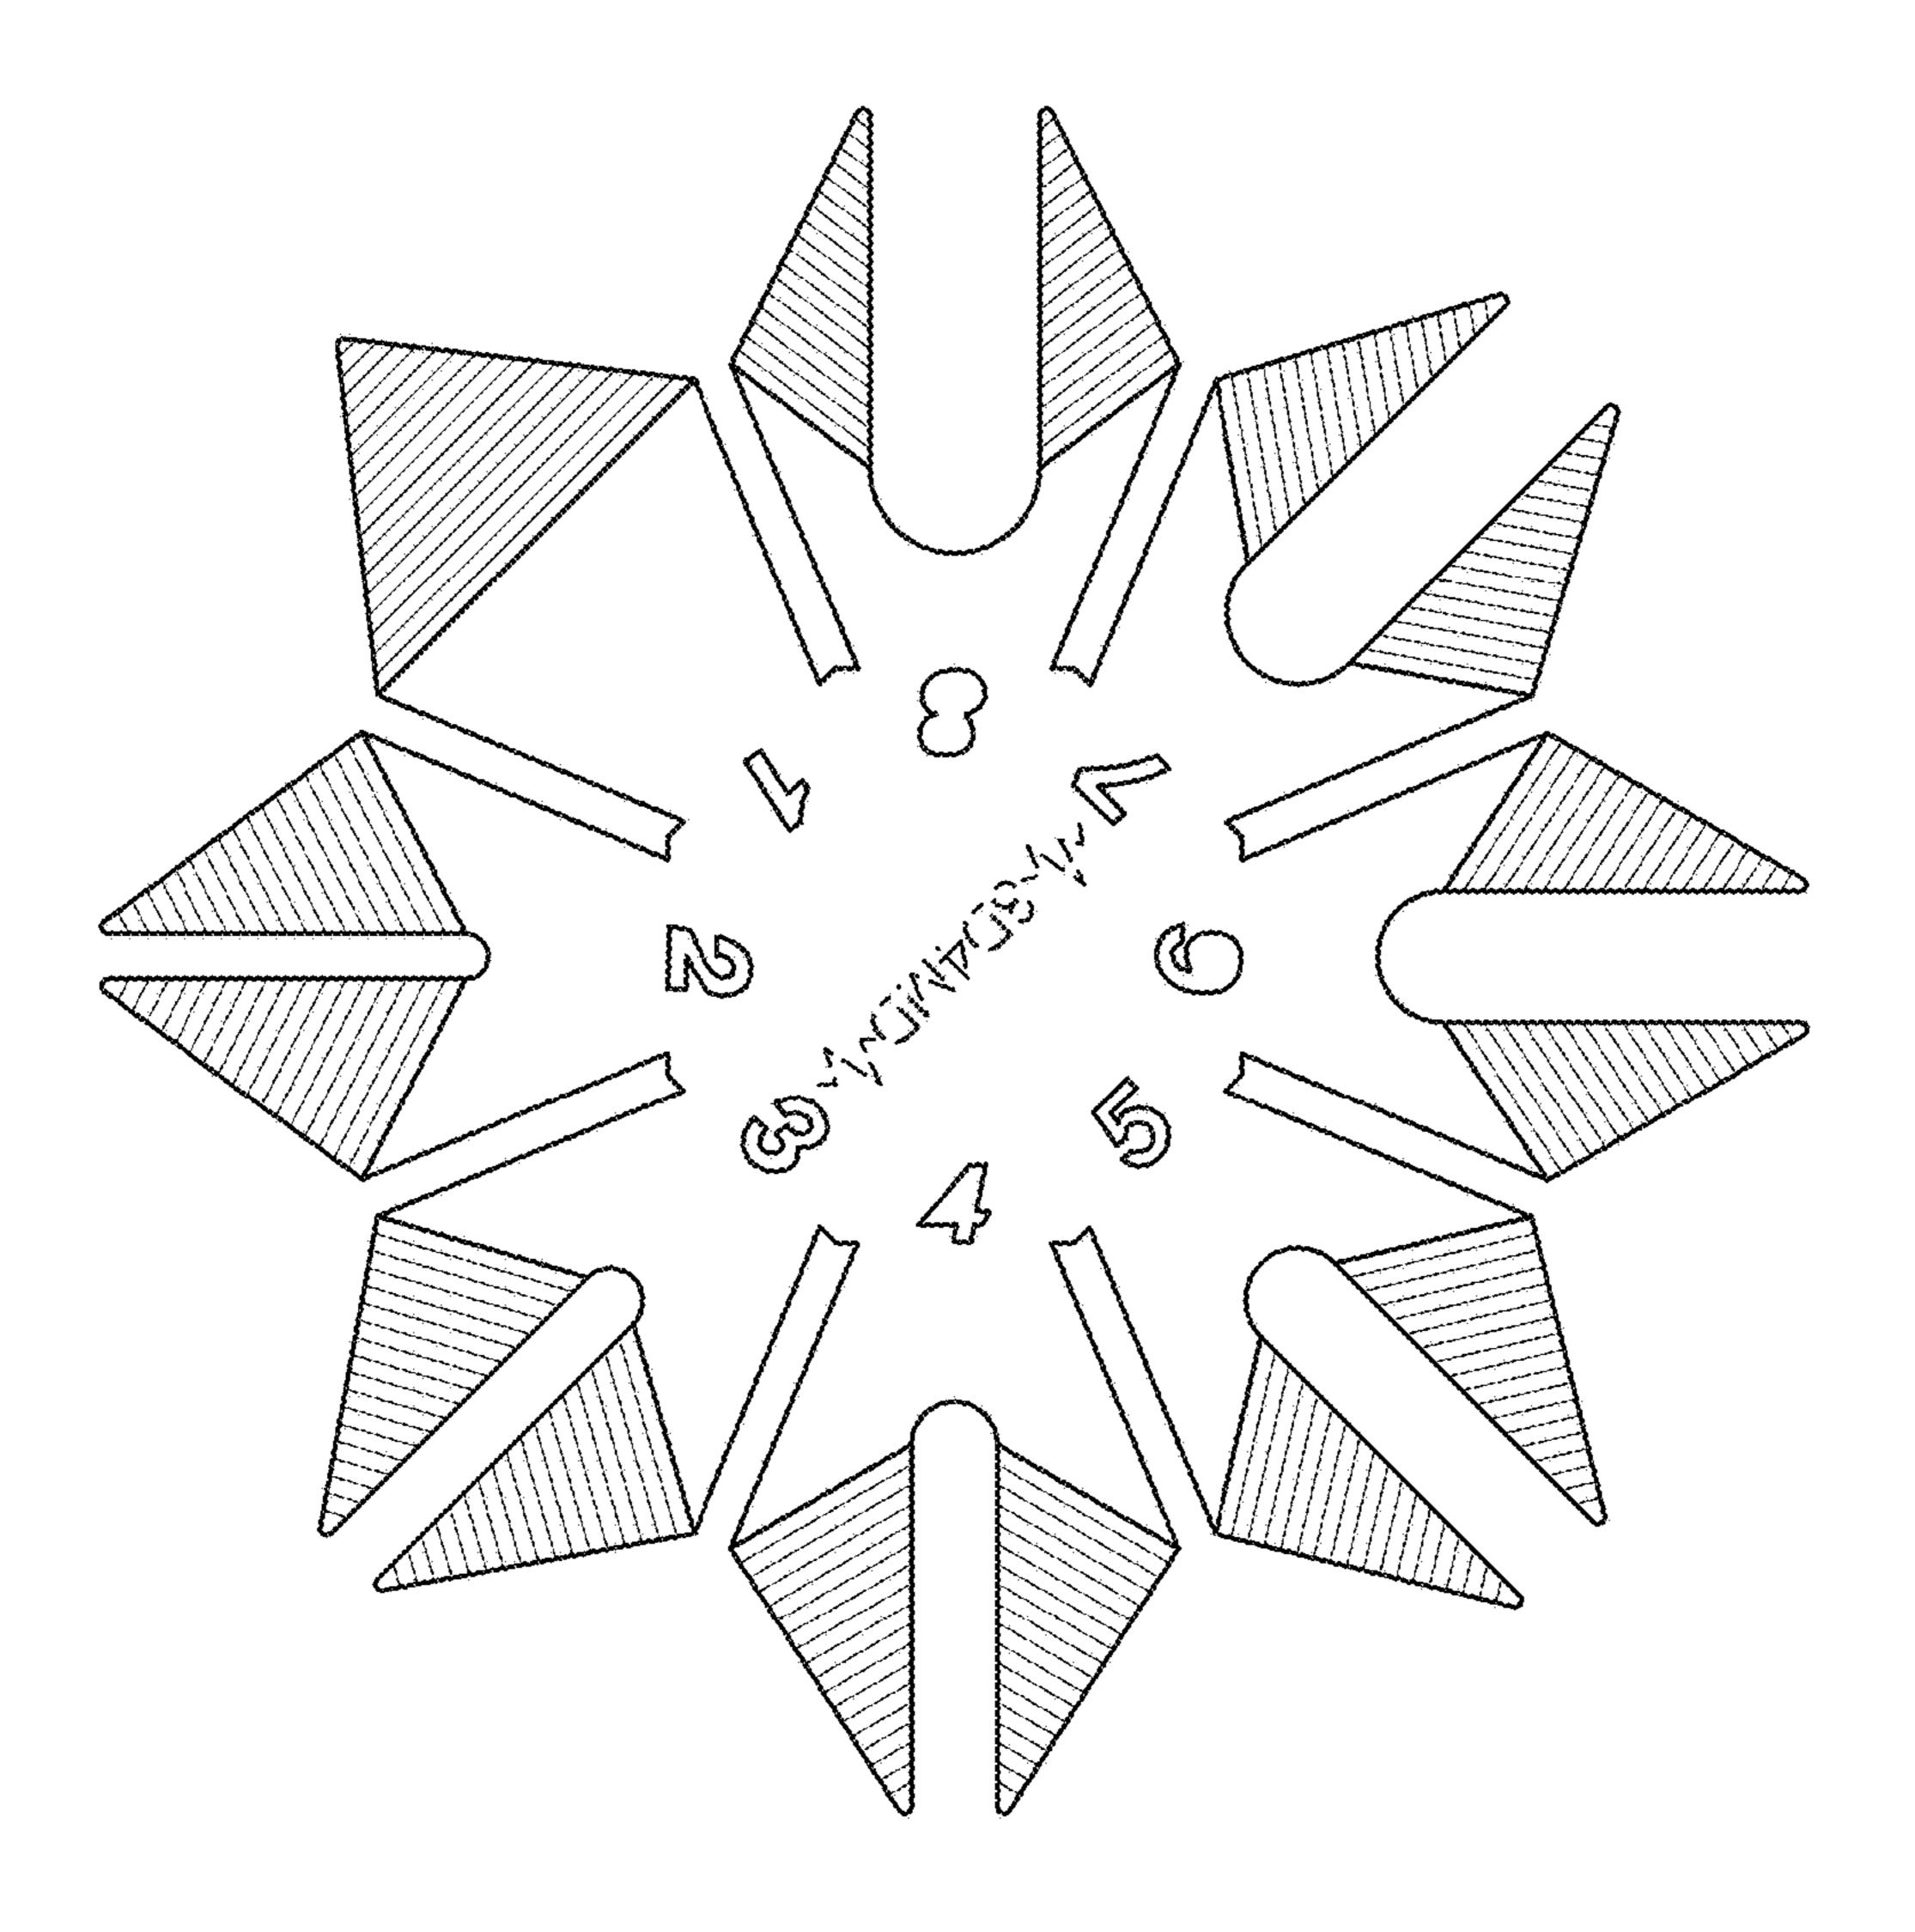


FIG. 9

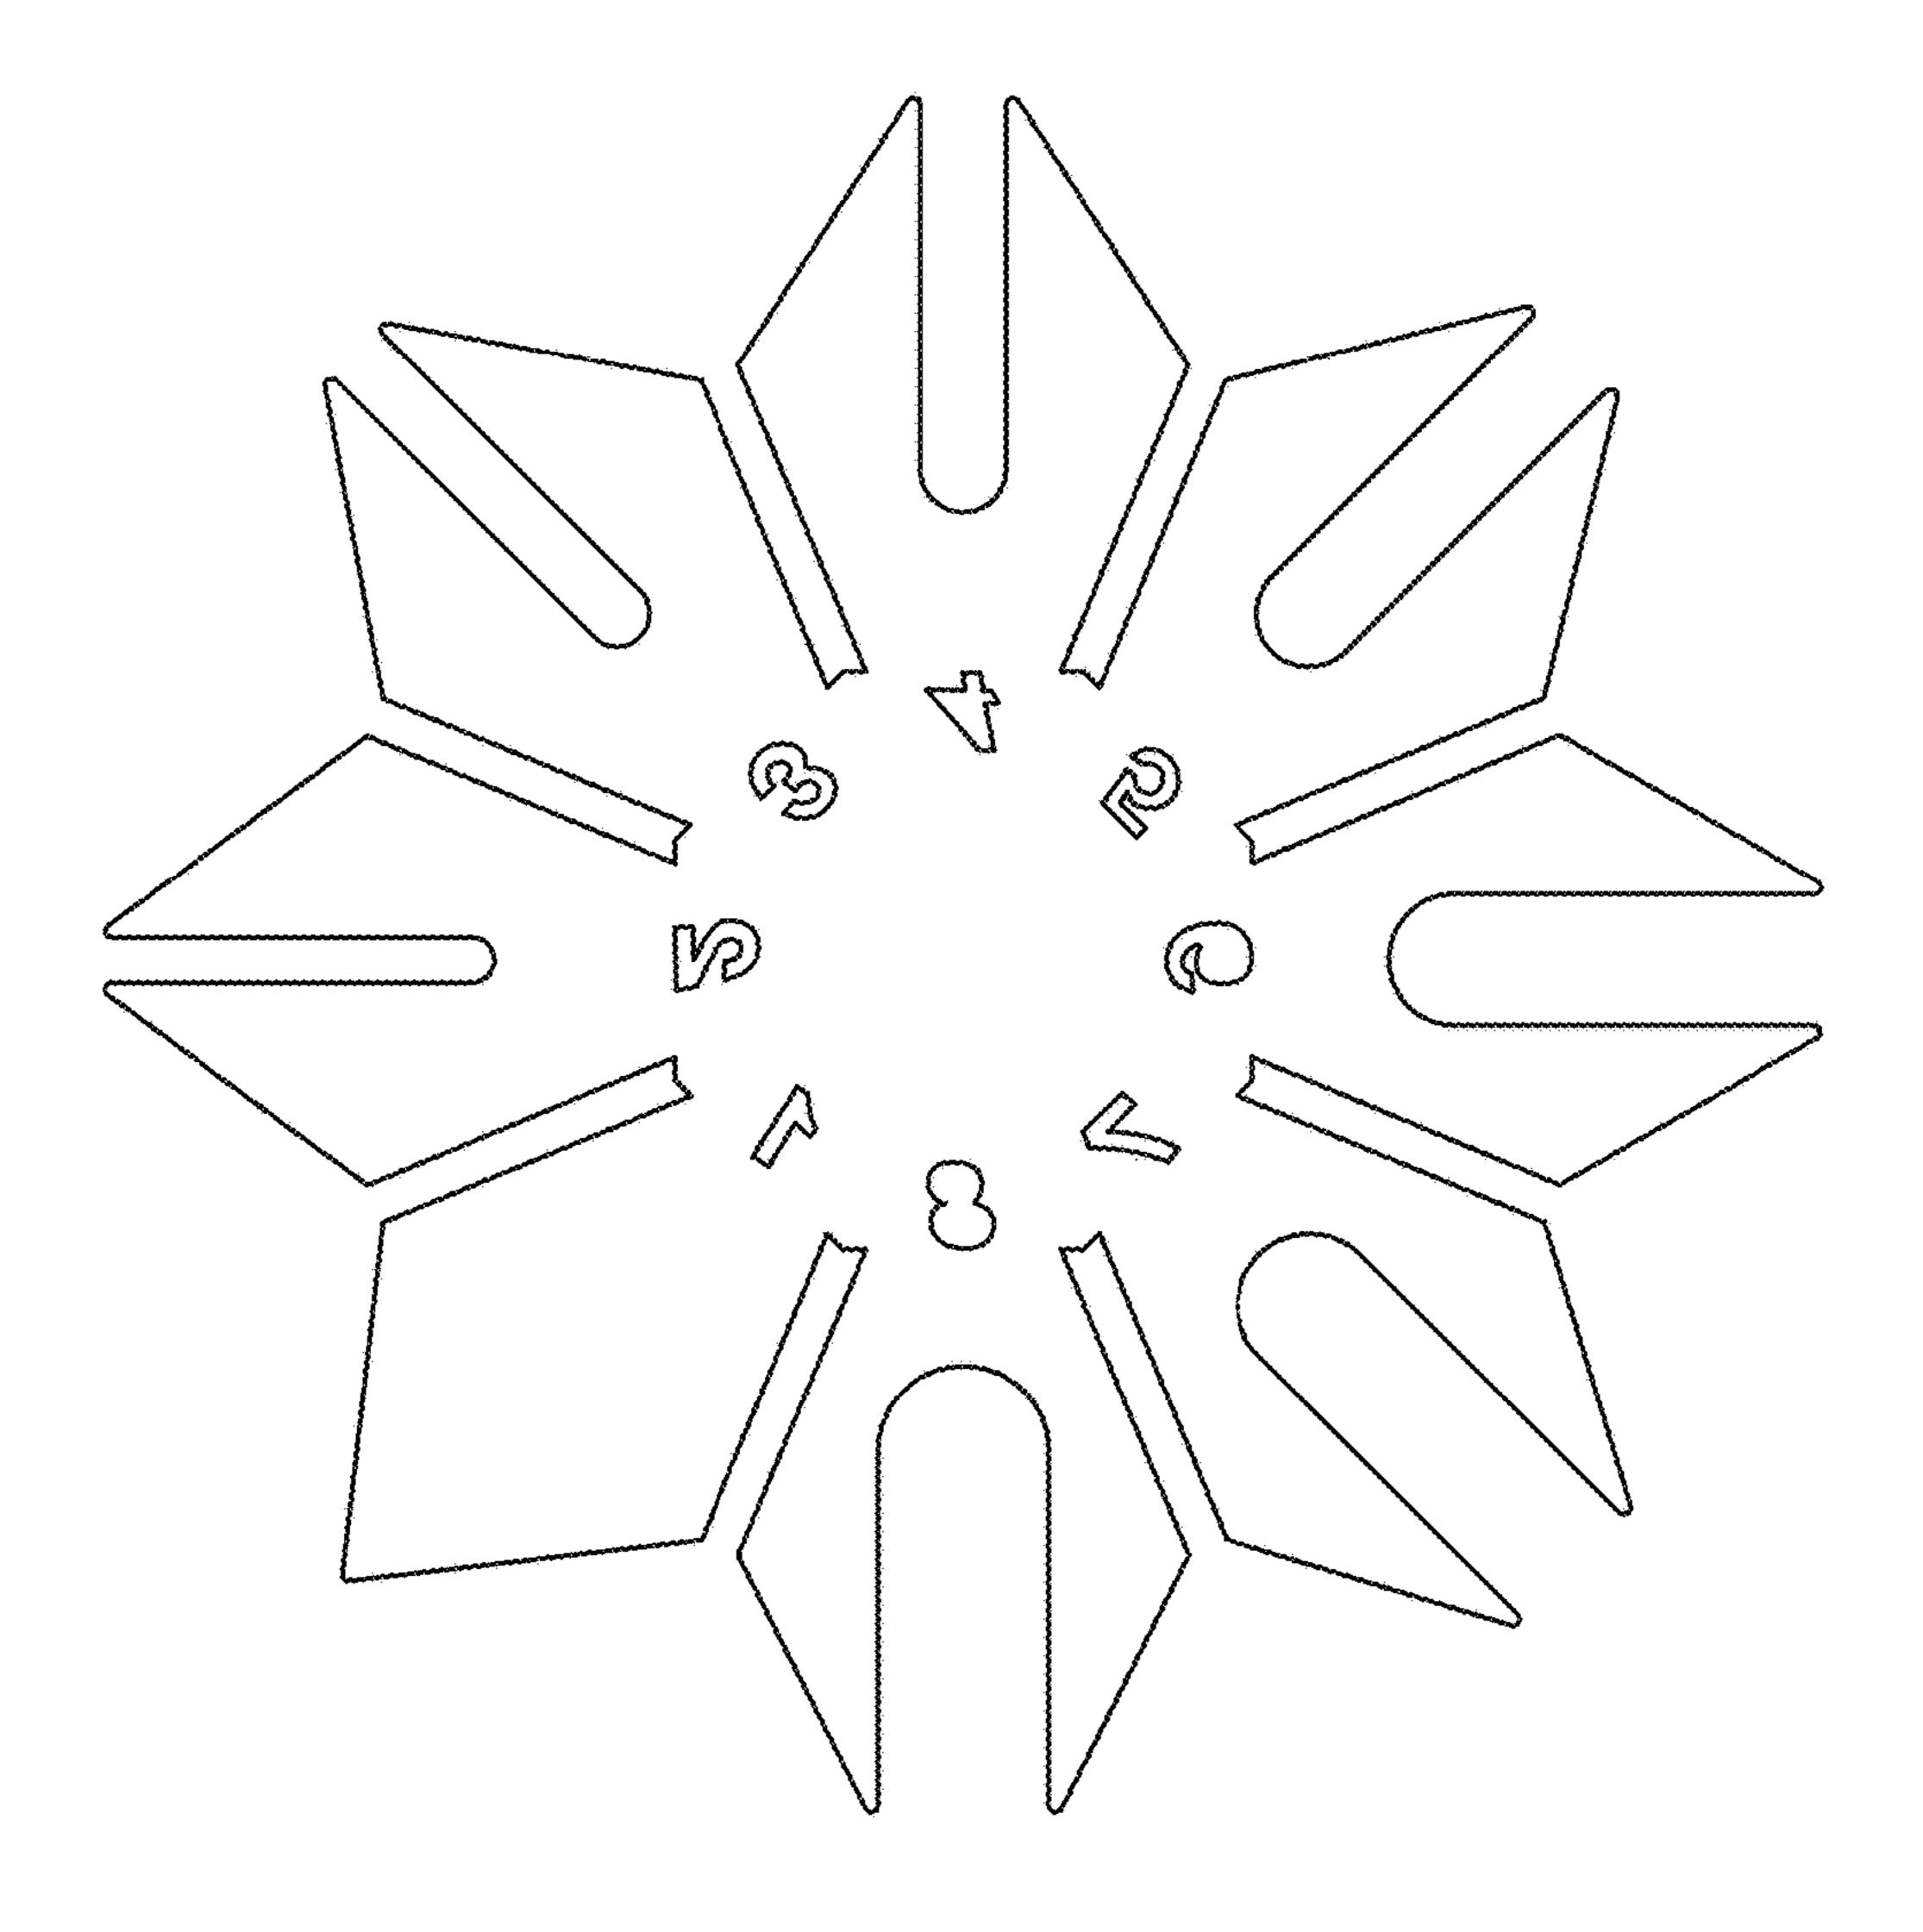


FIG. 10

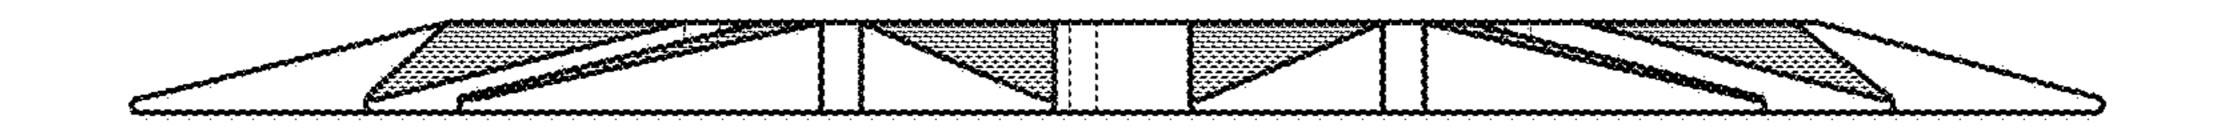


FIG. 11

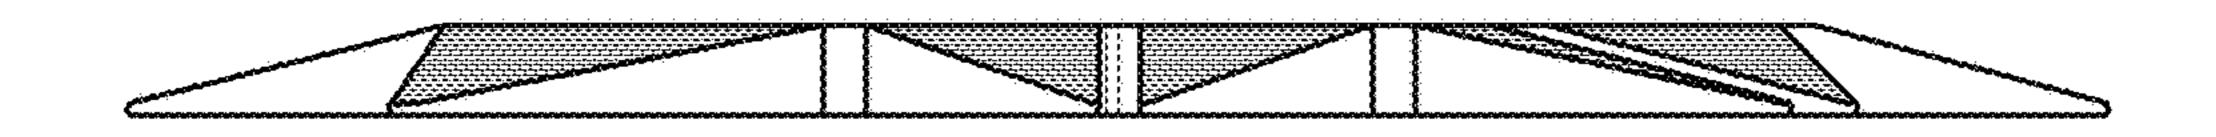


FIG. 12

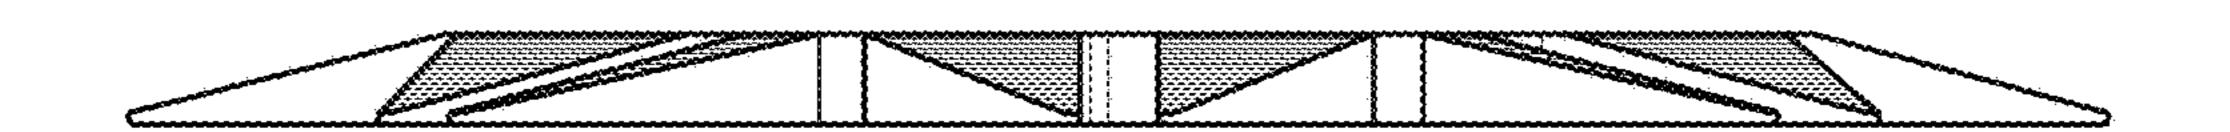


FIG. 13

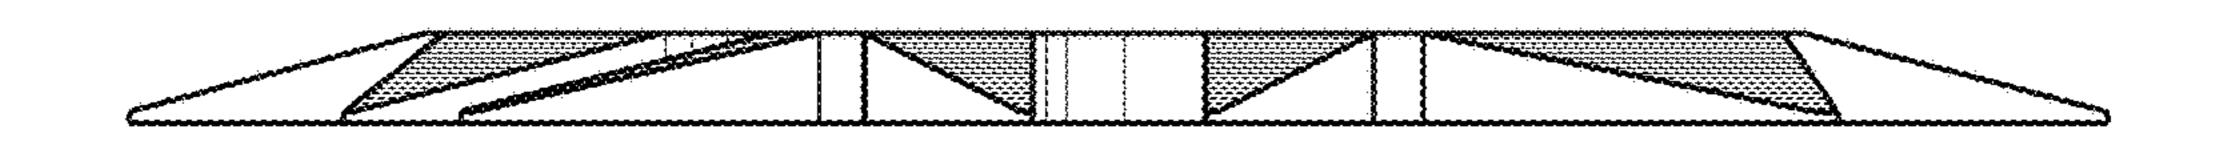
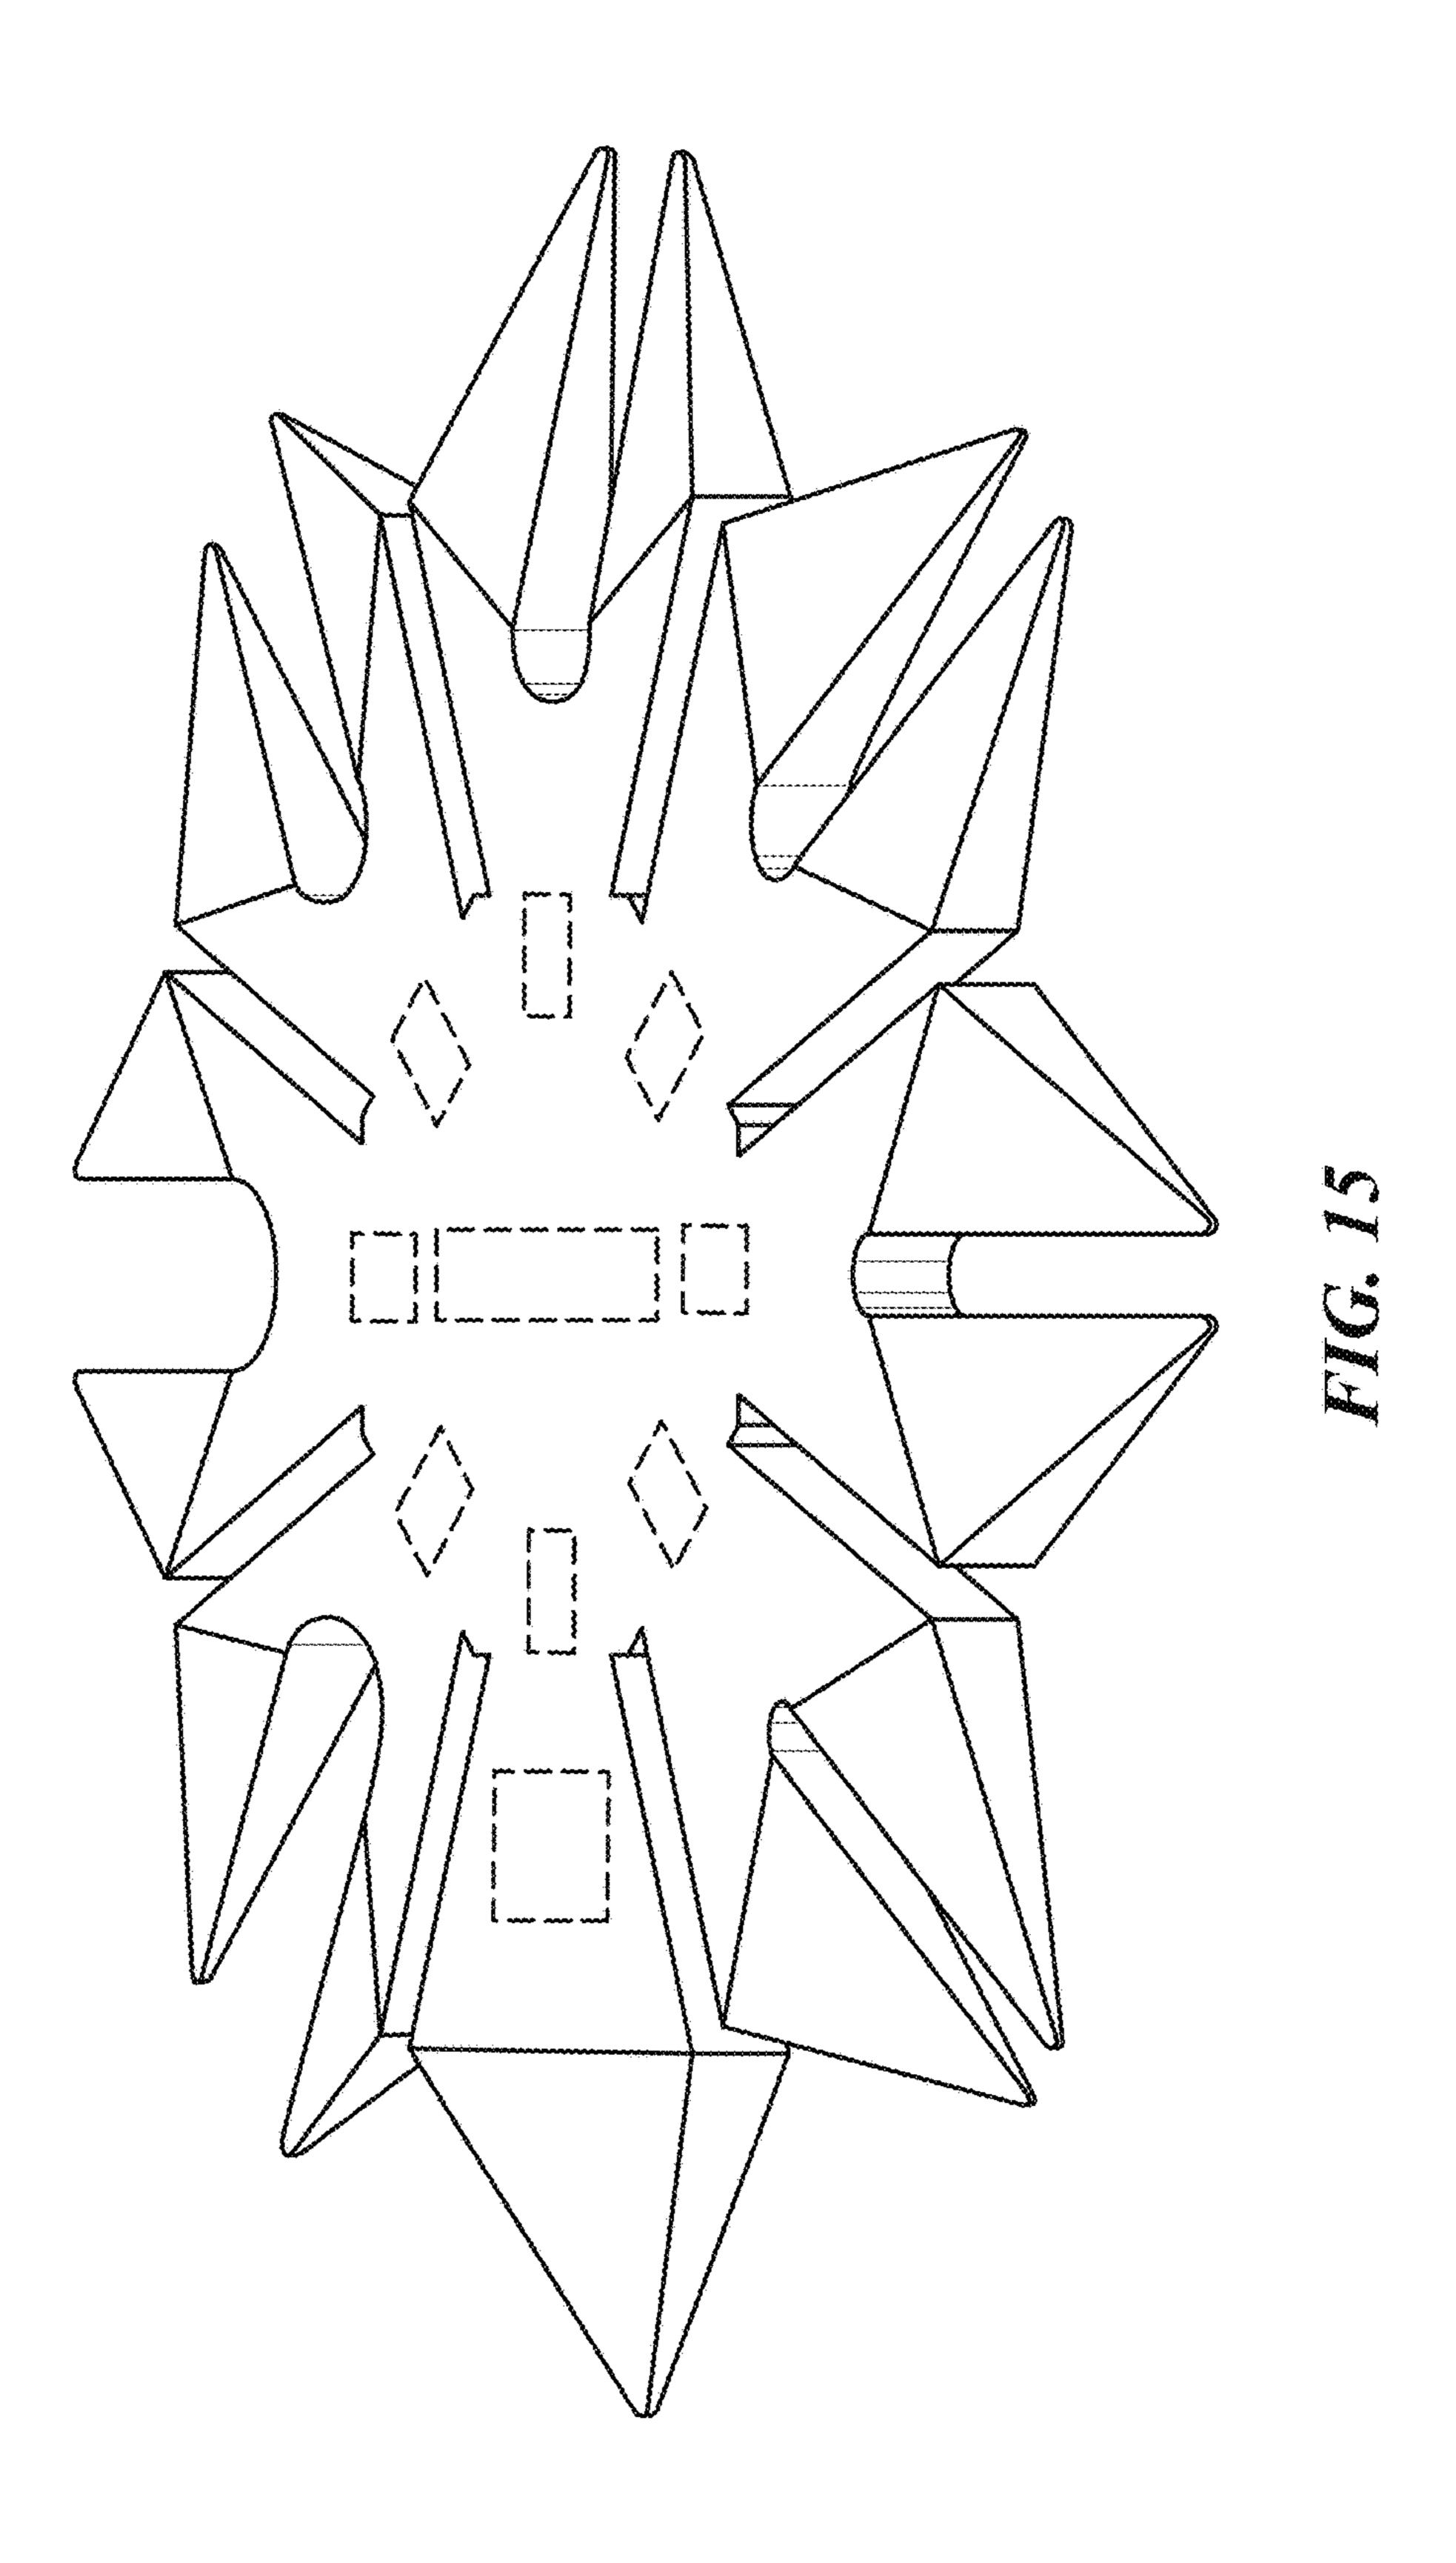


FIG. 14



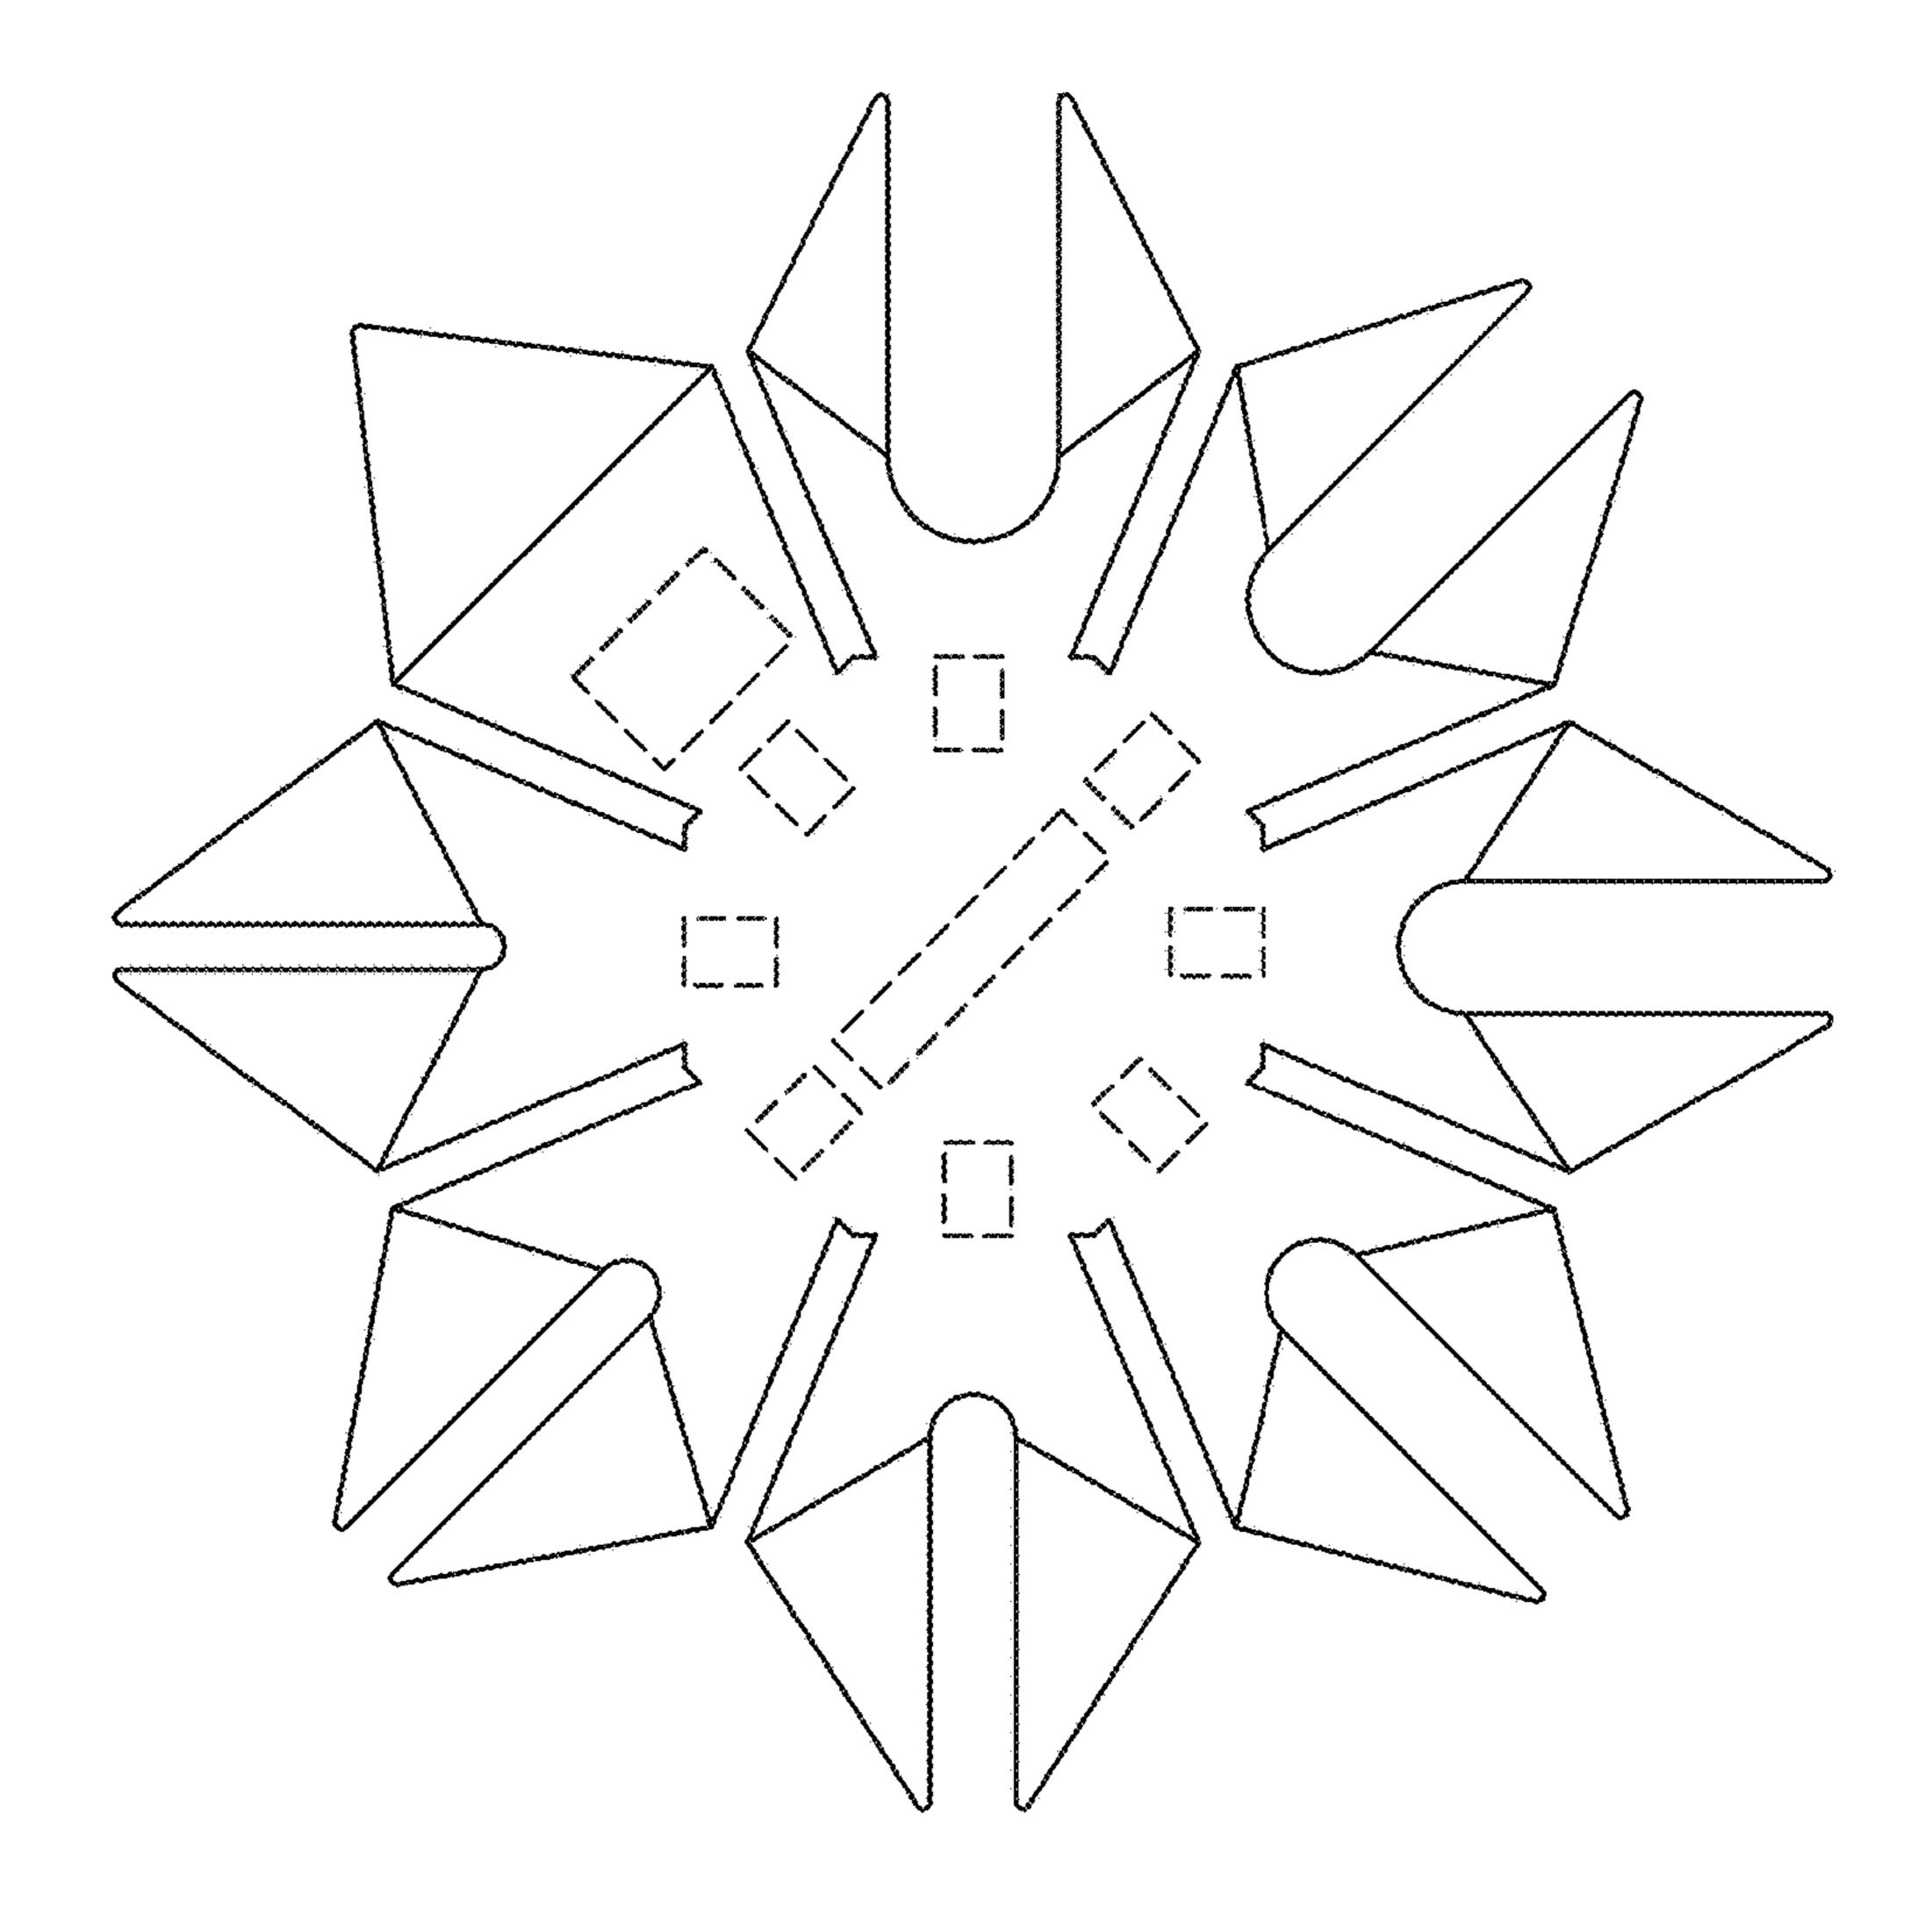


FIG. 16

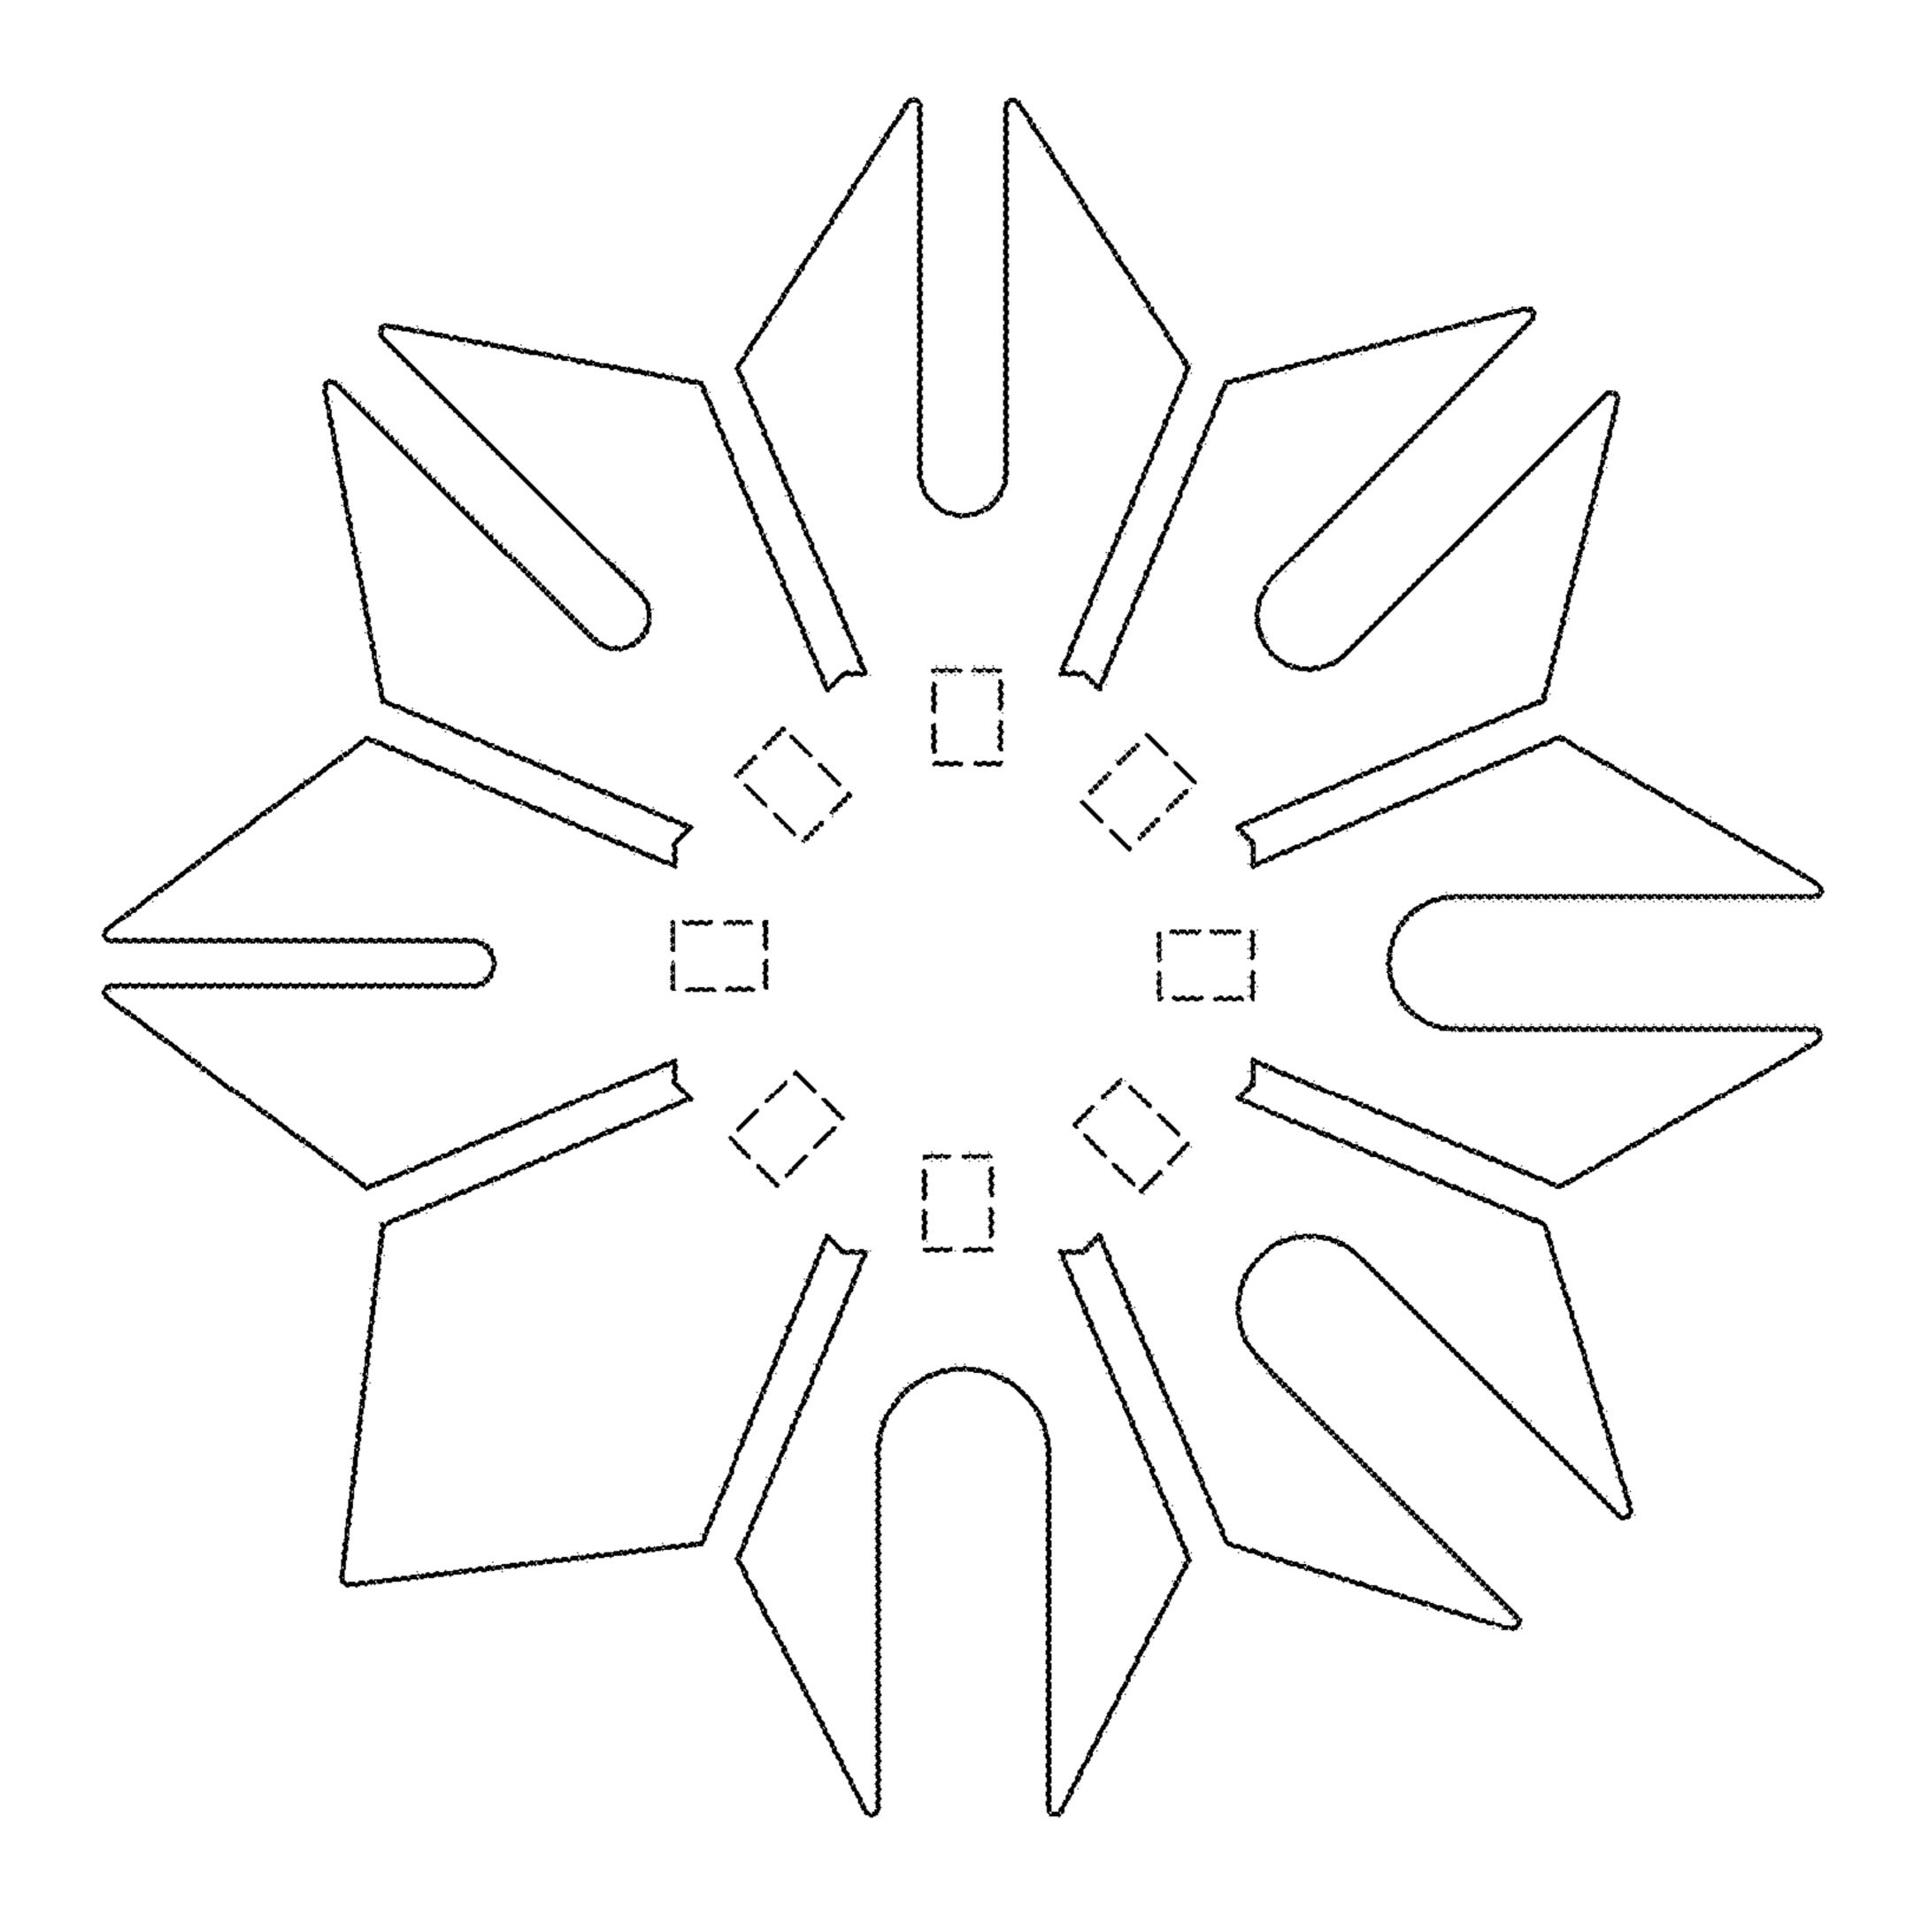


FIG. 17



FIG. 18

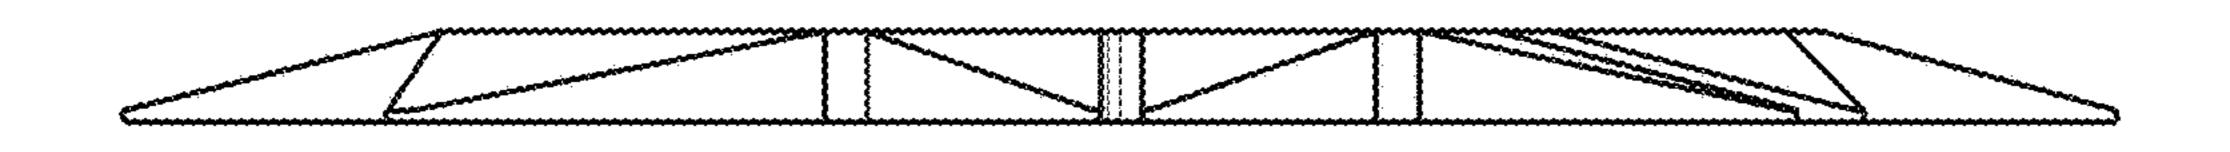


FIG. 19

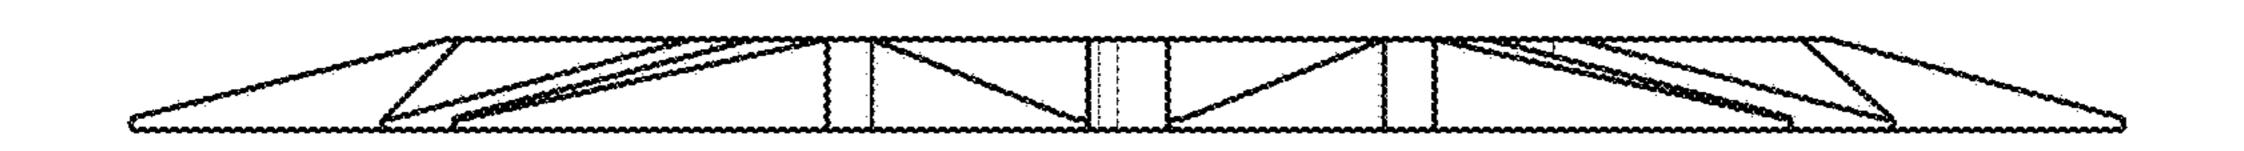


FIG. 20

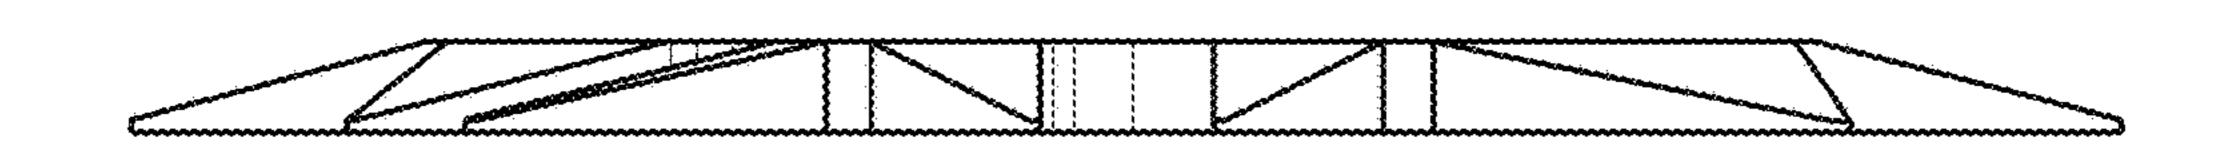
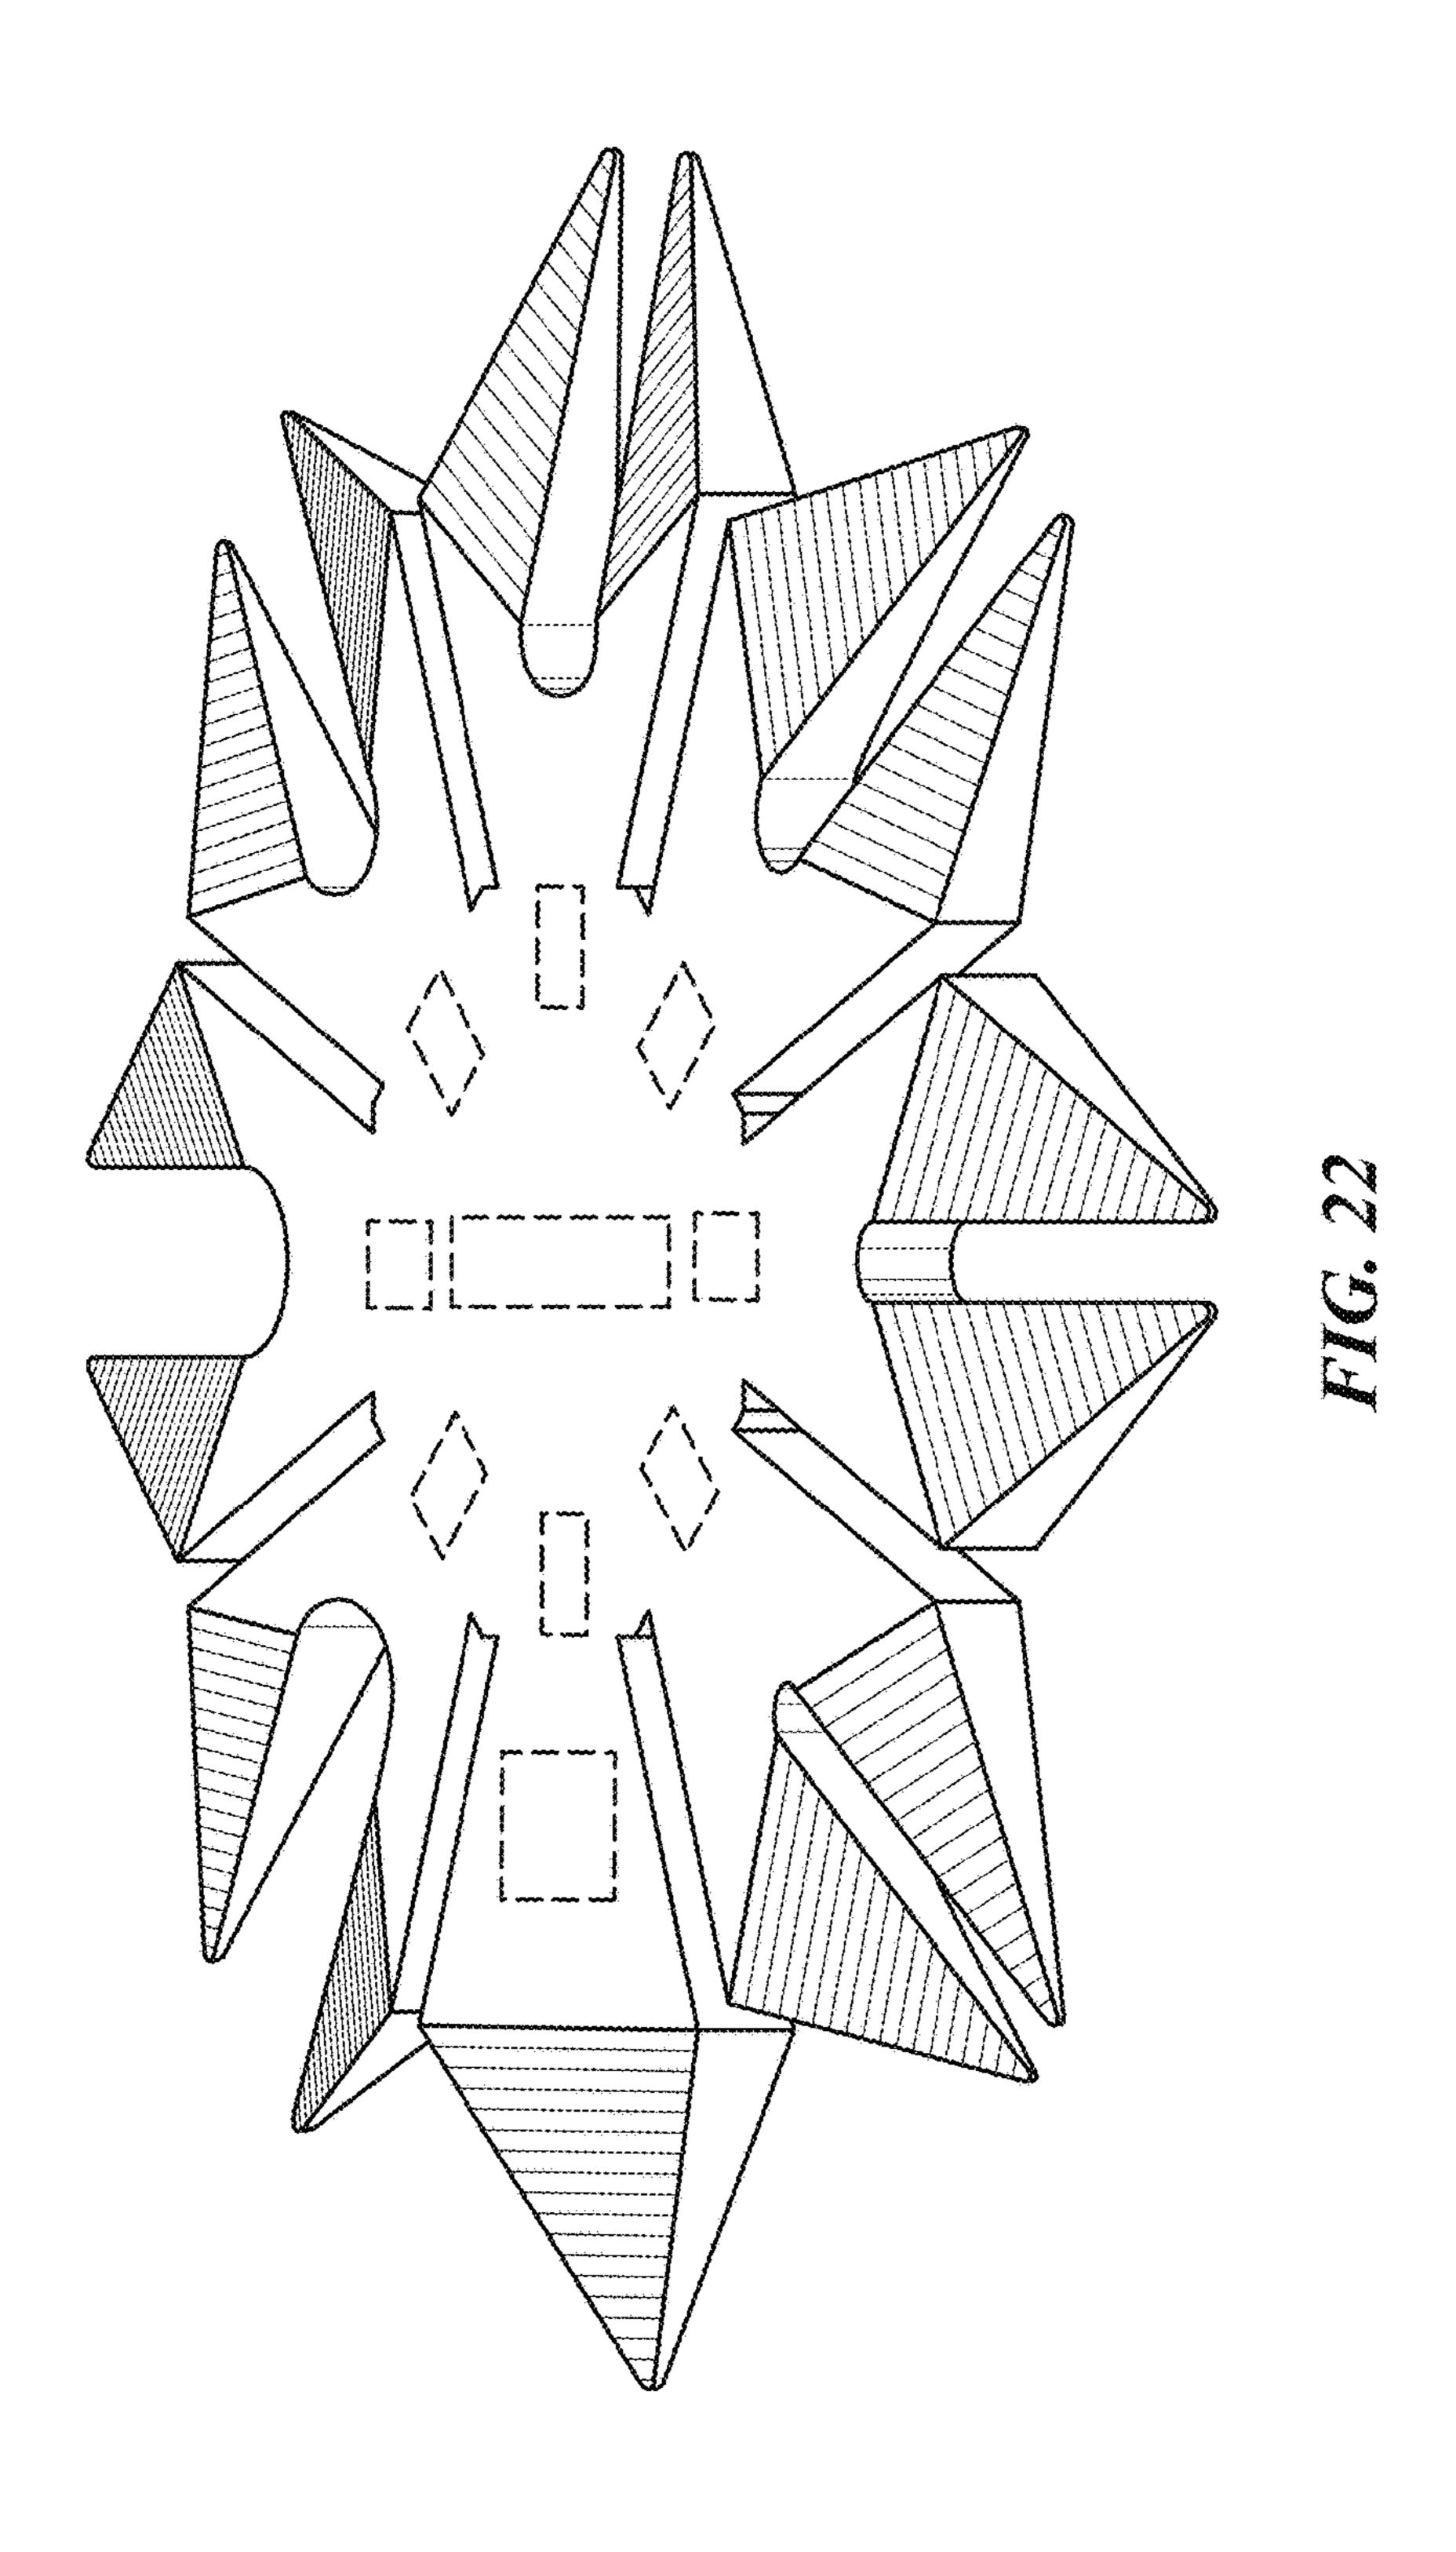


FIG. 21



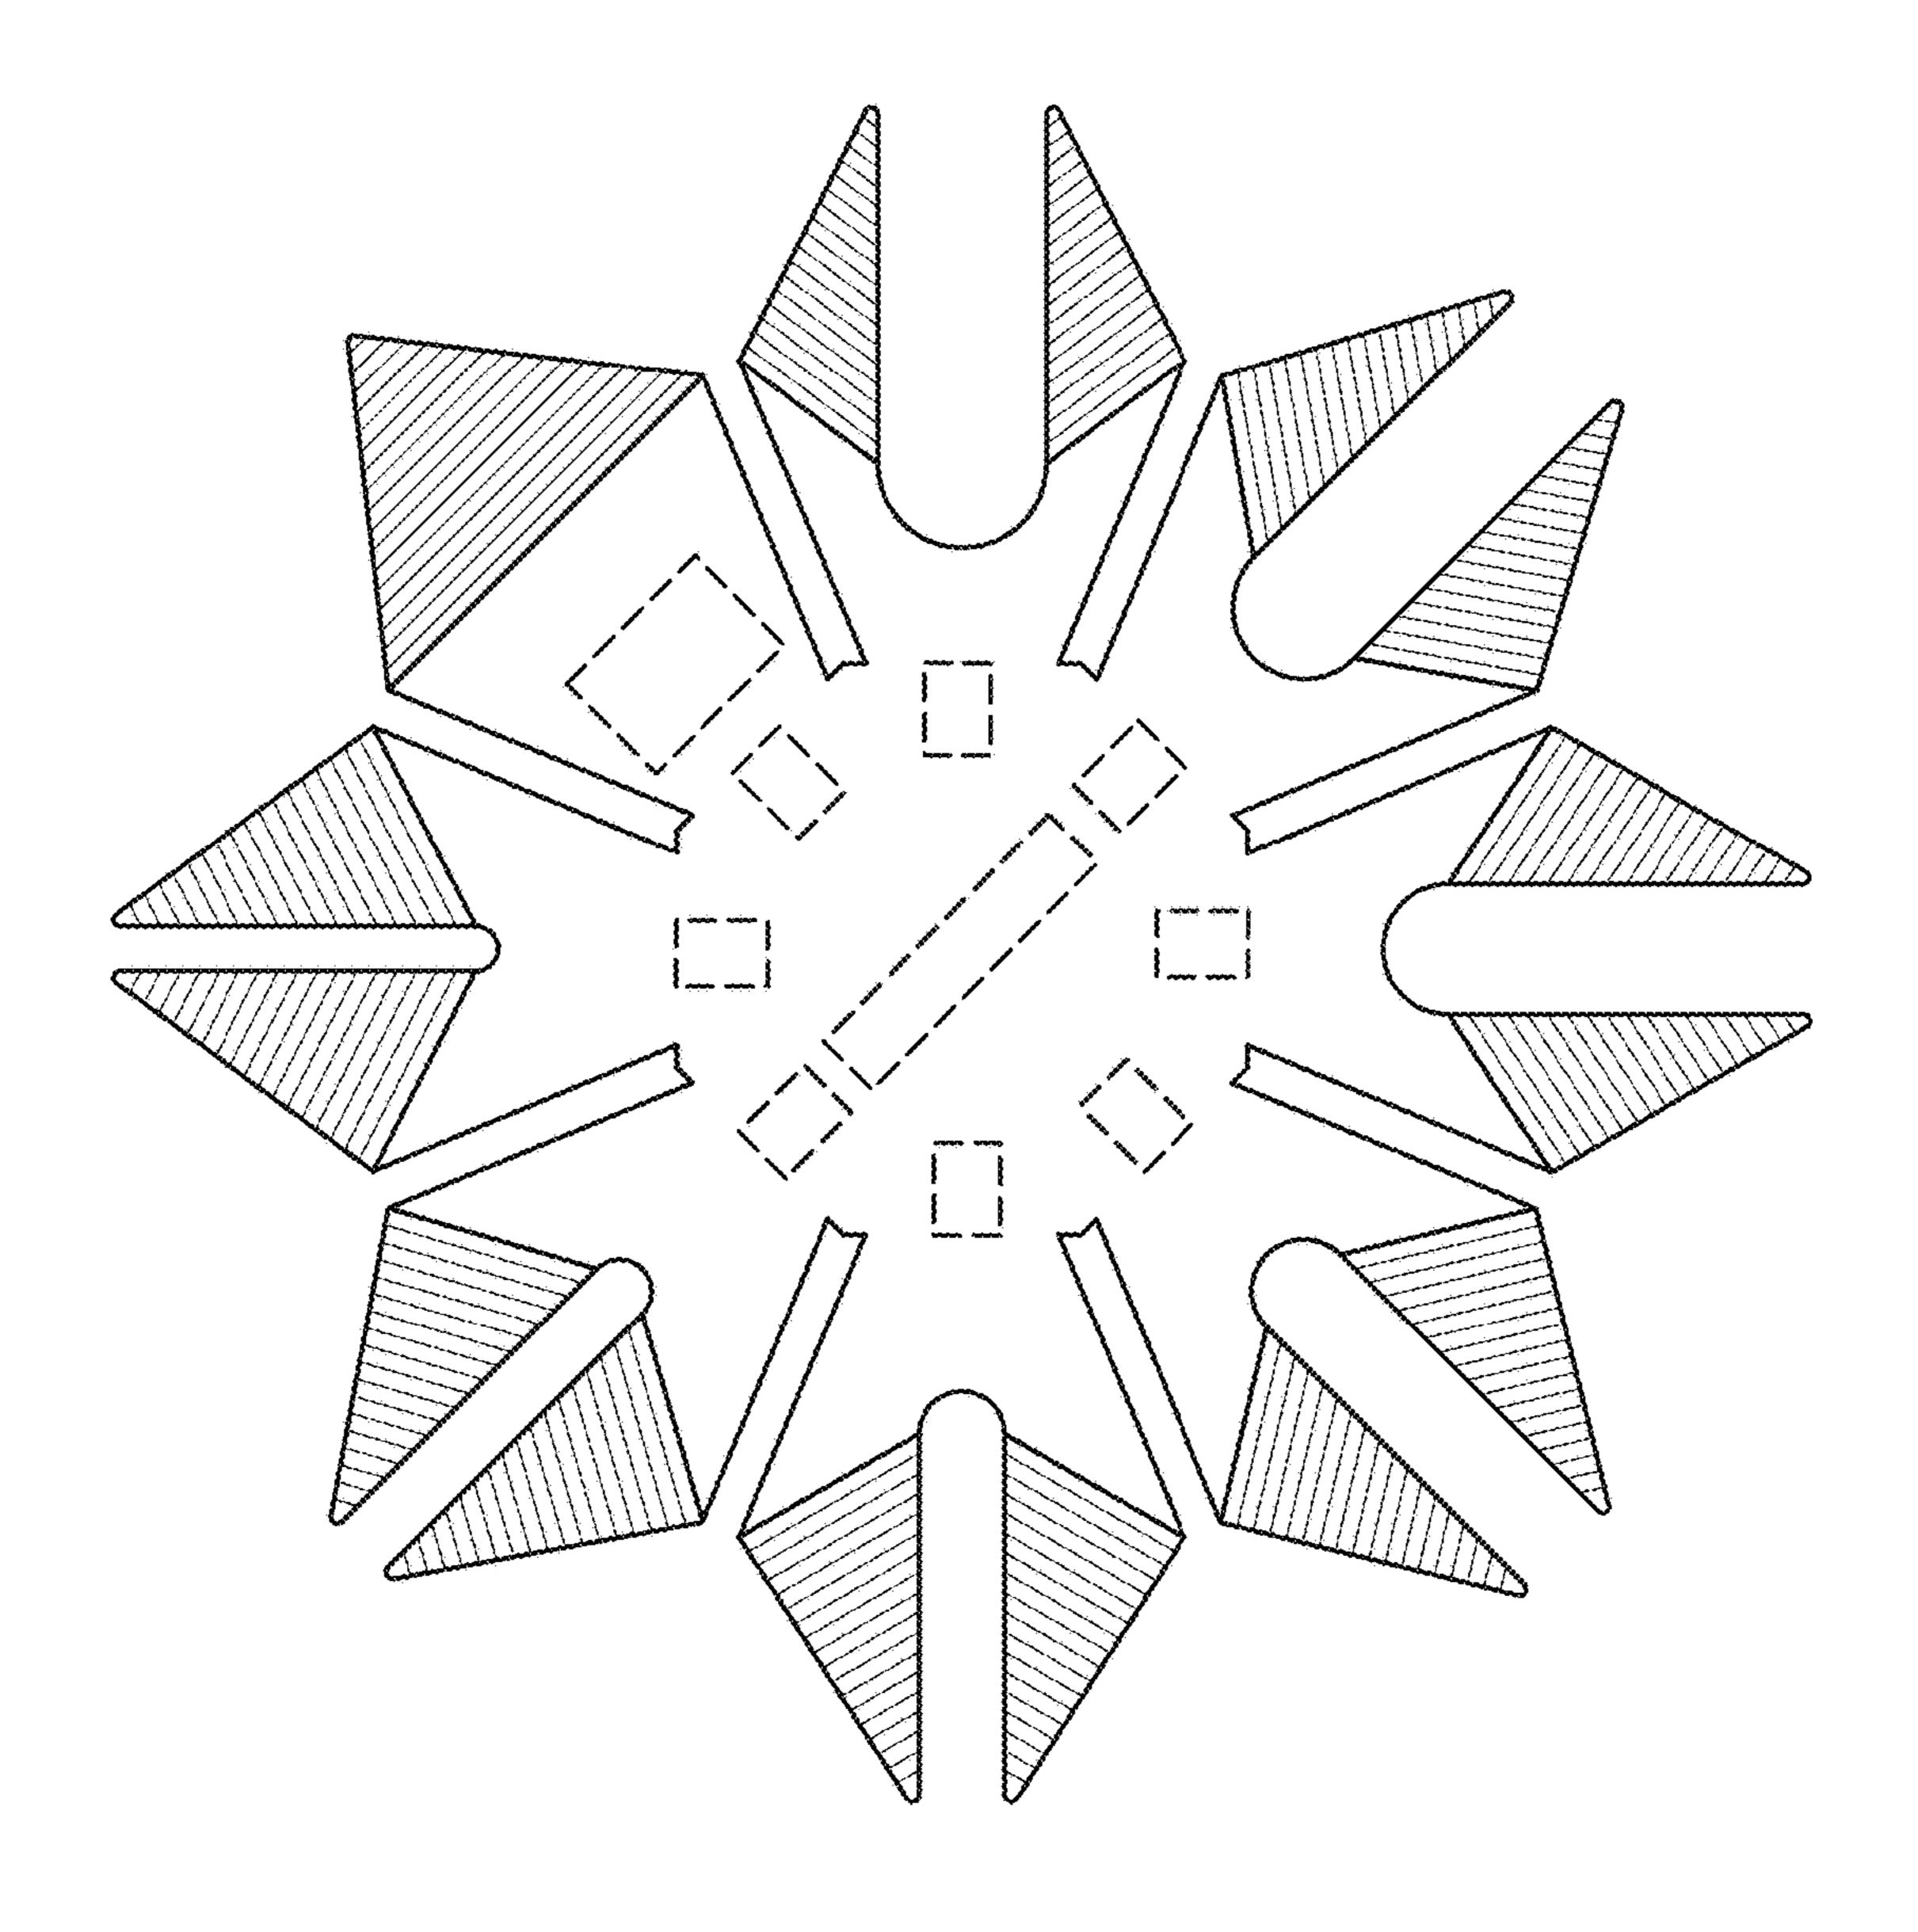


FIG. 23

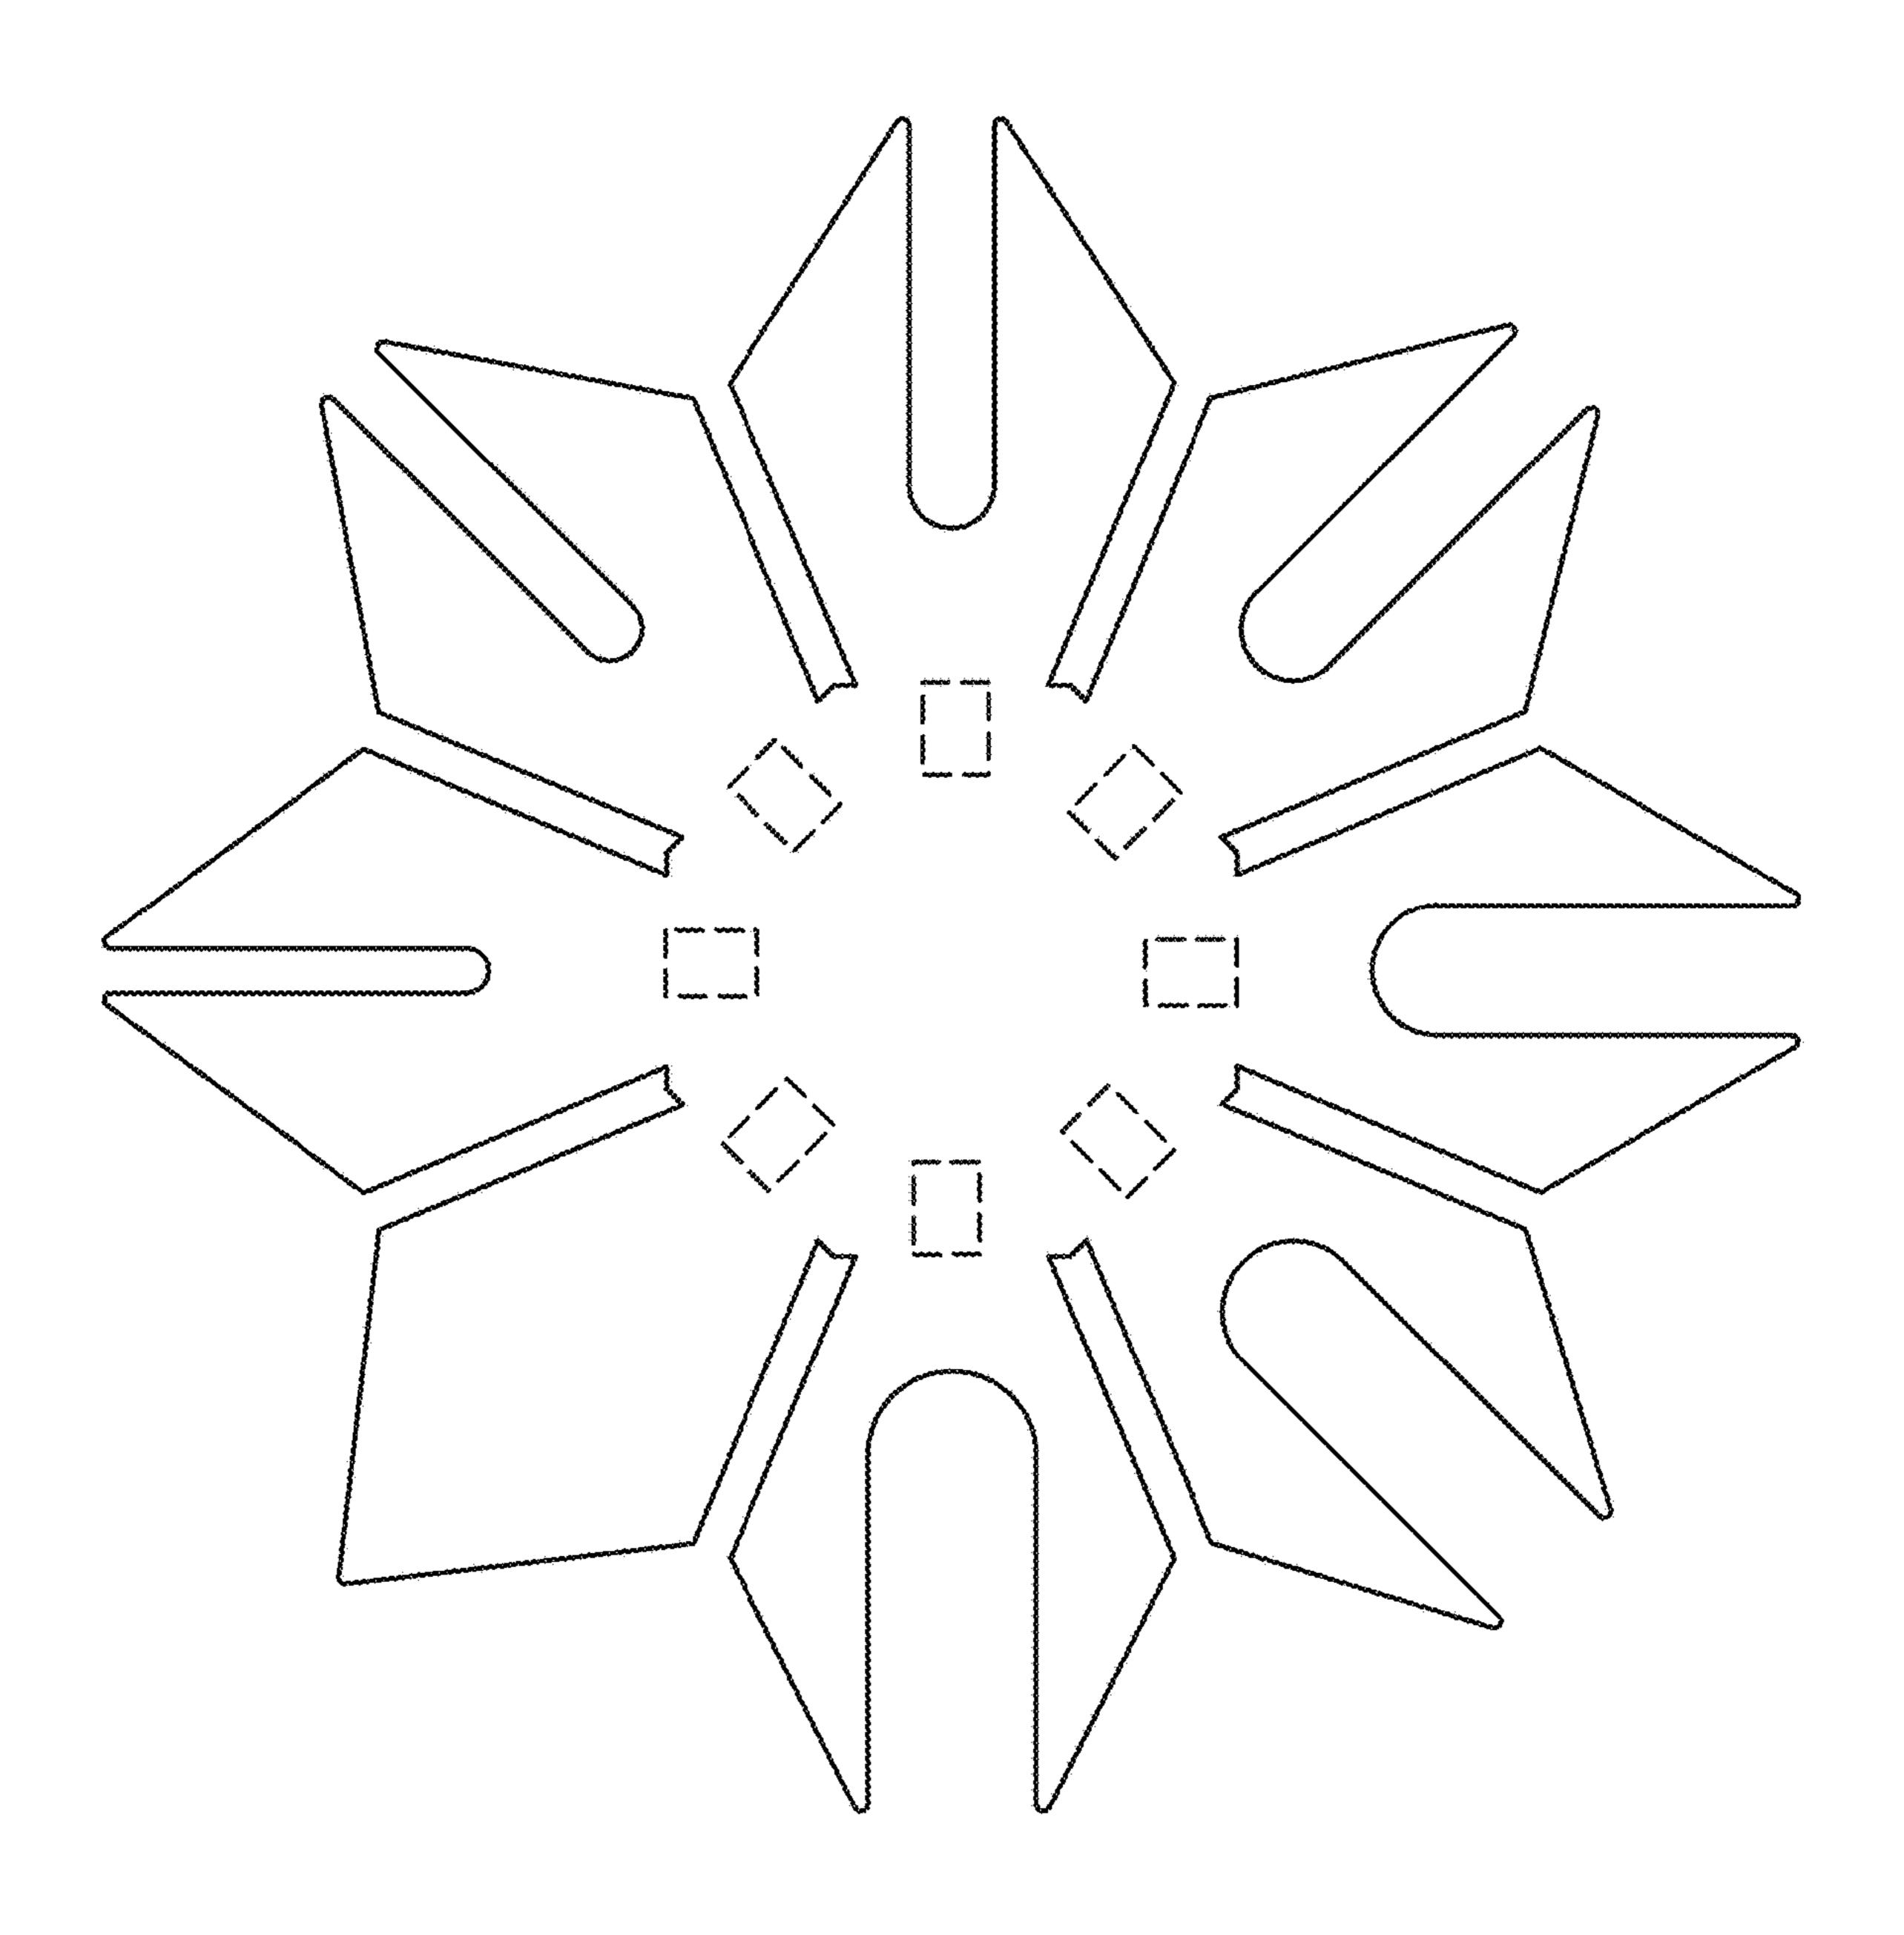


FIG. 24

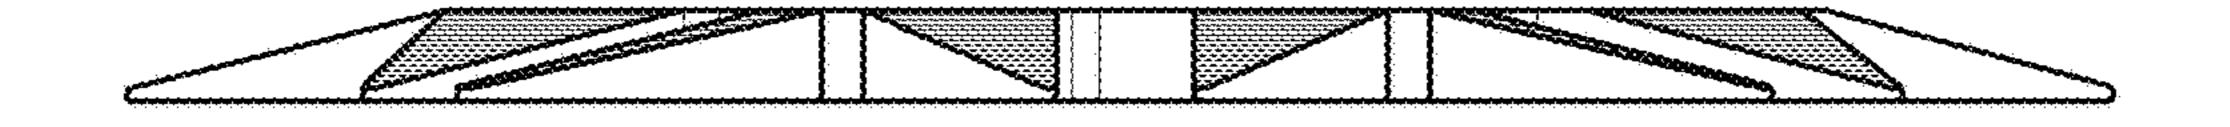


FIG. 25

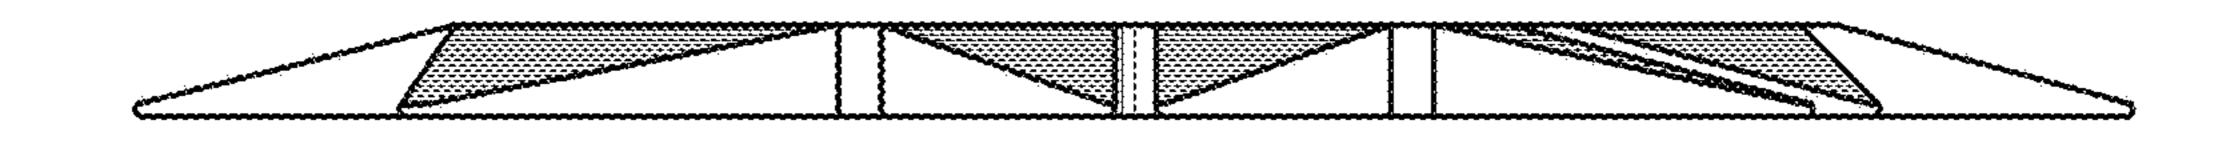


FIG. 26

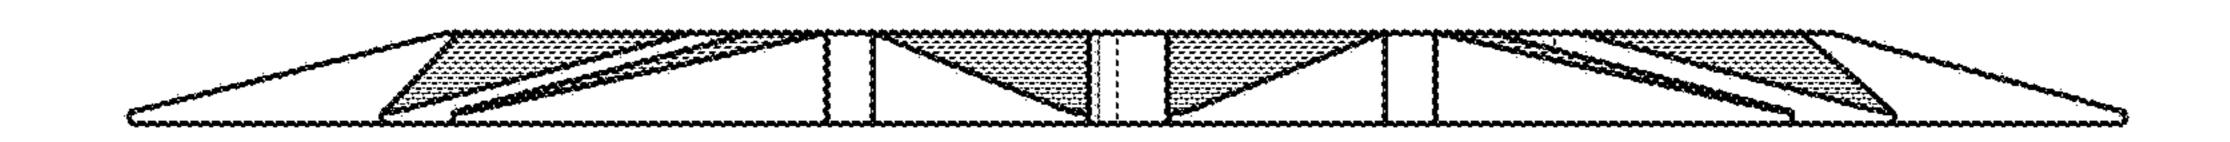


FIG. 27

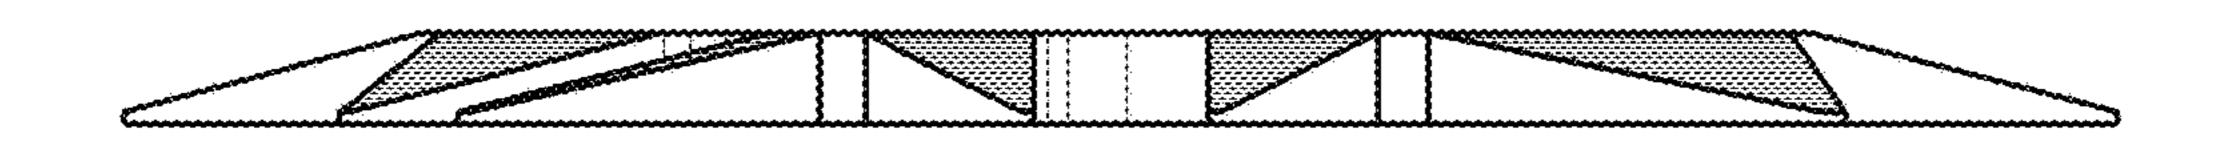


FIG. 28