



US00D840541S

(12) **United States Design Patent**
Yanagihara

(10) **Patent No.:** **US D840,541 S**

(45) **Date of Patent:** **** Feb. 12, 2019**

(54) **ULTRASONIC DIAGNOSIS APPARATUS**

(71) Applicant: **General Electric Company,**
Schenectady, NY (US)

(72) Inventor: **Koji Yanagihara,** Tokyo (JP)

(73) Assignee: **General Electric Company,**
Schenectady, NY (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/573,686**

(22) Filed: **Aug. 9, 2016**

(30) **Foreign Application Priority Data**

Mar. 17, 2016 (JP) 2016-005899

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/160**

(58) **Field of Classification Search**
USPC D24/107, 133, 137, 138, 141, 158-161,
D24/164, 165, 167, 170, 185-187;
D10/57, 60, 78, 80; 600/407, 439, 446,
600/459, 461; 378/98.7, 98.8, 189
CPC ... A61B 8/0437; A61B 8/0883; A61B 8/4405;
A61B 8/4411; A61B 8/4427; A61B
8/445; A61B 8/4455; A61B 8/4461; A61B
8/4483; A61B 8/46; A61B 8/462; A61B
5/0095

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D630,752 S * 1/2011 Suzuki D24/158
D662,208 S * 6/2012 Otoha D24/185
D707,359 S * 6/2014 Kim D24/185
D711,539 S * 8/2014 Hunt D24/158
D713,035 S * 9/2014 Kim D24/158

D716,949 S * 11/2014 Baba D24/160
D727,504 S * 4/2015 Ninomiya D24/158
9,055,910 B2 * 6/2015 Nakajima A61B 8/4405
2008/0009728 A1 * 1/2008 Malchow A61B 8/0833
600/437
2009/0156935 A1 * 6/2009 Frisa A61B 8/14
600/447
2011/0201927 A1 * 8/2011 Hayakawa A61B 8/4405
600/437
2016/0270764 A1 * 9/2016 Wodecki A61B 8/462

* cited by examiner

Primary Examiner — Anhdao Doan

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — McCoy Russell LLP

(57) **CLAIM**

The ornamental design for an ultrasonic diagnosis apparatus,
as shown and described.

DESCRIPTION

FIG. 1 is a front view of a design for an ultrasonic diagnosis
apparatus, as shown and described.

FIG. 2 is a back view of the ultrasonic diagnosis apparatus
of FIG. 1.

FIG. 3 is a right side view of the ultrasonic diagnosis
apparatus of FIG. 1.

FIG. 4 is a left side view of the ultrasonic diagnosis
apparatus of FIG. 1.

FIG. 5 is a top view of the ultrasonic diagnosis apparatus of
FIG. 1.


FIG. 6 is a bottom view of the ultrasonic diagnosis apparatus
of FIG. 1.

FIG. 7 is a front perspective view of the ultrasonic diagnosis
apparatus of FIG. 1; and,

FIG. 8 is a back perspective view of a design for the
ultrasonic diagnosis apparatus of FIG. 1.

The broken lines show portions of the ultrasonic diagnosis
apparatus that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

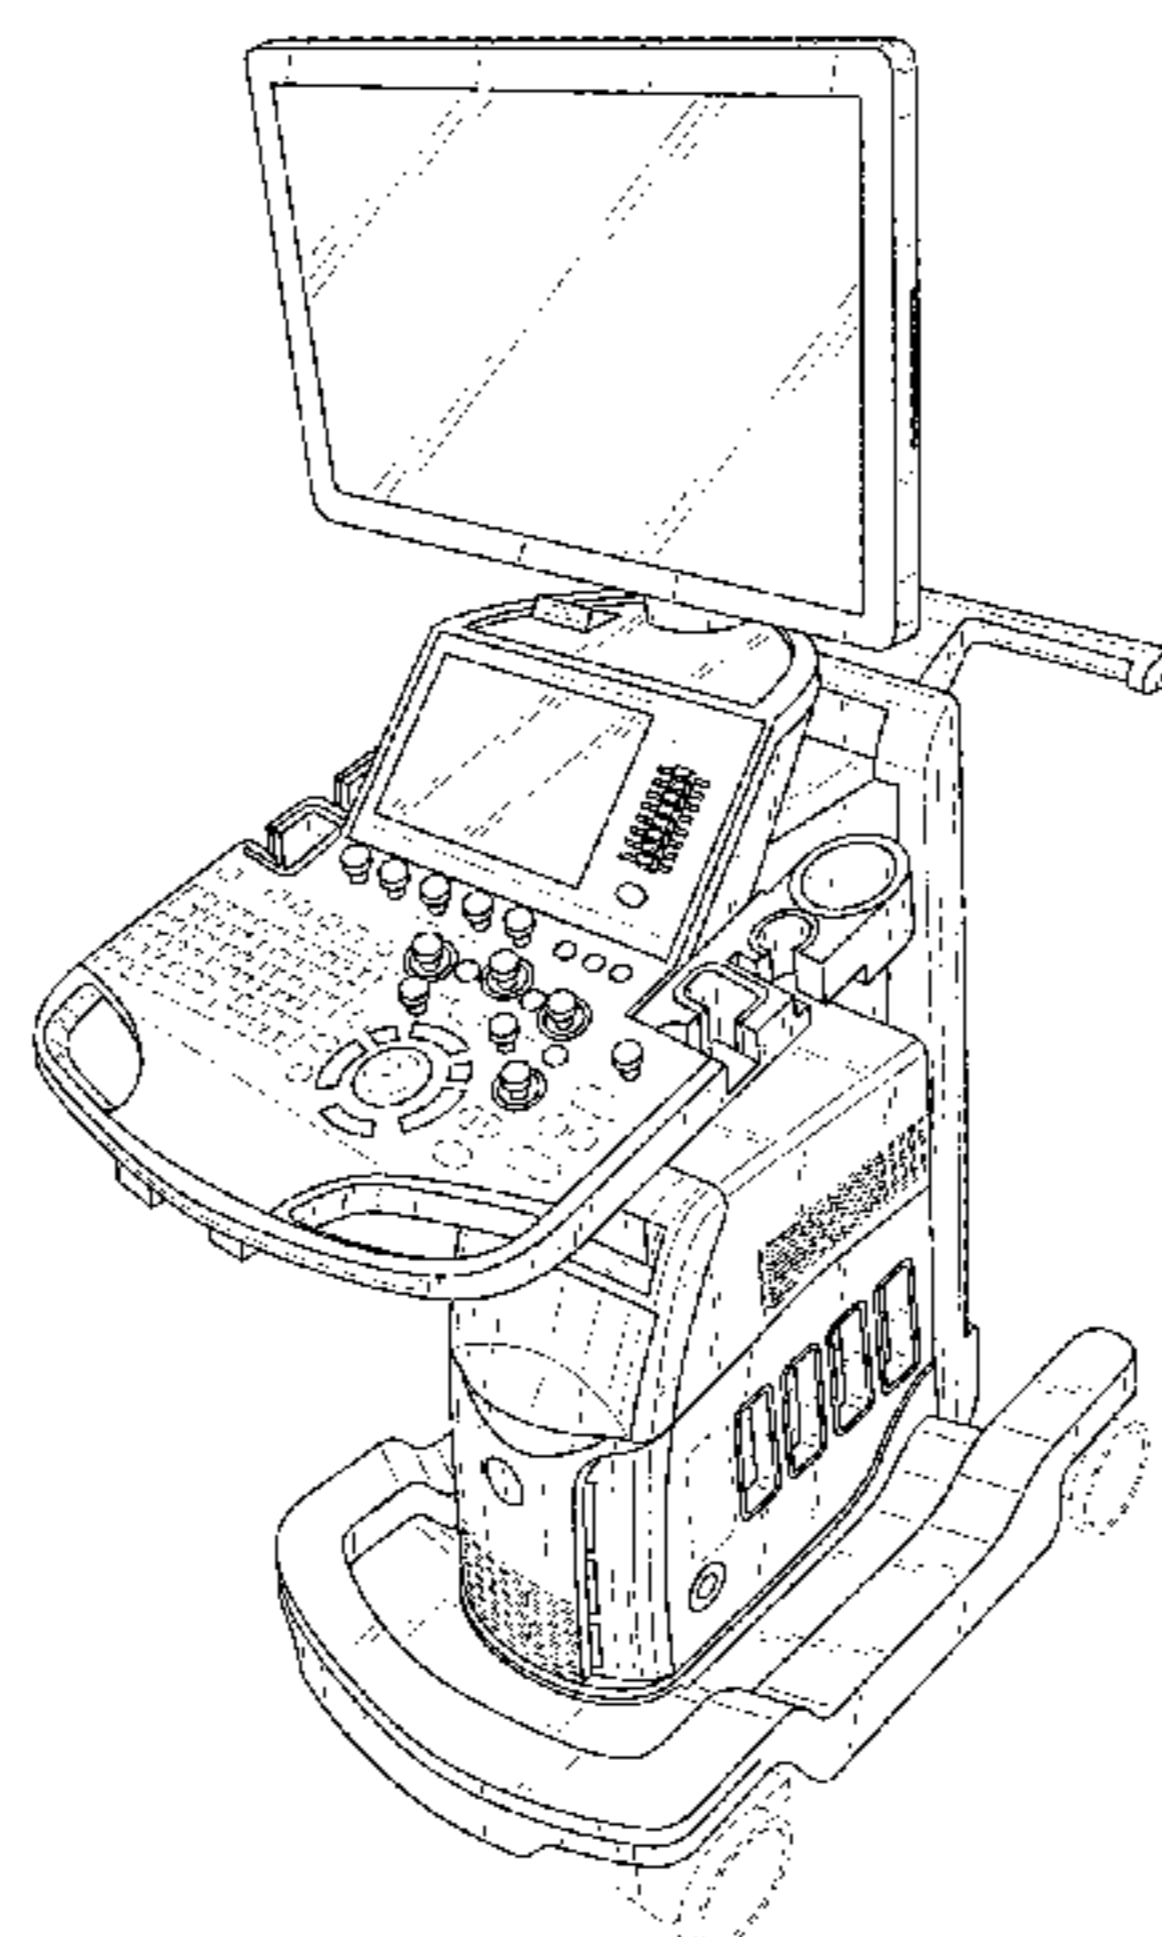

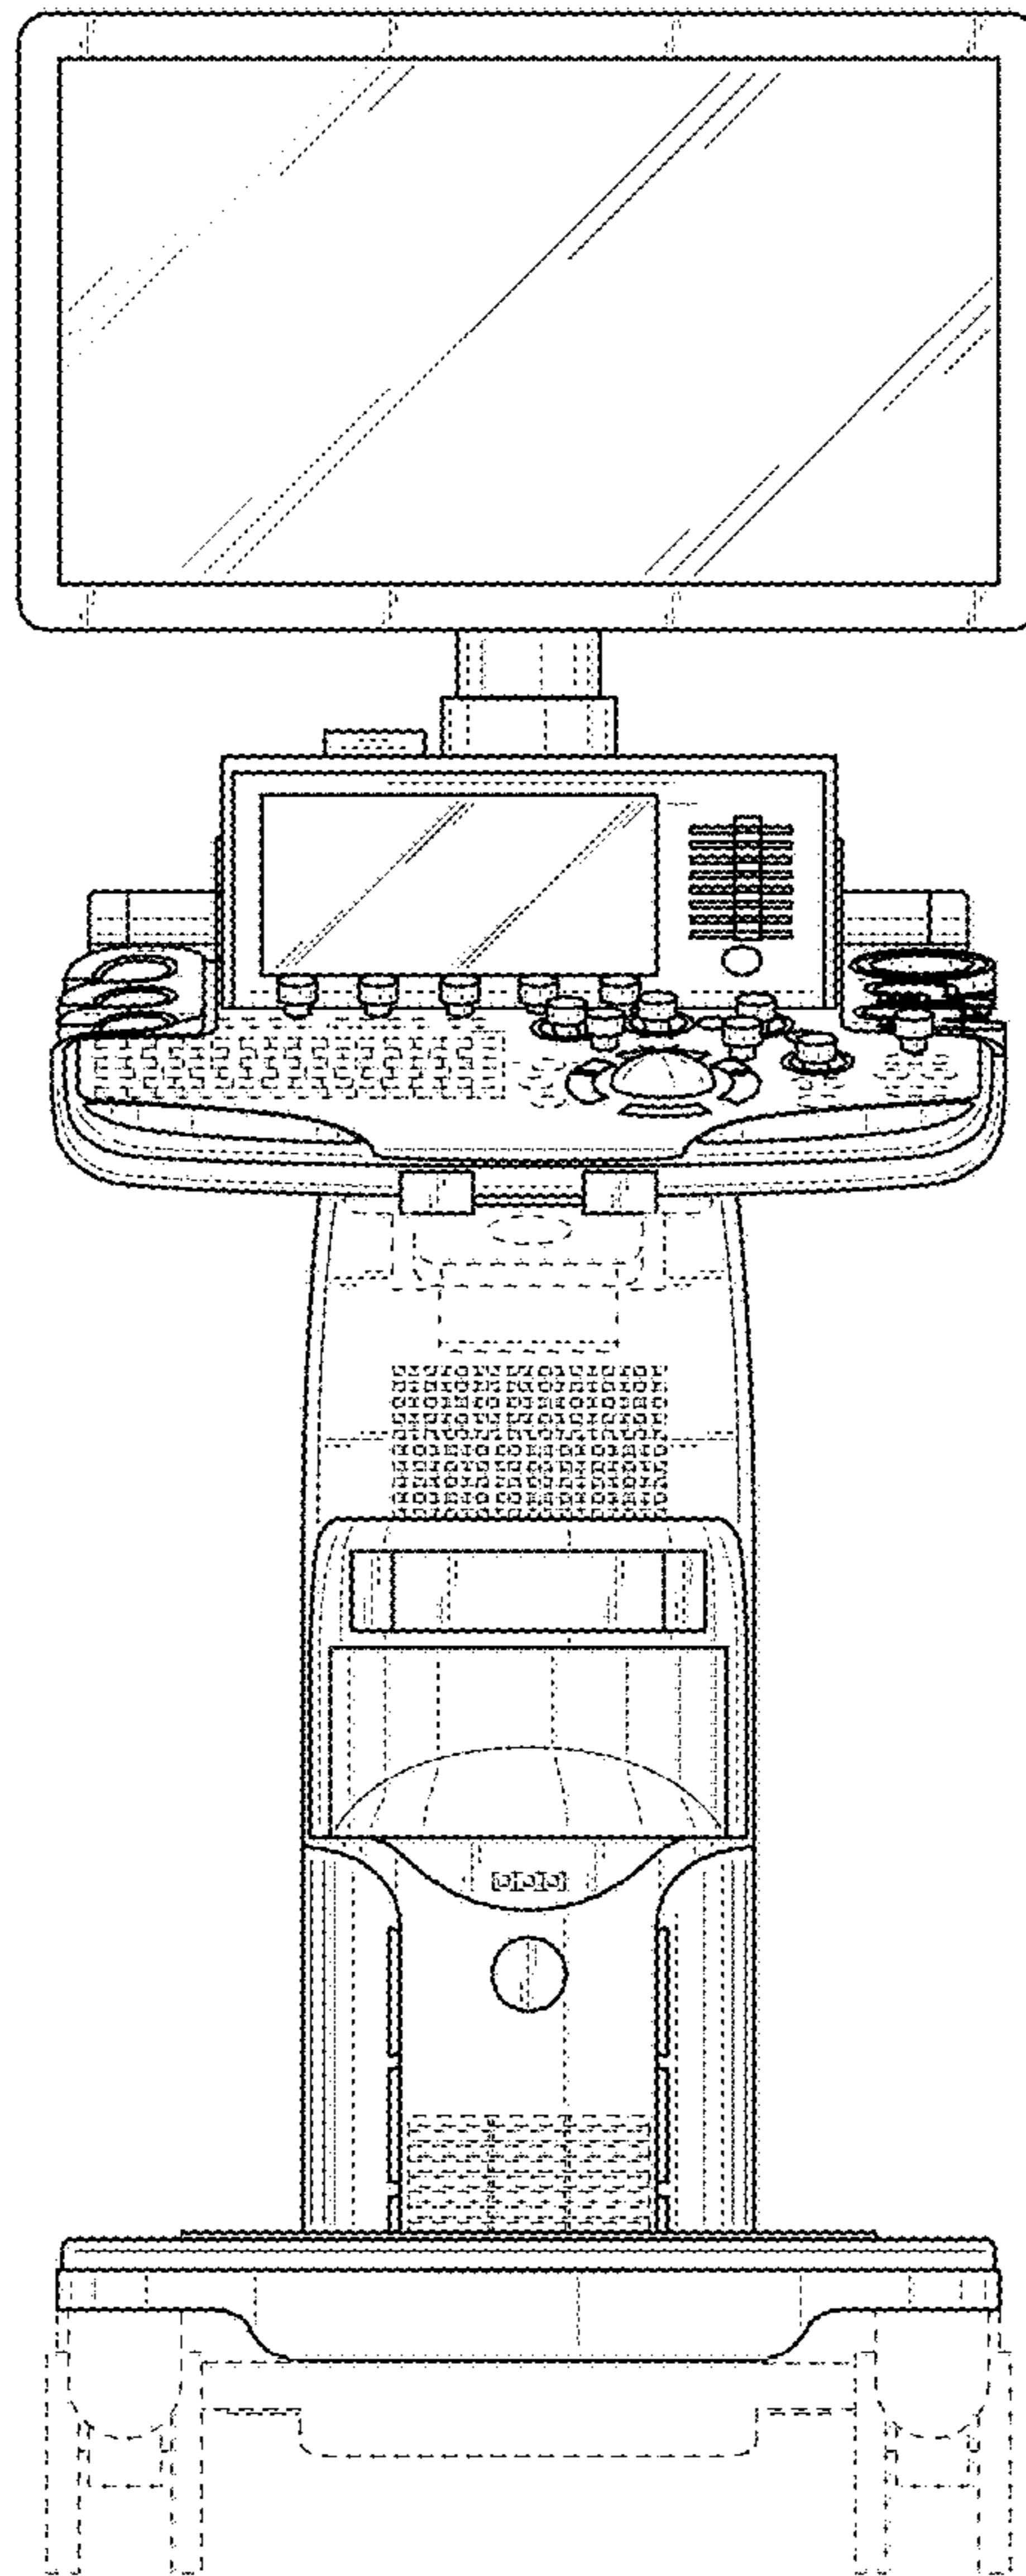


FIG. 1

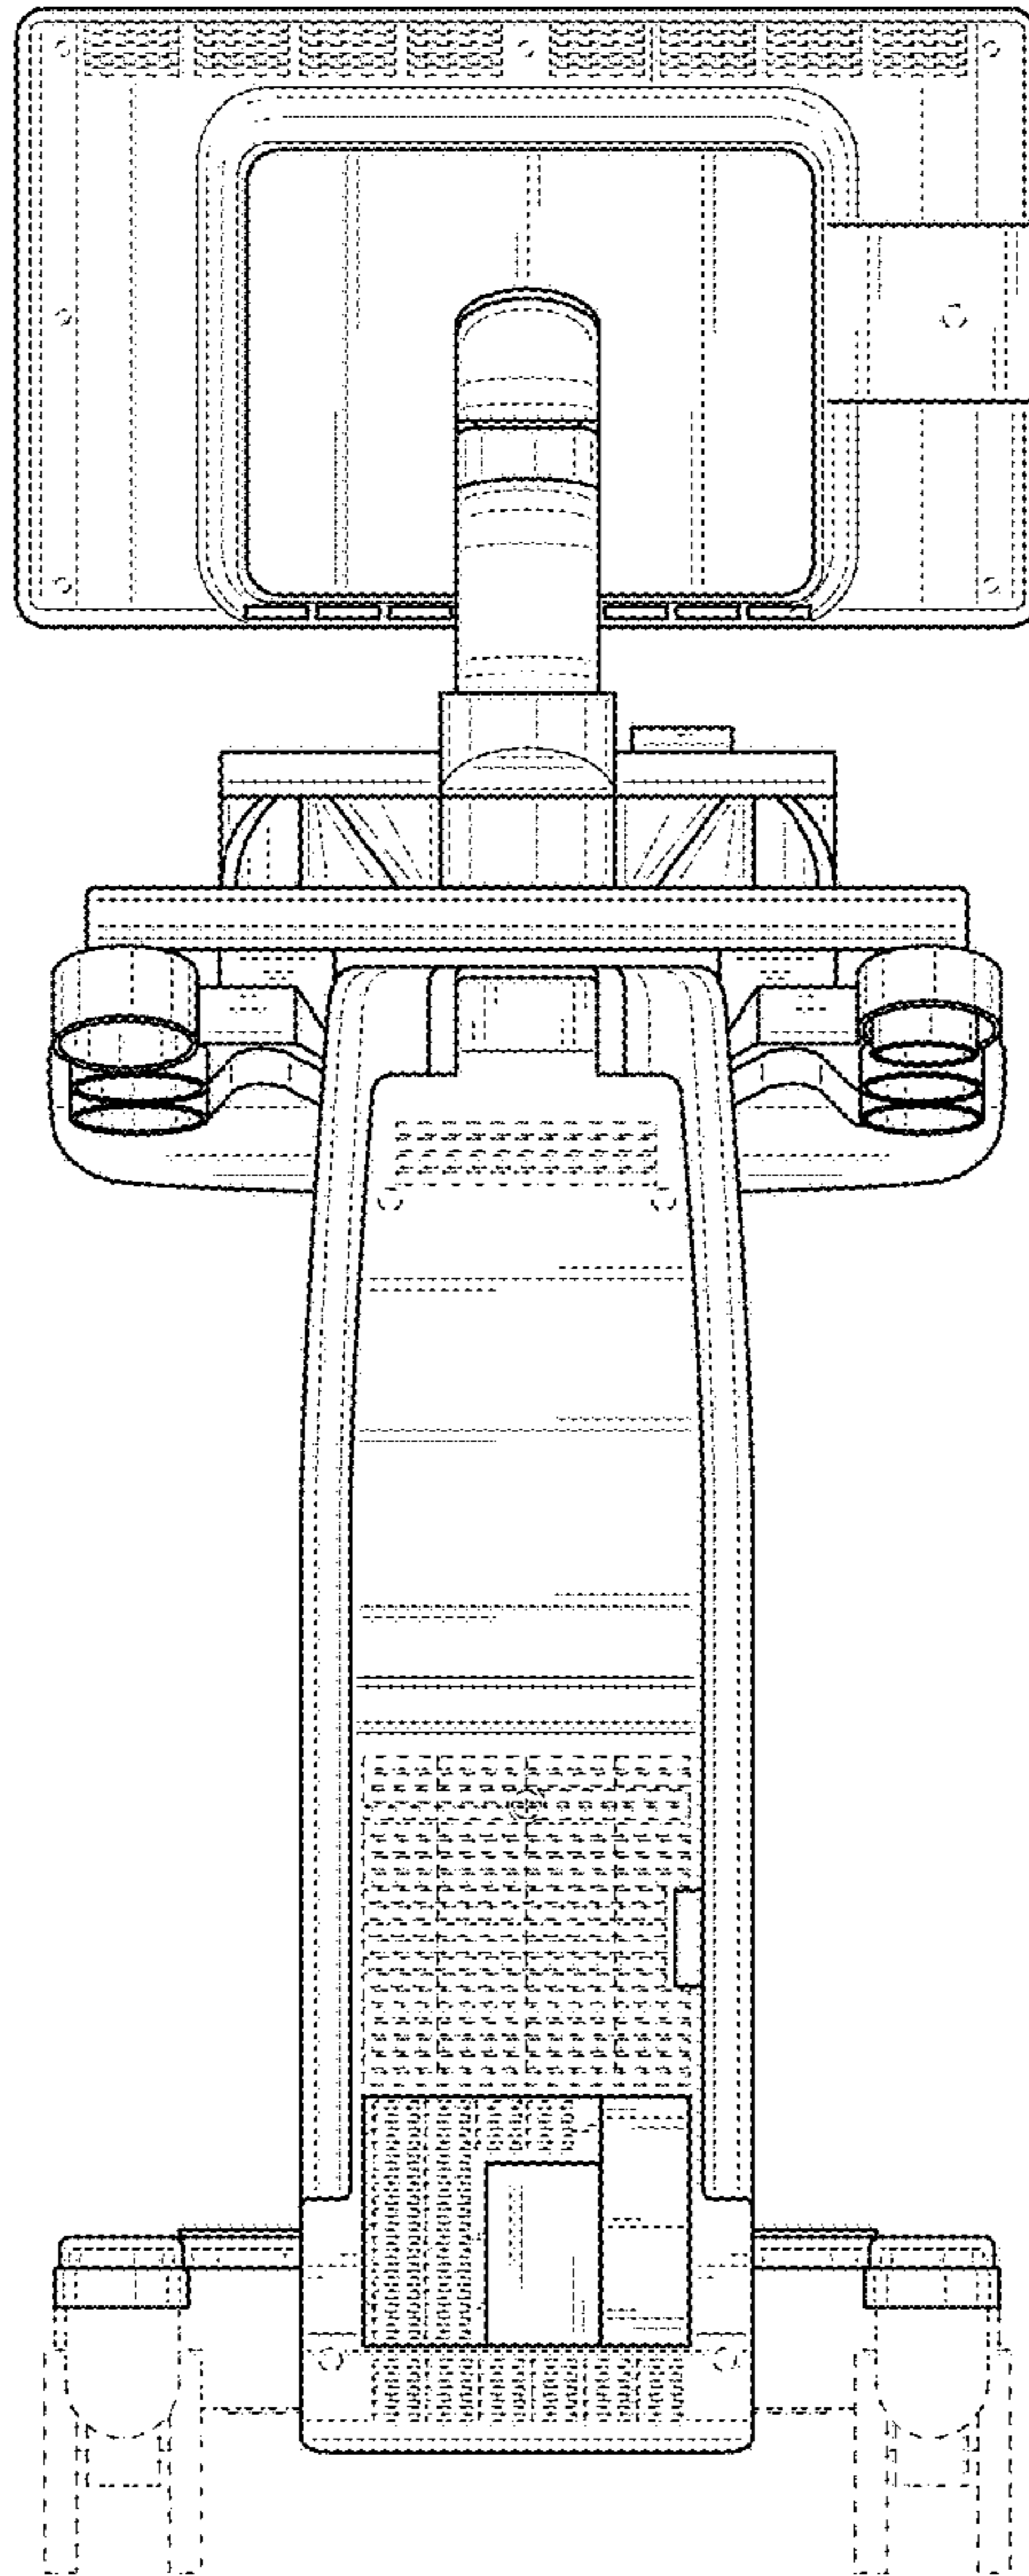


FIG. 2

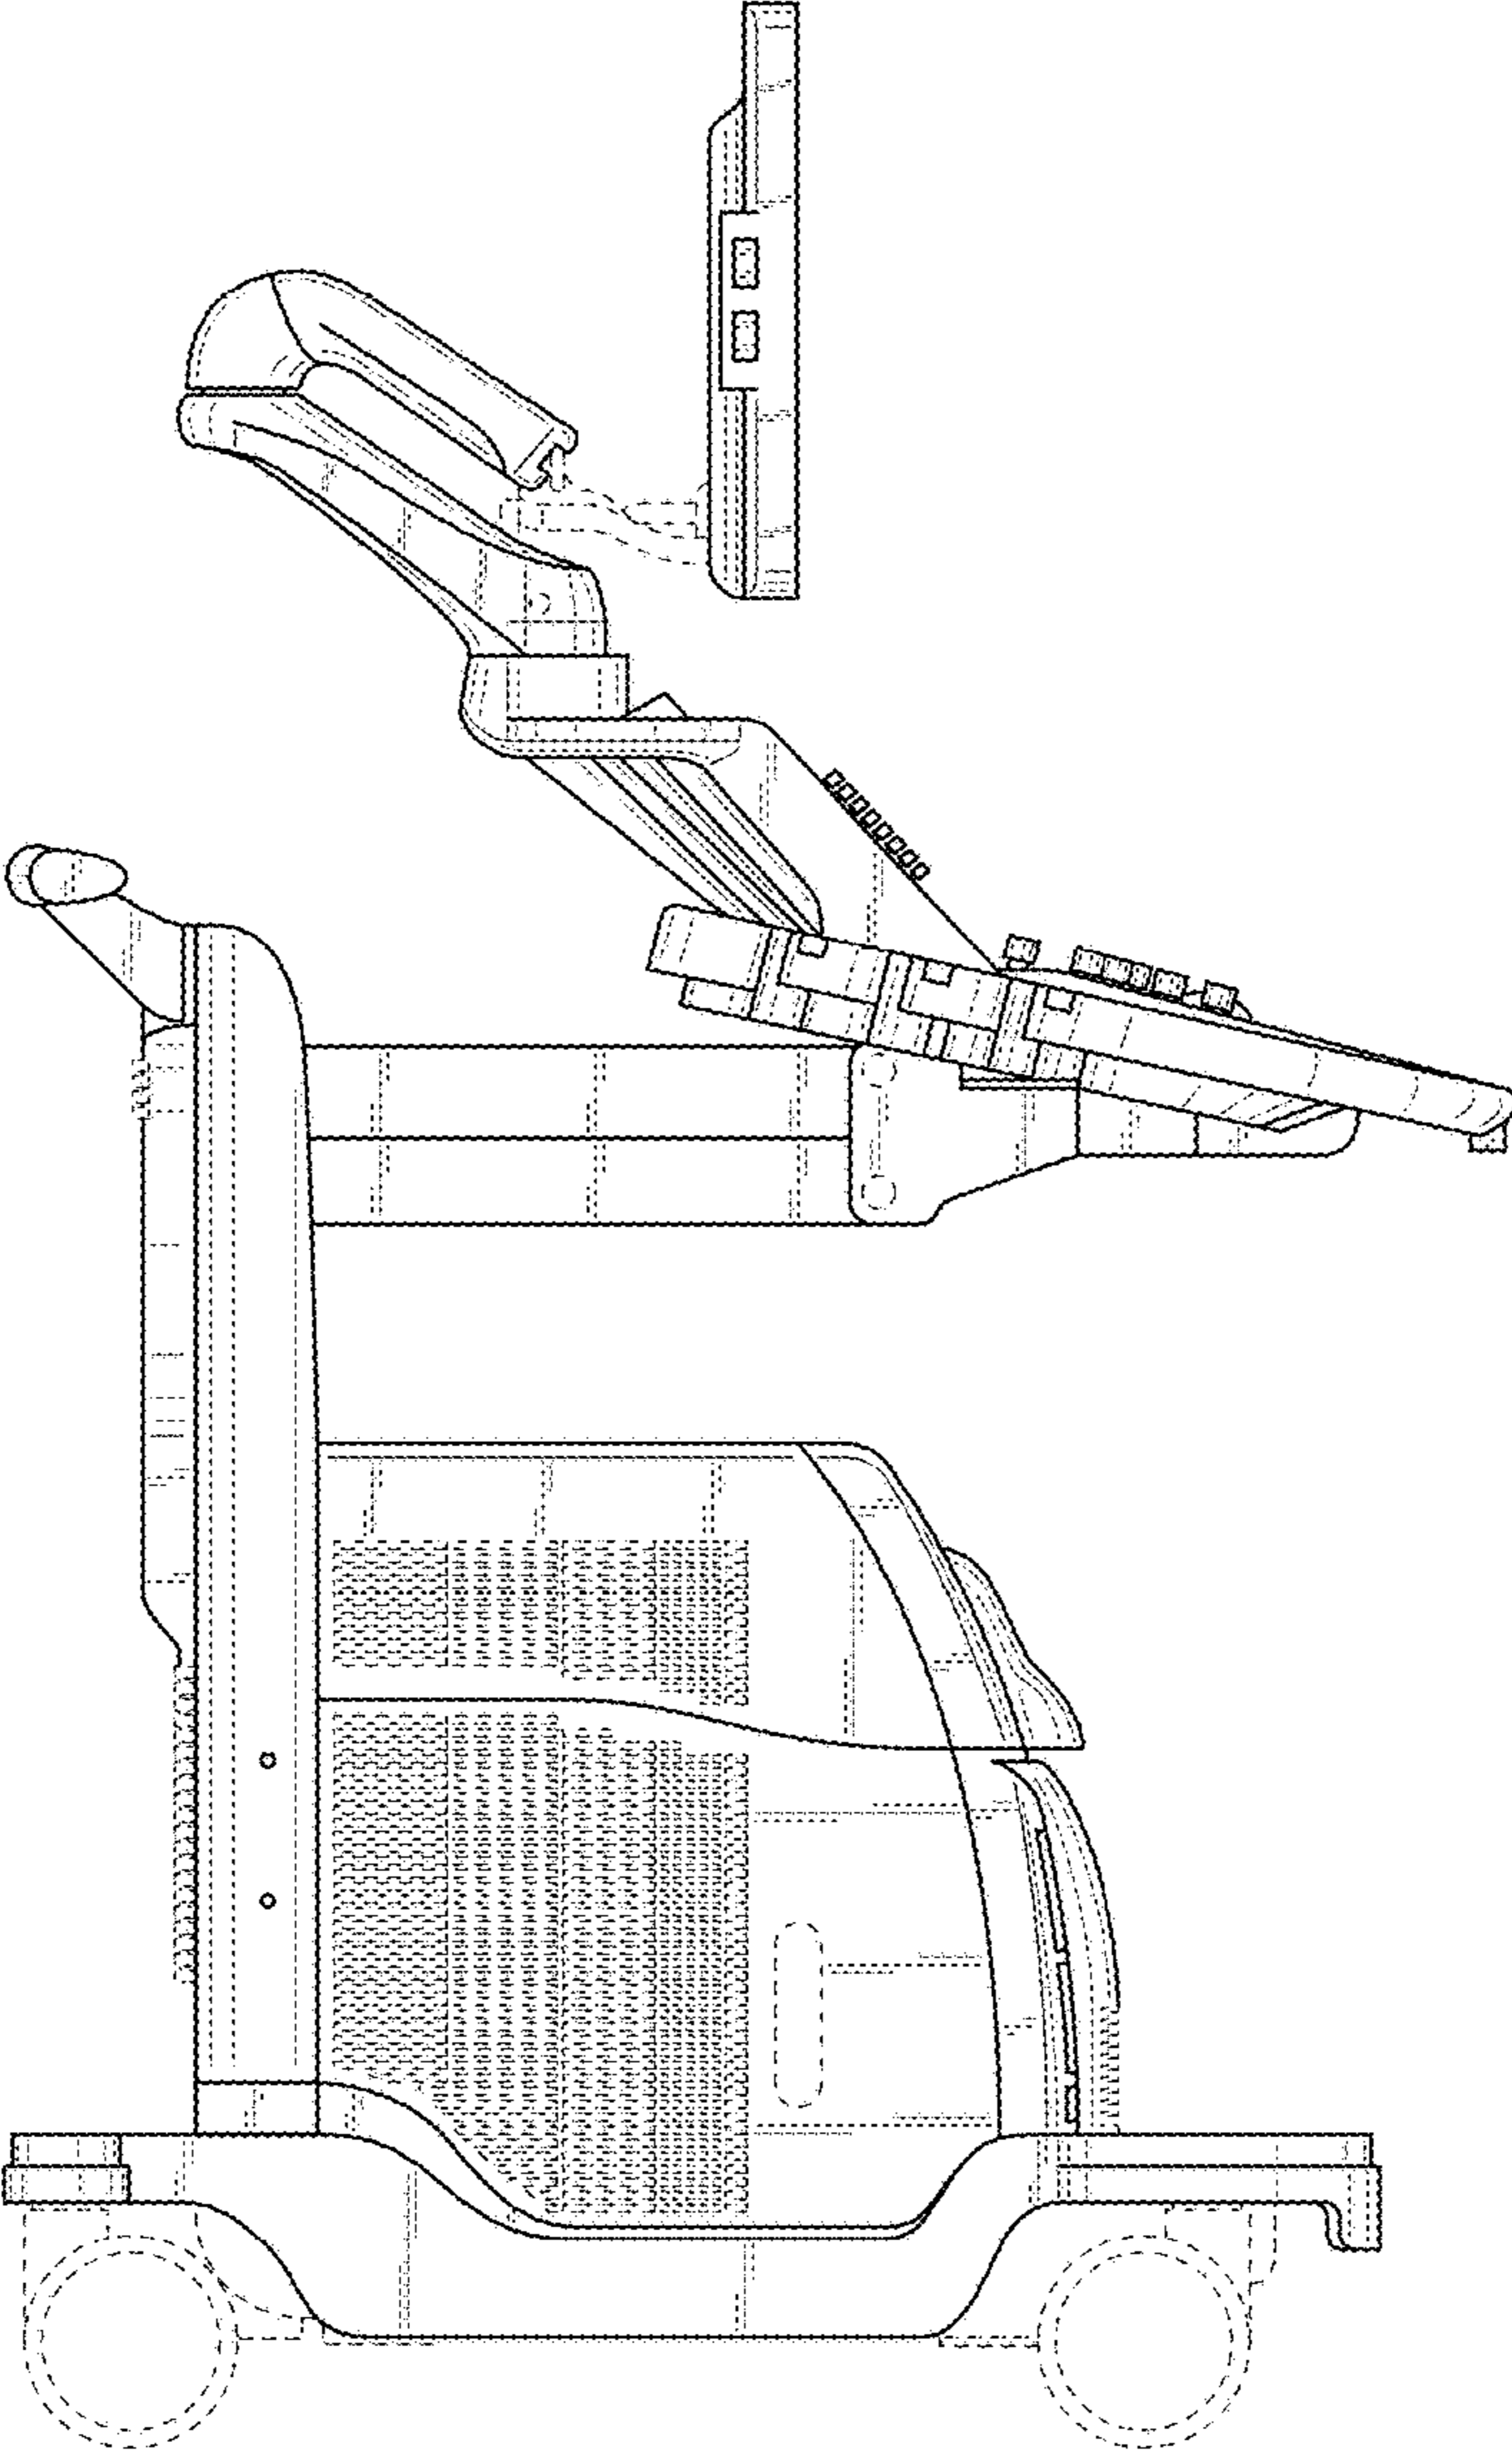


FIG. 3

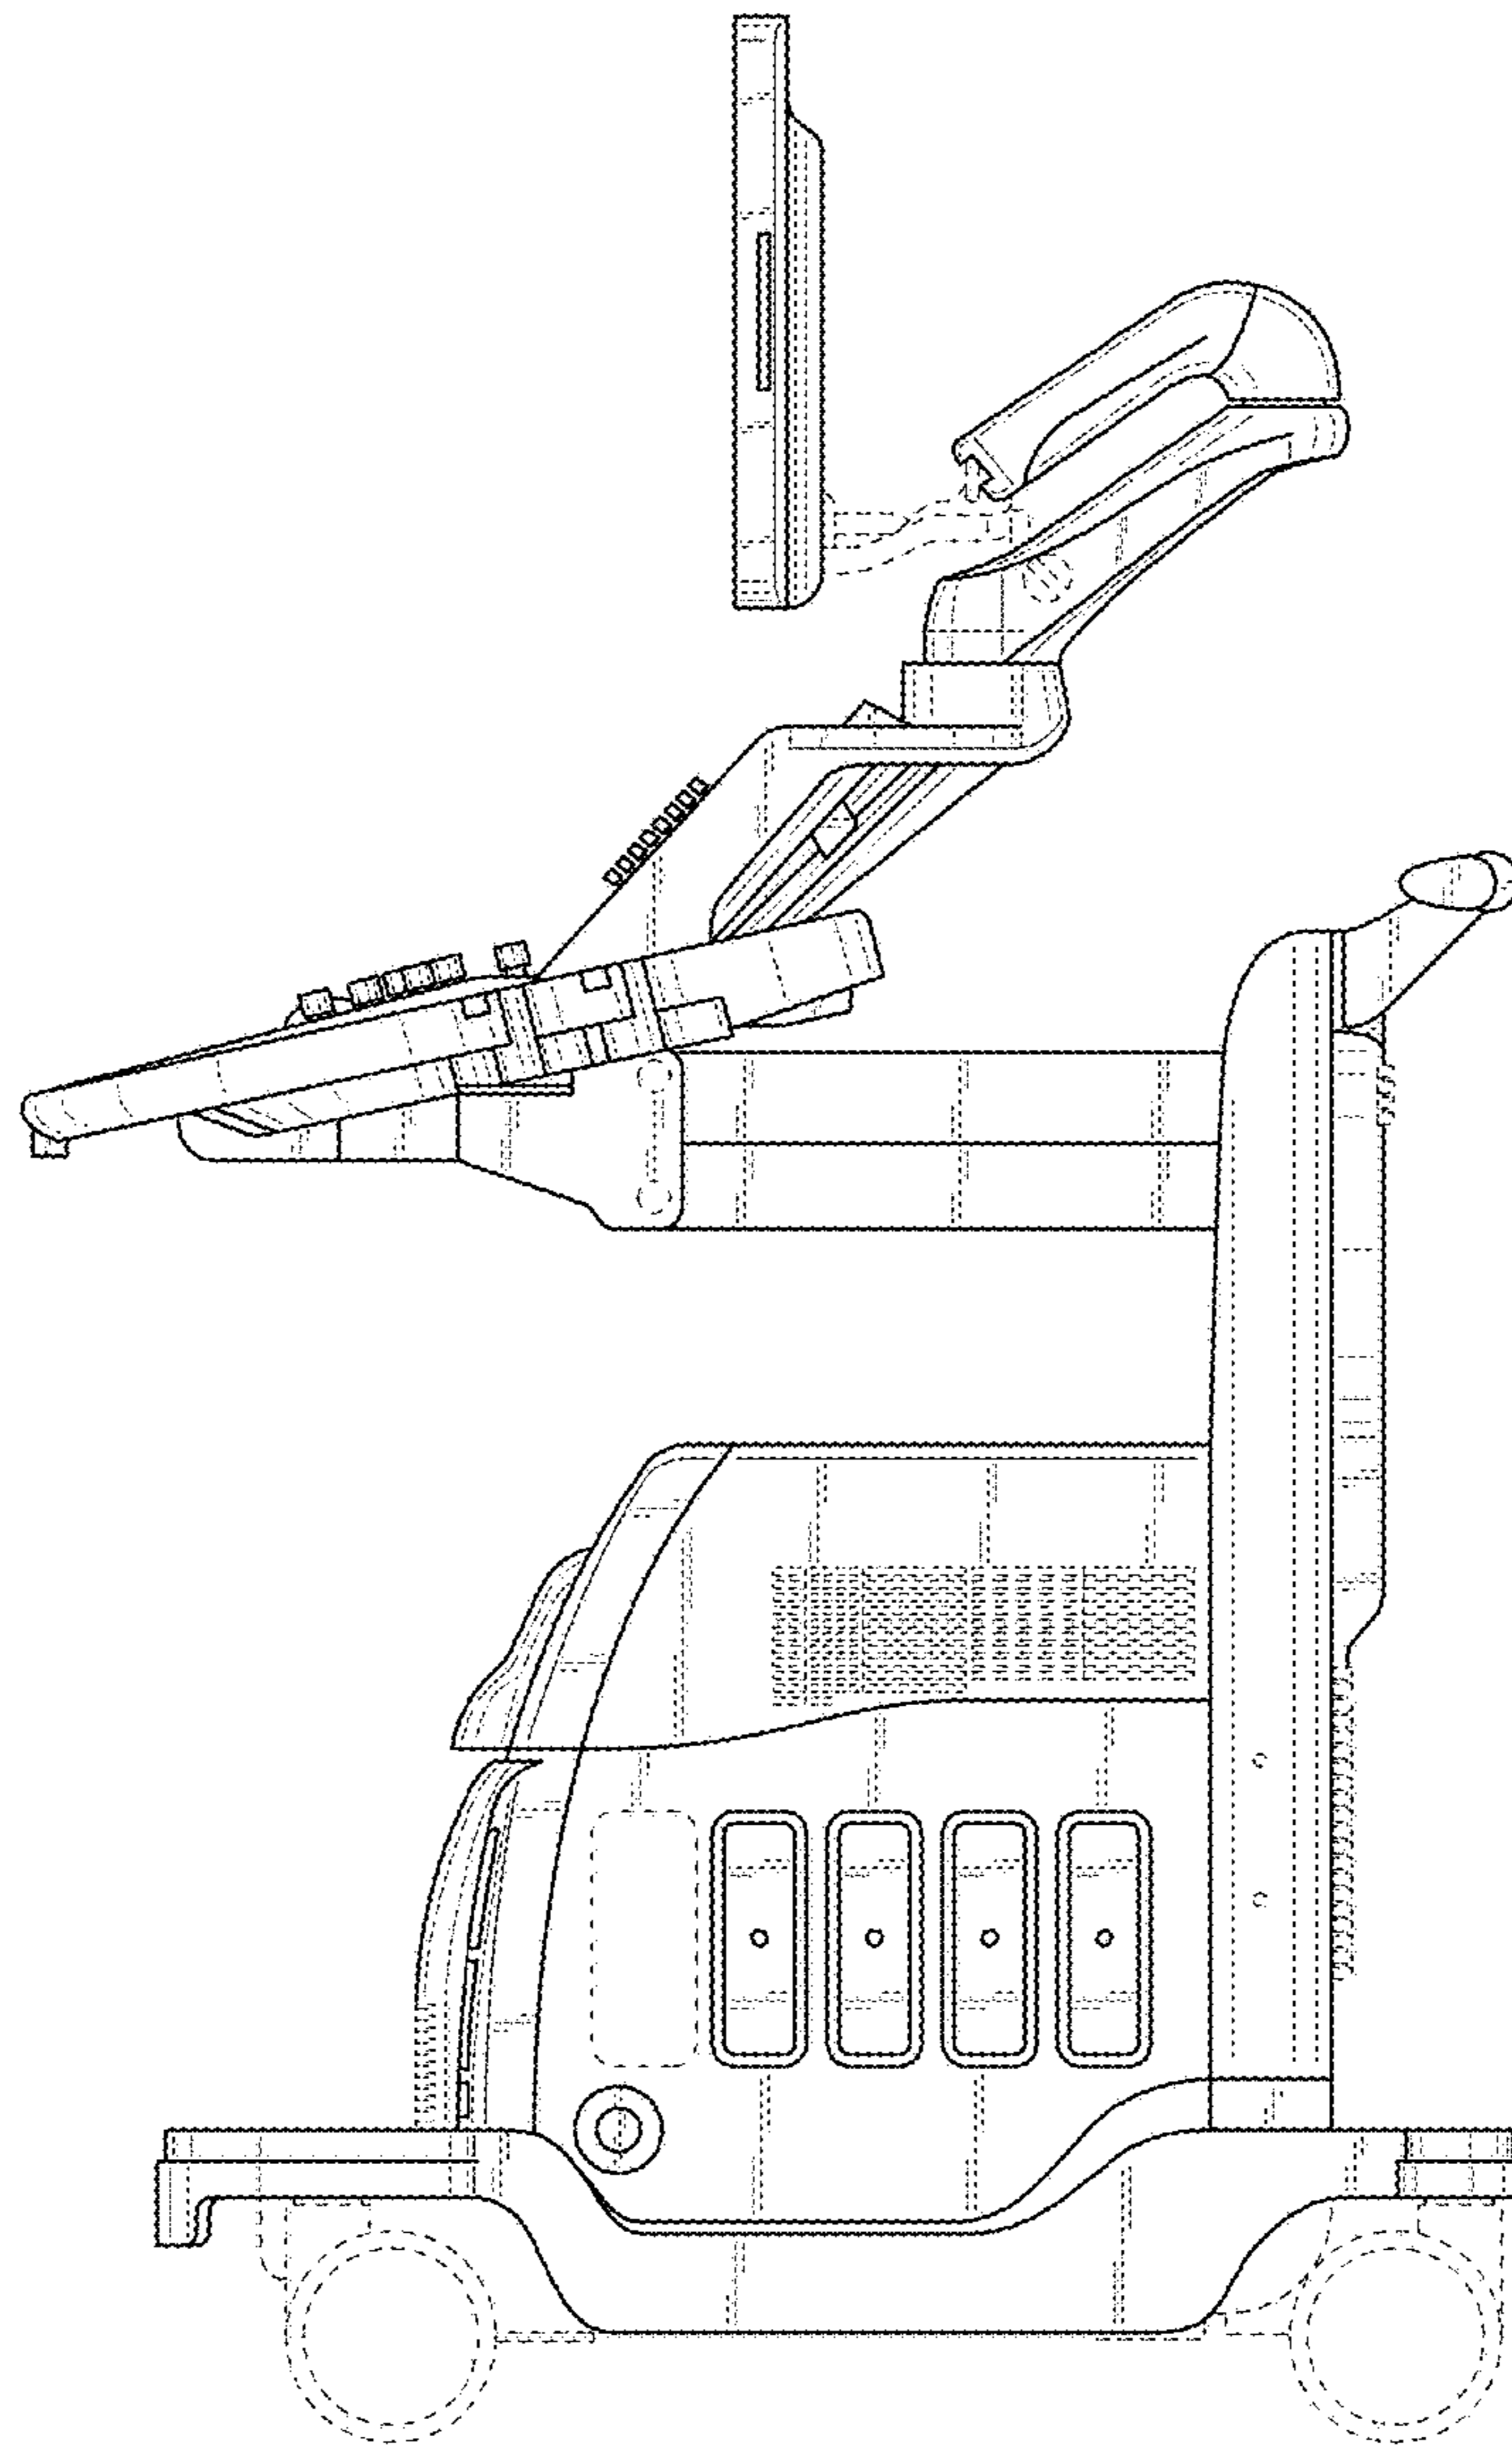


FIG. 4

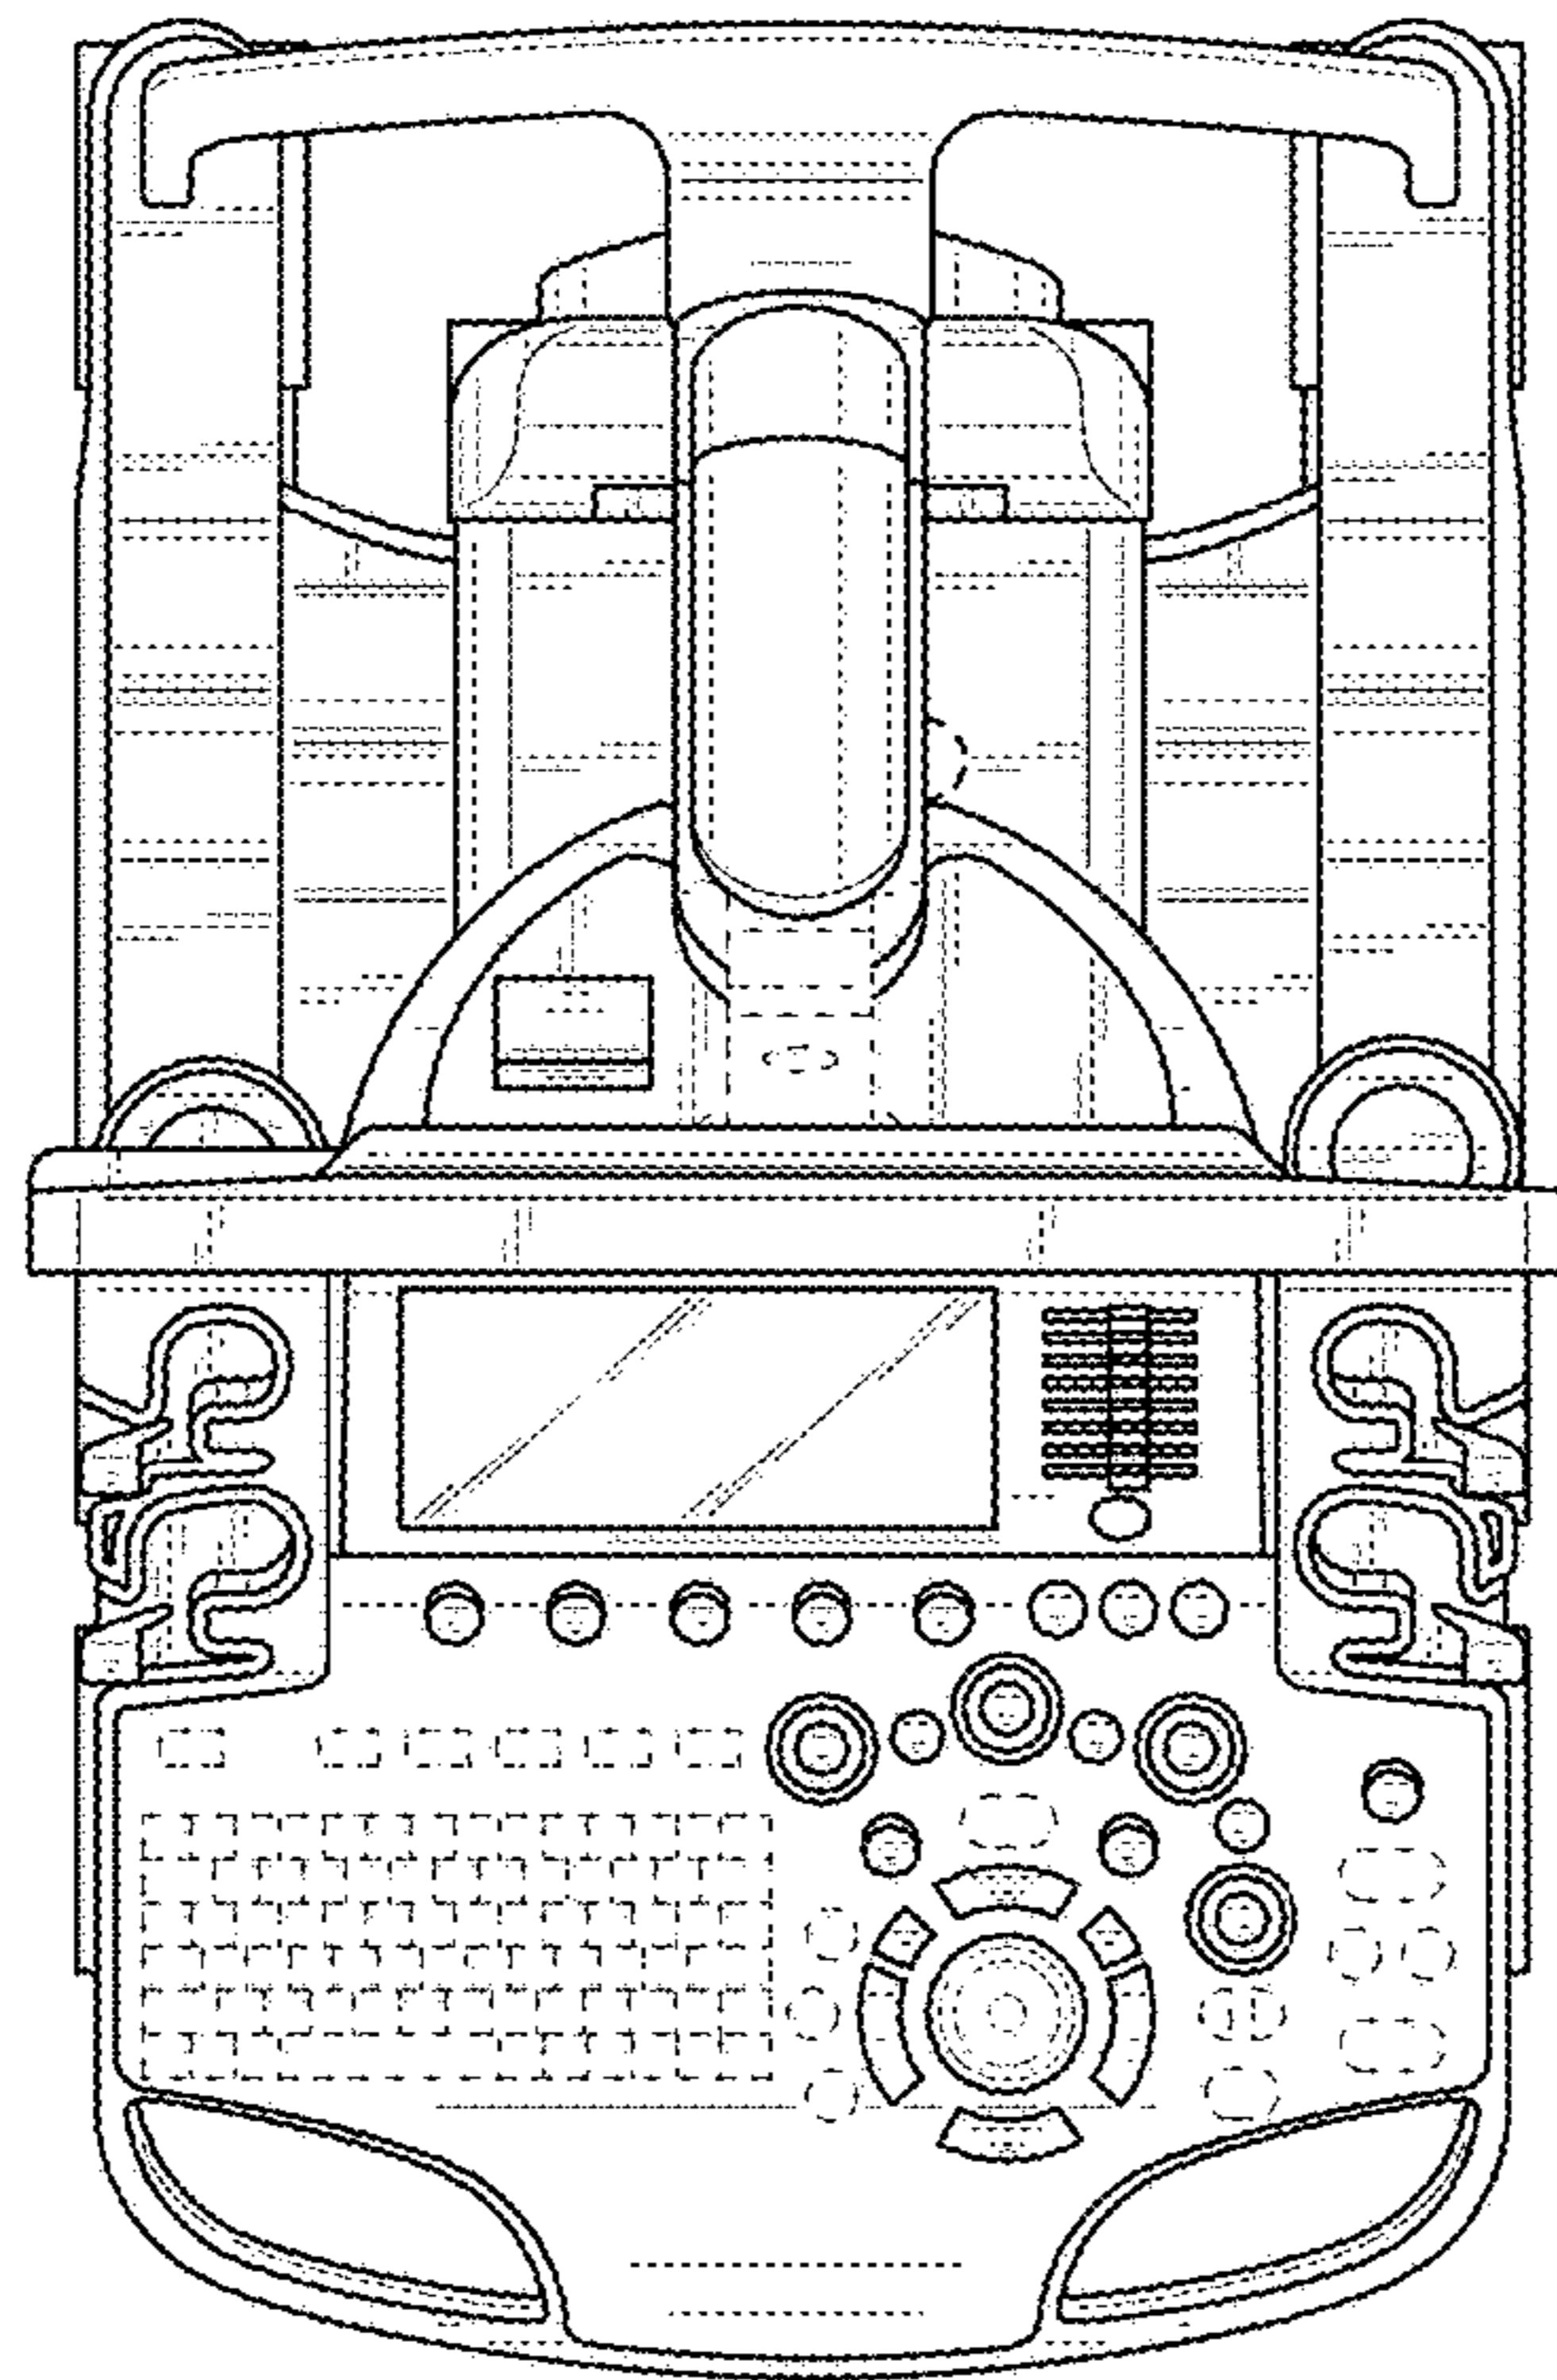


FIG. 5

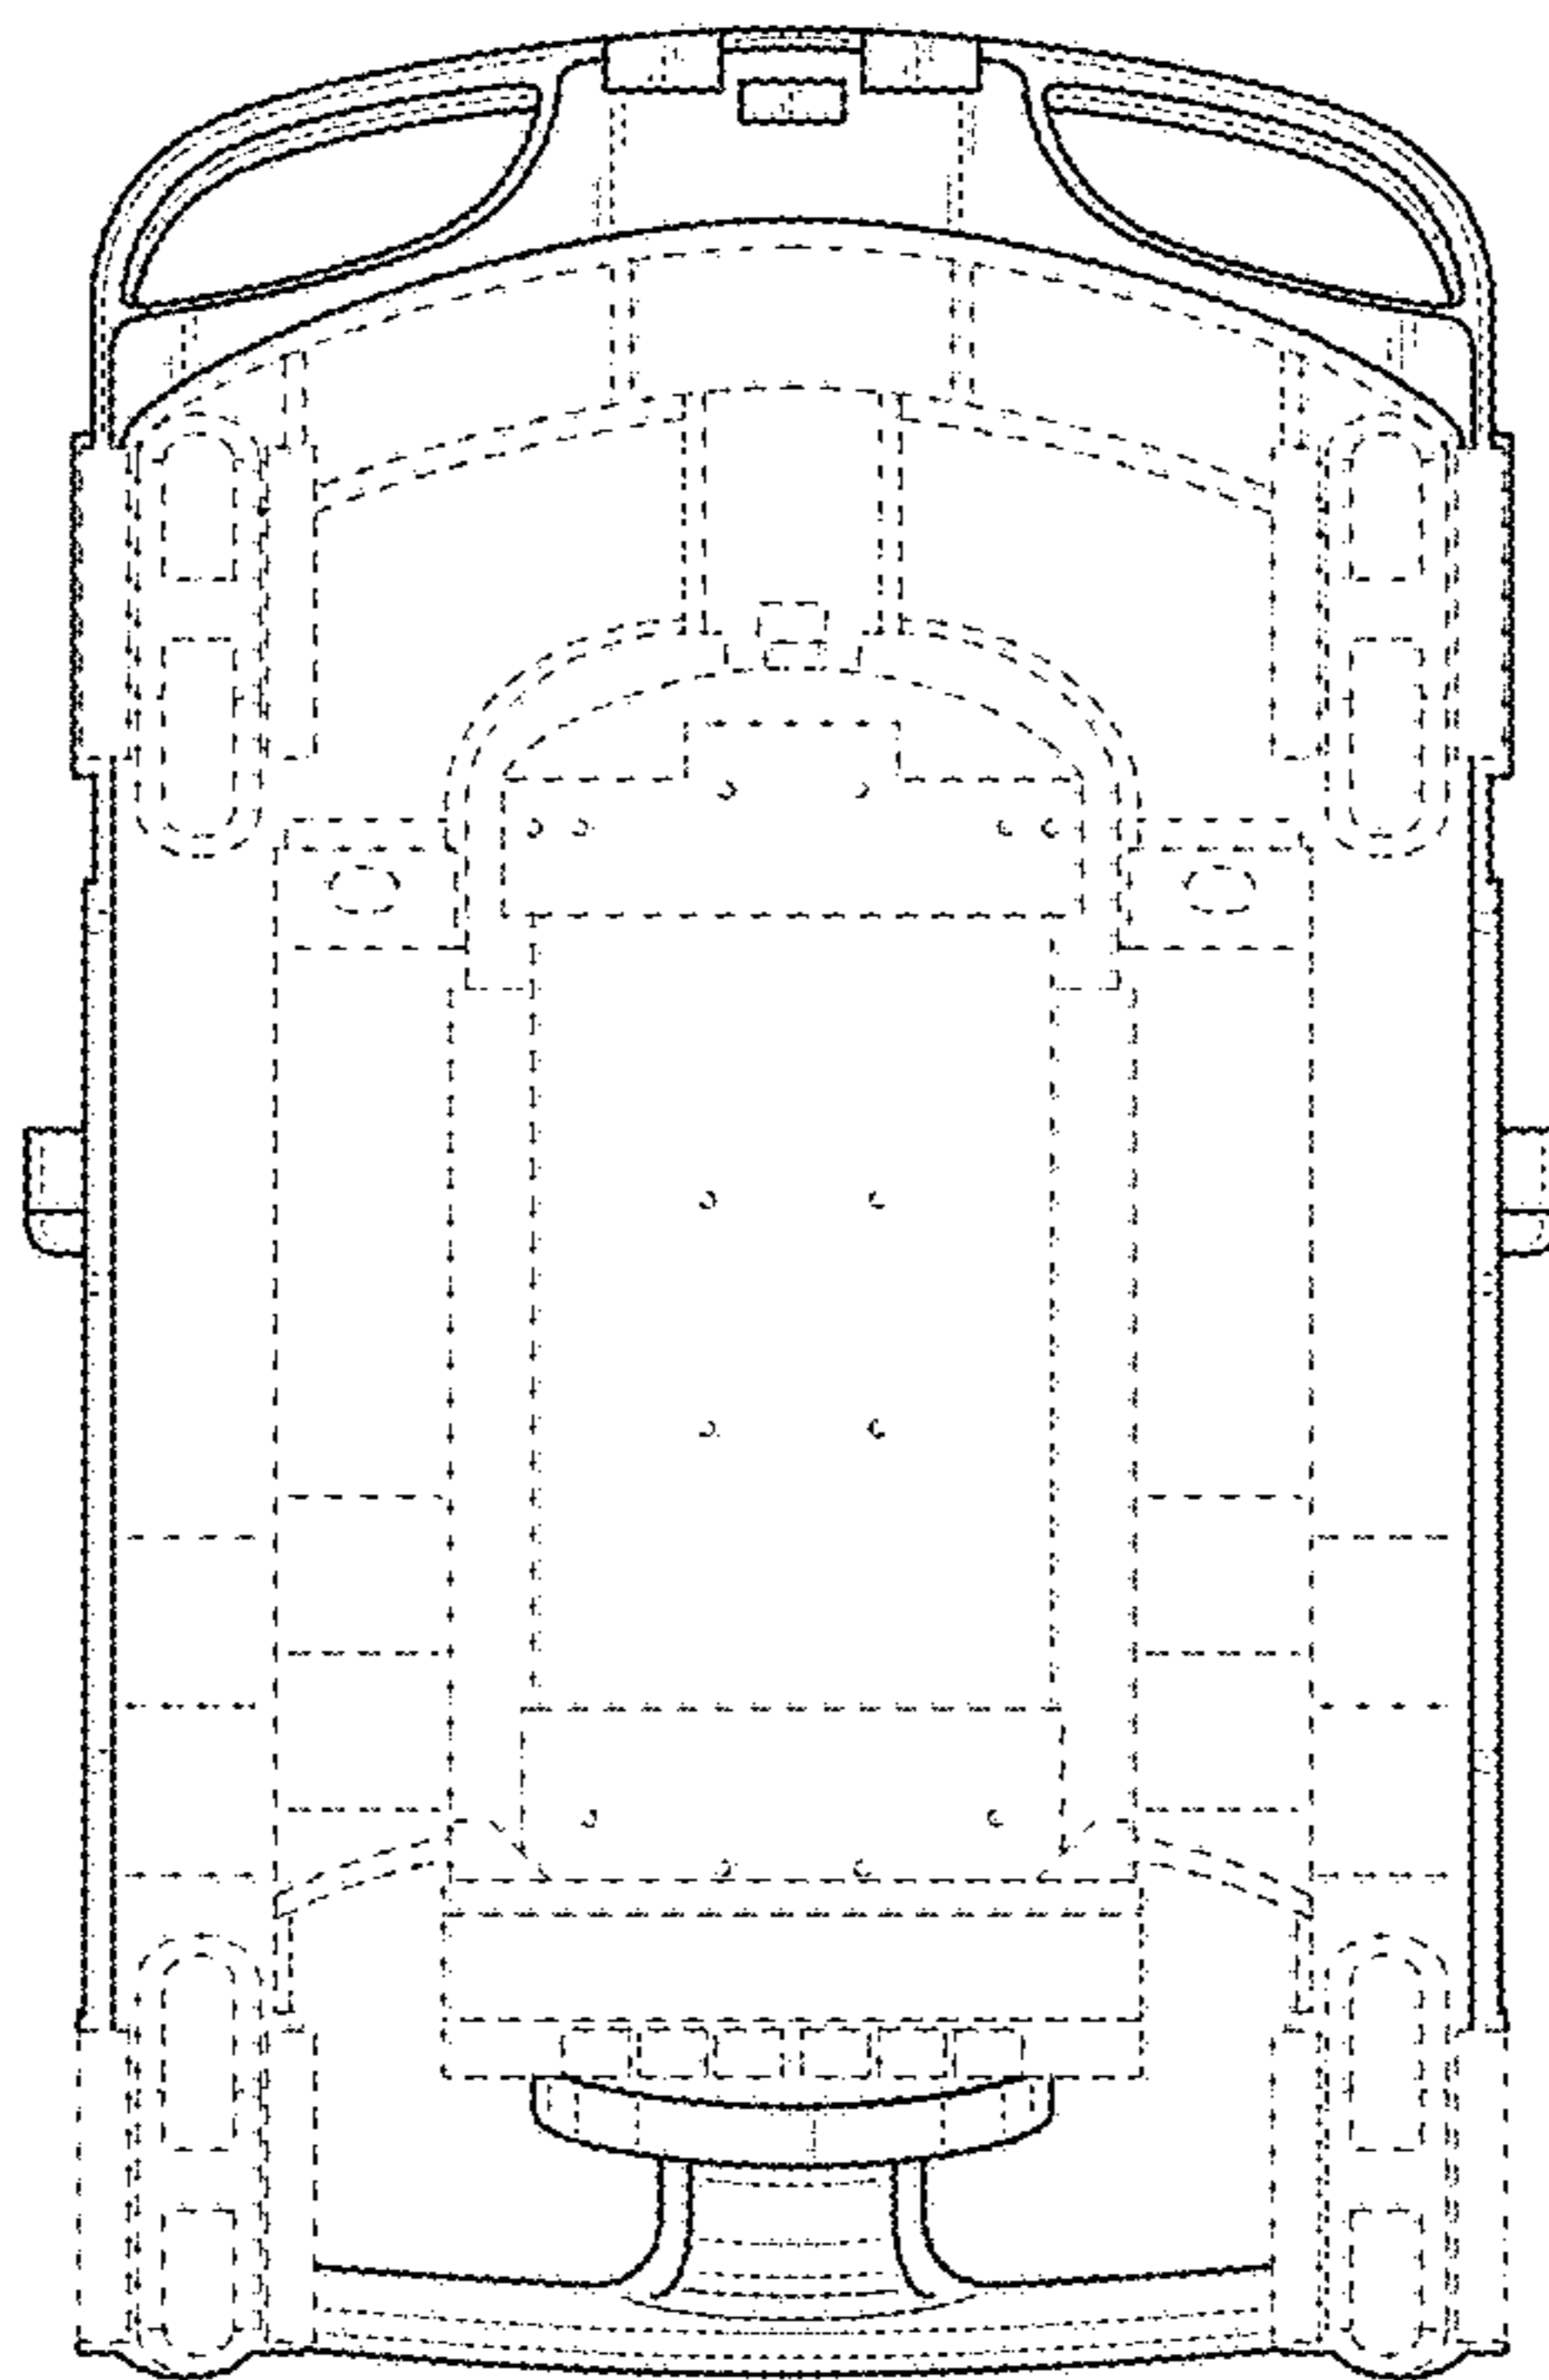


FIG. 6

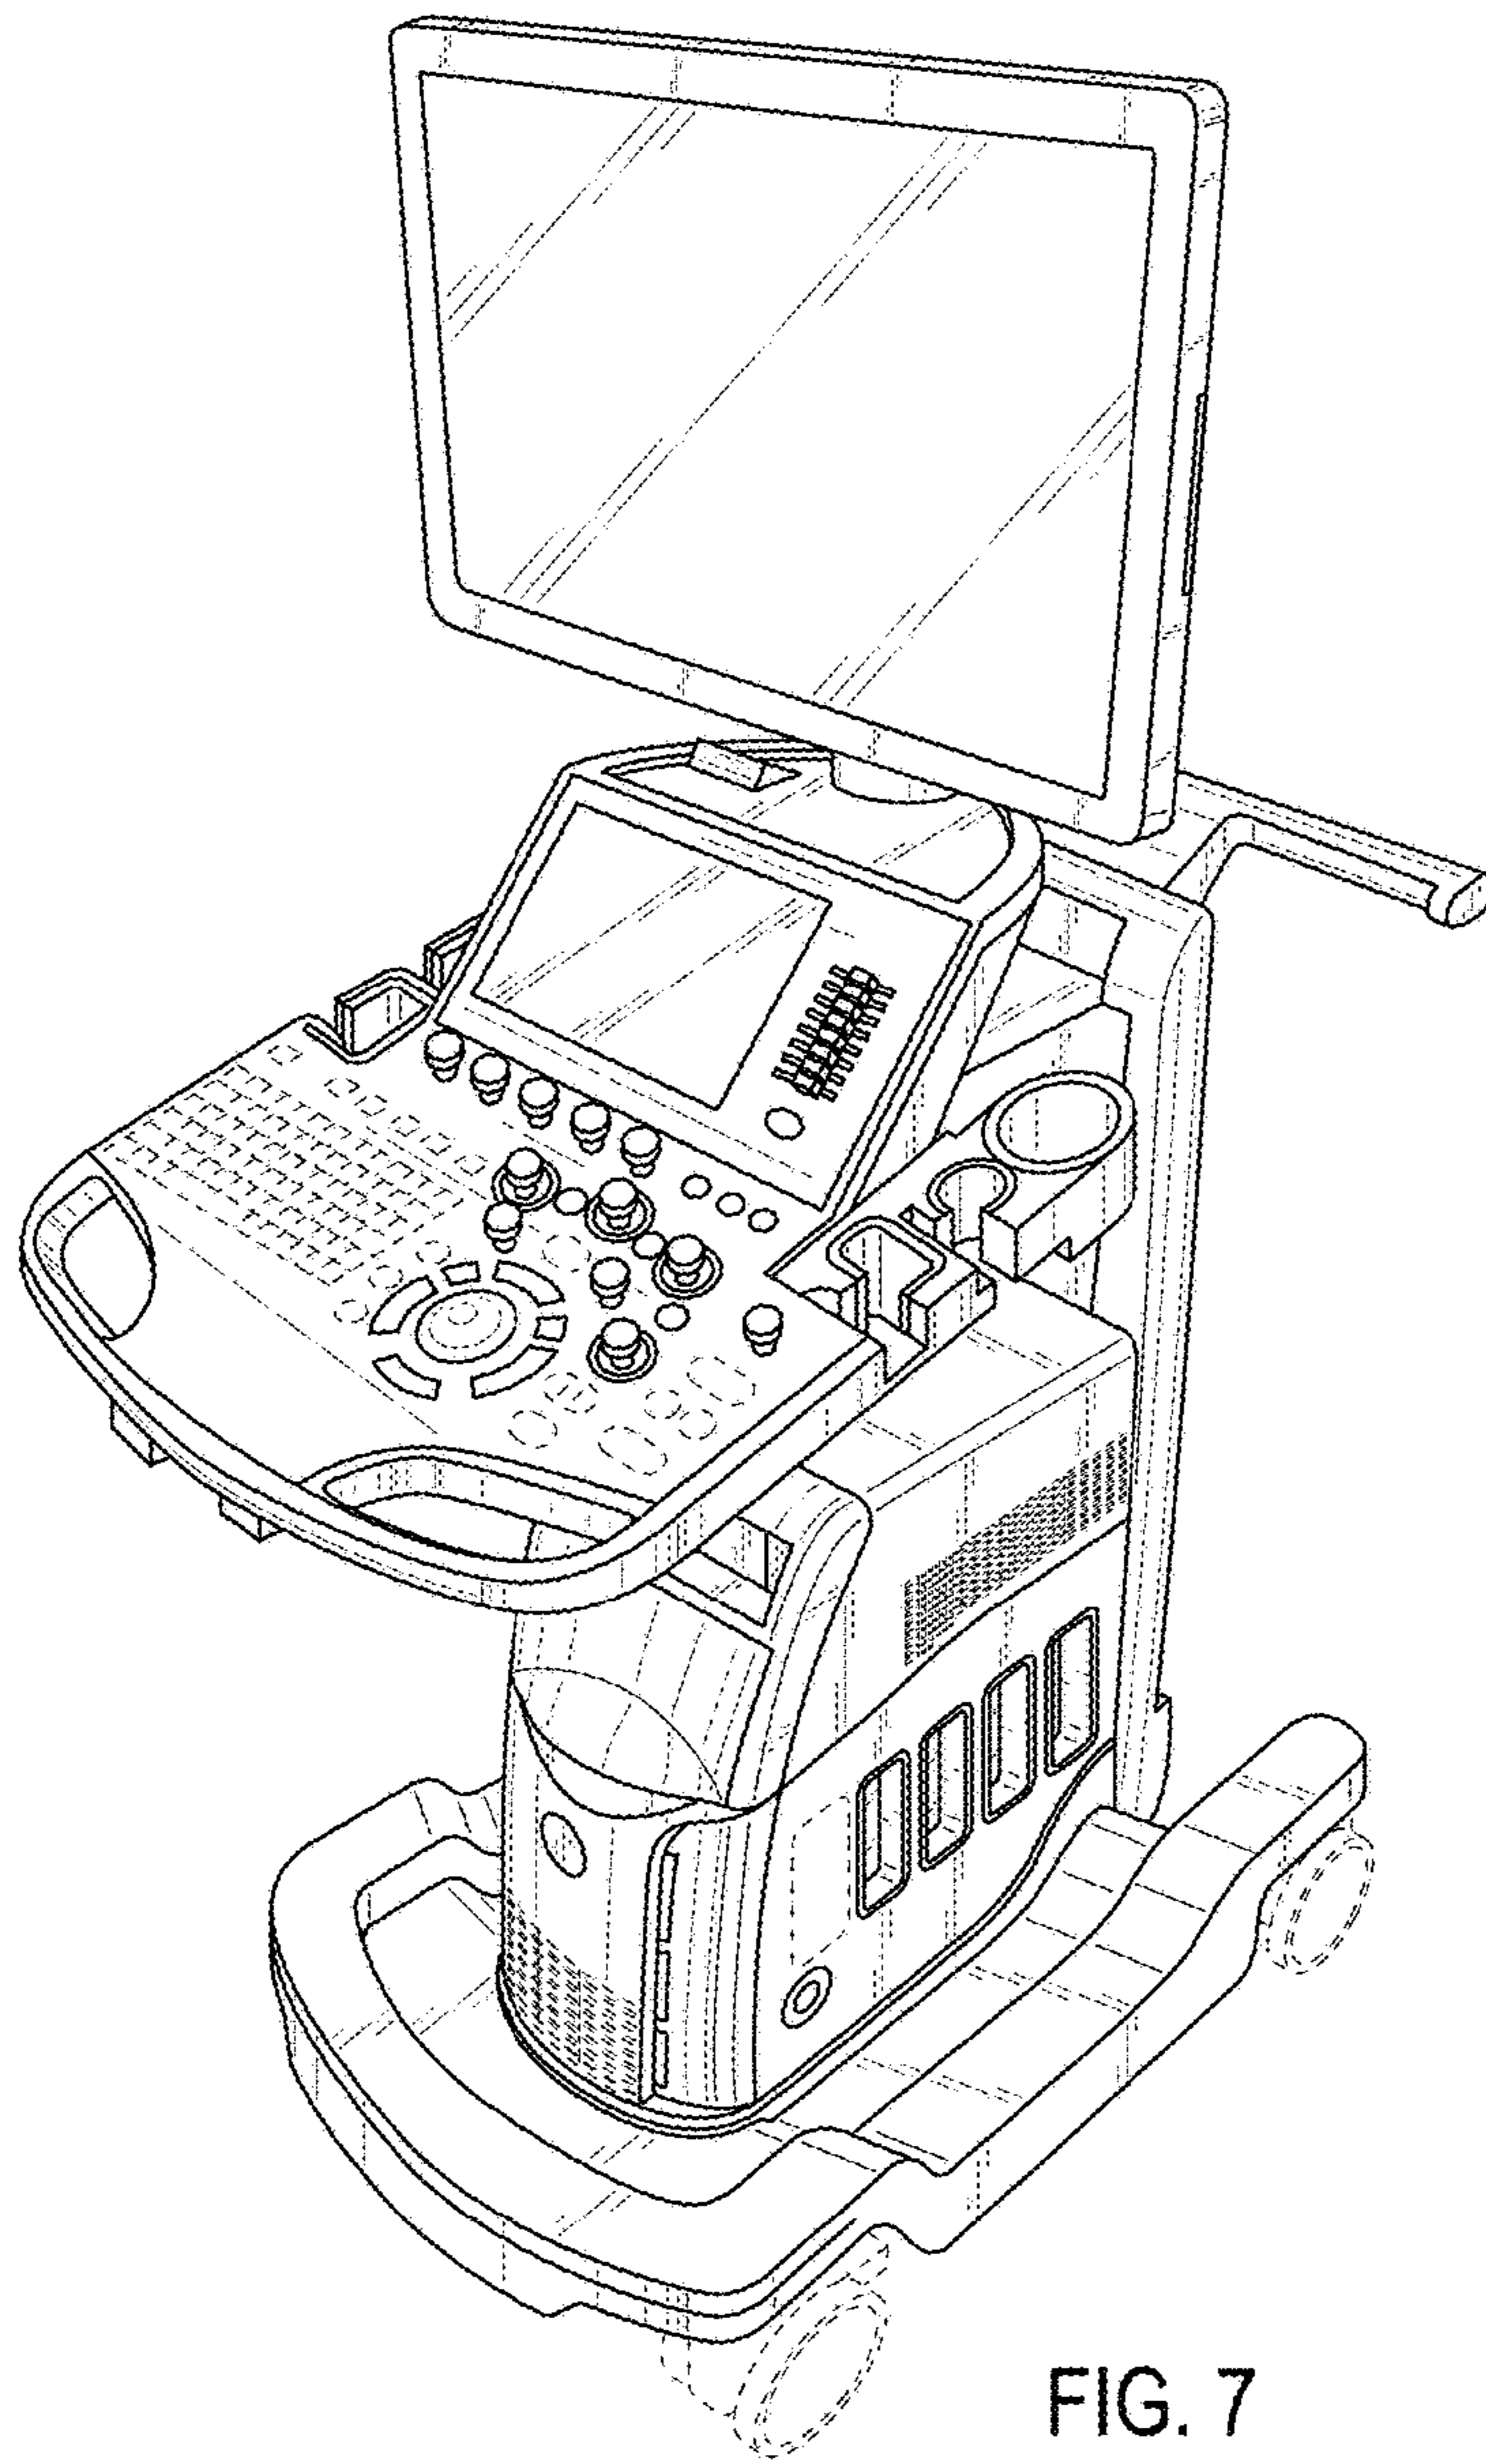


FIG. 7

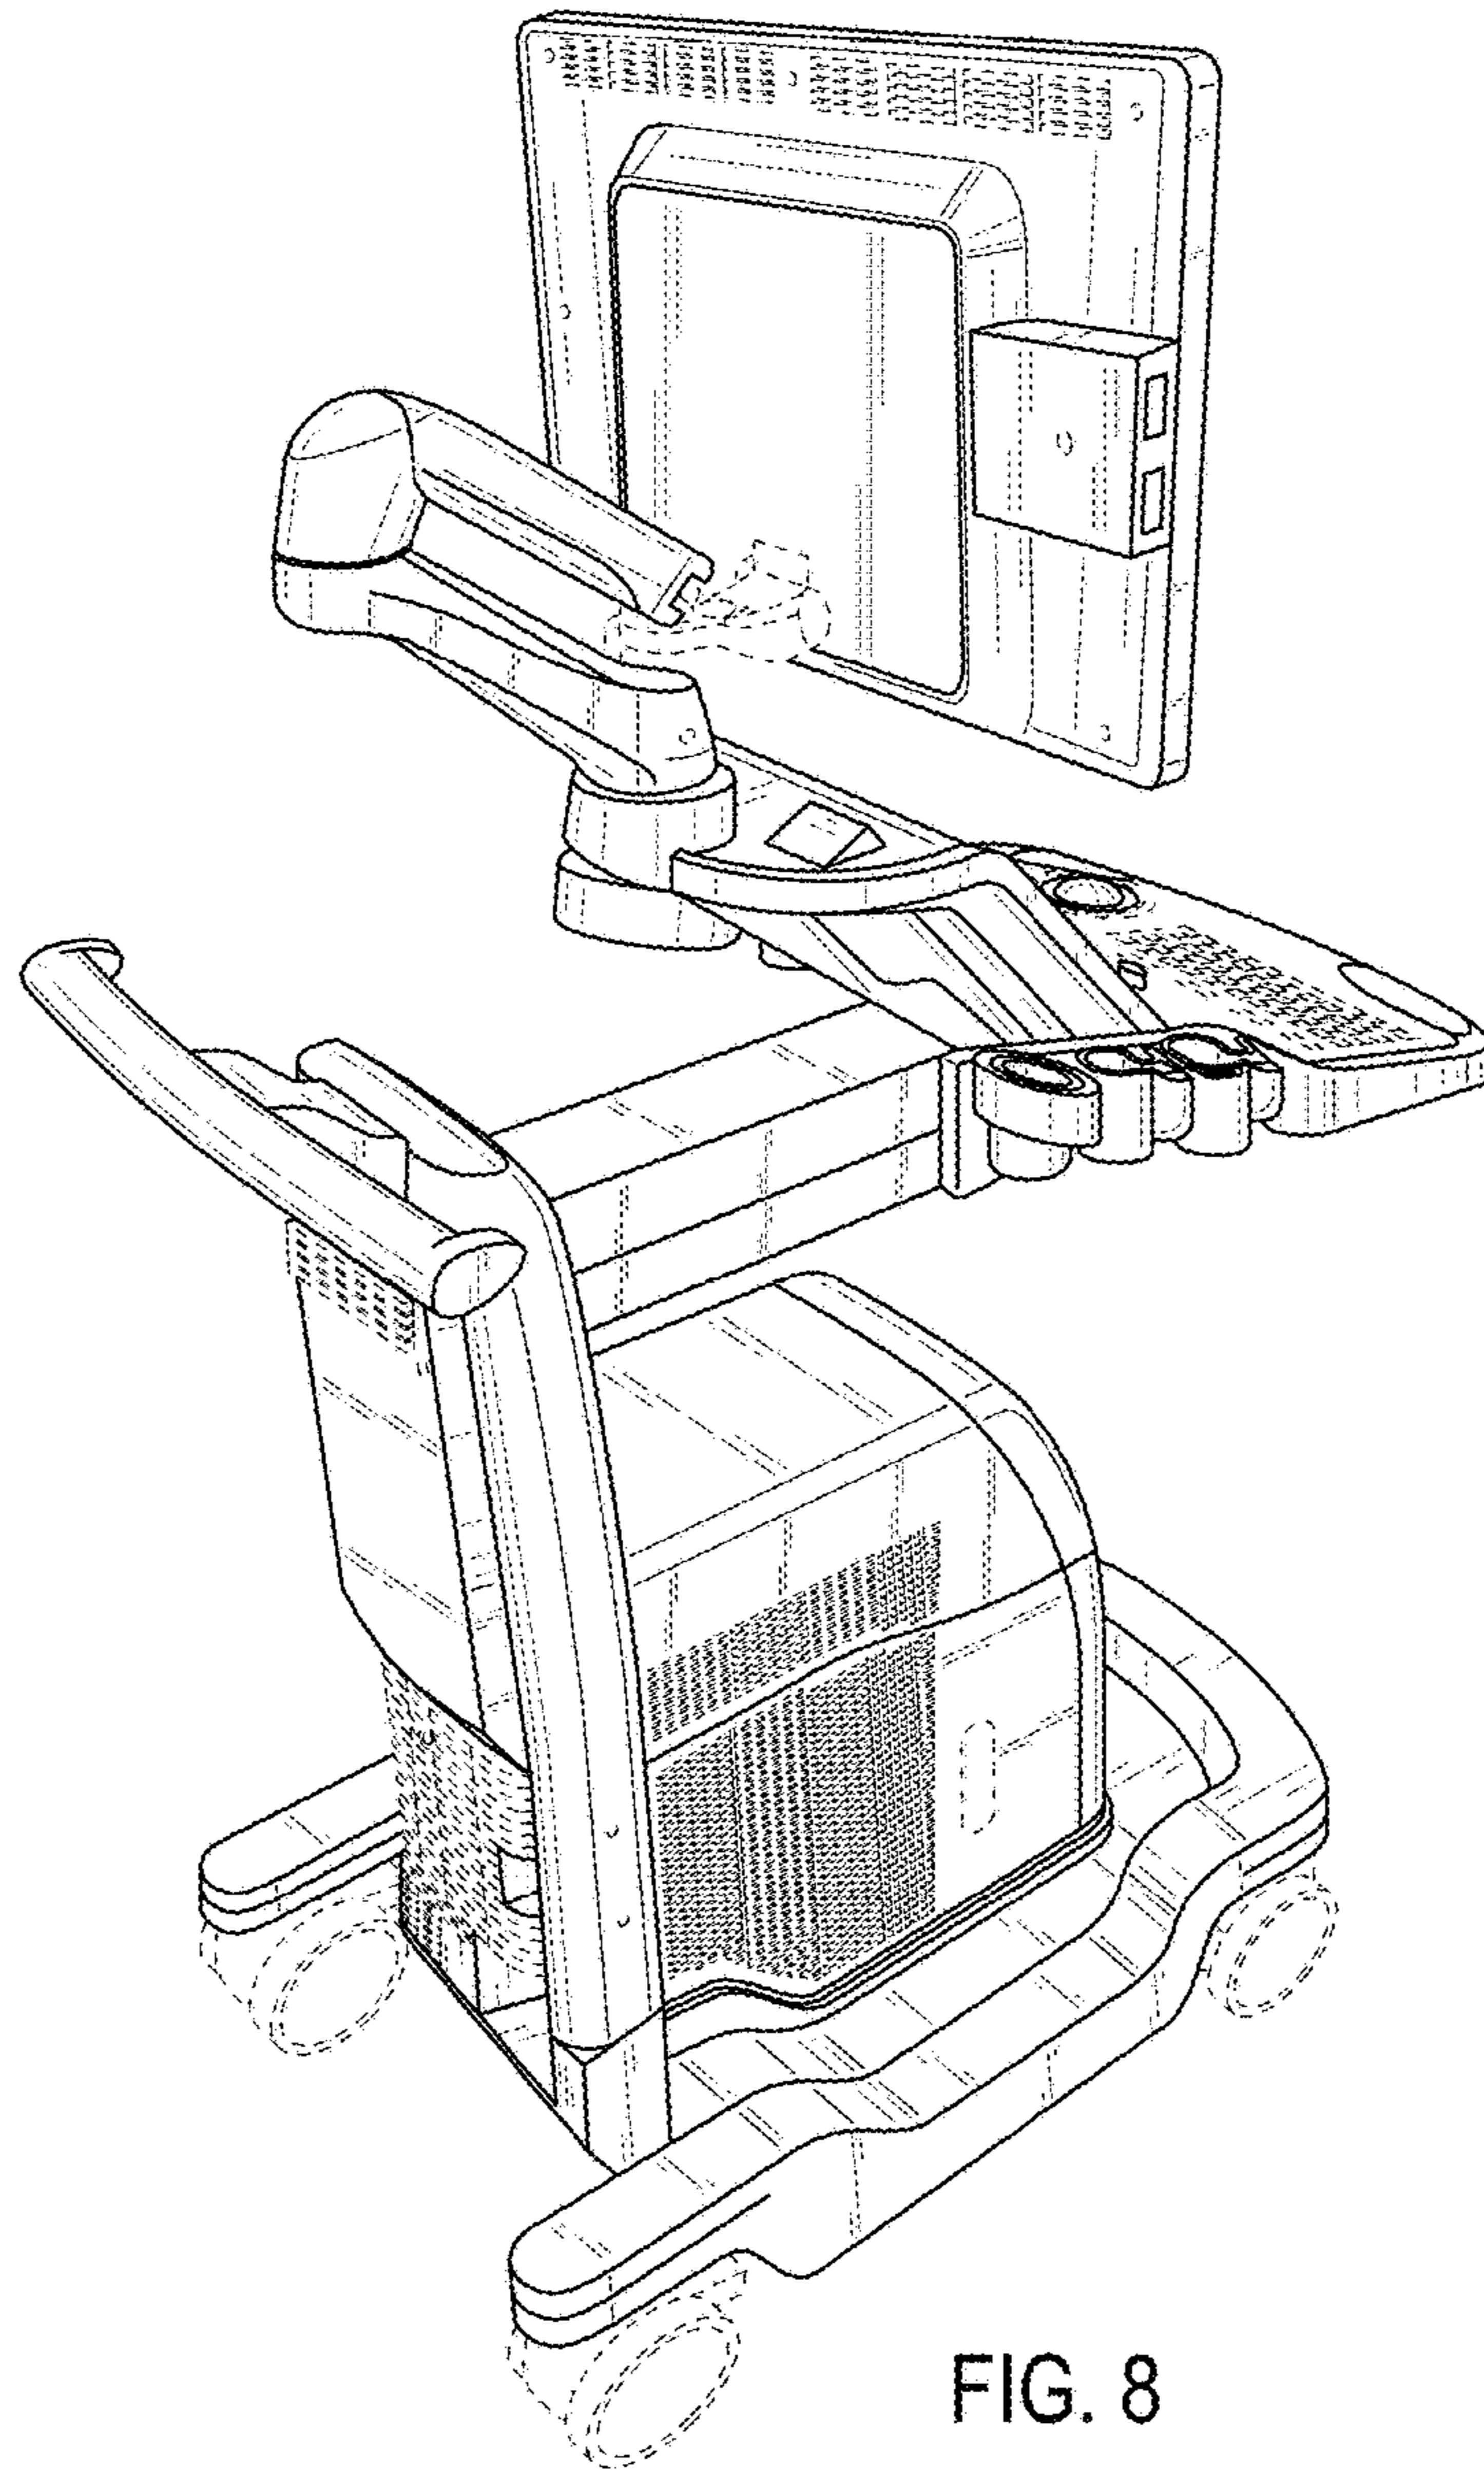


FIG. 8