



US00D841151S

(12) **United States Design Patent** (10) **Patent No.:** **US D841,151 S**
Bullington et al. (45) **Date of Patent:** **** Feb. 19, 2019**

(54) **BODILY-FLUID SAMPLING DEVICE**
(71) Applicant: **Magnolia Medical Technologies, Inc.**,
Seattle, WA (US)
(72) Inventors: **Gregory J. Bullington**, Bellevue, WA
(US); **Richard G. Patton**, Seattle, WA
(US); **Shan E. Gaw**, Seattle, WA (US);
Jay M. Miazga, Seattle, WA (US)
(73) Assignee: **Magnolia Medical Technologies, Inc.**,
Seattle, WA (US)
(**) Term: **15 Years**
(21) Appl. No.: **29/610,102**
(22) Filed: **Jul. 10, 2017**

Related U.S. Application Data

(62) Division of application No. 29/525,256, filed on Apr.
28, 2015, now Pat. No. Des. 794,779, which is a
division of application No. 29/434,421, filed on Oct.
12, 2012, now Pat. No. Des. 731,643.
(51) **LOC (11) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/117**
(58) **Field of Classification Search**
USPC D24/117, 112-114, 133, 186, 130, 127,
D24/129, 108; 600/400, 473-476, 101,
600/139, 143; 606/15-16, 181, 185;
604/264, 280, 256, 164, 283, 174;
128/200.24, 207.14, 207.15
CPC A61B 10/0045; A61B 10/0096; A61B
5/150099; A61B 5/150221; A61B
5/150236

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D286,426 S	10/1986	Lin	
4,832,232 A	5/1989	Broccoli	
5,307,994 A	5/1994	Hieronymus	
5,322,094 A	6/1994	Janesko	
5,458,640 A	10/1995	Gerrone	
5,485,857 A	1/1996	Amundsen	
5,807,338 A	9/1998	Smith et al.	
5,842,638 A	12/1998	Reents et al.	
6,056,766 A	5/2000	Thompson et al.	
6,159,164 A	12/2000	Neese et al.	
D461,226 S *	8/2002	Hunter	D23/225
D467,991 S *	12/2002	Ibele	D23/225
D477,384 S *	7/2003	Williams	D23/225
6,626,380 B1 *	9/2003	Williams	B05B 9/0861 222/333

(Continued)


Primary Examiner — David G Muller
Assistant Examiner — Nathan M Johnson
(74) *Attorney, Agent, or Firm* — Cooley LLP

(57) **CLAIM**
The ornamental design for a bodily-fluid sampling device, as
shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of the bodily-fluid sampling
device showing our new design;
FIG. 2 is a bottom perspective view thereof;
FIG. 3 is a front elevation view thereof;
FIG. 4 is a rear elevation view thereof;
FIG. 5 is a left side elevation view thereof;
FIG. 6 is a right side elevation view thereof;
FIG. 7 is a top plan view thereof; and,
FIG. 8 is a bottom plan view thereof.
The broken lines immediately adjacent the shaded areas
represent the bounds of the claimed design while all other
broken lines are directed to environment and are for illus-
trative purposes only; the broken lines form no part of the
claimed design.

1 Claim, 7 Drawing Sheets

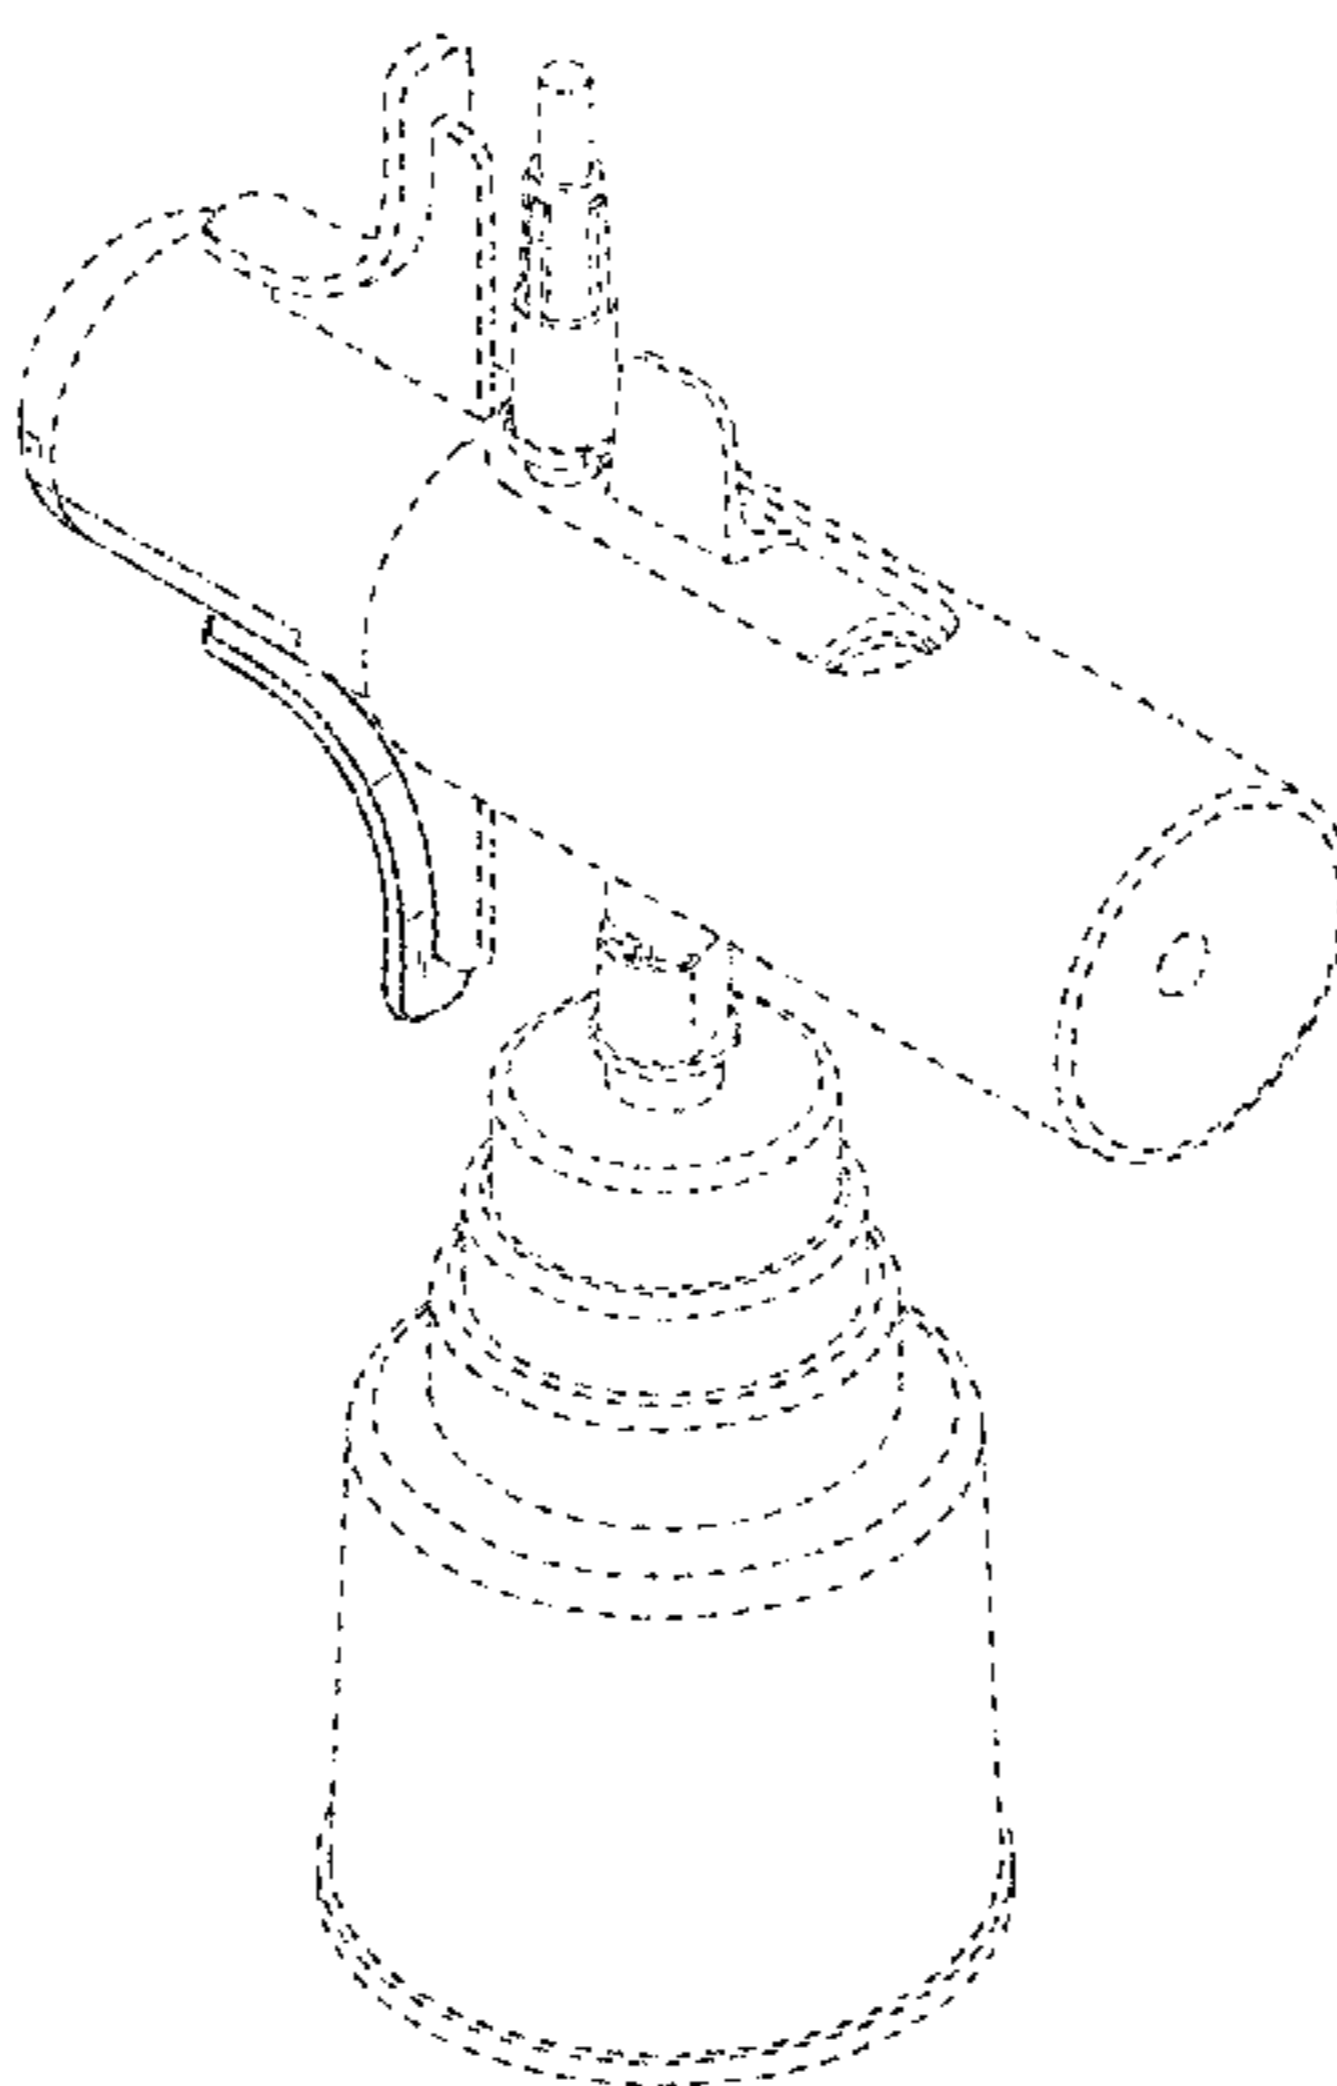

(56)

References Cited

U.S. PATENT DOCUMENTS

6,631,855 B2 * 10/2003 Huang B05B 9/0861
 239/302
 D490,500 S * 5/2004 Ye D23/225
 D495,400 S * 8/2004 Hopper D23/225
 D503,213 S 3/2005 Stevens et al.
 D503,215 S * 3/2005 Stevens D23/225
 D519,603 S 4/2006 Schumann et al.
 7,066,406 B2 * 6/2006 Williams B05B 15/40
 239/375
 D532,514 S 11/2006 Schmal
 D541,903 S * 5/2007 Hopper D23/225
 7,258,694 B1 8/2007 Choi et al.
 D564,623 S * 3/2008 Nathan D23/225
 7,377,452 B2 5/2008 Jones et al.
 D570,956 S 6/2008 Everett et al.
 D573,226 S * 7/2008 Everett D23/225
 D589,116 S * 3/2009 Bruggeman D23/225
 D604,393 S * 11/2009 Johnson D23/225
 D605,765 S 12/2009 Gaab
 D609,778 S * 2/2010 Woodgate D23/225
 7,798,429 B1 9/2010 Porter

D644,715 S * 9/2011 Woodling D23/225
 8,062,305 B2 11/2011 Wenchell
 D660,426 S * 5/2012 Hermle D24/138
 D660,941 S * 5/2012 Perez D23/225
 D664,628 S 7/2012 Zhou et al.
 8,267,332 B1 * 9/2012 Jones B05B 1/3436
 239/463
 8,308,083 B2 * 11/2012 Woodgate B05B 1/3046
 239/296
 8,535,241 B2 9/2013 Bullington et al.
 8,596,555 B2 * 12/2013 Thompson B05B 9/01
 239/152
 D713,500 S 9/2014 Muhl et al.
 8,864,684 B2 * 10/2014 Bullington A61B 5/150221
 600/576
 D731,643 S 6/2015 Bullington et al.
 9,060,724 B2 6/2015 Bullington et al.
 D740,393 S * 10/2015 Gehrung D23/226
 D759,199 S * 6/2016 Wrobel D23/225
 D772,380 S * 11/2016 Fontaine D23/225
 D794,779 S * 8/2017 Bullington D24/117
 2009/0005740 A1 1/2009 Smith
 2010/0322795 A1 12/2010 Jones et al.
 2011/0152910 A1 6/2011 Smith

* cited by examiner

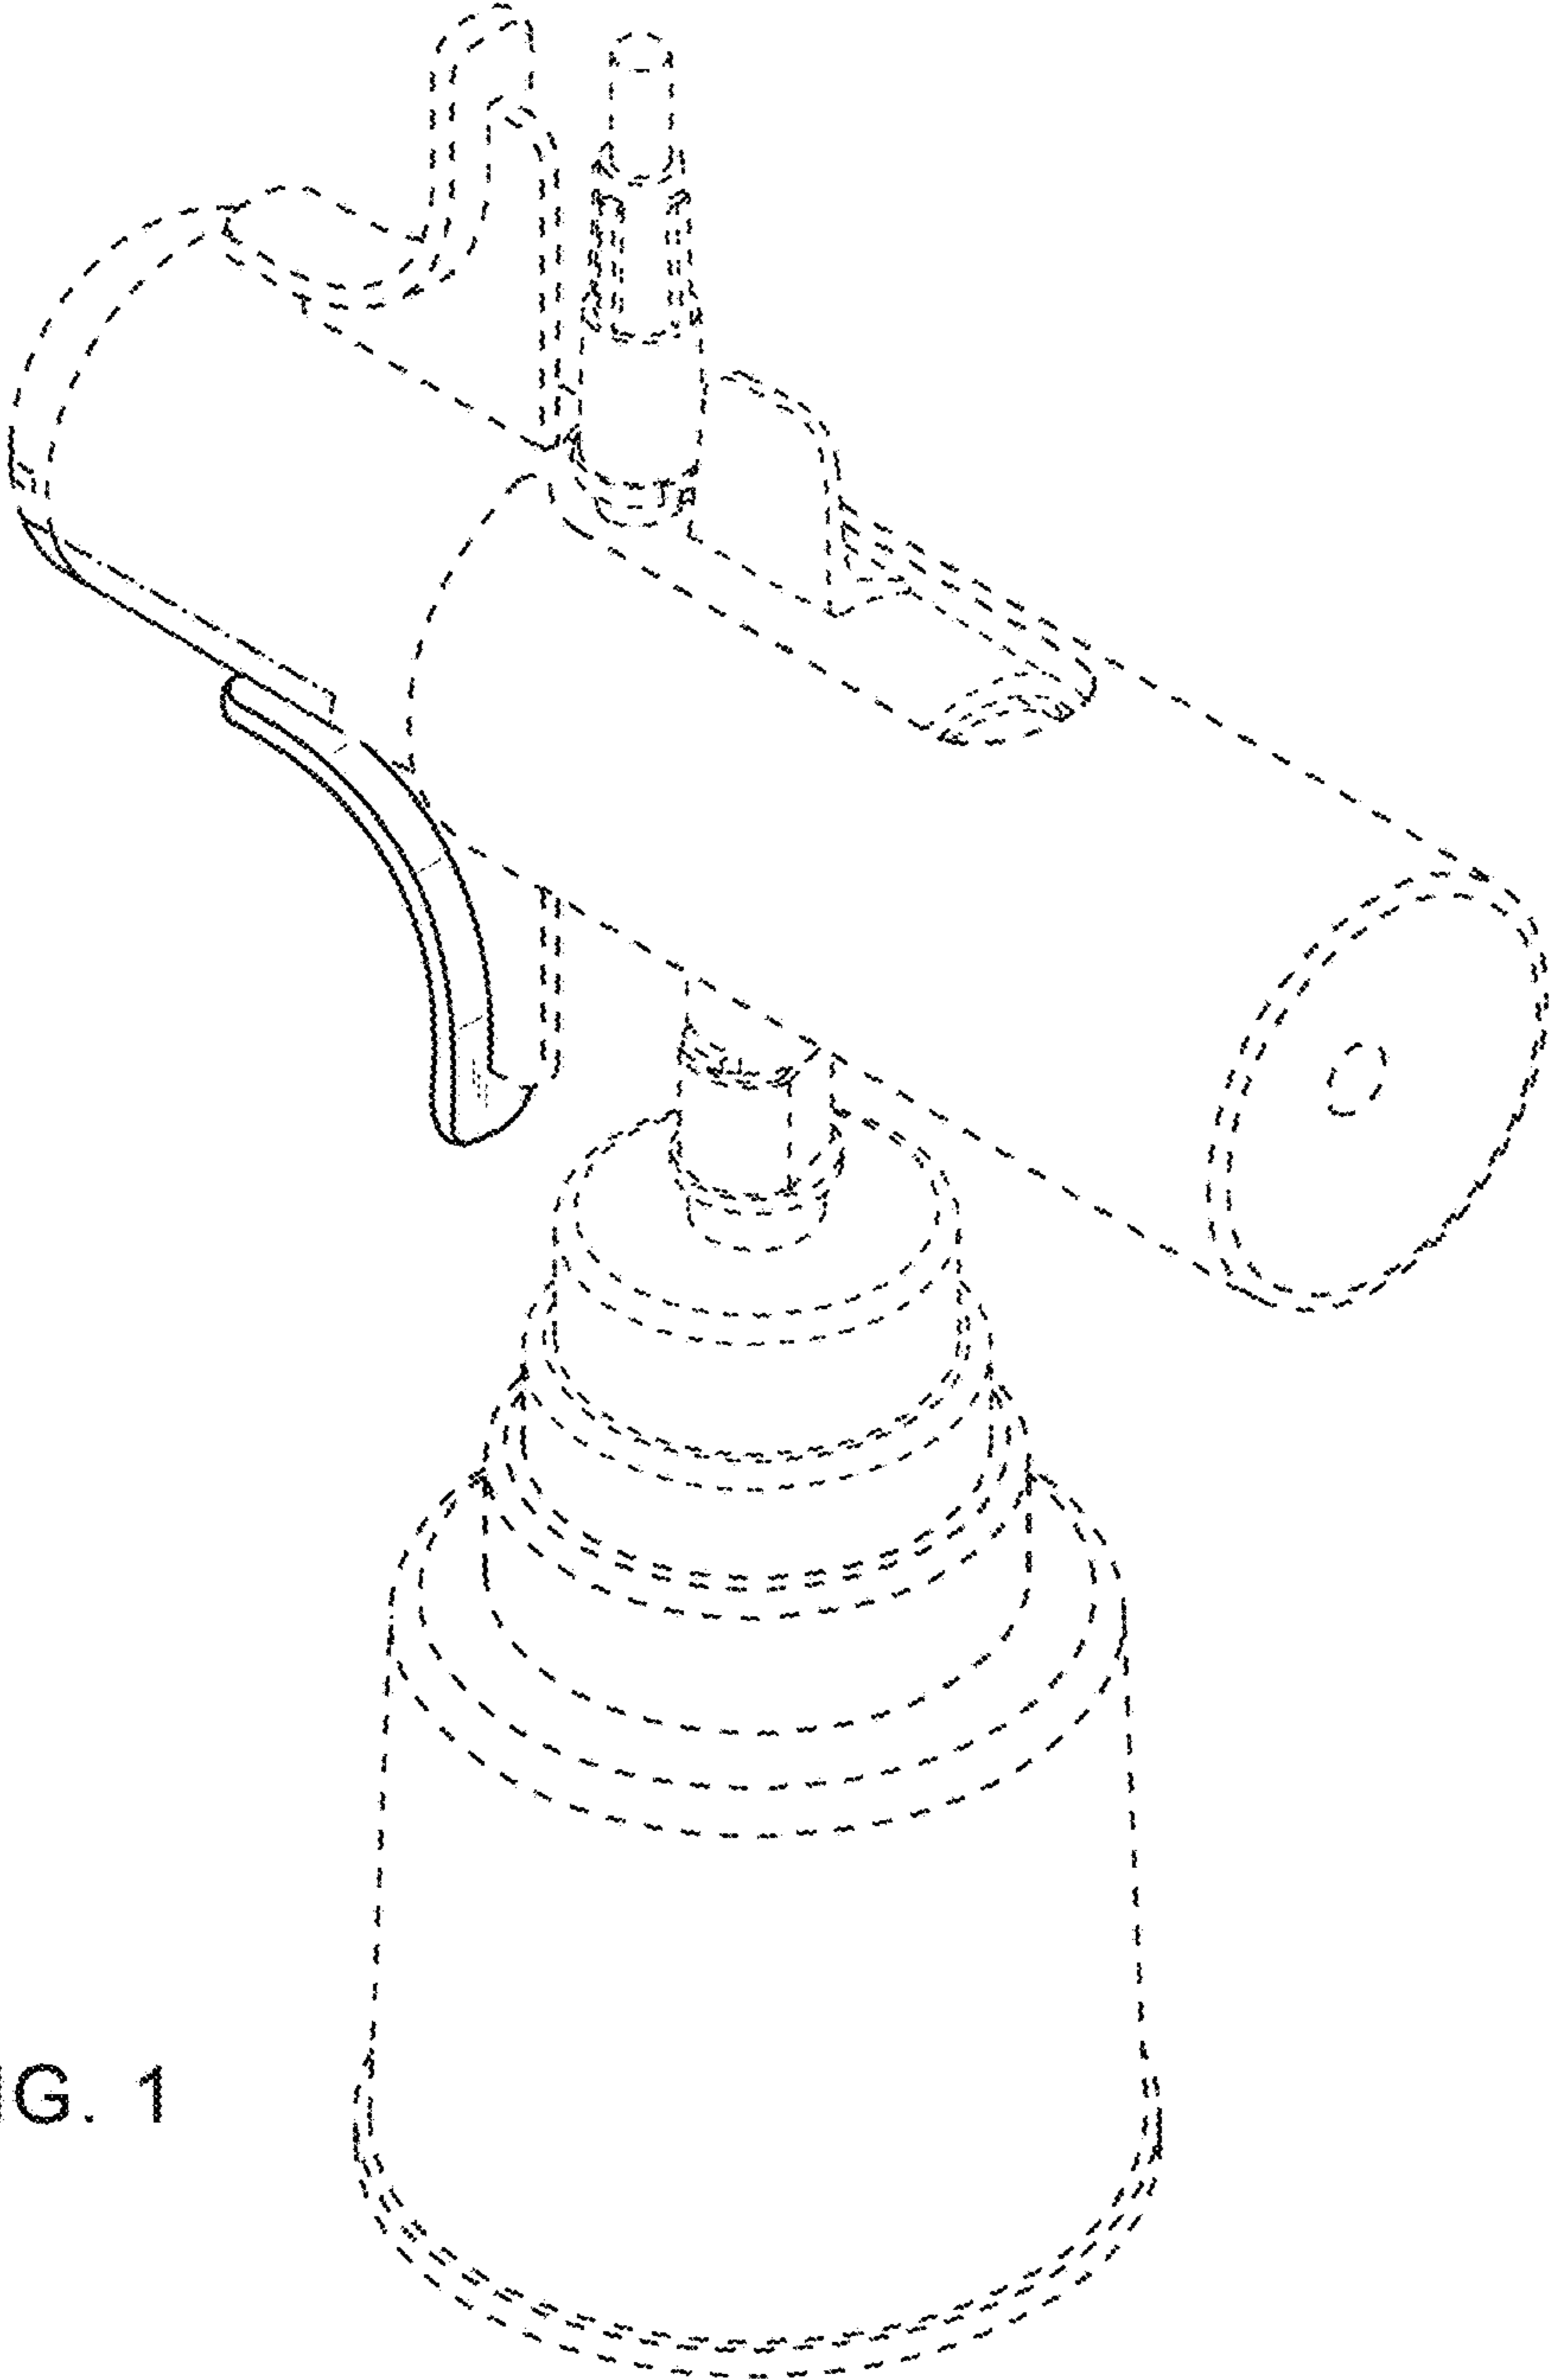


FIG. 1

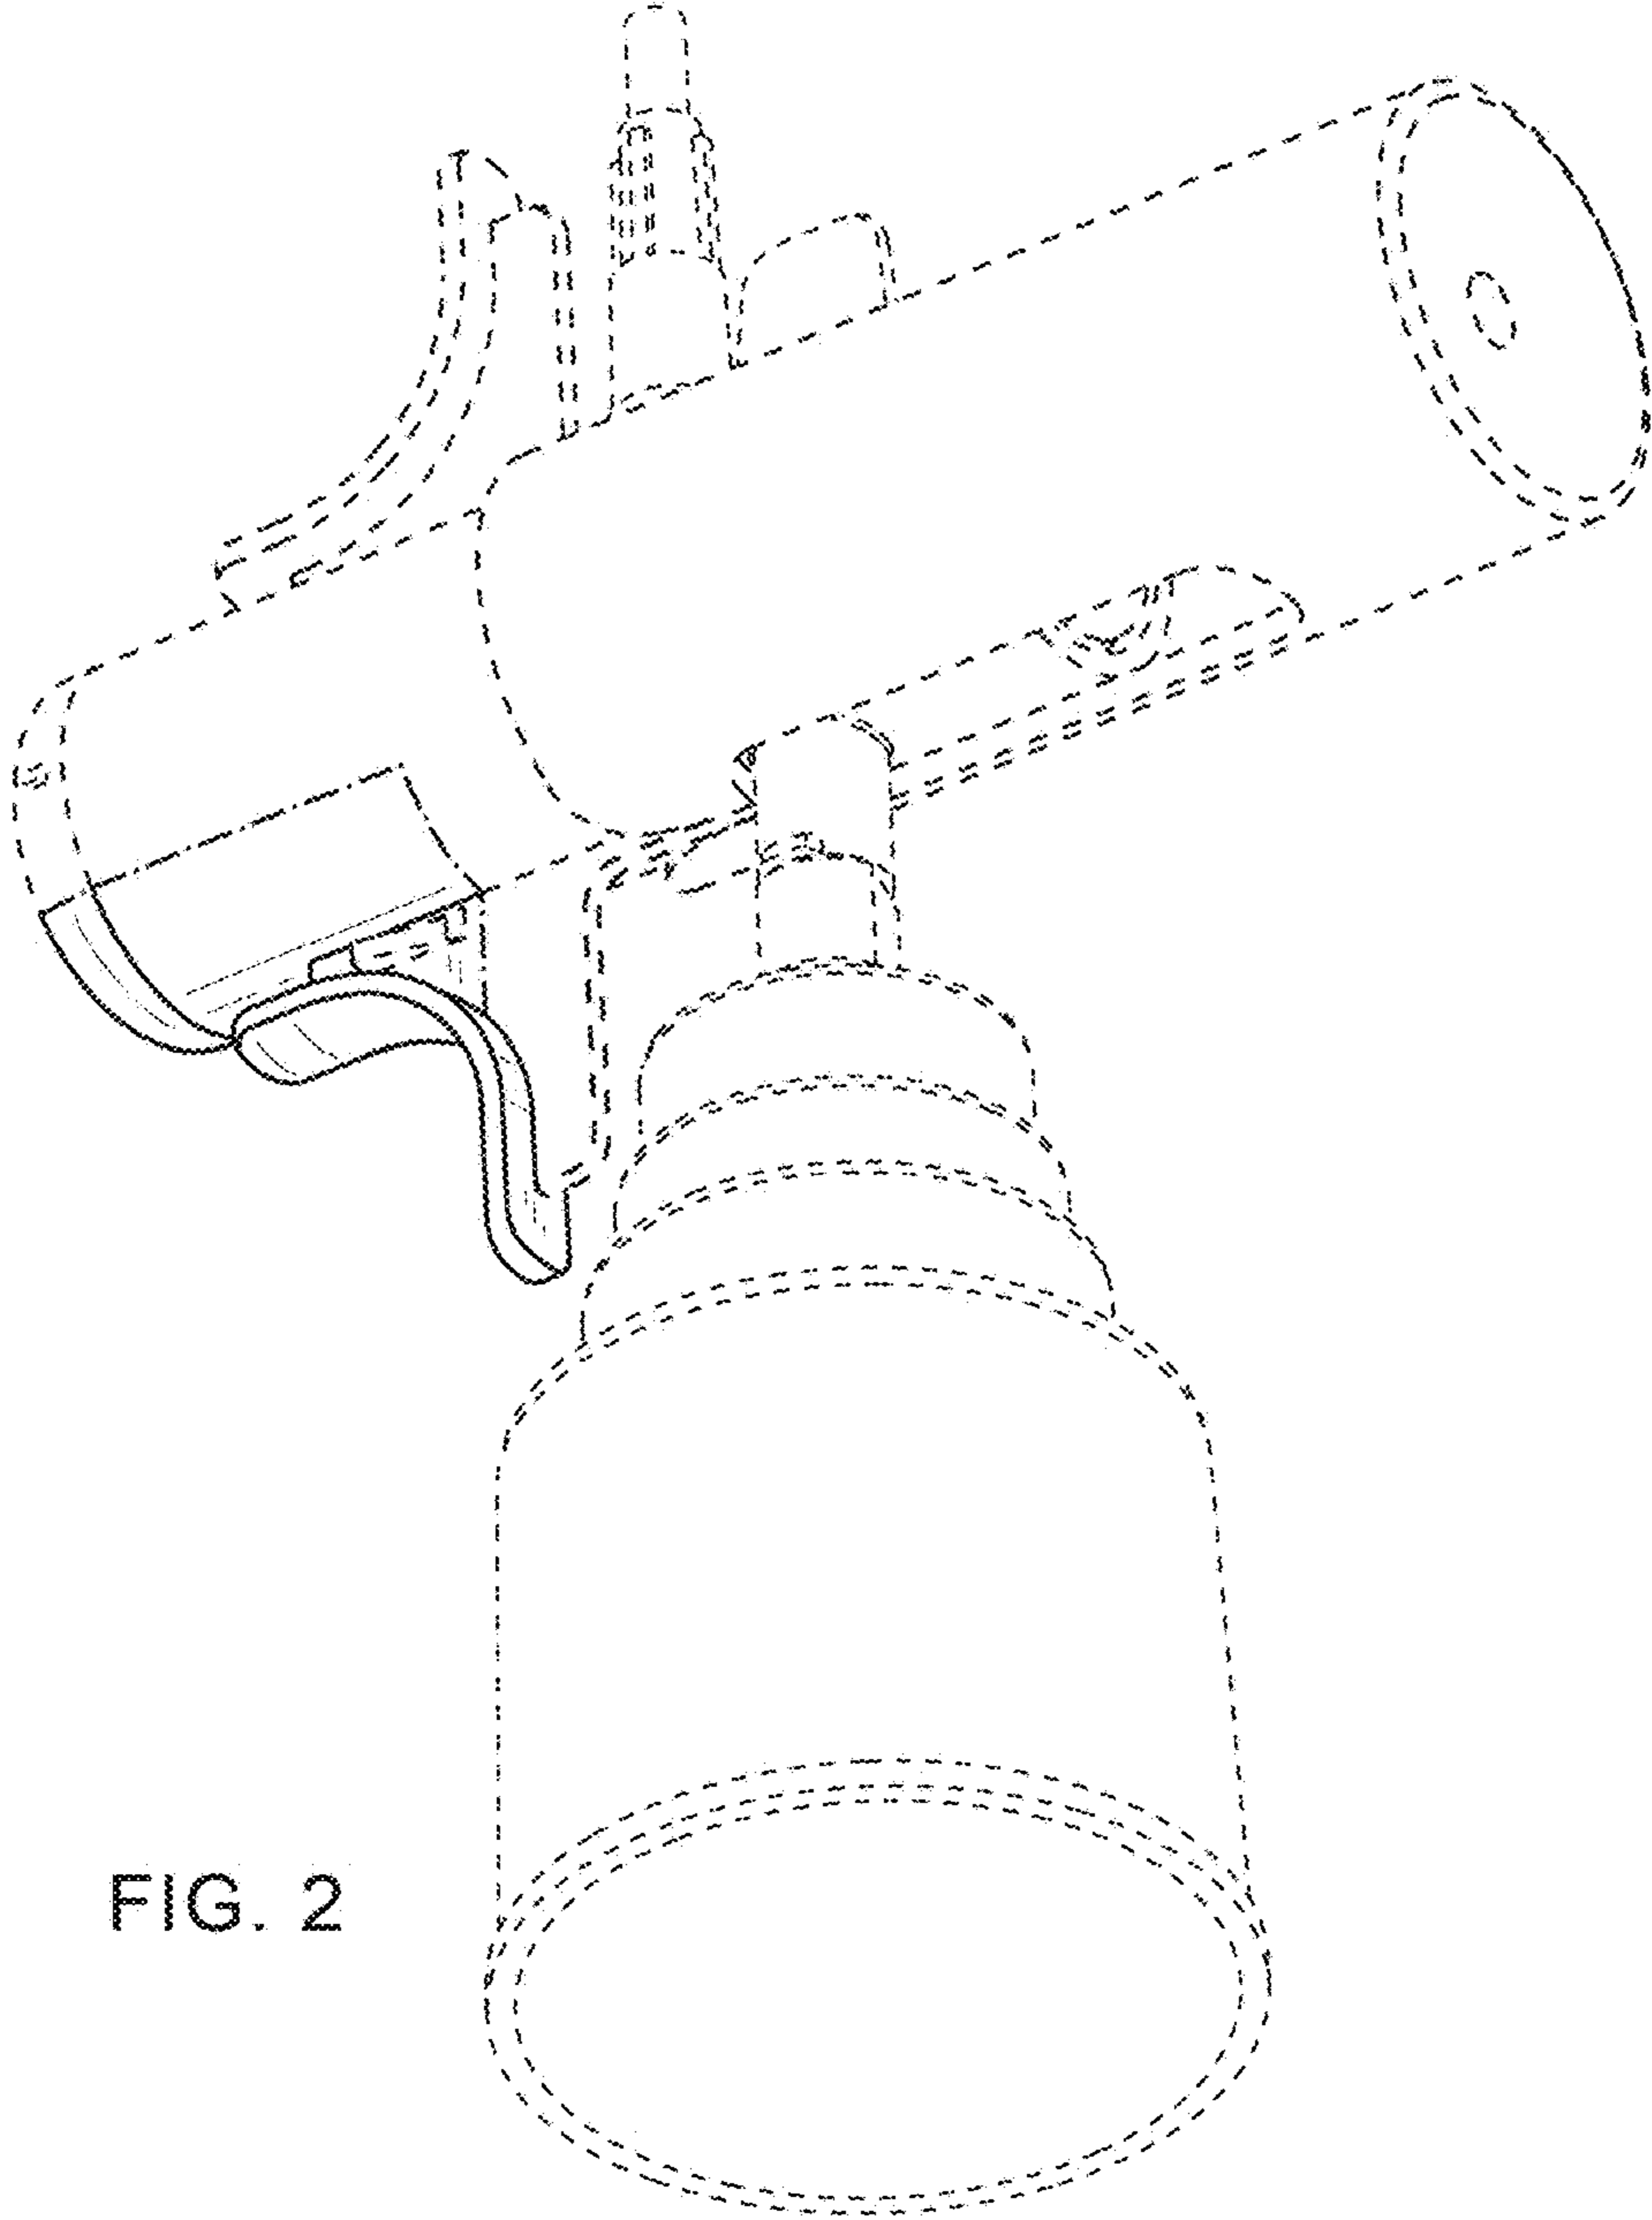


FIG. 2

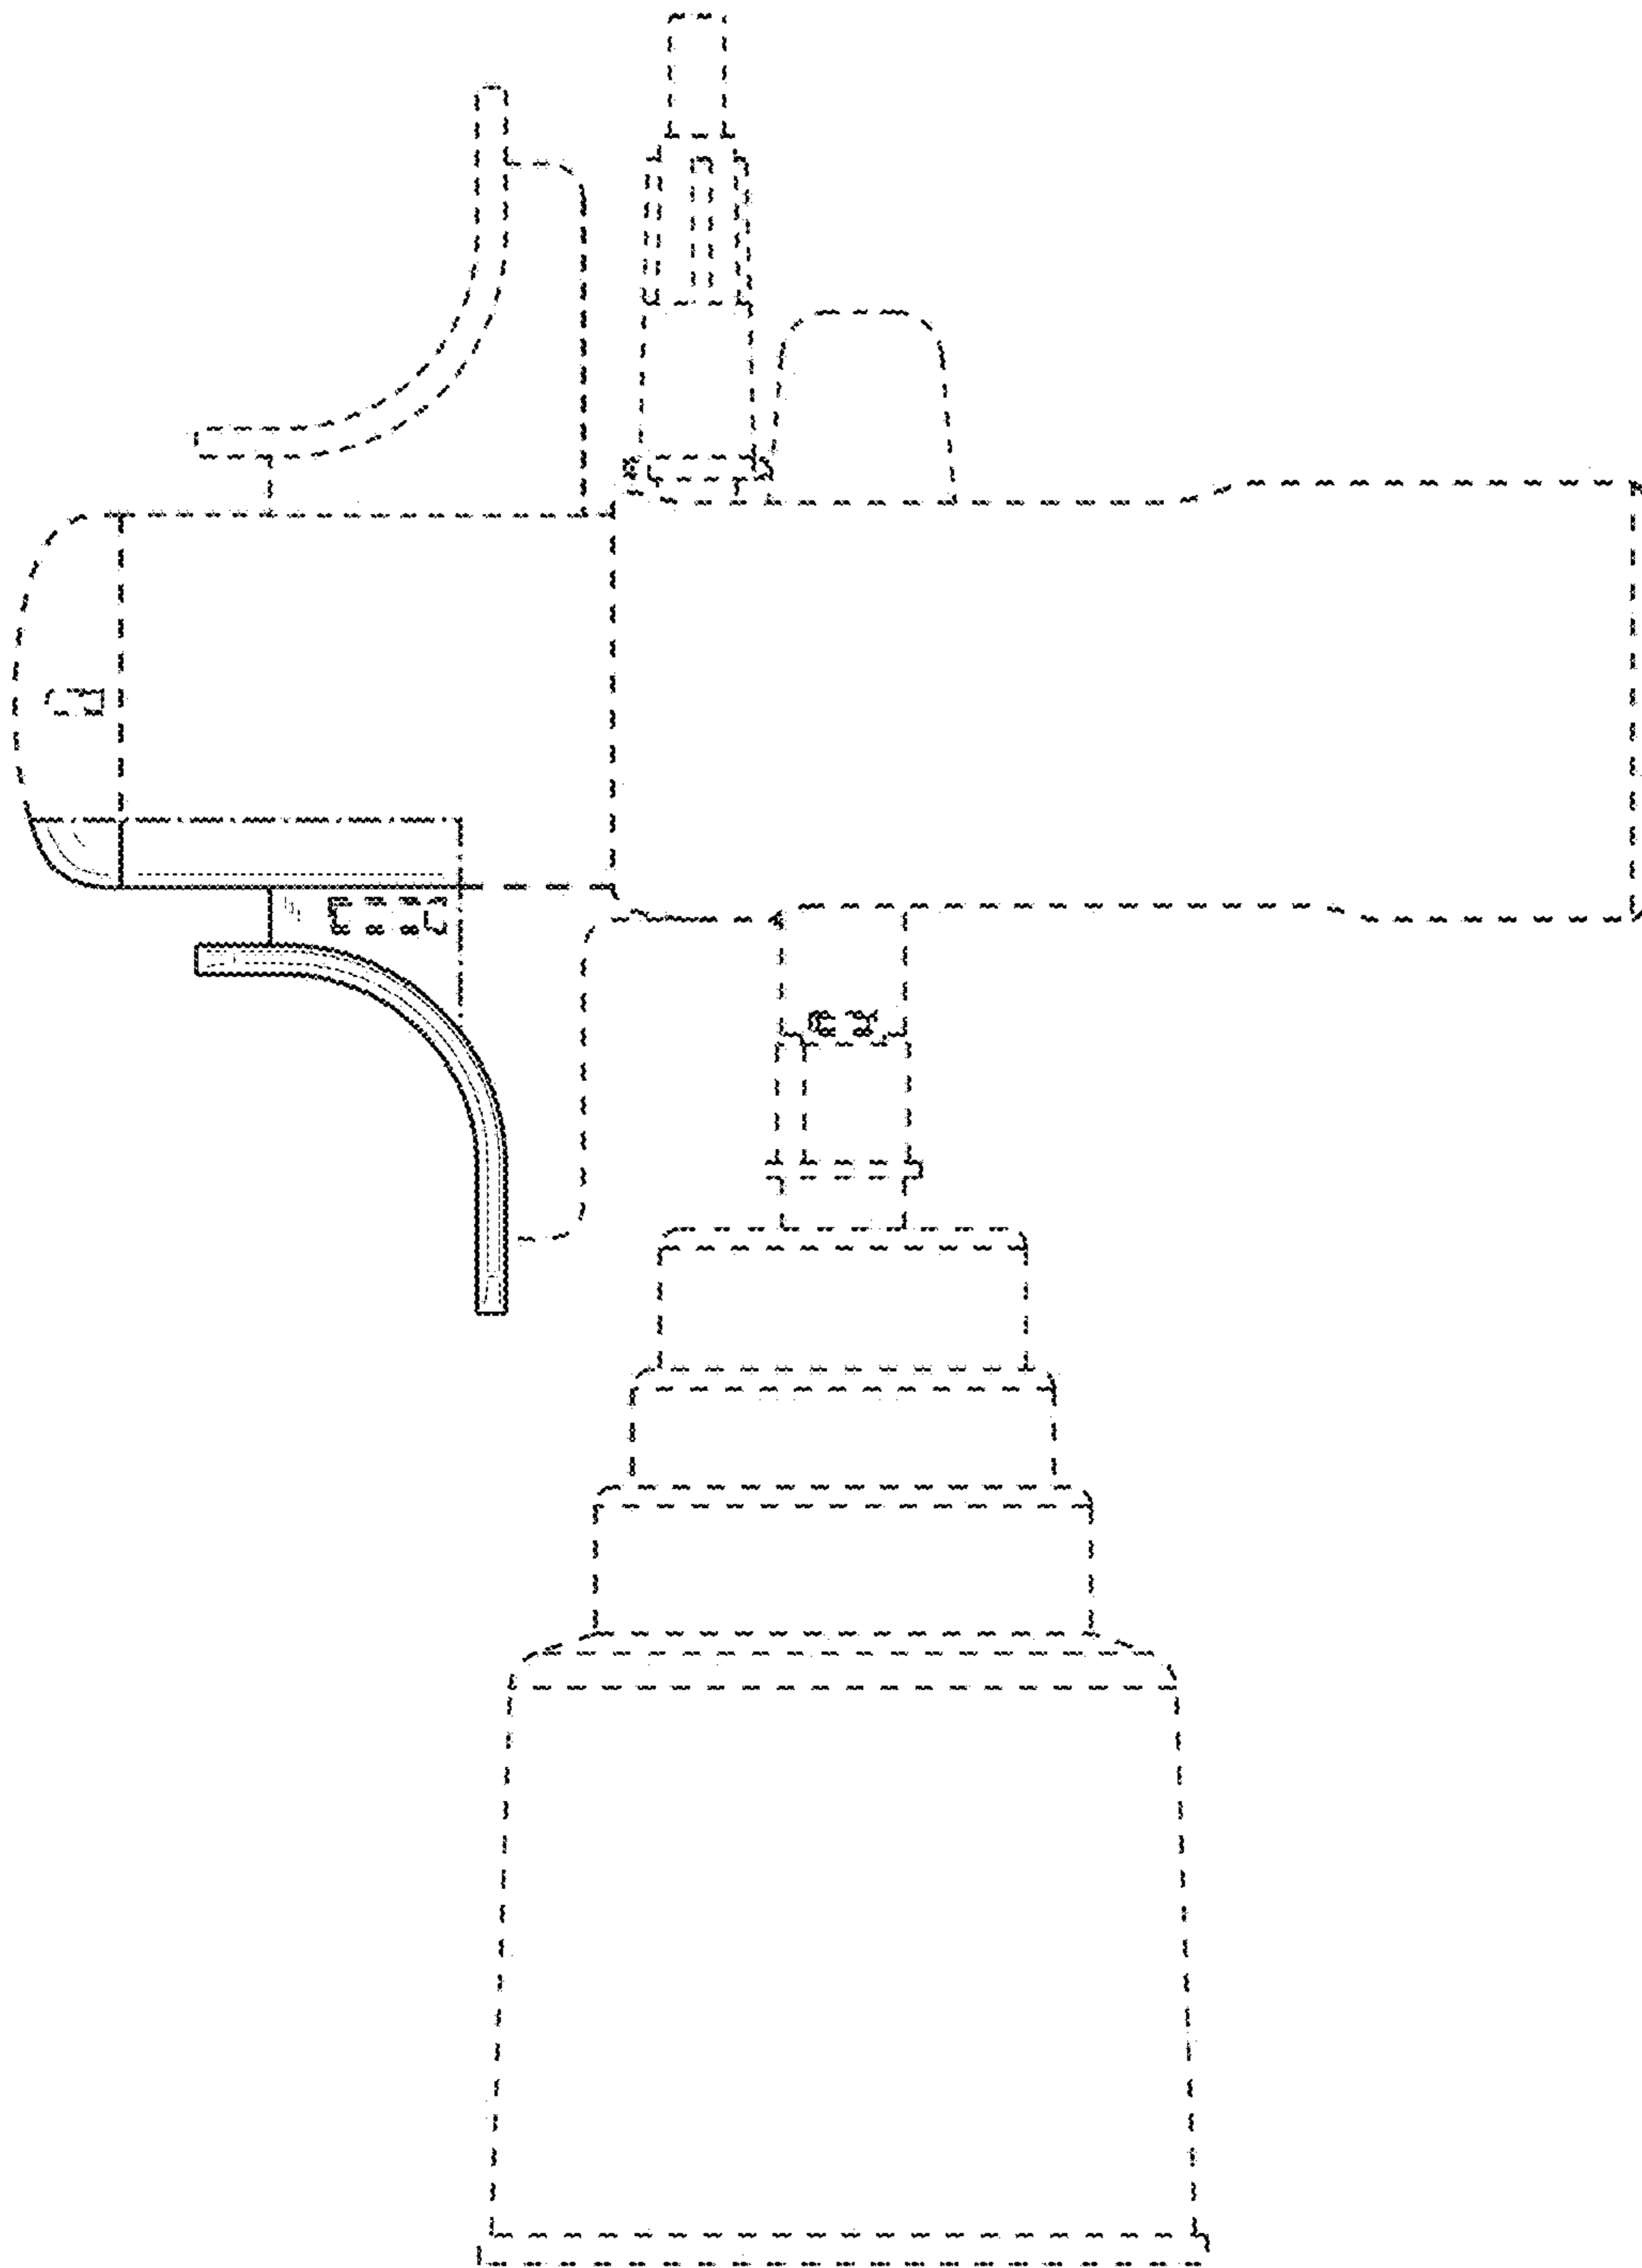


FIG. 3

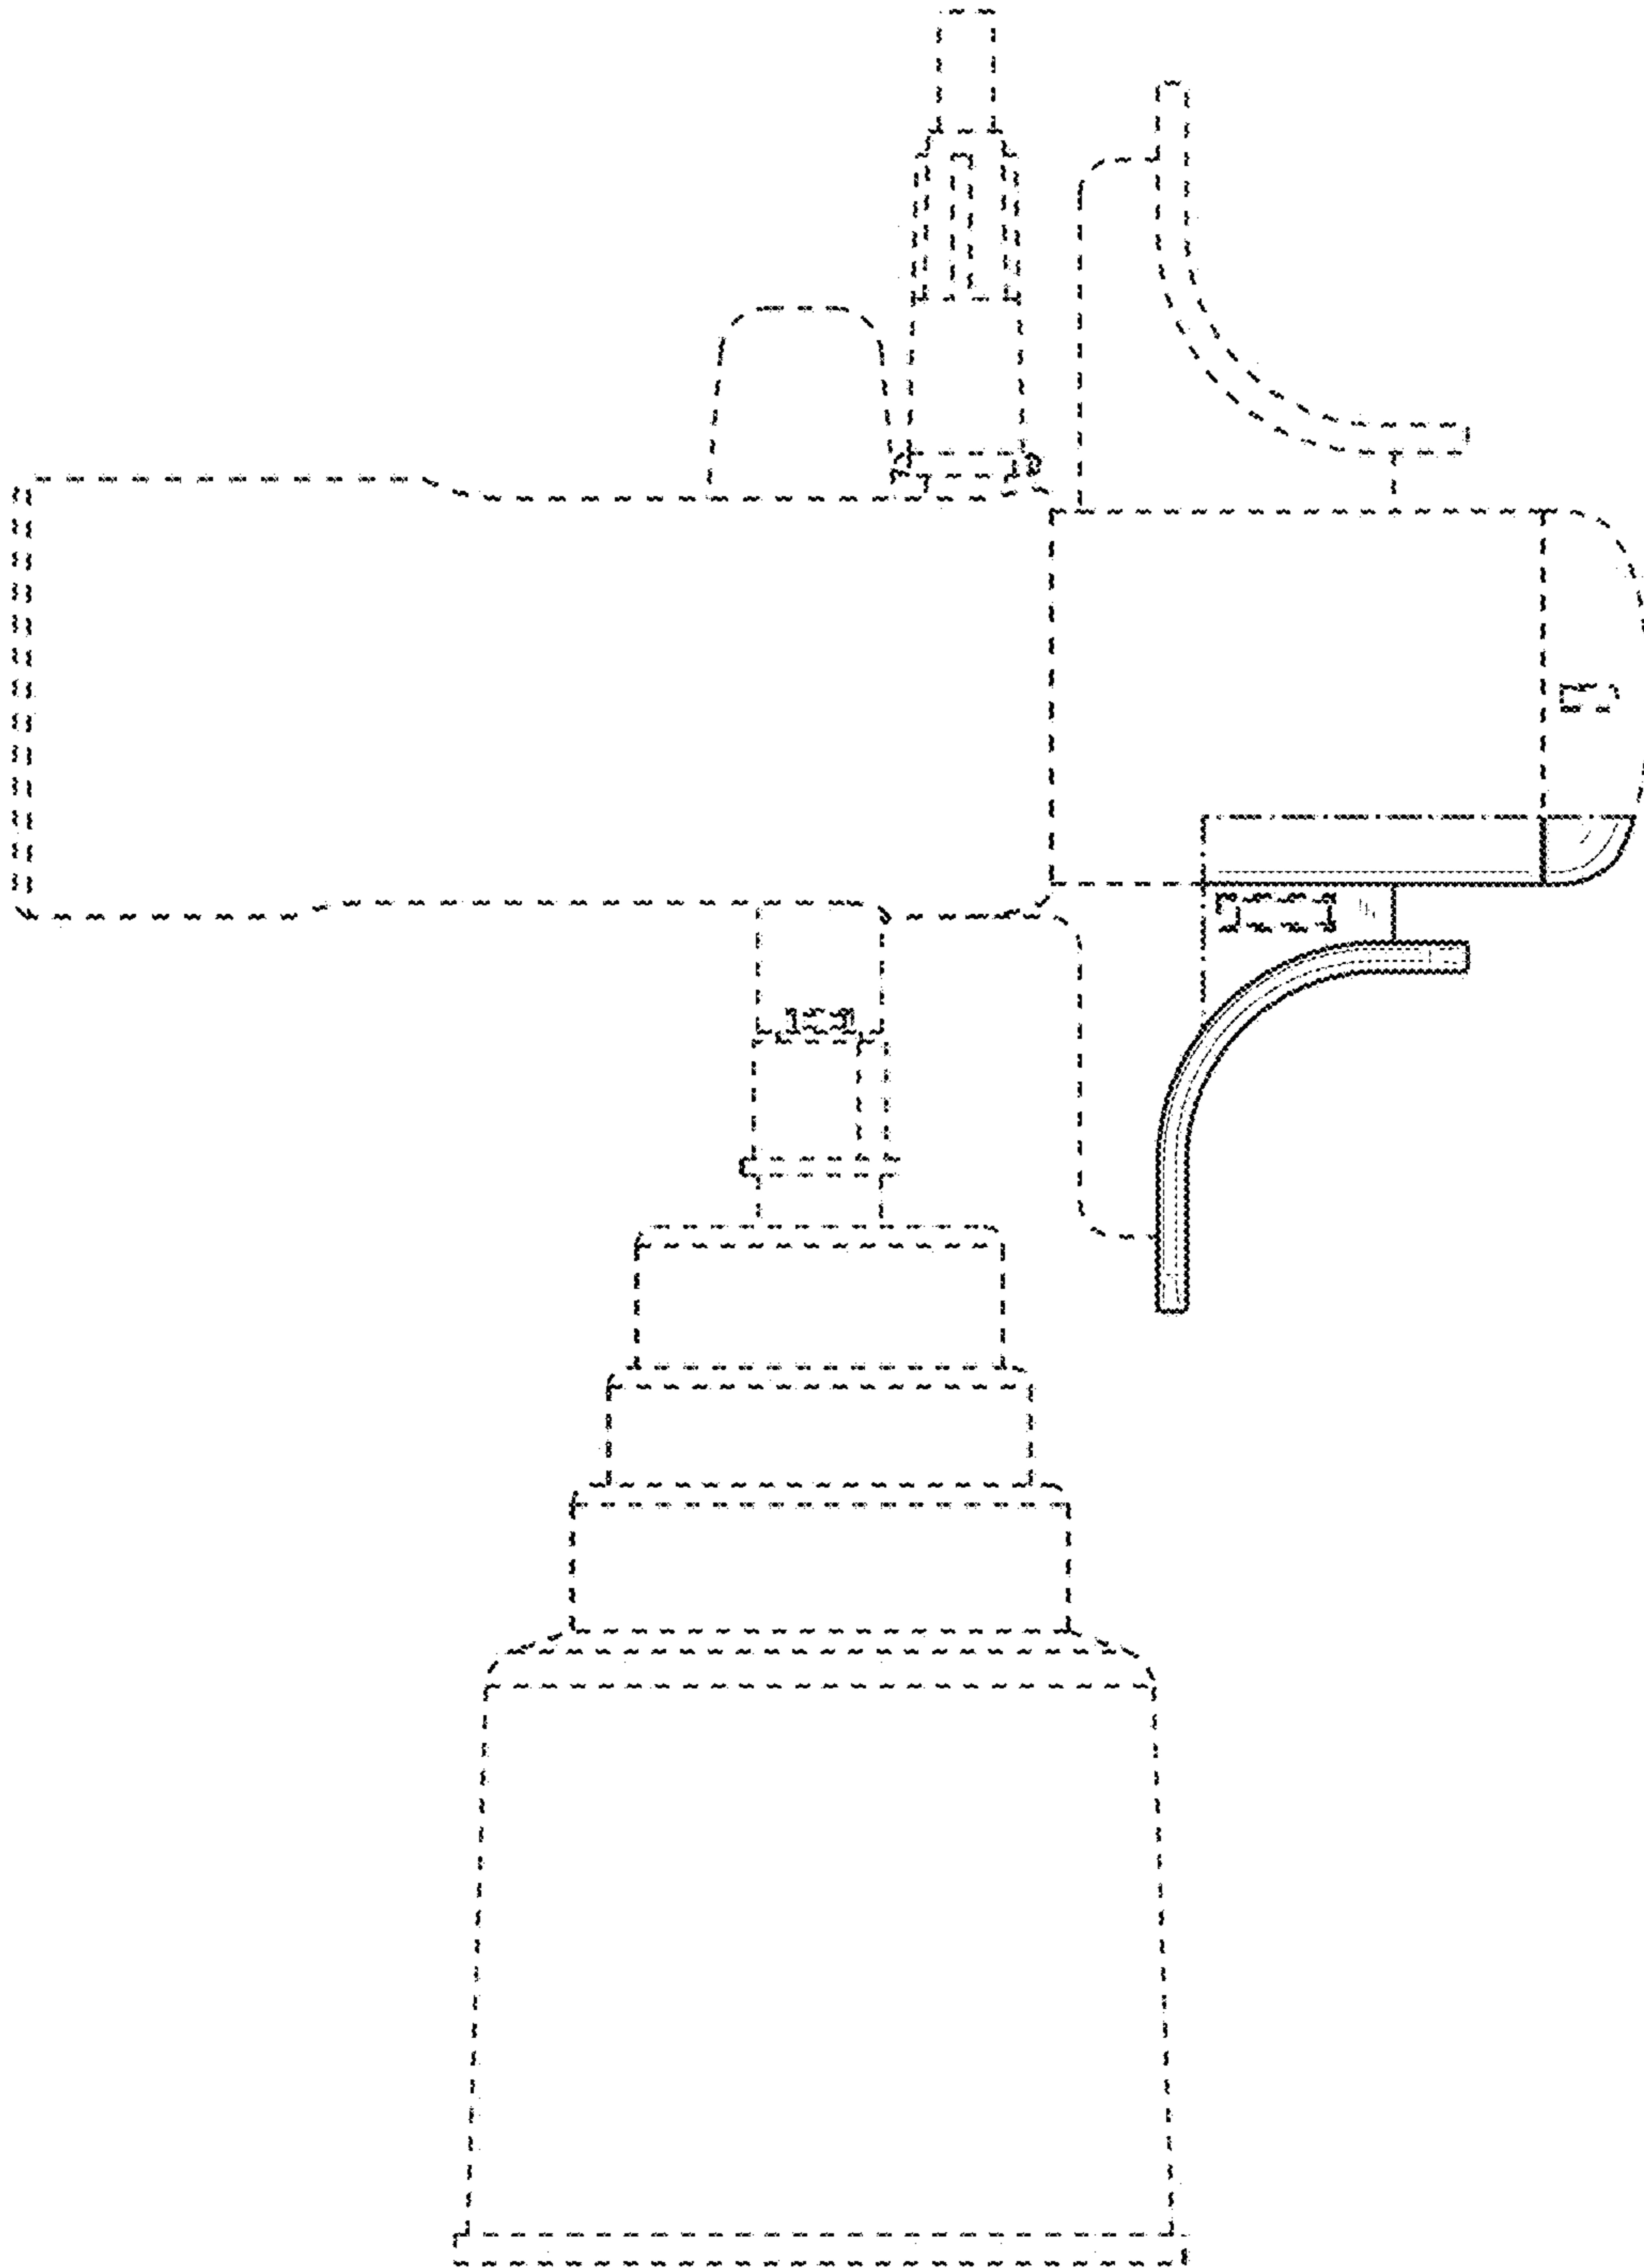


FIG. 4

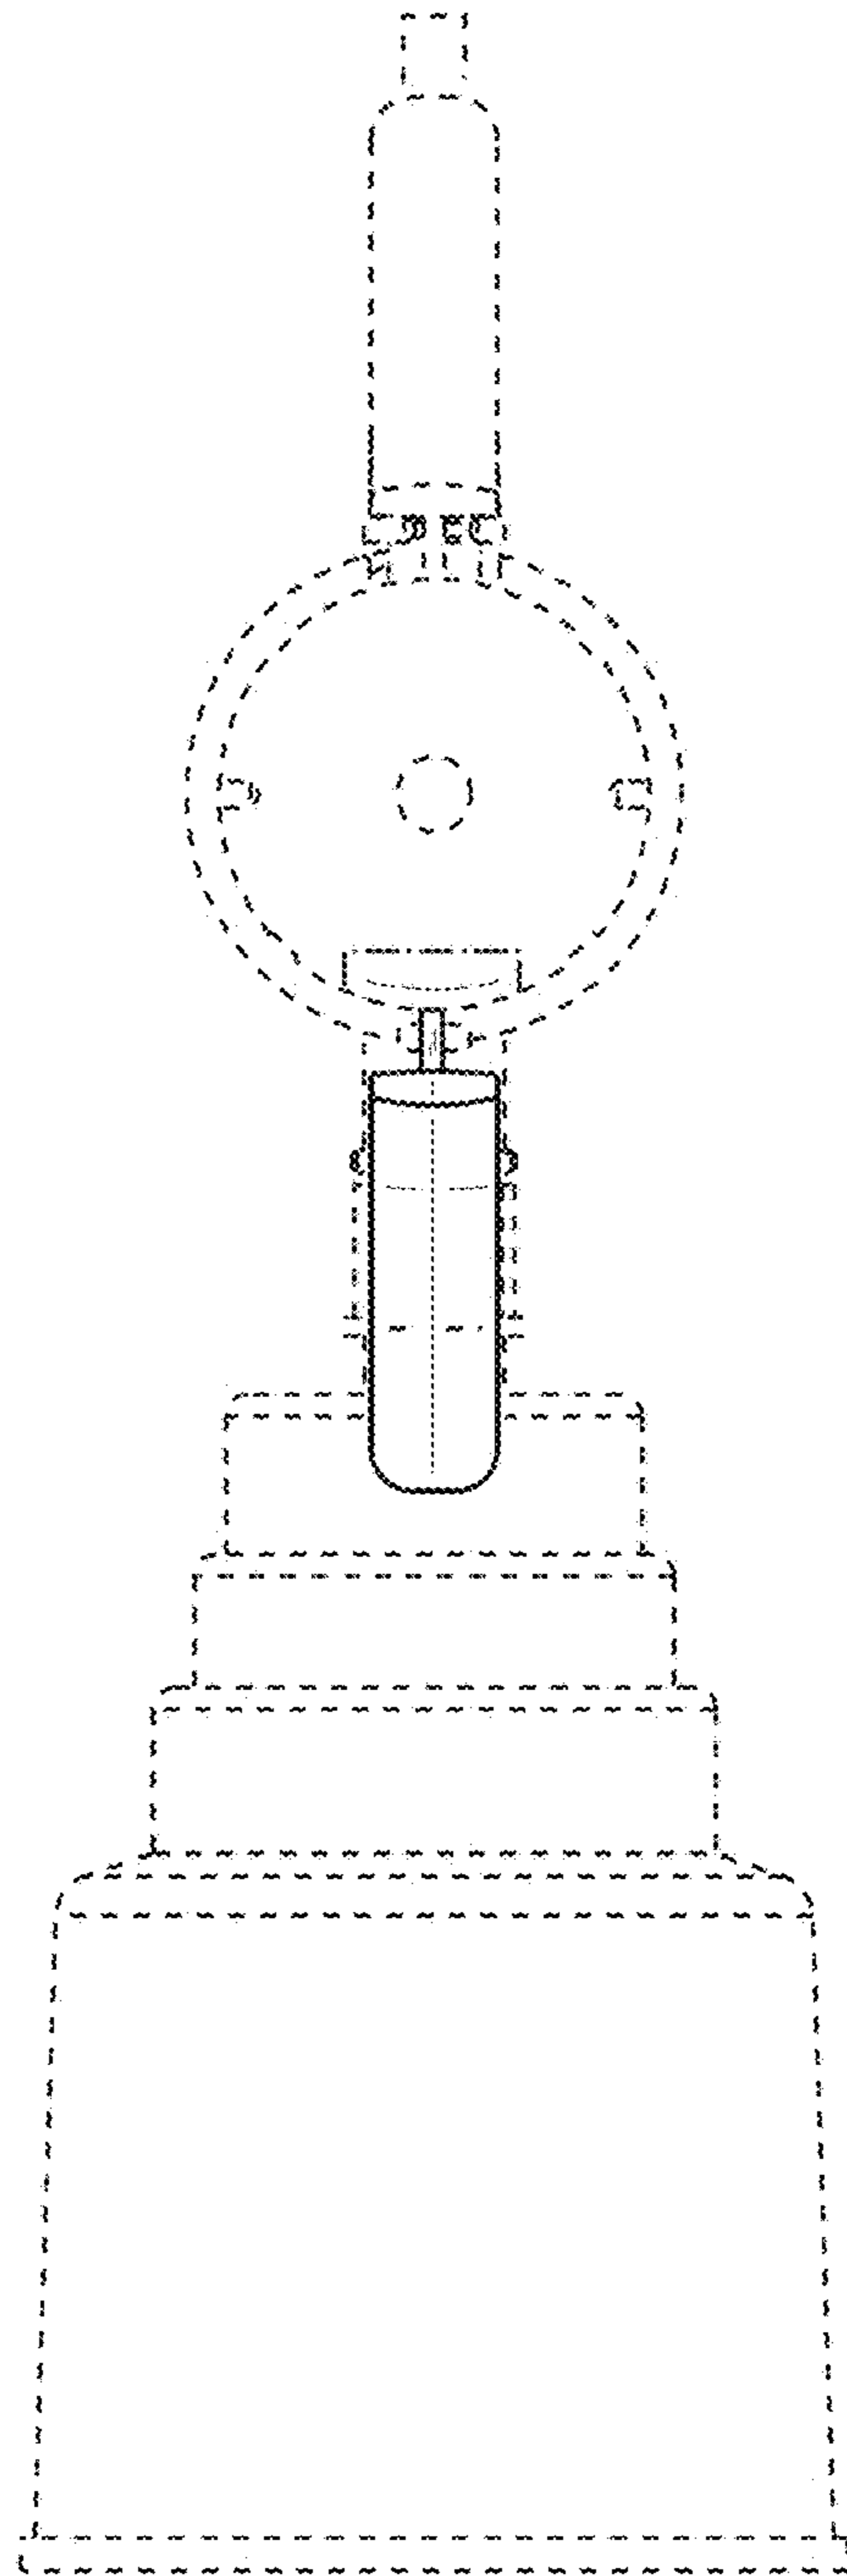


FIG. 5

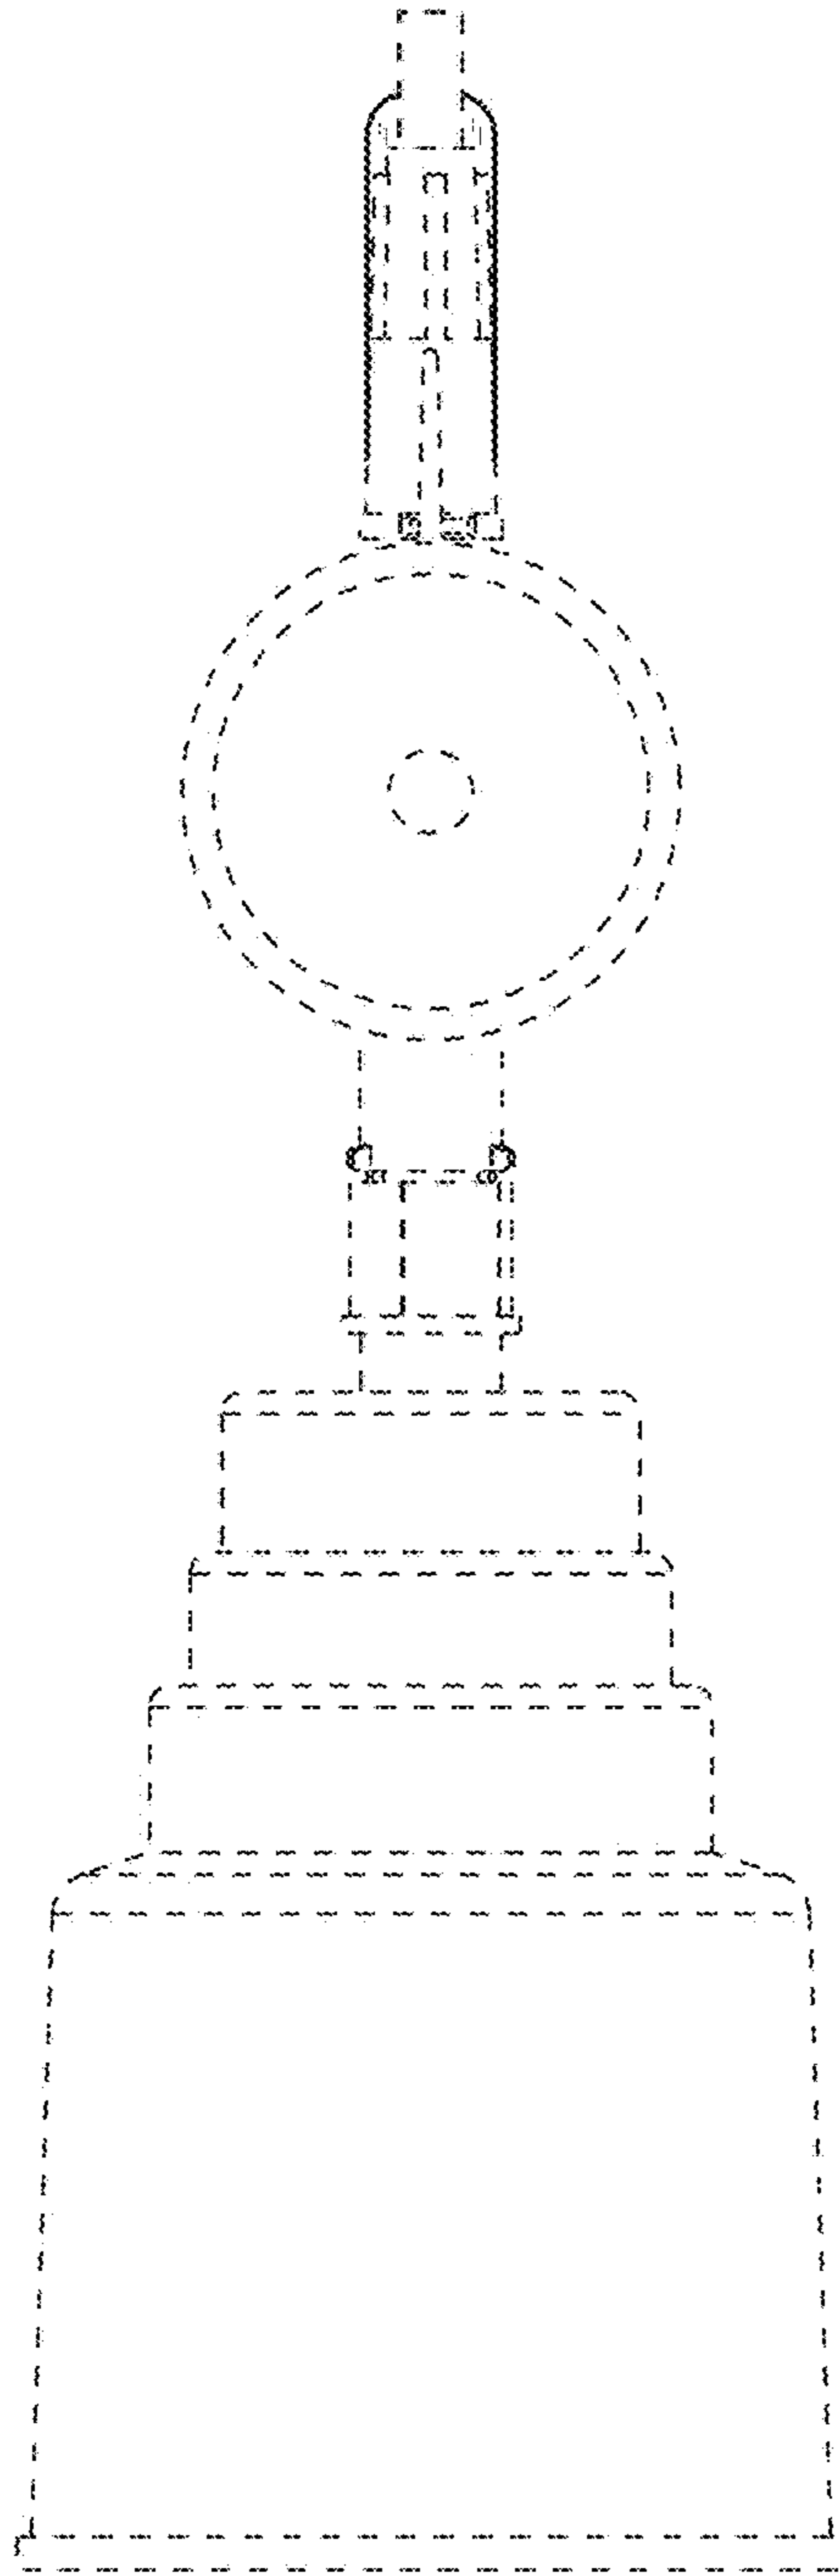


FIG. 6

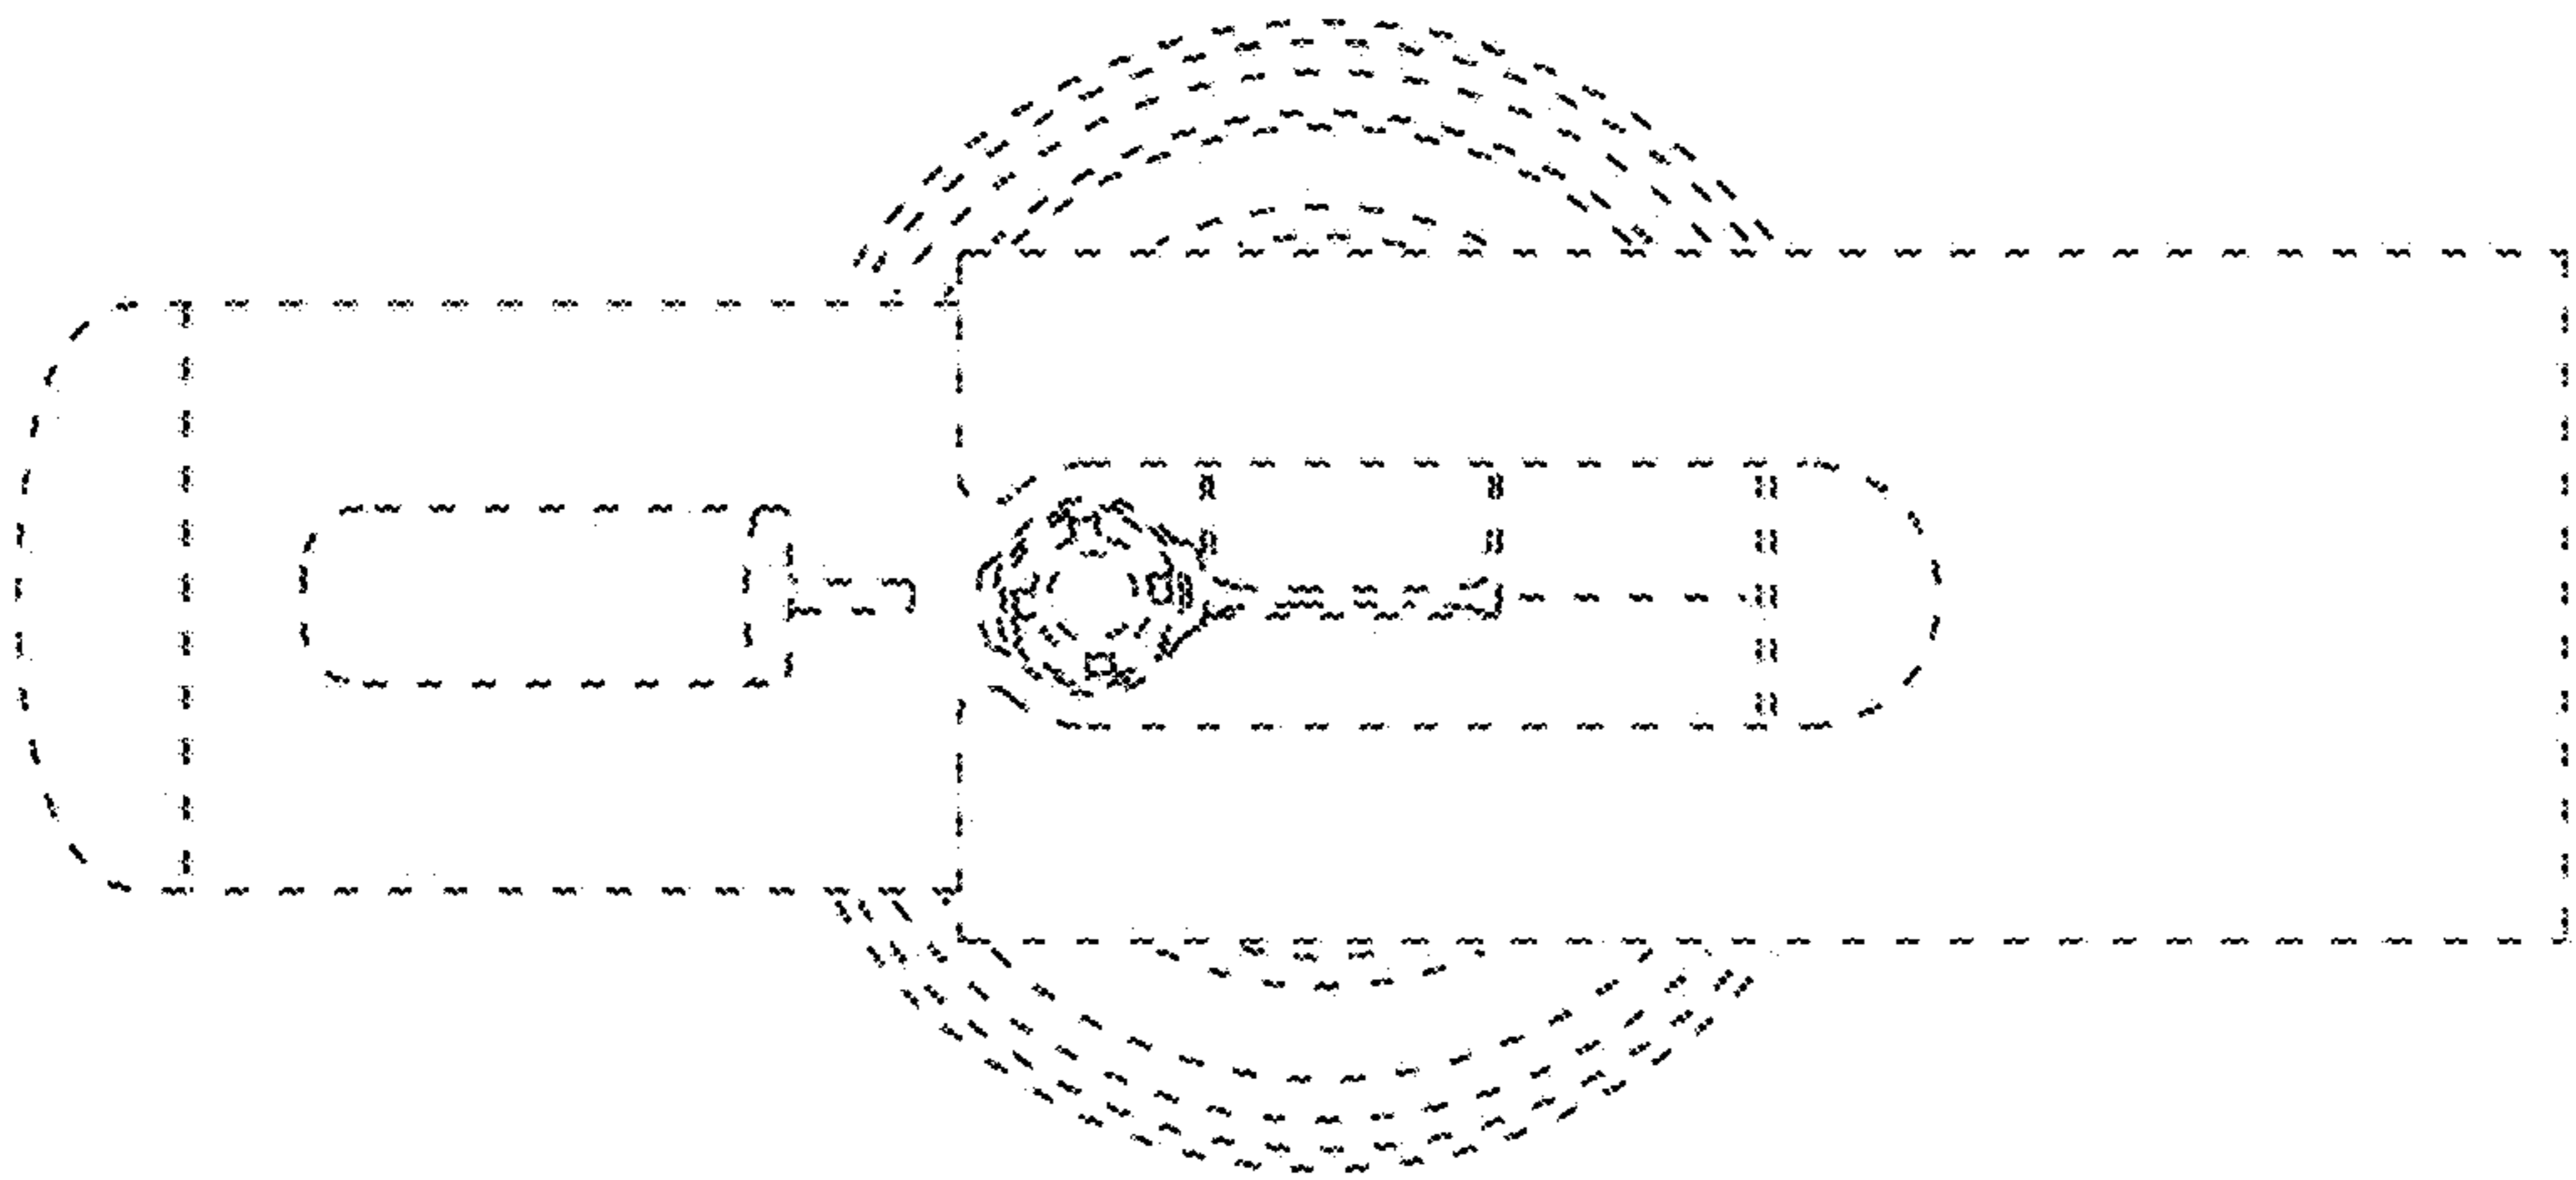


FIG. 7

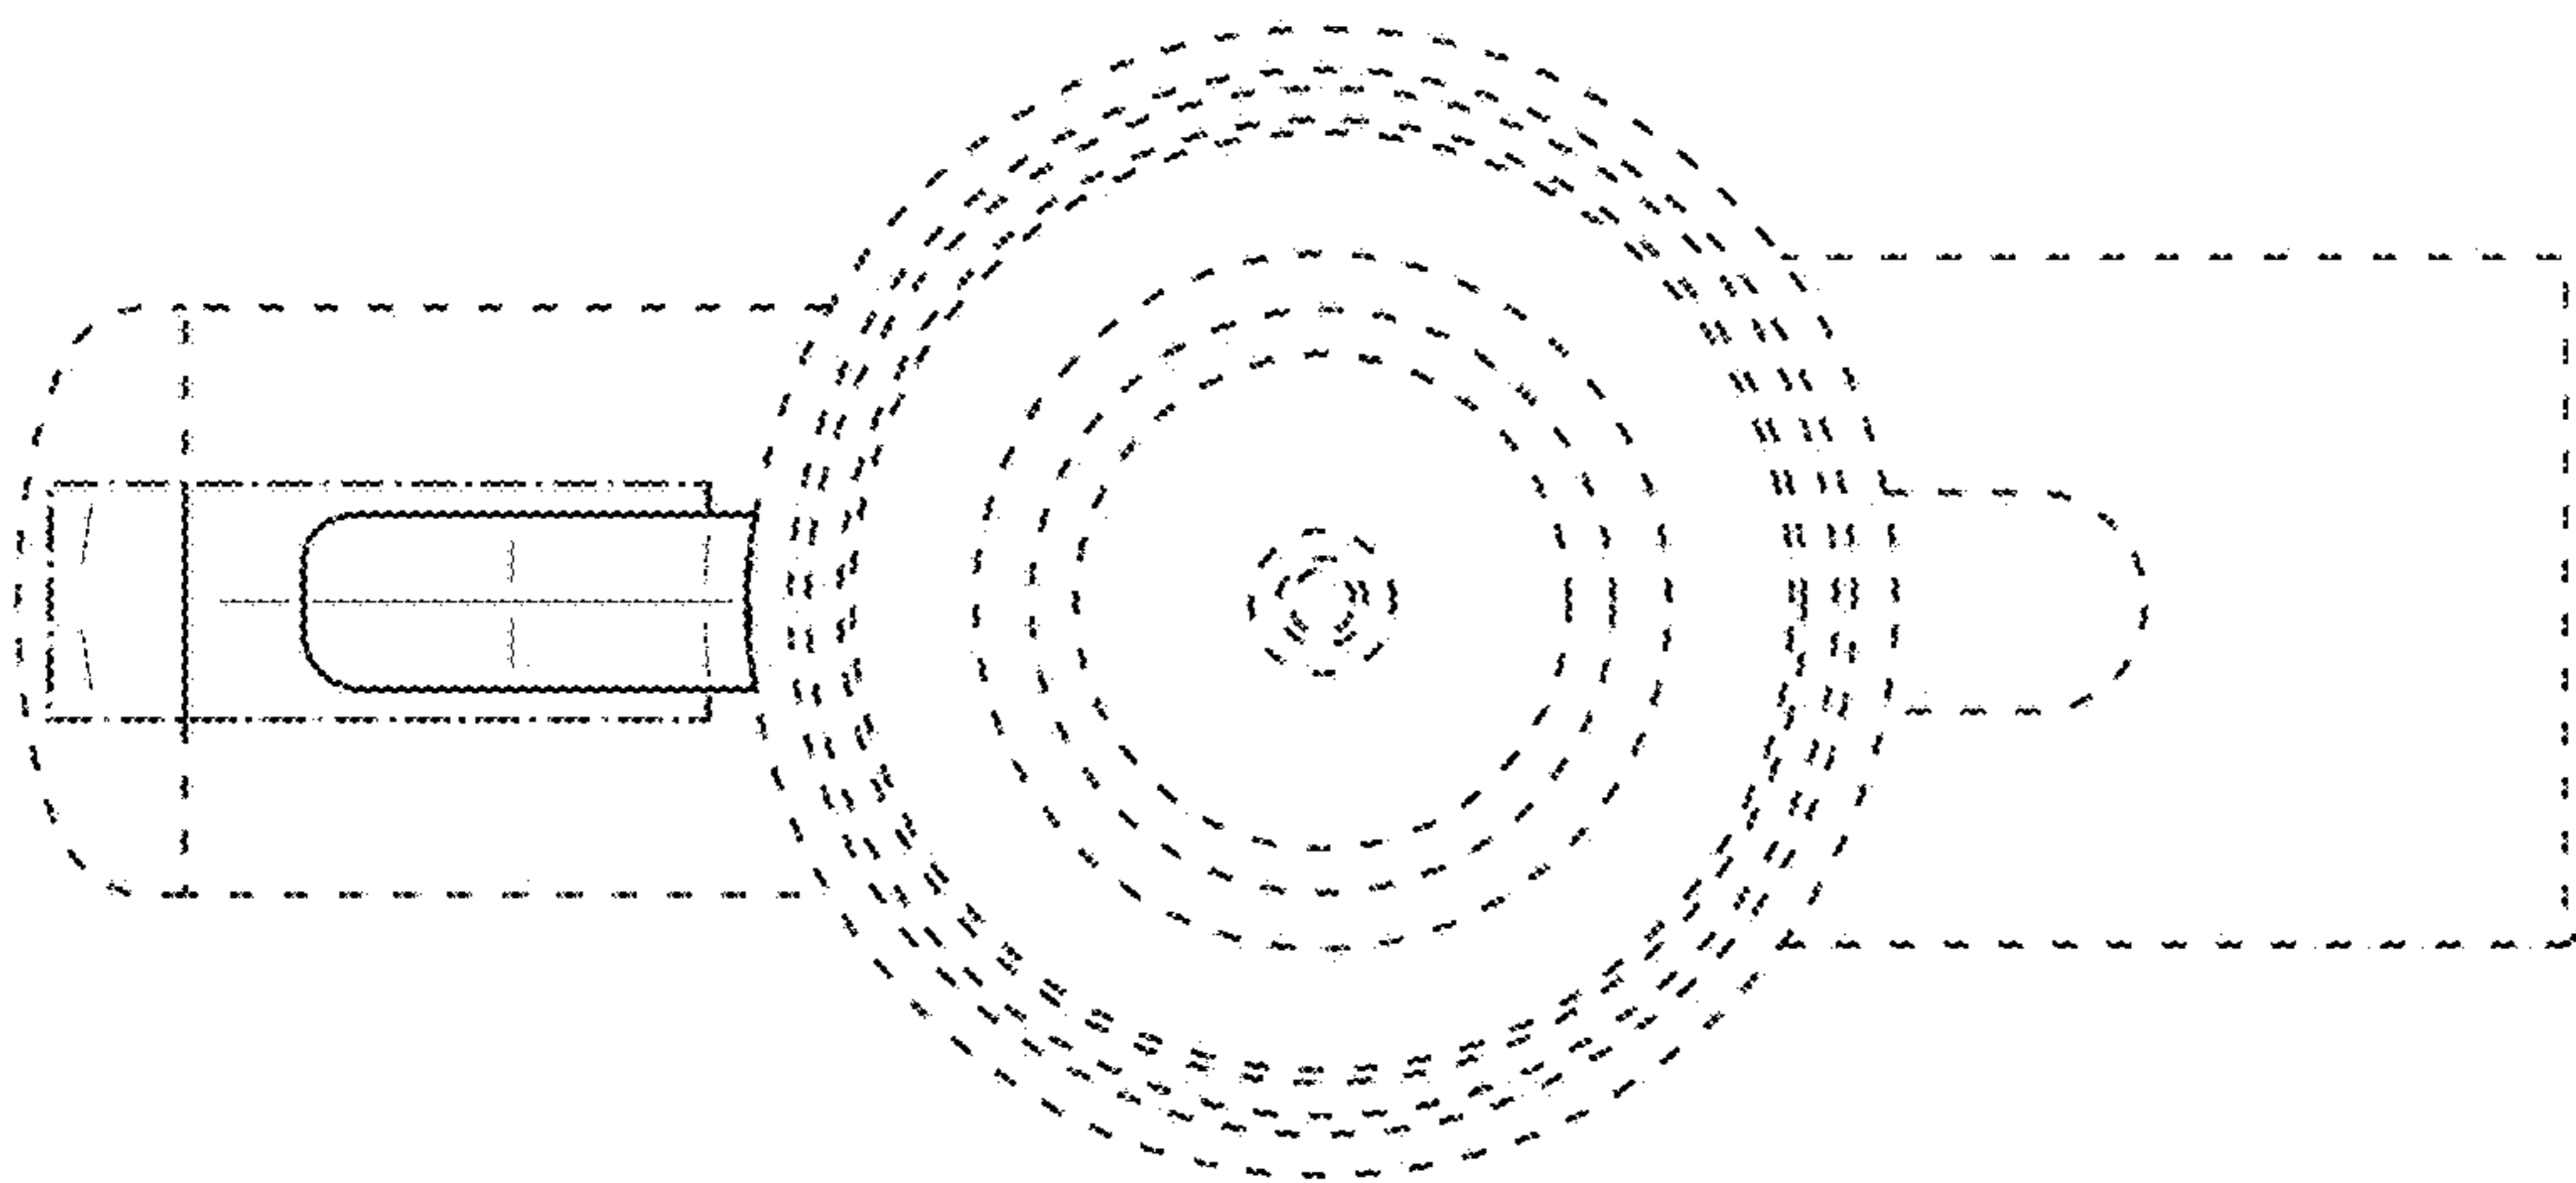


FIG. 8