



US00D842482S

(12) **United States Design Patent** (10) **Patent No.:** **US D842,482 S**
Harada (45) **Date of Patent:** **** Mar. 5, 2019**

(54) **PROBE FOR AN ULTRASONIC DIAGNOSIS APPARATUS**

(71) Applicant: **Canon Medical Systems Corporation**,
Otagawa-shi, Tochigi (JP)

(72) Inventor: **Rika Harada**, Tokyo (JP)

(73) Assignee: **Canon Medical Systems Corporation**,
Otagawa-shi (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/609,406**

(22) Filed: **Jun. 30, 2017**

(30) **Foreign Application Priority Data**

Mar. 30, 2017 (JP) 2017-006582

Mar. 30, 2017 (JP) 2017-006584

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/133, 137, 138, 141, 158, 160, 164,
D24/165, 167, 170, 186-187, 200;
D10/57, 60, 78, 80

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D387,867 S * 12/1997 Henderson D24/187
6,436,050 B2 * 8/2002 Garrison B25F 5/02
600/459

(Continued)

FOREIGN PATENT DOCUMENTS

CN 302791147 4/2014
CN 201530319422 * 8/2015

(Continued)

OTHER PUBLICATIONS

3CRF Ultrasound Probe/Transducer. Online, published date unknown.
Retrieved on Sep. 10, 2018 from URL: <https://one-self.gehealthcare.co.uk/gehcstorefront/p/5196216>.*

Primary Examiner — Karen S Acker

Assistant Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson,
Farabow, Garrett & Dunner LLP

(57) **CLAIM**

The ornamental design for a probe for an ultrasonic diagnosis apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view 1 of a probe for an ultrasonic diagnosis apparatus showing my new design according to a first embodiment thereof,

FIG. 2 is a perspective view 2 thereof,

FIG. 3 is a front elevational view thereof,

FIG. 4 is a rear elevational view thereof,

FIG. 5 is a top plan view thereof,

FIG. 6 is a bottom plan view thereof,

FIG. 7 is a left side elevational view thereof,

FIG. 8 is a right side elevational view thereof,

FIG. 9 is a perspective view 1 of a probe for an ultrasonic diagnosis apparatus showing my new design according to a second embodiment thereof,

FIG. 10 is a perspective view 2 thereof,

FIG. 11 is a front elevational view thereof,

FIG. 12 is a rear elevational view thereof,

FIG. 13 is a top plan view thereof,


FIG. 14 is a bottom plan view thereof,

FIG. 15 is a left side elevational view thereof; and,

FIG. 16 is a right side elevational view thereof.

The broken lines in the drawings and the areas within them depict portions of the probe for an ultrasonic diagnosis apparatus that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

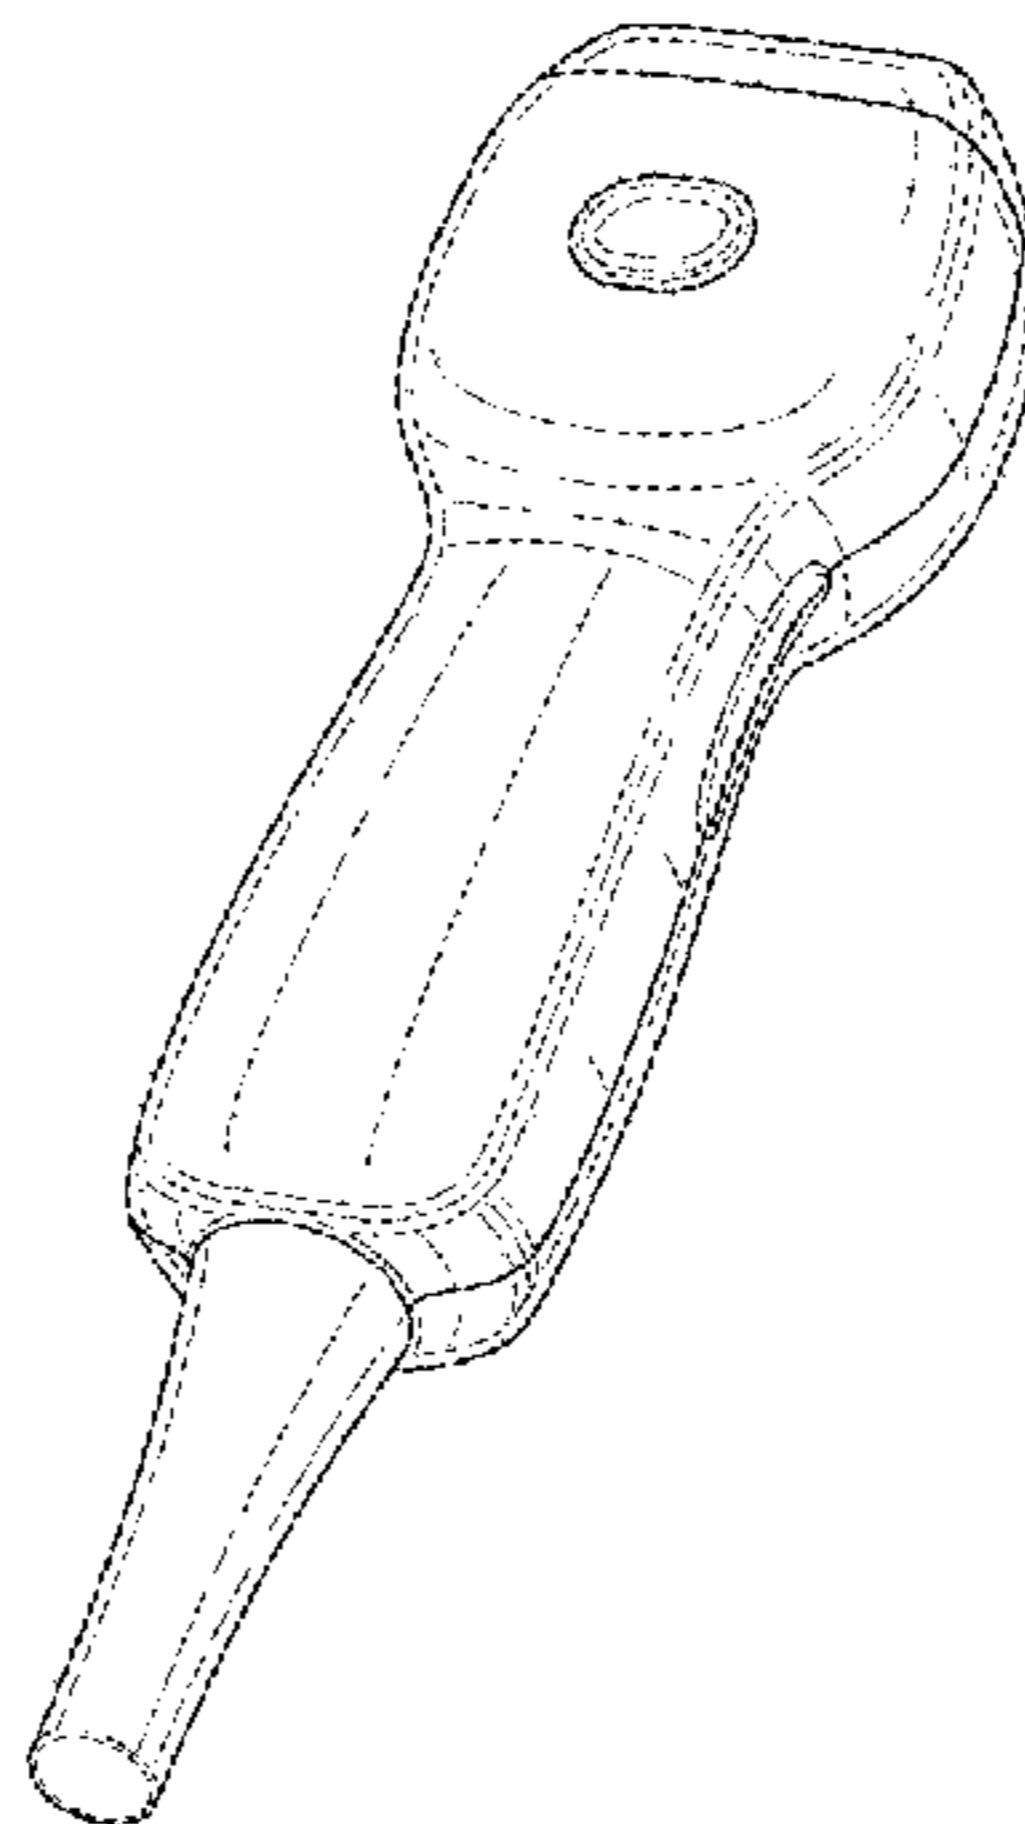

(58) **Field of Classification Search**
 CPC A61B 8/445; A61B 8/4455; A61B 8/4461;
 A61B 8/4483; A61B 8/46; A61B 5/0095
 See application file for complete search history.

D746,995 S *	1/2016	Matsumura	D24/187
D749,224 S *	2/2016	Iritani	D24/187
D754,357 S *	4/2016	Lindekugel	D24/187
D790,713 S *	6/2017	Rezzonico	D24/187
D811,606 S *	2/2018	Kitayama	D24/187
D811,607 S *	2/2018	Kitayama	D24/187
D811,608 S *	2/2018	Kitayama	D24/187
D822,837 S *	7/2018	Naka	D24/187
2015/0320402 A1*	11/2015	Ryu	A61B 8/4411 600/443

(56) **References Cited**

U.S. PATENT DOCUMENTS

D540,208 S *	4/2007	Mobley	D10/81
D545,433 S *	6/2007	Messerly	D24/158
D622,401 S *	8/2010	Suzuki	D24/186
D681,825 S	5/2013	Shinohara et al.	
D681,827 S	5/2013	Shinohara et al.	
D681,828 S	5/2013	Shinohara et al.	
D688,376 S *	8/2013	Bartlett	D24/187
D692,998 S *	11/2013	Broberg	D24/108
D703,332 S *	4/2014	Saeki	D24/187
D703,819 S *	4/2014	Moon	D24/187
D703,821 S *	4/2014	Moon	D24/187
D704,844 S	5/2014	Saeki	
D745,175 S *	12/2015	Kitayama	D24/187
D745,972 S *	12/2015	Kitayama	D24/187

FOREIGN PATENT DOCUMENTS

CN	303936878	11/2016
JP	D1128470	12/2001
JP	D1166141	2/2003
JP	D1458591	1/2013
JP	D1458933	1/2013
JP	D1499369	6/2014
JP	D1563113	11/2016
KR	30-0631494	1/2013

* cited by examiner

Fig. 1

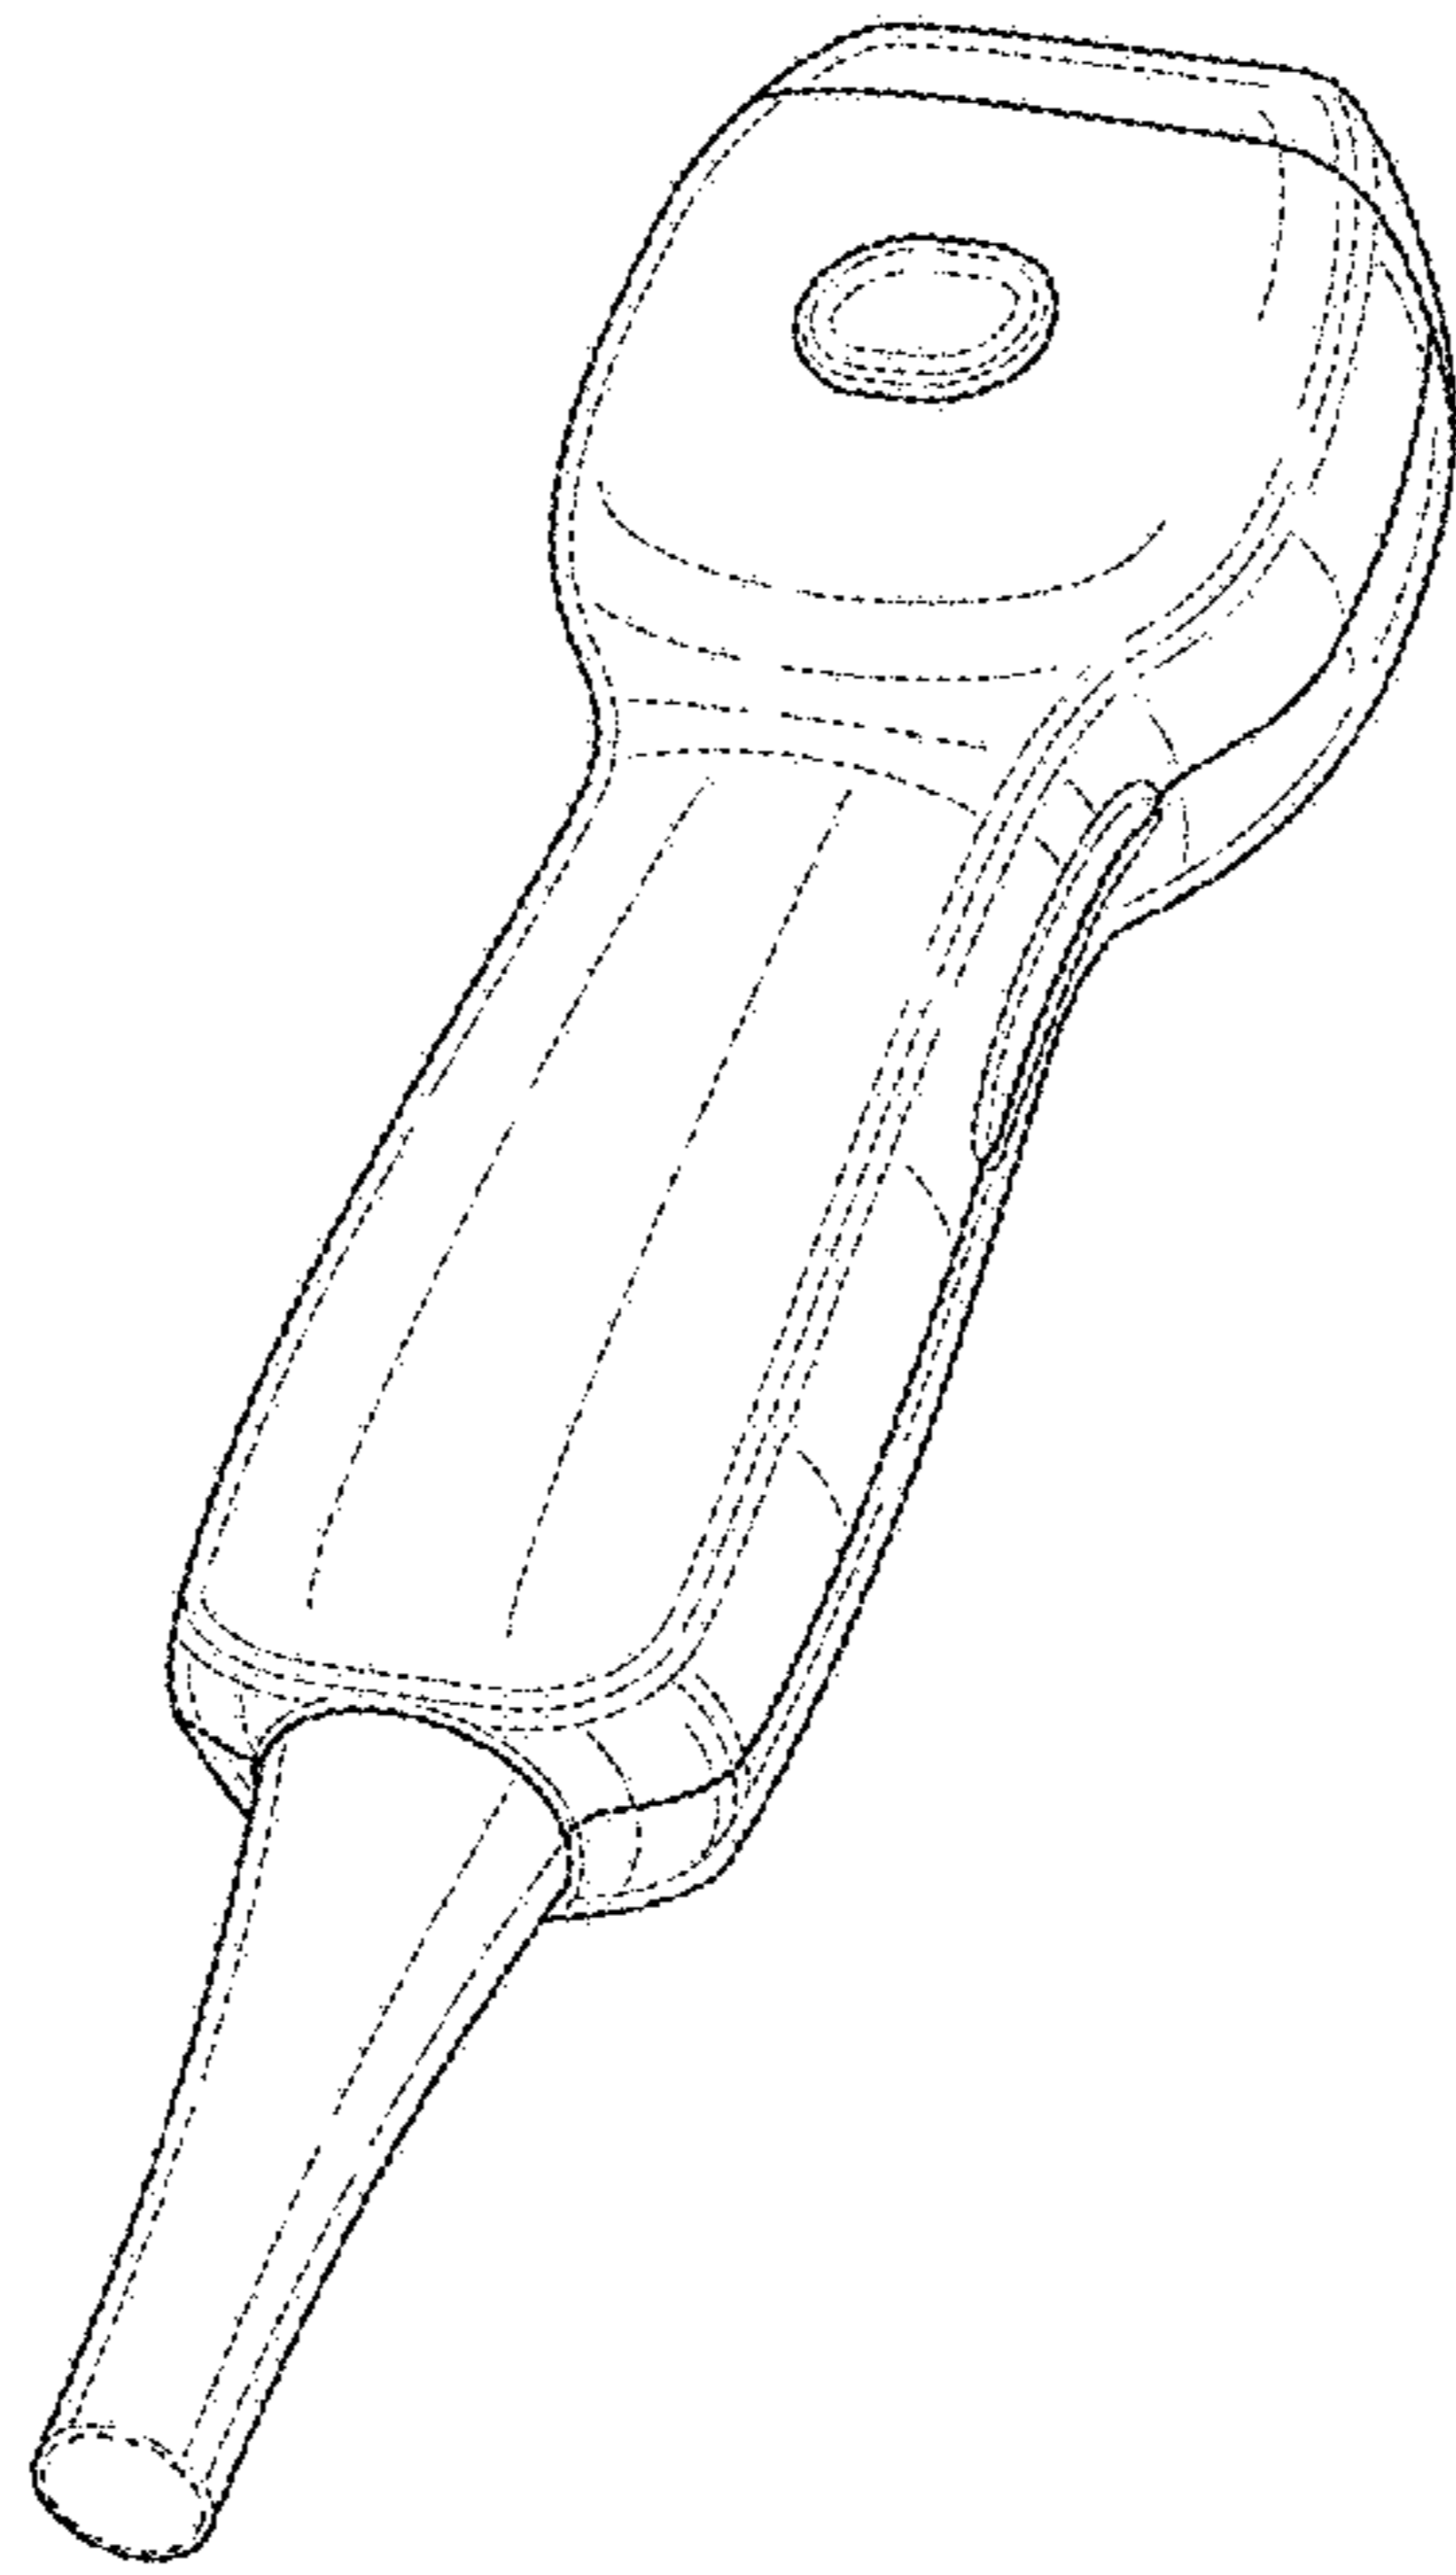


Fig. 2

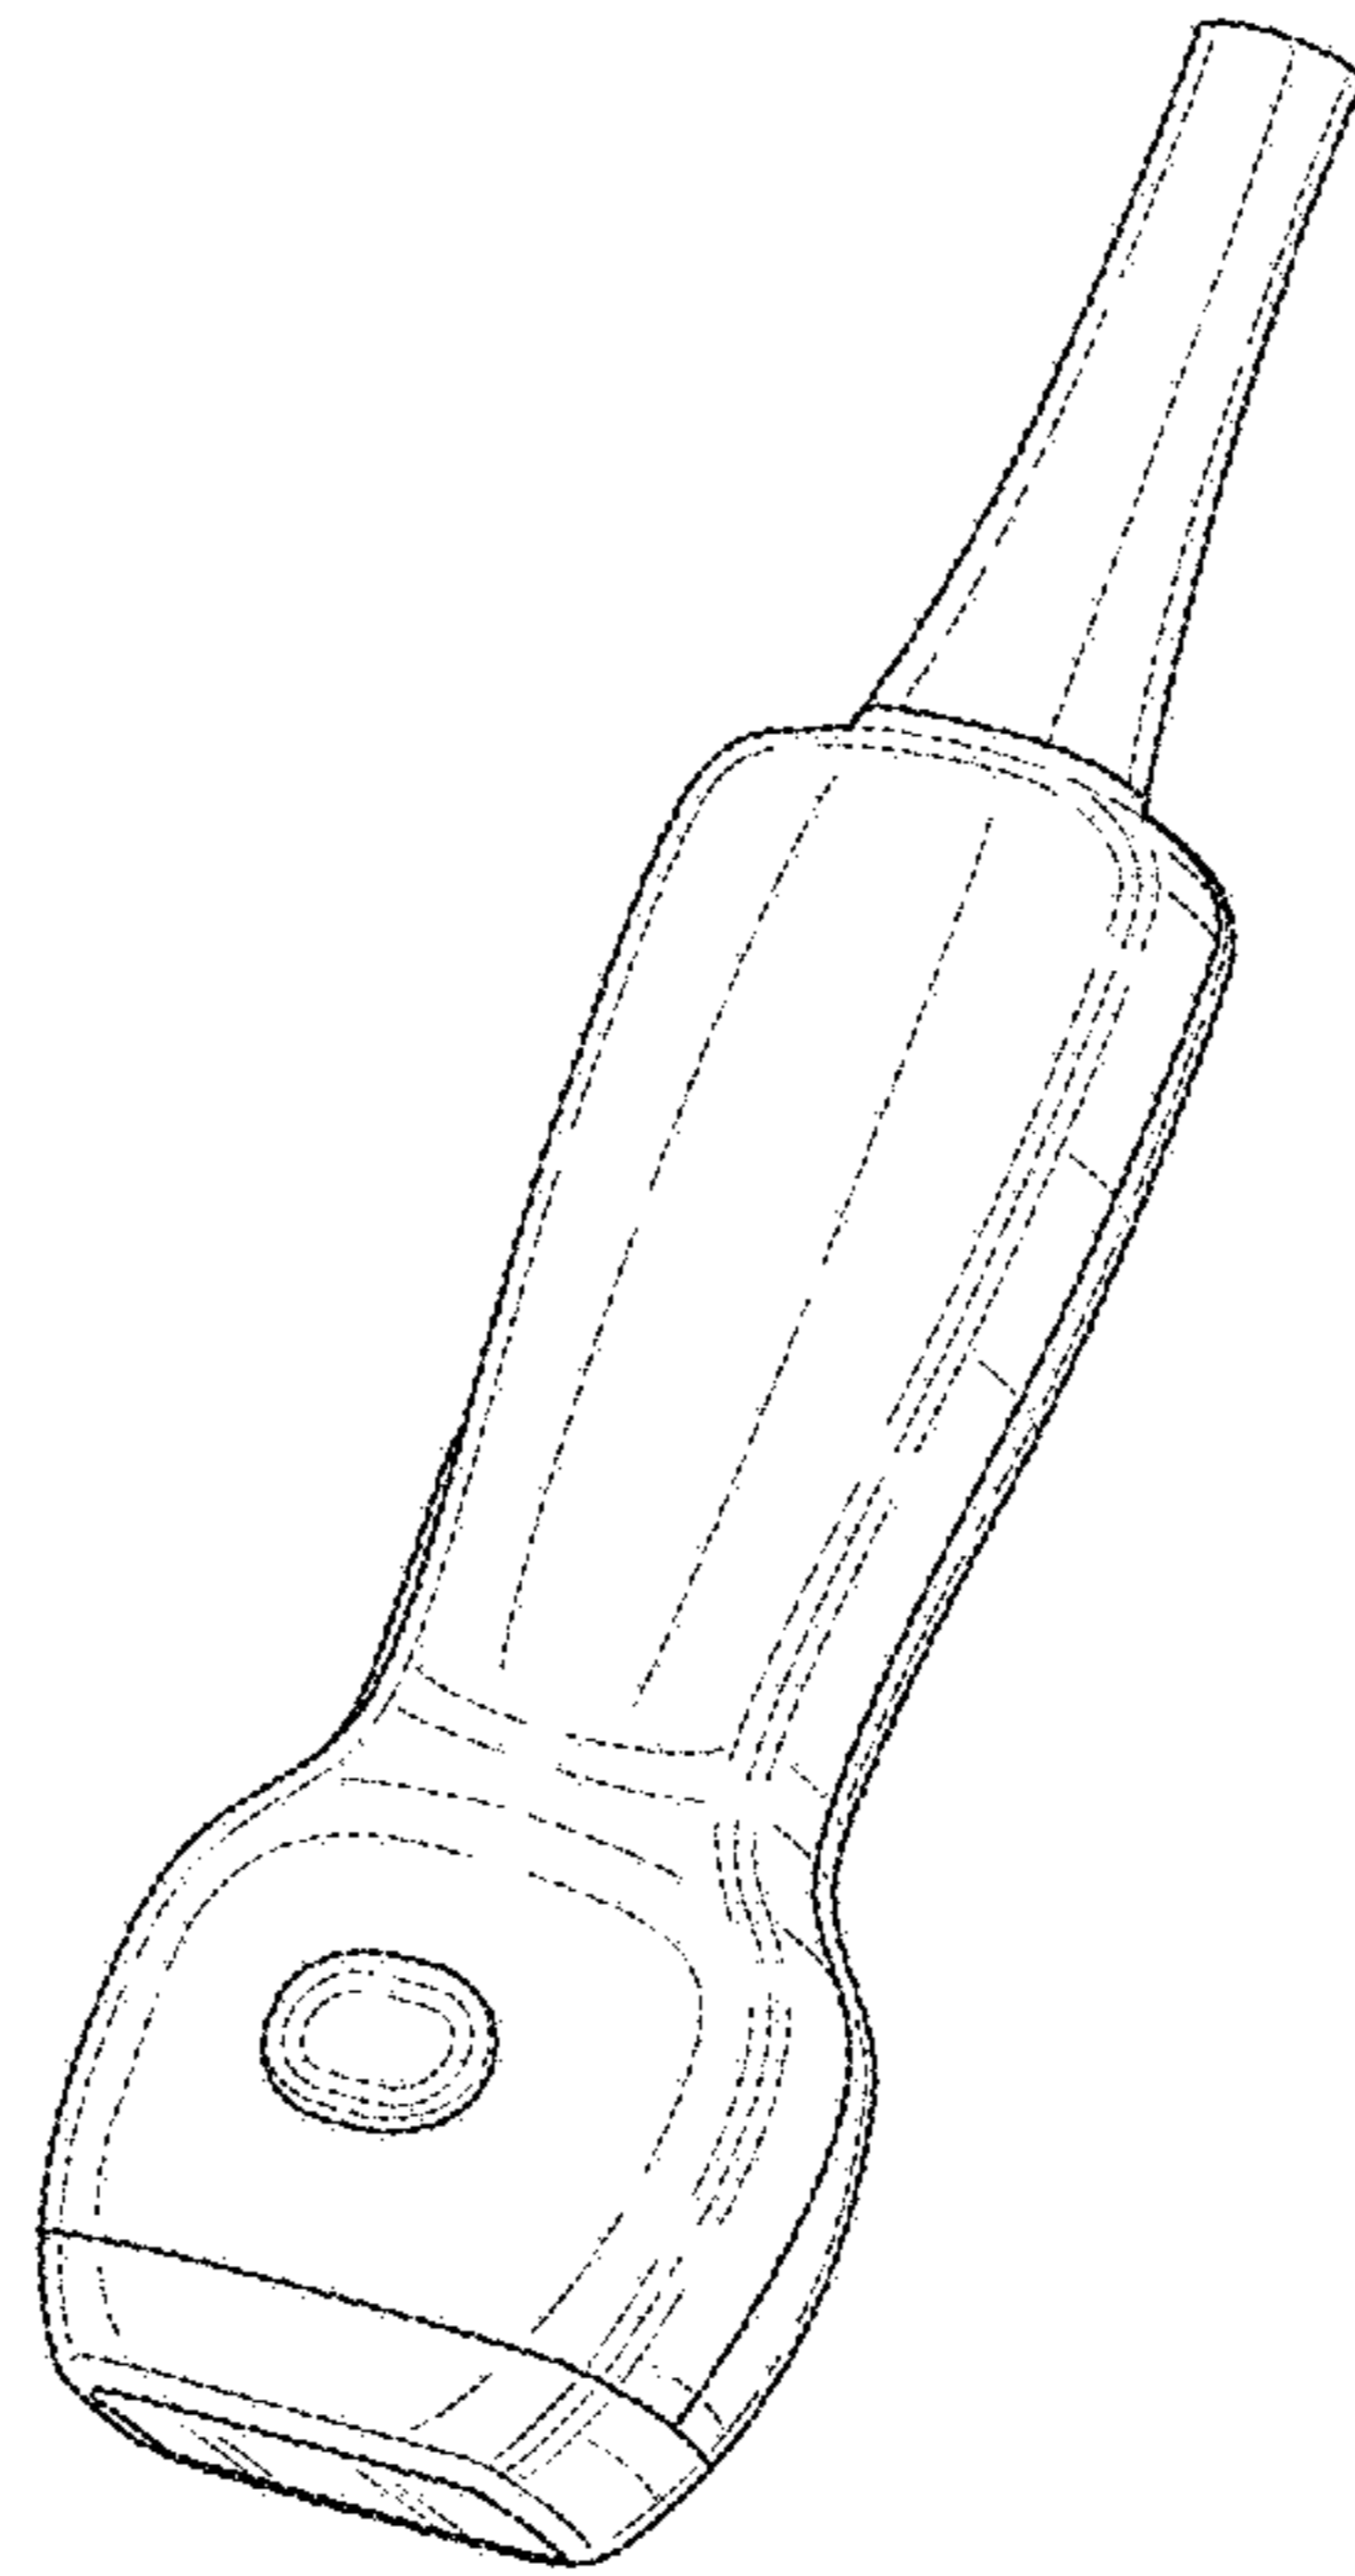


Fig. 3

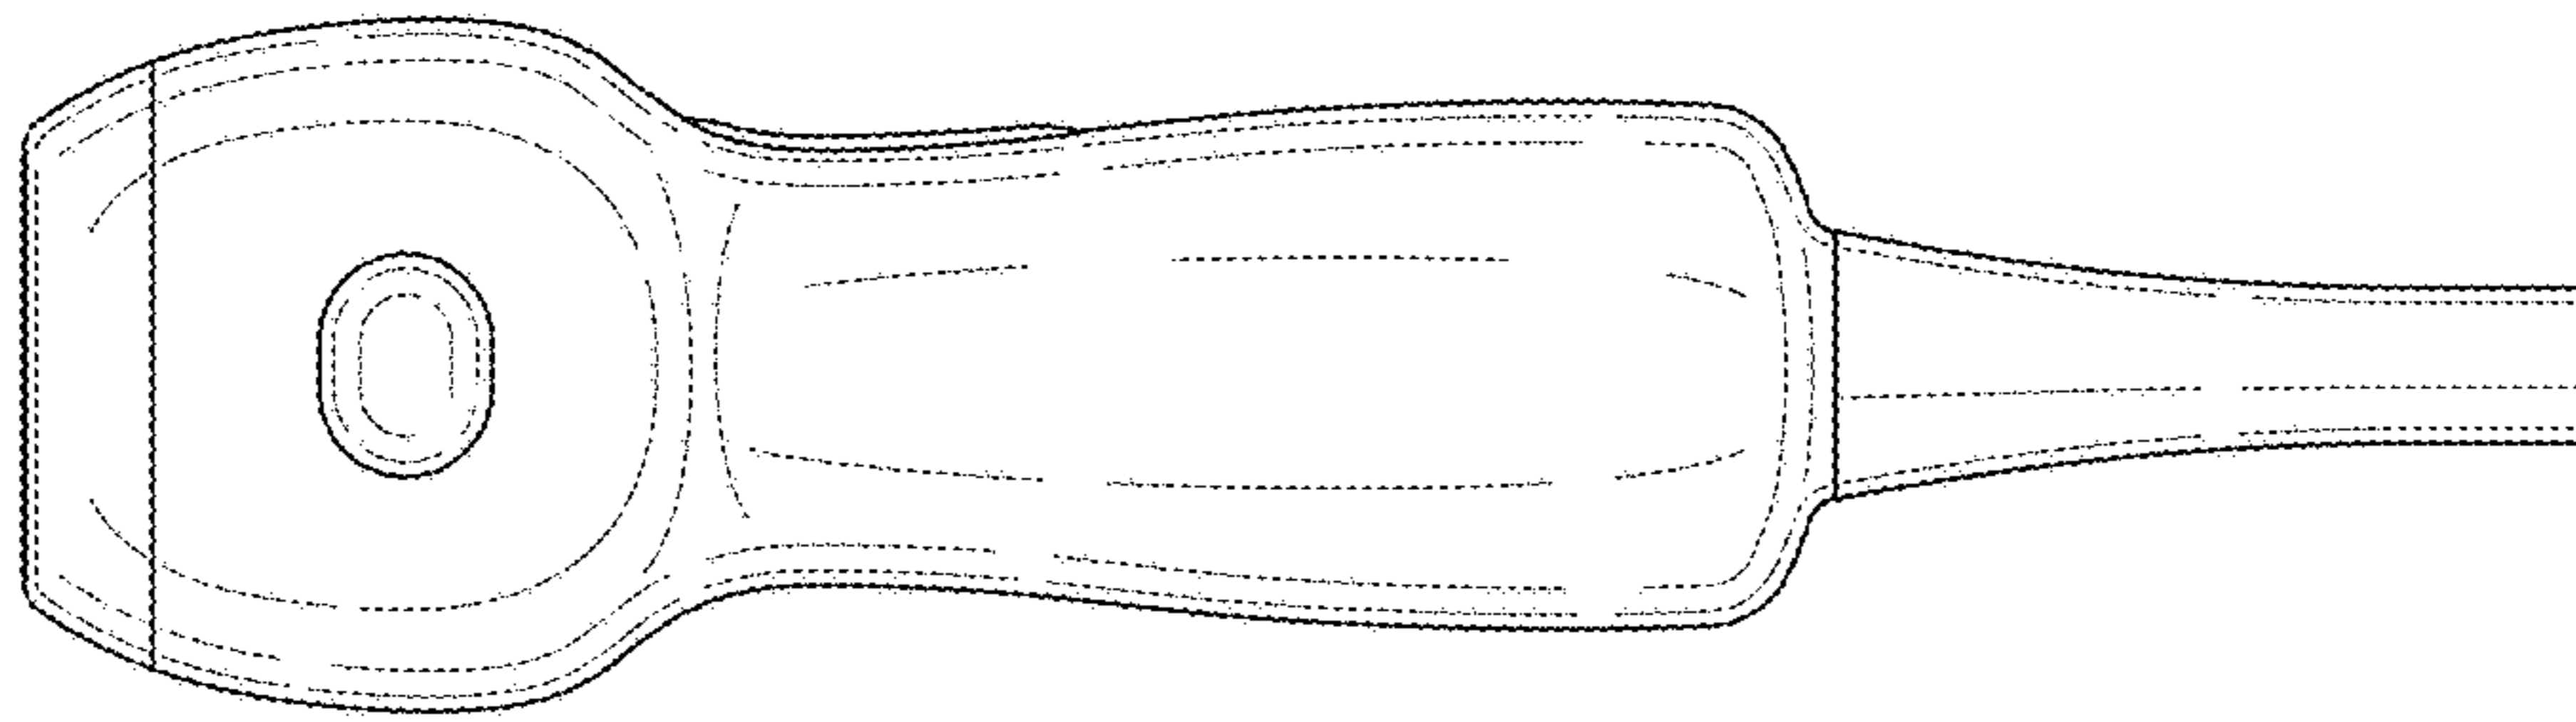


Fig. 4

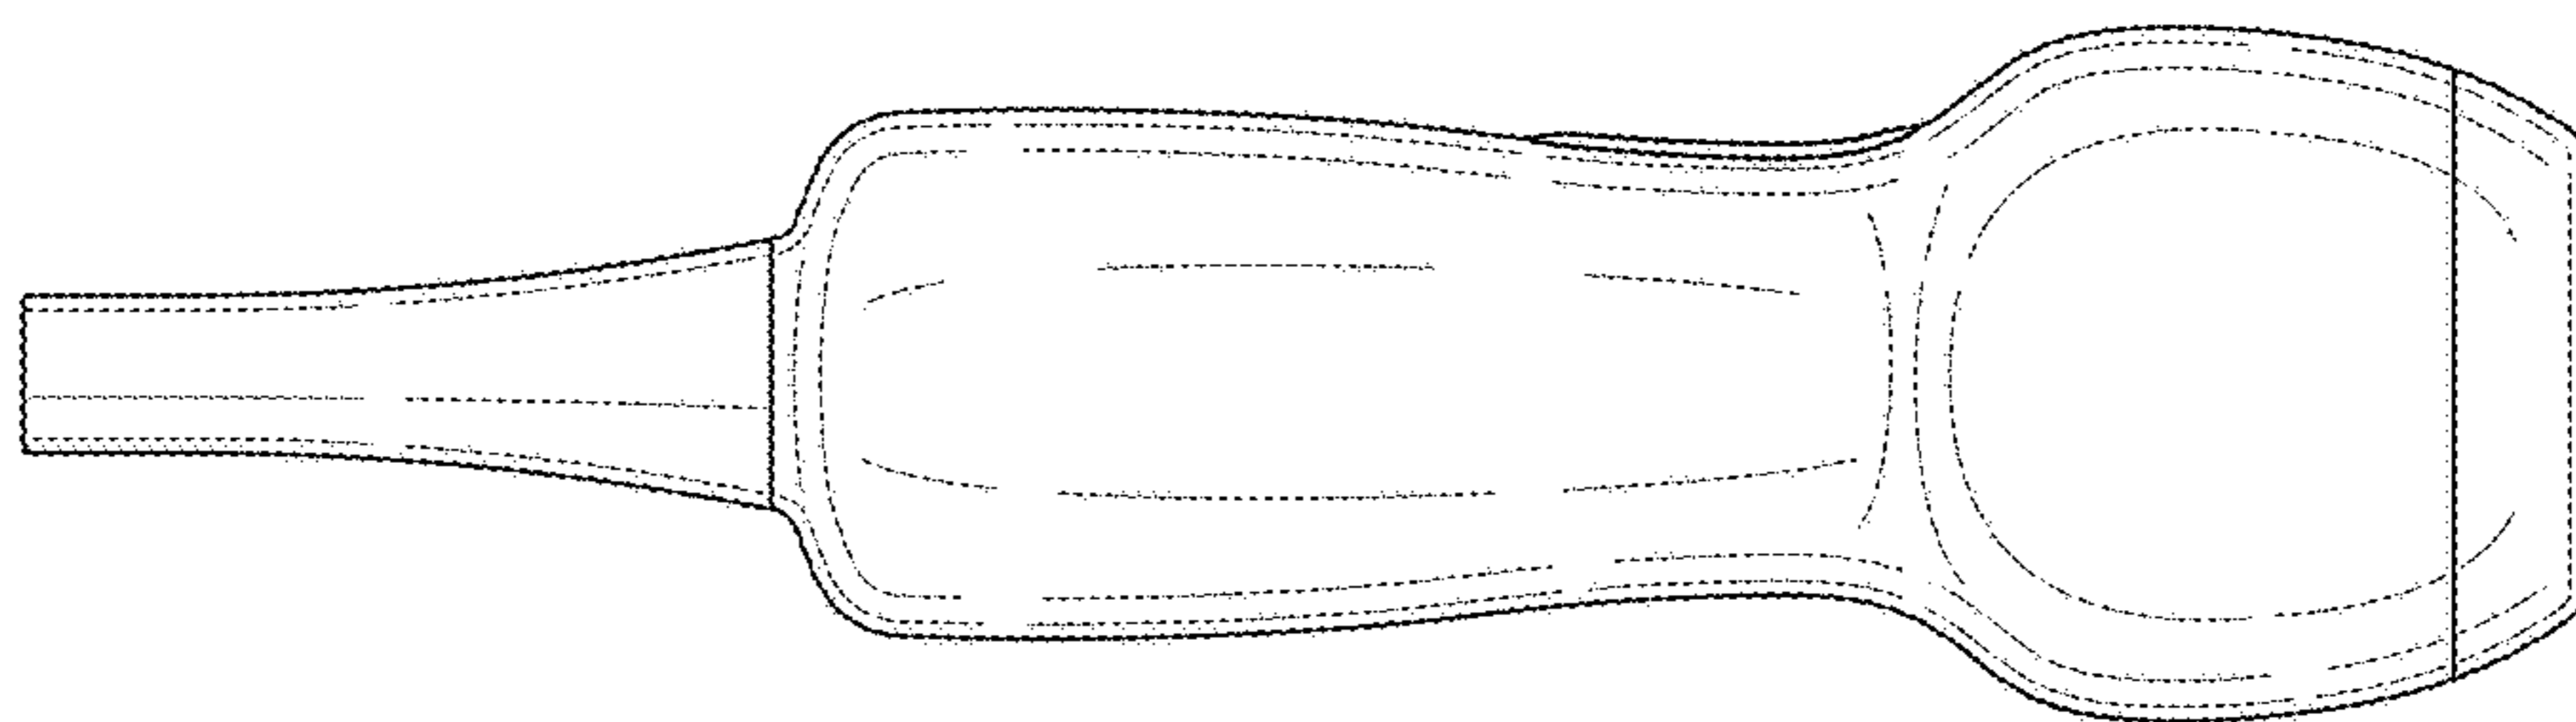


Fig. 5

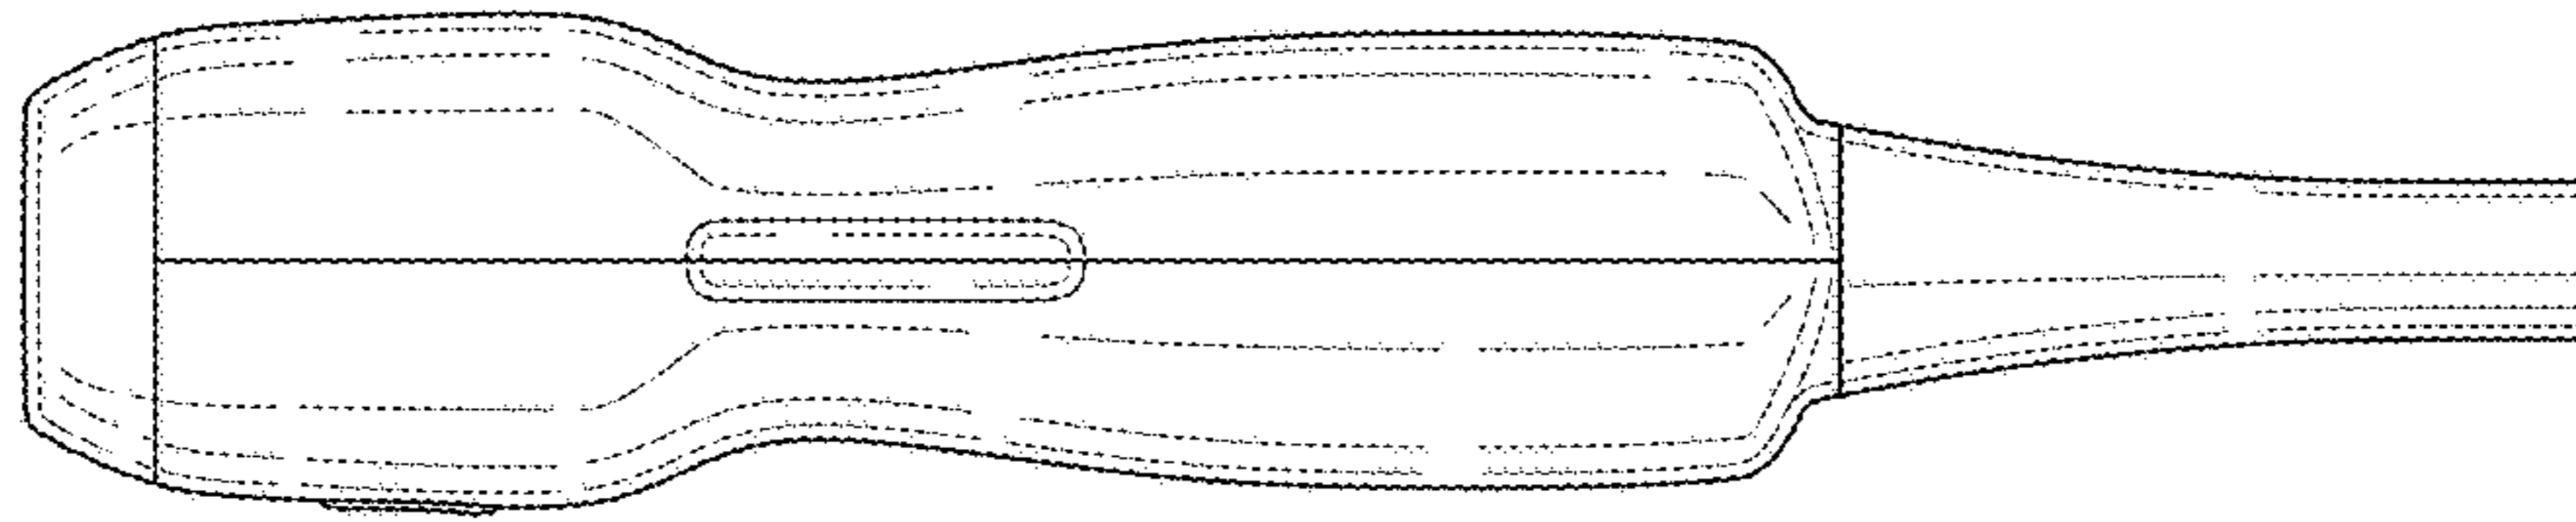


Fig. 6

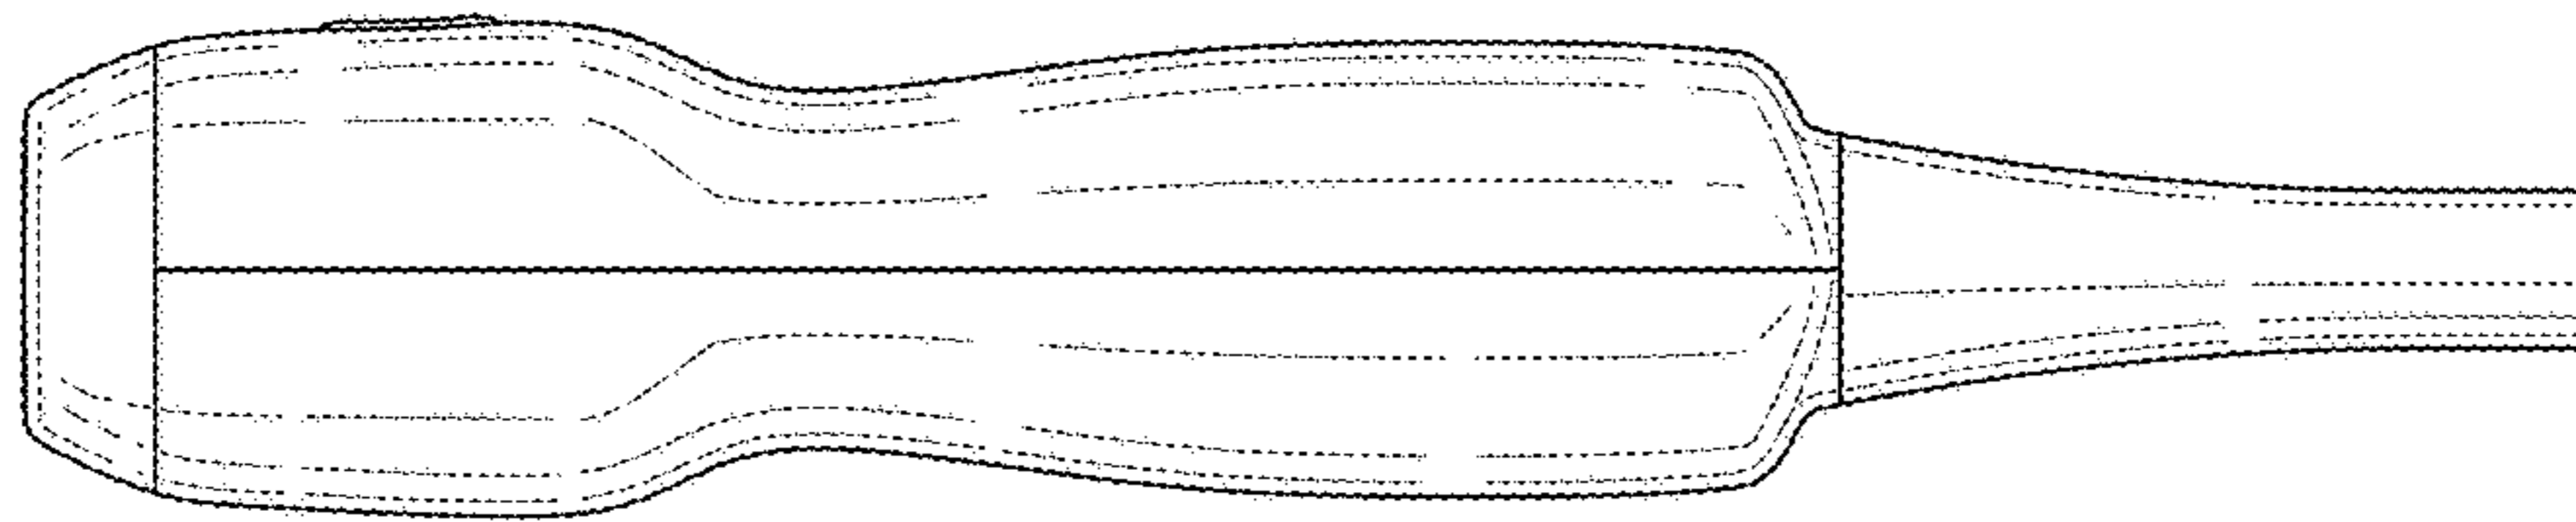


Fig. 7

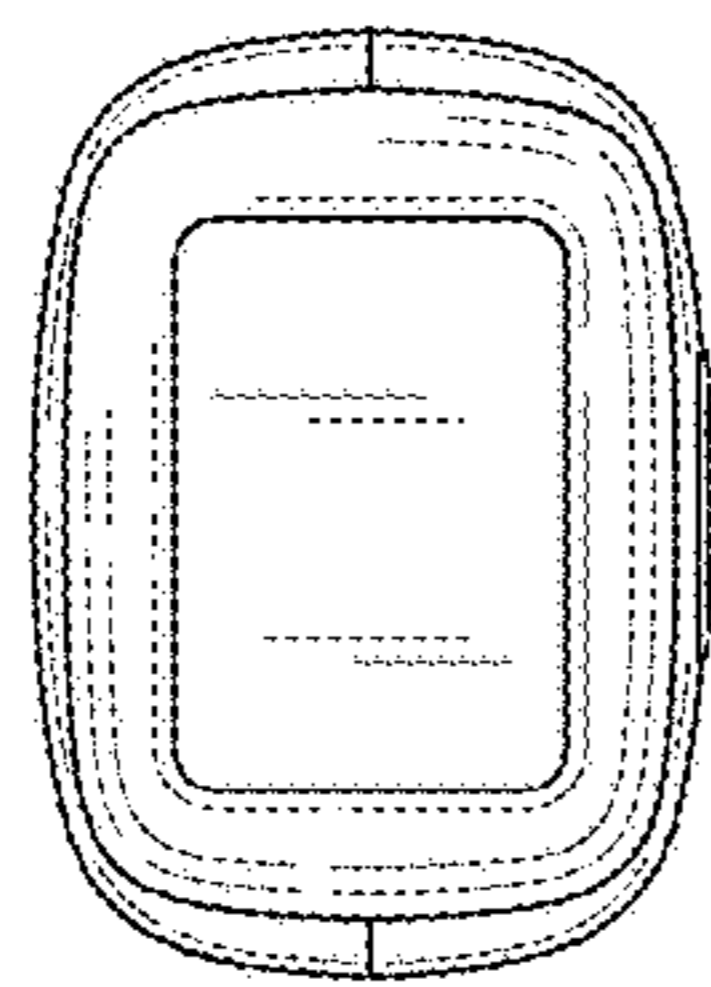


Fig. 8

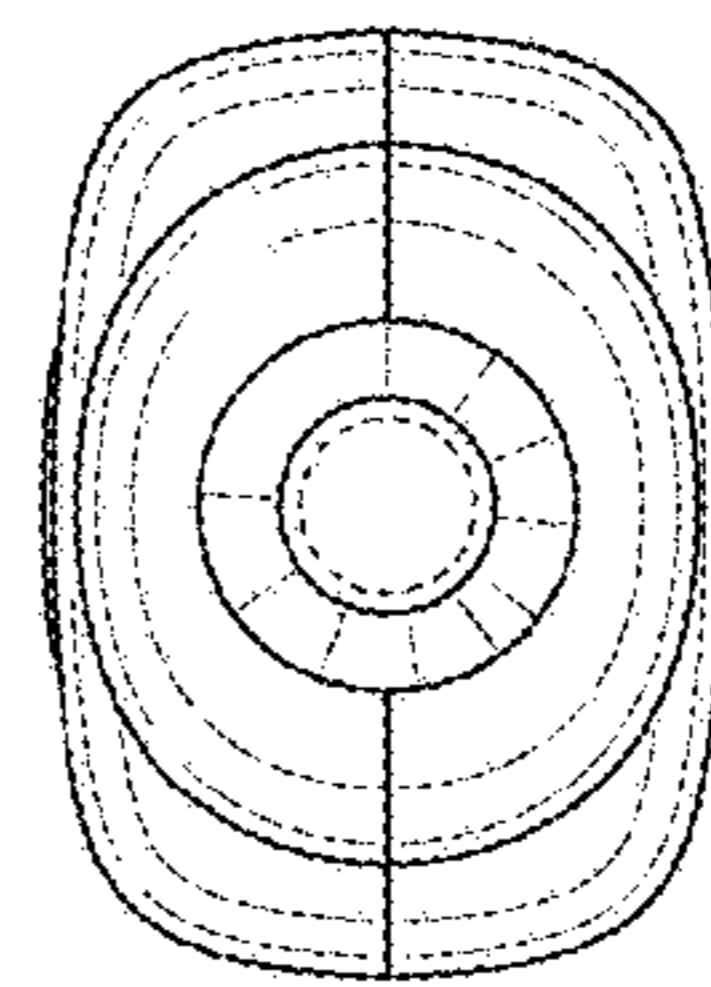


Fig. 9

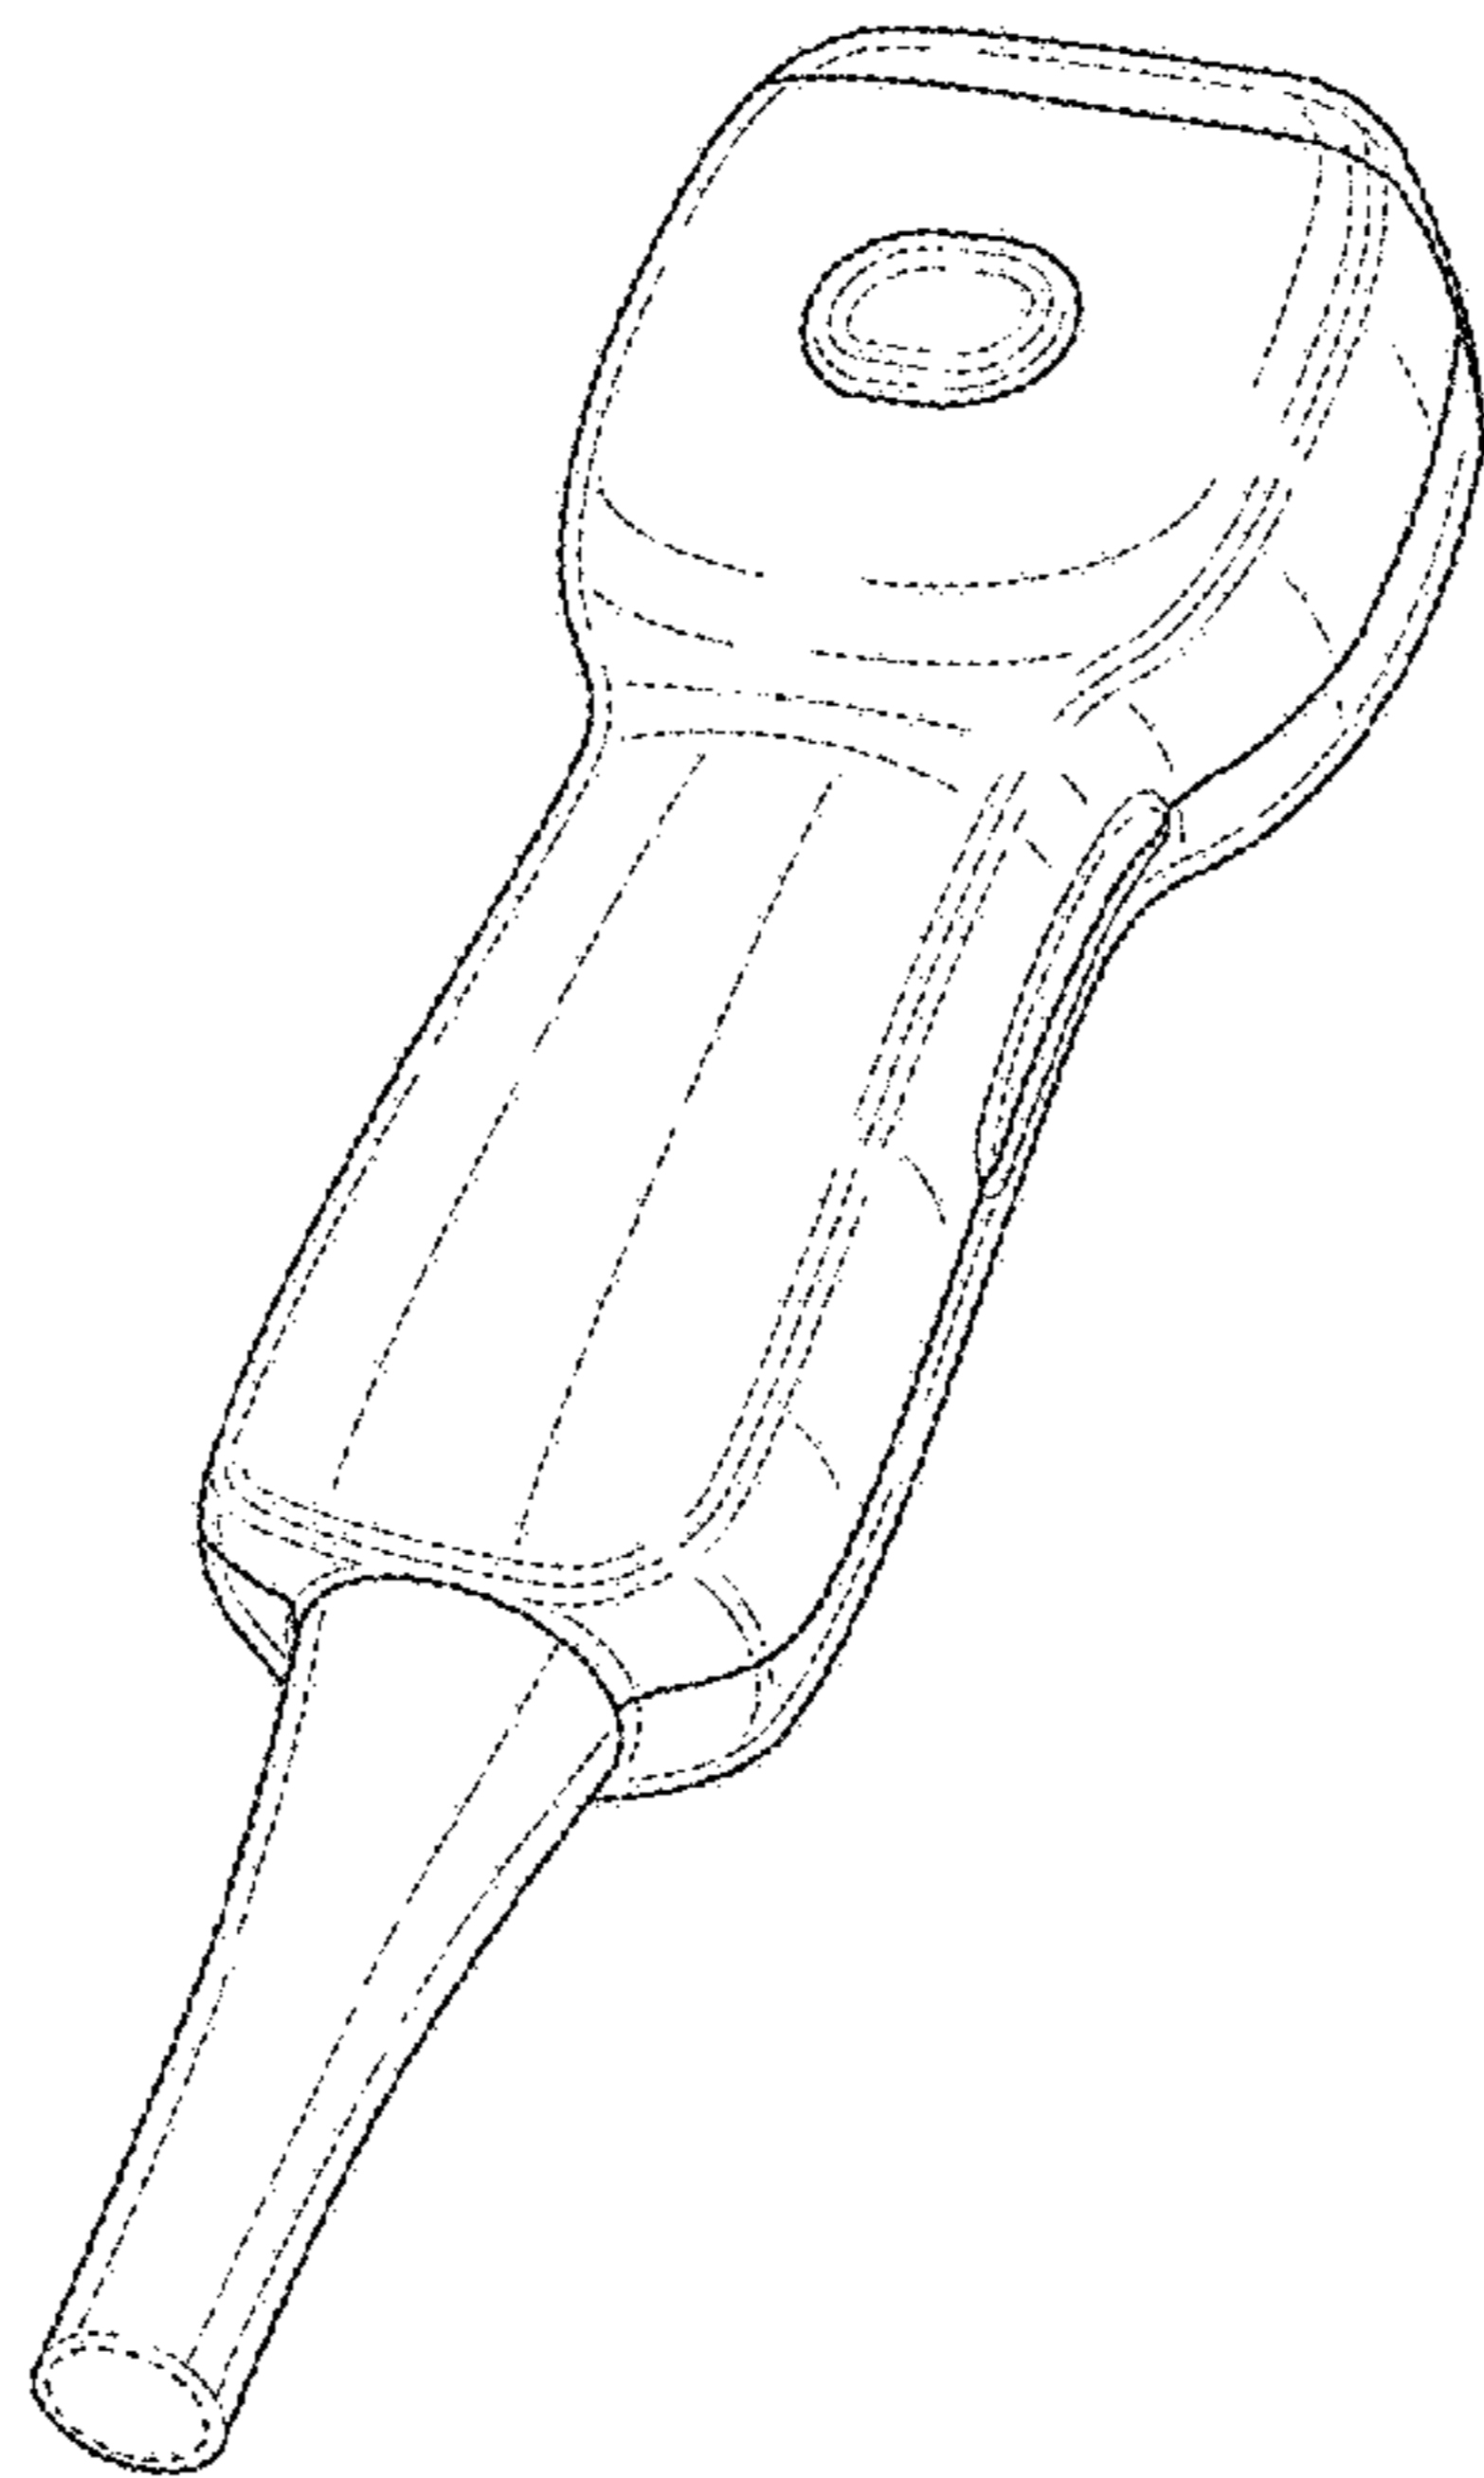


Fig. 10

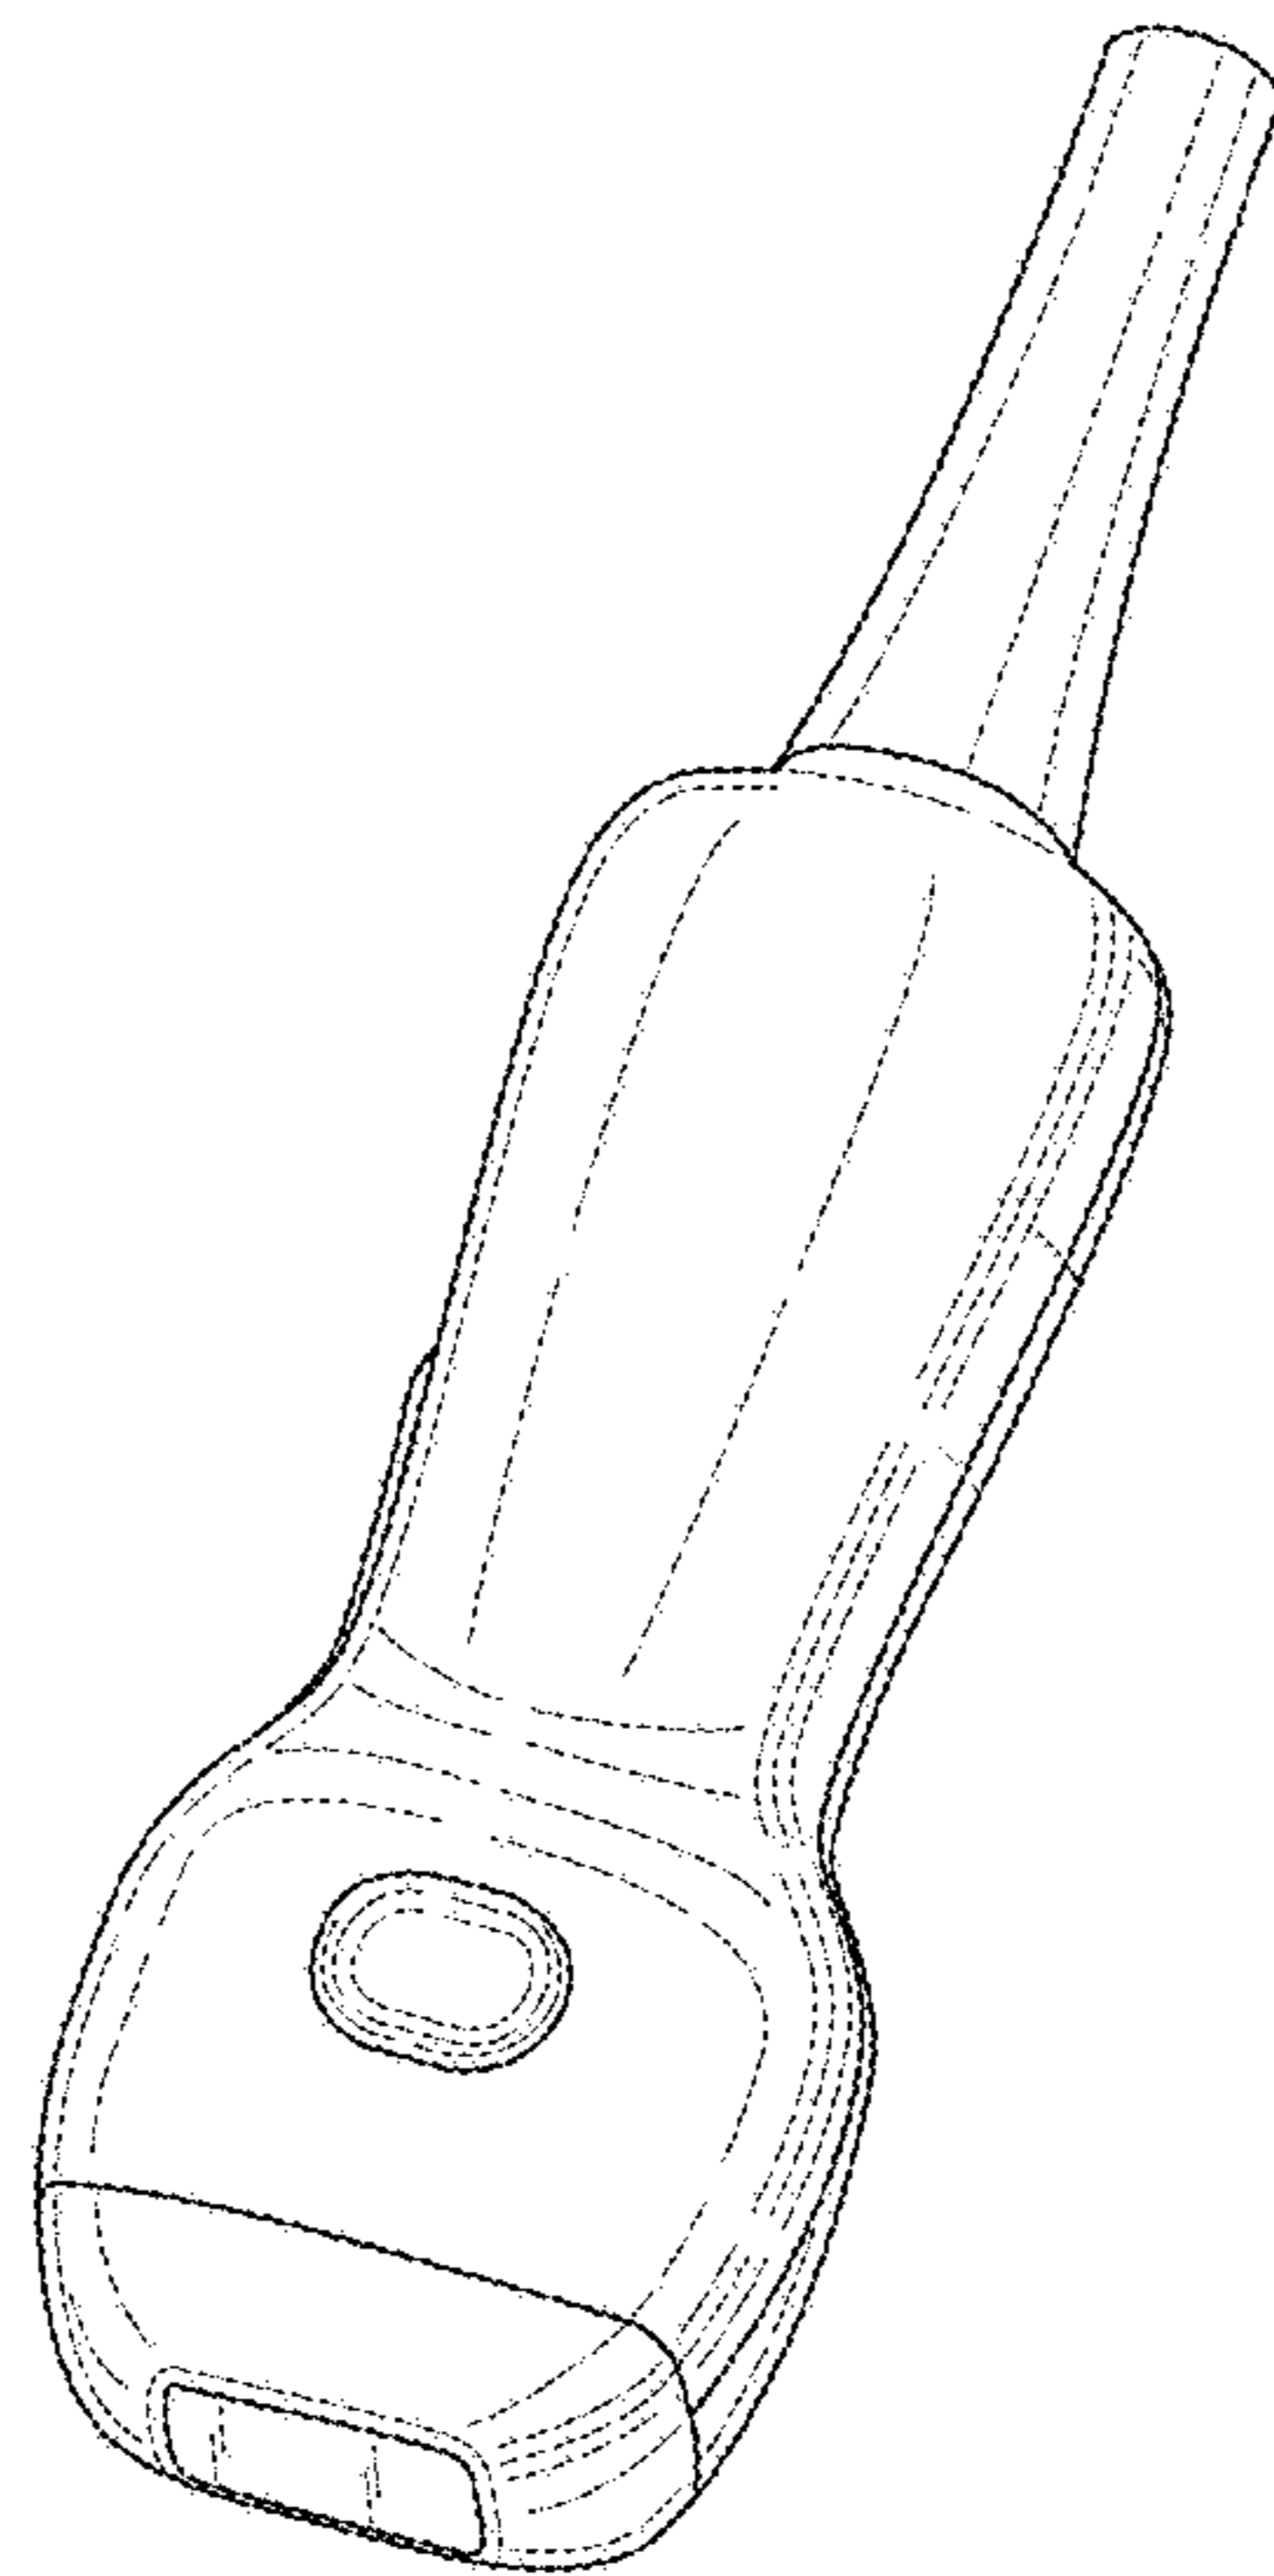


Fig. 11

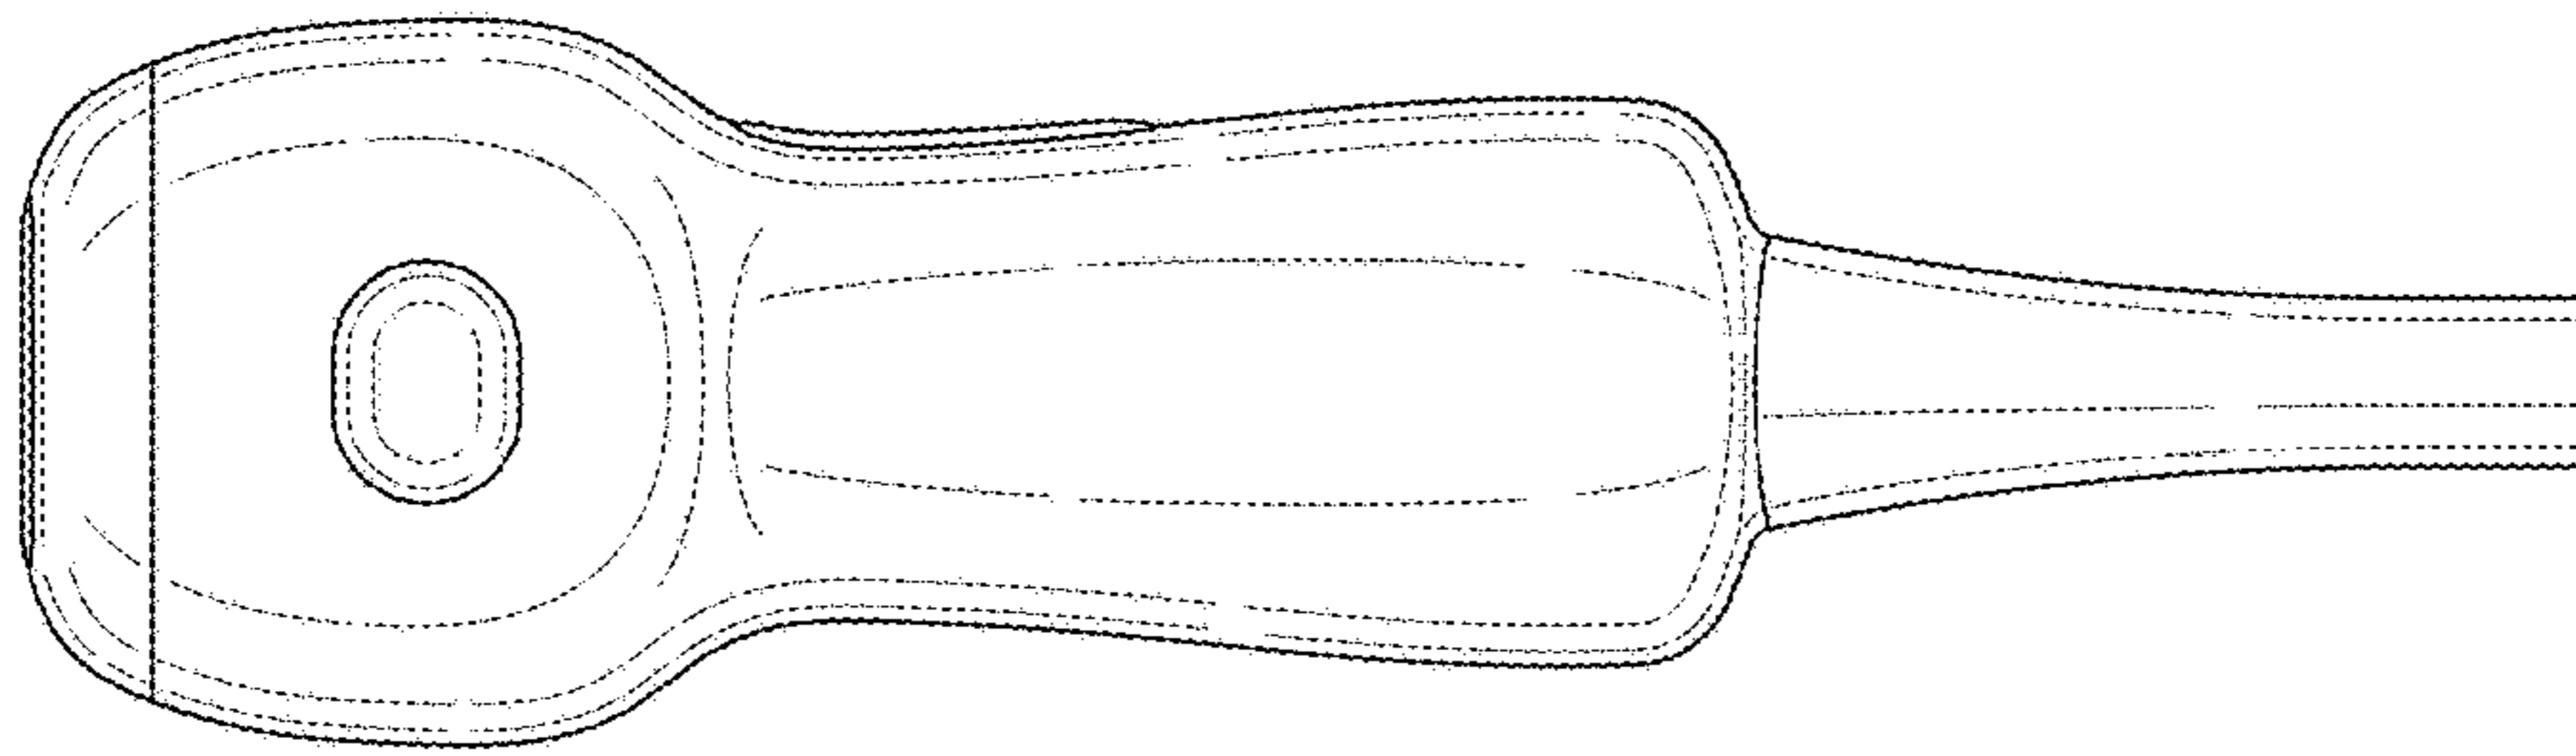


Fig. 12

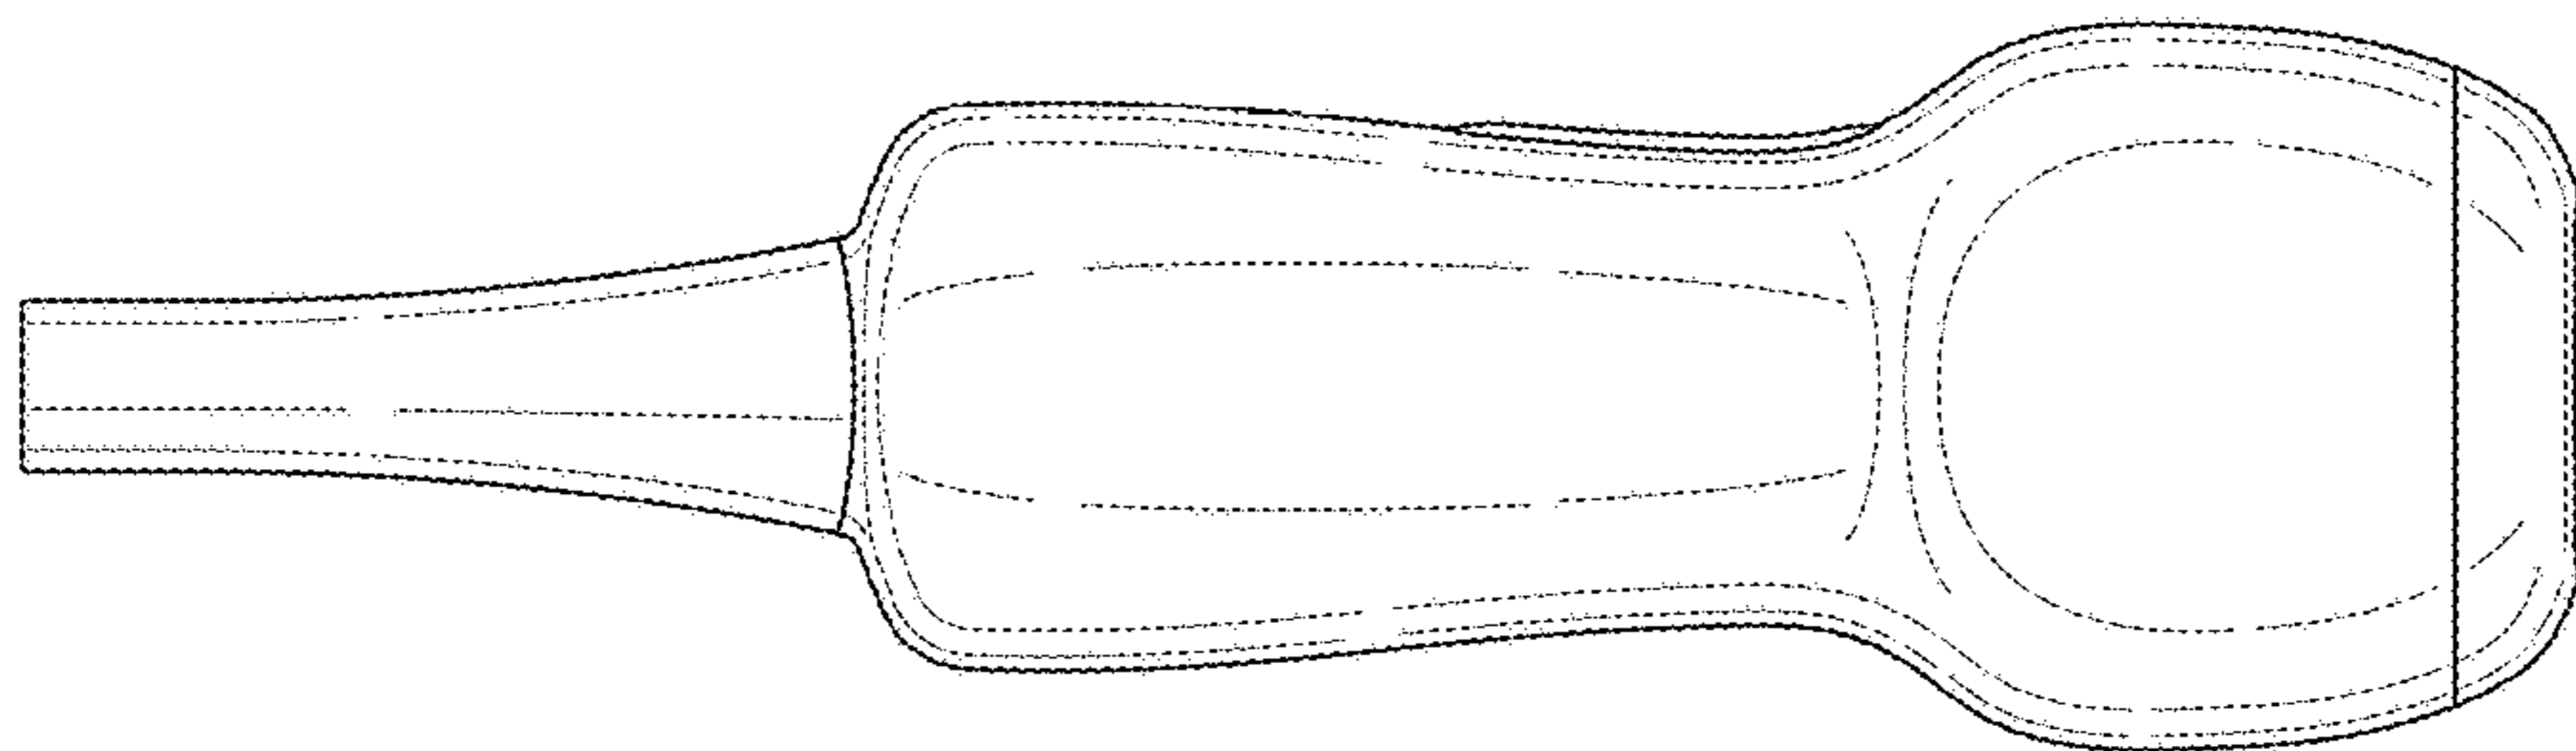


Fig. 13

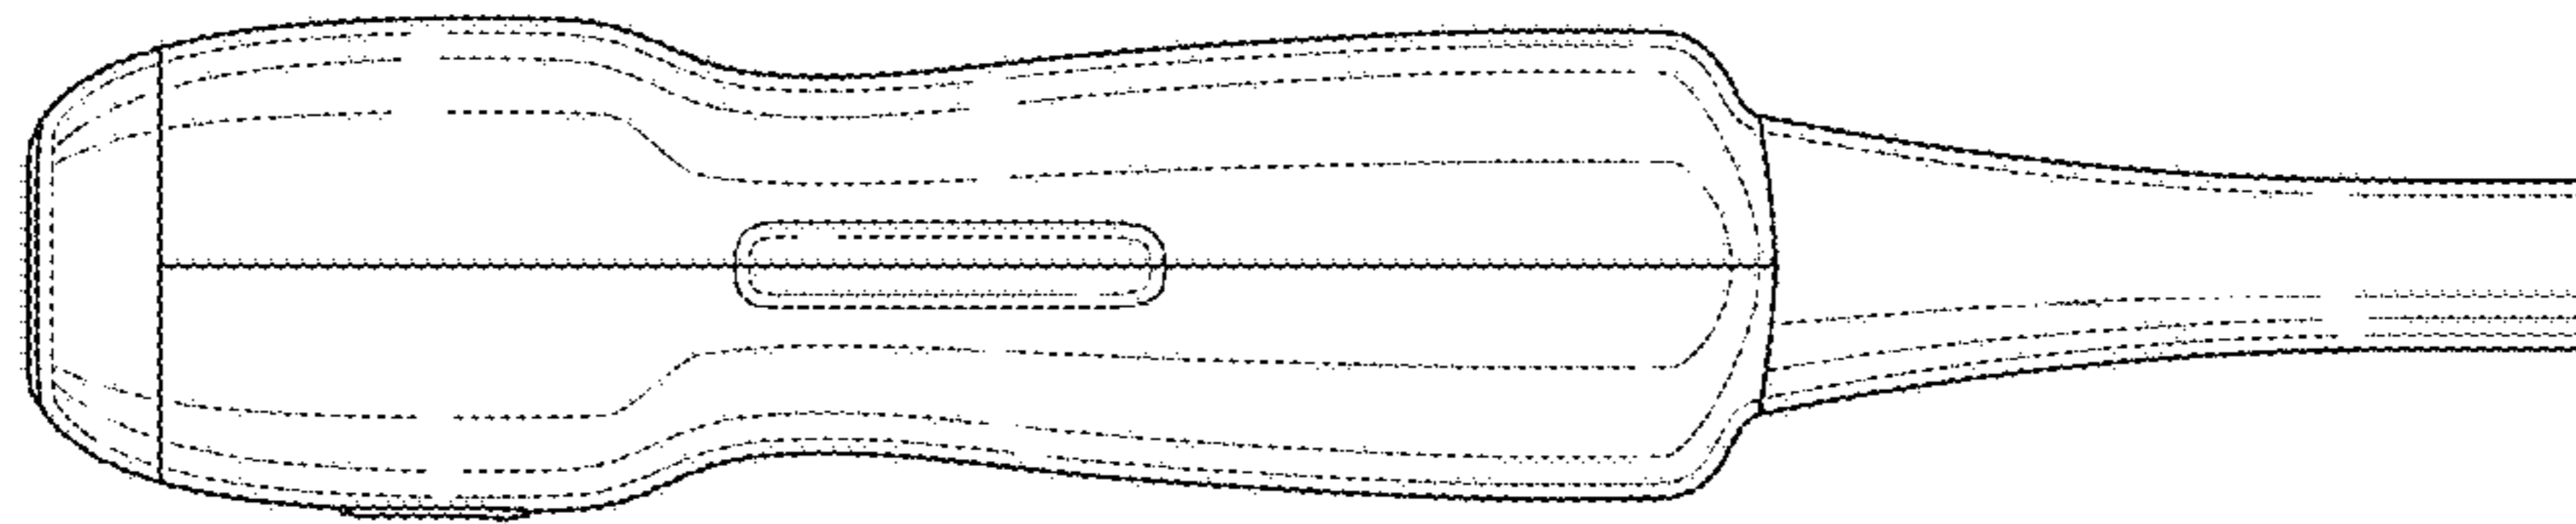


Fig. 14

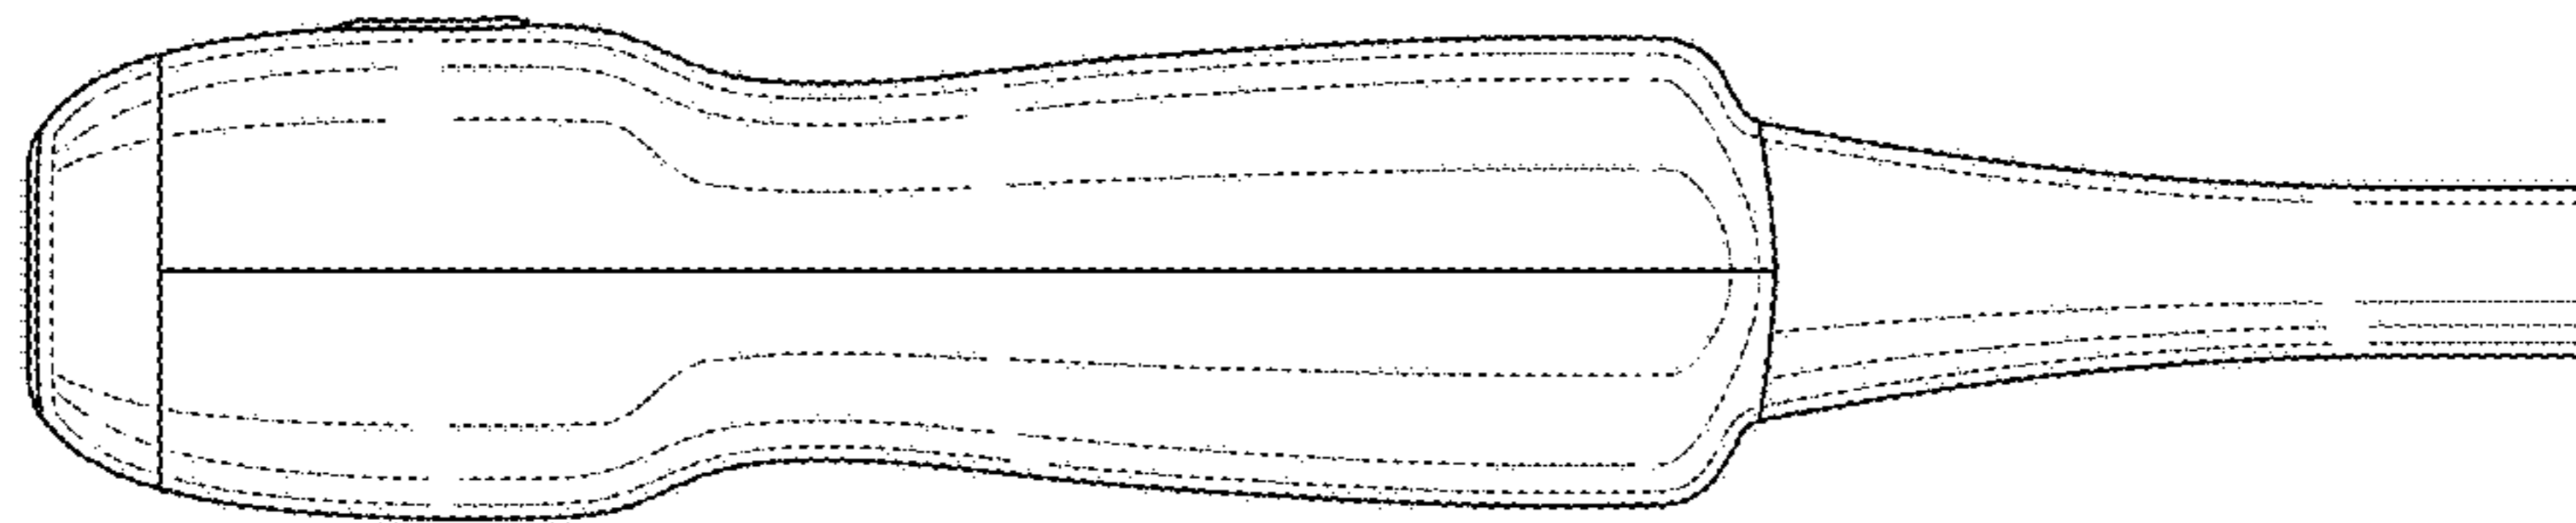


Fig. 15

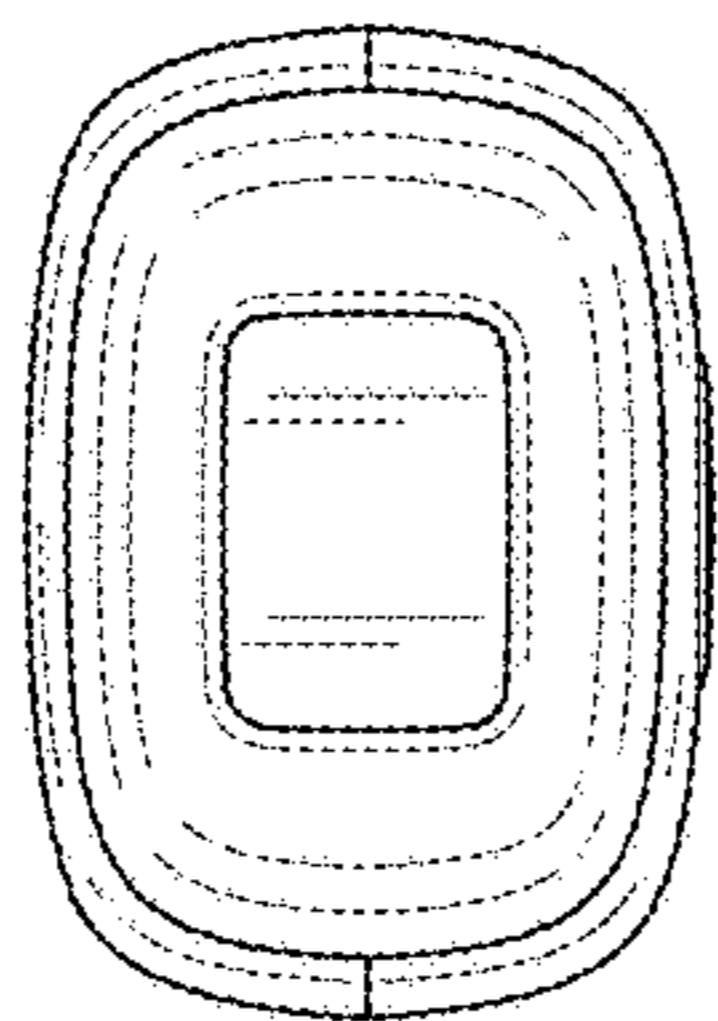


Fig. 16

