



US00D844133S

(12) **United States Design Patent**
Choi

(10) **Patent No.:** **US D844,133 S**
(45) **Date of Patent:** **** Mar. 26, 2019**

- (54) **SYRINGE PLUNGER**
- (71) Applicant: **HAUDONGCHUN Co., Ltd.**, Seoul (KR)
- (72) Inventor: **Won-seok Choi**, Seoul (KR)
- (73) Assignee: **HAUDONGCHUN Co., Ltd.**, Seoul (KR)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/610,788**
- (22) Filed: **Jul. 14, 2017**
- (30) **Foreign Application Priority Data**
Mar. 7, 2017 (KR) 30-2017-0010507
- (51) **LOC (11) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/130**
- (58) **Field of Classification Search**
USPC D24/127-131, 112-114, 133, 186;
606/181, 185; 604/264, 523-528, 272,
604/187, 158, 164.01-164.11, 181, 184,
604/227; 600/101, 139, 143;
128/200.24, 207.14, 207.15
CPC A61M 5/178; A61M 3/00; A61M 5/20;
A61M 5/31; A61M 5/3146; A61M
5/3129; A61M 5/3148; A61M 5/315
See application file for complete search history.

- D638,122 S * 5/2011 Kosinski A61M 5/31511
D24/130
- D713,525 S * 9/2014 Oguro D24/130
- D726,305 S * 4/2015 Furukawa D24/114
- D729,931 S * 5/2015 Takeuchi D24/114
- D730,515 S * 5/2015 Shahidi Bonjar D24/114
- D733,870 S * 7/2015 Broyles D24/114
- D747,797 S * 1/2016 Fourt D24/114
- D750,768 S * 3/2016 Davidian D24/114
- D771,249 S * 11/2016 Heath D24/133
- 9,517,328 B2 * 12/2016 Mellejor A61M 5/31501
- D789,520 S * 6/2017 Tseng D24/114
- 9,968,769 B2 * 5/2018 Sasayama A61M 39/10
- D819,805 S * 6/2018 Knight D24/114

* cited by examiner

Primary Examiner — David G Muller
(74) *Attorney, Agent, or Firm* — Novick, Kim & Lee, PLLC; Jae Youn Kim

(57) **CLAIM**


I claim, the ornamental design for a syringe plunger, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a syringe plunger, showing my new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a left side elevational view thereof;
FIG. 5 is a right side elevational view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof; and,
FIG. 8 is a cross-sectional view taken along line 8-8 of FIG. 2.
The broken lines shown in the drawings depict portions of the syringe plunger which form no part of the claimed design.

1 Claim, 4 Drawing Sheets

- (56) **References Cited**
U.S. PATENT DOCUMENTS
D515,207 S * 2/2006 Tarumi D24/114
D515,209 S * 2/2006 Tarumi D24/114
D574,954 S * 8/2008 Smith D24/114
D618,347 S * 6/2010 Bradshaw D24/108

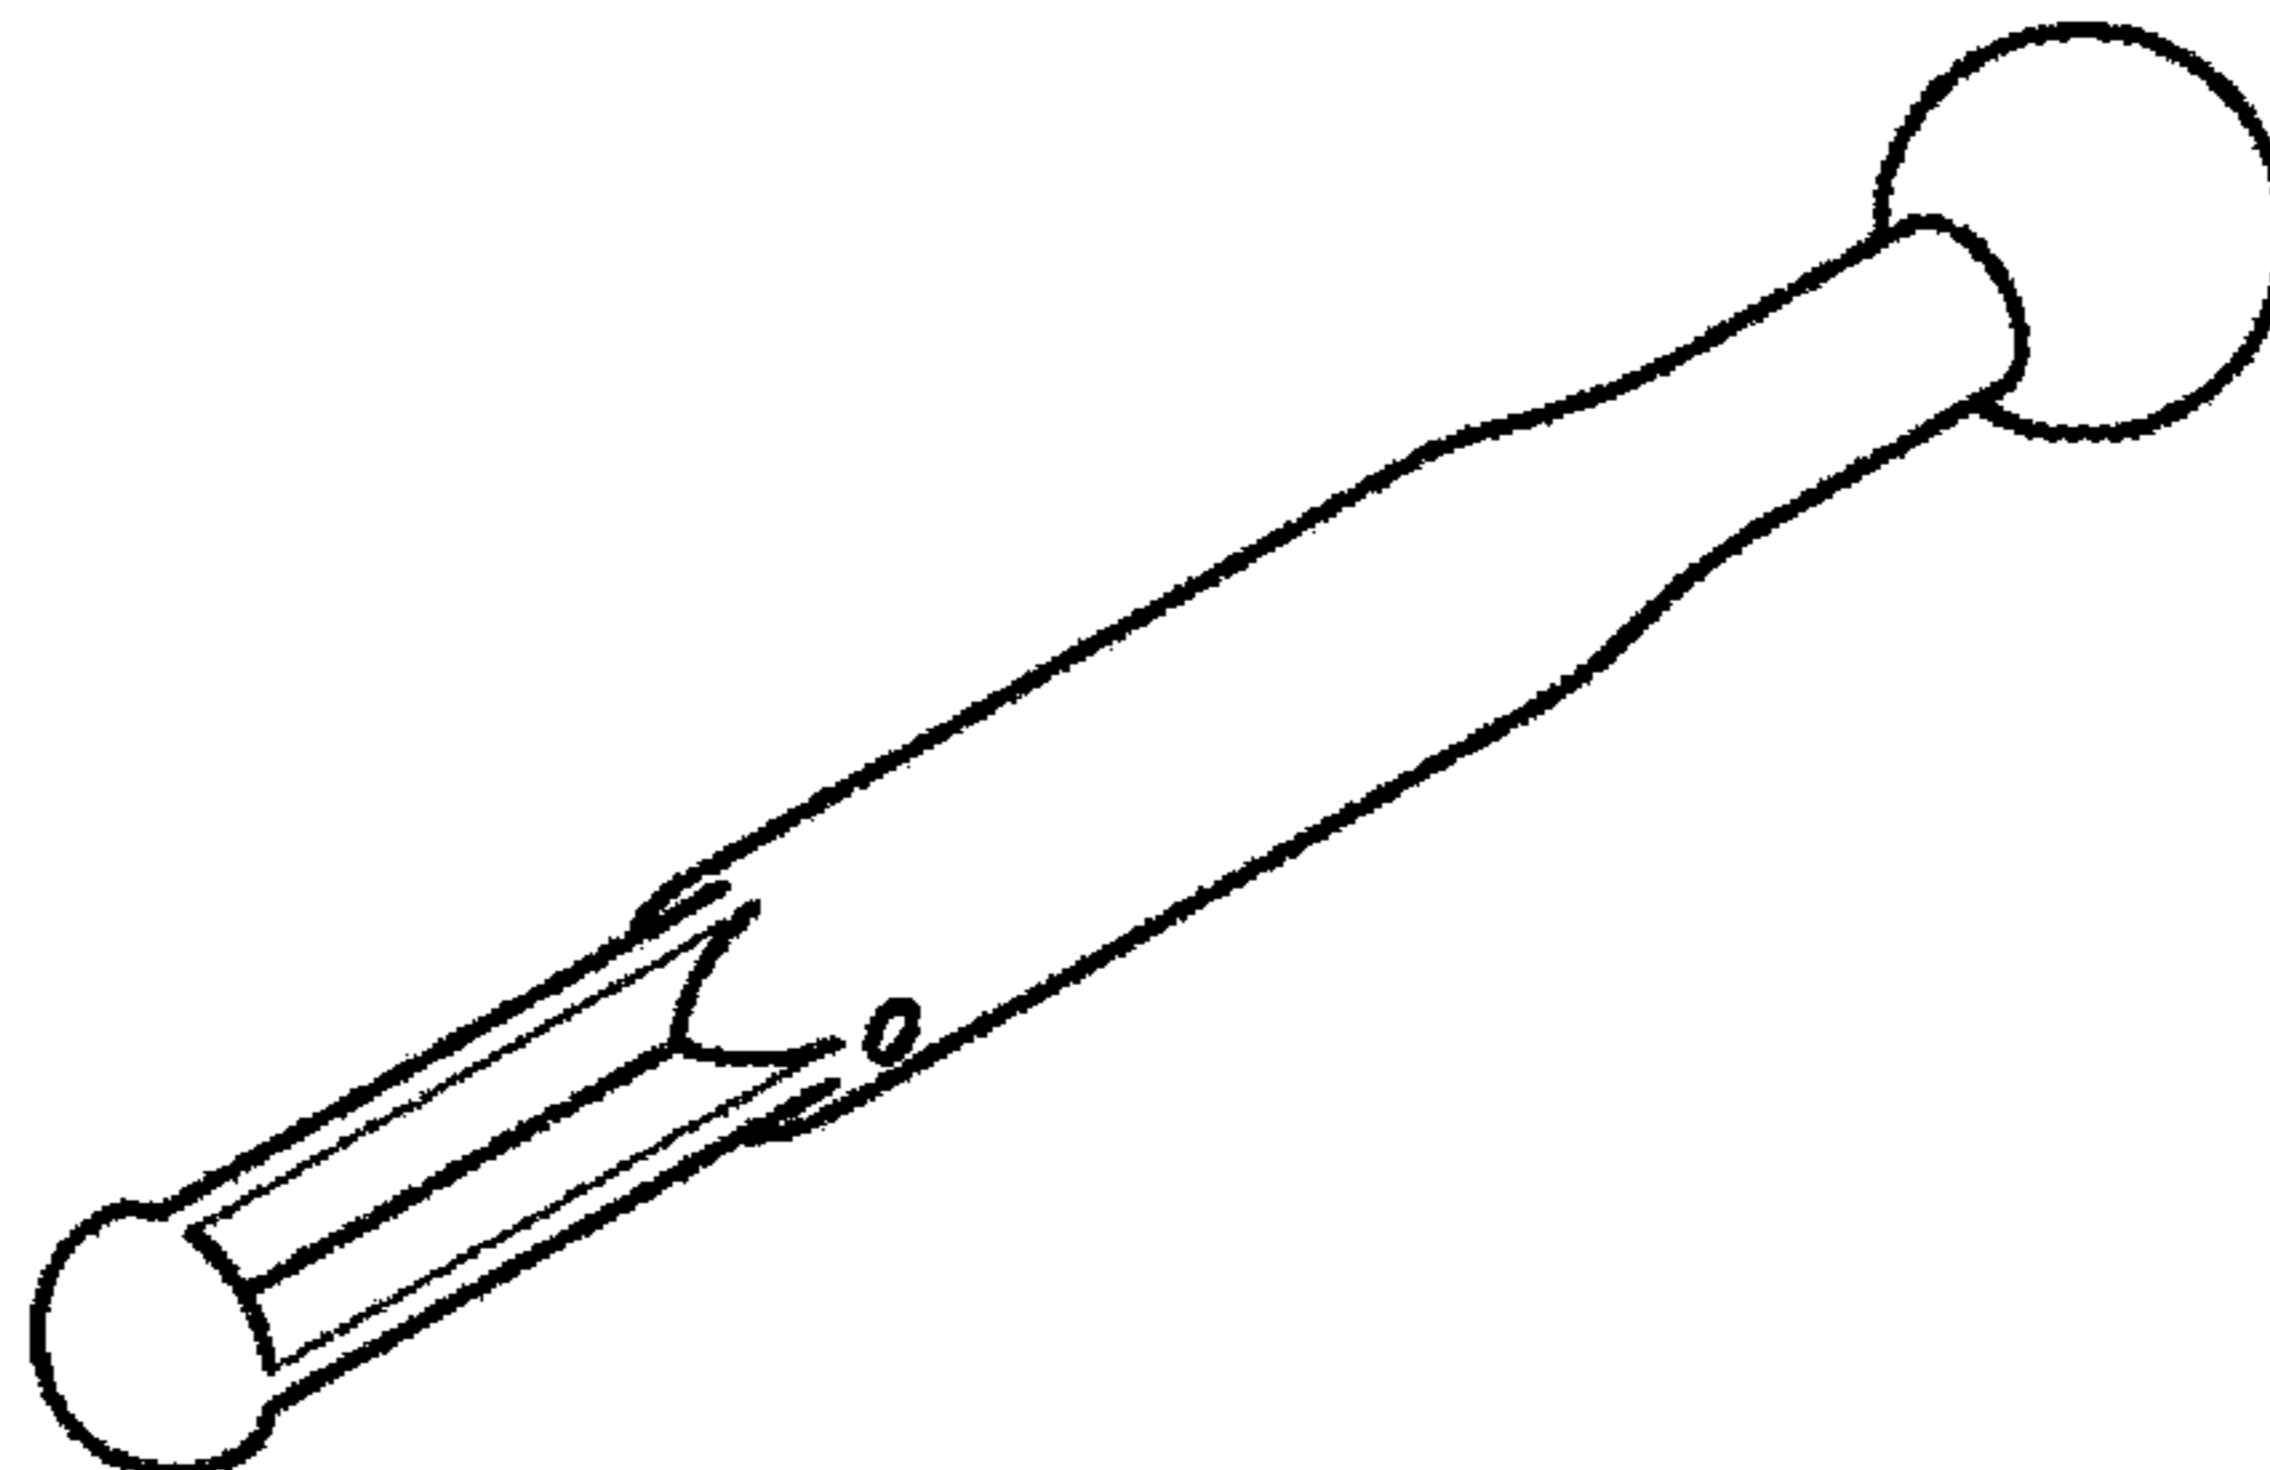

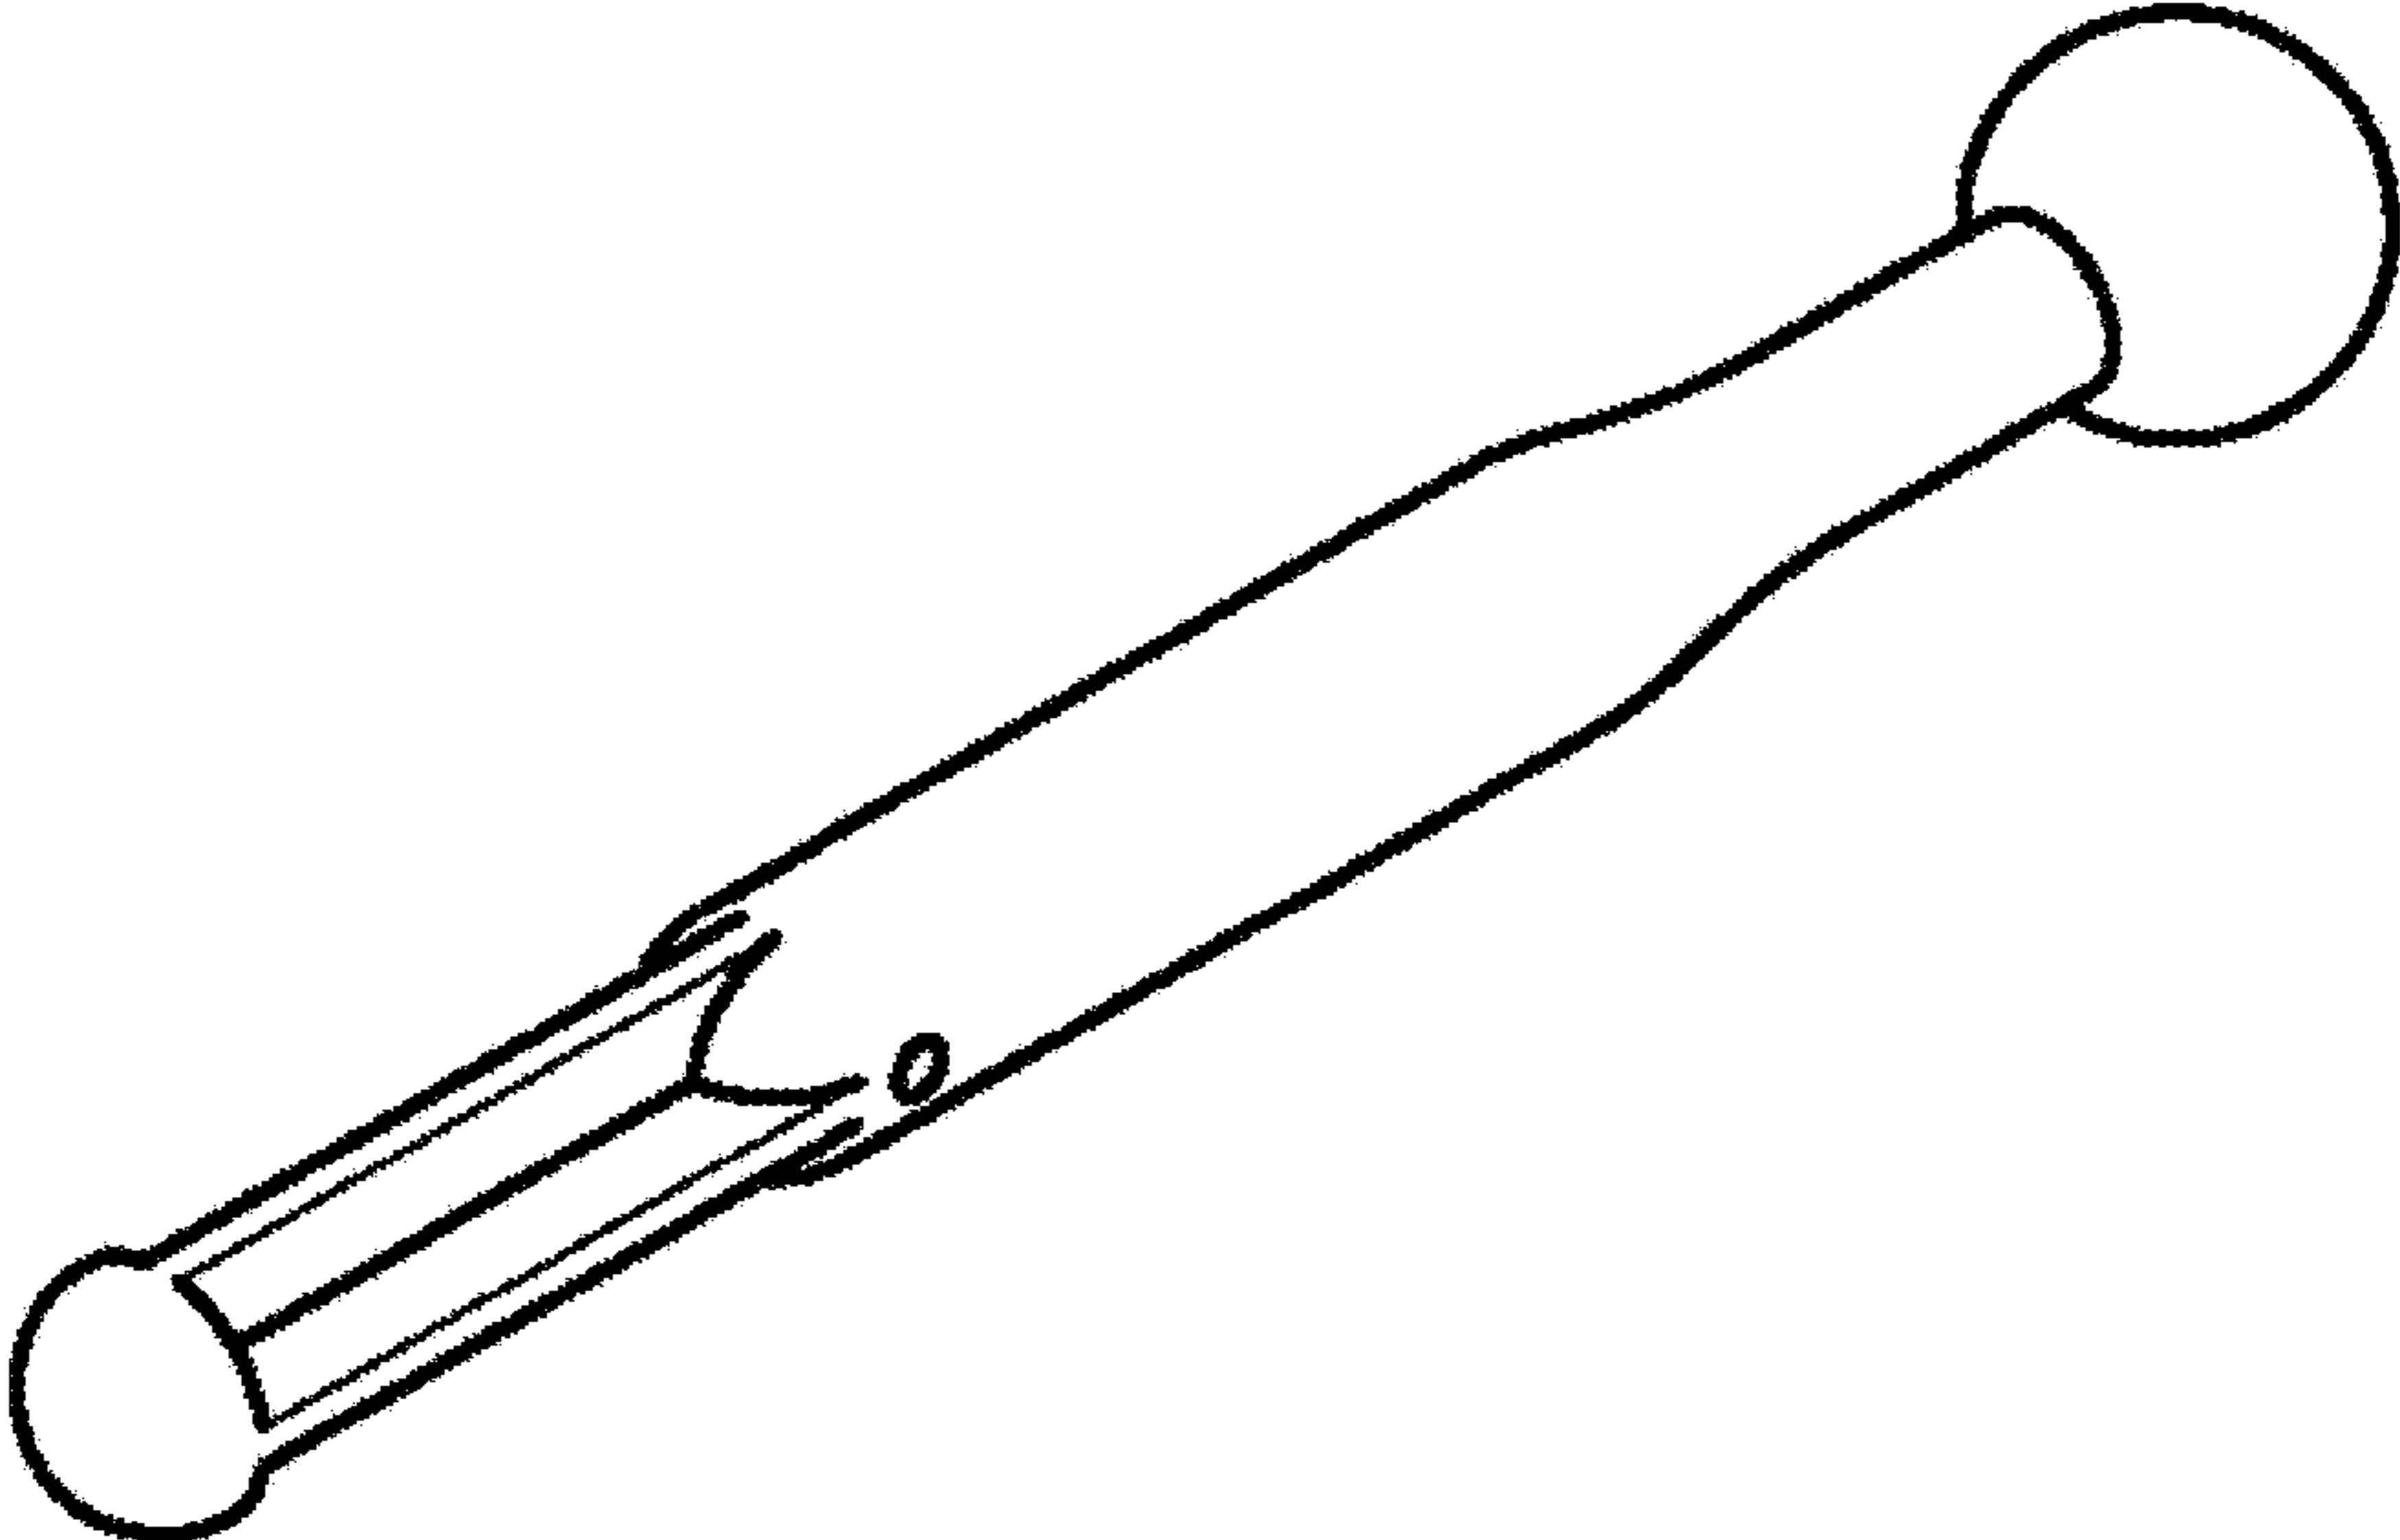


FIG. 1

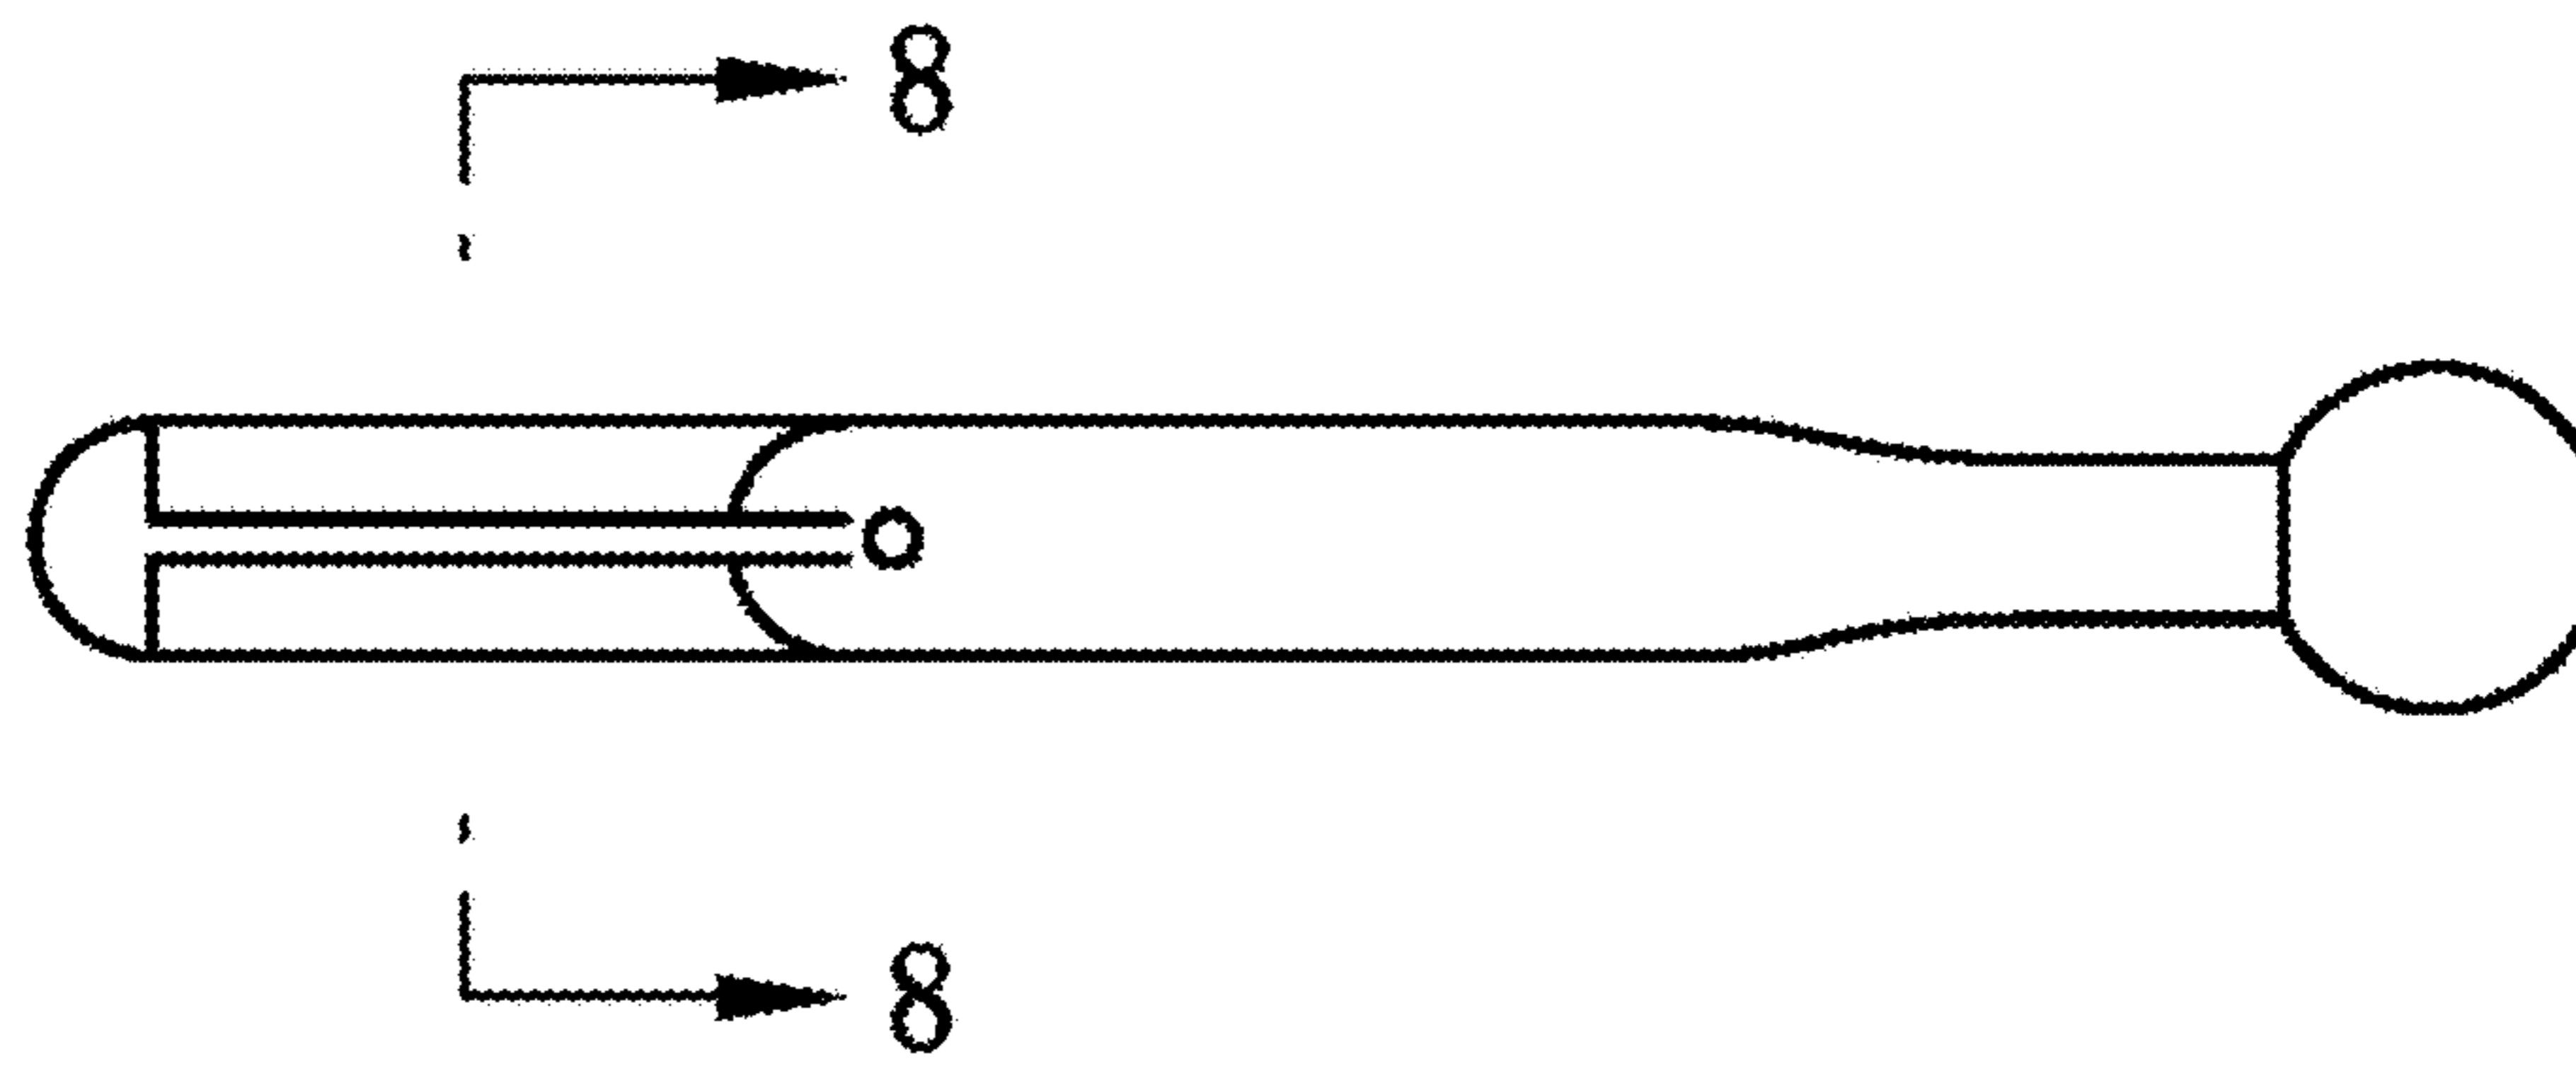


FIG. 2



FIG. 3

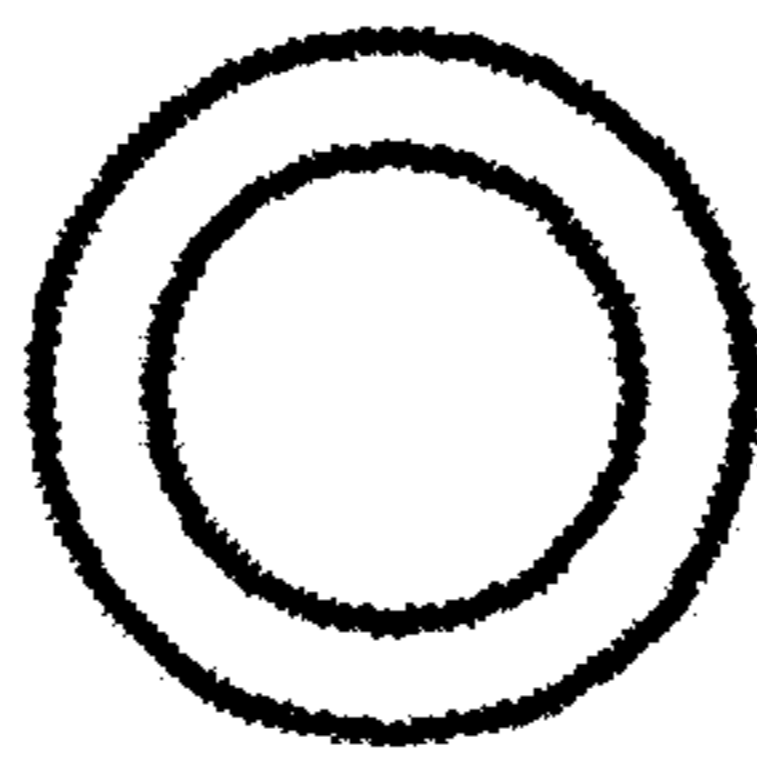


FIG. 4

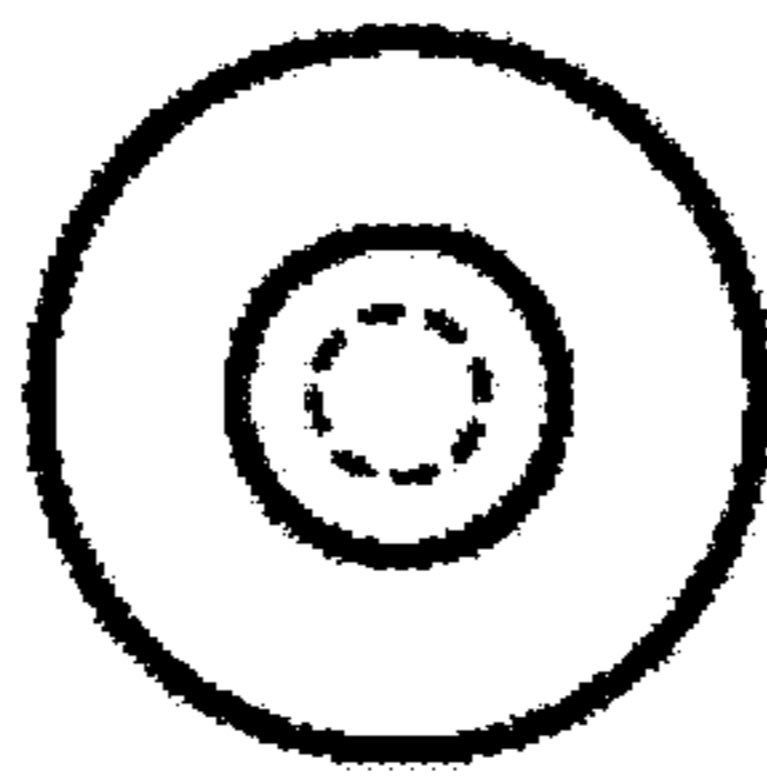


FIG. 5



FIG. 6

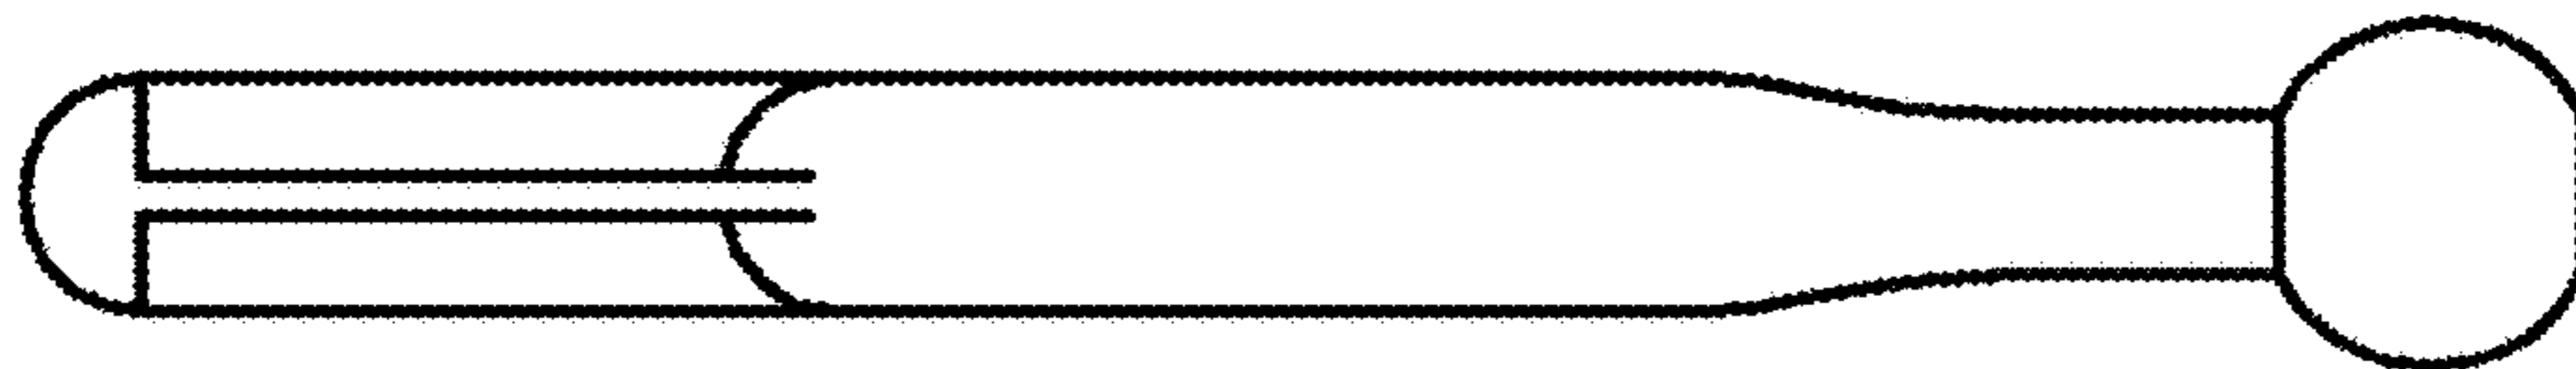


FIG. 7

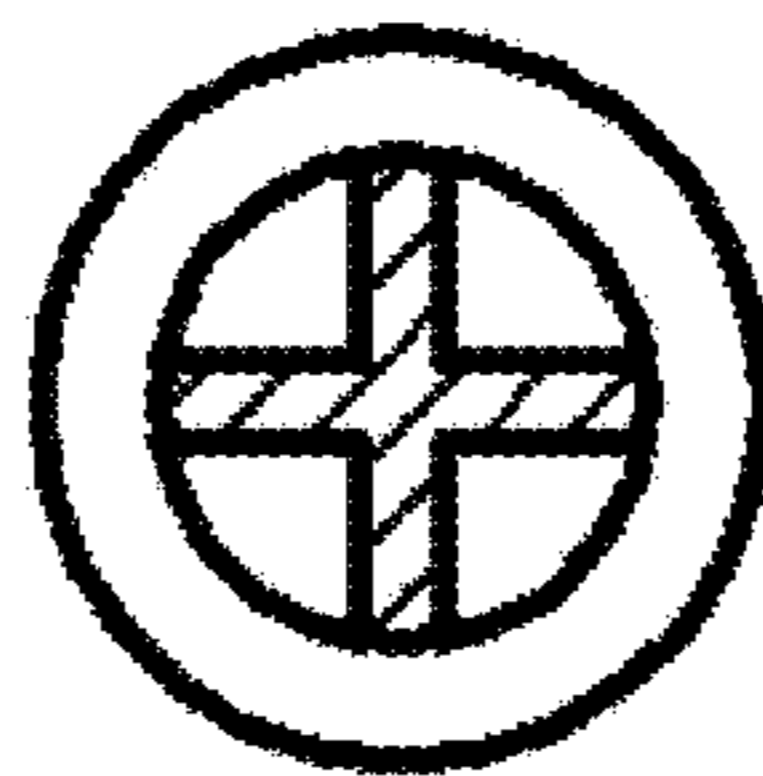


FIG. 8