



US00D845475S

(12) **United States Design Patent**  
**Serfati**

(10) **Patent No.:** **US D845,475 S**

(45) **Date of Patent:** **\*\* Apr. 9, 2019**

(54) **FILTERED LUER SLIP IV SET FOR SERUM BOTTLE HIGH VOLUME INFUSION FOR VETERINARY USE**

(71) Applicant: **Biogalenic, LLC.**, Aventura, FL (US)

(72) Inventor: **Jacob Serfati**, Aventura, FL (US)

(73) Assignee: **Biogalenic, LLC.**, Aventura, FL (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/621,797**

(22) Filed: **Oct. 11, 2017**

(51) **LOC (11) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/129**

(58) **Field of Classification Search**  
USPC ..... D24/127-131, 112-114, 133, 186;  
606/181, 185; 604/264, 523-528, 272,  
604/187, 158, 164.01-164.11, 181, 184,  
604/227; 600/101, 139, 143;  
128/200.24, 207.14, 207.15  
CPC .. A61M 25/065; A61M 5/42; A61M 25/0612;  
A61M 25/00; A61M 39/00; A61M 27/00;  
A61M 25/0043; A61M 25/0067; A61M  
25/0097; A61F 2/958  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,569,294 A \* 10/1996 Parkola ..... A61M 25/00  
604/103.05  
5,695,466 A \* 12/1997 Lopez ..... A61M 5/14  
250/462.1

6,447,489 B1 \* 9/2002 Peterson ..... A61B 17/3439  
600/204  
6,461,336 B1 \* 10/2002 Larre ..... A61F 2/954  
604/264  
D658,298 S \* 4/2012 Prpa ..... D24/186  
D701,304 S \* 3/2014 Lair ..... D24/129  
D709,178 S \* 7/2014 Tanaka ..... D24/110  
D751,699 S \* 3/2016 Mills ..... D24/127  
D757,260 S \* 5/2016 Lombardi, III ..... D24/129  
D805,193 S \* 12/2017 Shoji ..... D24/129  
D805,629 S \* 12/2017 Fiorenza ..... D24/110  
D816,831 S \* 5/2018 Sacchetti ..... D24/127  
D820,441 S \* 6/2018 Ketelhohn ..... A61B 17/22012  
D24/127

\* cited by examiner

*Primary Examiner* — David G Muller

(74) *Attorney, Agent, or Firm* — Albert Bordas, P.A.


(57) **CLAIM**

The ornamental design for a filtered luer slip IV set for serum bottle high volume infusion for veterinary use, as shown and described.

**DESCRIPTION**

FIG. 1 is a top plan view of a filtered luer slip IV set for serum bottle high volume infusion for veterinary use; FIG. 2 is a front elevational view thereof; FIG. 3 is a bottom plan view thereof; FIG. 4 is a right-side elevational view thereof; FIG. 5 is a left-side elevational view thereof; FIG. 6 is a rear elevational view thereof; and, FIG. 7 is an isometric view thereof, showing my design being used with a bottle to administrate liquid matter. The broken line showing of parts of the drawings is included for the purpose of illustrating use and environment and forms no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

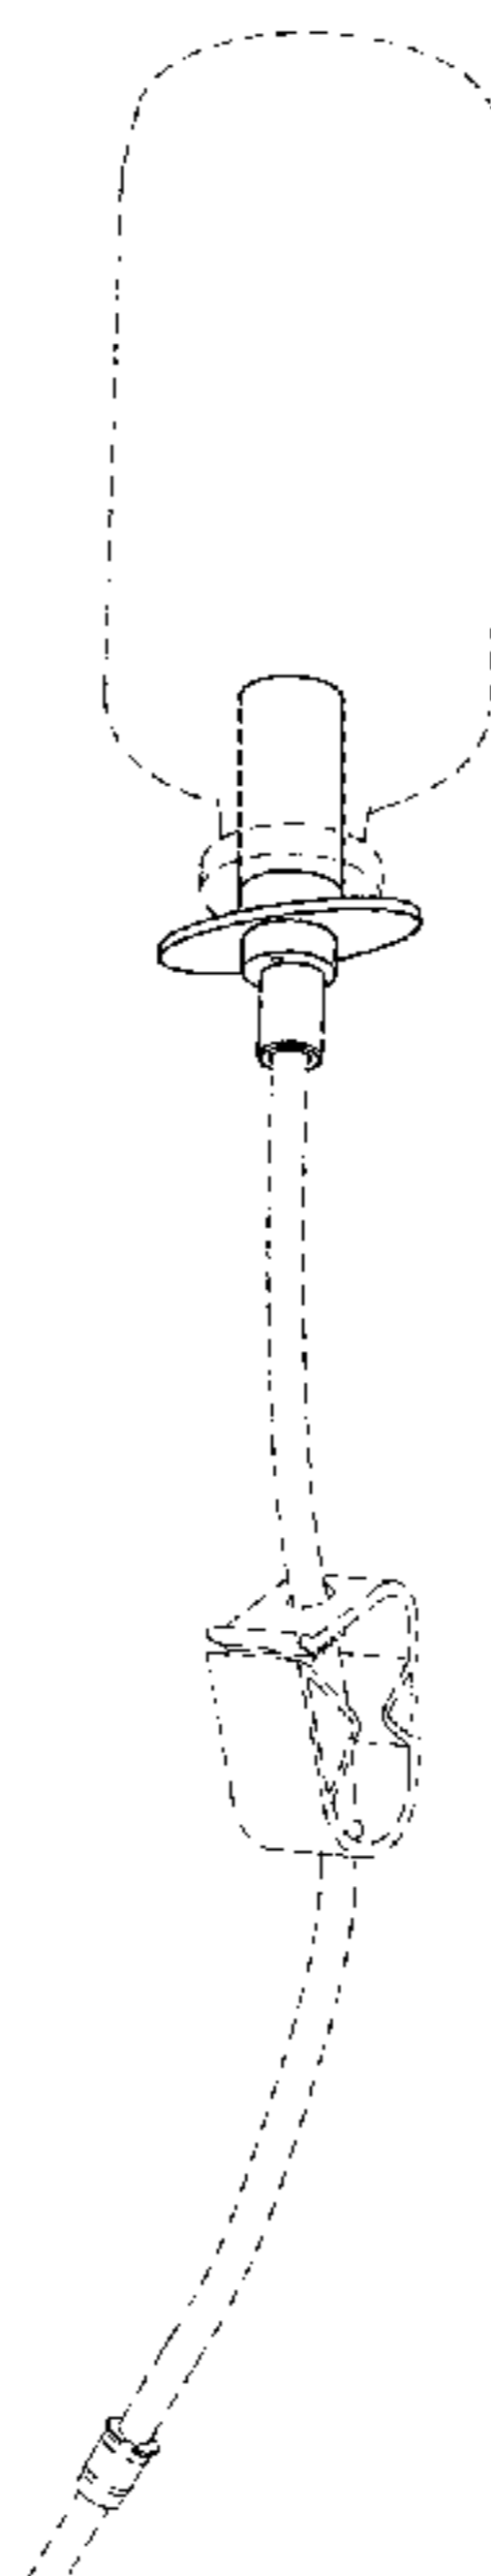

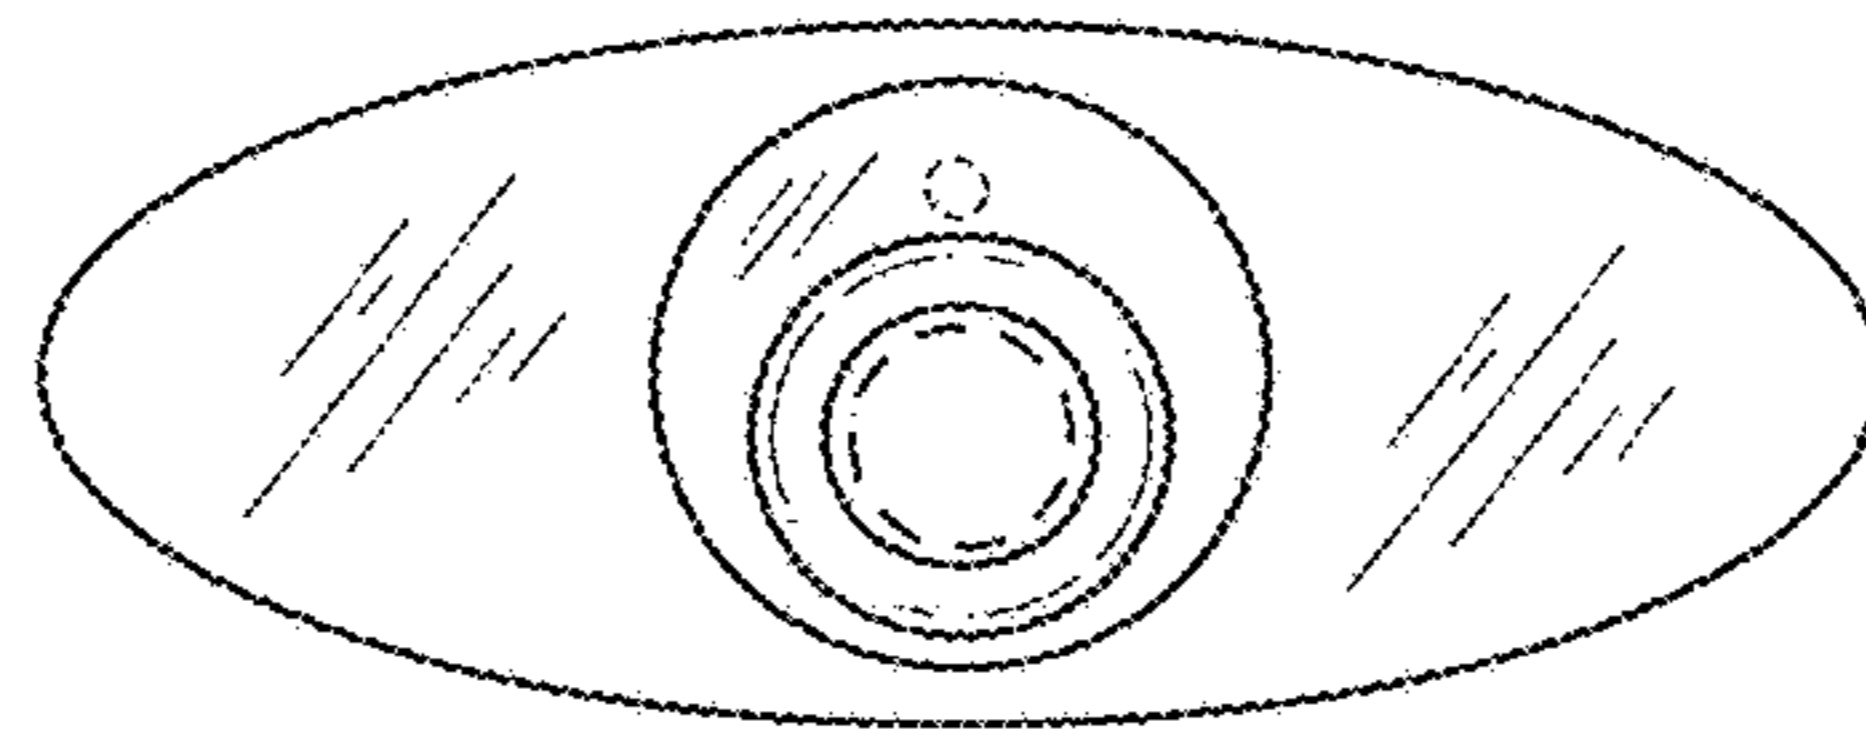


Fig. 1

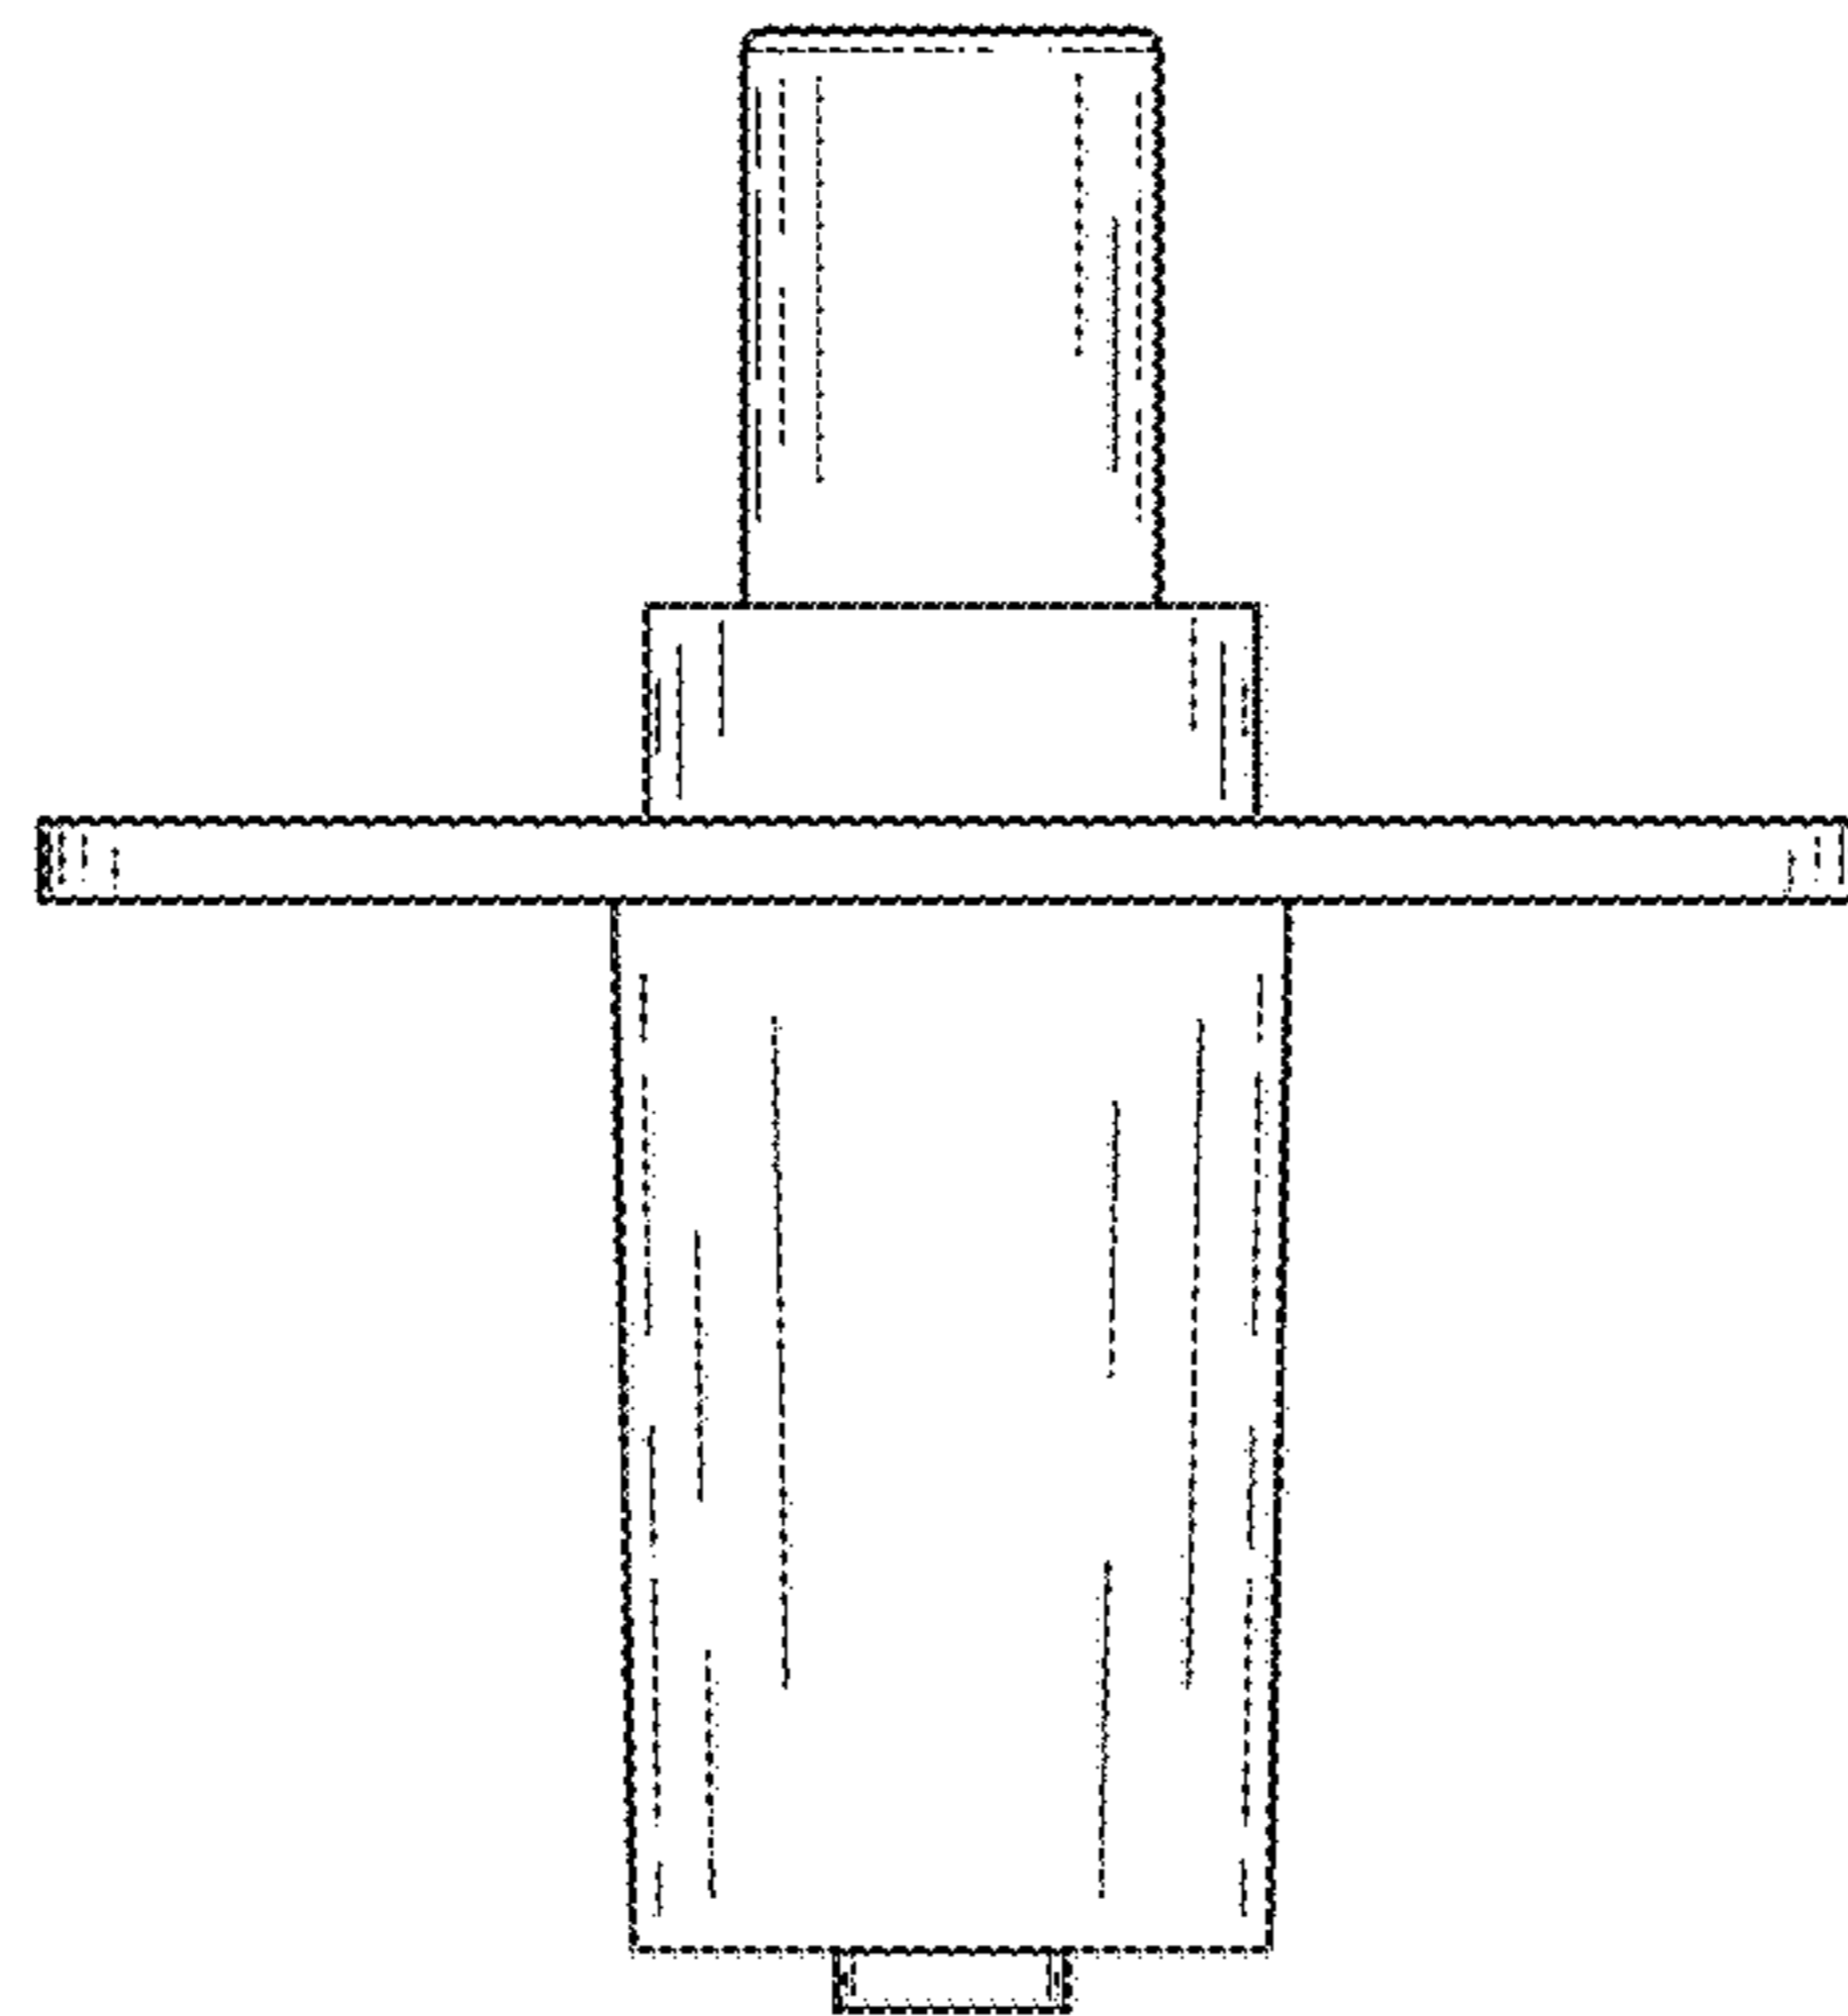


Fig. 2

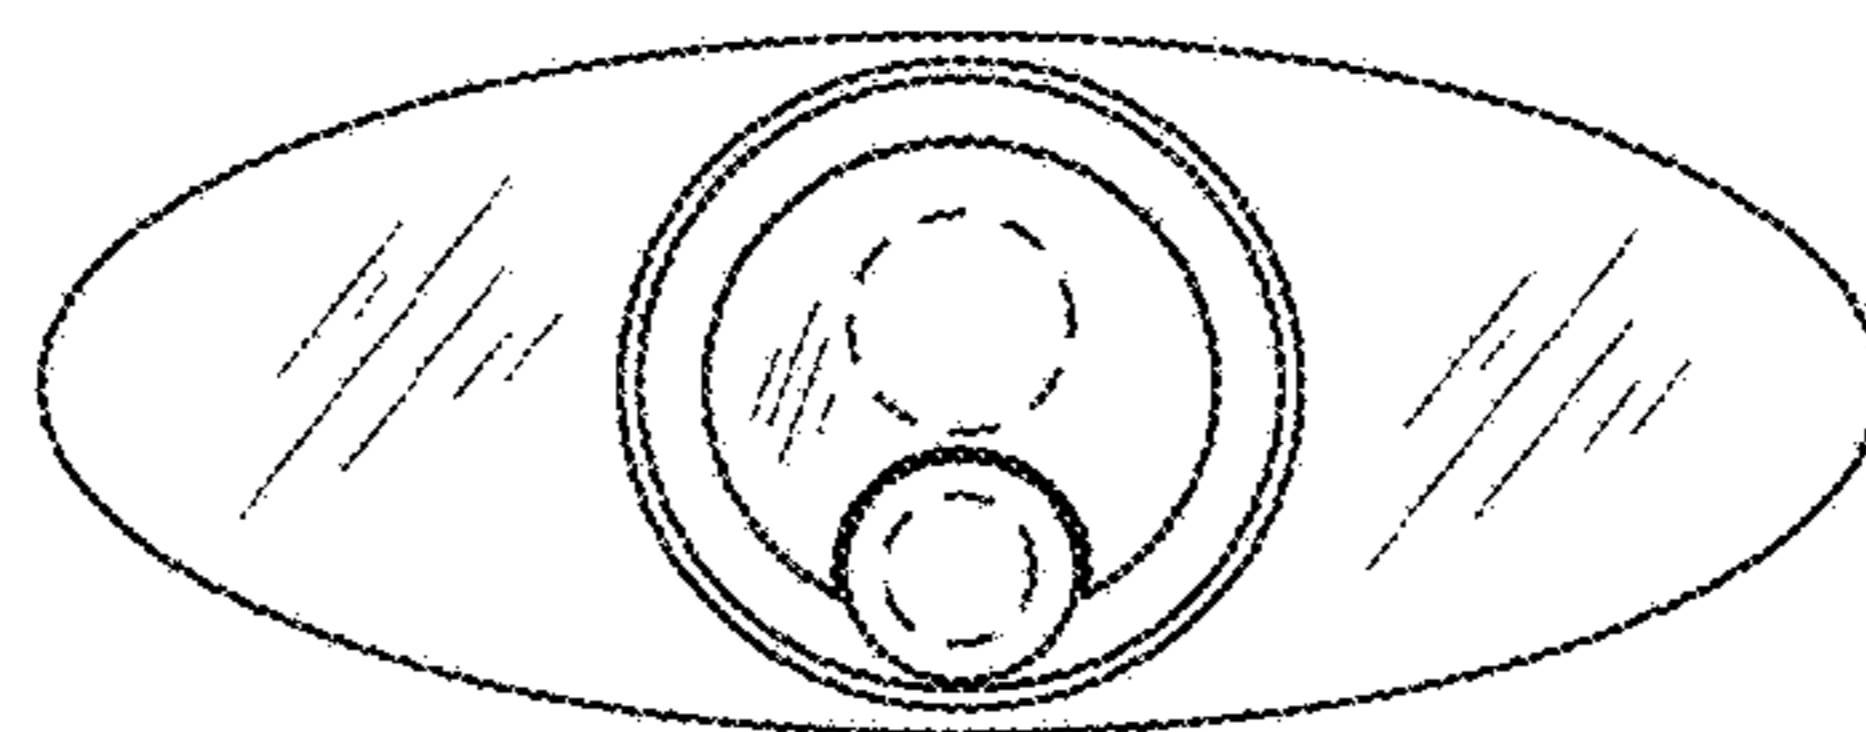


Fig. 3

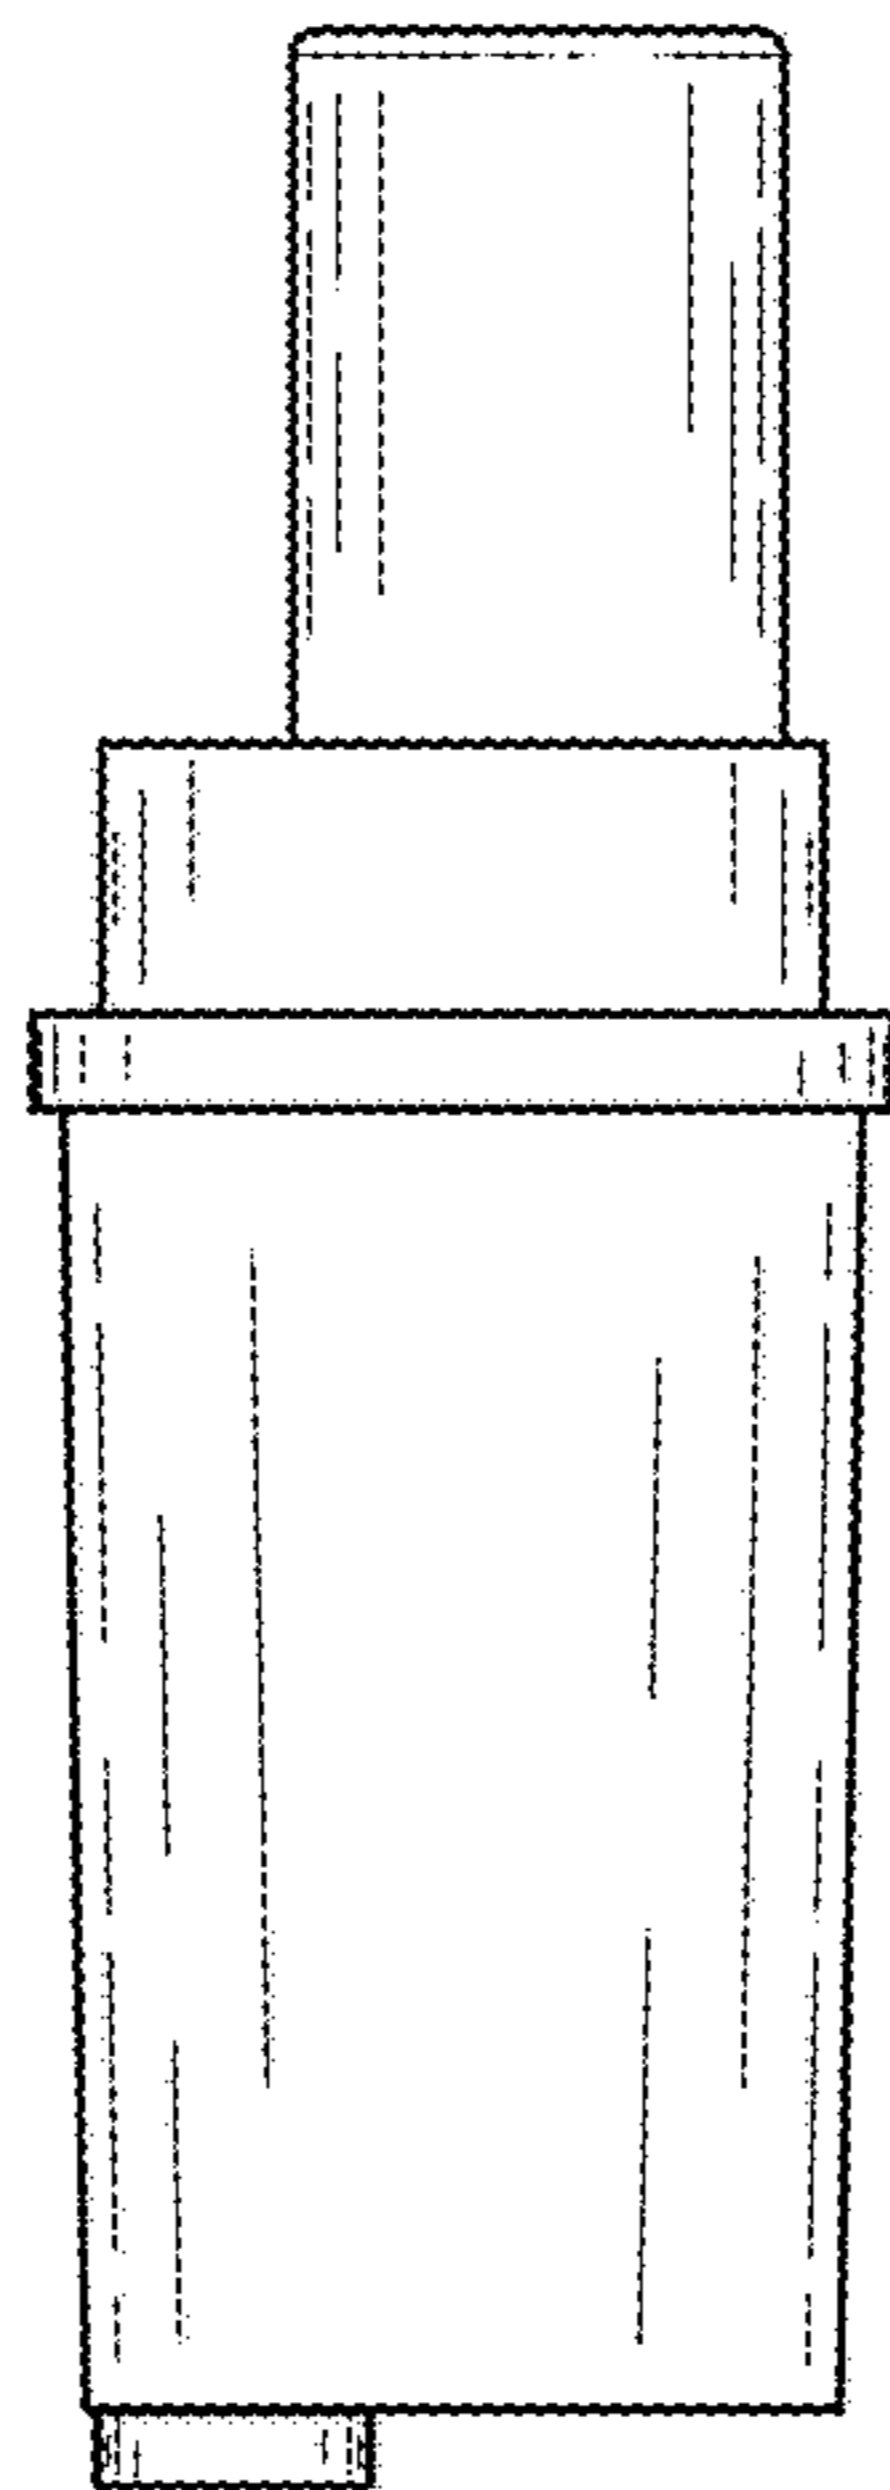


Fig. 4

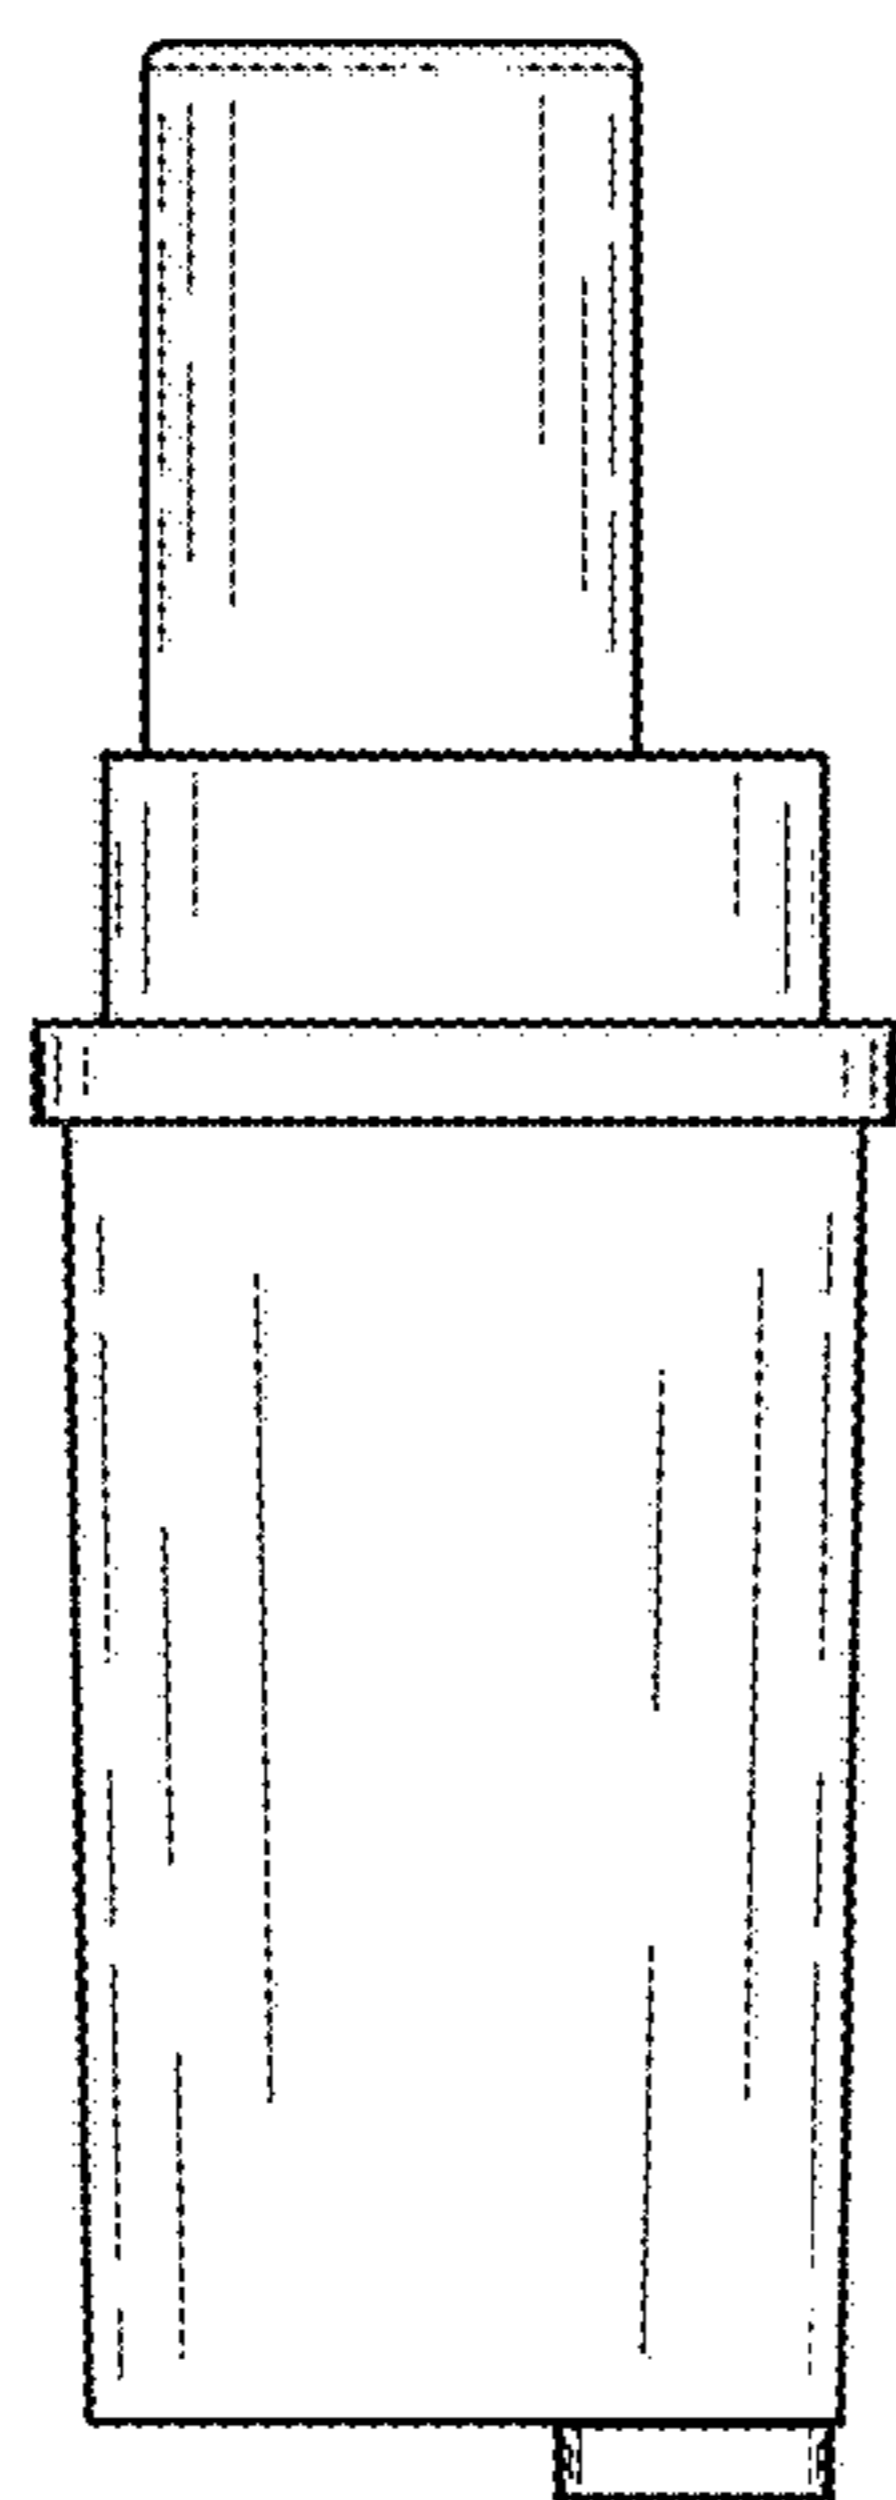


Fig. 5

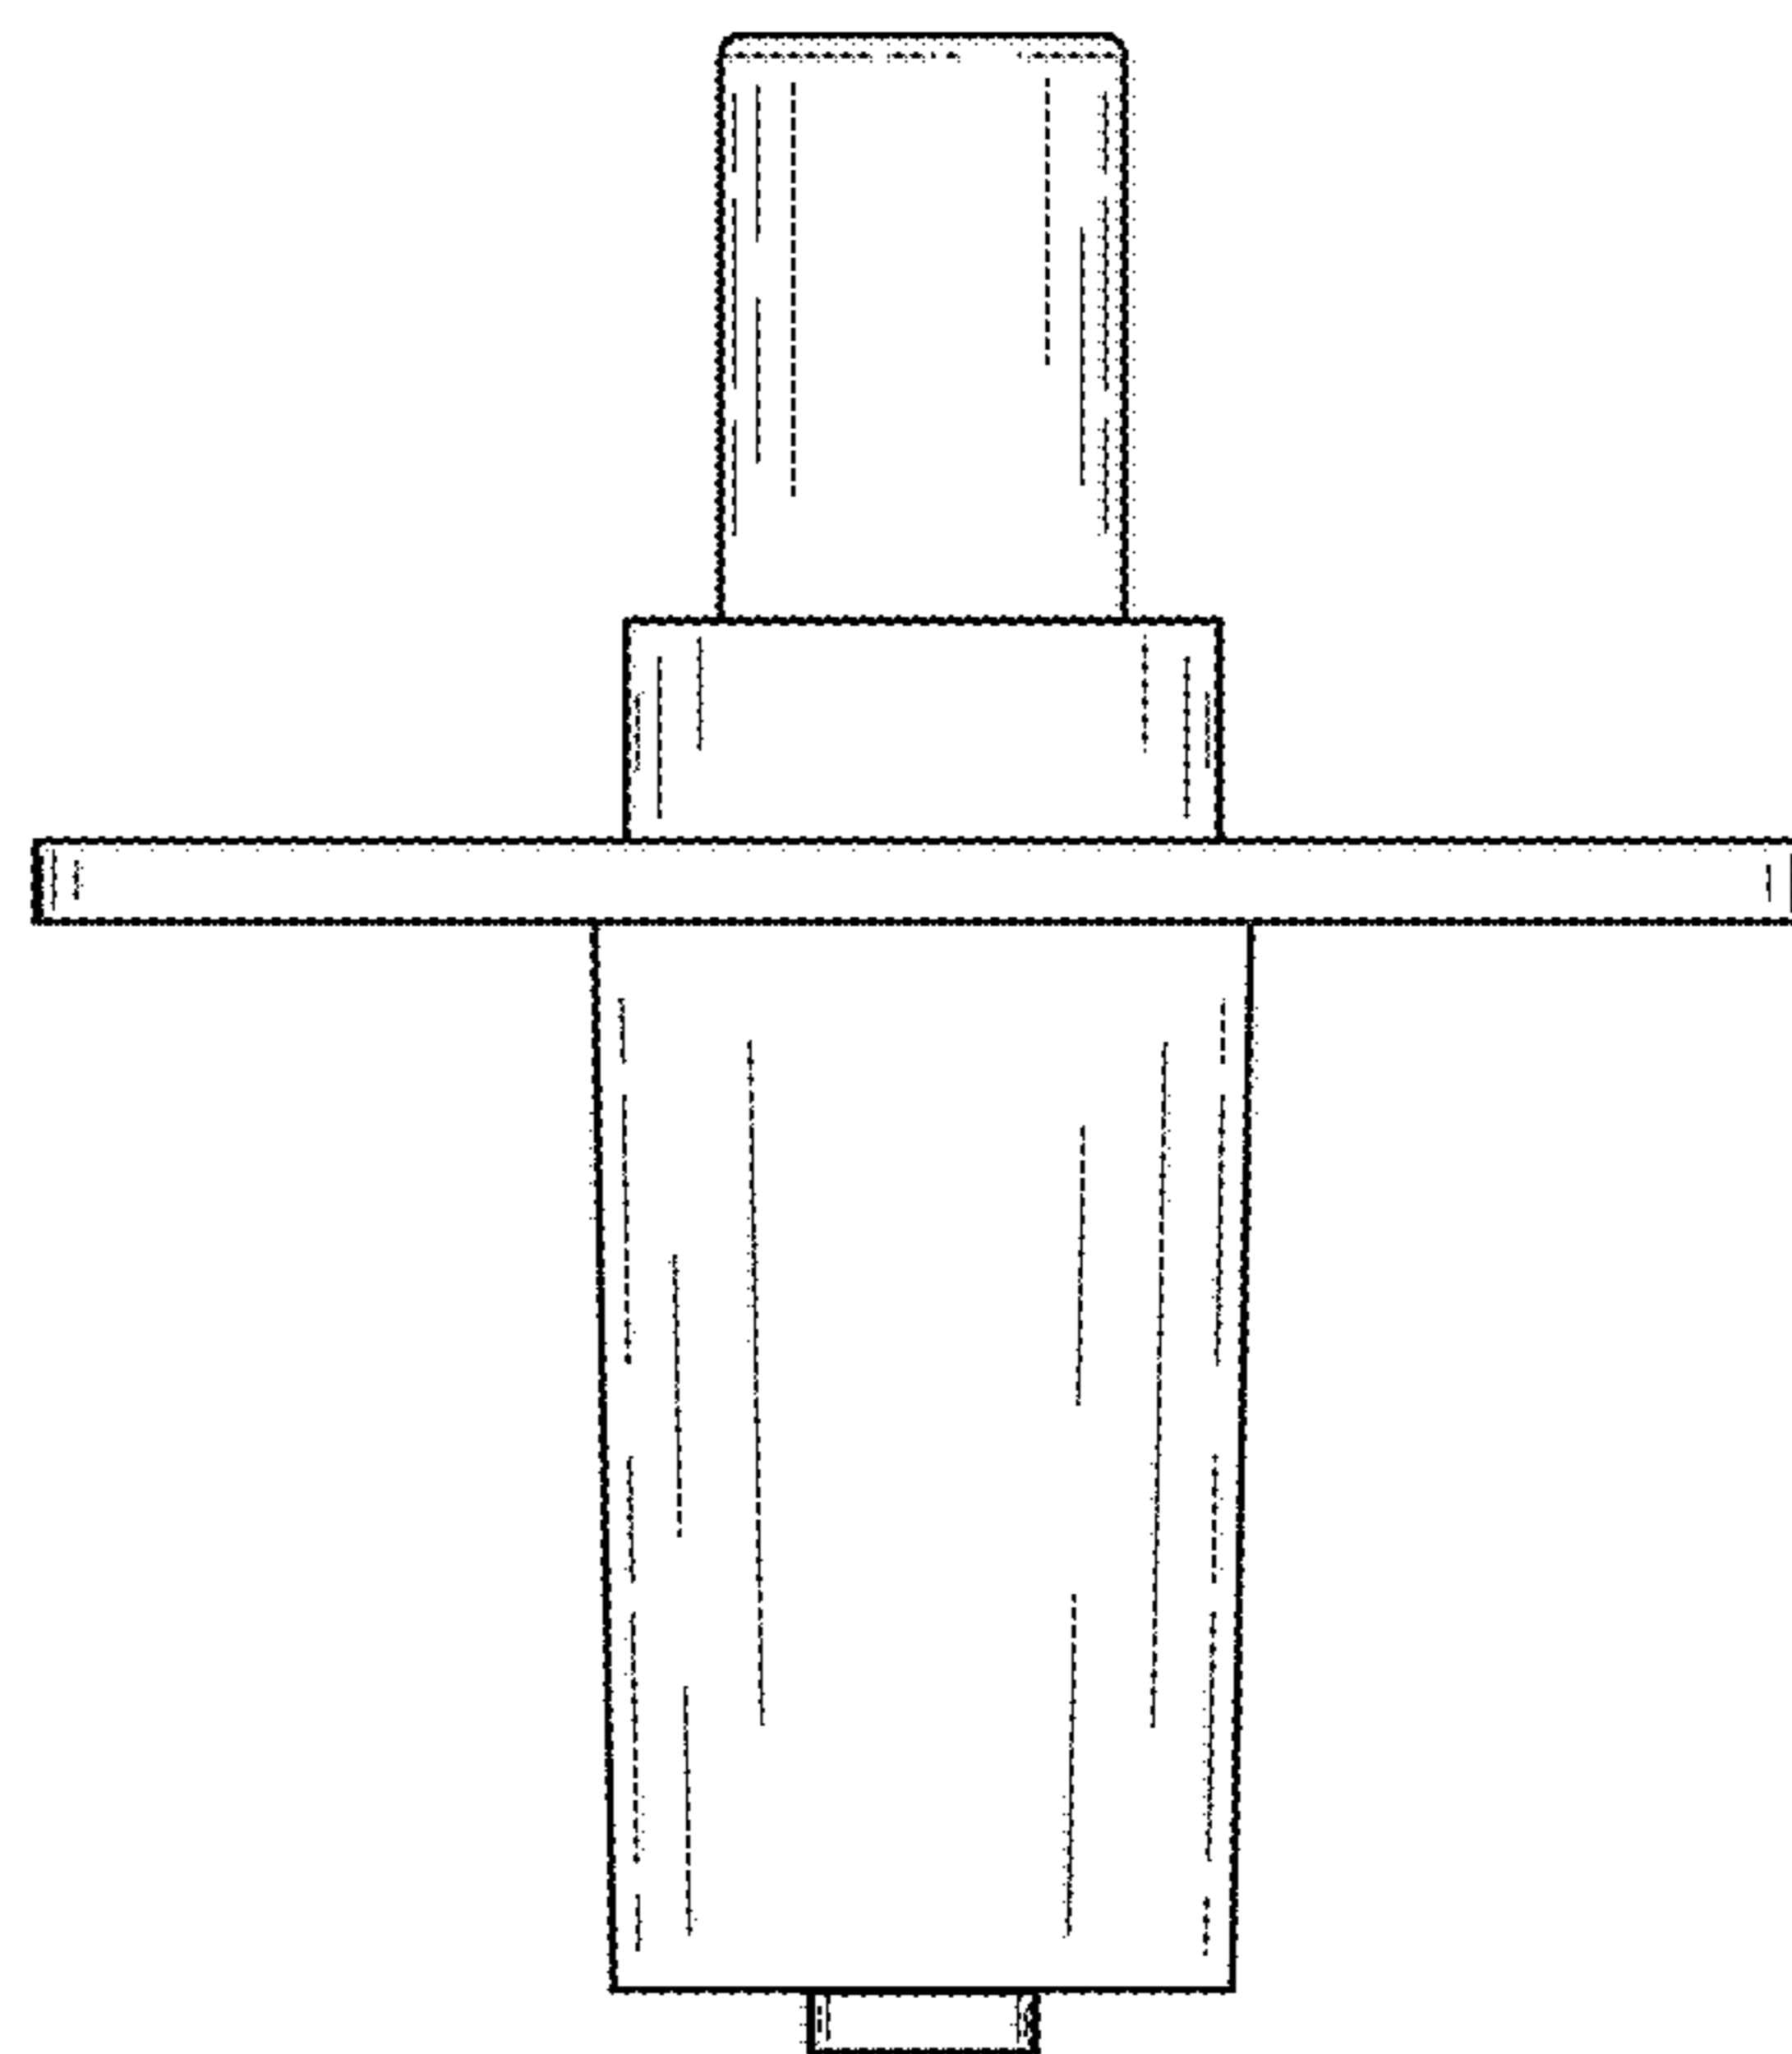


Fig. 6

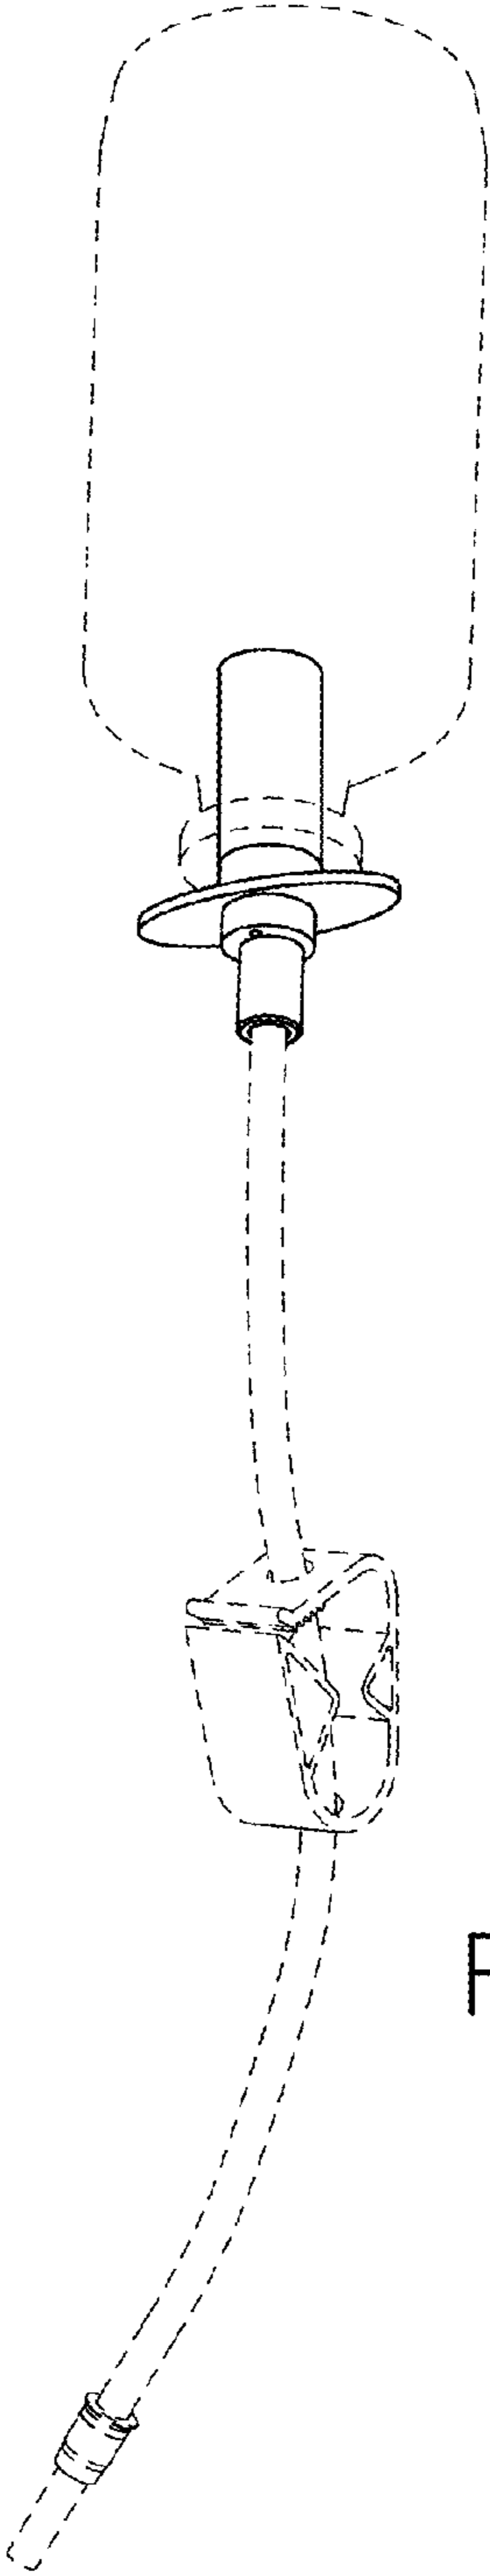


Fig. 7