



US00D847147S

(12) **United States Design Patent** (10) **Patent No.:** **US D847,147 S**
Wesley et al. (45) **Date of Patent:** **** Apr. 30, 2019**

(54) **GRAPHICAL DATA DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE**

(71) Applicant: **Park Nicollet Institute**, St. Louis Park, MN (US)

(72) Inventors: **David M. Wesley**, Hudson, WI (US); **Richard M. Bergenstal**, Plymouth, MN (US)

(73) Assignee: **Park Nicollet Institute**, St. Louis Park, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/581,882**

(22) Filed: **Oct. 24, 2016**

Related U.S. Application Data

(62) Division of application No. 29/450,104, filed on Mar. 15, 2013, now Pat. No. Des. 773,478.

(51) **LOC (11) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485-488
CPC A61B 5/742; A61B 5/743; A61B 5/14532
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,559,868 B2	5/2003	Alexander et al.
D519,517 S	4/2006	Reynolds et al.
D525,264 S	7/2006	Chotai et al.
D573,601 S	7/2008	Gregov et al.
D589,976 S	4/2009	Hosokawa et al.
D630,648 S	1/2011	Tokunaga et al.
D630,649 S	1/2011	Tokunaga et al.

D632,699 S	2/2011	Judy et al.
D633,514 S	3/2011	Tokunaga et al.
8,041,714 B2	10/2011	Aymeloglu et al.
D652,048 S	1/2012	Joseph
D652,052 S	1/2012	Judy et al.
8,133,178 B2	3/2012	Brauker
D661,313 S	6/2012	Nenoki
D667,417 S	9/2012	Long et al.
D674,404 S	1/2013	Pearcy et al.
D674,812 S	1/2013	Joseph
D681,651 S	5/2013	Fletcher et al.
D684,172 S	6/2013	Rytt et al.

(Continued)

OTHER PUBLICATIONS

Bergenstal, Ricard M. et. al., Recommendations for Standardizing Glucose Reporting and Analysis to Optimize Clinical Decision Making in Diabetes: The Ambulatory Glucose Profile (AGP), Diabetes Technology & Therapeutics 15(3), <https://www.researchgate.net/publication/235755545>, Feb. 2013, 2 pages.

(Continued)

Primary Examiner — Richelle G Shelton

(74) *Attorney, Agent, or Firm* — Merchant & Gould P.C.


(57) **CLAIM**

The ornamental design for a graphical data display screen with graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a first embodiment of a graphical data display screen with graphical user interface; and, FIG. 2 is a front view of a second embodiment thereof. The alternating long and short dashes which represent the display screen and the boundary of the claimed design form no part of the claimed design. The remaining broken lines represent elements of the graphical user interface and form no part of the claimed design.

1 Claim, 2 Drawing Sheets

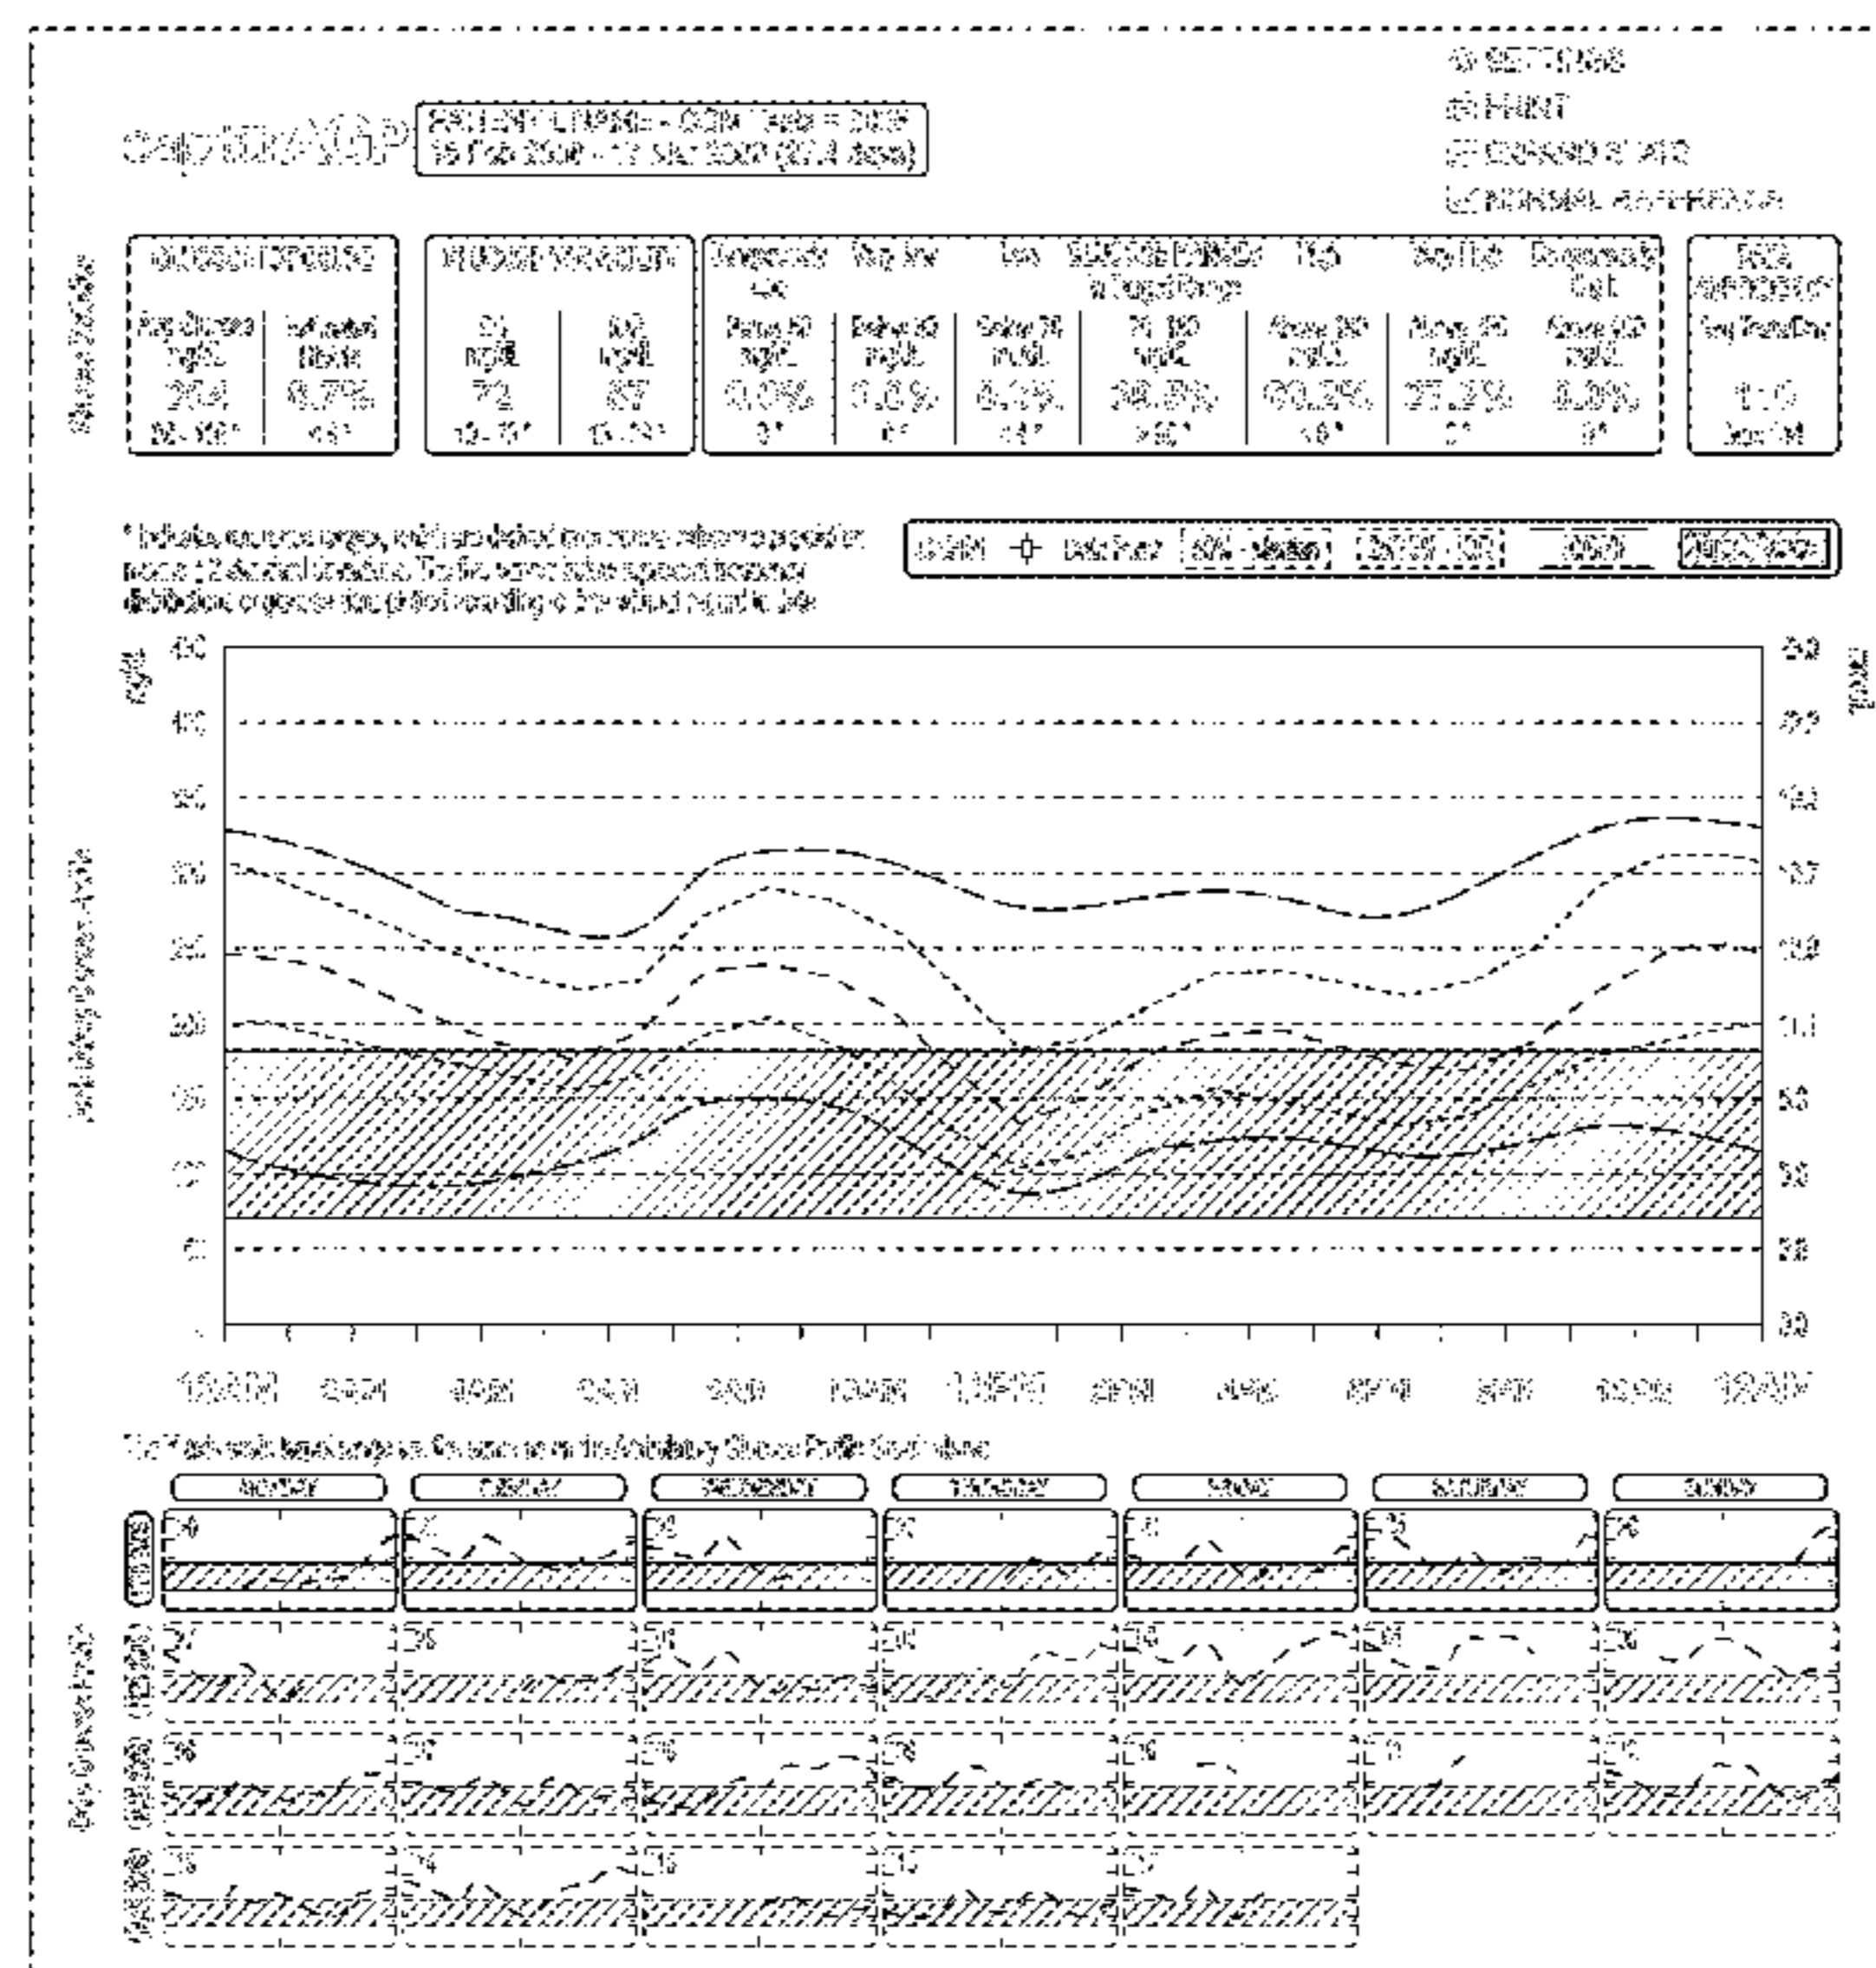

(56)

References Cited

U.S. PATENT DOCUMENTS

D685,810 S 7/2013 Way et al.
 D690,309 S 9/2013 Wenz et al.
 D692,911 S 11/2013 Pearcy et al.
 D709,082 S 7/2014 Meegan et al.
 D709,518 S 7/2014 Meegan et al.
 D710,373 S 8/2014 Meegan et al.
 D717,328 S 11/2014 Lin
 D717,331 S 11/2014 Lin
 D756,371 S 5/2016 Bertnick
 D757,071 S 5/2016 Kouvas et al.
 D759,073 S 6/2016 Winklevoss
 D773,478 S 12/2016 Wesley et al.
 D774,058 S 12/2016 Dias et al.
 D775,144 S 12/2016 Vazquez
 D780,199 S 2/2017 Croan
 D785,008 S 4/2017 Lim et al.
 D800,757 S 10/2017 Mullen et al.
 D802,001 S * 11/2017 Javed D14/486
 D817,977 S * 5/2018 Kato D14/485
 2002/0193679 A1 12/2002 Malave et al.
 2003/0216621 A1* 11/2003 Alpert A61B 5/0215
 600/300
 2008/0127052 A1 5/2008 Rostoker
 2009/0029631 A1 1/2009 Offer et al.
 2009/0147026 A1 6/2009 Buck et al.
 2009/0238597 A1 9/2009 Cao et al.
 2010/0096474 A1 4/2010 Zhang et al.

2010/0100470 A1 4/2010 Buchanan et al.
 2012/0004947 A1 1/2012 Dombrowski et al.
 2014/0028682 A1 1/2014 Omiya
 2014/0188400 A1 7/2014 Dunn et al.
 2014/0206970 A1 7/2014 Wesley et al.

OTHER PUBLICATIONS

Verdeccia, Paolo et. al., Ambulatory Blood Pressure and Cardiovascular Outcome in Relation to Perceived Sleep Deprivation, <http://hyper.ahajournals.org/content/49/4/777/tab-article-info>, Mar. 21, 2011, 2 pages.
 Designing Information Systems, 1.2 Designing Information Systems, <https://saylordotorg.github.io>, Mar. 26, 2011, 3 pages.
 Wall St. Warrior, Technical Picture—Bearish Island Reversal Within a Bear Flag Pattern, <http://traderjamie.blogspot.com/2011/09/technical-picture-bearish-island.html>, Sep. 3, 2011, 2 pages.
 PCT International Searching Authority, International Search Report and Written Opinion dated Sep. 5, 2014 for Int'l Application No. PCT/US2014/012549, 11 pages.
 Bergenstal MD, Rich, SMBG & CGM in Clinical Practice, Barbara Davis Center Keystone Conference 2012, Jul. 15, 2012, 50 pages.
 Mazze, Roger S., Characterizing Glucose Exposure for Individuals with Normal Glucose Tolerance Using Continuous Glucose Monitoring and Ambulatory Glucose Profile Analysis, Diabetes Technology & Therapeutics, vol. 10, No. 3, Jun. 1, 2008, pp. 149-159.

* cited by examiner

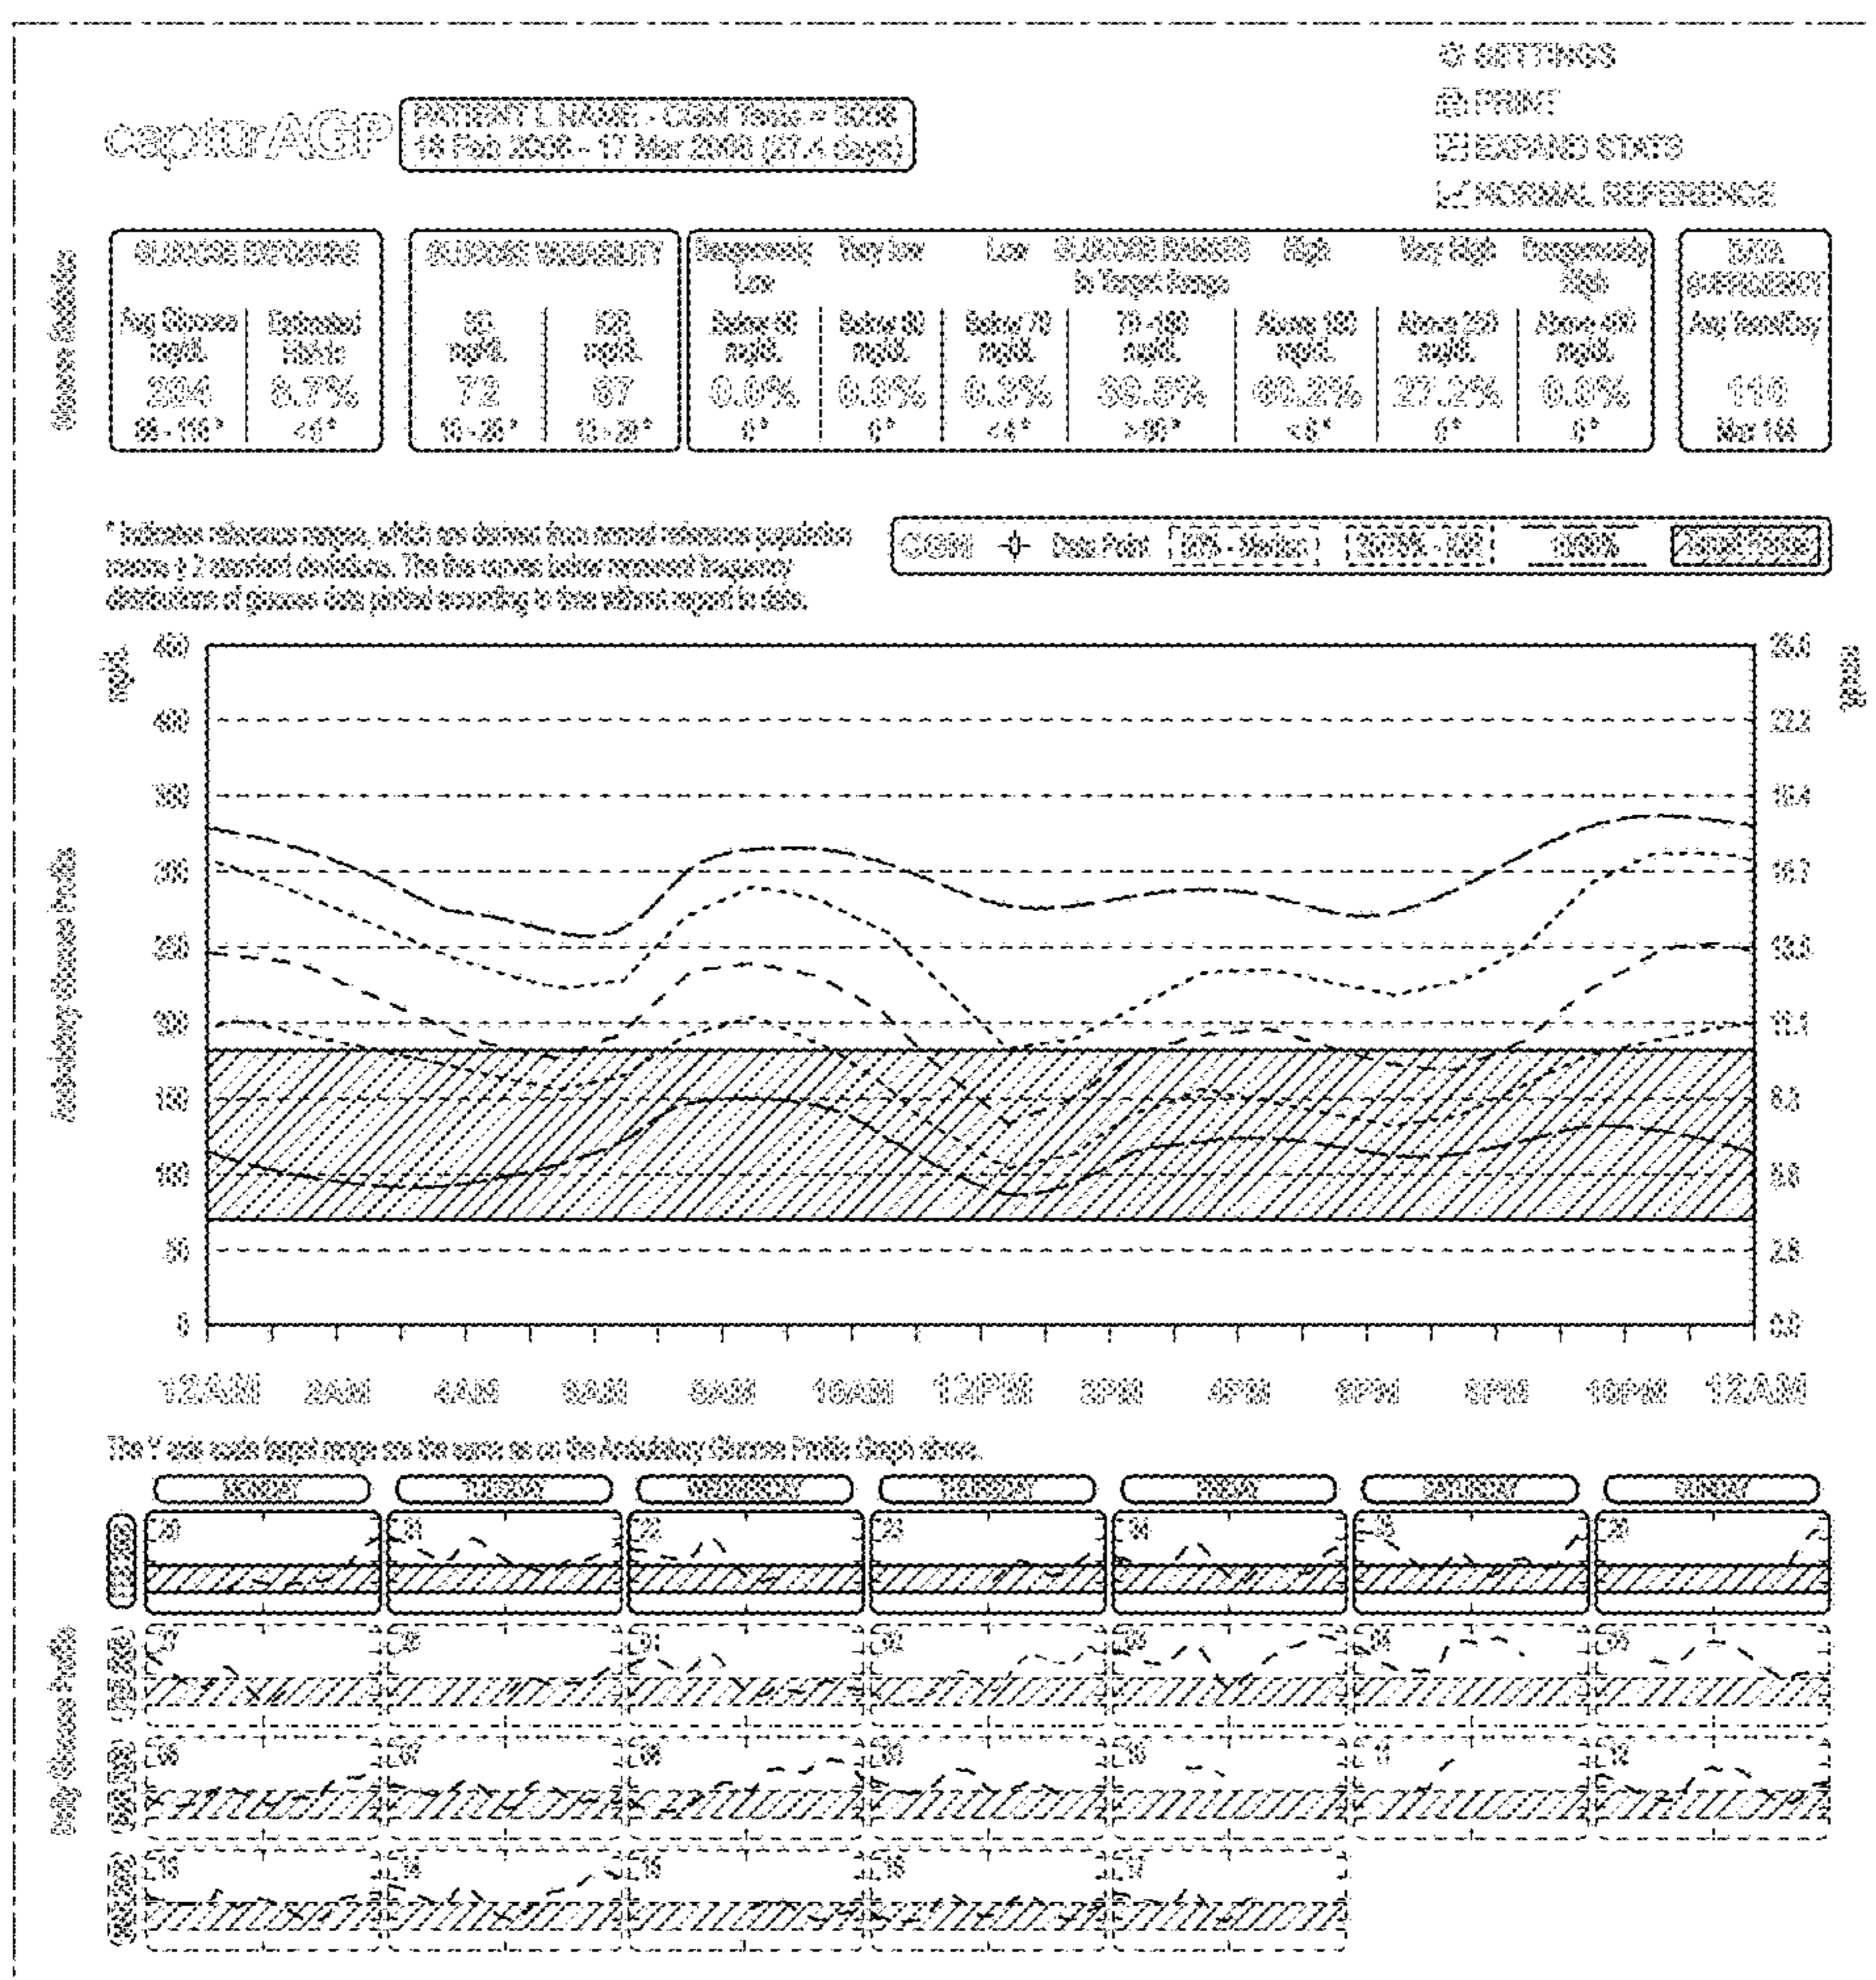


FIG. 1

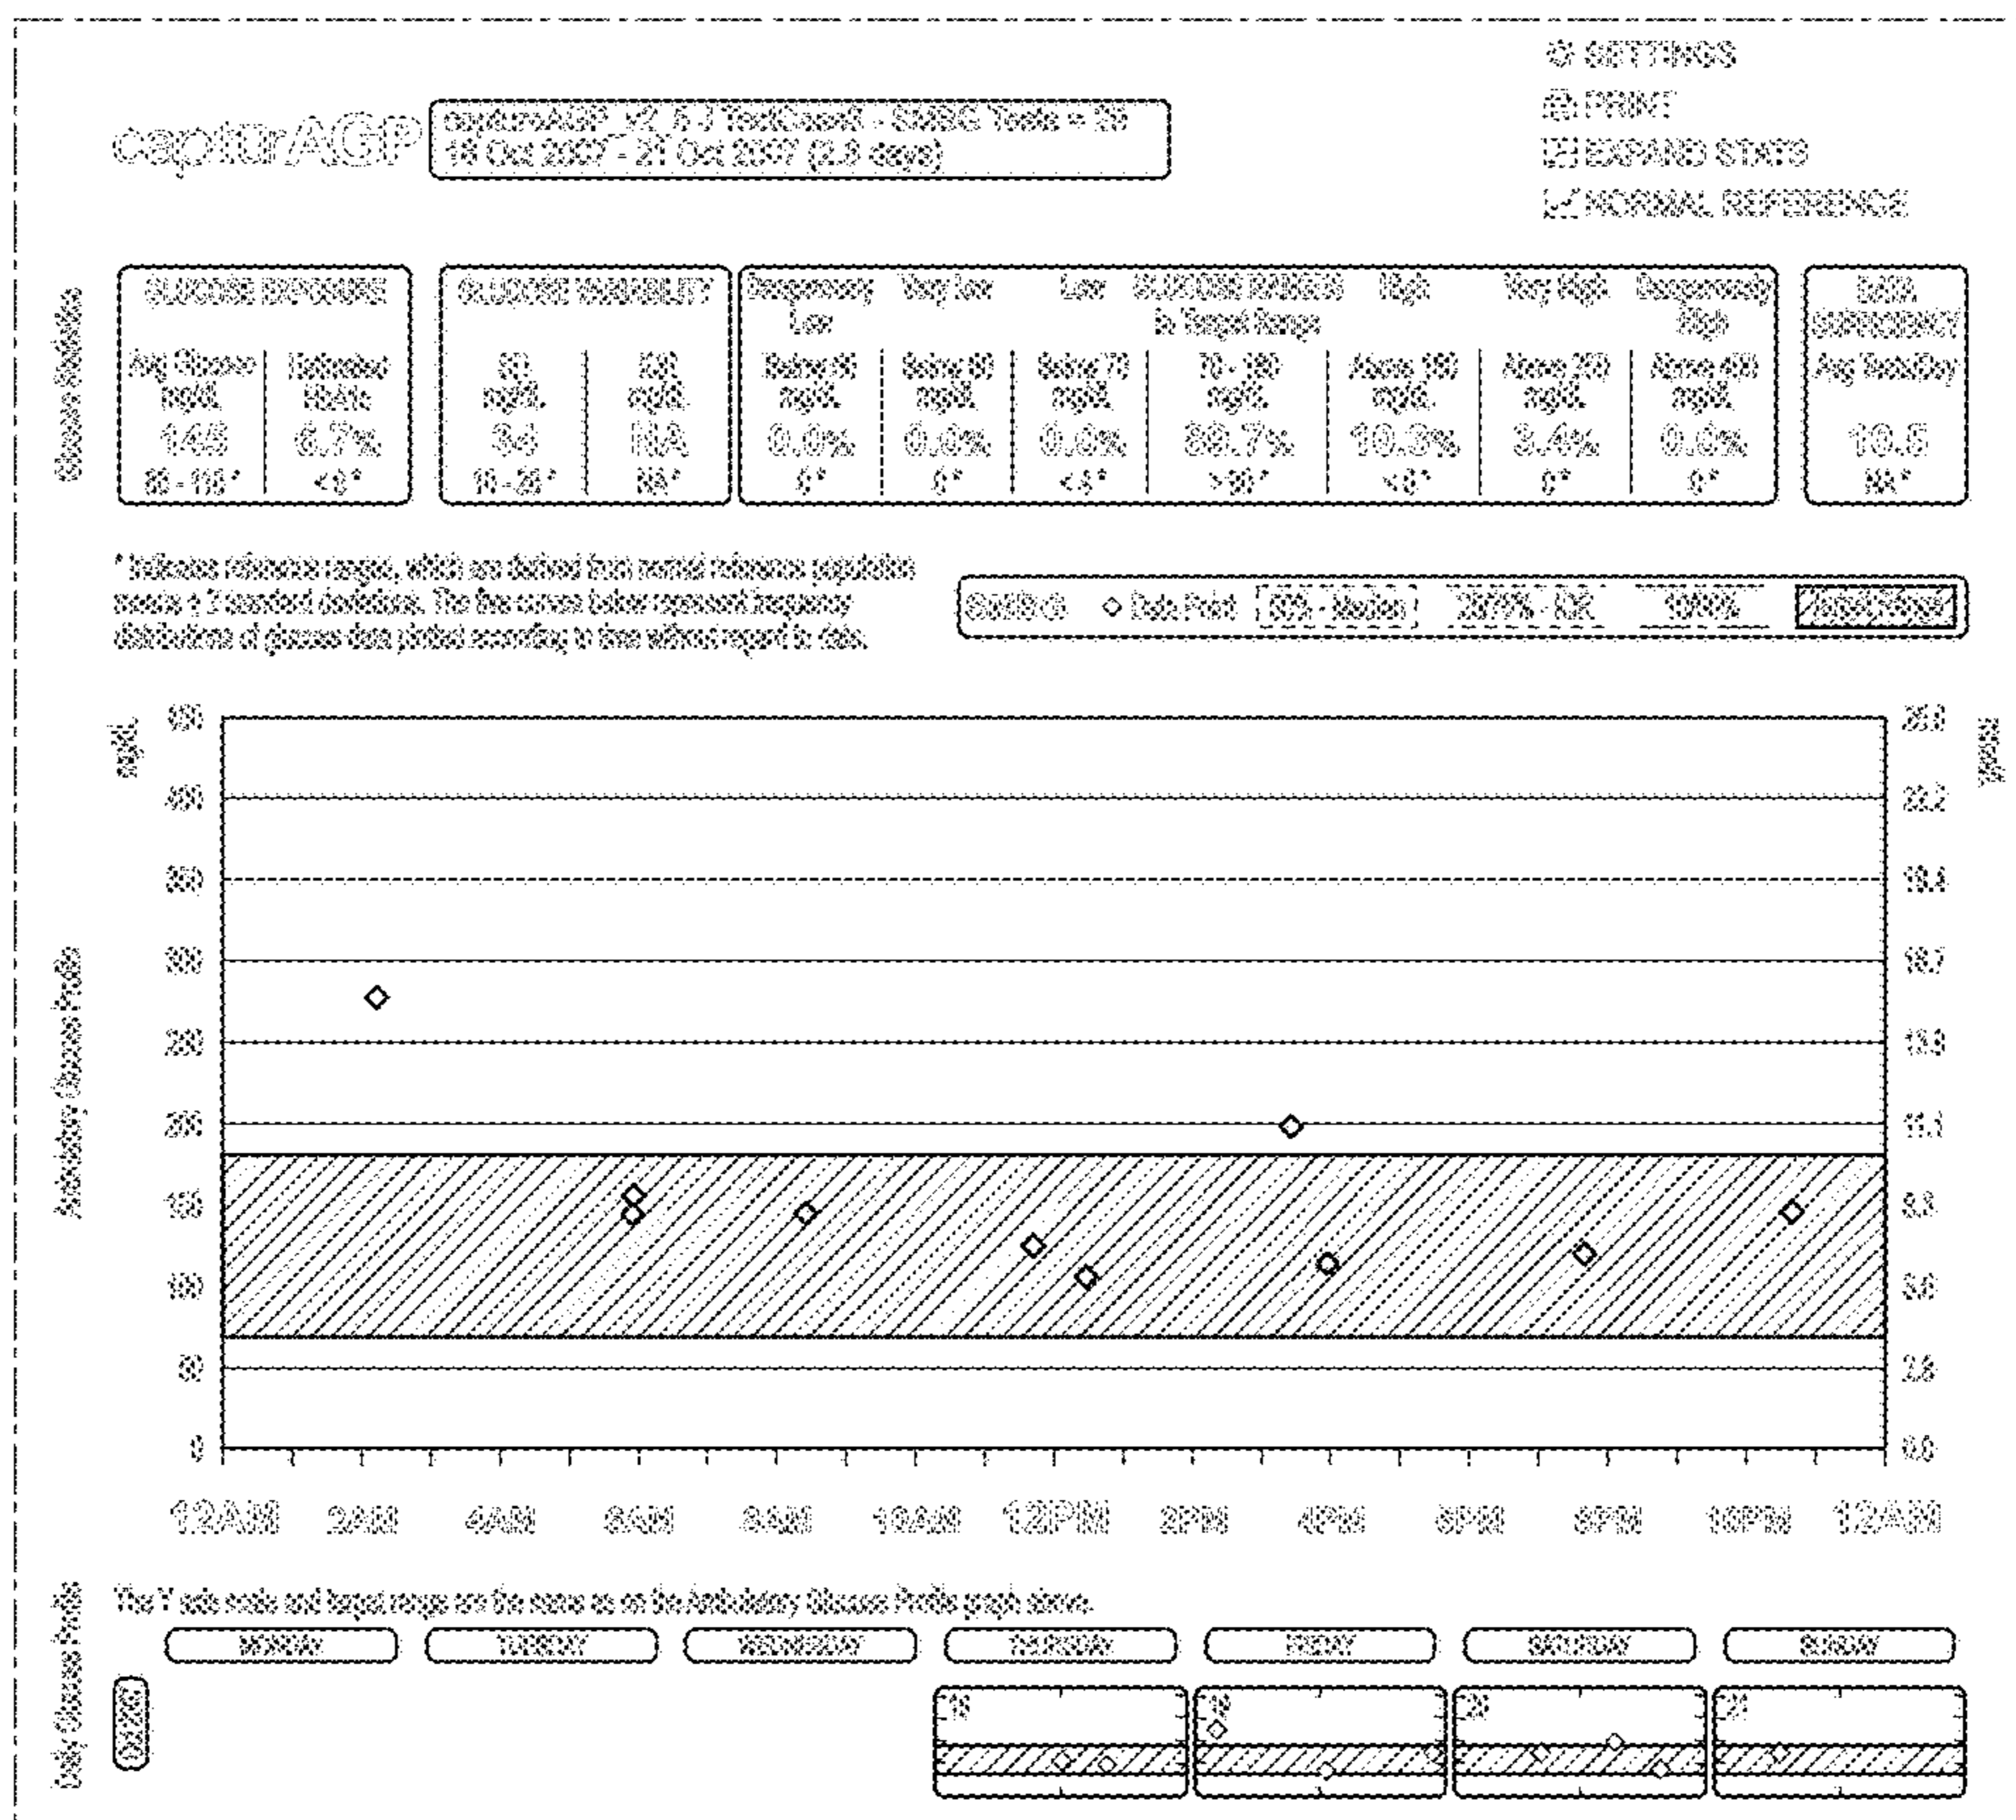


FIG. 2