



US00D847992S

(12) **United States Design Patent** (10) **Patent No.:** **US D847,992 S**
Adams et al. (45) **Date of Patent:** **** May 7, 2019**

(54) **MEDICAL DEVICE HANDLE** D329,092 S * 9/1992 Carusillo D24/146
5,190,542 A 3/1993 Nakao et al.
(71) Applicant: **POLYGON MEDICAL, INC.,** 5,201,740 A 4/1993 Nakao et al.
Newton, MA (US) 5,271,414 A 12/1993 Partika et al.
5,327,896 A 7/1994 Schmieding
(72) Inventors: **Ronald D. Adams**, Holliston, MA 5,336,227 A 8/1994 Nakao et al.
(US); **Danial Ferreira**, Woodbridge, CT 5,347,991 A 9/1994 Nakao et al.
(US); **Paul Dicesare**, Easton, CT (US) 5,363,860 A 11/1994 Nakao et al.
5,395,313 A 3/1995 Naves et al.
(73) Assignee: **POLYGON MEDICAL, INC.,** 5,417,697 A 5/1995 Wilk et al.
Newton, MA (US) 5,423,830 A 6/1995 Schneebaum et al.
(Continued)

(**) Term: **15 Years**

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **29/608,903**
(22) Filed: **Jun. 27, 2017**
(51) **LOC (11) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/146**
(58) **Field of Classification Search**
USPC D24/127, 130, 133, 146, 147, 148;
D8/93, 97, 300, 310, 311, 313; D19/110,
D19/115; D7/649
CPC B26B 3/00; B26B 1/10; A61B 17/089;
A61B 17/1617; A61B 17/3211; A61B
17/3417; A61B 17/1411; A61B 17/1624;
A61B 17/162; A61B 17/1622; A61B
17/00424
See application file for complete search history.

WO WO 2014/081812 5/2014
Primary Examiner — Cathron C Brooks
Assistant Examiner — Samantha Q Lawrence
(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson
& Bear LLP

(57) **CLAIM**

The ornamental design for a medical device handle, as shown and described.


DESCRIPTION

FIG. 1 is a front, top, and side perspective view of a medical device handle embodying our new design.
FIG. 2 is a left side view thereof.
FIG. 3 is a right side view thereof.
FIG. 4 is a front view thereof.
FIG. 5 is a back view thereof.
FIG. 6 is a top view thereof; and,
FIG. 7 is a bottom view thereof.
Broken lines are used to illustrate features of the medical device handle which form no part of the claimed design. Break lines are used to indicate that any portion of the medical device handle between the break lines forms no part of the claimed design.

(56) **References Cited**
U.S. PATENT DOCUMENTS

3,882,849 A 5/1975 Jamshidi
4,603,694 A 8/1986 Wheeler
4,620,547 A 11/1986 Boebel
4,651,753 A 3/1987 Lifton
4,678,459 A 7/1987 Onik et al.
4,811,734 A 3/1989 McGurk-Burleson et al.
4,958,625 A 9/1990 Bates et al.
4,961,430 A 10/1990 Sheahon
5,061,238 A 10/1991 Shuler

1 Claim, 7 Drawing Sheets

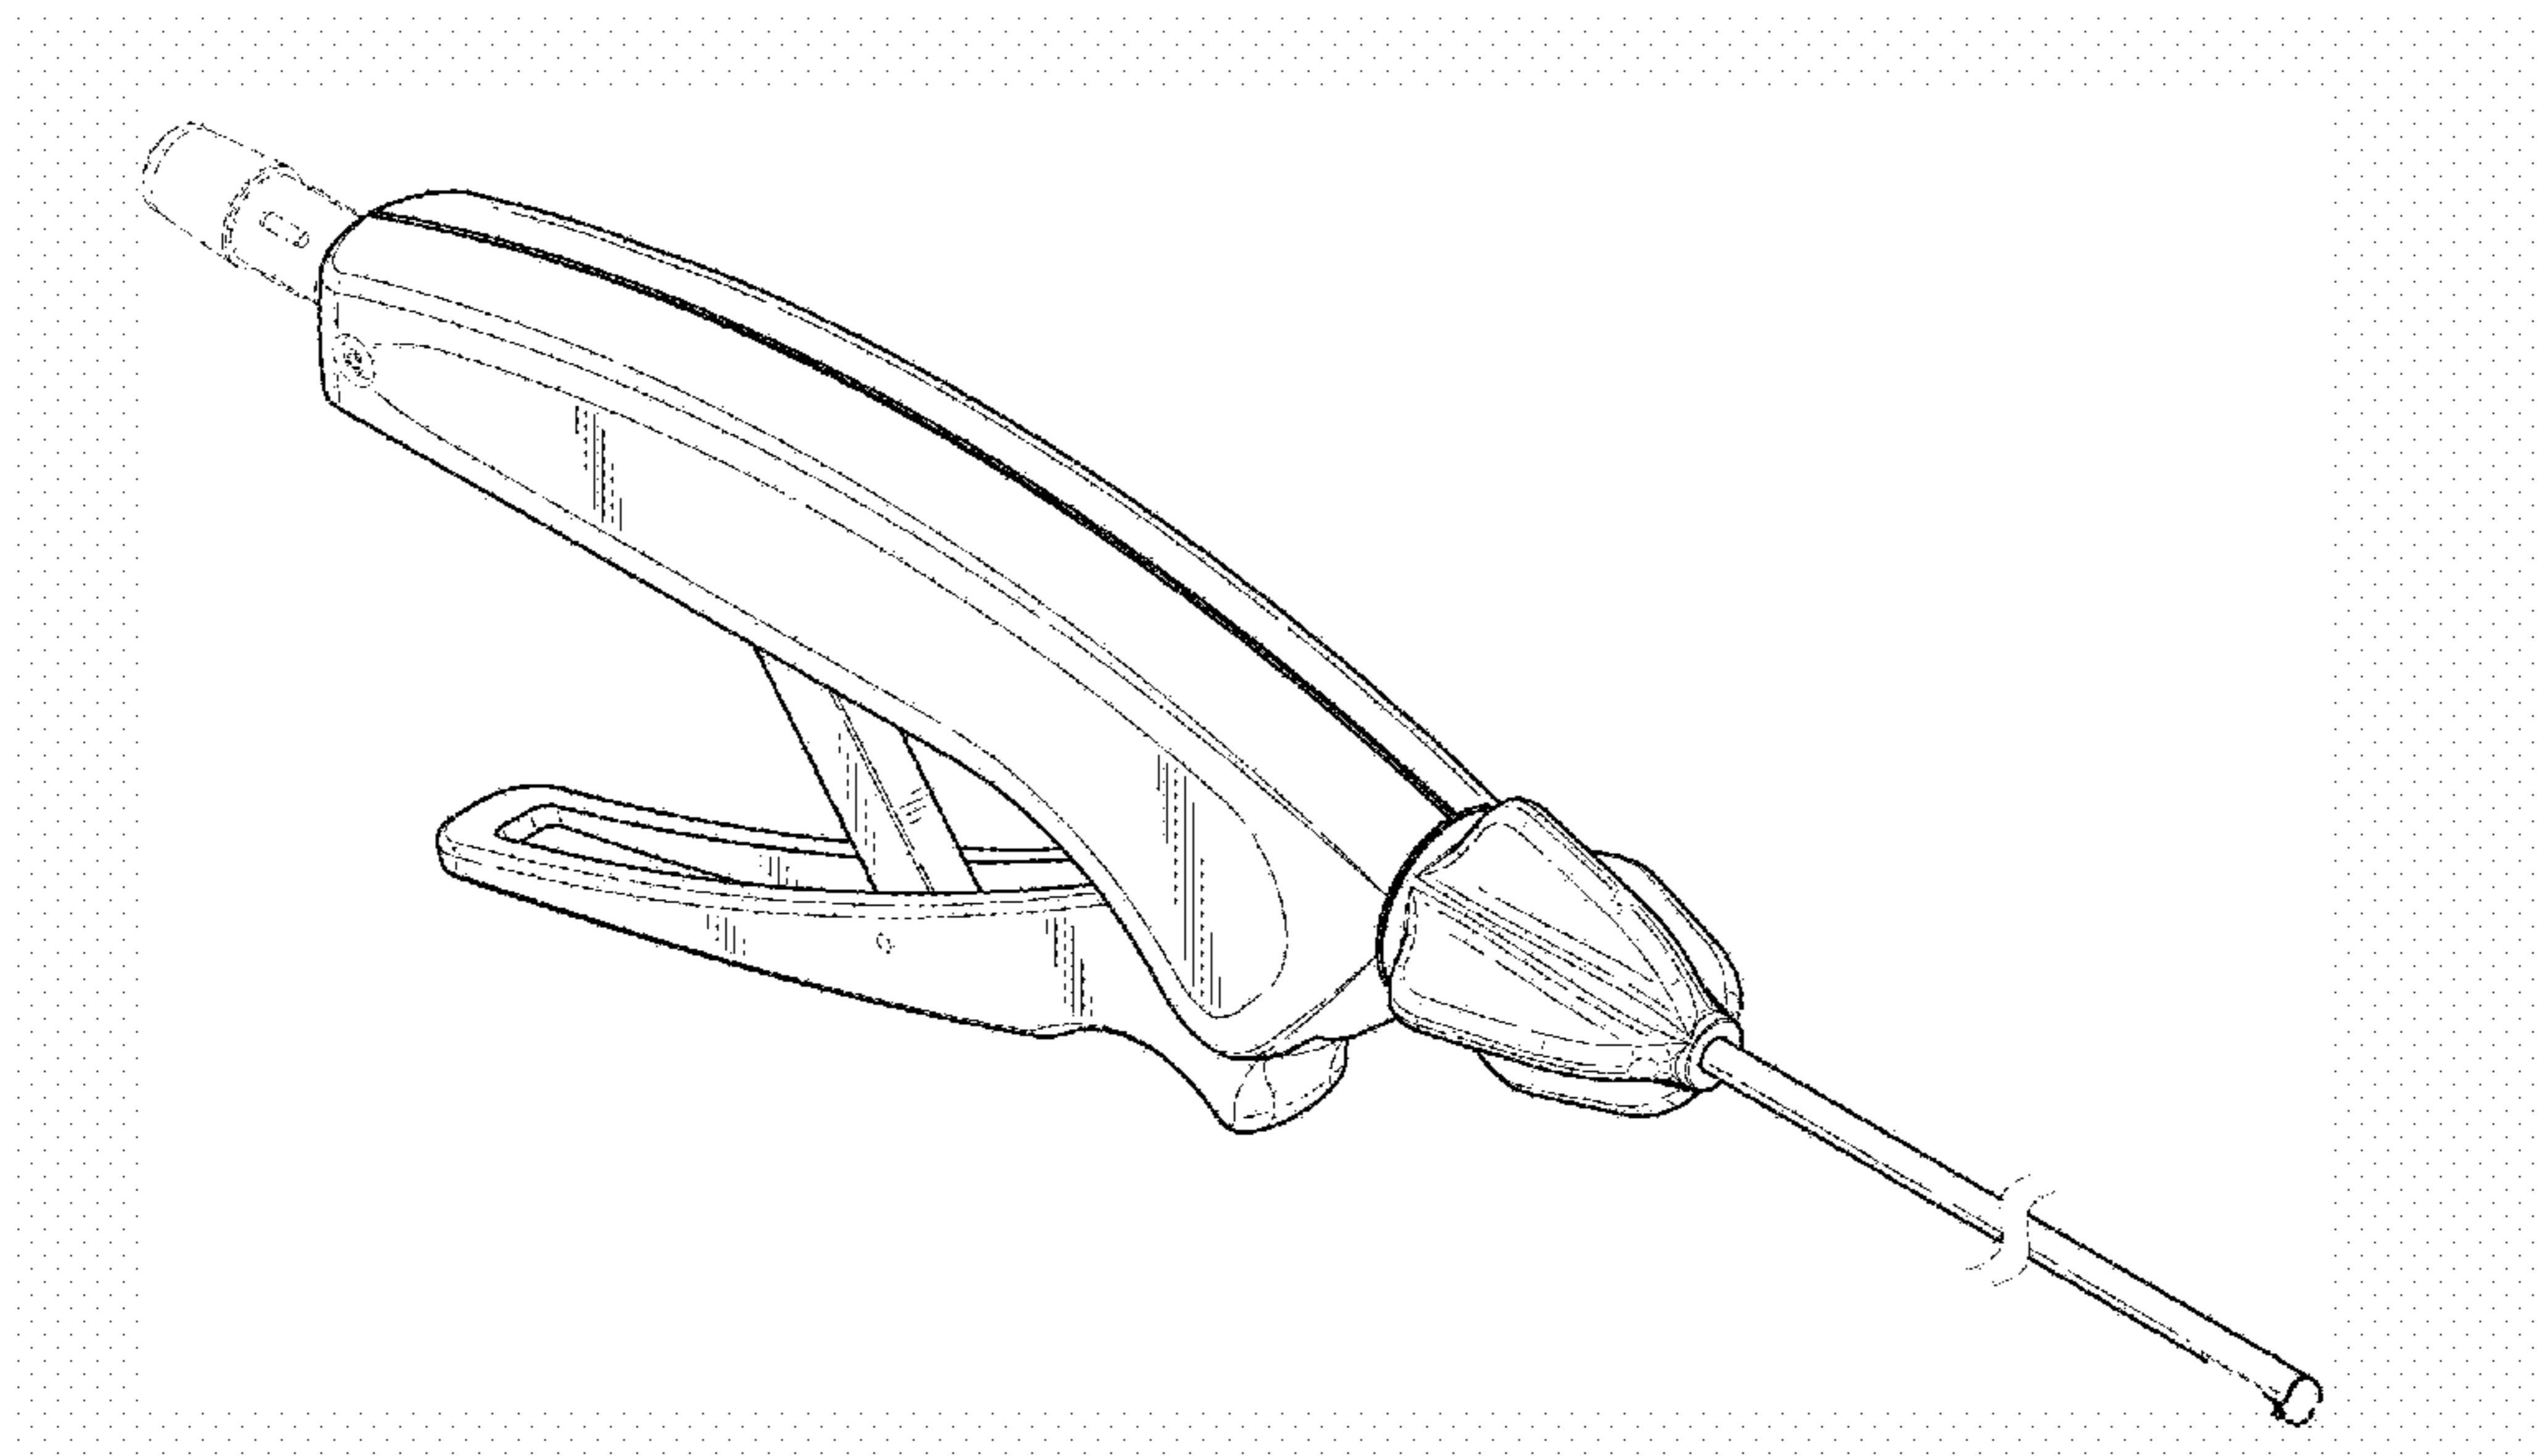

(56)

References Cited

U.S. PATENT DOCUMENTS

5,423,844	A	6/1995	Miller	
5,439,474	A	8/1995	Li	
D364,463	S *	11/1995	Pitzen	D24/146
5,486,182	A	1/1996	Nakao et al.	
5,527,332	A	6/1996	Clement	
5,601,583	A	2/1997	Donahue et al.	
5,649,547	A	7/1997	Ritchart et al.	
5,741,271	A	4/1998	Nakao et al.	
5,741,287	A	4/1998	Alden et al.	
5,746,747	A	5/1998	McKeating	
5,759,187	A	6/1998	Nakao et al.	
5,782,849	A	7/1998	Miller	
5,797,907	A	8/1998	Clement	
5,810,806	A	9/1998	Ritchart et al.	
5,814,052	A	9/1998	Nakao et al.	
5,871,454	A	2/1999	Majlessi	
5,906,620	A	5/1999	Nakao et al.	
5,993,454	A *	11/1999	Longo	A61B 17/1624 606/80
5,997,547	A	12/1999	Nakao et al.	
6,007,495	A	12/1999	Matula	
6,022,362	A	2/2000	Lee et al.	
6,068,603	A	5/2000	Suzuki	
6,165,137	A	12/2000	Milliman et al.	
6,171,315	B1	1/2001	Chu et al.	
6,383,198	B1	5/2002	Hamilton	
6,428,498	B2	8/2002	Uflacker	
6,454,727	B1	9/2002	Burbank et al.	
6,530,923	B1	3/2003	Dubrul et al.	
6,616,659	B1	9/2003	de la Torre et al.	
6,626,850	B1	9/2003	Chau et al.	
6,638,235	B2	10/2003	Miller et al.	
6,887,209	B2	5/2005	Kadziauskas et al.	
6,960,172	B2	11/2005	McGuckin, Jr. et al.	
7,115,125	B2	10/2006	Nakao et al.	
D594,983	S *	6/2009	Price	D24/133
D618,797	S *	6/2010	Price	D24/133
D620,593	S *	7/2010	Tran	D24/144
7,806,894	B1	10/2010	Rosenblatt et al.	
7,854,706	B2	12/2010	Hibner	
D631,965	S *	2/2011	Price	D24/133
7,922,737	B1	4/2011	Cesarini et al.	
7,988,642	B2	8/2011	Hardin et al.	
8,202,229	B2	6/2012	Miller et al.	
8,277,393	B2	10/2012	Miller et al.	
8,292,909	B1	10/2012	DuBois et al.	
8,298,254	B2	10/2012	DuBois et al.	
D670,380	S *	11/2012	Sapalev	D24/133
8,357,103	B2	1/2013	Mark et al.	
8,430,825	B2	4/2013	Mark et al.	
8,485,989	B2	7/2013	Videbaek	
D687,549	S *	8/2013	Johnson	D24/133
D700,966	S *	3/2014	O'Leary	D24/146
8,690,793	B2	4/2014	Ranpura et al.	
D709,194	S *	7/2014	Miller	D24/143
8,790,276	B2	7/2014	Ritchart et al.	
8,845,621	B2	9/2014	Fojtik	
8,893,722	B2	11/2014	Emanuel	
8,979,890	B2 *	3/2015	Boudreaux	A61B 18/1445 606/207
9,060,760	B2	6/2015	Sullivan et al.	
9,095,366	B2	8/2015	Sullivan et al.	
D743,547	S *	11/2015	Chang	D24/146
9,237,921	B2 *	1/2016	Messerly	A61B 17/32006
9,339,288	B2	5/2016	Sullivan et al.	
D759,237	S *	6/2016	Heath	D24/133
D763,442	S *	8/2016	Price	D24/133
D785,794	S *	5/2017	Magno, Jr.	D24/146
9,700,333	B2 *	7/2017	Strobl	A61B 18/1445
9,707,012	B2	7/2017	Adams et al.	
9,724,118	B2 *	8/2017	Schulte	A61B 17/32006
D806,245	S *	12/2017	Halbert	D24/133
9,848,902	B2 *	12/2017	Price	A61B 17/32009
2002/0082519	A1	6/2002	Miller et al.	
2002/0198467	A1	12/2002	Finer	
2005/0182339	A1	8/2005	Lee et al.	
2006/0144548	A1	7/2006	Beckman et al.	
2007/0161925	A1	7/2007	Quick et al.	
2008/0306406	A1	12/2008	Thompson et al.	
2011/0087260	A1	4/2011	Seipel et al.	
2012/0172889	A1	7/2012	Chin et al.	
2013/0046316	A1	2/2013	Sullivan et al.	
2013/0053759	A1	2/2013	McCawley	
2013/0103041	A1	4/2013	Regadas	
2013/0211321	A1	8/2013	Dubois et al.	
2015/0025541	A1	1/2015	Furlong et al.	
2015/0064165	A1	3/2015	Perry et al.	
2015/0141809	A1	5/2015	Costello et al.	
2015/0148836	A1	5/2015	Heeren	
2015/0238171	A1	8/2015	Shabaz	
2015/0335485	A1	11/2015	Rieger et al.	
2016/0095615	A1	4/2016	Orczy-Timko et al.	

* cited by examiner

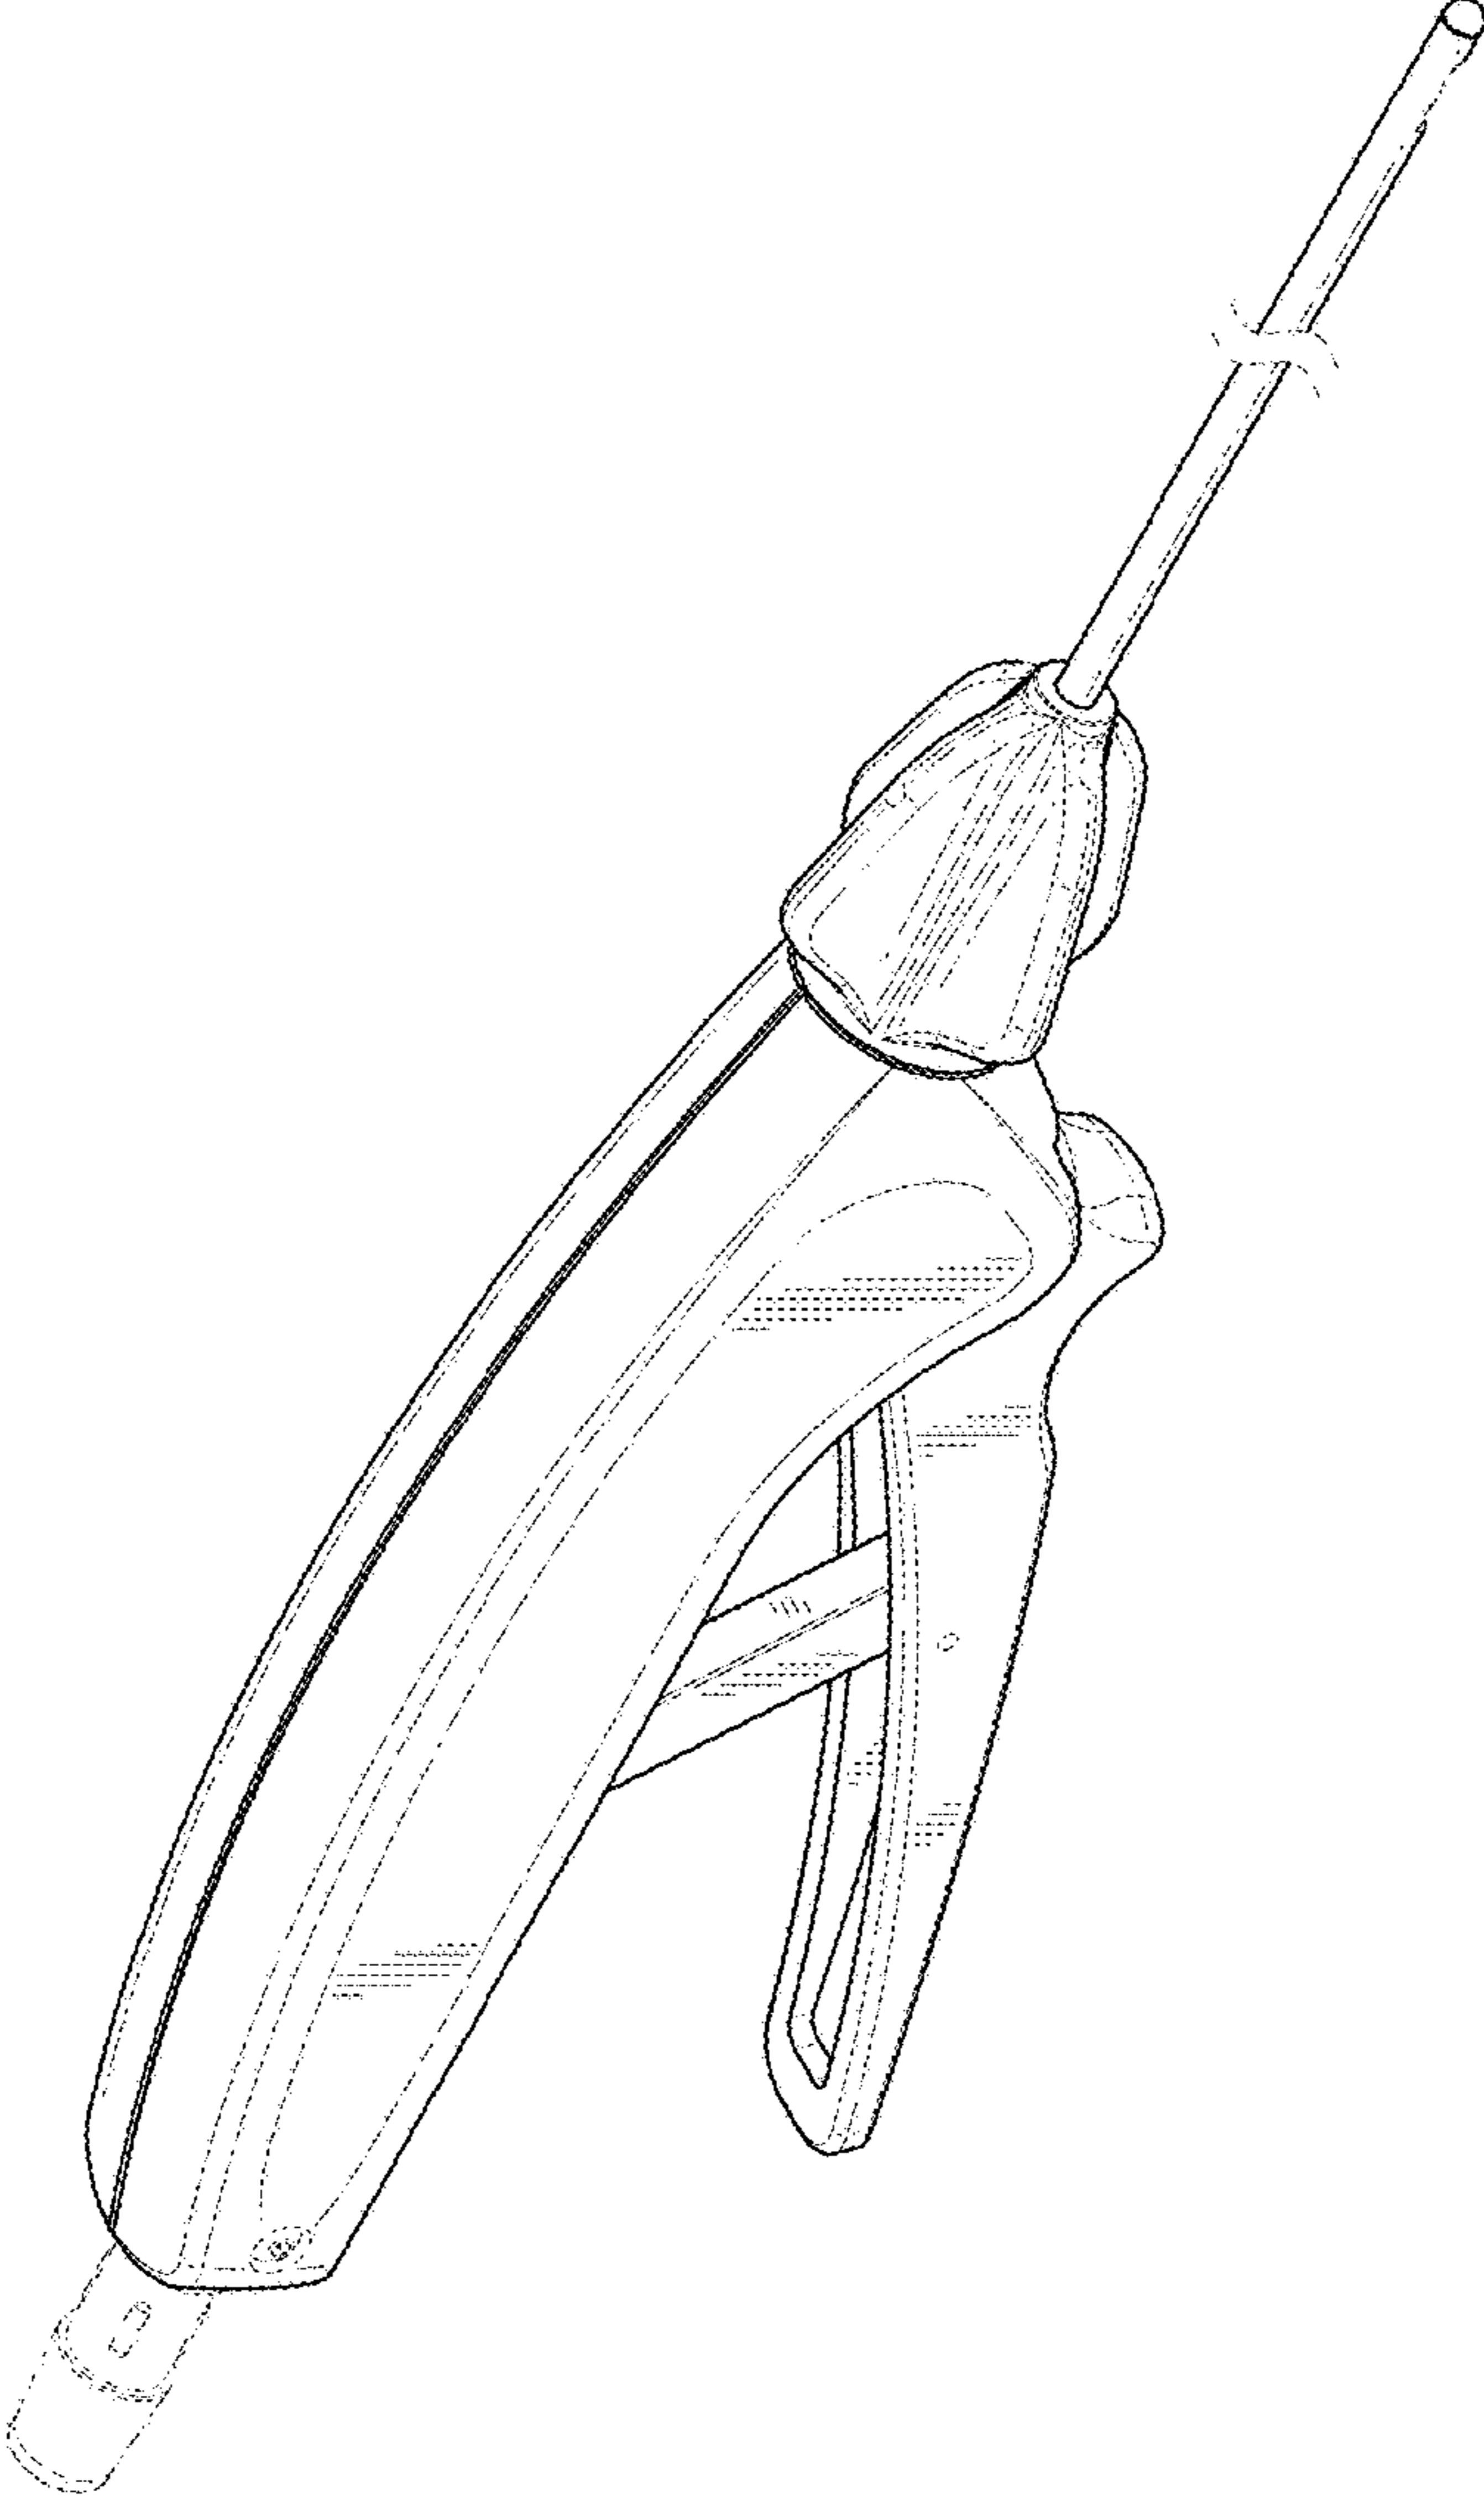


FIG. 1

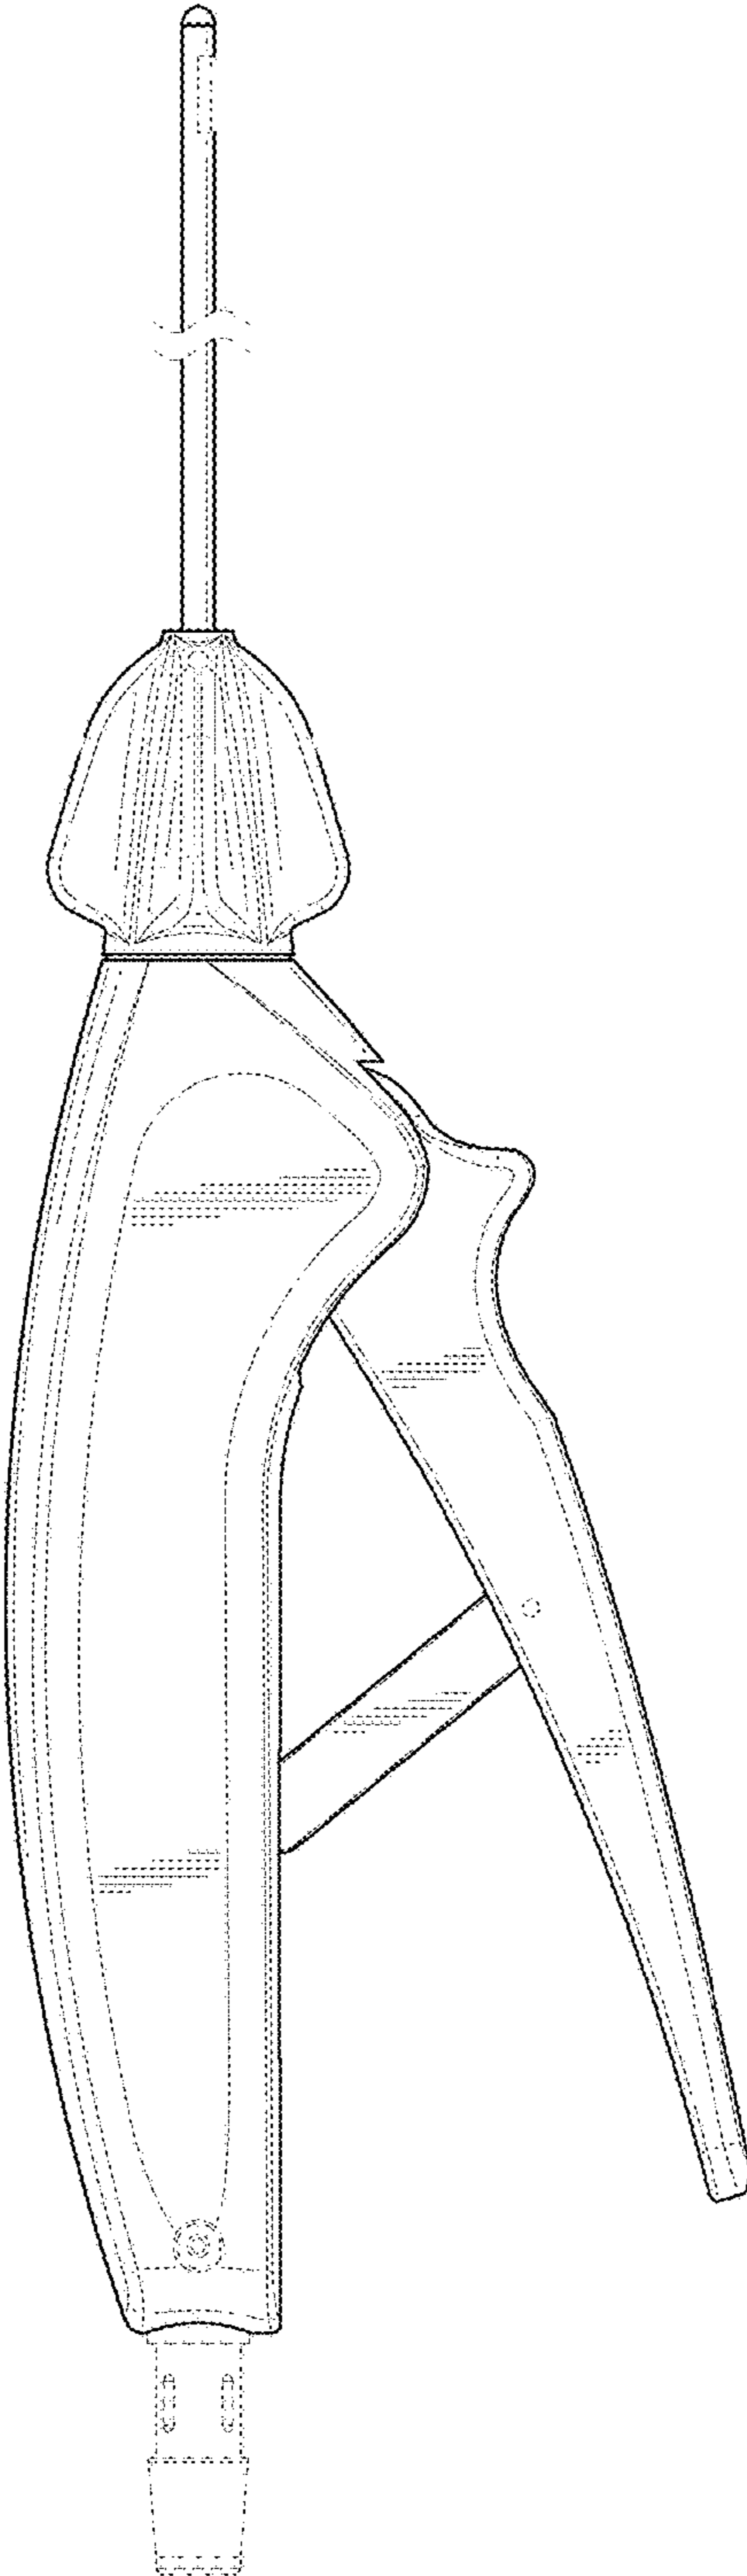


FIG. 2

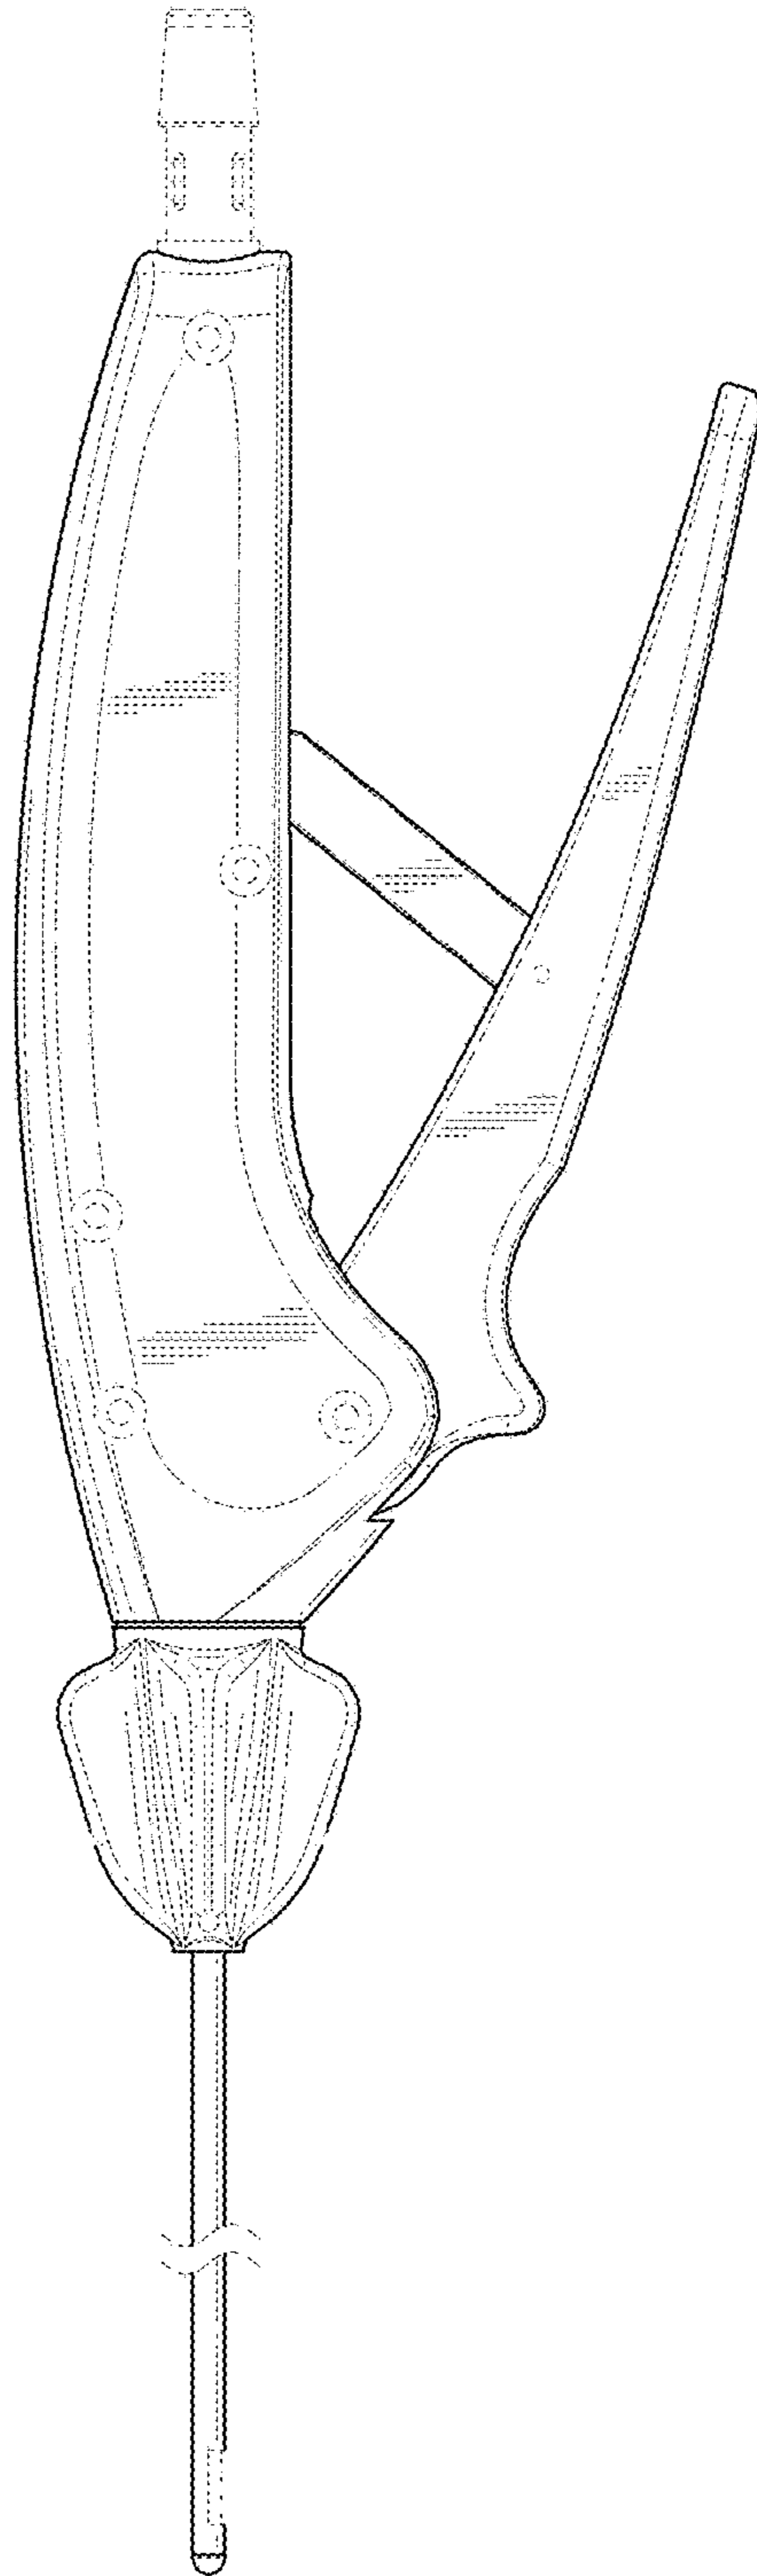


FIG. 3

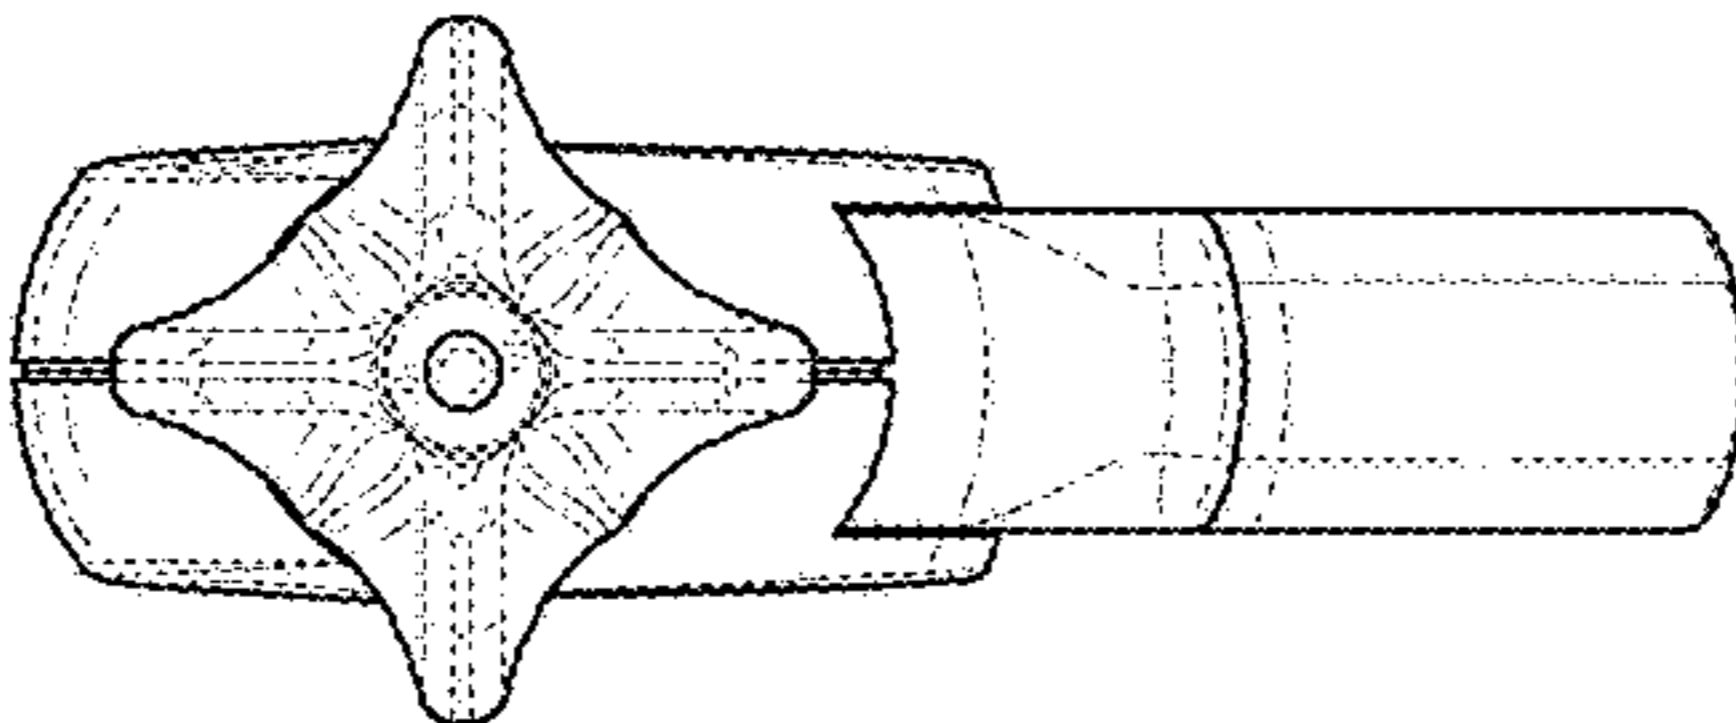


FIG. 4

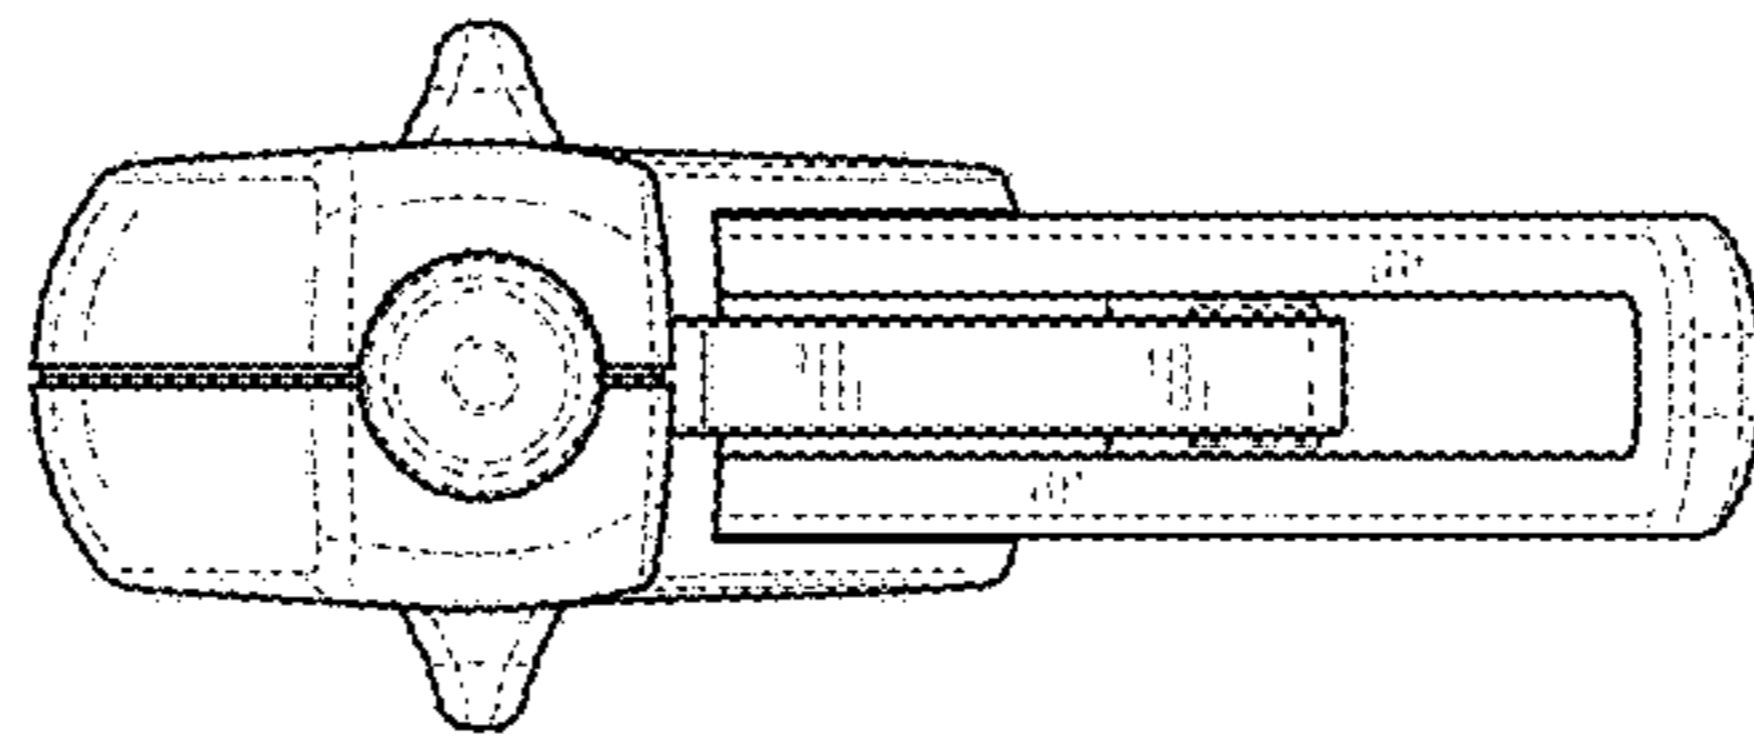


FIG. 5

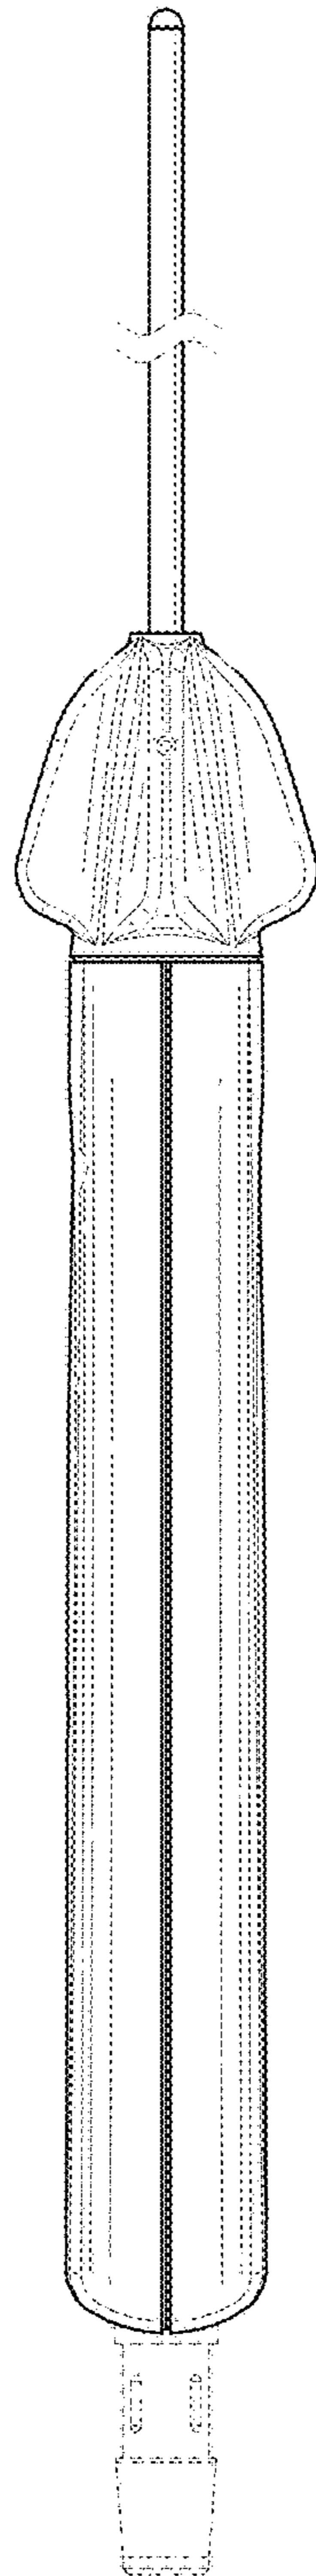


FIG. 6

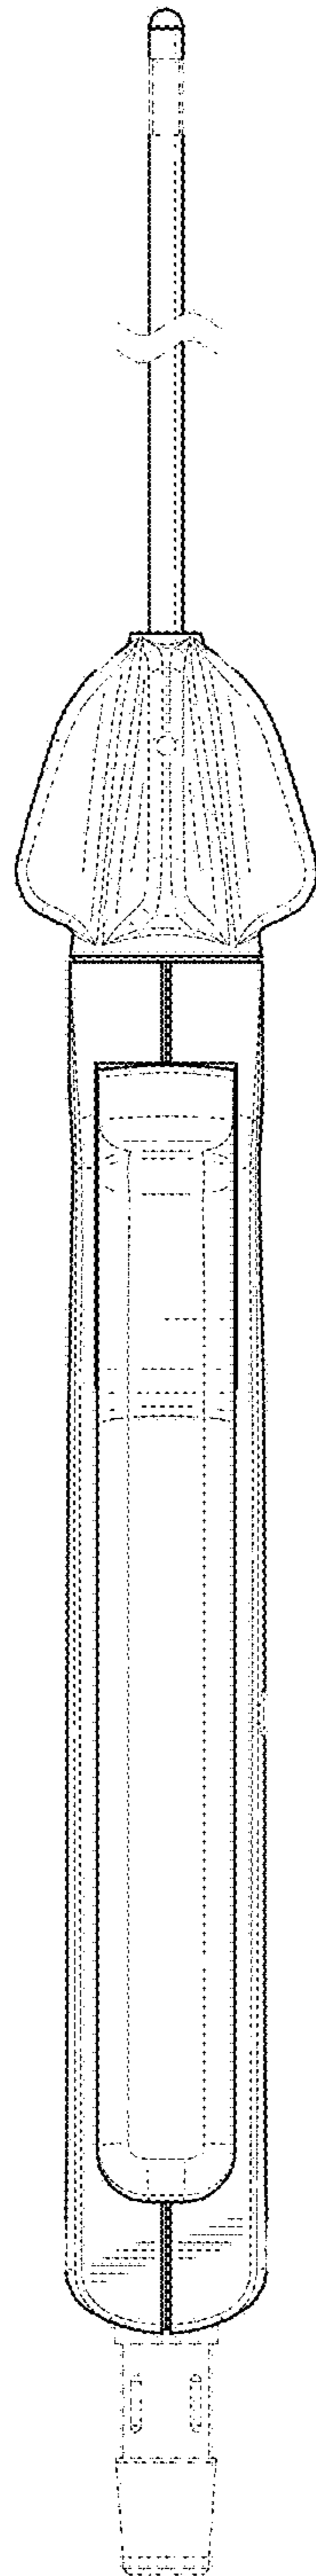


FIG. 7