



US00D849021S

(12) **United States Design Patent** (10) **Patent No.:** **US D849,021 S**  
**Fecteau et al.** (45) **Date of Patent:** **\*\* May 21, 2019**

(54) **DISPLAY SCREEN PORTION WITH GRAPHICAL USER INTERFACE**

(71) Applicant: **ICENTIA INC.**, Québec (CA)

(72) Inventors: **Pierre Fecteau**,  
St-Augustin-de-Desmaures (CA);  
**Germain Éthier**, Québec (CA)

(73) Assignee: **ICENTIA INC.**, Quebec (CA)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/643,421**

(22) Filed: **Apr. 9, 2018**

**Related U.S. Application Data**

(62) Division of application No. 29/583,407, filed on Nov. 4, 2016, now Pat. No. Des. 836,116.

(51) **LOC (11) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/485**

(58) **Field of Classification Search**  
USPC ..... D14/485-495  
CPC ..... A61B 5/02; A61B 5/044  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

6,370,423	B1	4/2002	Guerrero et al.	
6,409,659	B1	6/2002	Warner et al.	
D579,943	S *	11/2008	Clark	D14/485
D652,048	S	1/2012	Joseph	
D677,274	S	3/2013	Phelan	
D734,773	S	7/2015	Barbato	
D780,772	S *	3/2017	Kim	D14/485
2003/0142142	A1	7/2003	Jaffe	
2008/0097226	A1	4/2008	McConnell	
2009/0070054	A1	3/2009	Zeng et al.	

(Continued)

**FOREIGN PATENT DOCUMENTS**

JP 2004167006 A 6/2004

**OTHER PUBLICATIONS**

P. Kathirvel et al., "An Efficient R-peak Detection Based on New Nonlinear Transformation and First-Order Gaussian Differentiator", *Cardiovascular Engineering and Technology*, vol. 2, No. 4, Dec. 2011, pp. 408-425, India.

(Continued)

*Primary Examiner* — Richelle G Shelton

(74) *Attorney, Agent, or Firm* — Norton Rose Fulbright Canada LLP; Alexandre Daoust

(57) **CLAIM**

The ornamental design for a display screen portion with graphical user interface, as shown and described.

**DESCRIPTION**

The file of this patent contains at least one drawing/photograph executed in color. Copies of this patent with color drawing(s)/photograph(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a first view of a display screen portion with graphical user interface showing our new design, in accordance with a first embodiment;



FIG. 2 is an second view in accordance with a second embodiment;

FIG. 3 is a third view in accordance with a third embodiment; and,

FIG. 4 is a fourth view in accordance with a fourth embodiment.

The dashed line showing is included for the purpose of illustrating a display screen portion and forms no part of the claimed design.

**1 Claim, 4 Drawing Sheets**  
**(4 of 4 Drawing Sheet(s) Filed in Color)**

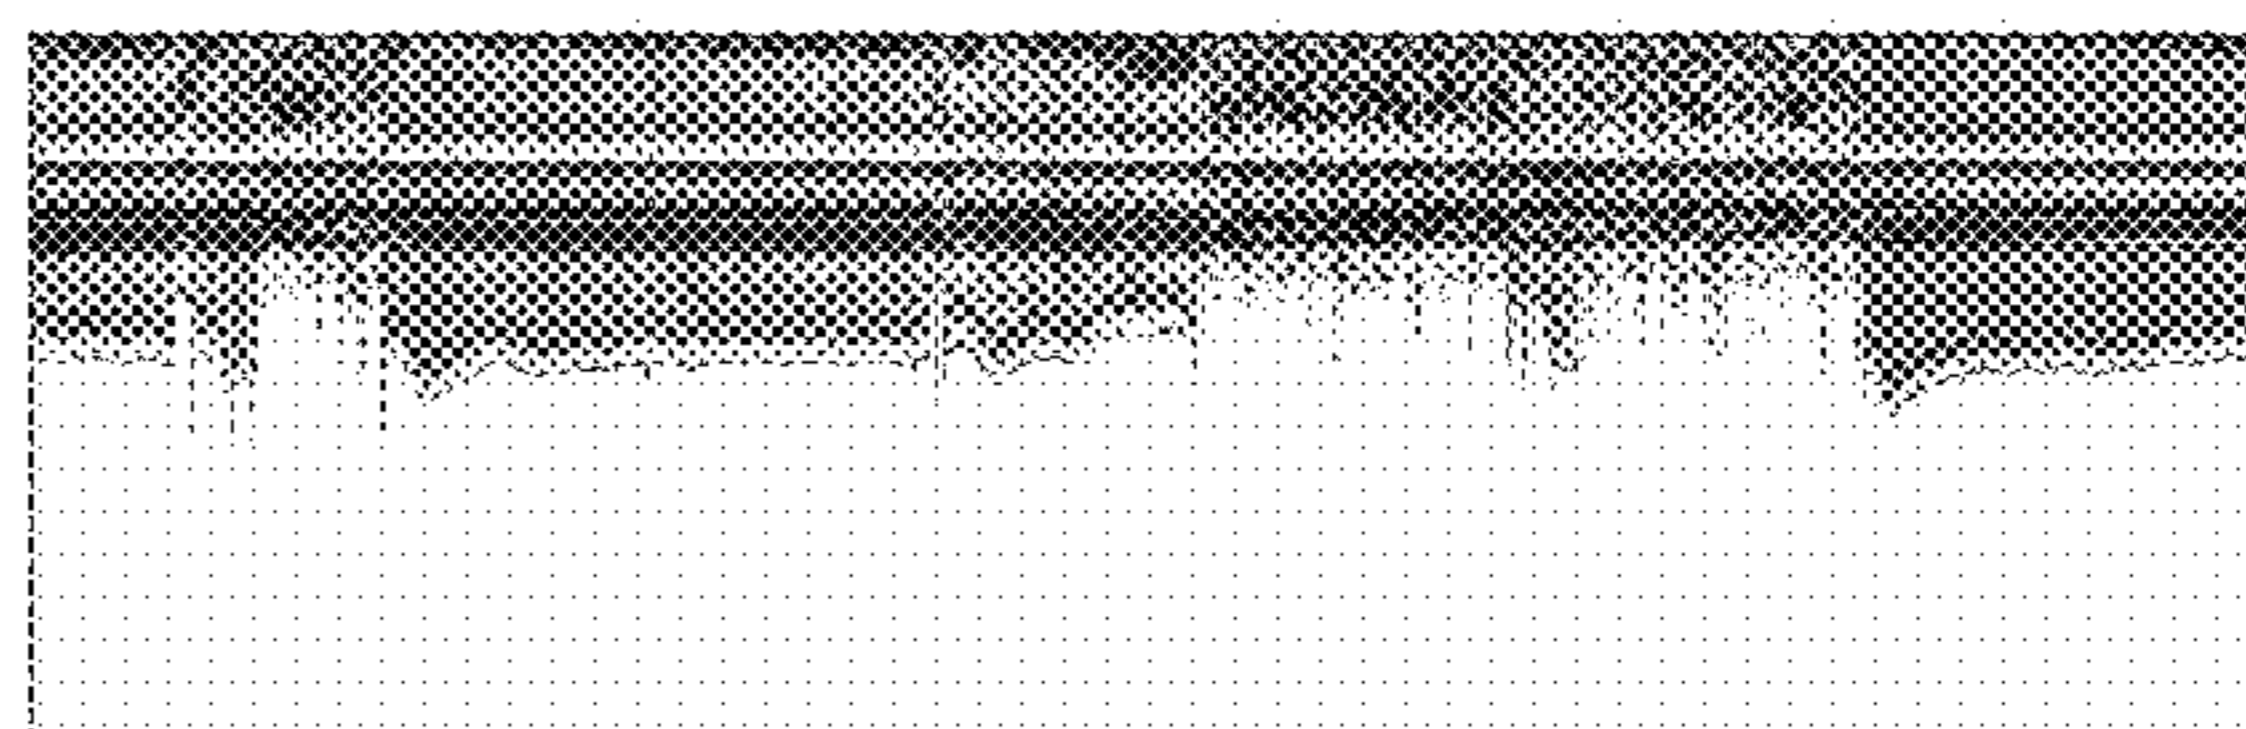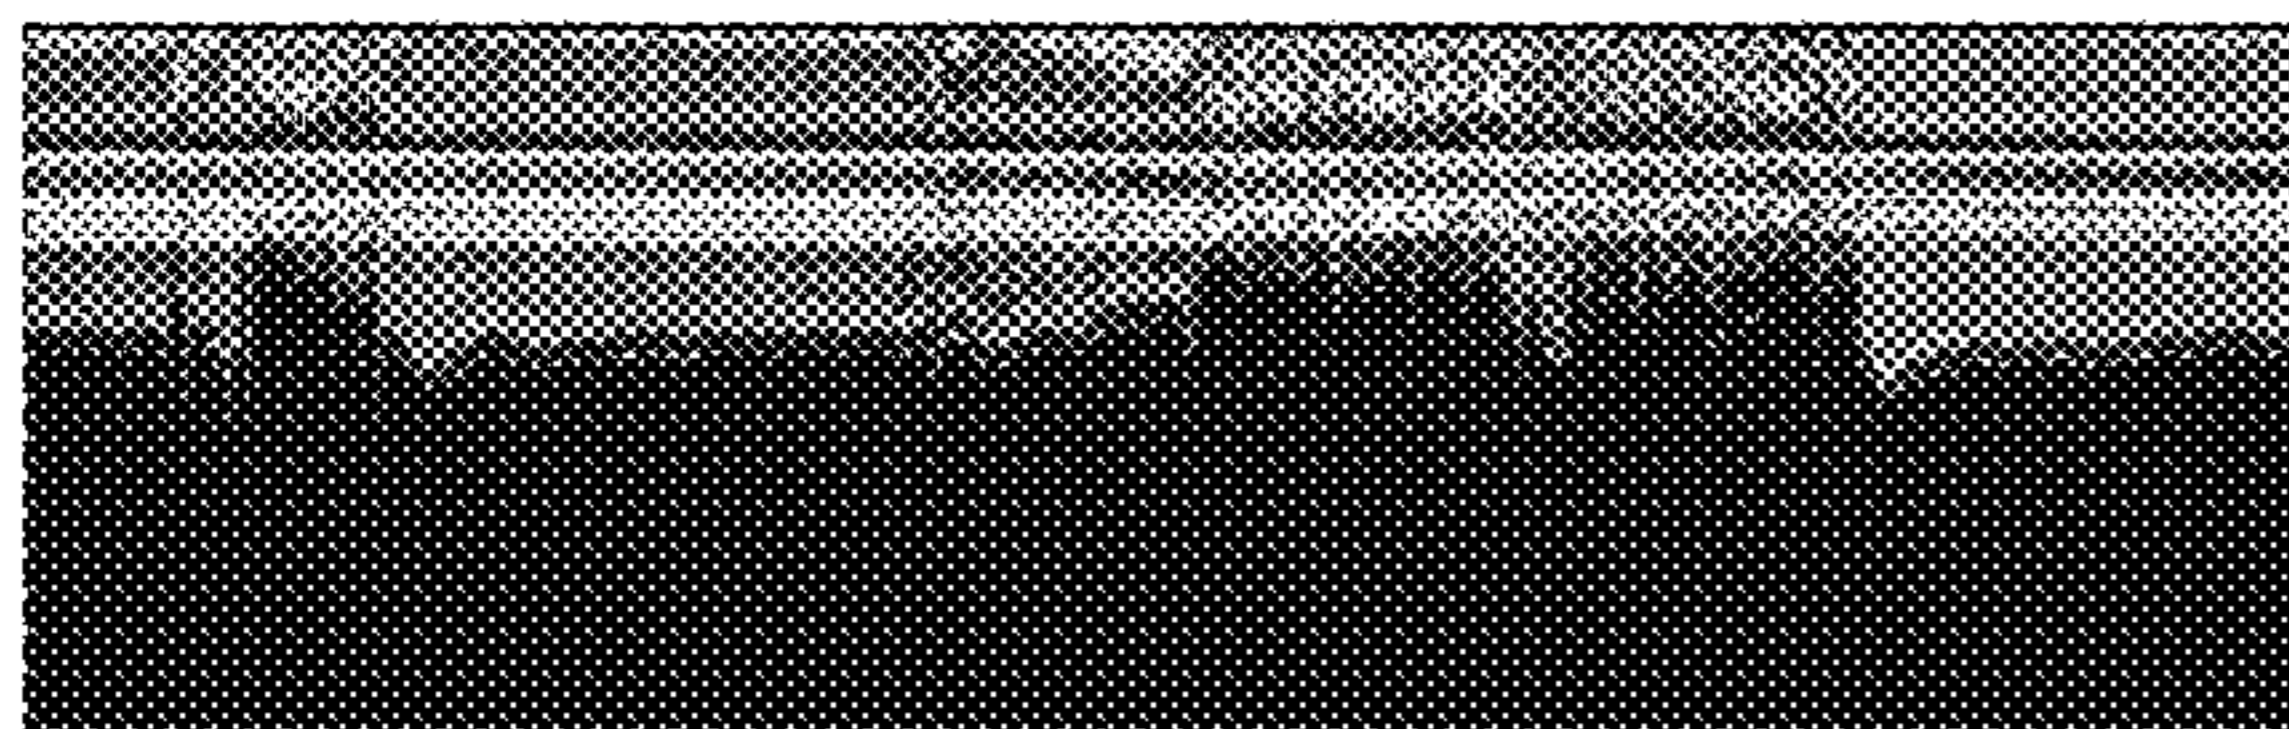

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2013/0096394 A1 4/2013 Gupta et al.  
2013/0109988 A1 5/2013 Kim et al.  
2014/0107541 A1 4/2014 Sullivan et al.  
2015/0297104 A1 10/2015 Chen et al.  
2016/0058318 A1 3/2016 Borjigin et al.  
2016/0143594 A1 5/2016 Moorman et al.  
2016/0192853 A1 7/2016 Bardy et al.  
2016/0206921 A1\* 7/2016 Szabados ..... A61B 5/0024  
2016/0292894 A1 10/2016 Huang et al.  
2016/0331258 A1 11/2016 Du et al.  
2017/0196472 A1 7/2017 Felix et al.

OTHER PUBLICATIONS

Warner, R.A. et al, "Marquette Waterfall Display", GE Healthcare, Apr. 2002, General Electric Company, U.S.A.  
"Schiller's Medilog Holter system", Schiller The Art of Diagnostics, 2013, Switzerland.

\* cited by examiner

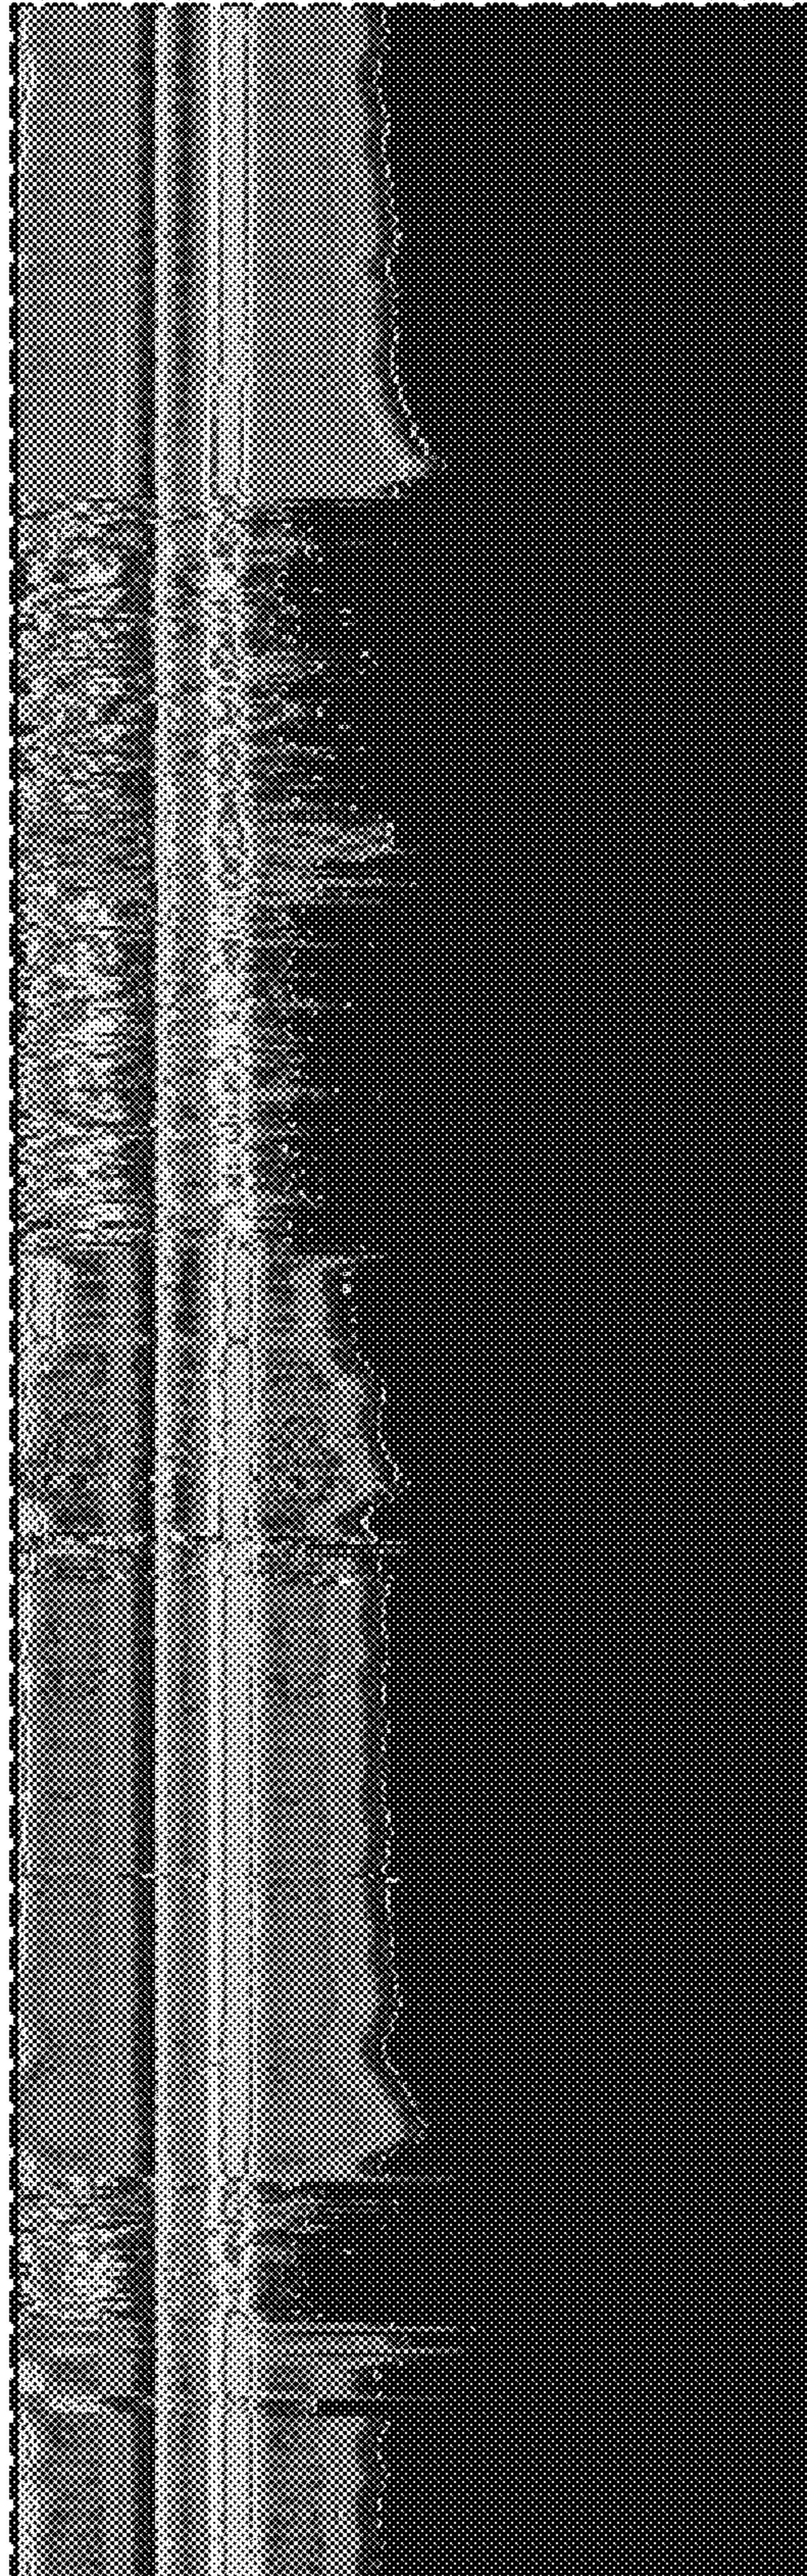


FIG. 1

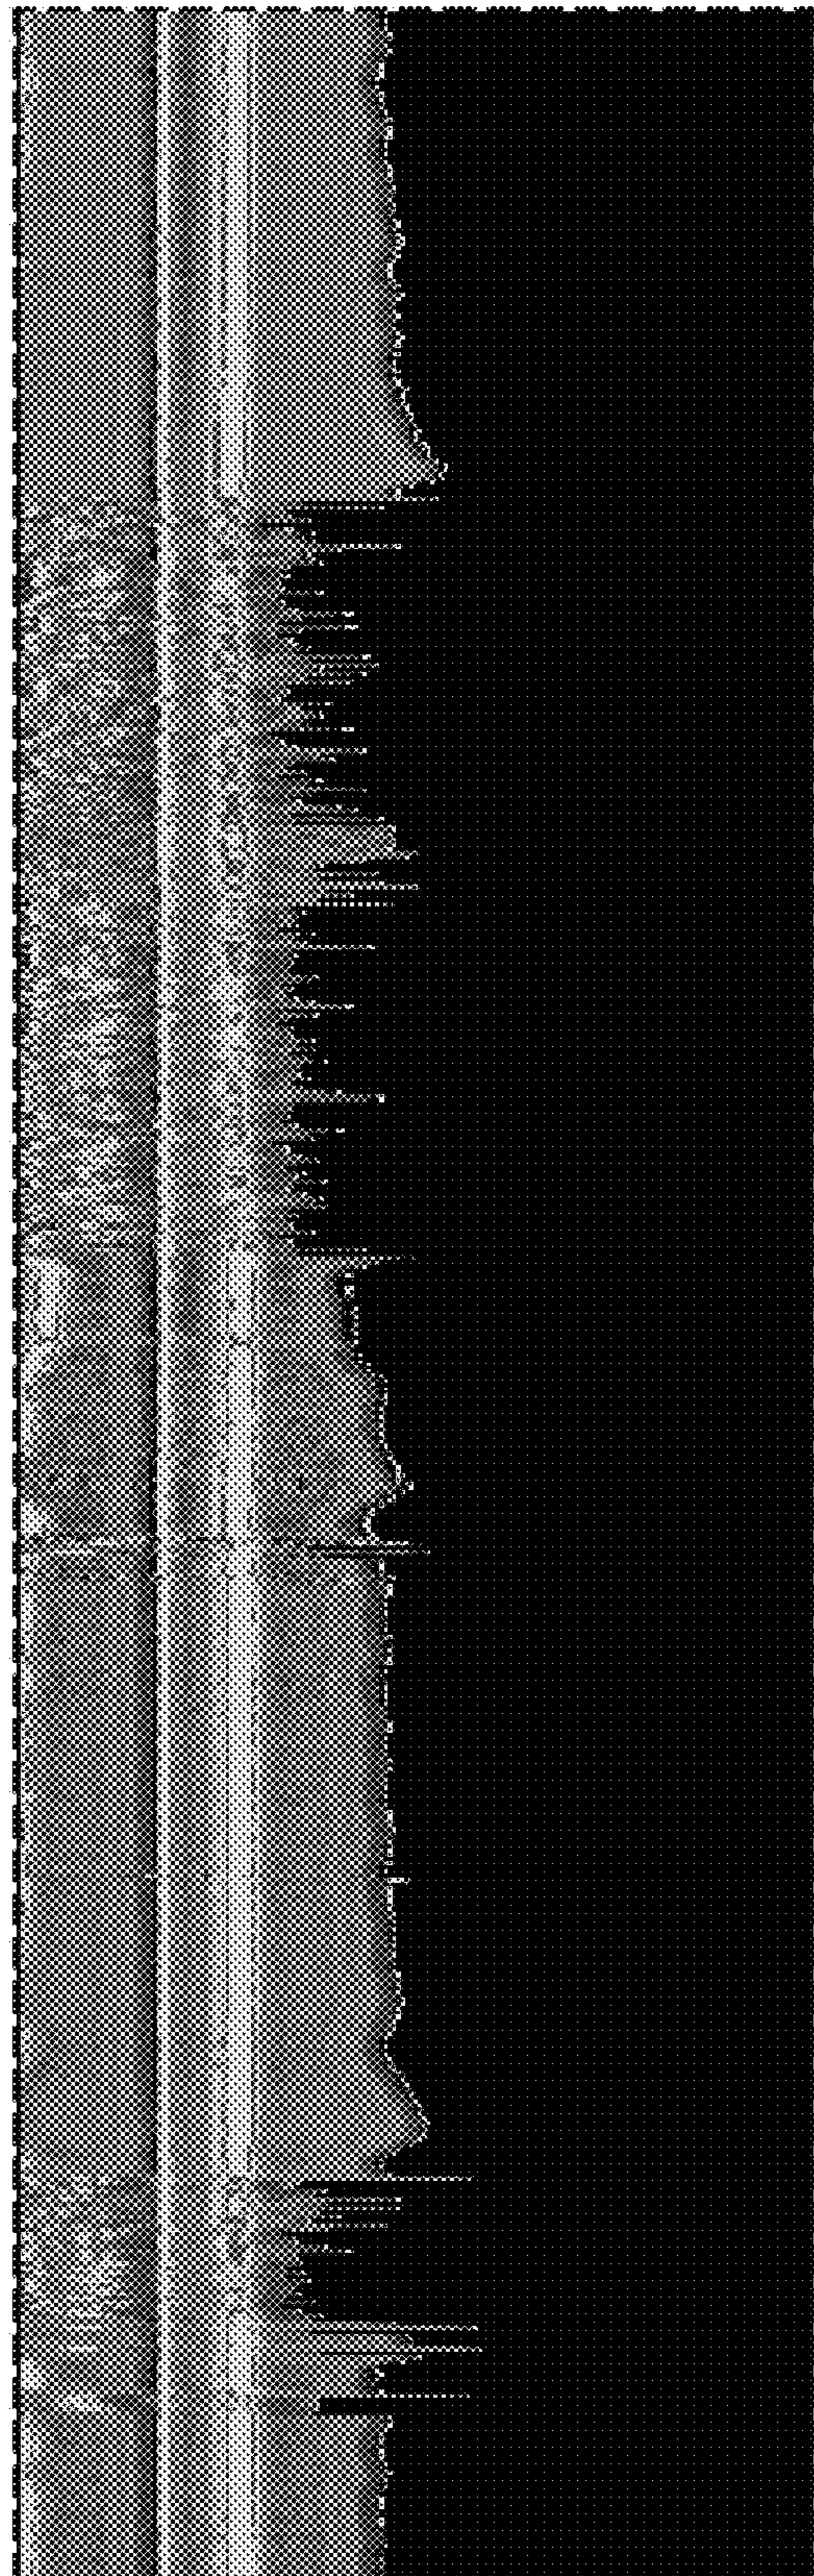


FIG. 2

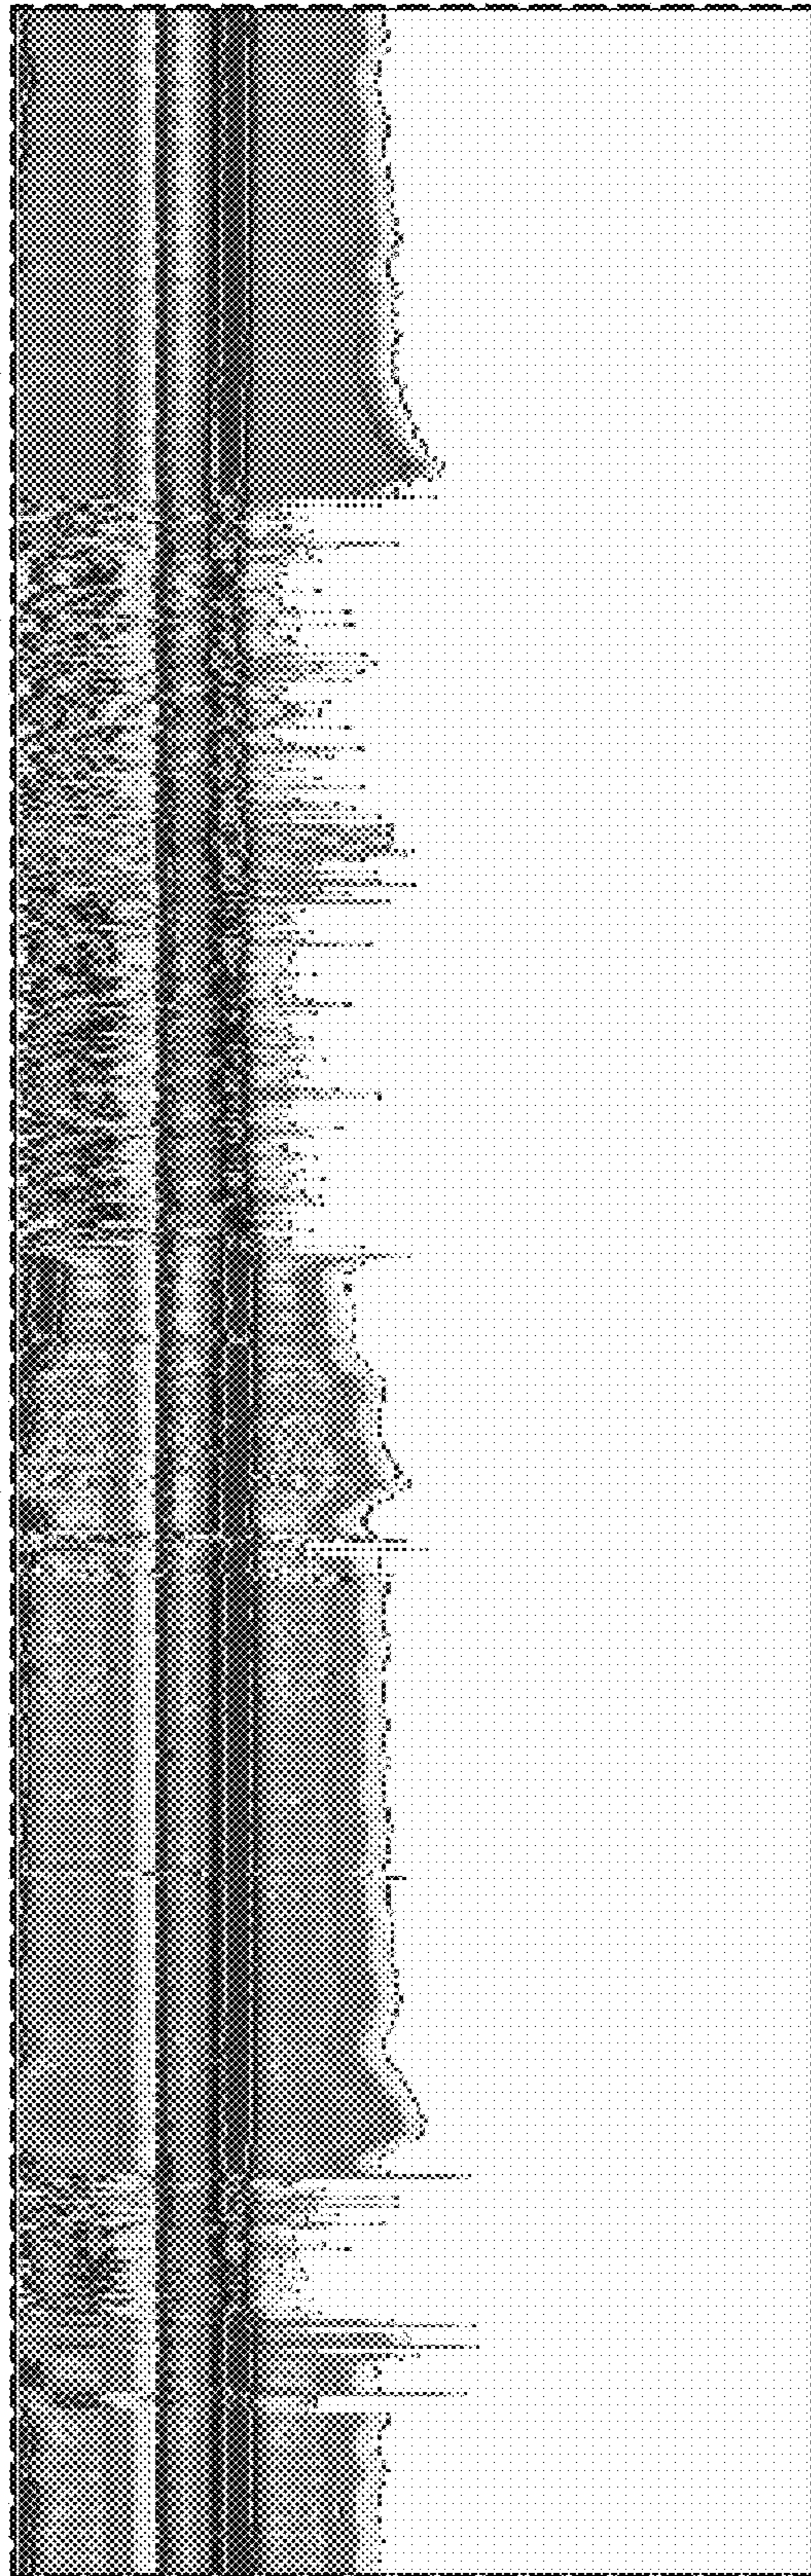


FIG. 3

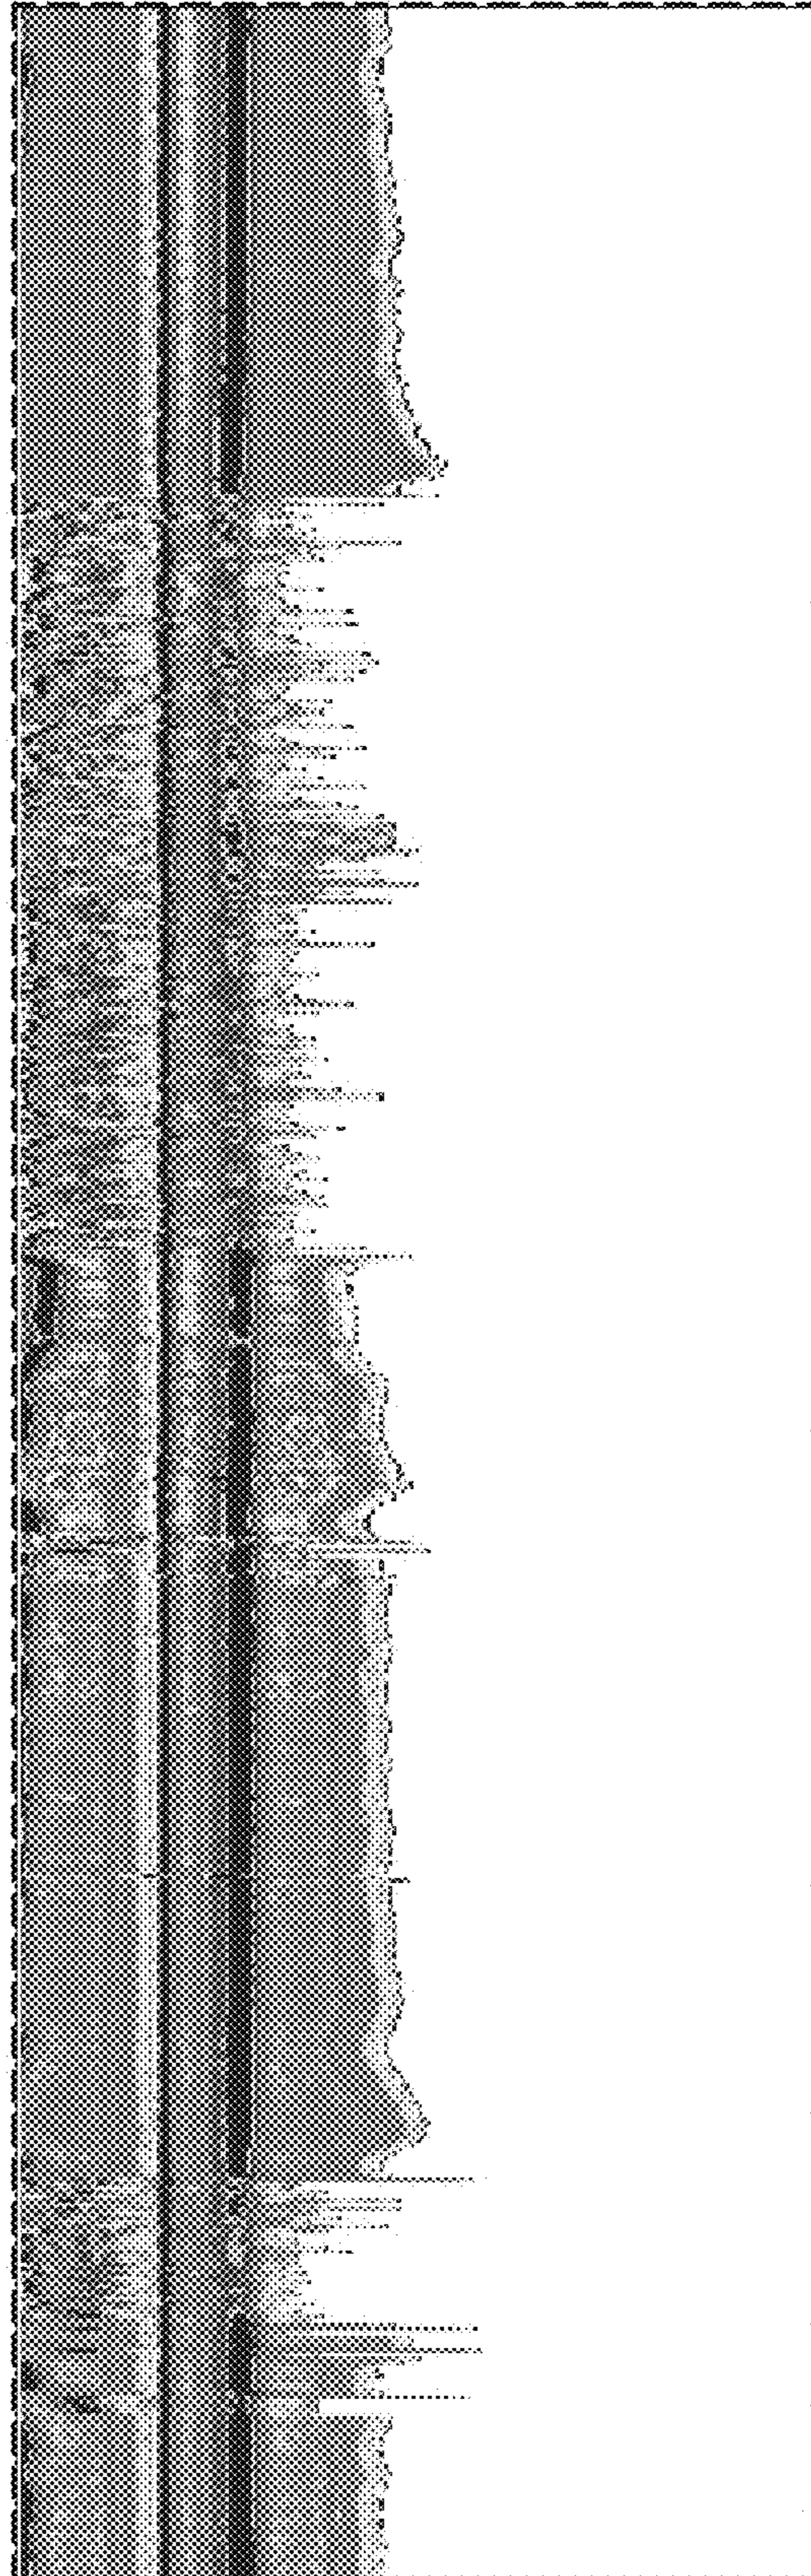


FIG. 4