



US00D849252S

(12) **United States Design Patent** (10) **Patent No.:** **US D849,252 S**
Rondoni et al. (45) **Date of Patent:** **** May 21, 2019**

(54) **PATIENT CONTROL**

(71) Applicant: **Inspire Medical Systems, Inc.**, Maple Grove, MN (US)

(72) Inventors: **John Rondoni**, Maple Grove, MN (US); **Blake Johnson**, Maple Grove, MN (US); **Jordon McIver**, Maple Grove, MN (US); **Casimir Sienkiewicz**, Maple Grove, MN (US); **Peter Young**, Maple Grove, MN (US); **Travis Yoch**, Maple Grove, MN (US); **Kevin Verzal**, Maple Grove, MN (US)

(73) Assignee: **Inspire Medical Systems, Inc.**, Golden Valley, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/623,409**

(22) Filed: **Oct. 25, 2017**

Related U.S. Application Data

(63) Continuation of application No. 29/548,747, filed on Dec. 16, 2015, now Pat. No. Des. 801,538.

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/186**

(58) **Field of Classification Search**
USPC D24/185, 186, 187, 107, 108, 200;
D13/162, 168, 171
CPC A61N 1/3611; A61N 1/37247; A61N
1/37235
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,172,698 A 12/1992 Stanko
D490,525 S 5/2004 Stein et al.
D544,605 S 6/2007 Gumisawa et al.

D642,281 S 7/2011 Bachinski
D732,673 S 6/2015 Lewis, Jr. et al.
D748,066 S 1/2016 Lee
D752,763 S * 3/2016 Rondoni D24/186
D768,866 S 10/2016 Shigeno
D774,007 S 12/2016 Ryan
D797,949 S * 9/2017 Carreon D24/200
D810,306 S * 2/2018 Rondoni D24/186
2004/0230246 A1 11/2004 Stein et al.
2007/0270921 A1 11/2007 Strother et al.
2008/0249591 A1 10/2008 Gaw et al.
2010/0064212 A1 3/2010 Snyder

(Continued)

FOREIGN PATENT DOCUMENTS

WO 9749454 12/1997

OTHER PUBLICATIONS

Partial International Search, dated Dec. 3, 2014, 6 pages.

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Dicke, Billig & Czaja, PLLC


(57) **CLAIM**

The ornamental design for a patient control, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, right perspective view of a patient control;
FIG. 2 is a top plan view thereof;
FIG. 3 is a bottom plan view thereof;
FIG. 4 is a front elevational view thereof;
FIG. 5 is a back elevational view thereof;
FIG. 6 is a right side elevational view thereof; and,
FIG. 7 is a left side elevational view thereof.
The broken lines in the Figures are included for the purpose of illustrating portions of the patient control that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

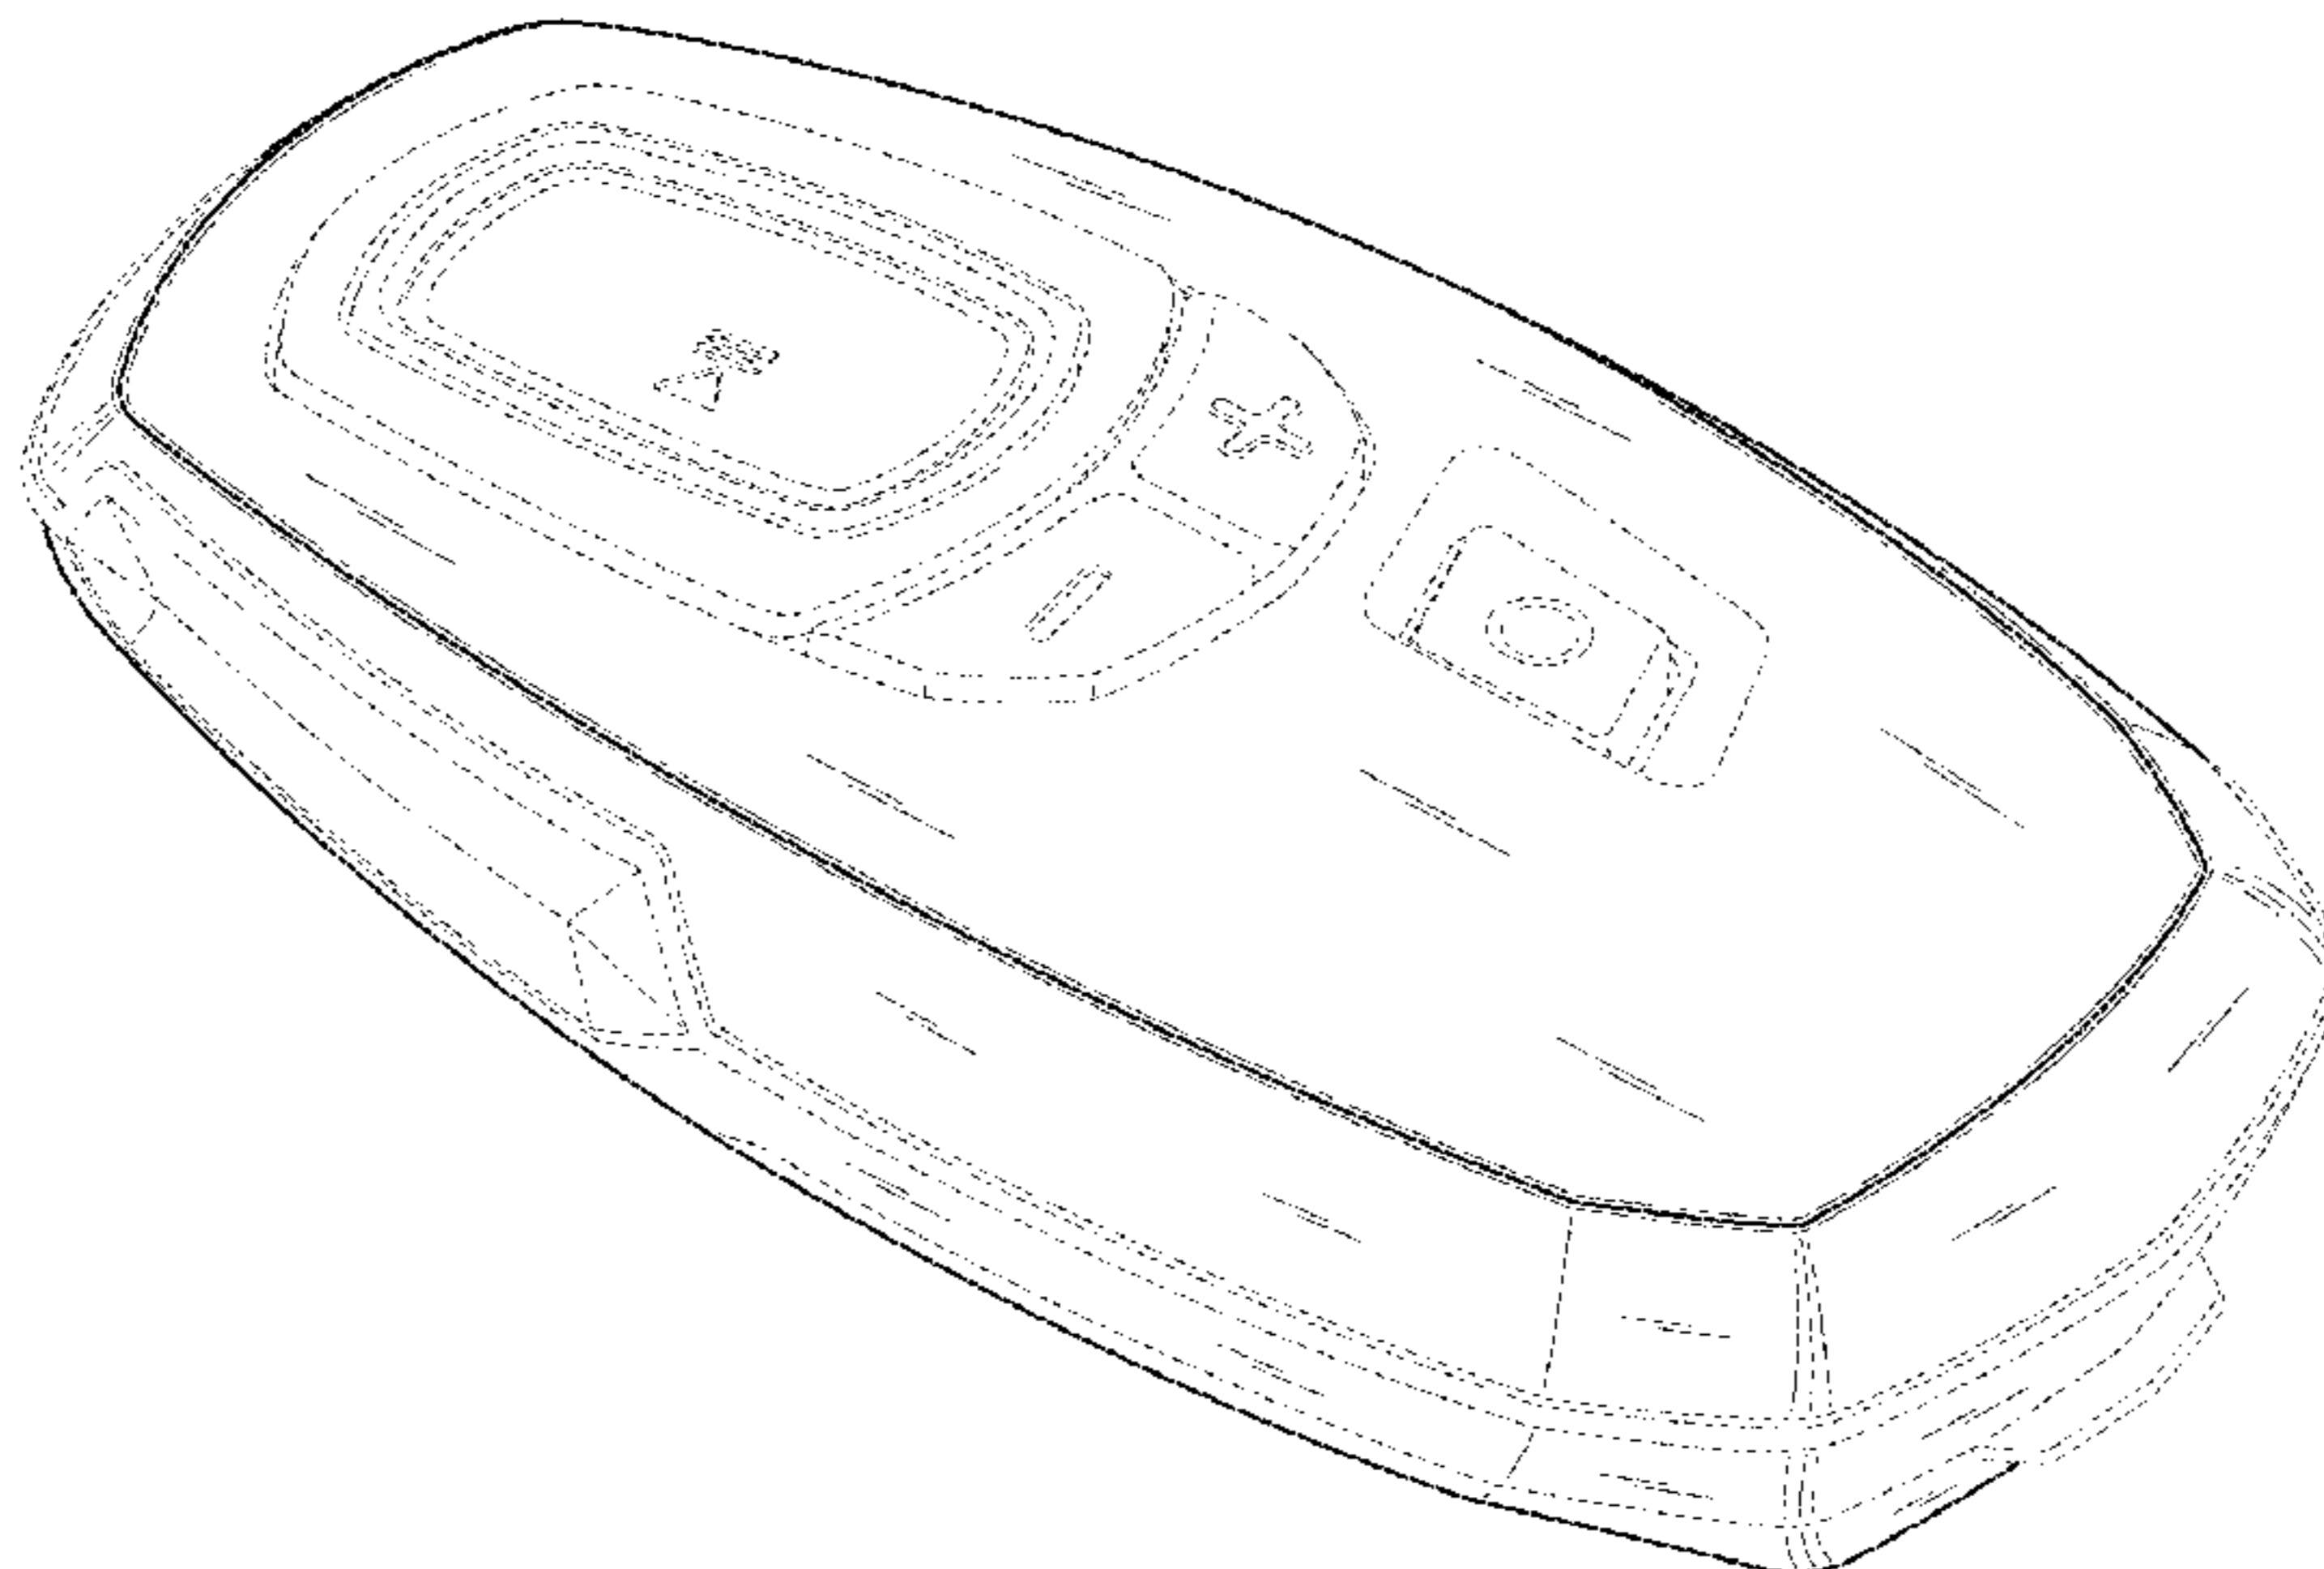

(56)

References Cited

U.S. PATENT DOCUMENTS

2010/0318159 A1 12/2010 Aghassian et al.
2010/0318519 A1 12/2010 Hadjieleftheriou et al.
2012/0101551 A1 4/2012 Aghassian et al.
2013/0197607 A1 8/2013 Wilder et al.
2013/0204314 A1 8/2013 Miller, III et al.

* cited by examiner

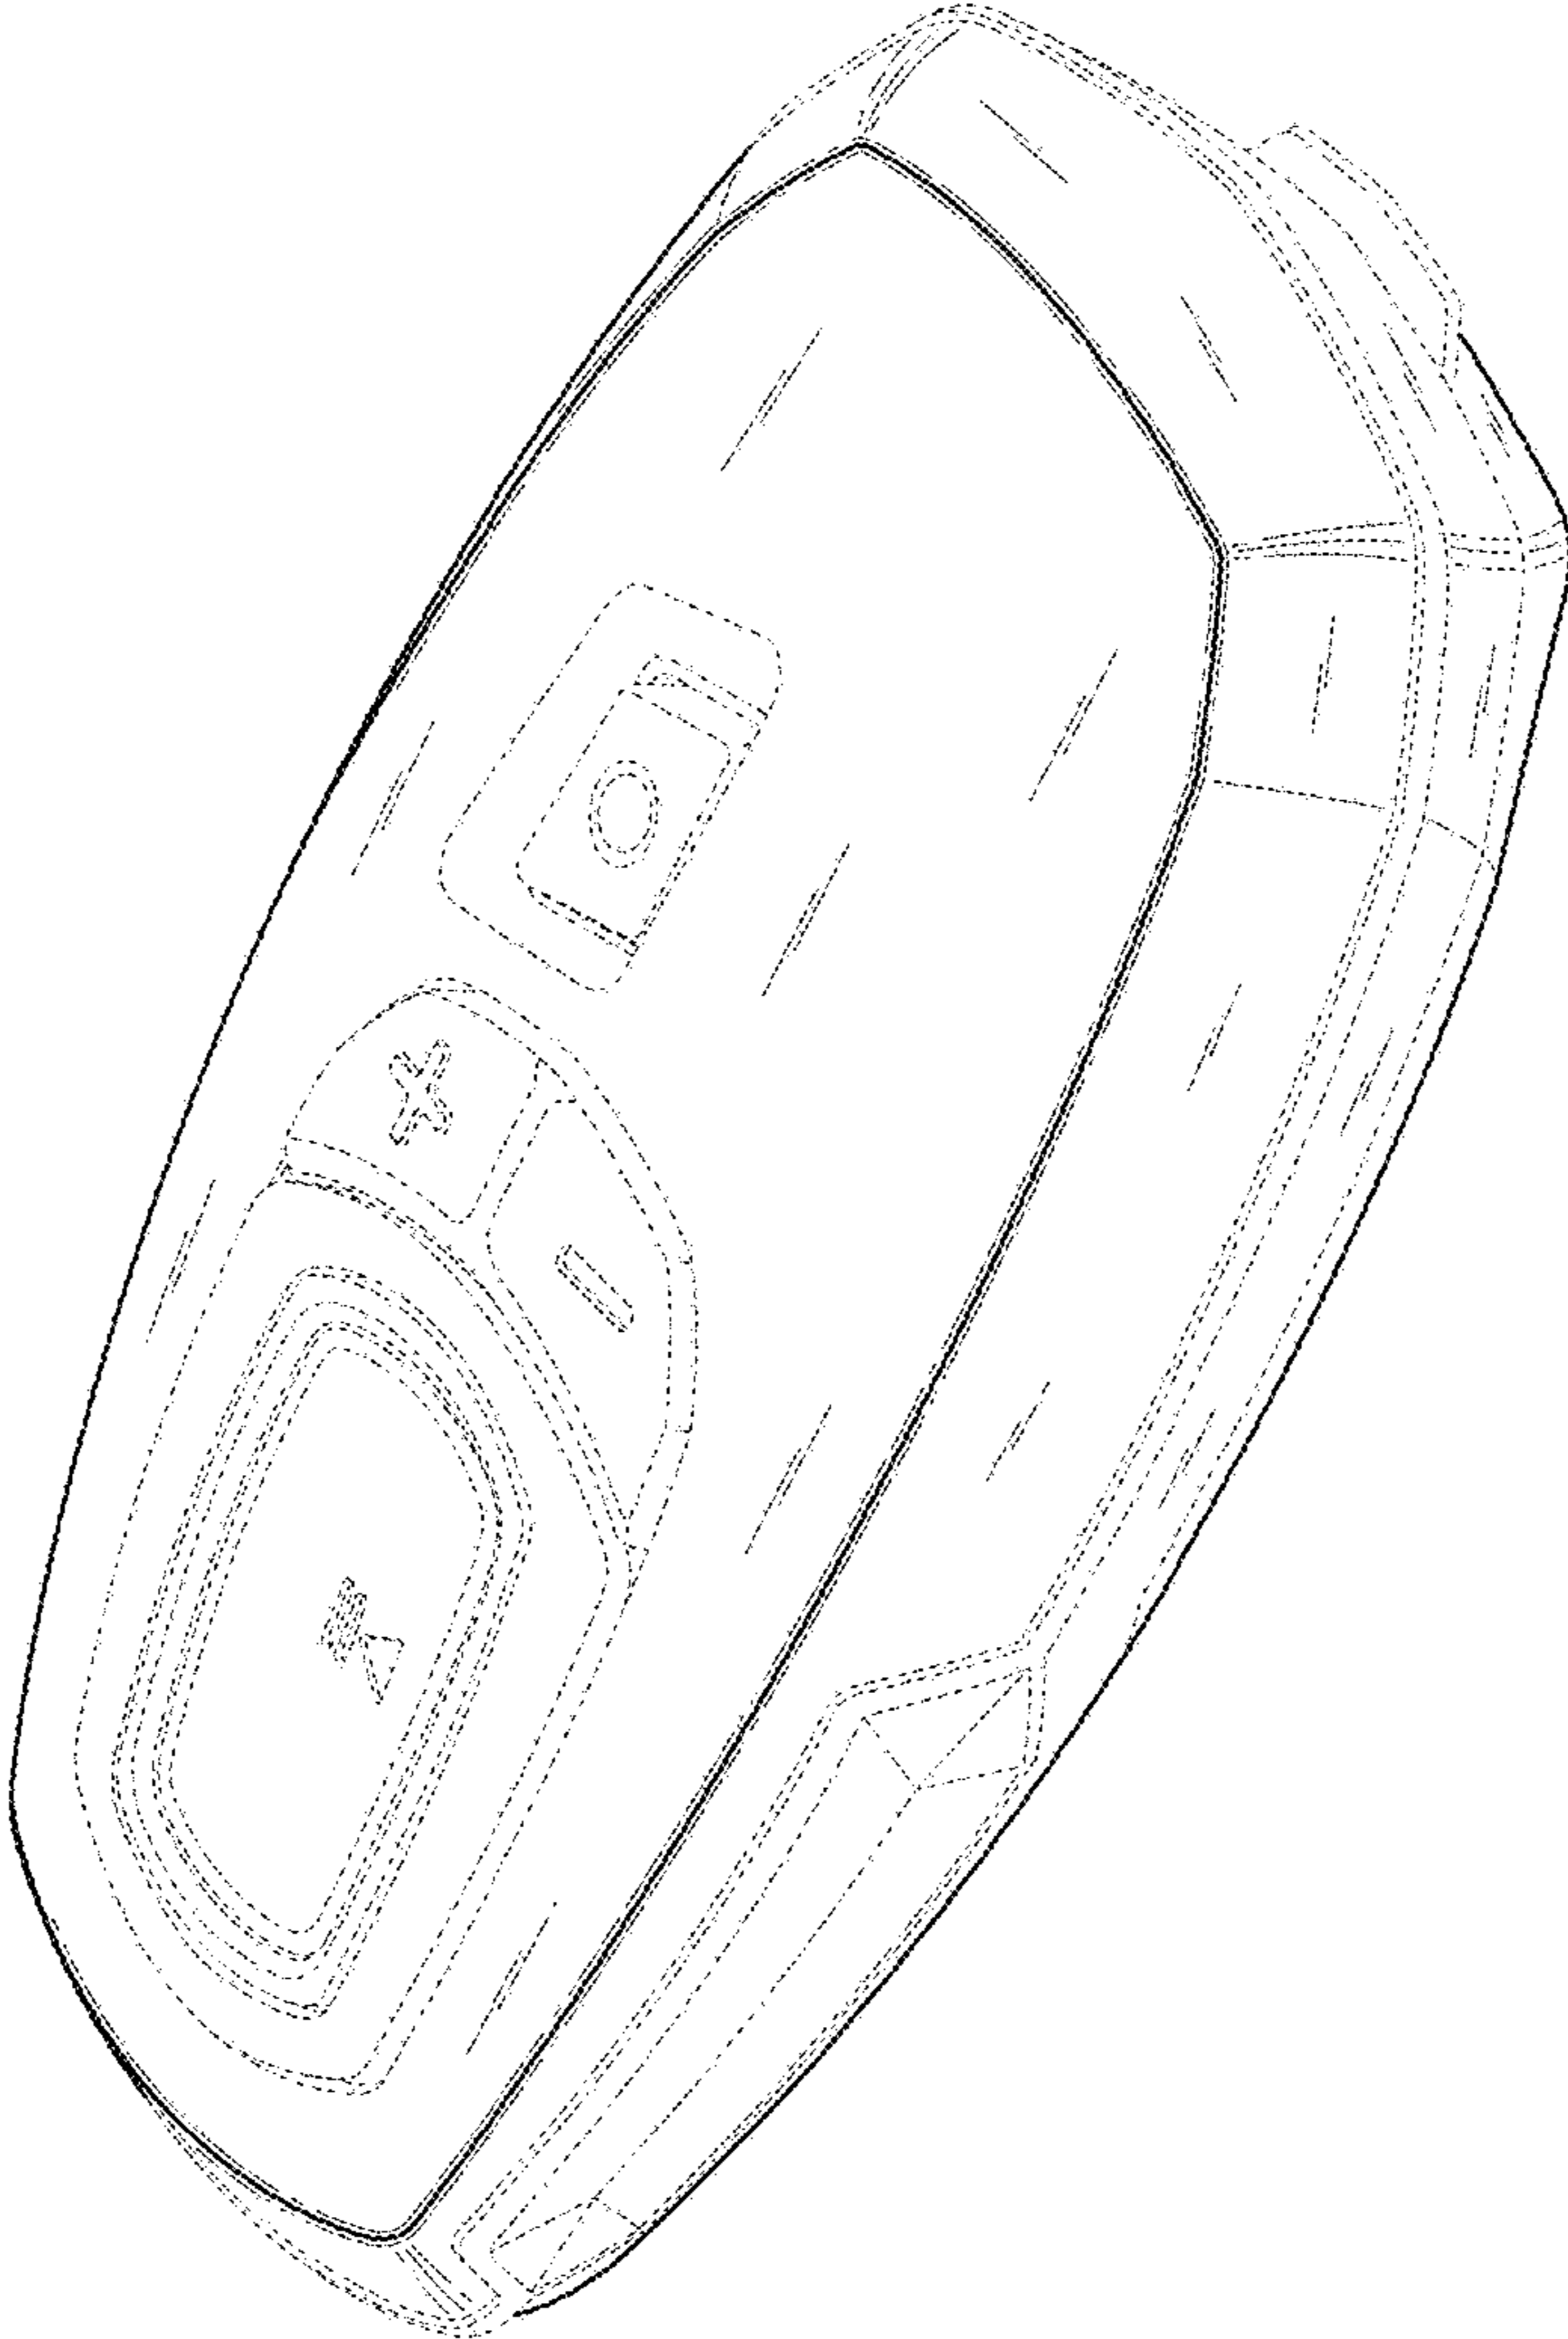


Fig. 1

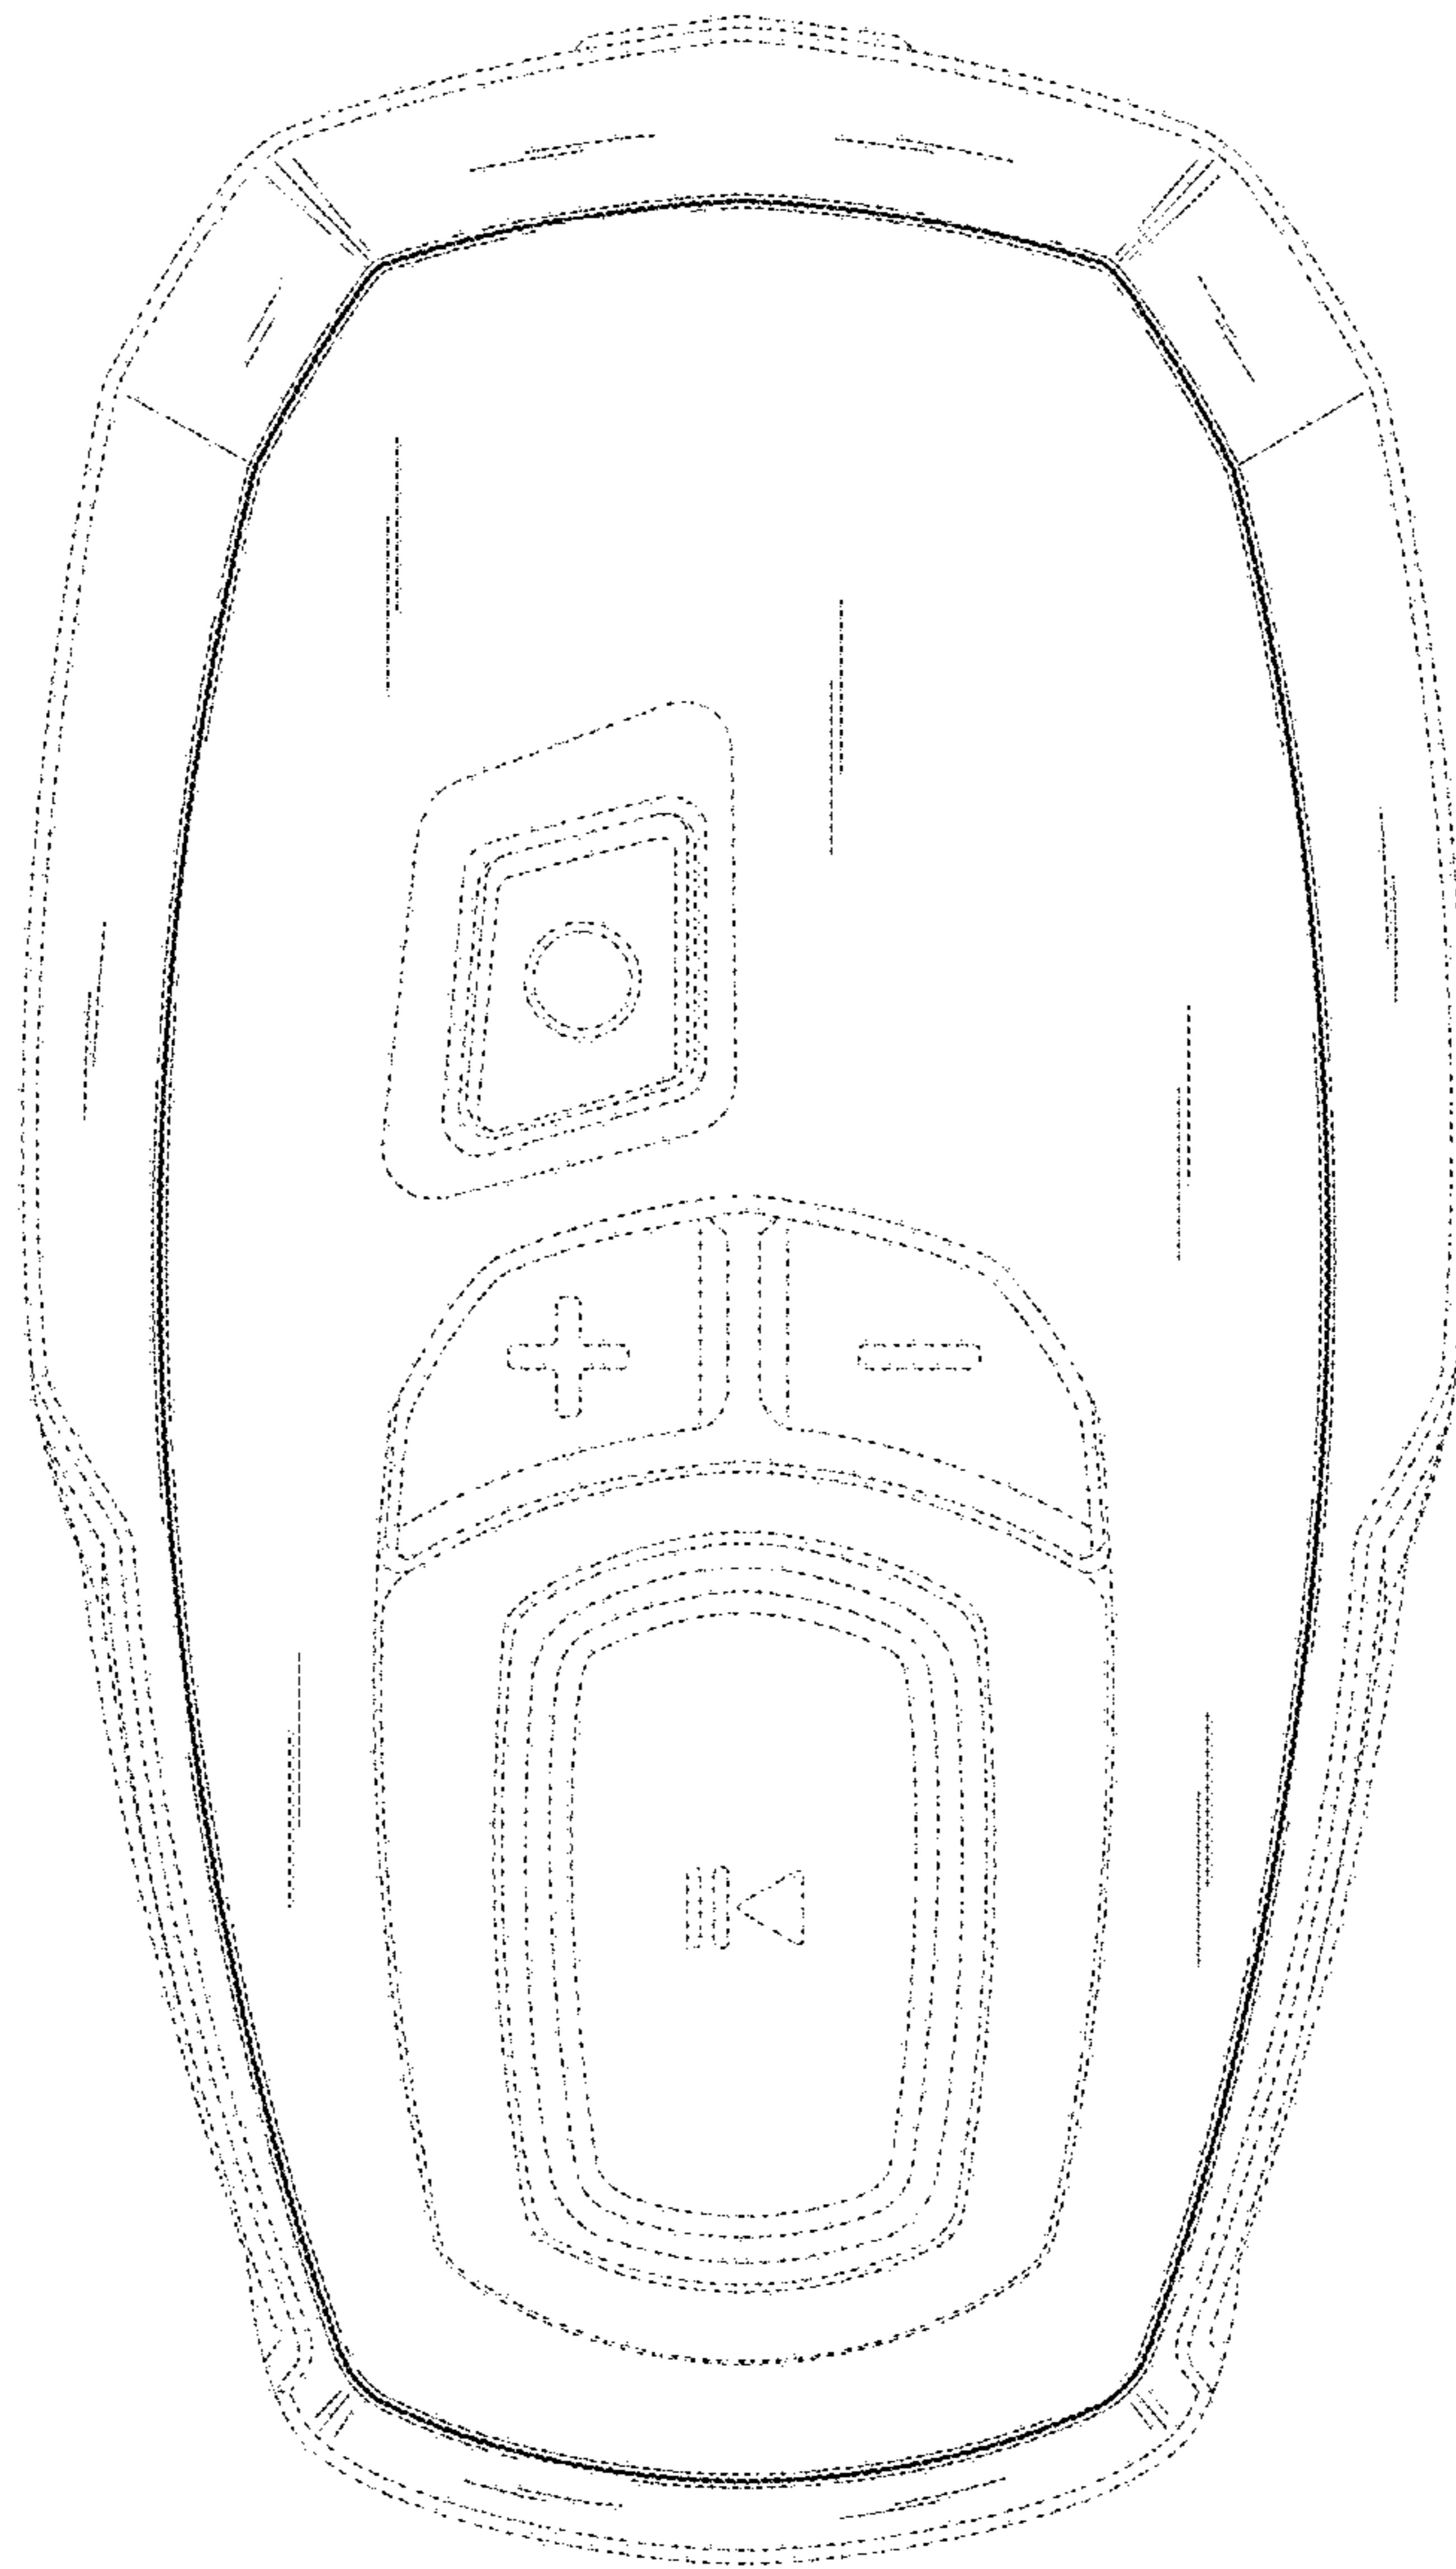


Fig. 2

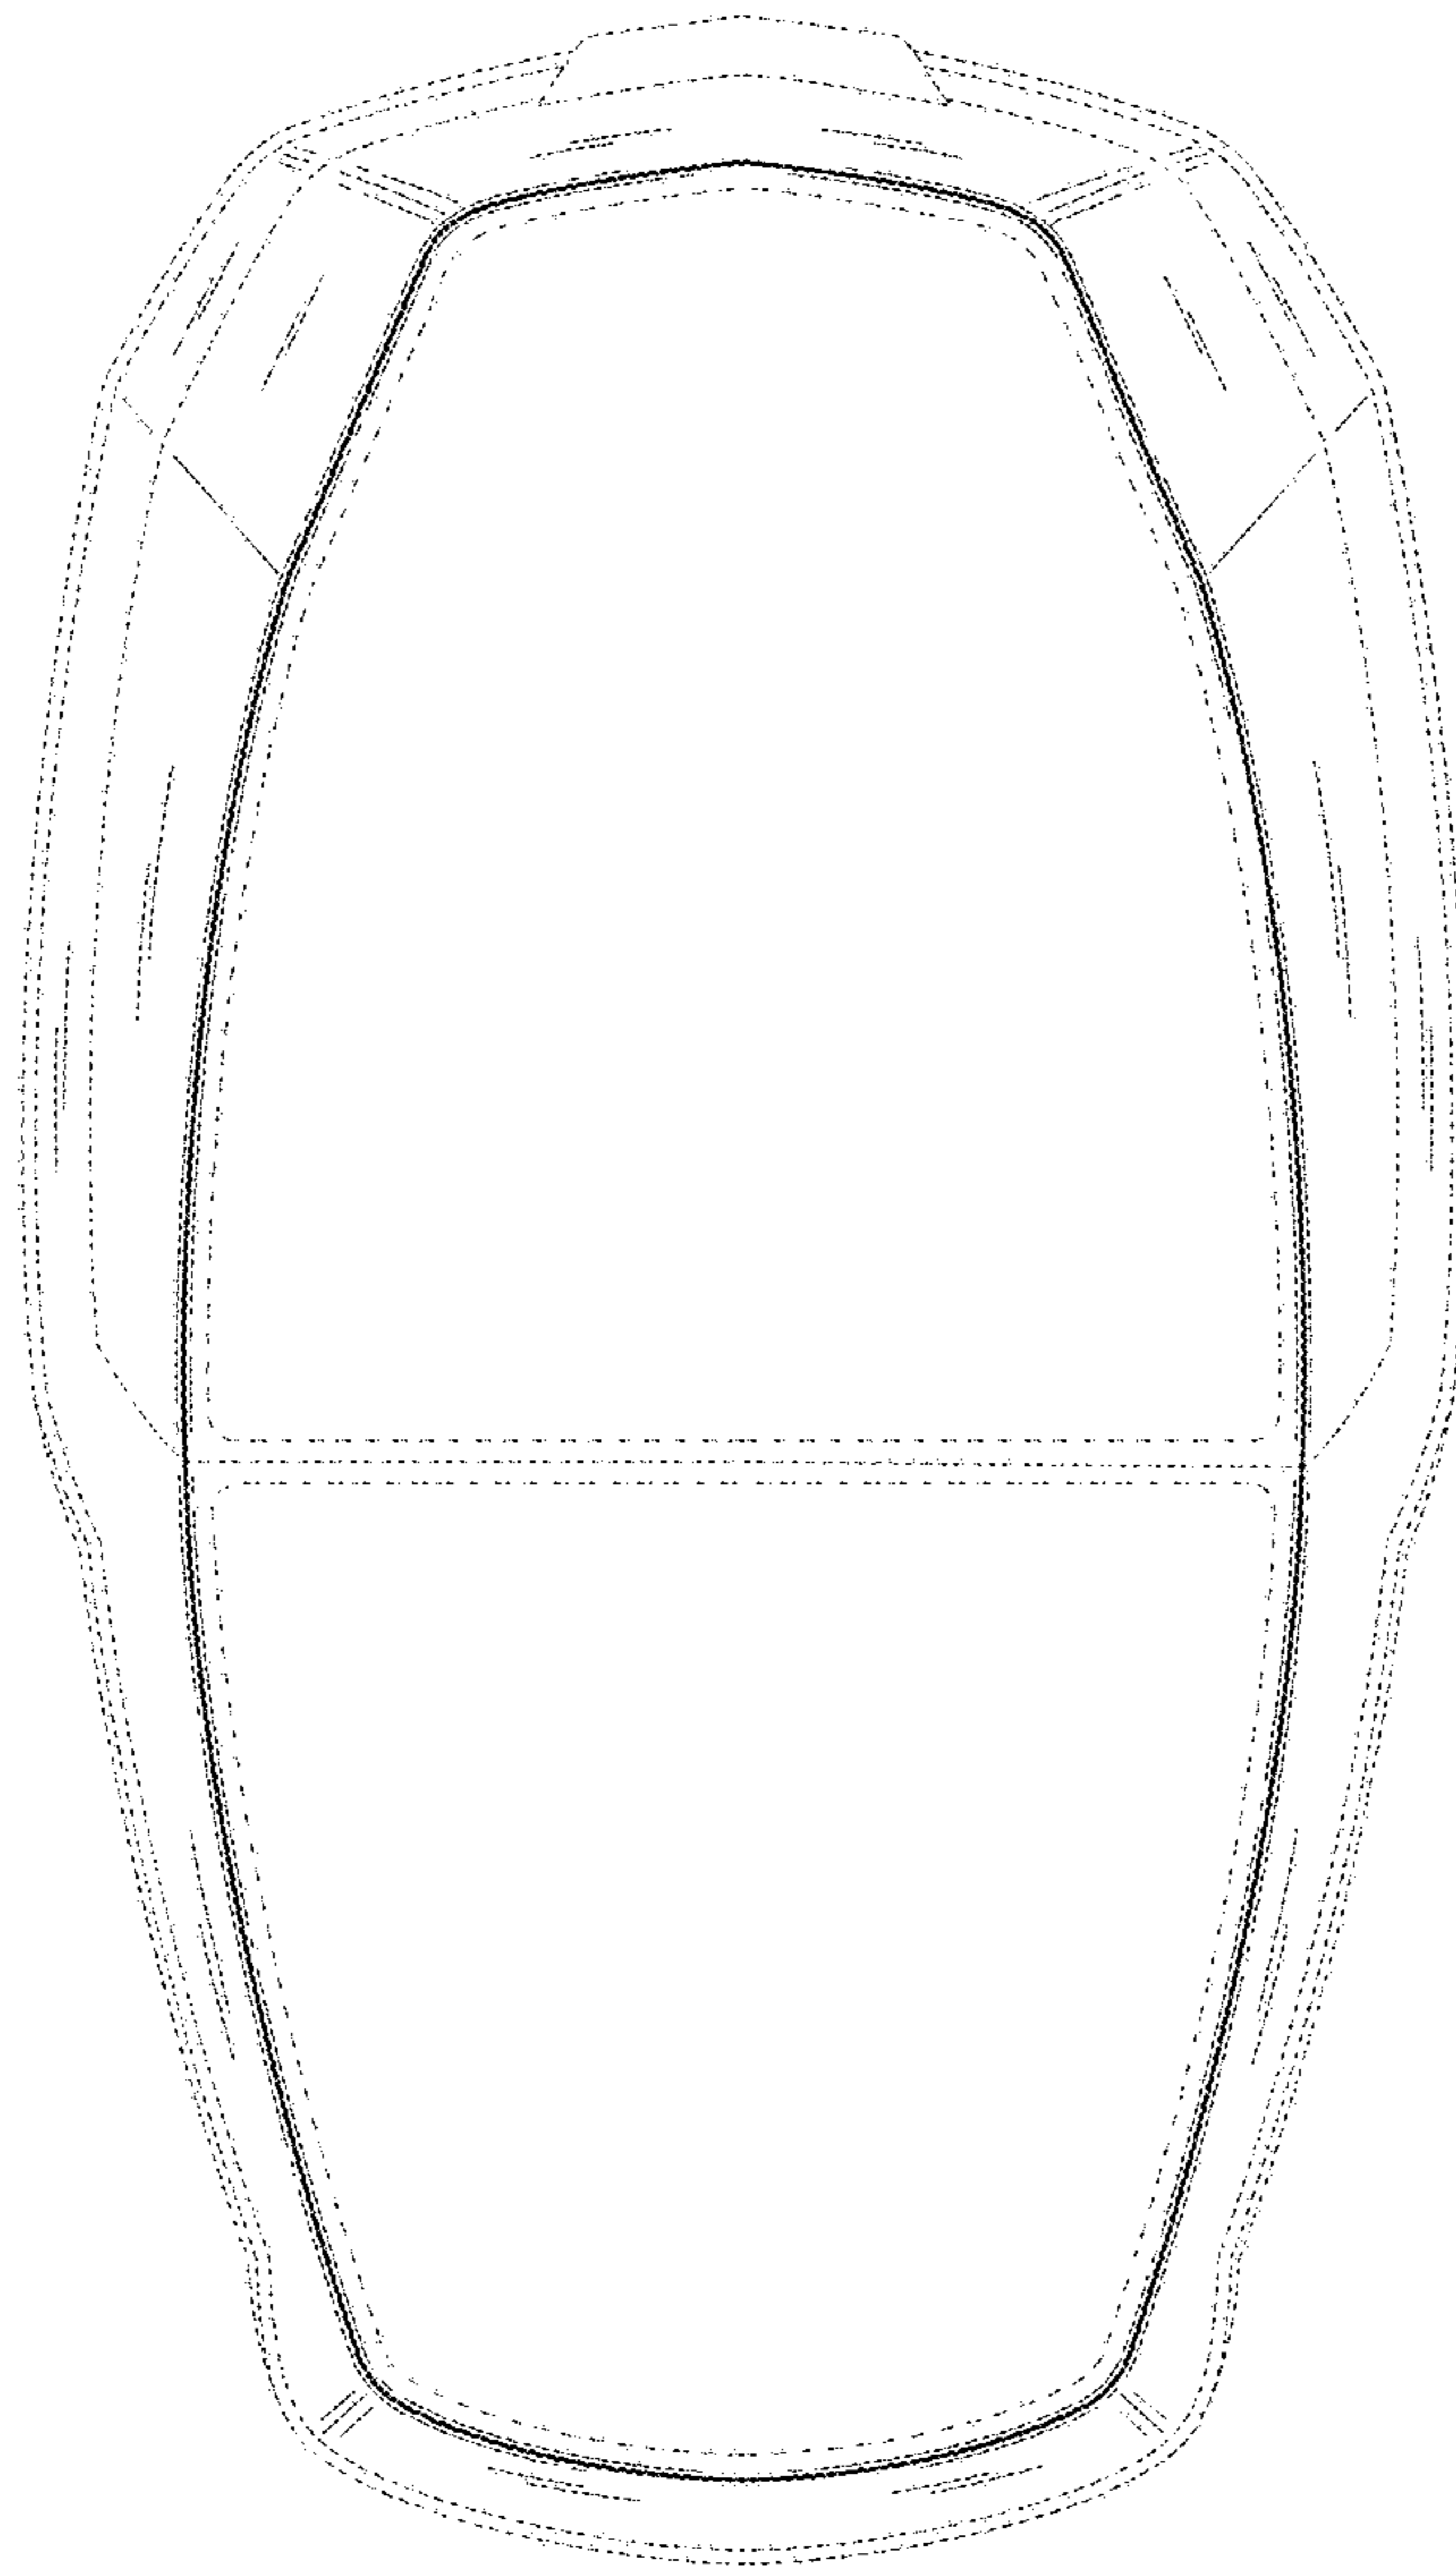


Fig. 3

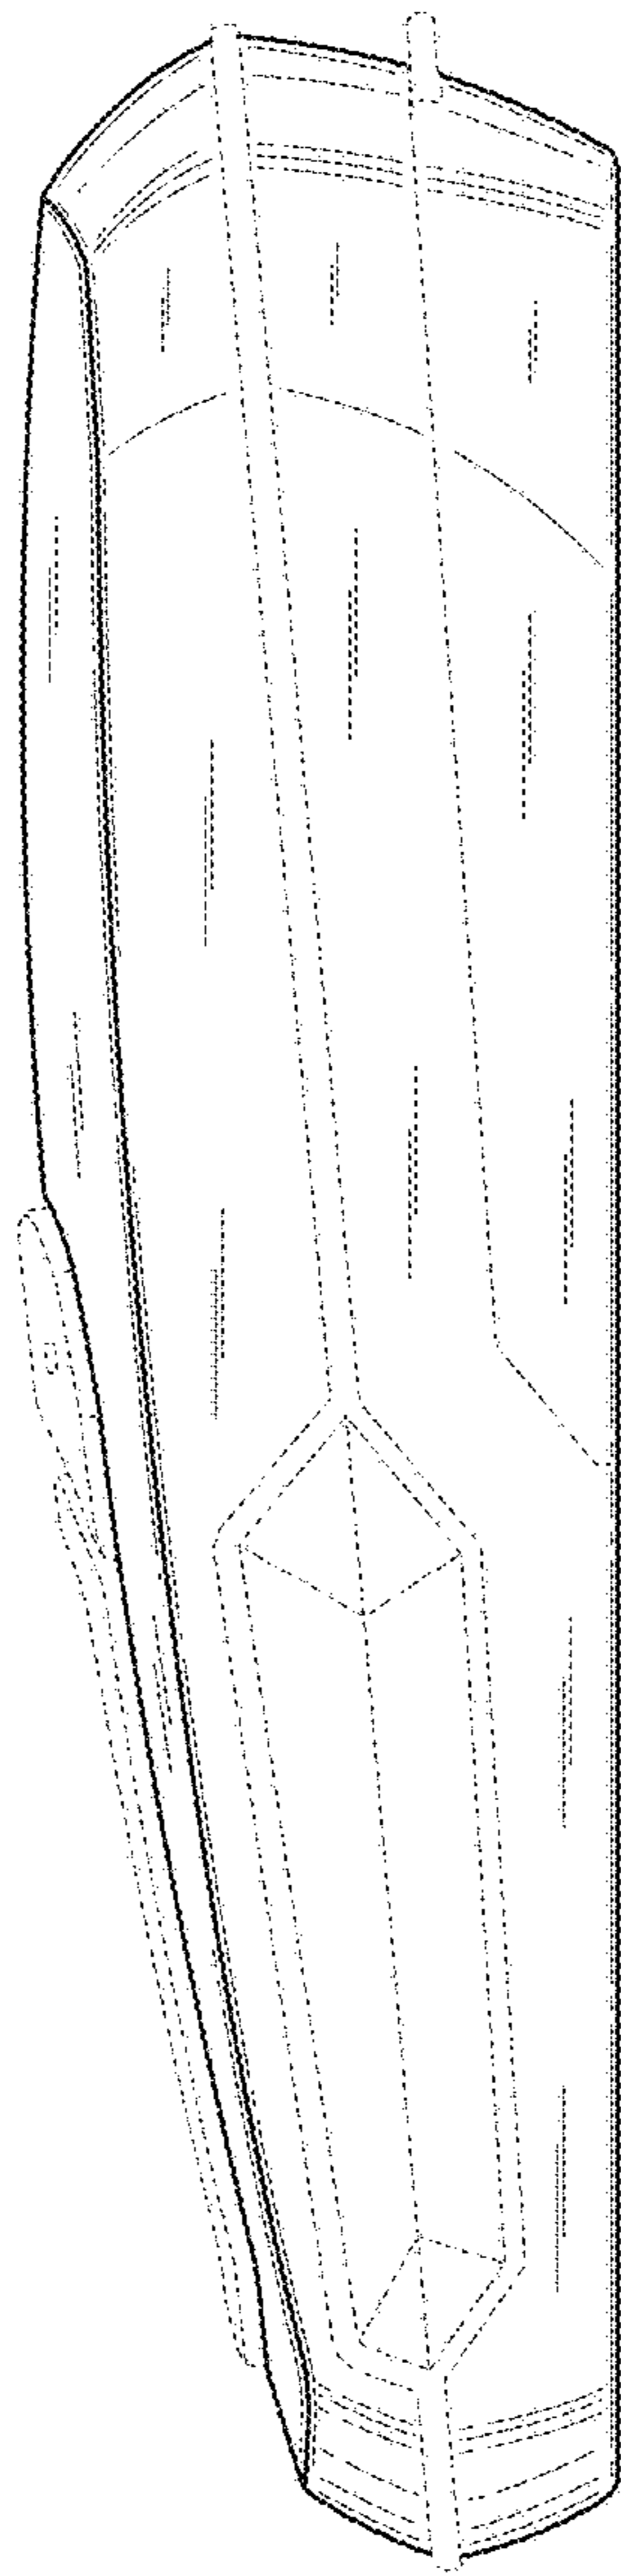


Fig. 4

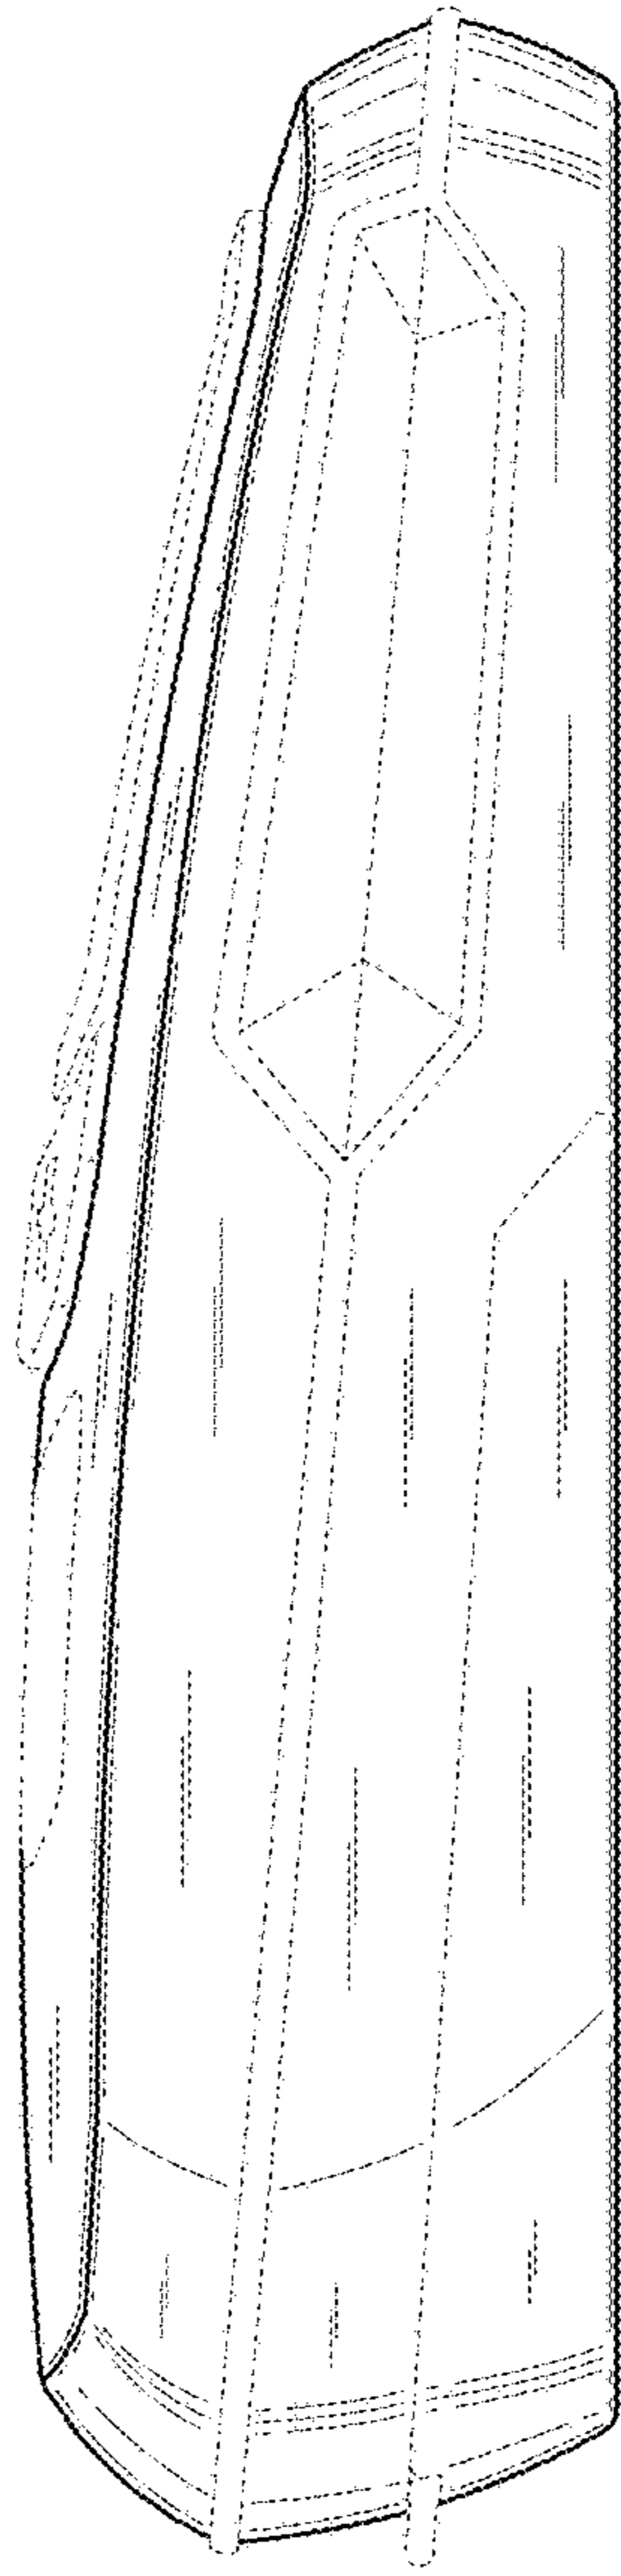


Fig. 5

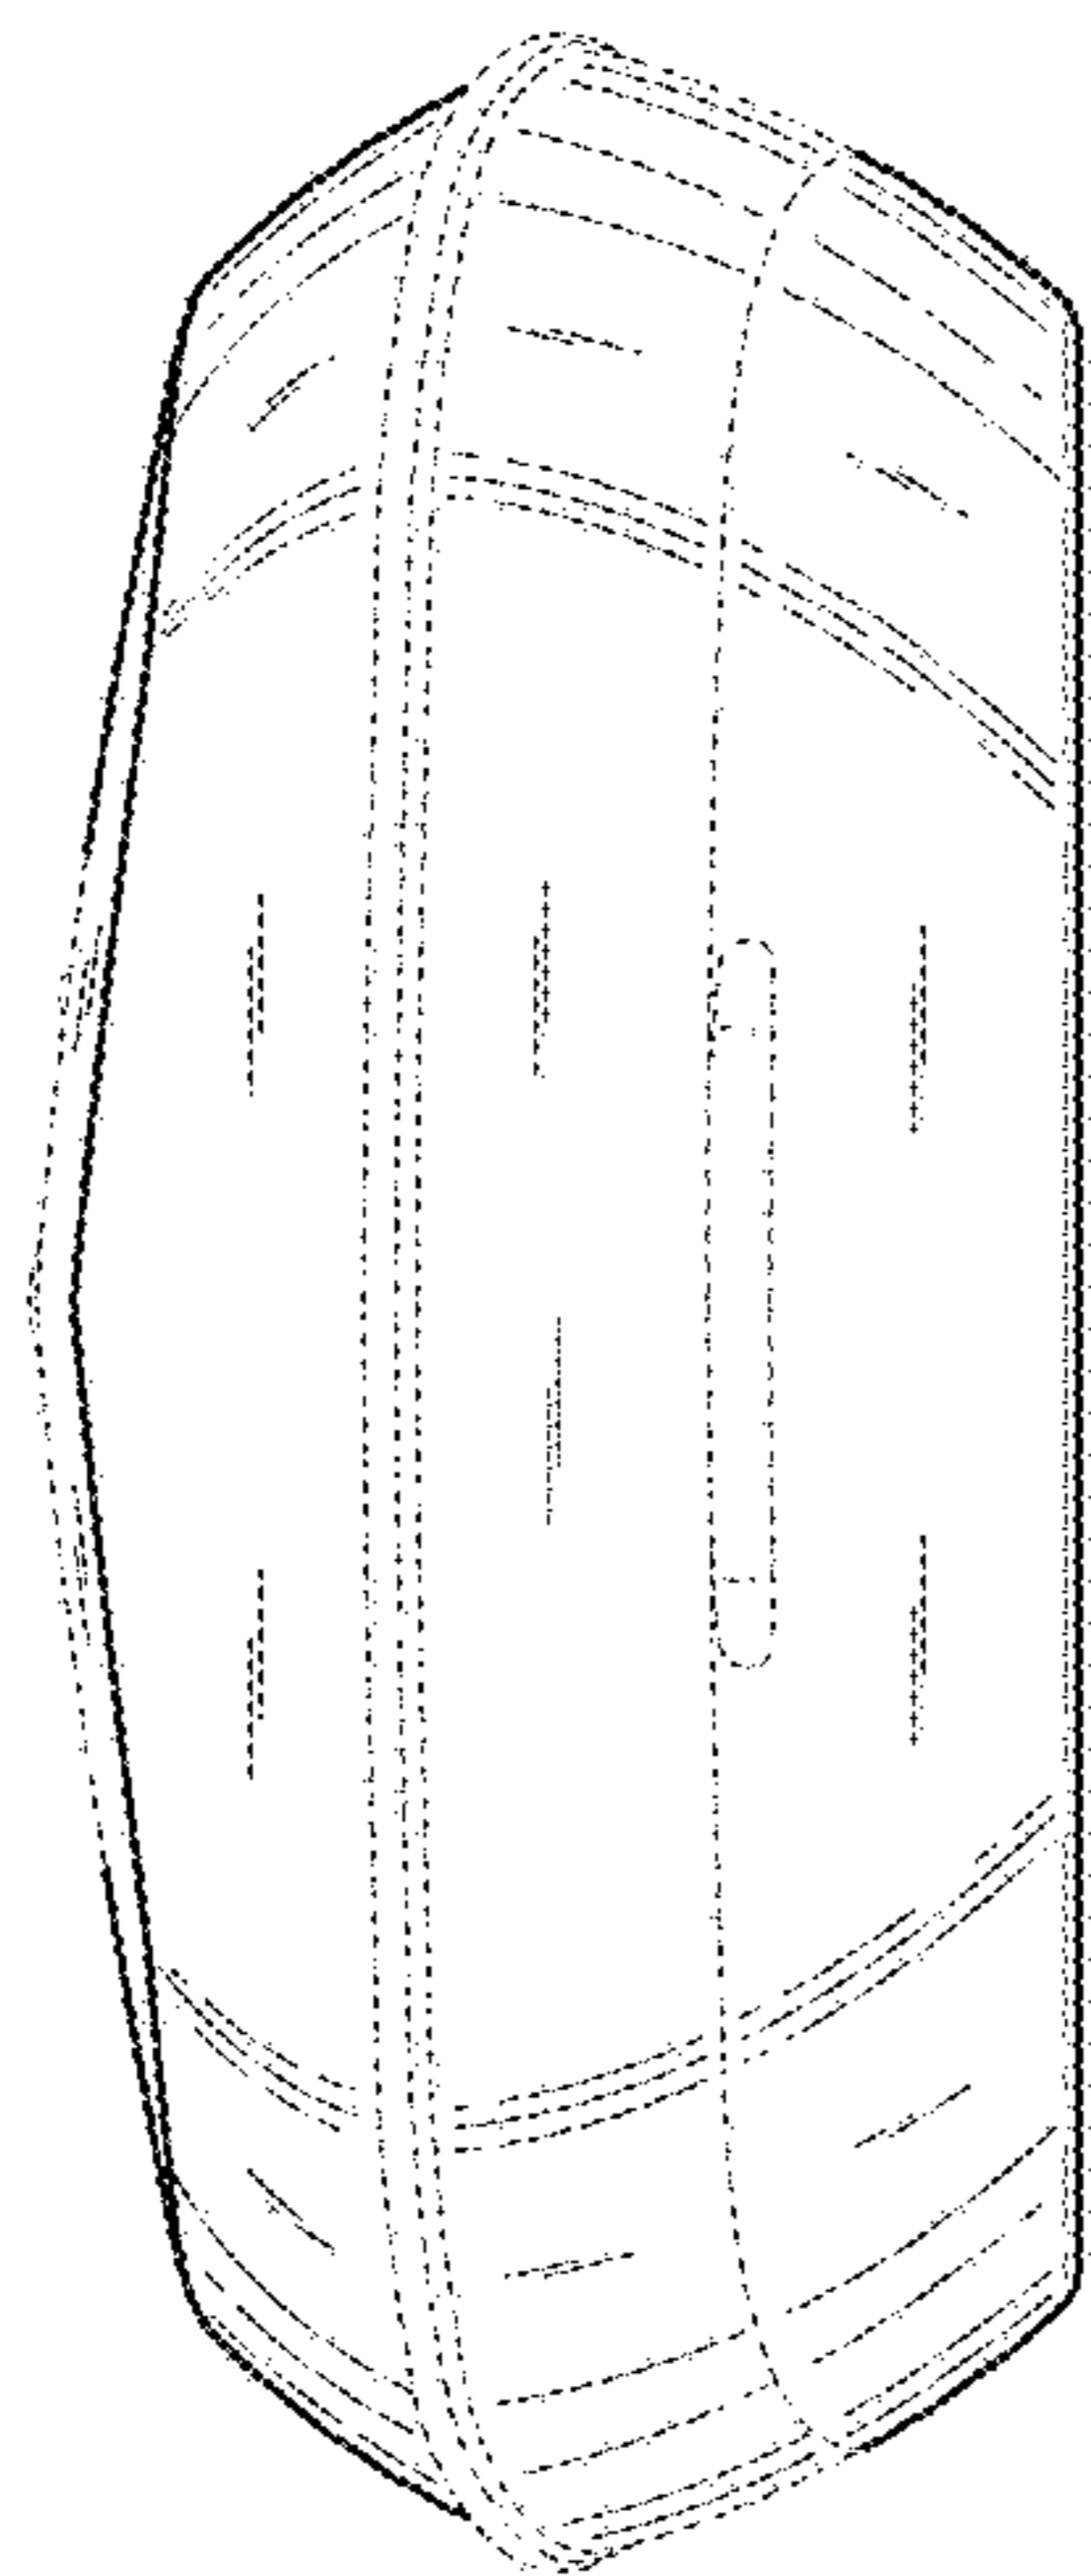


Fig. 6

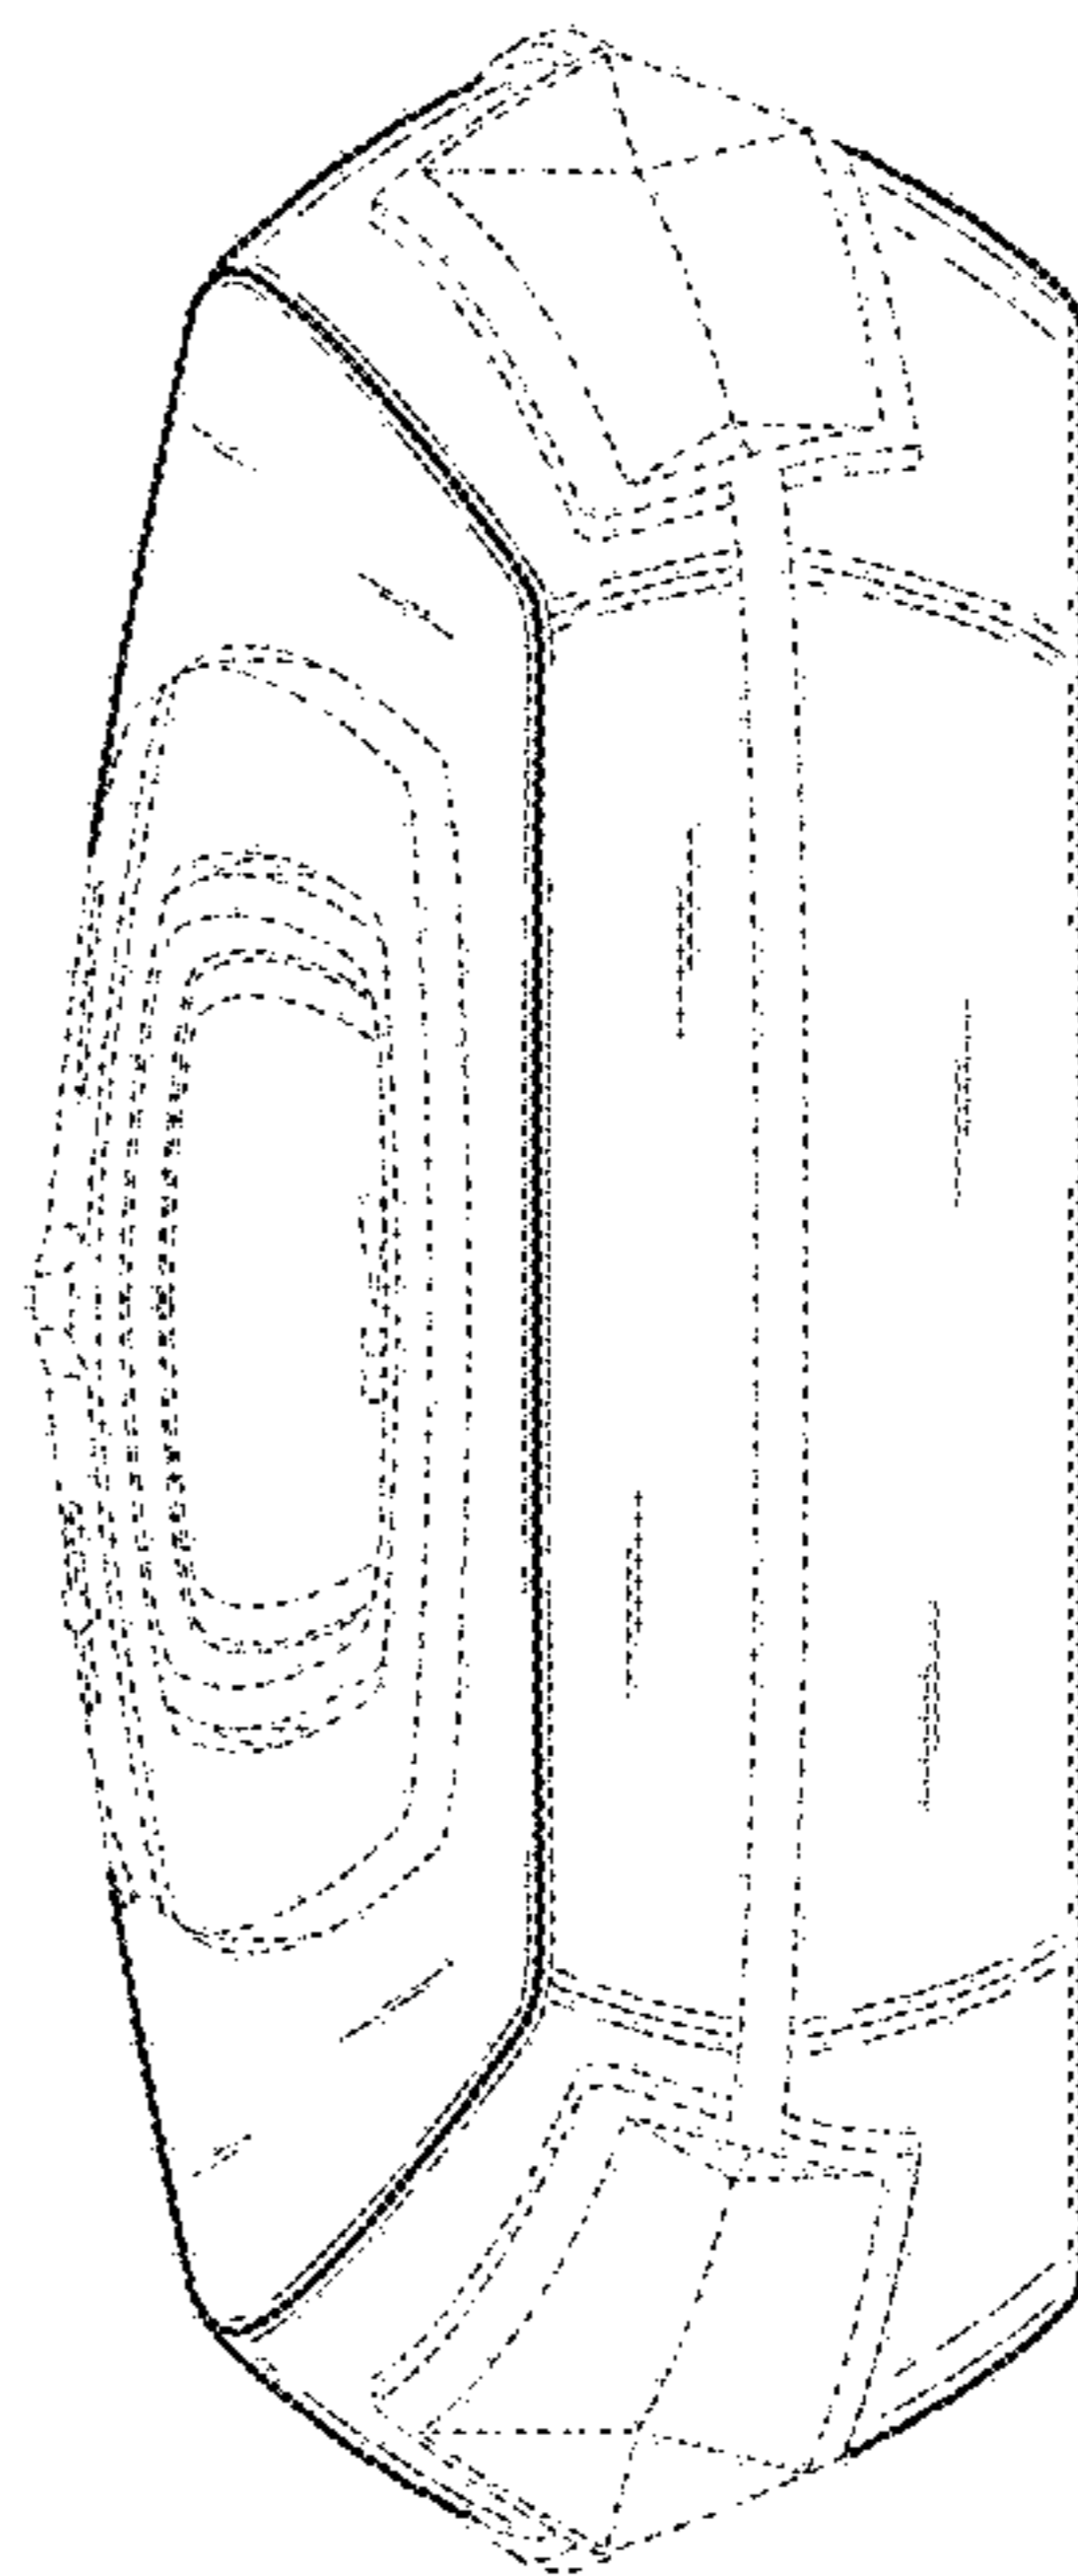


Fig. 7