



US00D850613S

(12) **United States Design Patent**  
**Kern et al.**

(10) **Patent No.:** **US D850,613 S**  
(45) **Date of Patent:** **\*\* Jun. 4, 2019**

- (54) **DRUG DELIVERY DEVICE**
- (71) Applicant: **Sanofi-Aventis Deutschland GMBH**,  
Frankfurt am Main (DE)
- (72) Inventors: **Daniel Kern**, Frankfurt am Main (DE);  
**Udo Stauder**, Frankfurt am Main (DE);  
**Marc Holtwick**, Frankfurt am Main  
(DE); **Steffen Raab**, Frankfurt am Main  
(DE)
- (73) Assignee: **Sanofi-Aventis Deutschland GMBH**,  
Frankfurt am Main (DE)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/577,185**
- (22) Filed: **Sep. 9, 2016**
- (51) **LOC (11) Cl.** ..... **24-02**
- (52) **U.S. Cl.**  
USPC ..... **D24/113**
- (58) **Field of Classification Search**  
USPC ..... D24/112–114, 108, 133, 130, 127, 186;  
606/181, 185; 604/264, 272, 187, 181,  
604/184, 227  
CPC ..... A61M 5/178; A61M 3/00; A61M 5/20;  
A61M 5/31; A61M 5/3146; A61M  
5/3129; A61M 5/3148; A61M 5/315  
See application file for complete search history.

- D746,444 S \* 12/2015 Jones ..... D24/113
- 9,314,576 B2 \* 4/2016 Mercer ..... A61M 5/3294
- D755,369 S \* 5/2016 Sanders ..... D24/113
- 9,440,027 B2 \* 9/2016 Kouyoumjian ..... A61M 5/2448
- D770,038 S \* 10/2016 Ahlgrim ..... D24/113
- D770,611 S \* 11/2016 Saussaye ..... D24/114
- D773,038 S \* 11/2016 Tanner ..... D24/113
- D773,646 S \* 12/2016 Amend Kwasnik ..... D24/113
- D776,261 S \* 1/2017 Jones ..... D24/113
- D777,907 S \* 1/2017 Amend Kwasnik ..... D24/113
- D780,909 S \* 3/2017 Burkett ..... D24/113

\* cited by examiner

*Primary Examiner* — David G Muller

(74) *Attorney, Agent, or Firm* — Fish & Richardson P.C.

(57) **CLAIM**

The ornamental design for a drug delivery device, substantially as shown and described.

**DESCRIPTION**

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent publication with color drawings(s) will be provided by the Office upon request and payment of the necessary fee.

- FIG. 1 is a rear view of the drug delivery device;
- FIG. 2 is a front view thereof;
- FIG. 3 is a right side view thereof;
- FIG. 4 is a left side view thereof;
- FIG. 5 is a bottom view thereof;
- FIG. 6 is a top view thereof; and,
- FIG. 7 is a perspective view thereof.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D725,771 S \* 3/2015 Sendatzki ..... D24/113
- D743,538 S \* 11/2015 Sanders ..... D24/113

**1 Claim, 7 Drawing Sheets**  
**(7 of 7 Drawing Sheet(s) Filed in Color)**

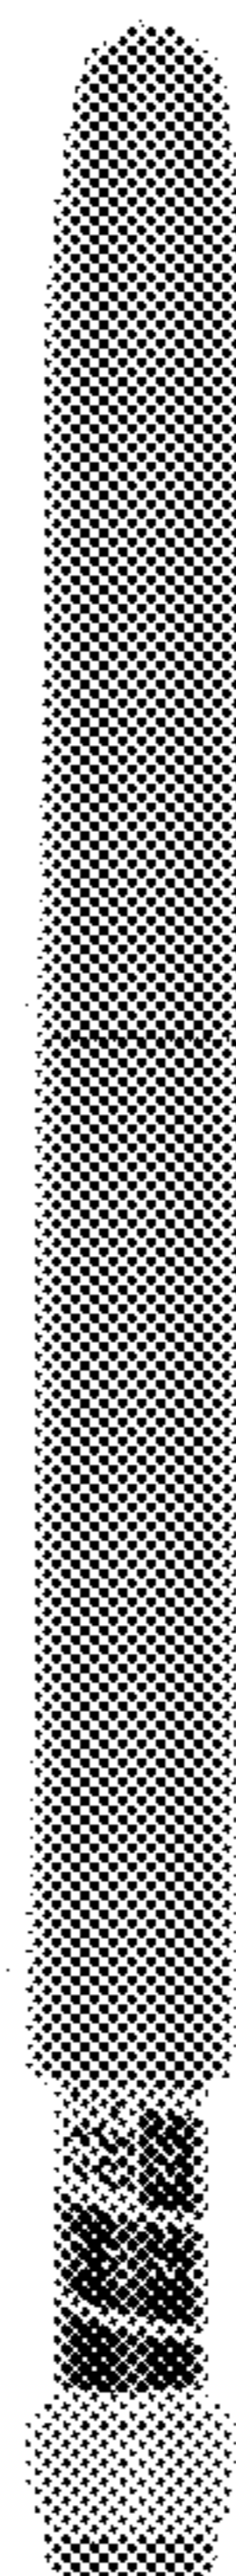




FIG. 1

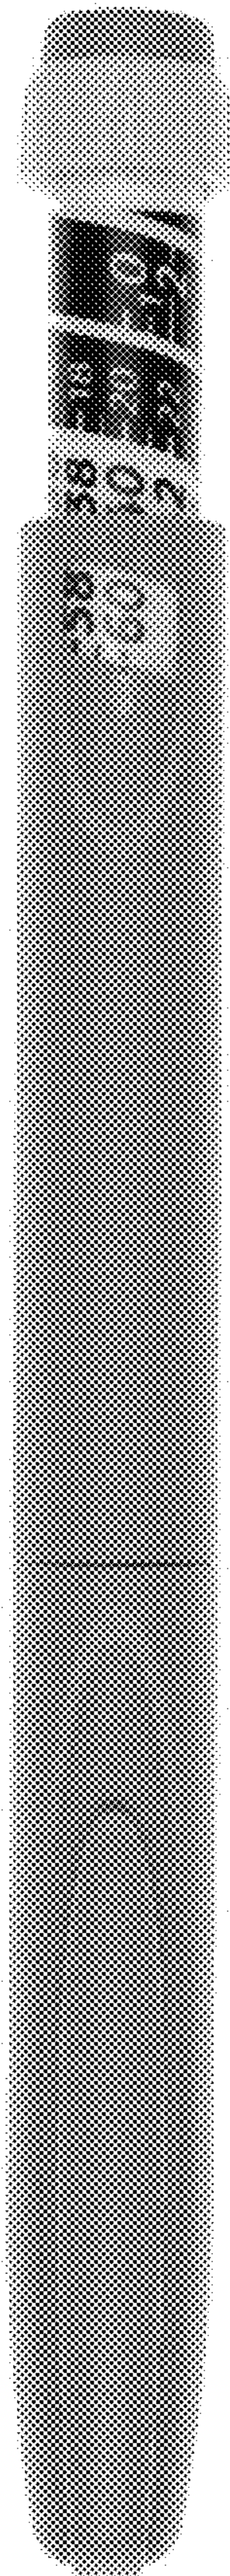


FIG. 2



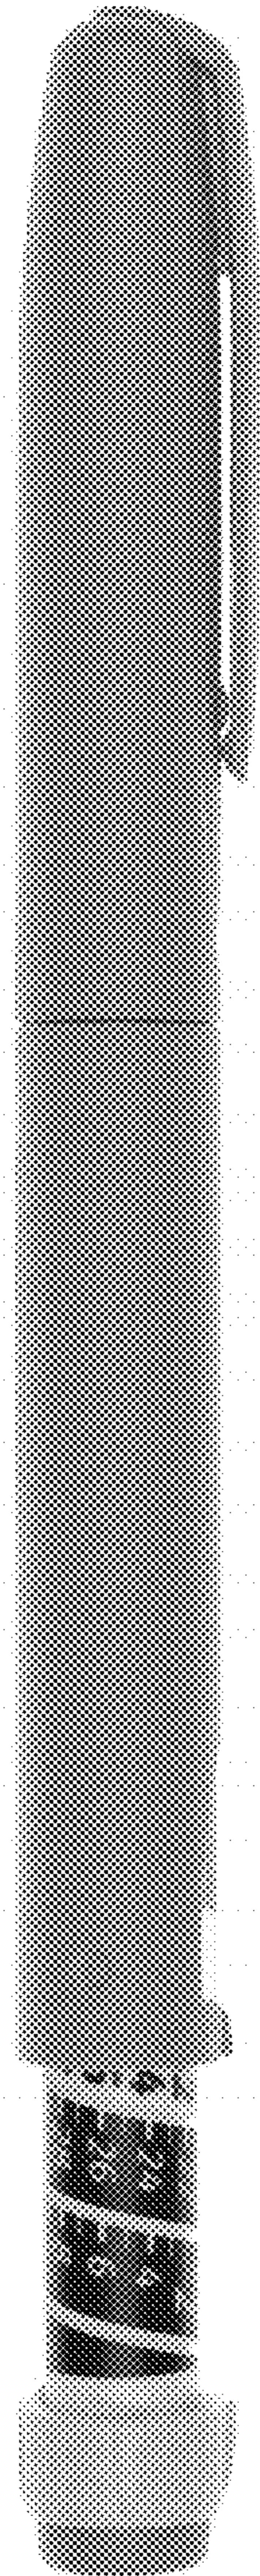


FIG. 3

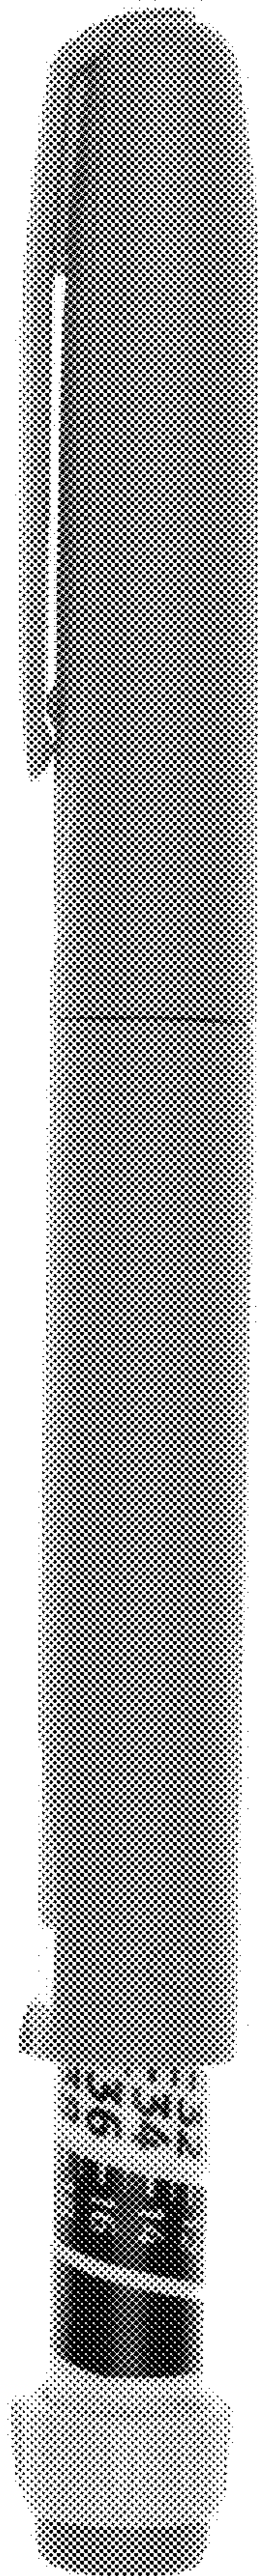
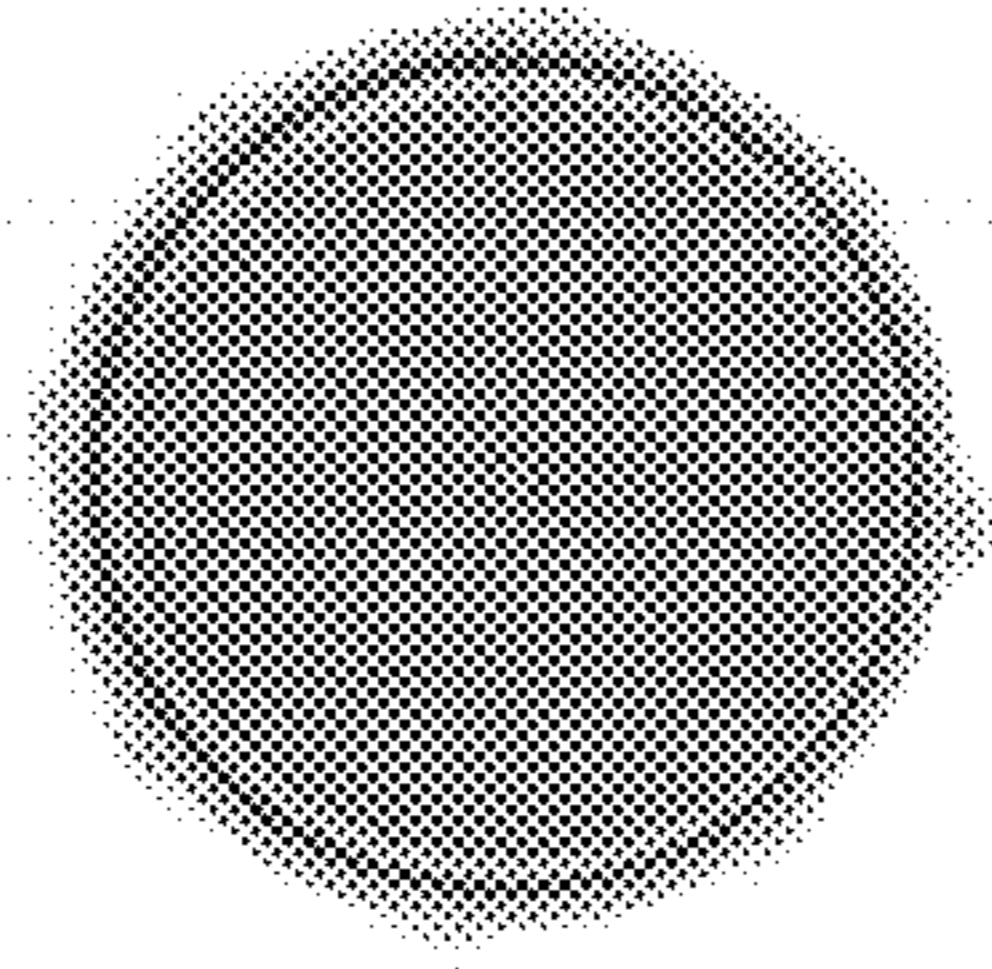


FIG. 4

FIG. 5




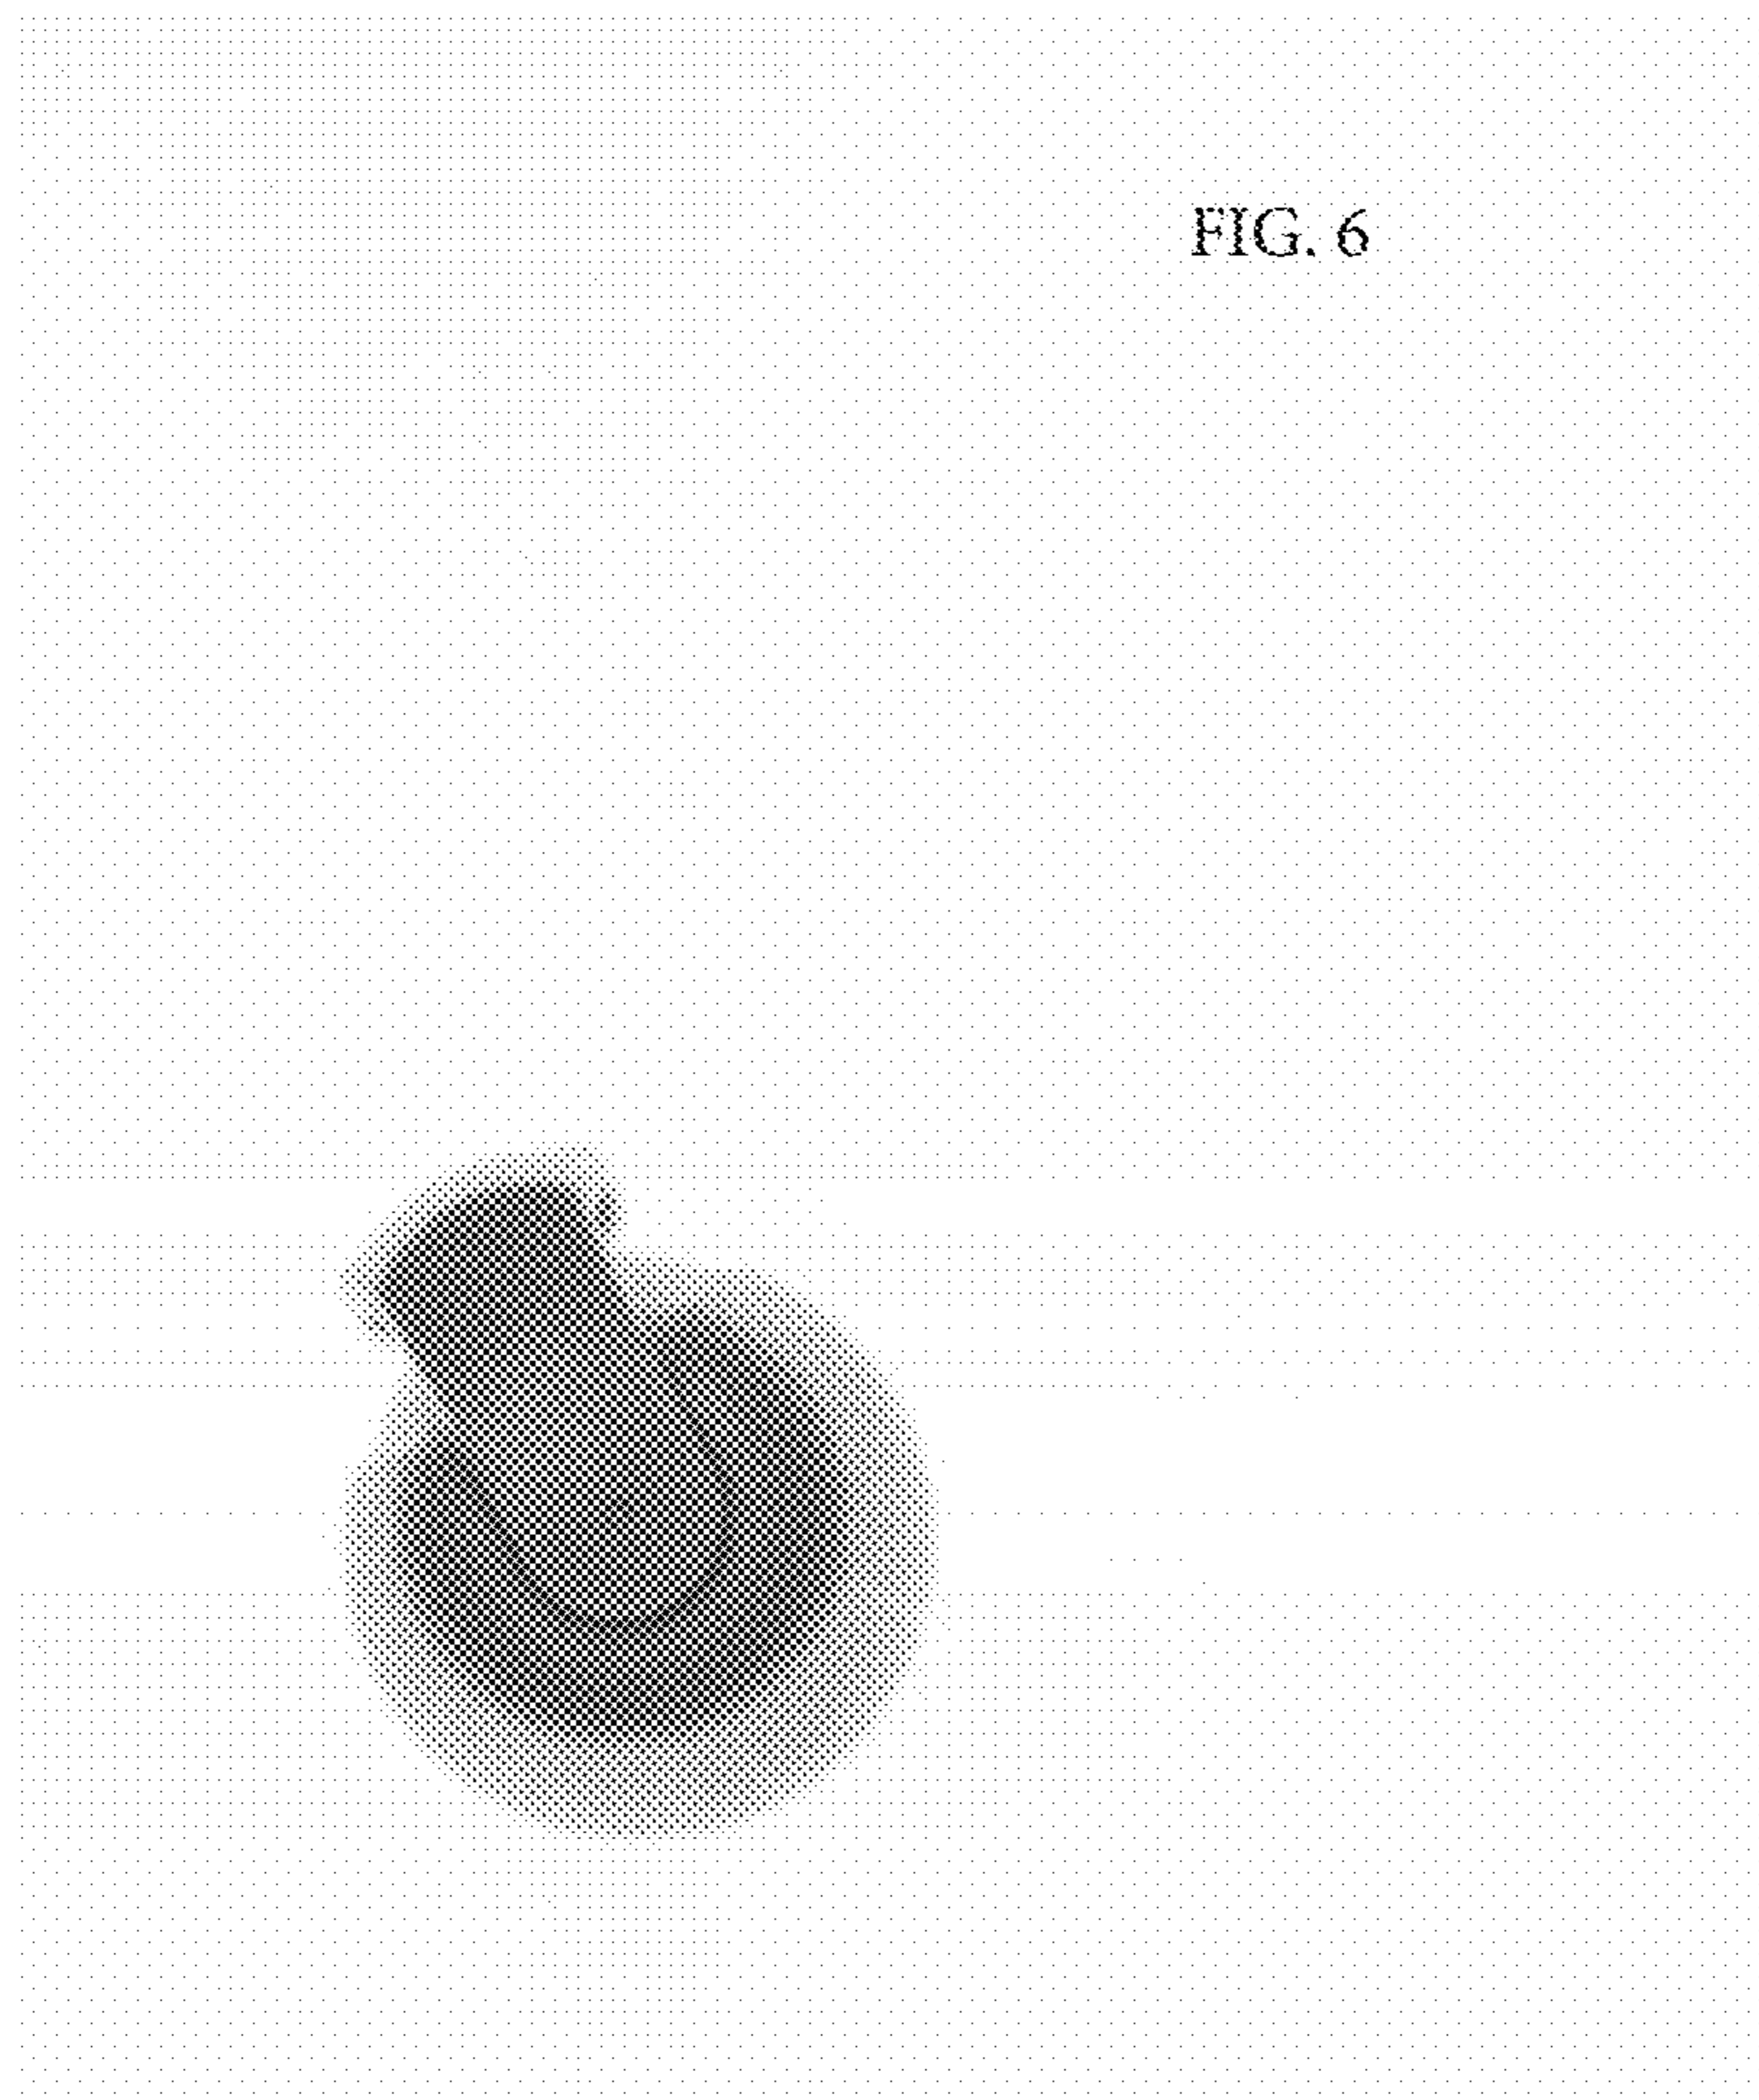




FIG. 7



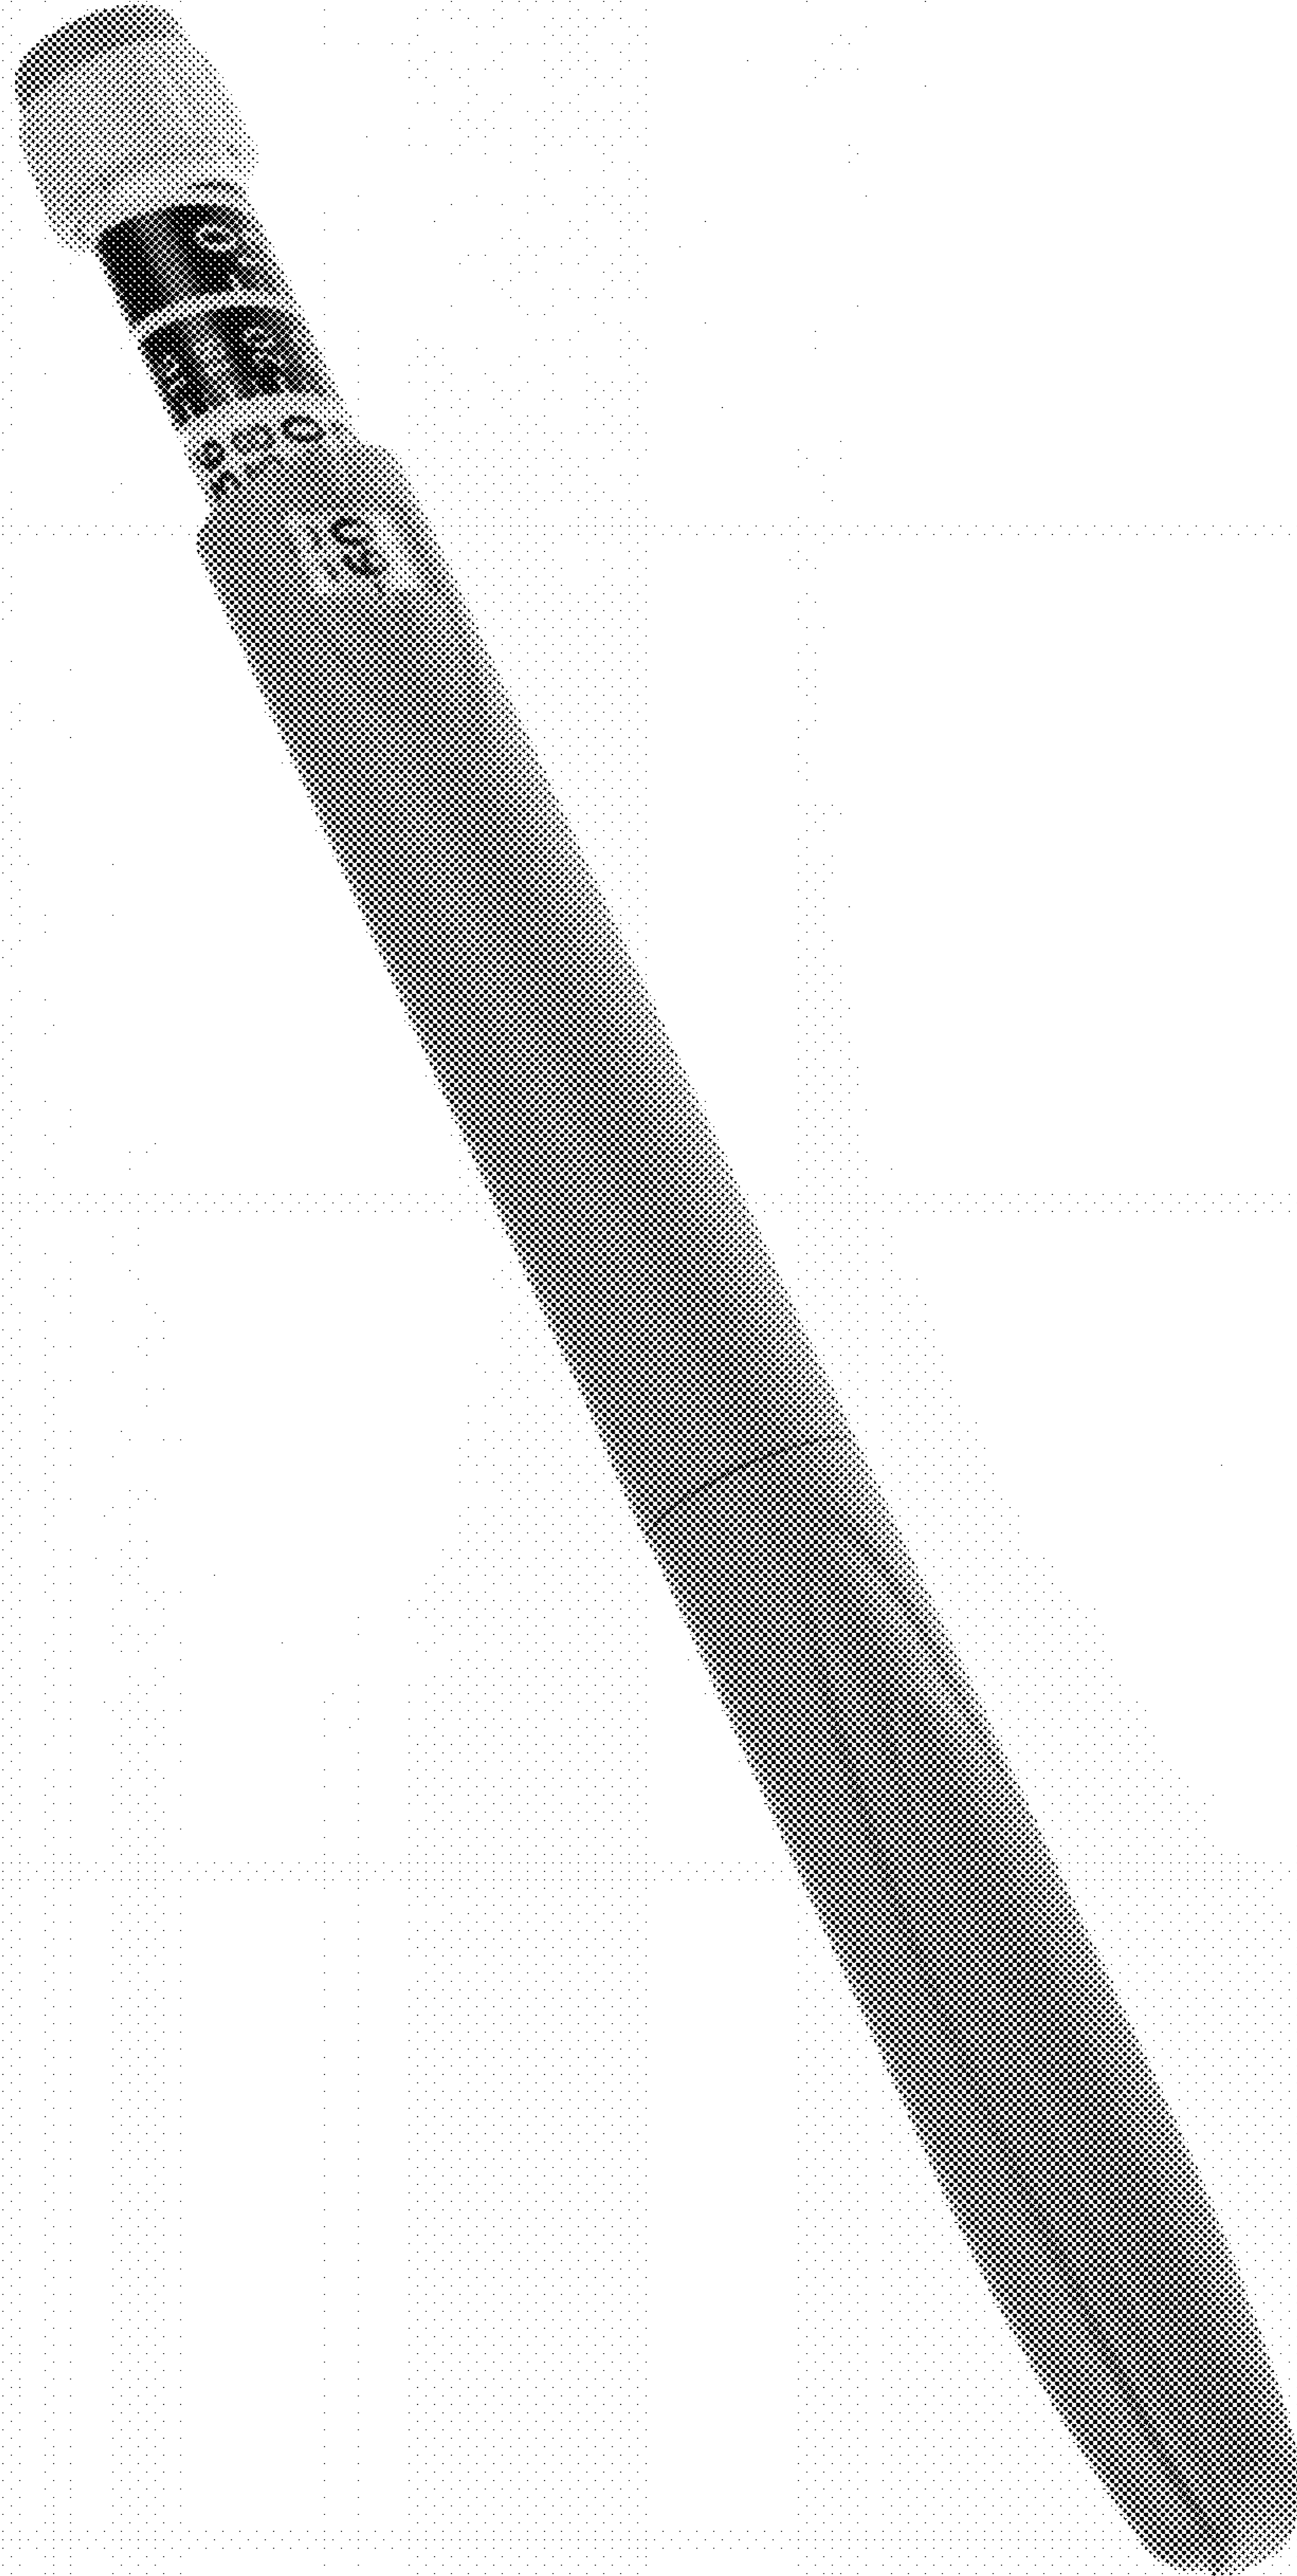

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : D850,613 S  
APPLICATION NO. : 29/577185  
DATED : June 4, 2019  
INVENTOR(S) : Daniel Kern et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:


On the Title Page

After Item (22) insert:

-- (30) **Foreign Application Priority Data**

003 149 657-0001	EU	2016-05-24
003 149 657-0002	EU	2016-05-24
003 149 657-0003	EU	2016-05-24
003 149 657-0004	EU	2016-05-24
003 149 657-0005	EU	2016-05-24
003 149 657-0006	EU	2016-05-24
003 372 697-0001	EU	2016-09-09
003 372 697-0002	EU	2016-09-09
003 372 697-0003	EU	2016-09-09 --

Signed and Sealed this  
Tenth Day of March, 2020

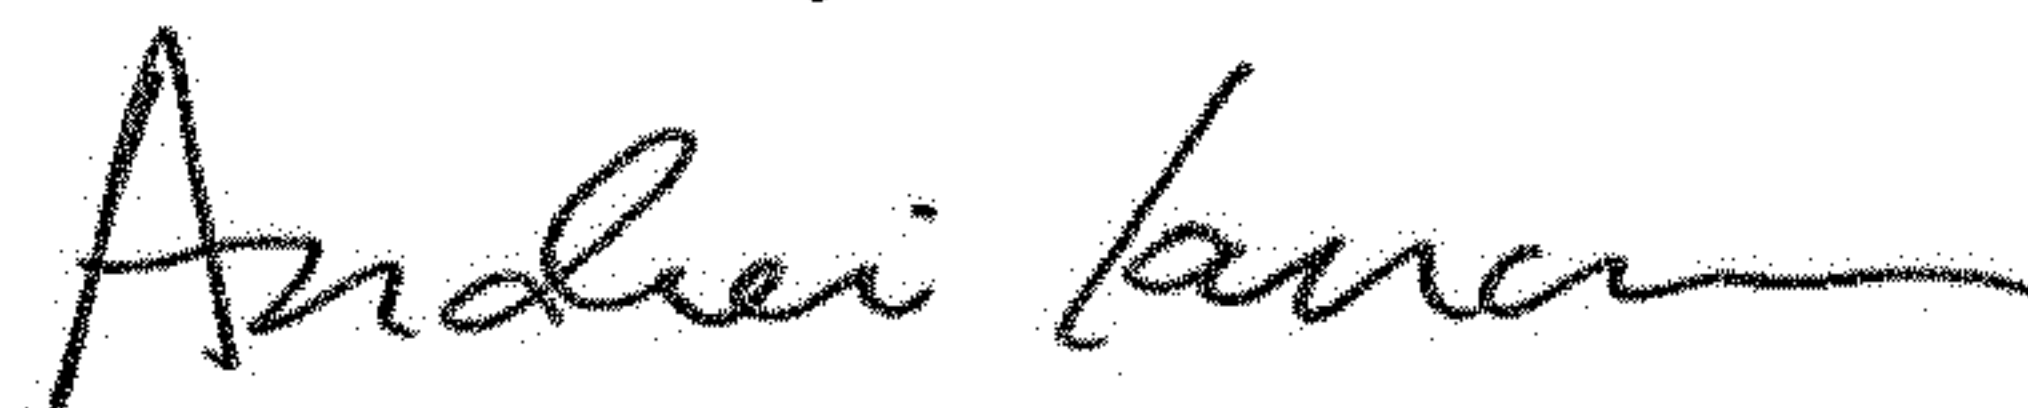

Andrei Iancu  
*Director of the United States Patent and Trademark Office*