



US00D850628S

(12) **United States Design Patent** (10) **Patent No.:** **US D850,628 S**  
**De Hoog et al.** (45) **Date of Patent:** **\*\* Jun. 4, 2019**

(54) **MEDICAL MONITORING DEVICE FOR SLEEP DISORDERS**

(71) Applicant: **NIGHTBALANCE B.V.**, The Hague (NL)

(72) Inventors: **Guus De Hoog**, Amsterdam (NL); **Robert Franciscus Van Der Hulst**, Leiden (NL); **Thijs van Oorschot**, Leiderdorp (NL)

(73) Assignee: **NIGHTBALANCE B.V.**, Delft (NL)

(\*\*) Term: **15 Years**

(21) Appl. No.: **35/503,711**

(22) Filed: **Mar. 24, 2017**

(80) **Hague Agreement Data**

Int. Filing Date: **Mar. 24, 2017**

Int. Reg. No.: **DM/097250**

Int. Reg. Date: **Mar. 24, 2017**

Int. Reg. Pub. Date: **Sep. 29, 2017**

(51) **LOC (11) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/186**

(58) **Field of Classification Search**  
USPC ..... D24/186, 165, 167, 168, 169; D10/75  
CPC . A61B 5/02438; A61B 5/6824; A61B 5/6825;  
A61B 5/024  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D452,012 S	*	12/2001	Phillips	.....	D24/186
D481,057 S	*	10/2003	Brady	.....	D14/371
D554,640 S	*	11/2007	Ponnert	.....	D14/388
D631,552 S	*	1/2011	Kasabach	.....	D24/186
D663,421 S	*	7/2012	Steiner	.....	D24/169

D712,541 S	*	9/2014	Brigham	.....	D24/167
D723,550 S	*	3/2015	Krueger	.....	D14/341
D726,680 S	*	4/2015	Kim	.....	D10/37
D726,924 S	*	4/2015	Tseng	.....	D24/186
D729,939 S	*	5/2015	Moon	.....	D24/169
D744,656 S	*	12/2015	Schempp	.....	D24/165
D757,275 S	*	5/2016	Lee	.....	D24/187
D760,903 S	*	7/2016	Lin	.....	D24/165
D768,858 S	*	10/2016	Komulainen	.....	D24/167
D769,867 S	*	10/2016	Aumiller	.....	D14/344
D780,928 S	*	3/2017	Hayakawa	.....	D24/169
D783,172 S	*	4/2017	Hilbig	.....	D24/186
D788,312 S	*	5/2017	Al-Ali	.....	A61B 5/002 D24/186
D794,805 S	*	8/2017	Kranz	.....	D24/186
D794,806 S	*	8/2017	Kranz	.....	D24/186
D804,042 S	*	11/2017	Cohrs	.....	D24/186
D814,463 S	*	4/2018	Haigh	.....	D14/358
D814,949 S	*	4/2018	Clapper	.....	D10/46
D821,595 S	*	6/2018	Ito	.....	D24/200
D822,216 S	*	7/2018	Barker	.....	D24/186
10,034,500 B2	*	7/2018	Kaneko	.....	A41D 13/1281
2013/0338518 A1	*	12/2013	Zoica	.....	A61B 5/7225 600/516

\* cited by examiner

*Primary Examiner* — Robert M. Spear


(57) **CLAIM**


The ornamental design for a medical monitoring device for sleep disorders, as shown and described.

**DESCRIPTION**


FIG. 1.1 is a front perspective view of a medical monitoring device for sleep disorders showing our new design; FIG. 1.2 is a rear perspective view thereof; FIG. 1.3 is a left side elevation view thereof; FIG. 1.4 is a front view thereof; FIG. 1.5 is a right side elevation view thereof; FIG. 1.6 is a rear elevation view thereof; and FIG. 1.7 is a top view thereof; and, FIG. 1.8 is a bottom view thereof.

**1 Claim, 5 Drawing Sheets**

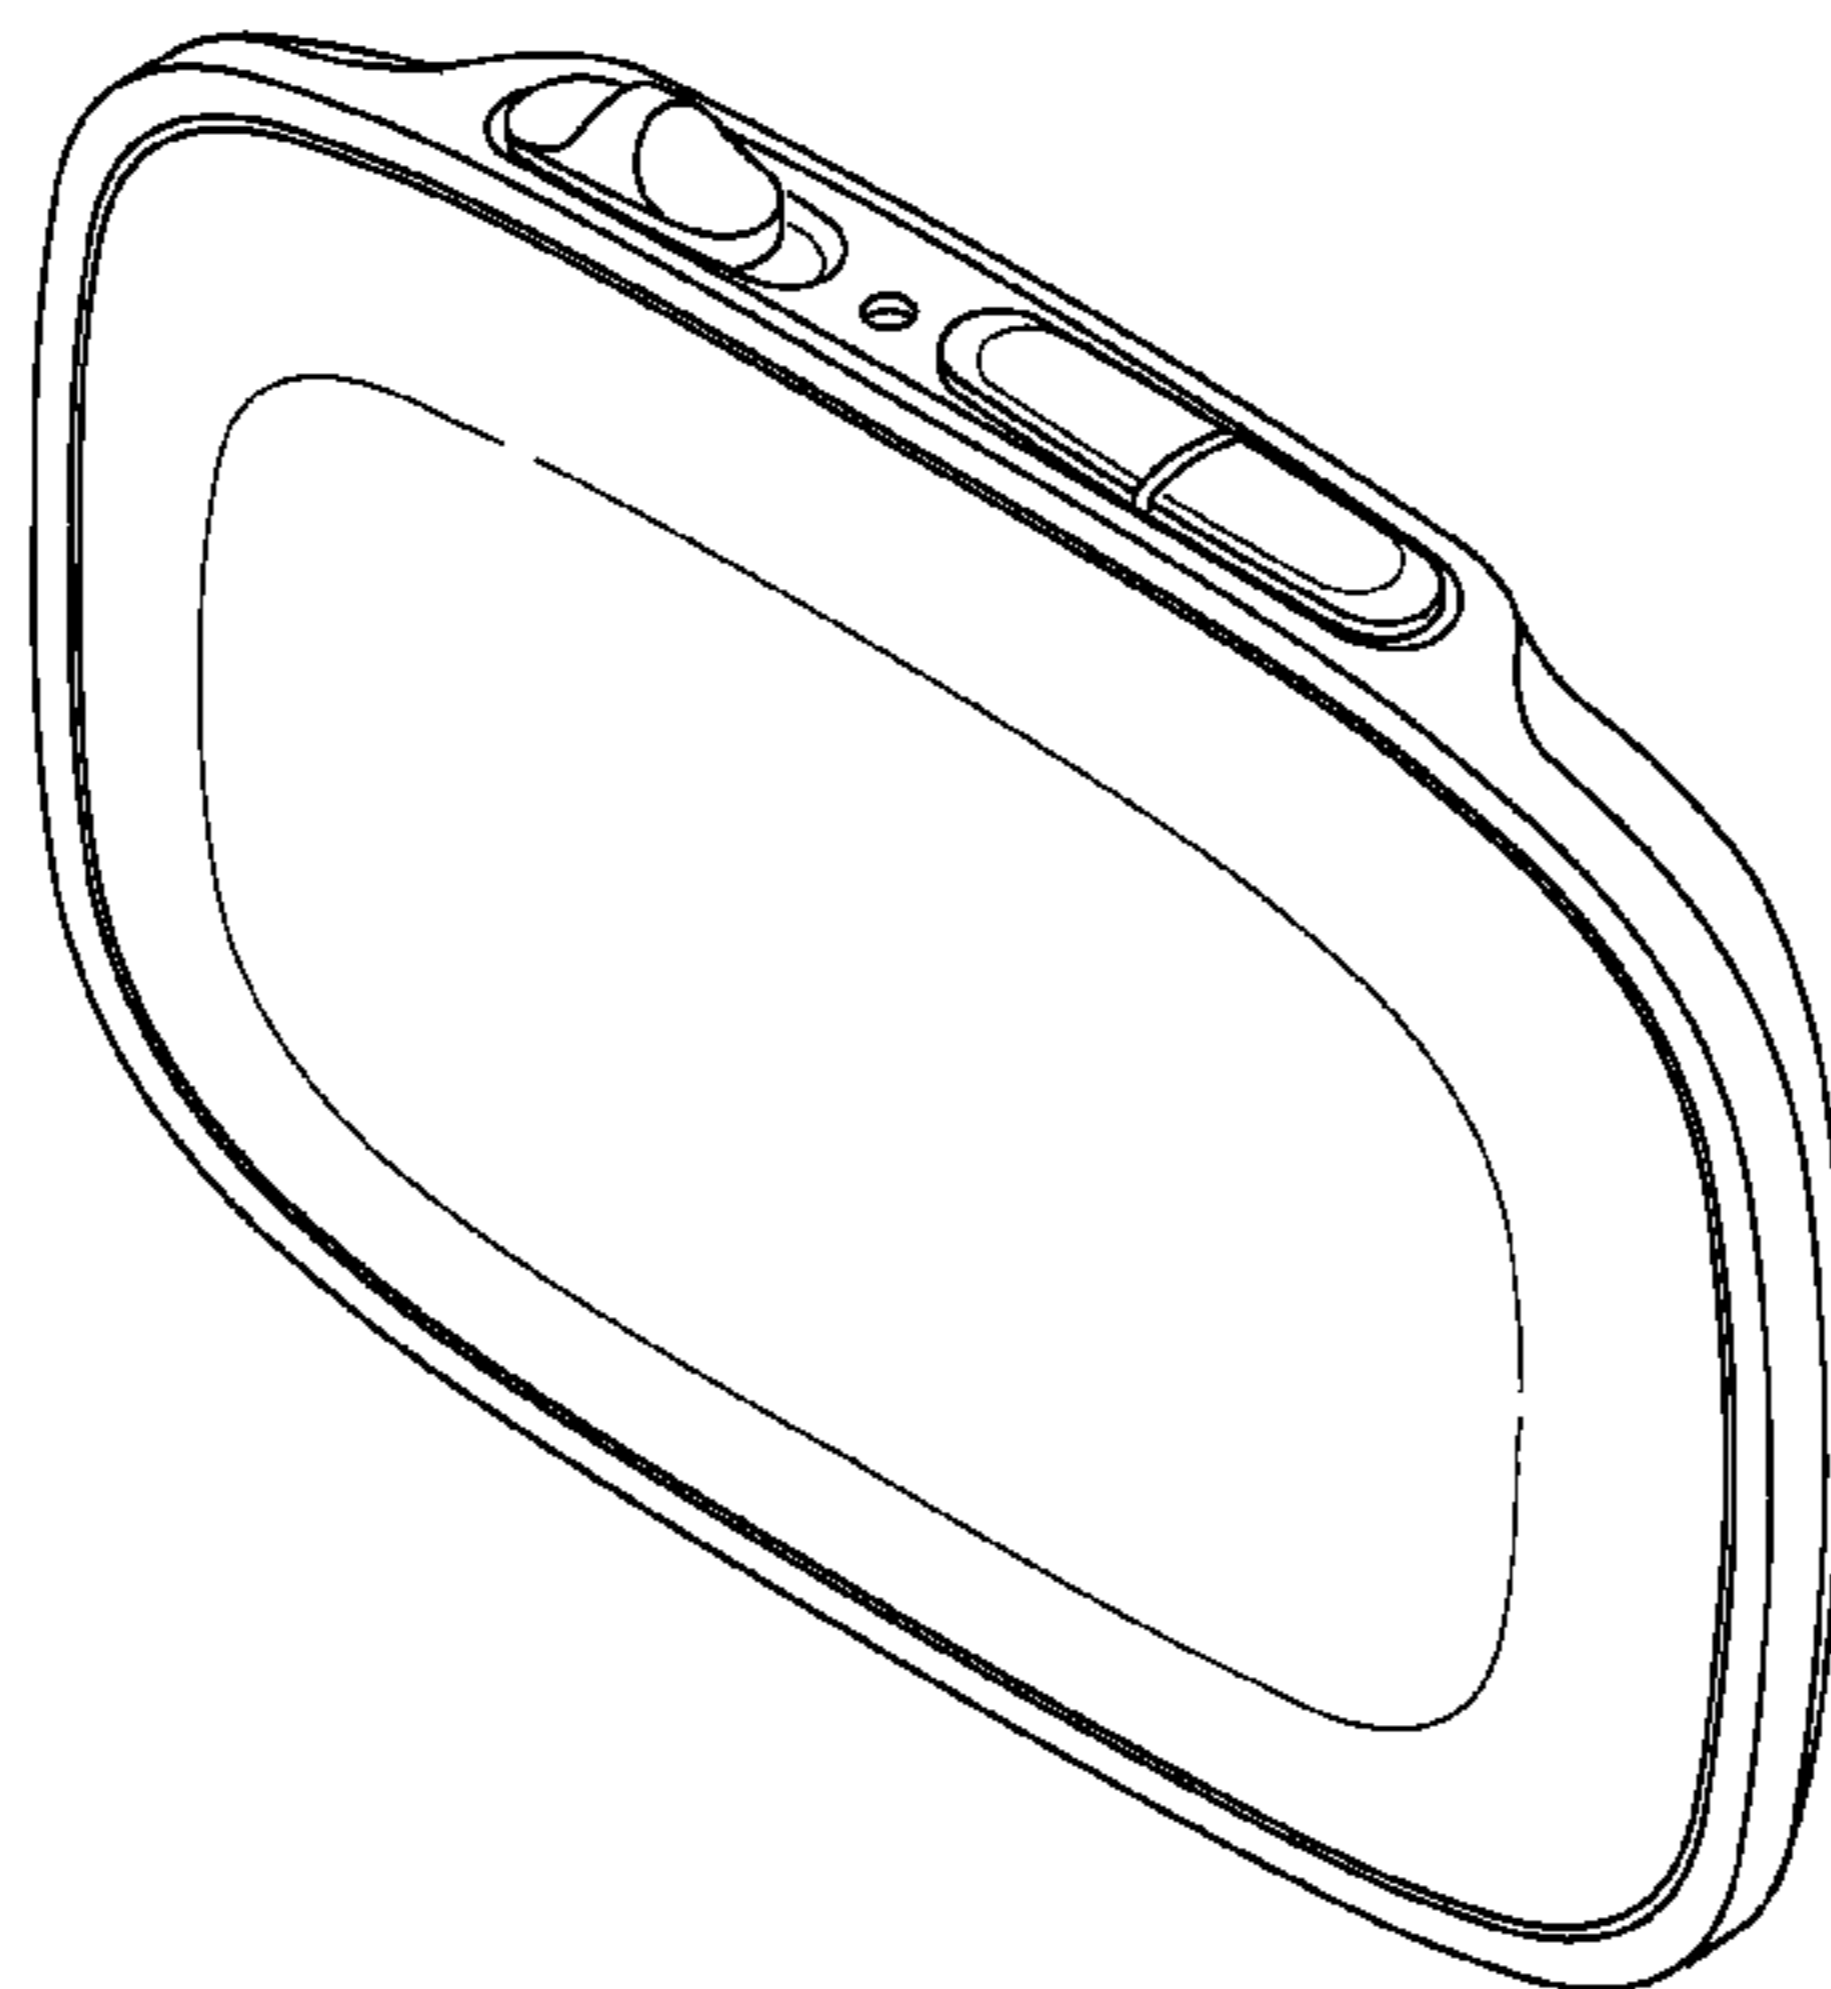


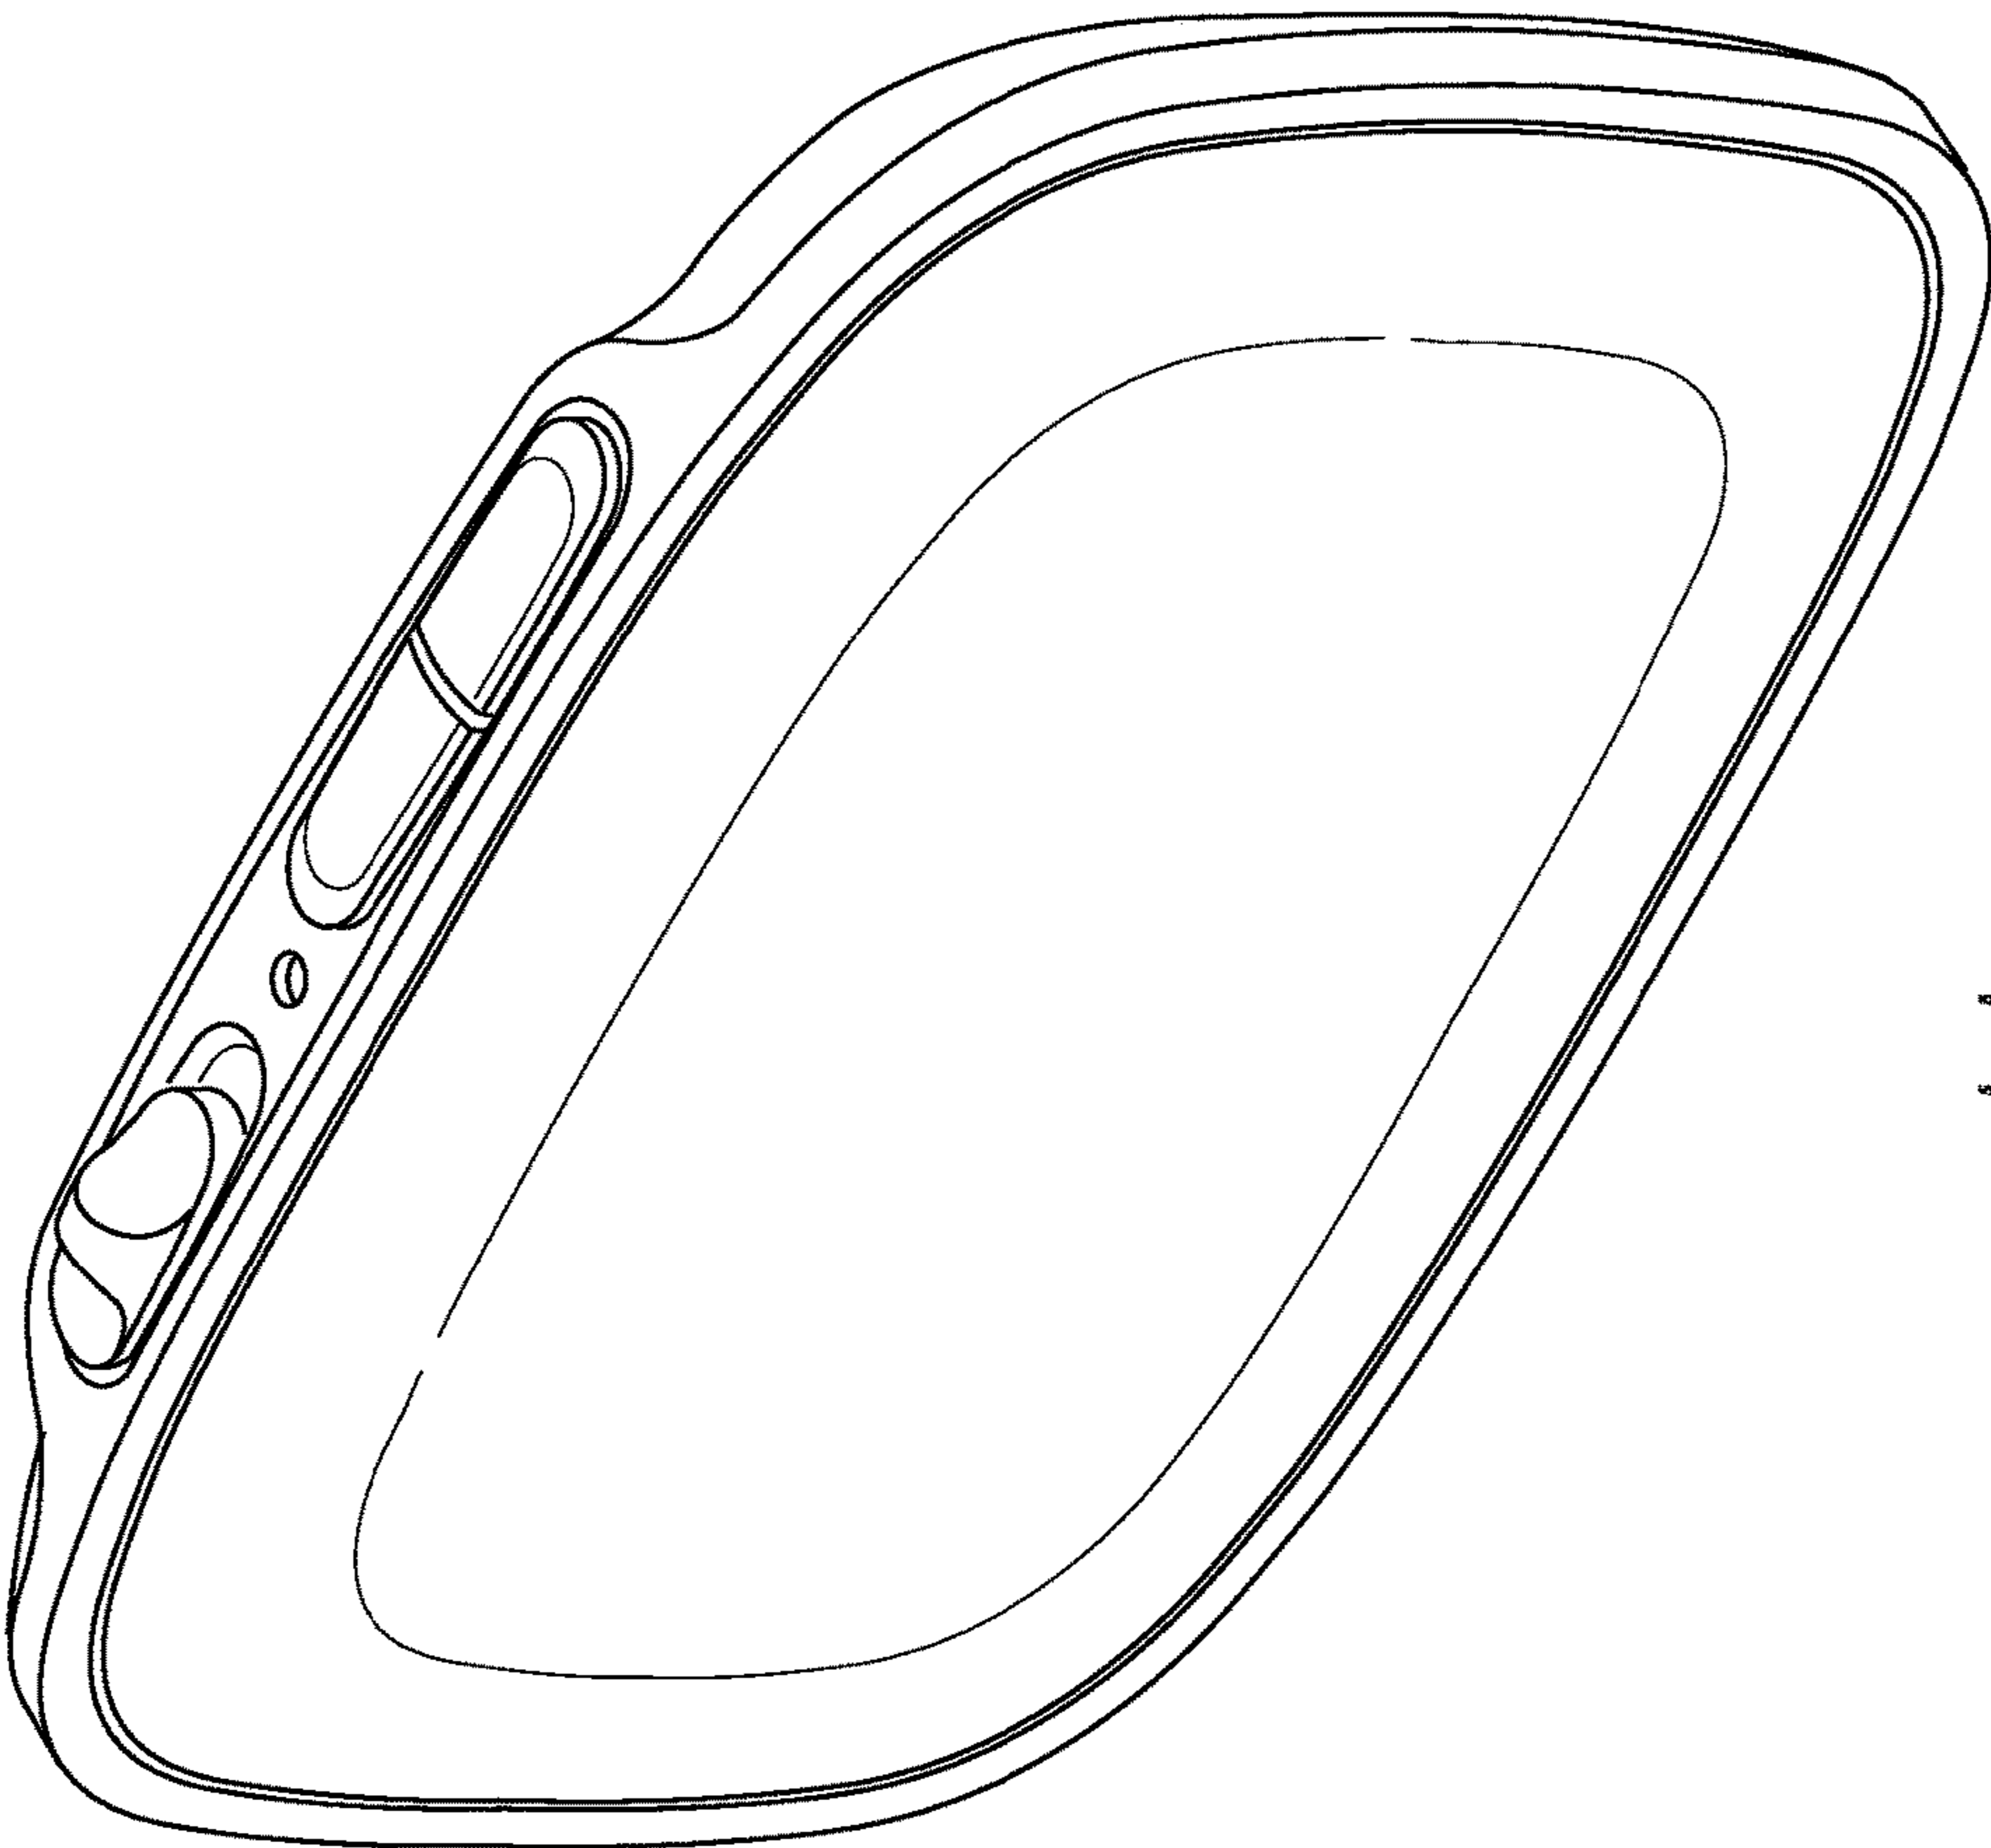

11

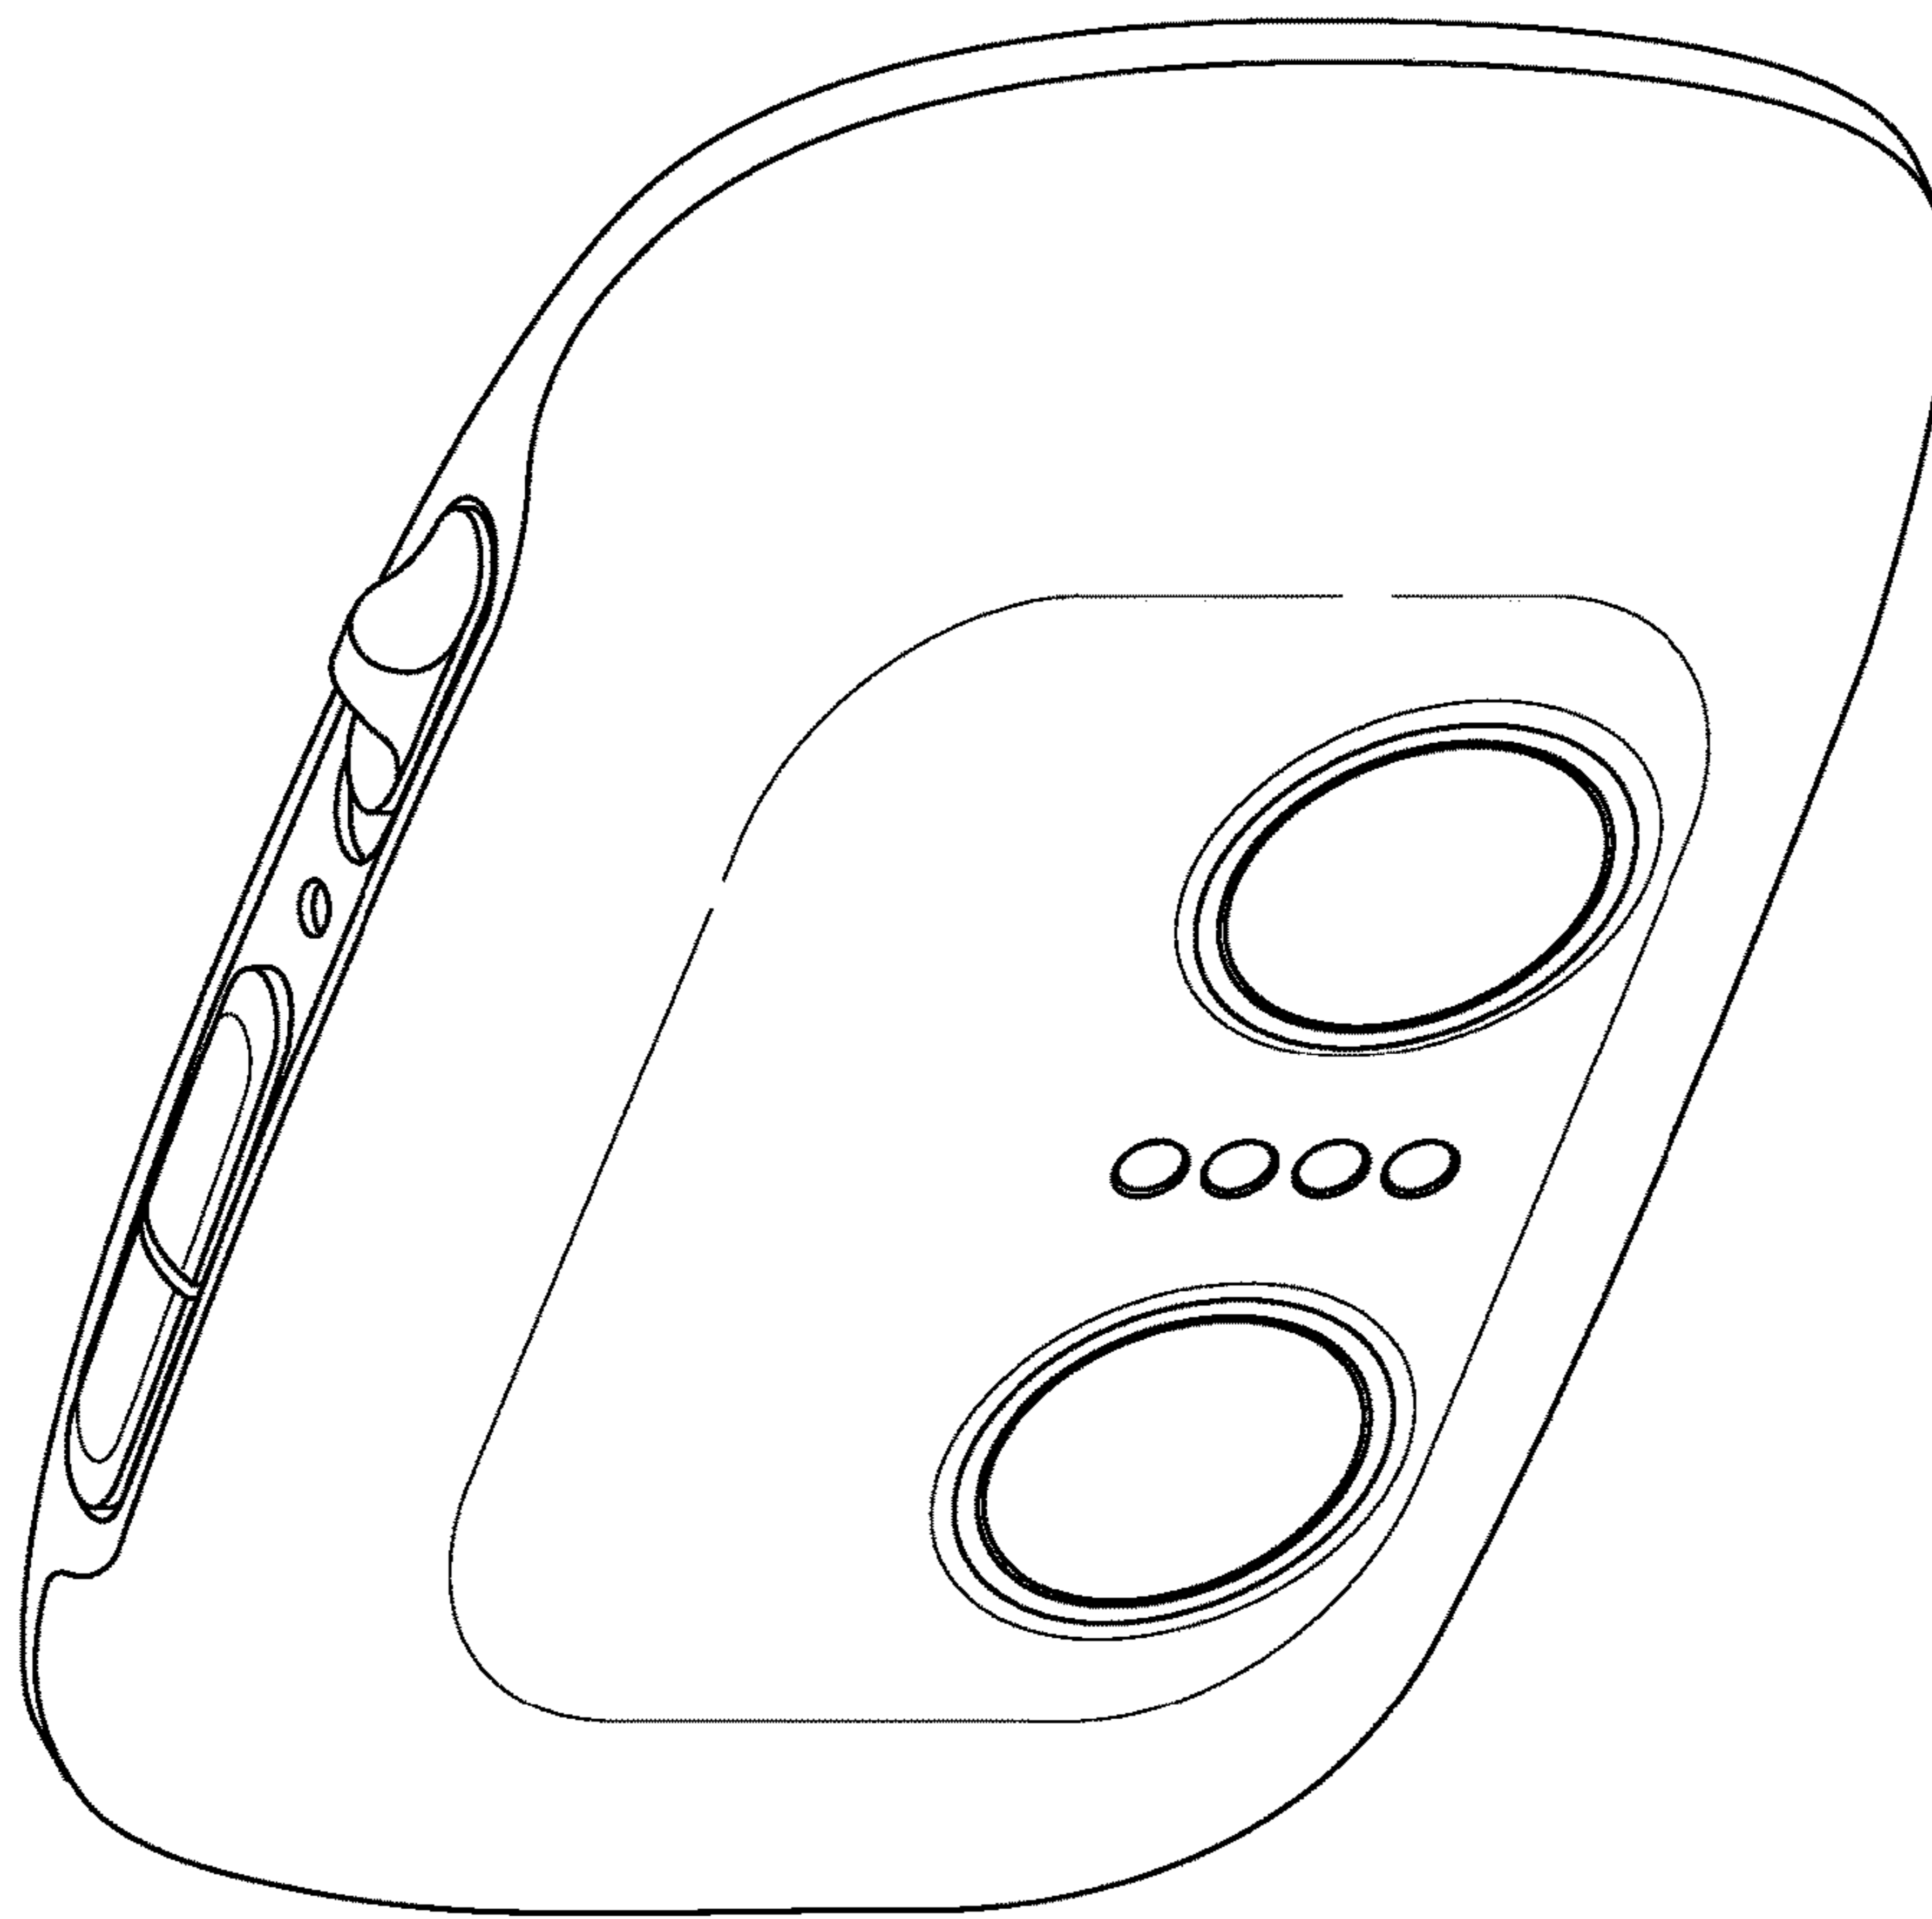


1.2

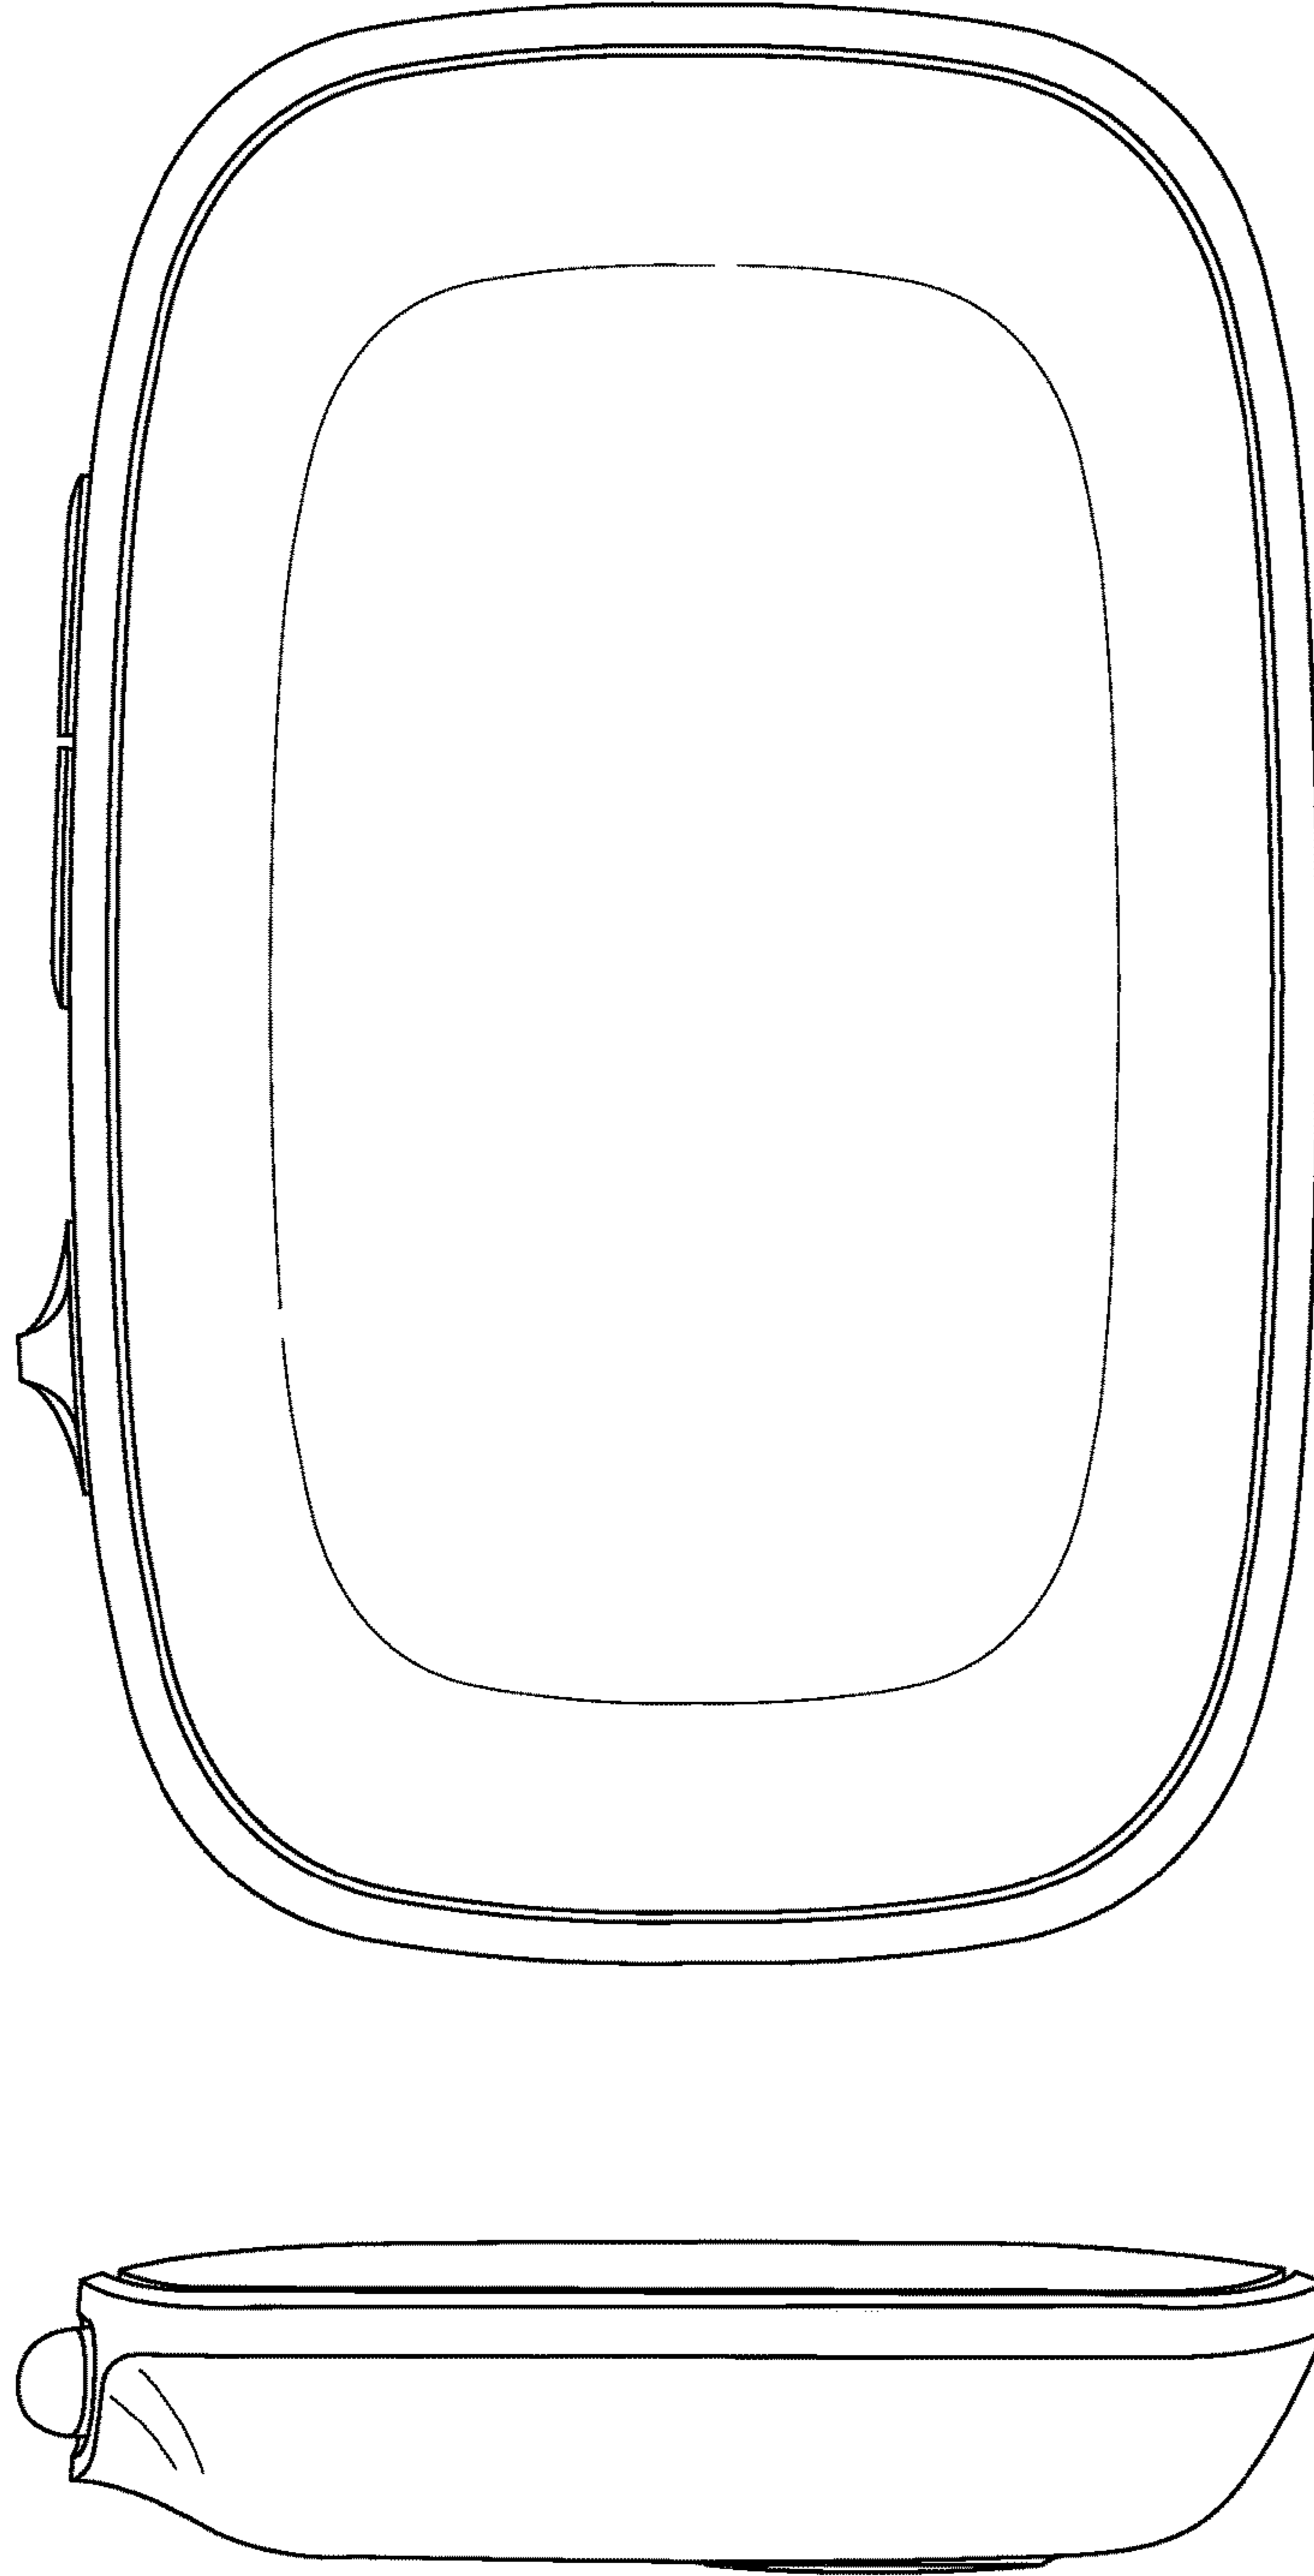


14

13

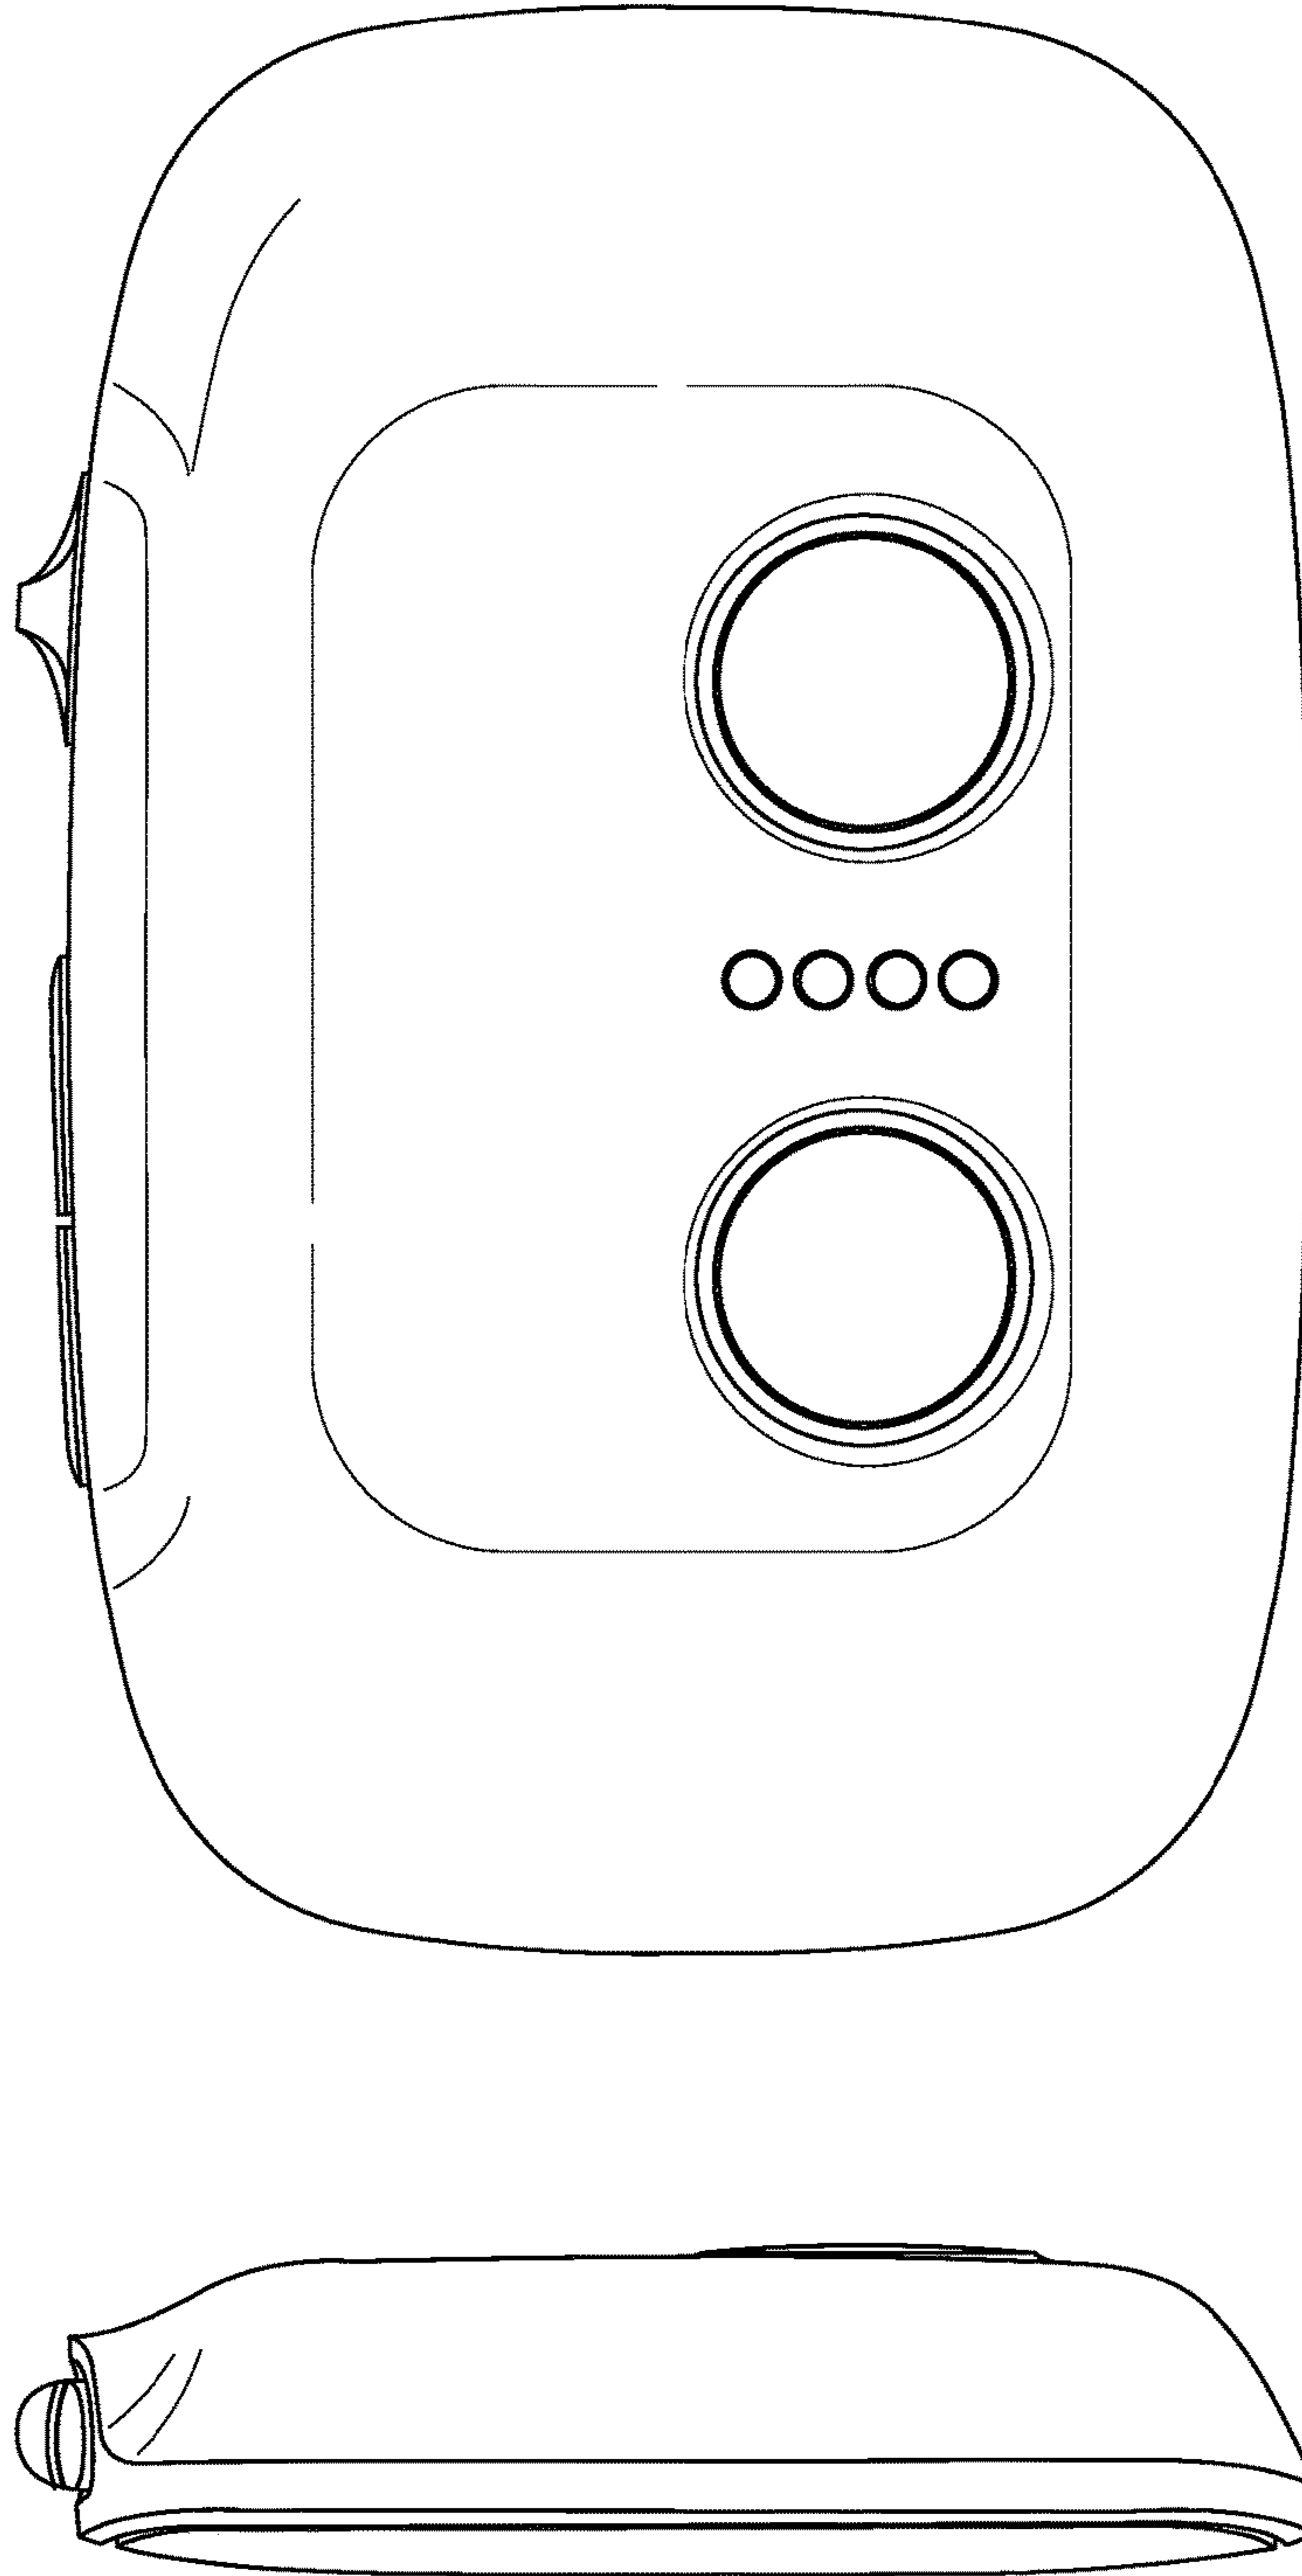


1.6

1.5

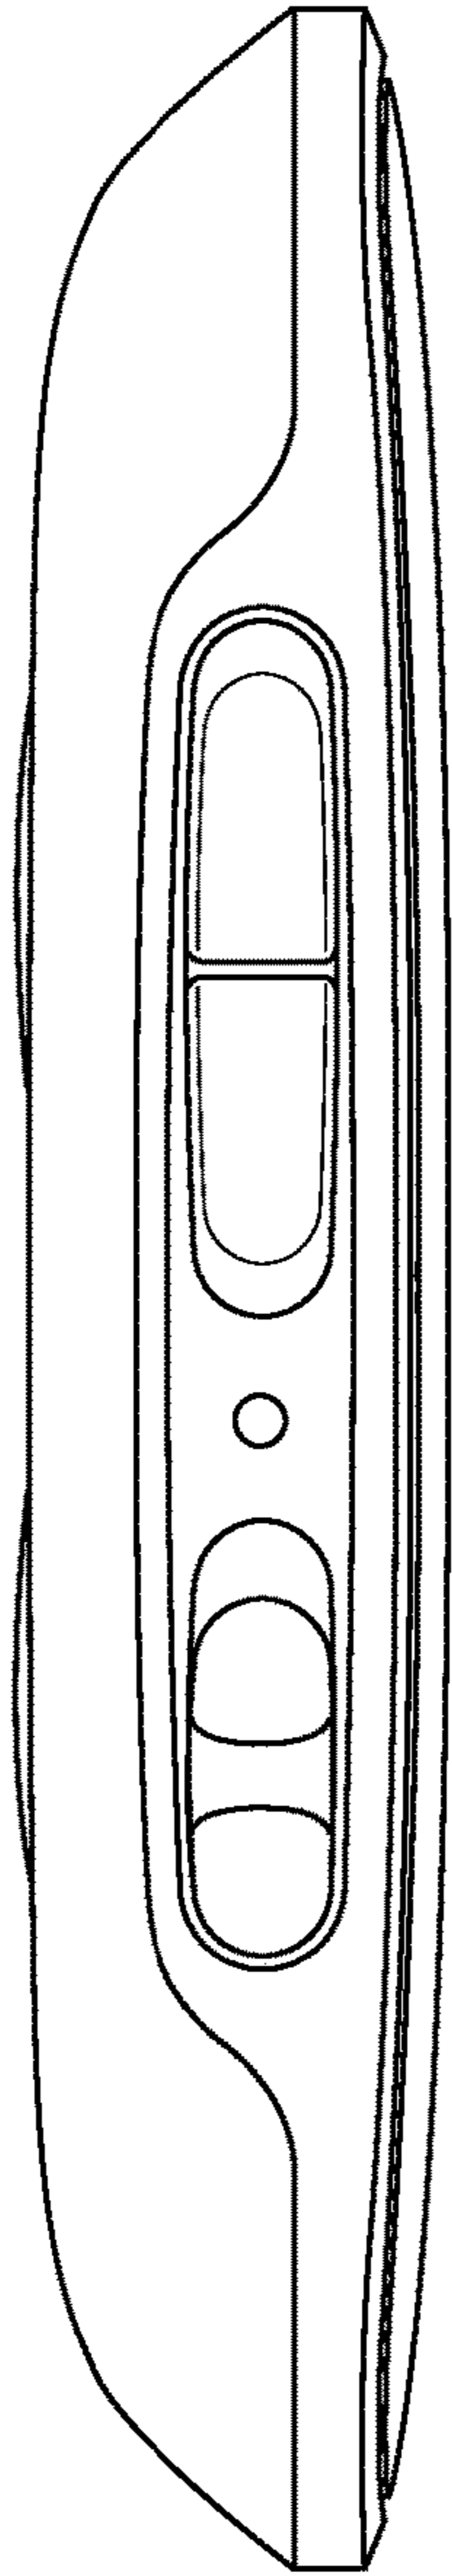

1.7

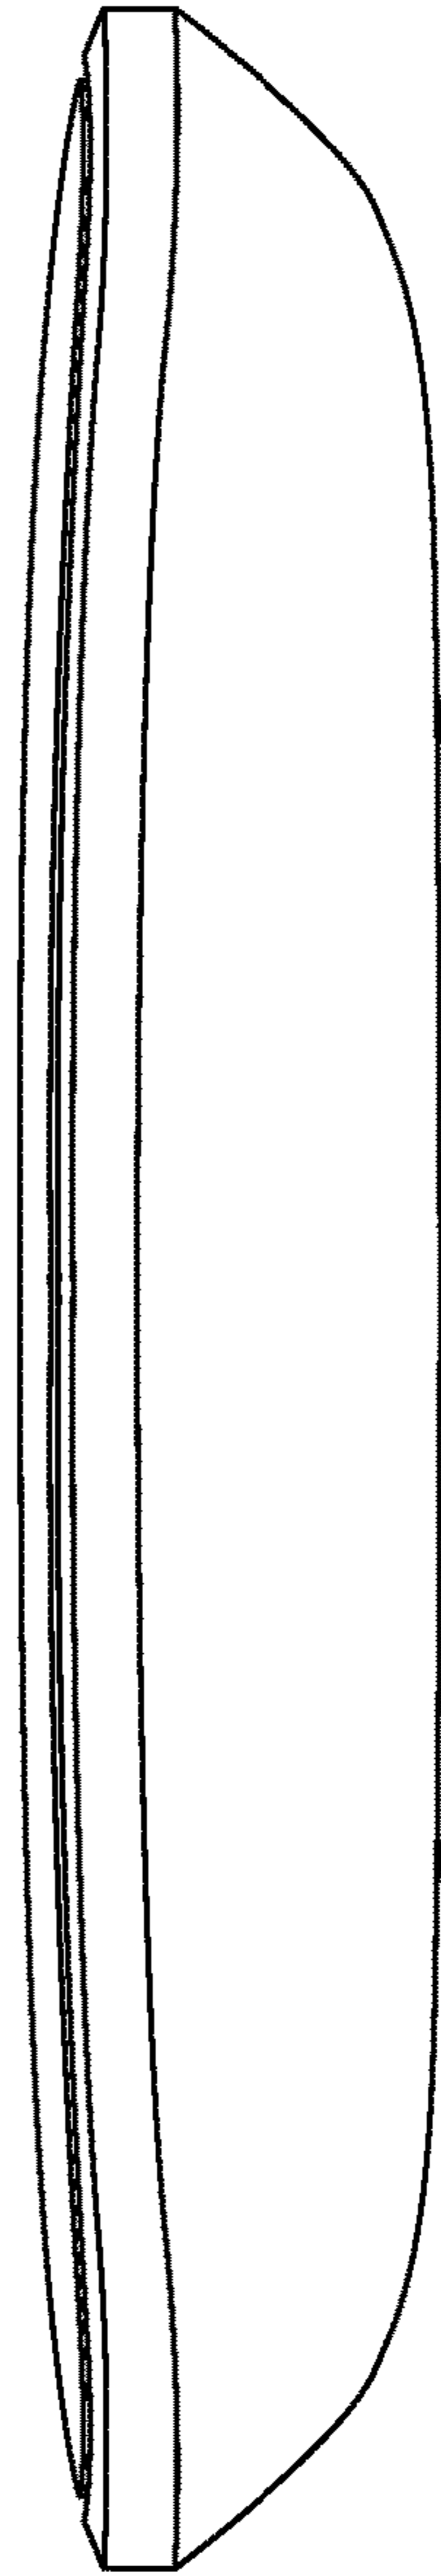

1.8