



US00D852373S

(12) **United States Design Patent**
Ständer

(10) **Patent No.:** **US D852,373 S**
(45) **Date of Patent:** **** Jun. 25, 2019**

(54) **LABORATORY APPARATUS**

(71) Applicant: **SARTORIUS LAB INSTRUMENTS GMBH & CO. KG**, Göttingen (DE)

(72) Inventor: **Malte Ständer**, Heiligenstadt (DE)

(73) Assignee: **SARTORIUS LAB INSTRUMENTS GMBH & CO.**, Göttingen (DE)

(**) Term: **15 Years**

(21) Appl. No.: **29/590,402**

(22) Filed: **Jan. 10, 2017**

(30) **Foreign Application Priority Data**

Jul. 12, 2016 (EM) 003304039

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**

USPC D24/185-186, 170, 158, 216, 232
CPC G01N 2035/00306; G01N 2035/00326;
G01N 2035/00336; G01N 2030/027;
A61B 2017/00973; A61B 2017/00115;
A61B 2017/00199; A61B 2017/00225

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D247,224 S * 2/1978 Pemberton D10/38
5,193,678 A * 3/1993 Janocik A61B 17/06161
206/363
D465,280 S * 11/2002 Huntley D14/489
D687,951 S * 8/2013 Della Torre D24/167
D785,811 S * 5/2017 Watts D24/224
D809,141 S * 1/2018 Adams D24/158

FOREIGN PATENT DOCUMENTS

DE 10100984 B4 11/2009
EP 1092473 A2 4/2001
EP 2759816 B1 1/2016

OTHER PUBLICATIONS

Photo of a SpeedCal, System for gravimetric testing of multichannel pipettes, accessed Jan. 13, 2015.

(Continued)

Primary Examiner — Anhdao Doan

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — McNees Wallace & Nurick LLC

(57) **CLAIM**

The ornamental design for a laboratory apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a top-front-left perspective view of a laboratory apparatus, showing the design;

FIG. 2 is a bottom view of the laboratory apparatus of FIG. 1;

FIG. 3 is a rear view of the laboratory apparatus of FIG. 1;

FIG. 4 is a right view of the laboratory apparatus of FIG. 1;

FIG. 5 is a front view of the laboratory apparatus of FIG. 1;


FIG. 6 is a left view of the laboratory apparatus of FIG. 1;

and,

FIG. 7 is a top view of the laboratory apparatus of FIG. 1.

The broken lines in the drawings and the surfaces within broken lines represent portions of the laboratory apparatus that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

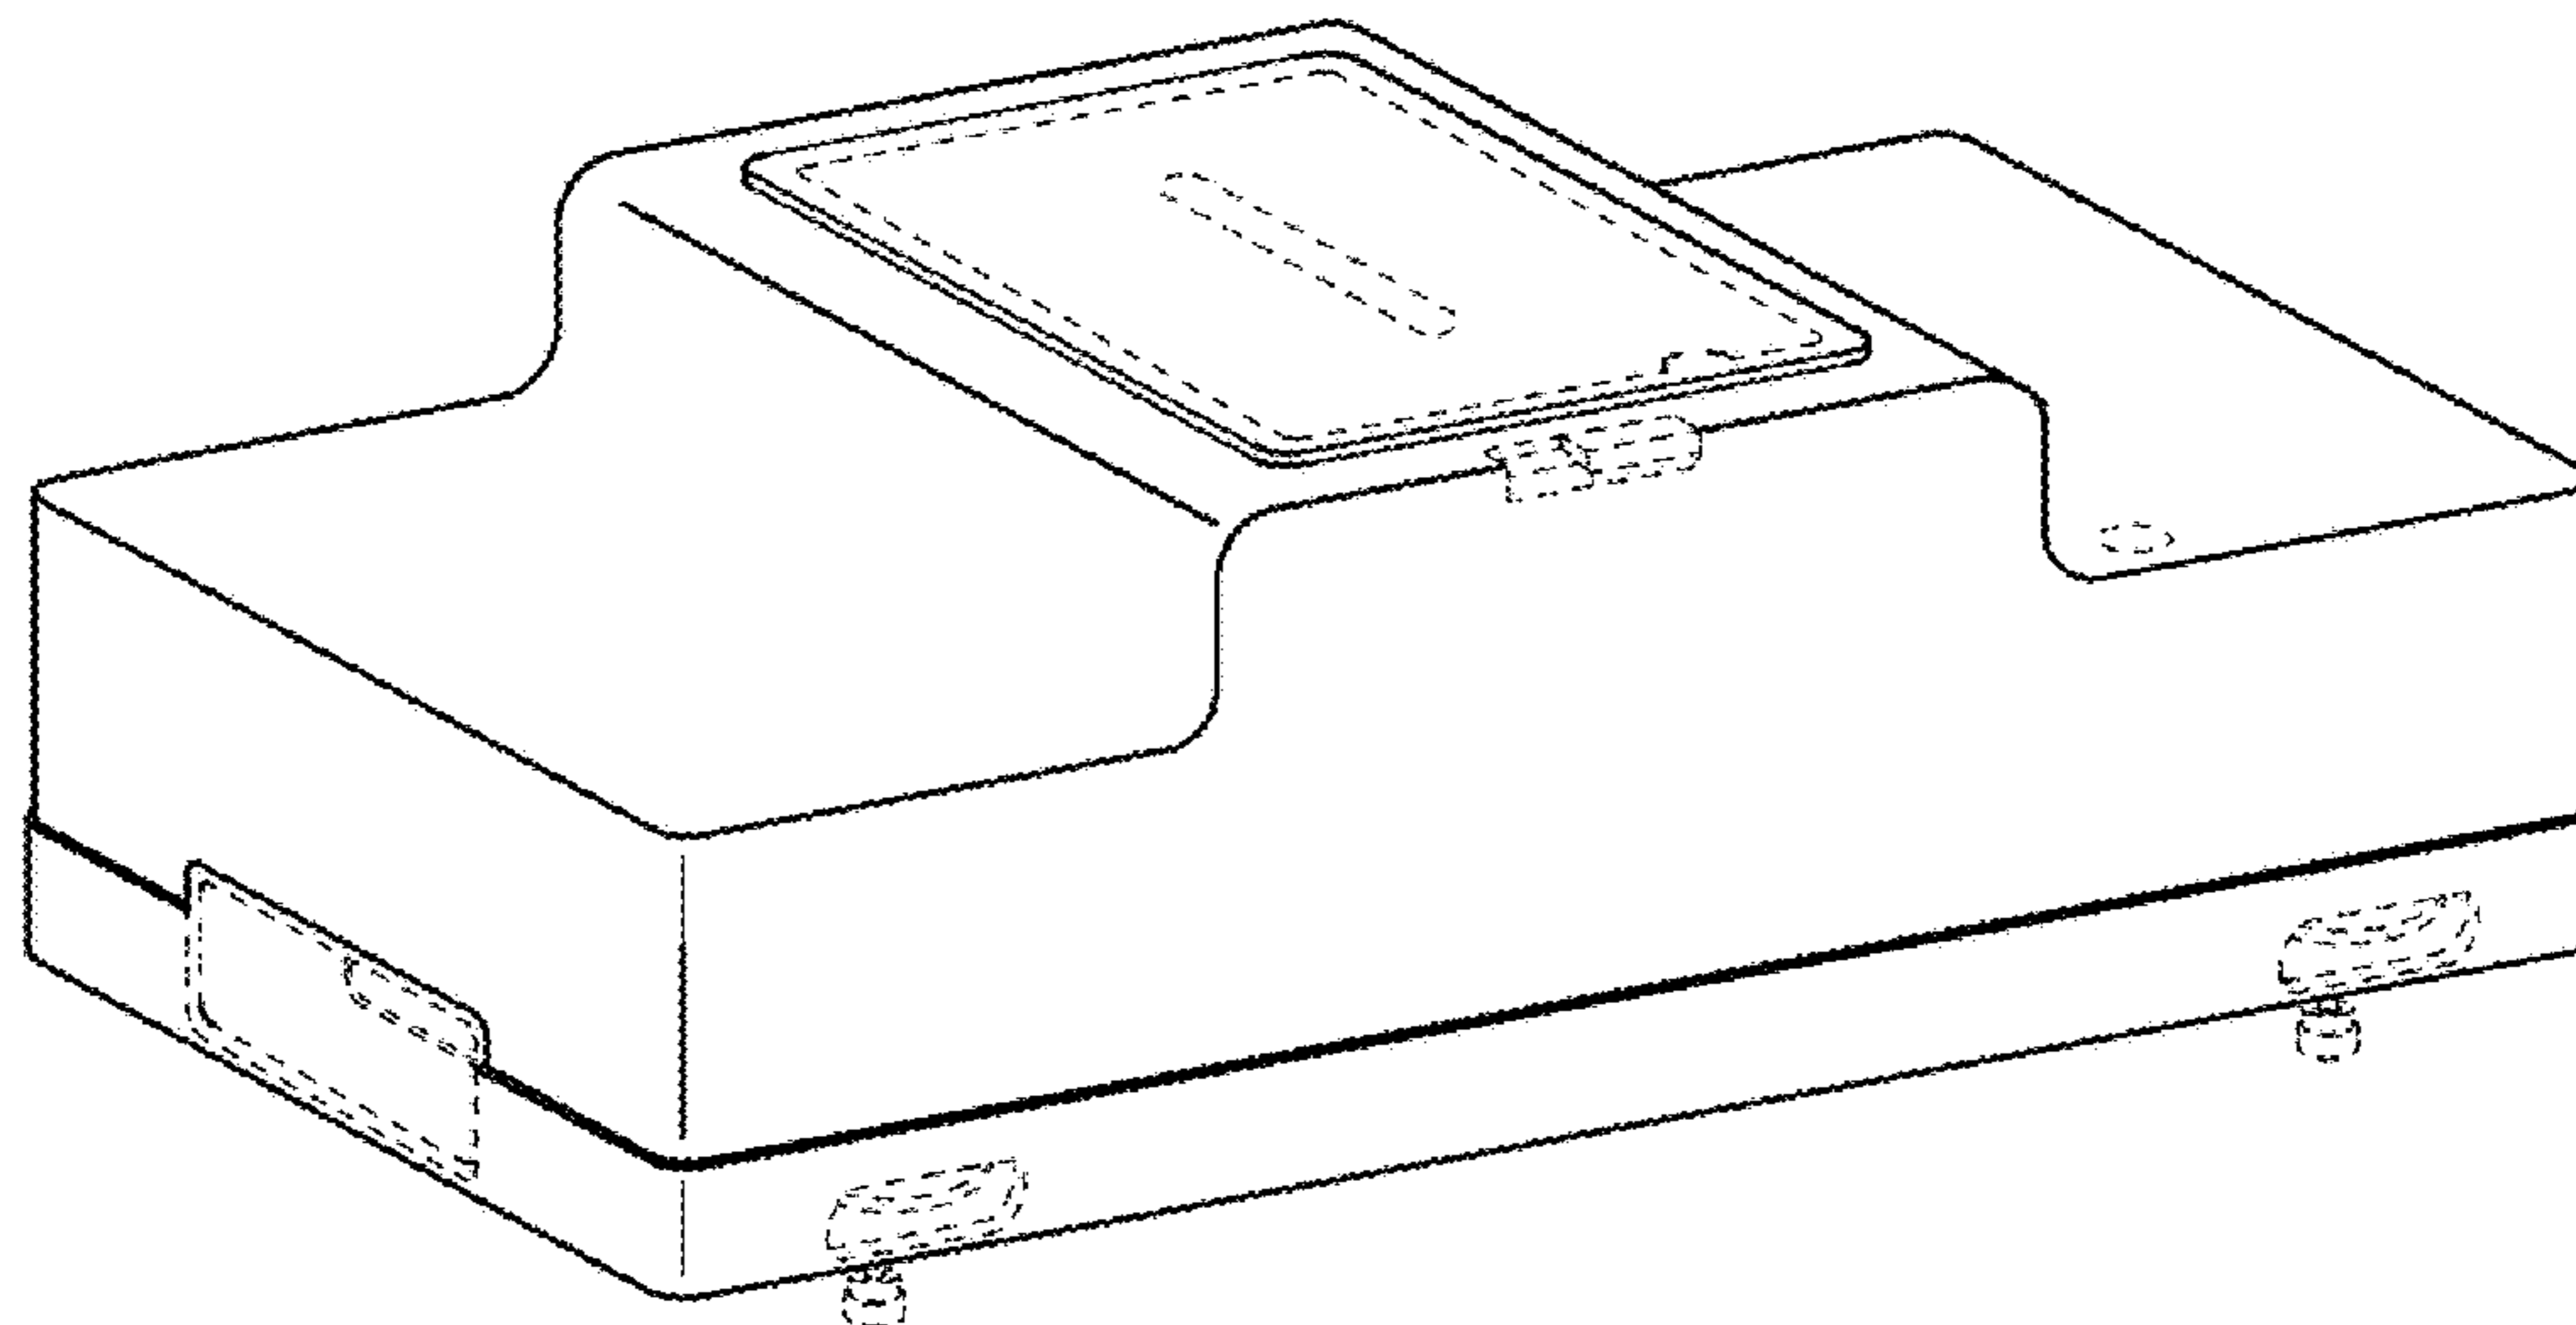

(56)

References Cited

OTHER PUBLICATIONS

Photo of a laboratory apparatus of Mettler-Toledo from the Internet, <http://www.directindustry.de/prod/mettler-toledo-schweiz-gmbh/product-5705-875583.html>, posted online Jun. 22, 2015.

Photo of SpeedCal Mobile, Multi-channel Pipette Calibration Balance, accessed Jan. 13, 2015.

Mettler-Toledo AG, Laboratory & Weighing Technologies, Multi-channel Pipettes Calibration System, Nov. 2013, www.mt.com, Switzerland.

Mettler-Toledo AG, Laboratory Catalog for Improved Customer Processes, Nov. 2010, www.mt.com, Switzerland.

* cited by examiner

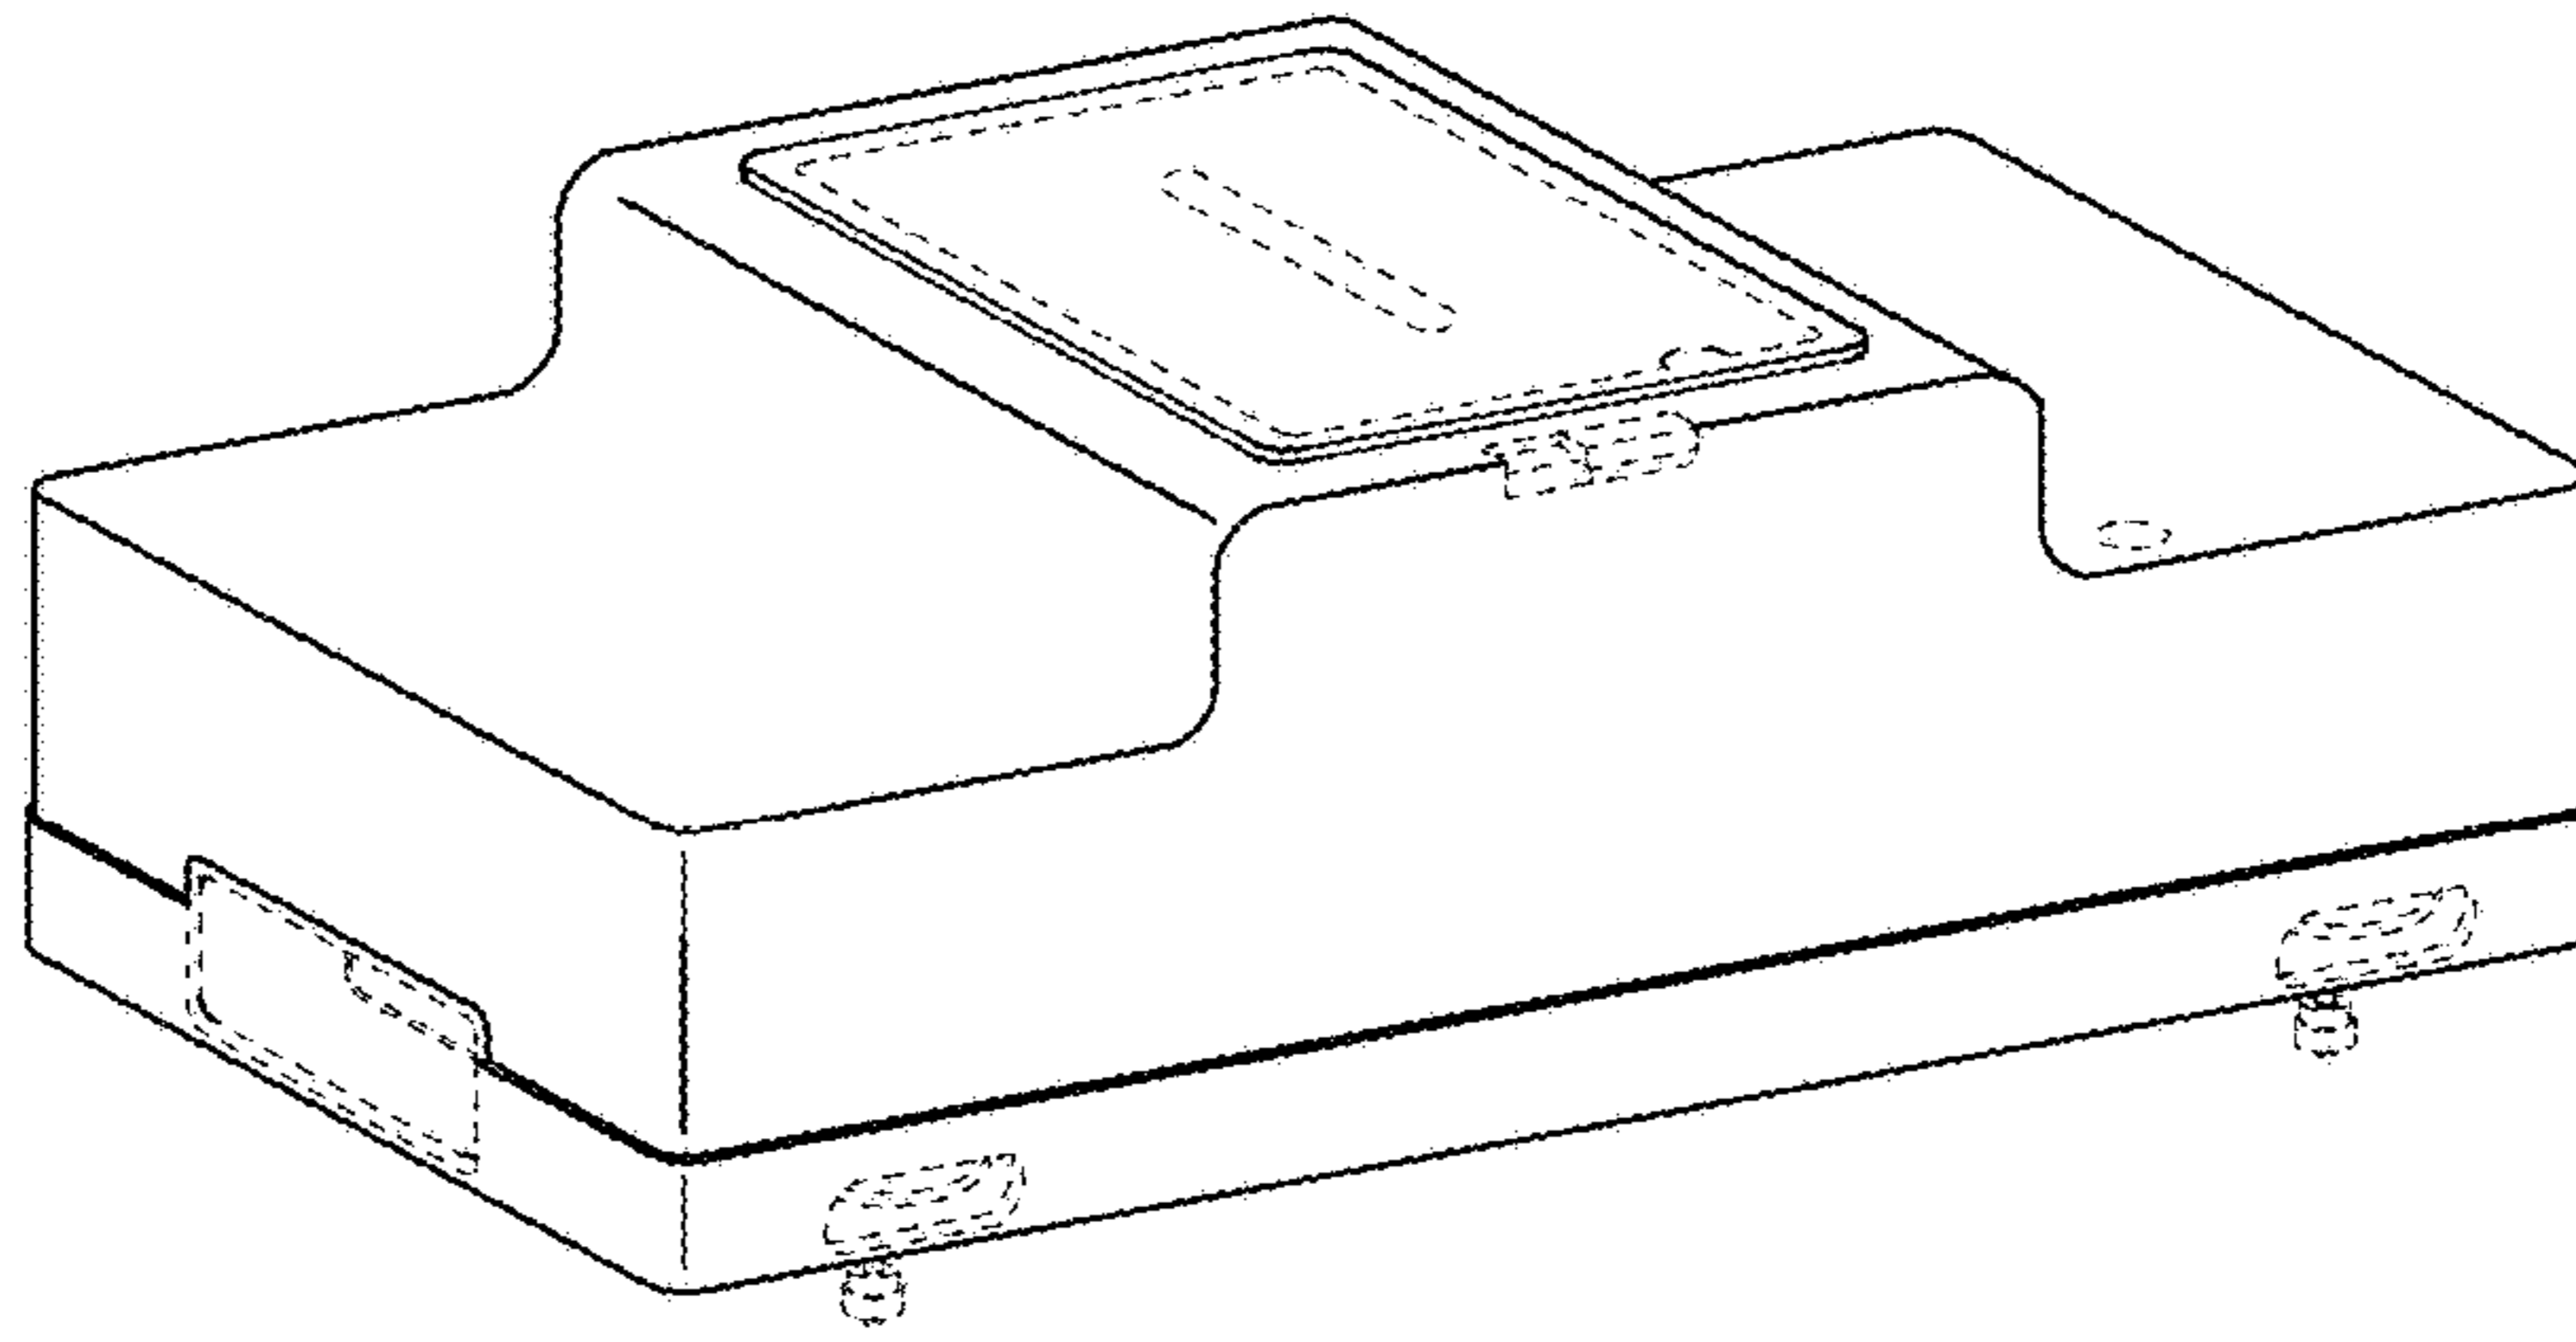


FIG. 1

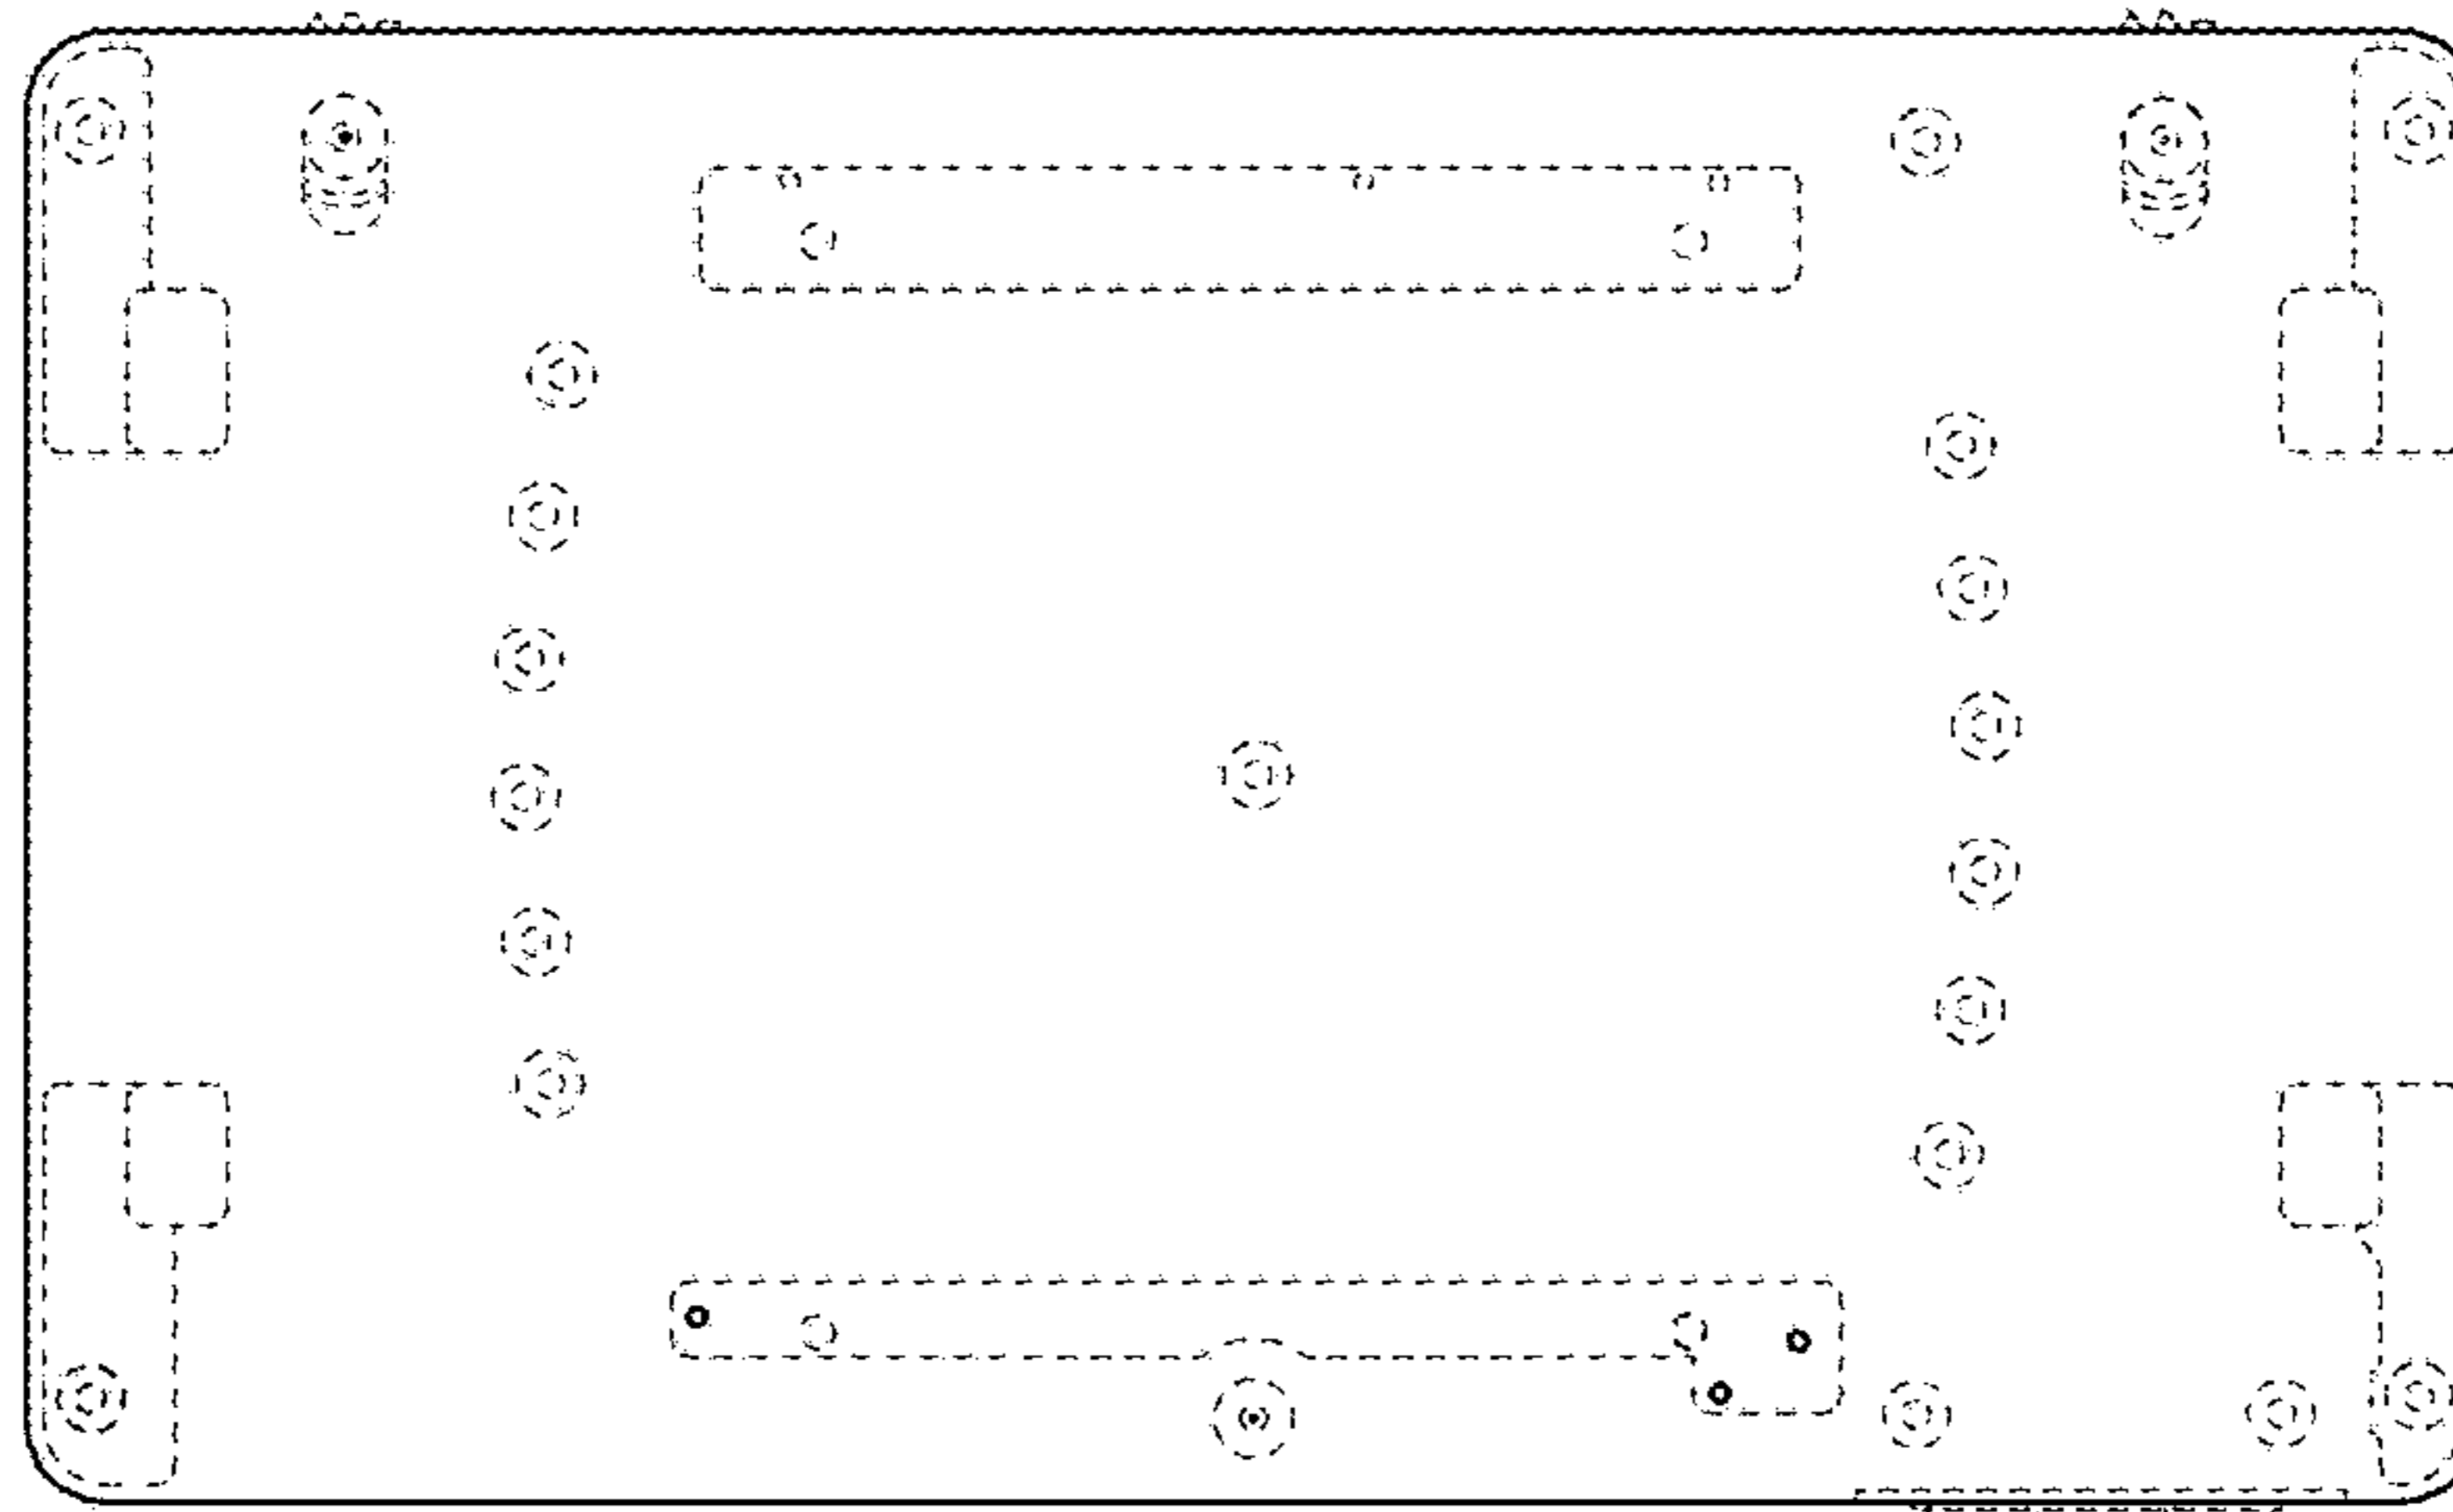


FIG. 2

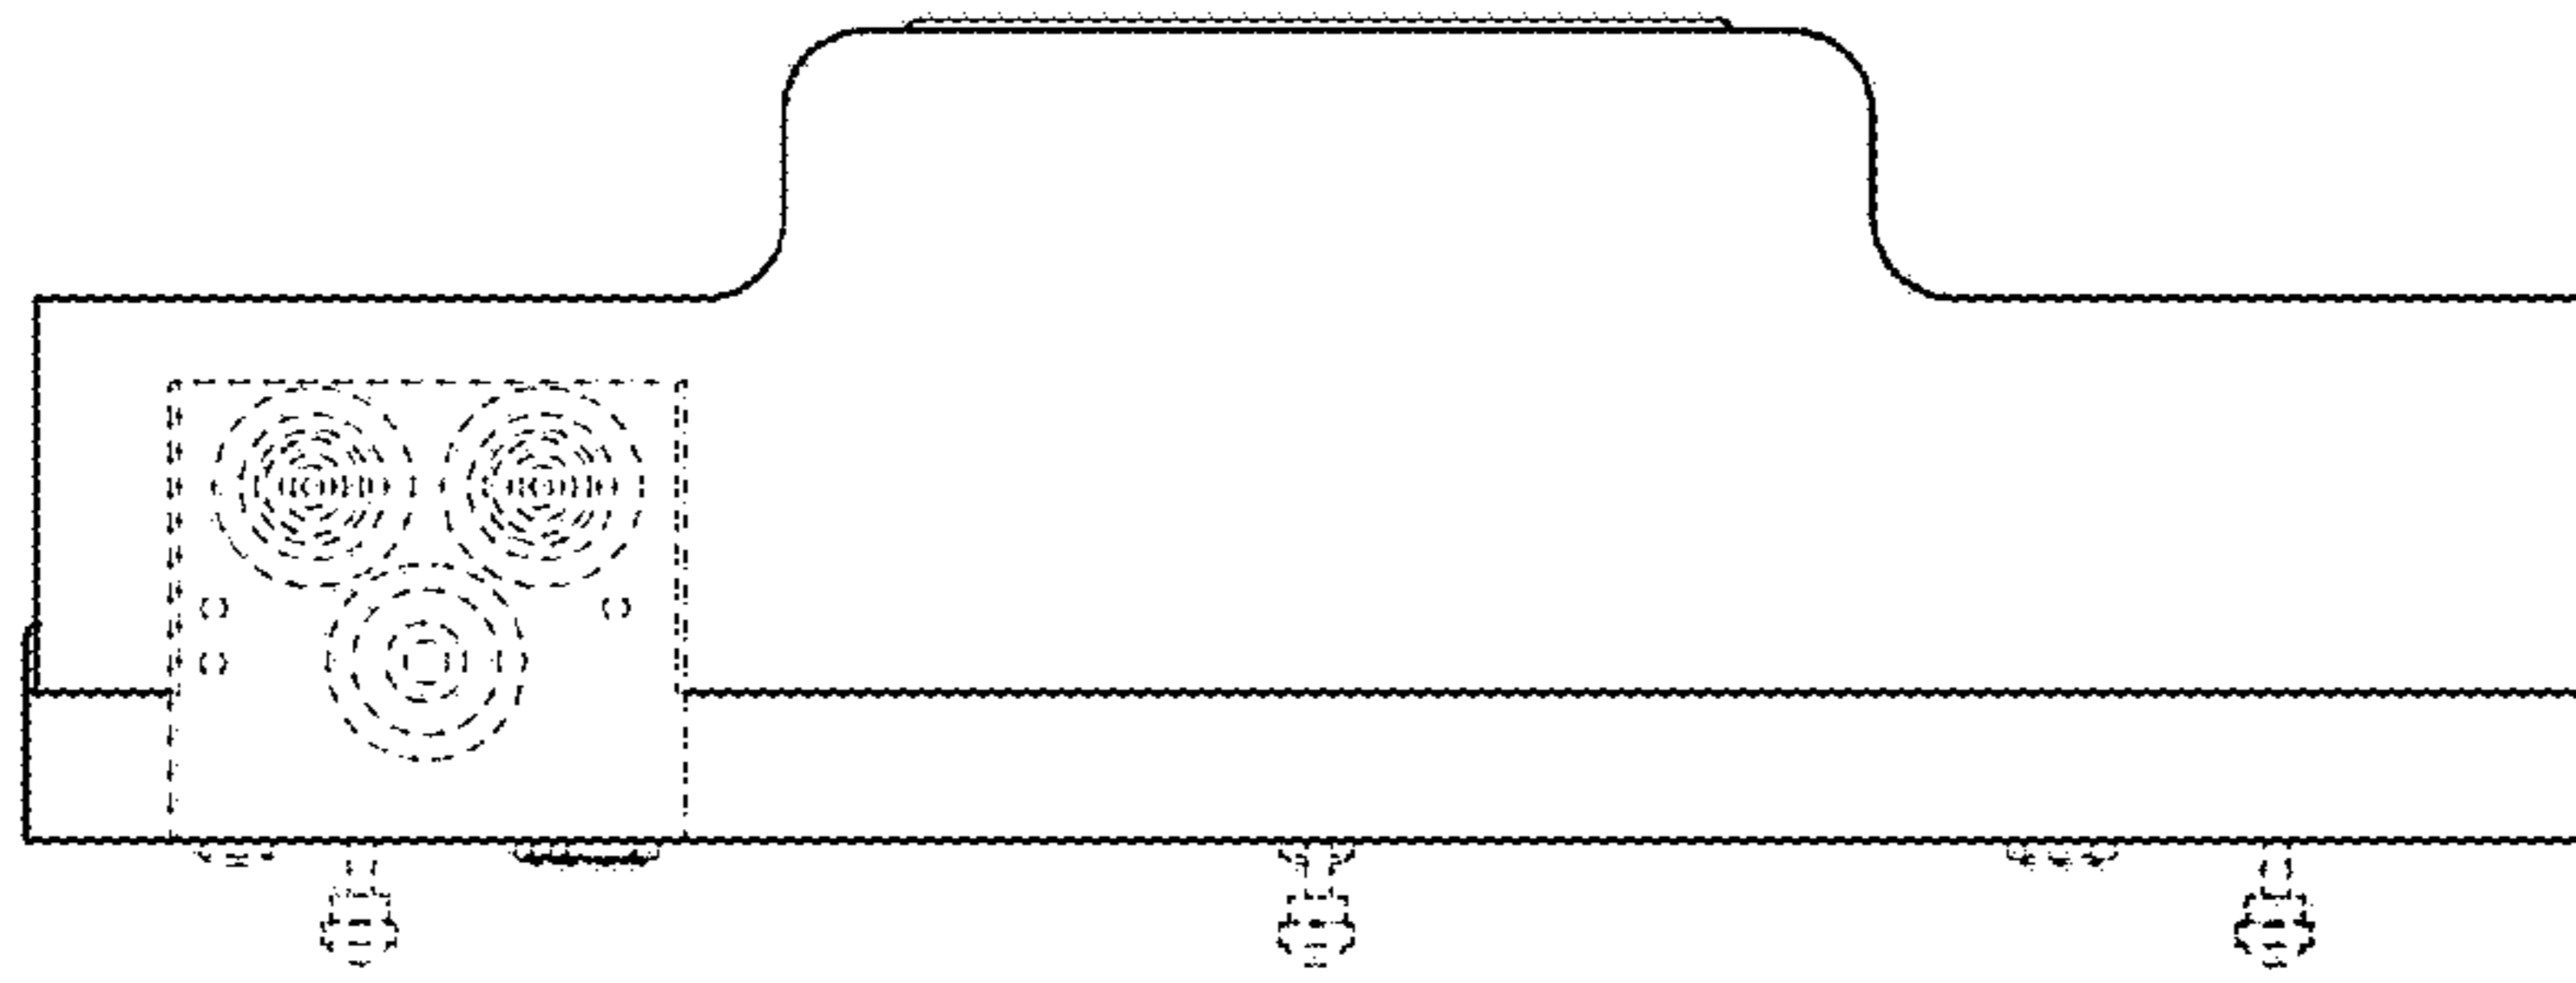


FIG. 3

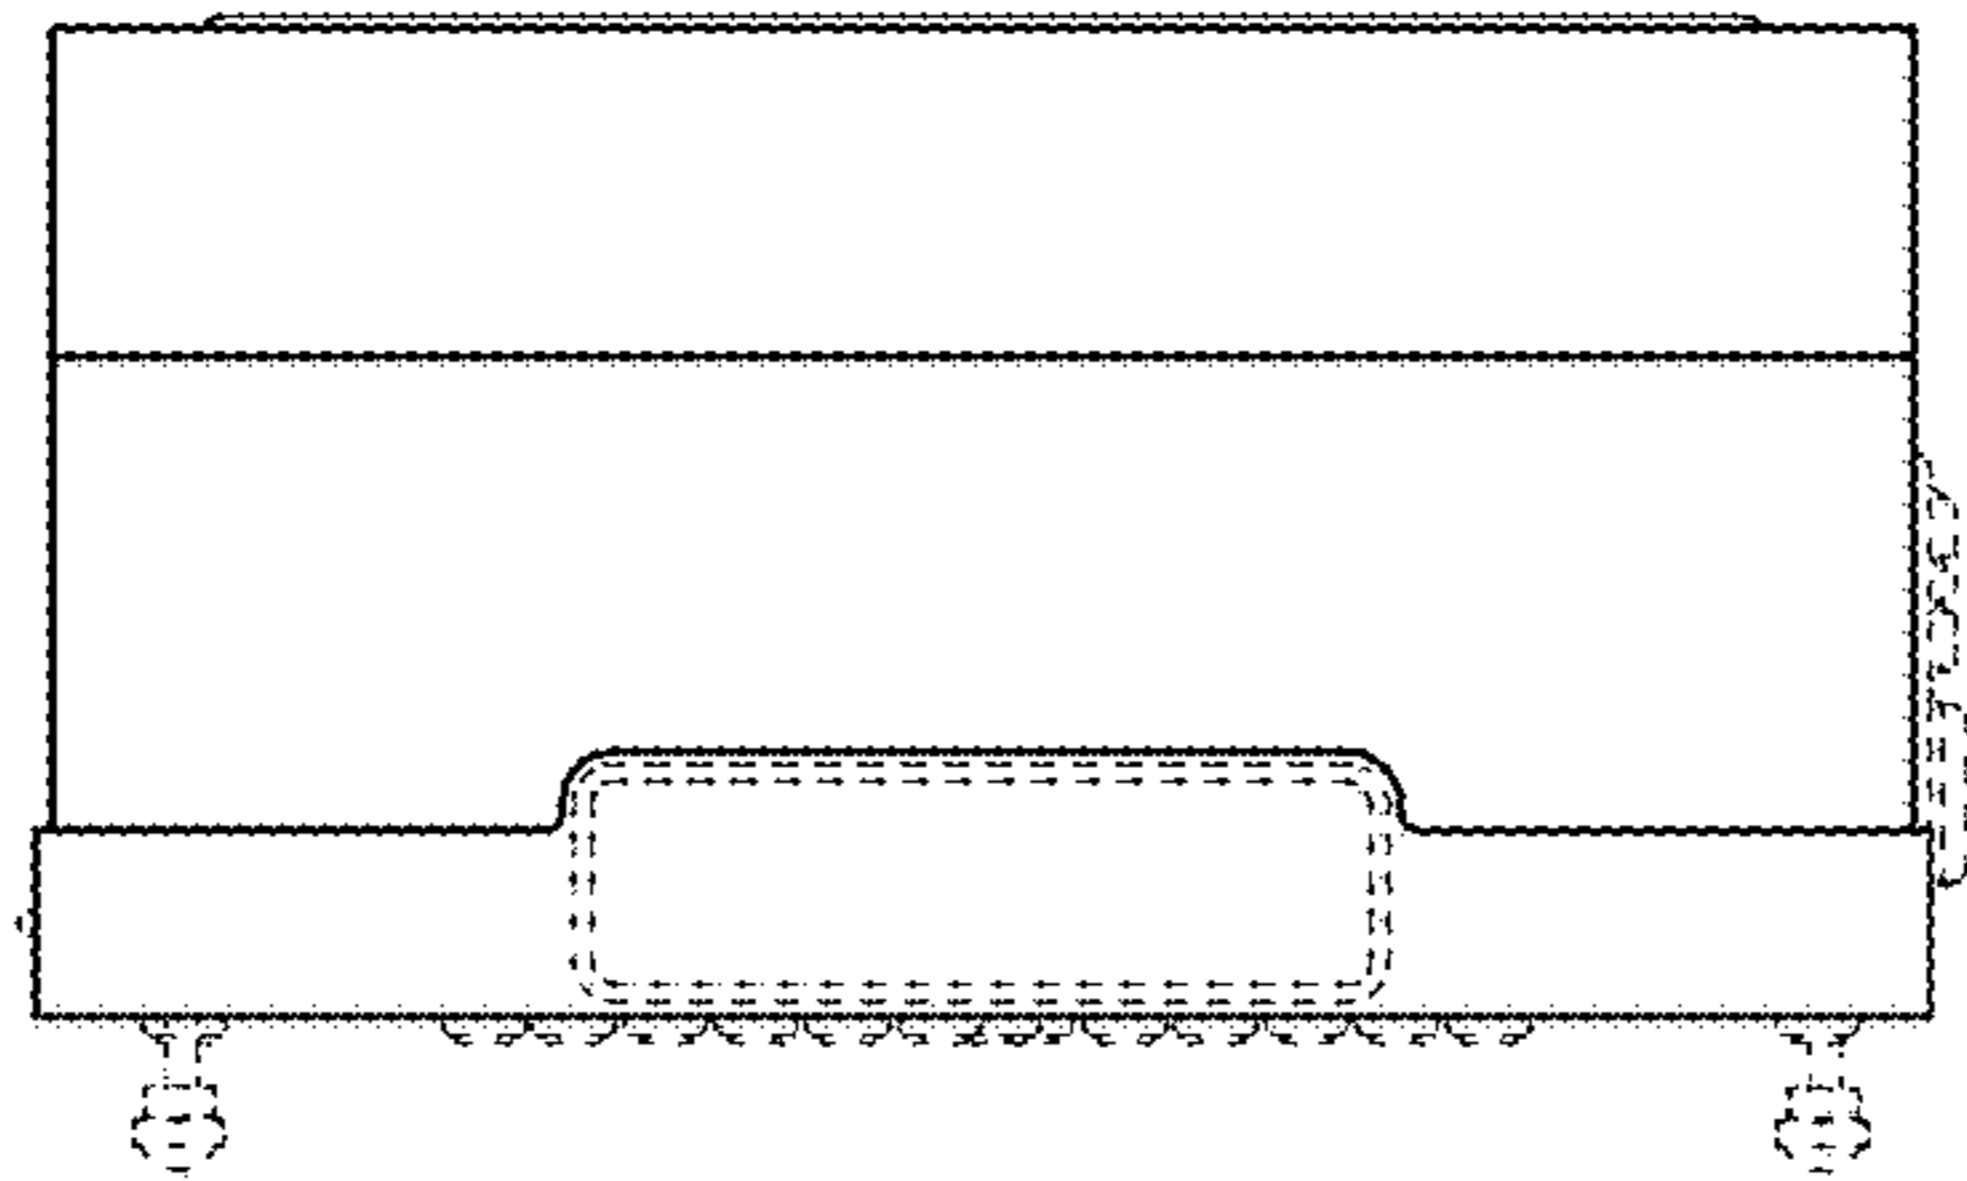


FIG. 4

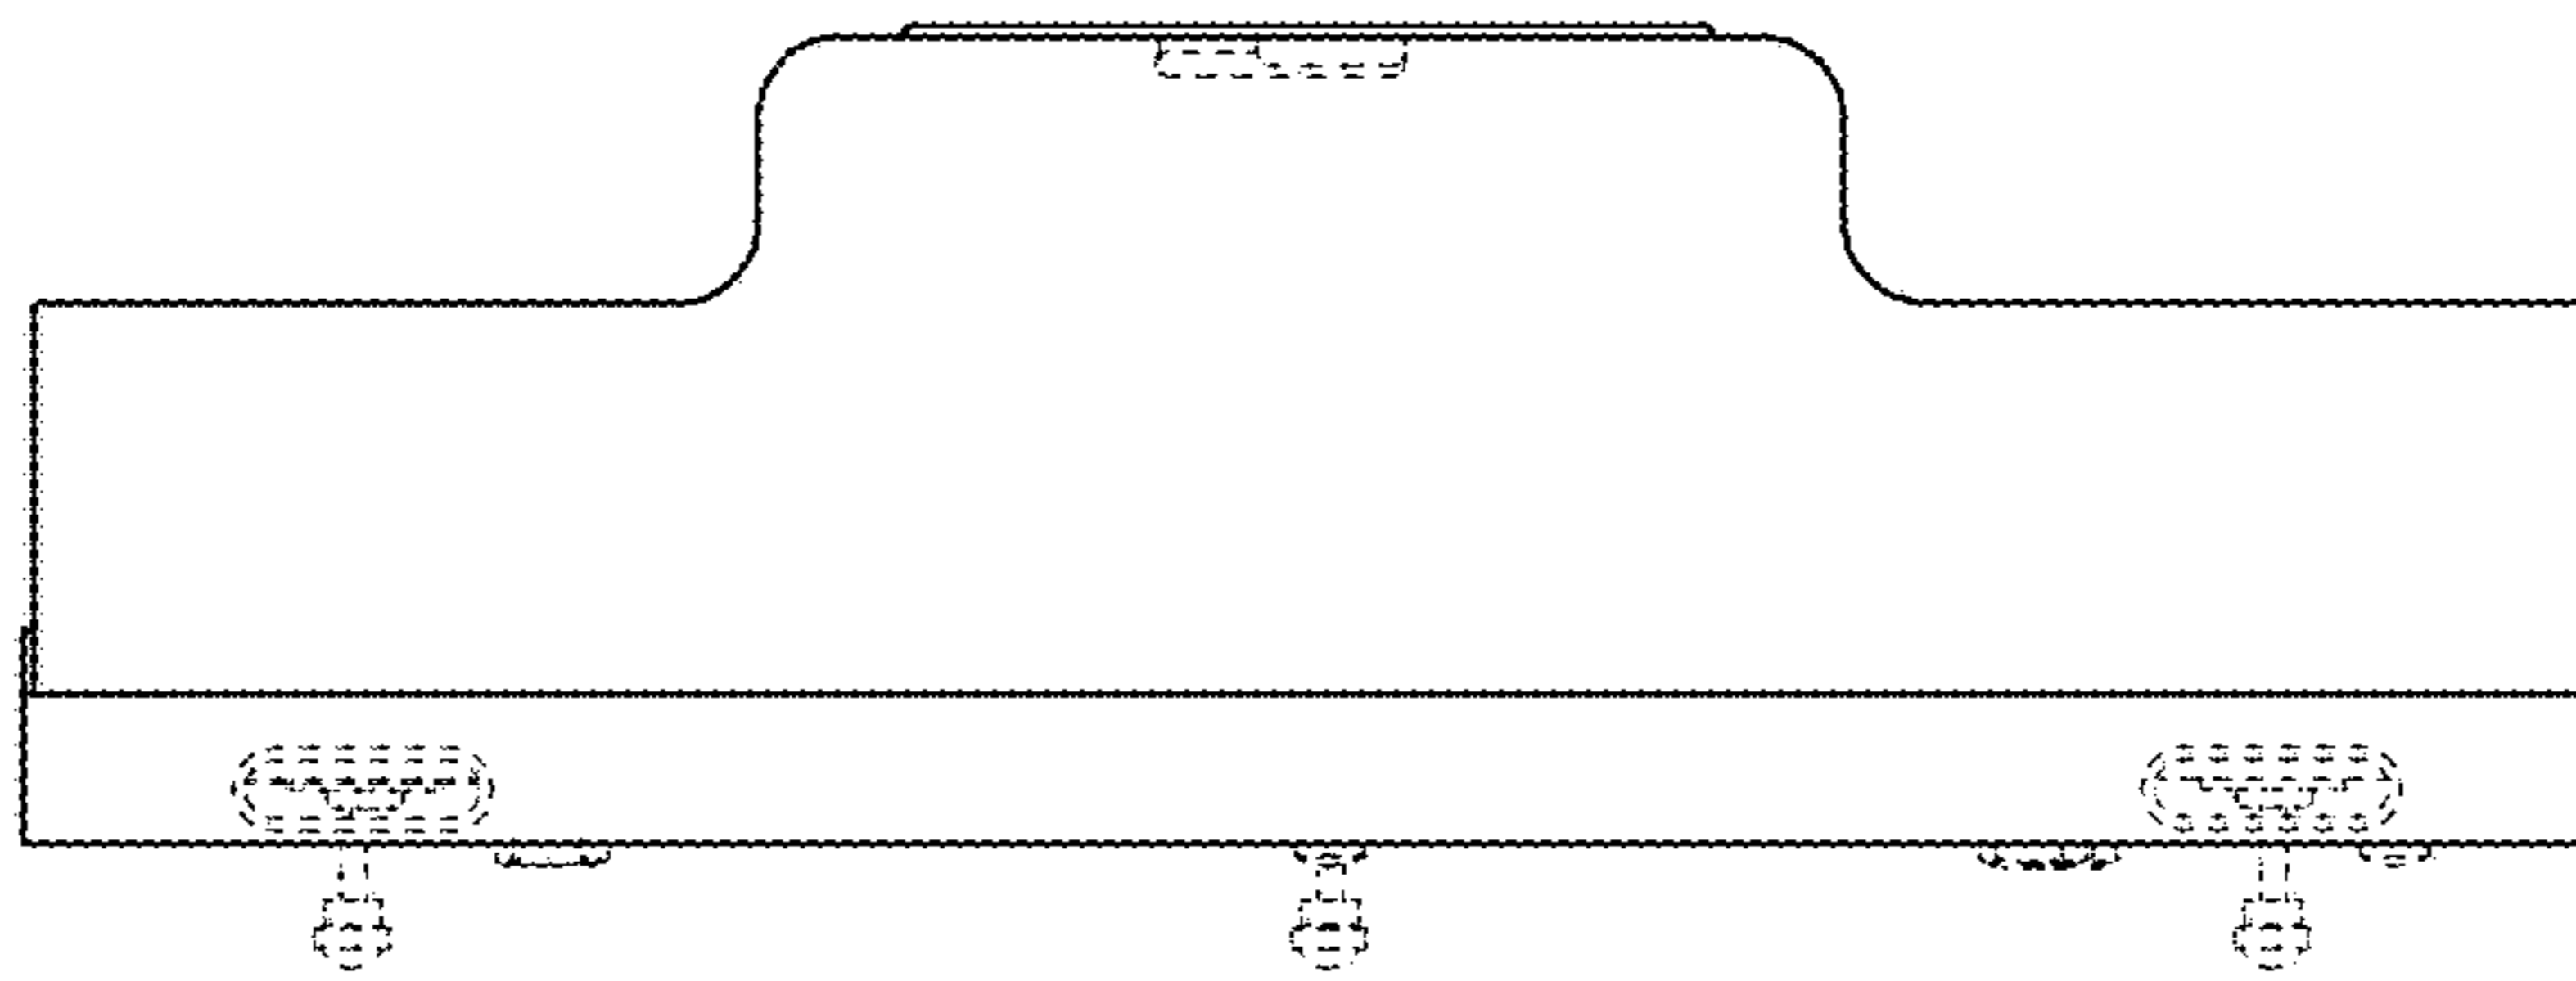


FIG. 5

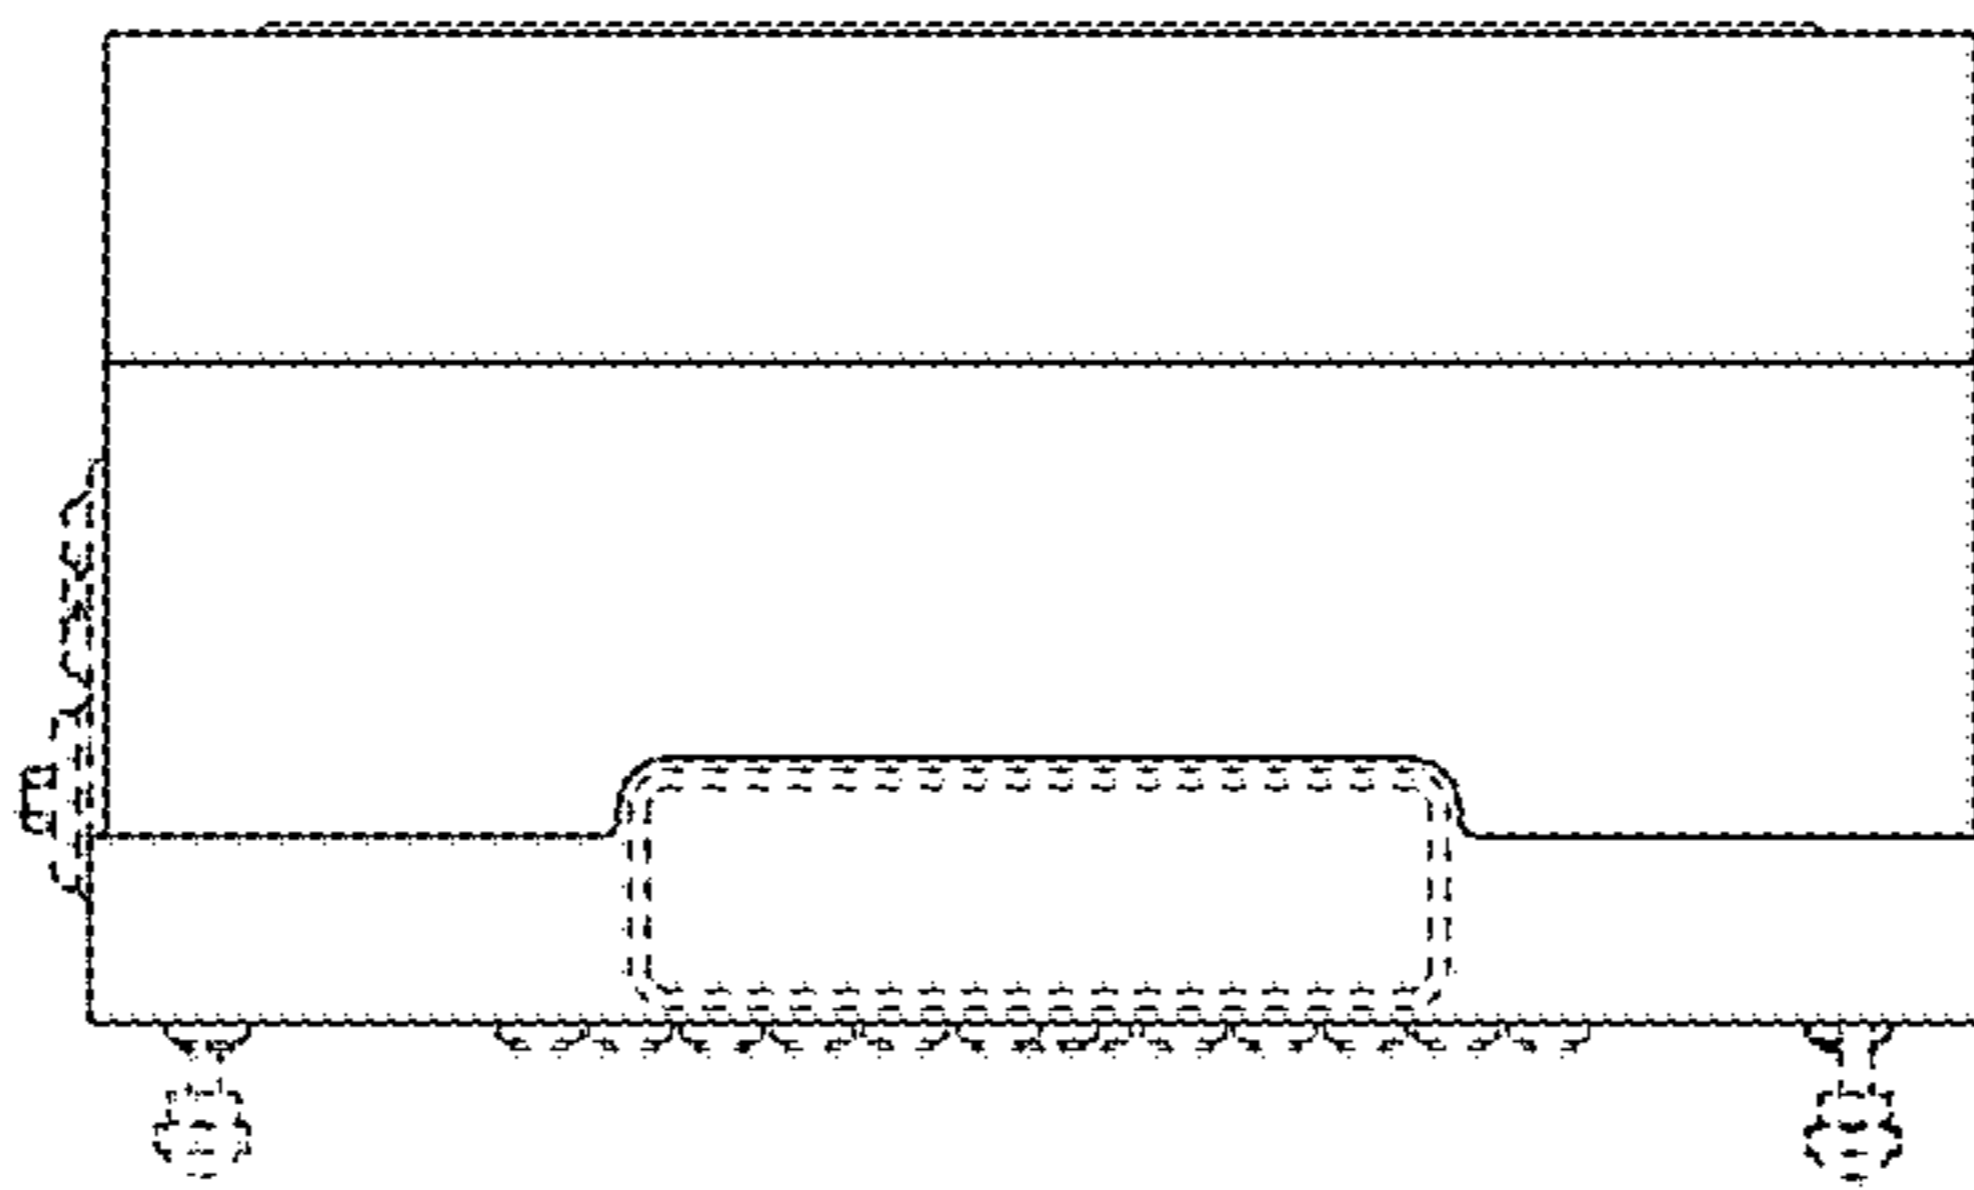


FIG. 6

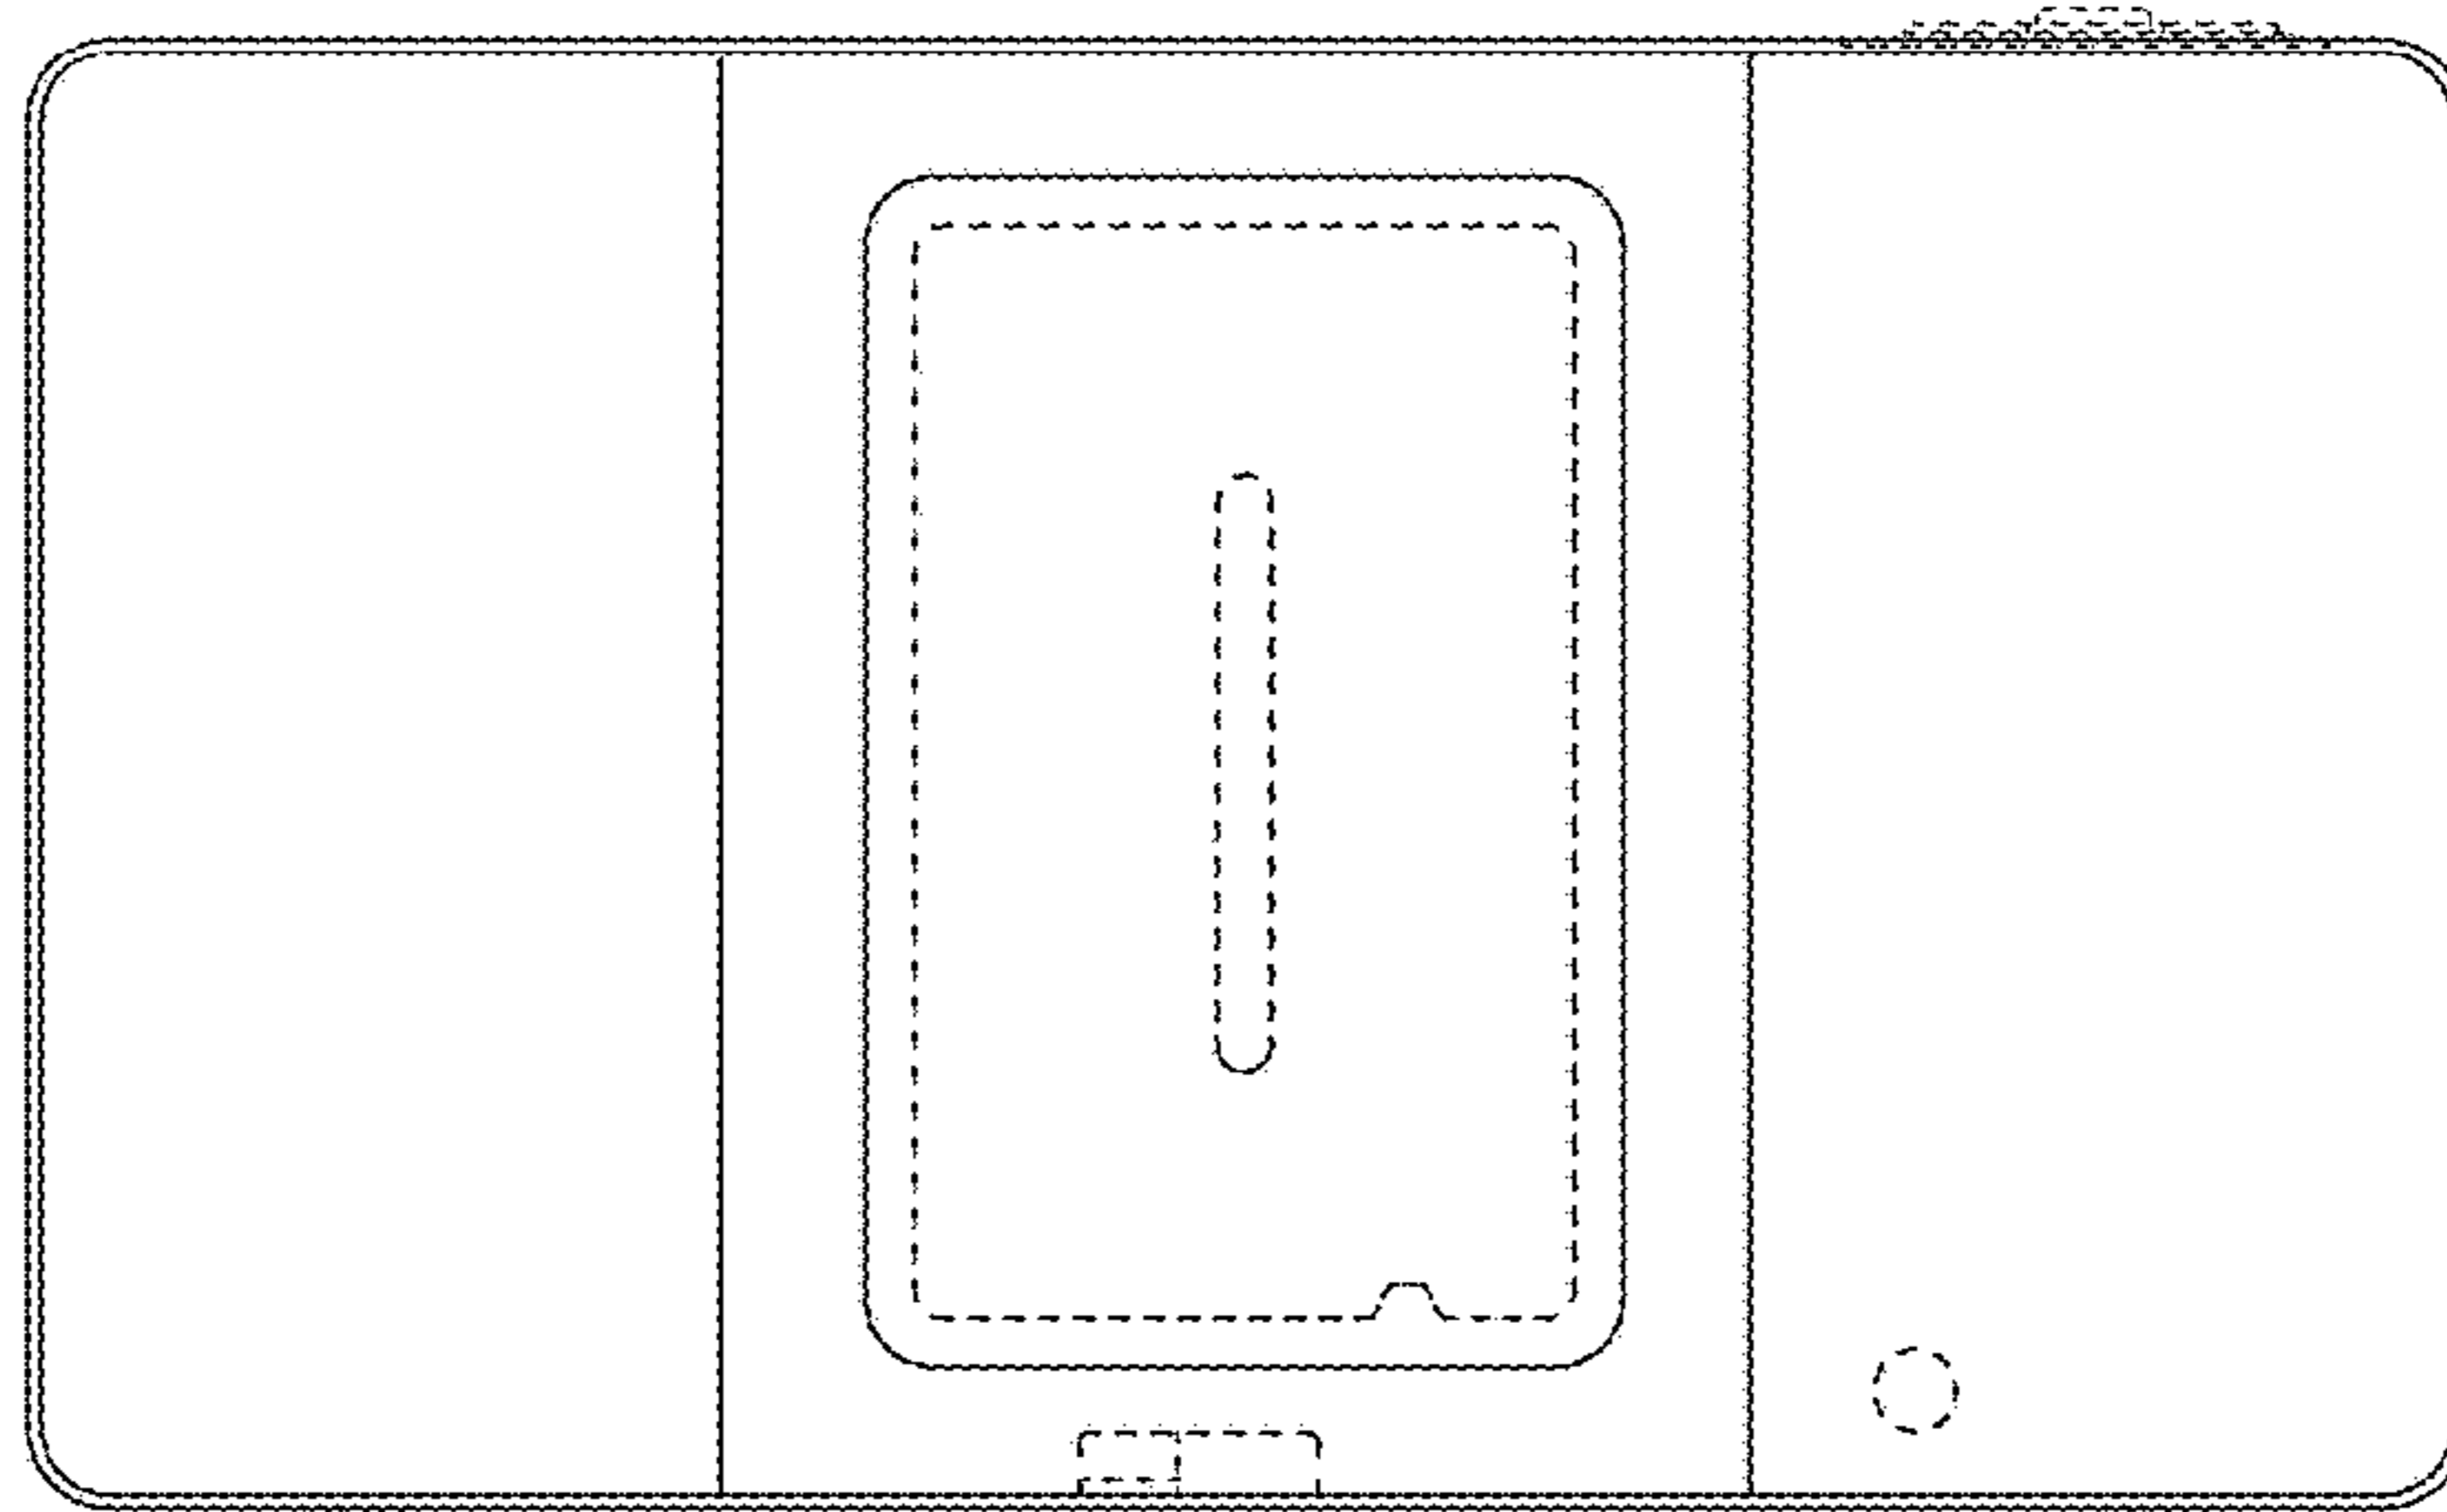


FIG. 7