



US00D852812S

(12) **United States Design Patent** (10) **Patent No.:** **US D852,812 S**  
**Babion et al.** (45) **Date of Patent:** **\*\* Jul. 2, 2019**

(54) **DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE FOR GLUCOSE MONITORING SYSTEM**

(71) Applicant: **Roche Diabetes Care, Inc.,**  
Indianapolis, IN (US)

(72) Inventors: **Nils Babion, Heidelberg (DE); Mark Gilmore Mears, Westfield, IN (US)**

(73) Assignee: **Roche Diabetes Care, Inc.,**  
Indianapolis, IN (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/593,963**

(22) Filed: **Feb. 14, 2017**

(51) **LOC (11) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/485**

(58) **Field of Classification Search**  
USPC ..... D14/485-495; D20/11; D21/324, 325  
CPC .... G06F 3/048; G06F 3/0481; G06F 3/04812;  
G06F 3/04817; G06F 3/0482; G06F  
3/0483; G06F 3/04842; G06F 3/0485;  
G06F 3/04855; G06F 3/0486; G06F  
3/0488; G06F 3/04886; G06F 9/4443;  
G06F 17/211; G06F 17/212; H02J  
7/0021; H02J 7/0047; G09B 19/00; A61B  
5/0002

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D392,267 S \* 3/1998 Mason ..... D14/491  
D428,399 S \* 7/2000 Kahn ..... D14/488  
D543,991 S \* 6/2007 Vigasaa ..... D14/487  
D593,111 S \* 5/2009 Danton ..... D14/485  
D605,657 S \* 12/2009 Danton ..... D14/487  
D612,398 S \* 3/2010 Lemay ..... D14/489  
D677,269 S \* 3/2013 Scott ..... D14/486

D684,160 S \* 6/2013 Truelove ..... D14/485  
D711,906 S \* 8/2014 Francisco ..... D14/486  
D768,147 S \* 10/2016 Yoo ..... D14/485  
D768,715 S \* 10/2016 Park ..... D14/491  
D769,322 S \* 10/2016 Rajeswaran ..... D14/491  
D775,138 S \* 12/2016 van Os ..... D14/485  
D777,747 S \* 1/2017 Derby ..... D14/486  
D789,417 S \* 6/2017 Yamasaki ..... D14/491  
D814,520 S \* 4/2018 Martin ..... D14/492  
2004/0172301 A1 \* 9/2004 Mihai ..... A61B 5/0002  
705/2

(Continued)

**OTHER PUBLICATIONS**

“Accuracy and . . .” Aug. 10, 2016, posted at senseonics.com, [site visited Aug. 21, 2018]. <http://www.senseonics.com/~media/Files/S/Senseonics-IR/documents/publications/accuracy-and-longevity-of-an-implantable-continous-glucose-sensor-in-the-precise-study-a-180-day-prospective-multi-center-pivotal-trial.pdf>.\*

(Continued)

*Primary Examiner* — Jack Reickel  
*Assistant Examiner* — John M Otte  
(74) *Attorney, Agent, or Firm* — Stinson Leonard Street LLP


(57) **CLAIM**

The ornamental design for a display screen with graphical user interface for glucose monitoring system, as shown and described.

**DESCRIPTION**

FIG. 1 is a front view of a display screen with graphical user interface for glucose monitoring system showing our new design; FIG. 2 is a front view of a second embodiment thereof; and, FIG. 3 is a front view of a third embodiment thereof. The broken lines showing in a portion of a display screen, text and other elements in the Figures are for illustrative purposes only and form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

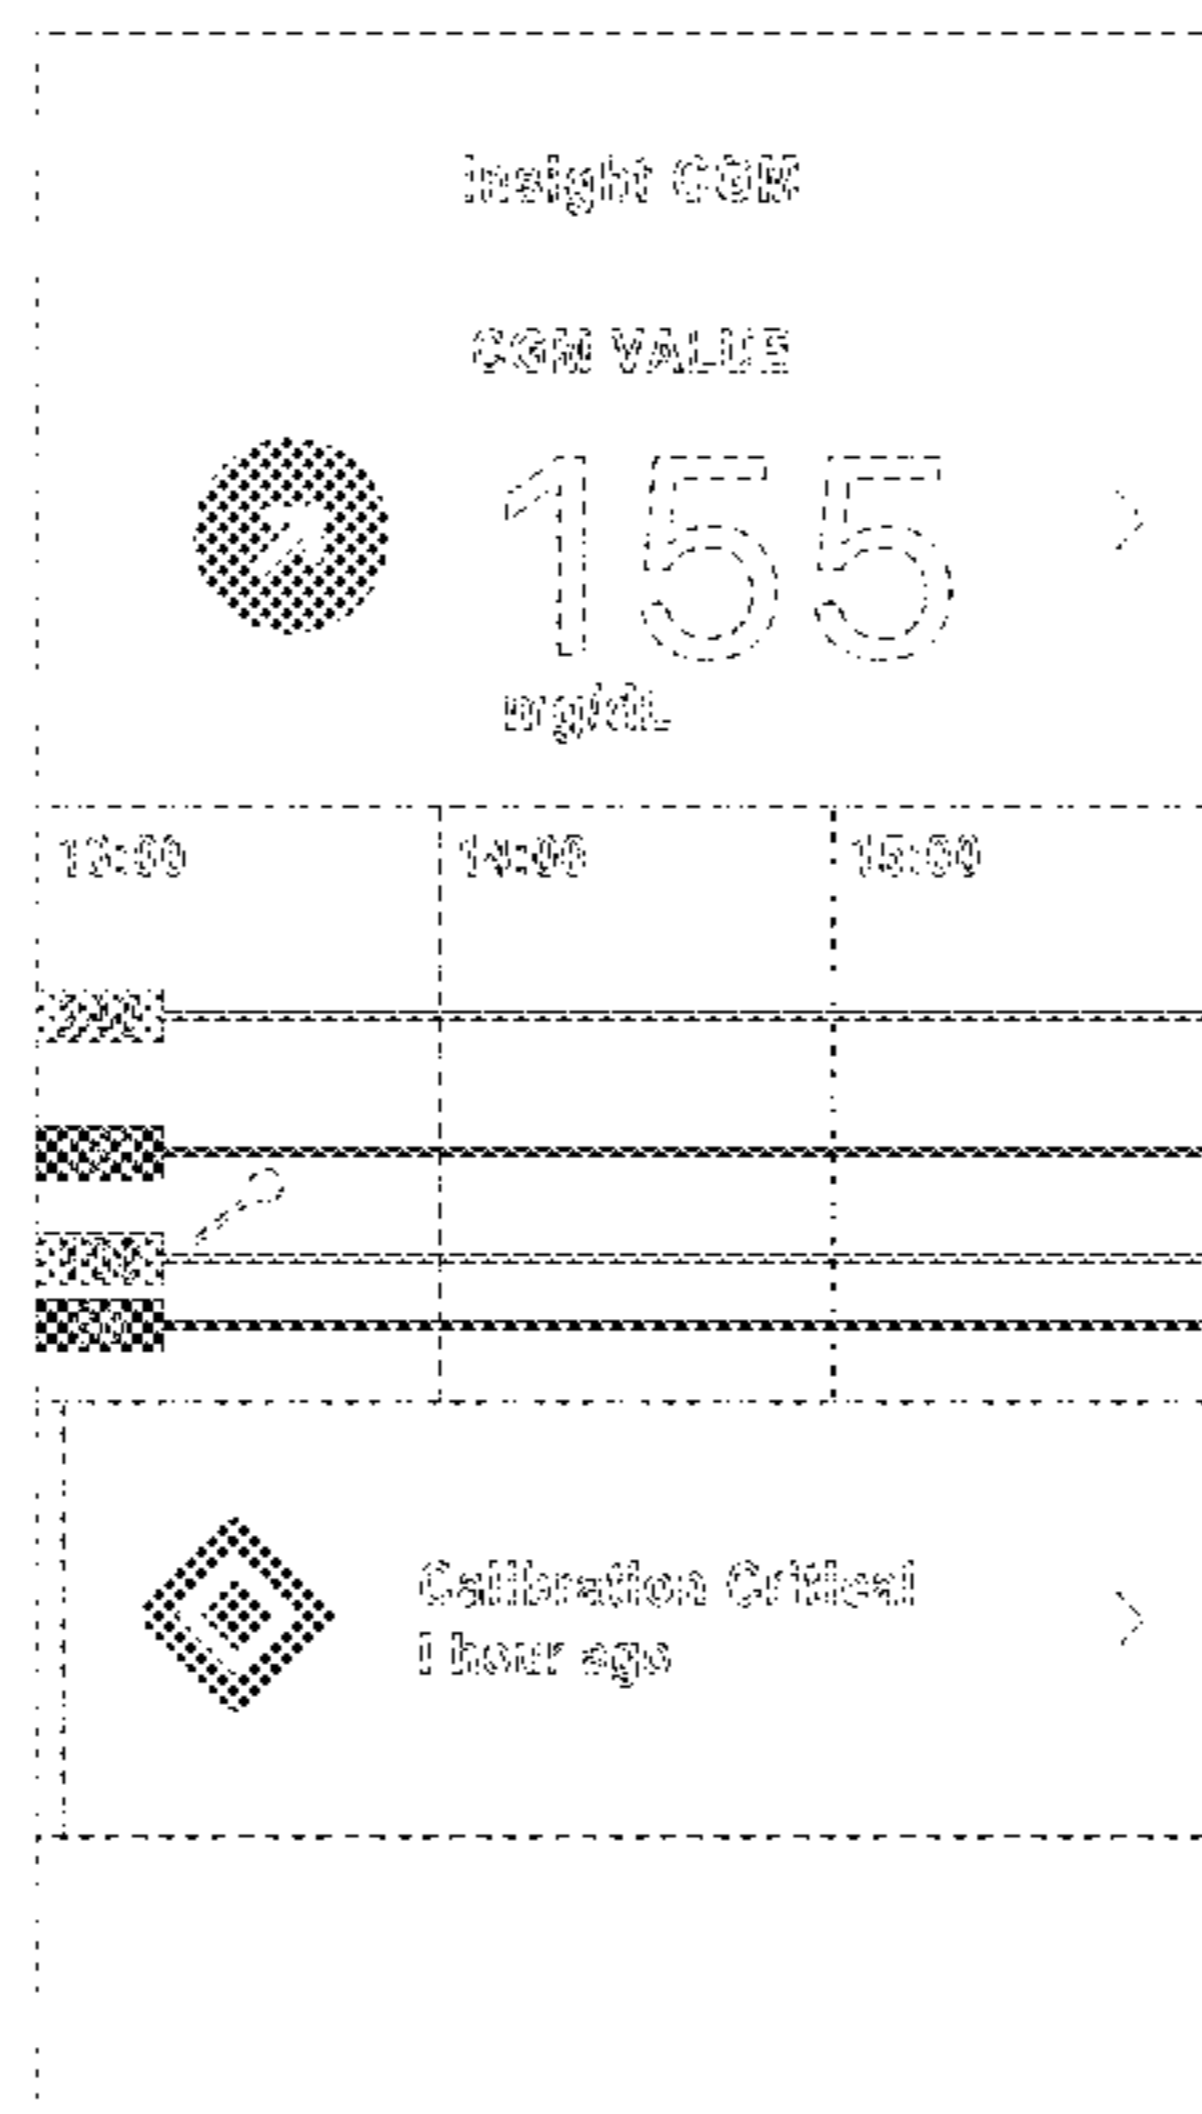

(56)

**References Cited**

## U.S. PATENT DOCUMENTS

2007/0177803 A1\* 8/2007 Elias ..... G06F 3/04883  
382/188  
2010/0087230 A1\* 4/2010 Peh ..... G06F 3/04817  
455/566  
2014/0181650 A1\* 6/2014 Polubinski ..... G06F 3/0482  
715/702  
2015/0286386 A1\* 10/2015 Kaufthal ..... G06F 17/21  
715/765  
2016/0212167 A1\* 7/2016 Dotan ..... H04L 63/20  
2018/0042559 A1\* 2/2018 Cabrera, Jr. .... A61B 5/14532

## OTHER PUBLICATIONS

Brown, Adam et al., "Dexcom G5 Mobile—CGM on Your Phone, Receiver Optional" Oct. 16, 2015, posted at diatribe.org, [site visited Aug. 21, 2018]. <https://diatribe.org/dexcom-g5-mobile-cgm-your-phone-receiver-optional>.\*

"Bigfoot Biomedical Reveals Its Automated Insulin Delivery System!" Jan. 25, 2016, posted at diatribe.org, [site visited Aug. 21, 2018]. <https://diatribe.org/bigfoot-biomedical-reveals-its-automated-insulin-delivery-system>.\*

"Learn to Drive Smart" Oct. 3, 2012, posted at issuu.com, [site visited Aug. 21, 2018]. <https://issuu.com/insurancecorporationofbc/docs/learntodrive/45>.\*

\* cited by examiner

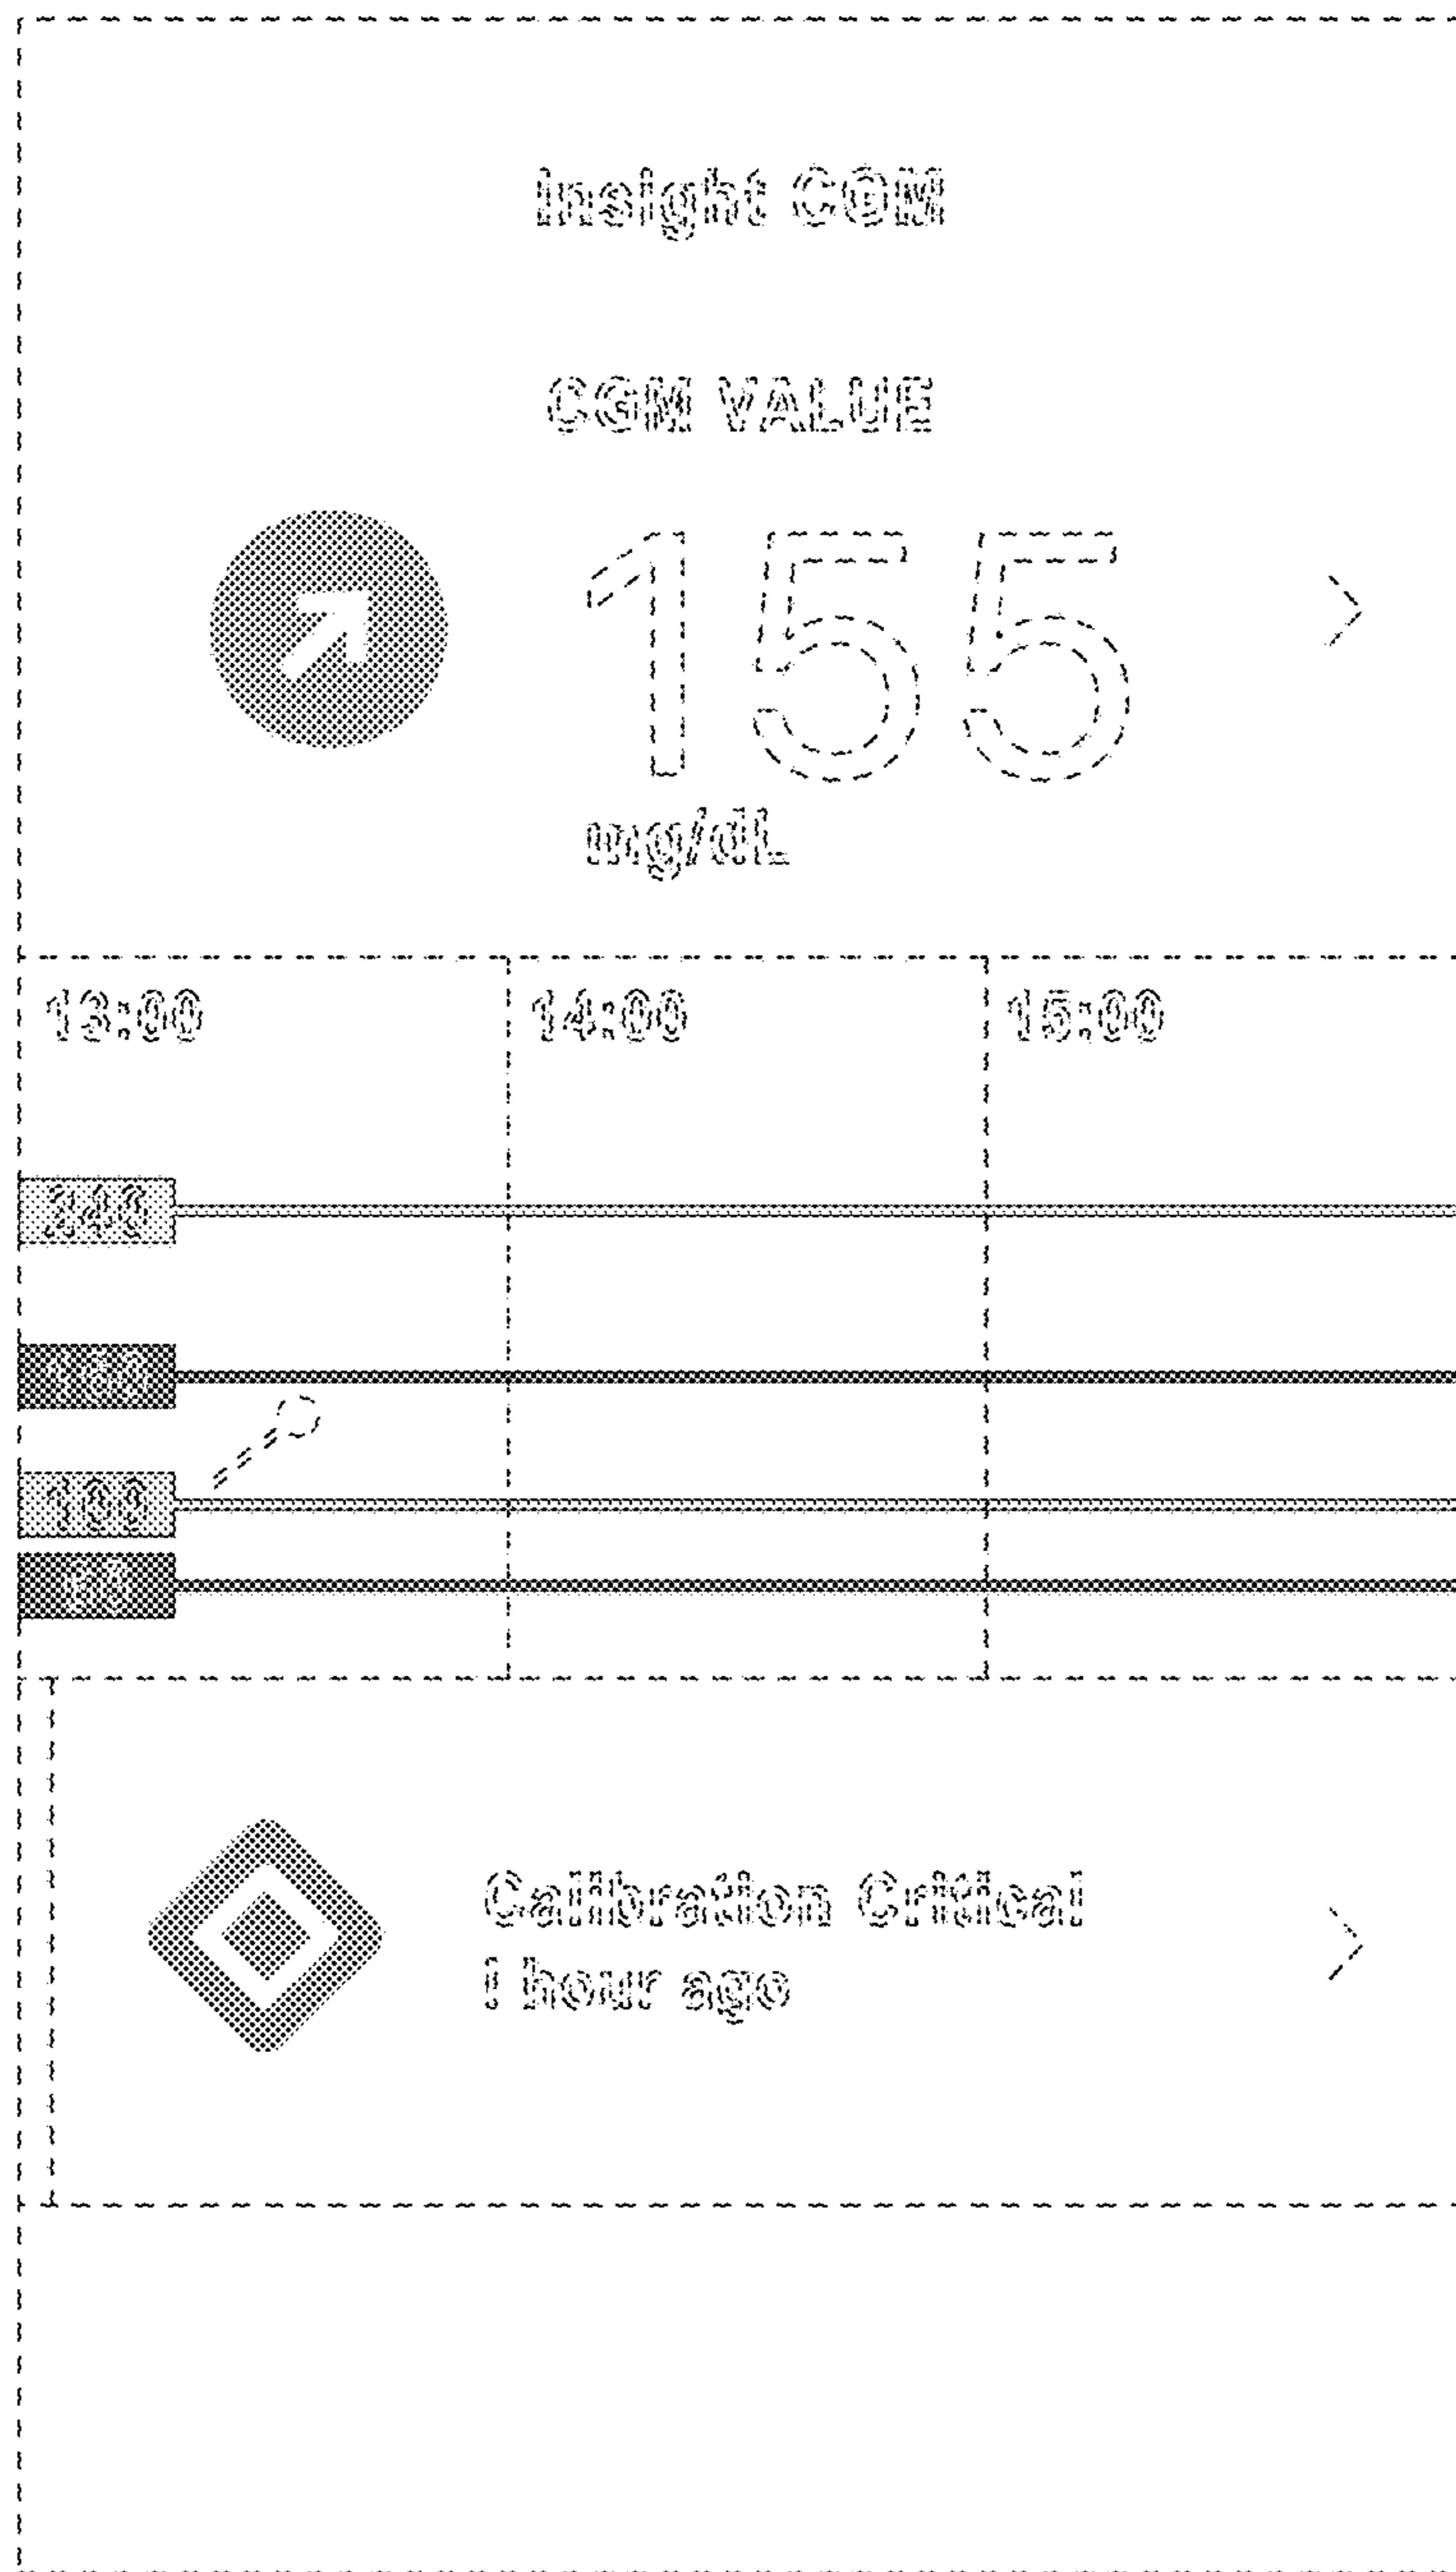


FIG. 1

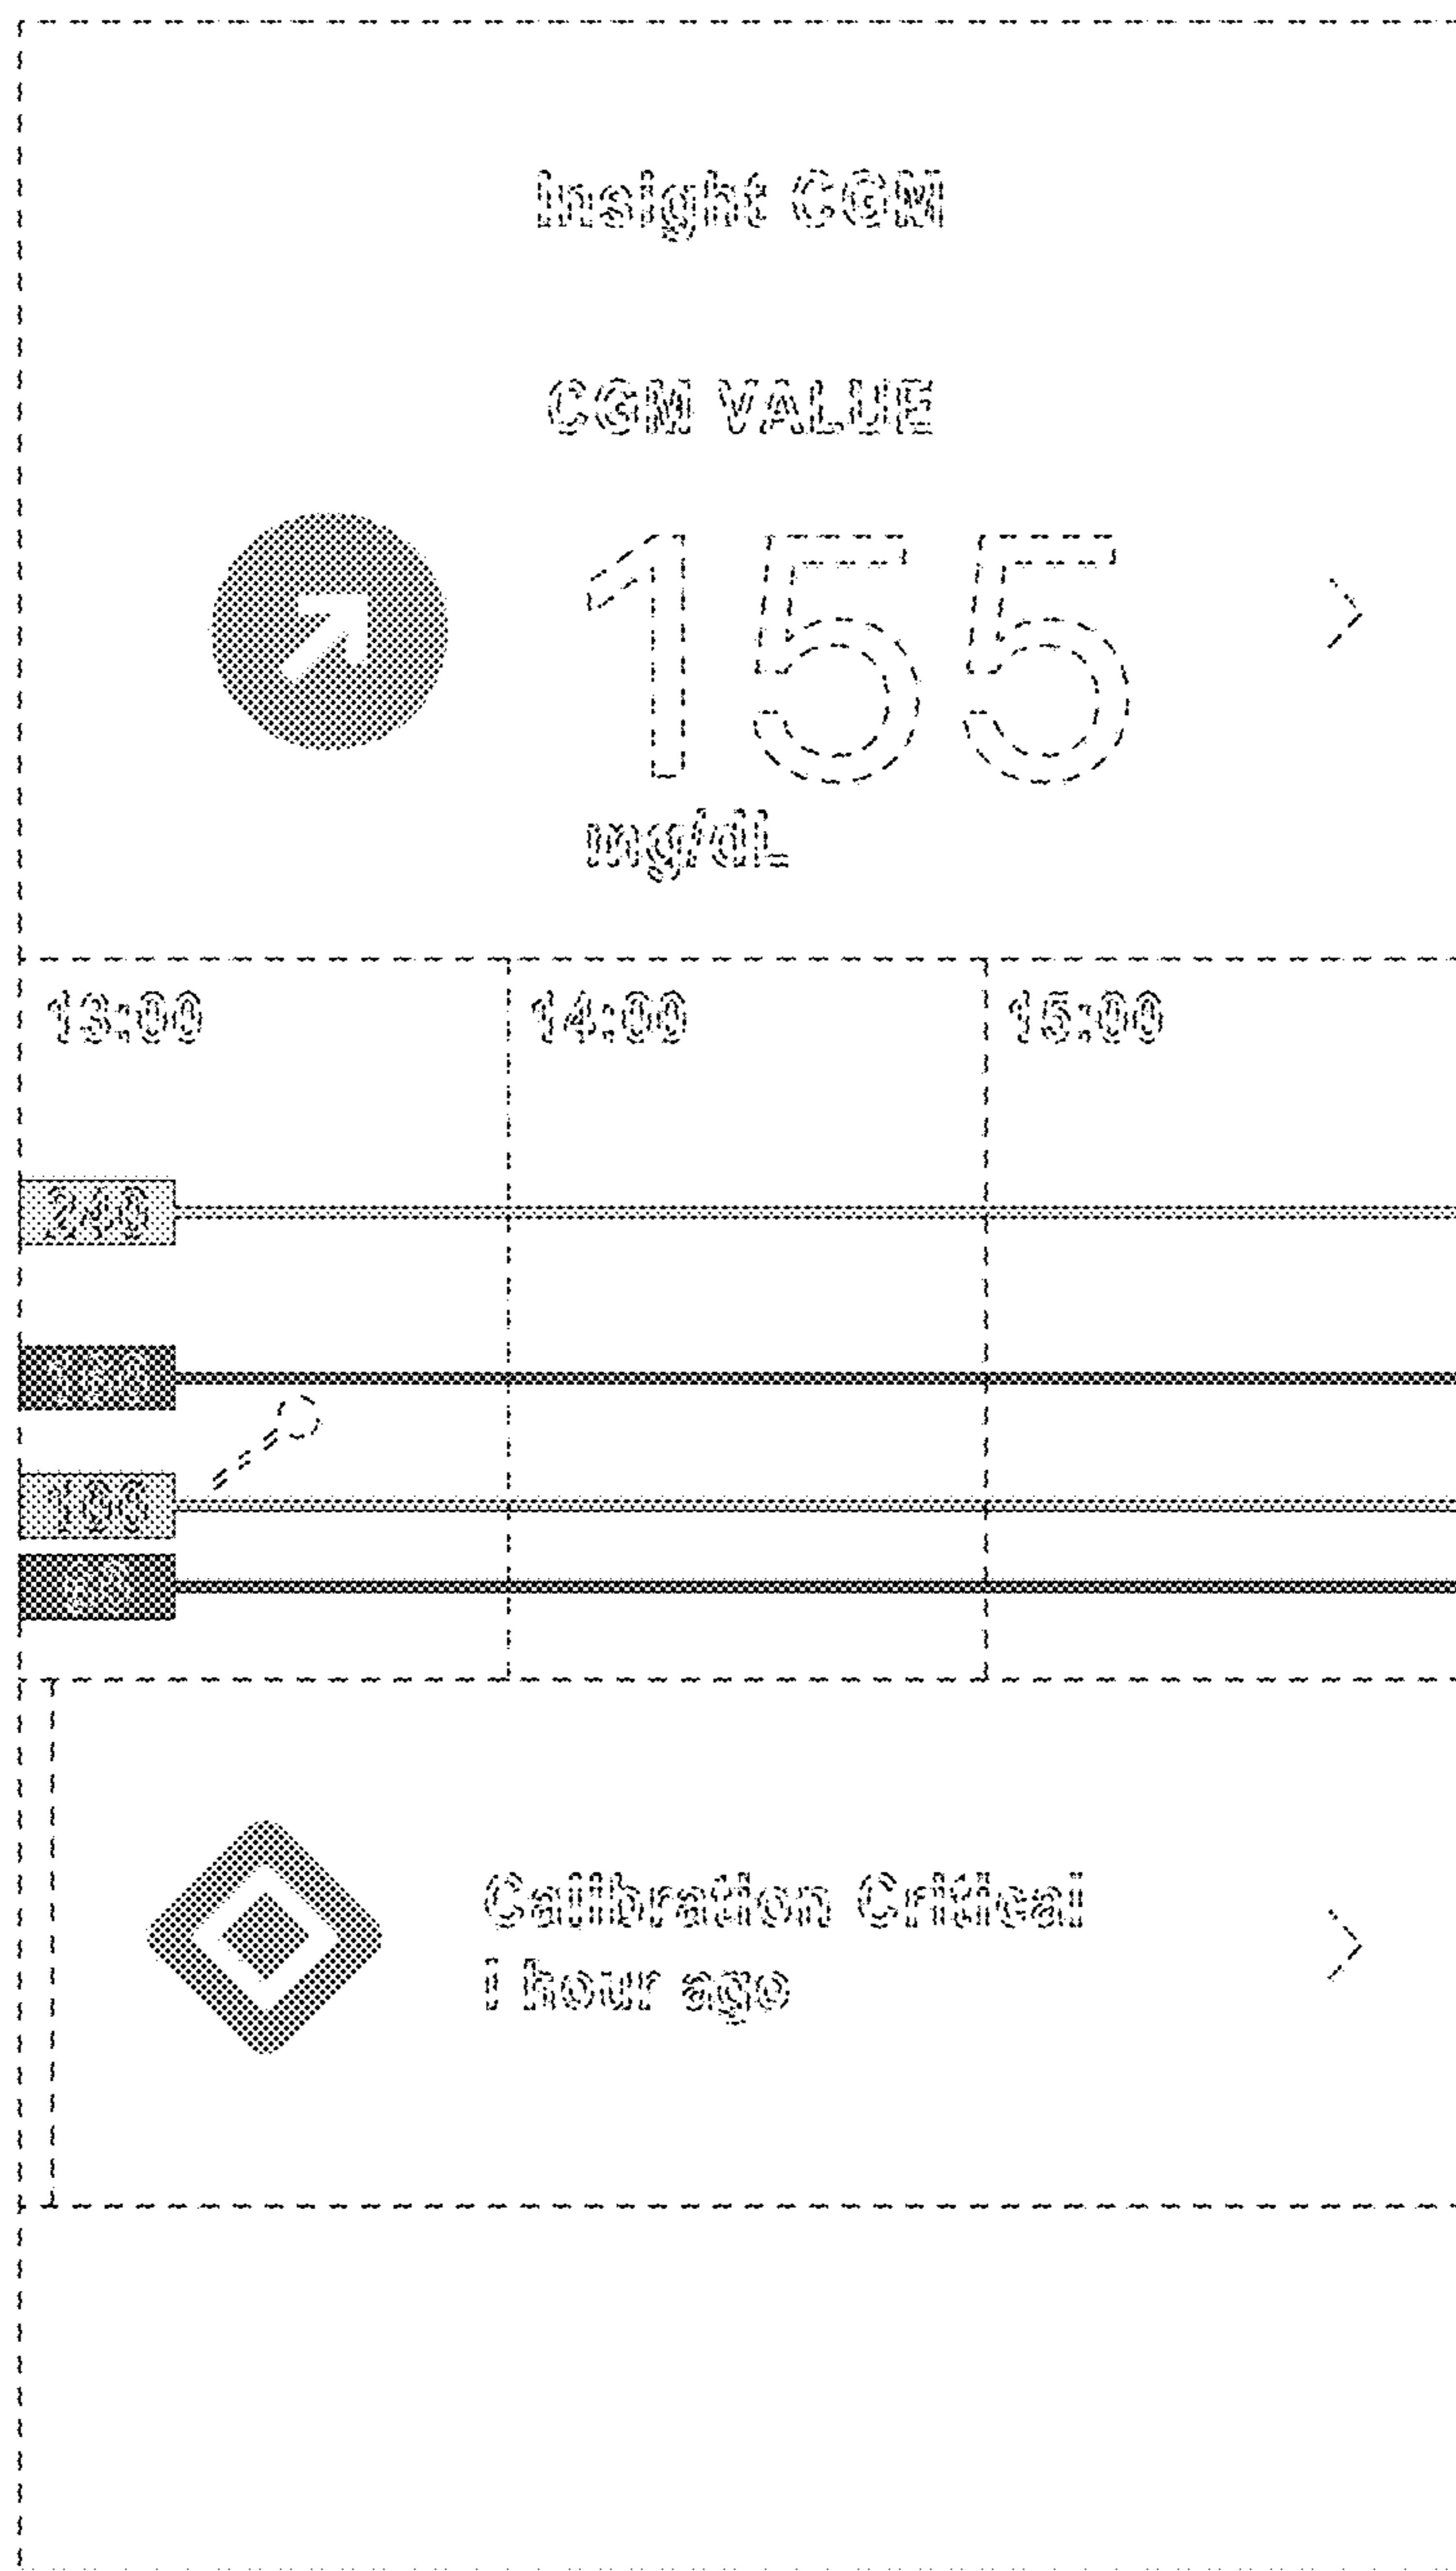


FIG. 2

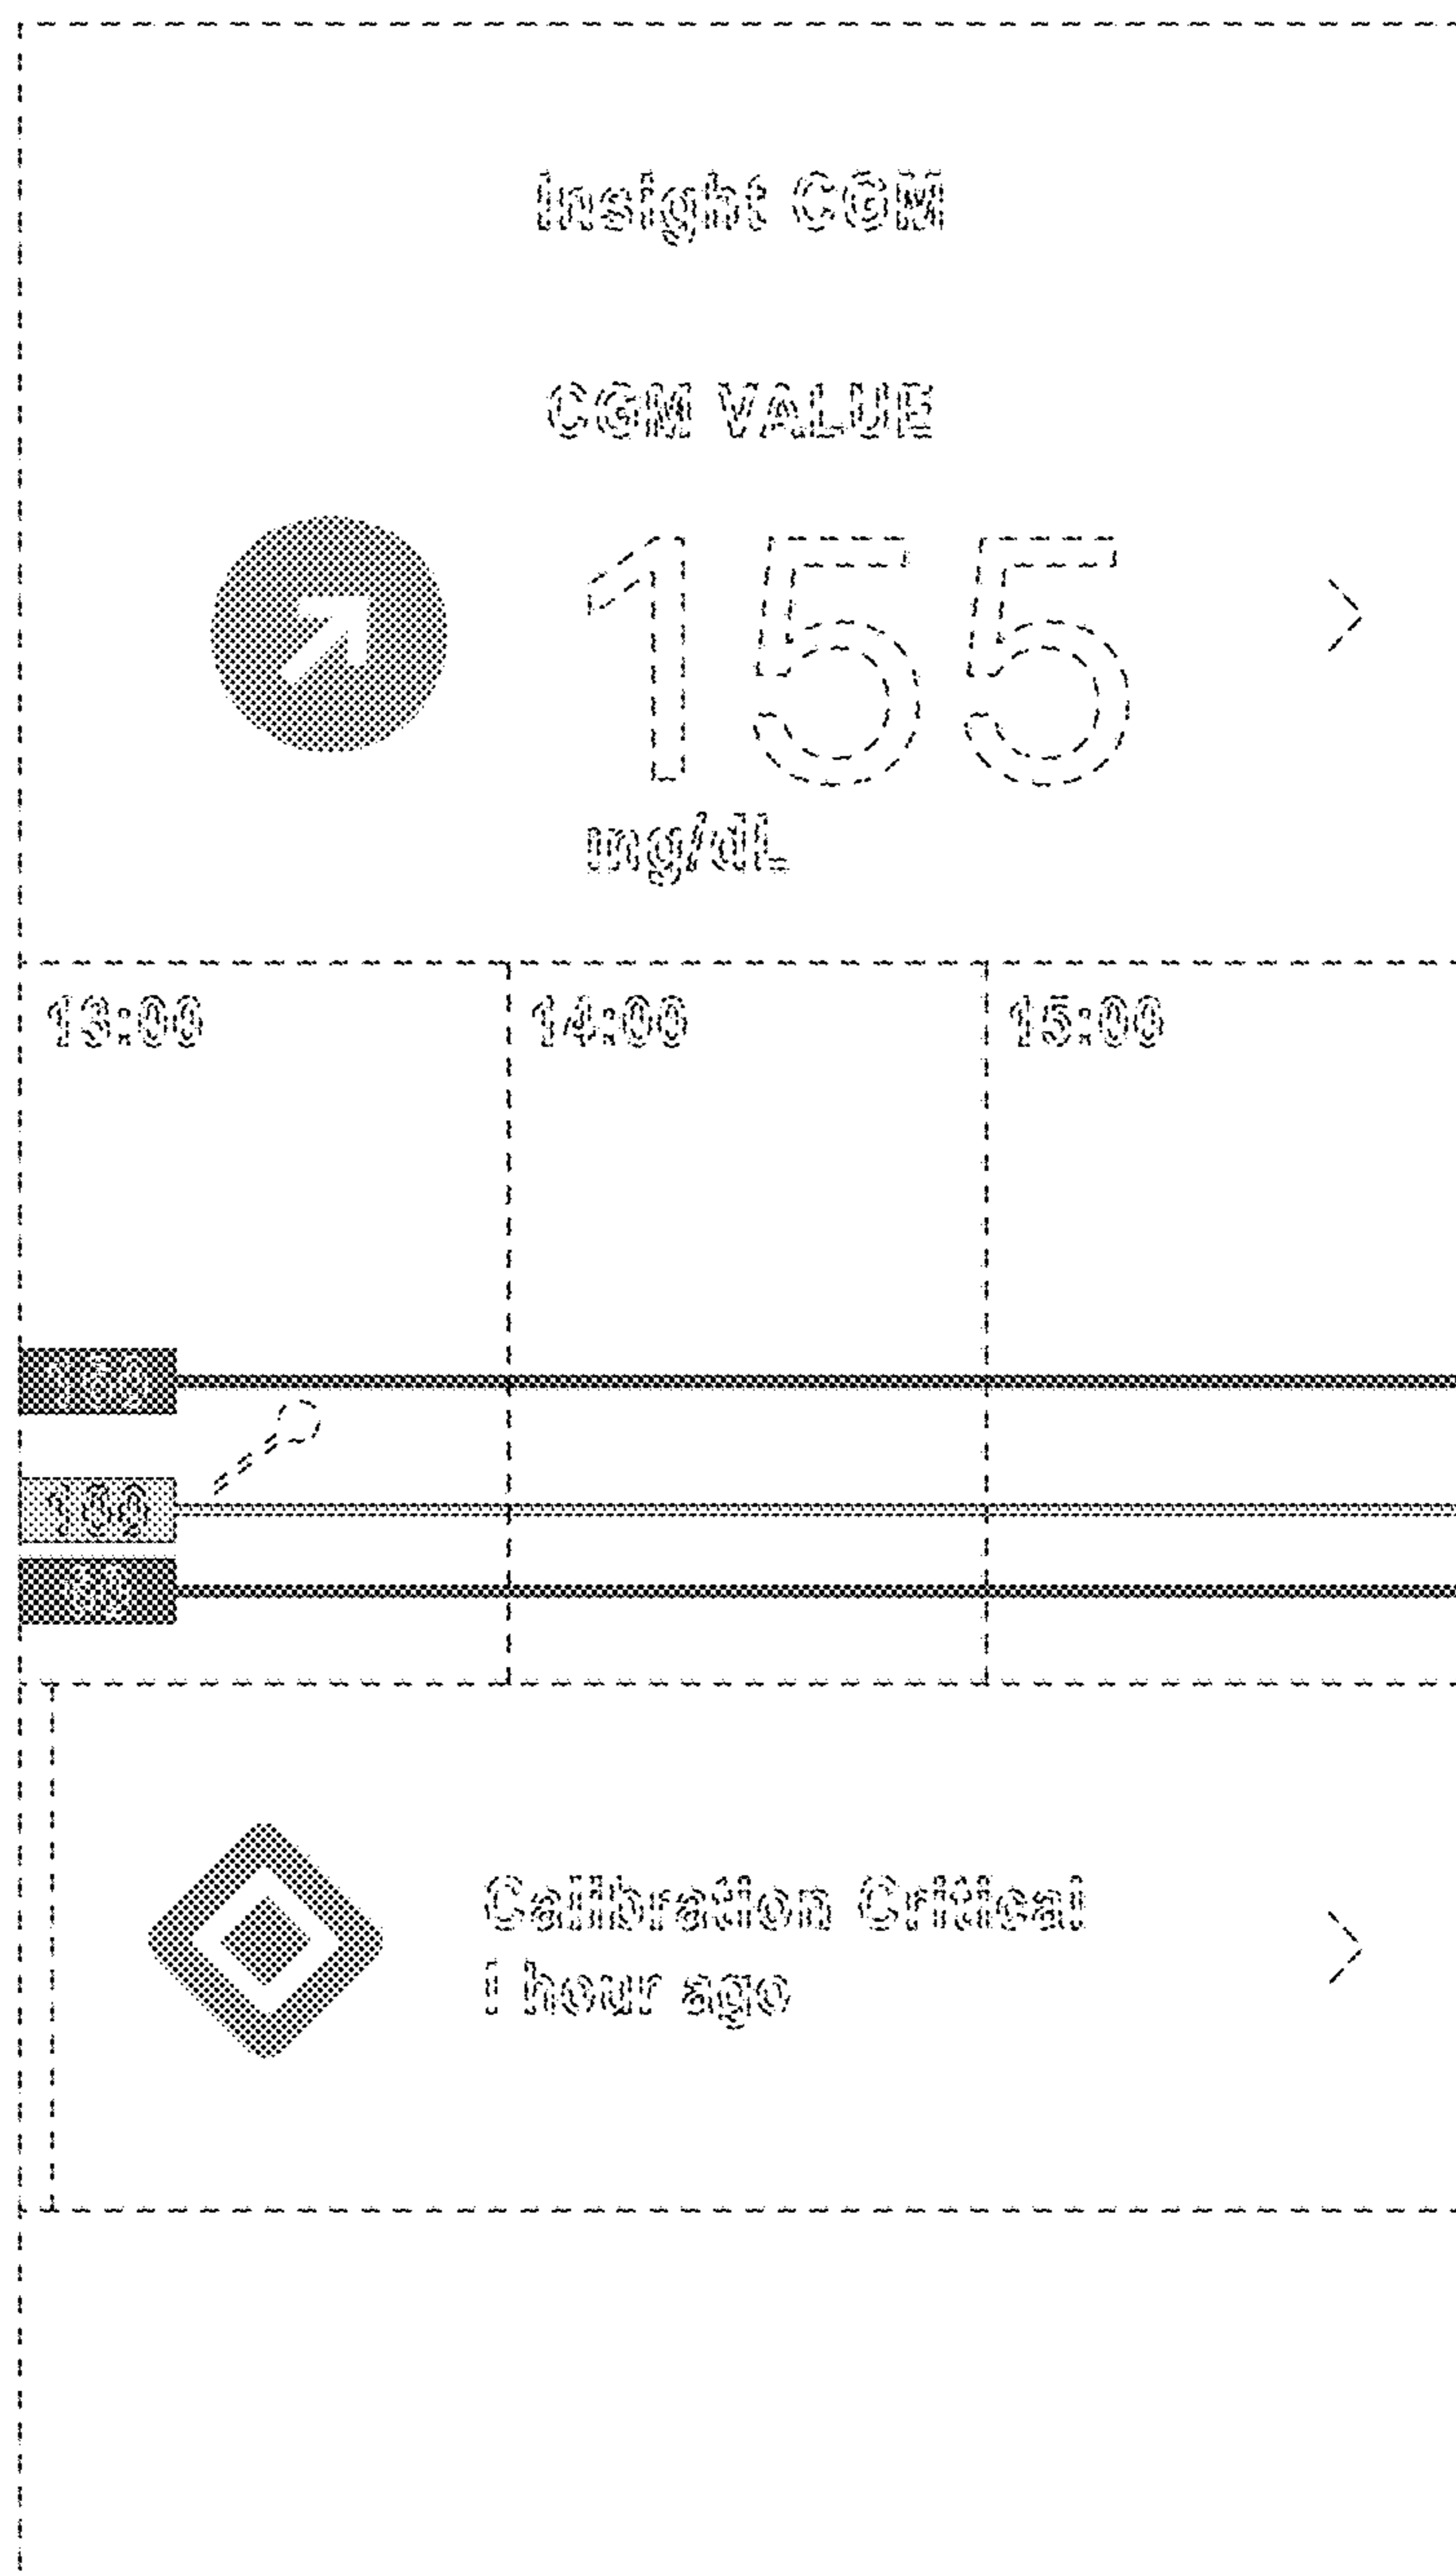


FIG. 3