



US00D852884S

(12) **United States Design Patent**
Munro et al.

(10) **Patent No.:** **US D852,884 S**
(45) **Date of Patent:** **** Jul. 2, 2019**

(54) **TRAINING DEVICE FOR MINIMALLY
INVASIVE MEDICAL PROCEDURES**

5,873,732 A 2/1999 Hasson
6,659,776 B1 12/2003 Aumann et al.
6,704,001 B1* 3/2004 Schena G05G 9/047
310/12.04

(71) Applicant: **American Association of Gynecologic
Laparoscopists**, Cypress, CA (US)

(Continued)

(72) Inventors: **Malcolm Munro**, Tarzana, CA (US);
James Messerschmidt, Prescott Valley,
AZ (US); **Ted Anderson**, Franklin, TN
(US); **Joseph Hudgens**, Madison, MS
(US)

FOREIGN PATENT DOCUMENTS

CA 2846386 A1 2/2013
WO 2016116567 A1 7/2016

(73) Assignee: **AMERICAN ASSOCIATION OF
GYNECOLOGICAL
LAPAROSCOPISTS, INC.**, Cypress,
CA (US)

OTHER PUBLICATIONS

Fast Tech. Link: <https://www.fasttech.com/product/9635622-9-medical-dental-stainless-steel-instrument-tray>. Visited Jul. 30, 2018.
Medical Dental Stainless Steel Instrument Tray. (Year: 2018).*

(Continued)

(**) Term: **15 Years**

Primary Examiner — Ian Simmons

Assistant Examiner — Lauren D McVey

(74) *Attorney, Agent, or Firm* — Merchant & Gould P.C.

(21) Appl. No.: **29/623,017**

(57) **CLAIM**

The ornamental design for a training device for minimally
invasive medical procedures, as shown and described.

(22) Filed: **Oct. 20, 2017**

DESCRIPTION

(51) **LOC (11) Cl.** **19-07**

(52) **U.S. Cl.**

USPC **D19/62**

(58) **Field of Classification Search**

USPC D19/59-64; D24/121, 227; D9/783,
D9/771, 431

CPC G06N 99/005; G09B 23/28; G09B 23/285;
G09B 23/30

See application file for complete search history.

FIG. 1 is top isometric view of a training device for
minimally invasive medical procedures, showing our new
design;

FIG. 2 is another top isometric view thereof;

FIG. 3 is another top isometric view thereof;

FIG. 4 is another top isometric view thereof;

FIG. 5 a right side view thereof;

FIG. 6 is a left side view thereof;

FIG. 7 is a rear view thereof;

FIG. 8 is a front view thereof;

FIG. 9 is a top view thereof; and,

FIG. 10 is a bottom view thereof.



The wire frame lines shown throughout the views are
intended to indicate surface contour. The stippled shading
represents a contrast in appearance.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,180,308 A * 1/1993 Garito G09B 23/28
248/300
D367,675 S * 3/1996 Welch D11/131
D389,054 S * 1/1998 Teags D9/431
5,722,836 A 3/1998 Younker

1 Claim, 10 Drawing Sheets

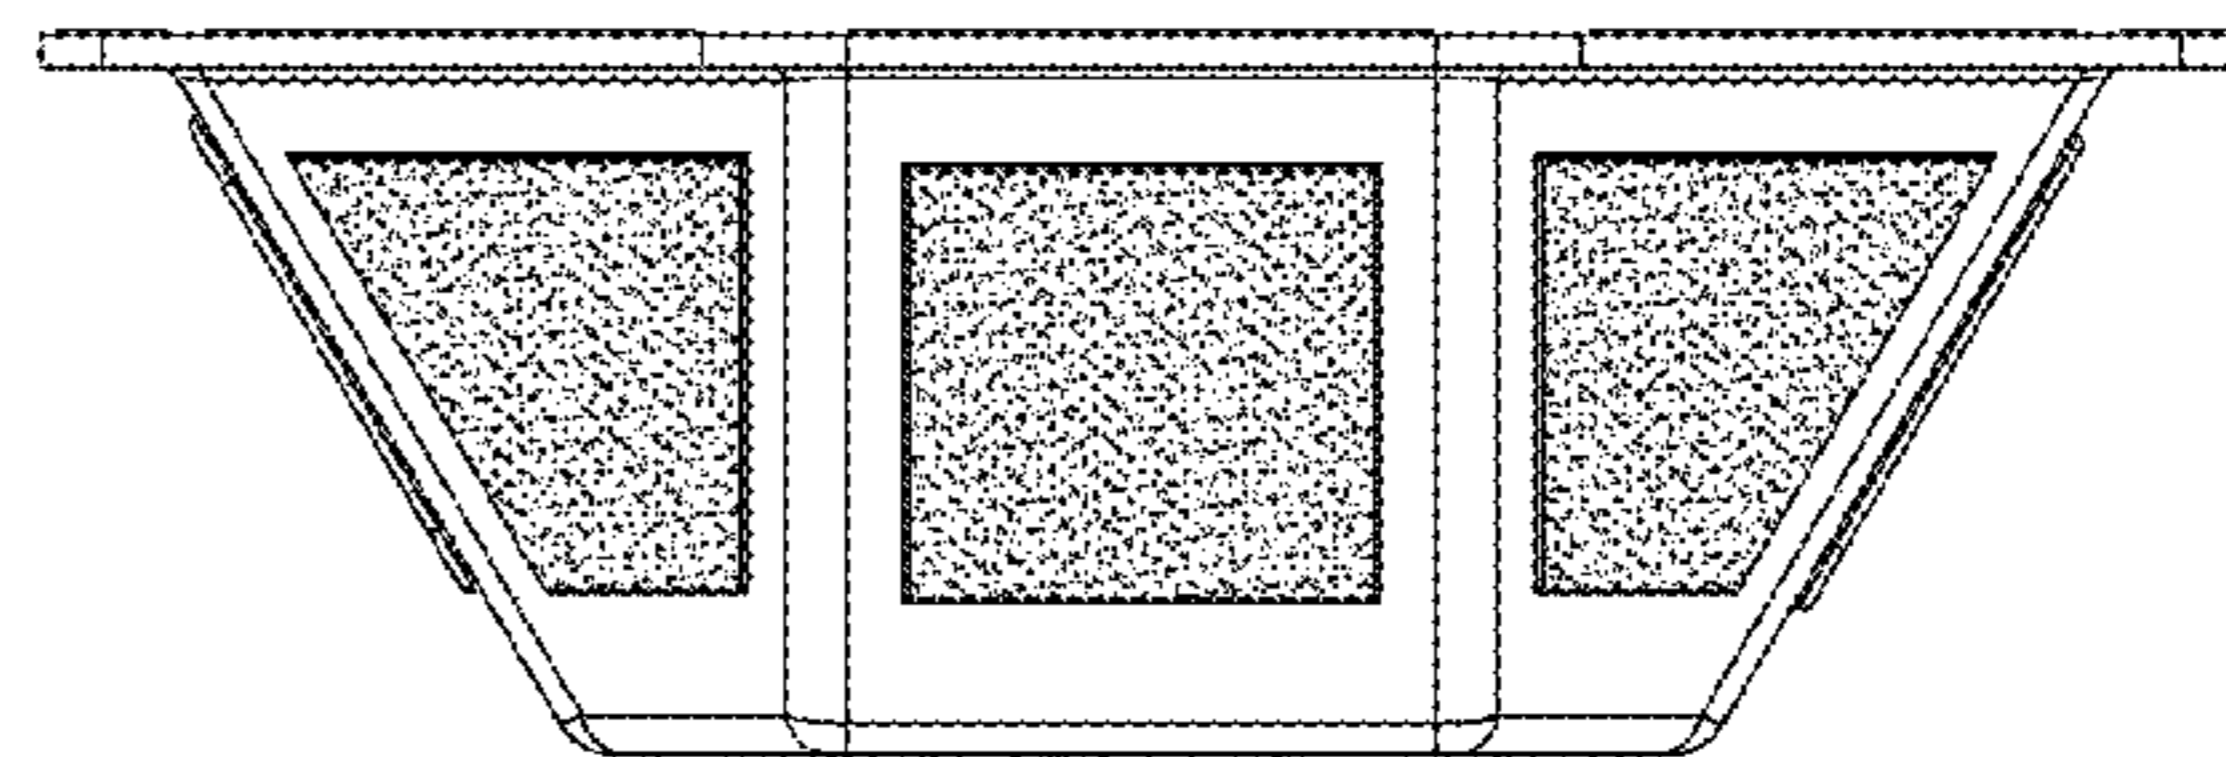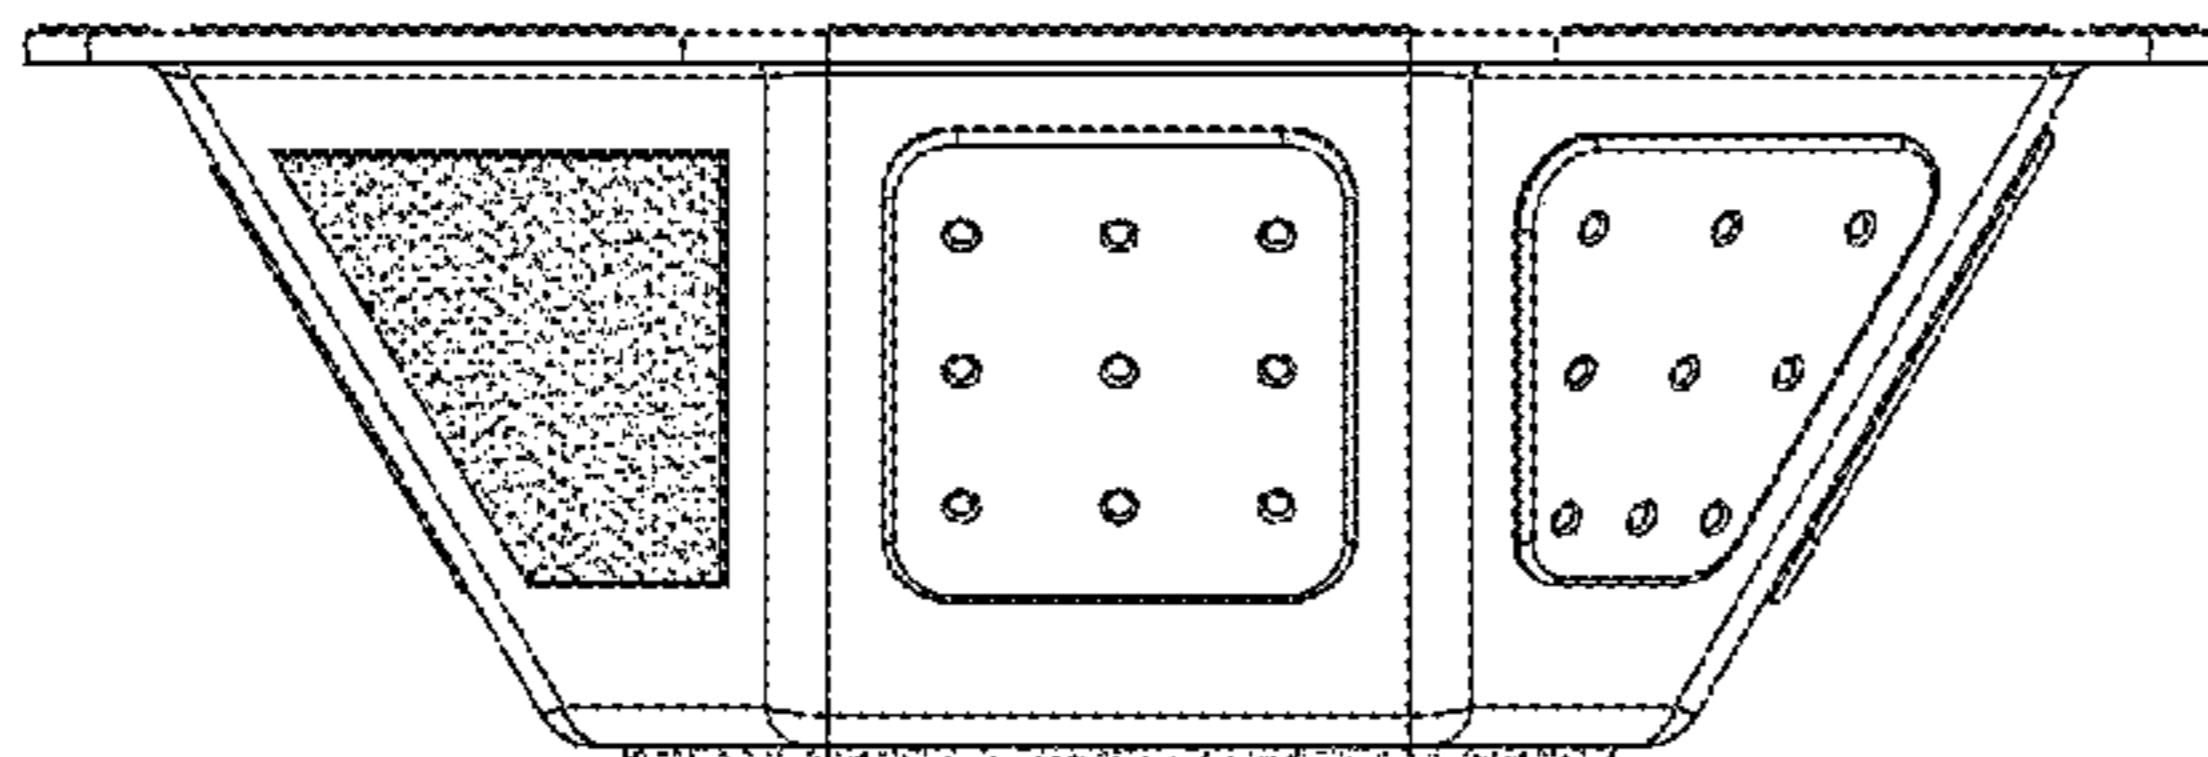

(56)

References Cited

U.S. PATENT DOCUMENTS

D581,505 S * 11/2008 North D23/356
 D594,063 S * 6/2009 Blackwell D19/59
 7,802,990 B2 9/2010 Korndorffer, Jr.
 7,837,473 B2 11/2010 Koh
 7,997,903 B2 8/2011 Hasson et al.
 8,007,281 B2 8/2011 Toly
 8,328,560 B2 12/2012 Niblock et al.
 8,460,002 B2 6/2013 Wang
 8,469,716 B2 6/2013 Fedotov et al.
 D688,126 S * 8/2013 Snedden D9/435
 8,764,452 B2 7/2014 Pravong et al.
 9,548,002 B2 1/2017 Black et al.
 9,959,786 B2 * 5/2018 Breslin G09B 23/285
 2004/0142314 A1 7/2004 Hasson
 2004/0175684 A1 9/2004 Kaasa et al.
 2005/0064378 A1 3/2005 Toly
 2005/0142525 A1 6/2005 Cotin et al.
 2007/0166682 A1 7/2007 Yarin et al.
 2008/0062299 A1 3/2008 Matanhelia

2009/0142741 A1* 6/2009 Ault G09B 23/285
 434/272
 2011/0269109 A2 11/2011 Miyazaki
 2012/0082970 A1 4/2012 Pravong et al.
 2012/0115118 A1* 5/2012 Marshall G09B 23/28
 434/262
 2012/0308977 A1 12/2012 Tortola
 2014/0220527 A1 8/2014 Li et al.
 2015/0037773 A1 2/2015 Quirarte
 2016/0133158 A1 5/2016 Sui et al.
 2016/0140876 A1 5/2016 Jabbour
 2017/0301263 A1* 10/2017 Souter G09B 23/30
 2018/0130380 A1* 5/2018 Snyder G09B 23/285

OTHER PUBLICATIONS

Limbs & Things Inc., Fundamentals of Laparoscopic Surgery
 Trainer System & Accessories Product Brochure, V.2 May 2016, 4
 pages.

* cited by examiner

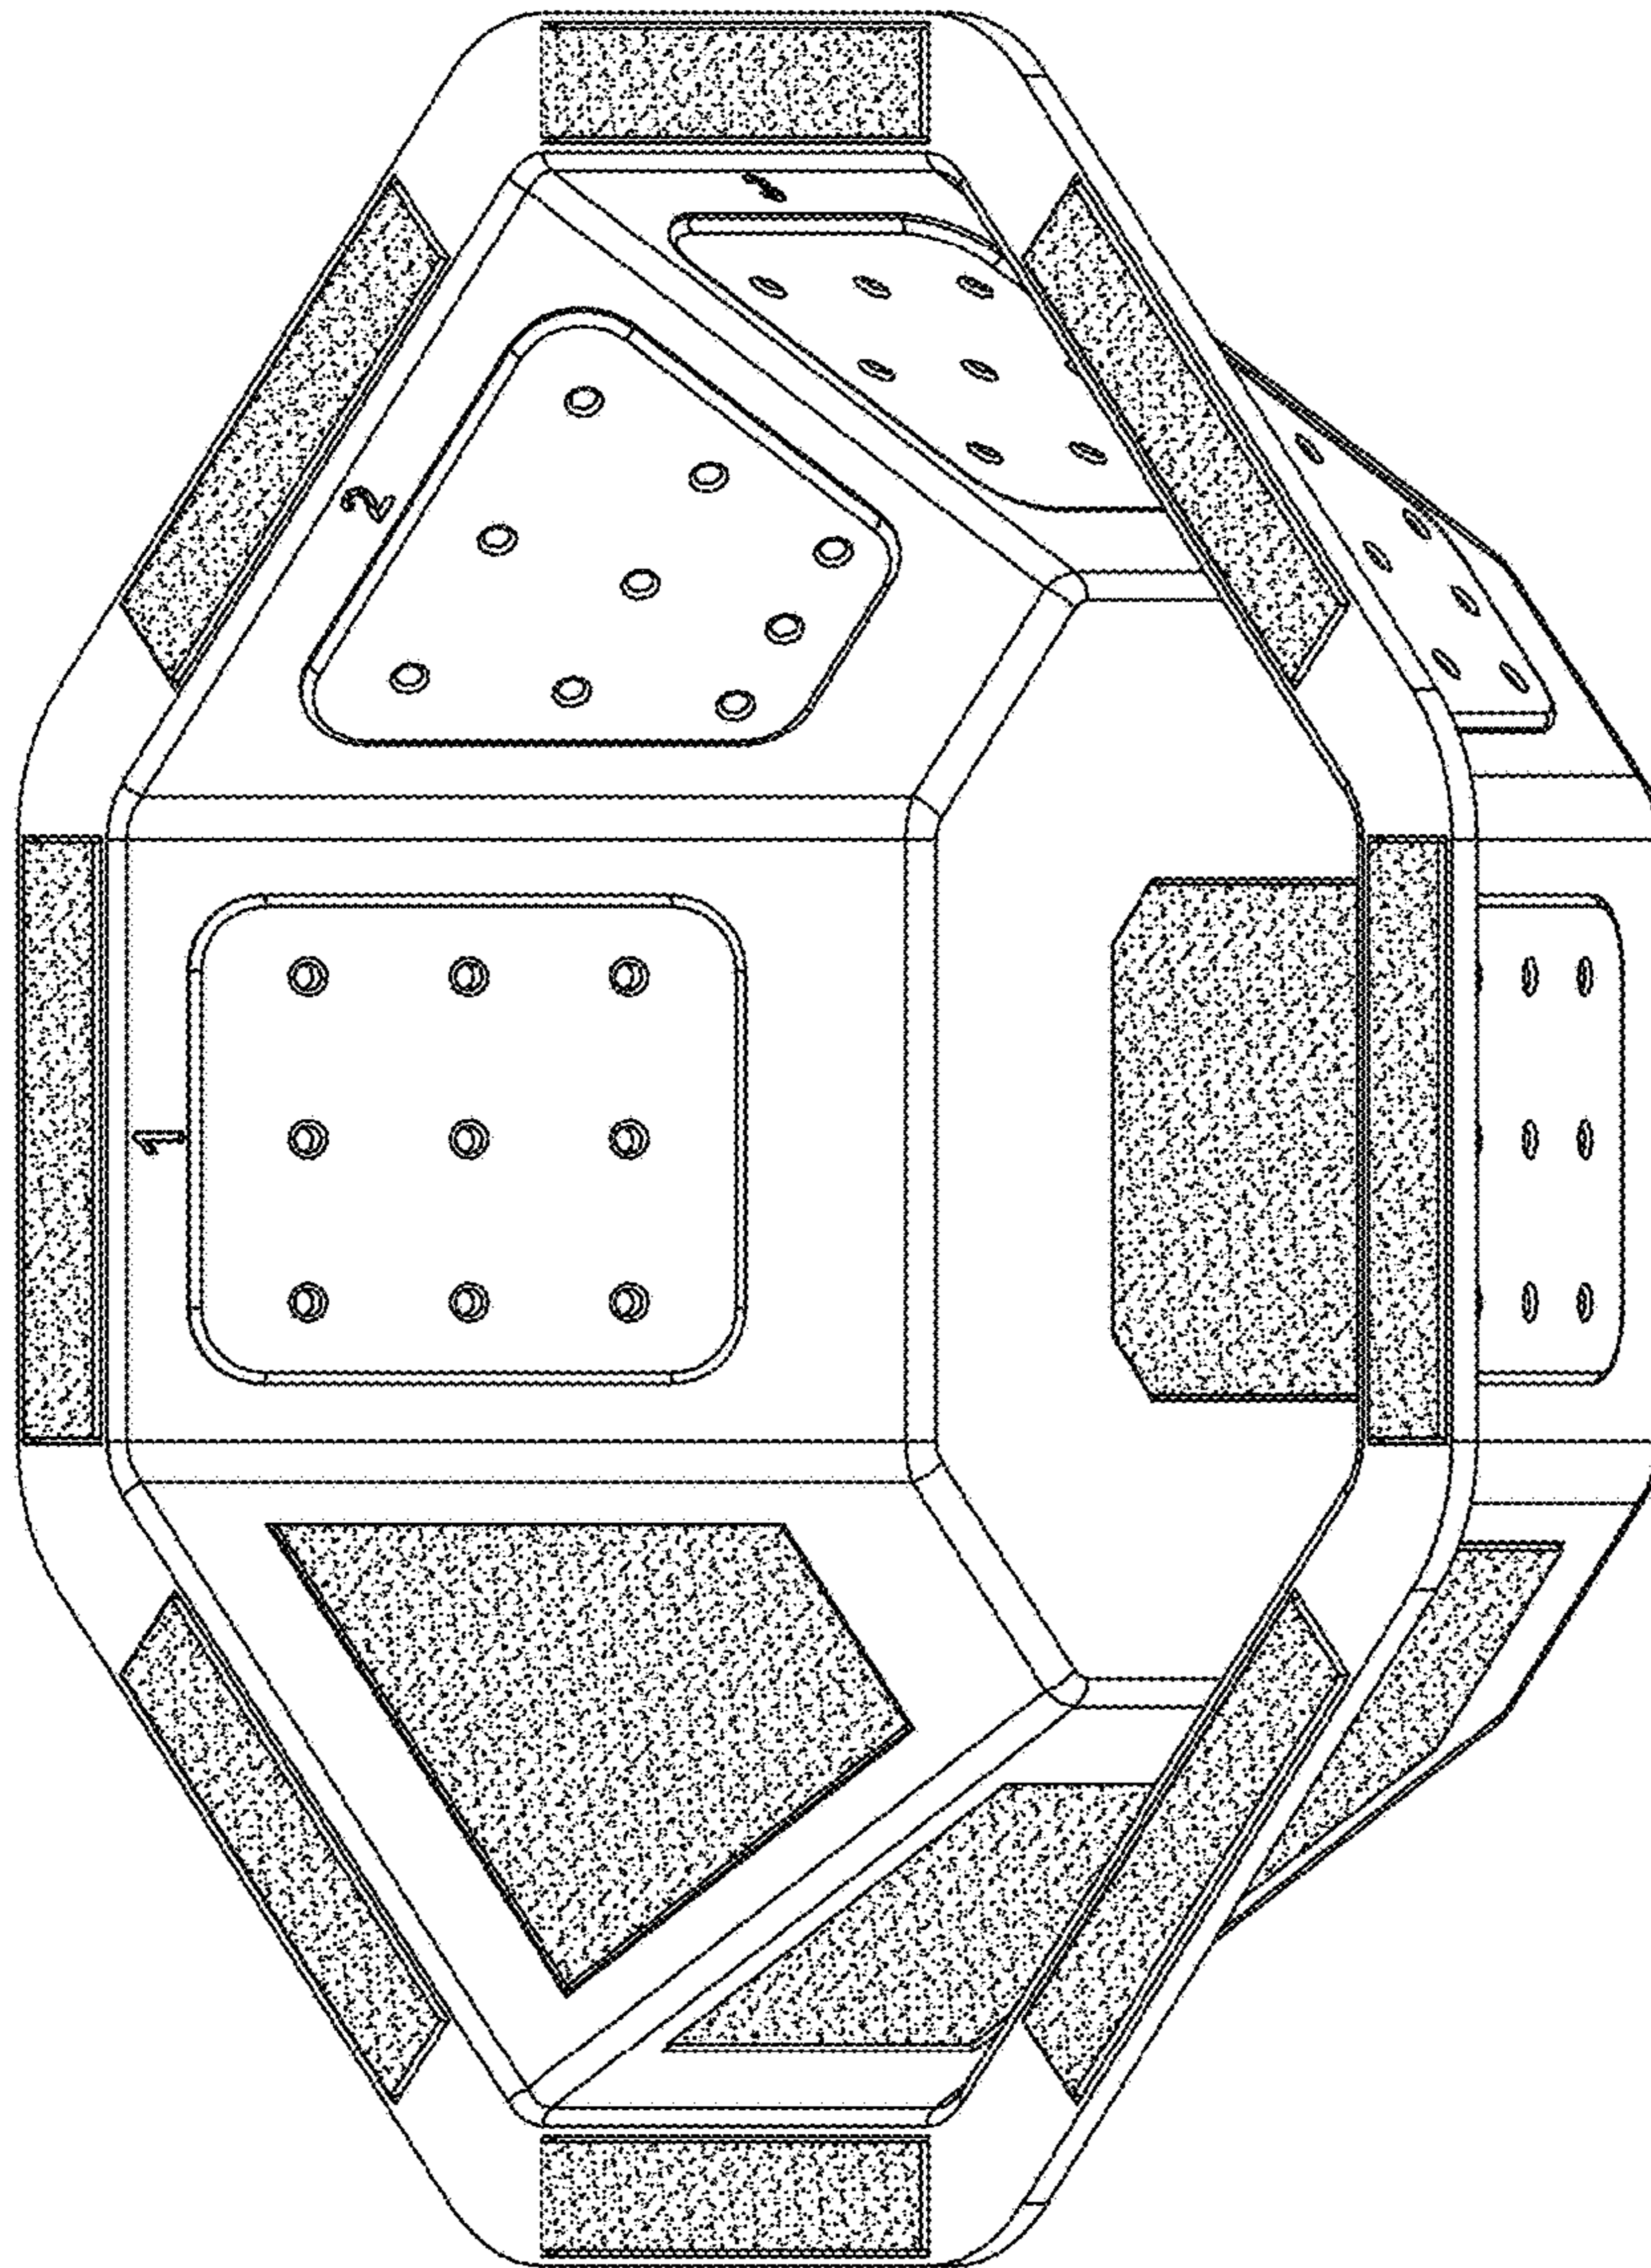


FIG. 1

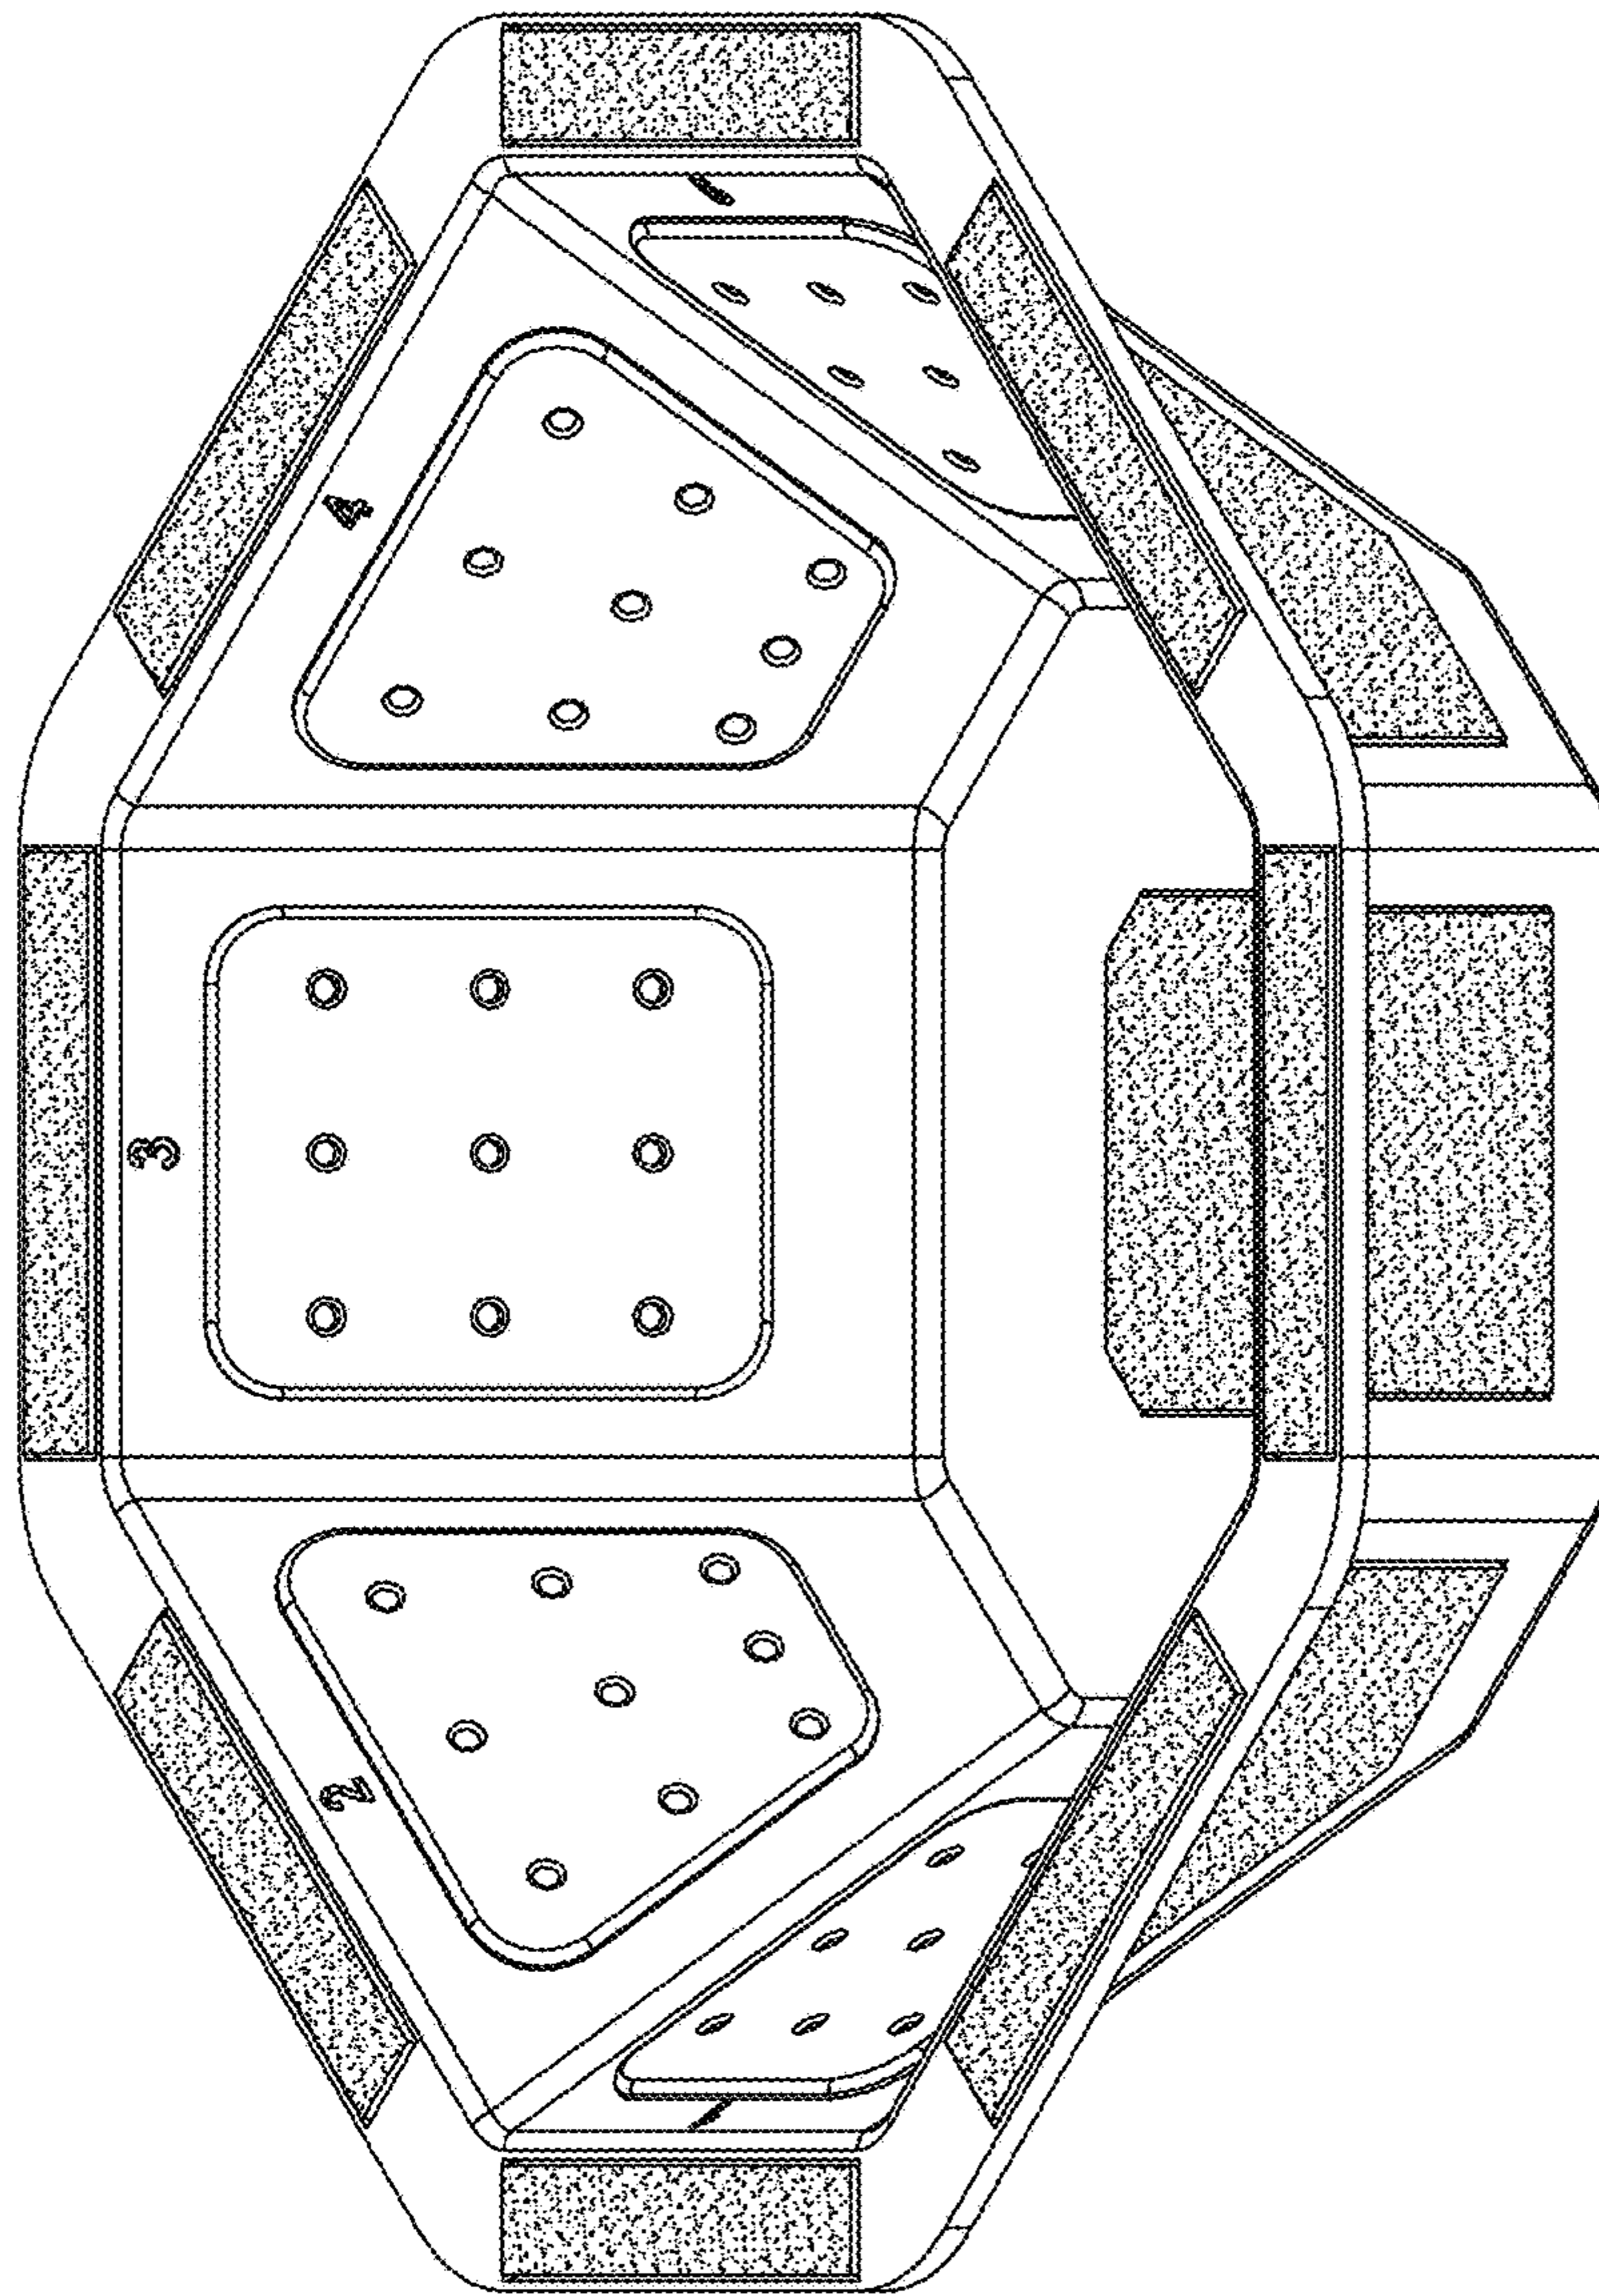


FIG. 2

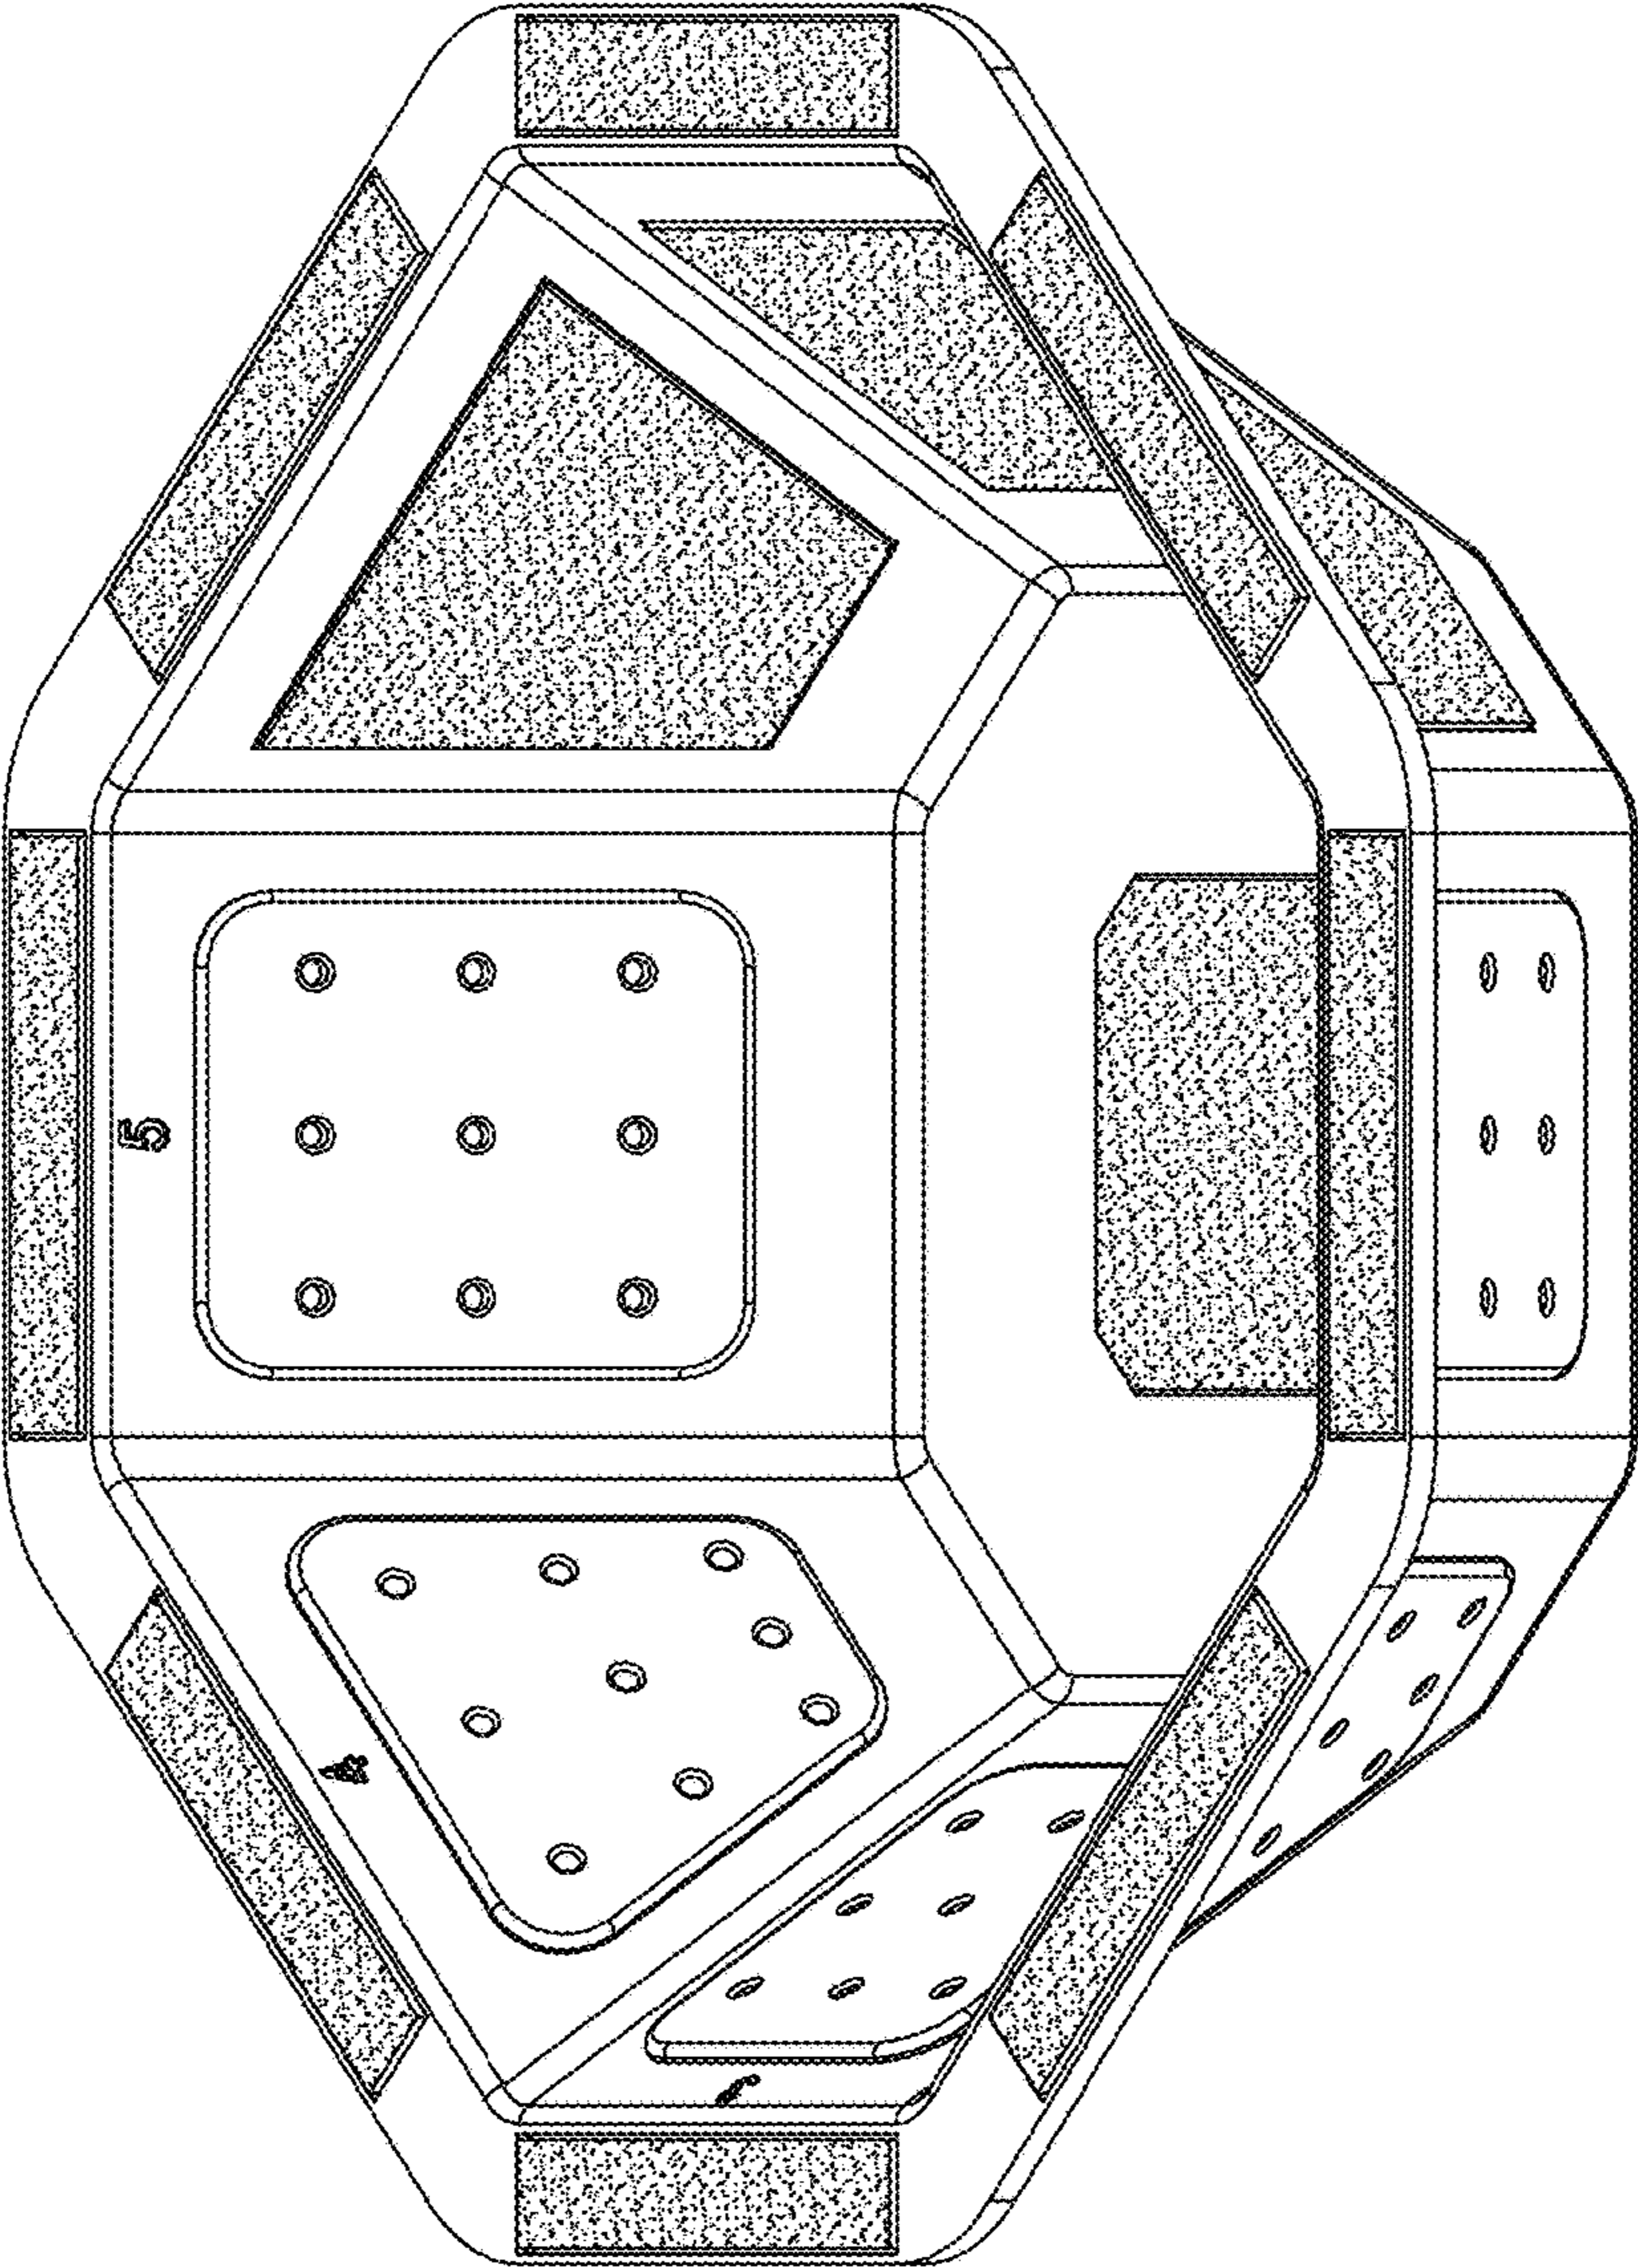


FIG. 3

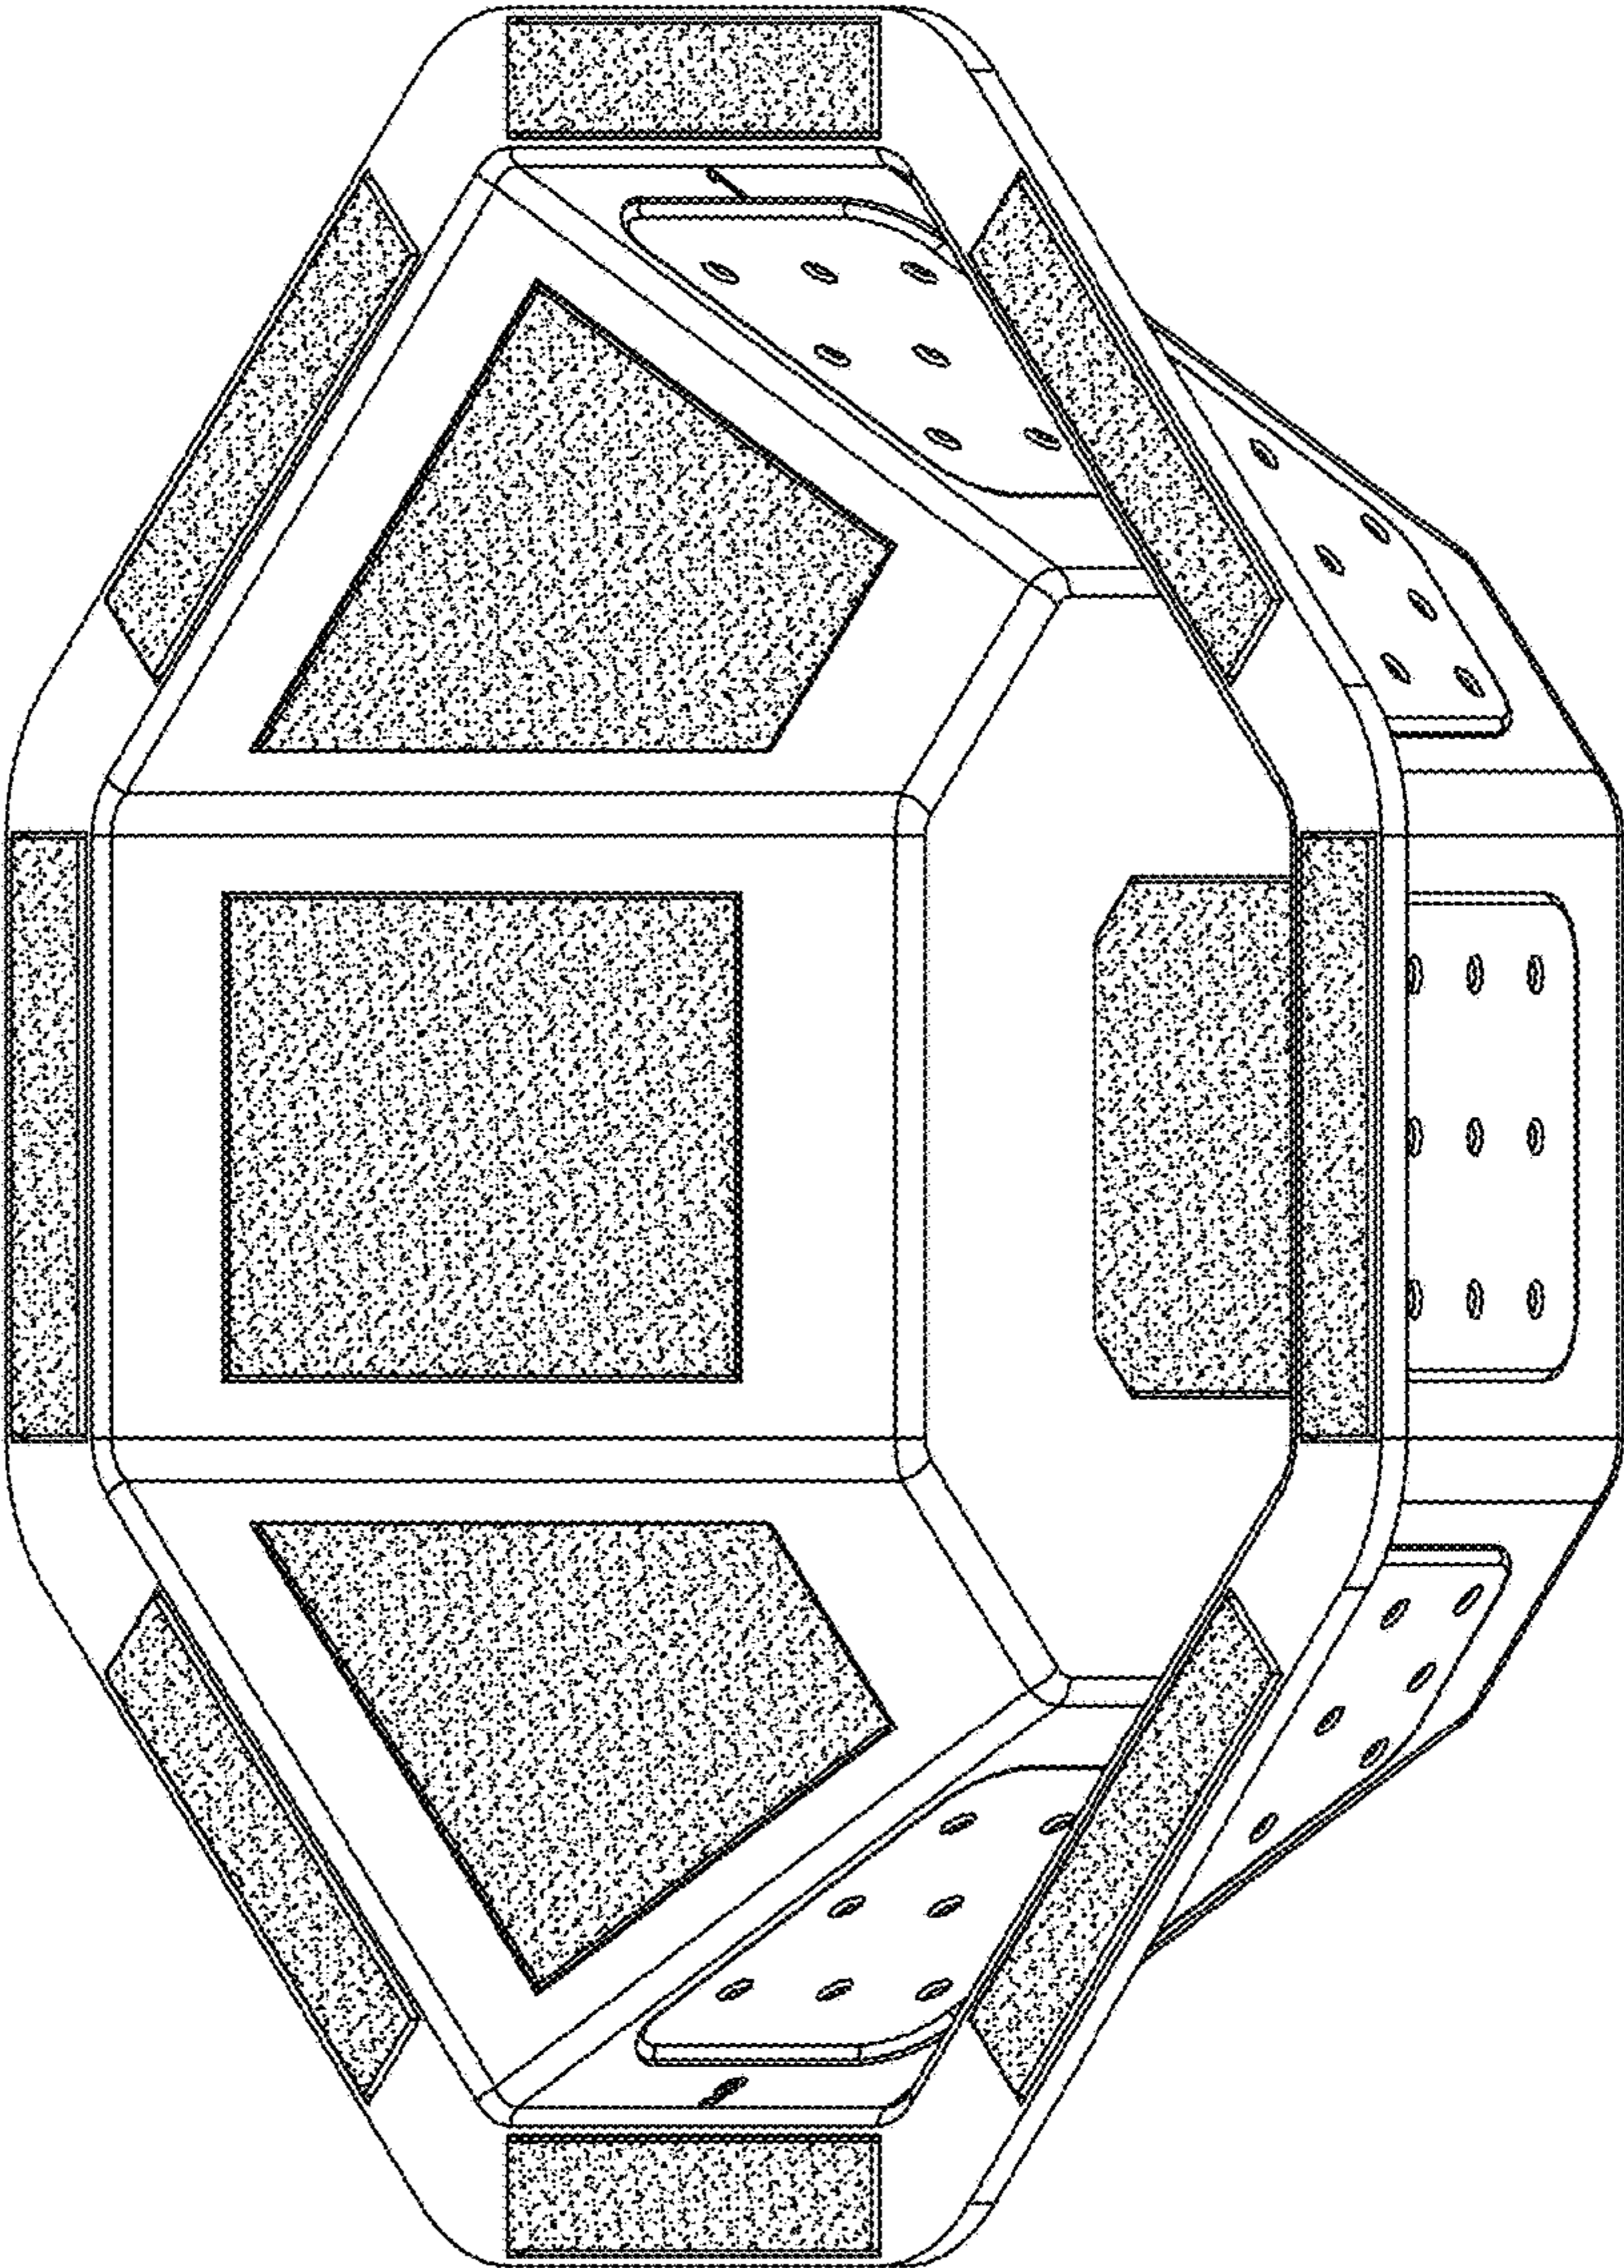


FIG. 4

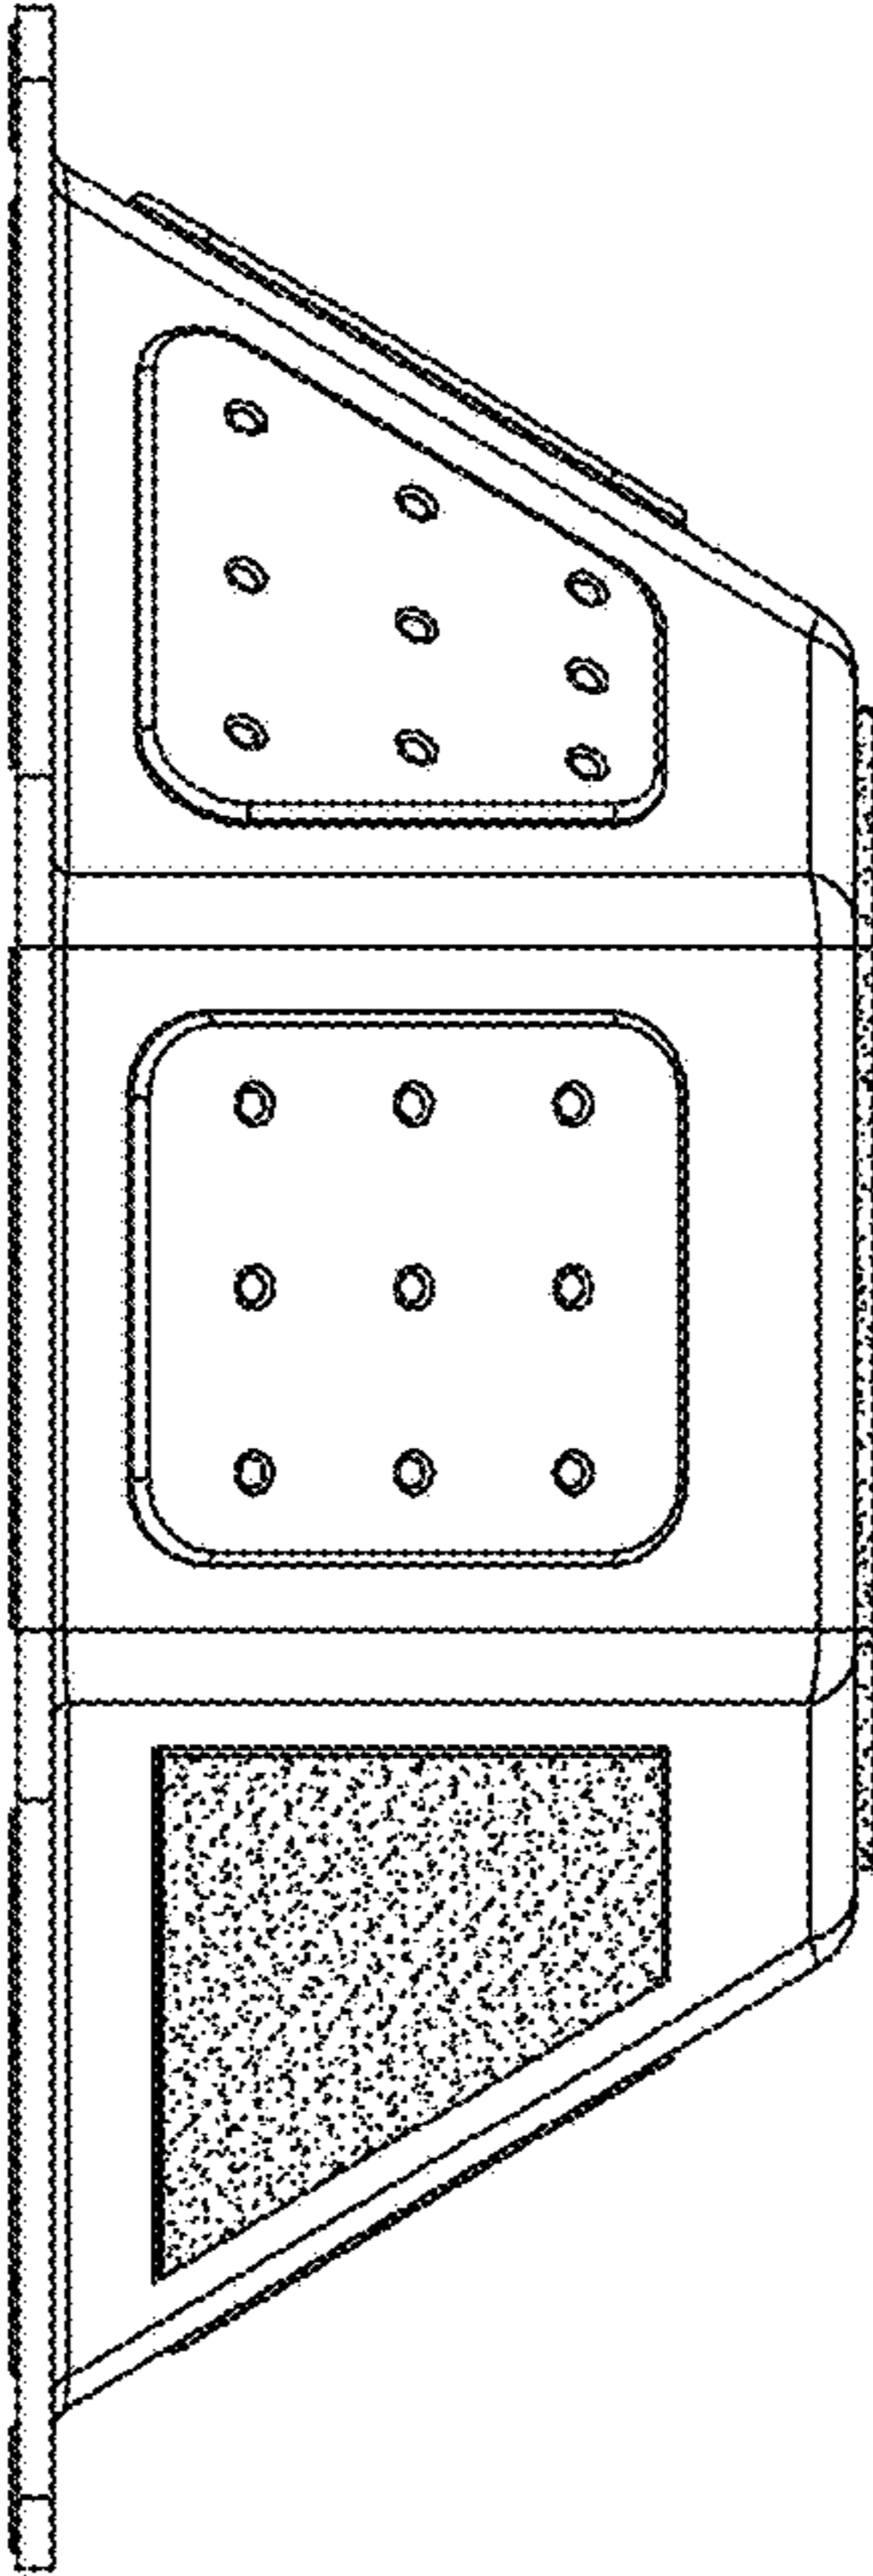


FIG. 5

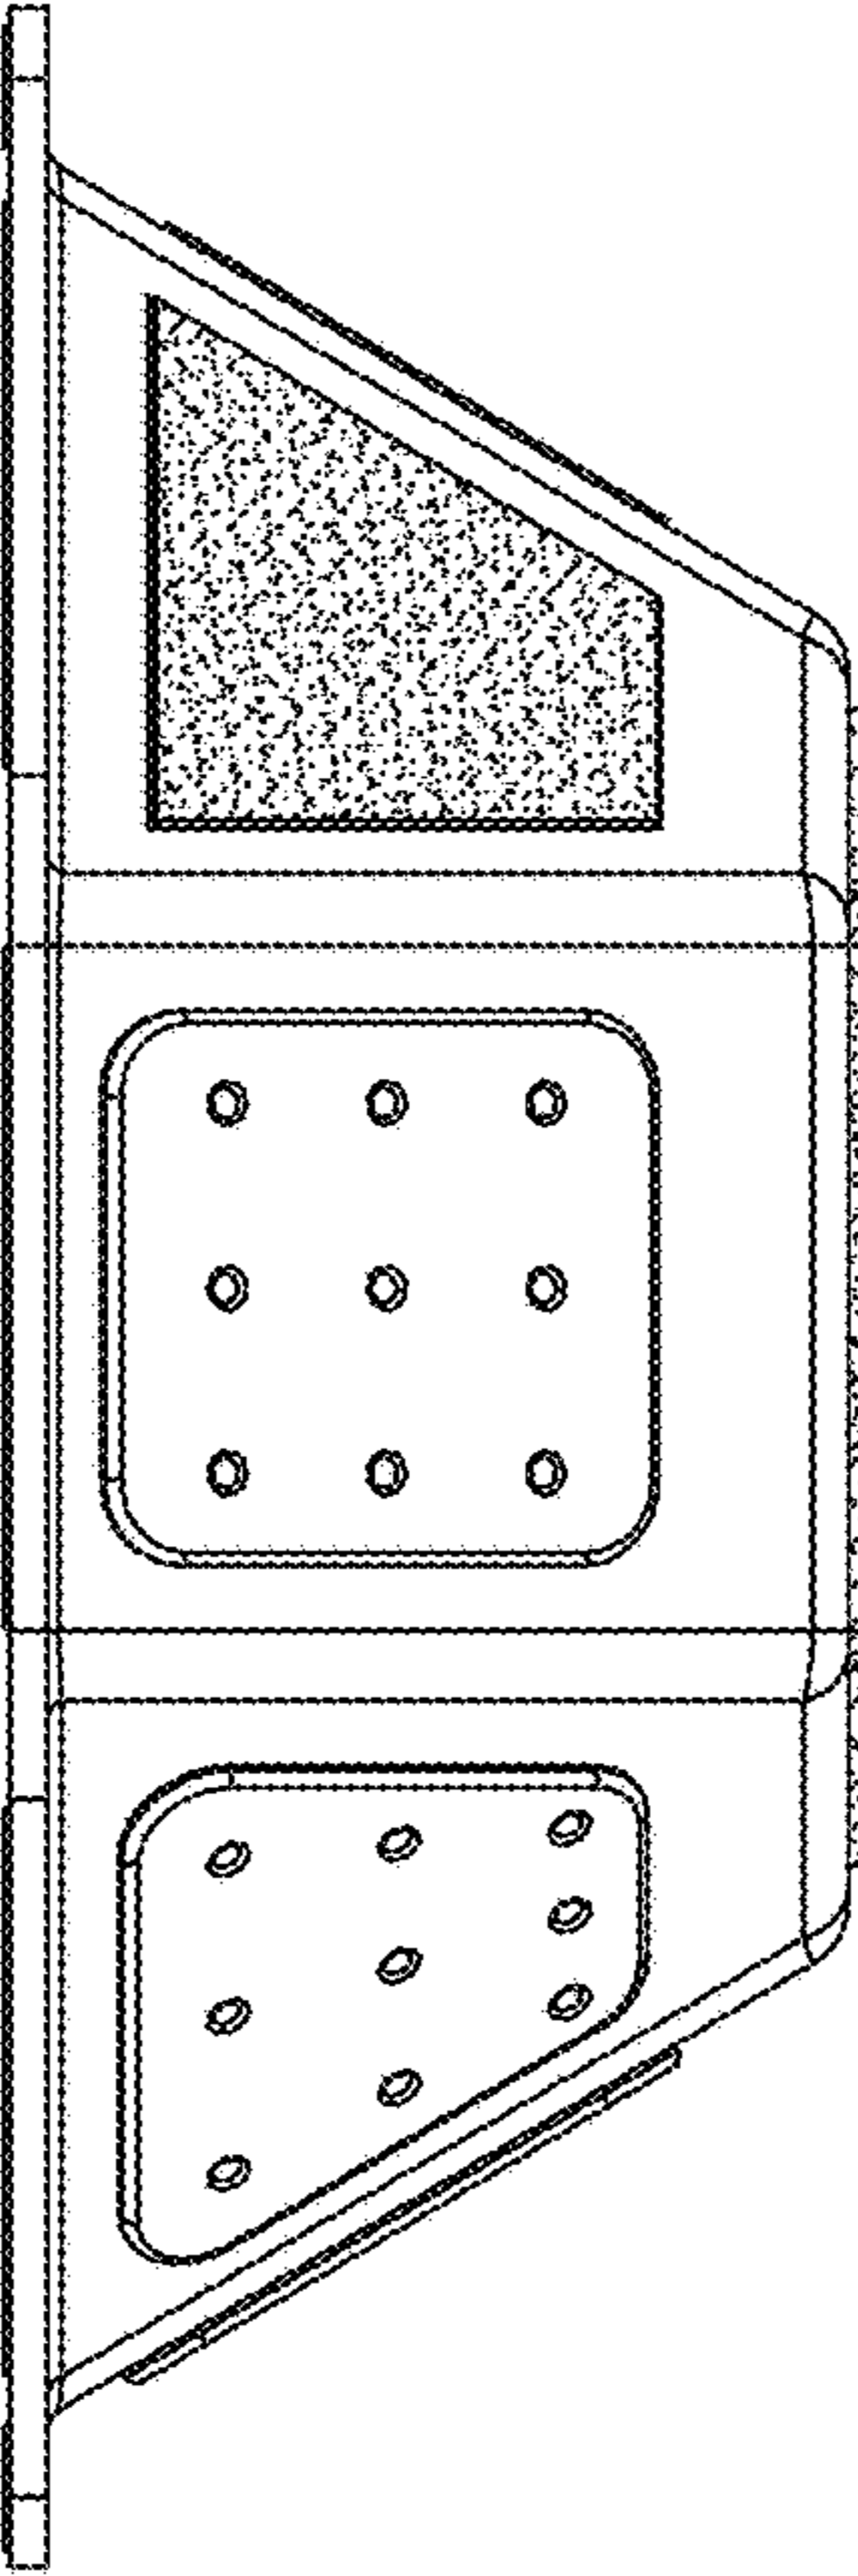


FIG. 6

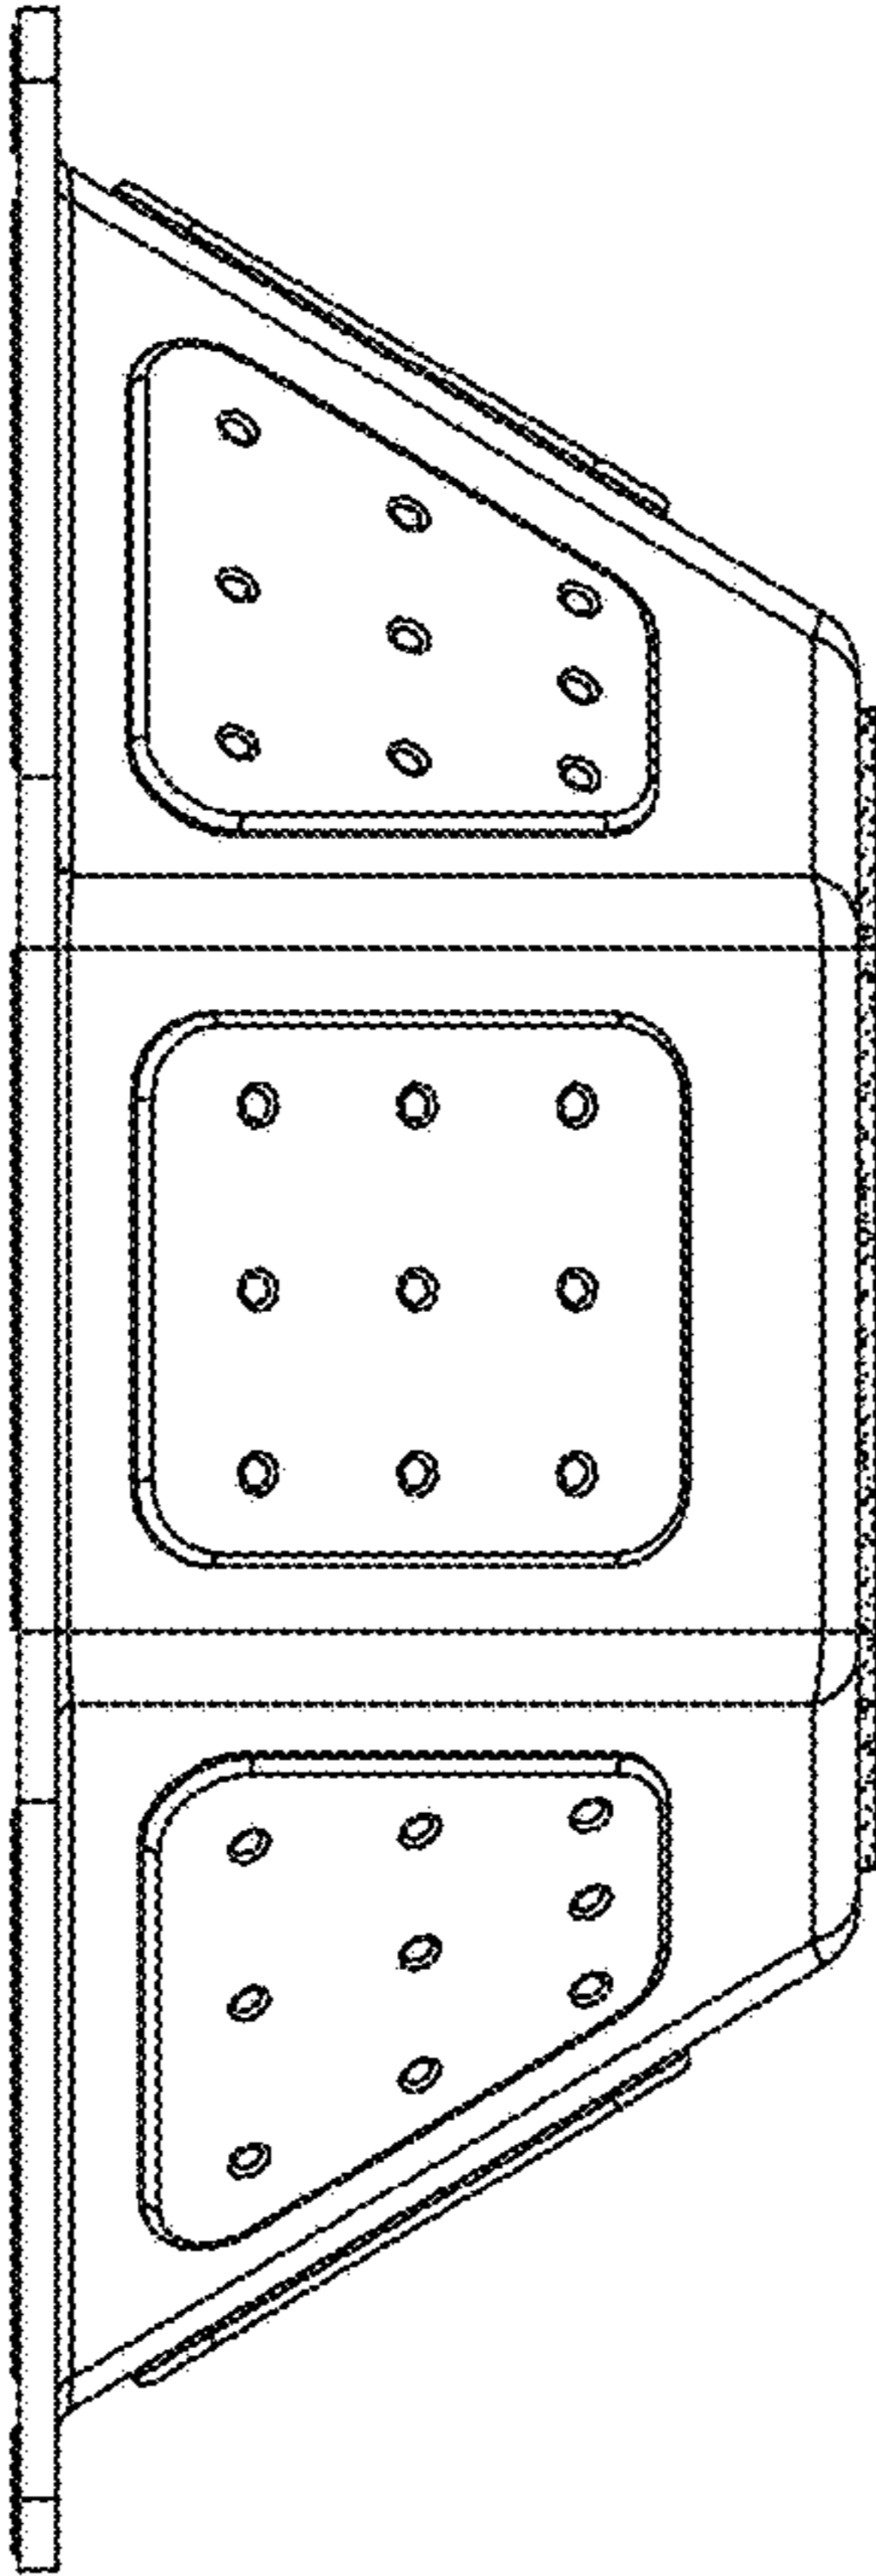


FIG. 7

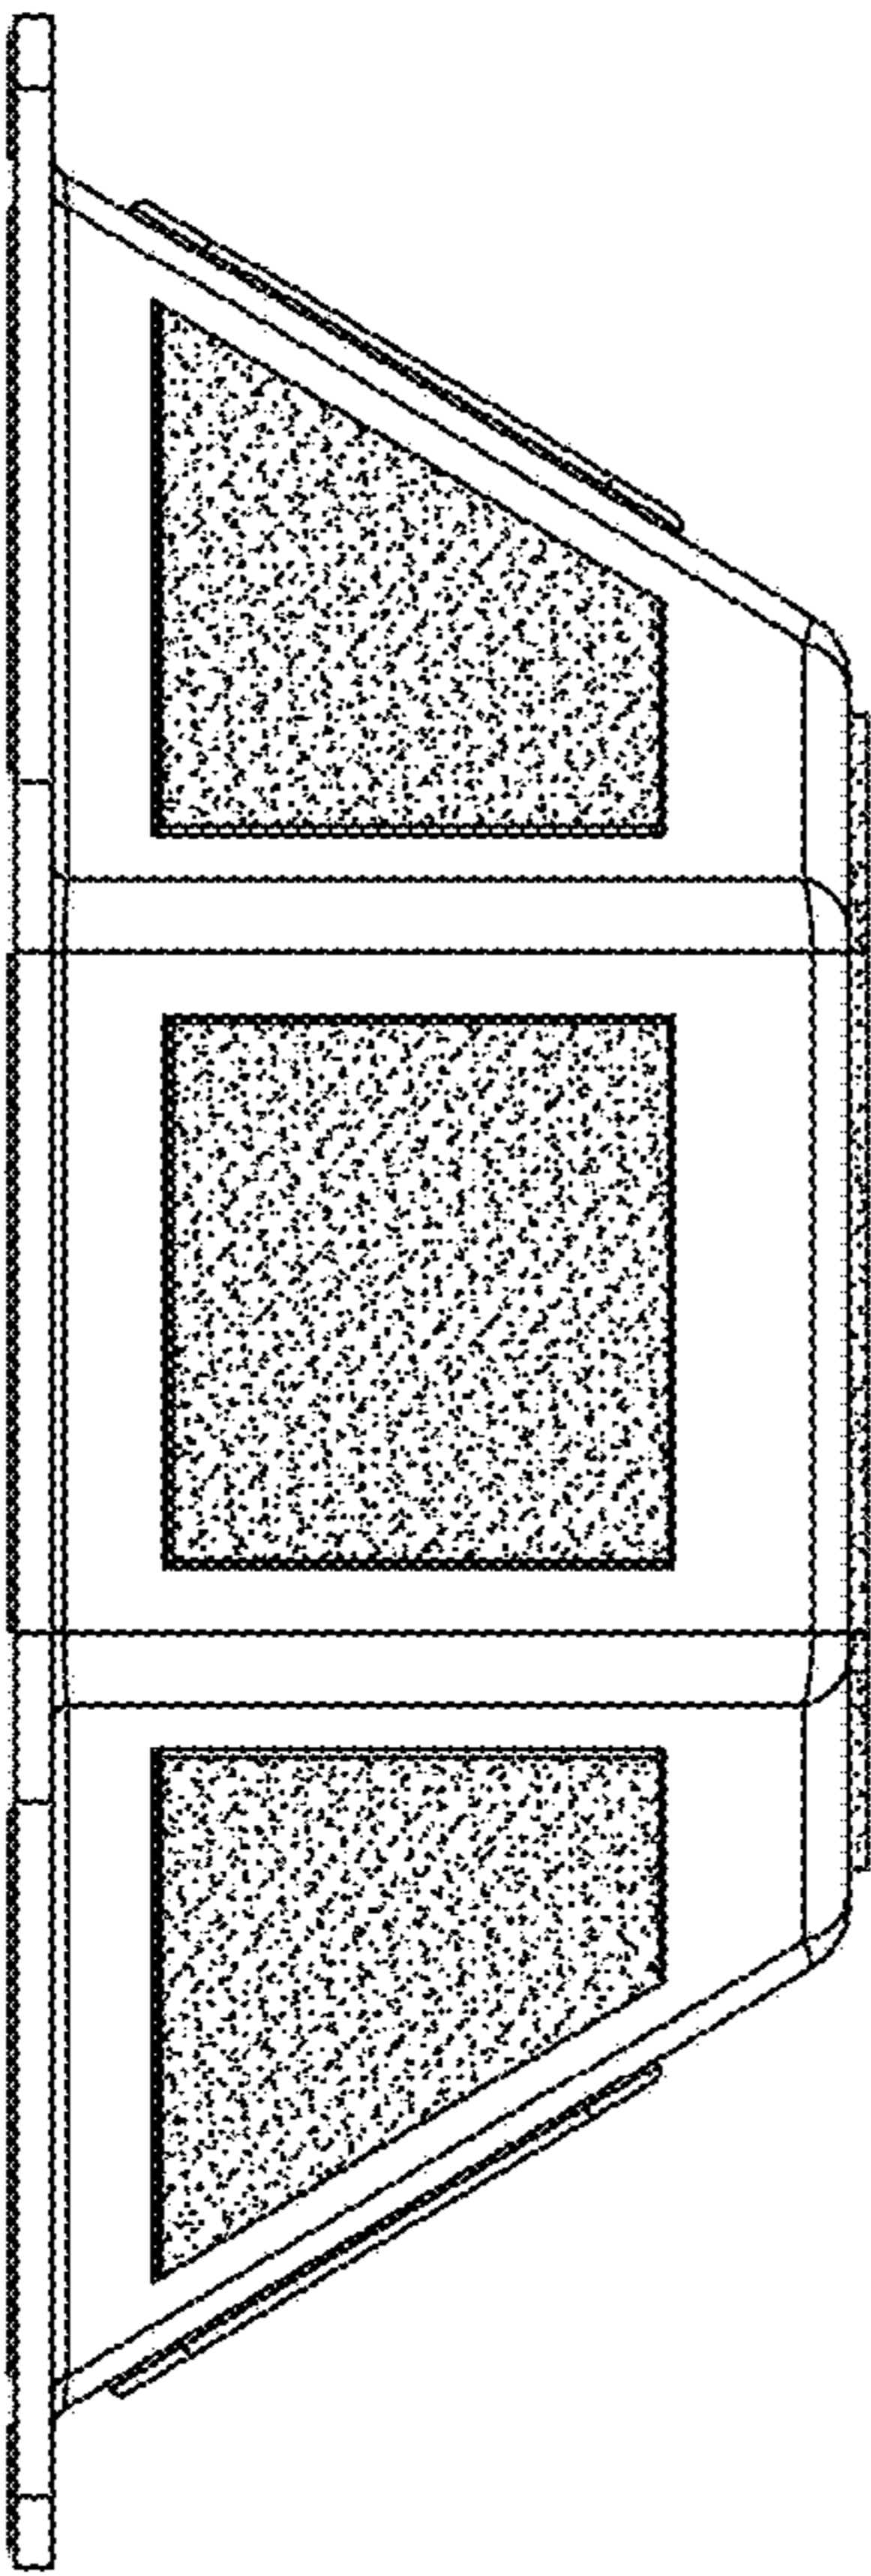


FIG. 8

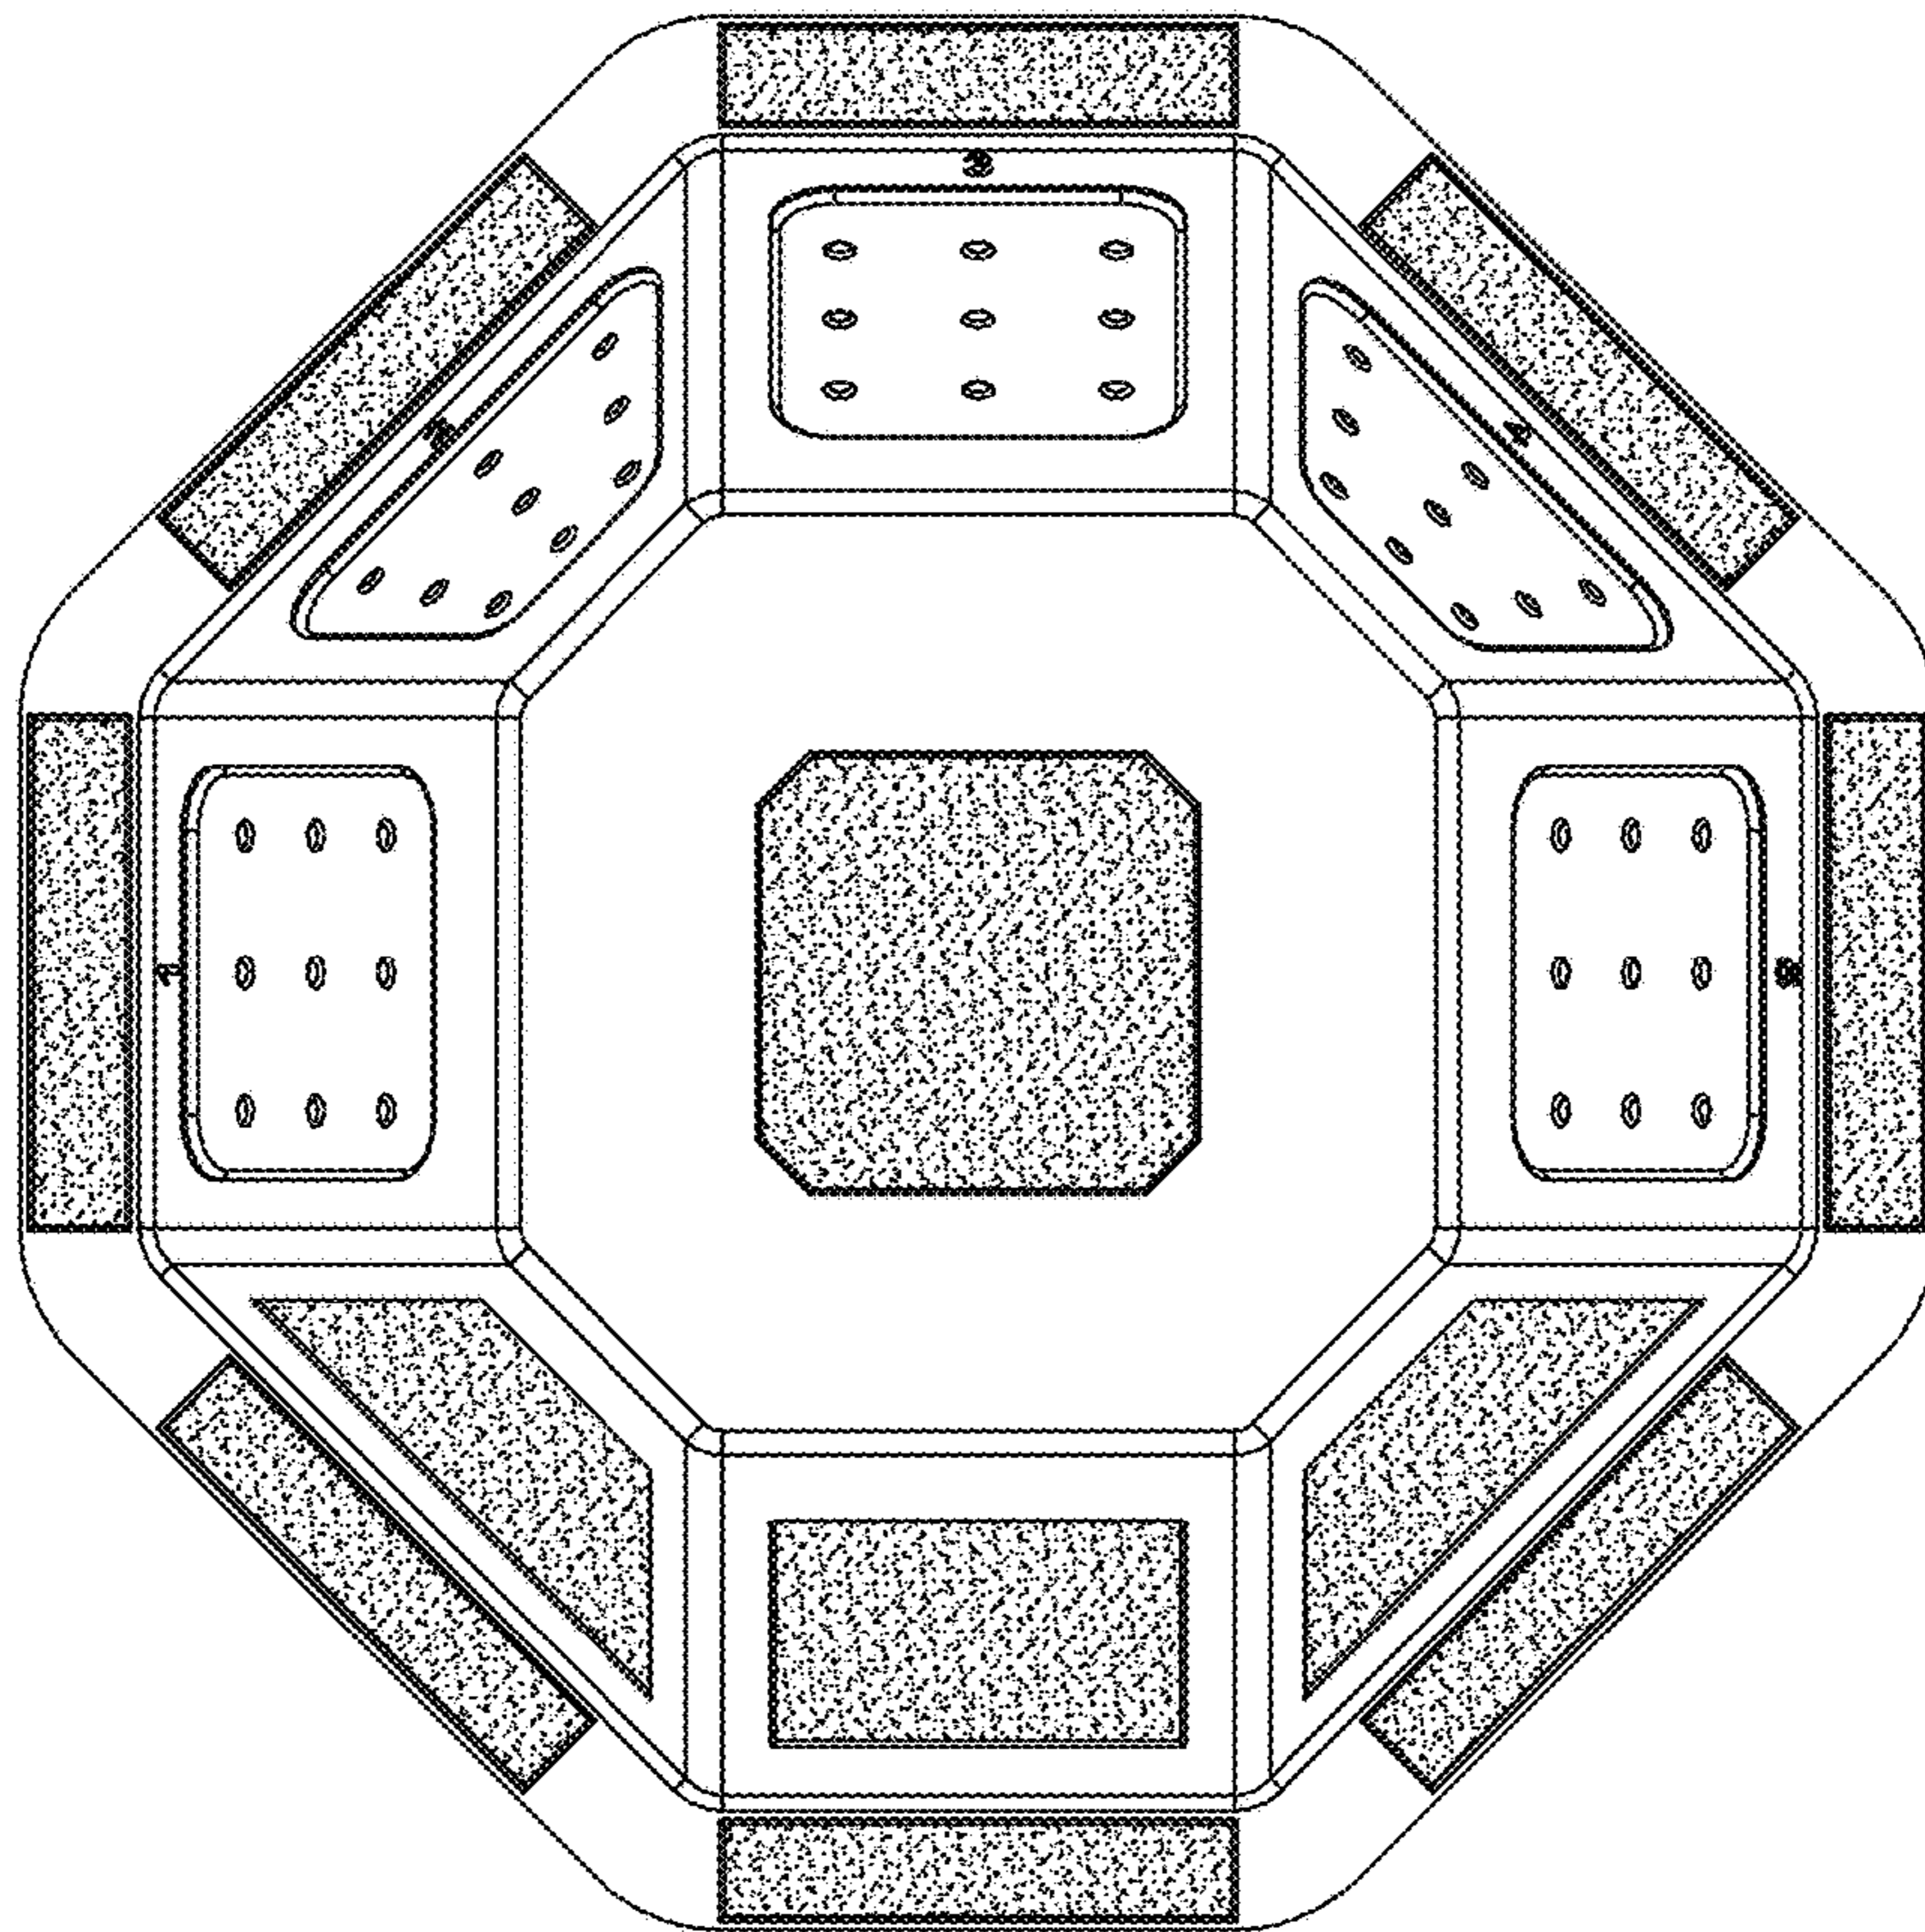


FIG. 9

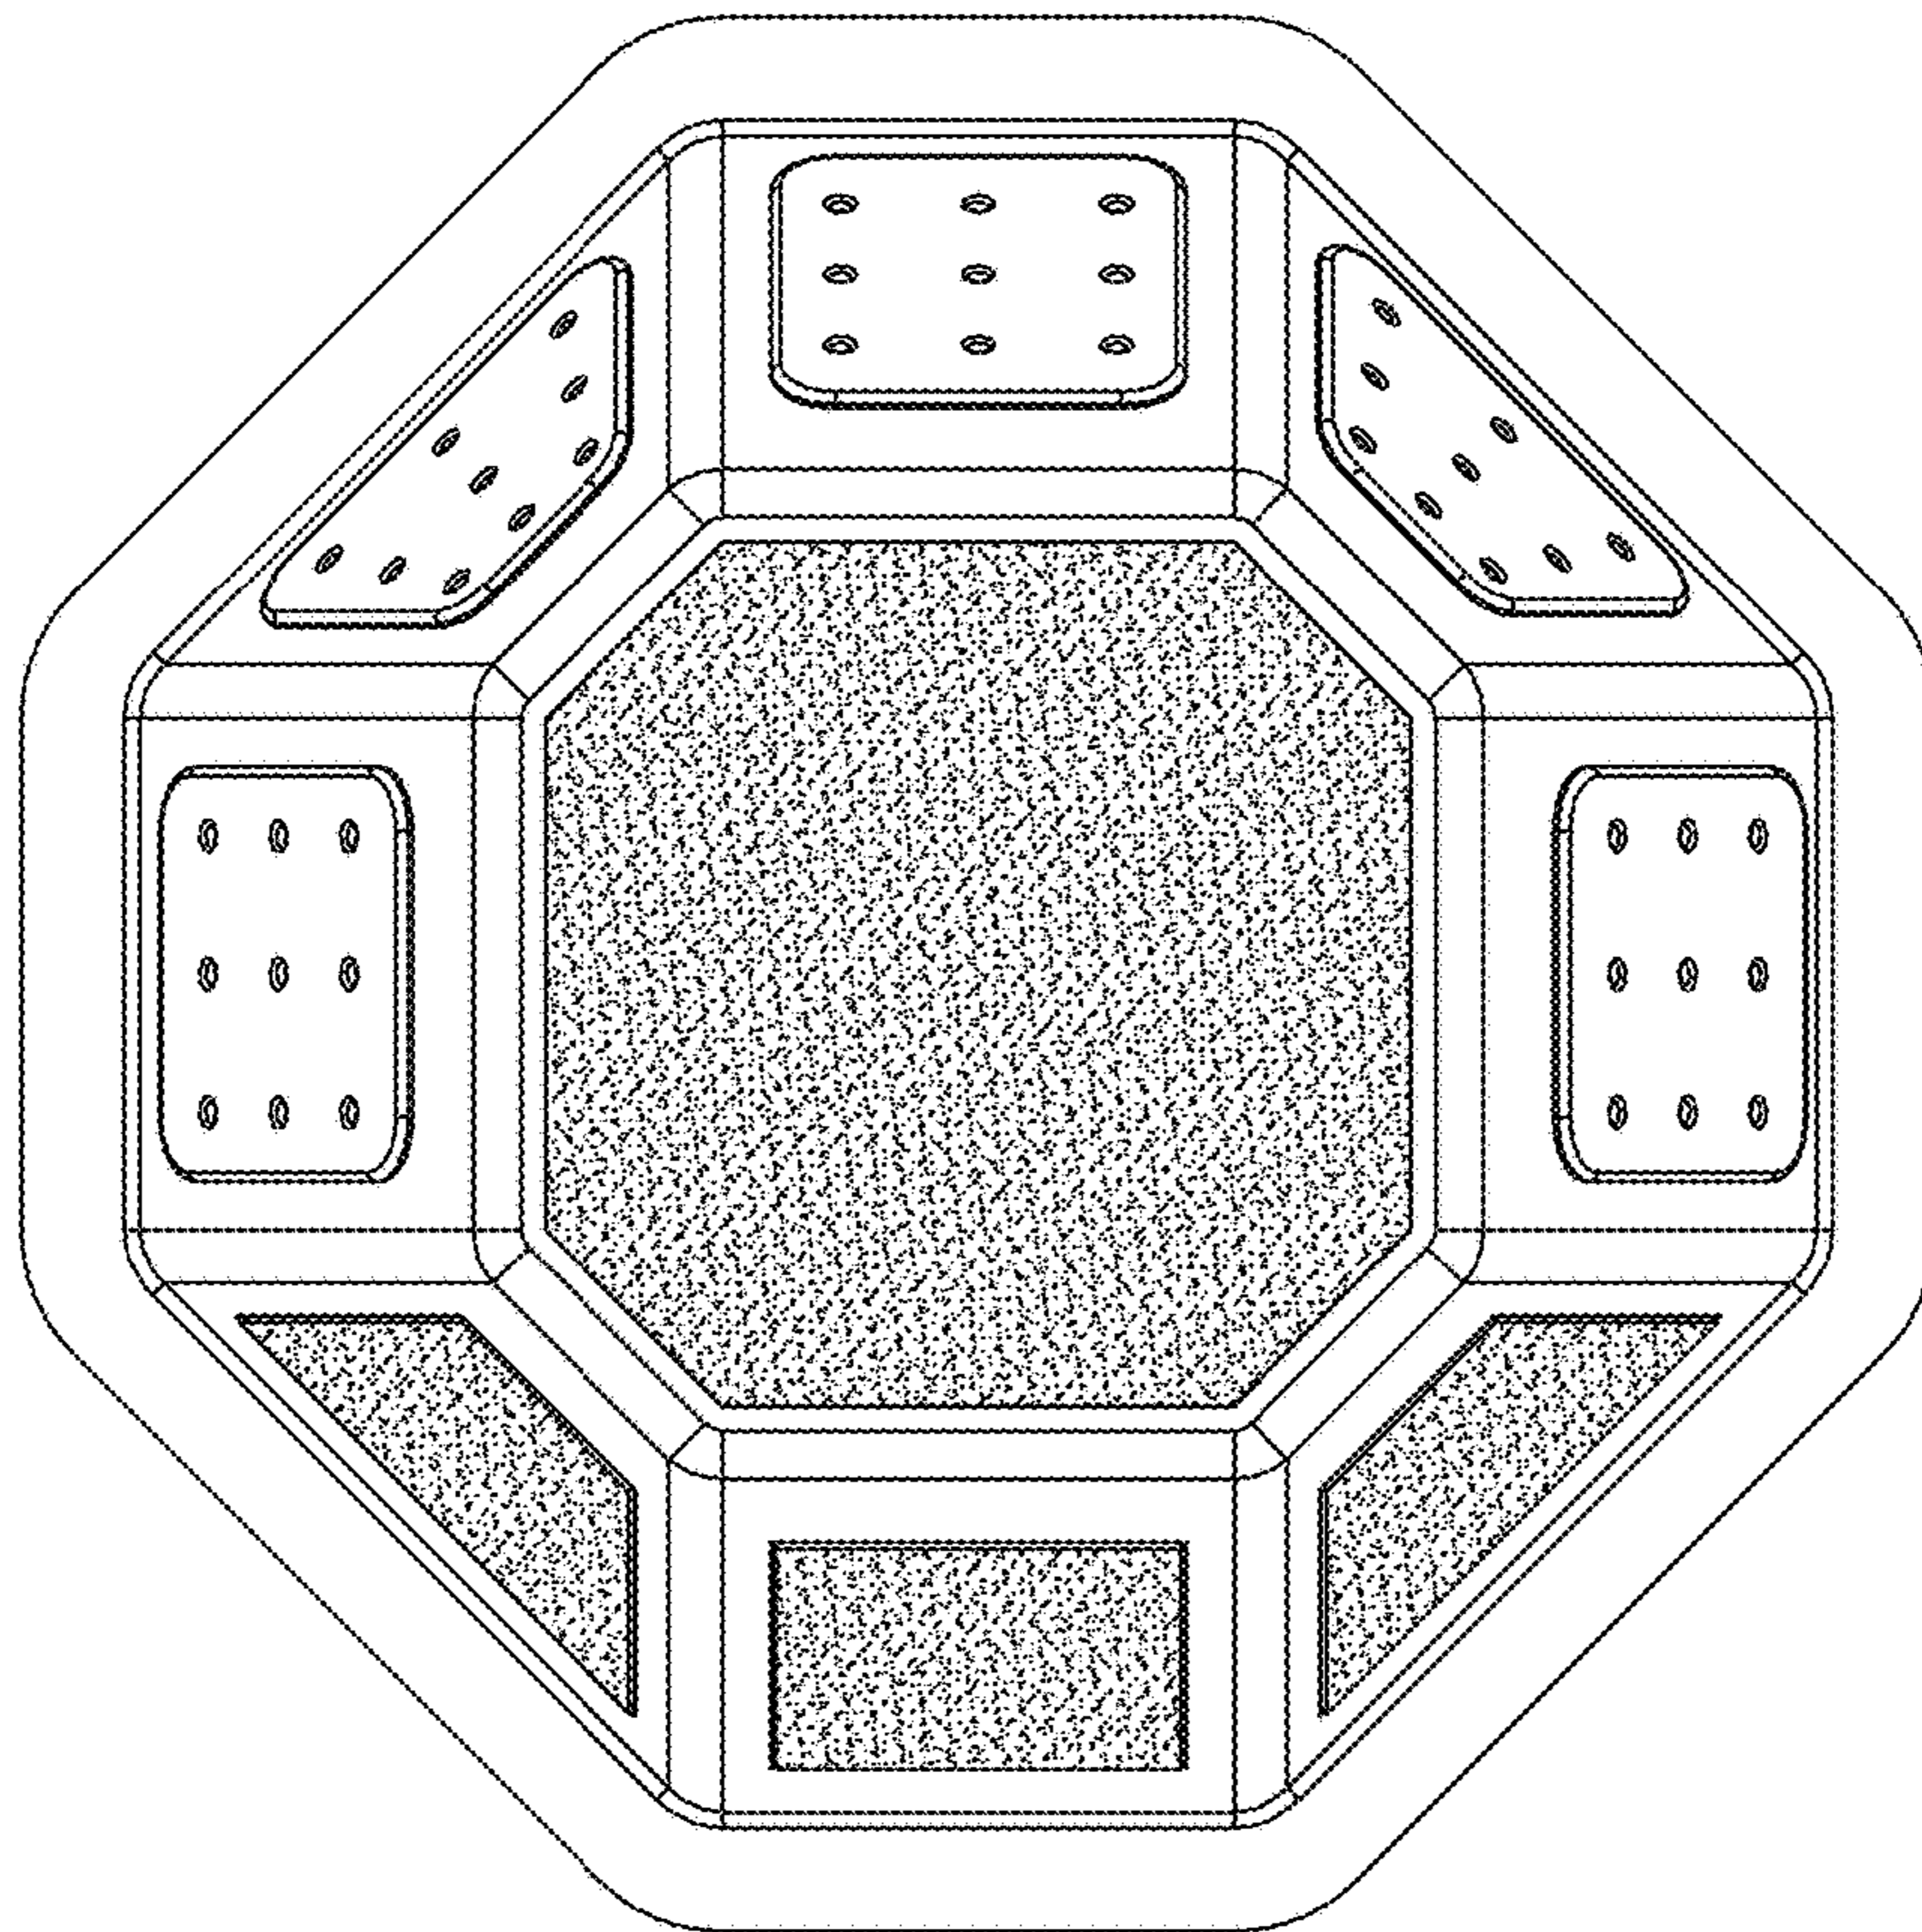


FIG. 10