



US00D852976S

(12) **United States Design Patent**  
**Newberg et al.**

(10) **Patent No.:** **US D852,976 S**  
(45) **Date of Patent:** **\*\* Jul. 2, 2019**

(54) **DIGITAL PATHOLOGY APPARATUS USER INTERFACE**

(71) Applicant: **Leica Biosystems Imaging, Inc.**, Vista, CA (US)

(72) Inventors: **Nicholas Newberg**, San Marcos, CA (US); **Prentash Djelosevic**, Oceanside, CA (US); **Peyman Najmabadi**, San Diego, CA (US); **Lance Mikus**, San Marcos, CA (US)

(73) Assignee: **LEICA BIOSYSTEMS IMAGING, INC.**, Vista, CA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/631,495**

(22) Filed: **Dec. 29, 2017**

(51) **LOC (11) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/216**

(58) **Field of Classification Search**  
USPC ..... D24/107, 169, 185, 186, 216–219, D24/231–234; D10/81  
CPC ..... G01N 2035/00306; G01N 2035/00326; G01N 2035/00336; G01N 2030/027; G01N 21/76; G01N 1/28; G01N 33/50; G01N 35/025  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D381,749 S \* 7/1997 Lawrence ..... D24/232  
D471,271 S \* 3/2003 Stromberg ..... D24/107

D482,796 S \* 11/2003 Oyama ..... D24/232  
D671,227 S \* 11/2012 Parker ..... D24/216  
D691,732 S \* 10/2013 Shibata ..... D24/216  
D720,079 S \* 12/2014 Oonuma ..... D24/216  
D732,185 S \* 6/2015 Kuechle ..... D24/216  
D742,767 S \* 11/2015 Saga ..... D10/81  
D761,439 S \* 7/2016 Ruiz Robles ..... D24/232  
D835,293 S \* 12/2018 Masuda ..... D24/232  
2015/0226759 A1\* 8/2015 Connolly ..... G01N 35/109  
435/287.3

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Procopio, Cory, Hargreaves & Savitch LLP


(57) **CLAIM**

The ornamental design for a digital pathology apparatus user interface, as shown and described.

**DESCRIPTION**

FIG. 1 is a front-right perspective view of a digital pathology apparatus user interface according to the present invention; FIG. 2 is a front side view thereof; FIG. 3 is a right side view thereof; FIG. 4 is a left side view thereof; and, FIG. 5 is a top side view thereof. All broken lines that represent environmental structure or boundaries form no part of the claimed design. The digital pathology apparatus user interface is intended for use with a slide rack carousel that is not shown in the drawing and forms no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

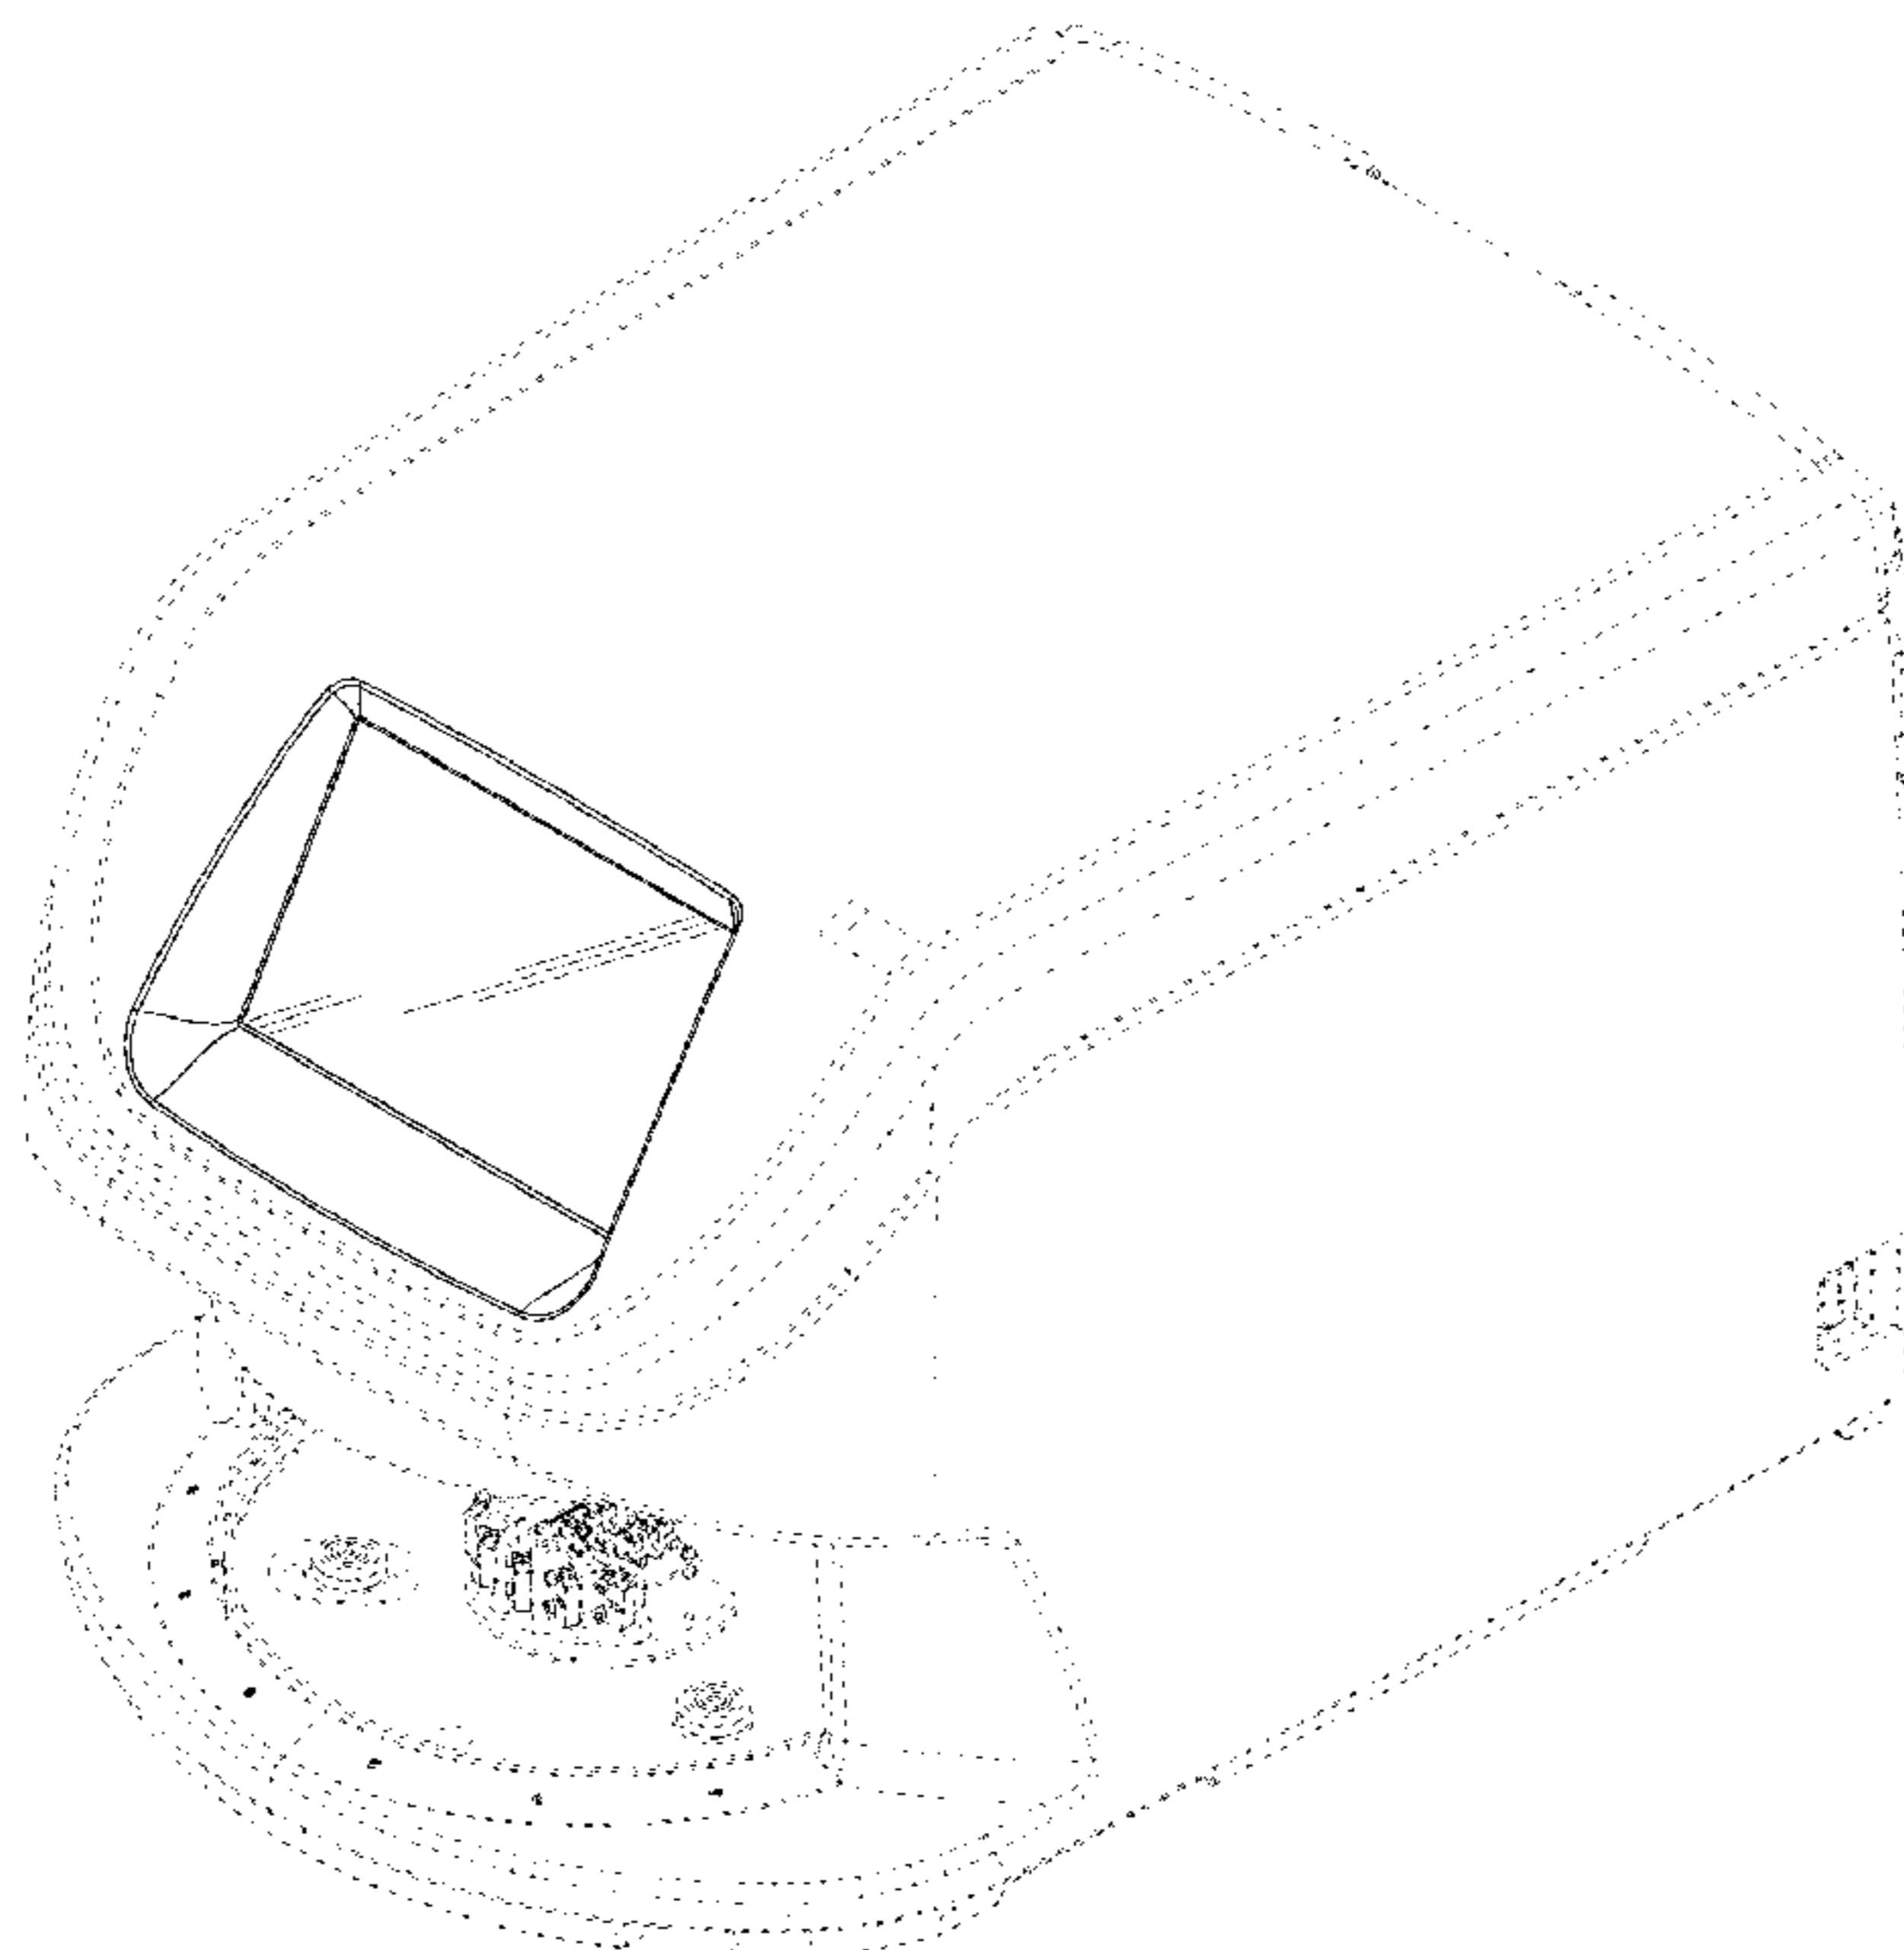

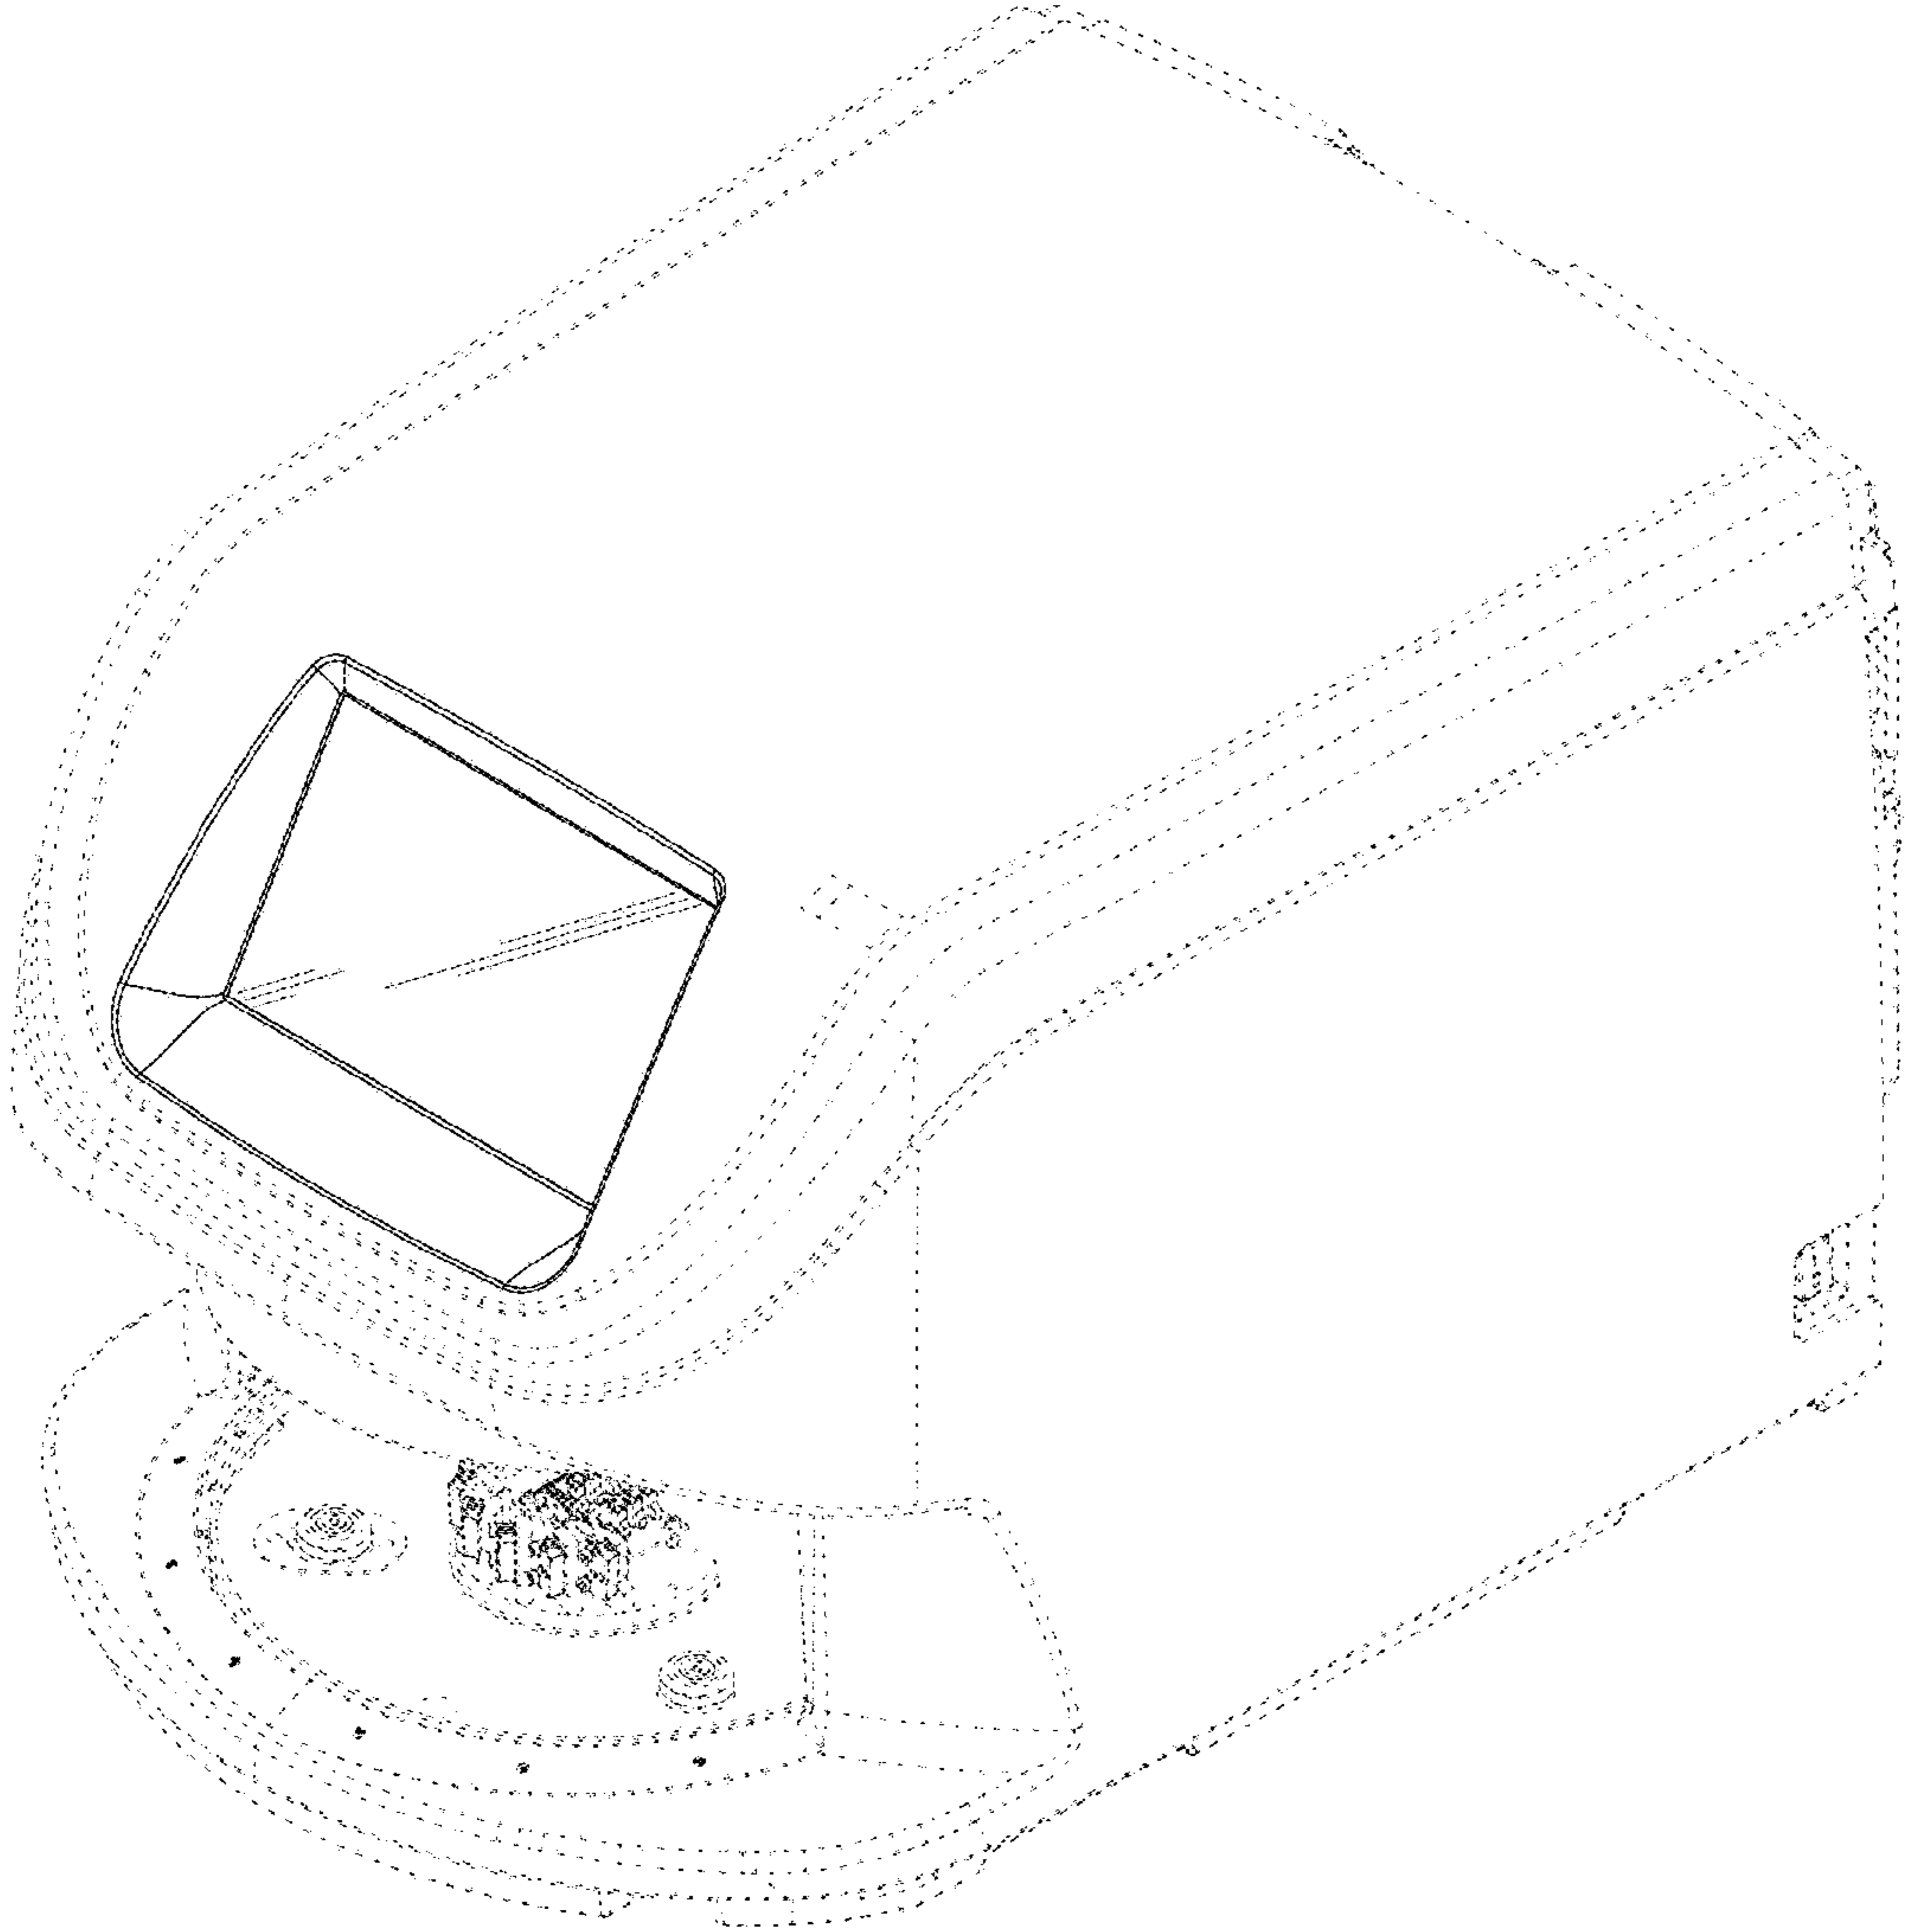


FIG. 1

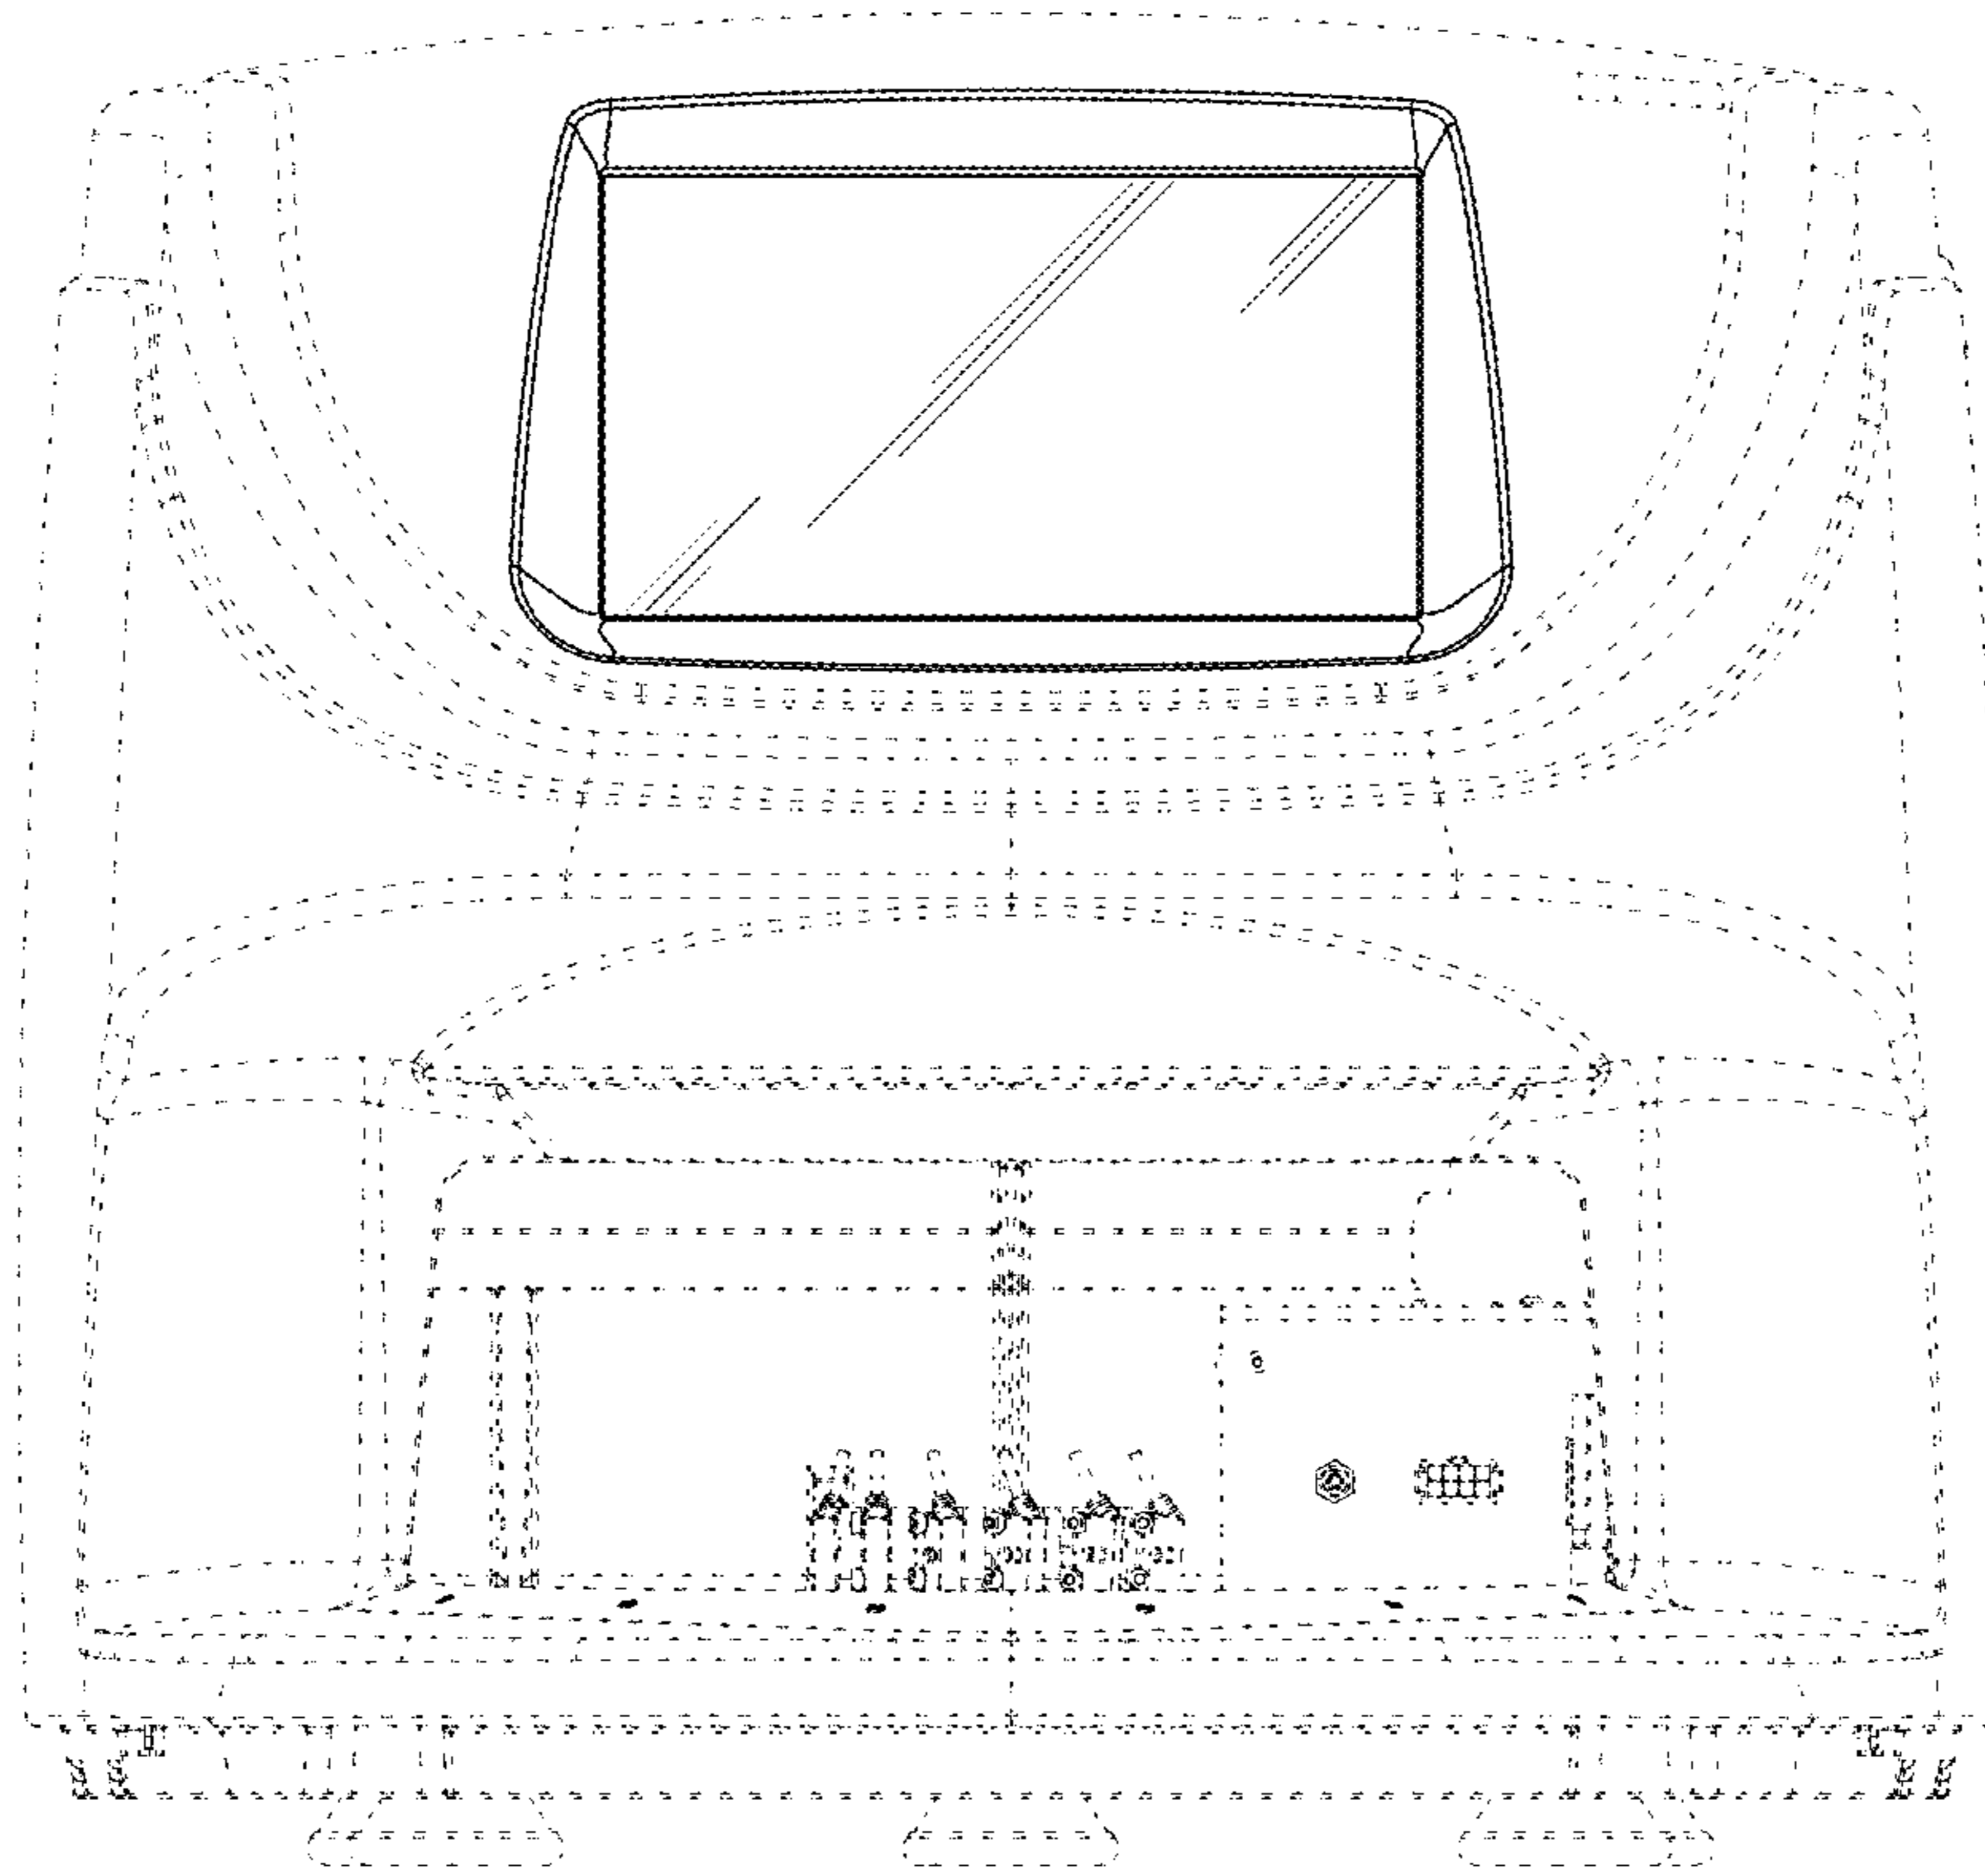


FIG. 2

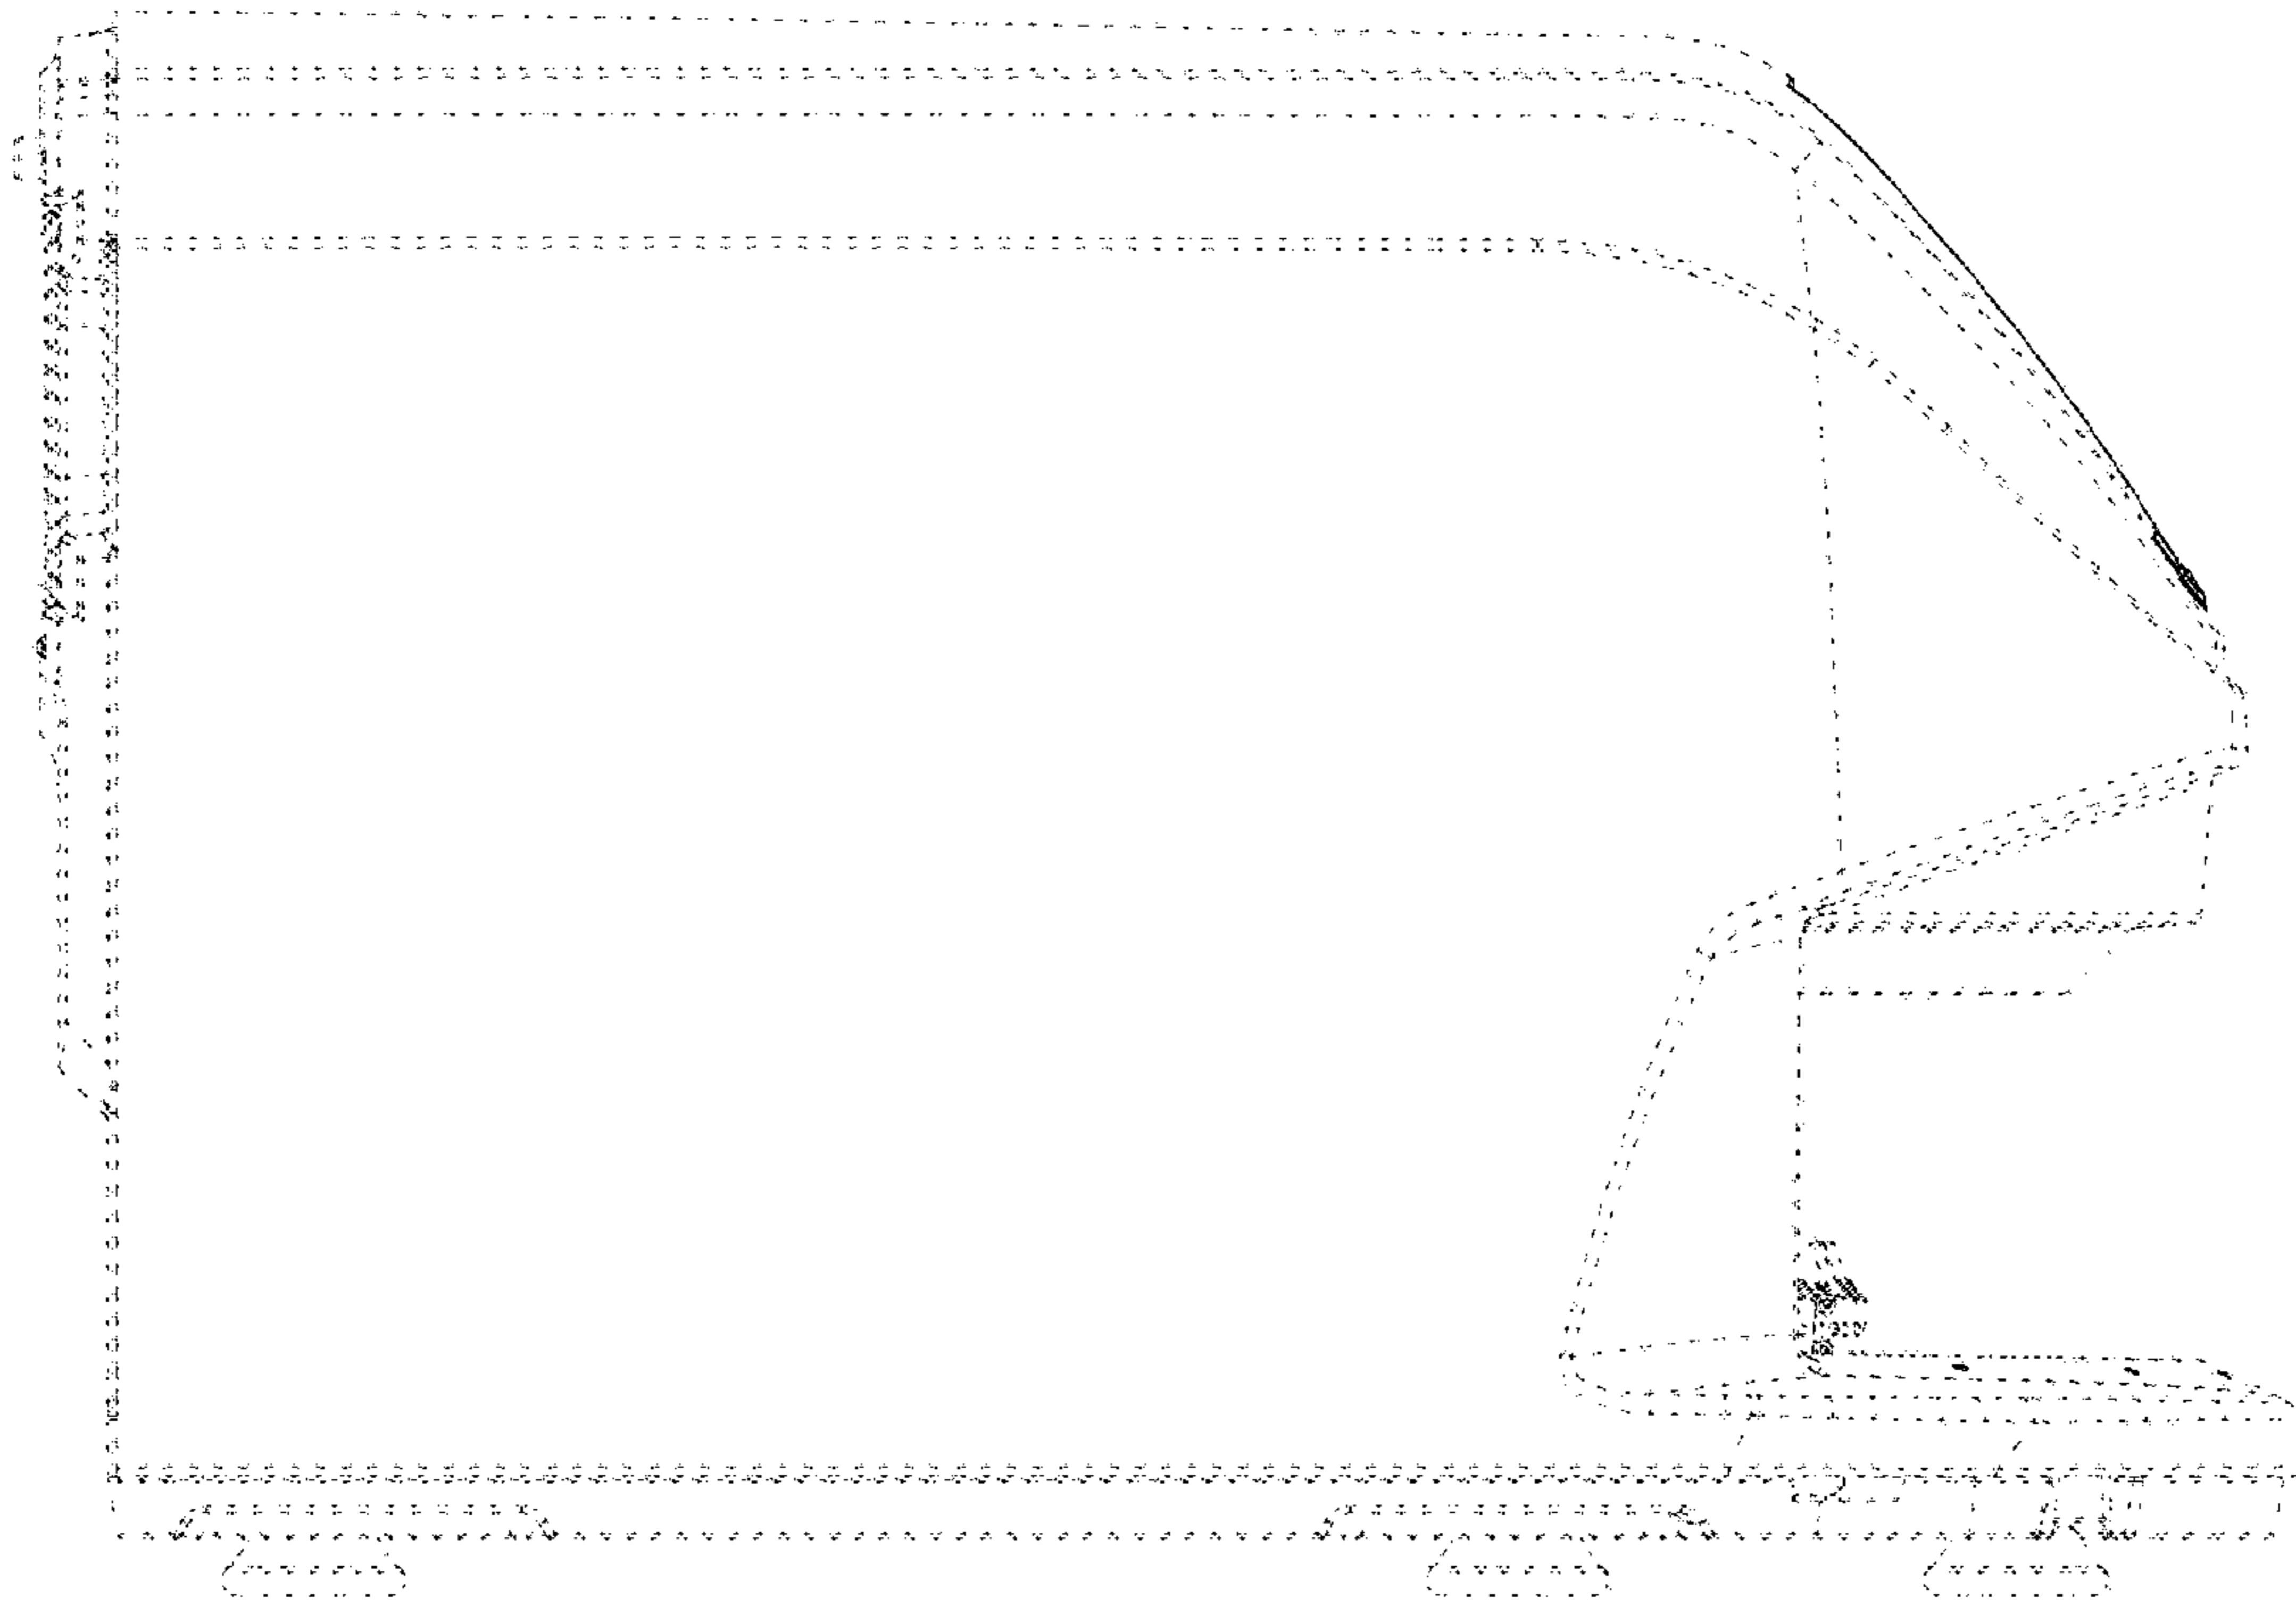


FIG. 3

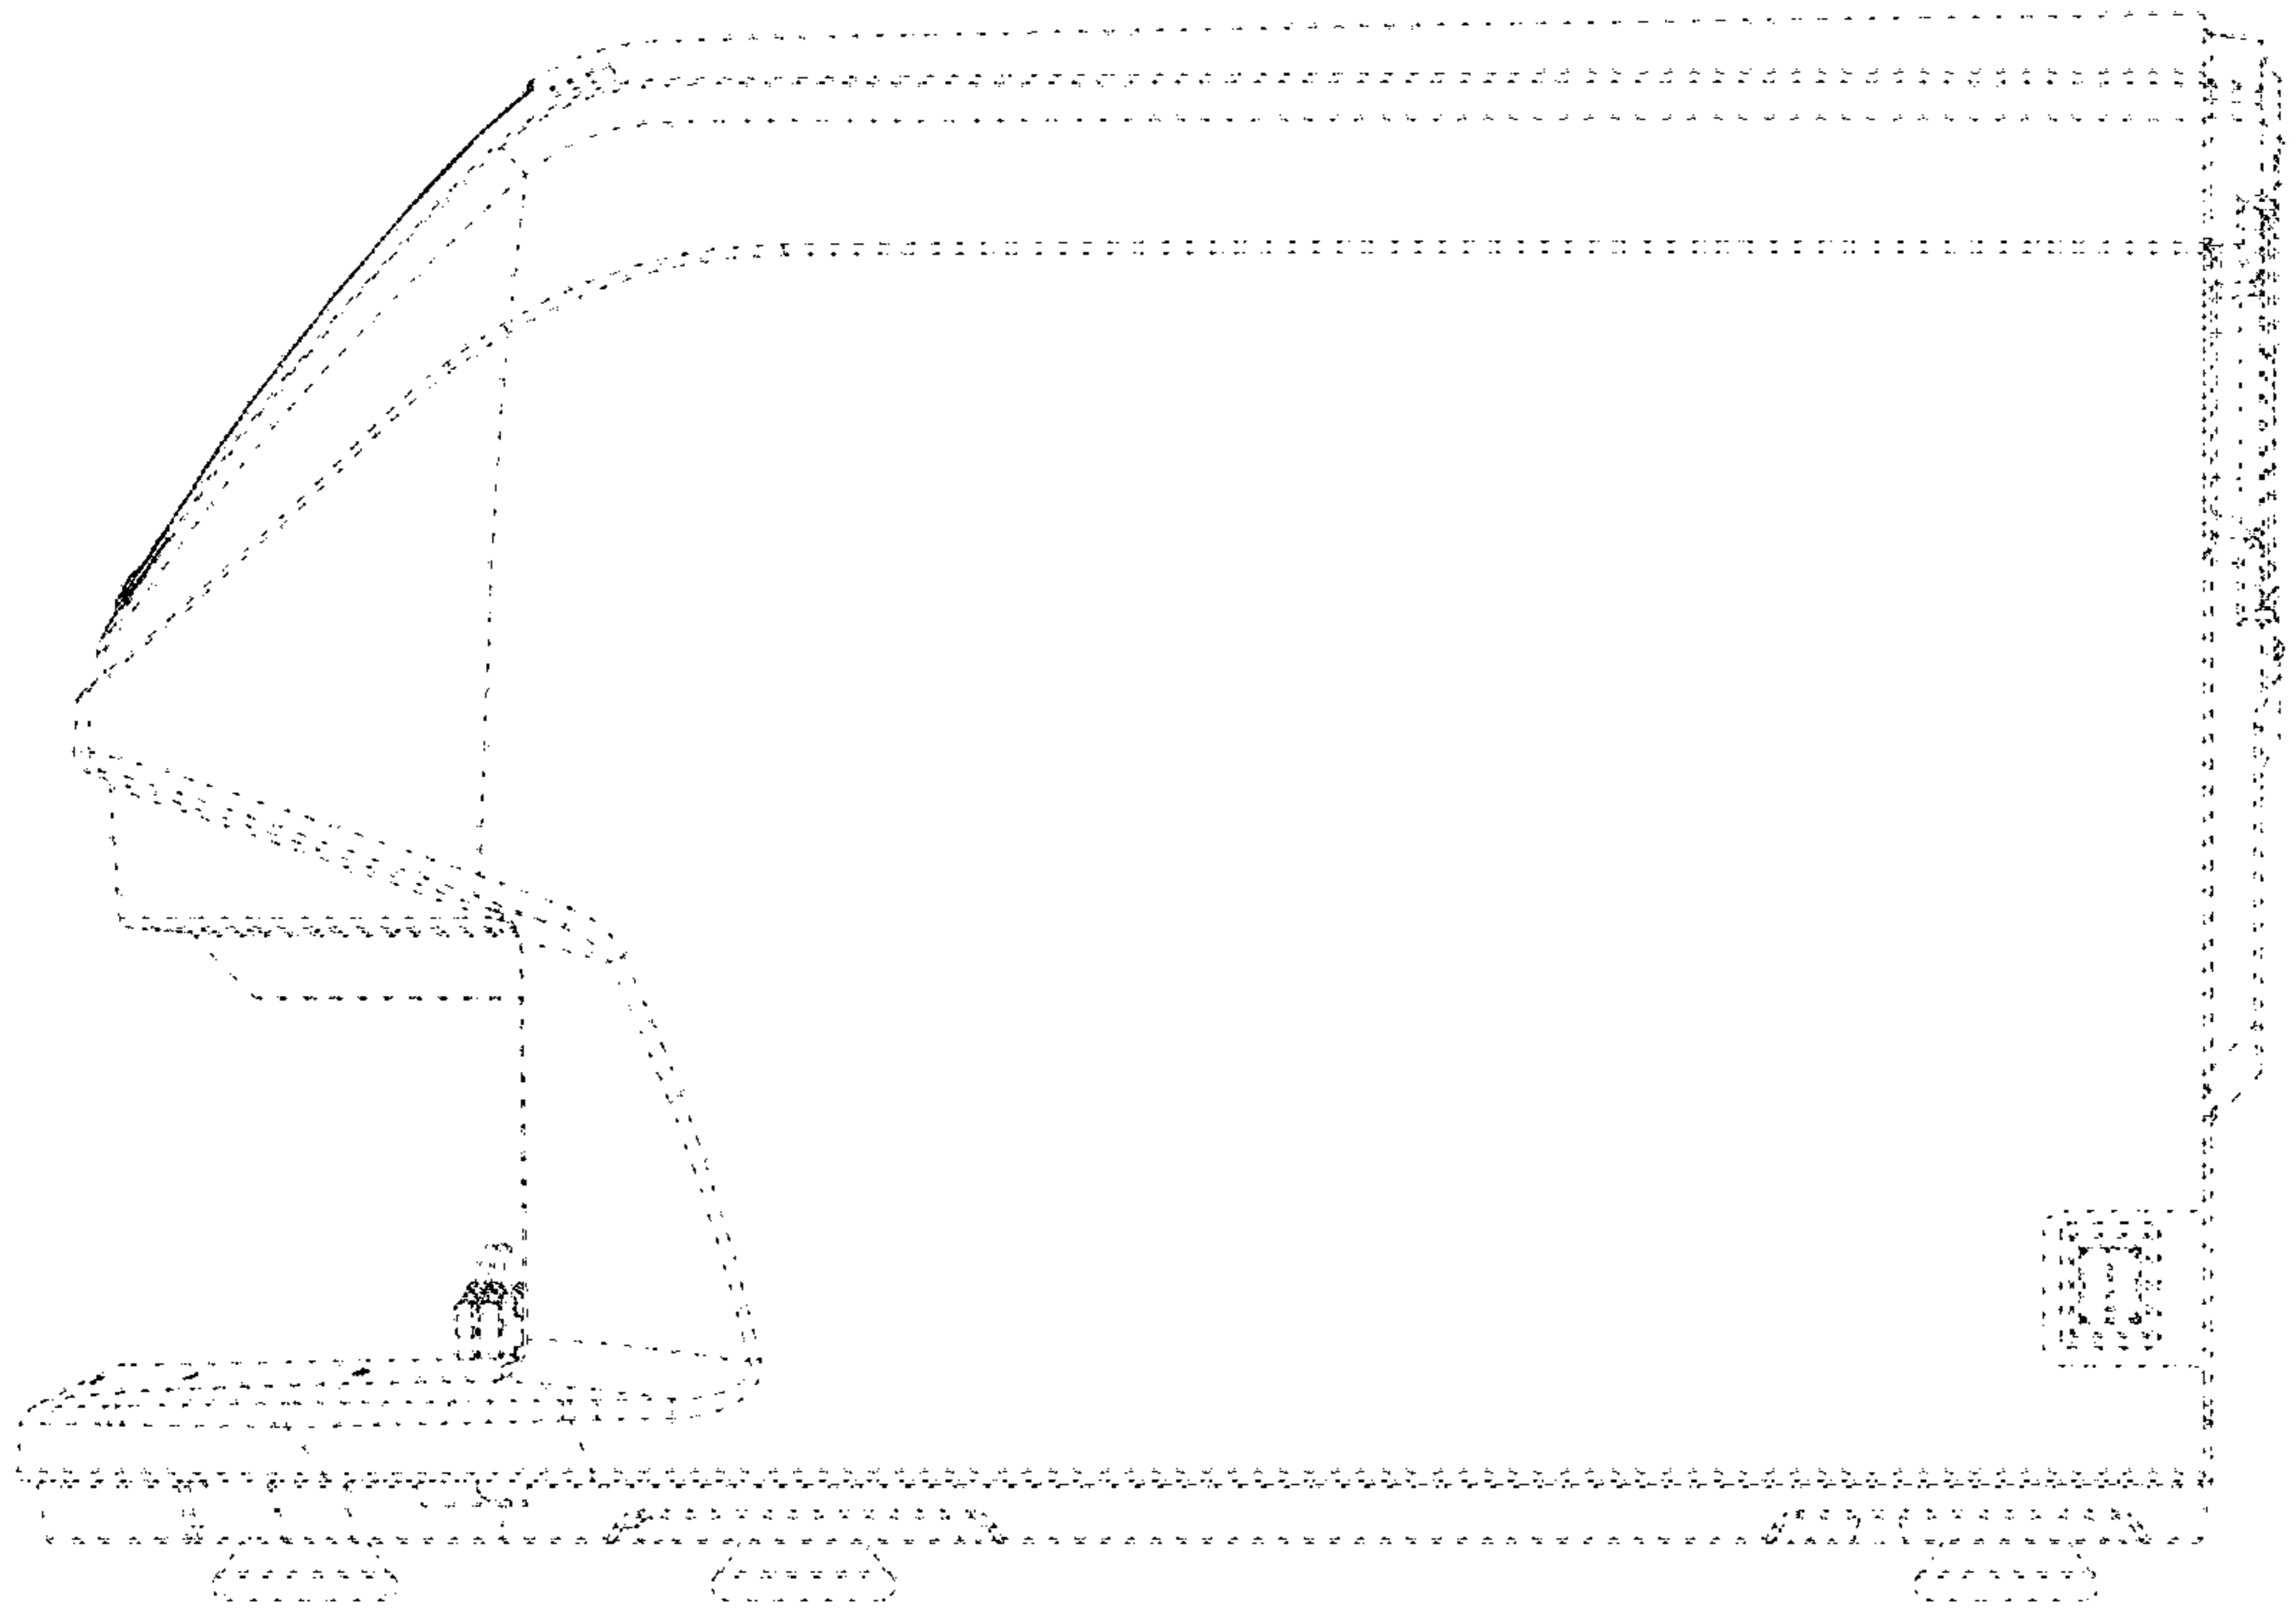


FIG. 4

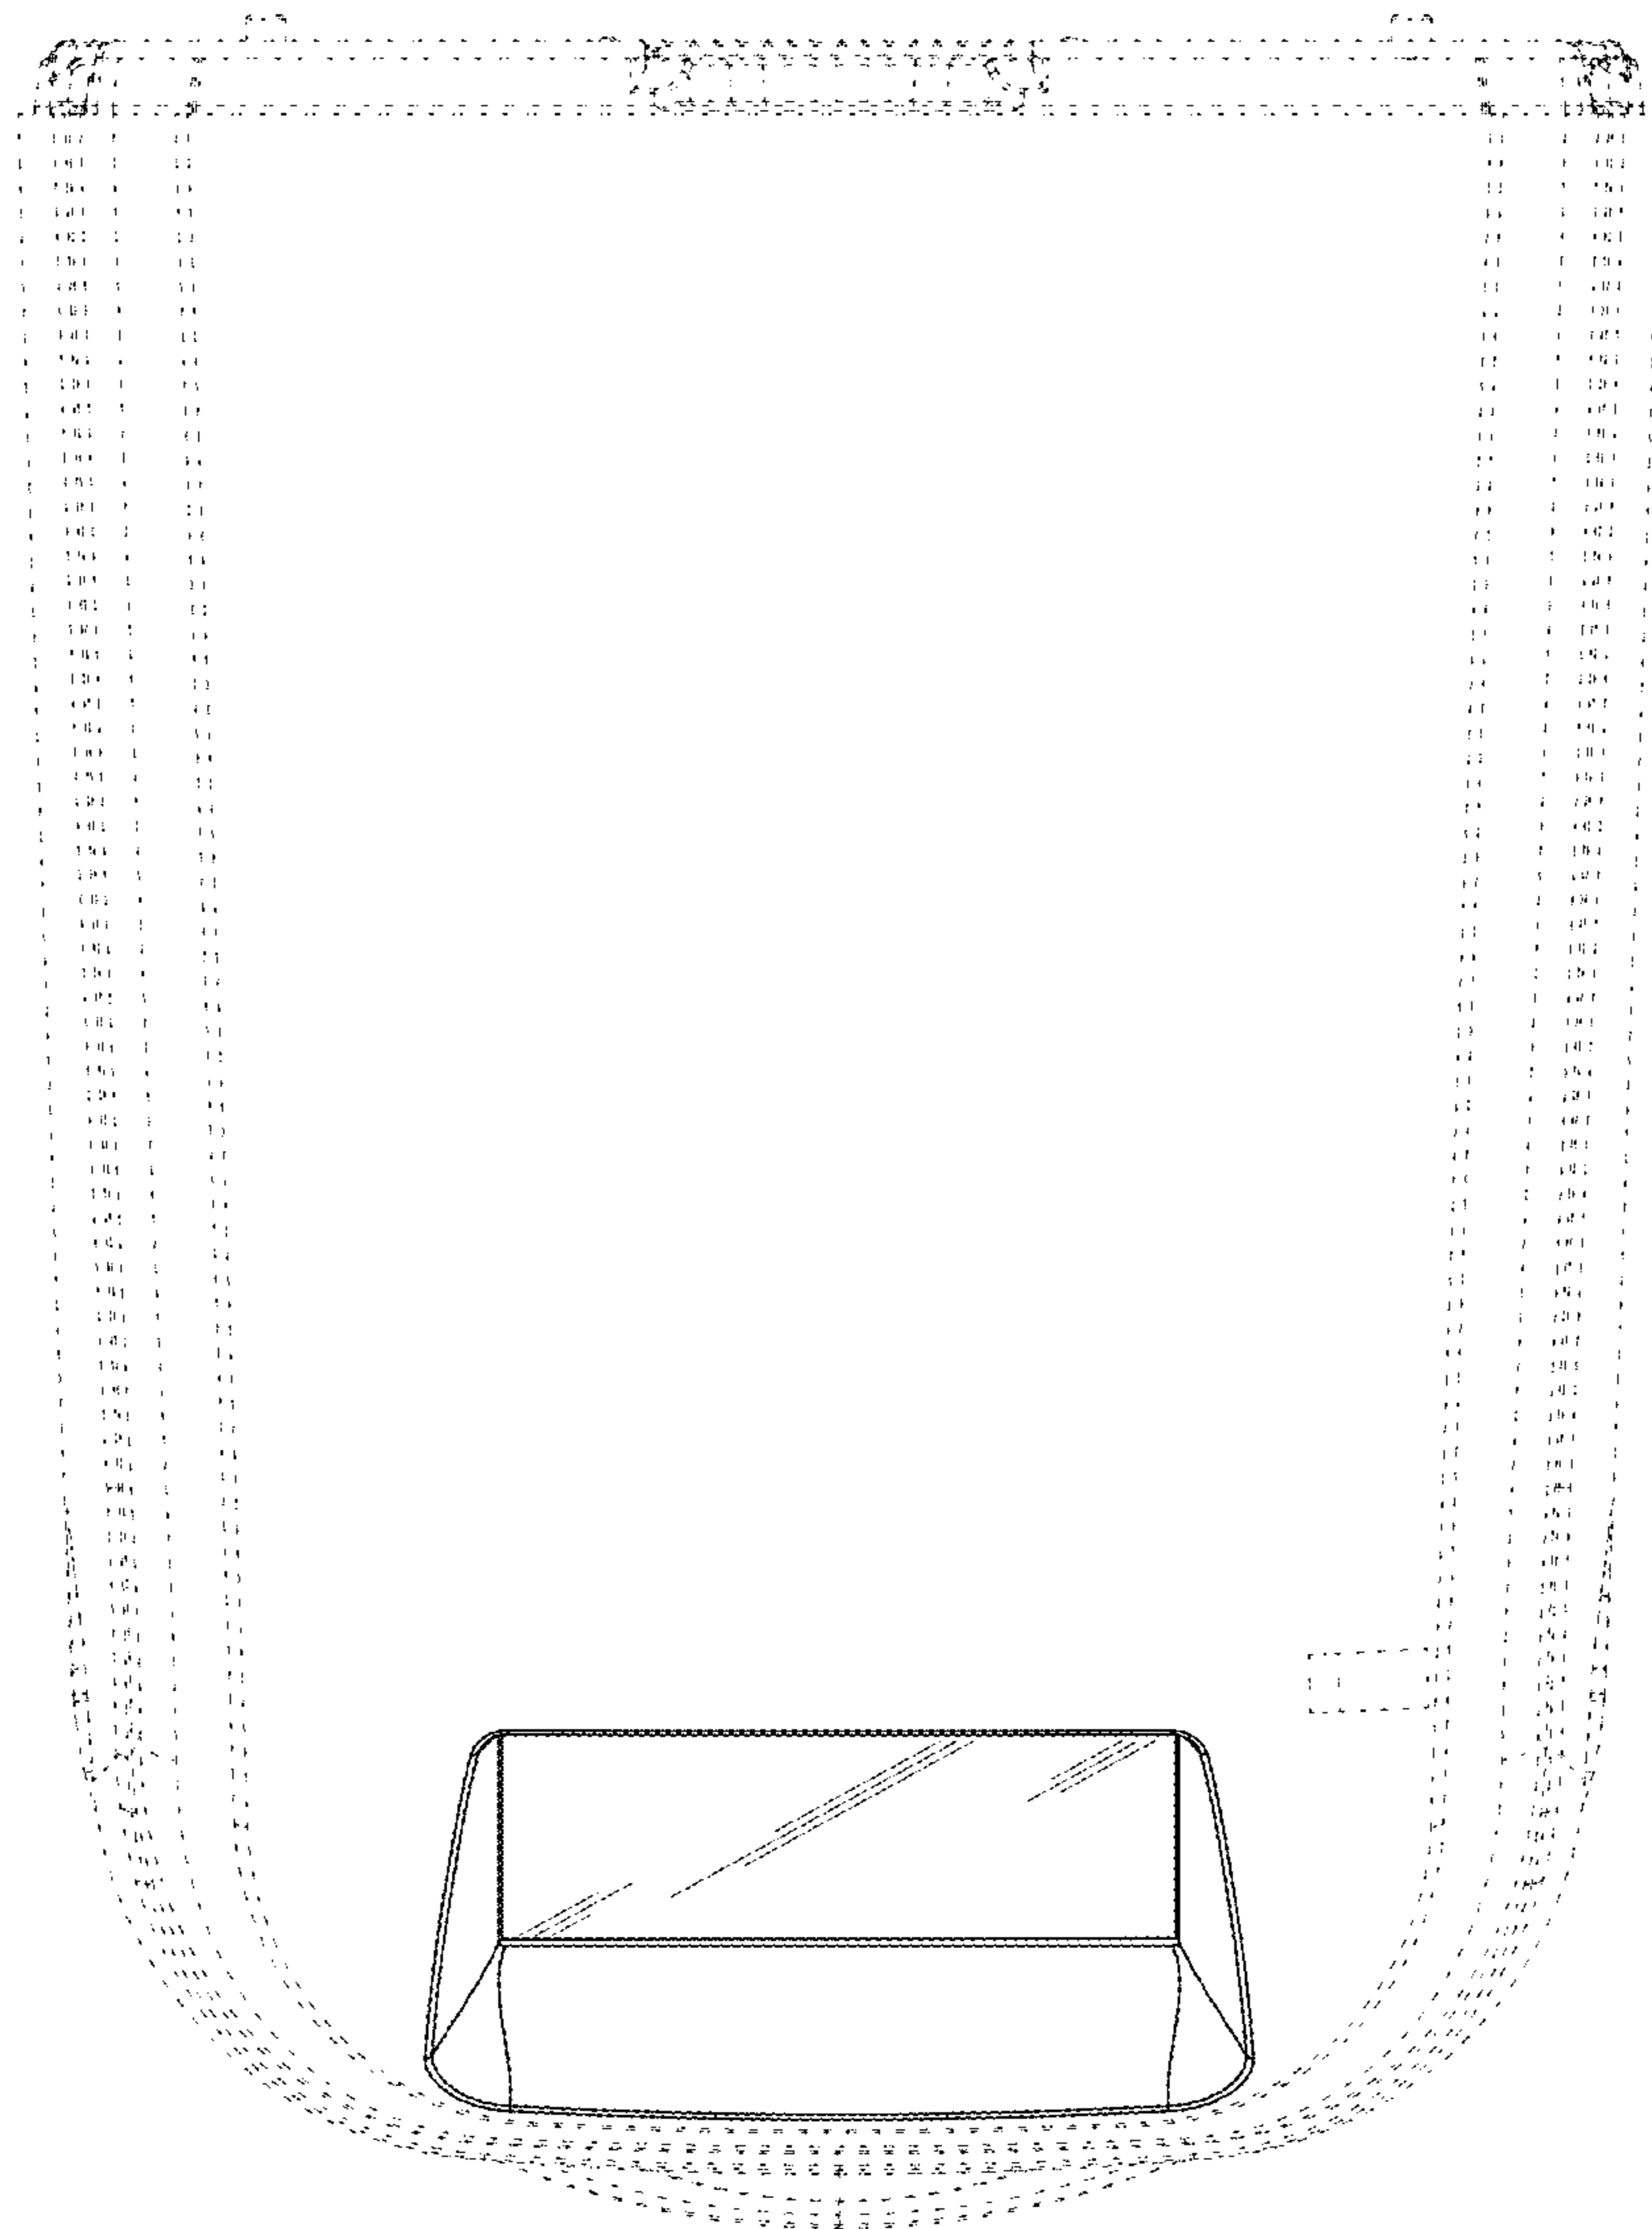


FIG. 5