



US00D854187S

(12) **United States Design Patent**
Meindl et al.

(10) **Patent No.:** **US D854,187 S**

(45) **Date of Patent:** **** Jul. 16, 2019**

(54) **APPARATUS FOR MEDICAL OR LABORATORY DIAGNOSIS**

(71) Applicant: **Siemens Healthcare Diagnostics Products GmbH, Marburg (DE)**

(72) Inventors: **Josef Meindl, Bad Soden Am Taunus (DE); Markus Mottscheller, Nuremberg (DE); Sabine Zillikens, Kriftel (DE)**

(73) Assignee: **Siemens Healthcare Diagnostics Products GmbH, Marburg (DE)**

(**) Term: **15 Years**

(21) Appl. No.: **29/622,596**

(22) Filed: **Oct. 18, 2017**

(30) **Foreign Application Priority Data**

Apr. 24, 2017 (EM) 003870138

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/232**

(58) **Field of Classification Search**
USPC D24/107, 169, 185, 186, 216-219,
D24/231-234; D10/81
CPC G01N 2035/00306; G01N 2035/00326;
G01N 2035/00336; G01N 2030/027;
G01N 21/76

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D472,645 S * 4/2003 Roepke D24/234
D682,440 S * 5/2013 Degn D24/216

D690,023 S * 9/2013 Chang D24/216
D691,283 S * 10/2013 Lee D24/234
D693,020 S * 11/2013 Degn D24/216
D716,966 S * 11/2014 Lizari Illarramendi D24/232
D787,695 S * 5/2017 Mottscheller D24/216
D802,156 S * 11/2017 Barton D24/216
2017/0269114 A1* 9/2017 Bryant G01N 35/04

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Schiff Hardin LLP

(57) **CLAIM**

The ornamental design for an apparatus for medical or laboratory diagnosis, as shown and described.

DESCRIPTION

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a front elevational view of an apparatus for medical or laboratory diagnosis showing our new design;

FIG. 2 is a back elevational view thereof;

FIG. 3 is a top plan view thereof;

FIG. 4 is a bottom plan view thereof;

FIG. 5 is a right side elevational view thereof;

FIG. 6 is a left side elevational view thereof; and,

FIG. 7 is a perspective view taken generally from the front, right-hand side thereof.

The broken lines and the unshaded surfaces illustrate portions of the apparatus for medical or laboratory diagnosis that form no part of the claimed design.

1 Claim, 7 Drawing Sheets
(6 of 7 Drawing Sheet(s) Filed in Color)

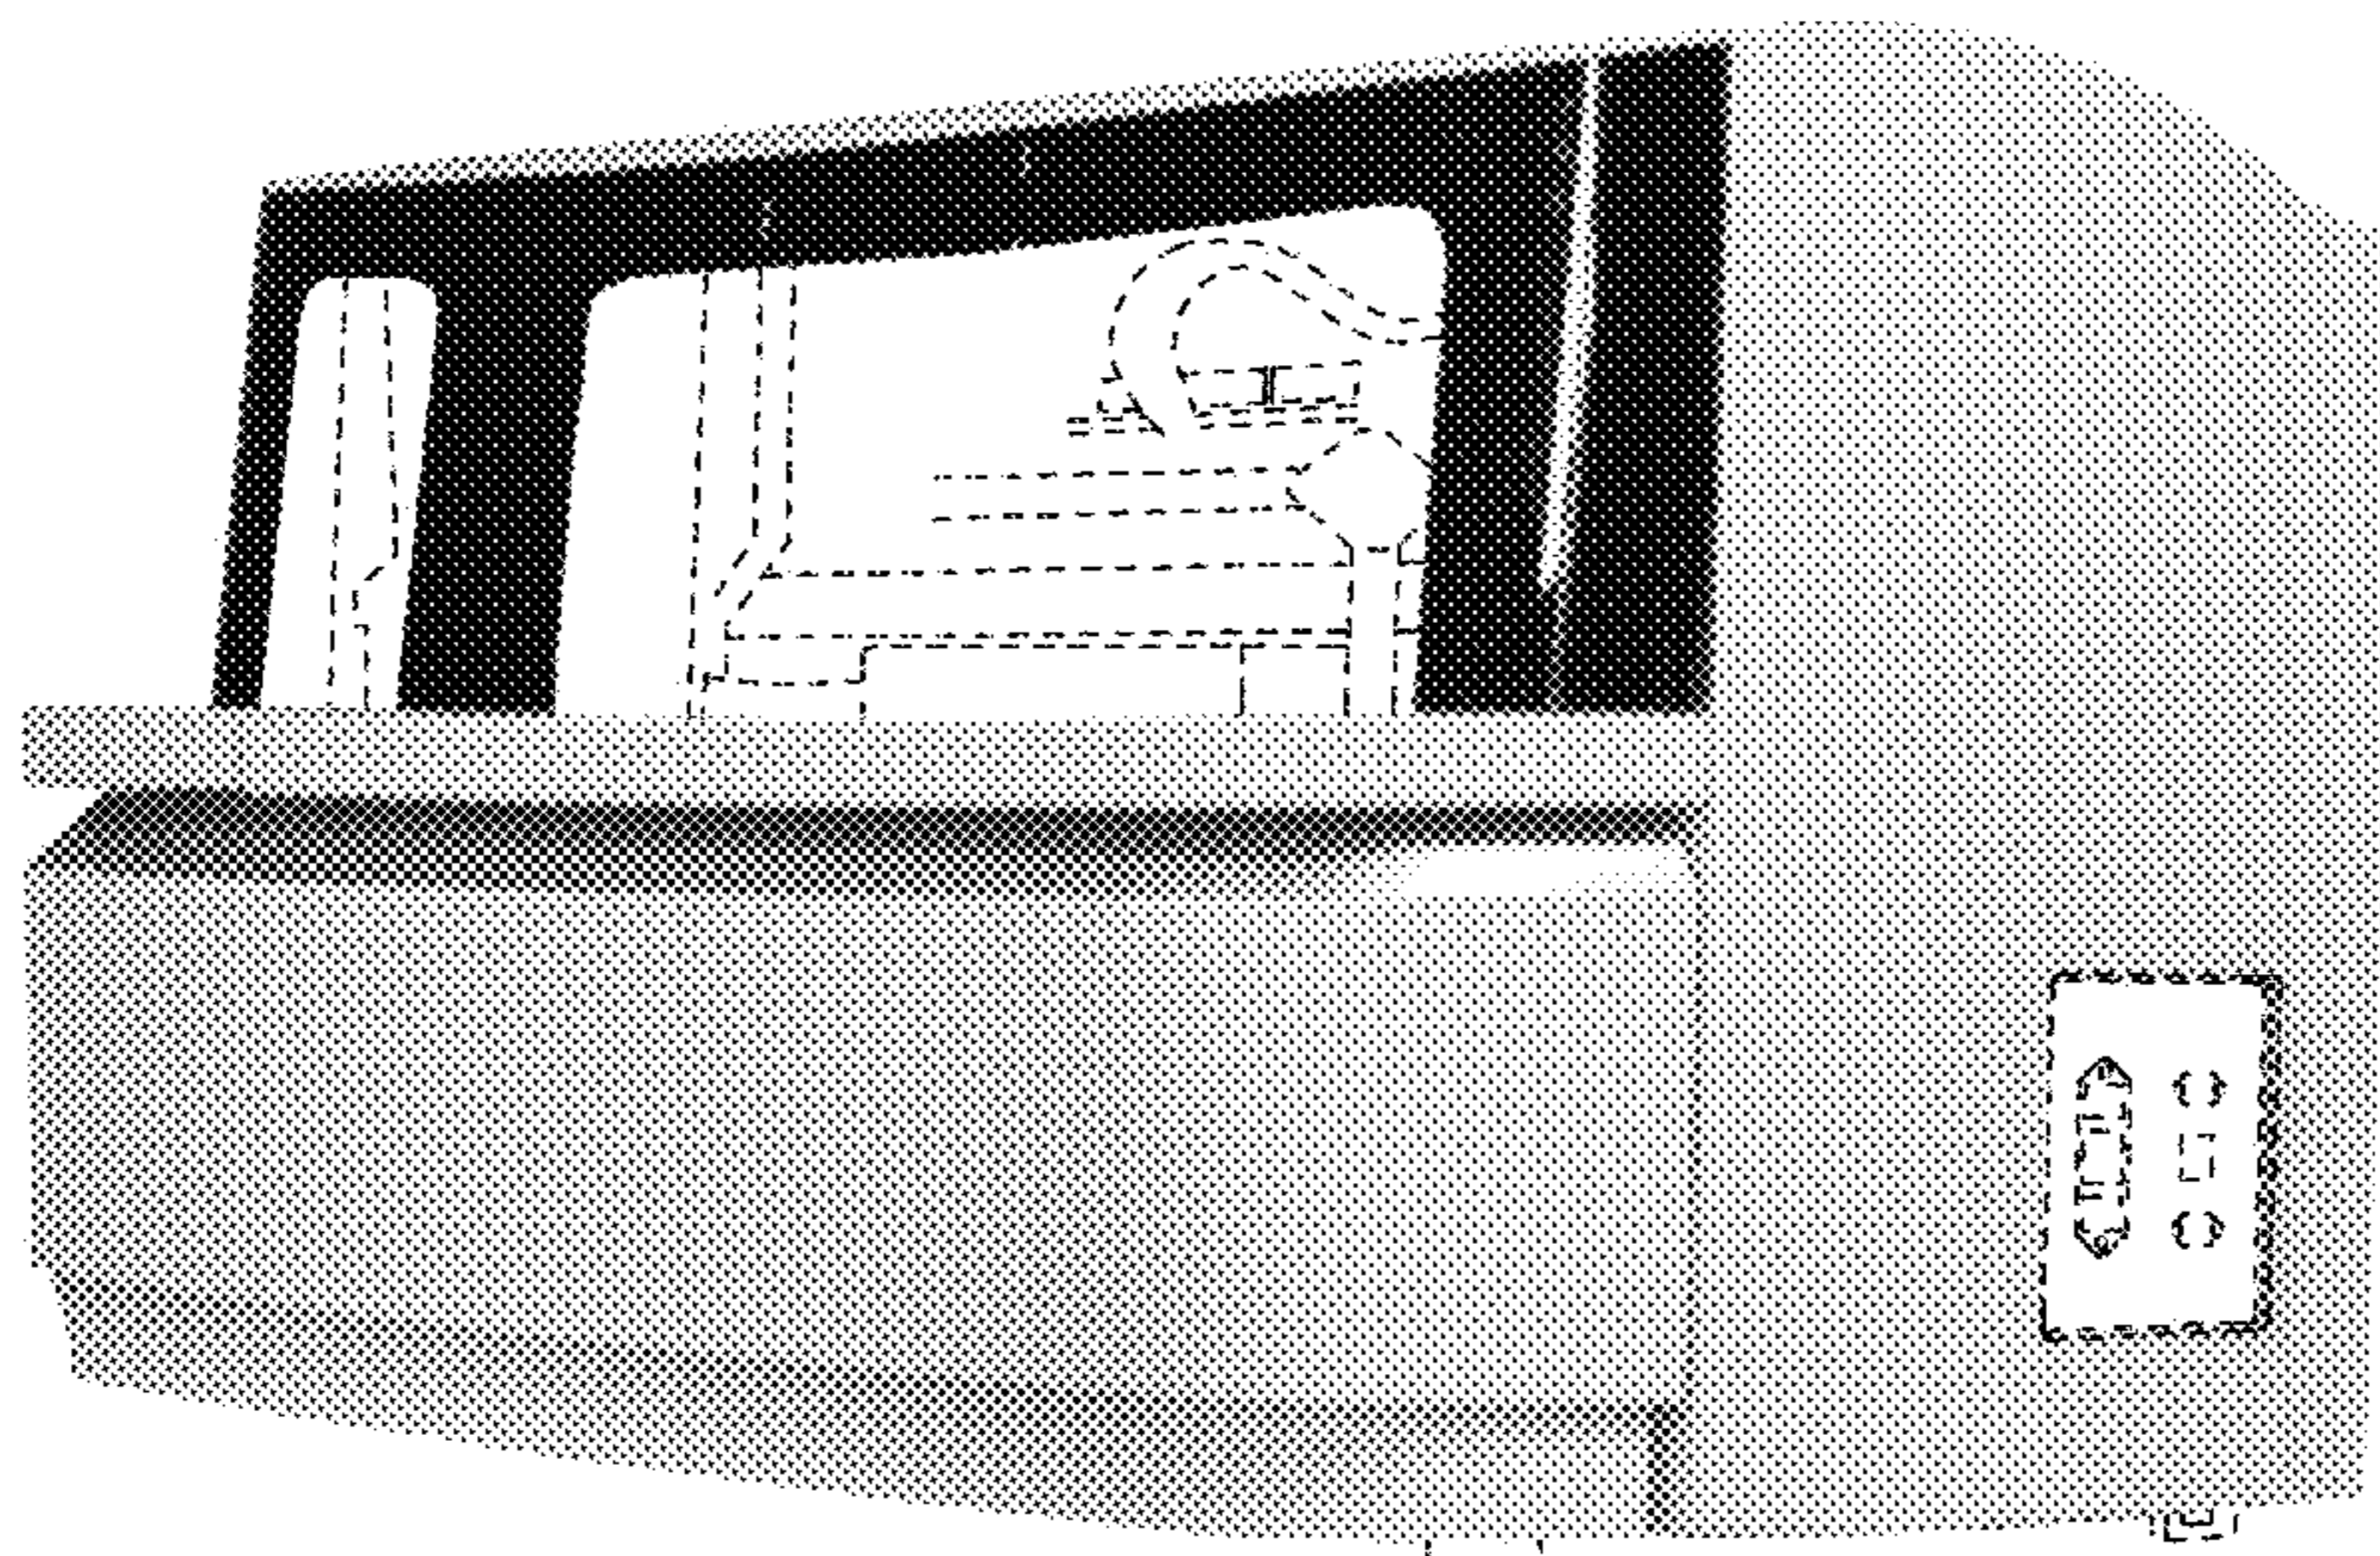


FIG. 1

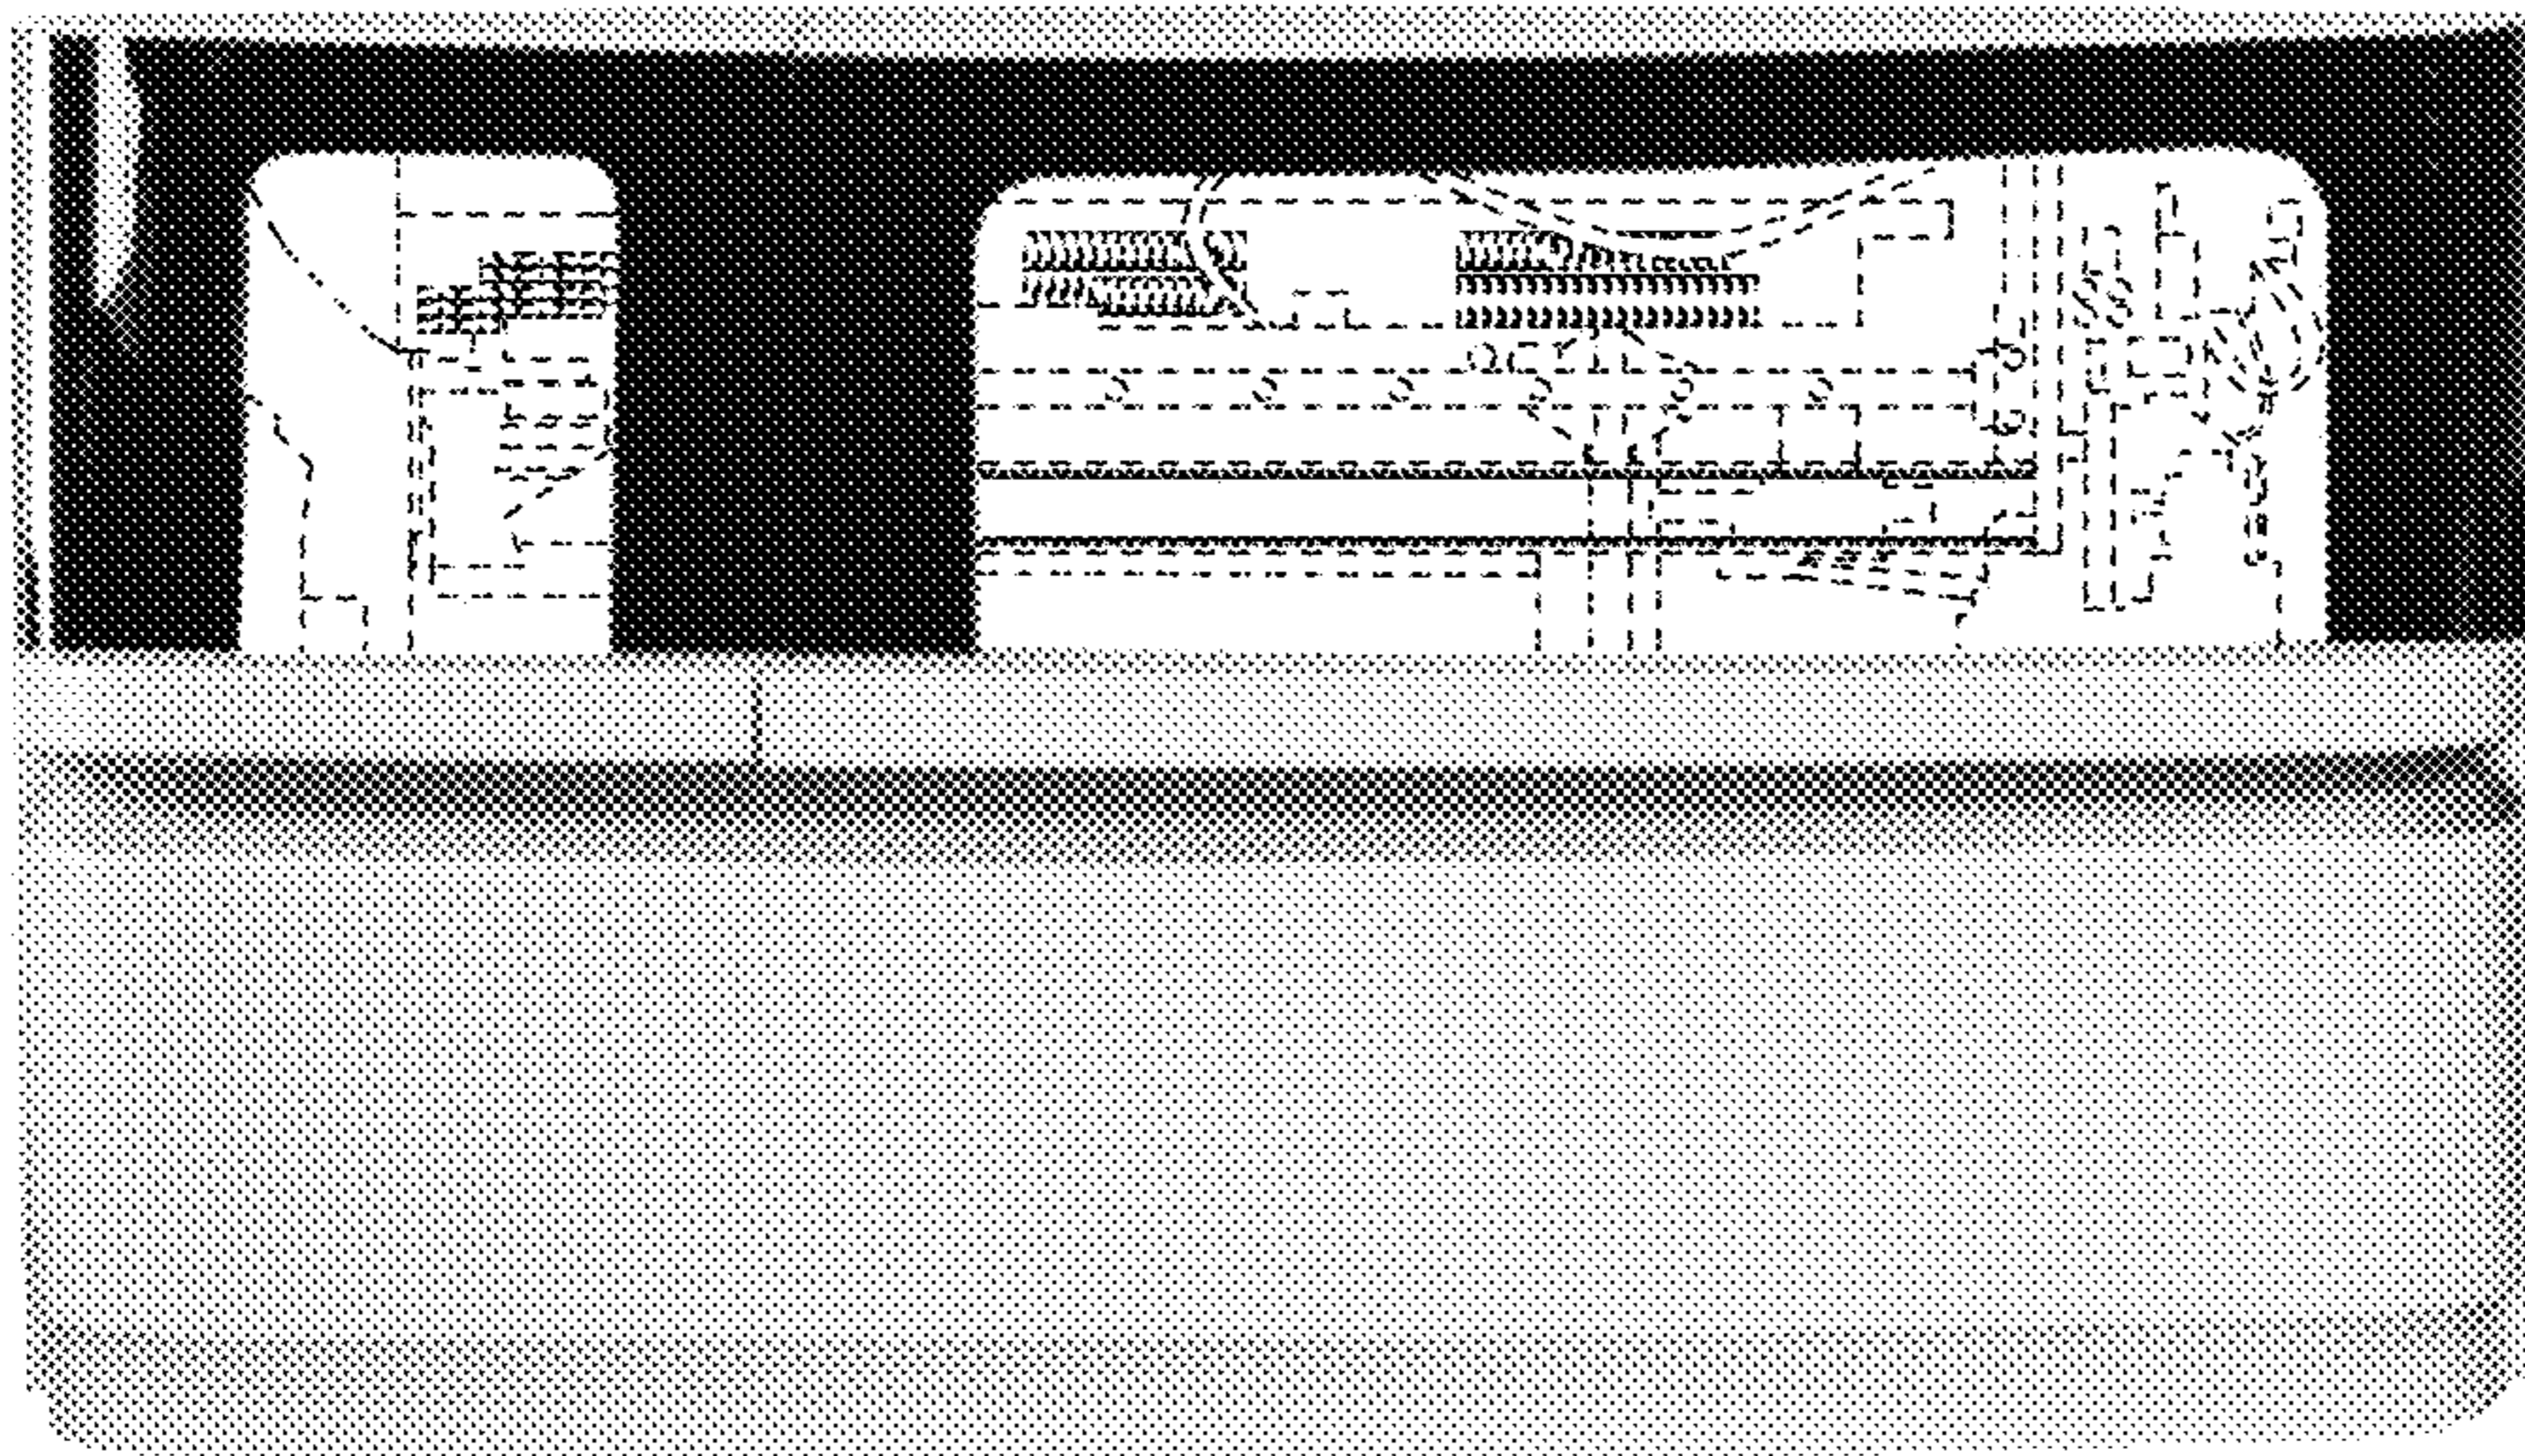


FIG. 3

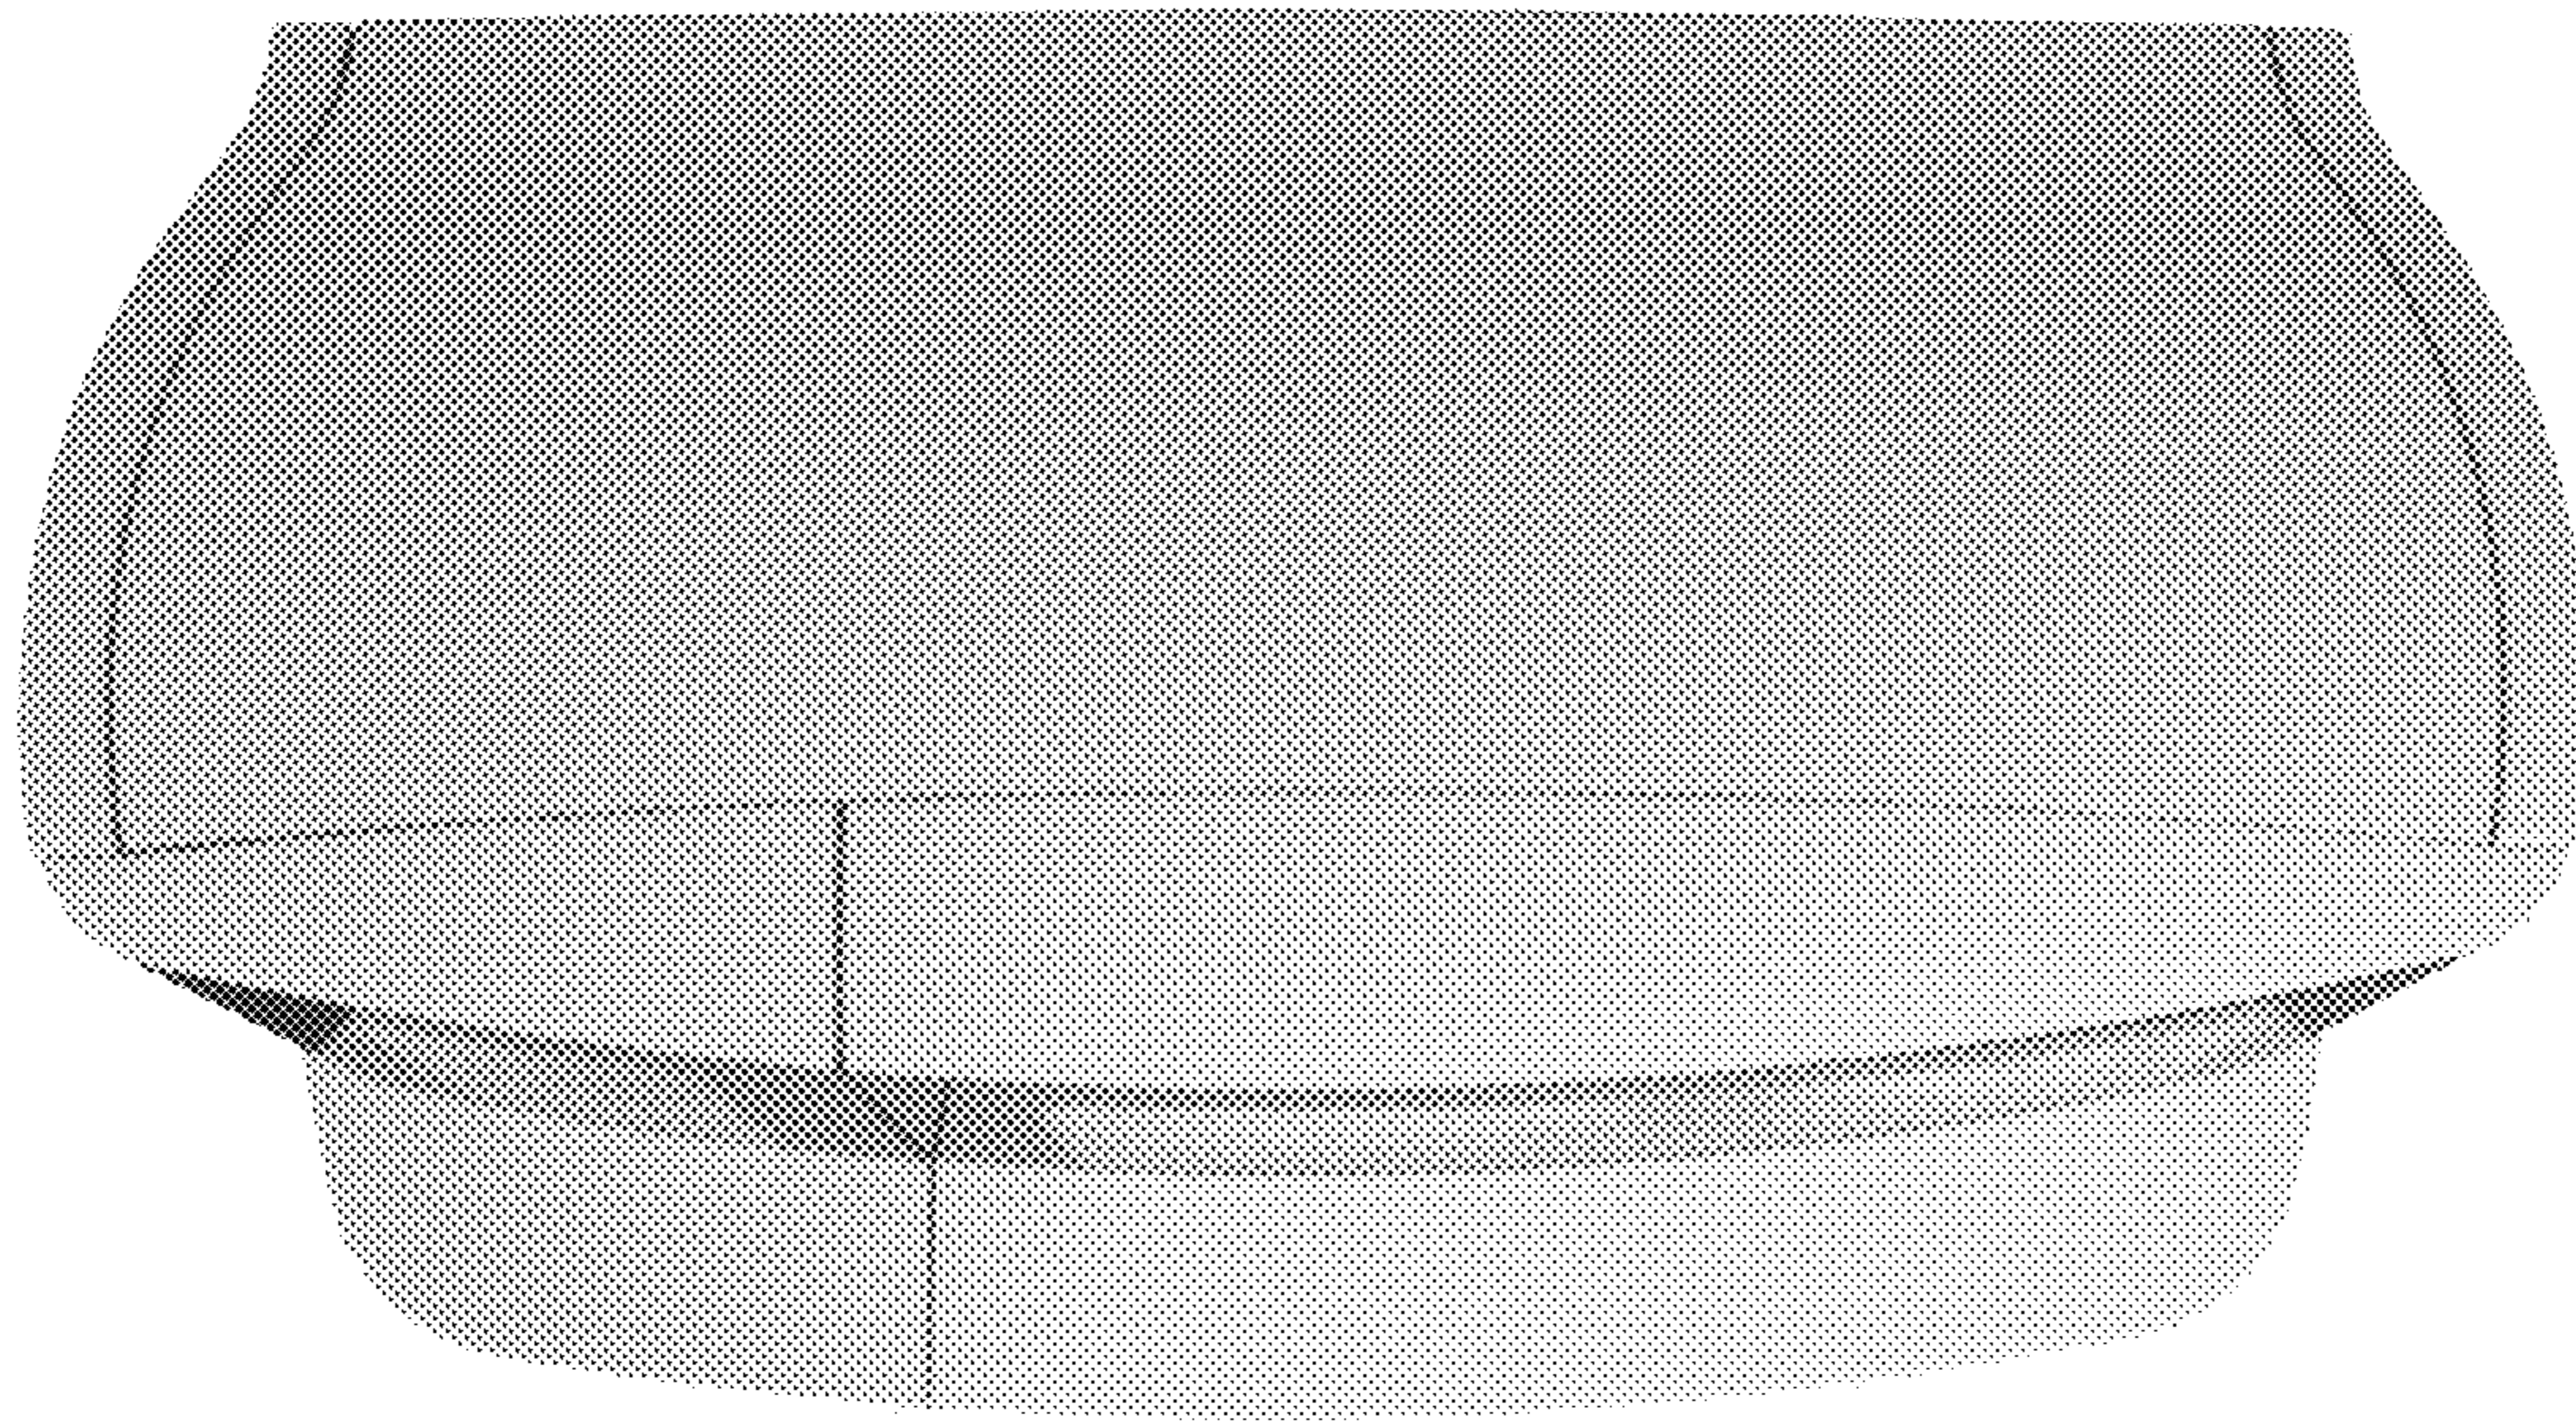


FIG. 4

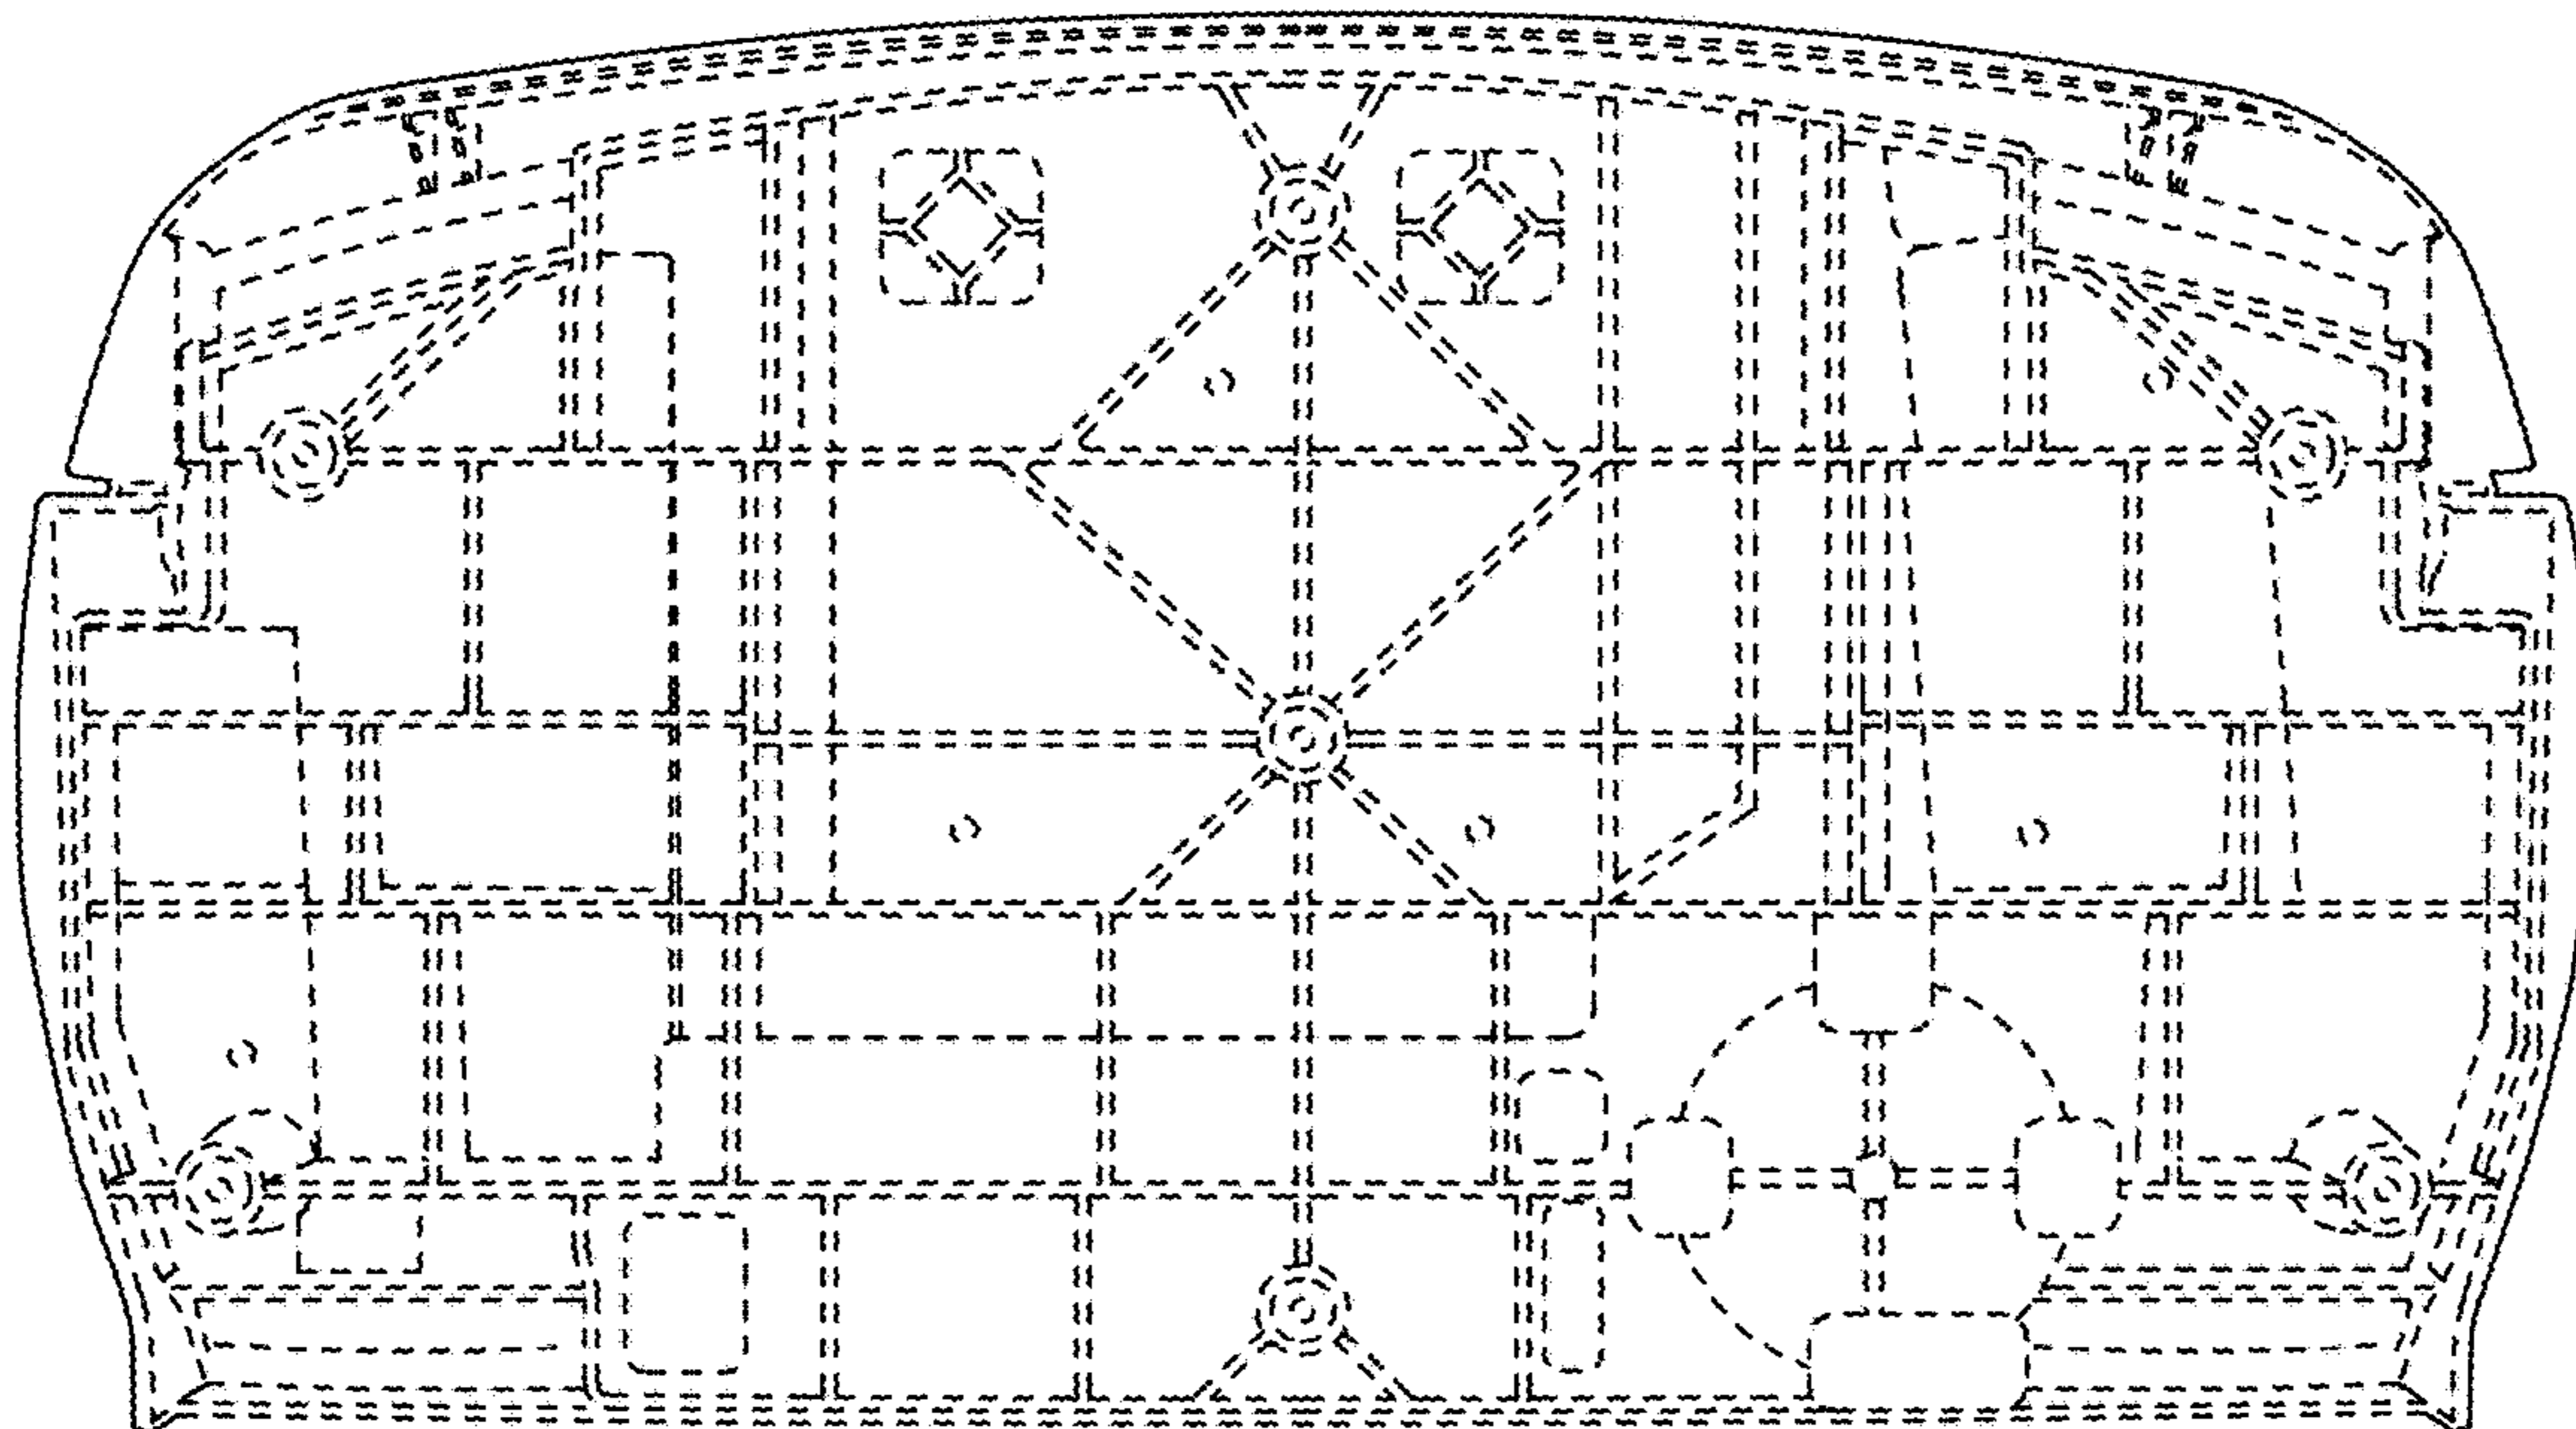


FIG. 5

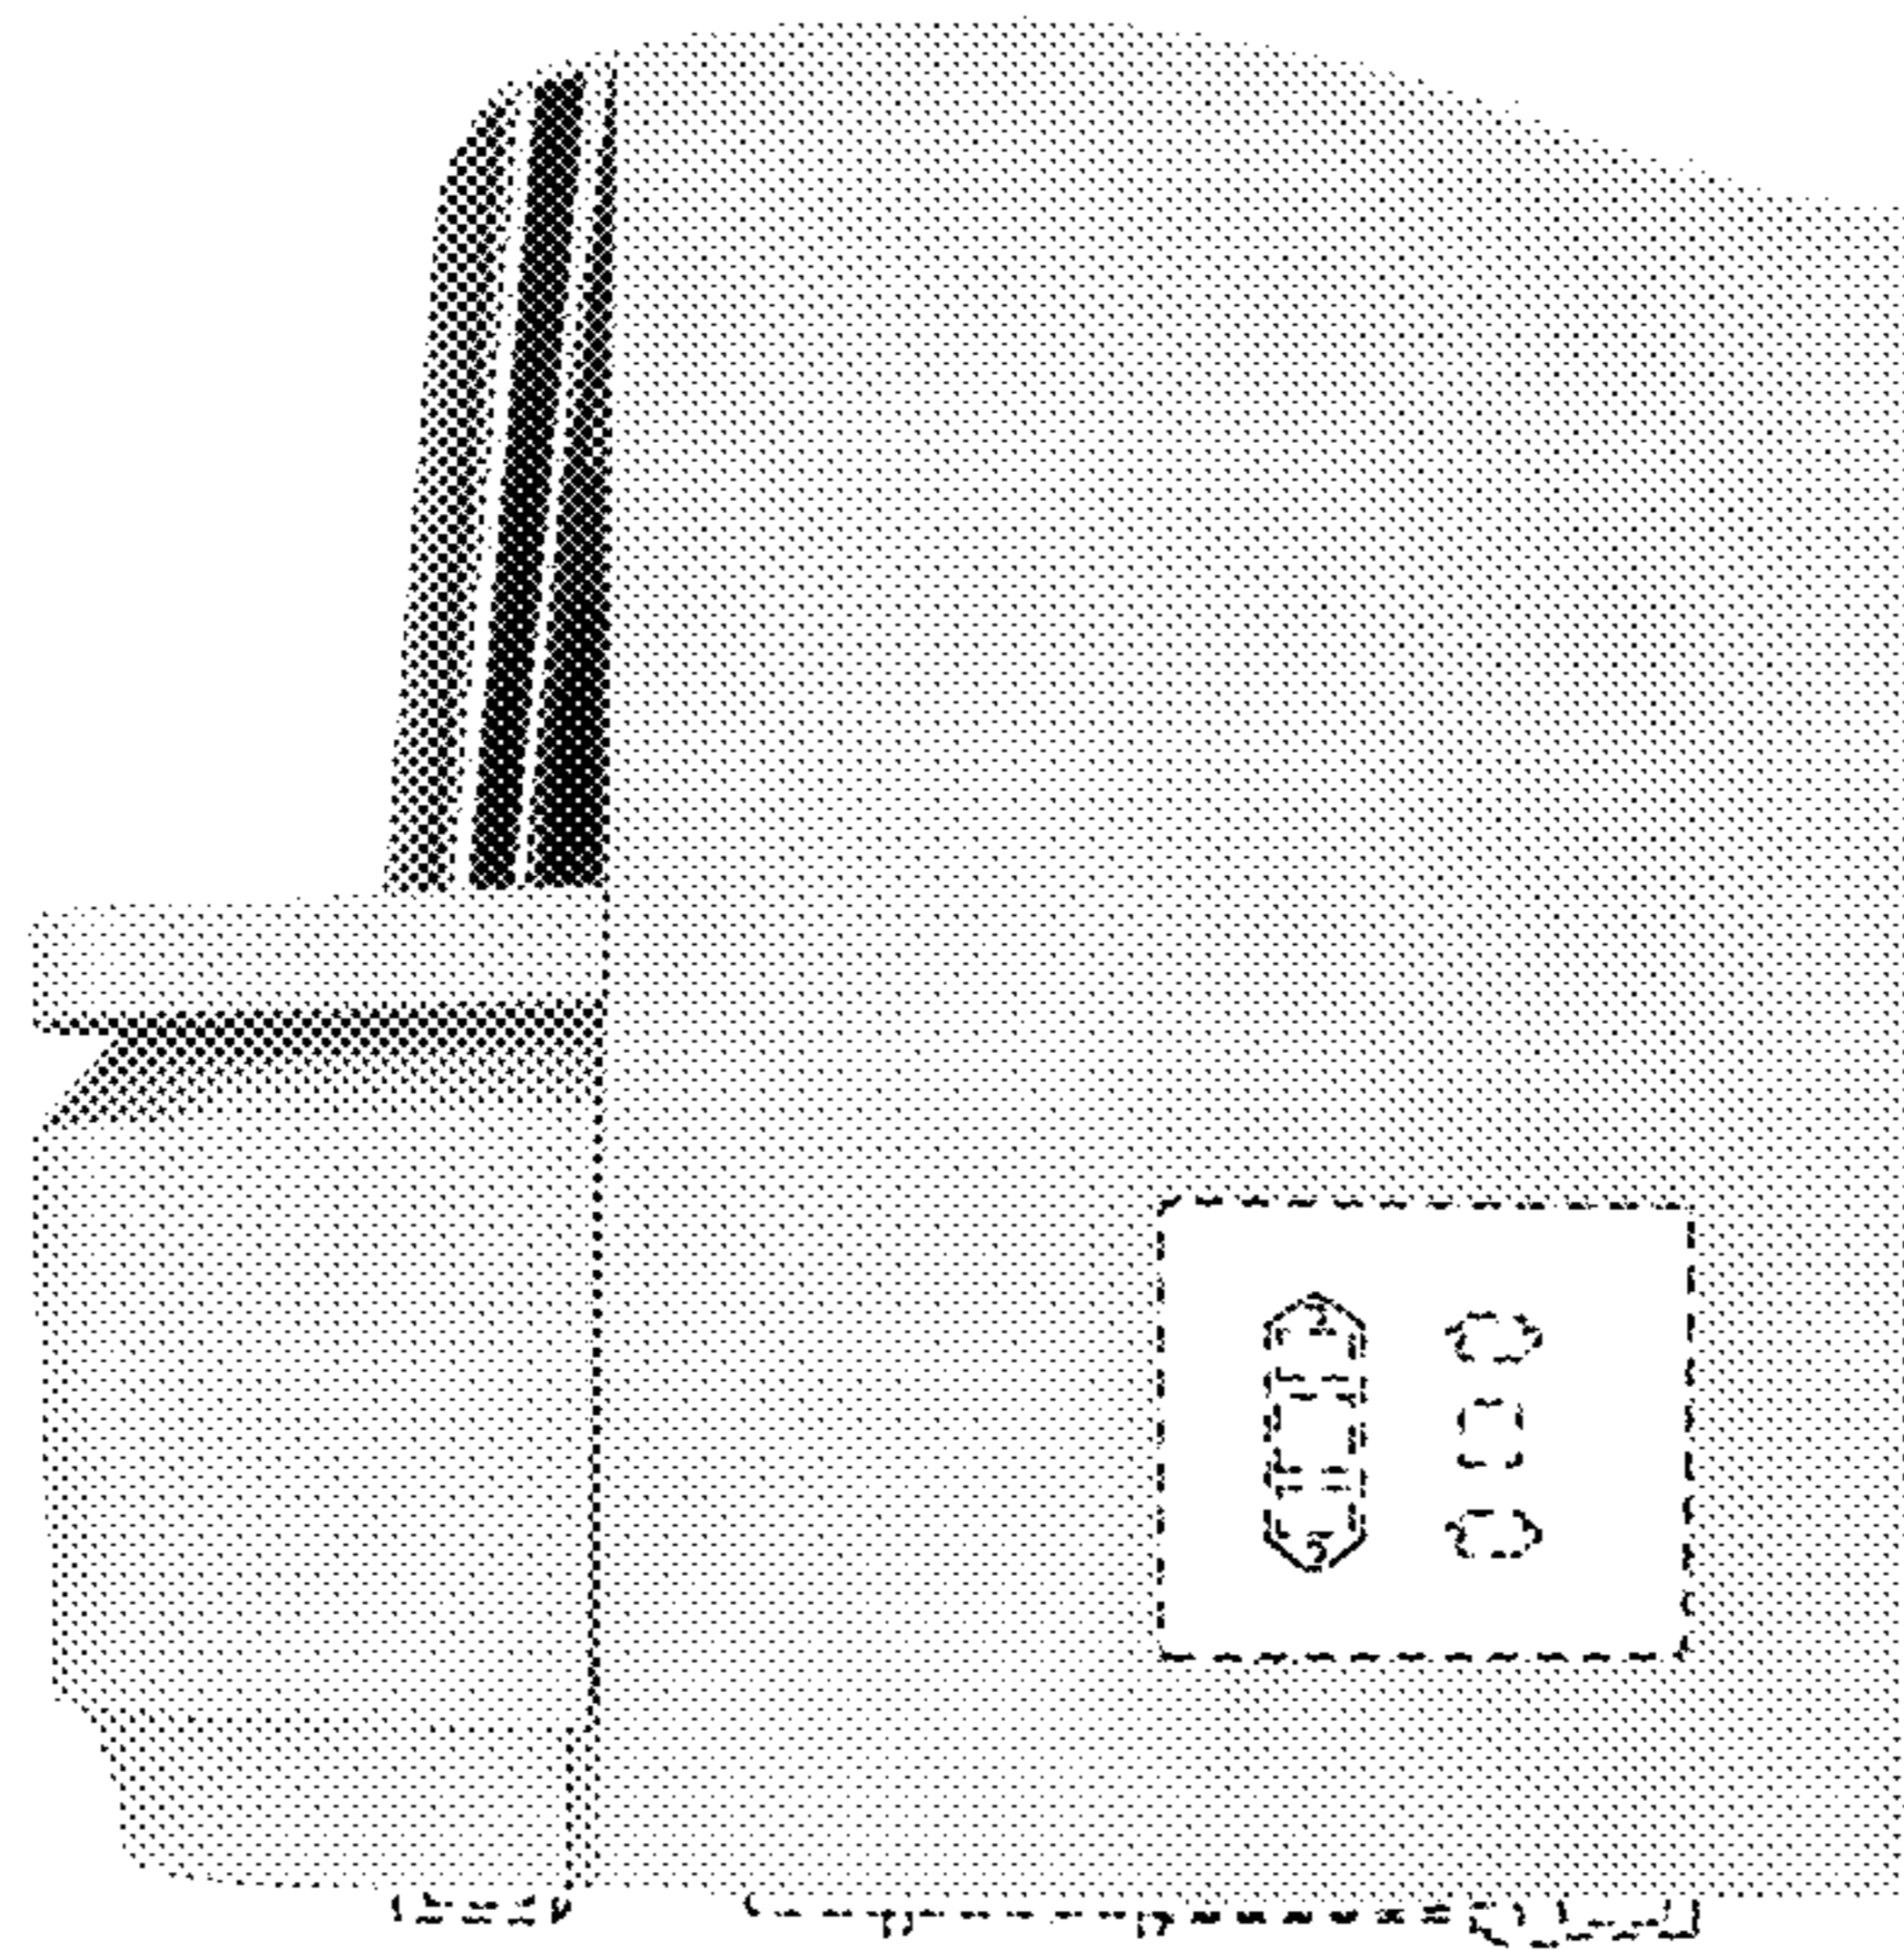


FIG. 6

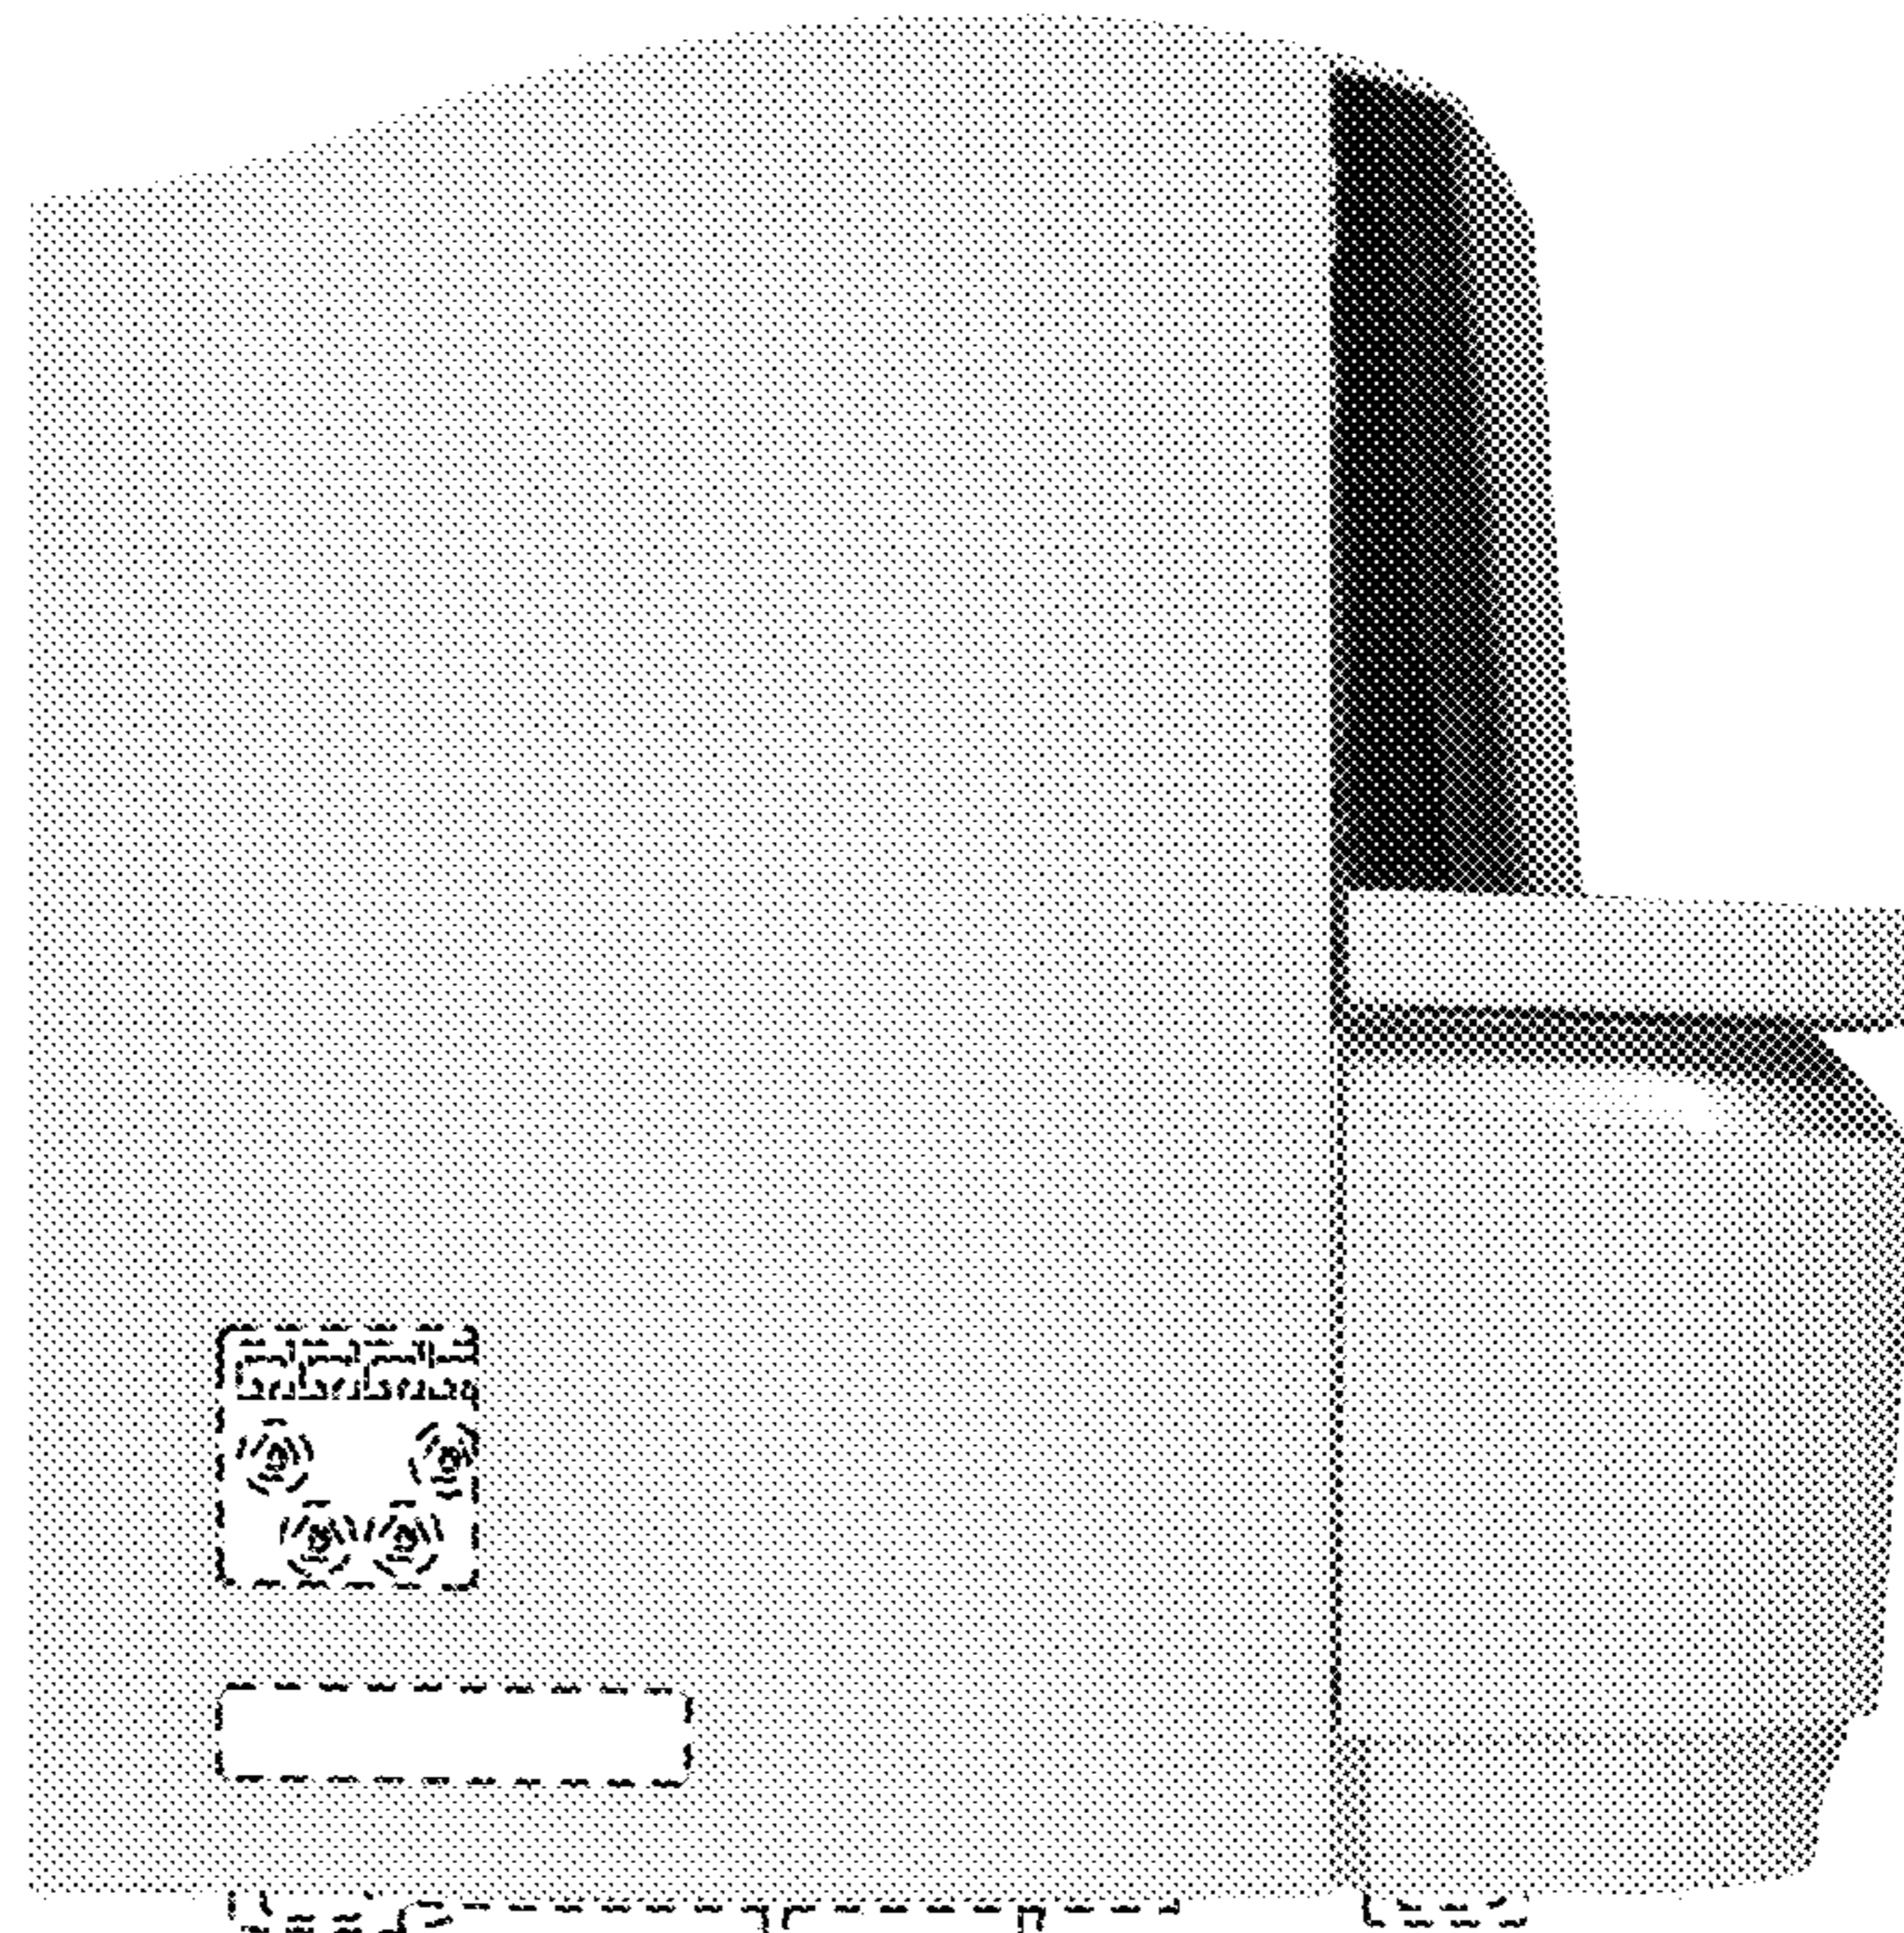


FIG. 7

