



US00D855185S

(12) **United States Design Patent** (10) **Patent No.:** **US D855,185 S**
Chang et al. (45) **Date of Patent:** **** Jul. 30, 2019**

(54) **BED FOR MAGNETIC RESONANCE TOMOGRAPHY DIAGNOSIS APPARATUS**

D748,804 S 2/2016 Eenboom et al.
D770,049 S * 10/2016 Yanagihara D24/159
D820,453 S * 6/2018 Personelli D24/159
D820,459 S * 6/2018 Eenboom D24/183
D829,913 S * 10/2018 Kitayama D24/159
D841,170 S * 2/2019 Sul D24/183

(71) Applicant: **Canon Medical Systems Corporation**,
Otawara-shi, Tochigi (JP)

(72) Inventors: **Shianwei Chang**, Kawasaki (JP);
Noriaki Baba, Tokyo (JP)

FOREIGN PATENT DOCUMENTS

CN 301709738 S 10/2011
CN 302691754 S 12/2013
JP 1061710 2/2000
JP 1241314 6/2005

(73) Assignee: **Canon Medical Systems Corporation**,
Otawara-shi (JP)

(**) Term: **15 Years**

(Continued)

(21) Appl. No.: **29/641,578**

Primary Examiner — Anhdao Doan

(22) Filed: **Mar. 22, 2018**

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson,
Farabow, Garrett & Dunner LLP

(30) **Foreign Application Priority Data**

(57) **CLAIM**

Nov. 8, 2017 (JP) 2017-024877

The ornamental design for a bed for magnetic resonance tomography diagnosis apparatus, as shown and described.

(51) **LOC (11) Cl.** **24-01**

DESCRIPTION

(52) **U.S. Cl.**

USPC **D24/159**; D24/183

(58) **Field of Classification Search**

USPC D24/107, 158–161, 185, 186, 187, 231,
D24/188, 183, 184

CPC .. A61B 6/03; A61B 6/035; A61B 5/05; A61B
5/055; A61B 6/04; A61B 6/0407; A61G
13/1235; A61G 2210/50; A61F 5/3723;
A61F 5/3761

See application file for complete search history.

FIG. 1 is a front perspective view of a bed for magnetic resonance tomography diagnosis apparatus showing our new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a top plan view thereof;

FIG. 5 is a bottom plan view thereof;

FIG. 6 is a left side elevational view thereof;

FIG. 7 is a right side elevational view thereof;

FIG. 8 is a sectional view taken along line 8-8 as shown in FIG. 2 thereof; and,

FIG. 9 is a sectional view taken along line 9-9 as shown in FIG. 4 thereof.


The broken lines illustrate portions of the bed for magnetic resonance tomography diagnosis that form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D553,246 S 10/2007 Banryu
D681,208 S * 4/2013 Ninomiya D24/159
D701,605 S 3/2014 Ohmukai
D727,509 S 4/2015 Tan et al.
D736,934 S * 8/2015 Kim D24/183

1 Claim, 9 Drawing Sheets

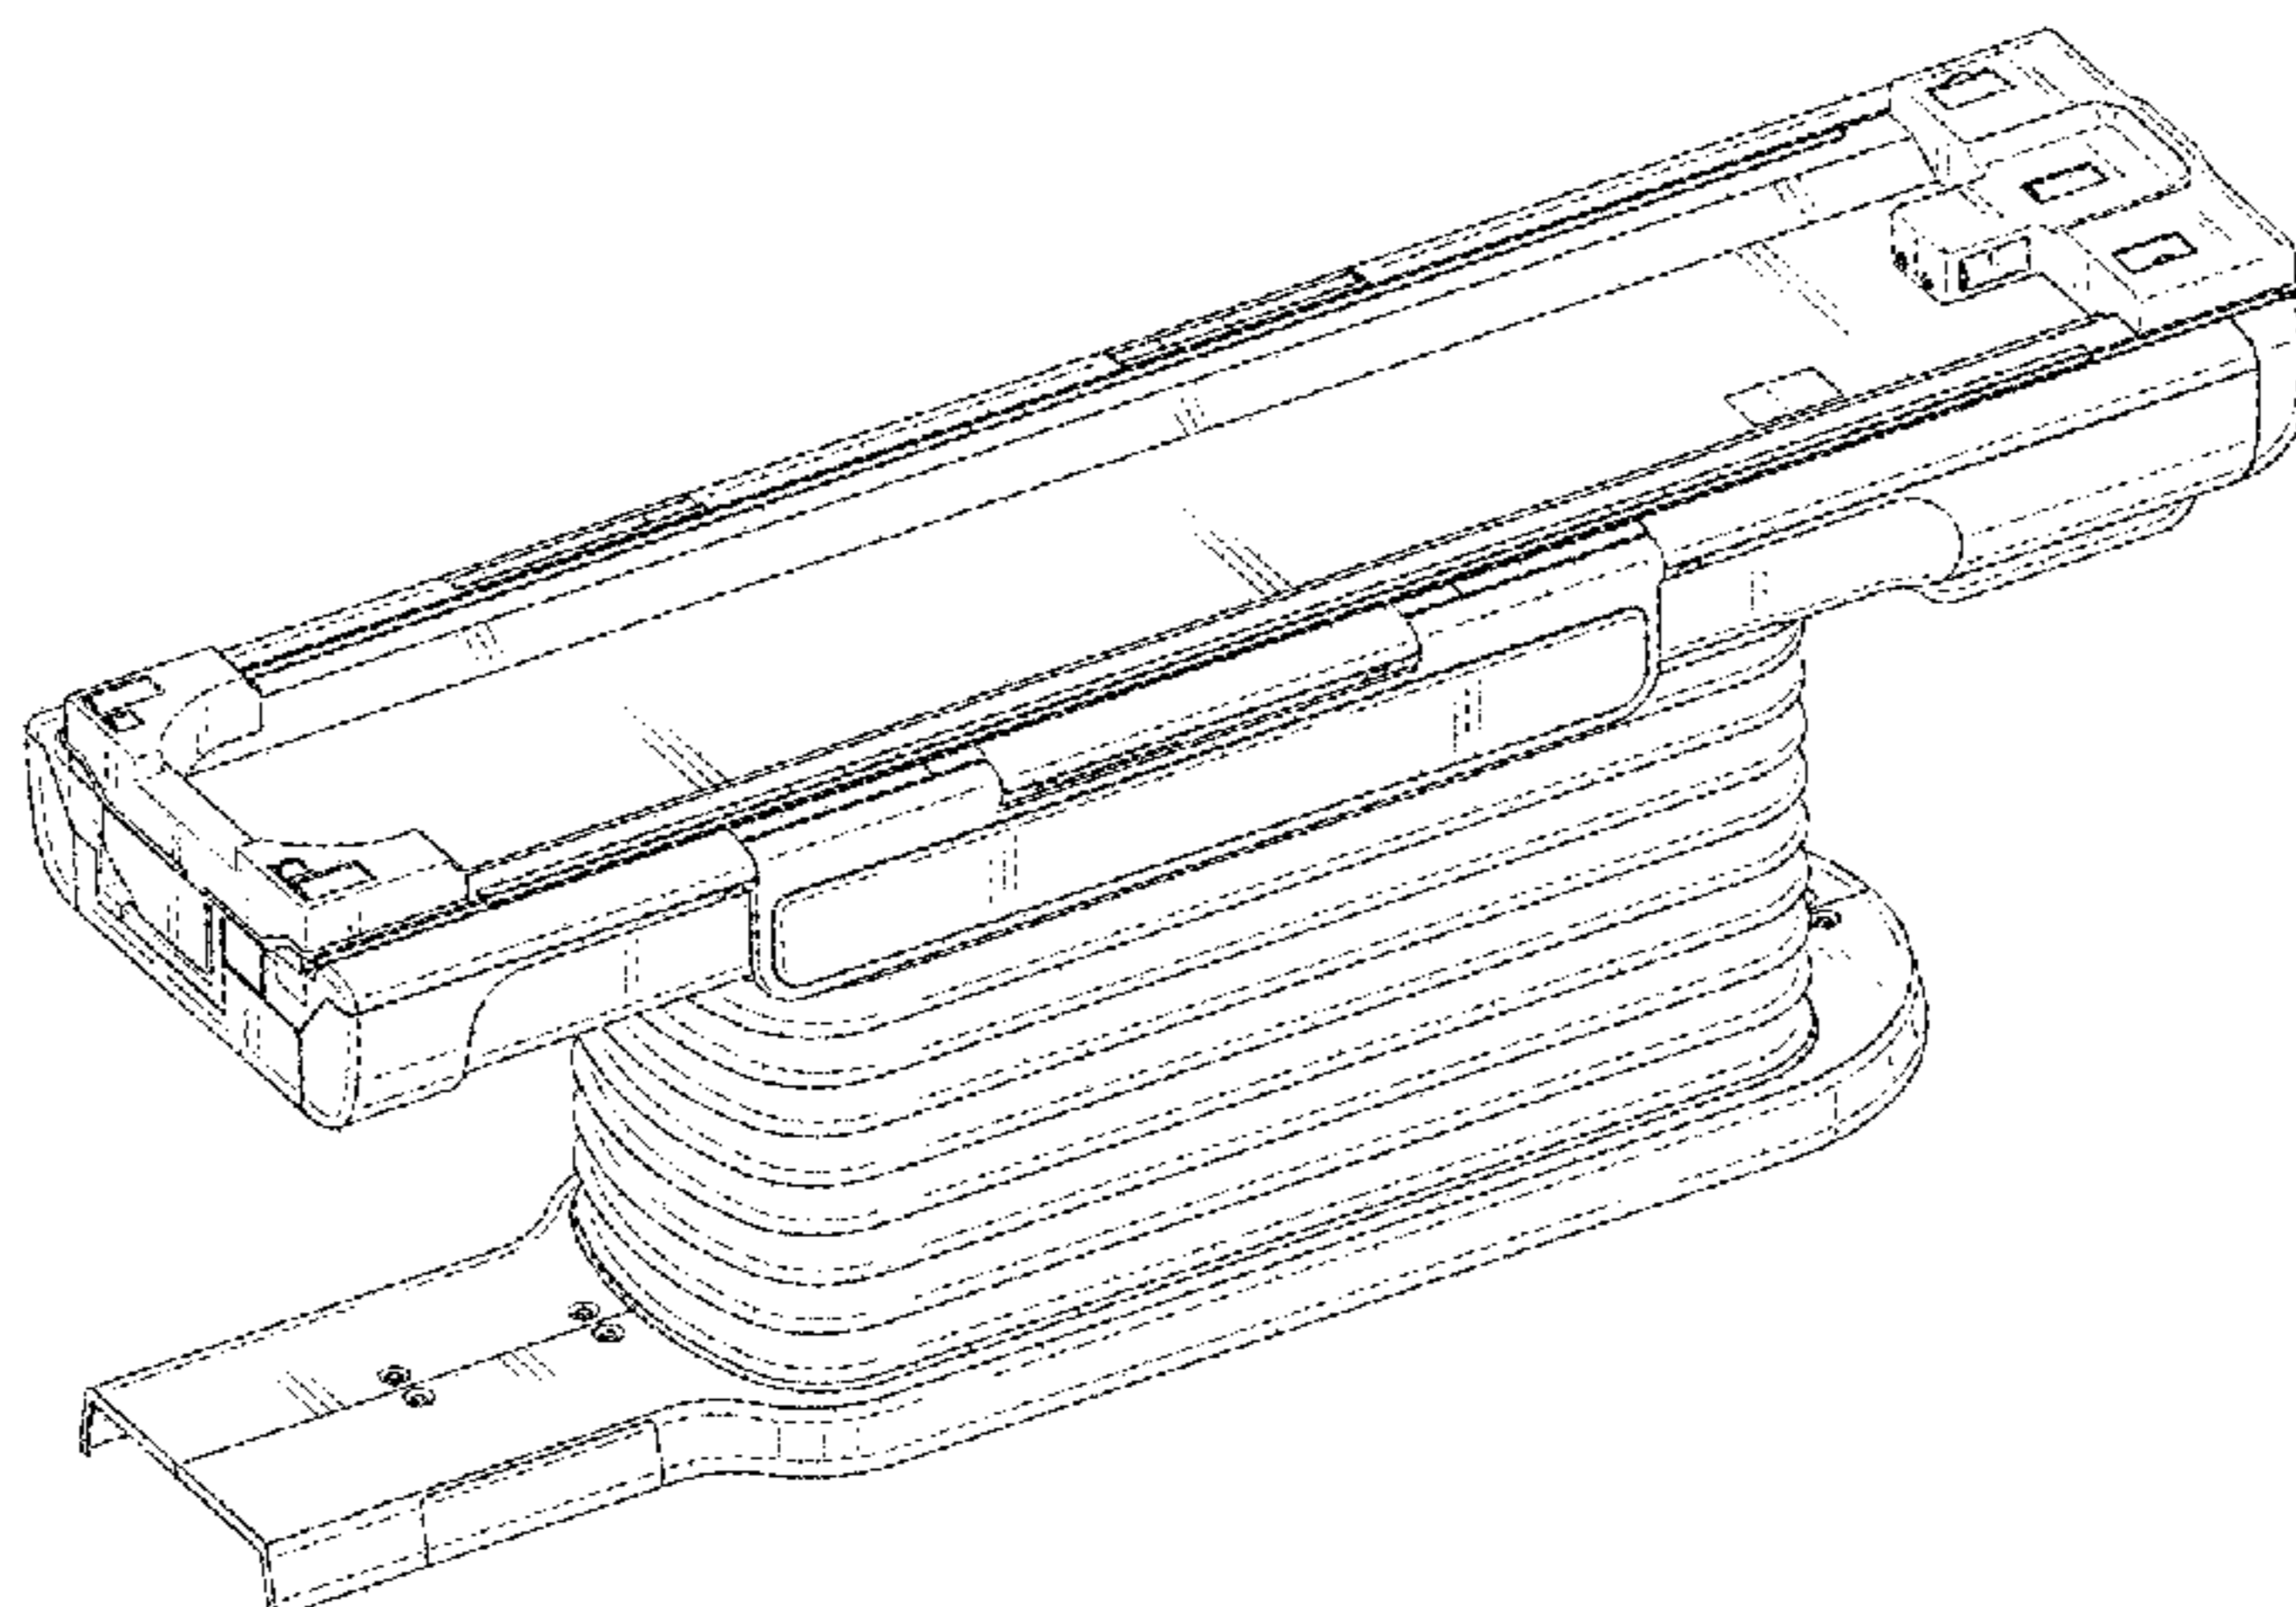

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP	1312226	10/2007
JP	1413751	5/2011
JP	1470200	5/2013
JP	1524449	5/2015
KR	30-0742674	5/2014
KR	30-0751905	7/2014
KR	30-0751918	7/2014
KR	30-0782186	2/2015
KR	30-0803219	6/2015

* cited by examiner

Fig. 1

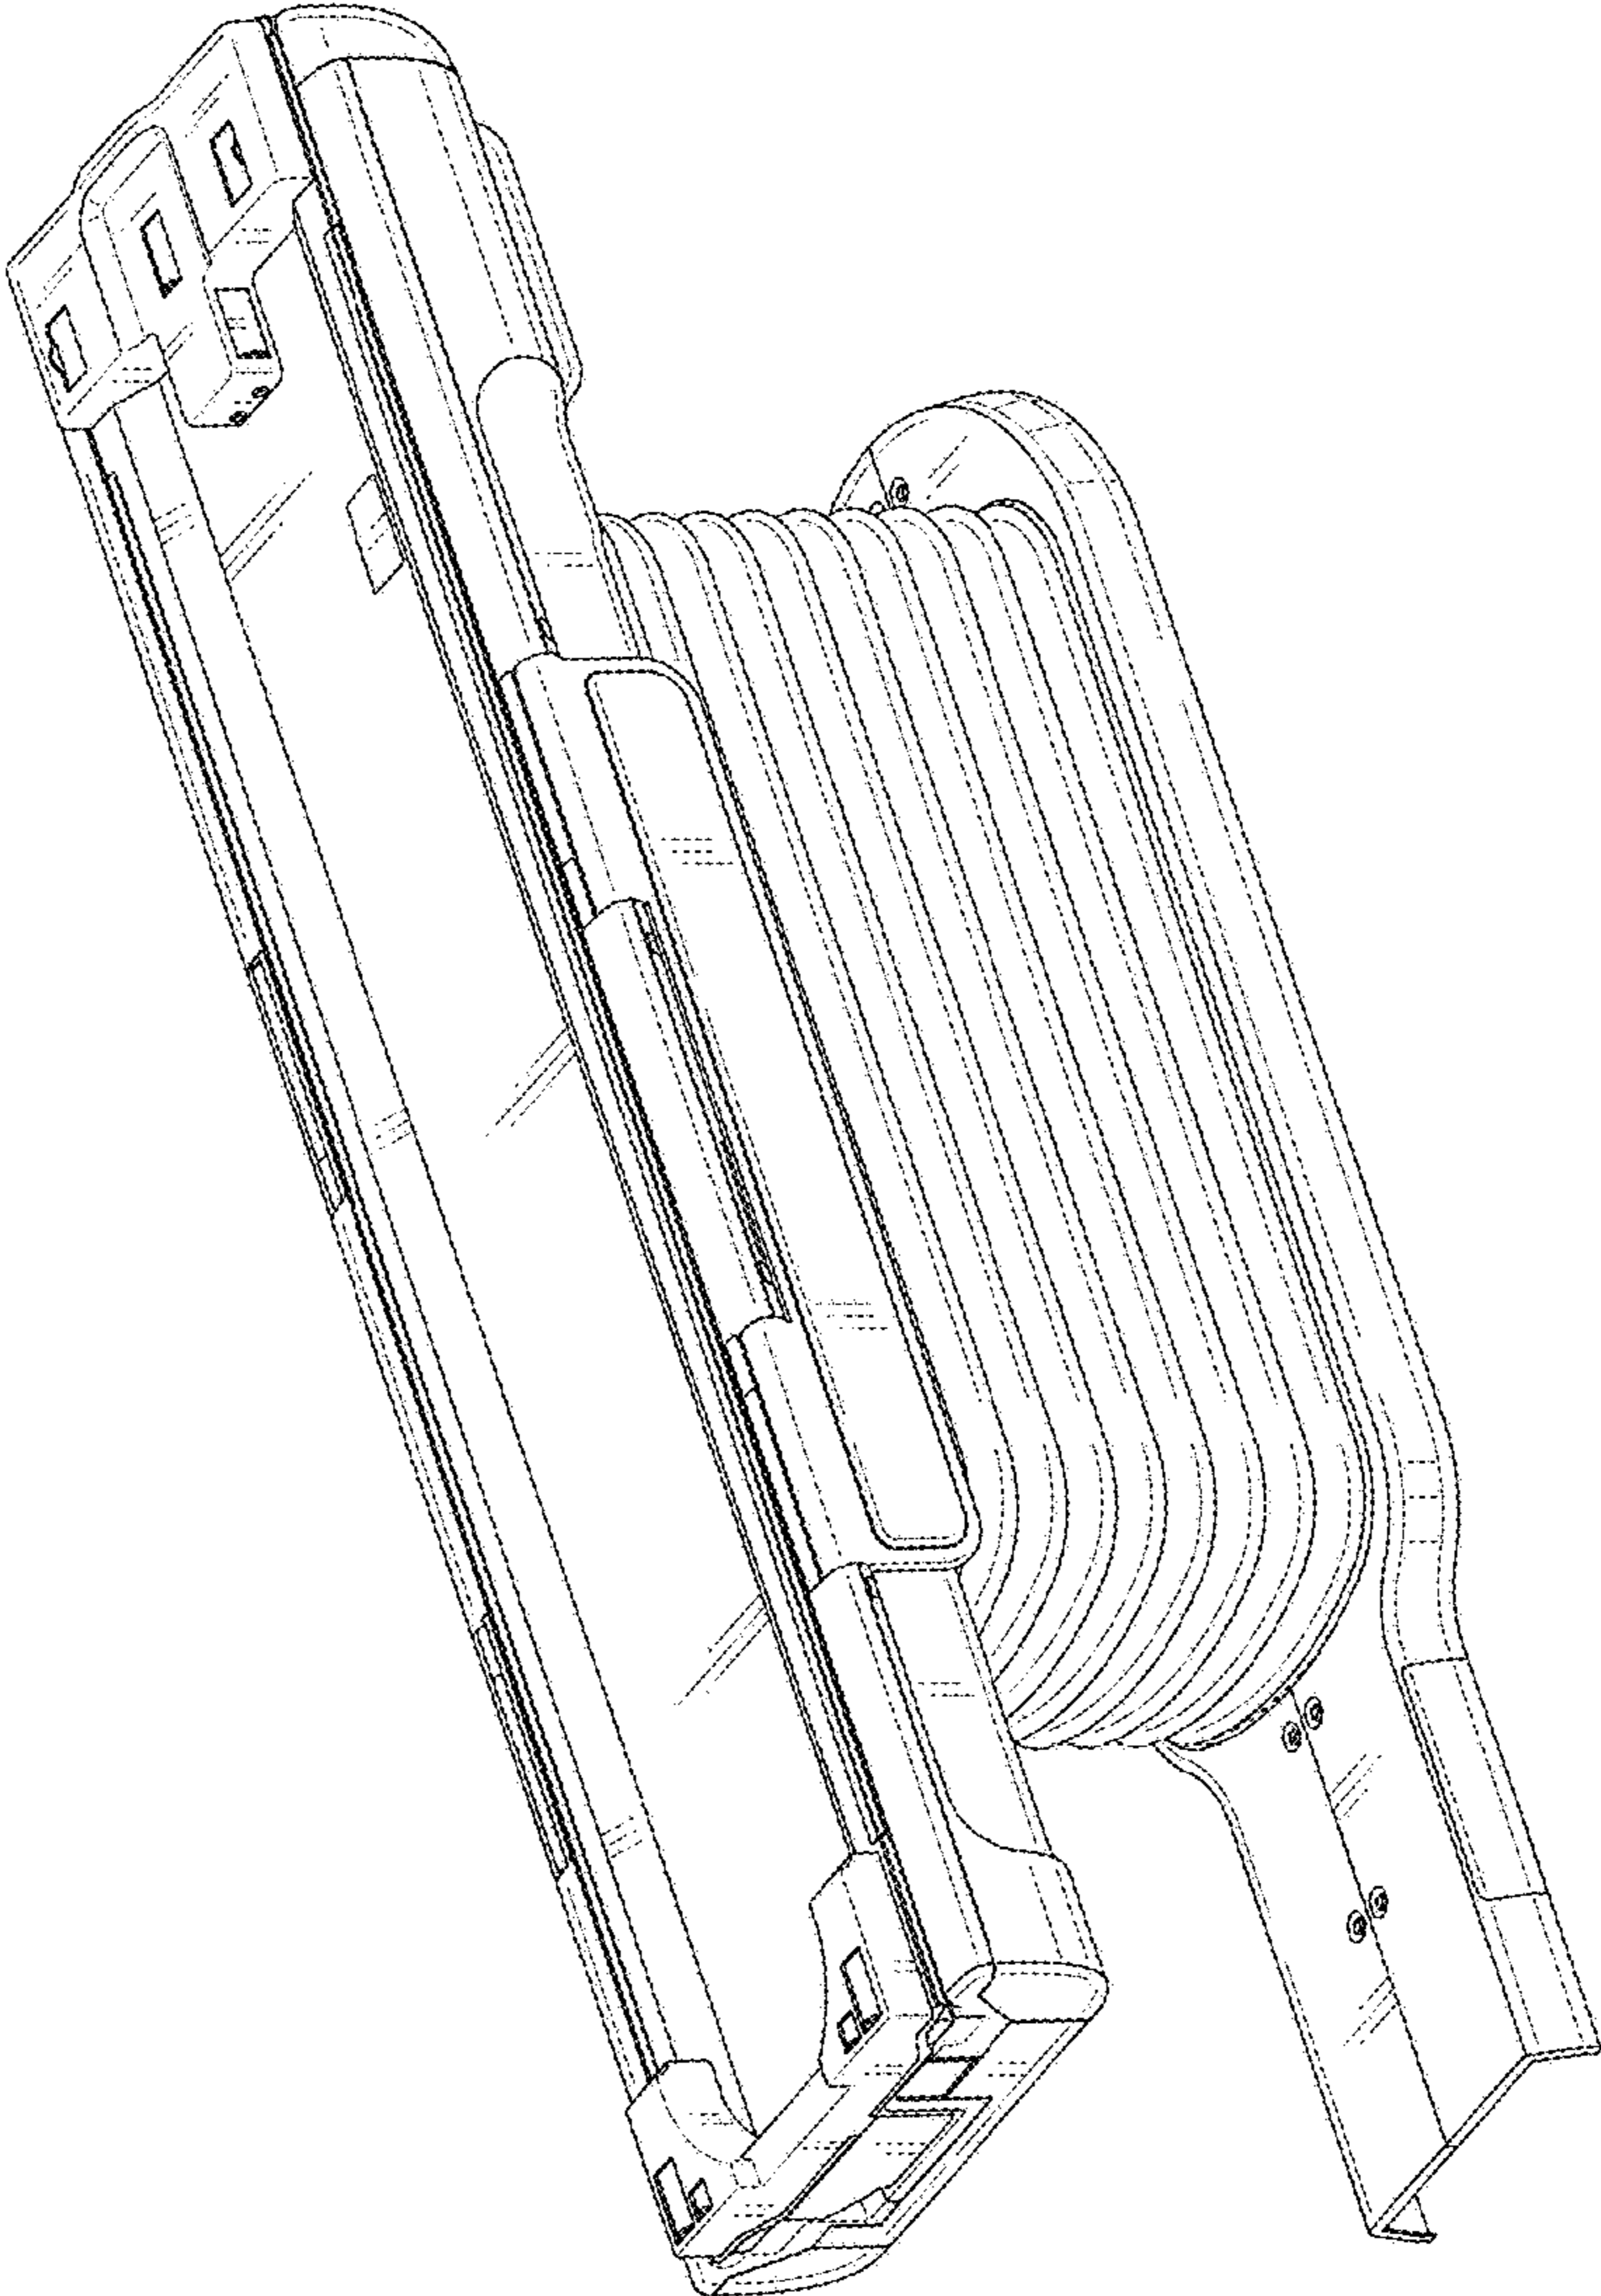


Fig. 2

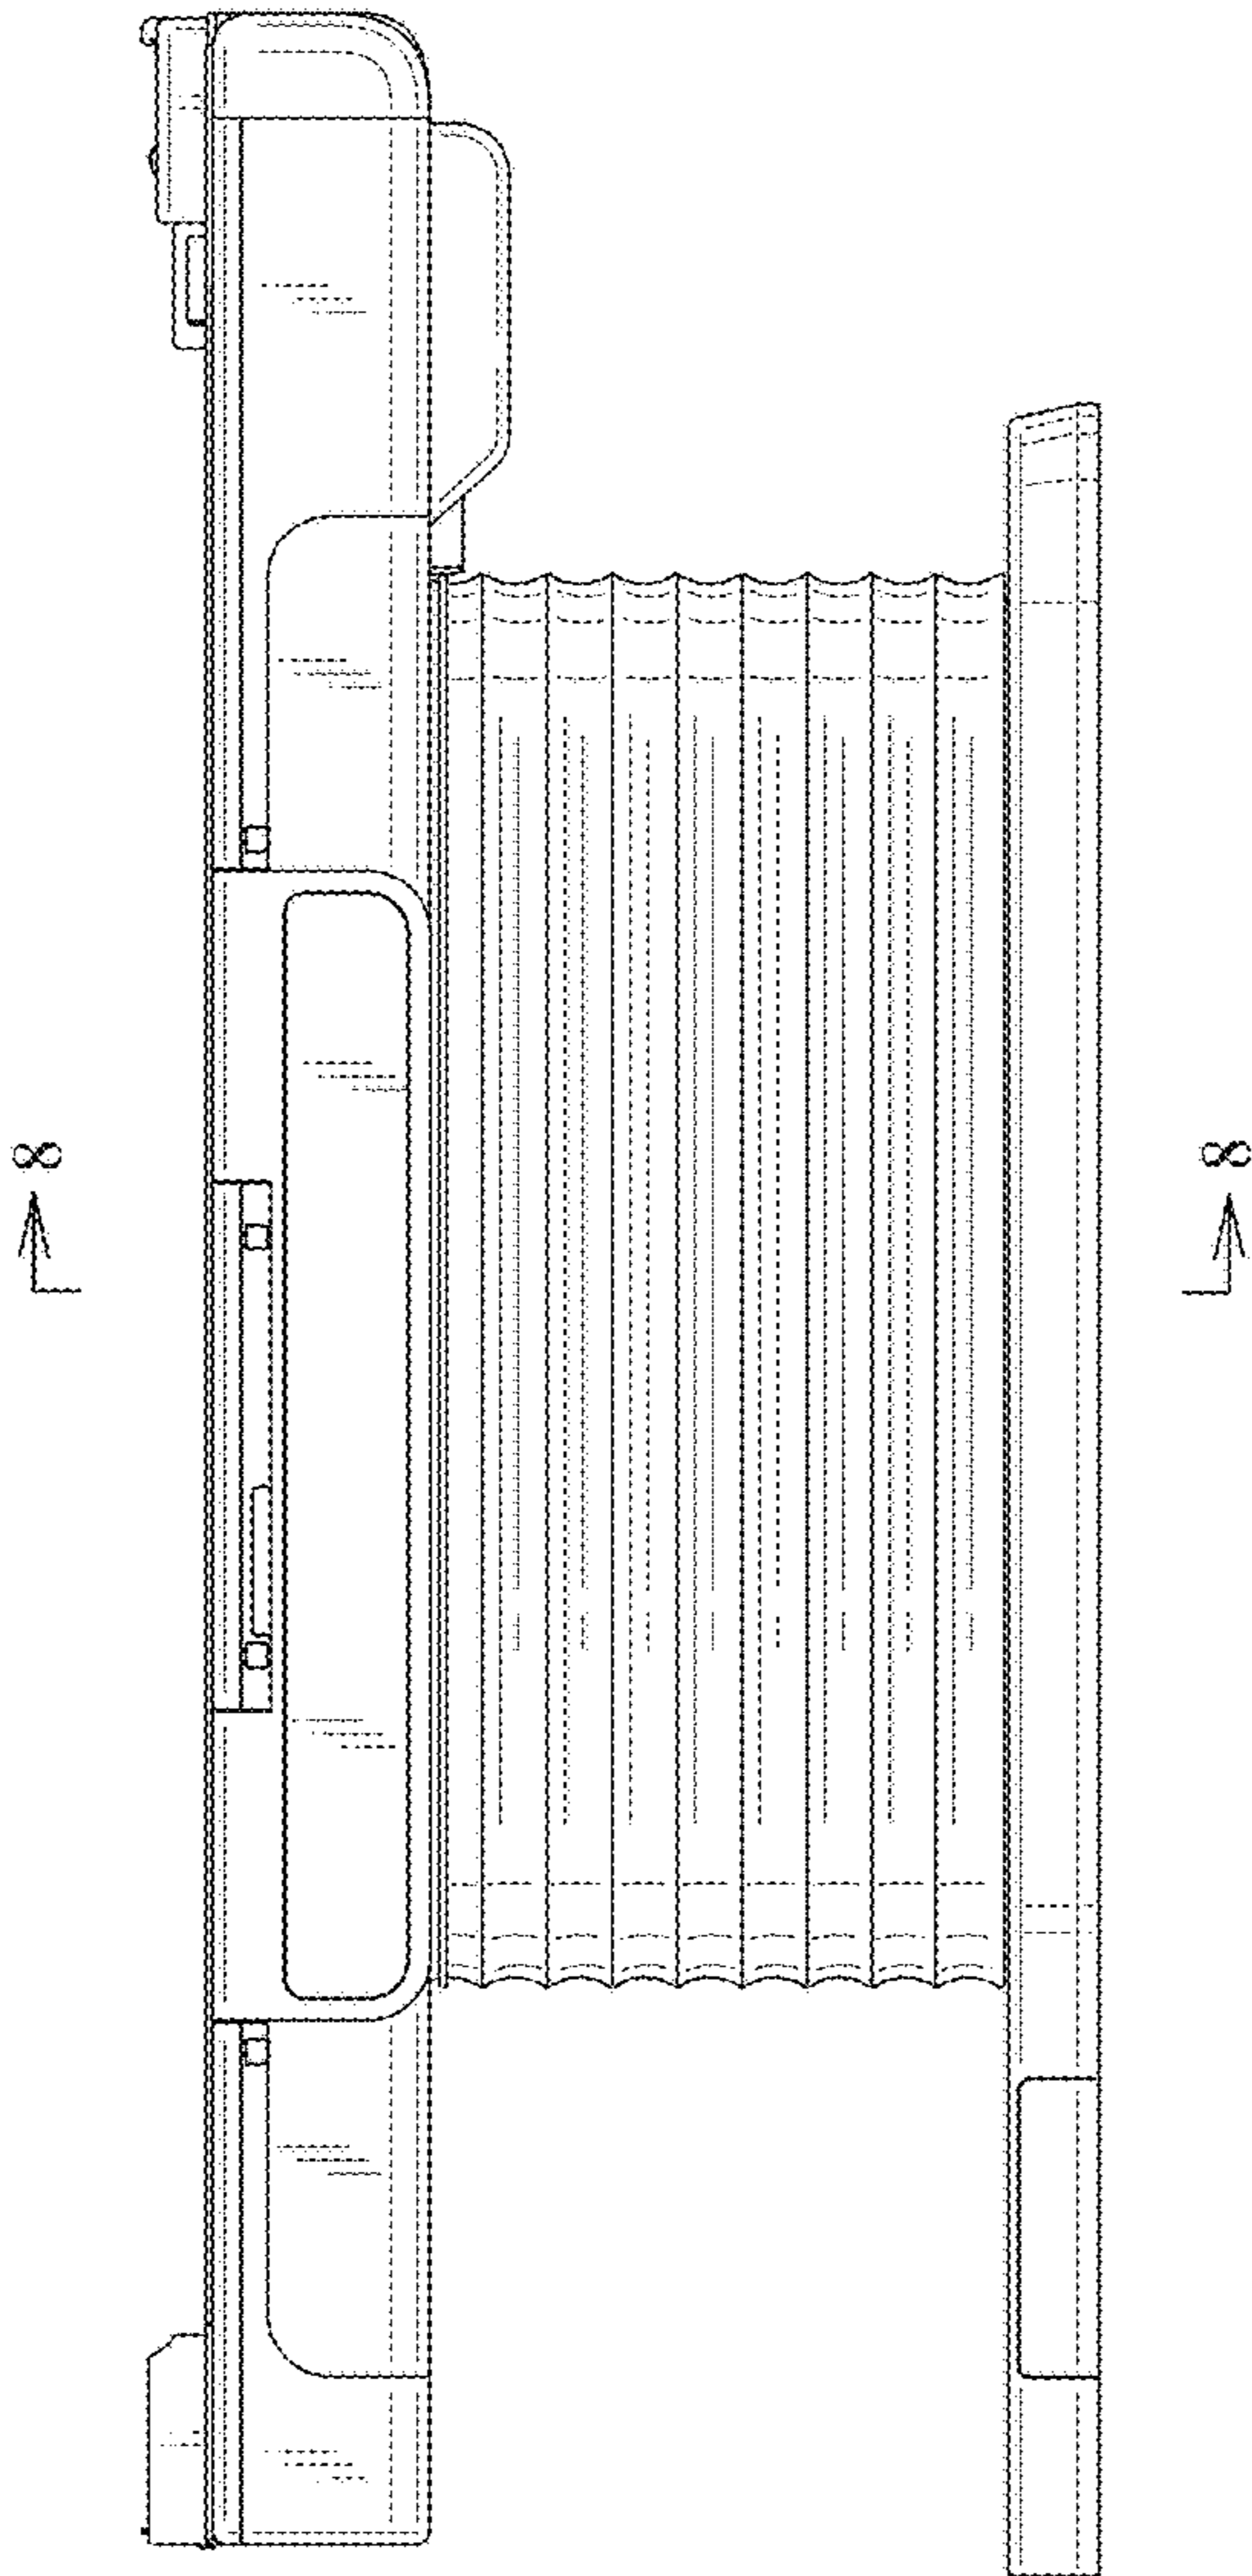


Fig. 3

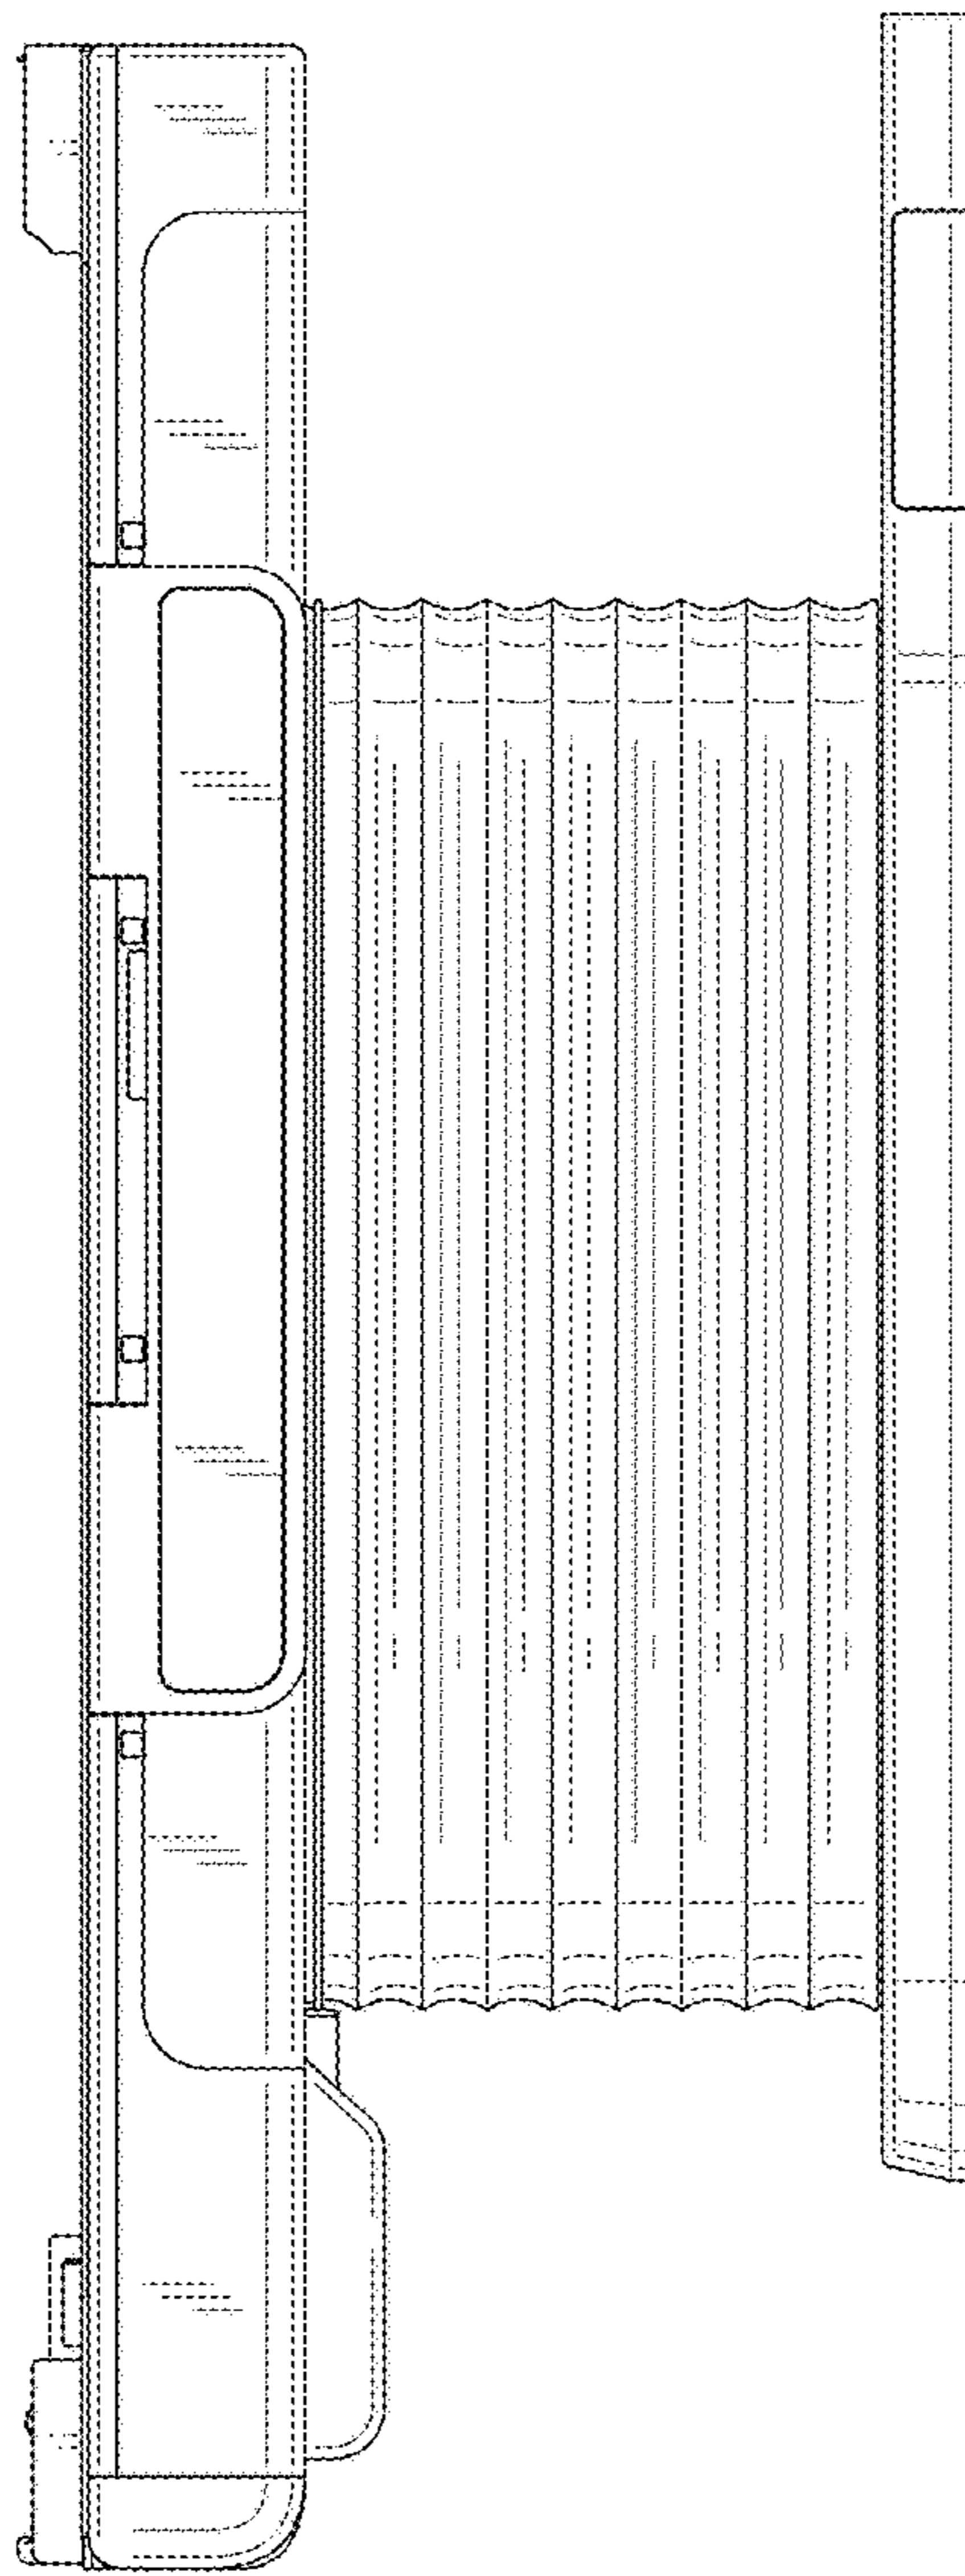


Fig. 4

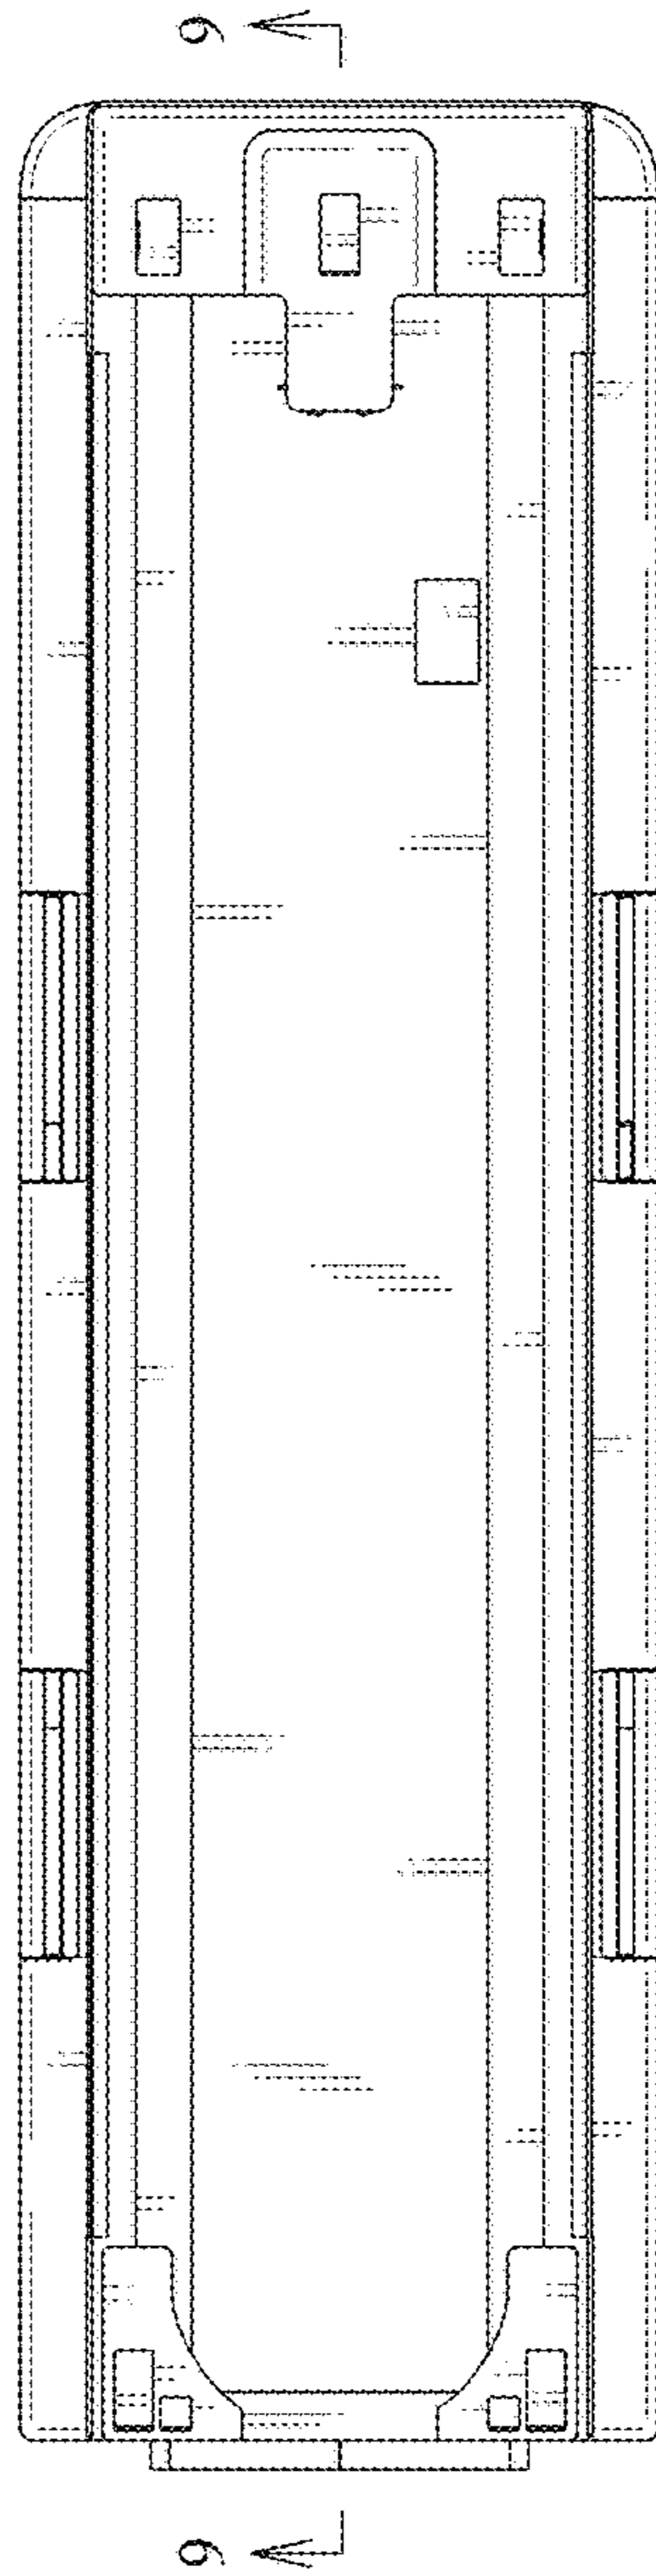


Fig. 5

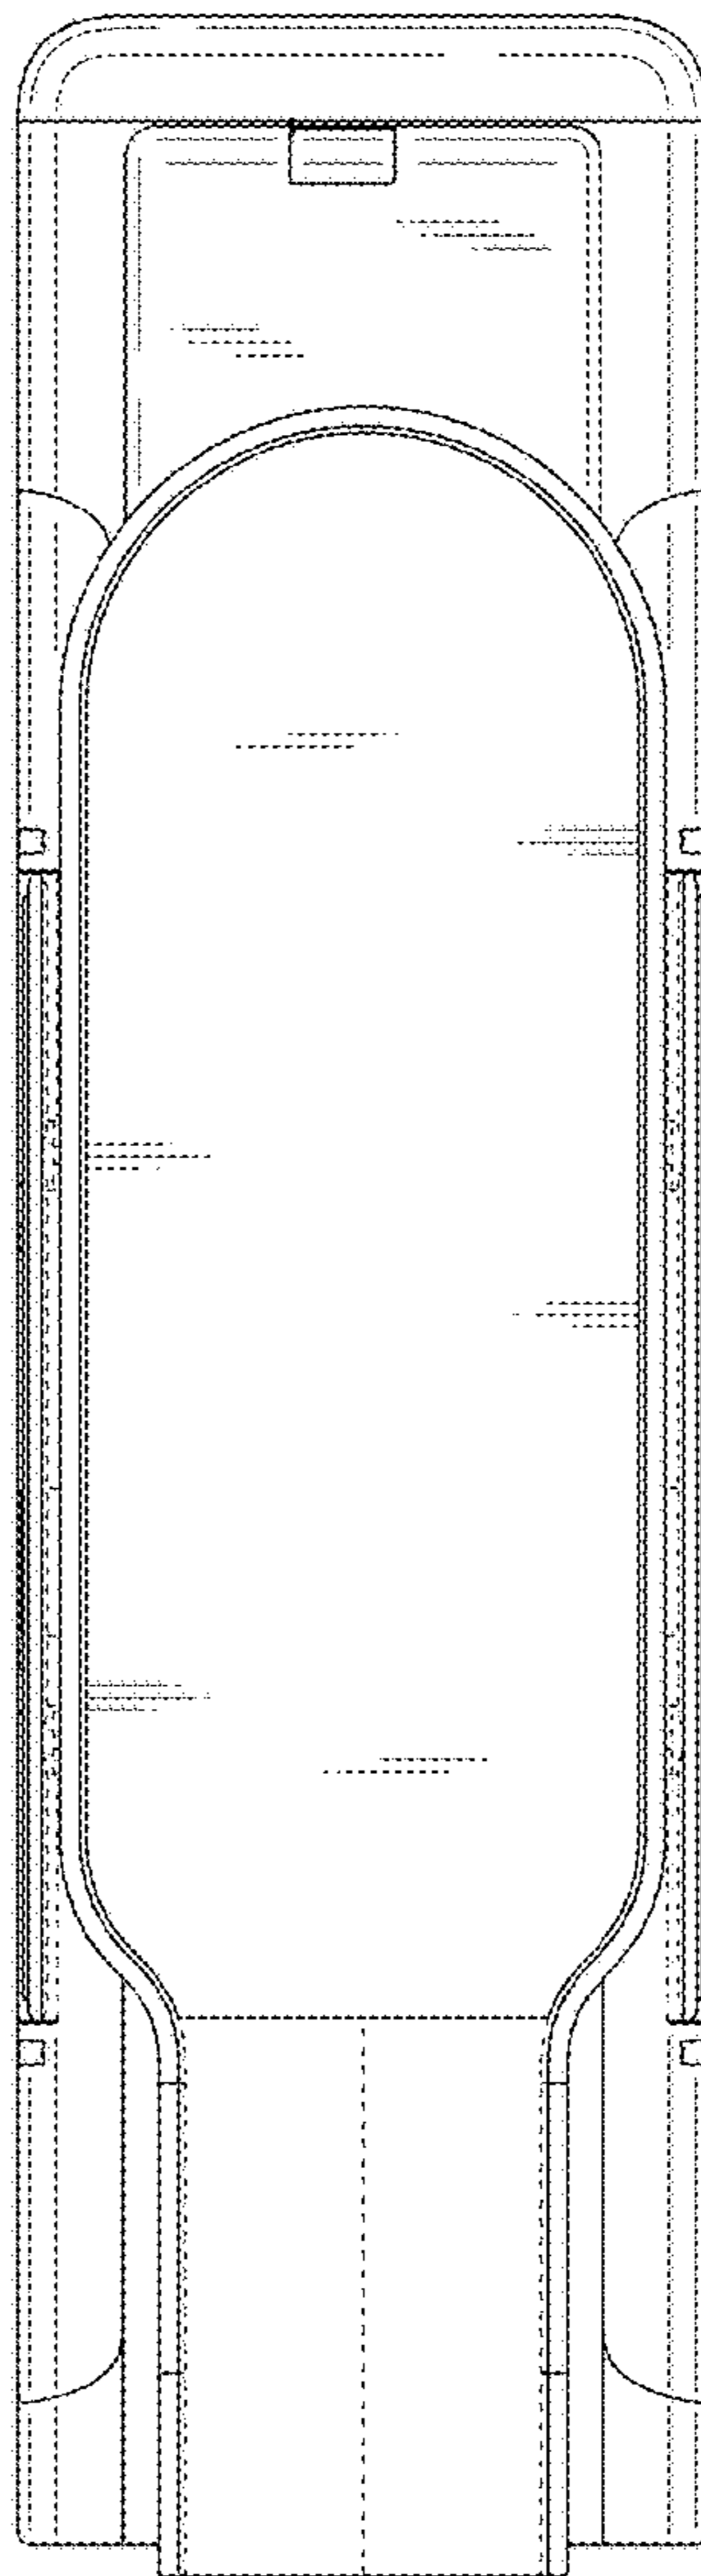


Fig. 6

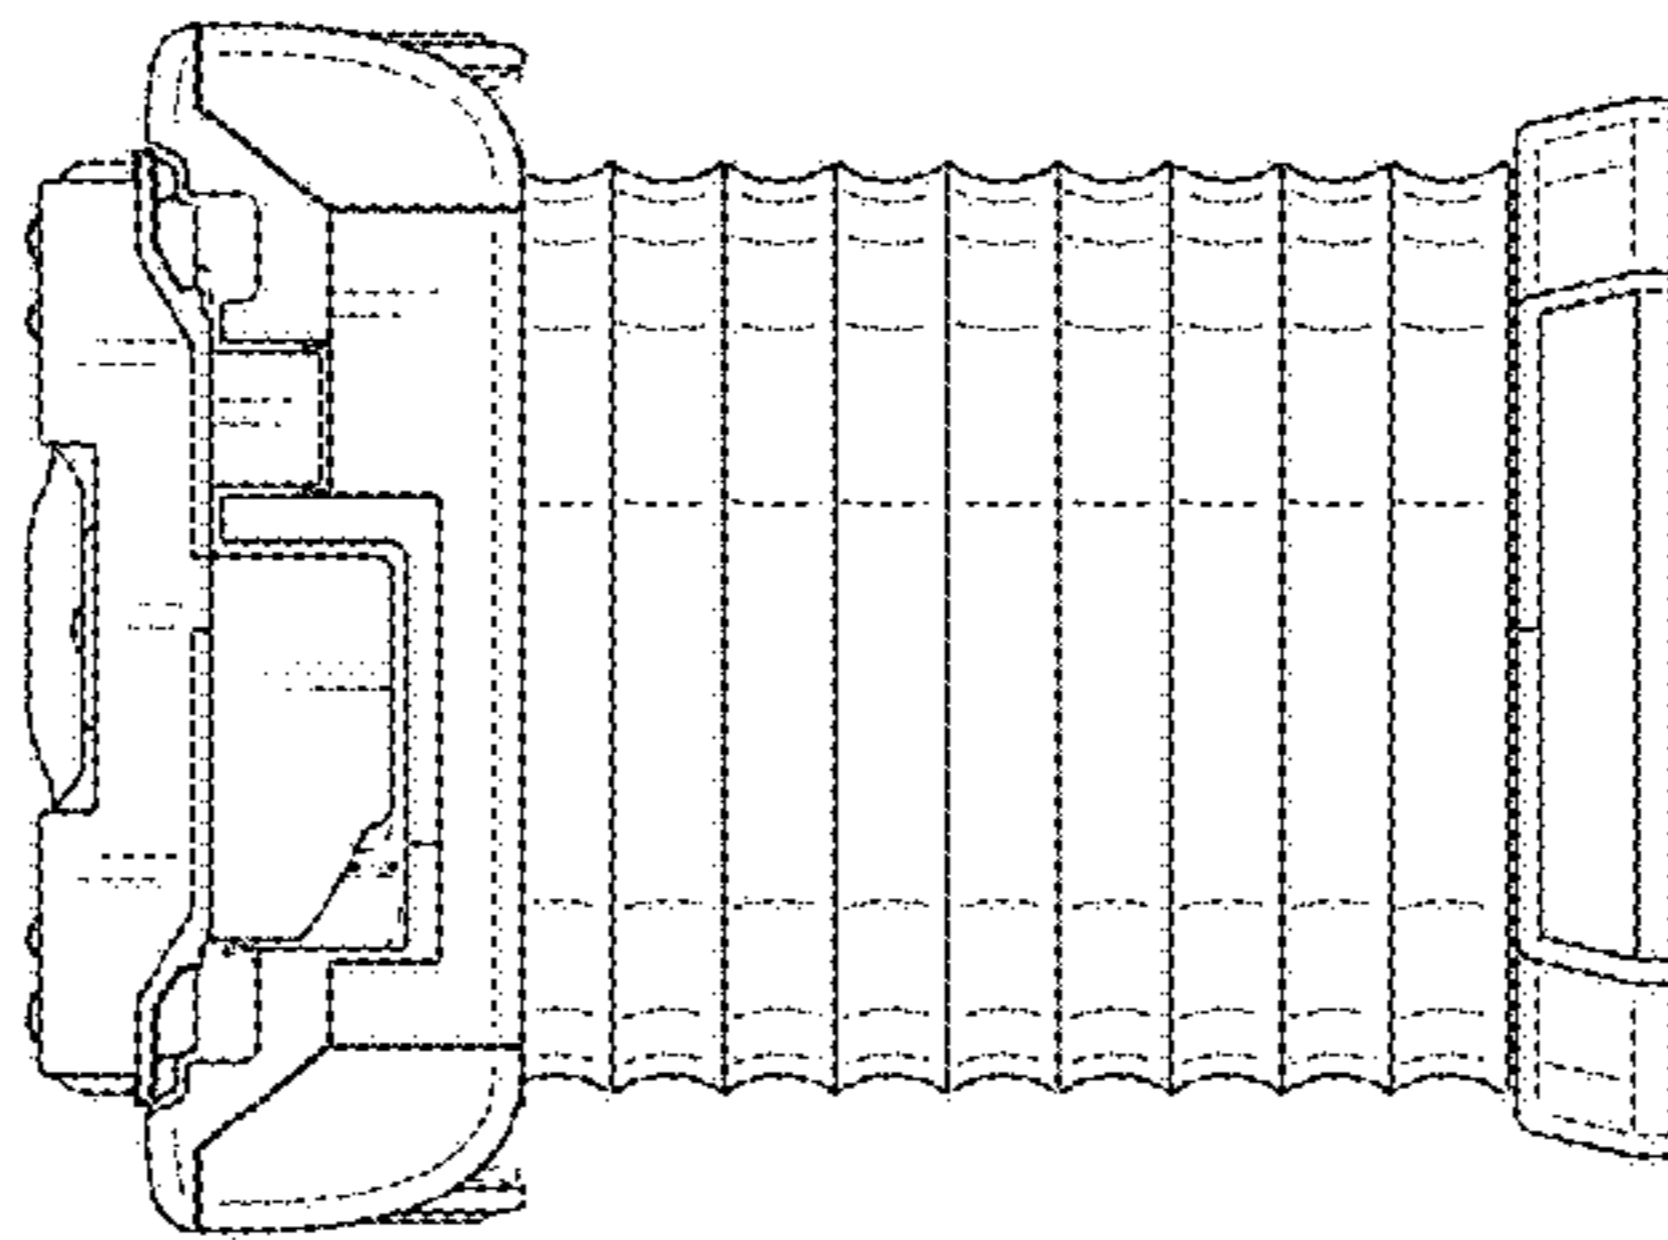


Fig. 7

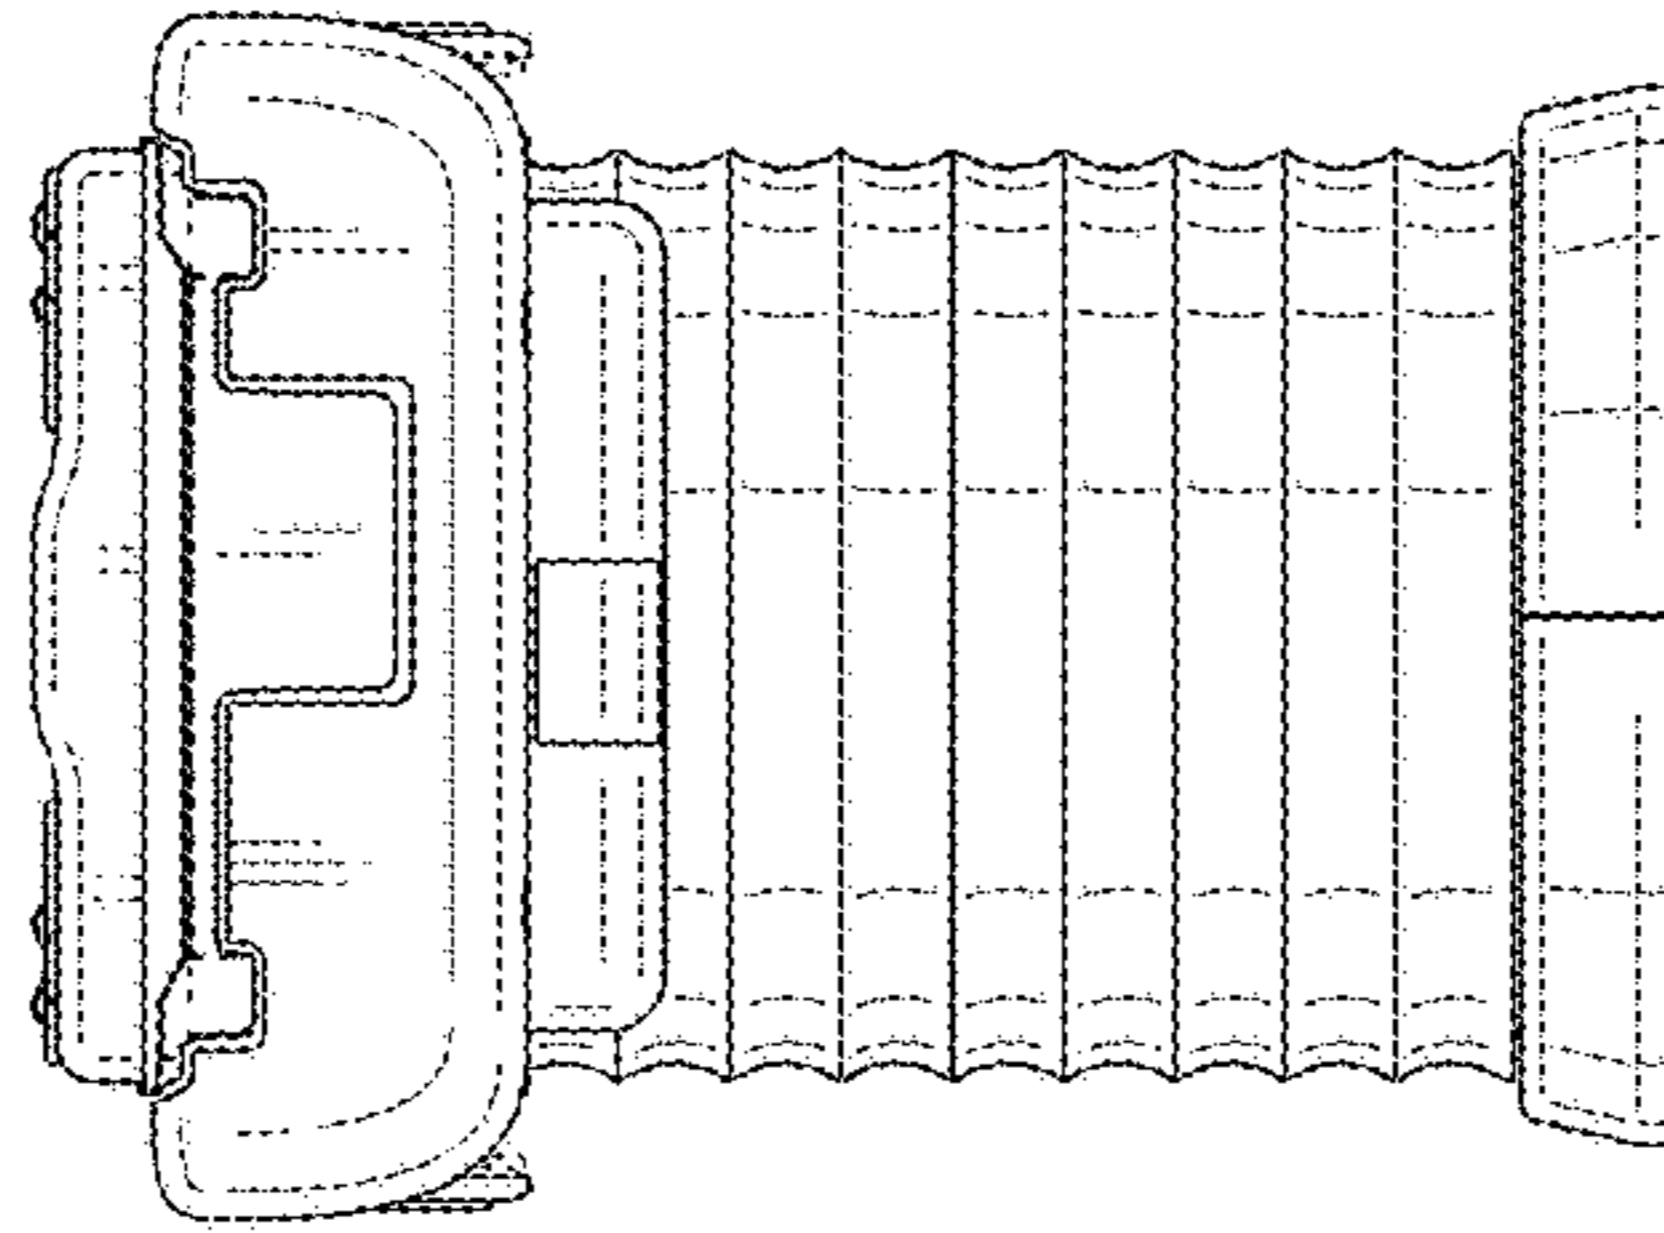


Fig. 8

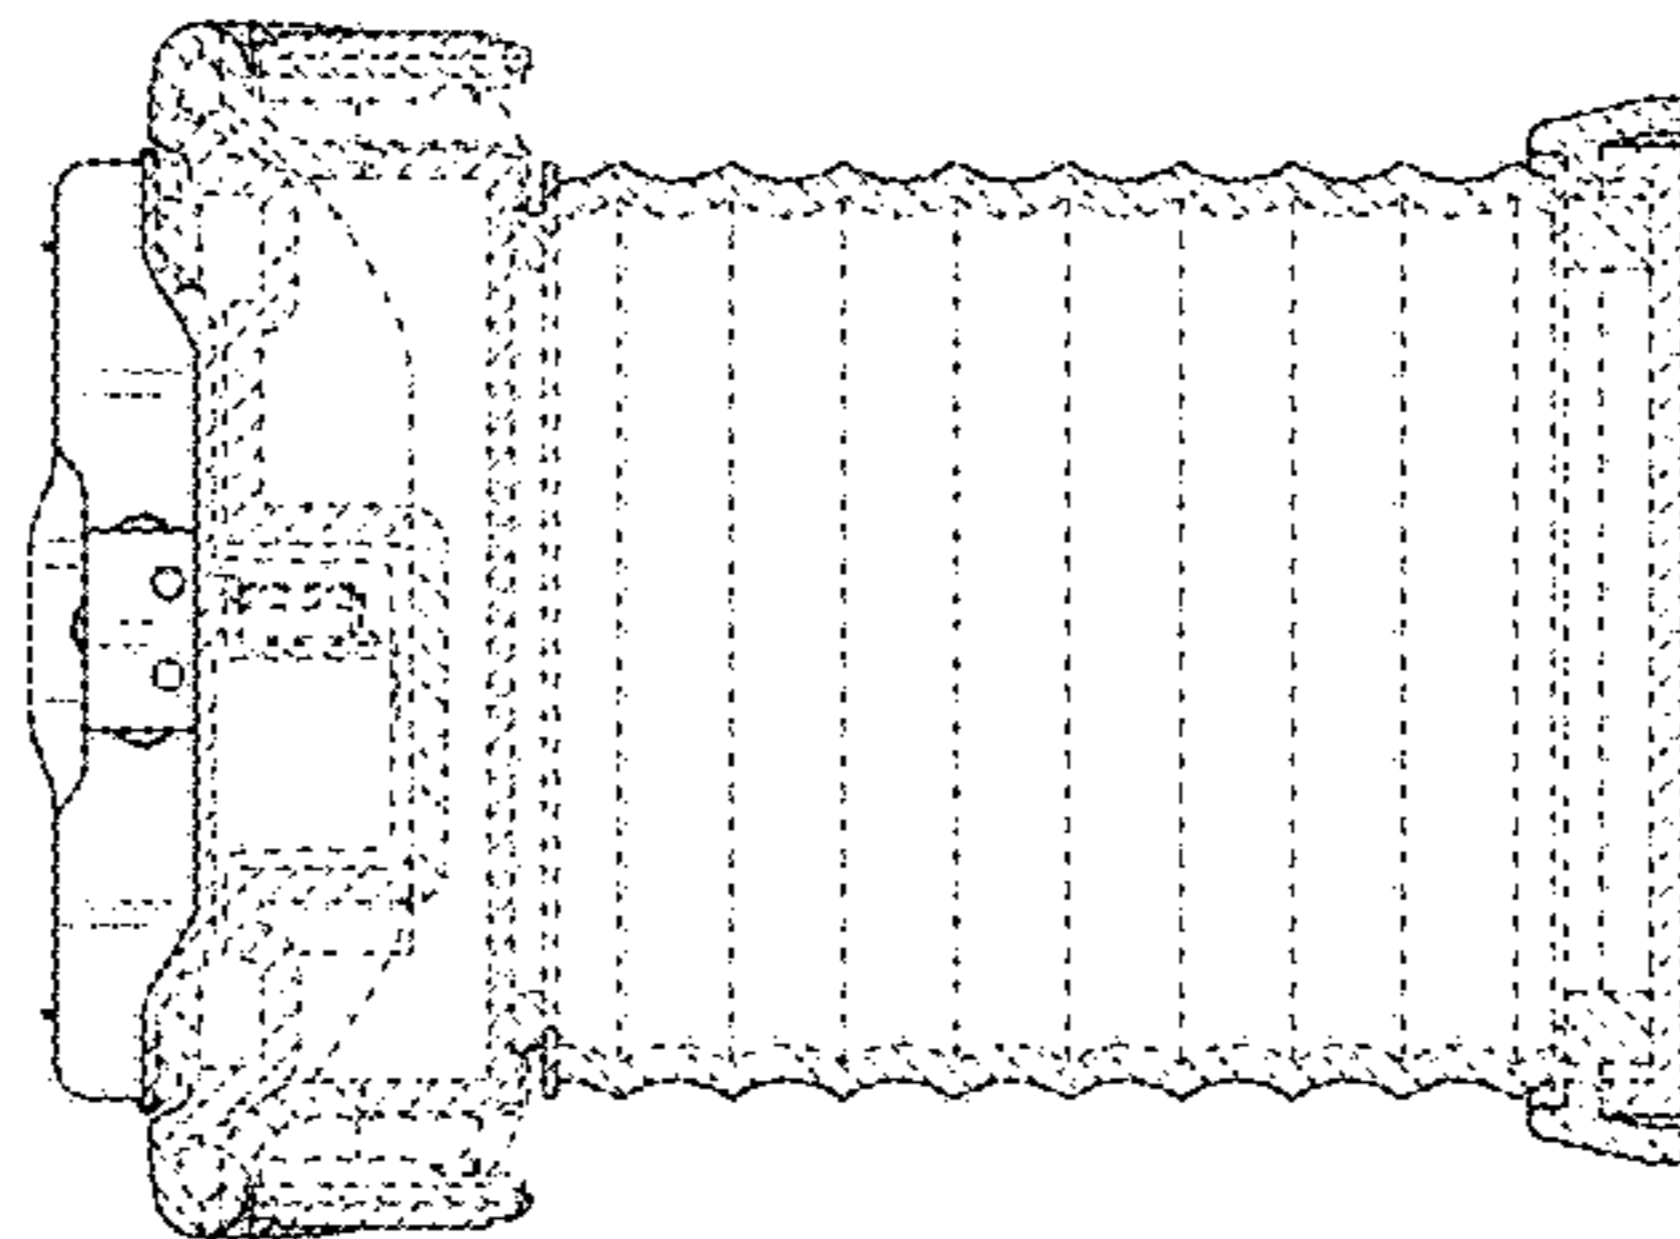


Fig. 9

