



US00D856519S

(12) **United States Design Patent** (10) **Patent No.:** **US D856,519 S**
Kim (45) **Date of Patent:** **** Aug. 13, 2019**

(54) **CHAIR FOR MAGNETIC RESONANCE IMAGING DEVICE**

D474,277 S * 5/2003 Juni D24/158
D492,998 S * 7/2004 Juni D24/158
D590,188 S * 4/2009 Tran D6/708.18
D595,981 S * 7/2009 Broering D6/367

(71) Applicant: **Samsung Electronics Co., Ltd.**,
Suwon-si (KR)

(Continued)

(72) Inventor: **Euisik Kim**, Seoul (KR)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **SAMSUNG ELECTRONICS CO., LTD.**, Gyeonggi-Do (KR)

CN 304001108 S 1/2017
EM 0024469480002 4/2014

(Continued)

(**) Term: **15 Years**

Primary Examiner — Anhdao Doan

(21) Appl. No.: **29/644,639**

(74) *Attorney, Agent, or Firm* — Cantor Colburn LLP

(22) Filed: **Apr. 19, 2018**

(57) **CLAIM**

(30) **Foreign Application Priority Data**

The ornamental design for a chair for magnetic resonance imaging device, as shown and described.

Nov. 15, 2017 (KR) 30-2017-0053326

DESCRIPTION

(51) **LOC (12) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/159**; D6/334

(58) **Field of Classification Search**
USPC D24/107, 158–161, 185, 186, 187, 231,
D24/183, 184; D6/334, 335, 349, 353,
D6/364, 708, 708.17, 708.18, 708.21
CPC .. A61B 6/03; A61B 6/035; A61B 5/05; A61B
5/055; A61B 6/04; A61B 6/0407; G01N
2223/1013; G01N 2223/1016; A61N
2005/1054; A61N 2005/1055; A61N
2005/1074; A61G 13/1235; A61G
2210/50; A61F 5/3723; A61F 5/3761
See application file for complete search history.

FIG. 1 is a front perspective view of a chair for magnetic resonance imaging (“MRI”) device, showing my new design;

FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a top view thereof;
FIG. 7 is a bottom view thereof.
FIG. 8 is a rear perspective view thereof;
FIG. 9 is another front perspective view thereof, in a reclined position; and,
FIG. 10 is another front perspective view thereof showing an environment of use, in which a seat, a headrest and an armrest are shown.


The broken lines illustrating portions of the chair for MRI device form no part of the claimed design. The broken lines illustrating the seat, the headrest and the armrest in FIG. 10 are for environmental purposes only and form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D255,077 S * 5/1980 Garza D6/708.17
D351,742 S * 10/1994 Phleps D24/183
D354,177 S * 1/1995 Schwaegerle D24/183
D462,189 S * 9/2002 Brockway D6/367

1 Claim, 10 Drawing Sheets

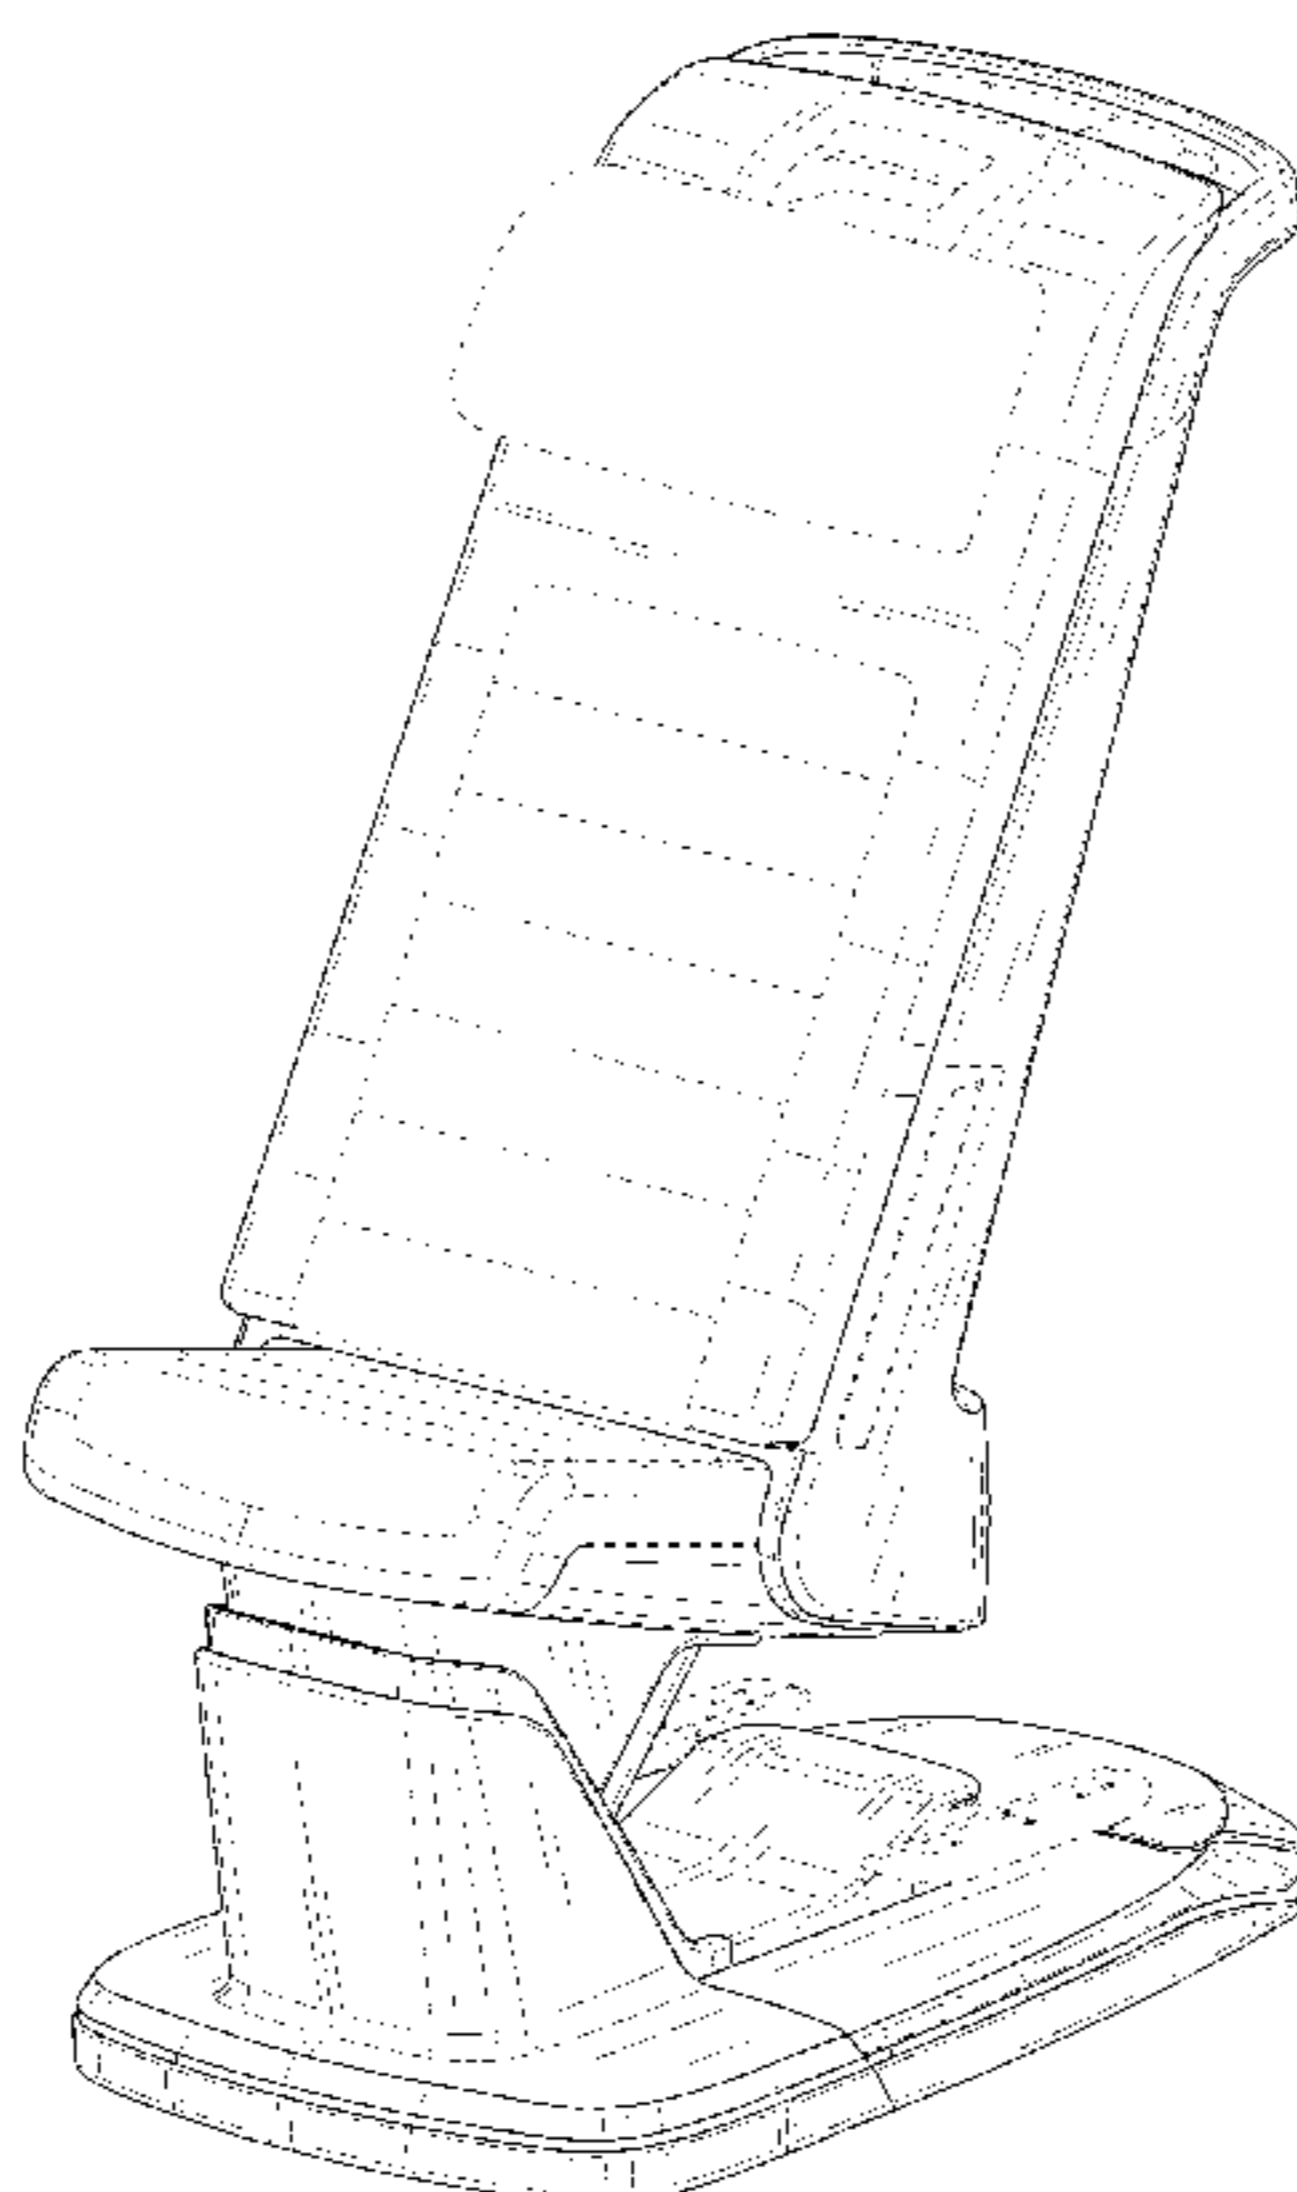

(56)

References Cited

U.S. PATENT DOCUMENTS

D678,686 S * 3/2013 Mizuno D6/335
D824,032 S * 7/2018 Poulsen D24/159
2015/0135441 A1* 5/2015 Sommer A61G 13/0036
5/613

FOREIGN PATENT DOCUMENTS

EM 0024613840001 5/2014
EM 0033391420006 8/2016

* cited by examiner

FIG. 1

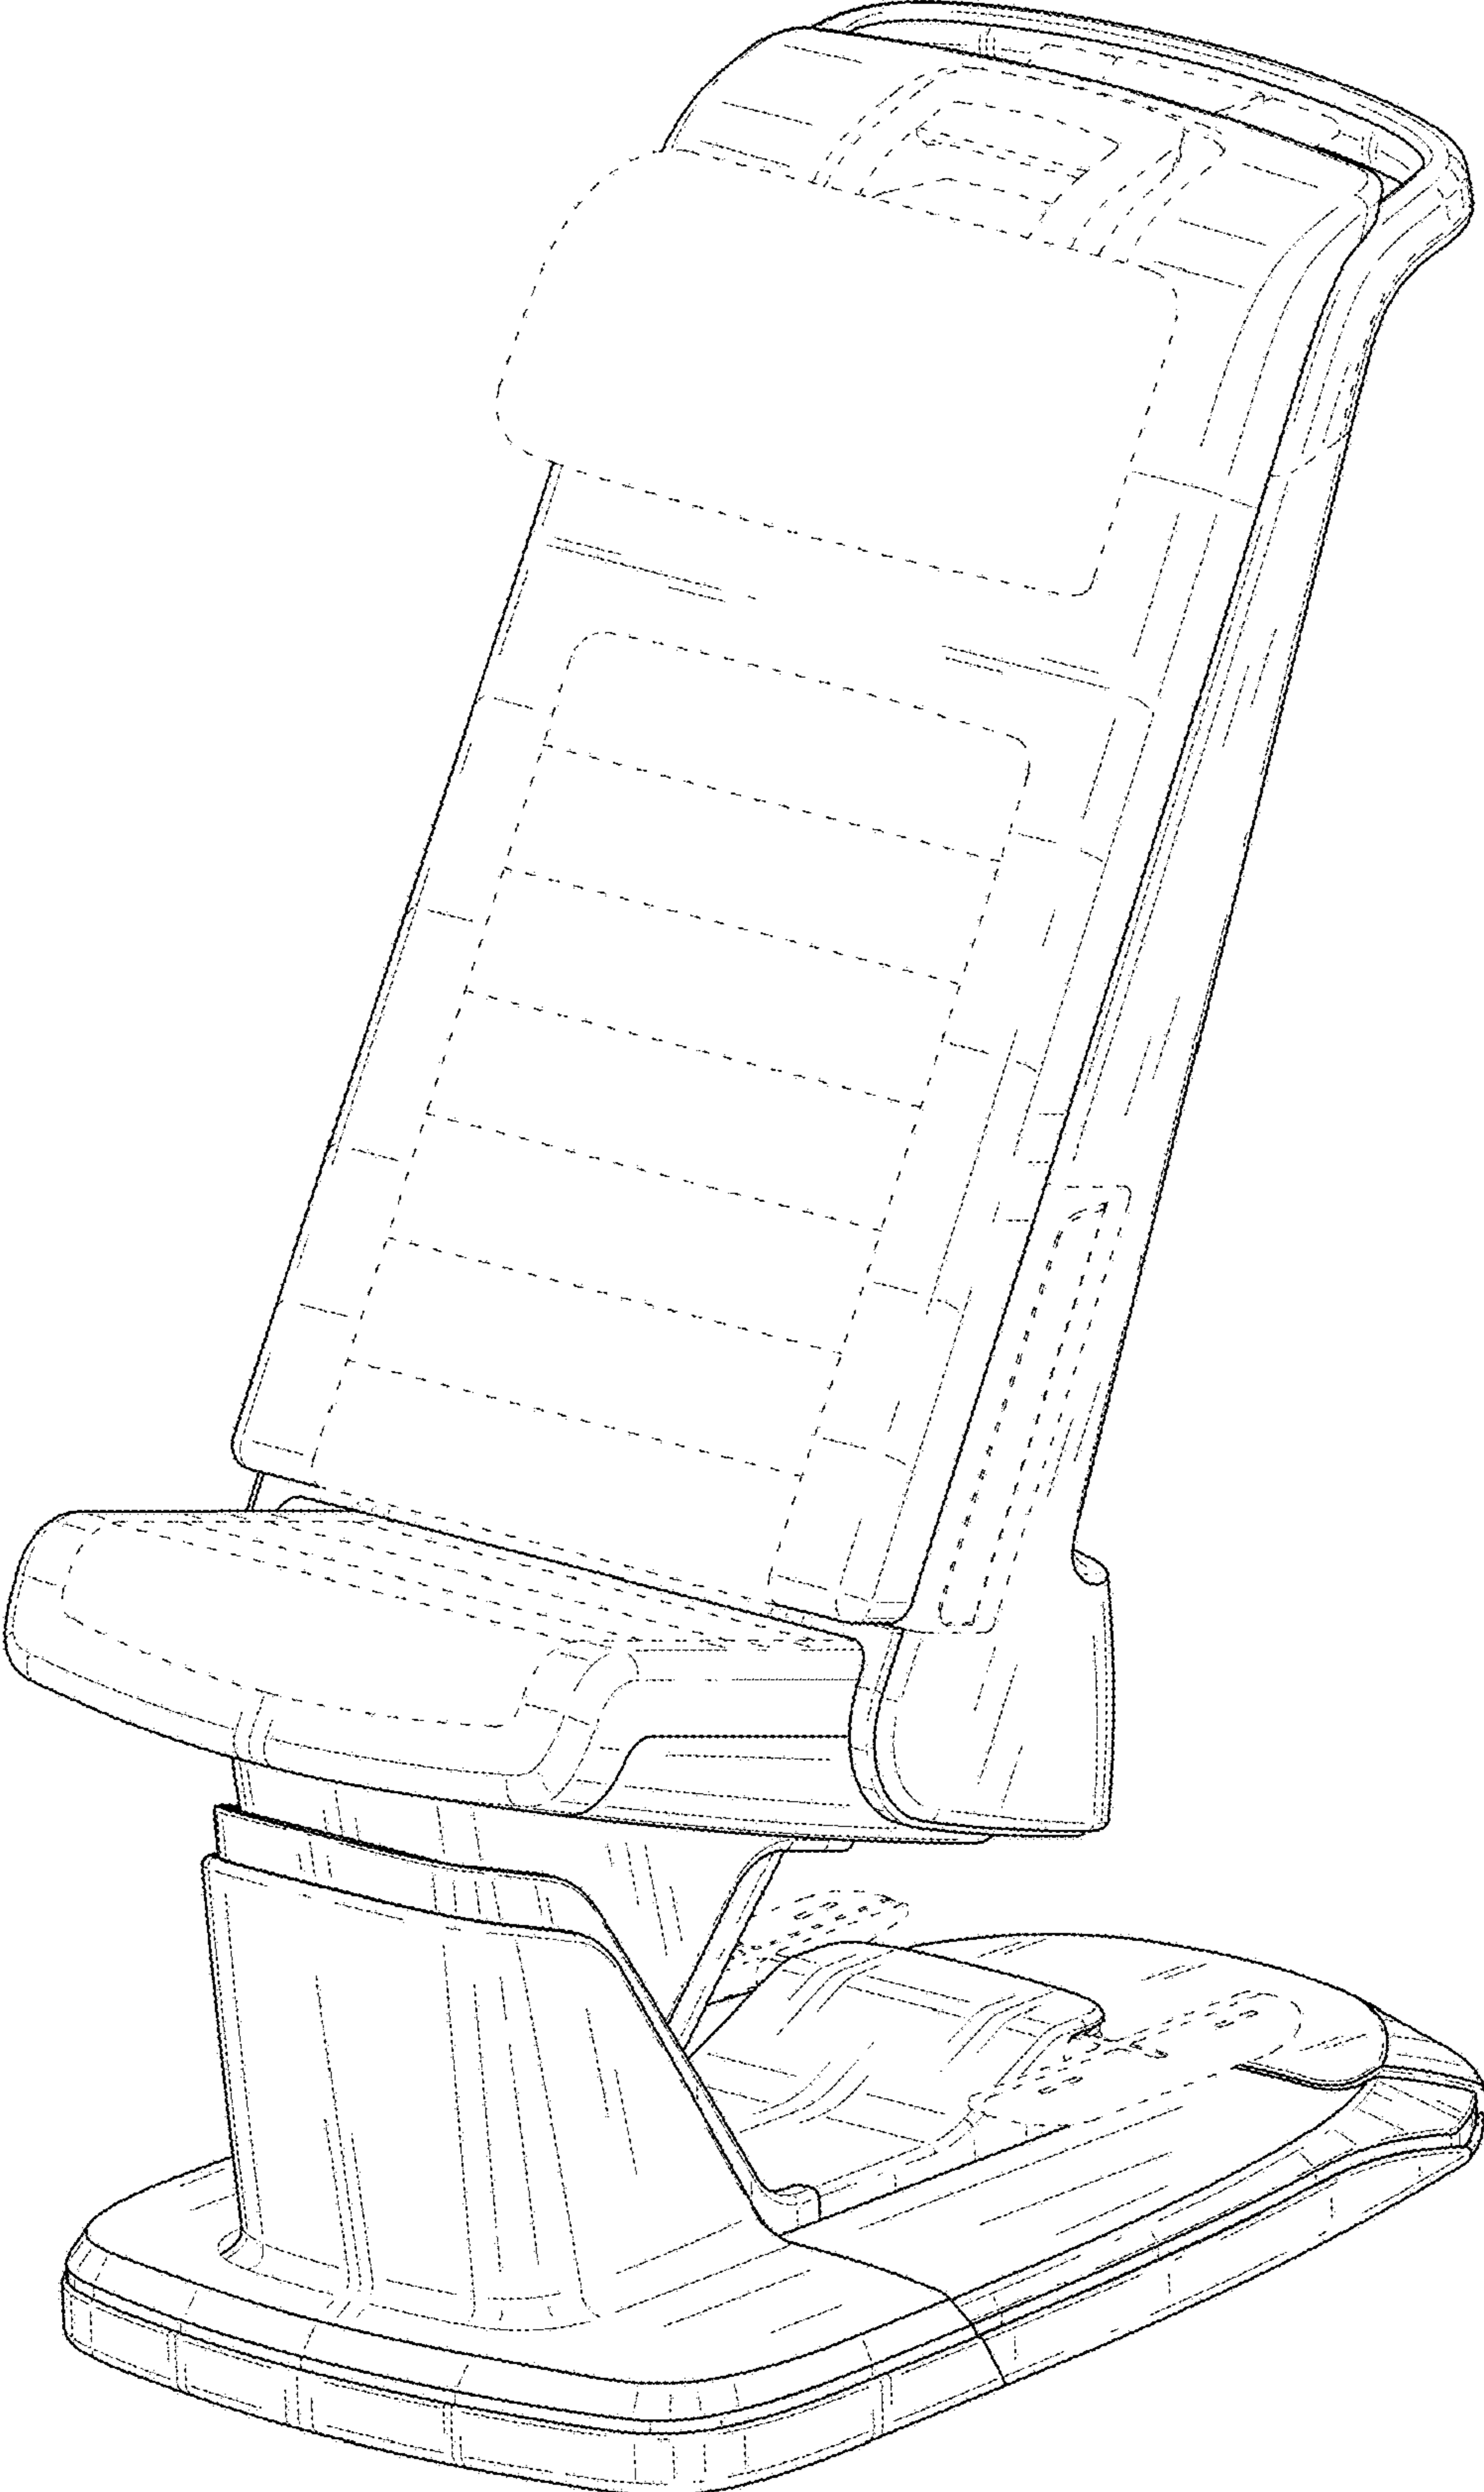


FIG. 2

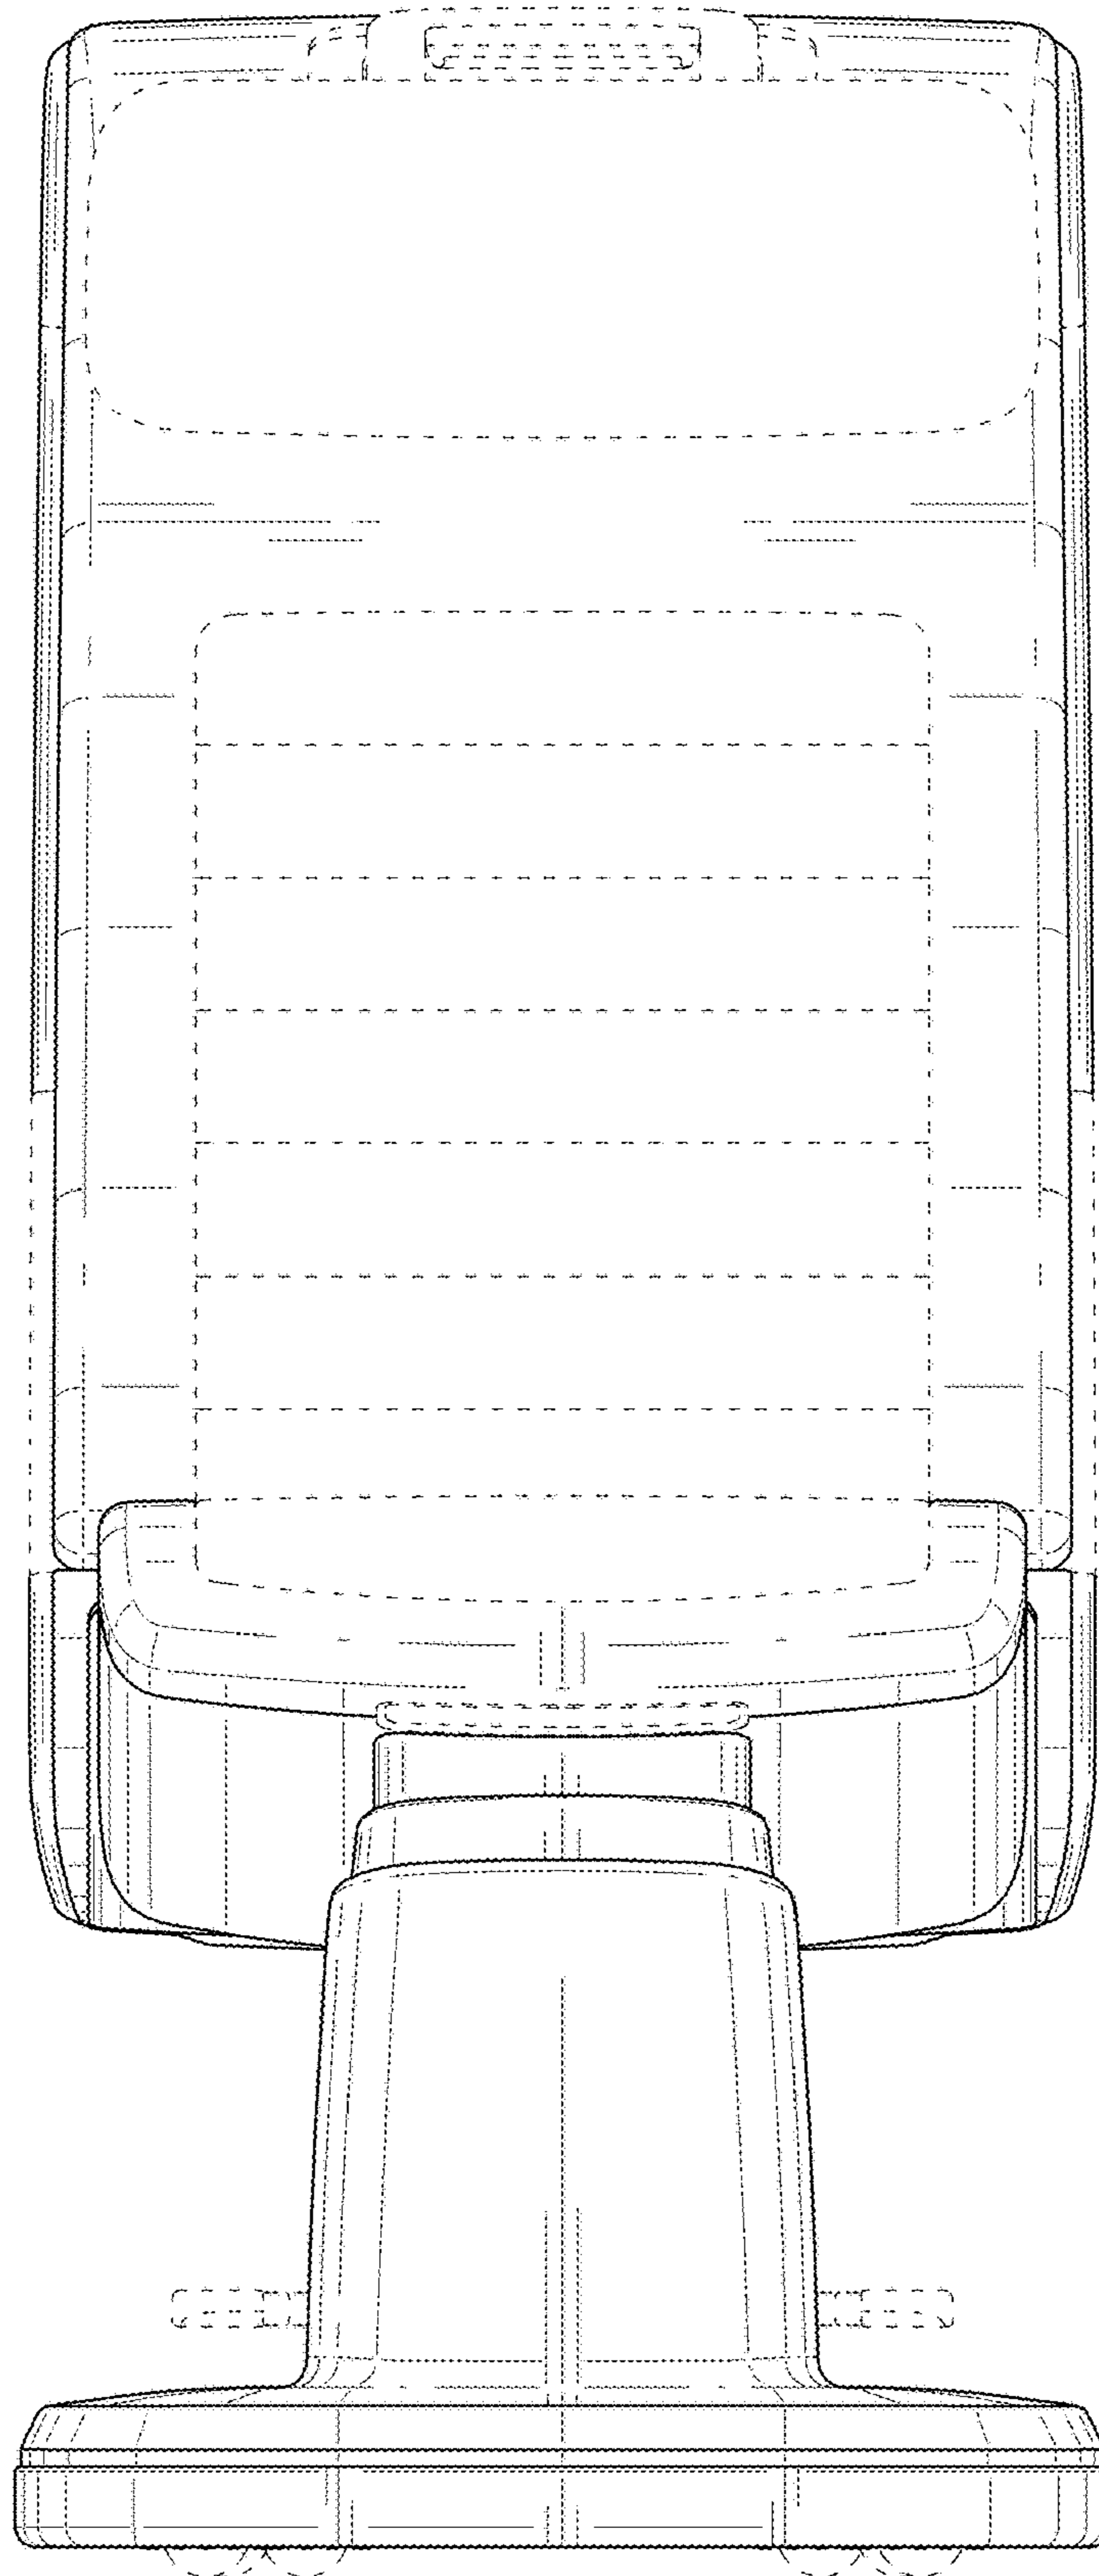


FIG. 3

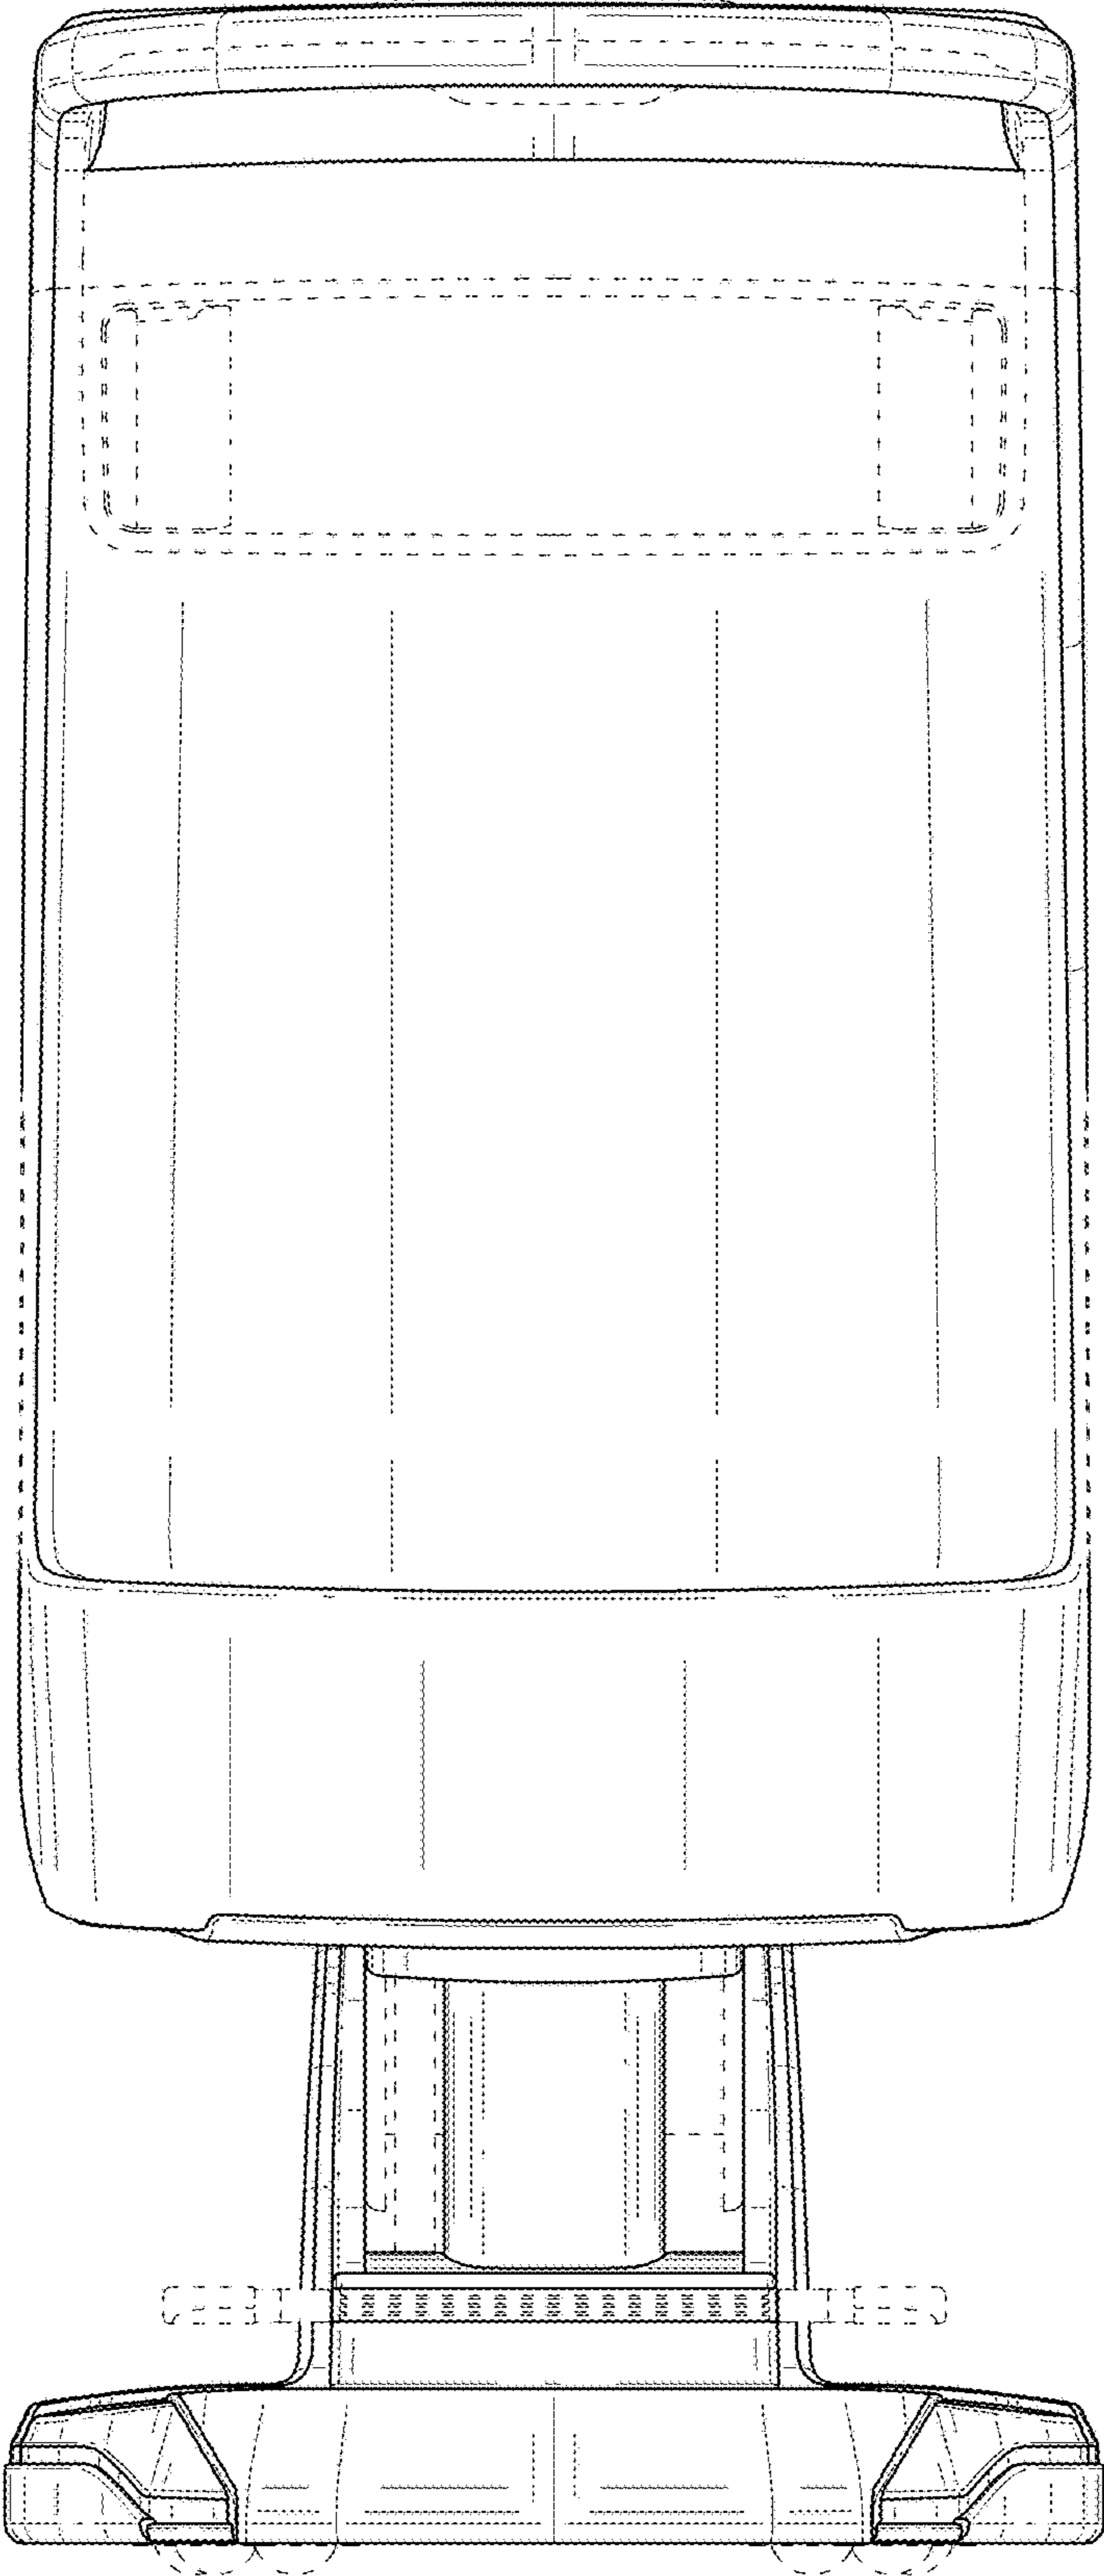


FIG. 4

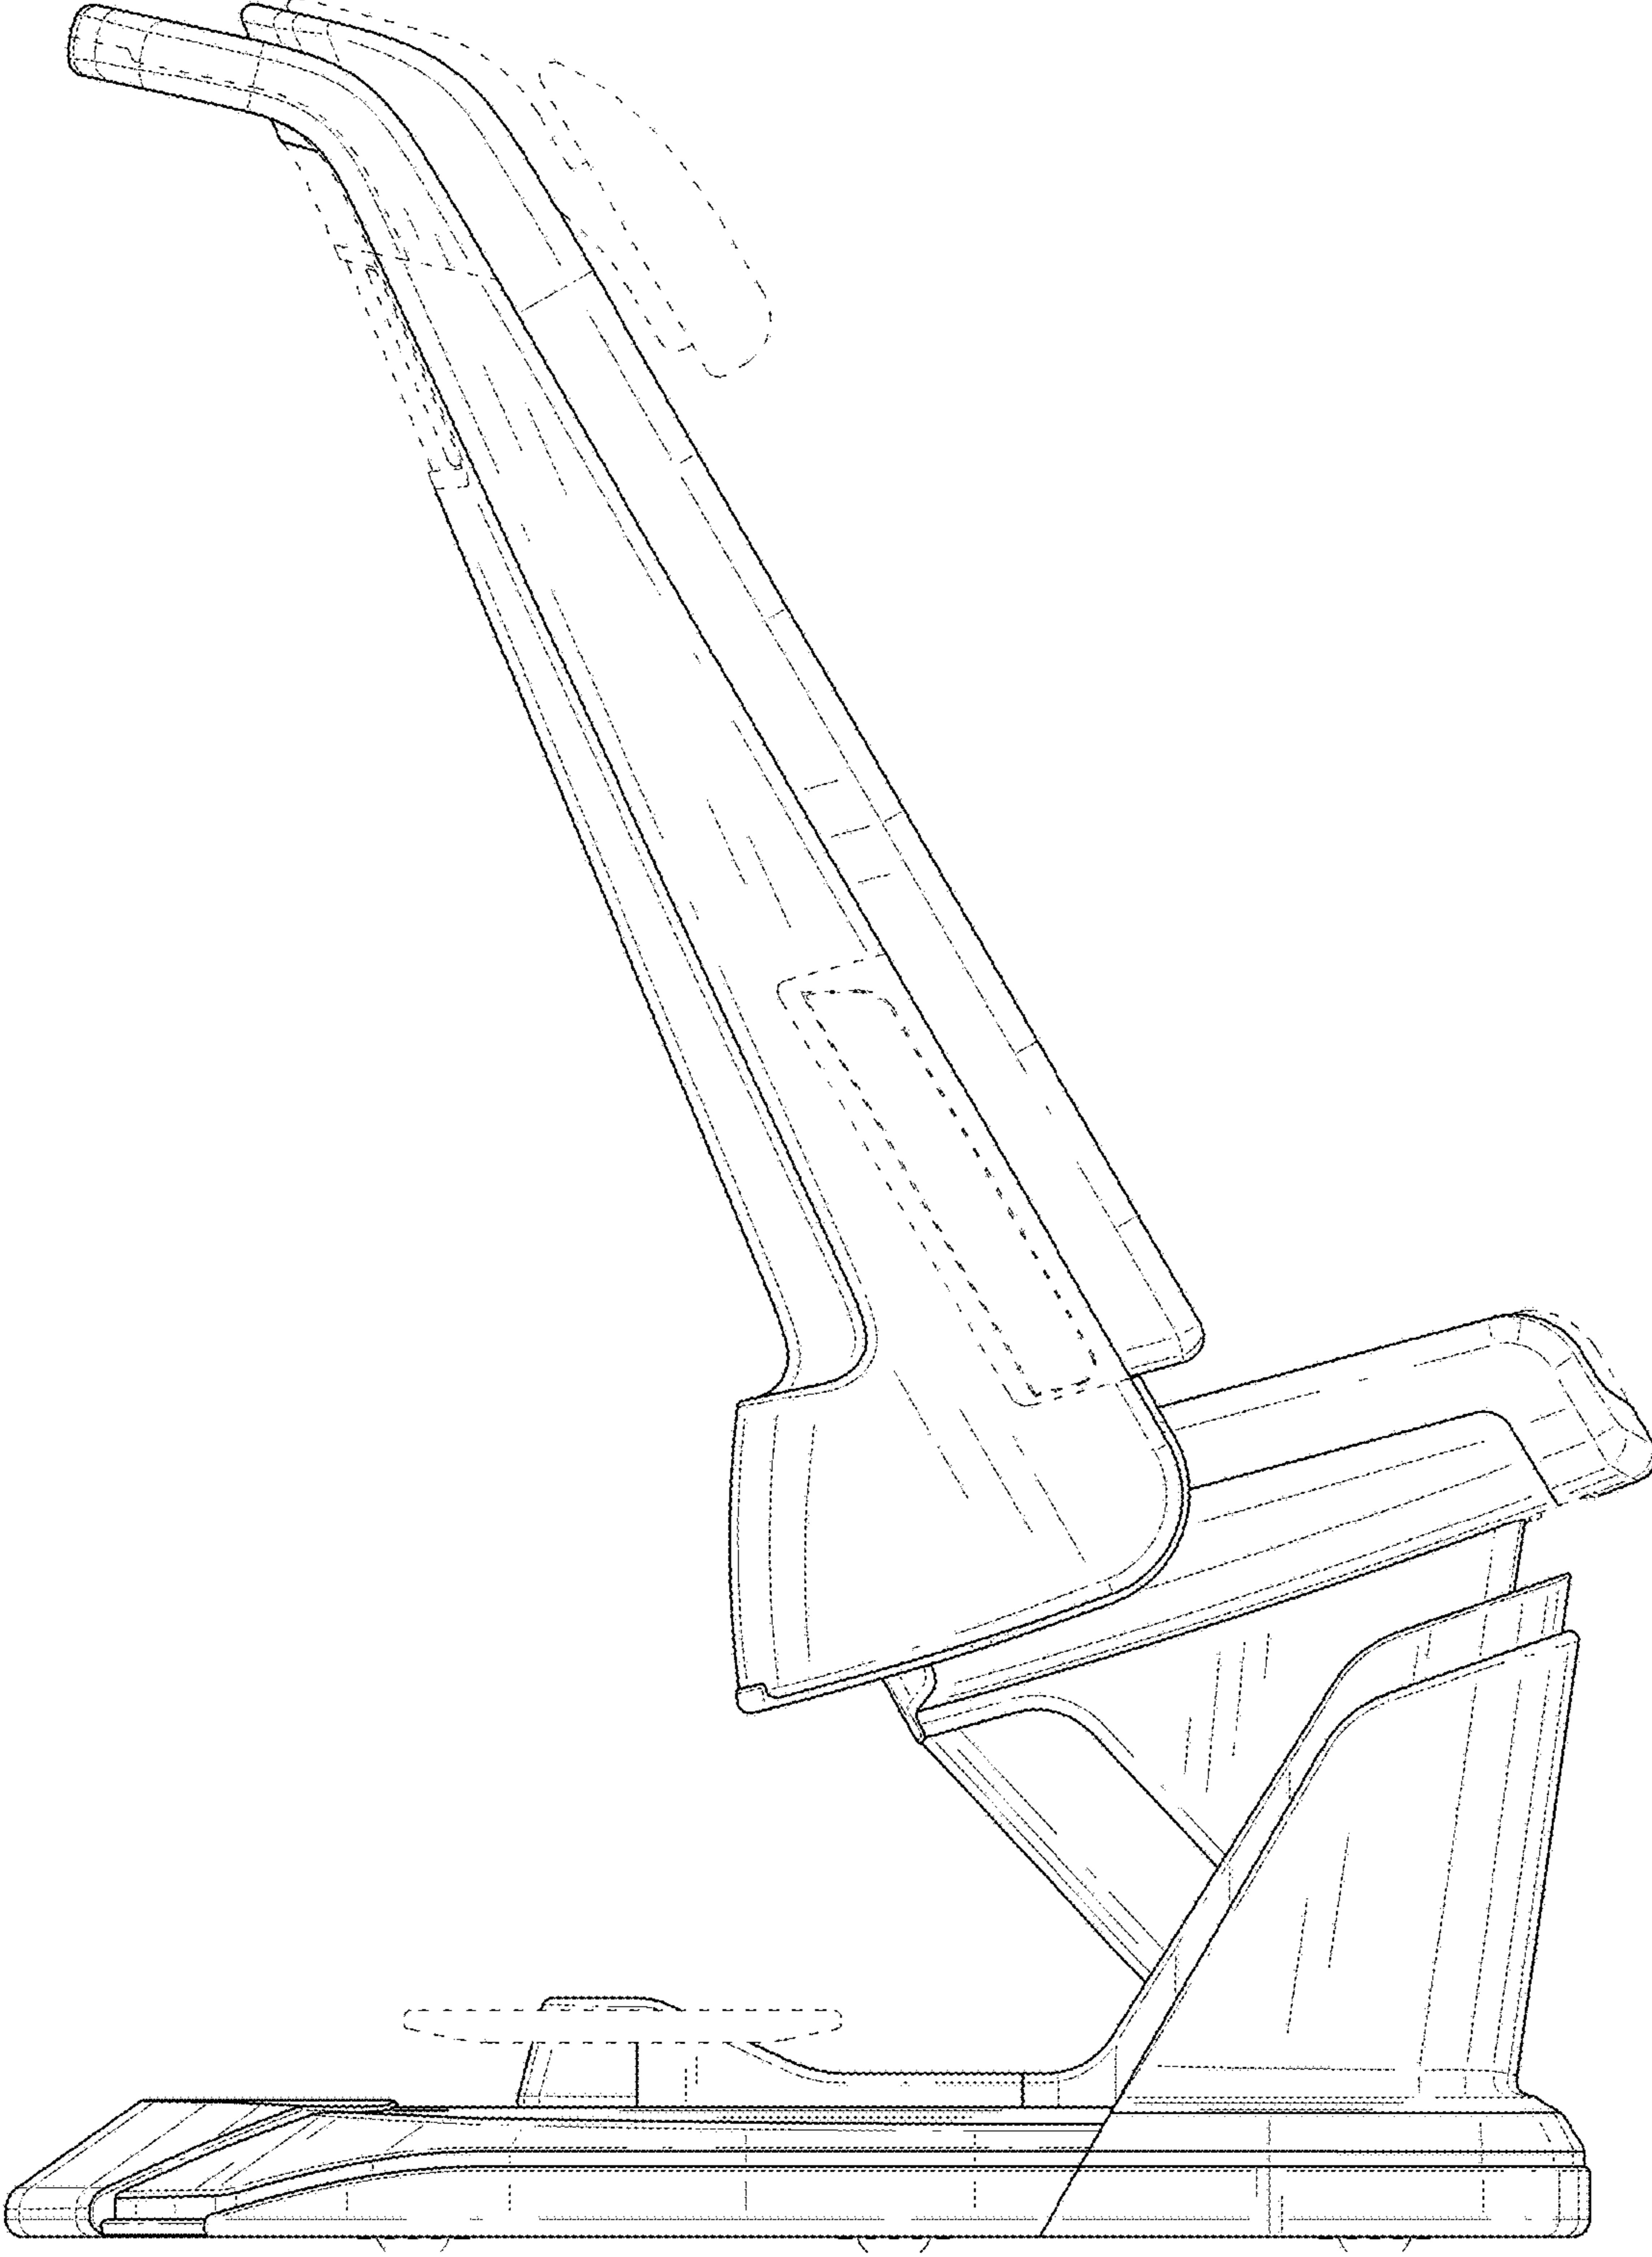


FIG. 5

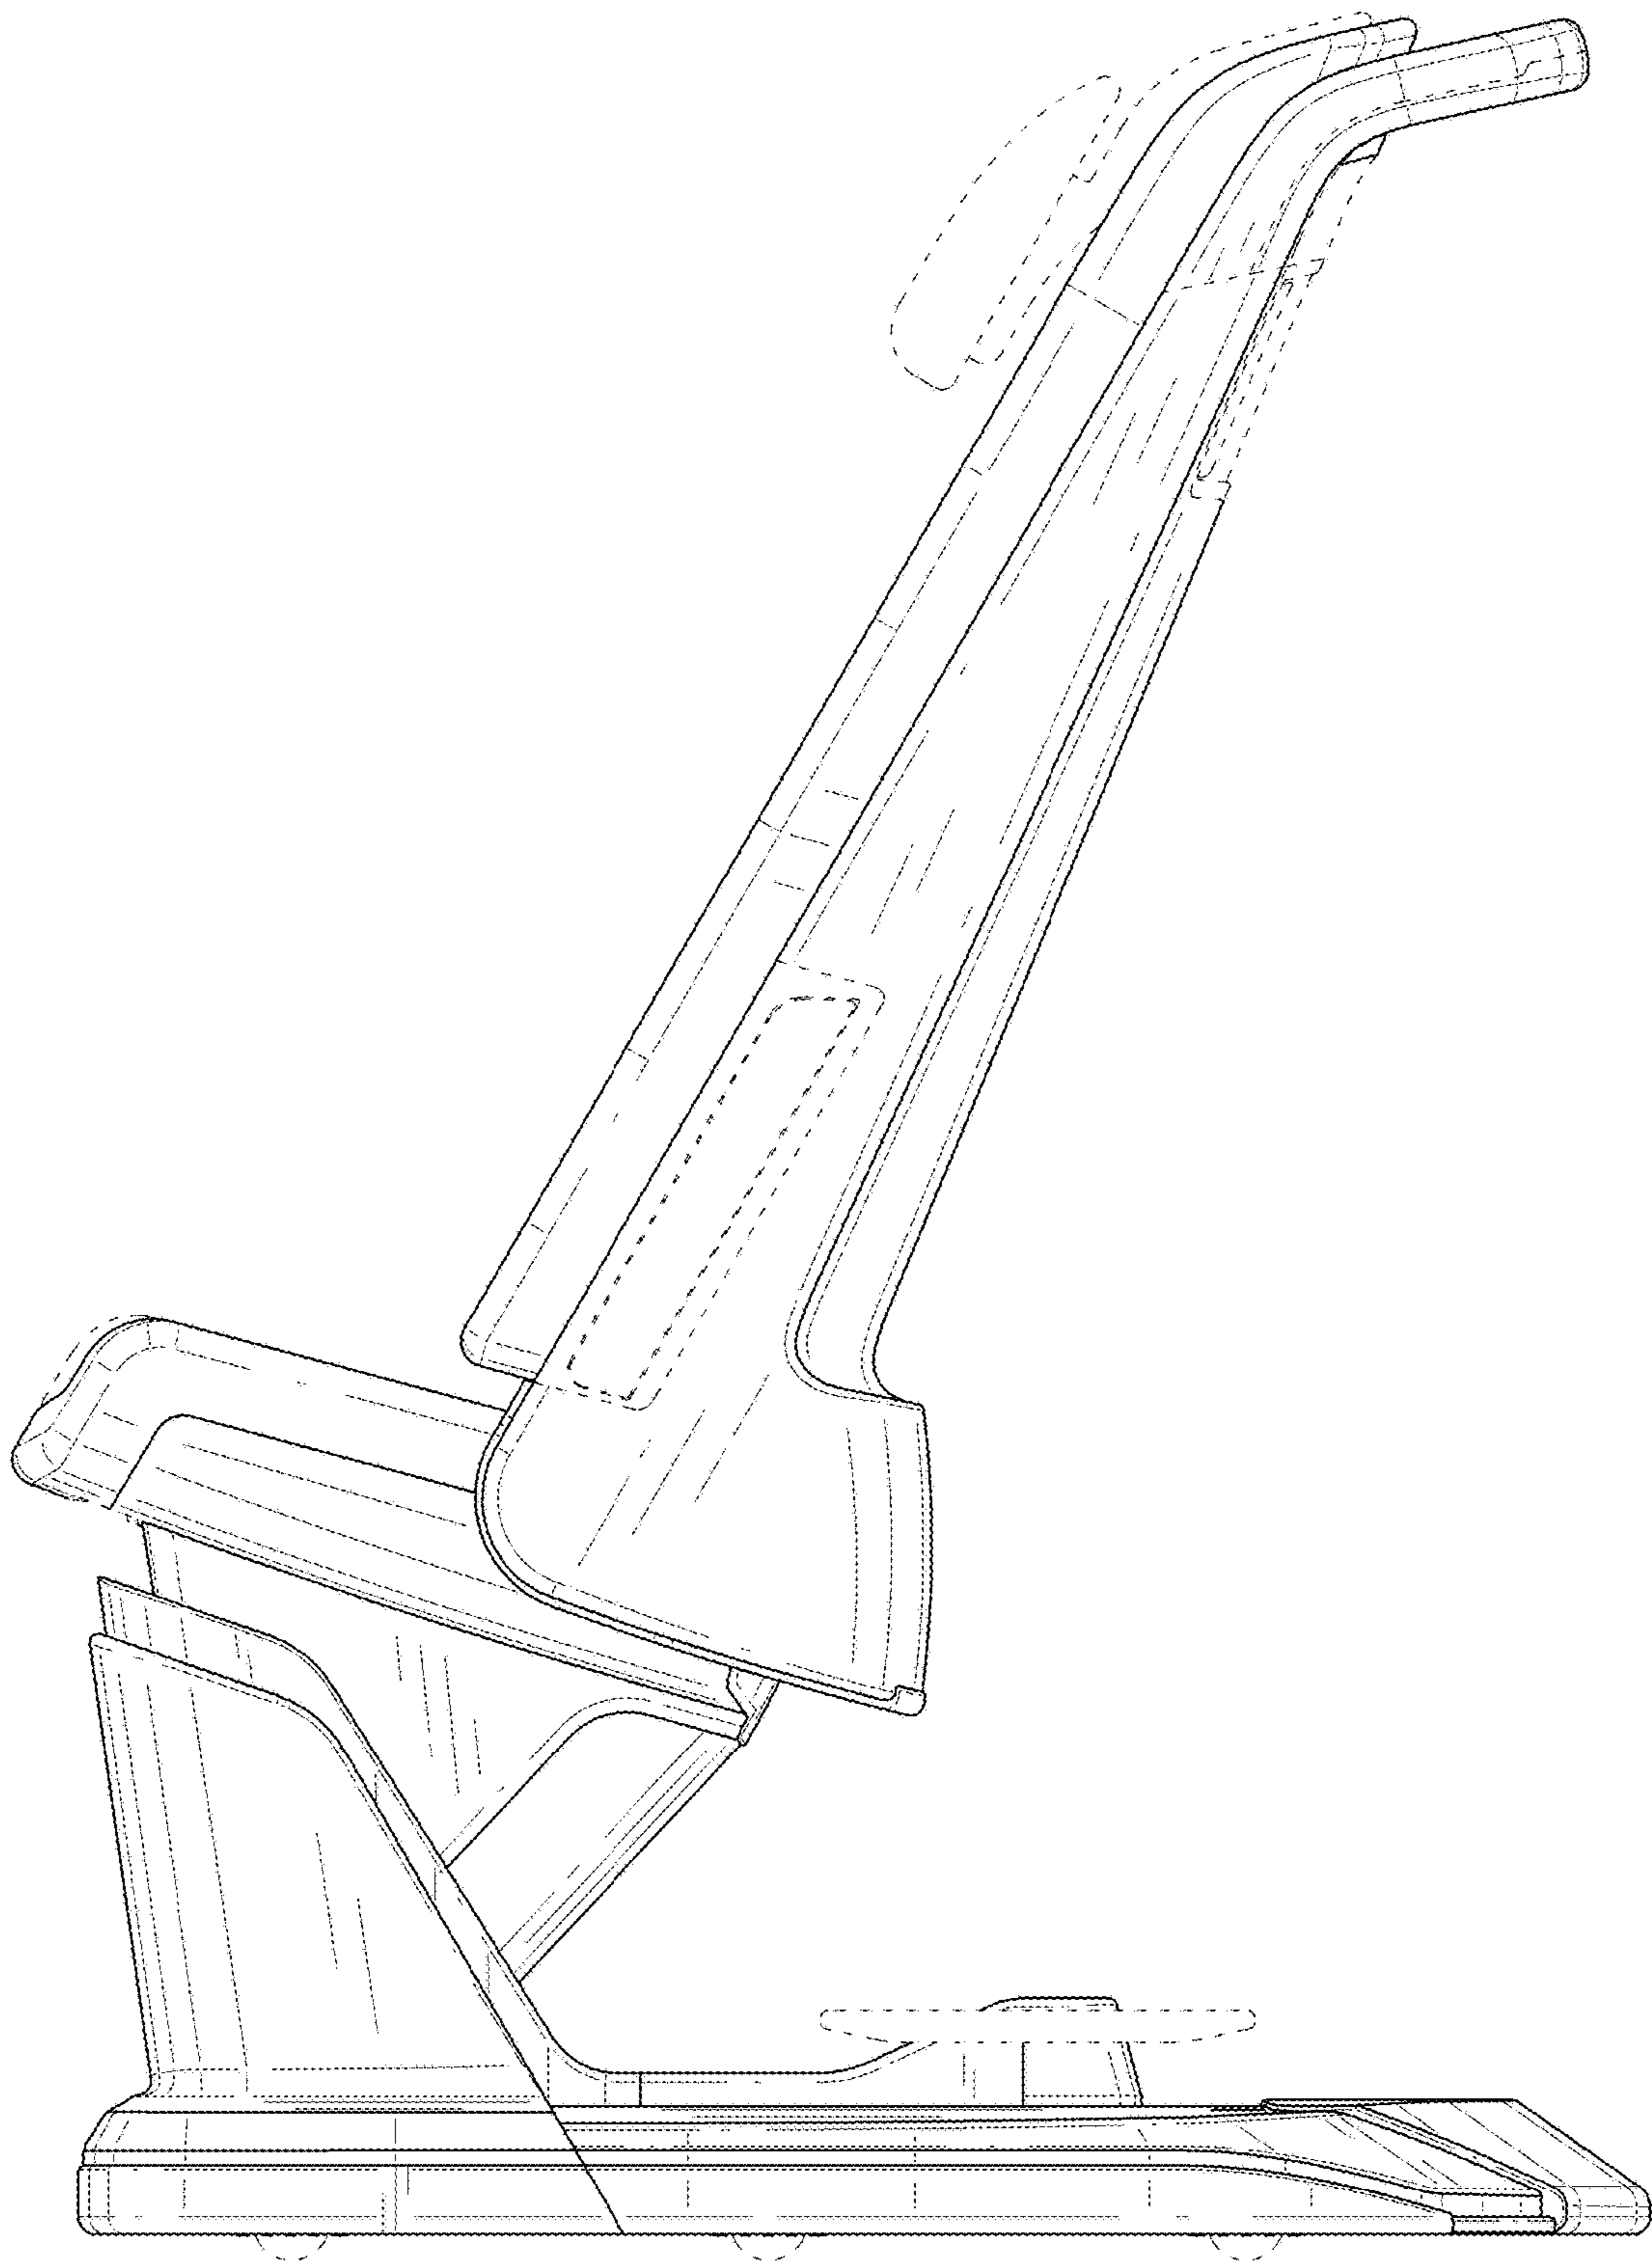


FIG. 6

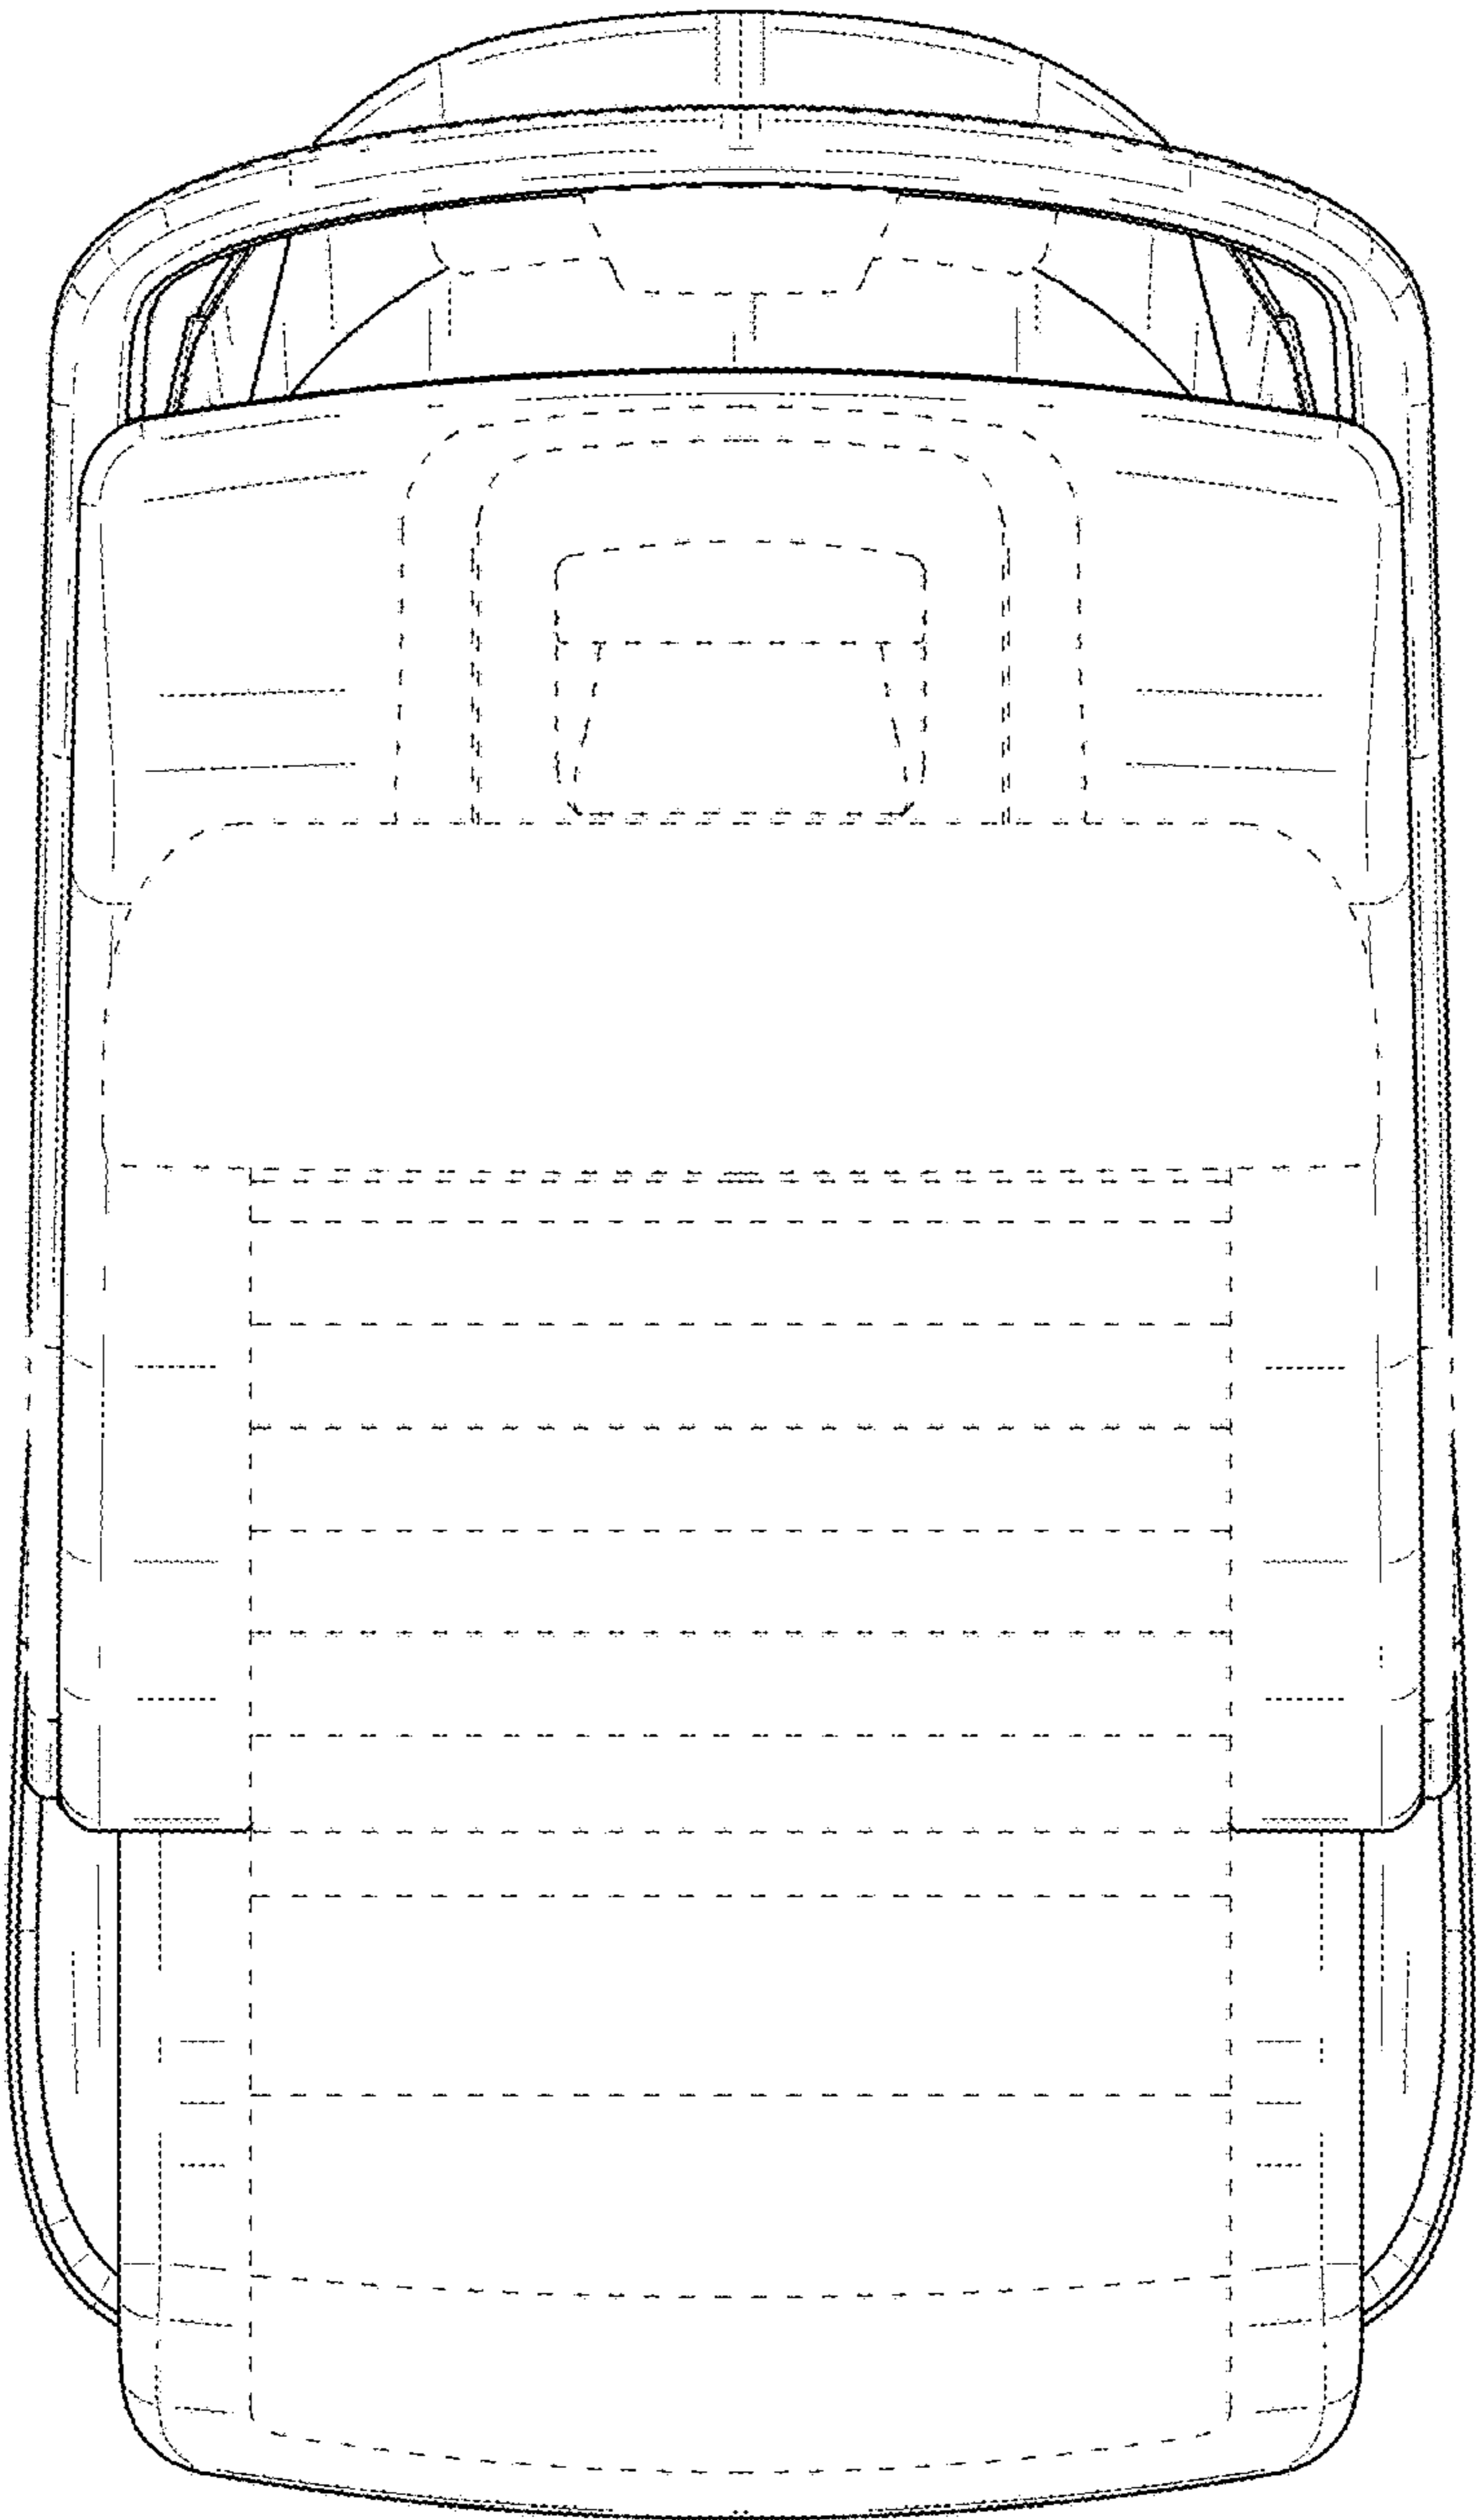


FIG. 7

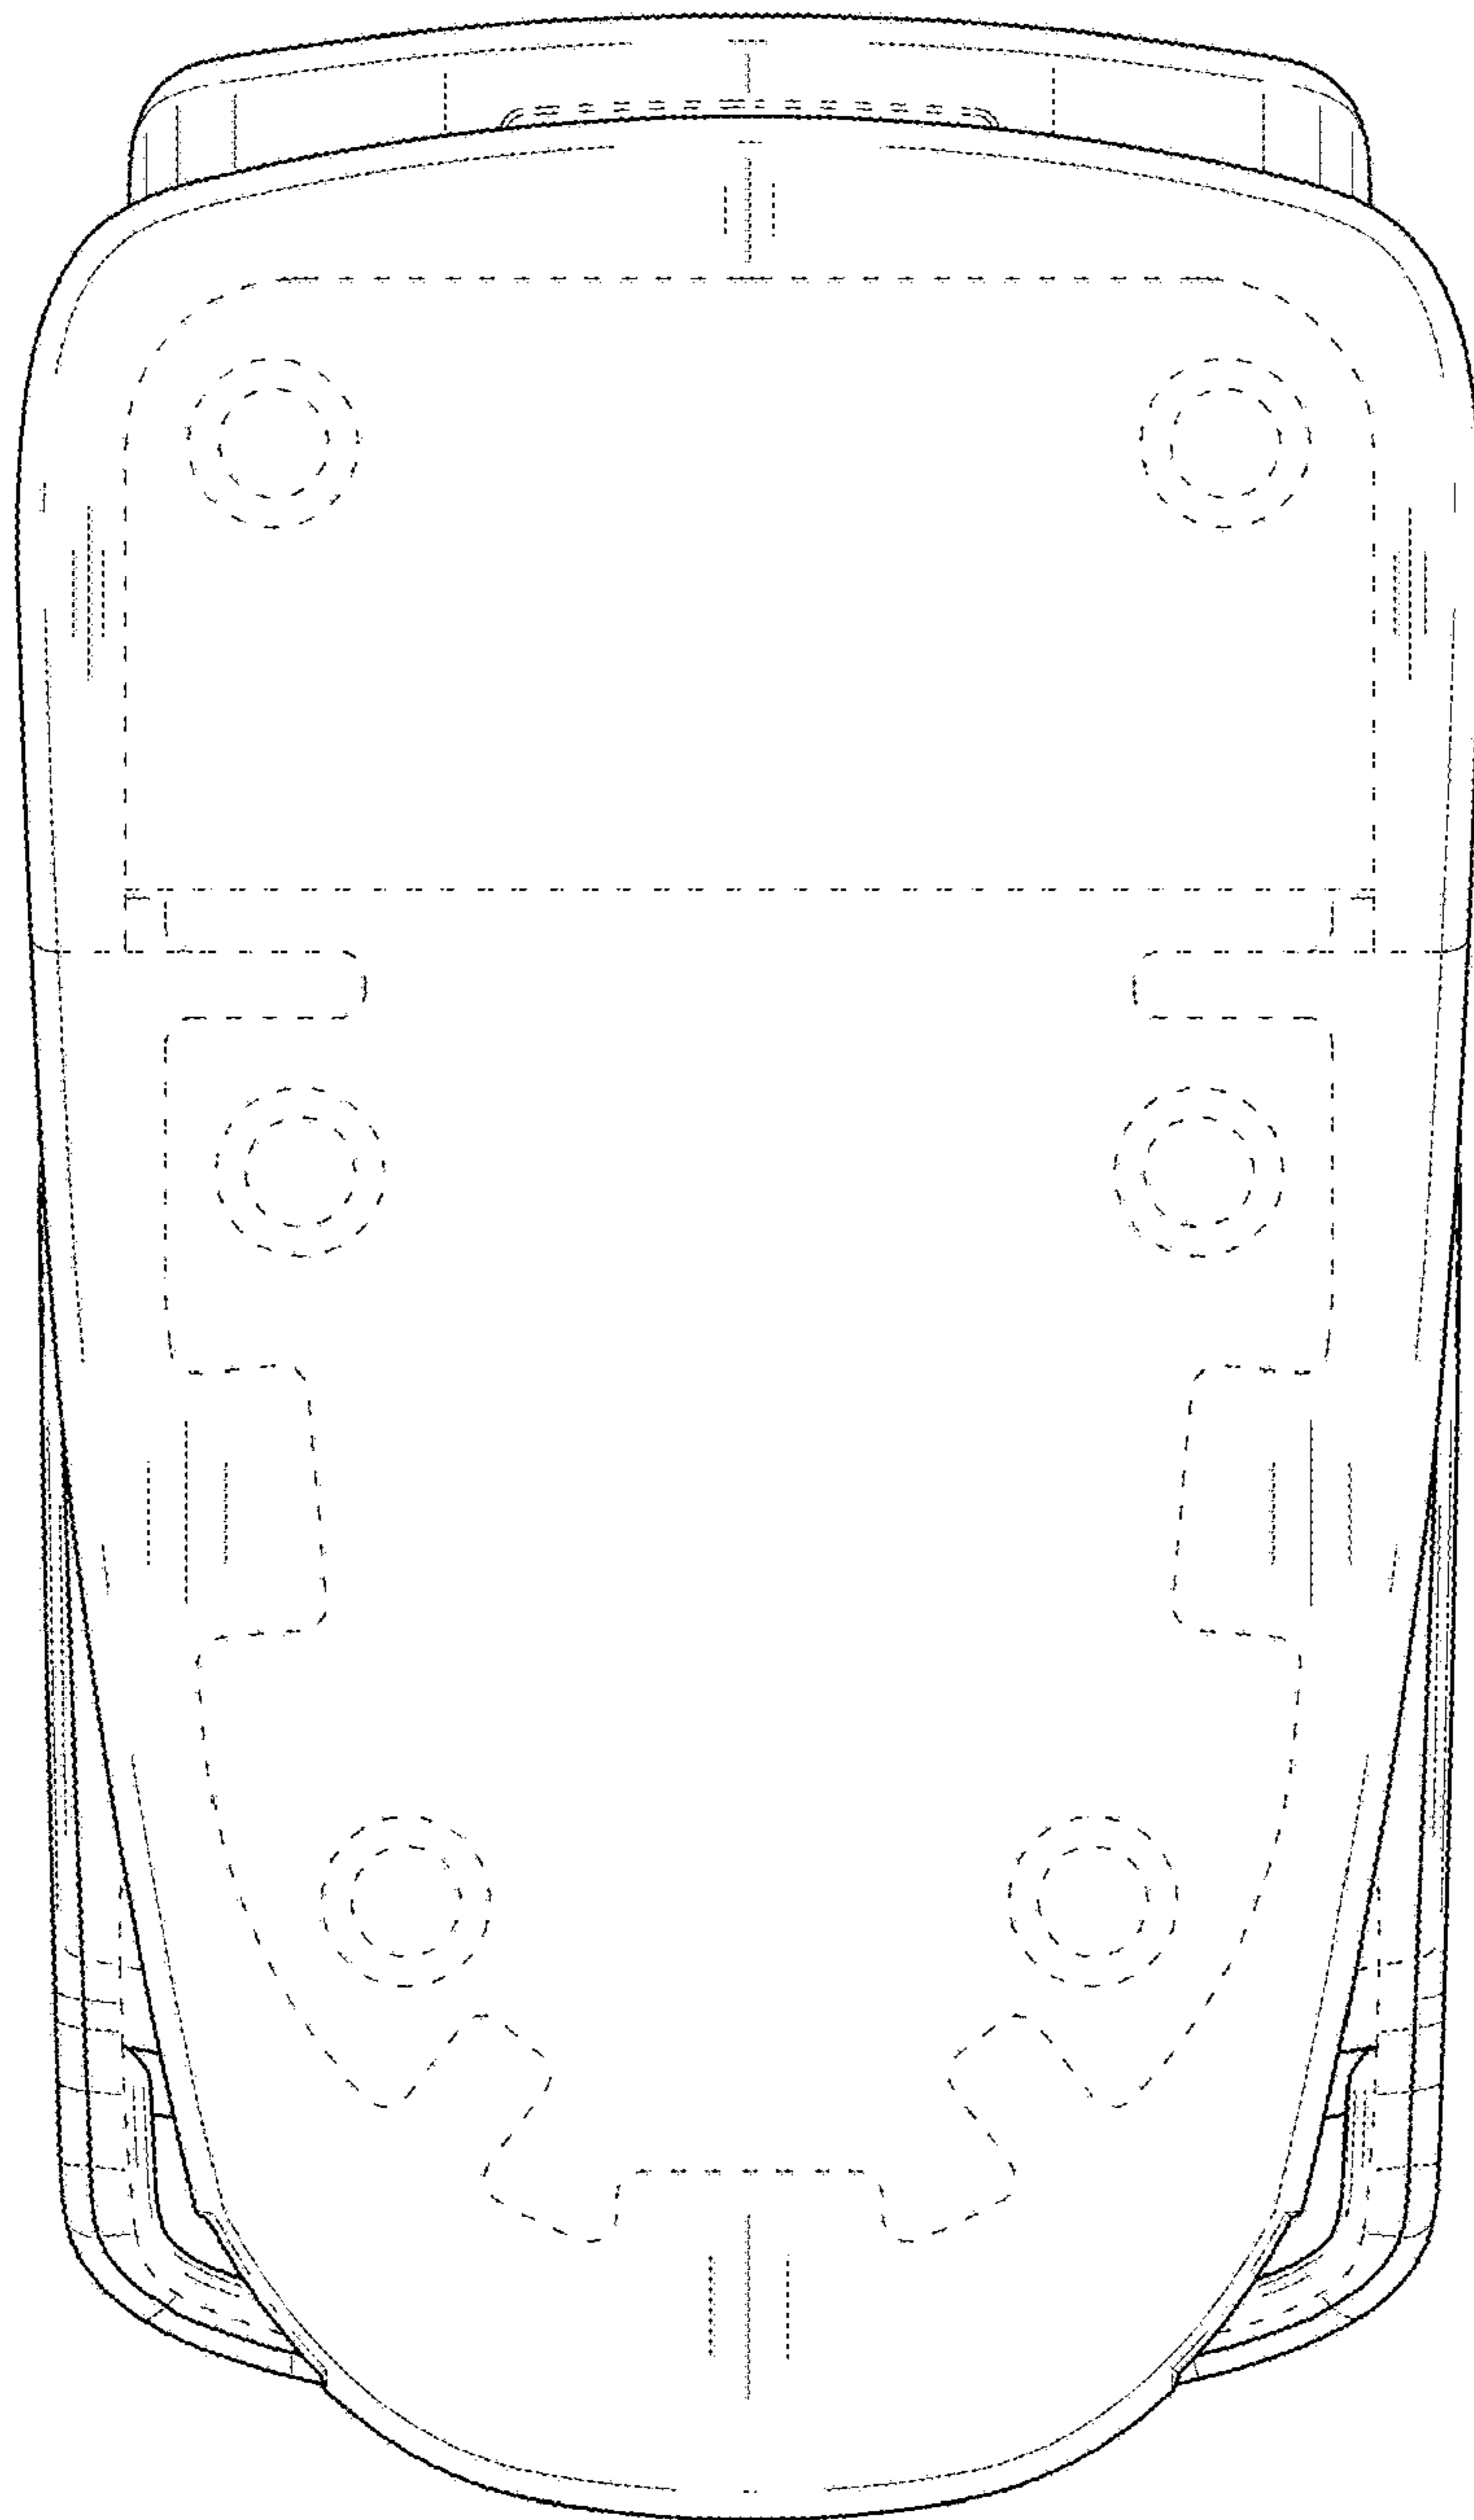


FIG. 8

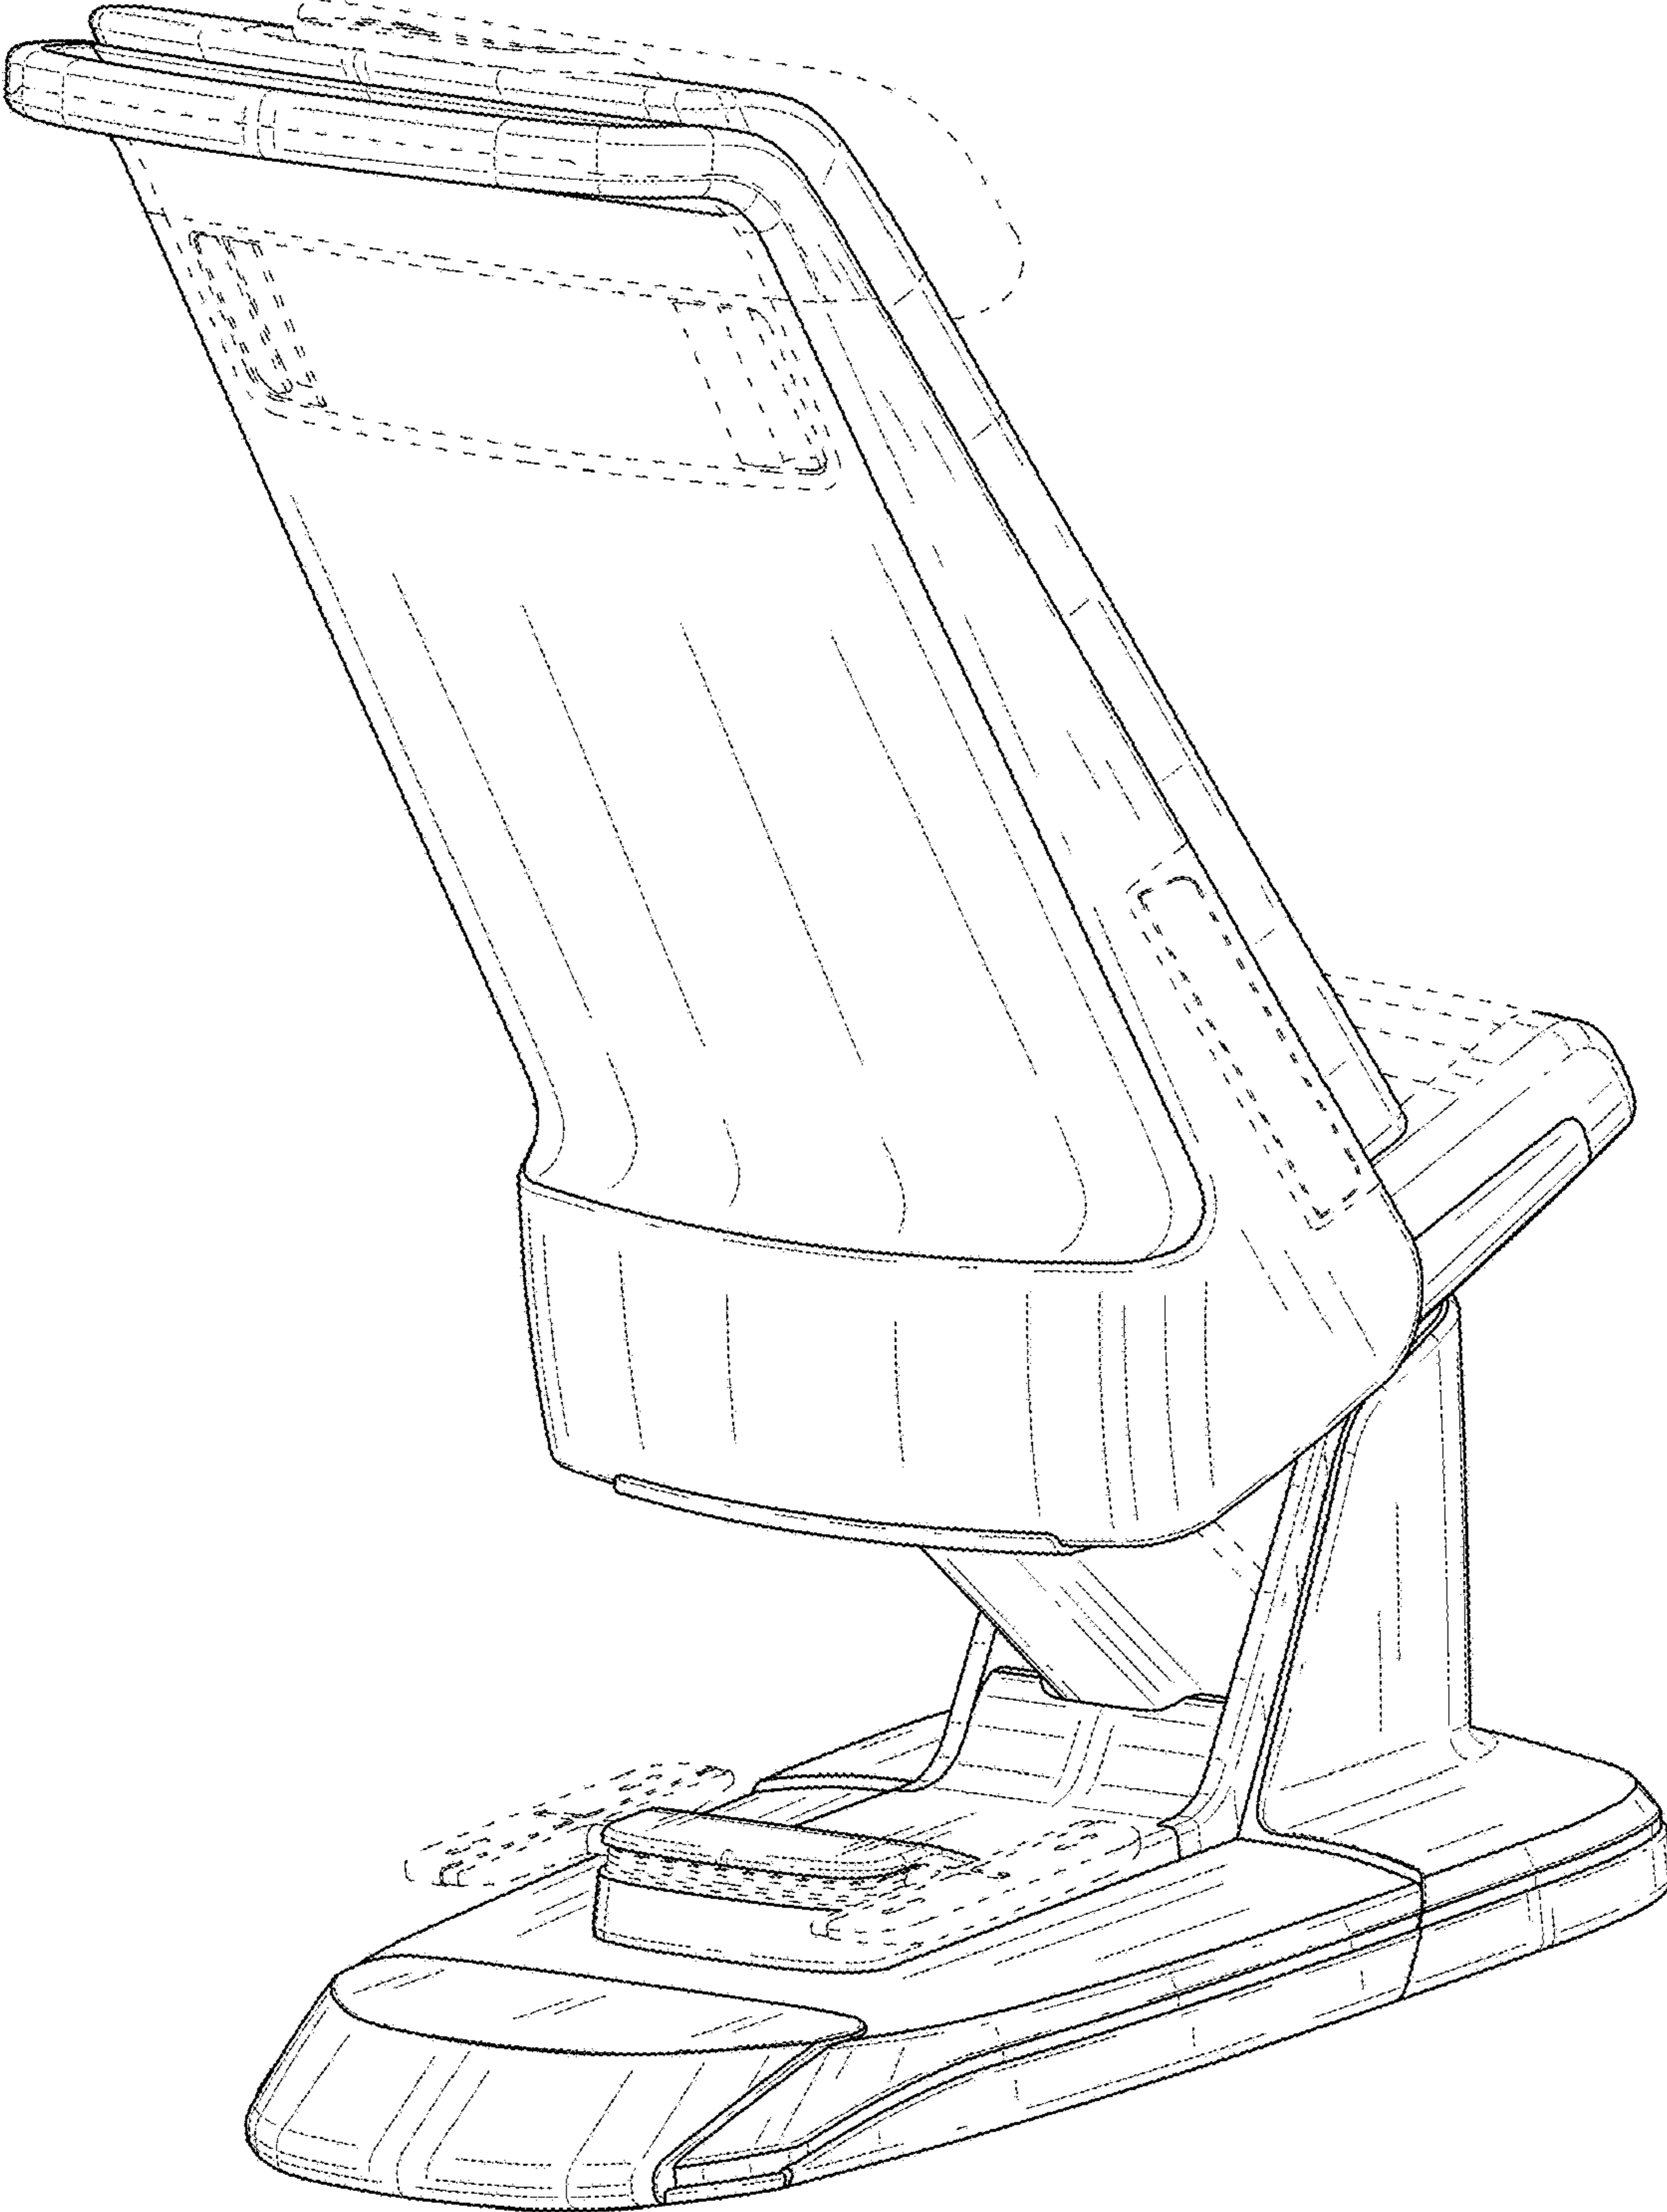


FIG. 9

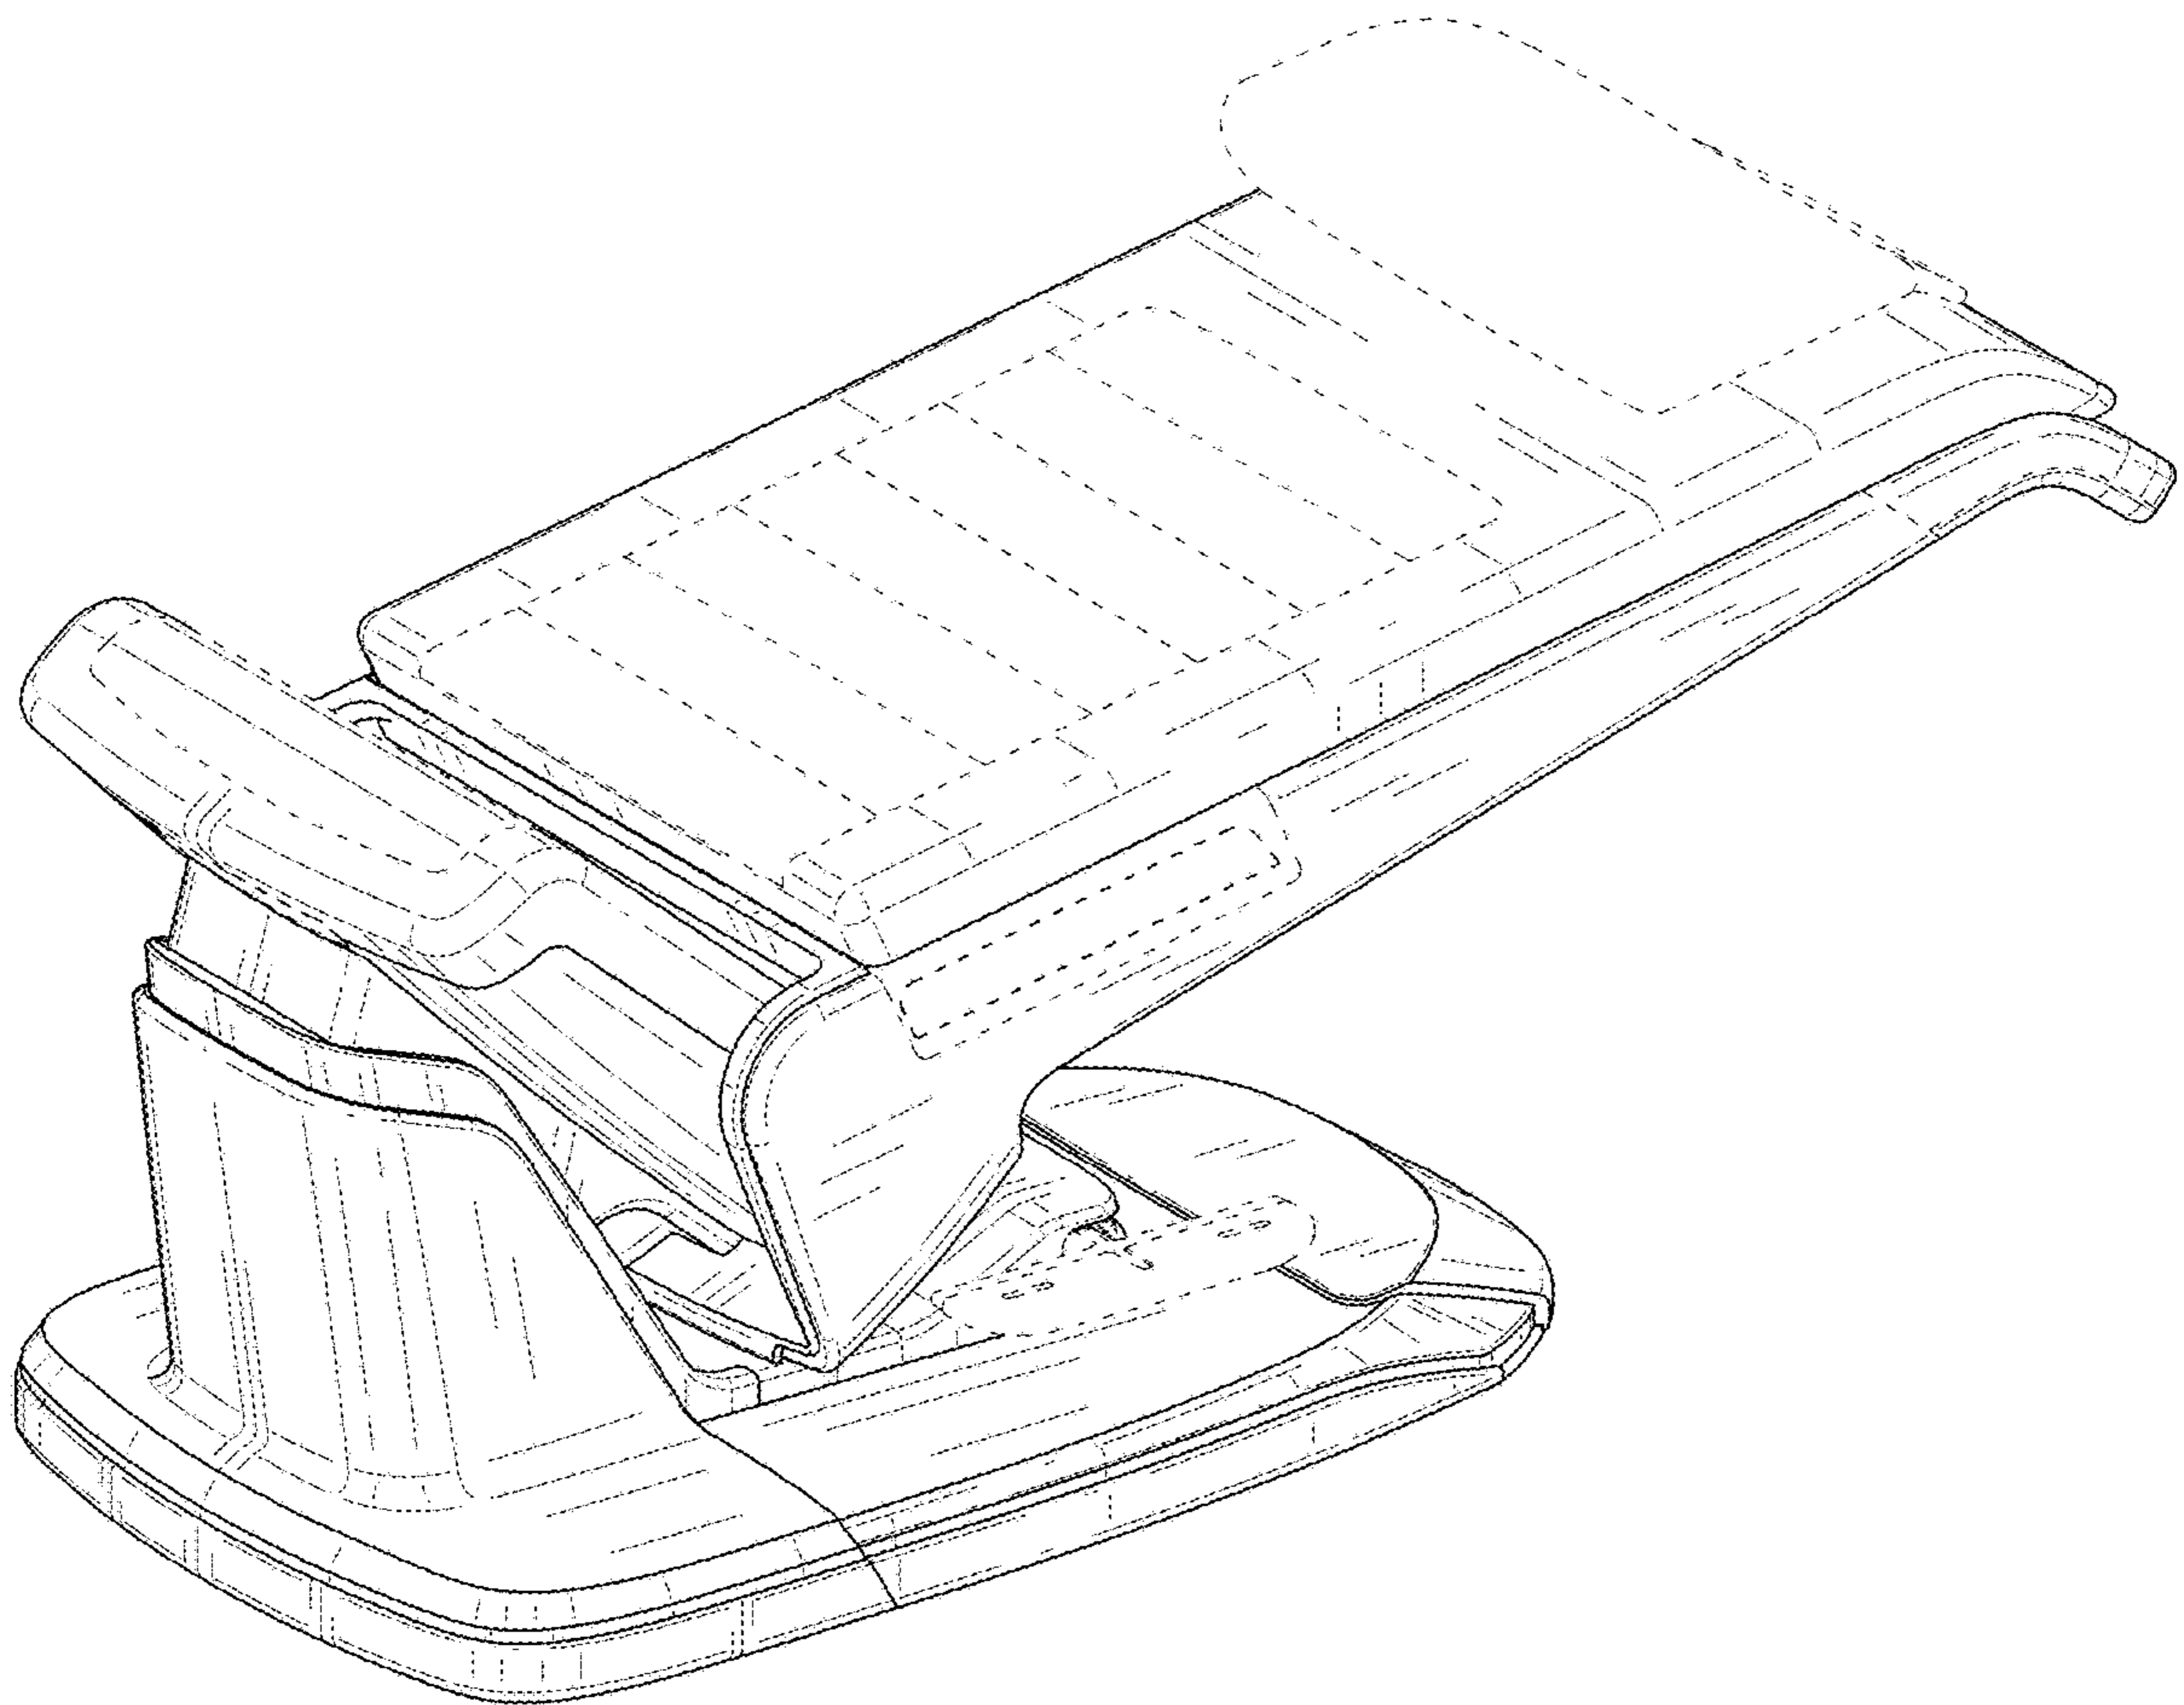


FIG. 10

