



US00D857203S

(12) **United States Design Patent** (10) **Patent No.:** **US D857,203 S**  
**Kim et al.** (45) **Date of Patent:** **\*\* Aug. 20, 2019**

(54) **MAGNETIC RESONANCE IMAGING DEVICE**

D804,031 S \* 11/2017 Hsu ..... D24/158  
 2017/0000433 A1\* 1/2017 Tsujii ..... A61B 6/4417  
 2018/0214108 A1\* 8/2018 Tsai ..... A61B 6/0428

(71) Applicant: **SAMSUNG ELECTRONICS CO., LTD.**, Suwon-si, Gyeonggi-do (KR)

**FOREIGN PATENT DOCUMENTS**

(72) Inventors: **Euisik Kim**, Seoul (KR); **Yunsu Kim**, Seongnam-si (KR)

CN 303218971 S 5/2015  
 JP D1186204 S 9/2003

(73) Assignee: **SAMSUNG ELECTRONICS CO., LTD.**, Gyeonggi-Do (KR)

**OTHER PUBLICATIONS**

(\*\*) Term: **15 Years**

YouTube. Introducing the GE Optima MR430s 1.5T [online]. p. 1 of 1 [retrieved on Mar. 21, 2011]. Retrieved from the Internet: <URL: <https://www.youtube.com/watch?v=-iQLpqoEgCA>.

(21) Appl. No.: **29/644,621**

\* cited by examiner

(22) Filed: **Apr. 19, 2018**

*Primary Examiner* — Anhdao Doan

(30) **Foreign Application Priority Data**

(74) *Attorney, Agent, or Firm* — Cantor Colburn LLP

Nov. 15, 2017 (KR) ..... 30-2017-0053323

(51) **LOC (12) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/158**

(58) **Field of Classification Search**  
USPC ..... D24/107, 158–161, 185, 186, 187, 231  
CPC .. A61B 6/03; A61B 6/035; A61B 5/05; A61B 5/055; G01N 2223/1013; G01N 2223/1016; A61N 2005/1054; A61N 2005/1055; A61N 2005/1074  
See application file for complete search history.

(57) **CLAIM**

The ornamental design for a magnetic resonance imaging device, as shown and described.

**DESCRIPTION**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,820,552 A \* 10/1998 Crosby ..... A61B 8/0825  
 600/407  
 D557,403 S \* 12/2007 Asai ..... D24/107  
 D713,962 S 9/2014 Wodecki  
 D740,944 S \* 10/2015 Zhao ..... D24/158  
 D746,464 S \* 12/2015 Rapoport ..... D24/158  
 D783,829 S \* 4/2017 Arishima ..... D24/158  
 D788,310 S \* 5/2017 Takeuchi ..... D24/158

FIG. 1 is a front perspective view of a magnetic resonance imaging (“MRI”) device, showing our new design;  
 FIG. 2 is a front view thereof;  
 FIG. 3 is a rear view thereof;  
 FIG. 4 is a left side view thereof;  
 FIG. 5 is a right side view thereof;  
 FIG. 6 is a top view thereof;  
 FIG. 7 is a bottom view thereof;  
 FIG. 8 is a rear perspective view thereof; and,  
 FIG. 9 is a cross-sectional view thereof, taken along line 9-9 in FIG. 2.

The broken lines immediately adjacent the shaded areas represent the bounds of the claim, while all other broken lines are directed to environment and are for illustrative purposes only; the broken lines form no part of the claimed design.

**1 Claim, 9 Drawing Sheets**

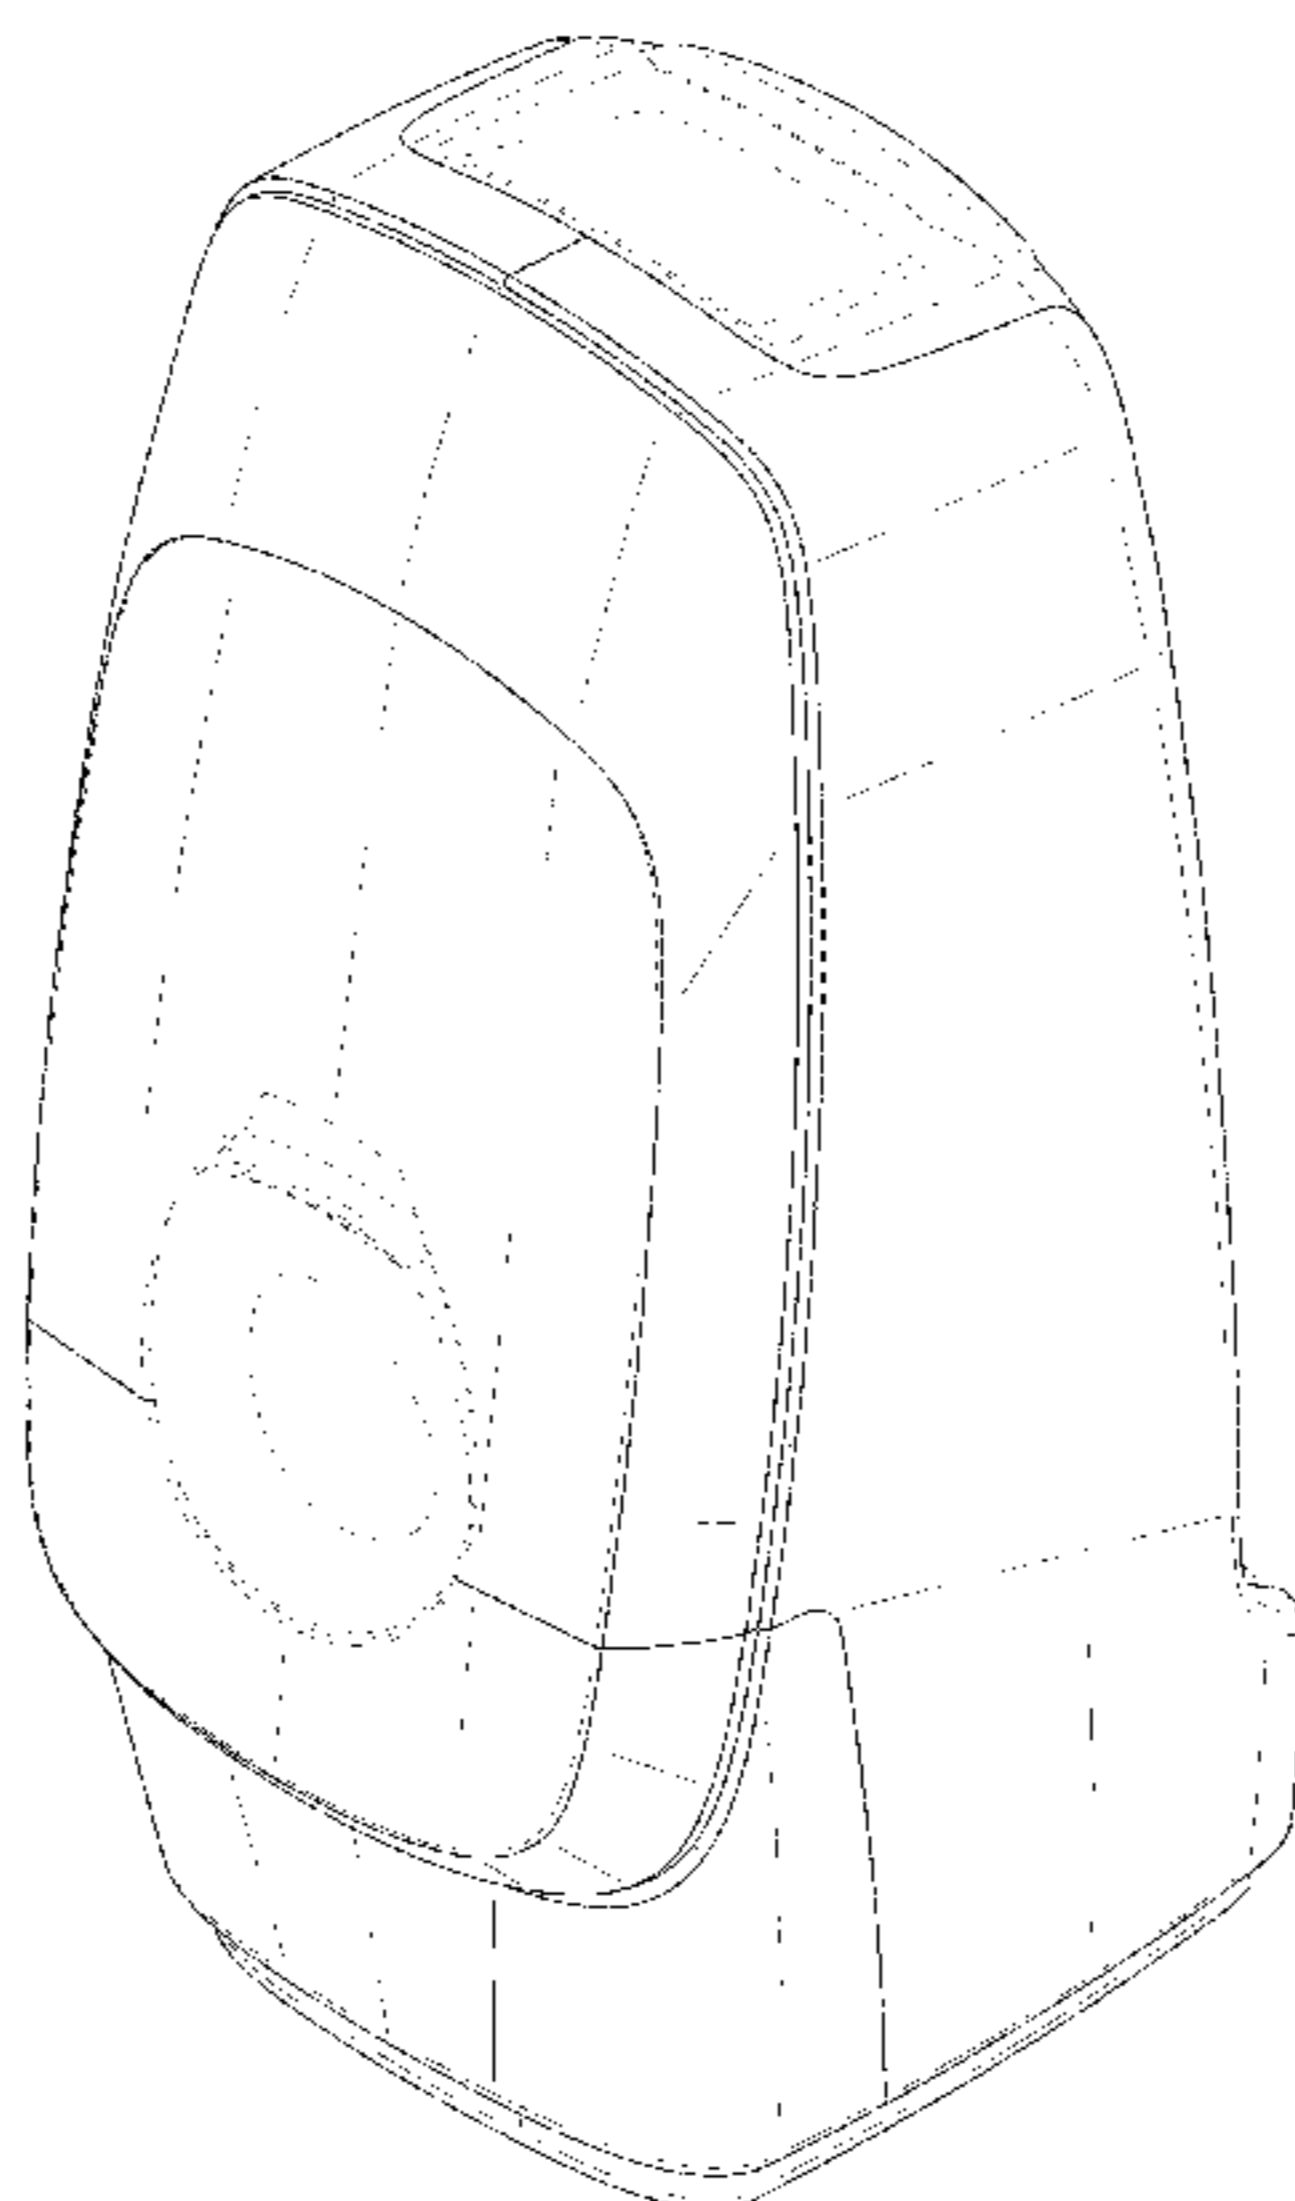


FIG. 1

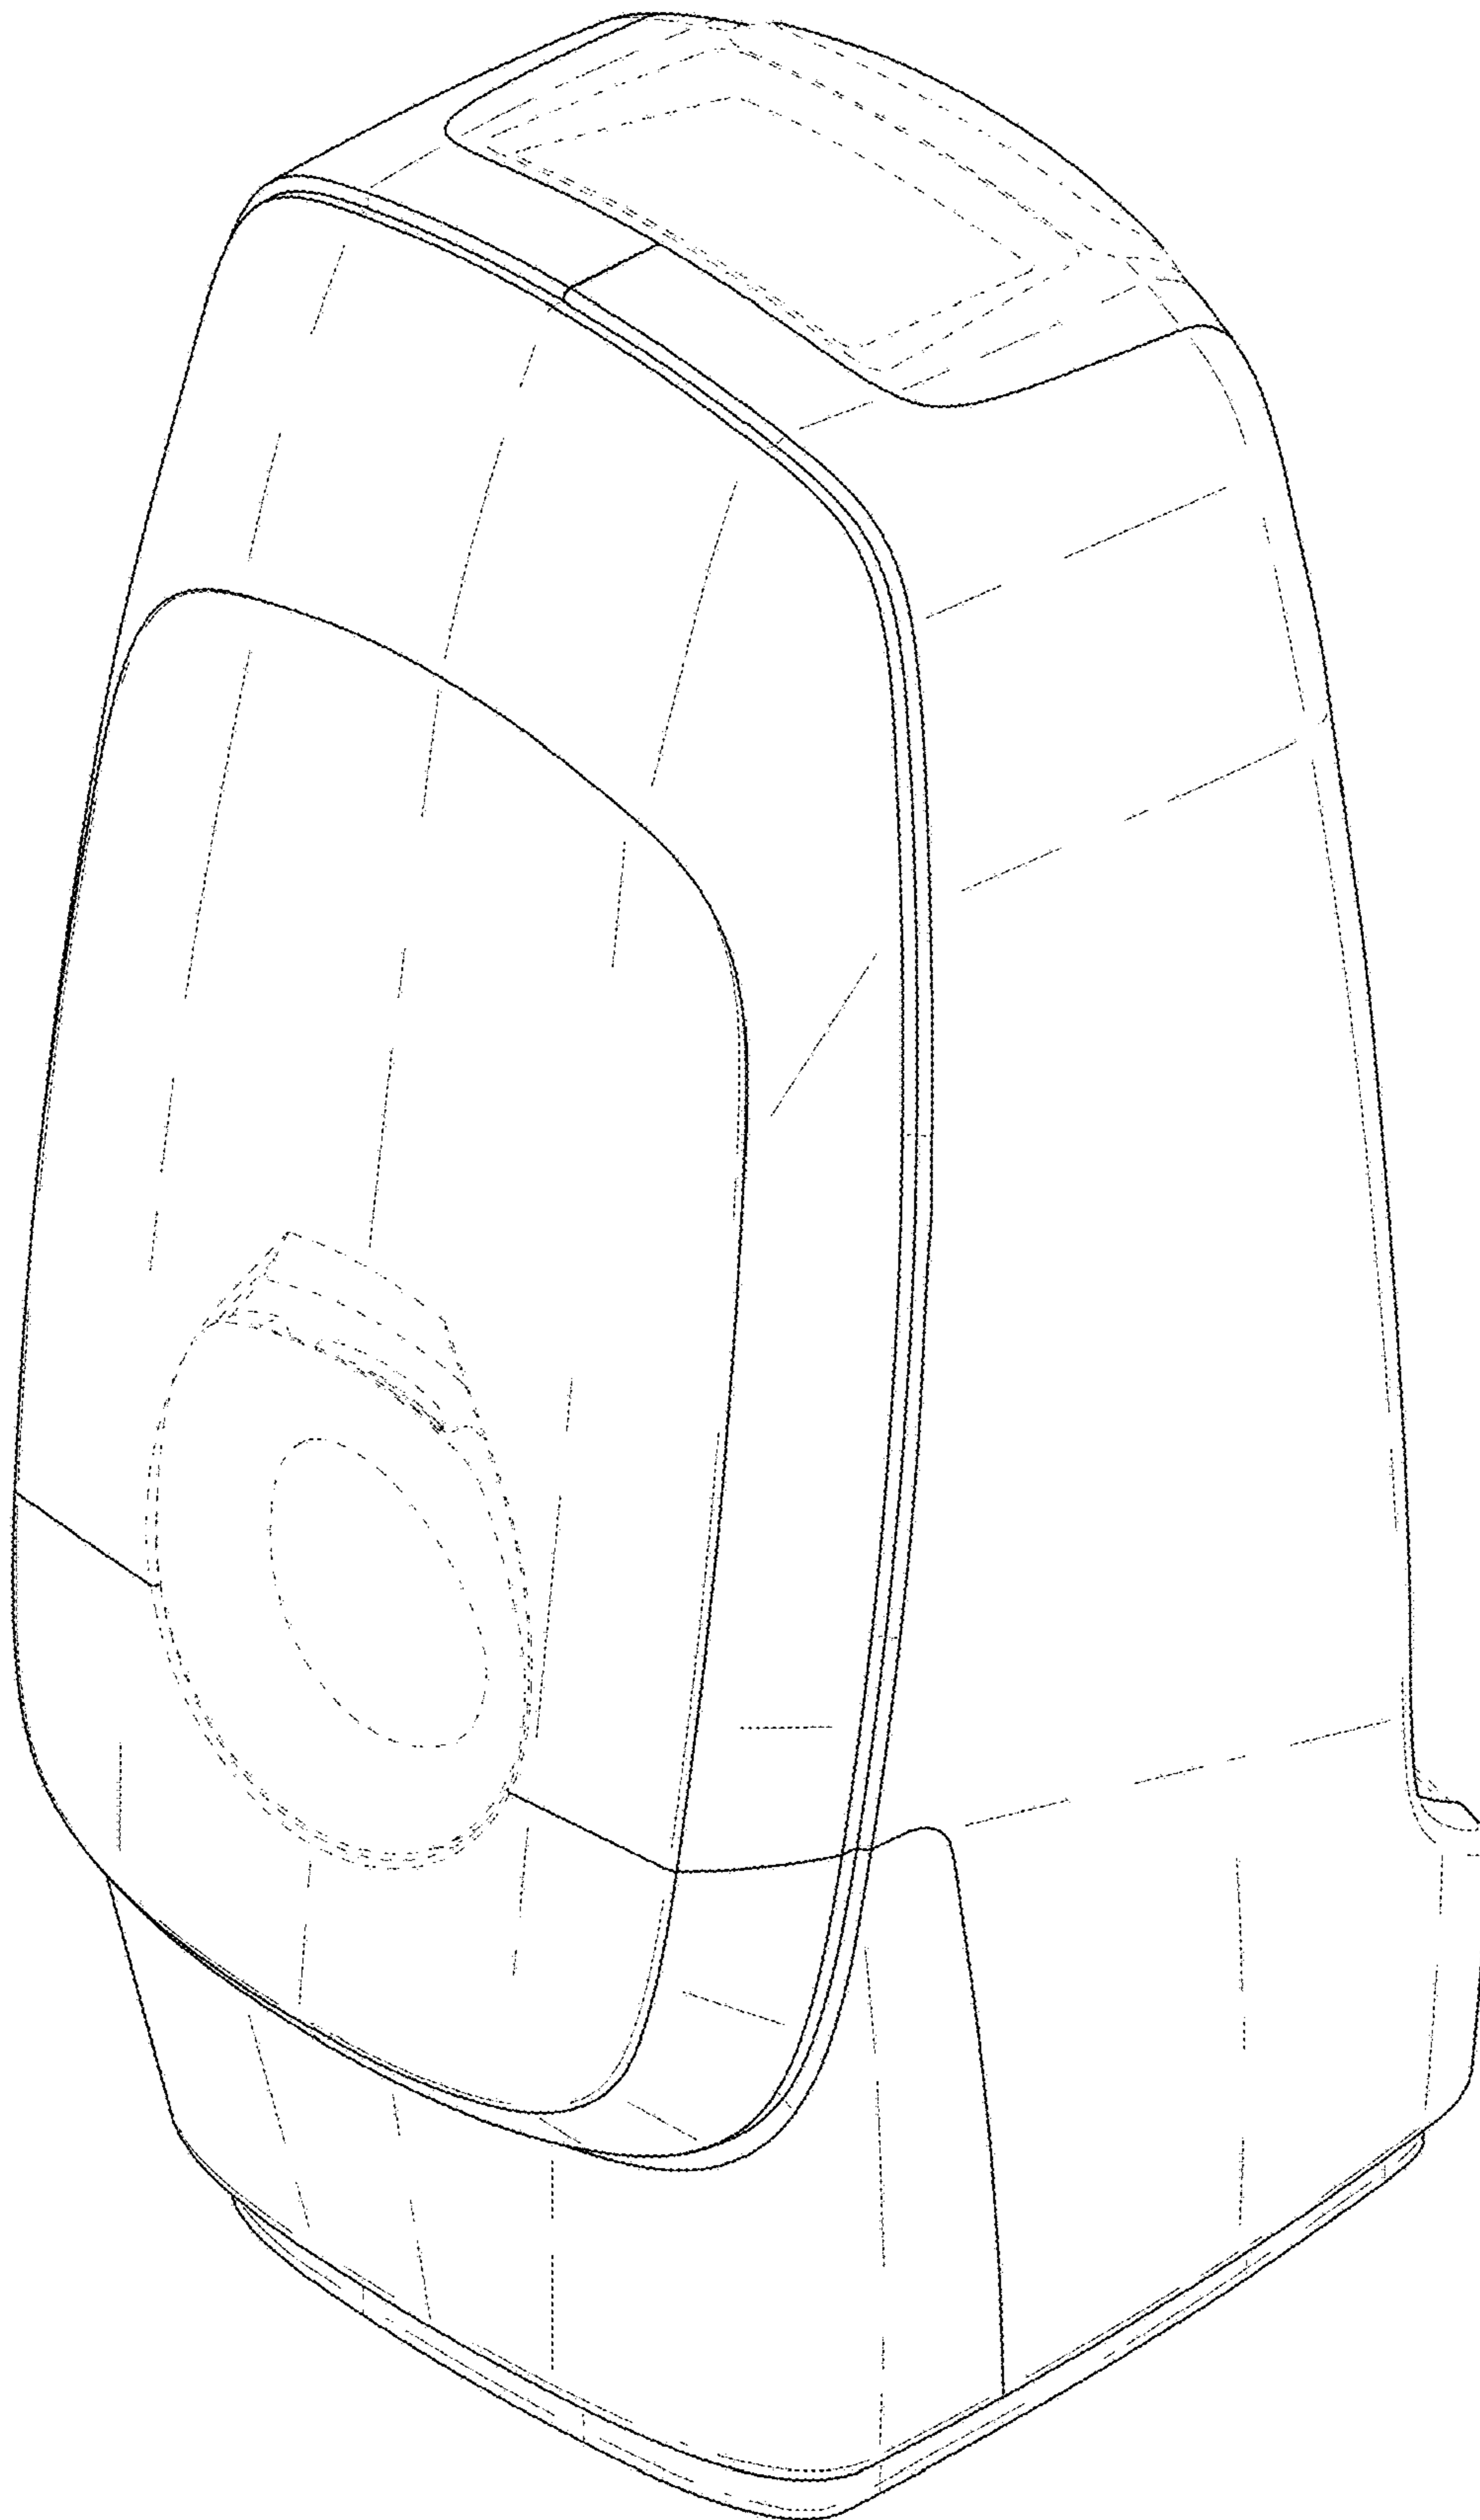


FIG. 2

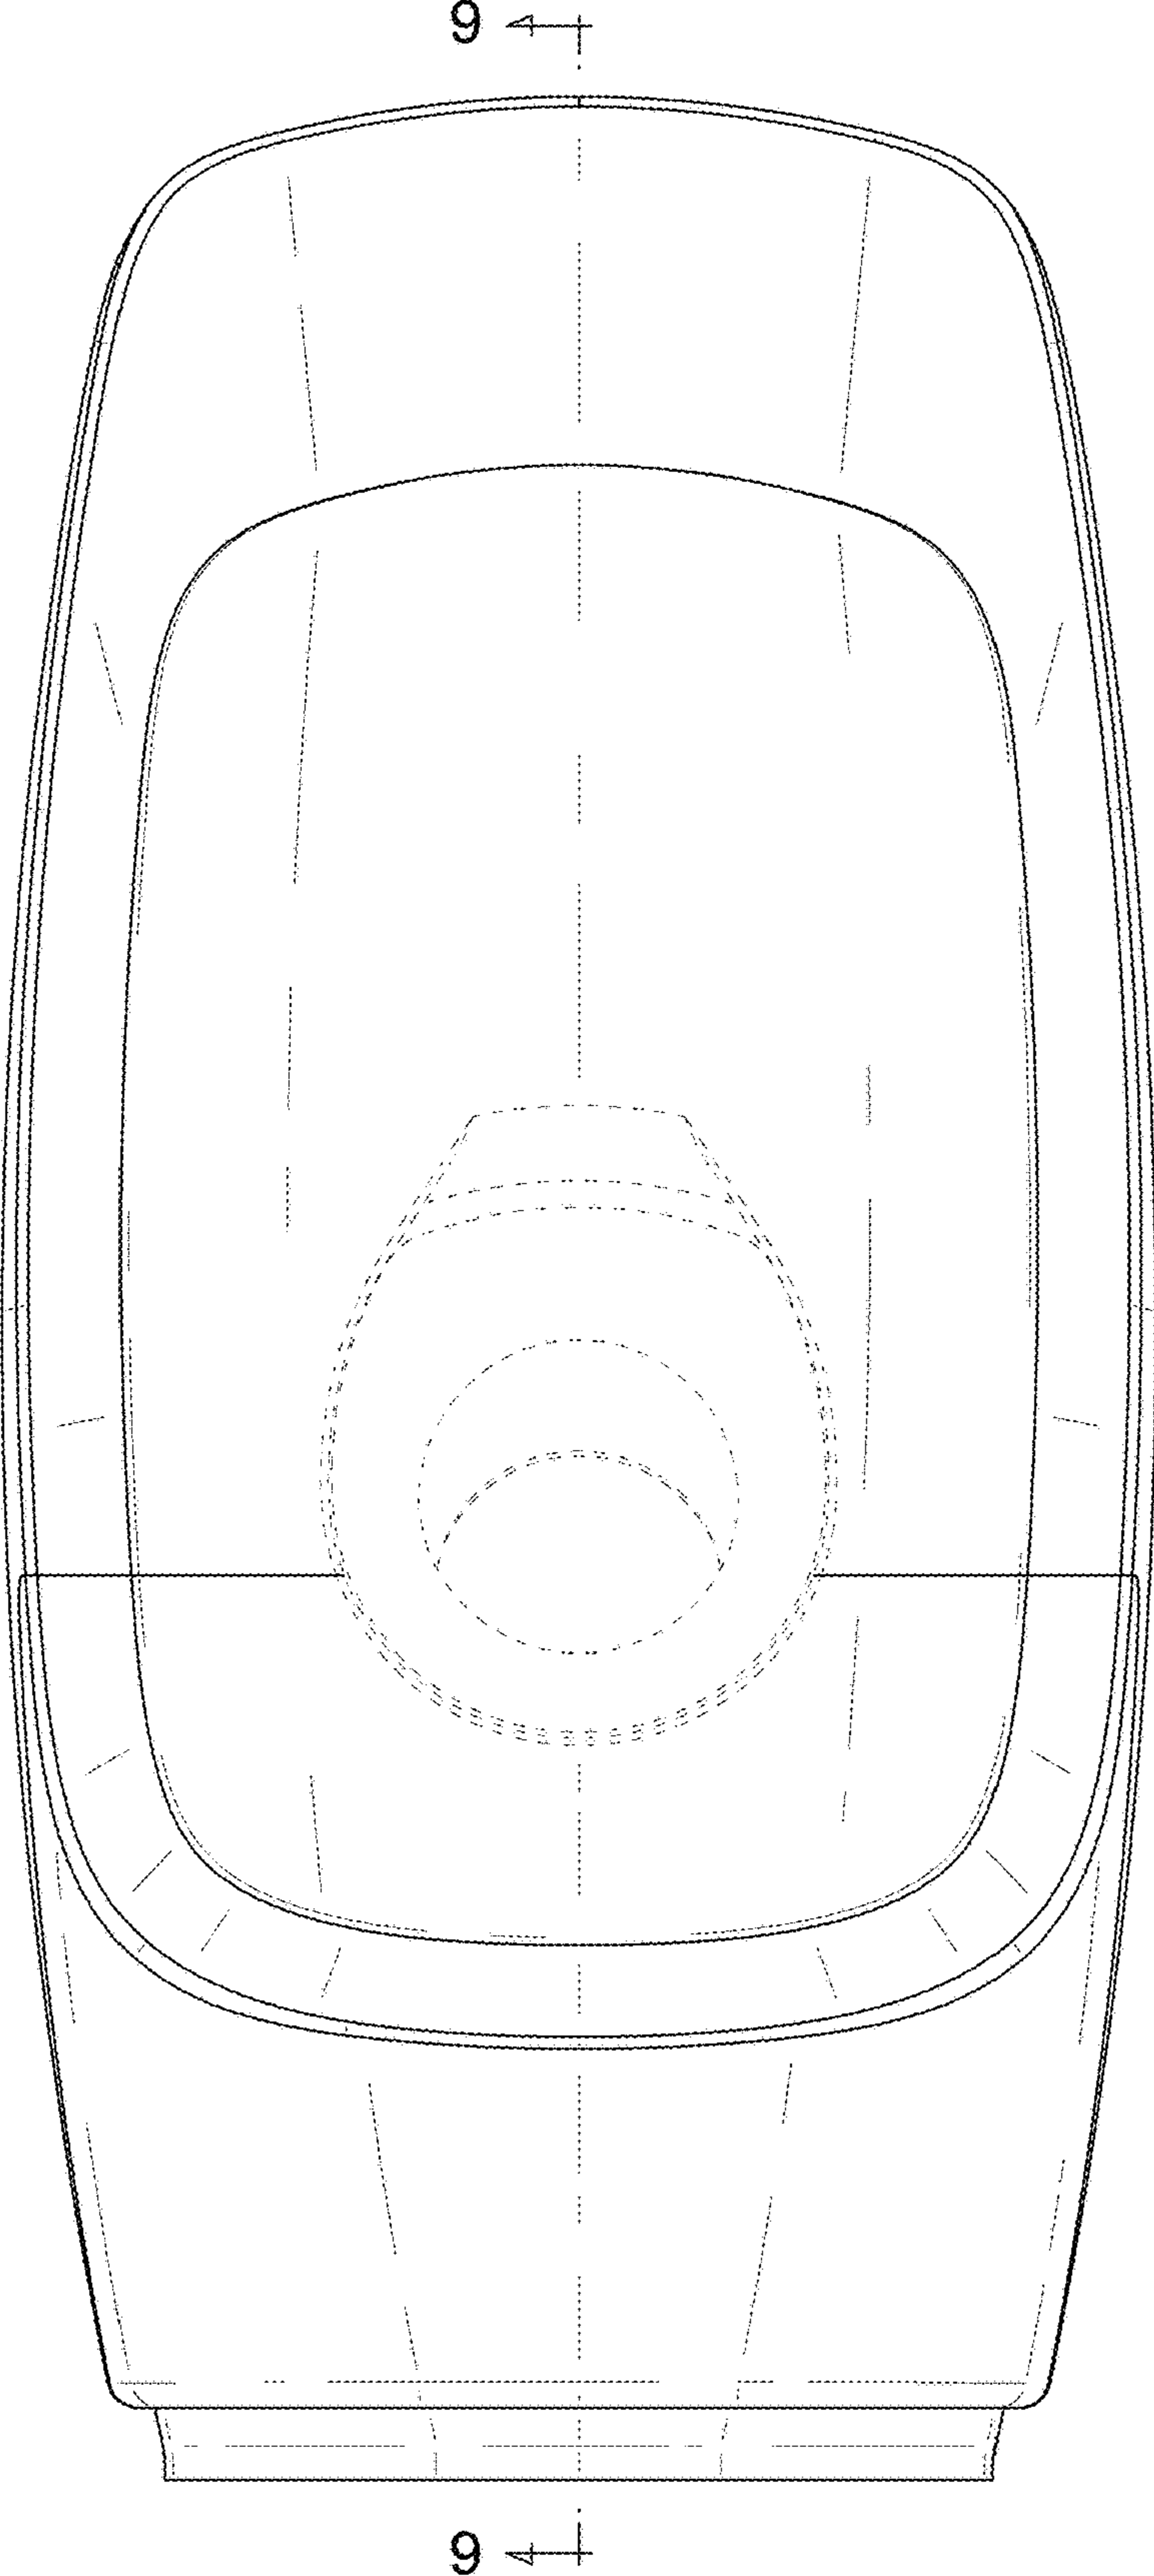


FIG. 3

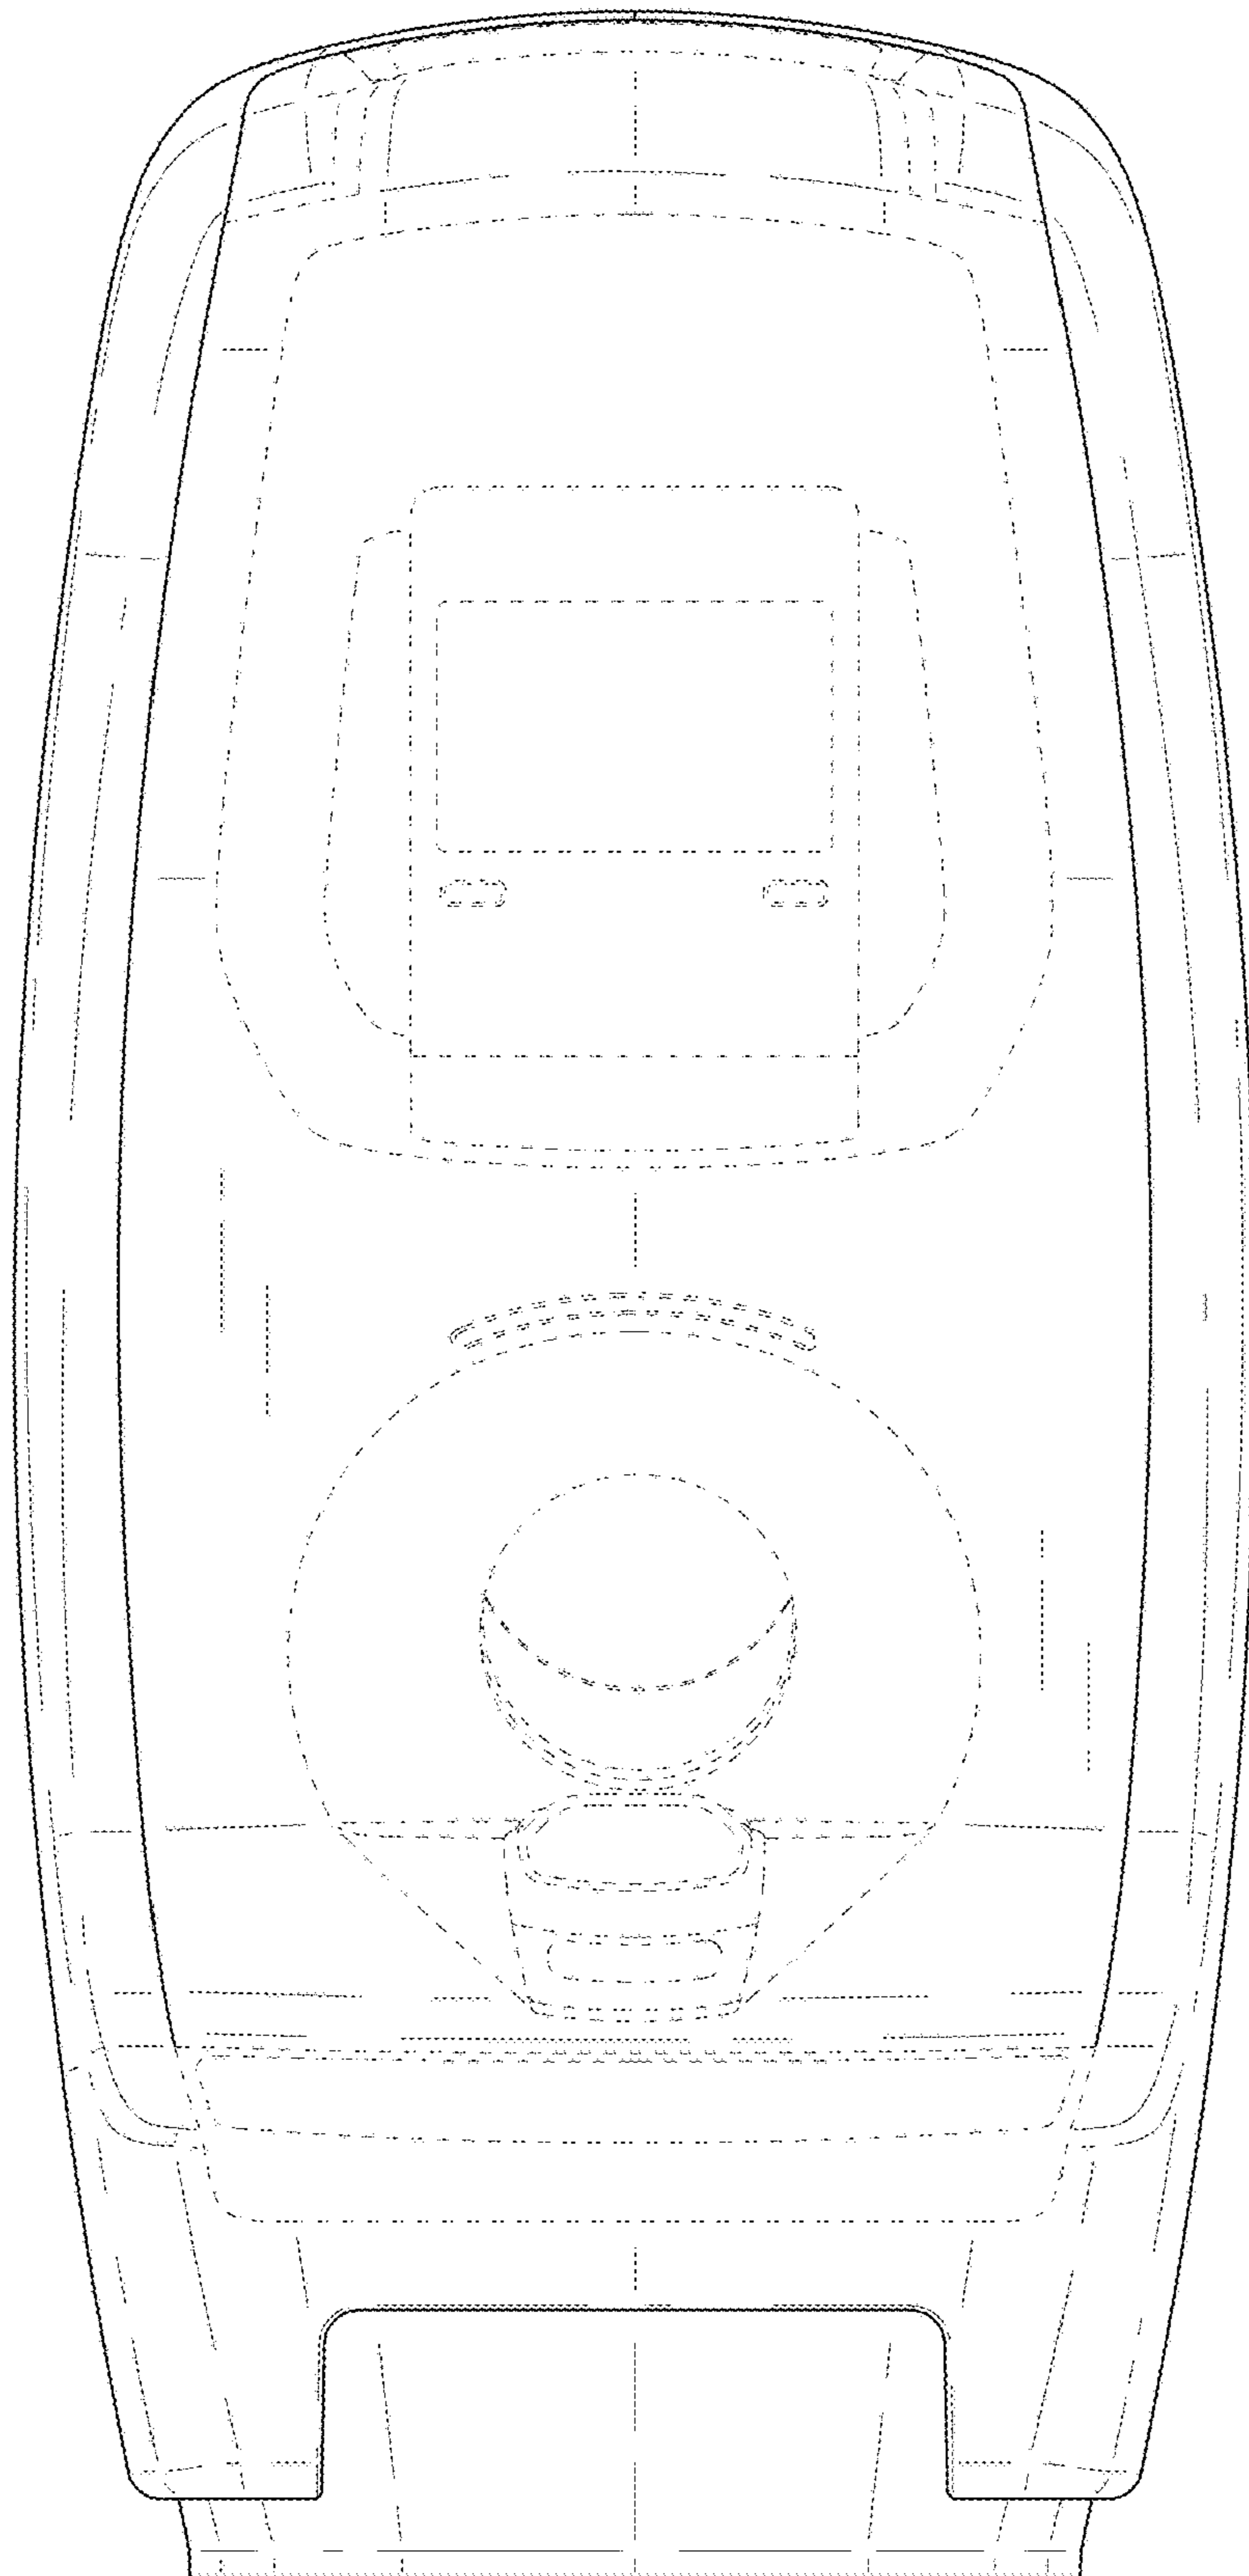




FIG. 4

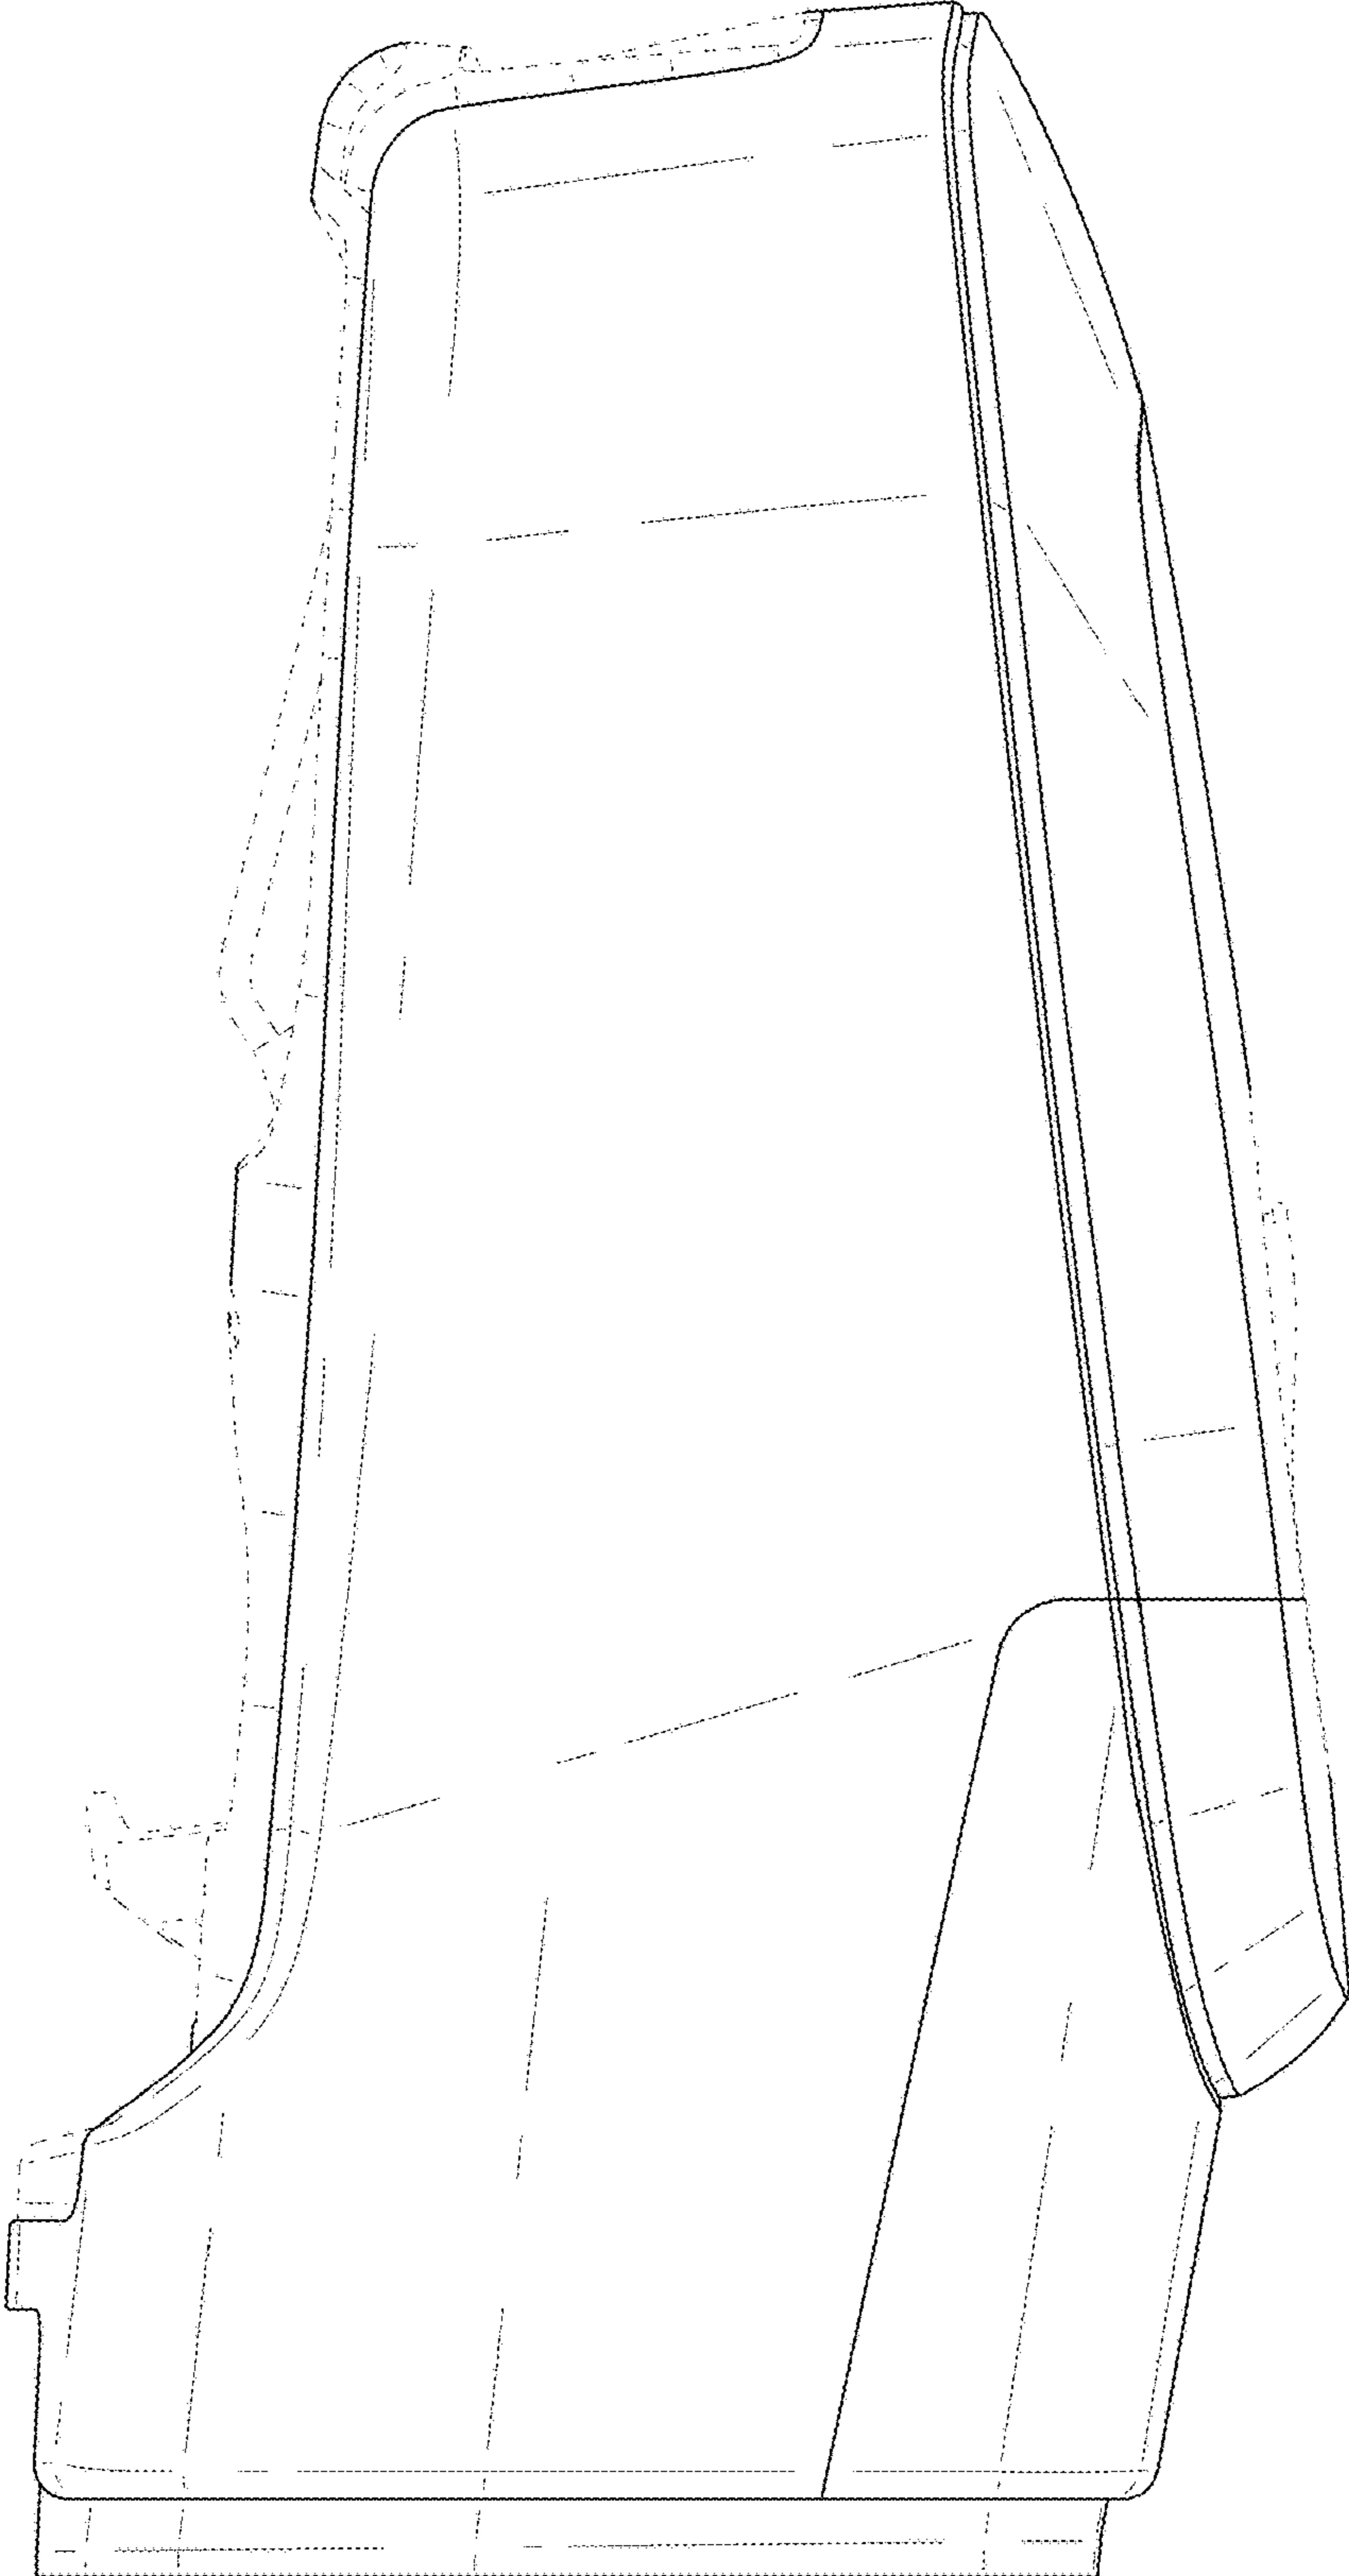


FIG. 5

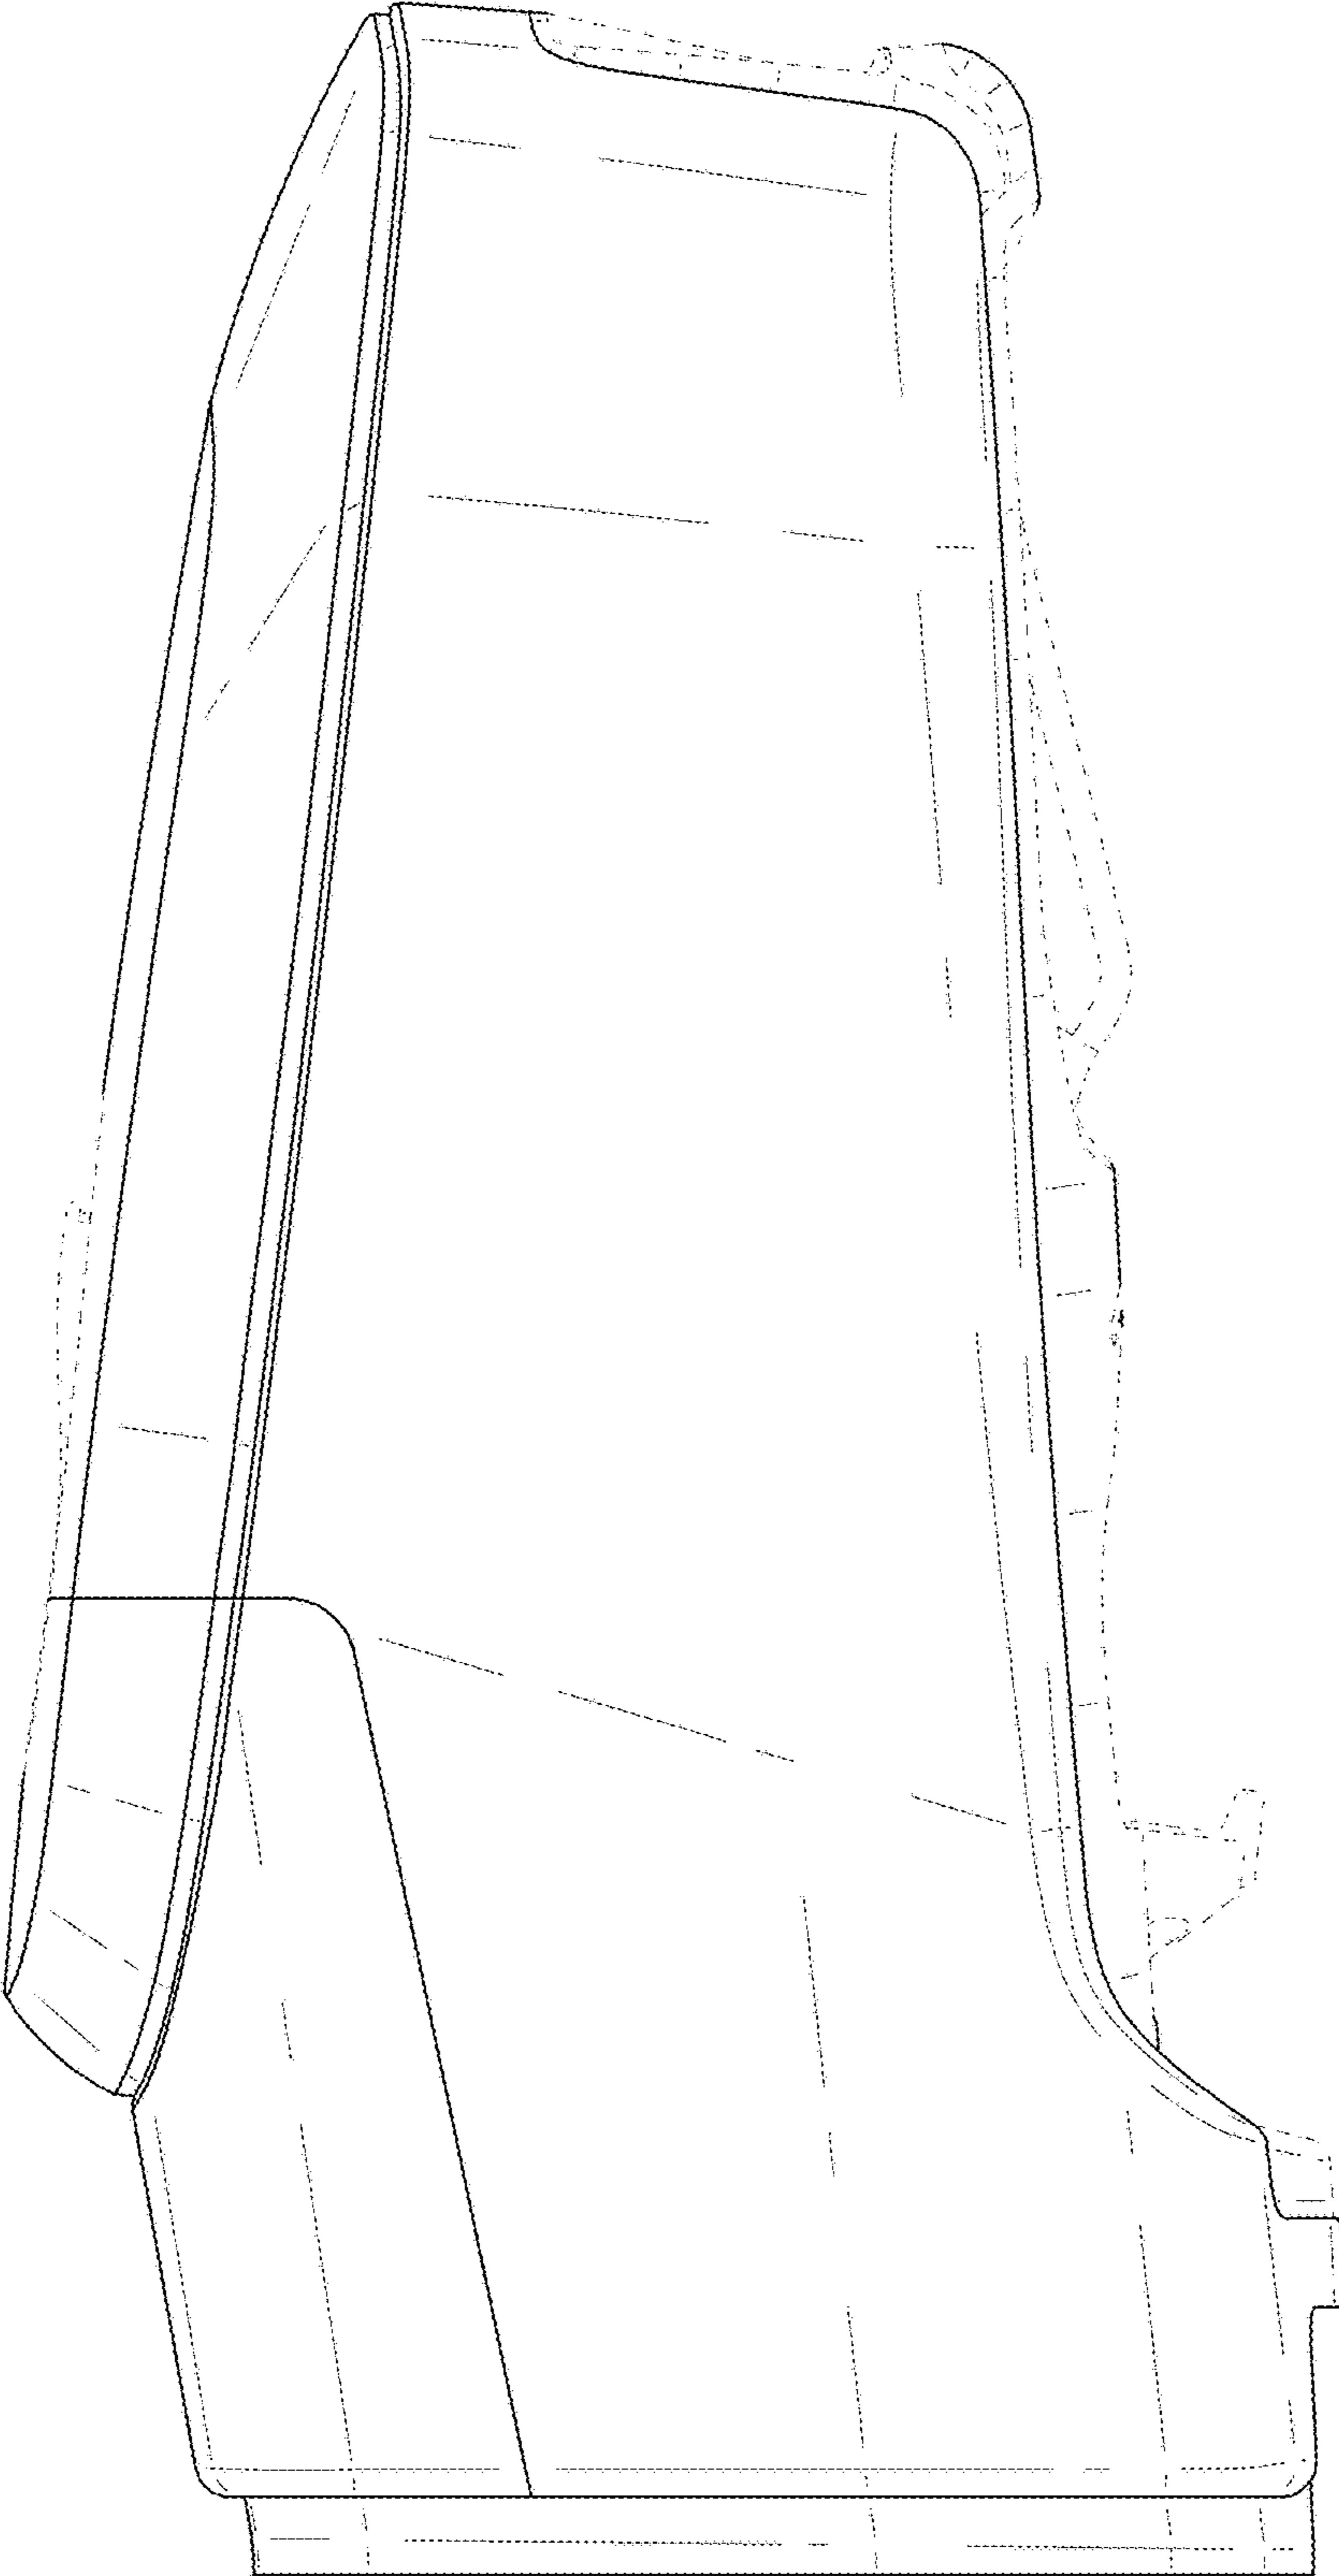


FIG. 6

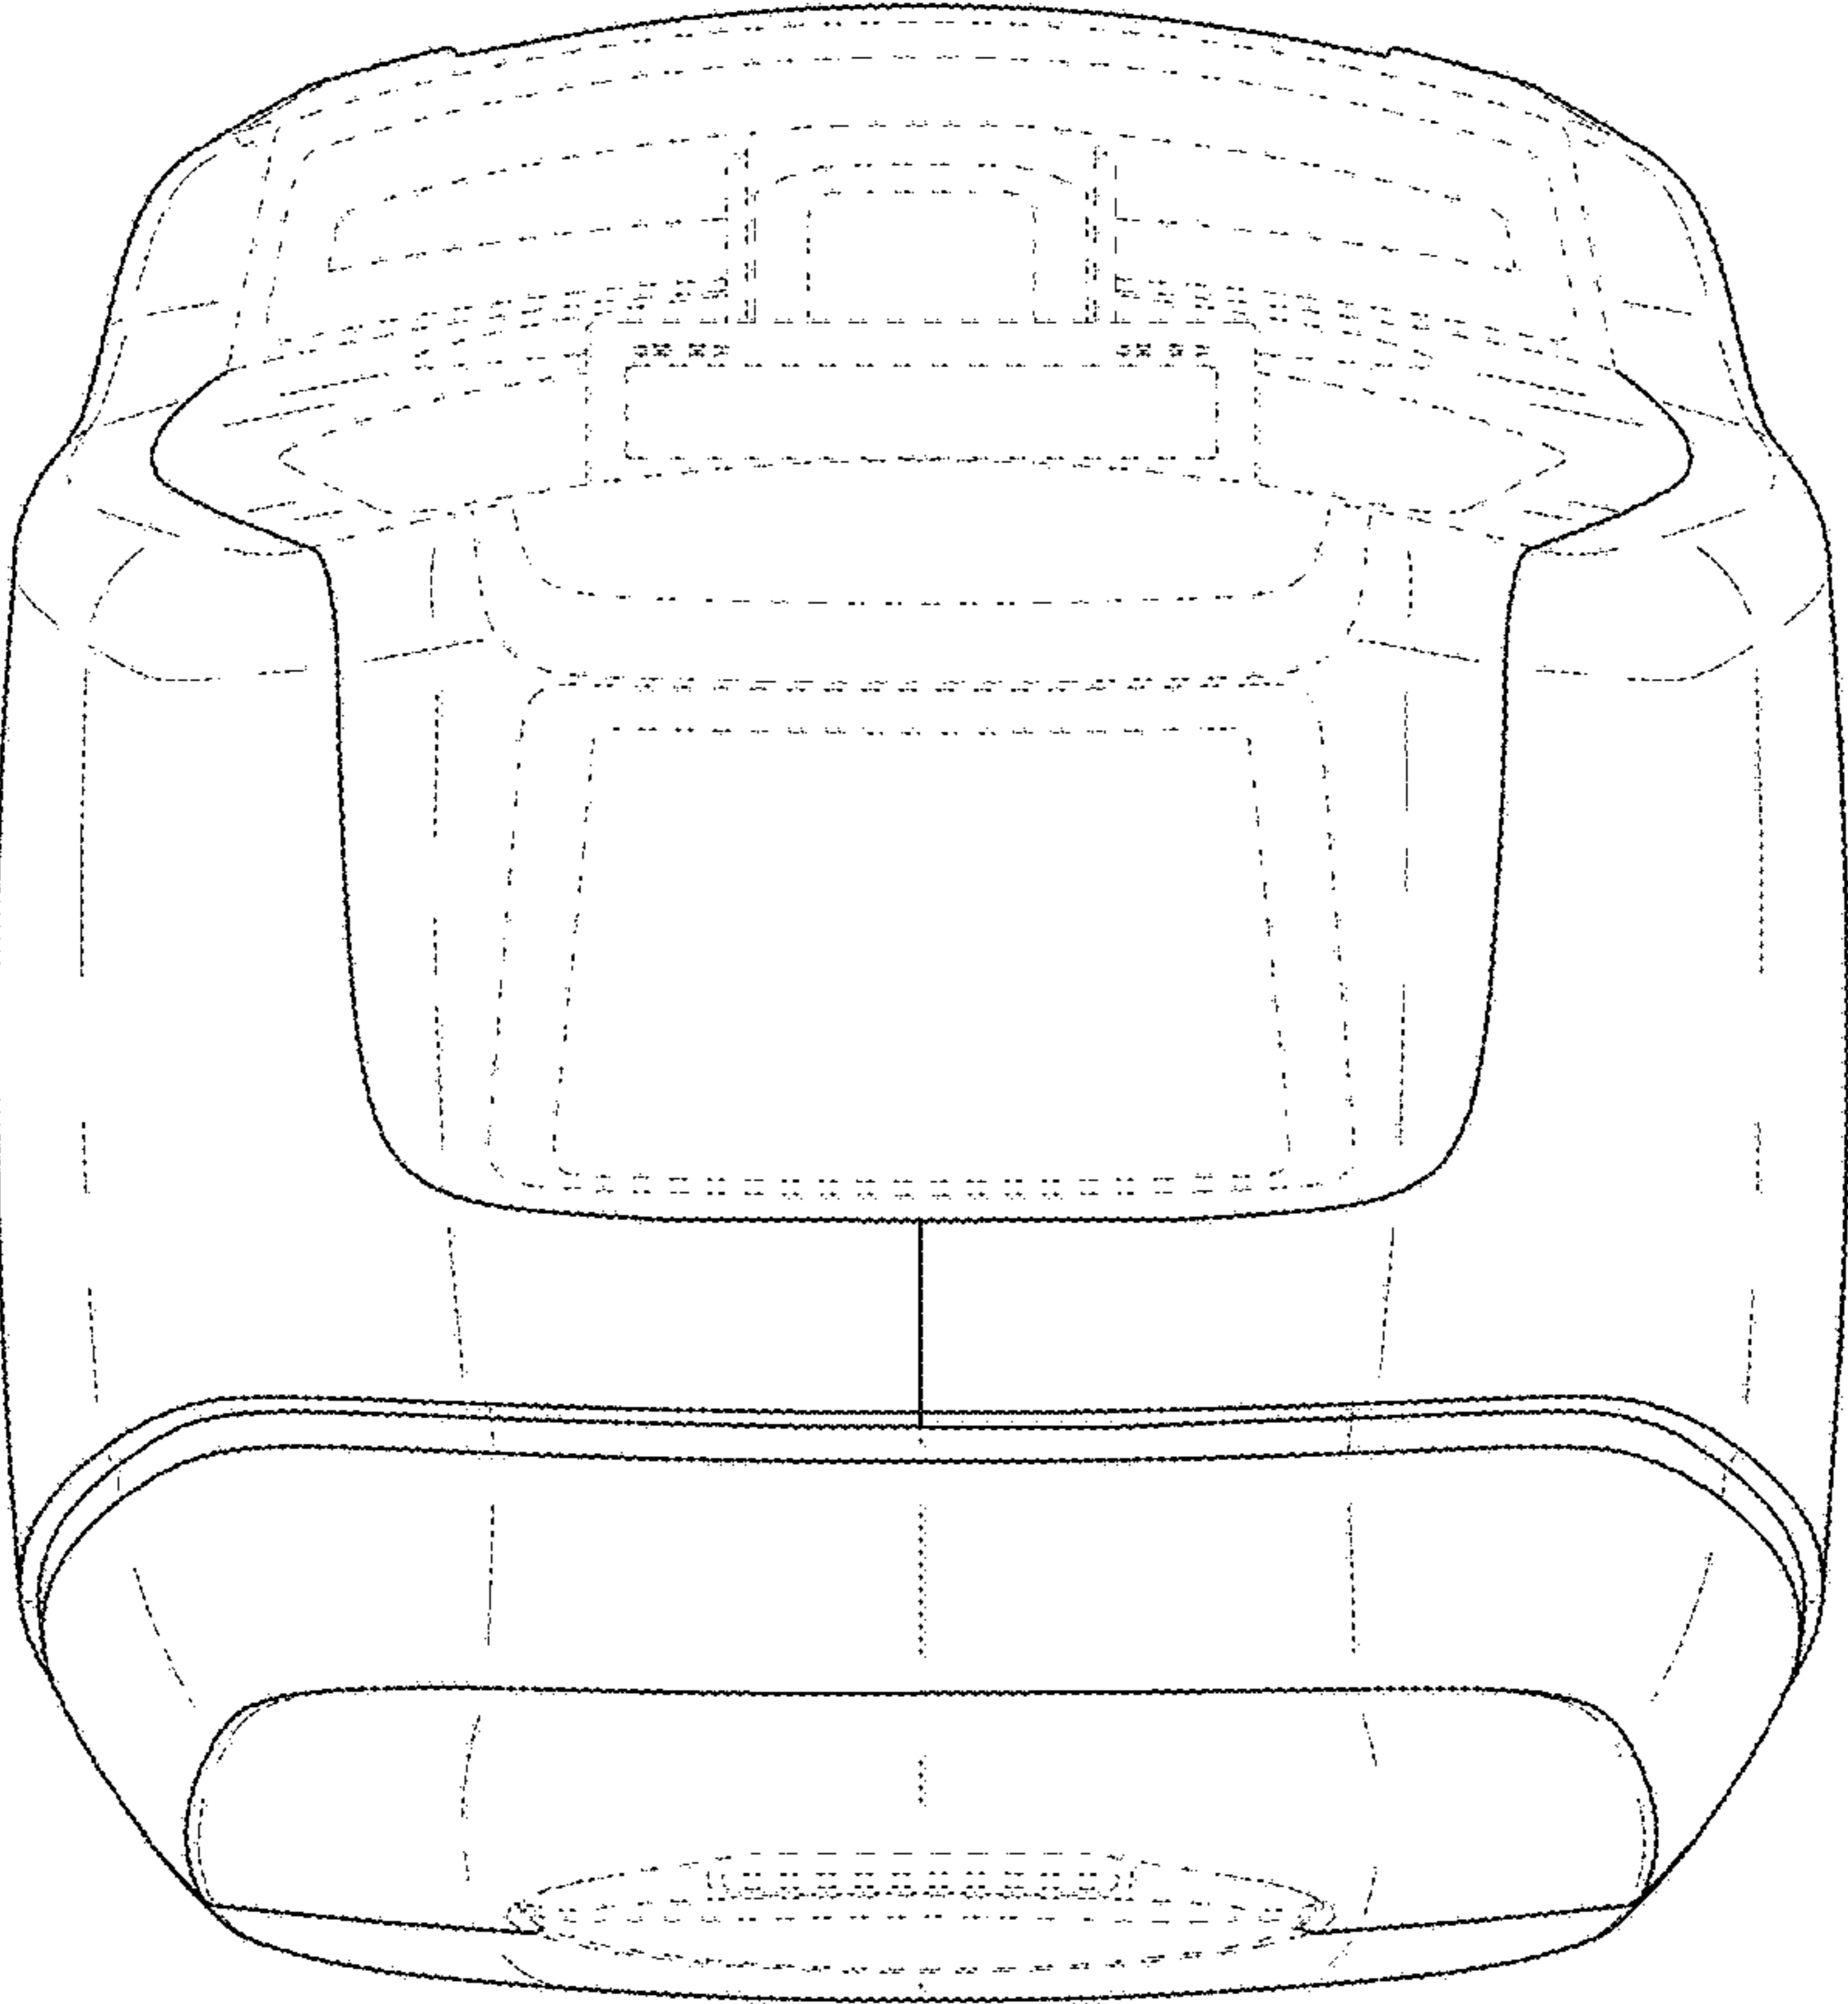


FIG. 7

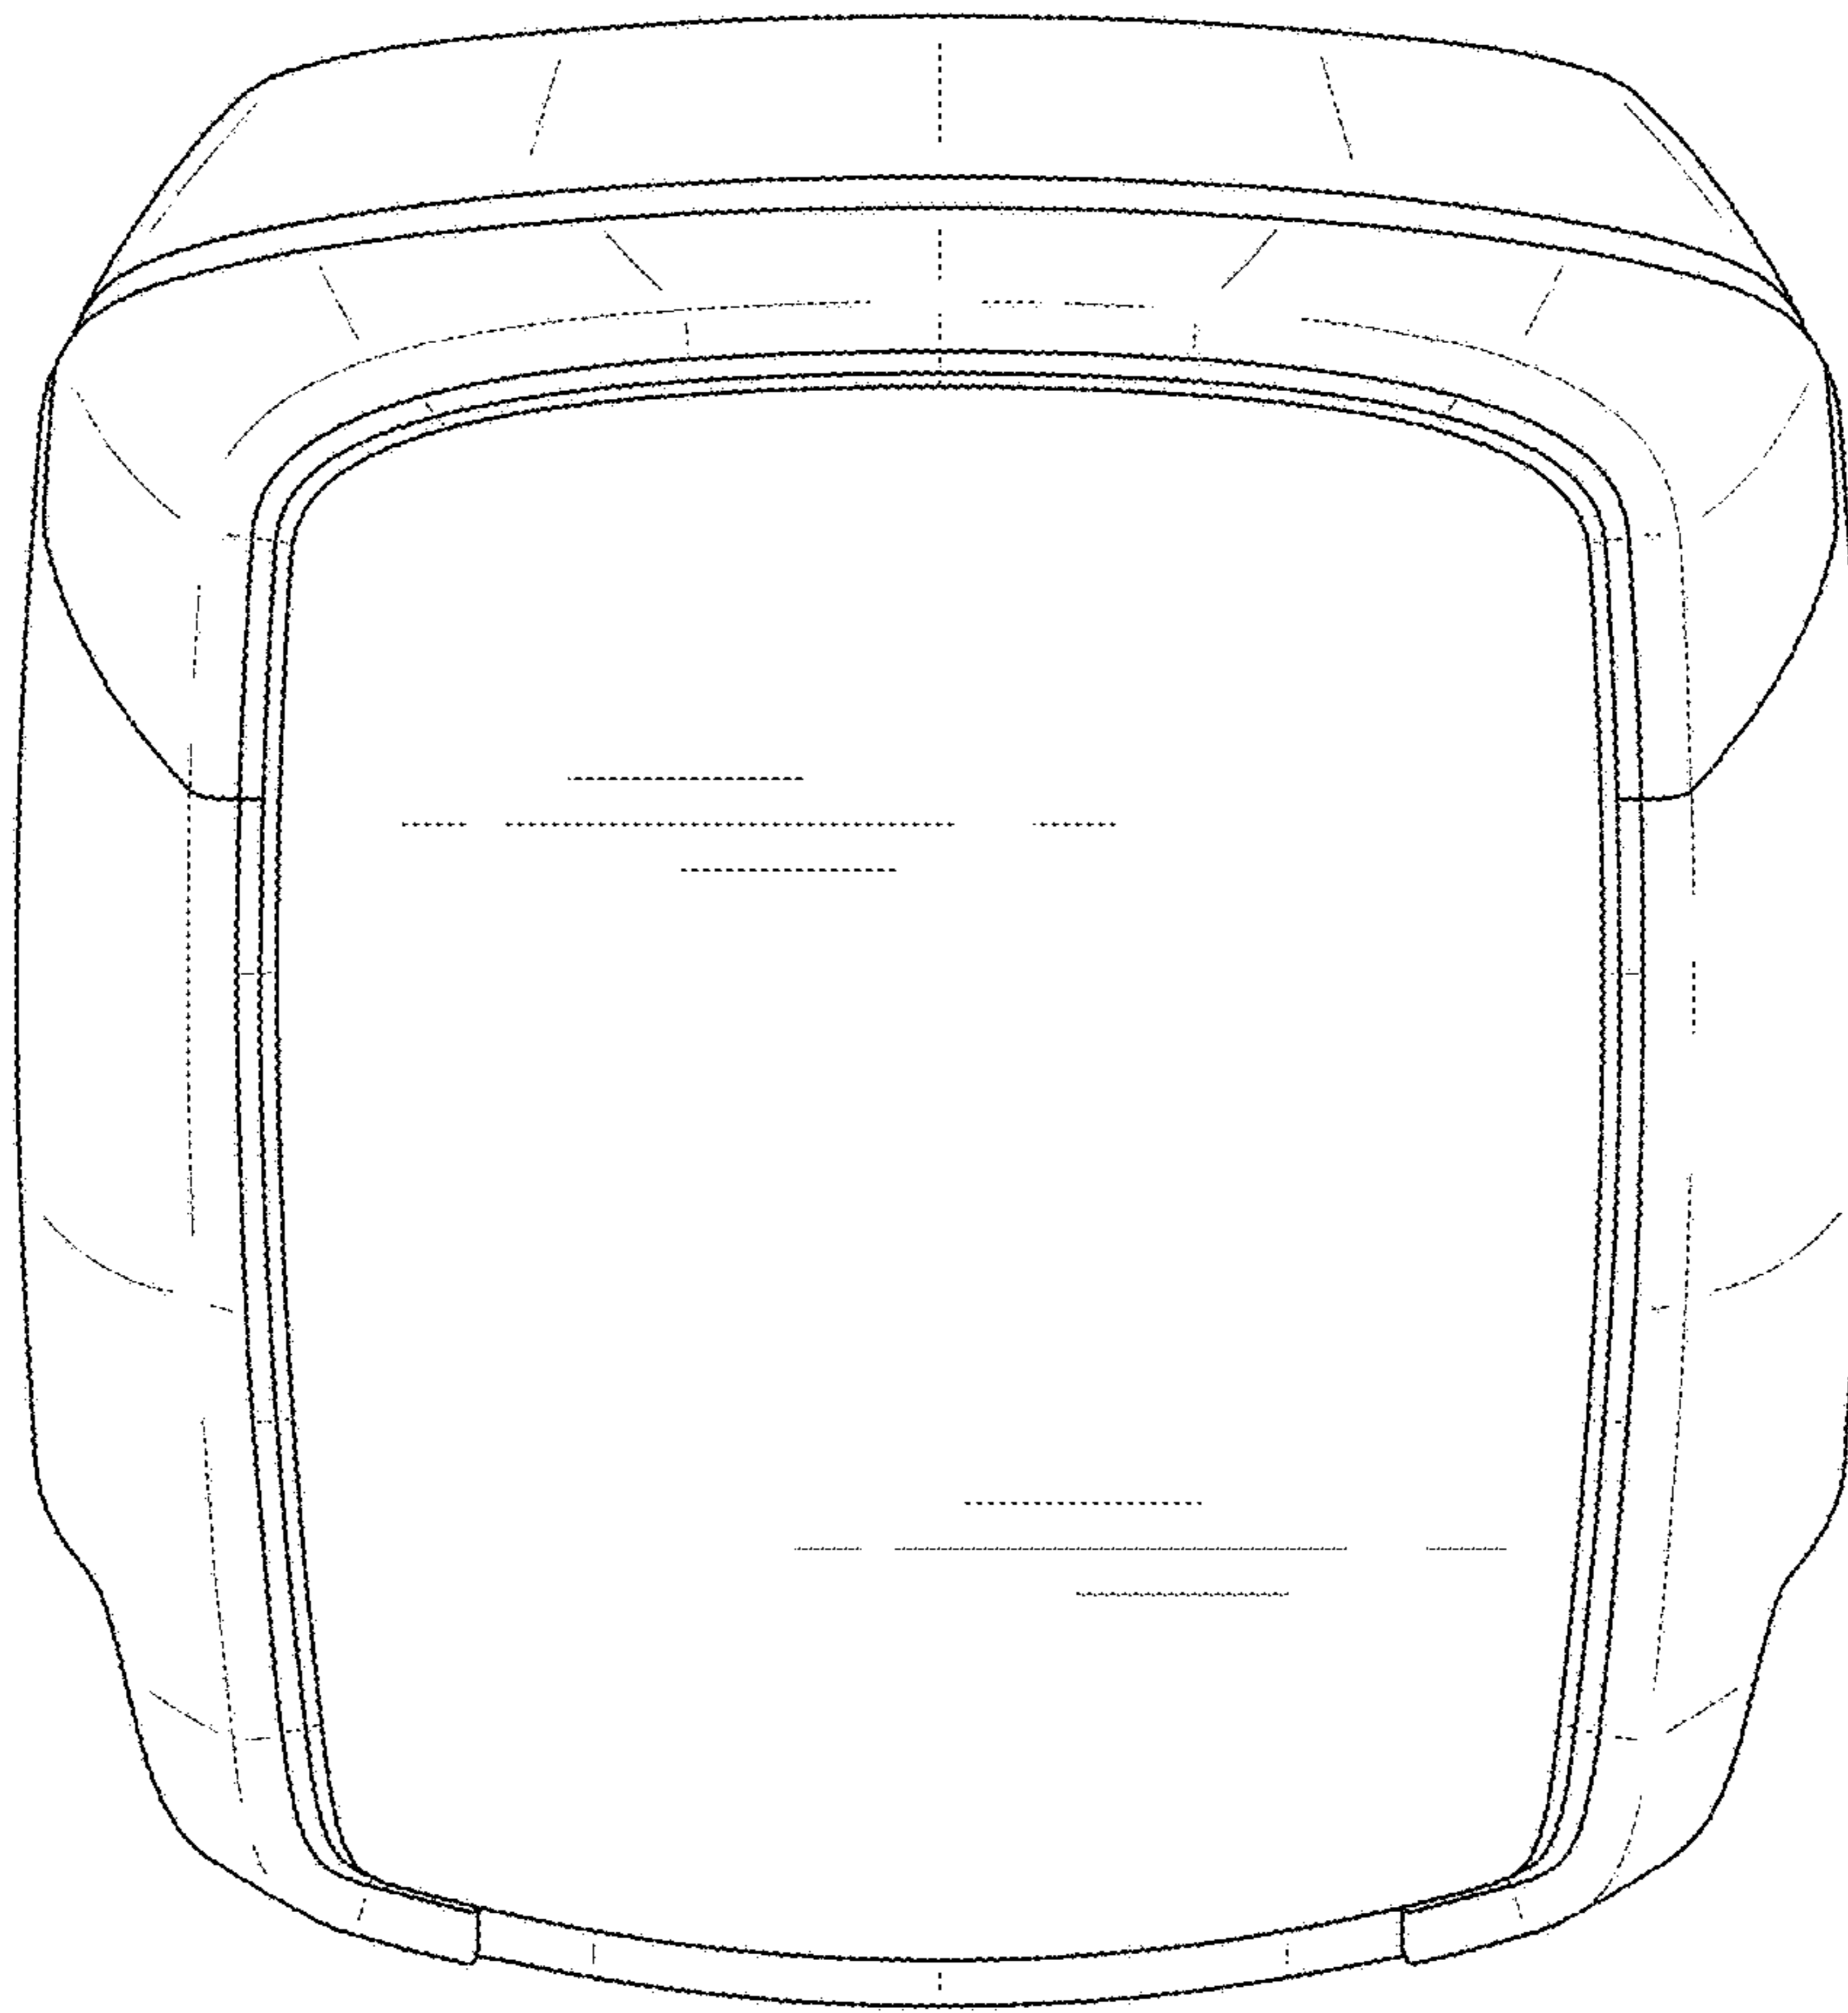




FIG. 8

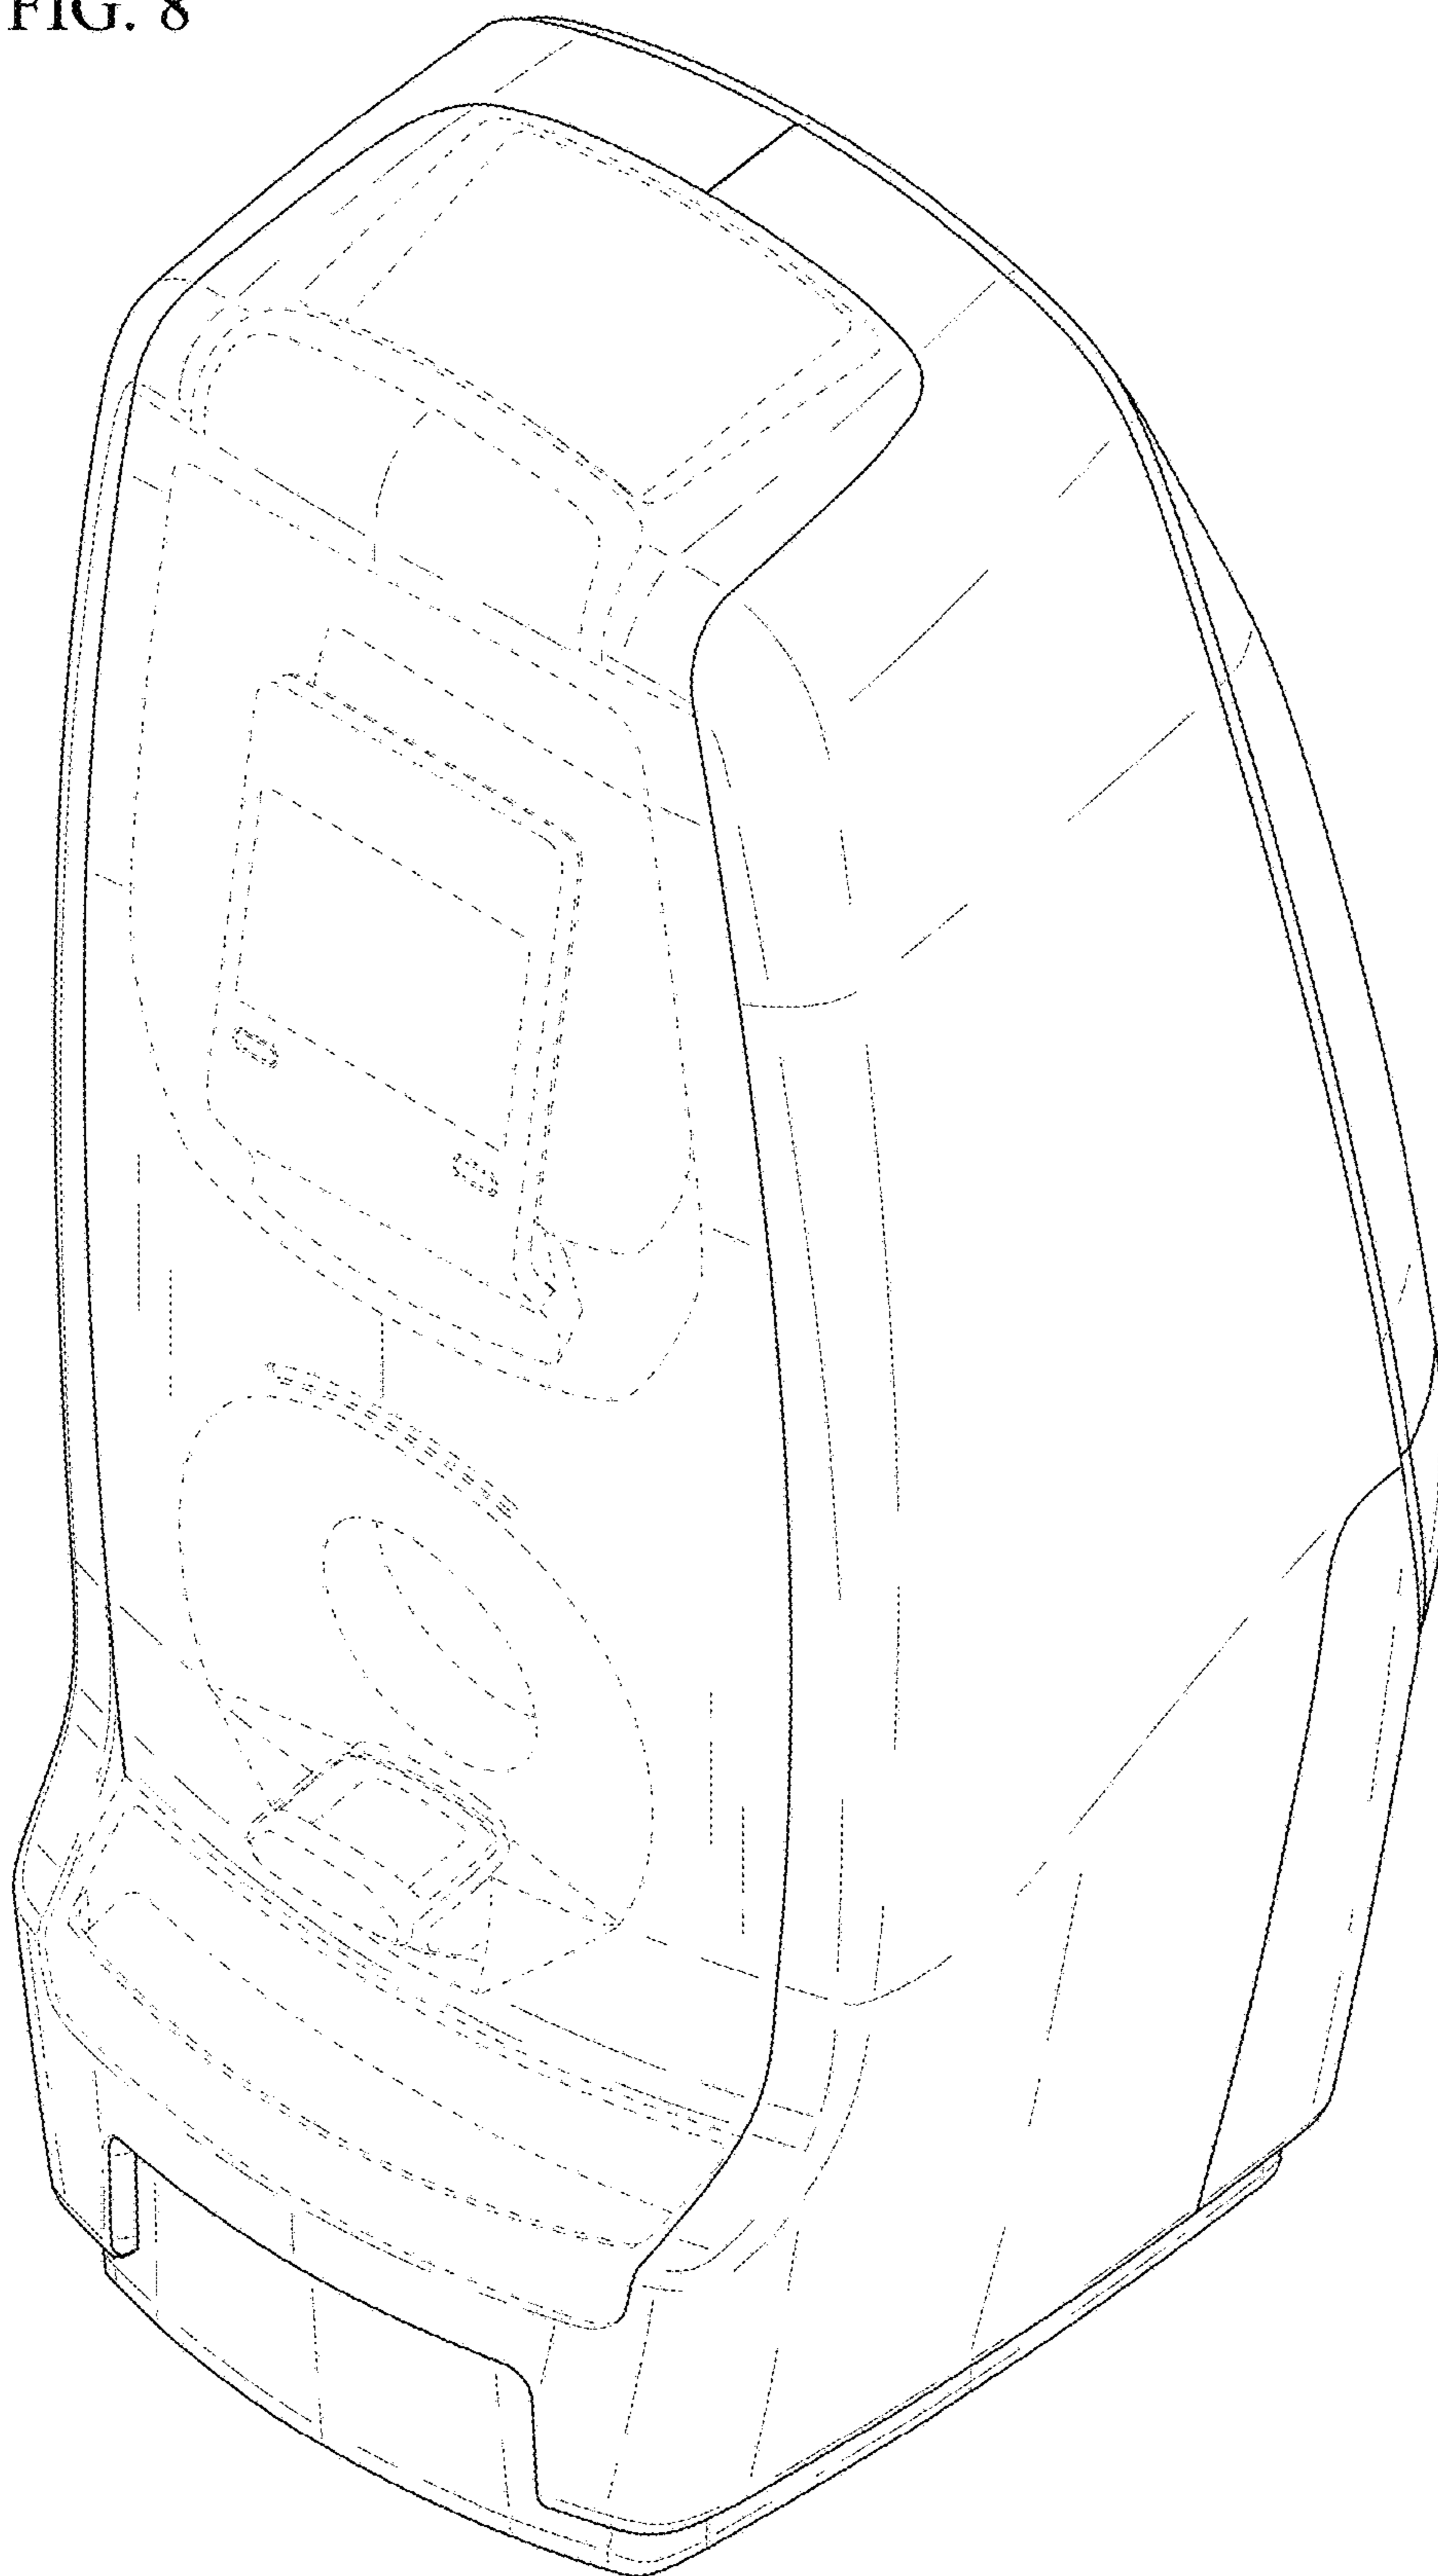


FIG. 9

