



US00D858753S

(12) **United States Design Patent** (10) **Patent No.:** **US D858,753 S**
Yosef et al. (45) **Date of Patent:** **** Sep. 3, 2019**

(54) **MEDICAL DEVICE**

(71) Applicant: **NYXOAH S.A.**, Mont-St-Guilbert (BE)

(72) Inventors: **Yoel Ben Yosef**, Givatayim (IL); **Ronen Adimor**, Ness Ziyona (IL); **Roi Moshe Tsukran**, Ramat Gan (IL)

(73) Assignee: **NYXOAH S.A.**, Mont-St-Guibert (BE)

(**) Term: **15 Years**

(21) Appl. No.: **29/610,459**

(22) Filed: **Jul. 12, 2017**

(30) **Foreign Application Priority Data**

Jan. 17, 2017 (EM) 003646660-0001
Jan. 17, 2017 (EM) 003646660-0002
Jan. 17, 2017 (EM) 003646660-0003

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/113**

(58) **Field of Classification Search**
USPC D24/133, 113

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,856,499 A * 8/1989 Kelly A61F 5/41
600/38
D349,958 S * 8/1994 Hollis D24/112

(Continued)

FOREIGN PATENT DOCUMENTS

JP 09234189 A * 9/1997

OTHER PUBLICATIONS

Direct Home Medical. Link: https://www.directhomemedical.com/cart/merchant.mvc?Screen=PROD&Product_Code=z1-travel-cpap-

powershell-module-hdmusa&Store_Code=DHM&gclid=EAlaIQobChMIkea7sdvj3gIV9f_jBx2jLQa5EAQYBSABEgLckfD_BwE visited Nov. 20, 2018. PowerShell Z1 Series CPAP Machines. (Year: 2018).*

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Lauren D McVey

(74) *Attorney, Agent, or Firm* — Dorsey & Whitney LLP

(57) **CLAIM**

The ornamental design for a medical device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a medical device, showing our new design in a combined state;

FIG. 2 is a top plan view of the medical device of FIG. 1; FIG. 3 is a bottom plan view of the medical device of FIG. 1;

FIG. 4 is a front elevational view of the medical device of FIG. 1;

FIG. 5 is a rear elevational view of the medical device of FIG. 1;

FIG. 6 is a side elevational view of the medical device of FIG. 1;

FIG. 7 is another side elevational view of the medical device of FIG. 1;

FIG. 8 is a perspective view of a medical device, showing our new design in a separated state with portions removed in order to show aspects of the design not otherwise apparent;

FIG. 9 is a top plan view of the medical device of FIG. 8;

FIG. 10 is a bottom plan view of the medical device of FIG. 8;

FIG. 11 is a front elevational view of the medical device of FIG. 8;

FIG. 12 is a rear elevational view of the medical device of FIG. 8;

FIG. 13 is a side elevational view of the medical device of FIG. 8;

FIG. 14 is another side elevational view of the medical device of FIG. 8;

(Continued)

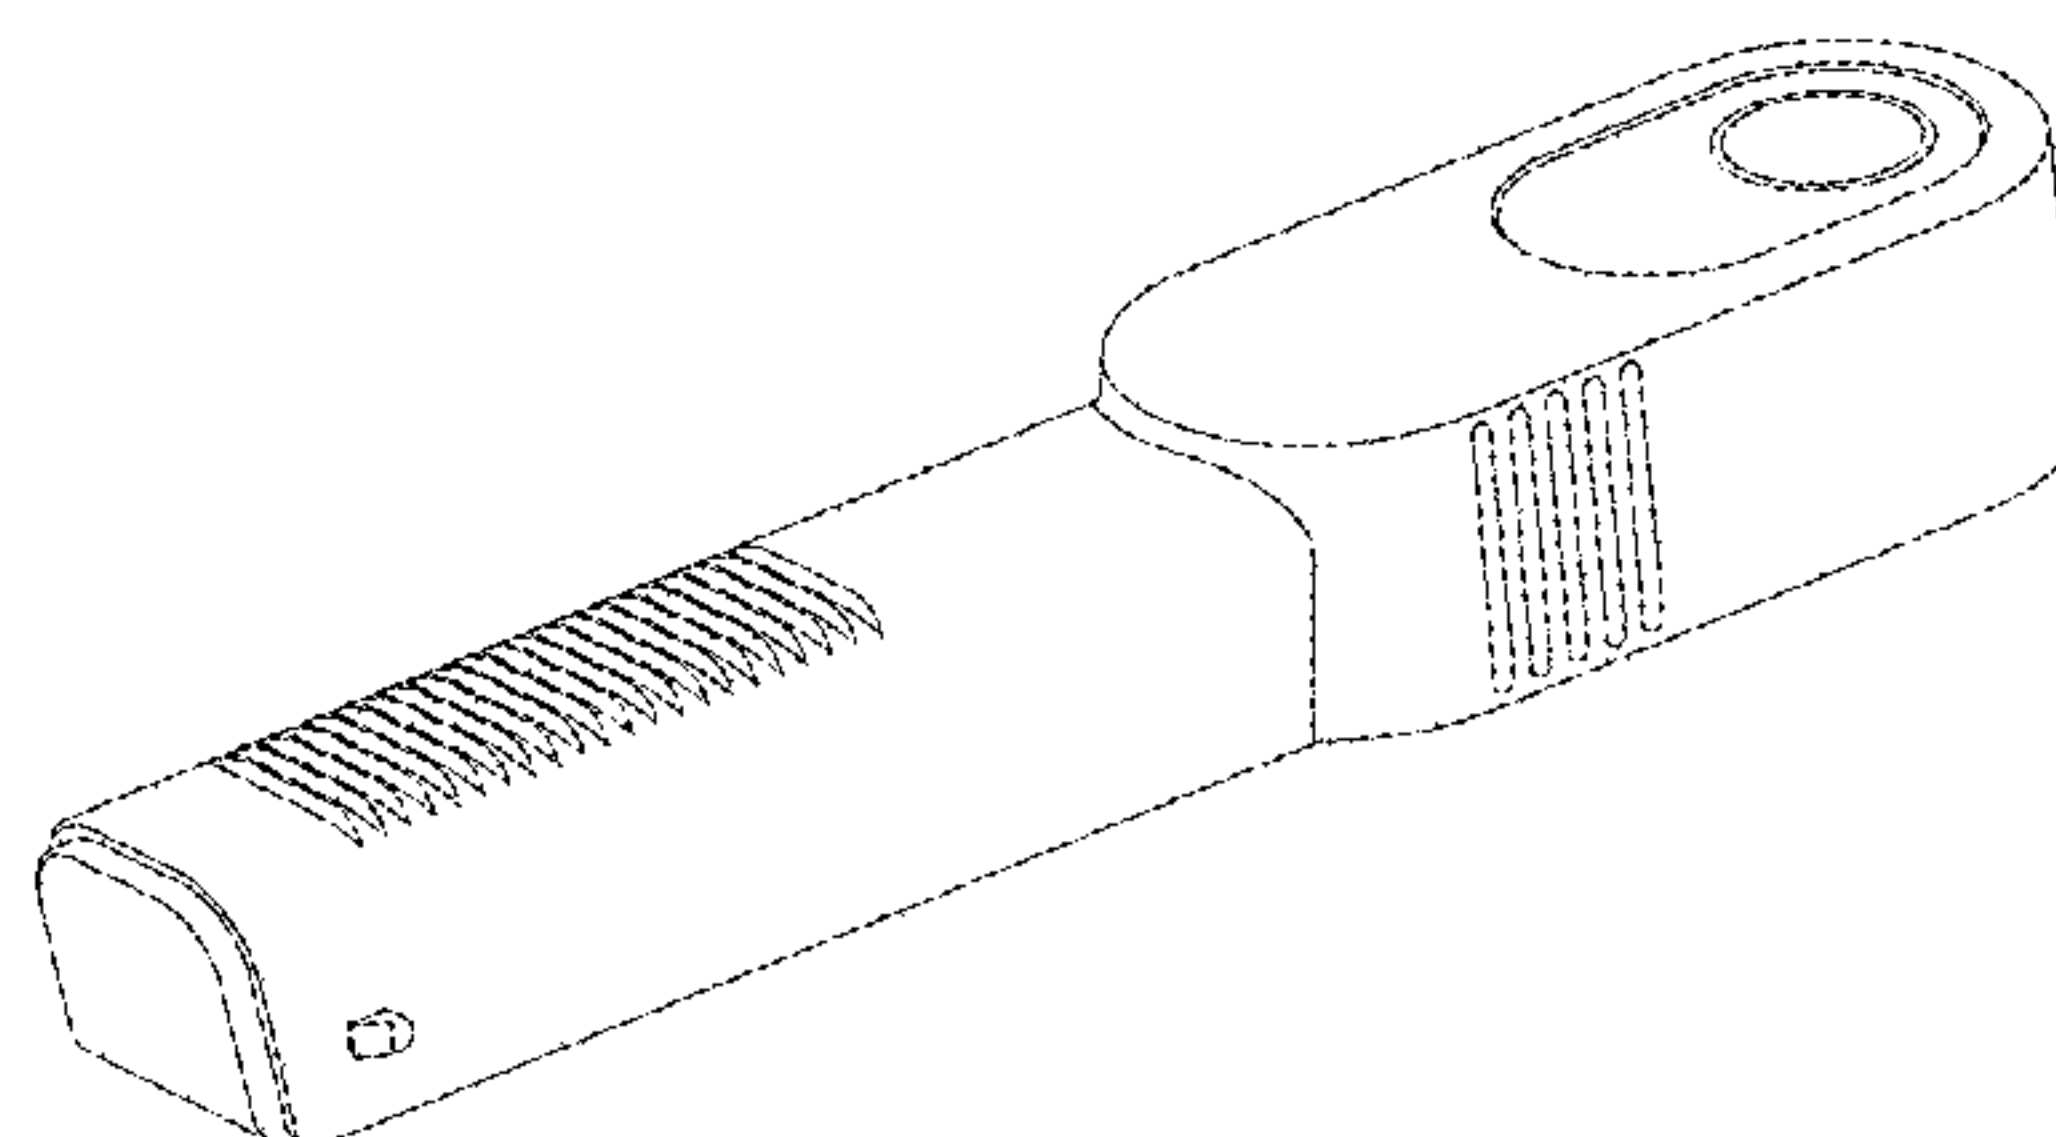
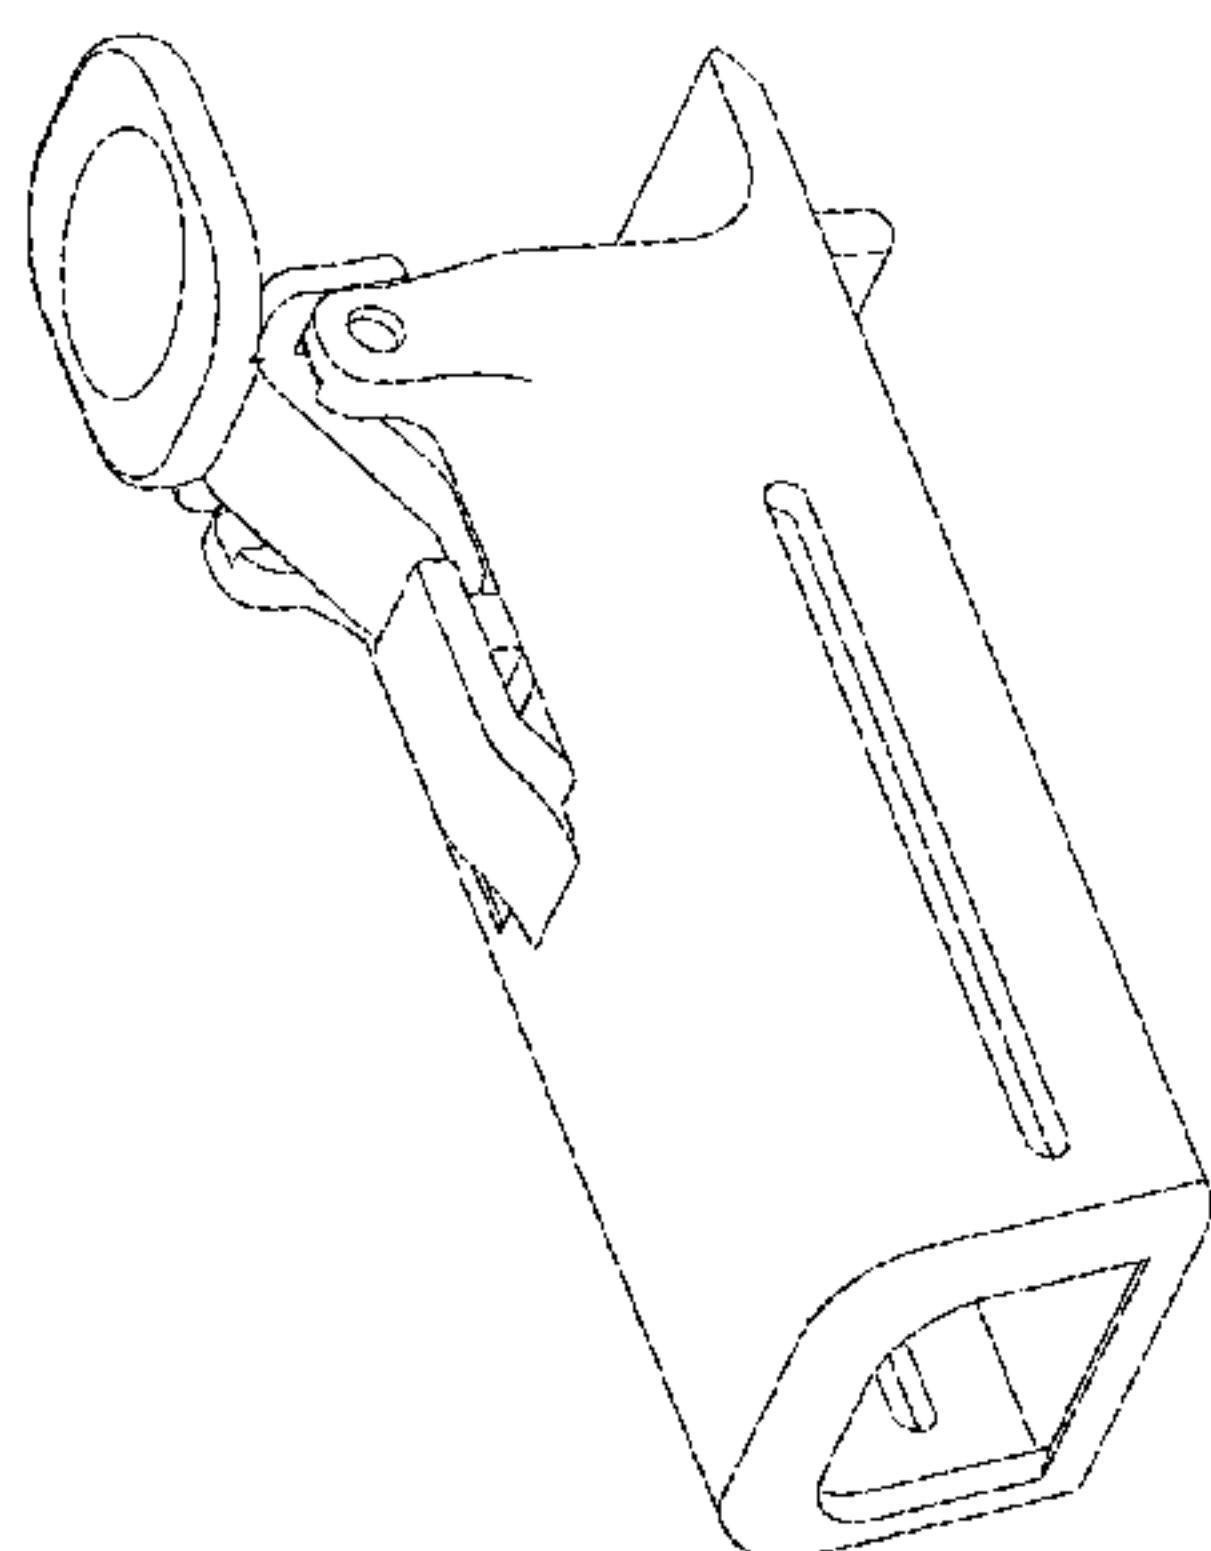


FIG. 15 is a perspective view of a medical device, showing our new design in a separated state with portions removed in order to show aspects of the design not otherwise apparent; FIG. 16 is a top plan view of the medical device of FIG. 15; FIG. 17 is a bottom plan view of the medical device of FIG. 15; FIG. 18 is a front elevational view of the medical device of FIG. 15; FIG. 19 is a rear elevational view of the medical device of FIG. 15; FIG. 20 is a side elevational view of the medical device of FIG. 15; and, FIG. 21 is another side elevational view of the medical device of FIG. 15. The broken lines in the drawings depict portions of the medical device that form no part of the claimed design.

1 Claim, 21 Drawing Sheets

(58) **Field of Classification Search**
CPC A61M 16/0677; A61M 16/0683; A61M 16/0866; A61N 1/3601; A61N 1/36003; A61N 1/36078
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D610,677	S *	2/2010	Tyce	D24/113
D655,807	S *	3/2012	Mogensen	D24/108
D683,851	S *	6/2013	Greenhalgh	D24/133
D735,322	S *	7/2015	Tyce	D24/113
D756,513	S *	5/2016	Cheney	D24/133
D764,657	S *	8/2016	Bokelman	D24/113
9,962,500	B2 *	5/2018	Holtwick	A61M 5/158
2002/0077599	A1 *	6/2002	Wojcik	A61M 5/158
				604/162
2004/0010233	A1 *	1/2004	Hjertman	A61M 5/3129
				604/187
2017/0007442	A1 *	1/2017	Dietz	A61F 5/566
2018/0200520	A1 *	7/2018	Tranchina	A61B 5/0488

* cited by examiner

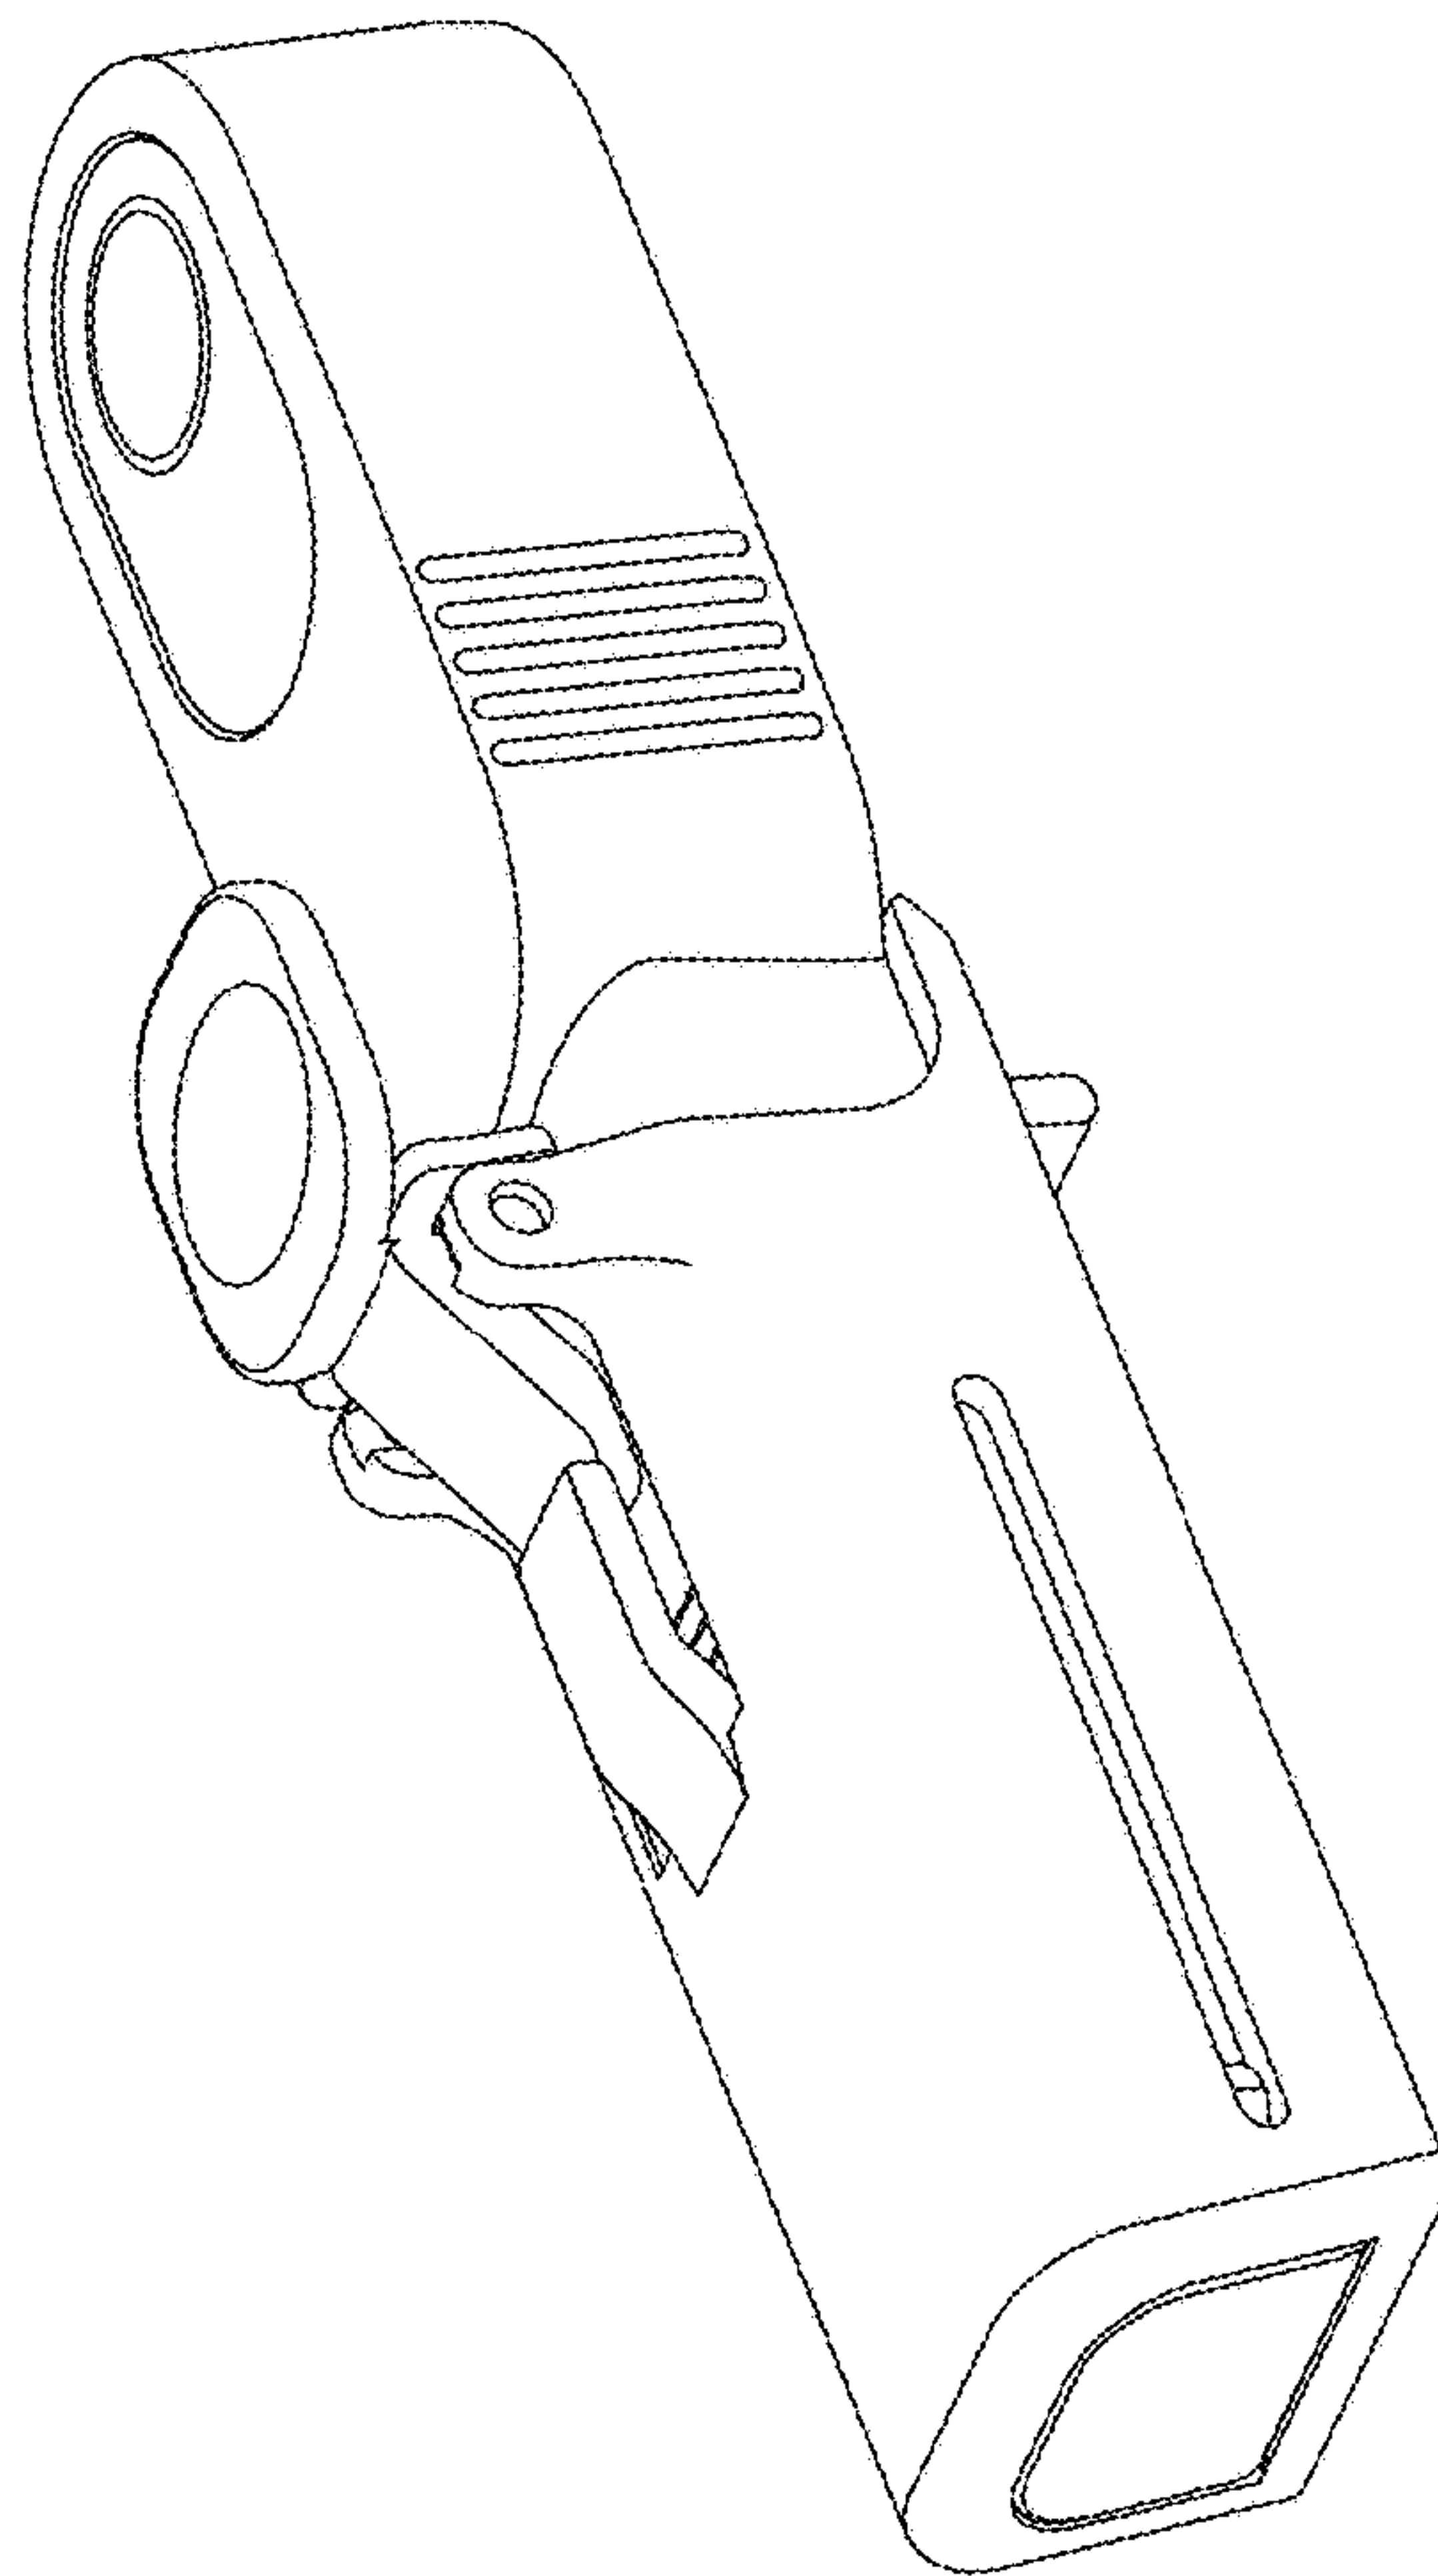


FIG. 1

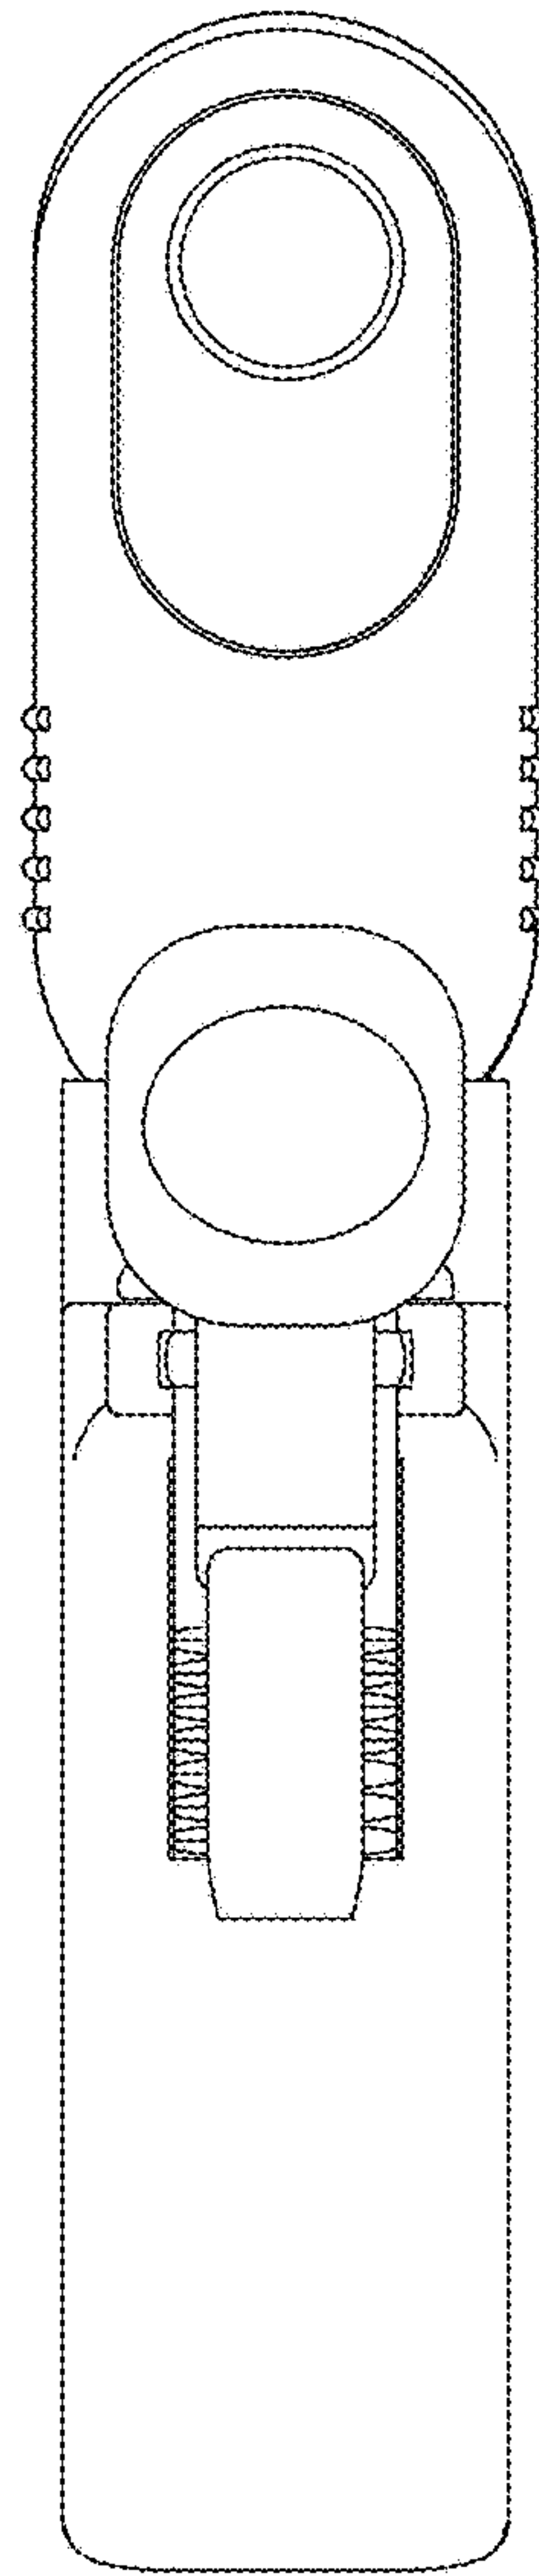


FIG. 2

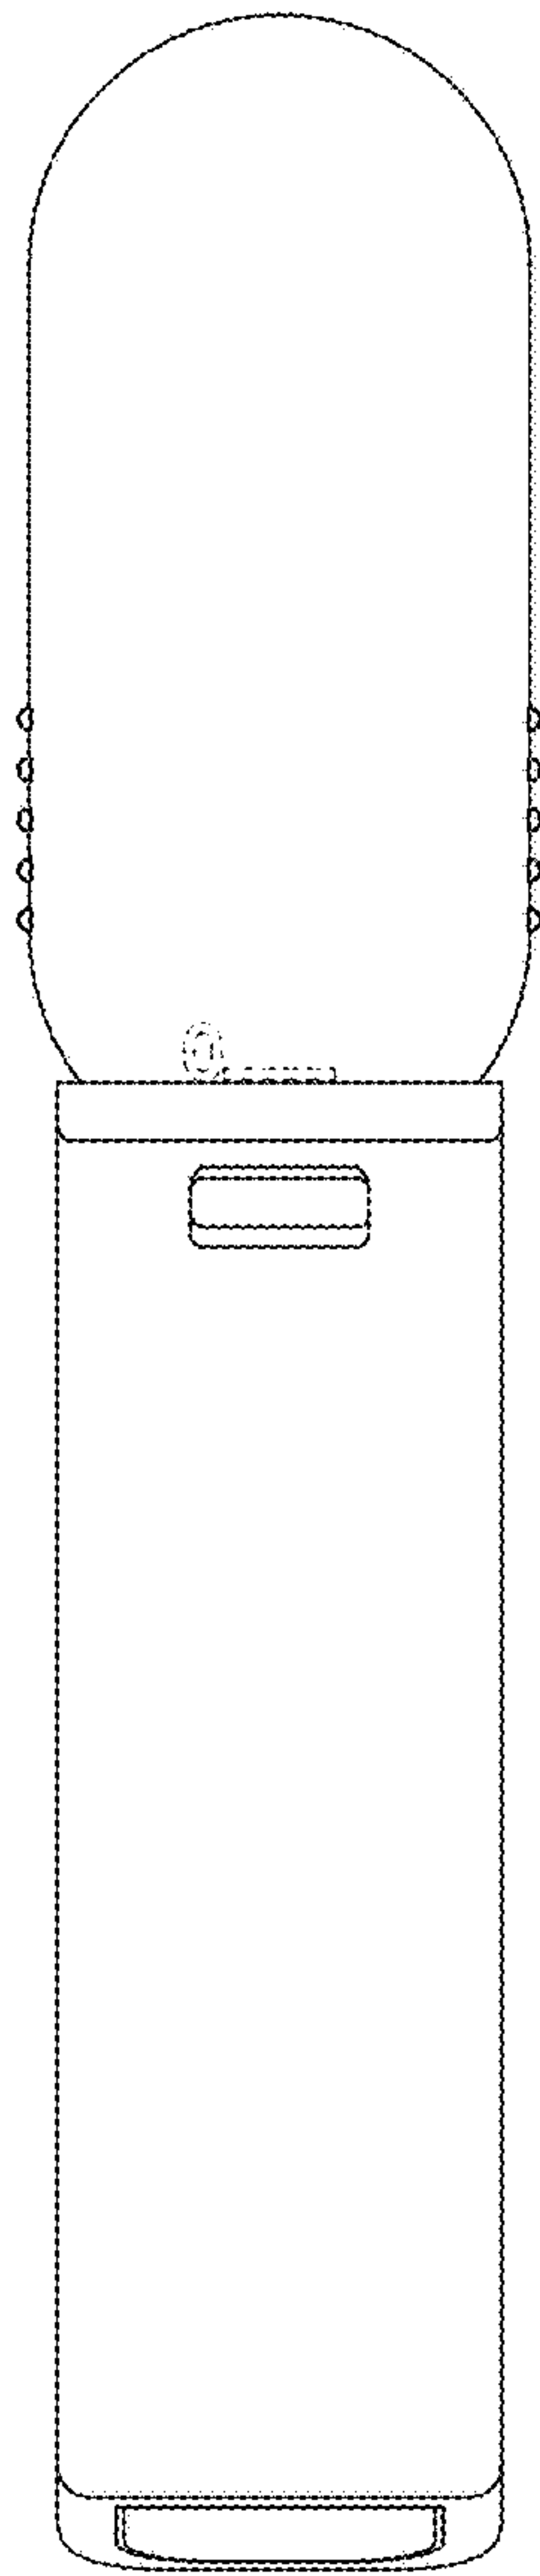


FIG. 3

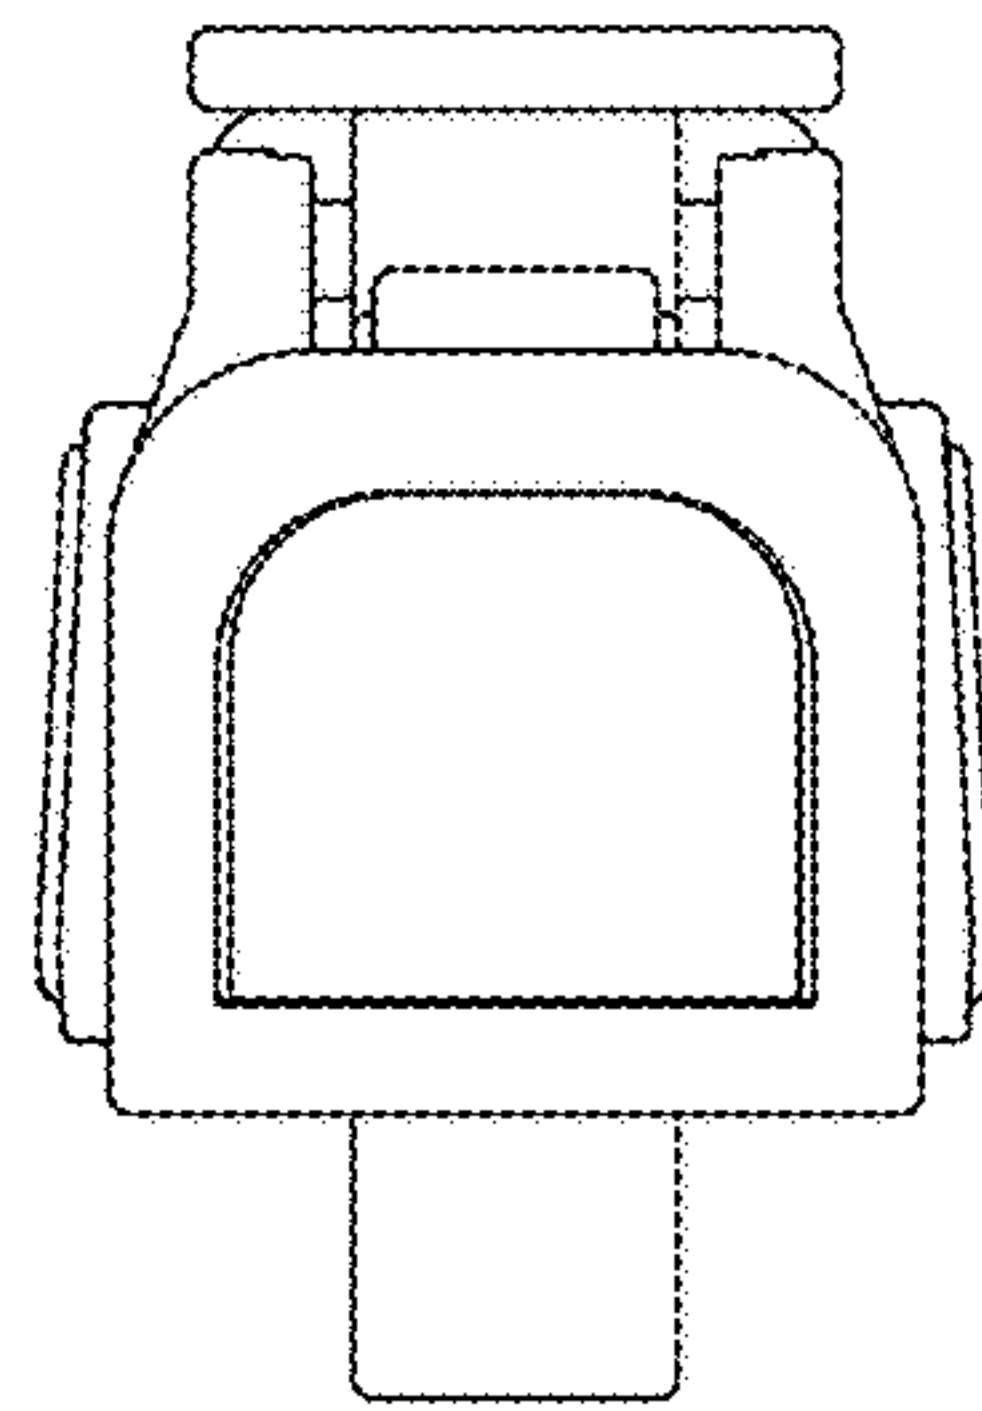


FIG. 4

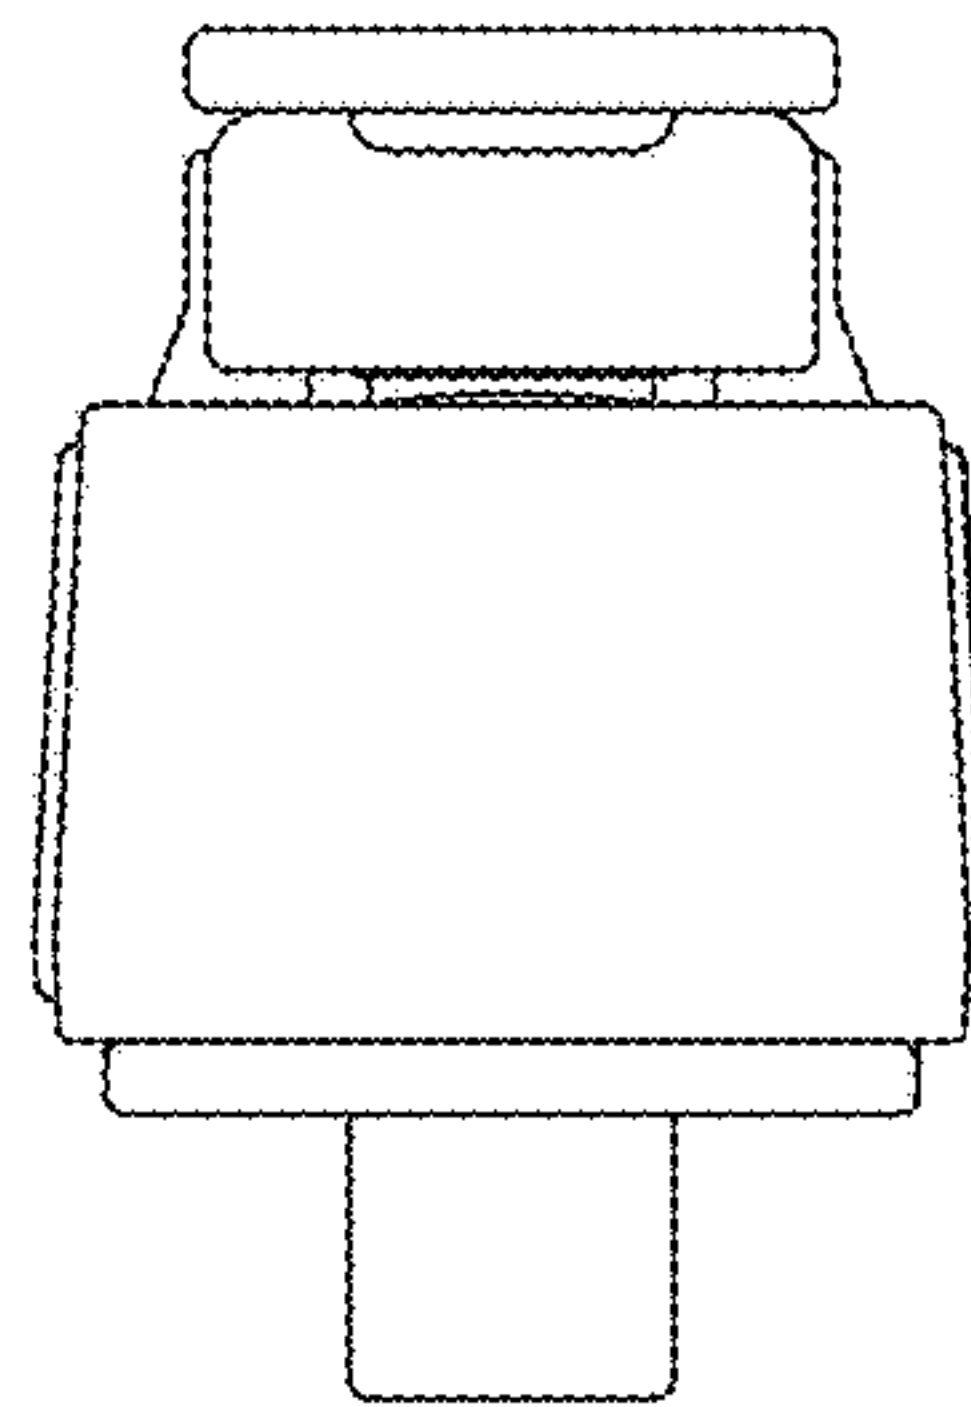


FIG. 5

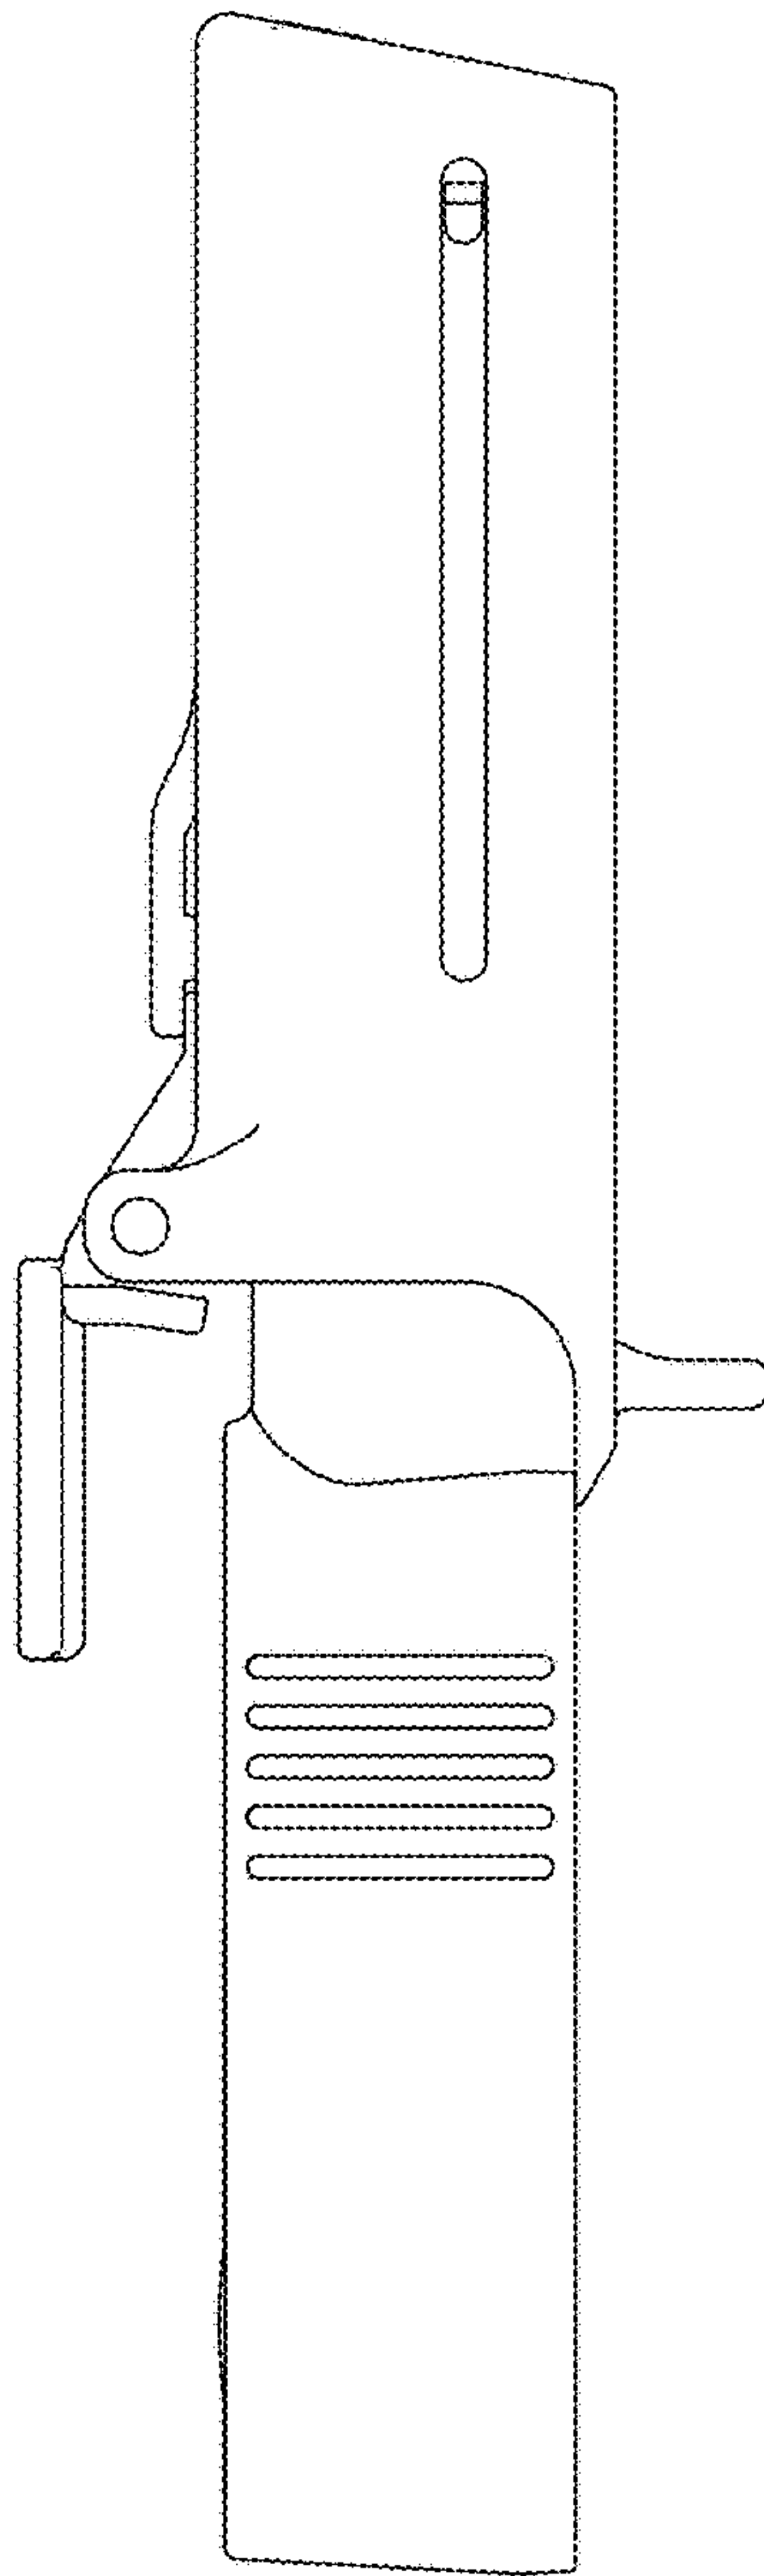


FIG. 6

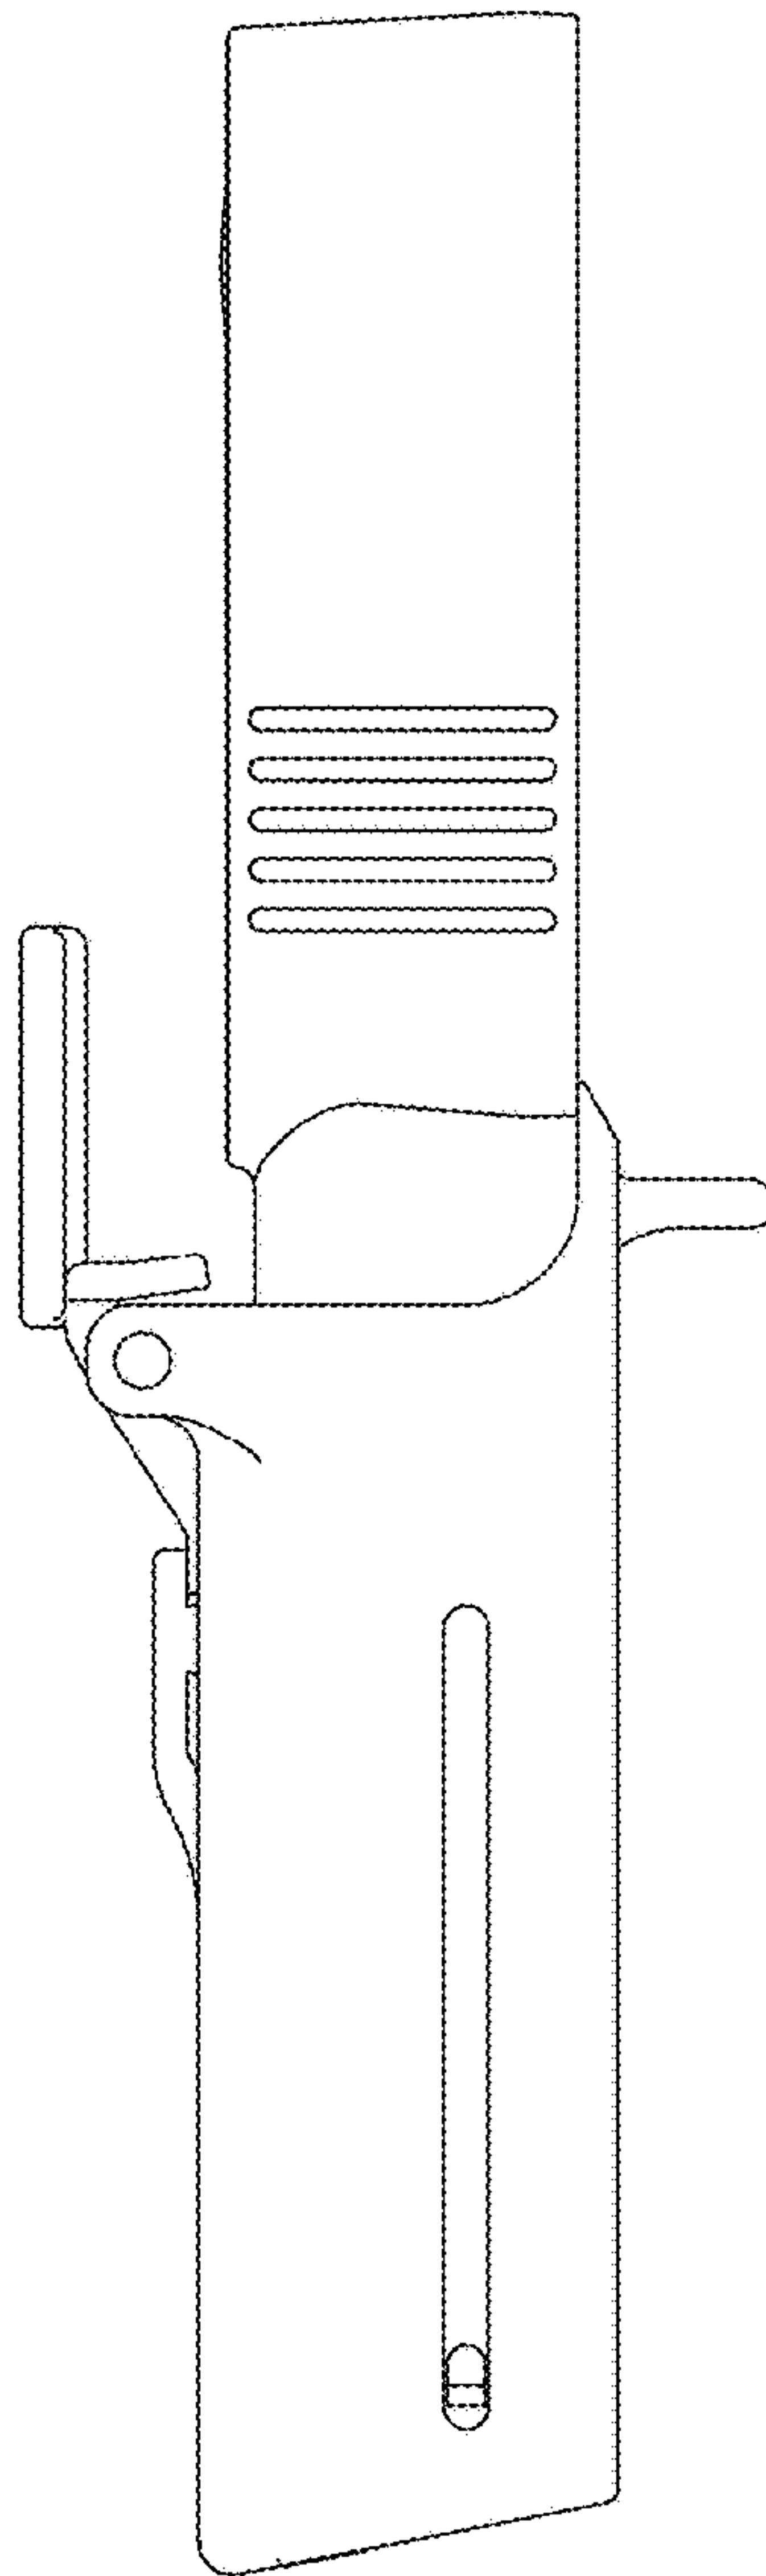


FIG. 7

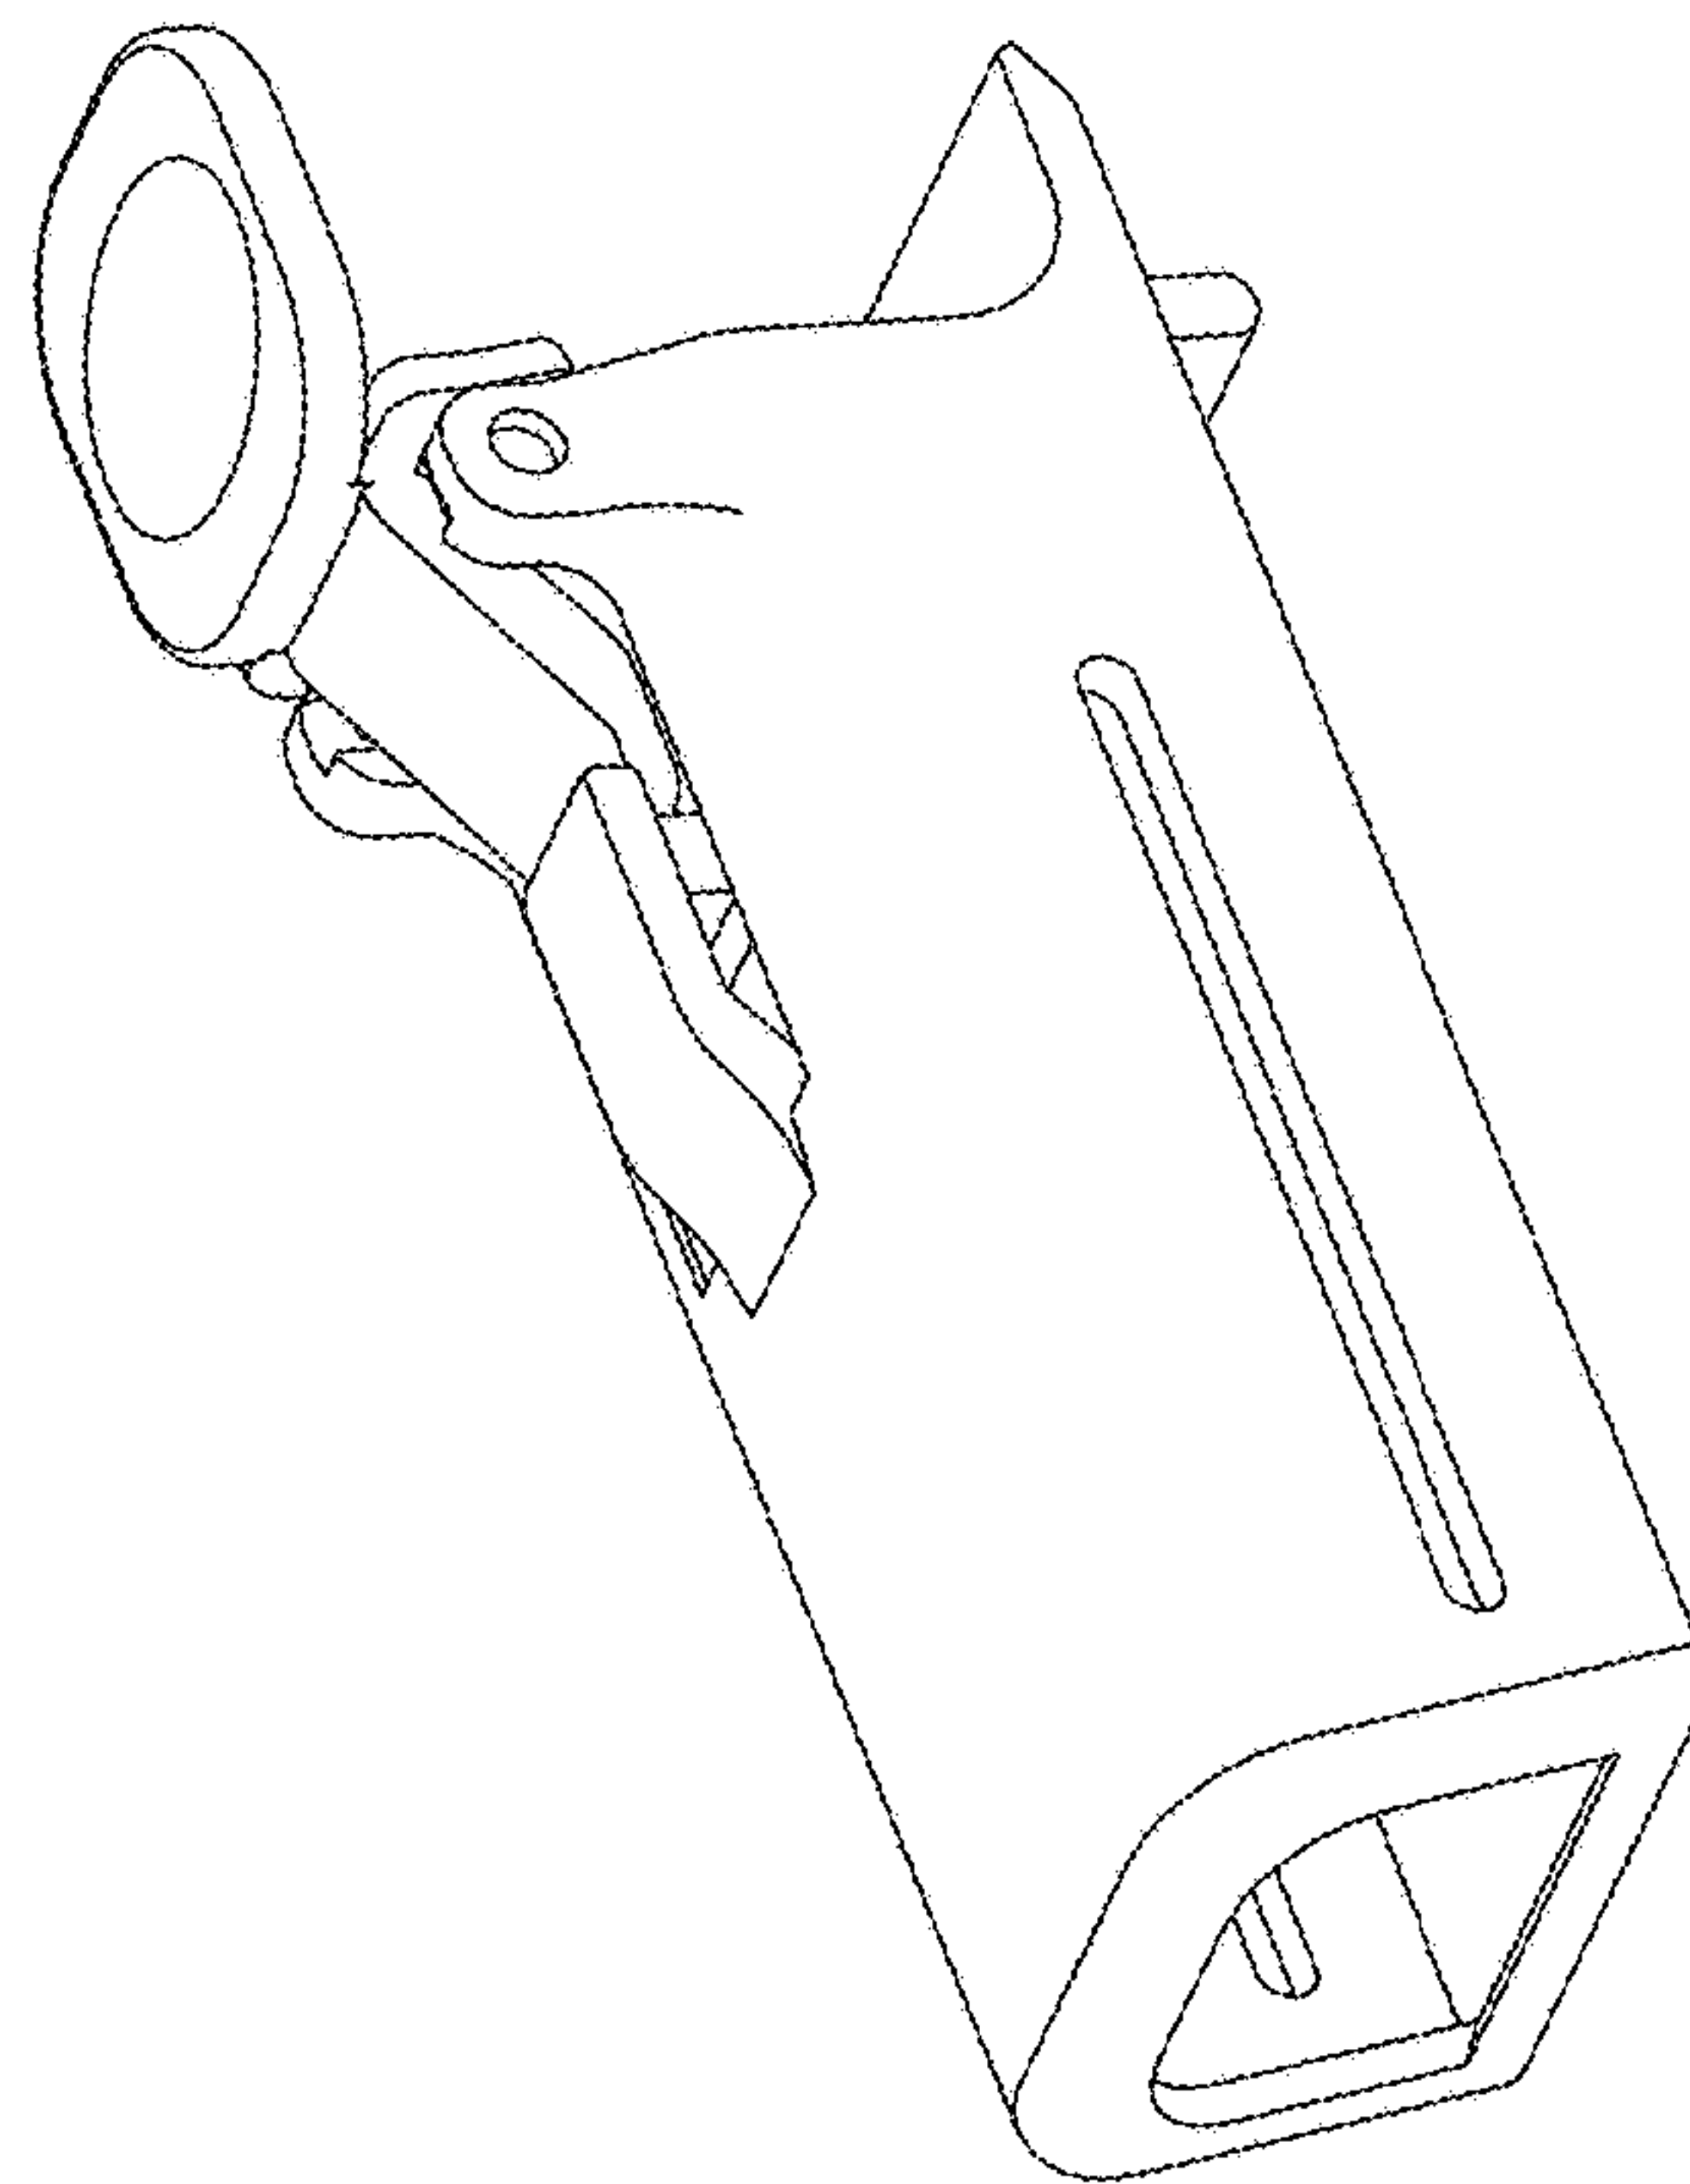


FIG. 8

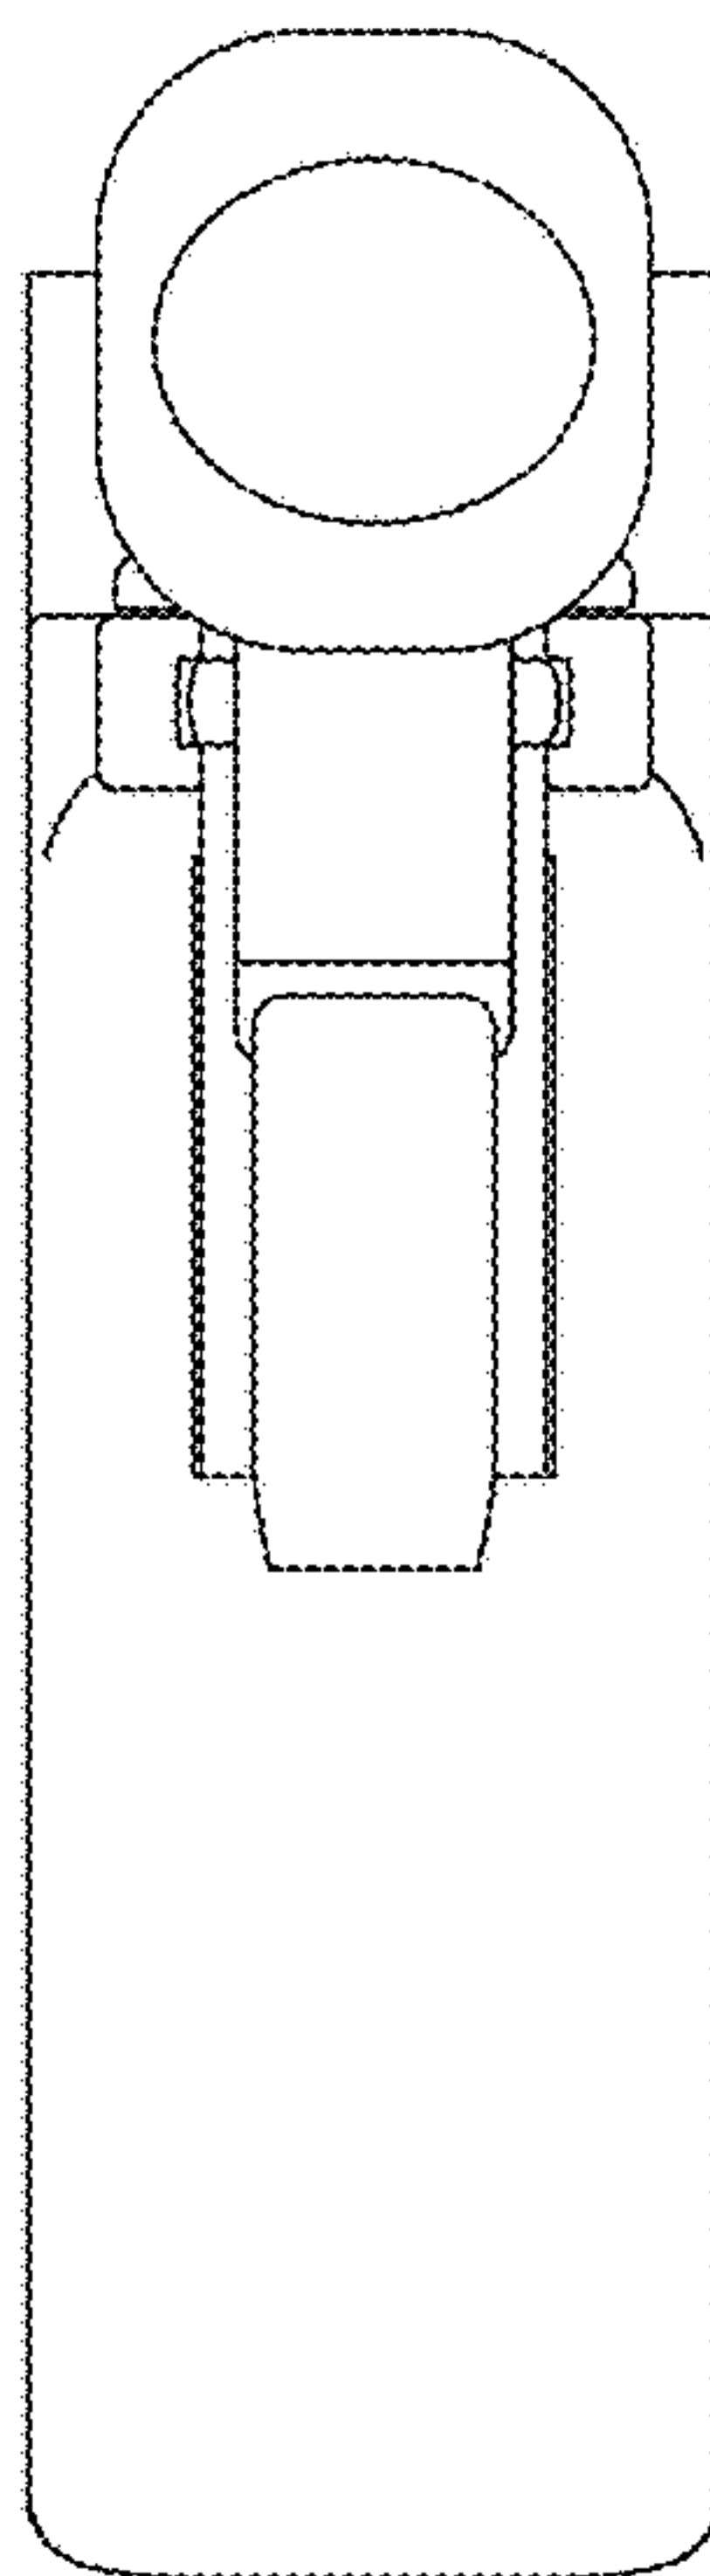


FIG. 9

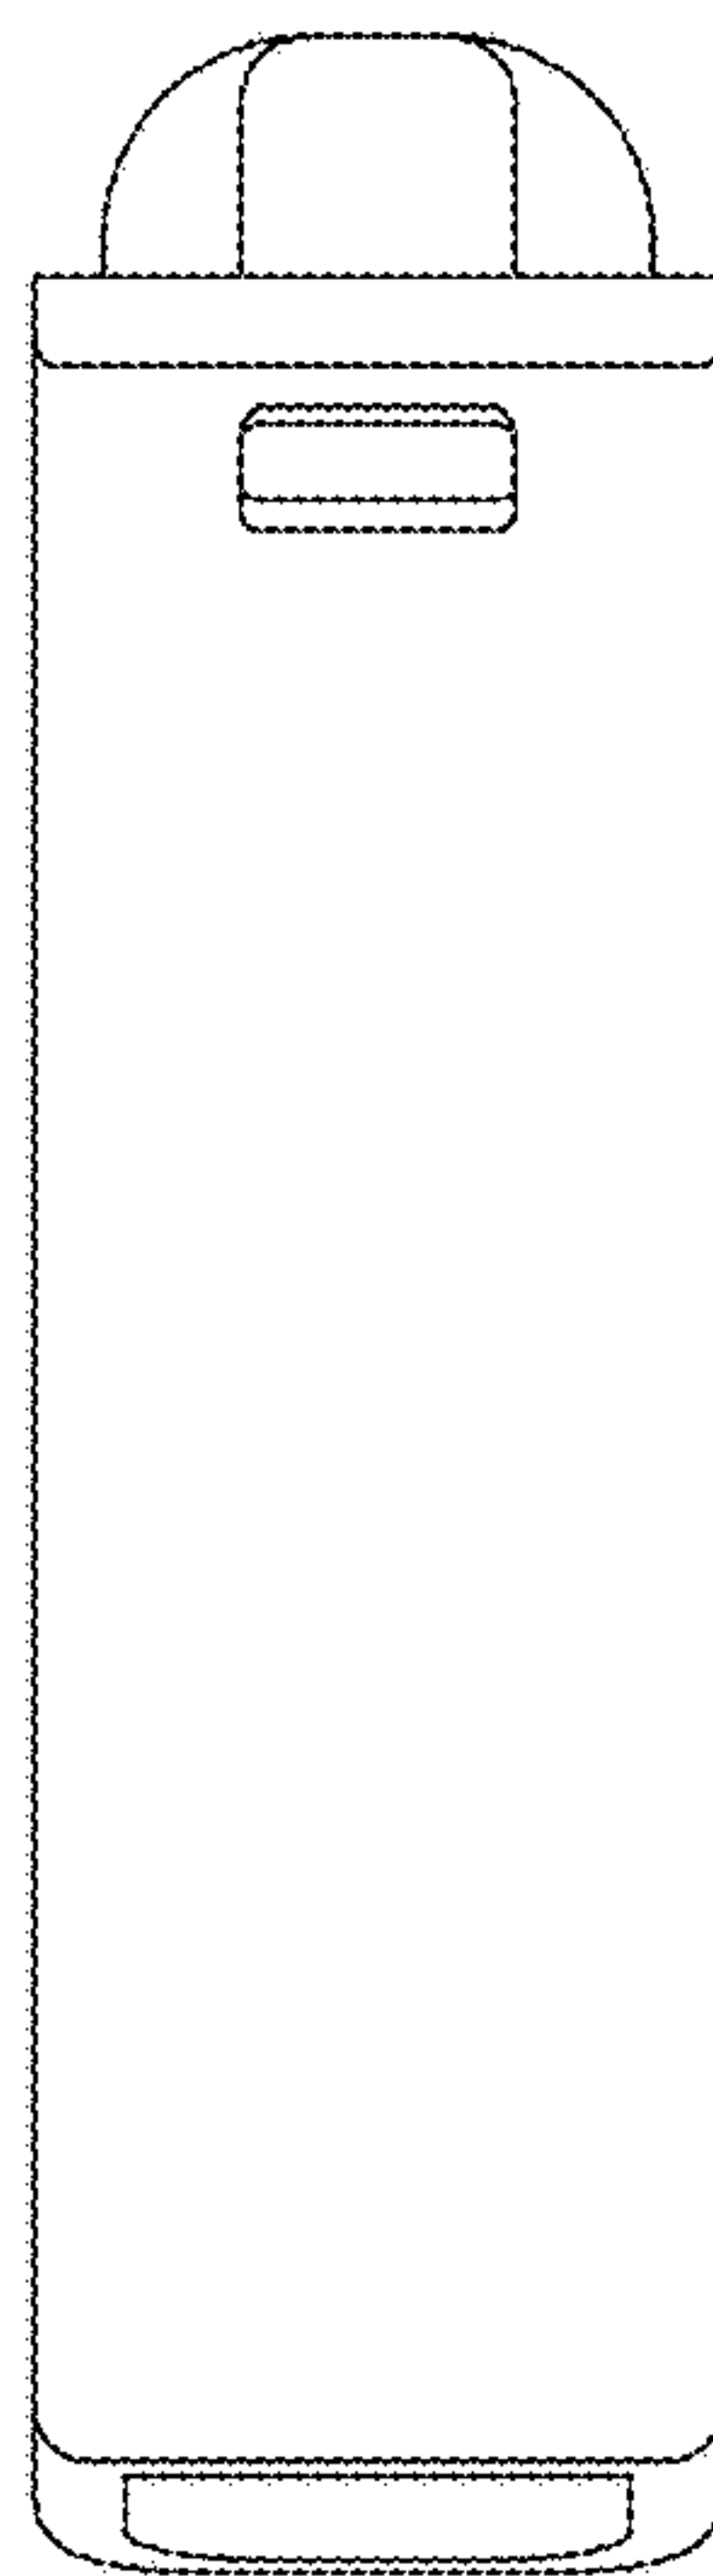


FIG. 10

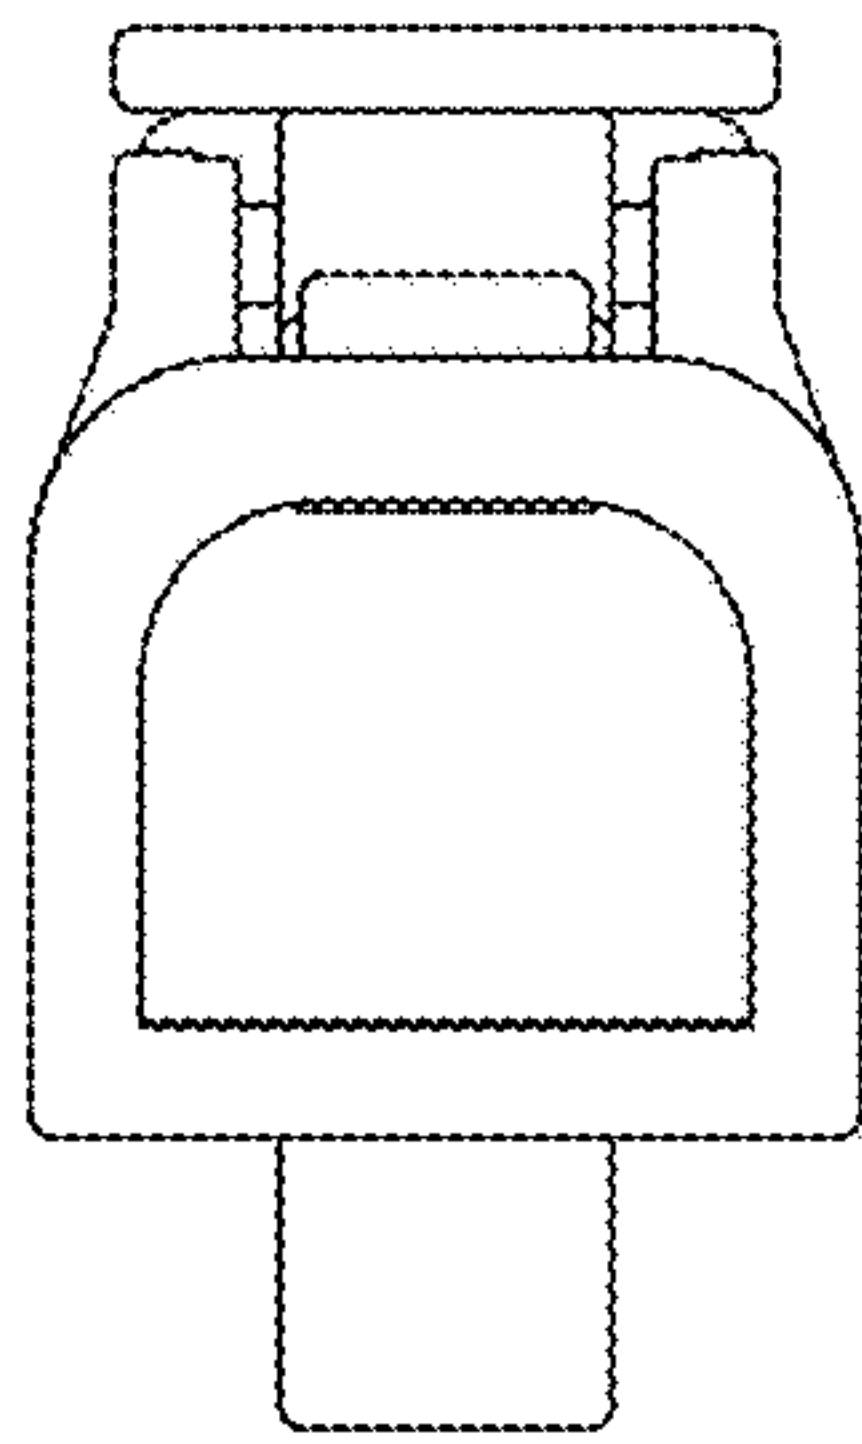


FIG. 11

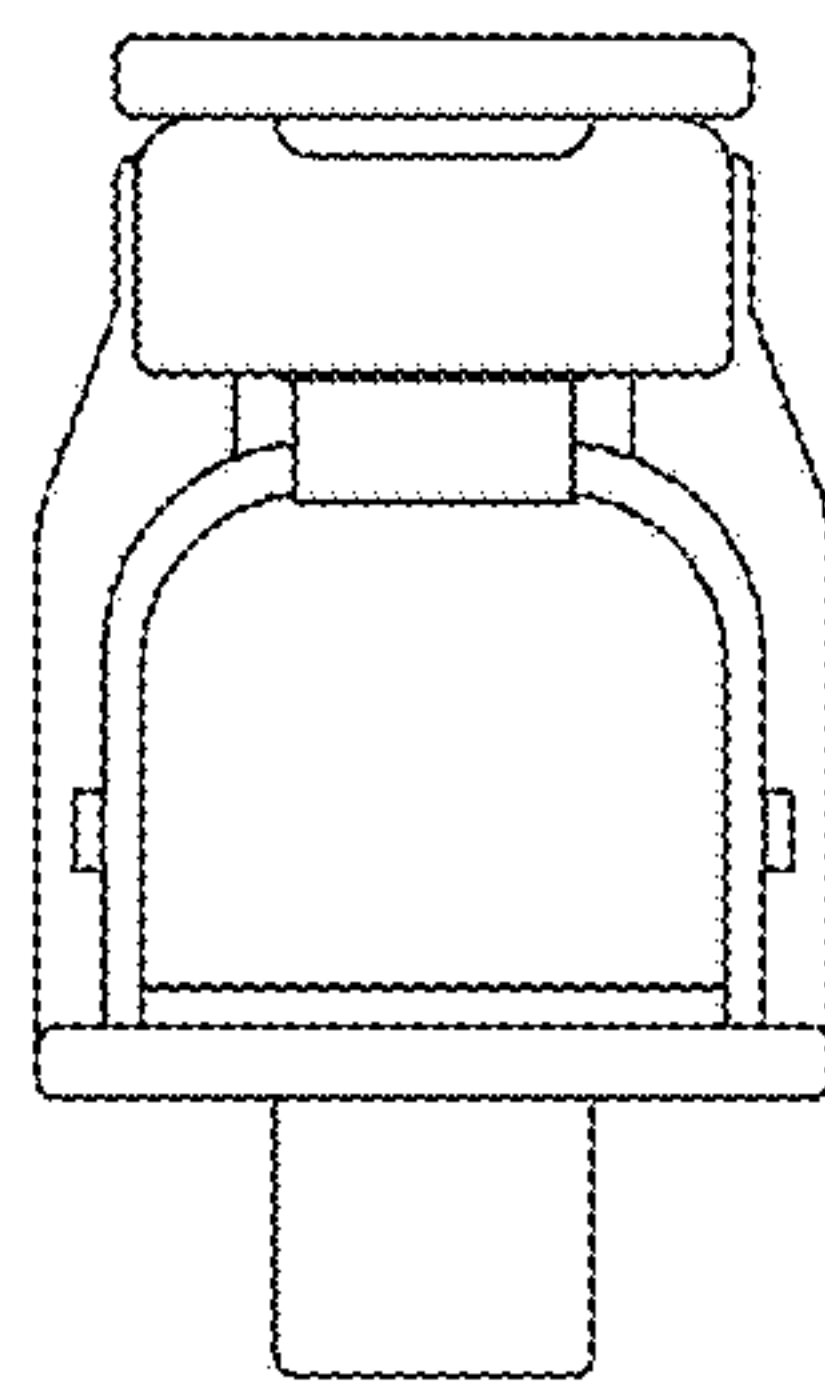


FIG. 12

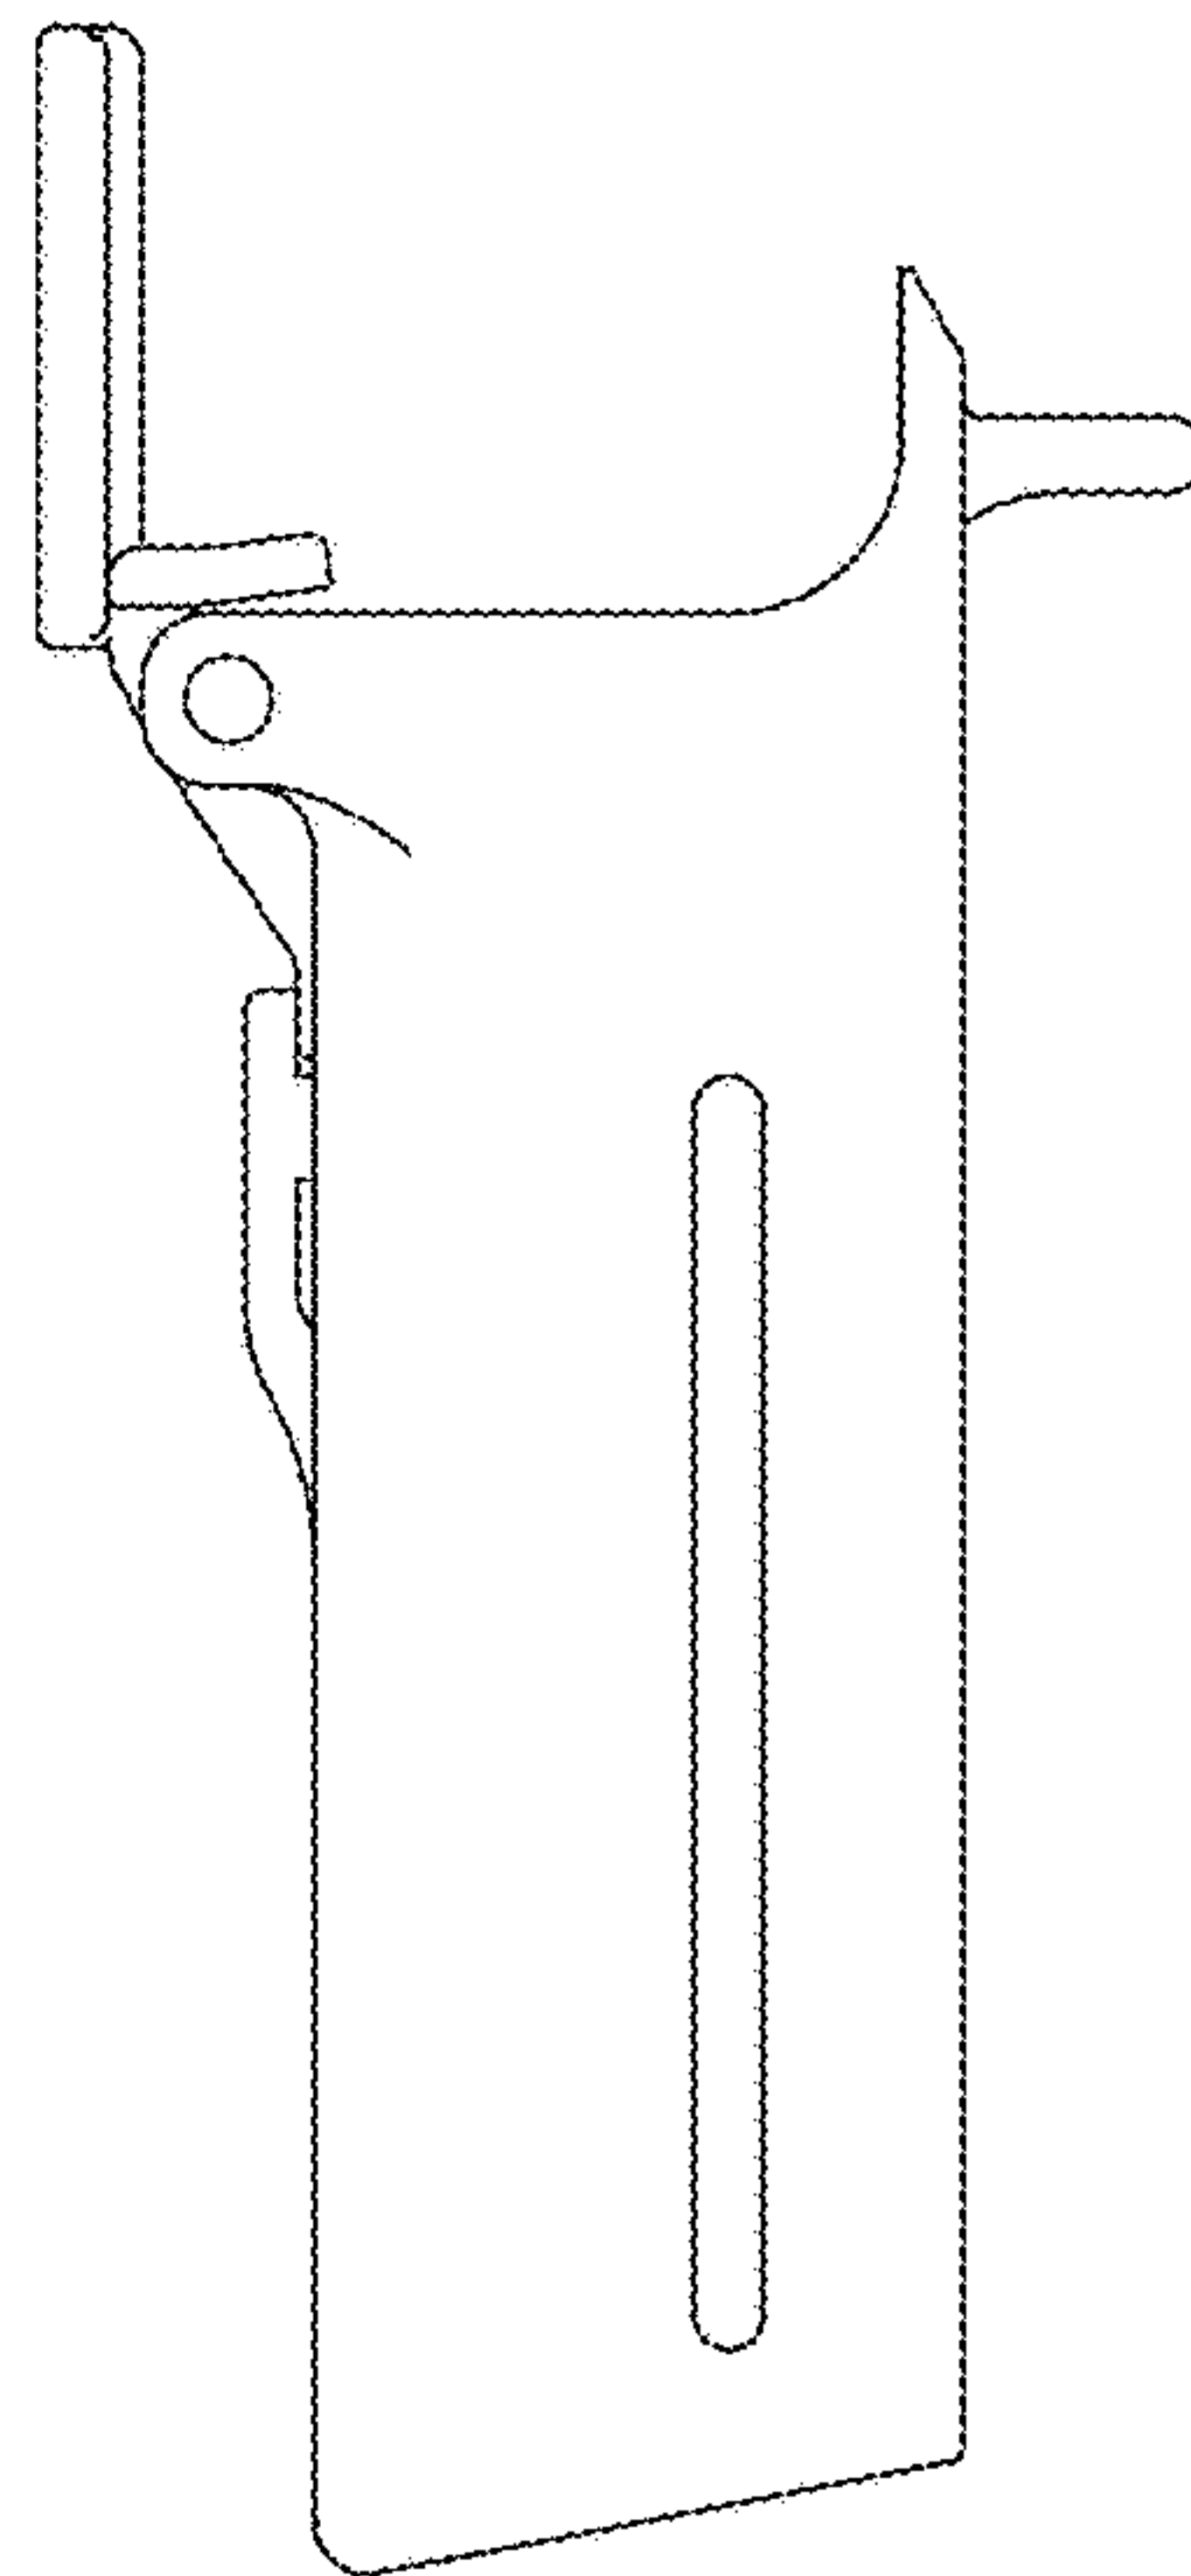


FIG. 13

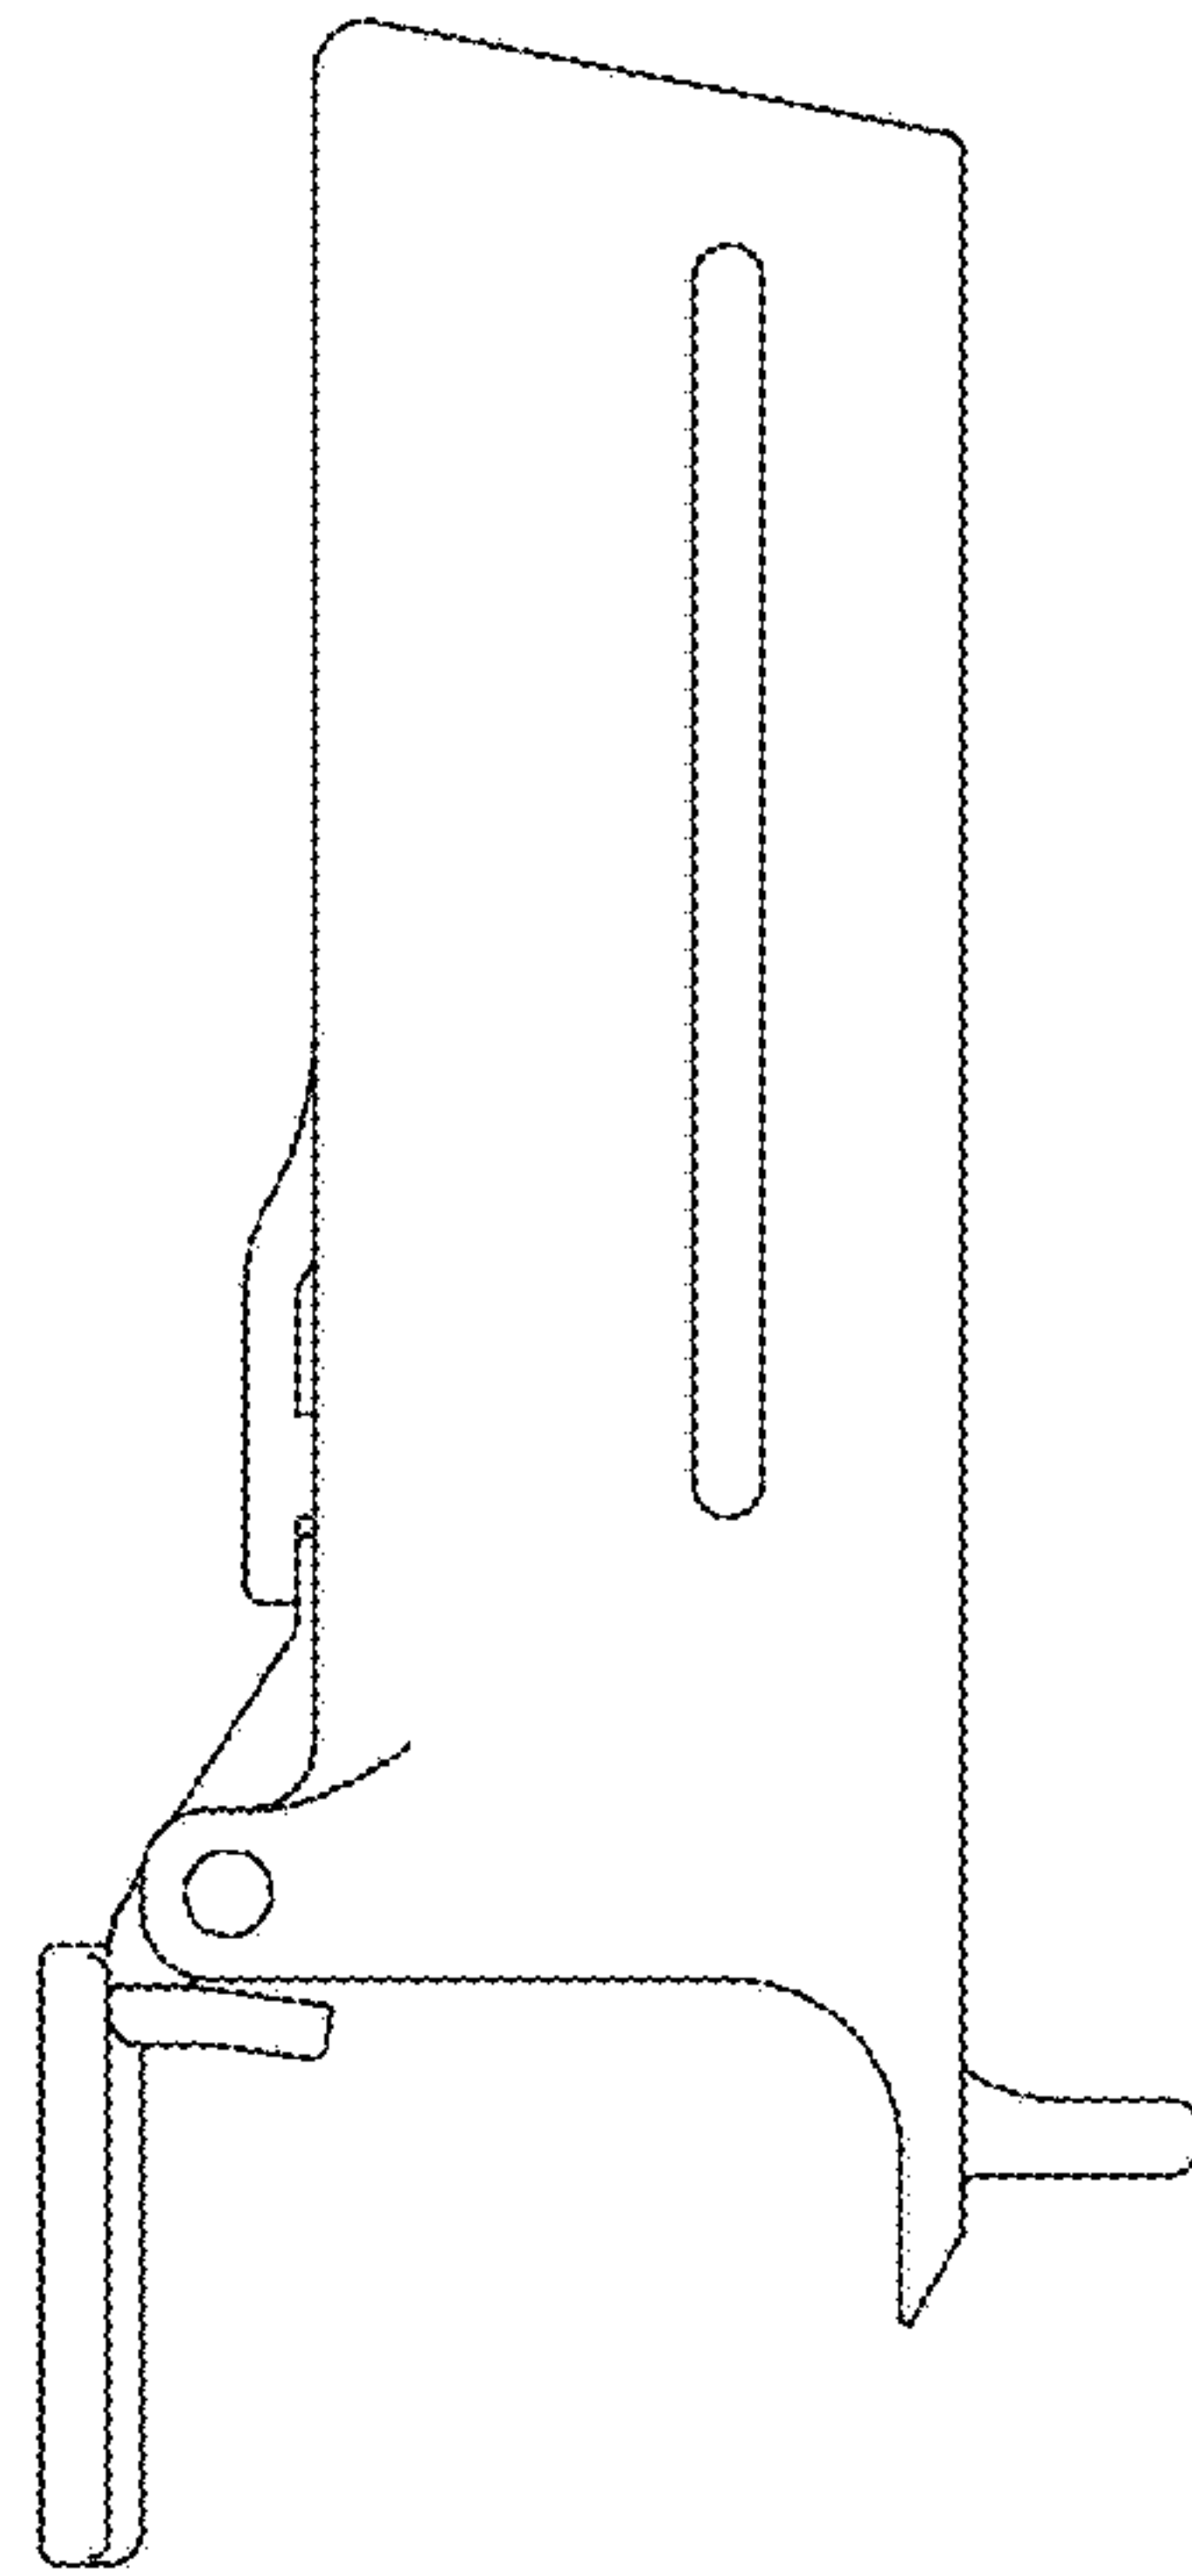


FIG. 14

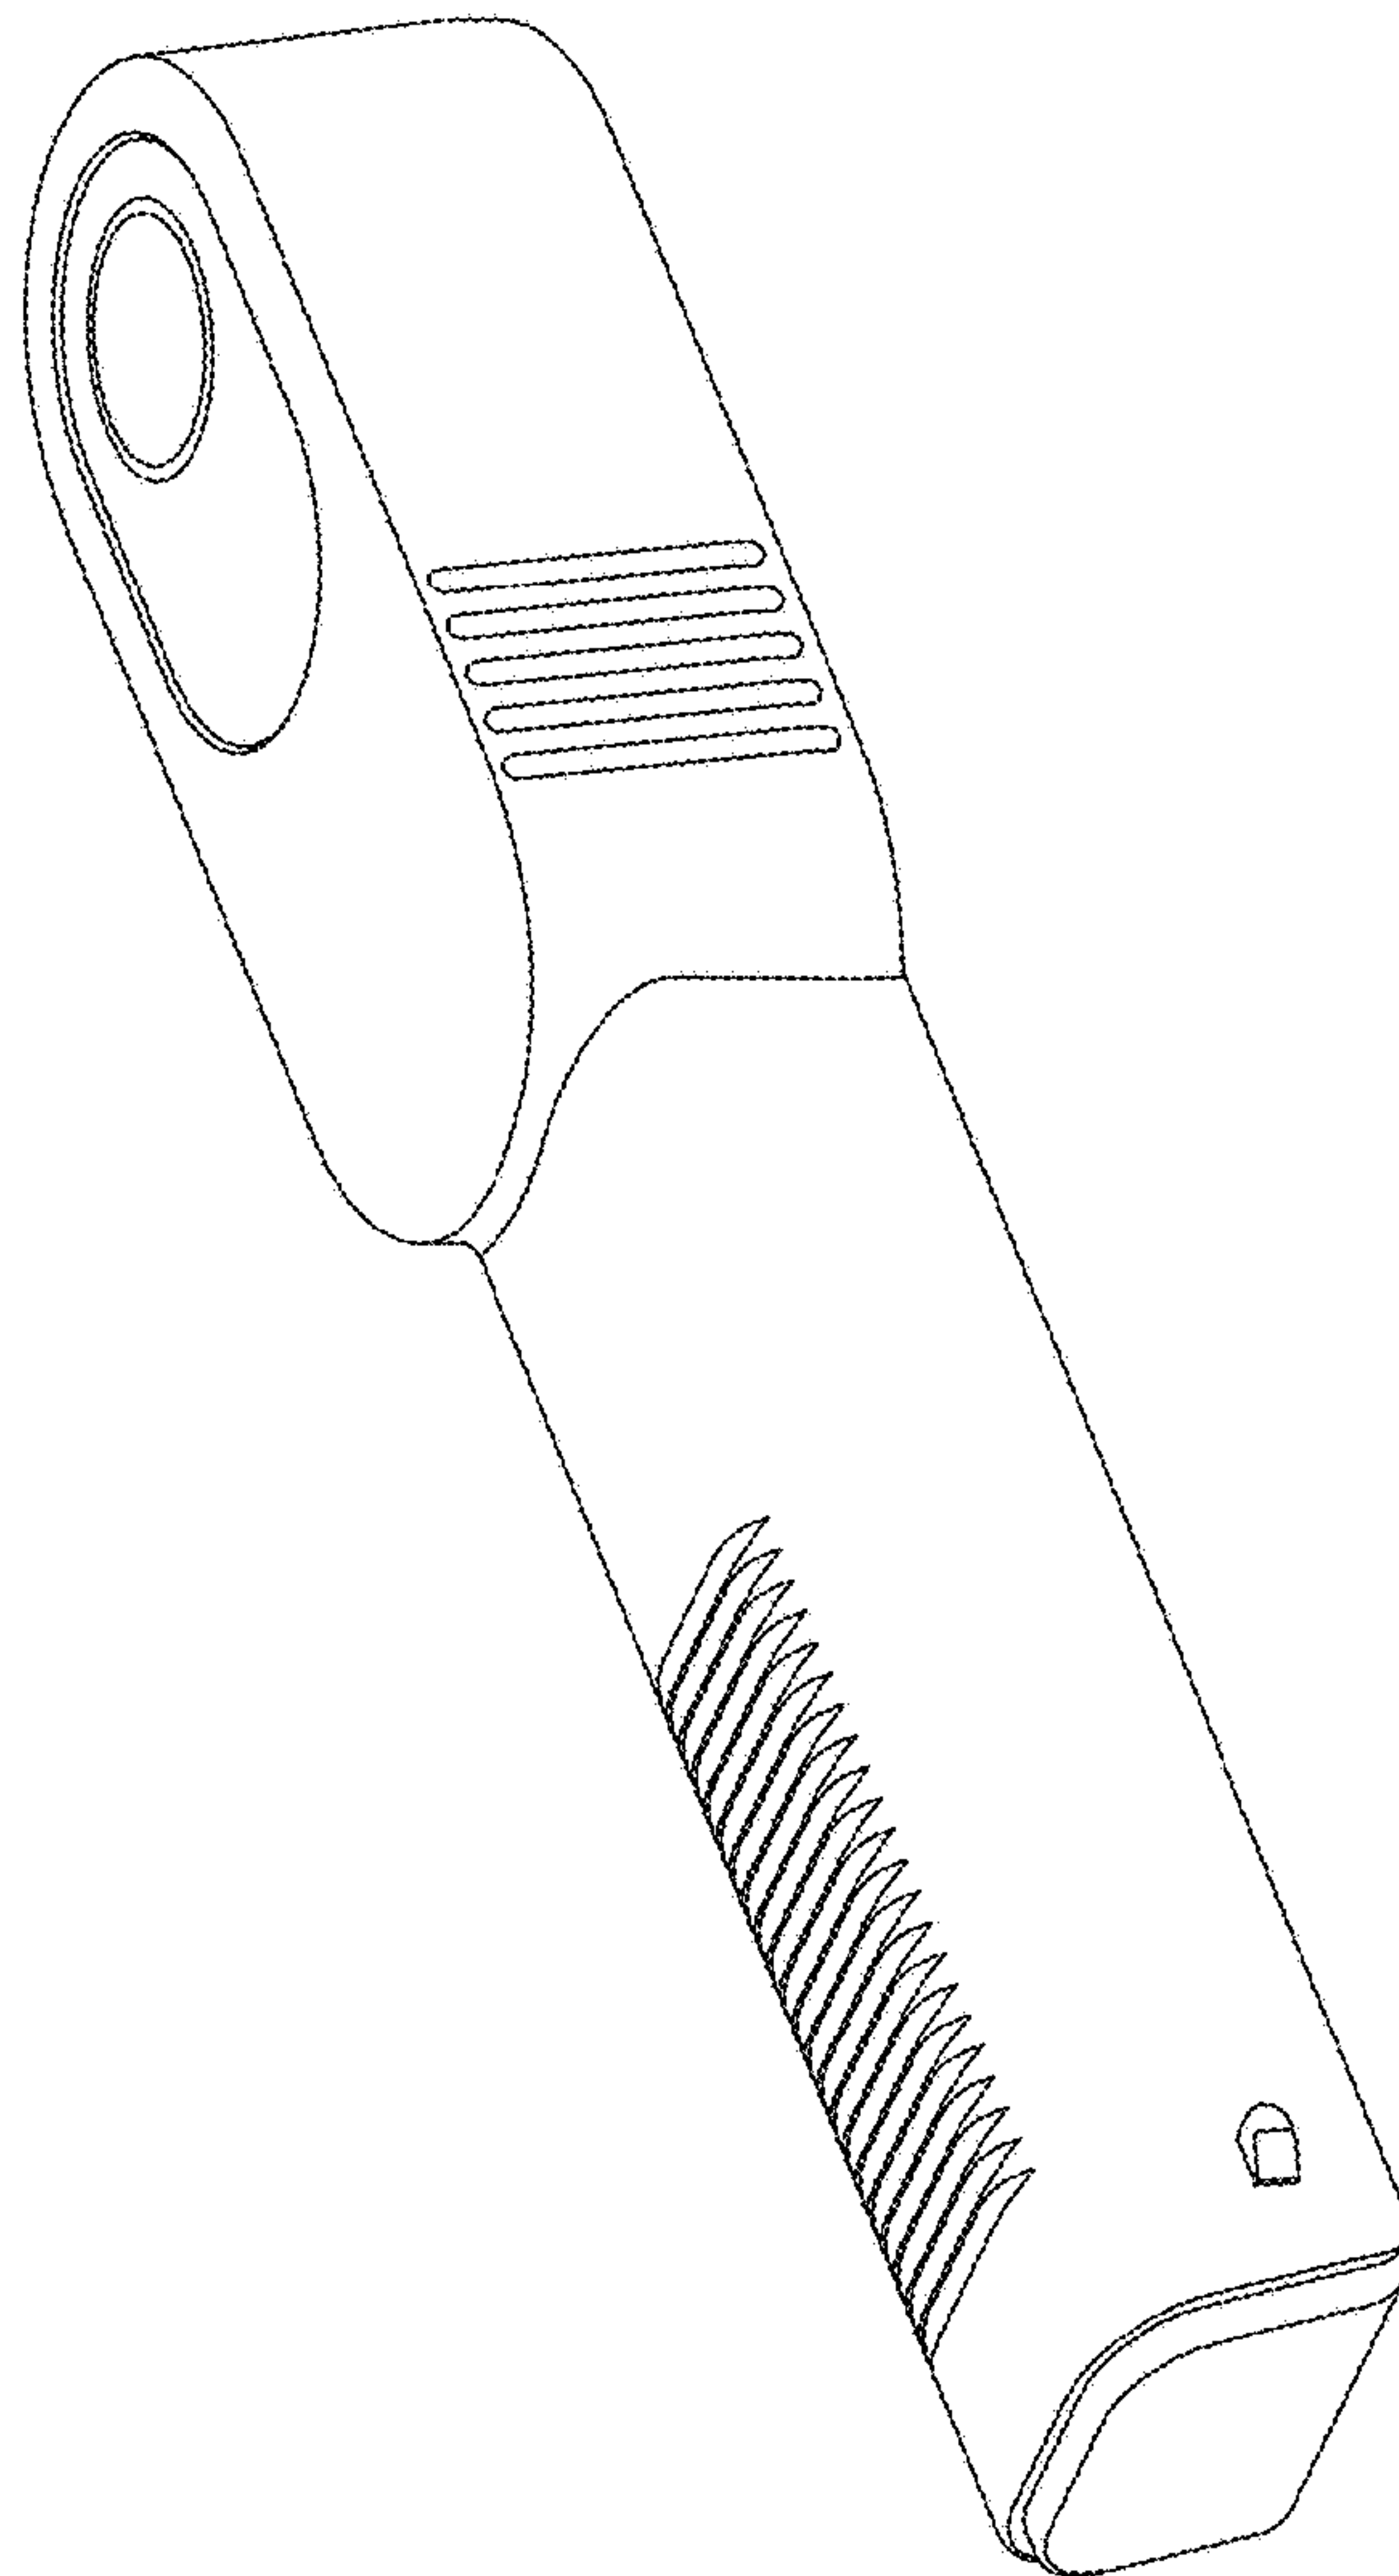


FIG. 15

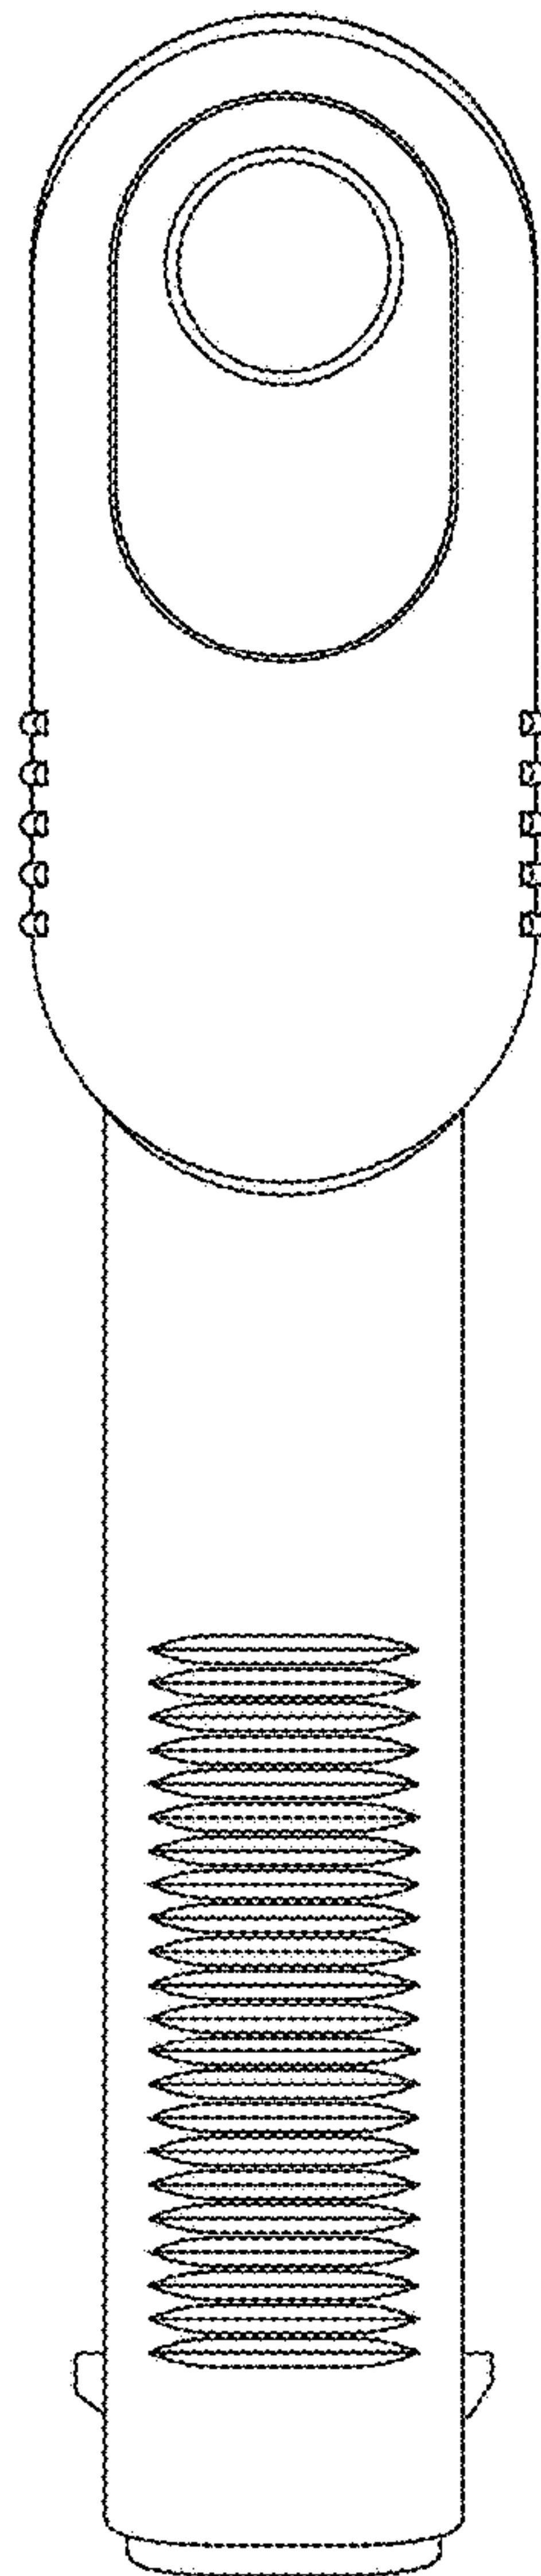


FIG. 16

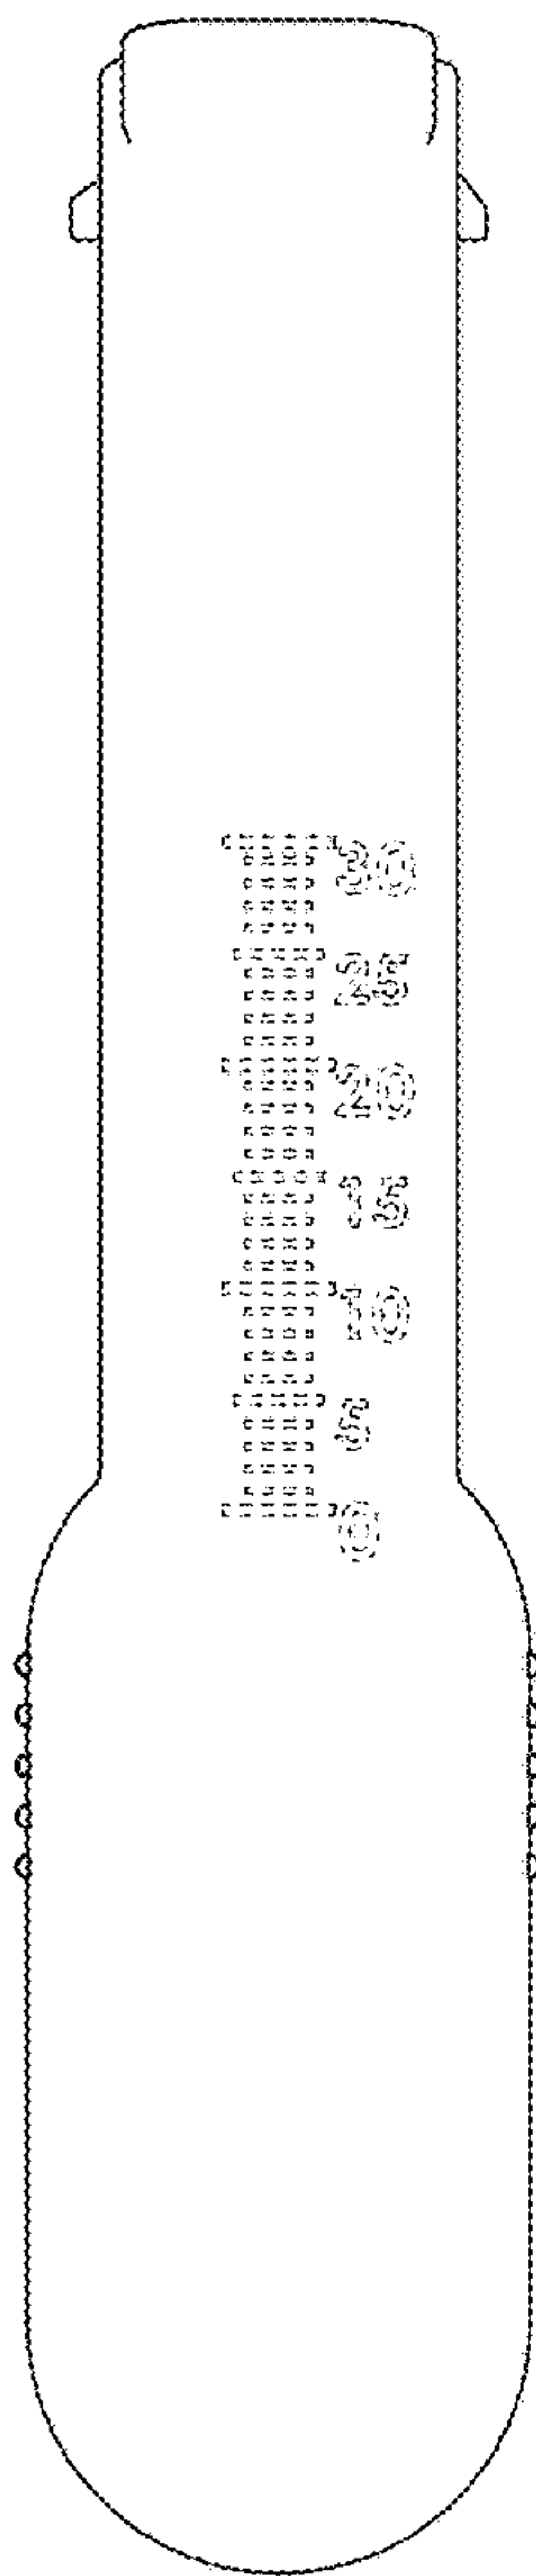


FIG. 17

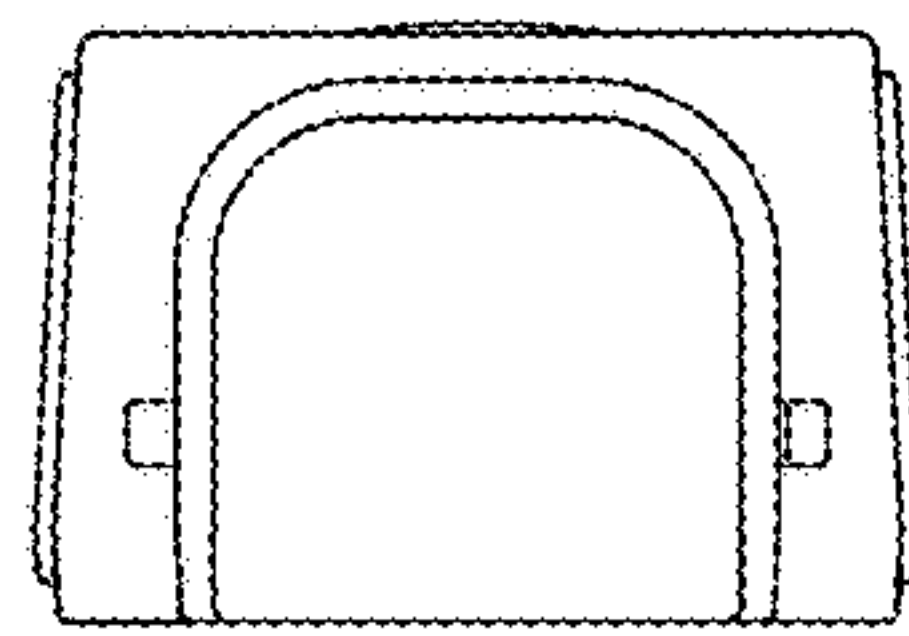


FIG. 18

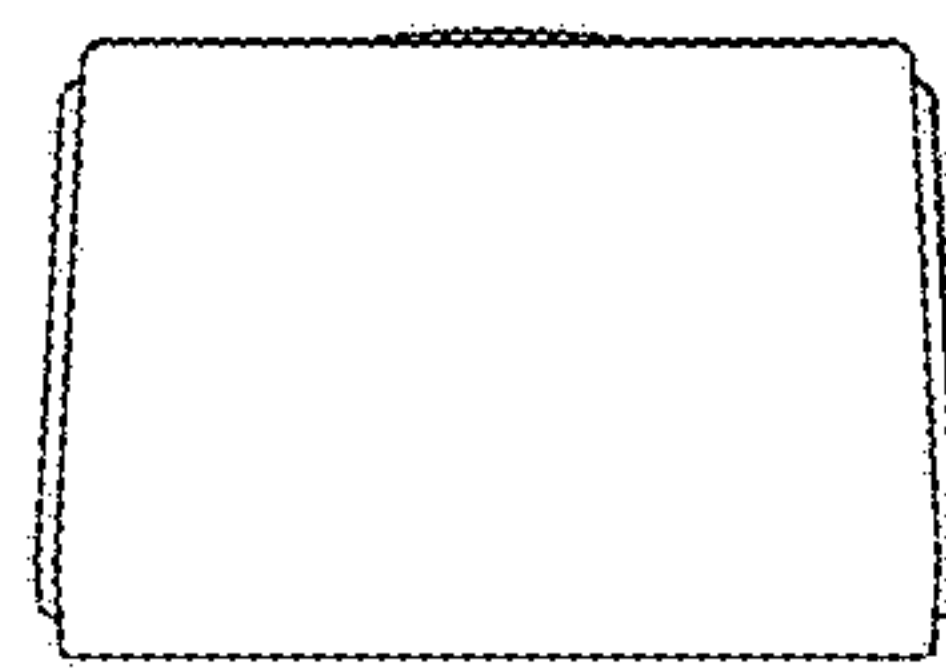


FIG. 19

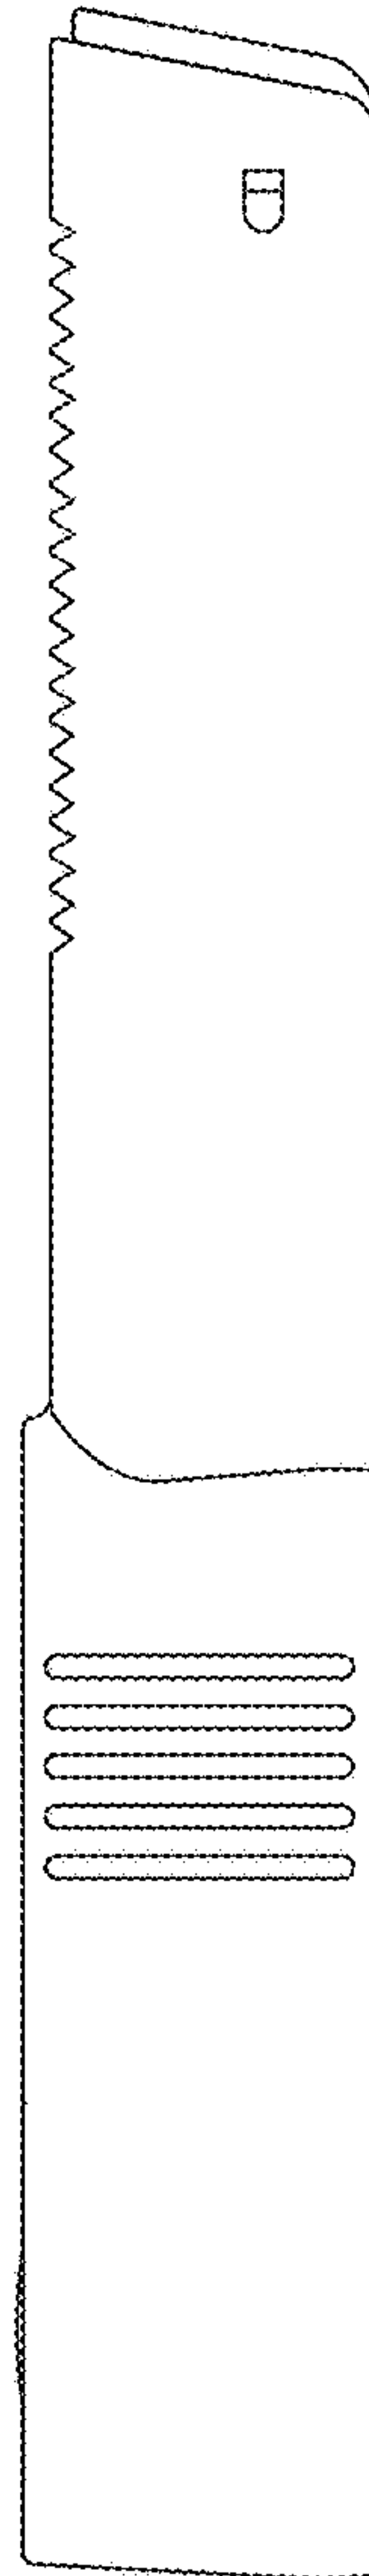


FIG. 20

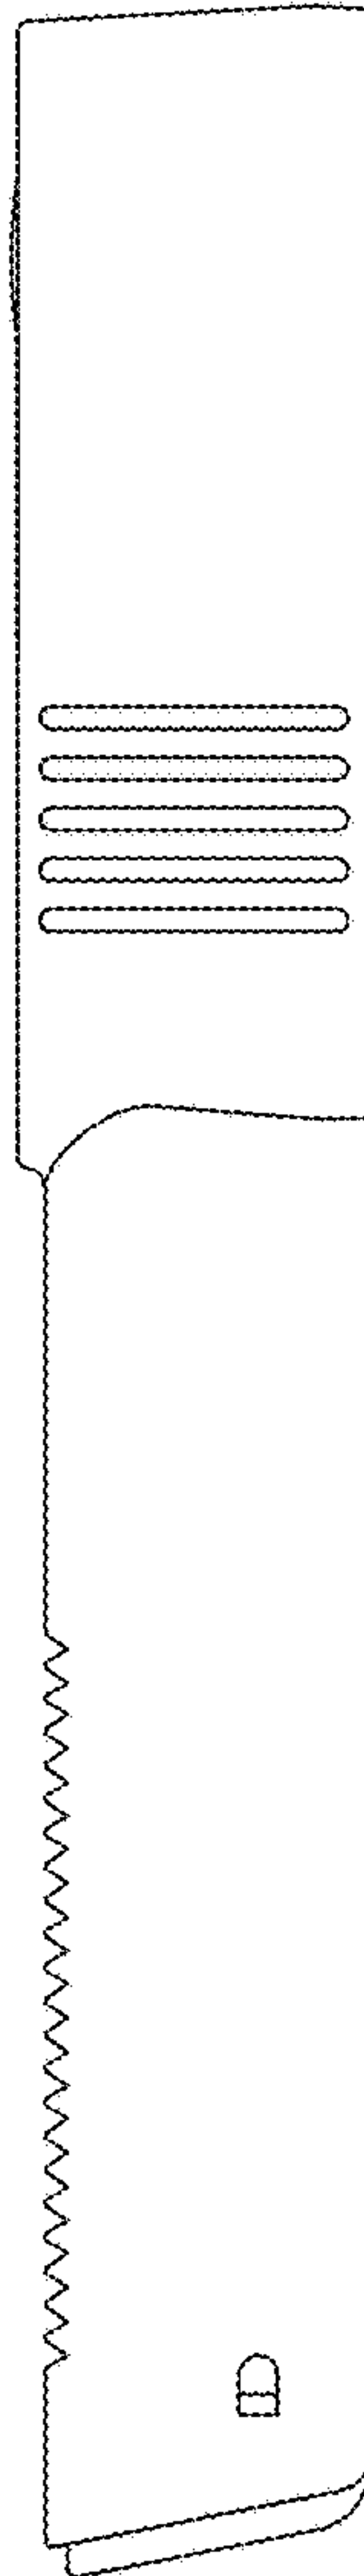


FIG. 21