



US00D858757S

(12) **United States Design Patent**  
**Joyce et al.**

(10) **Patent No.:** **US D858,757 S**  
(45) **Date of Patent:** **\*\* Sep. 3, 2019**

- (54) **SHARPS BIN**
- (71) Applicant: **HealthBeacon Limited**, Dublin (IE)
- (72) Inventors: **James Joyce**, Dublin (IE); **Kieran Daly**, Dublin (IE)
- (73) Assignee: **HEALTHBEACON LIMITED**, Dublin (IE)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/595,655**
- (22) Filed: **Mar. 1, 2017**
- (51) **LOC (12) Cl.** ..... **24-01**
- (52) **U.S. Cl.**  
USPC ..... **D24/131**
- (58) **Field of Classification Search**  
USPC ..... D24/103, 131, 231; D34/7, 8, 10, 11  
CPC ..... A61B 50/30; A61B 50/362; A61B 50/364;  
A61B 2050/005; A61B 2050/0051; A61B  
2050/0059  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D287,756 S *	1/1987	Szablak	.....	D24/131
D302,291 S *	7/1989	Heubel	.....	D24/131
D436,170 S *	1/2001	Gaba	.....	D24/131
D451,195 S *	11/2001	Daniels	.....	D24/131
D485,906 S *	1/2004	Danssaert	.....	D24/131
D538,500 S *	3/2007	Lin	.....	D34/7
D699,842 S *	2/2014	Bang	.....	D24/131
D733,320 S *	6/2015	Perry	.....	D24/231

D807,504 S *	1/2018	Pena	.....	D24/131
D809,729 S *	2/2018	Chen	.....	D34/7
2017/0273753 A1 *	9/2017	Bischoff	.....	A61B 50/30
2018/0078326 A1 *	3/2018	Sall	.....	A61B 50/362

**OTHER PUBLICATIONS**

HealthBeacon raises \$1.1M for medication adherence-tracking needle disposal container, posted at mobihealthnews.com, posted on Feb. 9, 2016 available online, URL:<http://www.mobihealthnews.com/content/healthbeacon-raises-11m-medication-adherence-tracking-needle-disposal-container> (Year: 2016).\*

\* cited by examiner

*Primary Examiner* — Anhdao Doan

*Assistant Examiner* — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Adler Pollock & Sheehan P.C.

(57) **CLAIM**



The ornamental design for a sharps bin, as shown and described.

**DESCRIPTION**

FIG. 1 is a front view of the present design for a sharps bin; FIG. 2 is a back view; FIG. 3 is a left side view; FIG. 4 is a right side view; FIG. 5 is a bottom view; and, FIG. 6 is a top view thereof.

The broken lines show portions of the sharps bin that form no part of the claimed design.

**1 Claim, 4 Drawing Sheets**

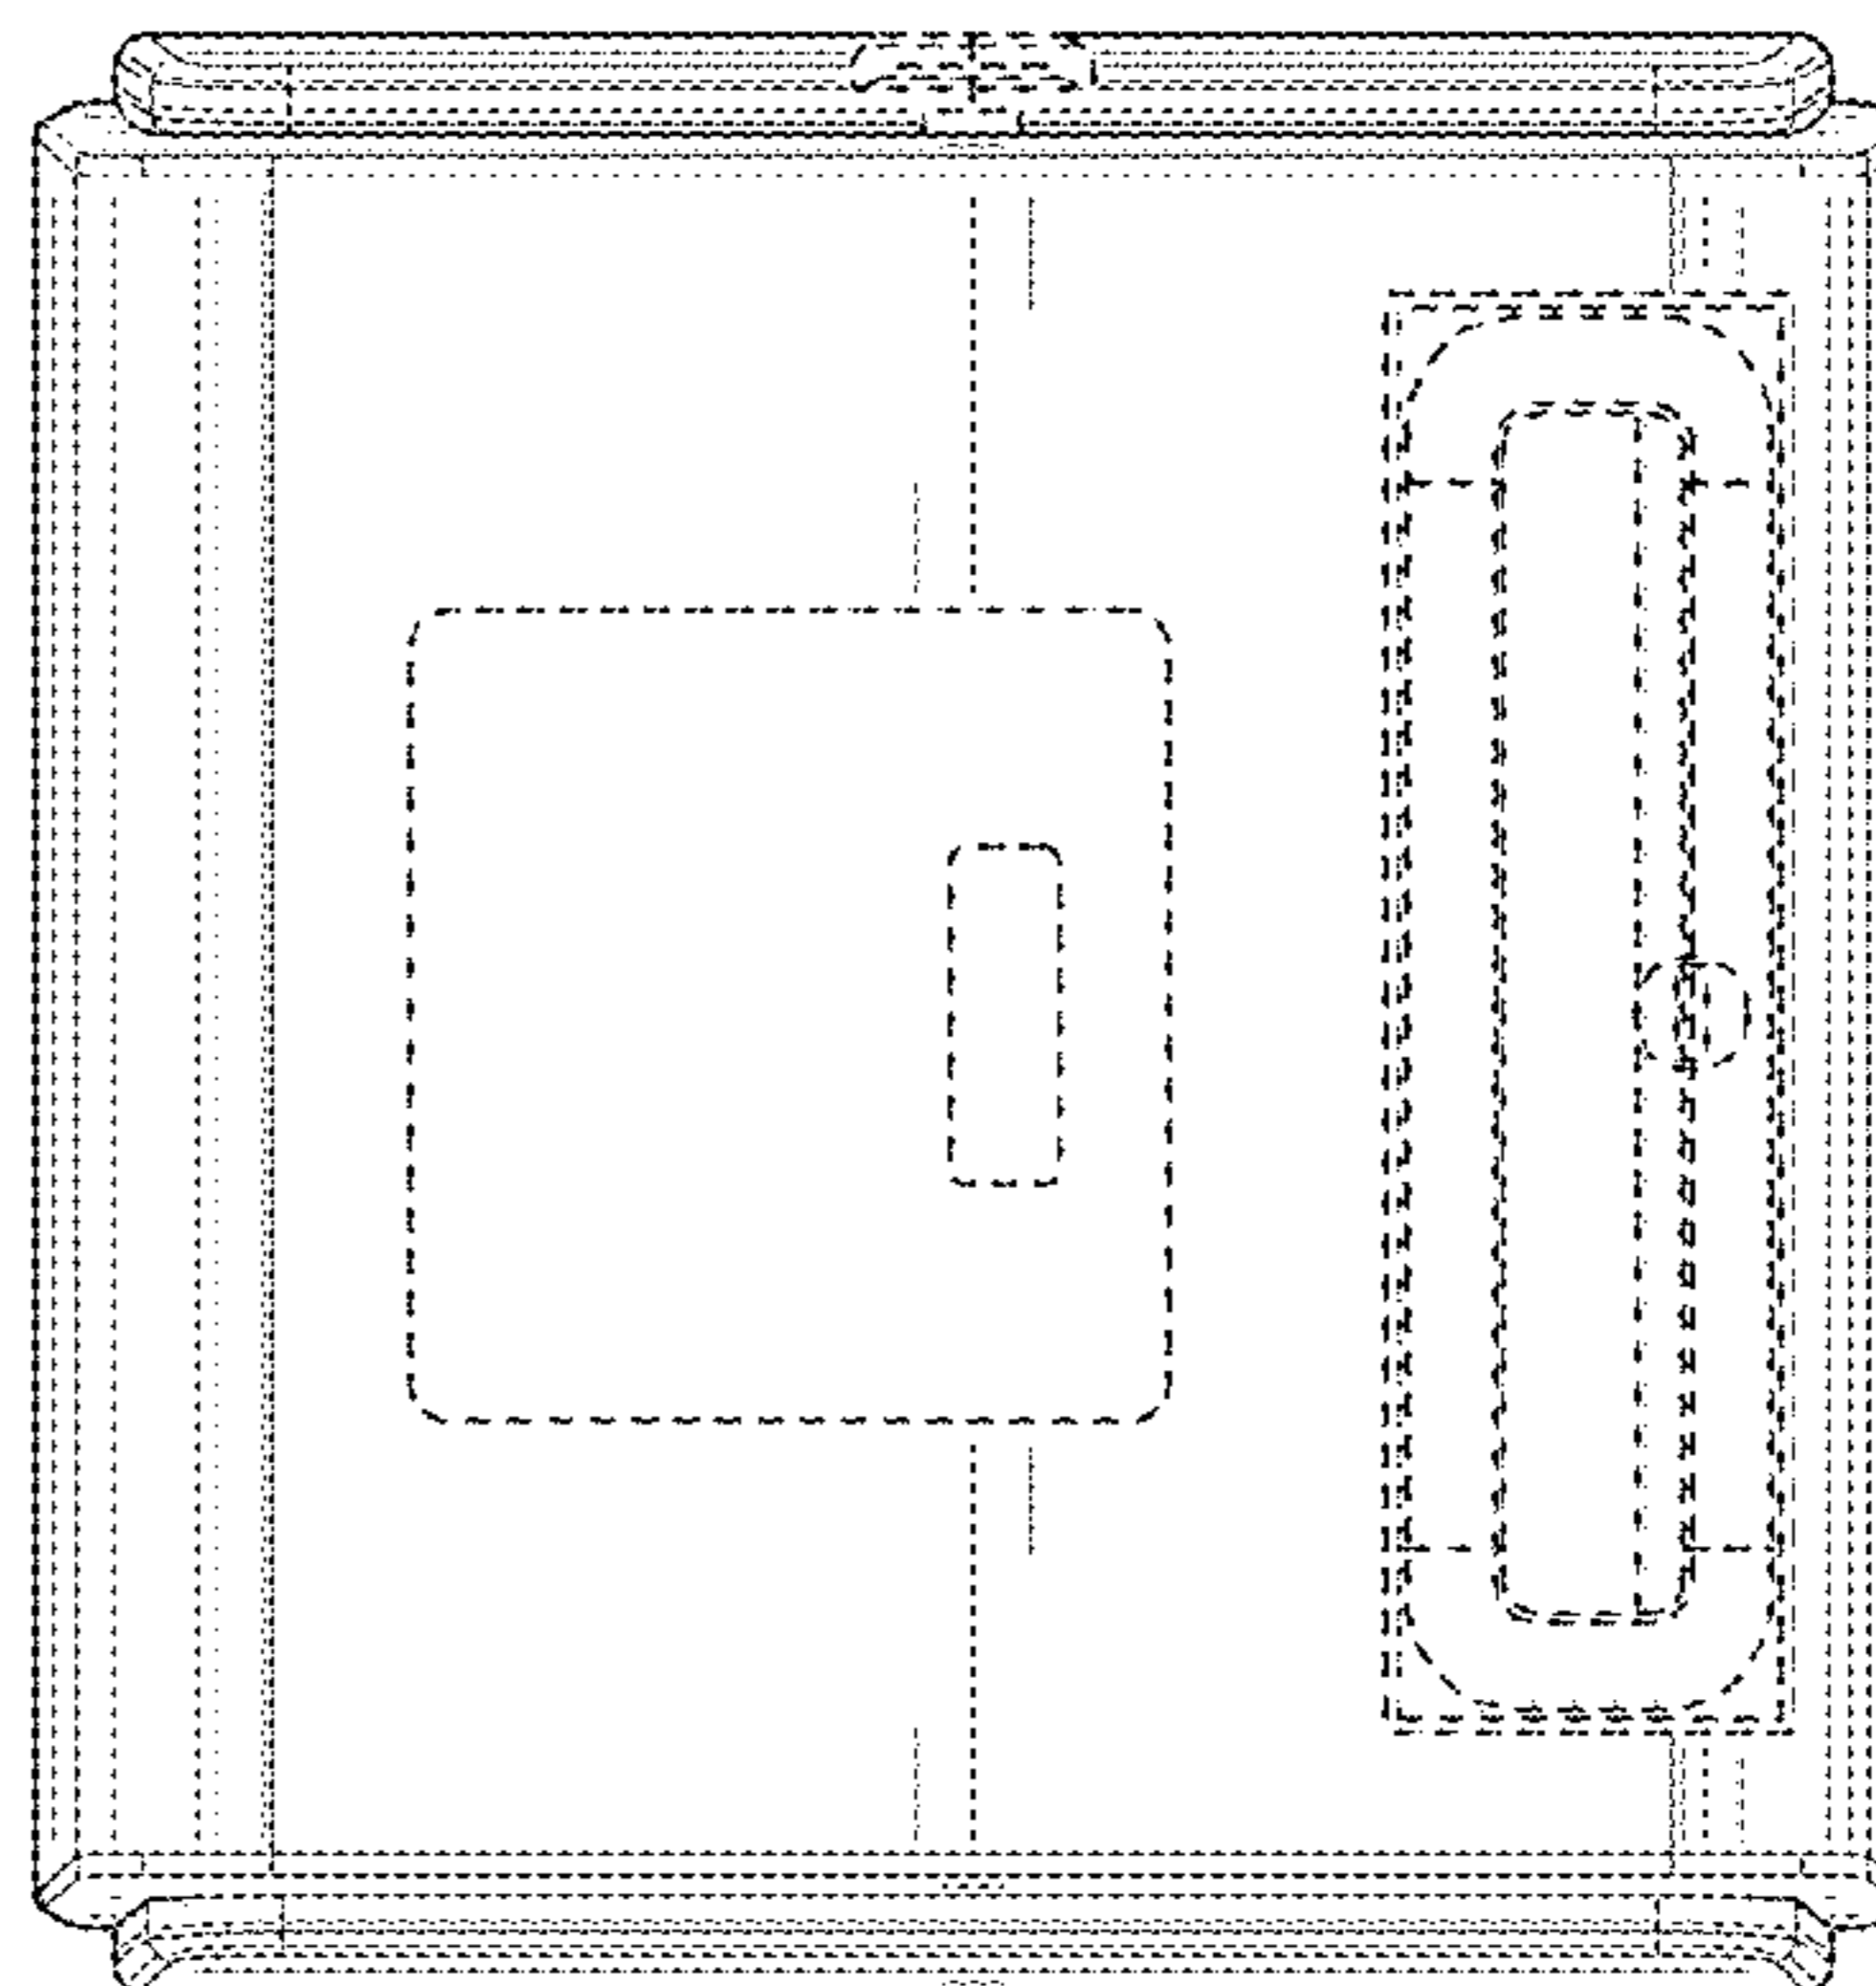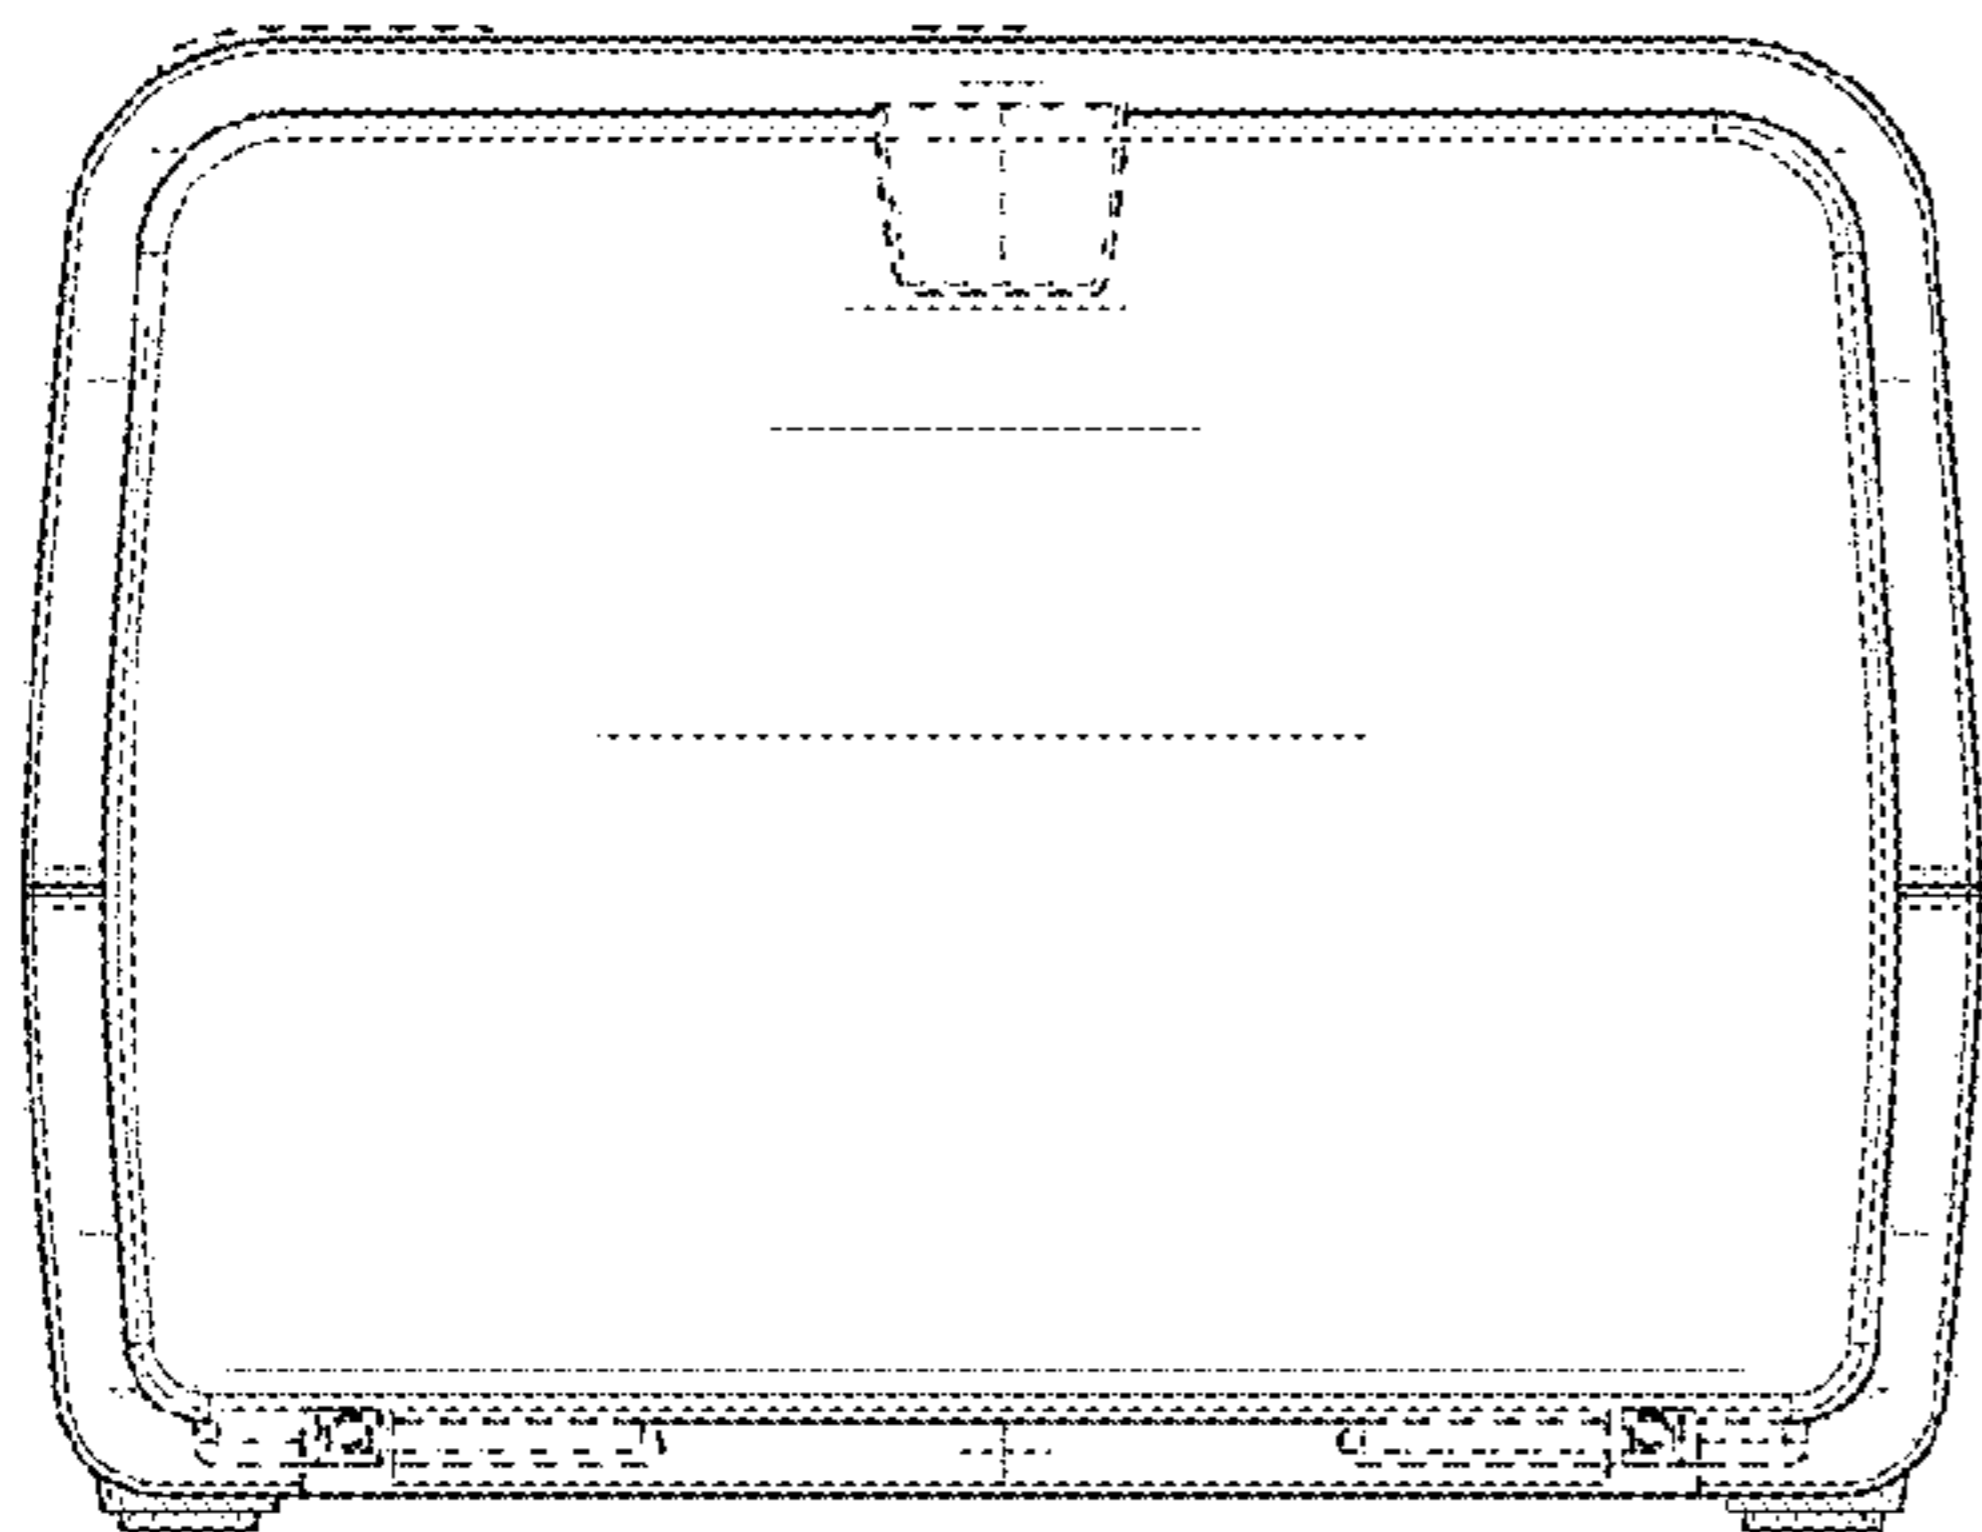

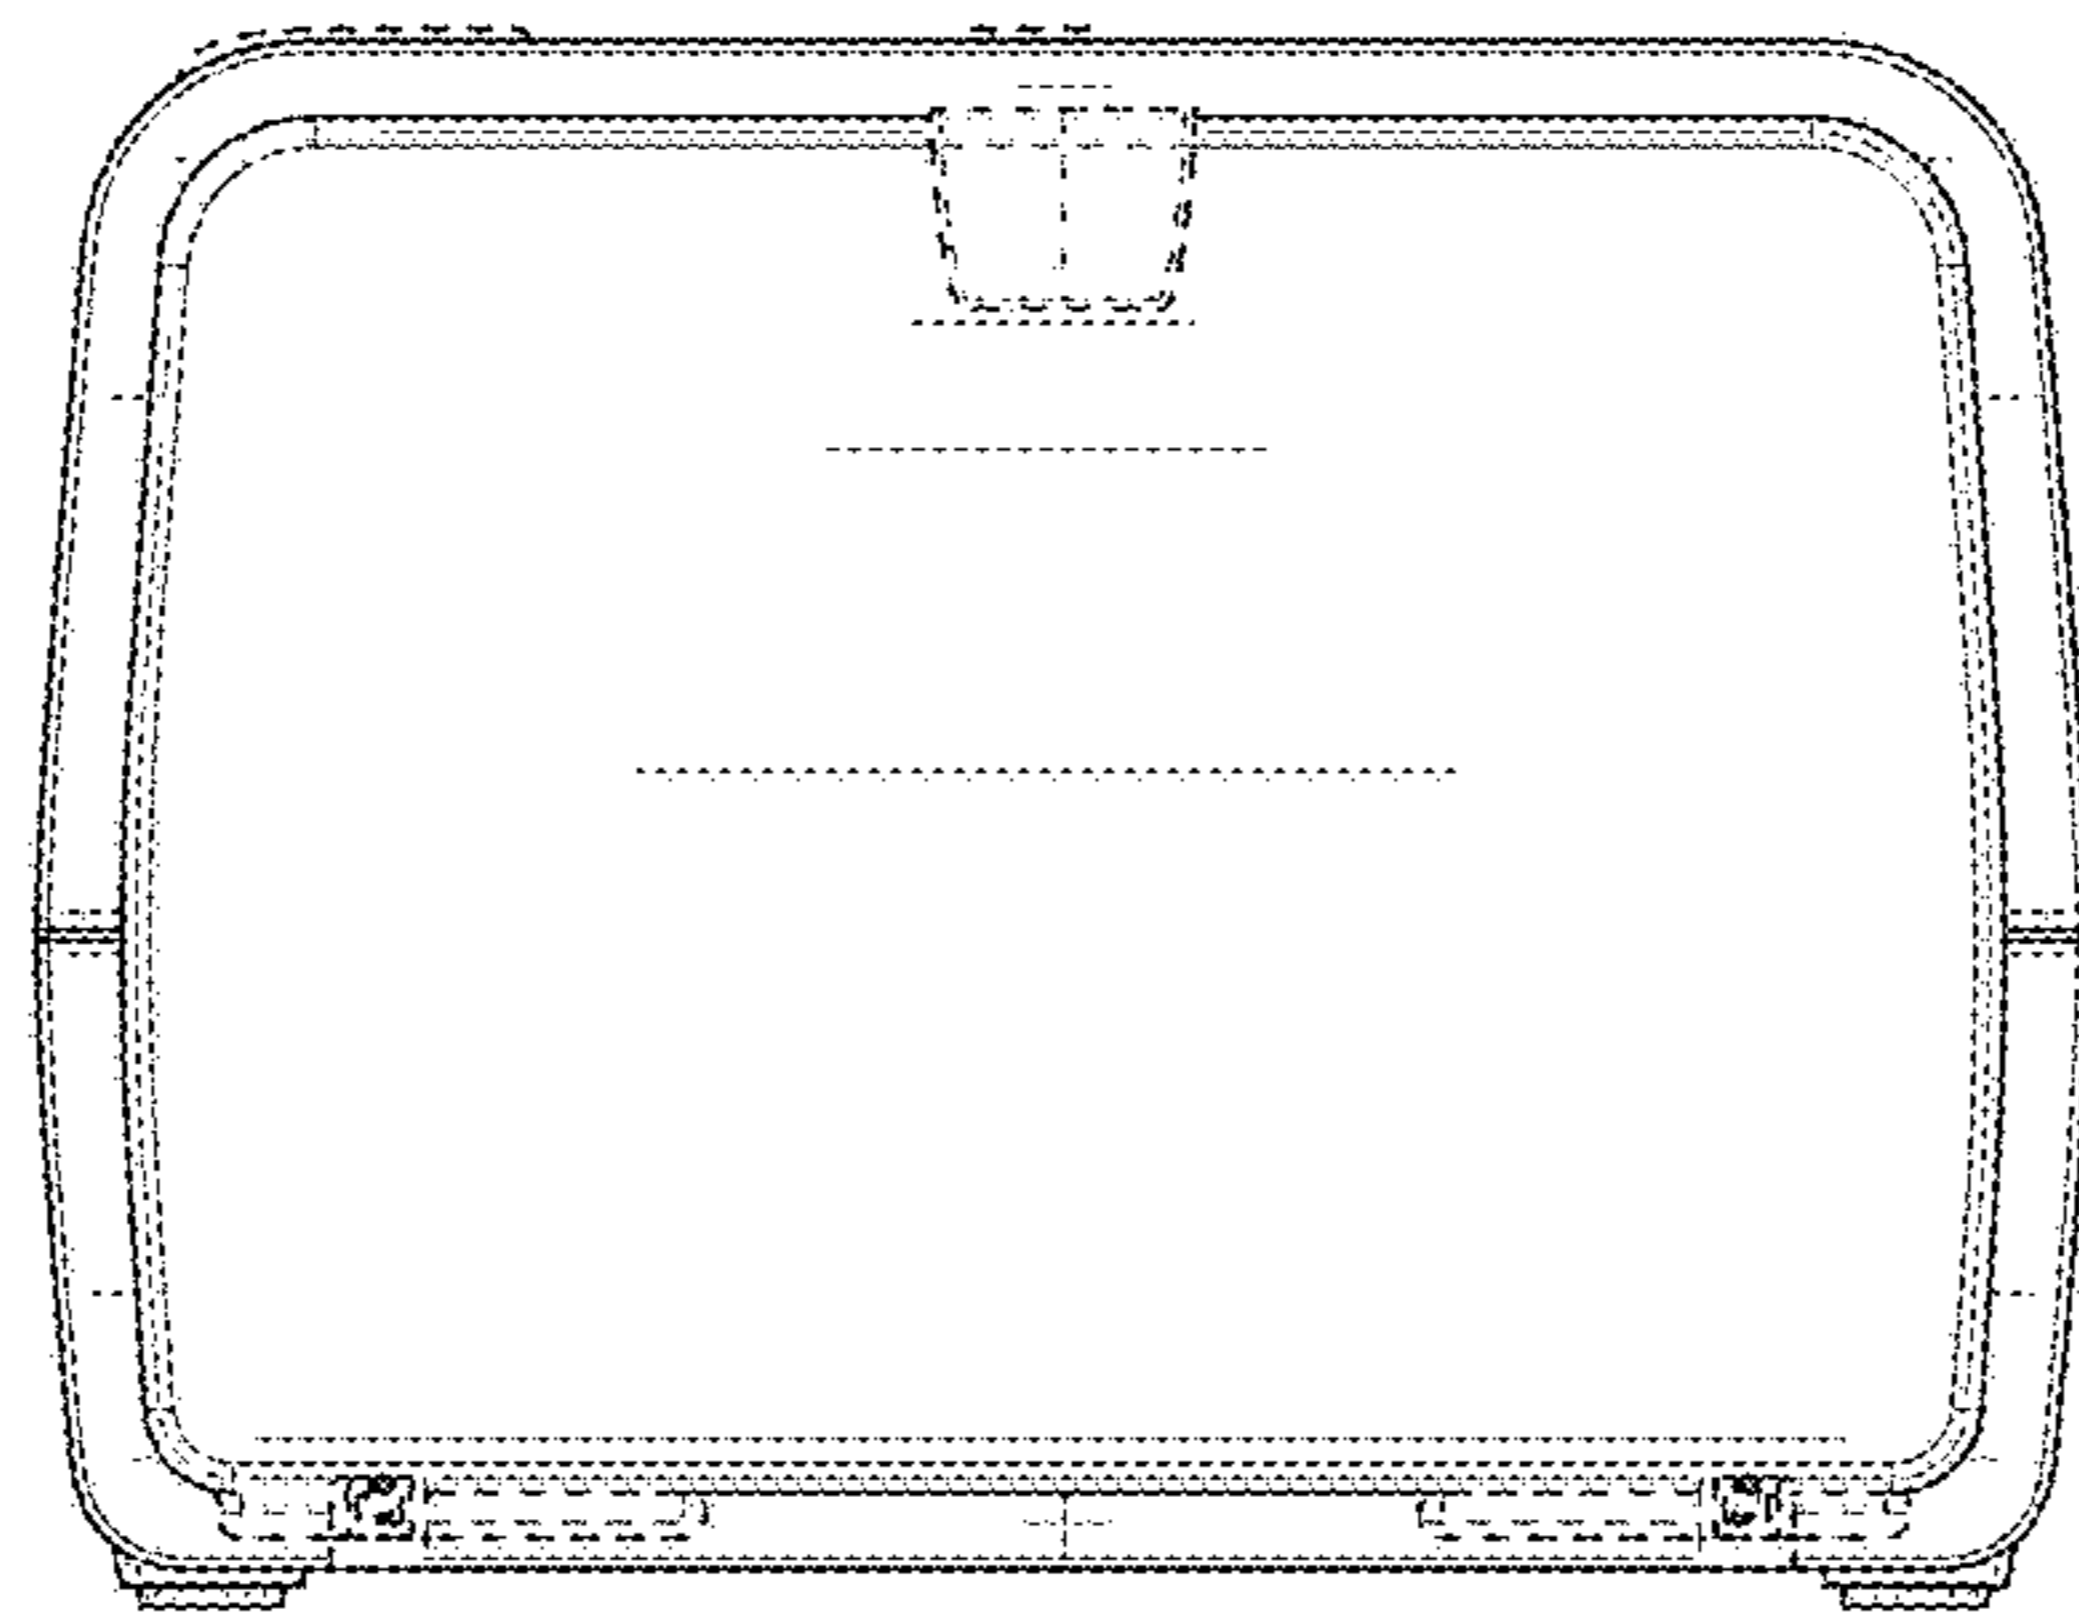


FIG. 1

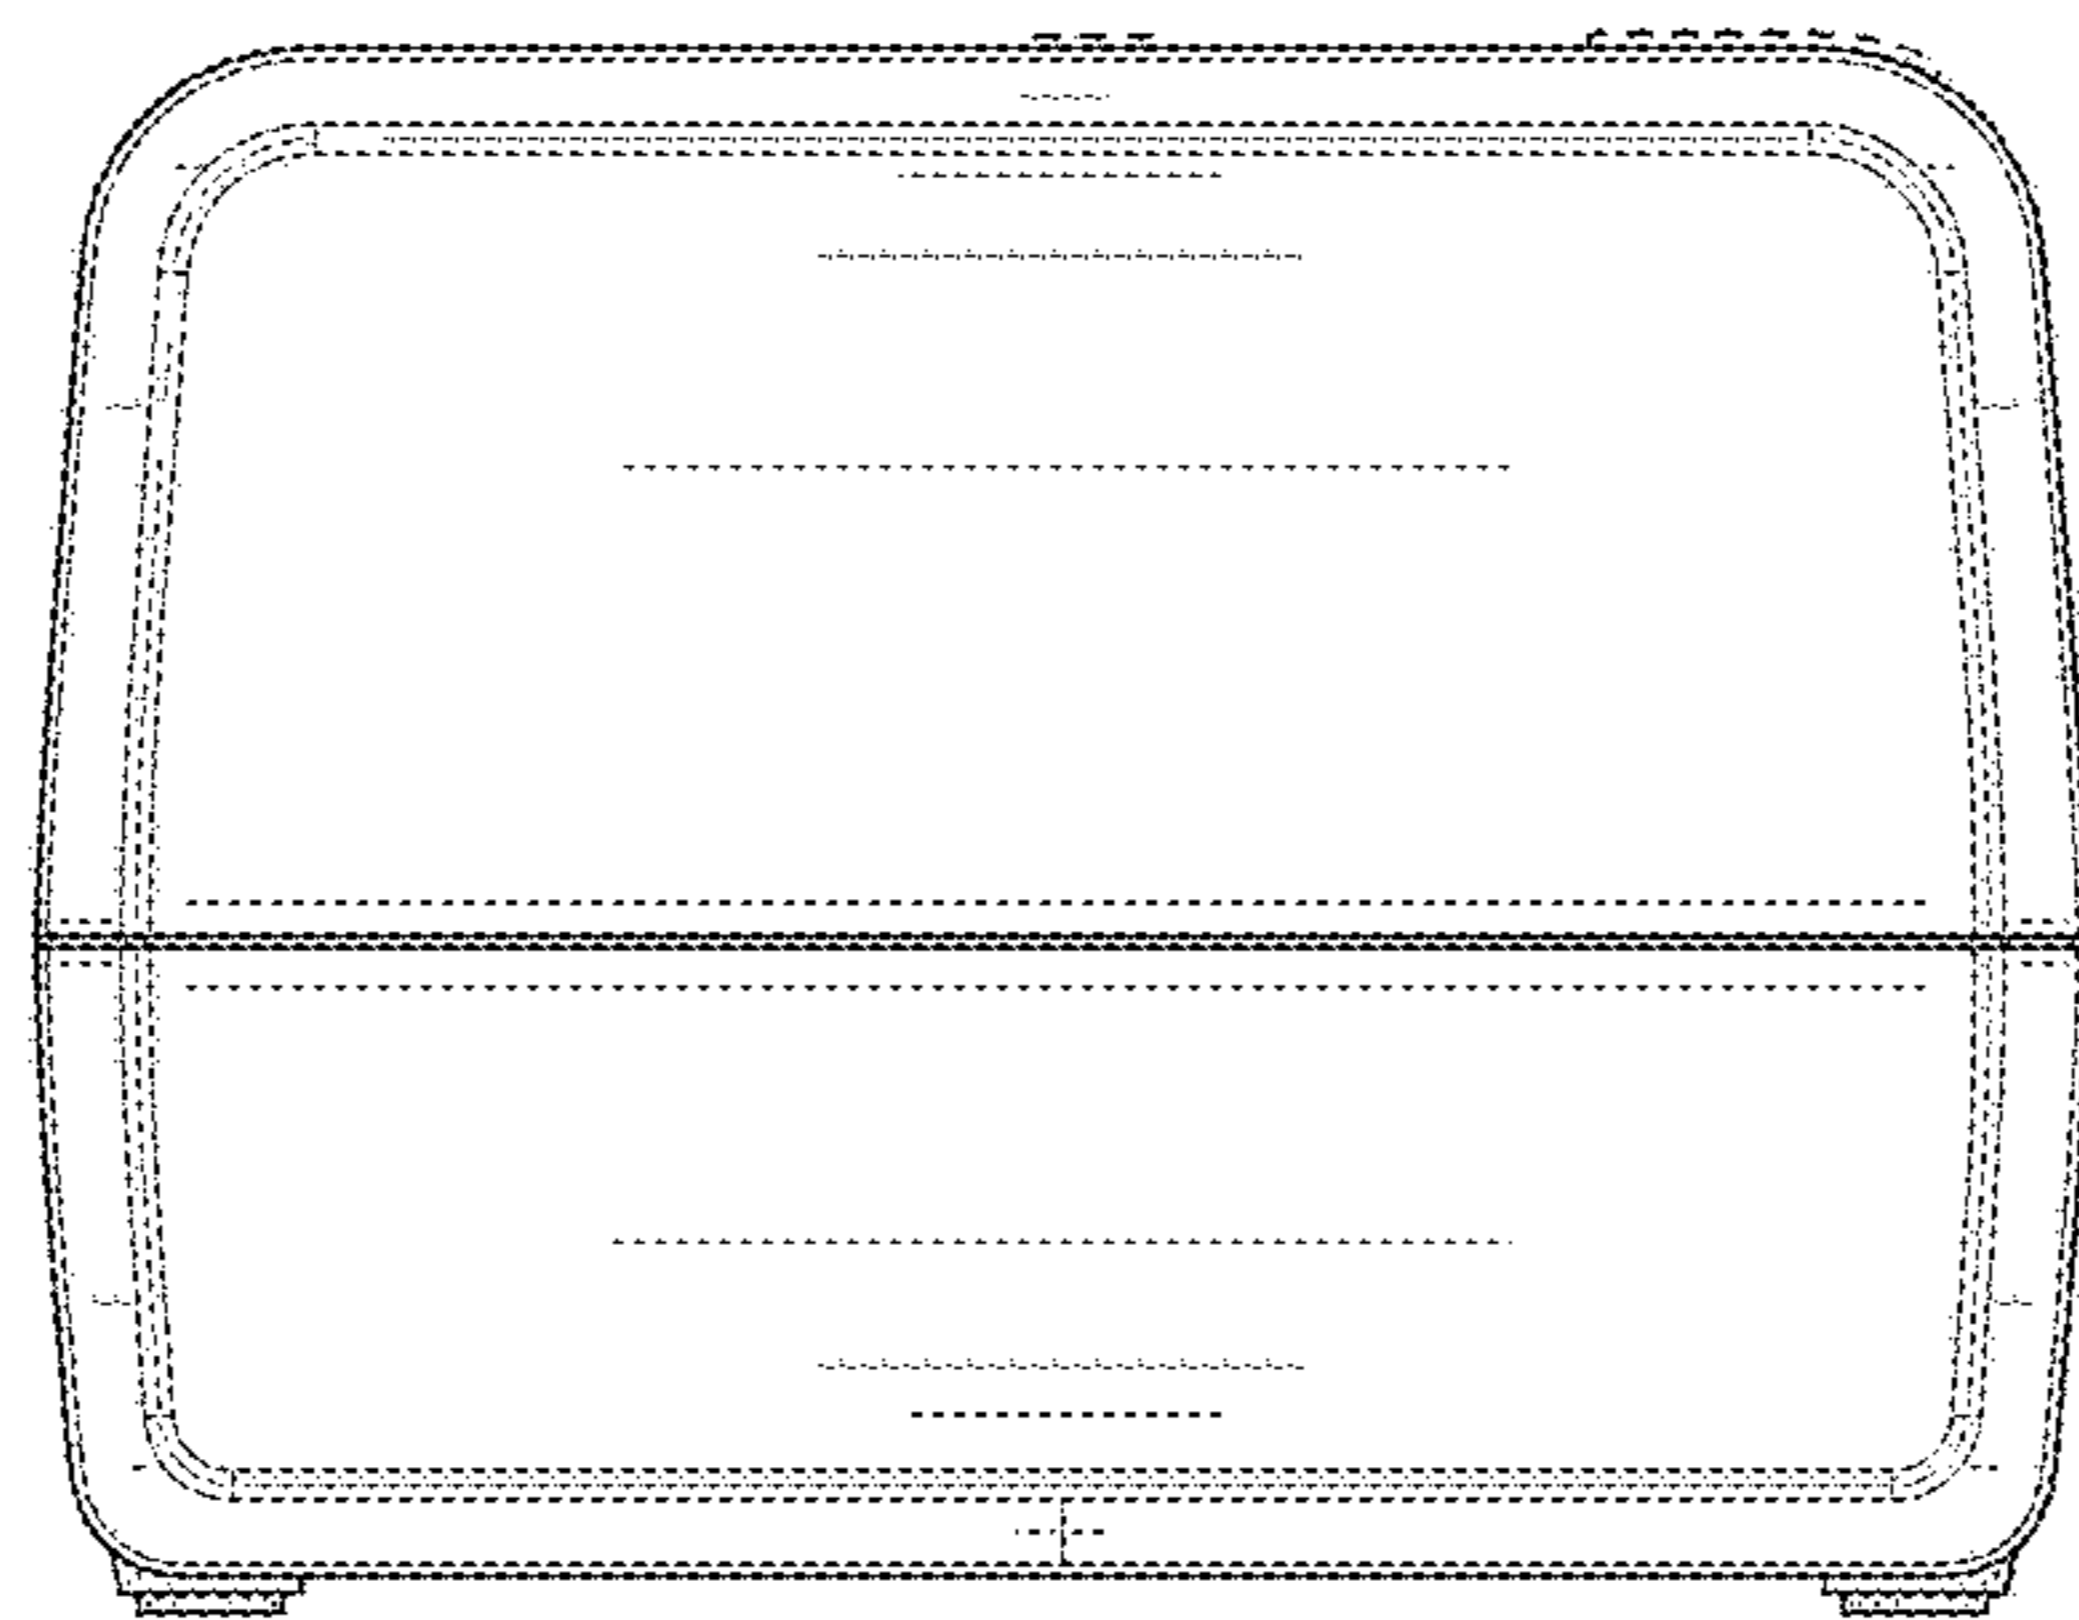


FIG. 2

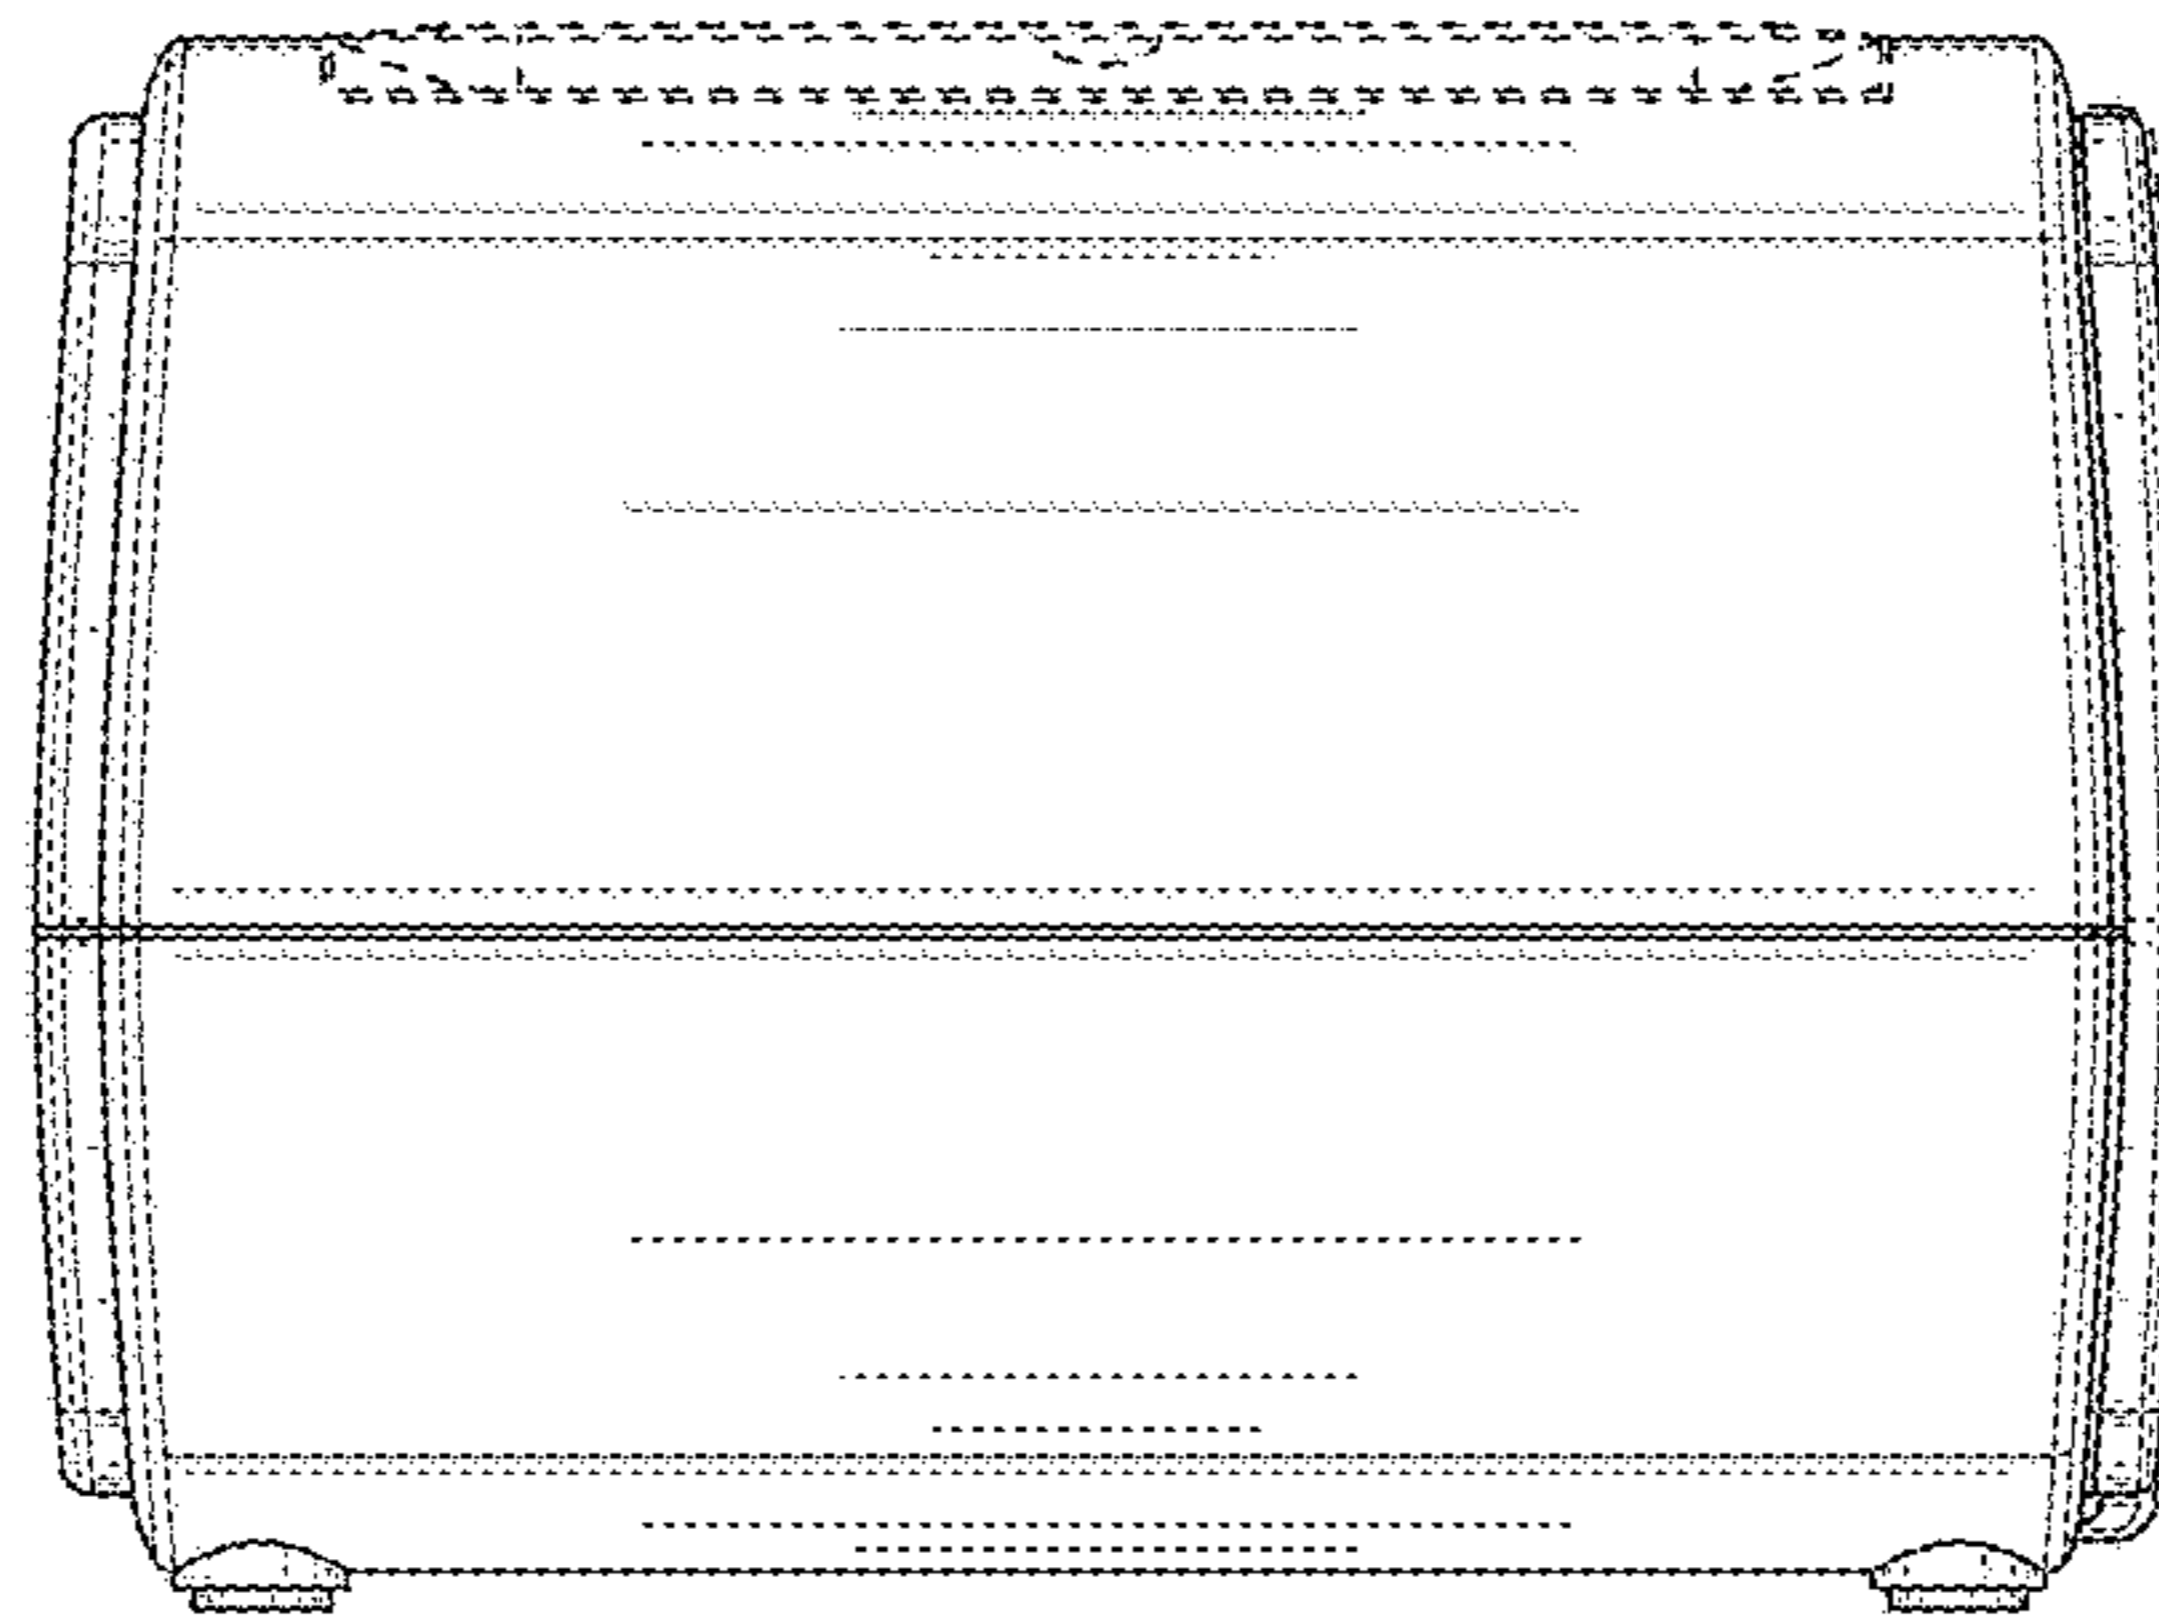


FIG. 3

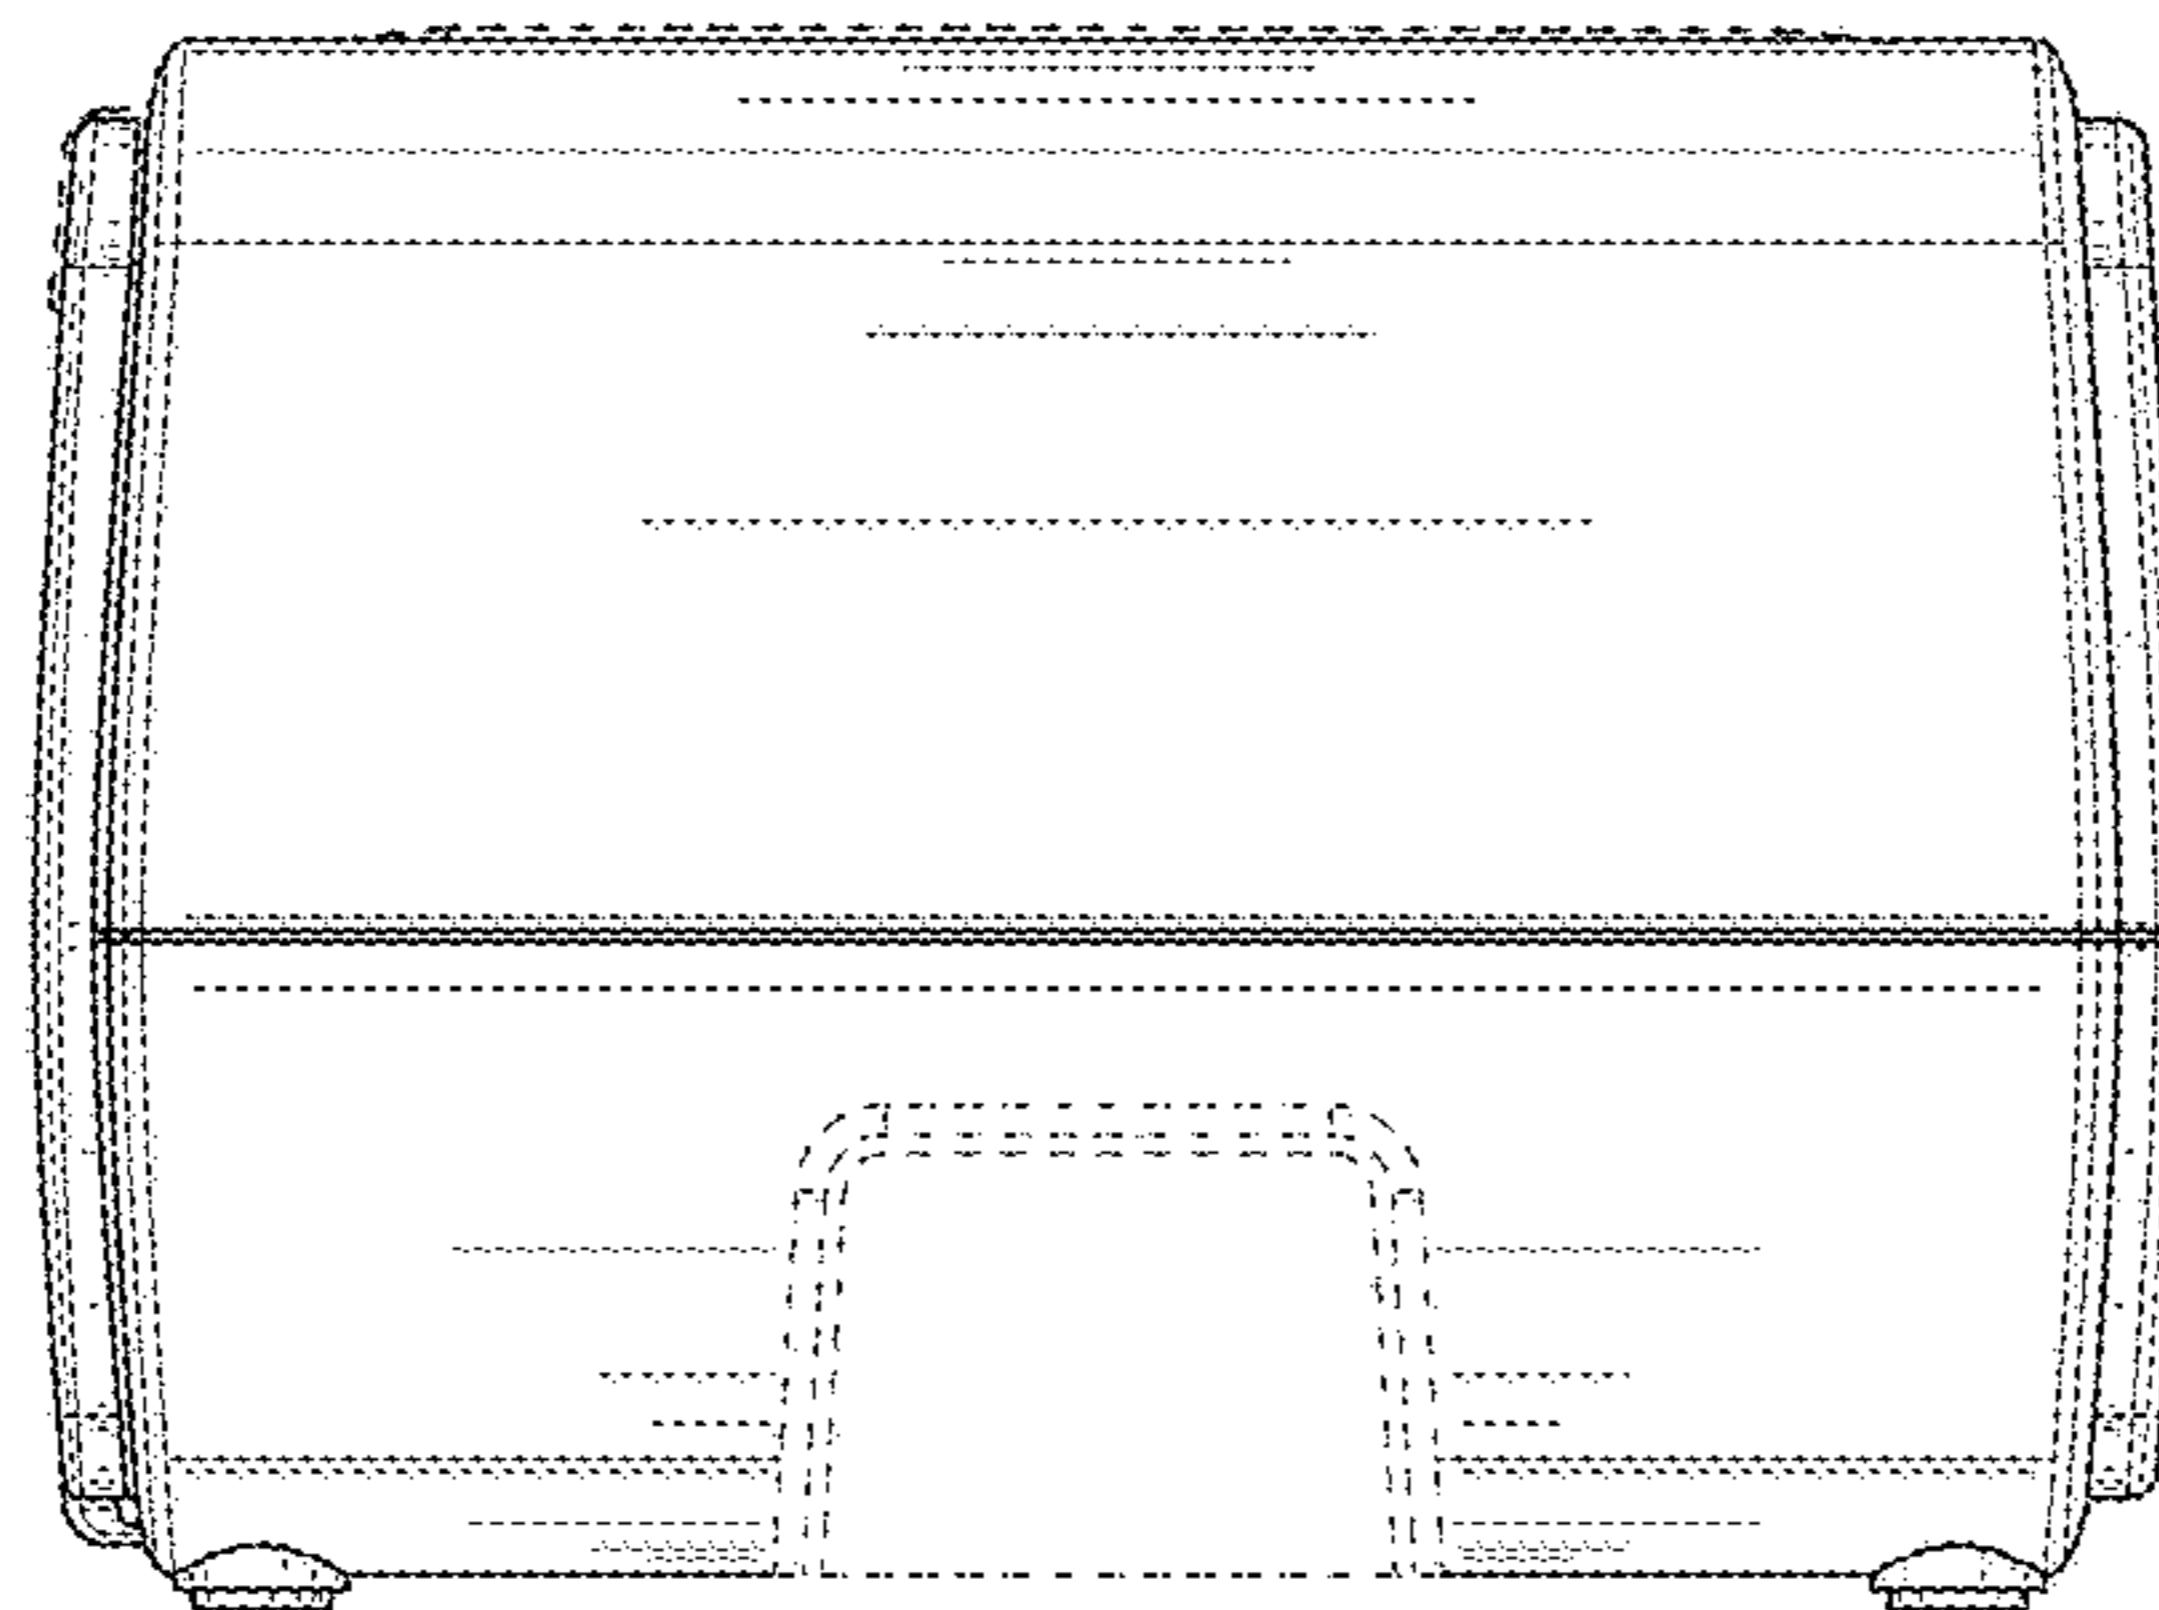


FIG. 4

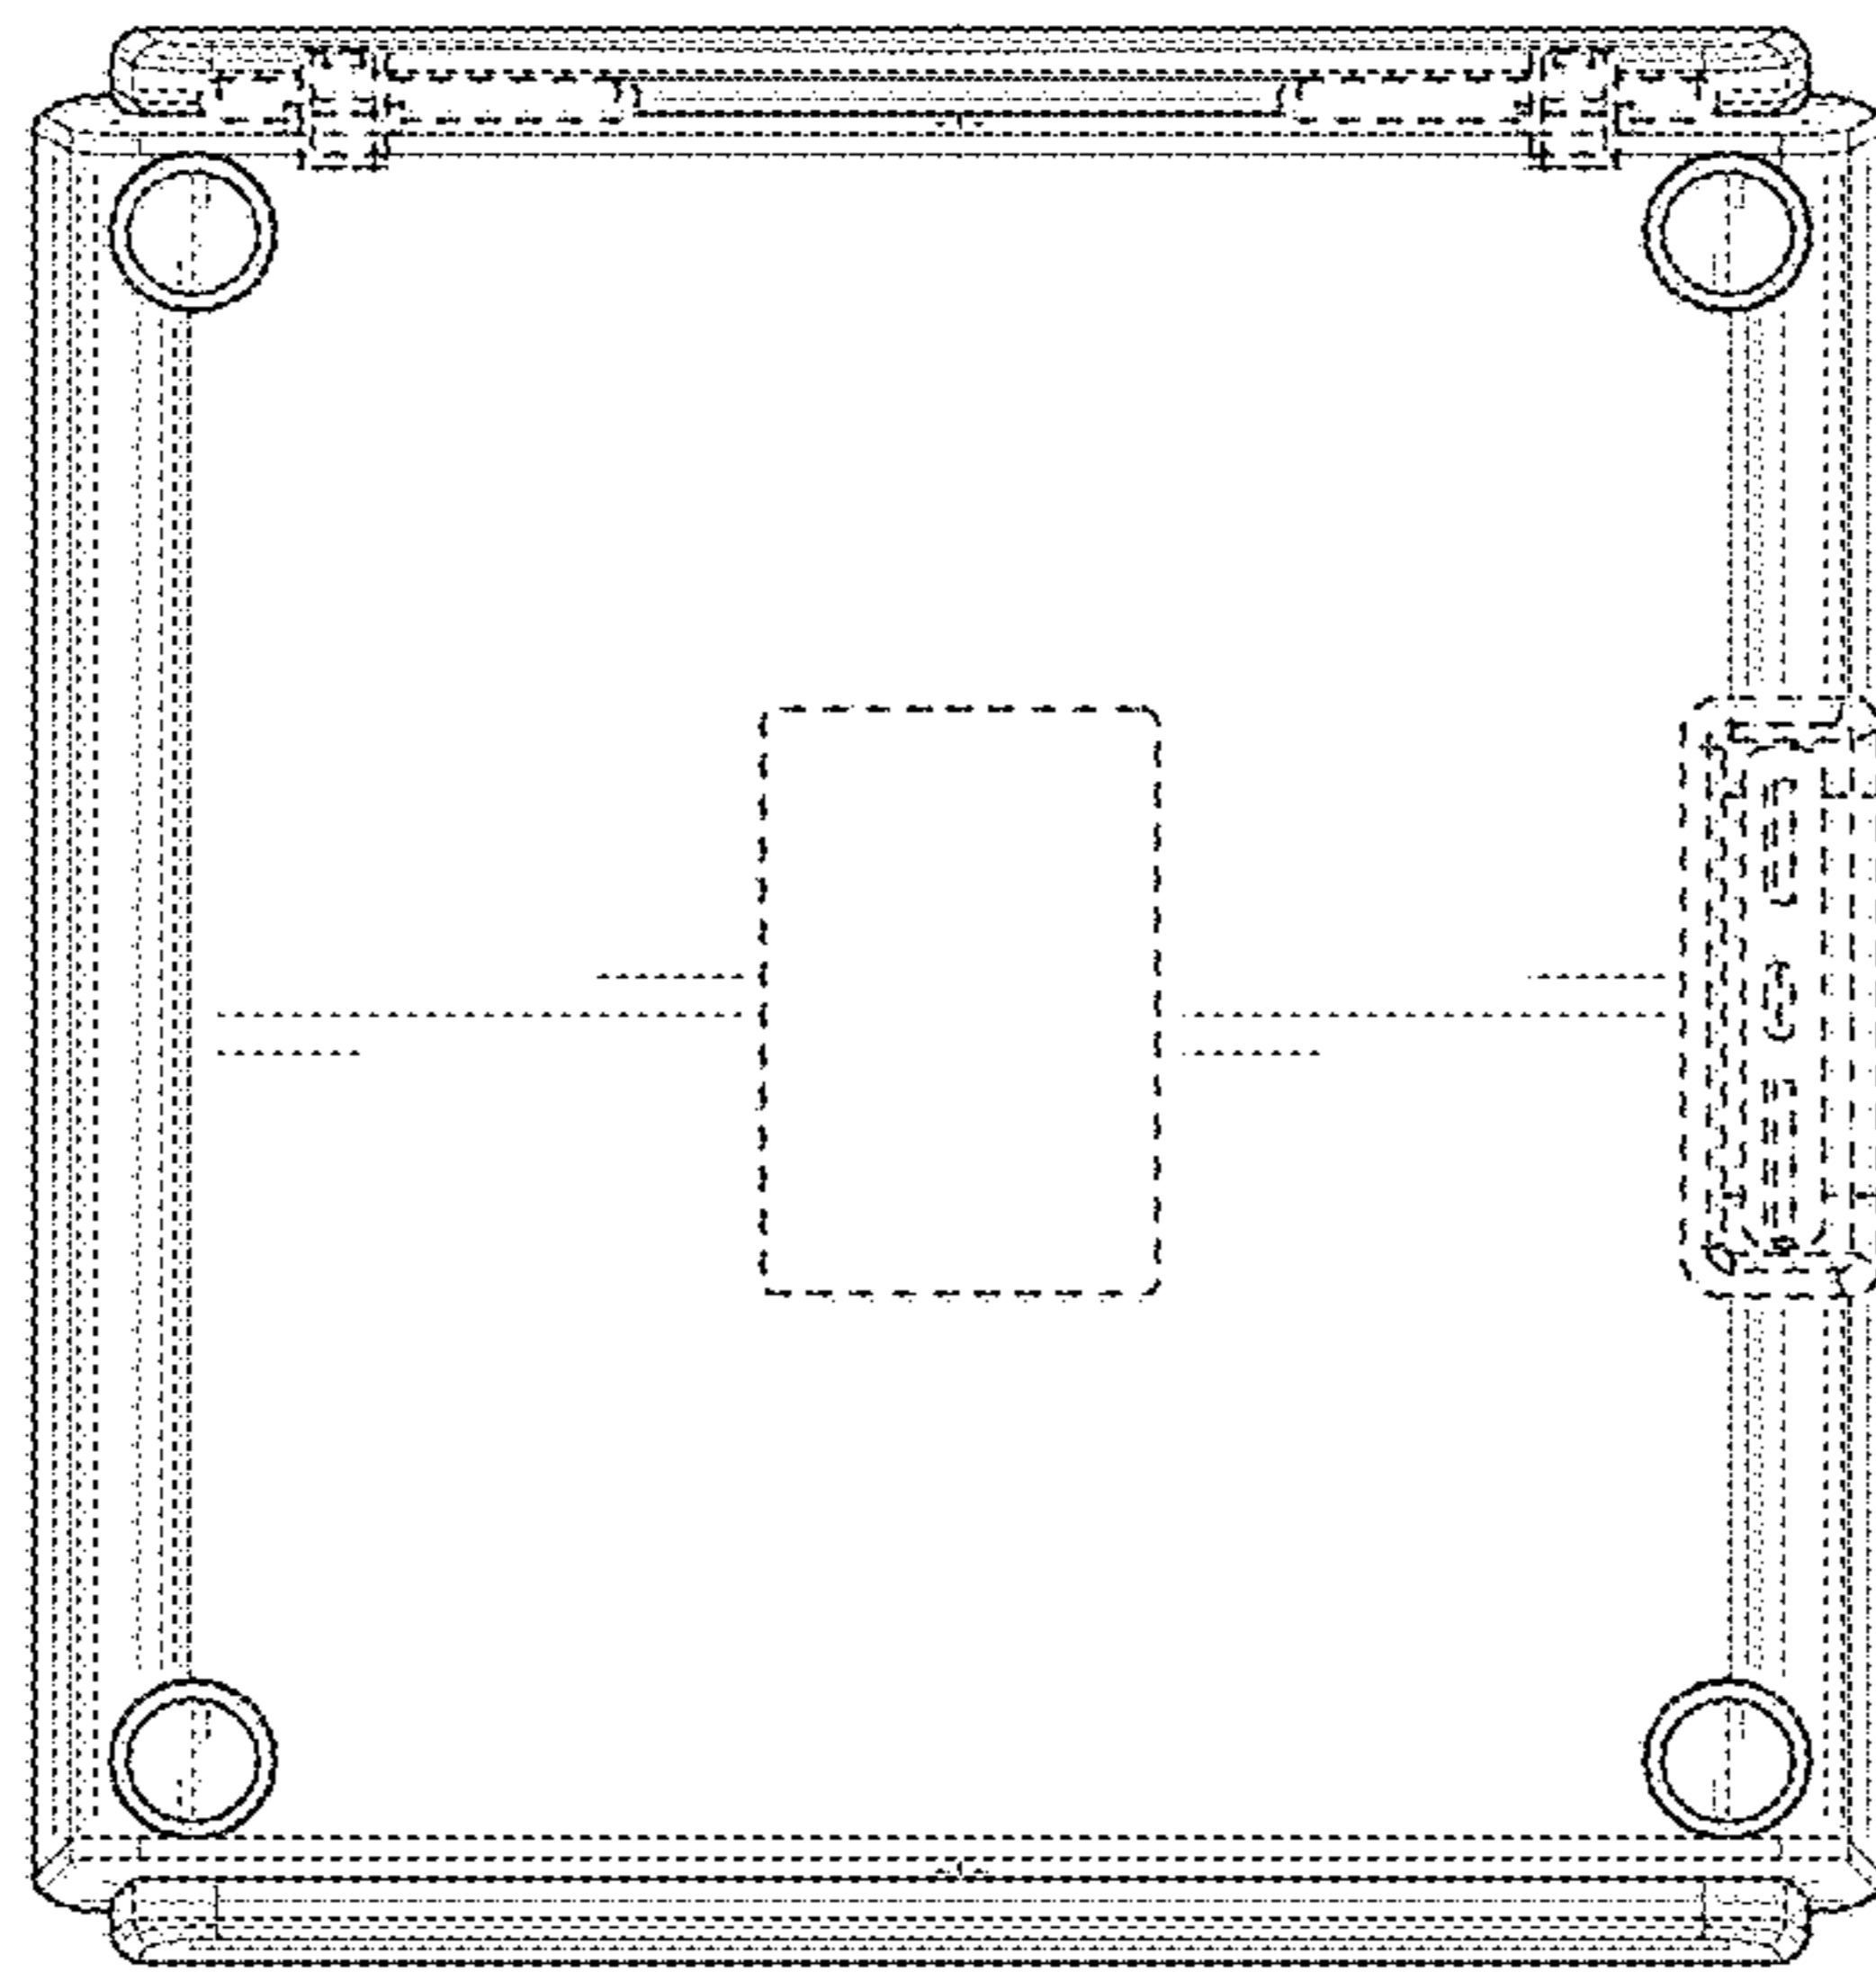


FIG. 5

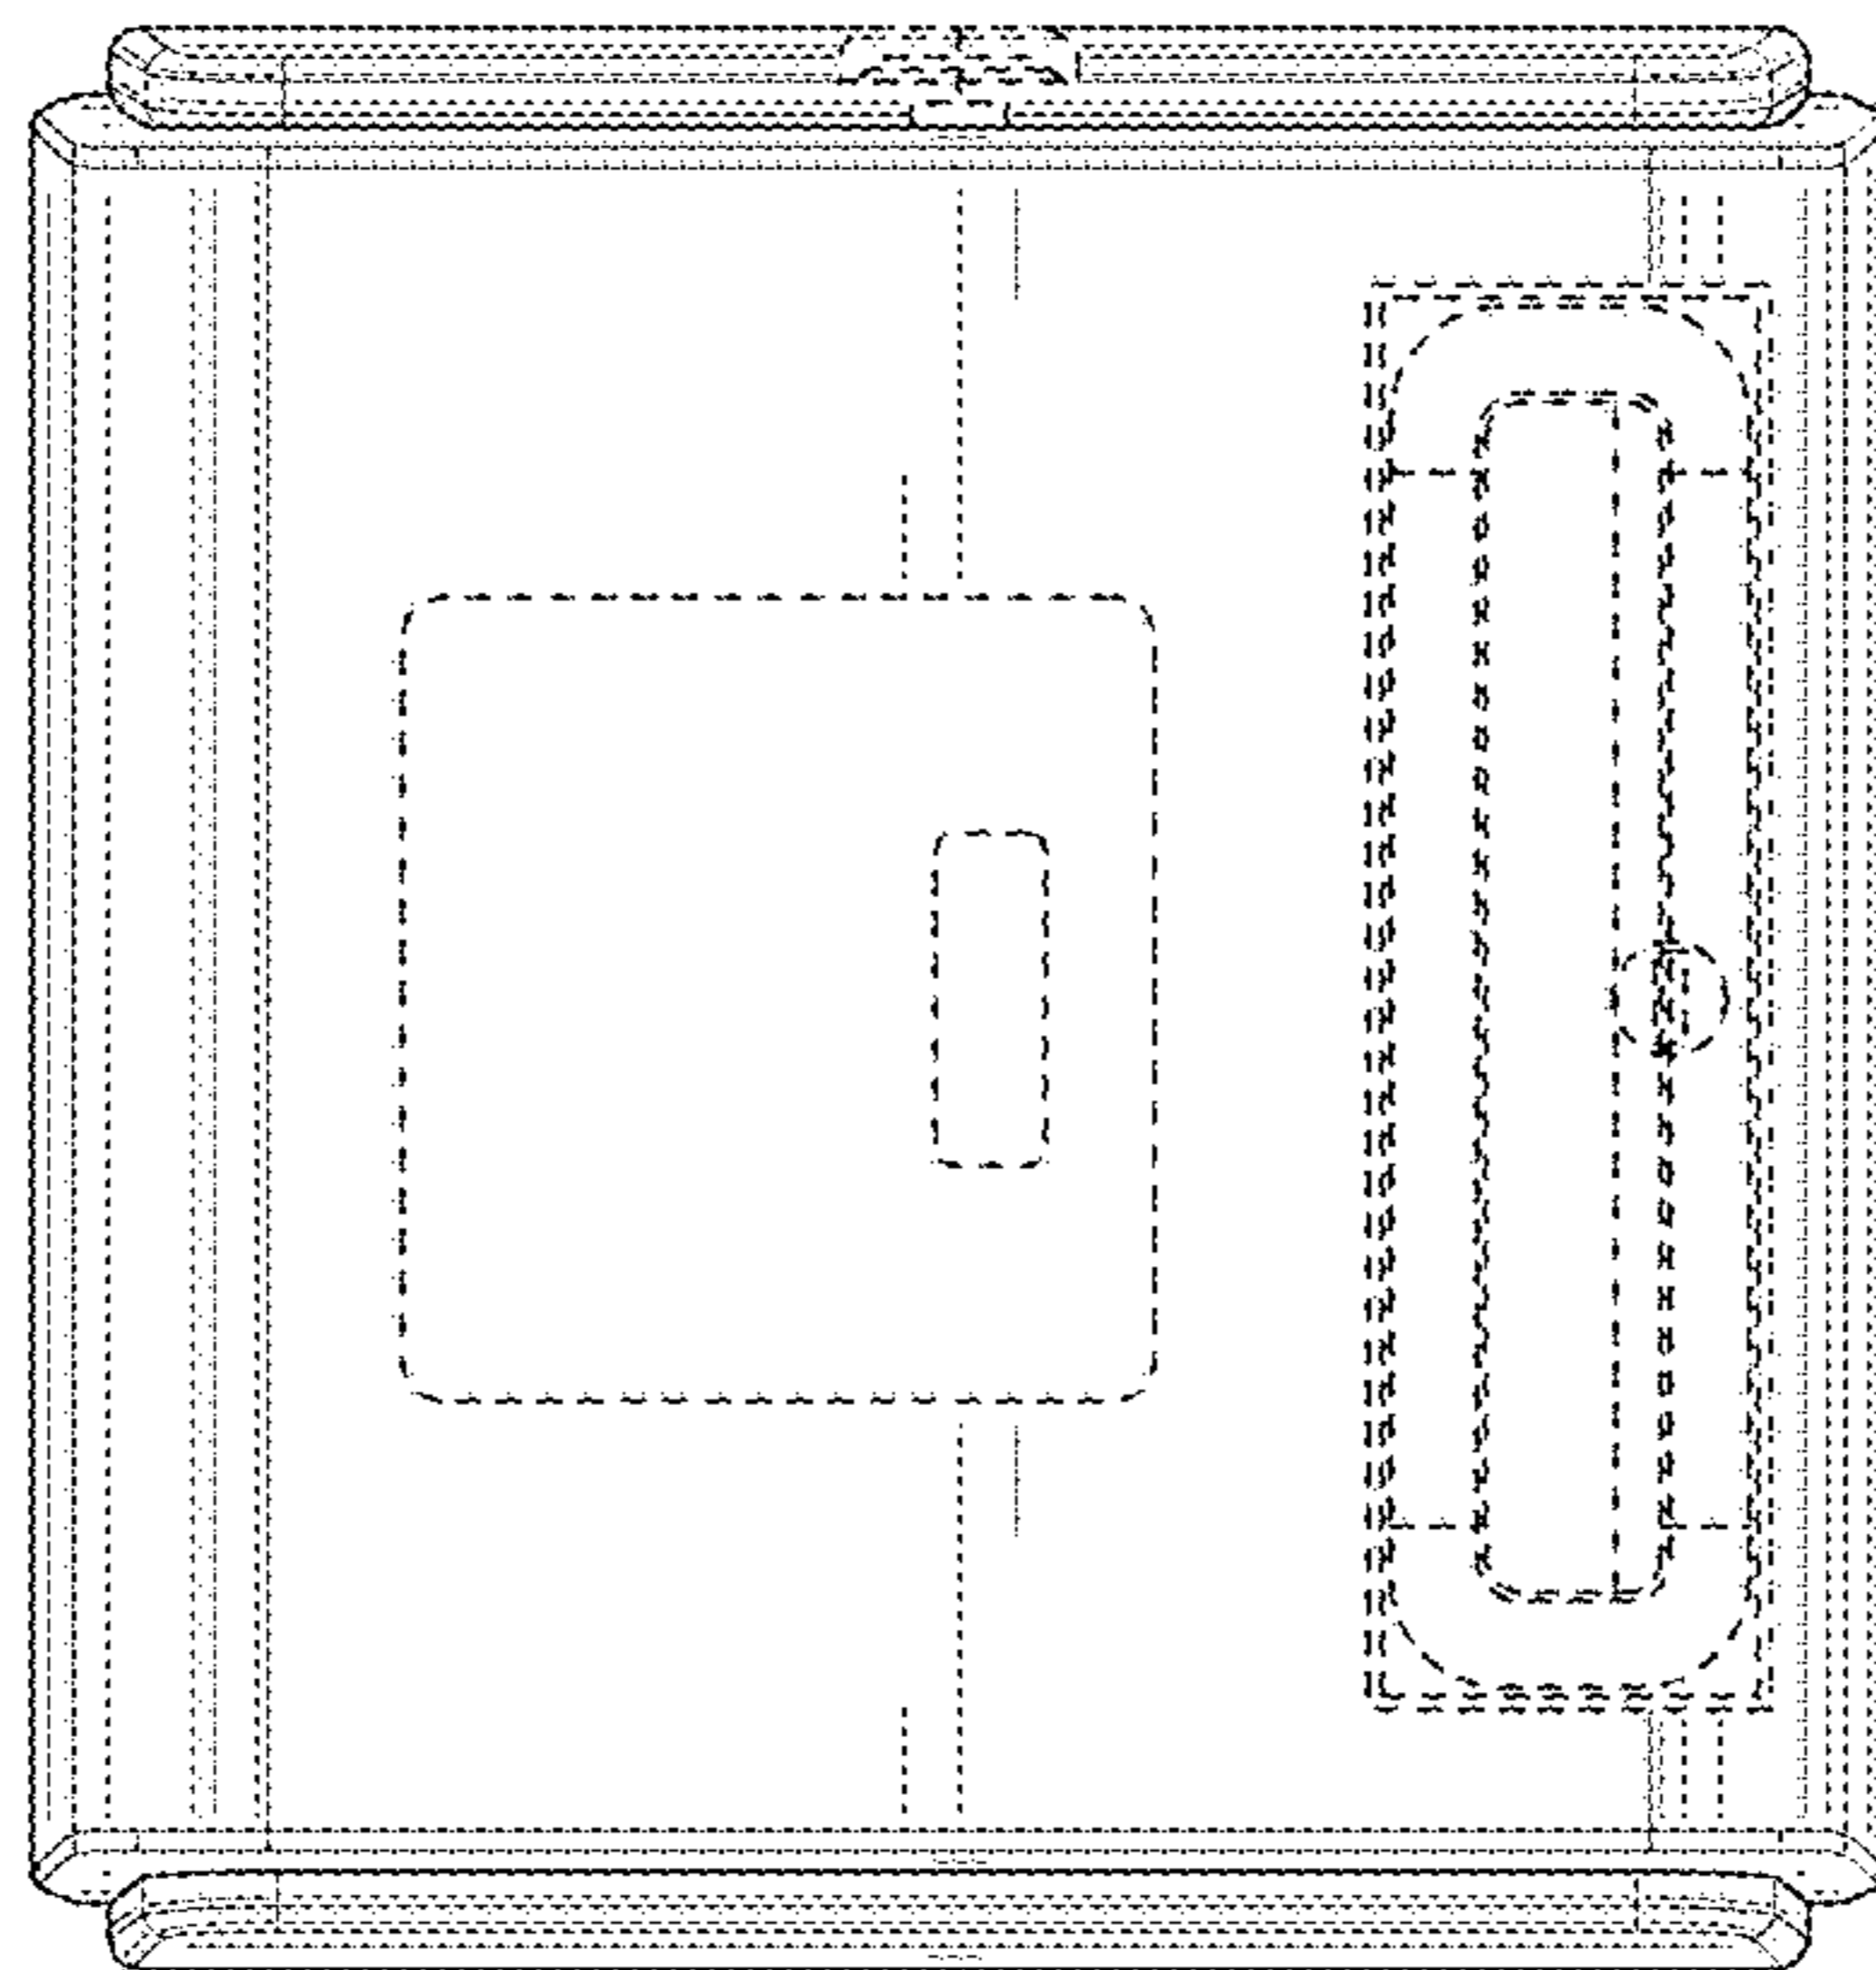


FIG. 6