



US00D859672S

(12) **United States Design Patent** (10) **Patent No.:** **US D859,672 S**
Blake (45) **Date of Patent:** **** Sep. 10, 2019**

(54) **MEDICAL DEVICE**

(71) Applicant: **Orthofix Inc.**, Lewisville, TX (US)

(72) Inventor: **Steve Blake**, Allen, TX (US)

(73) Assignee: **ORTHOFIX INC.**, Lewisville, TX (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/639,259**

(22) Filed: **Mar. 5, 2018**

(51) **LOC (12) Cl.** **28-03**

(52) **U.S. Cl.**
USPC **D24/200**

(58) **Field of Classification Search**
USPC D24/200, 214–215, 190, 171, 107;
600/9–10, 13–15
CPC A61F 5/01; A61F 5/0109; A61F 5/0111;
A61N 2/004; A61N 2/006; A61N 2/02;
A61N 2/12; A61N 1/326; A61N 1/36;
A61N 1/36003; A61N 1/40
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,266,532	A *	5/1981	Ryaby	A61N 2/02 600/14
4,548,208	A *	10/1985	Niemi	A61N 2/02 600/14
5,067,940	A *	11/1991	Liboff	A61N 2/02 600/13
D326,913	S *	6/1992	Staples	D24/200
5,318,561	A *	6/1994	McLeod	A61N 2/02 600/14
5,743,844	A *	4/1998	Tepper	A61N 2/02 600/13

(Continued)

OTHER PUBLICATIONS

Orthofix Holdings, Inc. "A Patient's Guide to Spine Fusion Stimulation," dated Jun. 2014 //pdf.medicalexpo.com/pdf/orthofix/cervical-stim-patient-q/74966-148857.html, 4 pgs.

(Continued)

Primary Examiner — Wan Laymon

(74) *Attorney, Agent, or Firm* — Haynes and Boone, LLP

(57) **CLAIM**

The ornamental design for a medical device, as shown and described.

DESCRIPTION

This application is related to U.S. application Ser. Nos. 29/639,249, 29/639,258, 29/369,241, 29/639,287 and 29/639,289, all filed Mar. 5, 2018, the entire disclosures of which are hereby incorporated herein by reference.

FIG. 1 is a front perspective view of a medical device showing my new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a right side elevational view thereof;

FIG. 5 is a left side elevational view thereof;

FIG. 6 is a top plan view thereof;

FIG. 7 is a bottom plan view thereof;

FIG. 8 is a rear perspective view thereof; and,


FIG. 9 is another front perspective view thereof, the front perspective view of FIG. 9 being similar to the front perspective view of FIG. 1 but for the depiction in broken lines of unclaimed environmental structure in FIG. 9.

The broken lines in FIGS. 2, 3, 7, and 8 depict portions of the medical device that form no part of the claimed design.

The broken lines in FIG. 9 depict environmental structure that forms no part of the claimed design.

The different surface shadings (line shading and stippled shading) in FIGS. 1, 8, and 9 are used to indicate contrasting materials.

1 Claim, 7 Drawing Sheets

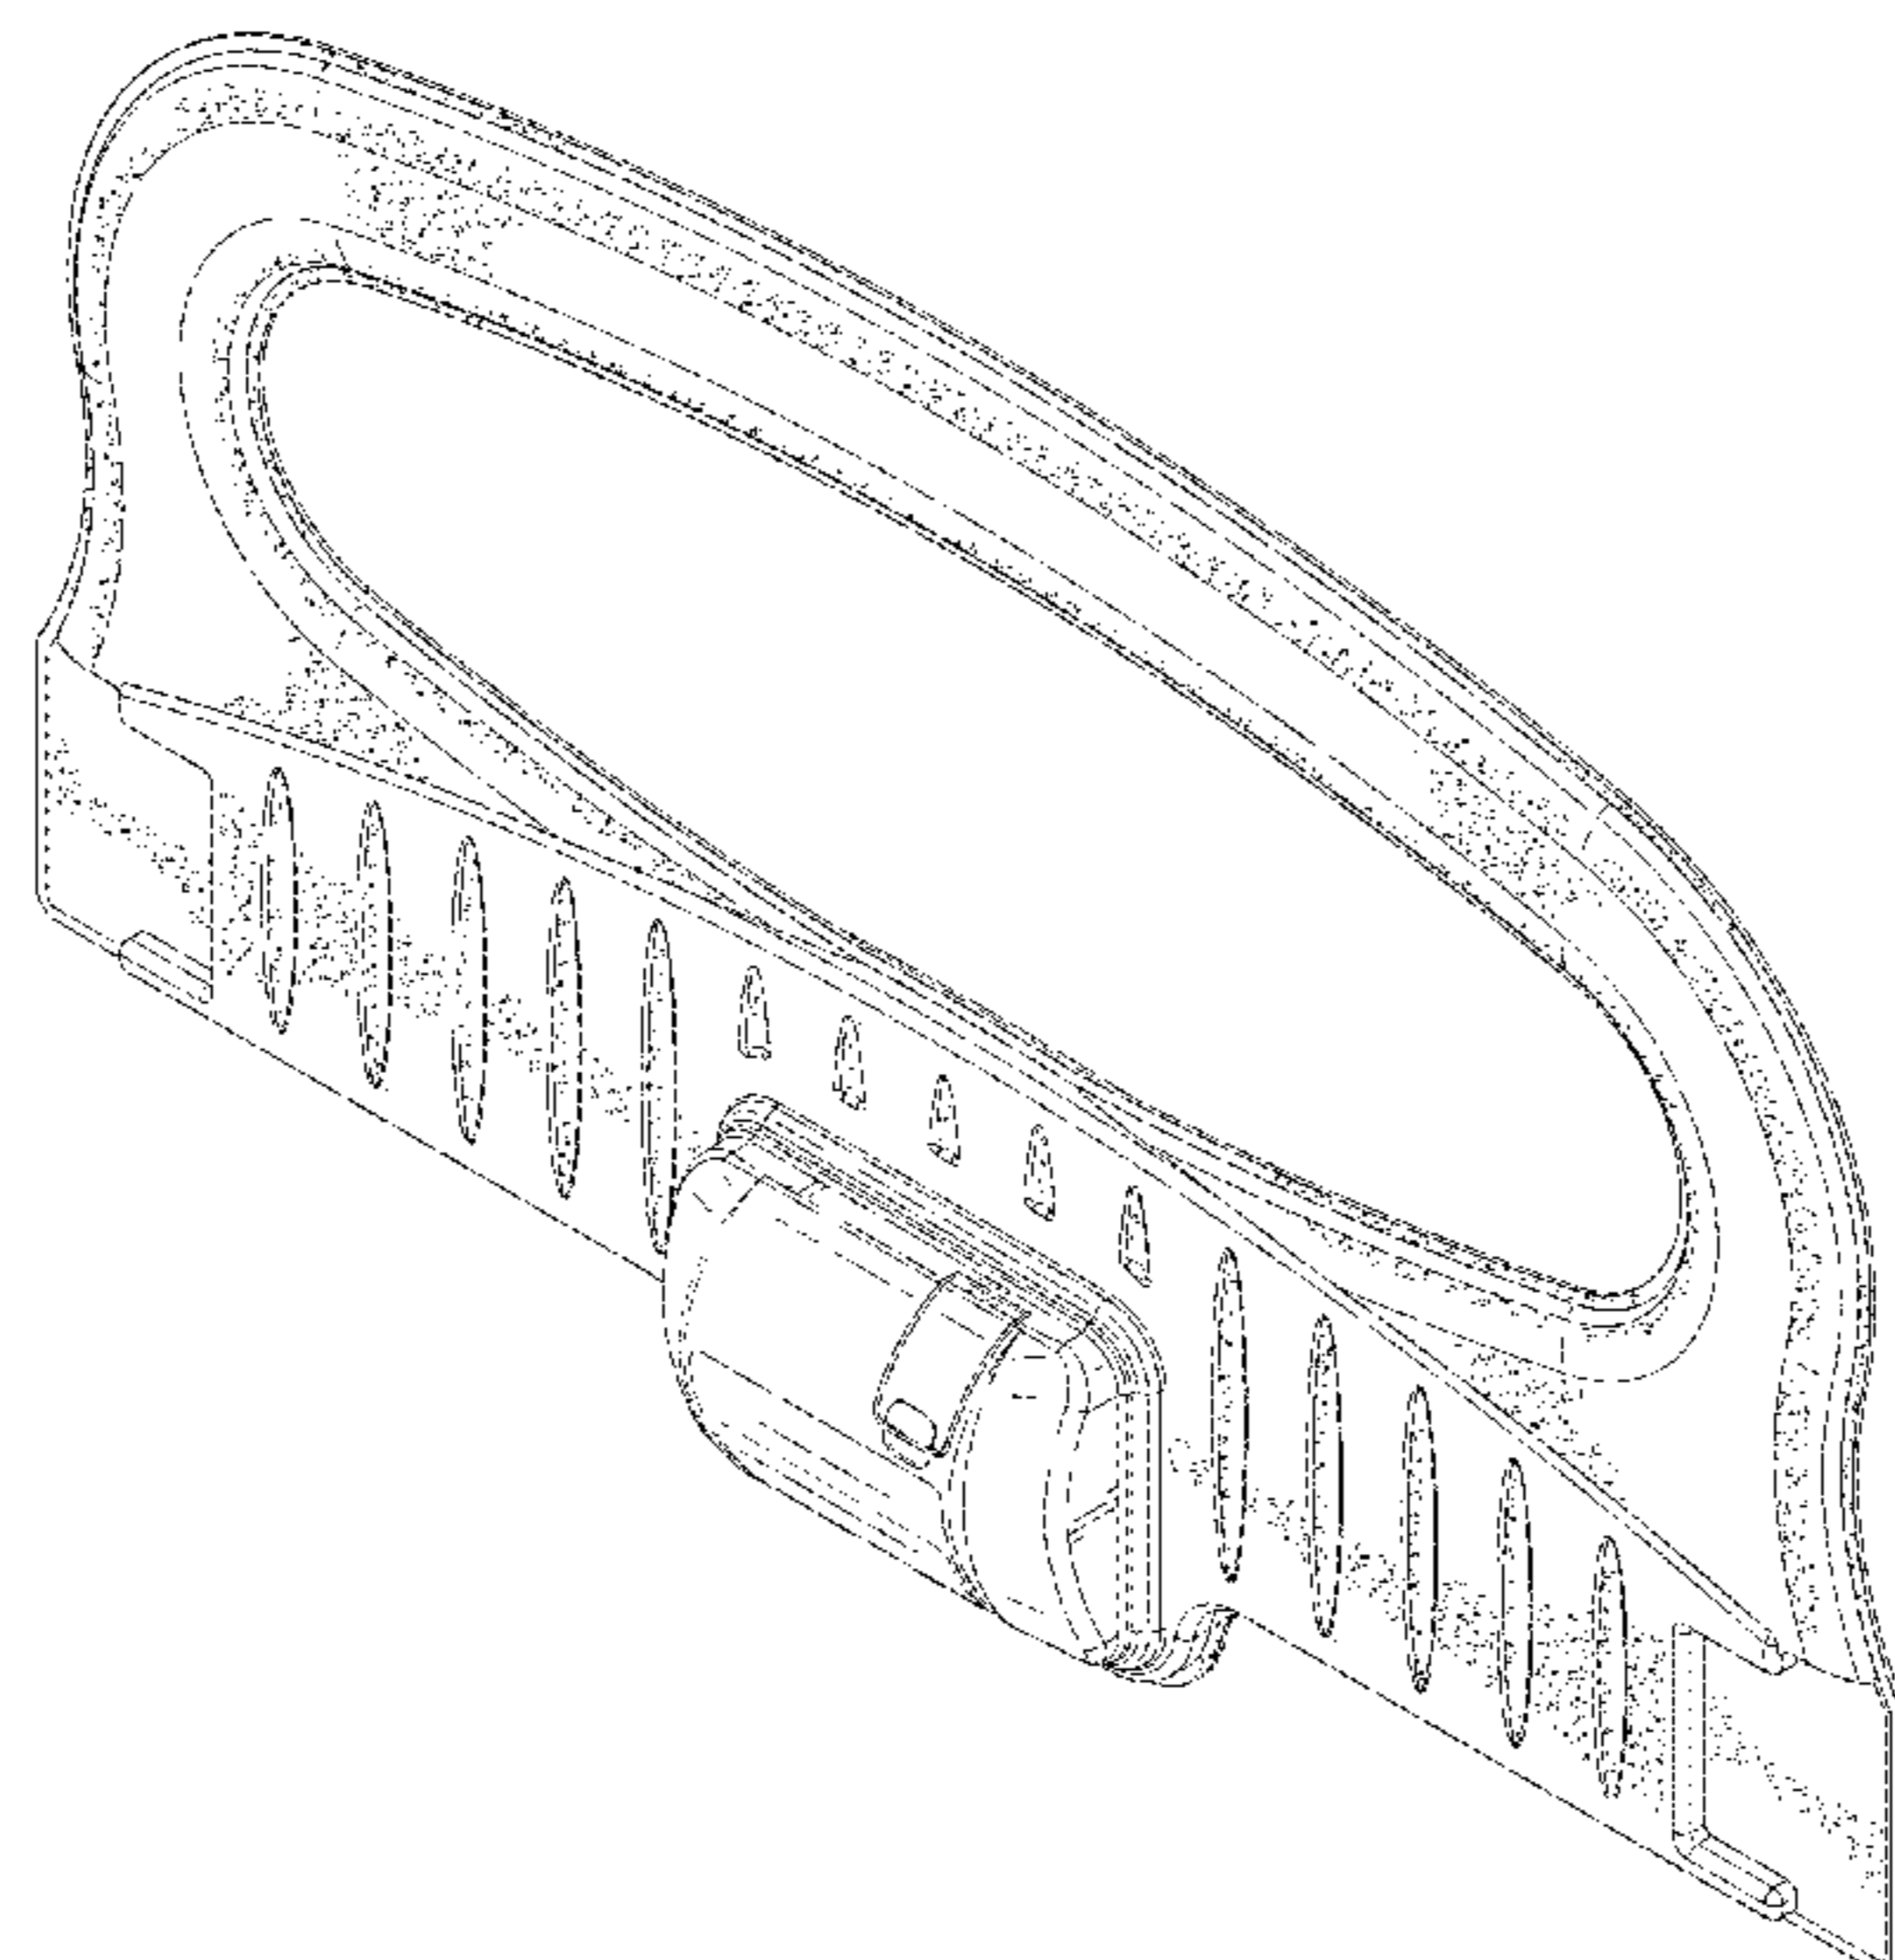

(56)

References Cited

U.S. PATENT DOCUMENTS

5,792,040	A *	8/1998	Koeneman	A61N 2/02 600/13
6,024,691	A *	2/2000	Tepper	A61N 2/02 600/13
6,364,824	B1	4/2002	Fitzsimmons	
6,592,509	B1 *	7/2003	Hunter, Jr.	A61N 2/02 600/9
7,465,269	B2 *	12/2008	Culhane	A61N 2/004 600/13
D742,020	S *	10/2015	Russold	D24/200
D834,719	S *	11/2018	Theriot	D24/200
2013/0245358	A1 *	9/2013	Johnson	A61N 2/02 600/13

OTHER PUBLICATIONS

Orthofix Holdings, Inc. "A Patient's Guide to Insurance Coverage for Bone Growth Therapy," Sep. 16, 2016, 5 pages.

Abrexis Medical, "The Healing Advantage Cervical-Stim," Aug. 8, 2013, retrieved from Twitter Apr. 4, 2018 <https://pbs.twimg.com/media/BRLVrARCYAAOY2T.jpg:large>, 2 pages.

Abrexis Medical, "The Healing Advantage Spinal-Stim," Aug. 8, 2013, retrieved from Twitter Apr. 4, 2018 <https://pbs.twimg.com/media/BRLVjnGCQAAYU9A.jpg:large>, 2 pages.

* cited by examiner

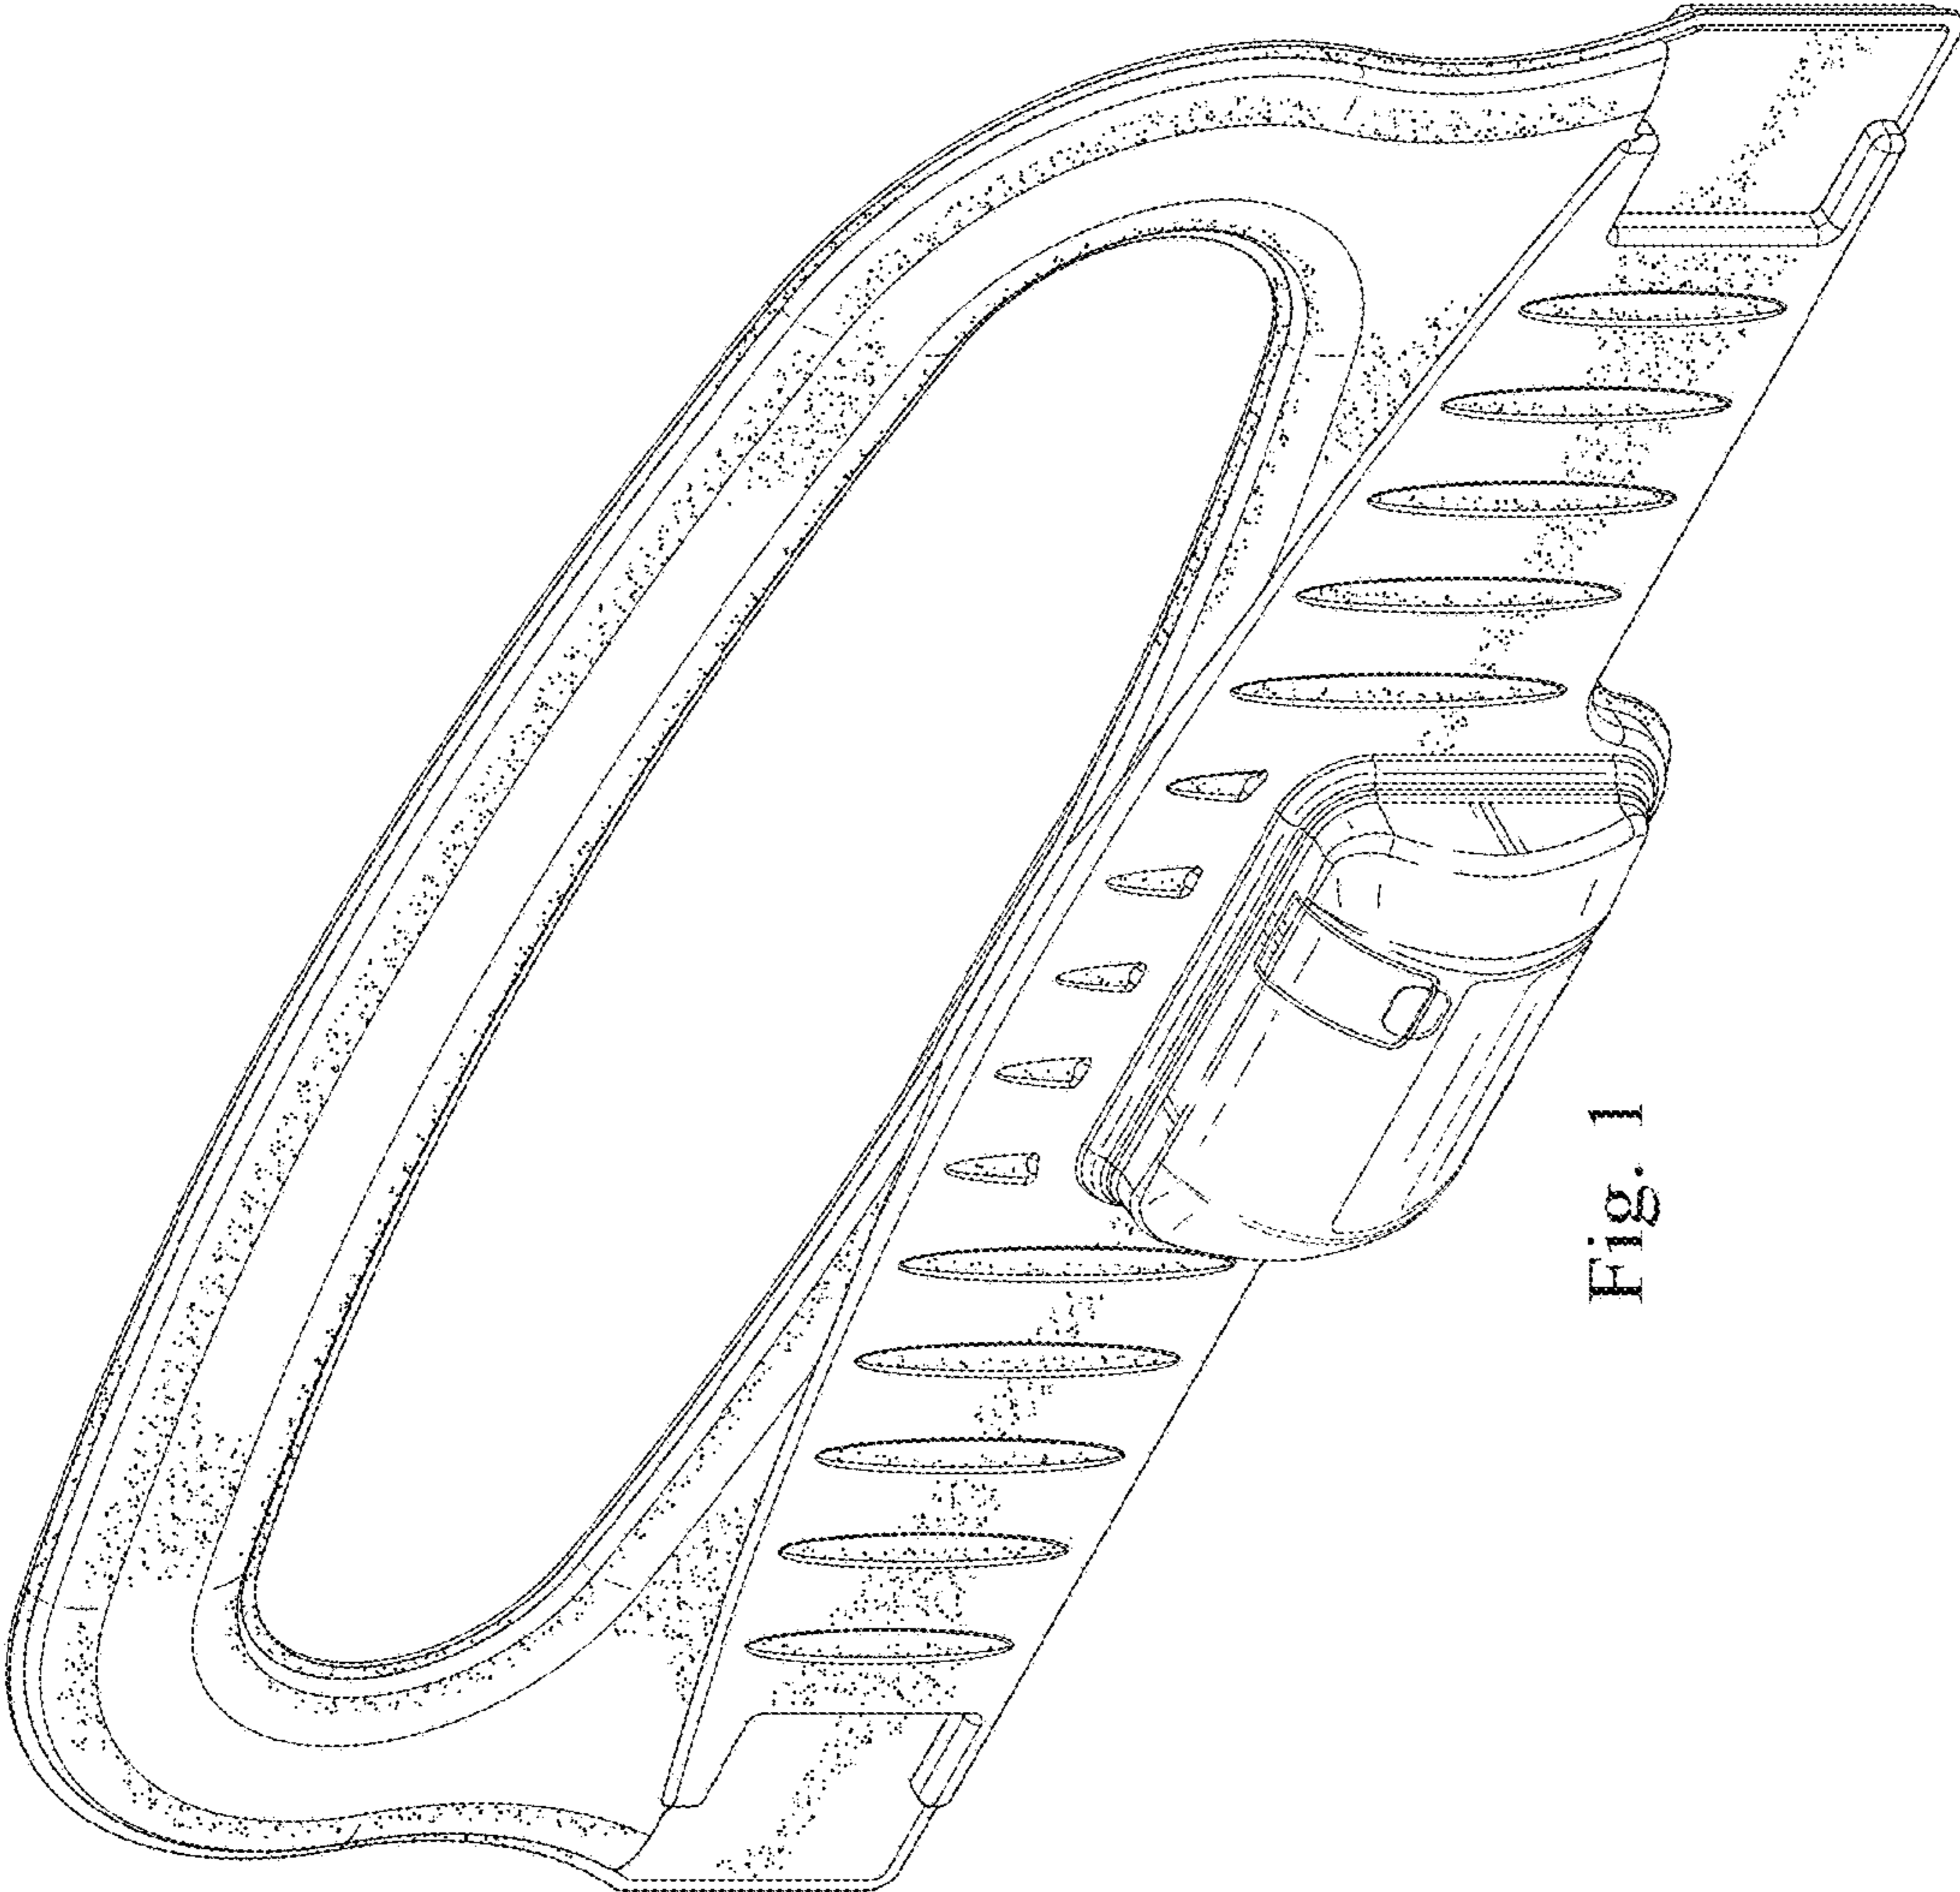


Fig. 1

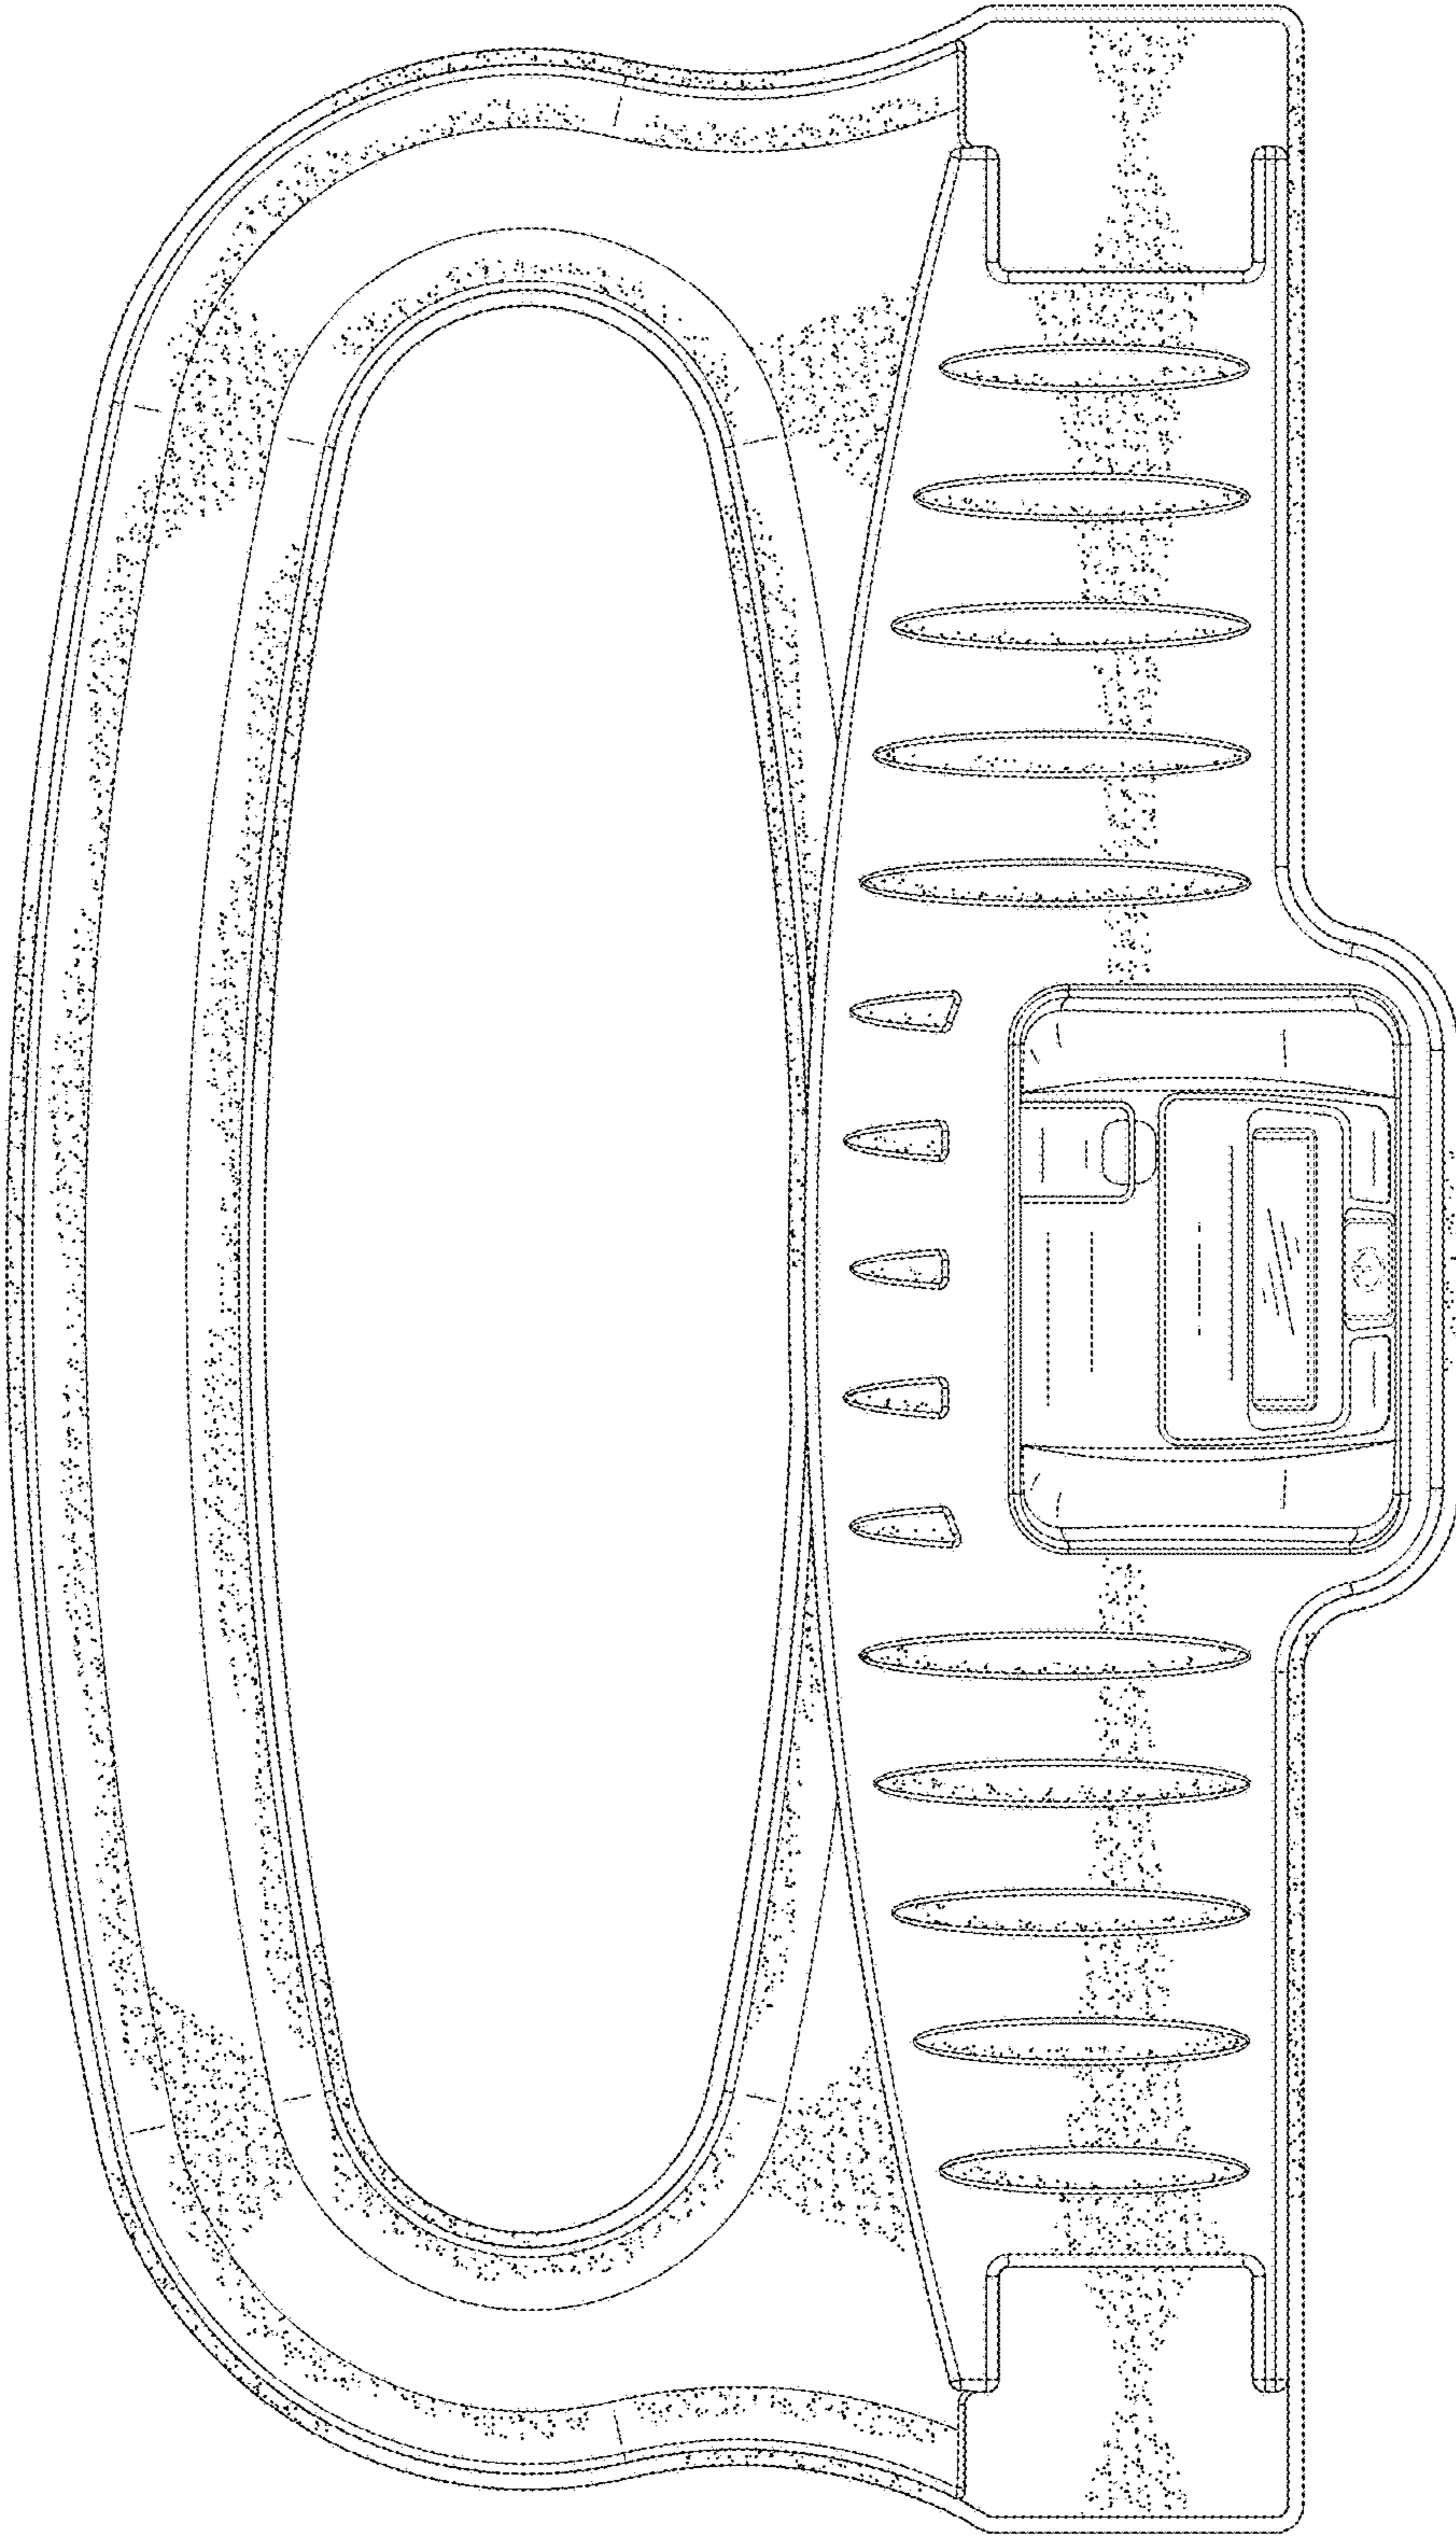


Fig. 2

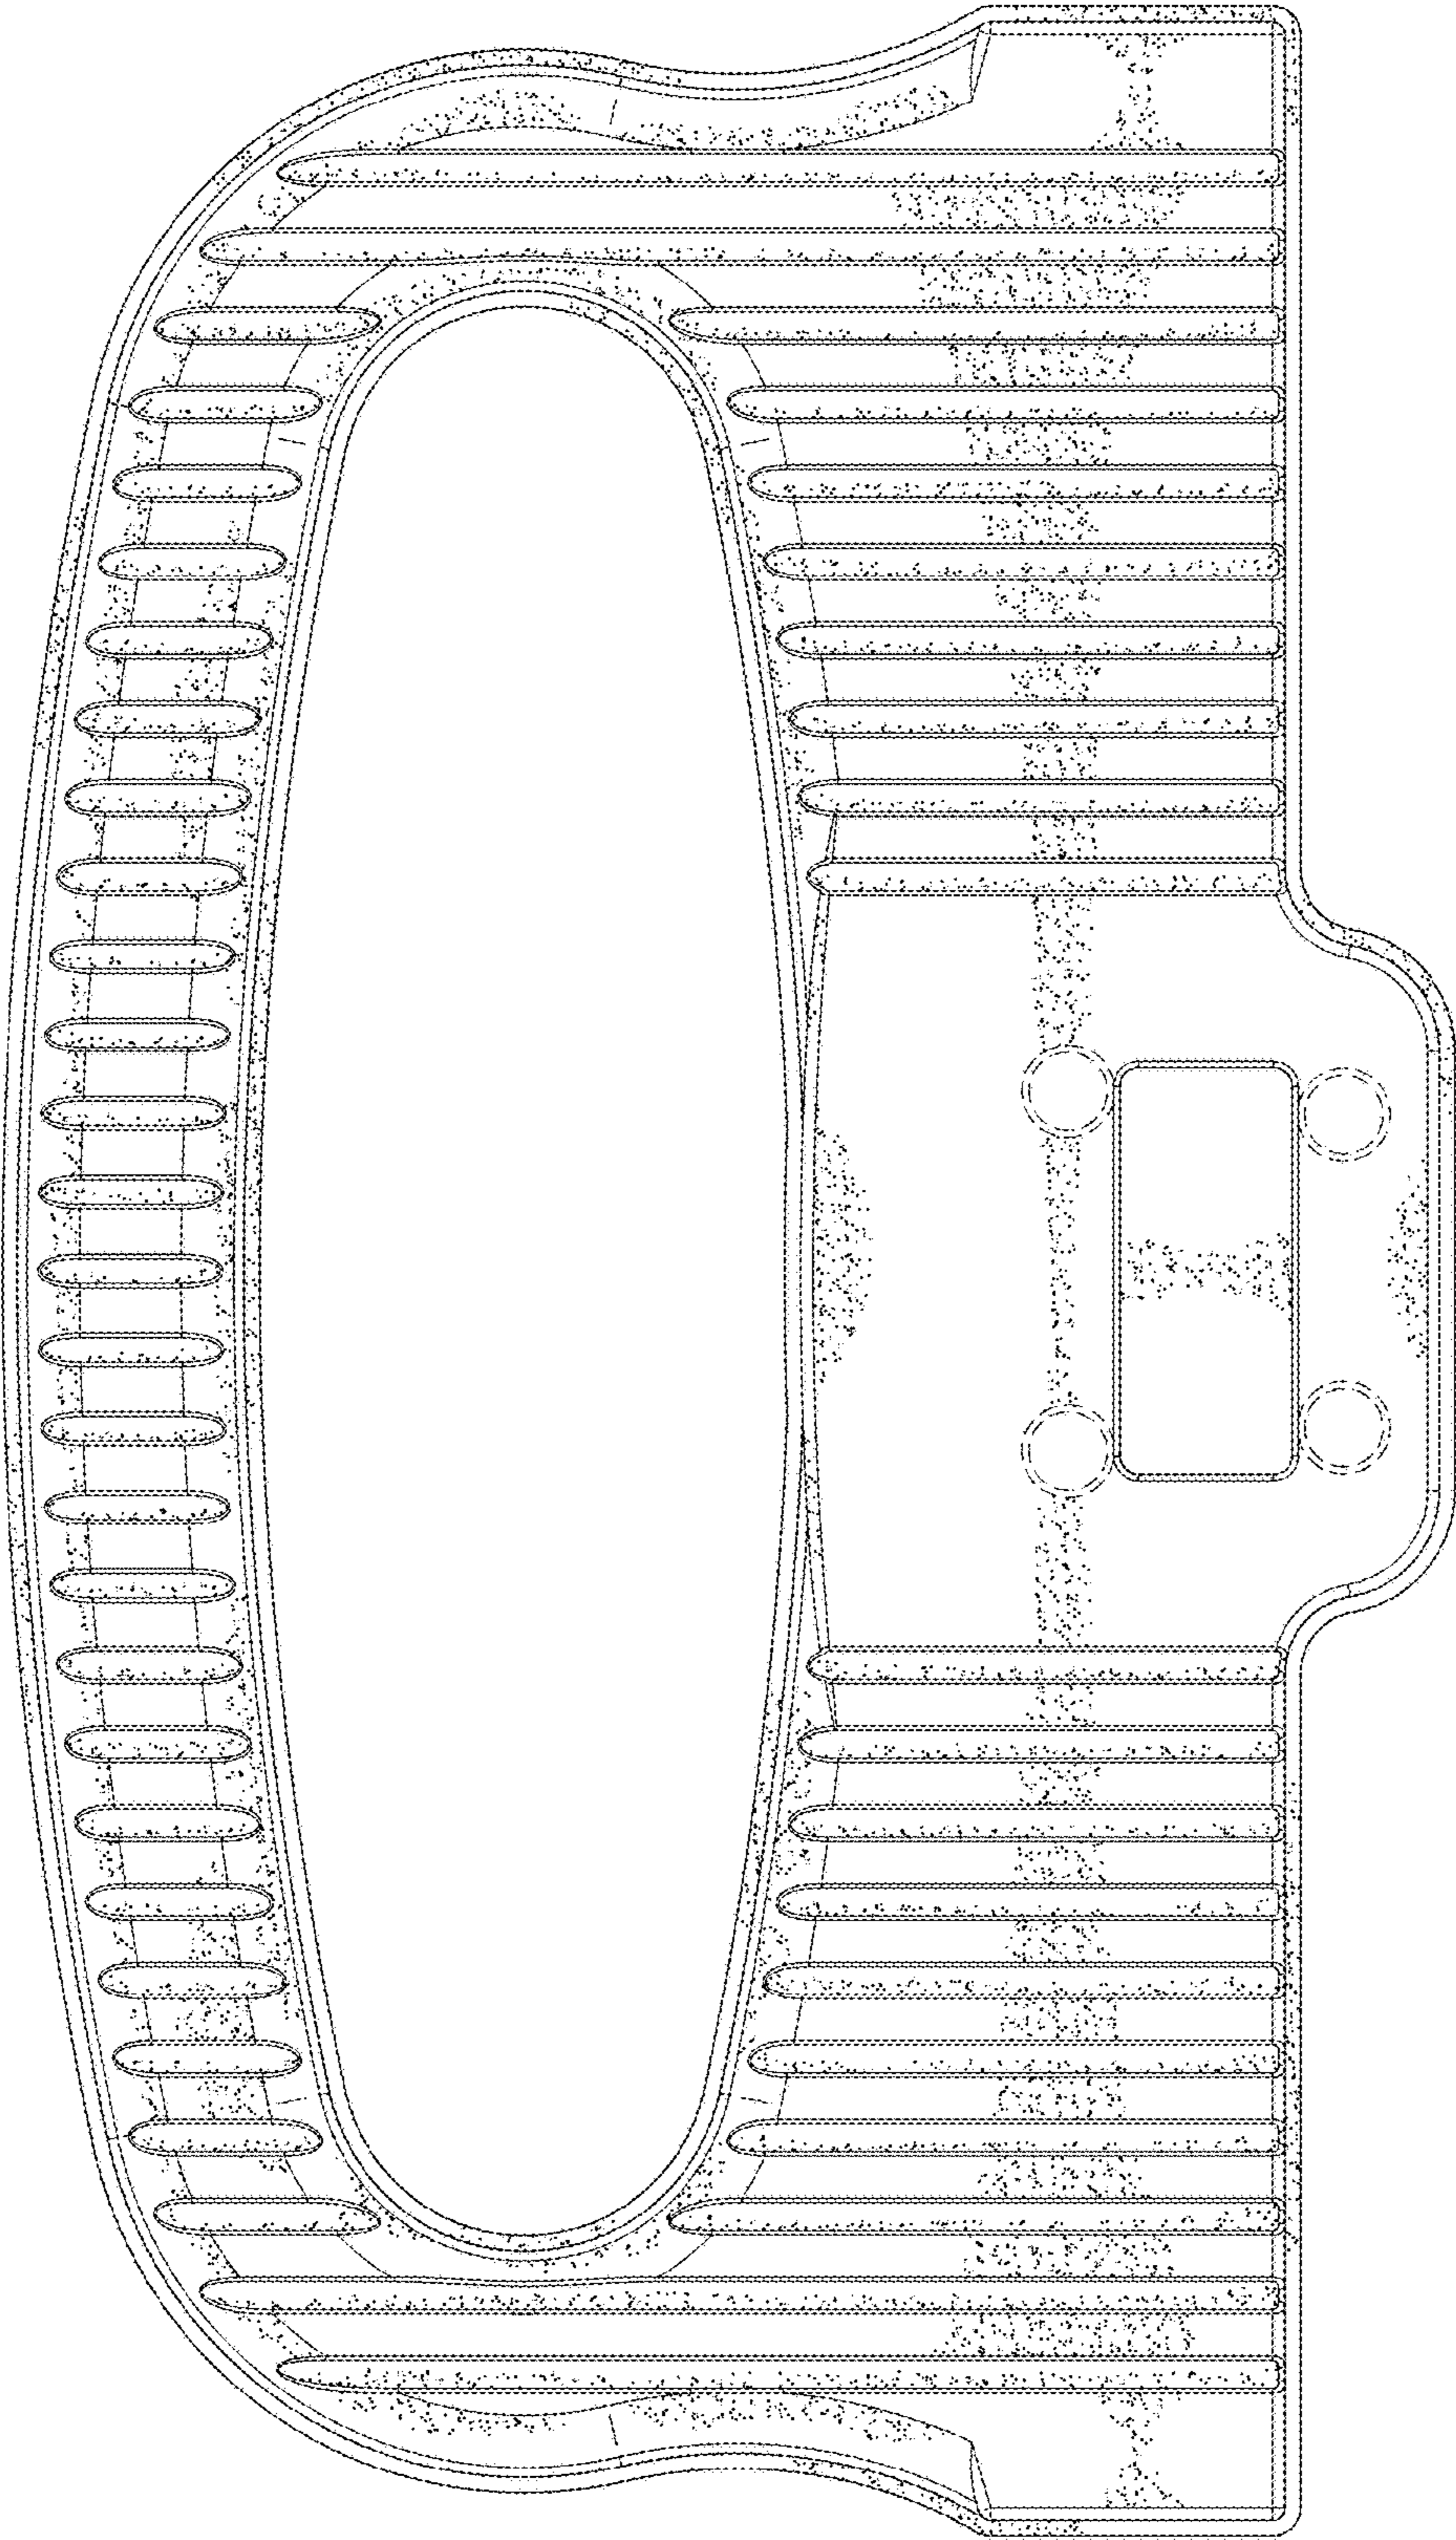


Fig. 3

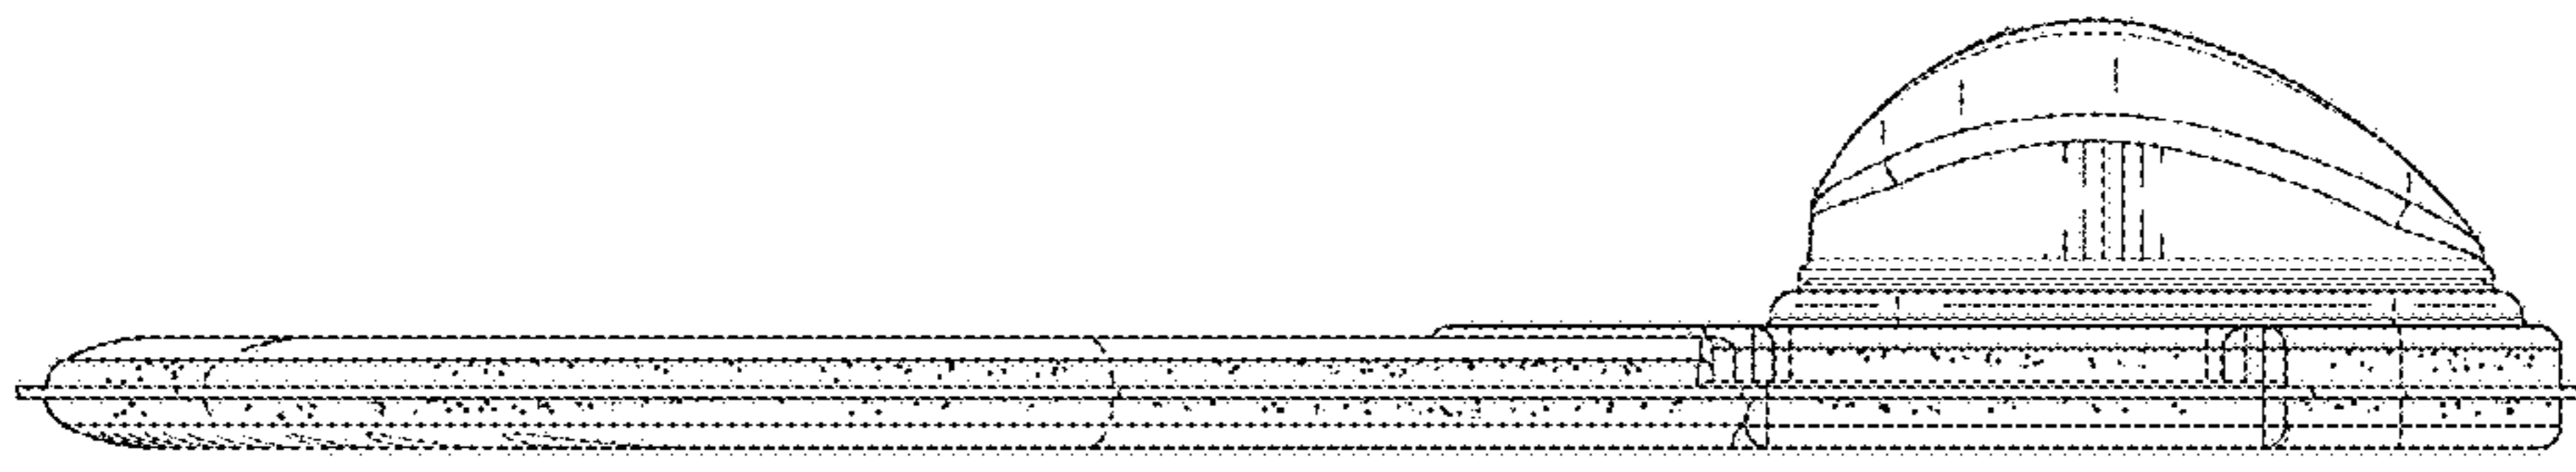


Fig. 5

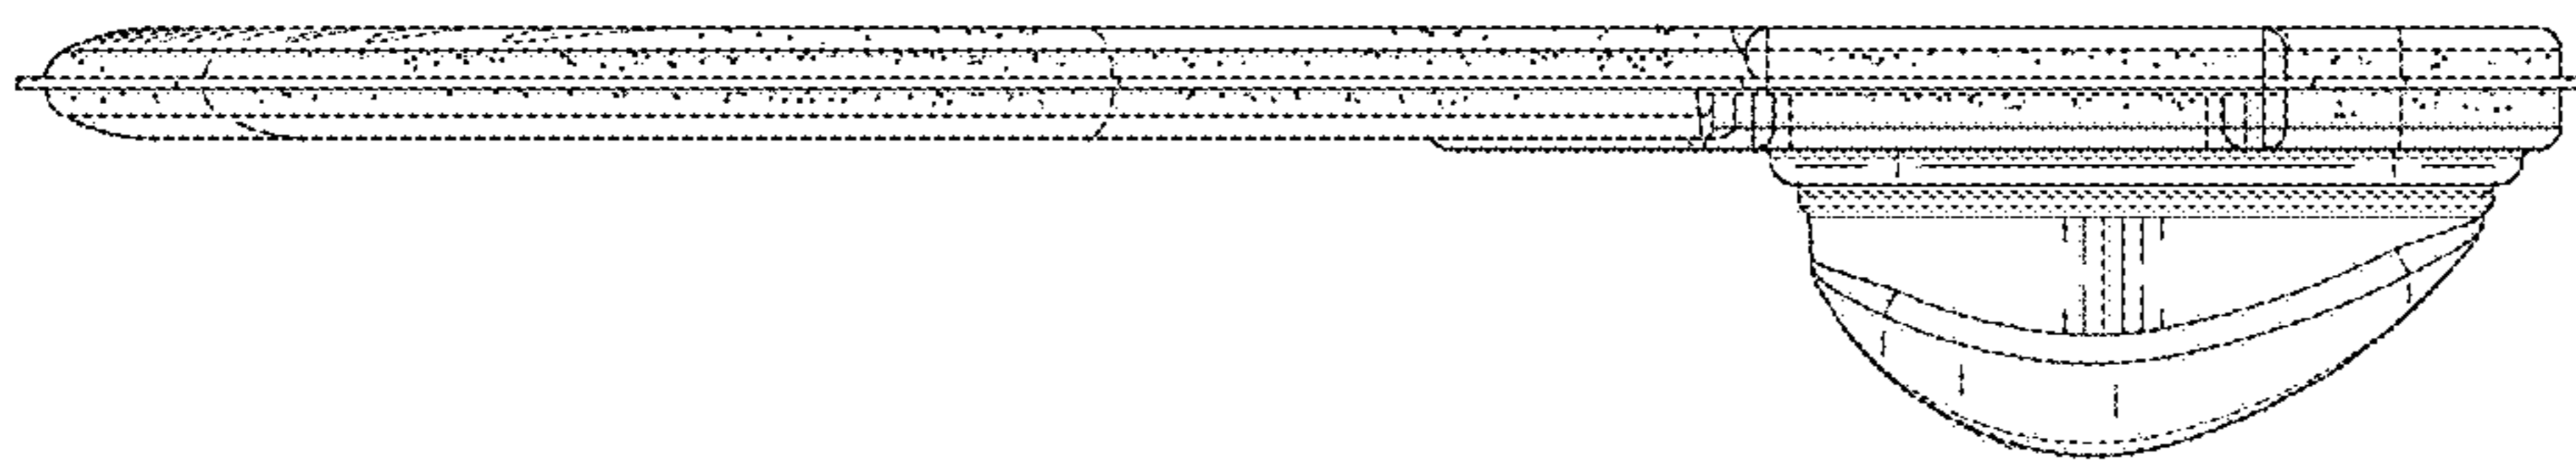


Fig. 4

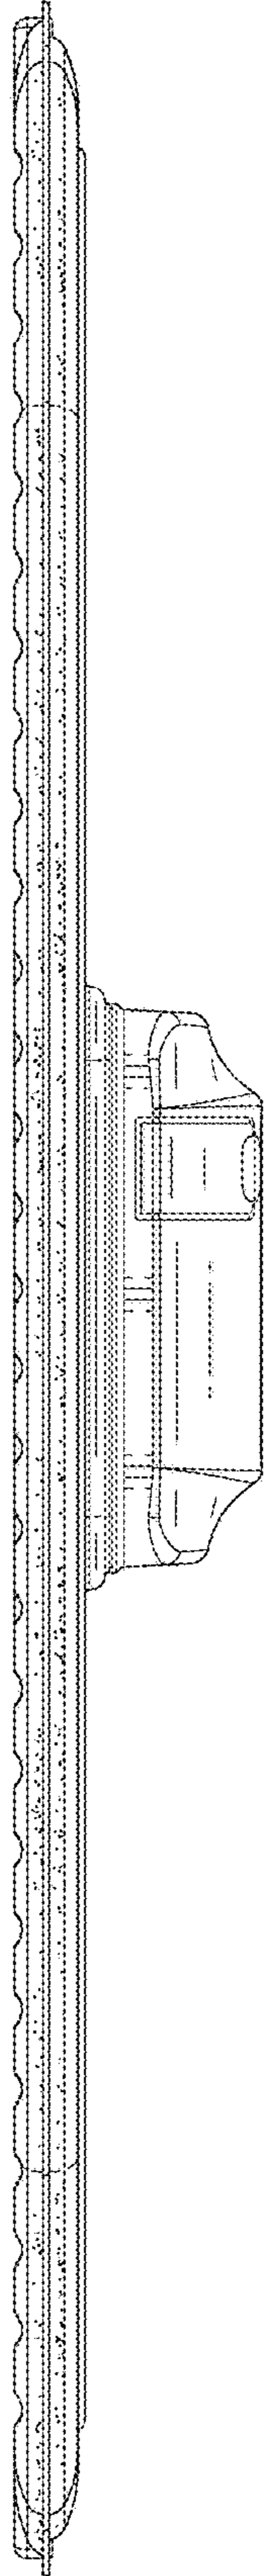


Fig. 6

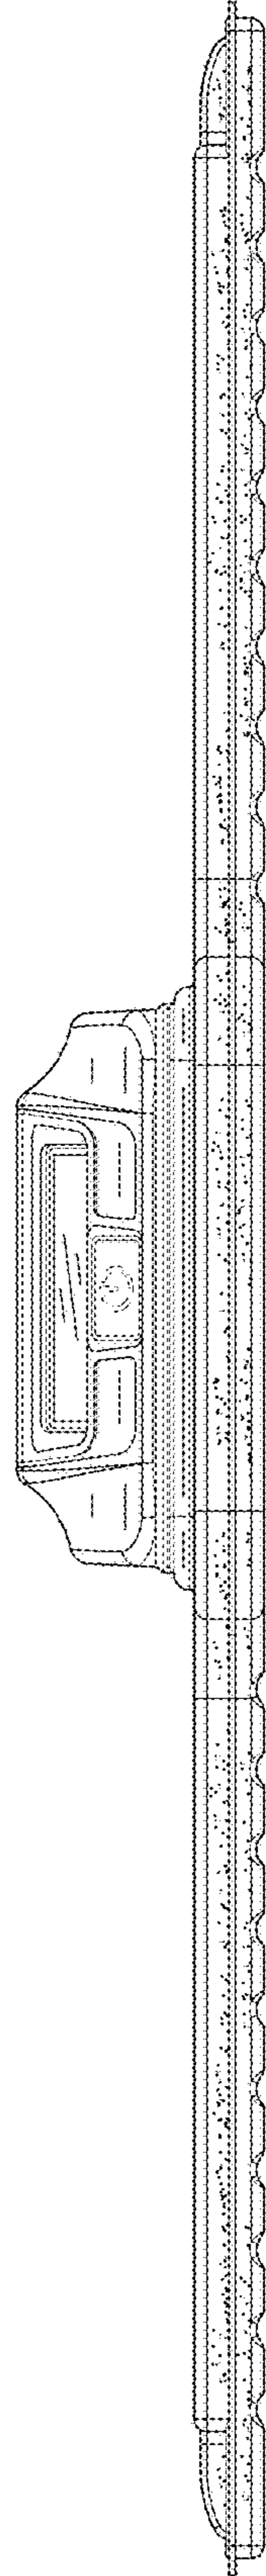


Fig. 7

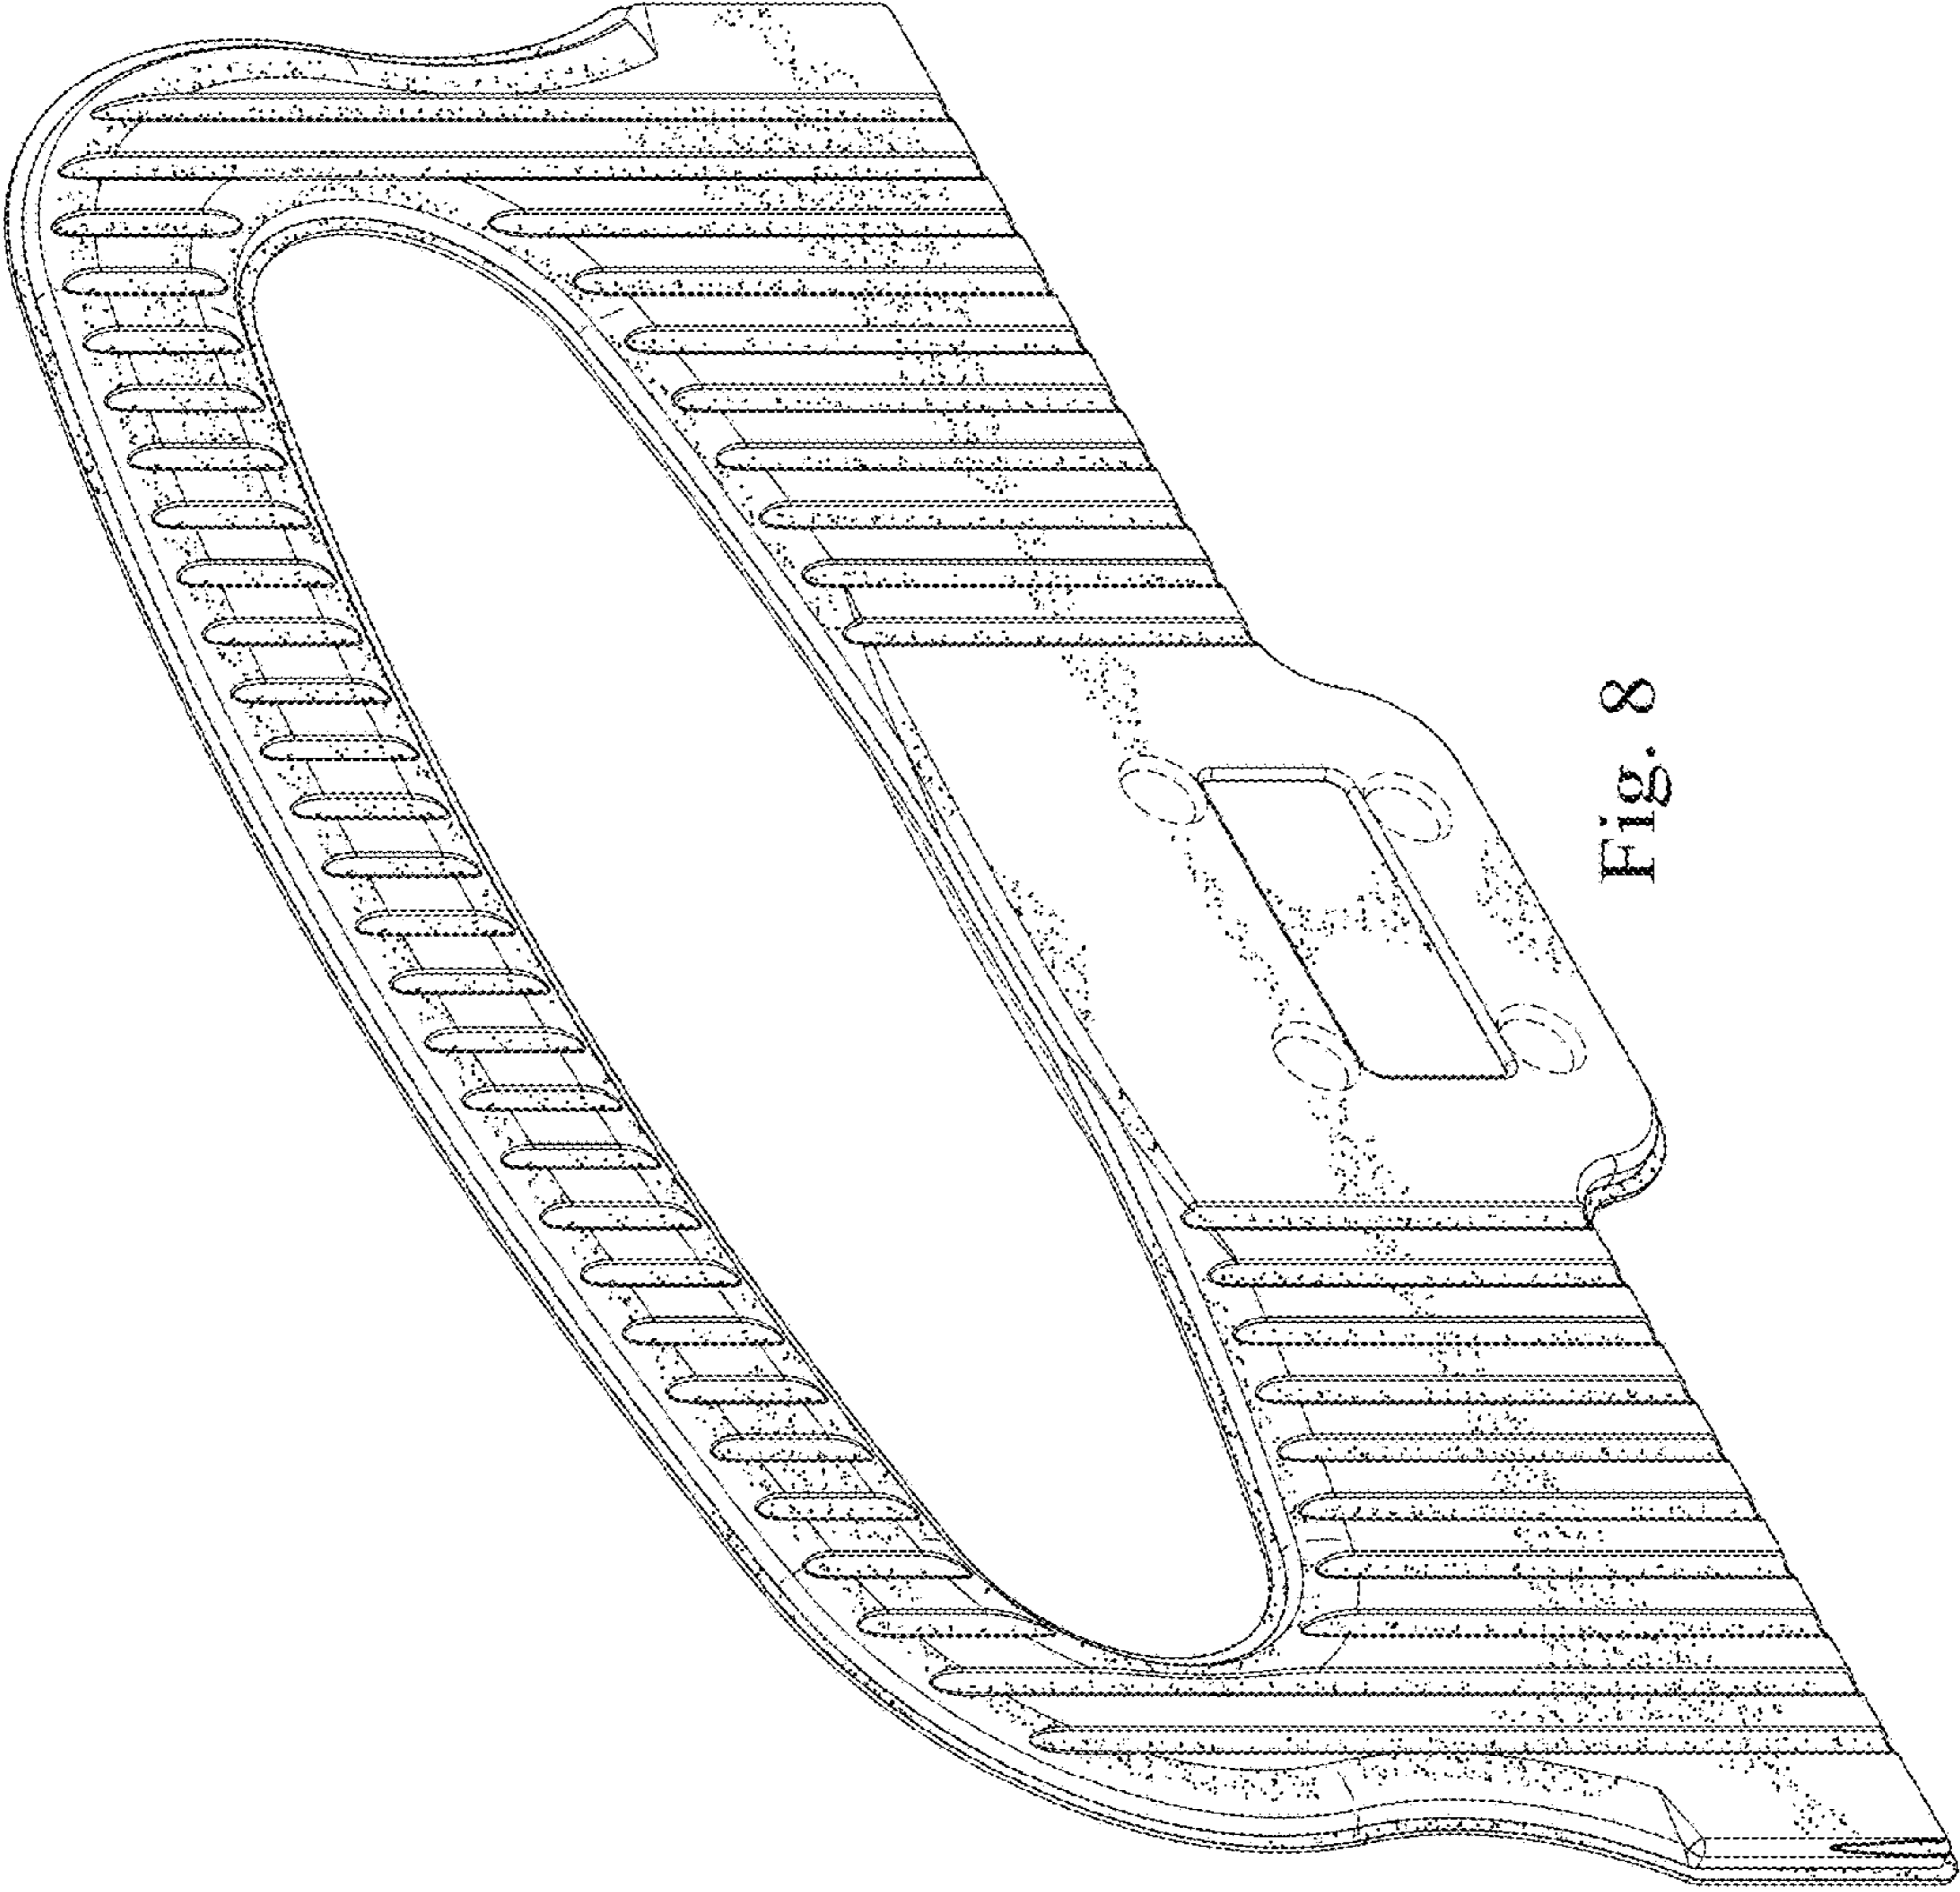


Fig. 8

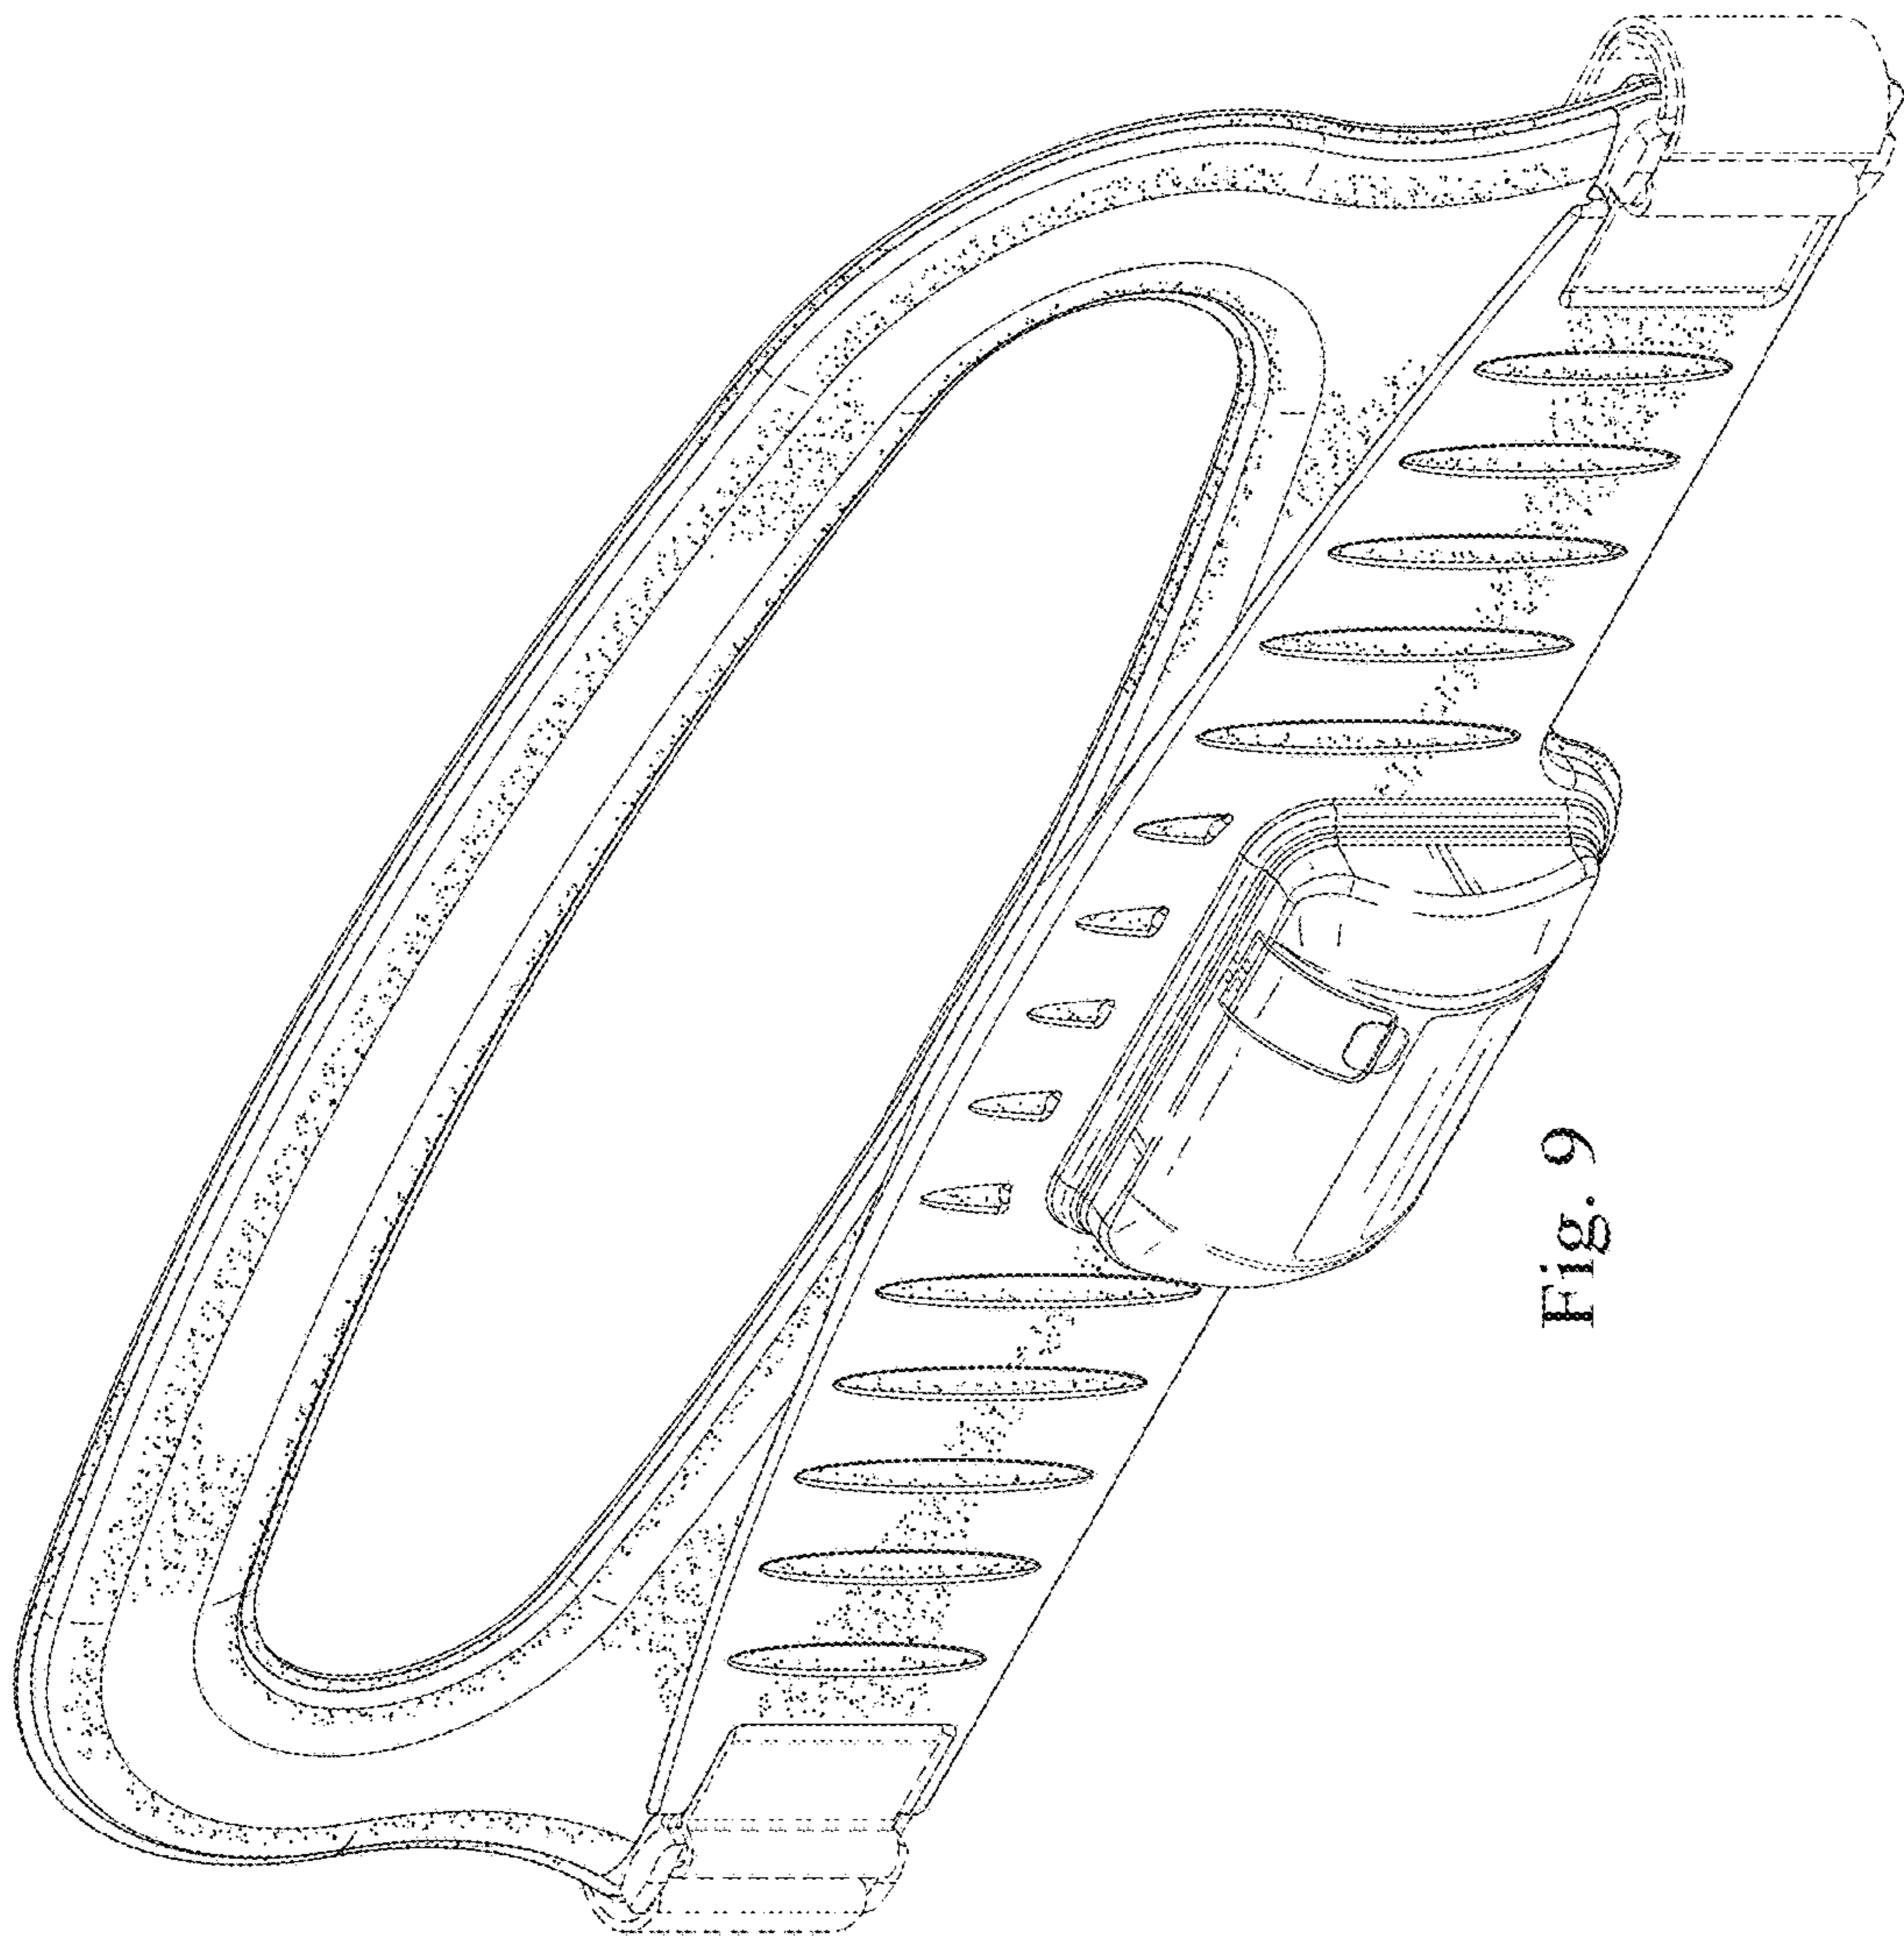


Fig. 9