

US00D860437S

(12) **United States Design Patent** (10) **Patent No.:** **US D860,437 S**
Collins (45) **Date of Patent:** **** Sep. 17, 2019**

(54) **APPARATUS TO CONTROL FLUID FLOW THROUGH A TUBE**

3,831,600 A 8/1974 Buckles
4,038,982 A 8/1977 Burke
4,105,028 A 8/1978 Sadlier
4,155,362 A 5/1979 Jess
4,247,077 A 1/1981 Banick et al.
(Continued)

(71) Applicant: **DEKA Products Limited Partnership**,
Manchester, NH (US)

(72) Inventor: **David E. Collins**, Merrimac, MA (US)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **DEKA Products Limited Partnership**,
Manchester, NH (US)

AU 2247783 A 6/1985
CA 1213749 A1 11/1986
(Continued)

(**) Term: **15 Years**

OTHER PUBLICATIONS

(21) Appl. No.: **29/575,331**

(22) Filed: **Aug. 24, 2016**

“The OpenCV Reference Manual Release 2.3”, May 10, 2011, pp. 1-263.

(Continued)

Related U.S. Application Data

(63) Continuation of application No. 29/565,908, filed on May 25, 2016.

Primary Examiner — Lilyana Bekic

(51) **LOC (12) Cl.** **24-02**

(74) *Attorney, Agent, or Firm* — James D. Wyninegar, Jr.

(52) **U.S. Cl.**
USPC **D24/111**

(57) **CLAIM**

(58) **Field of Classification Search**
USPC D24/107, 108, 111, 169, 185, 186
CPC A61M 5/142; A61M 2205/502; A61M 5/1452; A61M 2205/505; A61M 2205/3331; A61M 2205/3334; A61M 5/168; A61M 5/16886

The ornamental design for an apparatus to control fluid flow through a tube, as shown and described.

DESCRIPTION

See application file for complete search history.

FIG. 1 is a front, top, and right side perspective view of the apparatus to control fluid flow through a tube, showing my new design;

(56) **References Cited**


U.S. PATENT DOCUMENTS

2,880,764 A 4/1959 Pelvavin
2,888,877 A 6/1959 Shellman
3,173,372 A 3/1965 Baldwin
3,384,336 A 5/1968 Pulman
3,609,379 A 9/1971 Hildebrandt
3,685,787 A 8/1972 Adelberg
3,733,149 A 5/1973 Jacobson
3,790,042 A 2/1974 McCormick

FIG. 2 is a front side elevational view thereof;
FIG. 3 is a back side elevational view thereof;
FIG. 4 is a left side elevational view thereof;
FIG. 5 is a right side elevational view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.

The broken lines in the drawings depict portions of the apparatus to control fluid flow through a tube that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

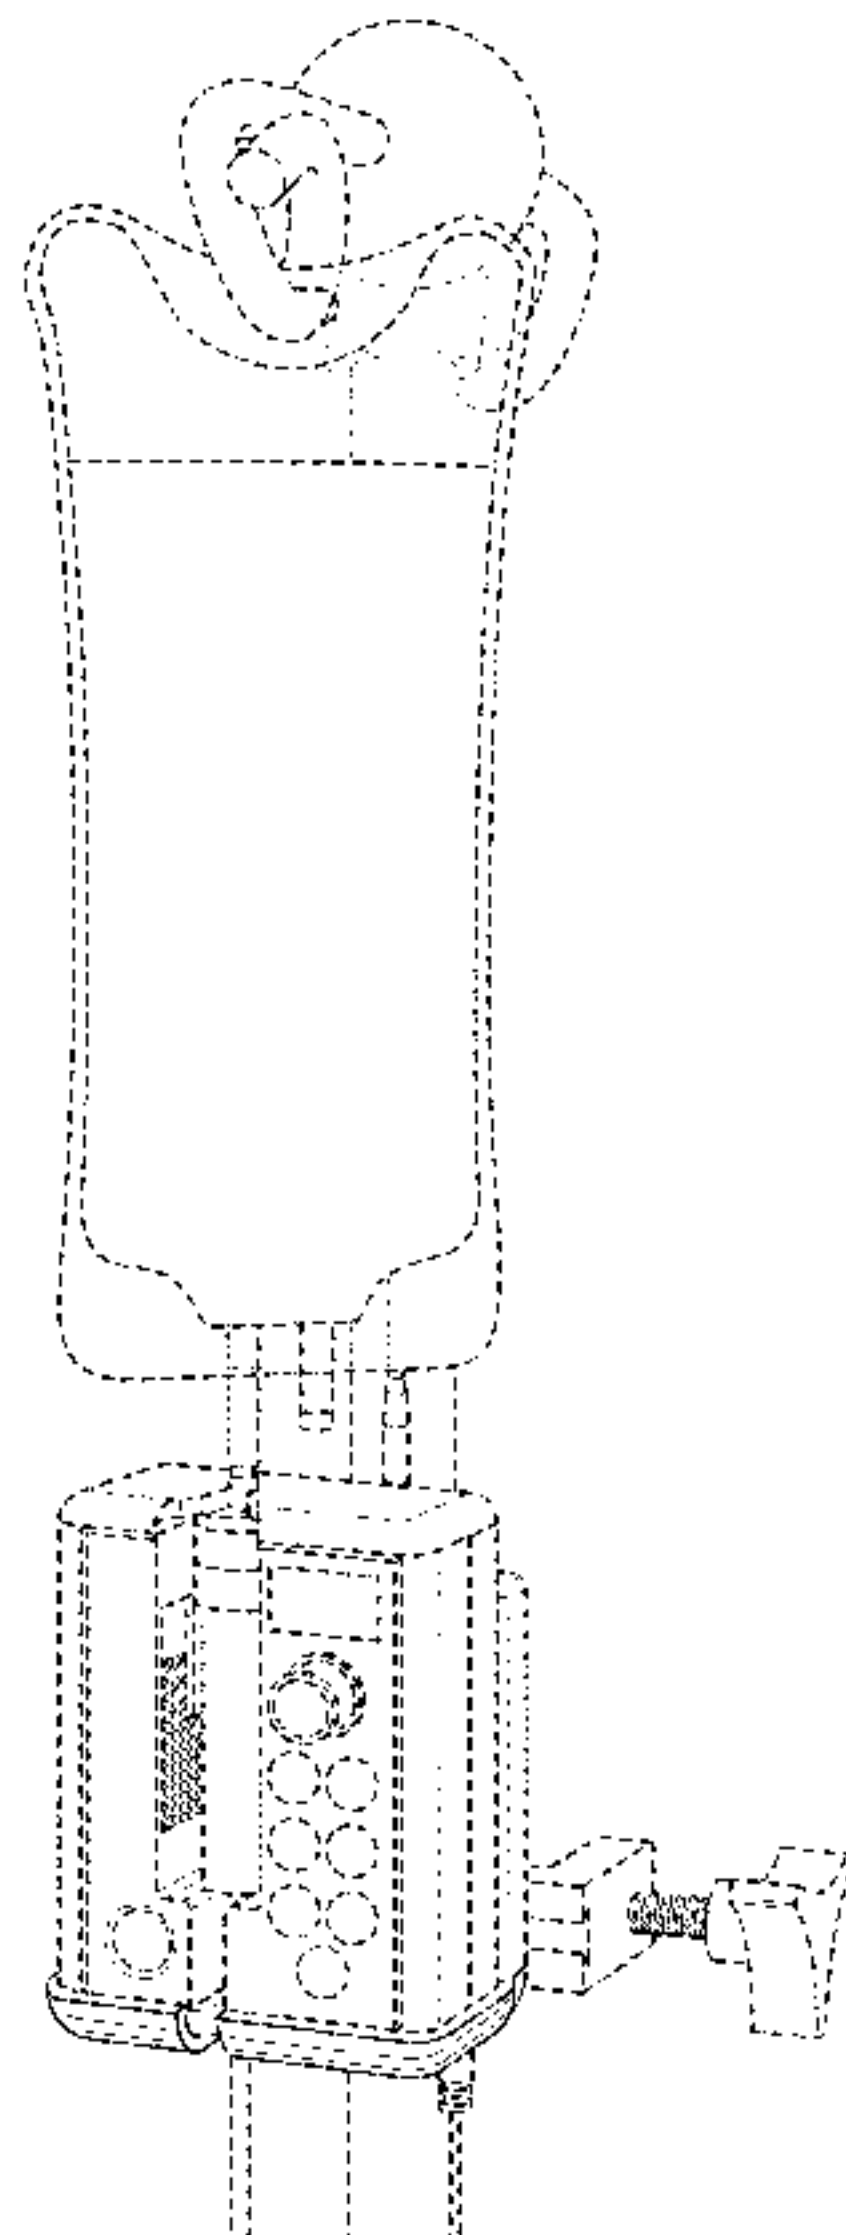

US D860,437 S

(56)

References Cited

U.S. PATENT DOCUMENTS

4,303,376	A	12/1981	Siekmann	5,707,588	A	1/1998	Tsukishima
4,321,461	A	3/1982	Walter	5,718,562	A	2/1998	Lawless
4,328,800	A	5/1982	Marx	5,753,820	A	5/1998	Reed
4,328,801	A	5/1982	Marx	5,782,805	A	7/1998	Meinzer
4,383,252	A	5/1983	Purcell	5,800,140	A	9/1998	Forni
4,397,642	A	8/1983	Lamadrid	5,800,386	A	9/1998	Bellifemine
4,421,506	A	12/1983	Danby	5,814,015	A *	9/1998	Gargano A61M 5/1456
4,449,534	A	5/1984	Leibinsohn Saul				604/67
4,469,480	A	9/1984	Figler	5,843,045	A	12/1998	DuPont
4,490,140	A	12/1984	Carr	5,896,195	A	4/1999	Juvinall
4,496,351	A	1/1985	Hillel et al.	5,899,665	A	5/1999	Makino
4,504,263	A	3/1985	Steuer	5,920,361	A	7/1999	Gibeau
4,525,163	A	6/1985	Slavik	D416,999	S	11/1999	Miyamoto
4,577,197	A	3/1986	Crean	6,015,083	A	1/2000	Hayes
4,583,975	A	4/1986	Pekkarinen	6,049,381	A	4/2000	Reintjes
RE32,294	E	11/1986	Knute	6,050,713	A	4/2000	O'Donnell
4,634,426	A	1/1987	Kamen	6,083,206	A	7/2000	Molko
4,635,281	A	1/1987	Jones	6,091,483	A	7/2000	Guirguis
4,648,869	A	3/1987	Bobo, Jr.	6,091,492	A	7/2000	Strickland
4,662,829	A	5/1987	Nehring	6,110,153	A	8/2000	Davis
4,668,216	A	5/1987	Martin	6,144,453	A	11/2000	Hallerman
4,673,161	A	6/1987	Flynn et al.	6,149,631	A	11/2000	Haydel, Jr.
4,673,820	A	6/1987	Kamen	6,159,186	A	12/2000	Wickham
4,680,977	A	7/1987	Conero	6,213,354	B1	4/2001	Kay
4,703,314	A	10/1987	Spani	6,213,739	B1	4/2001	Phallen et al.
4,718,896	A	1/1988	Arndt	6,228,047	B1	5/2001	Dadson
4,720,636	A	1/1988	Benner, Jr.	D446,860	S	8/2001	Mezière
4,722,224	A	2/1988	Scheller et al.	6,270,478	B1 *	8/2001	Mernøe A61M 5/142
4,775,368	A	10/1988	Iwatschenki				604/122
4,778,451	A	10/1988	Kamen	6,305,908	B1	10/2001	Hermann
4,787,406	A	11/1988	Edwards et al.	6,328,712	B1	12/2001	Cartledge
4,812,904	A	3/1989	Maring	6,362,887	B1	3/2002	Meisberger
4,820,268	A	4/1989	Kawamura	6,491,659	B1	12/2002	Miyamoto
4,820,281	A	4/1989	Lawler	6,500,151	B1	12/2002	Cobb
4,834,744	A	5/1989	Ritson	6,503,221	B1	1/2003	Briggs
4,837,708	A	6/1989	Wright	6,523,414	B1	2/2003	Malmstrom
4,846,792	A	7/1989	Bobo, Jr.	D471,274	S	3/2003	Diaz et al.
4,909,786	A	3/1990	Gijsselhart	6,554,791	B1	4/2003	Cartledge et al.
4,920,336	A	4/1990	Meijer	6,562,012	B1	5/2003	Brown
4,936,828	A	6/1990	Chiang	6,574,050	B1	6/2003	Lin et al.
4,959,050	A	9/1990	Bobo, Jr.	6,599,282	B2	7/2003	Burko
4,979,940	A	12/1990	Bobo, Jr.	6,641,556	B1	11/2003	Shigezawa
4,981,467	A	1/1991	Bobo	6,657,545	B1	12/2003	Lin
5,002,539	A	3/1991	Coble	6,736,801	B1	5/2004	Gallagher
5,045,069	A	9/1991	Imparato	6,810,290	B2	10/2004	Lebel et al.
5,047,014	A	9/1991	Mosebach et al.	6,814,547	B2	11/2004	Childers et al.
5,057,090	A	10/1991	Bessman	6,975,898	B2	12/2005	Seibel
5,083,741	A	1/1992	Sancoff	6,984,052	B1	1/2006	Del Castillo
5,154,693	A	10/1992	East et al.	7,001,365	B2	2/2006	Makkink
5,154,704	A	10/1992	Archibald	7,068,831	B2	6/2006	Florent
5,181,910	A	1/1993	Scanlon	7,070,121	B2	7/2006	Schramm
5,186,057	A	2/1993	Everhart	7,092,796	B2 *	8/2006	Vanderveen G05D 7/0629
RE34,413	E	10/1993	McCullough				604/131
5,267,980	A	12/1993	Dirr, Jr.	7,118,549	B2	10/2006	Chan
5,278,626	A	1/1994	Poole	7,163,740	B2	1/2007	Rosati
5,279,558	A	1/1994	Kriesel	7,190,275	B2	3/2007	Goldberg
D347,472	S *	5/1994	Sunderland D24/111	D564,087	S	3/2008	Yodfat et al.
5,314,316	A	5/1994	Shibamoto	7,338,475	B2	3/2008	Brown
D348,730	S *	7/1994	Walker D24/108	7,420,151	B2	9/2008	Fengler et al.
5,328,341	A	7/1994	Forni	7,448,706	B2	11/2008	Yamanobe
5,331,309	A	7/1994	Sakai	7,467,055	B2	12/2008	Seshimo et al.
D353,667	S *	12/1994	Tsubota D24/111	7,498,563	B2	3/2009	Mandro
D355,716	S *	2/1995	Nash D24/111	7,499,581	B2	3/2009	Tribble
5,411,052	A	5/1995	Murray	7,540,859	B2	6/2009	Claude
5,415,641	A	5/1995	Yerlikaya	7,677,689	B2	3/2010	Kim
5,439,442	A	8/1995	Bellifemine	7,695,448	B2	4/2010	Cassidy
D362,721	S	9/1995	Peeler et al.	7,767,991	B2	8/2010	Sacchetti
5,482,446	A	1/1996	Williamson	7,776,927	B2	8/2010	Chu
D367,527	S *	2/1996	Marston D24/111	7,783,107	B2	8/2010	Zandifar
5,489,265	A *	2/1996	Montalvo A61M 5/141	D629,503	S	12/2010	Caffey et al.
			604/67	7,892,201	B1	2/2011	Laguna
5,526,285	A	6/1996	Campo	7,892,204	B2	2/2011	Kraus
5,562,615	A	10/1996	Nassif	7,905,859	B2	3/2011	Bynum
5,588,963	A	12/1996	Roelofs	7,914,483	B2	3/2011	Simmons
5,601,980	A	2/1997	Gordon	7,918,834	B2	4/2011	Mernoe
				7,924,424	B2	4/2011	Erickson et al.
				7,933,780	B2	4/2011	De La Huerga
				7,952,698	B2	5/2011	Friedrich
				8,004,683	B2	8/2011	Tokhtuev et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,025,634 B1	9/2011	Moubayed		9,677,555 B2	6/2017	Kamen et al.
8,038,657 B2	10/2011	Davis		9,687,417 B2	6/2017	Demers et al.
8,038,663 B2	10/2011	Miner		D792,963 S	7/2017	Gill
8,103,461 B2	1/2012	Glaser et al.		D795,424 S	8/2017	Sloss
8,112,814 B2	2/2012	Shimizu		D795,805 S	8/2017	Gray et al.
8,137,083 B2	3/2012	Zhou		9,719,964 B2	8/2017	Blumberg
8,147,447 B2	4/2012	Sundar et al.		9,724,465 B2	8/2017	Peret et al.
8,147,448 B2	4/2012	Sundar		9,724,466 B2	8/2017	Peret et al.
8,147,464 B2	4/2012	Spohn		9,724,467 B2	8/2017	Peret et al.
8,184,848 B2	5/2012	Wu		9,730,731 B2	8/2017	Langenfeld et al.
8,256,984 B2	9/2012	Fathallah		9,744,300 B2	8/2017	Kamen et al.
8,257,779 B2	9/2012	Abernathy		9,746,093 B2	8/2017	Peret et al.
8,282,894 B2	10/2012	Lee		9,746,094 B2	8/2017	Peret et al.
D676,551 S	2/2013	Desai et al.		9,759,343 B2	9/2017	Peret et al.
D677,784 S	3/2013	Marguerie		9,759,369 B2	9/2017	Gray et al.
8,394,062 B2	3/2013	Powers		9,772,044 B2	9/2017	Peret et al.
8,439,880 B2	5/2013	Rondeau		D799,025 S *	10/2017	Johnson D24/111
8,447,069 B2	5/2013	Huang et al.		D801,519 S	10/2017	Sabin et al.
8,471,231 B2	6/2013	Paz		9,789,247 B2	10/2017	Kamen et al.
8,523,797 B2	9/2013	Lowery et al.		D802,118 S *	11/2017	Peret D24/111
8,523,829 B2	9/2013	Miner et al.		D803,386 S	11/2017	Sabin et al.
8,523,839 B2	9/2013	Siefert		D803,387 S	11/2017	Bodwell et al.
8,529,511 B2	9/2013	Boulanger		D804,017 S	11/2017	Sabin
8,531,517 B2	9/2013	Tao		9,808,572 B2	11/2017	Kamen et al.
8,552,361 B2	10/2013	Mandro		D805,183 S	12/2017	Sabin et al.
8,622,979 B2	1/2014	Hungerford		9,856,990 B2	1/2018	Peret et al.
8,638,358 B2	1/2014	Dabiri et al.		D813,376 S *	3/2018	Peret D24/111
8,647,074 B2	2/2014	Moberg et al.		D814,021 S	3/2018	Sabin
8,692,678 B2	4/2014	Warner et al.		D815,730 S *	4/2018	Collins D24/111
8,733,178 B2 *	5/2014	Bivans A61M 5/14228		D816,685 S	5/2018	Kendler et al.
		73/169		D816,829 S *	5/2018	Peret D24/111
				D817,479 S	5/2018	Sabin et al.
8,777,897 B2	7/2014	Butterfield		D817,480 S	5/2018	Sabin et al.
D712,043 S	8/2014	Sliger		9,968,730 B2	5/2018	Blumberg, Jr. et al.
8,834,429 B2	9/2014	Grant		9,976,665 B2	5/2018	Peret et al.
D720,449 S	12/2014	Galbraith et al.		10,044,791 B2	8/2018	Kamen et al.
D728,779 S	5/2015	Sabin et al.		2001/0026292 A1	10/2001	Ishizaki
D735,319 S	7/2015	Sabin et al.		2001/0055462 A1	12/2001	Seibel
D736,370 S	8/2015	Sabin et al.		2002/0194933 A1	12/2002	Roelofs
9,095,652 B2	8/2015	Dewey		2003/0045840 A1	3/2003	Burko
9,128,051 B2	9/2015	Bui		2003/0055406 A1	3/2003	Lebel
9,134,735 B2	9/2015	Lowery et al.		2003/0107819 A1	6/2003	Lin et al.
9,134,736 B2	9/2015	Lowery et al.		2003/0217962 A1	11/2003	Childers
9,144,644 B2	9/2015	Hungerford		2004/0044306 A1	3/2004	Lynch et al.
9,151,646 B2	10/2015	Kamen et al.		2004/0171994 A1	9/2004	Goldberg
D745,661 S	12/2015	Collins et al.		2005/0096581 A1	5/2005	Chan
9,216,279 B2	12/2015	Travis et al.		2005/0171491 A1	8/2005	Minh Miner et al.
9,234,850 B2	1/2016	Hammond et al.		2006/0096660 A1	5/2006	Diaz
D749,206 S	2/2016	Johnson et al.		2006/0140466 A1	6/2006	Seshimo
D751,689 S	3/2016	Peret et al.		2006/0146077 A1	7/2006	Song
D751,690 S	3/2016	Peret et al.		2006/0291211 A1	12/2006	Rodriguez
D752,209 S	3/2016	Peret et al.		2007/0088269 A1	4/2007	Valego et al.
9,295,778 B2	3/2016	Kamen et al.		2007/0102623 A1	5/2007	Fengler
D754,065 S	4/2016	Gray et al.		2007/0228071 A1	10/2007	Kamen et al.
D756,386 S	5/2016	Kendler et al.		2007/0293817 A1	12/2007	Feng
D756,505 S	5/2016	Park		2008/0004574 A1	1/2008	Dyar
D758,399 S	6/2016	Kendler et al.		2008/0051732 A1	2/2008	Chen
D760,288 S	6/2016	Kendler et al.		2008/0147008 A1	6/2008	Lewis
D760,289 S	6/2016	Kendler et al.		2008/0147016 A1	6/2008	Faries
9,364,394 B2	6/2016	Demers et al.		2008/0154214 A1	6/2008	Spohn
9,372,486 B2	6/2016	Peret et al.		2008/0235765 A1	9/2008	Shimizu
D760,782 S	7/2016	Kendler et al.		2008/0237502 A1	10/2008	Fago
D760,888 S	7/2016	Gill et al.		2008/0252472 A1	10/2008	Su et al.
9,400,873 B2	7/2016	Kamen et al.		2009/0097029 A1	4/2009	Tokhtuev
9,408,966 B2	8/2016	Kamen		2009/0112115 A1	4/2009	Huang
D767,756 S	9/2016	Sabin		2009/0180106 A1	7/2009	Friedrich
9,435,455 B2	9/2016	Peret et al.		2009/0224638 A1	9/2009	Weber
D768,716 S	10/2016	Kendler et al.		2009/0254025 A1	10/2009	Simmons
9,465,919 B2	10/2016	Kamen et al.		2009/0262351 A1	10/2009	Erickson
9,468,716 B2 *	10/2016	Hariharsan A61M 5/14232		2009/0276167 A1	11/2009	Glaser
9,488,200 B2	11/2016	Kamen et al.		2009/0281460 A1	11/2009	Lowery
D774,645 S	12/2016	Gill et al.		2010/0021933 A1	1/2010	Okano
9,518,958 B2	12/2016	Wilt et al.		2010/0097451 A1	4/2010	Bruce
9,636,455 B2	5/2017	Kamen et al.		2010/0114027 A1	5/2010	Jacobson
D789,516 S	6/2017	Gill et al.		2010/0120601 A1	5/2010	Hayamizu
9,675,756 B2	6/2017	Kamen et al.		2010/0168671 A1	7/2010	Faries, Jr.
				2010/0204650 A1	8/2010	Hungerford et al.
				2010/0211003 A1	8/2010	Sundar
				2010/0217229 A1	8/2010	Miner

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	2319551	A2	5/2011
EP	2793977	B1	11/2015
FR	2042606	A1	2/1971
FR	2273264	A1	12/1975
FR	2458804		1/1981
FR	2617593		1/1989
GB	1301033	A	12/1972
GB	2020735	A	11/1979
GB	2207239	B	1/1989
GB	2328982	A	3/1999
JP	58163843		9/1983
JP	04-280582	A	10/1992
JP	3110458	B2	11/2000
JP	2007229928	A	9/2007
JP	2009298012	A	12/2009
JP	2011062371	A	3/2011
KR	1020050039780	A	4/2005
KR	1020060111424	A	10/2006
KR	1020100037914	A	4/2010
NL	7006908		11/1970
NL	8801680	A	2/1989
NL	9101825	A	5/1993
SE	376843	B	6/1975
WO	WO1981002770	A1	10/1981
WO	WO1993009407	A1	5/1993
WO	WO2000072181	A3	11/2000
WO	WO2002040084	A2	5/2002
WO	WO2002100262	A1	12/2002
WO	WO2004035116	A1	4/2004
WO	WO2005094919	A1	10/2005
WO	WO2006086723	A2	8/2006
WO	WO2008022880	A1	2/2008
WO	WO2008079023	A1	7/2008
WO	WO2009039203	A2	3/2009
WO	WO2009039214	A2	3/2009
WO	WO2009055639	A2	4/2009
WO	WO2010020397	A1	4/2010
WO	WO2010129720	A2	11/2010
WO	WO2011021098	A1	2/2011
WO	WO2011136667	A1	11/2011
WO	WO2012104779	A1	8/2012
WO	PCT/US12/71142		12/2012
WO	WO2013017949	A2	2/2013
WO	WO2013070337	A1	5/2013
WO	WO2013095459	A9	6/2013
WO	WO2013096713	A2	6/2013
WO	WO2013096718	A2	6/2013
WO	WO2013096722	A2	6/2013
WO	WO2013096909	A2	6/2013
WO	WO2013176770	A2	11/2013
WO	WO2013177357	A1	11/2013
WO	PCT/US14/29020		3/2014
WO	WO2014100557	A2	6/2014
WO	WO2014100571	A2	6/2014
WO	WO2014100658	A1	6/2014
WO	WO2014100687	A2	6/2014
WO	WO2014100736	A2	6/2014
WO	WO2014100744	A2	6/2014
WO	WO2014144557	A2	9/2014
WO	WO2014025736	A1	10/2014
WO	WO2014160058	A2	10/2014
WO	WO2014160249	A1	10/2014
WO	WO2014160307	A1	10/2014
WO	WO2015017275	A1	2/2015
WO	WO2015116557	A1	8/2015
WO	PCT/U S2017/15382		1/2017

OTHER PUBLICATIONS

Invitation to Respond to Written Opinion from the Intellectual Property Office of Singapore for Application 11201507504S, dated Nov. 23, 2015.

First Examination Report from the Intellectual Property Office of New Zealand for Application 626382, dated Apr. 1, 2015.

Report of substantive examination from Superintendent of Industry and Commerce of Colombia for Patent Application 14155193, dated Nov. 19, 2015.

Notice of Preliminary Rejection (Non-Final) from the Korean Intellectual Property Office (“KIPO”) for Korean Patent Application No. 10-2014-7019883, dated Dec. 15, 2015.

First Examination report from the New Zealand Intellectual Property Office for New Zealand IP No. 715098, dated Jan. 12, 2016.

“Microcomputer Intravenous Infusion Drip Controller”, Longfian Scitech Co., Ltd., Mar. 18, 2016 (retrieved). Advertisement listed as having a valid price starting at Mar. 10, 2016, 2 pgs, <http://marina.en.made-in-china.com/productimage/bKvQTtJcJEhs-2f1j00FZetfT-SdnhcU/China-Microcomputer-Intravenous-Infusion-Drip-Controller.html>.

“DripAssist Specificaiton”, Shift Labs, Mar. 18, 2016 (retrieved). 2 pgs, <http://www.shiftlabs.com/products/dripassist/specifications>.

“DripAssist Product Overview”, Shift Labs, Mar. 18, 2016 (retrieved). 2 pgs, <http://www.shiftlabs.com/products/dripassist/overview>.

“DripAssist Product Brochure”, Shift Labs, Mar. 18, 2016 (retrieved). 1 pg., <http://www.shiftlabs.com/sites/default/files/DripAssistOnesheet.pdf>.

“IUV Drip monitor”, Allison Lipper, Mar. 18, 2016 (retrieved). 3 pgs., <http://cnx.org/contents/WmaFki2-@3/IV-Drip-Monitor>.

“AutoClamp”, Ace Medical, Mar. 18, 2016 (retrieved). 2 pgs., http://ace-medical.com/2014/en/product/product/view.asp?po_no=31.

Extended European Search Report dated Mar. 3, 2016, received in European patent application No. 15192051.9, 7 pgs.

Notice of Eligibility for Grant from the Intellectual Property Office of Singapore for Application 11201507504S, dated Jun. 6, 2016, 12 pgs.

Second Office Action and Search Report dated 27 Jun. 2016, received in Republic of China patent application No. 201280069373.3, 6 pgs.

First Office Action dated 20 Oct. 2015, received in Republic of China patent application No. 201280069373.3, 4 pgs.

First Office Action dated Jul. 28, 2016, received in Australian patent application No. 2012358397, 3 pgs.

European Community Design Registration 002381699/0.01-0005, Filed Jan. 8, 2014 and published on May 12, 2016, 42 pgs.

Notification from the Eurasian Patent Organization for Application 201491218, dated Apr. 27, 2015, 2 pgs.

Second Report of substantive examination from Superintendent of Industry and Commerce of Colombia for Patent Application 14.155.193, dated Sep. 8, 2016, 18 pgs.

First Examination Report from IP Australia for Patent Application 2012358397, dated Jul. 28, 2016, 3 pgs.

Notice of Acceptance from IP Australia for Patent Application 2012358397, dated Jan. 5, 2017, 3 pgs.

English Search Report from the People’s Republic of China for Patent Application 201280069373.3, dated Jul. 12, 2016, 2 pgs.

First Examination Report from Mexican Patent Office for Patent Application Mx/a/2014/007751, dated Sep. 8, 2016, 5 pgs.

Further Examination Report from the New Zealand Intellectual Property Office for Patent Application 626382, dated Jan. 12, 2016, 2 pgs.

Notice of Acceptance from the New Zealand Intellectual Property Office for Patent Application 626382, dated Feb. 9, 2016, 1 pg.

Rule 161 Communication from the European Patent Office for Patent Application 14720397.0-1662, dated Oct. 28, 2015, 2 pgs.

Decision to Grant from the European Patent Office for Patent Application 15192051.9-1664/3006010, dated Jan. 19, 2017, 3 pgs.

Further Examination Report from the New Zealand Intellectual Property Office for Patent Application 715098, dated Jun. 13, 2016, 2 pgs.

Notice of Acceptance from the New Zealand Intellectual Property Office for Patent Application 715098, Sep. 9, 2016, 3 pgs.

Notice of Acceptance from the New Zealand Intellectual Property Office for Patent Application 723930, dated Nov. 16, 2016, 3 pgs.

Notice of Acceptance from IP Australia for Patent Application 2016225879, dated Oct. 26, 2016, 3 pgs.

First Examination Report from the New Zealand Intellectual Property Office for Patent Application 725469, dated Nov. 8, 2016, 2 pgs.

(56)

References Cited

OTHER PUBLICATIONS

AAMI and FDA, Infusing Patients Safely: Priority Issues from the AAMI/FDA Infusion Device Summit, Symposium, Oct. 5-6, 2010, pp. 1-48, AAMI, Arlington, VA, USA.

Conway, "Analytical Analysis of Tip Travel in a Bourdon Tube", Master's Thesis, Naval Postgraduate School Monterey, Dec. 1995, pp. i-89.

Darzynkiewicz, 'Cytometry', Methods in Cell Biology, 2011, Third Edition Part A, vol. 63, pp. 44-48, Academic Press, San Diego, 2001. And please see whole document generally.

"Feature Detection", OpenCV Wiki, Oct. 31, 2011 (retrieved), 7 pgs, http://opencv.willowgarage.com/documentation/cpp/imgproc_feature_detection.html.

International Search Report & Written Opinion dated Jun. 18, 2013, received in International patent application No. PCT/US2012/071142, 14 pgs.

International Search Report & Written Opinion dated Oct. 1, 2013, received in International patent application No. PCT/US2012/071490, 19 pgs.

International Search Report & Written Opinion dated Nov. 7, 2013, received in International patent application no. PCT/US2013/042350, 18 pgs.

Invitation to Pay Additional Fees and, Where Applicable, Protest Fee dated Sep. 9, 2013, received in International patent application No. PCT/US2013/032445, 10 pgs.

Invitation to Pay Additional Fees and, Where Applicable, Protest Fee dated Sep. 26, 2013, received in International patent application No. PCT/US2013/042350, 7 pgs.

International Preliminary Report on Patentability dated Jul. 3, 2014, received in International patent application No. PCT/US2012/071142, 9 pgs.

International Search Report dated Feb. 2015, received in International patent application No. PCT/US2014/029020, 7 pgs.

International Preliminary Report on Patentability and Written Opinion, dated Sep. 15, 2015, received in International patent application No. PCT/US2014/029020, 11 pgs.

Hofmann, "Modeling Medical Devices for Plug-and-Play Interoperability", MIT Department of Electrical Engineering and Computer Science, Jun. 2007, pp. 1-187.

King et al. Prototyping closed loop physiologic control with the medical device coordination framework. In SEHC 2010: Proceedings of the 2010 ICSE Workshop on Software Engineering in Health Care (pp. 1-11). New York, Ny: ACM. (2010).

Jetley et al., "Safety Requirements Based Analysis of Infusion Pump Software", Proceedings of the IEEE Real Time Systems Symposium, Tuscon, Dec. 2007 pp. 1-4.

FDA US Food and Drug Administration, "SEDASYS® Computer-Assisted Personalized Sedation System P08000", Jul. 16, 2013, pp. 1-2, www.fda.gov/MedicalDevices/ProductsandMedicalProcedures/DeviceApprovalsandClearances/Recently-ApprovedDevices/ucm353950.htm.

Luerkens, David W. "Theory and Application of Morphological Analysis: Fine Particles and Surfaces". Boca Raton: CRC, 1991. 5-7.

Matas et al., 'Progressive Probabilistic Hough Transform', University of Surrey, Czech Technical University, 1998, pp. 1-10.

"Miscellaneous Image Transformations", OpenCV Wiki, 2011, 9 pgs., http://opencv.willowgarage.com/documentation/cpp/miscellaneous_image_transformations.

National Patient Safety Agency, Design for Patient Safety: A Guide to the Design of Electronic Infusion Devices, booklet, 2010, pp. 1-96, Edition 1, National Patient Safety Agency, London.

"Object Detection", OpenCV Wiki, 2011, 2 pgs., http://opencv.willowgarage.com/documentation/cpp/object_detection.html.

"The OpenCV Reference Manual Release 2.4.6.0", Jul. 1, 2013, pp. 1-813.

Leor at al., "A System for the Measurement of Drop Volume of Intravenous Solutions", Proceedings Computers in Cardiology 1990, pp. 405-406, Los Alamitos, California.

Butterfield, "Alaris SE Pump, Monitoring and Detection of IV Line Occlusions.", CareFusion Corporation, 2010, 4 pgs.

"Vista Basic: Instructions for Use: Software Ifvb", manual, 2002, pp. 3, B. Braun Medical Inc.

Hugli et al., "Drop volume measurement by vision." Proceedings of SPIE Electronic Imaging Conference, San Diego, Jan. 2000. SPIE vol. 3866-11, pp. 60-66.

Notification of Non-Compliance With Substantive Requirements and Invitation to Submit Observations and/or Amended Application from The African Regional Intellectual Property Organization (ARIPO) for Application AP/P/2014/007721 (J79AP), dated Apr. 25, 2017. Results of Substantive Examination from IMPI for Application MX/a/2014/007751, dated Mar. 31, 2017.

First Office Action for Chinese Patent Application 201610248658.3 (R81CN), dated Feb. 13, 2017.

International Search Report & Written Opinion dated Jul. 6, 2017, received in International patent application No. PCT/US2017/015382, 21 pgs.

Notification from the Eurasian Patent Organization for Application 201491218/32, date Apr. 19, 2017, 1 pg.

Examination Report from the European Patent Office for EPO Application No. 16 167 576.4-1662, dated Oct. 11, 2016, 6 pgs.

U.S. Appl. No. 61/679,117, filed Aug. 3, 2012.

U.S. Appl. No. 13/834,030, filed Mar. 15, 2013.

U.S. Appl. No. 61/900,431, filed Nov. 6, 2013.

U.S. Appl. No. 29/552,943, filed Jan. 27, 2016.

U.S. Appl. No. 62/288,132, filed Jan. 28, 2016.

U.S. Appl. No. 29/553,094, filed Jan. 28, 2016.

U.S. Appl. No. 29/565,908, filed May 25, 2016.

U.S. Appl. No. 62/341,396, filed May 25, 2016.

U.S. Appl. No. 29/575,316, filed Aug. 24, 2016.

U.S. Appl. No. 16/136,753, filed Sep. 20, 2018.

U.S. Appl. No. 16/162,609, filed Oct. 17, 2018.

* cited by examiner

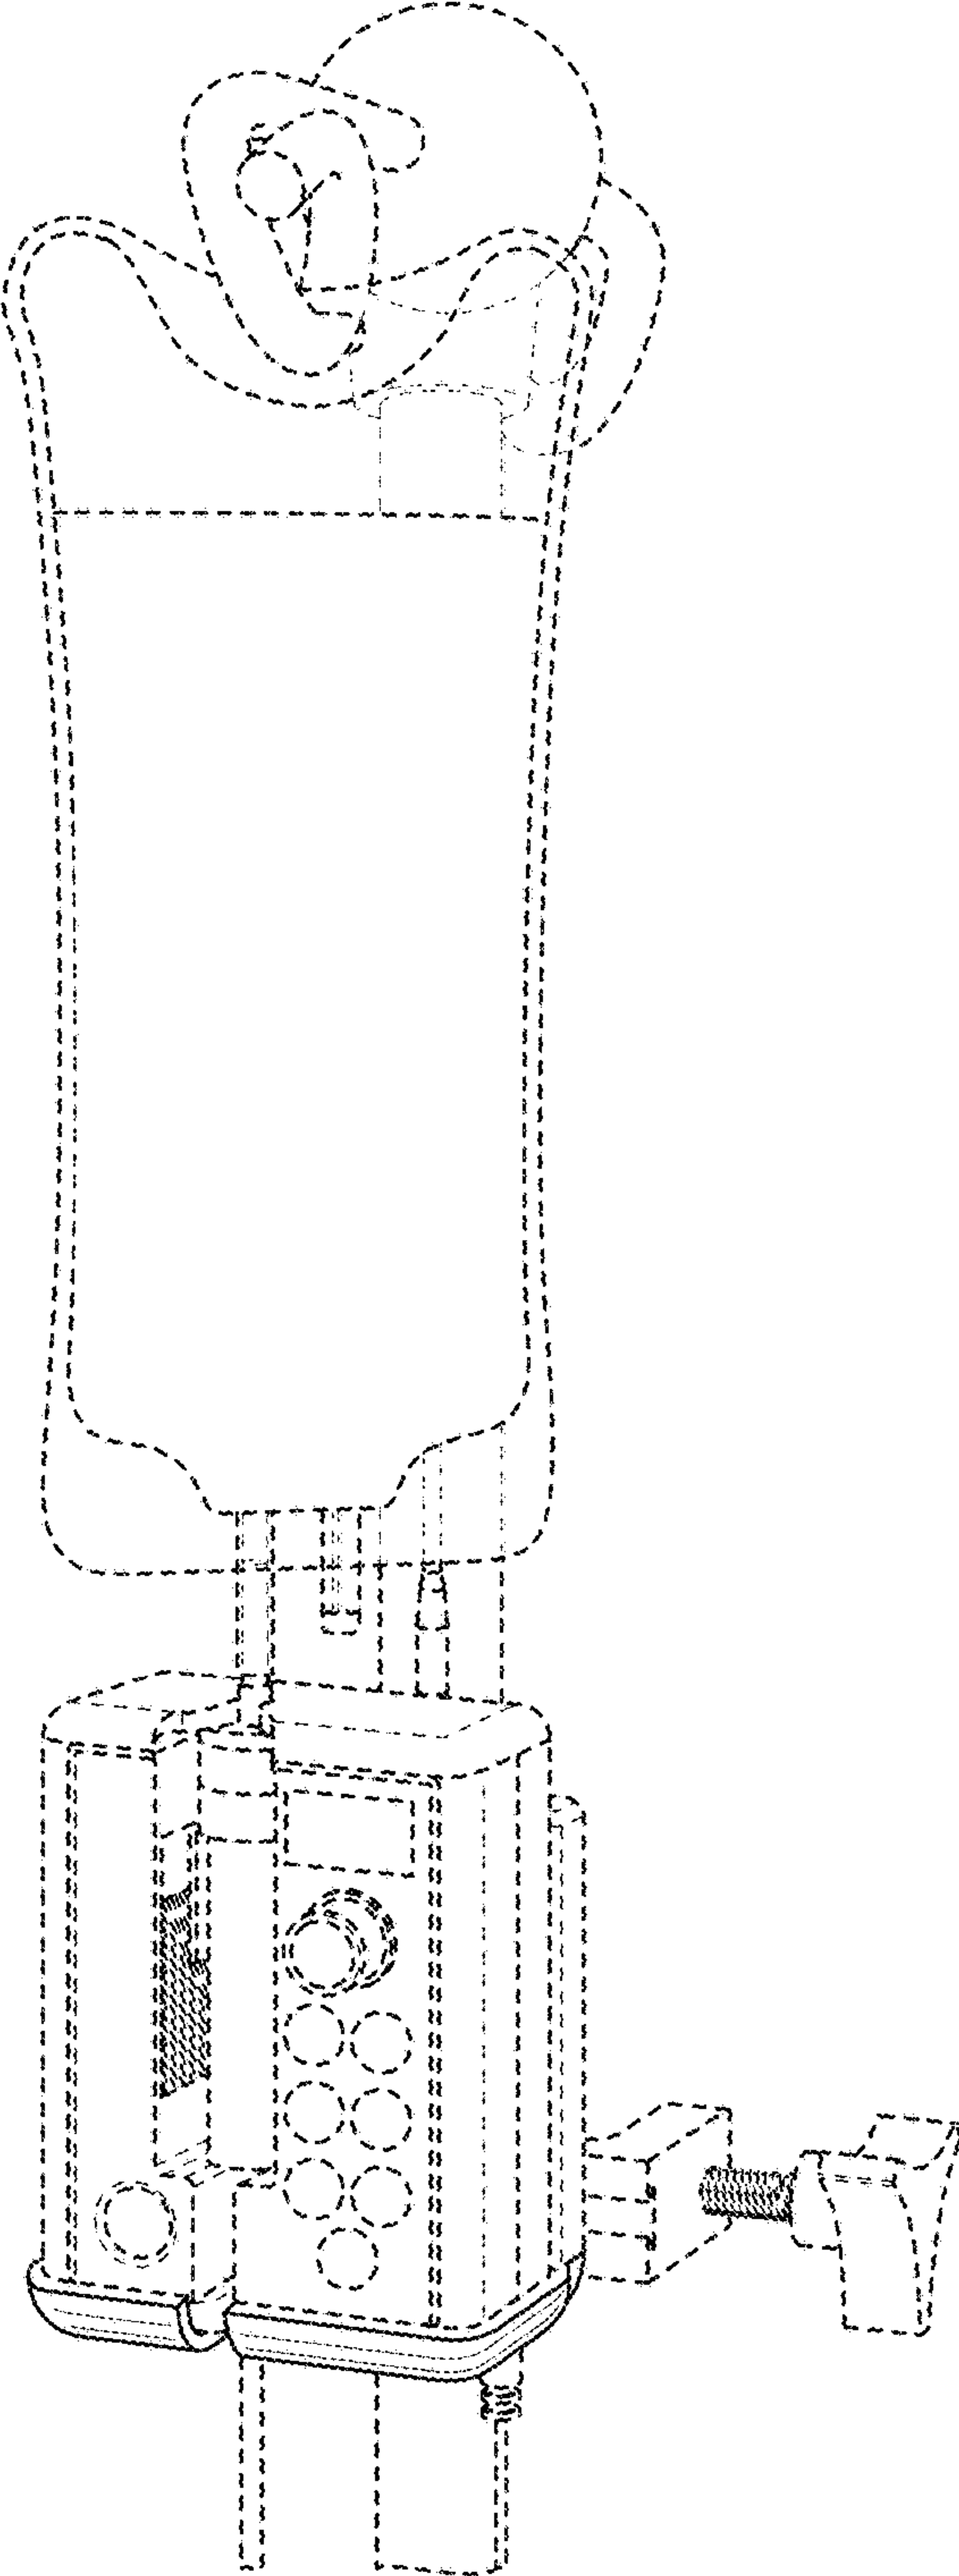


FIG. 1

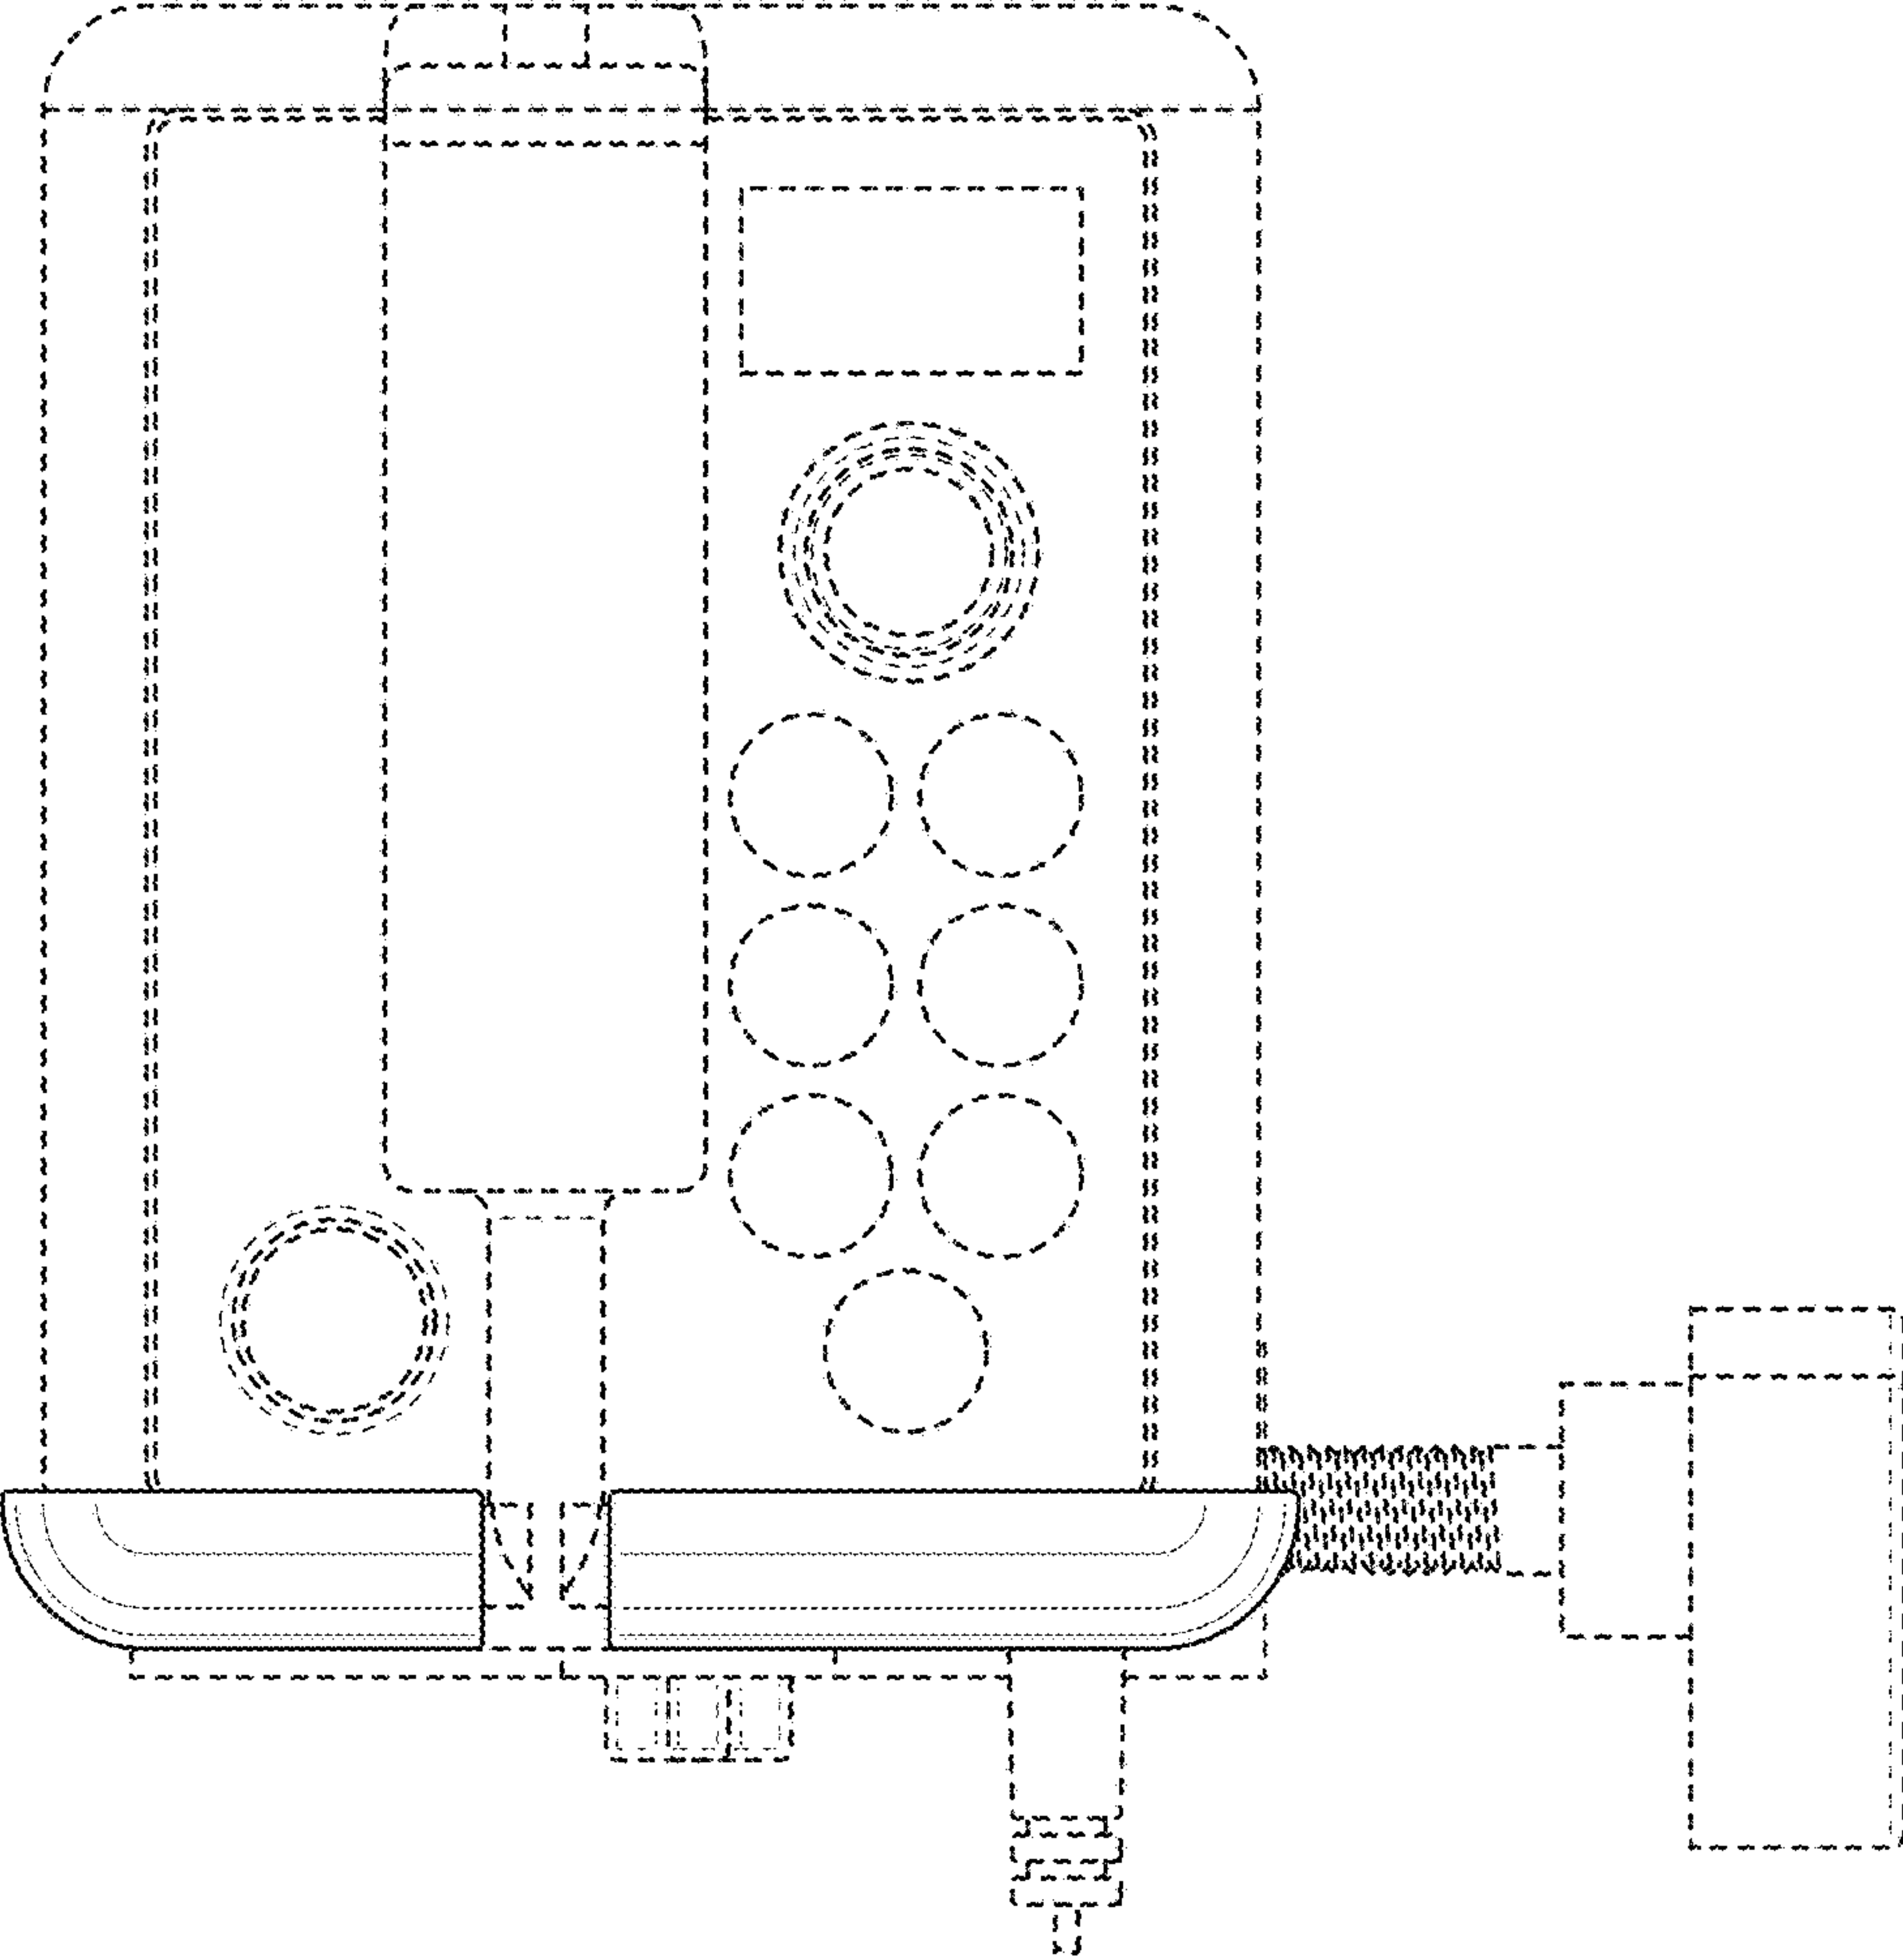


FIG. 2

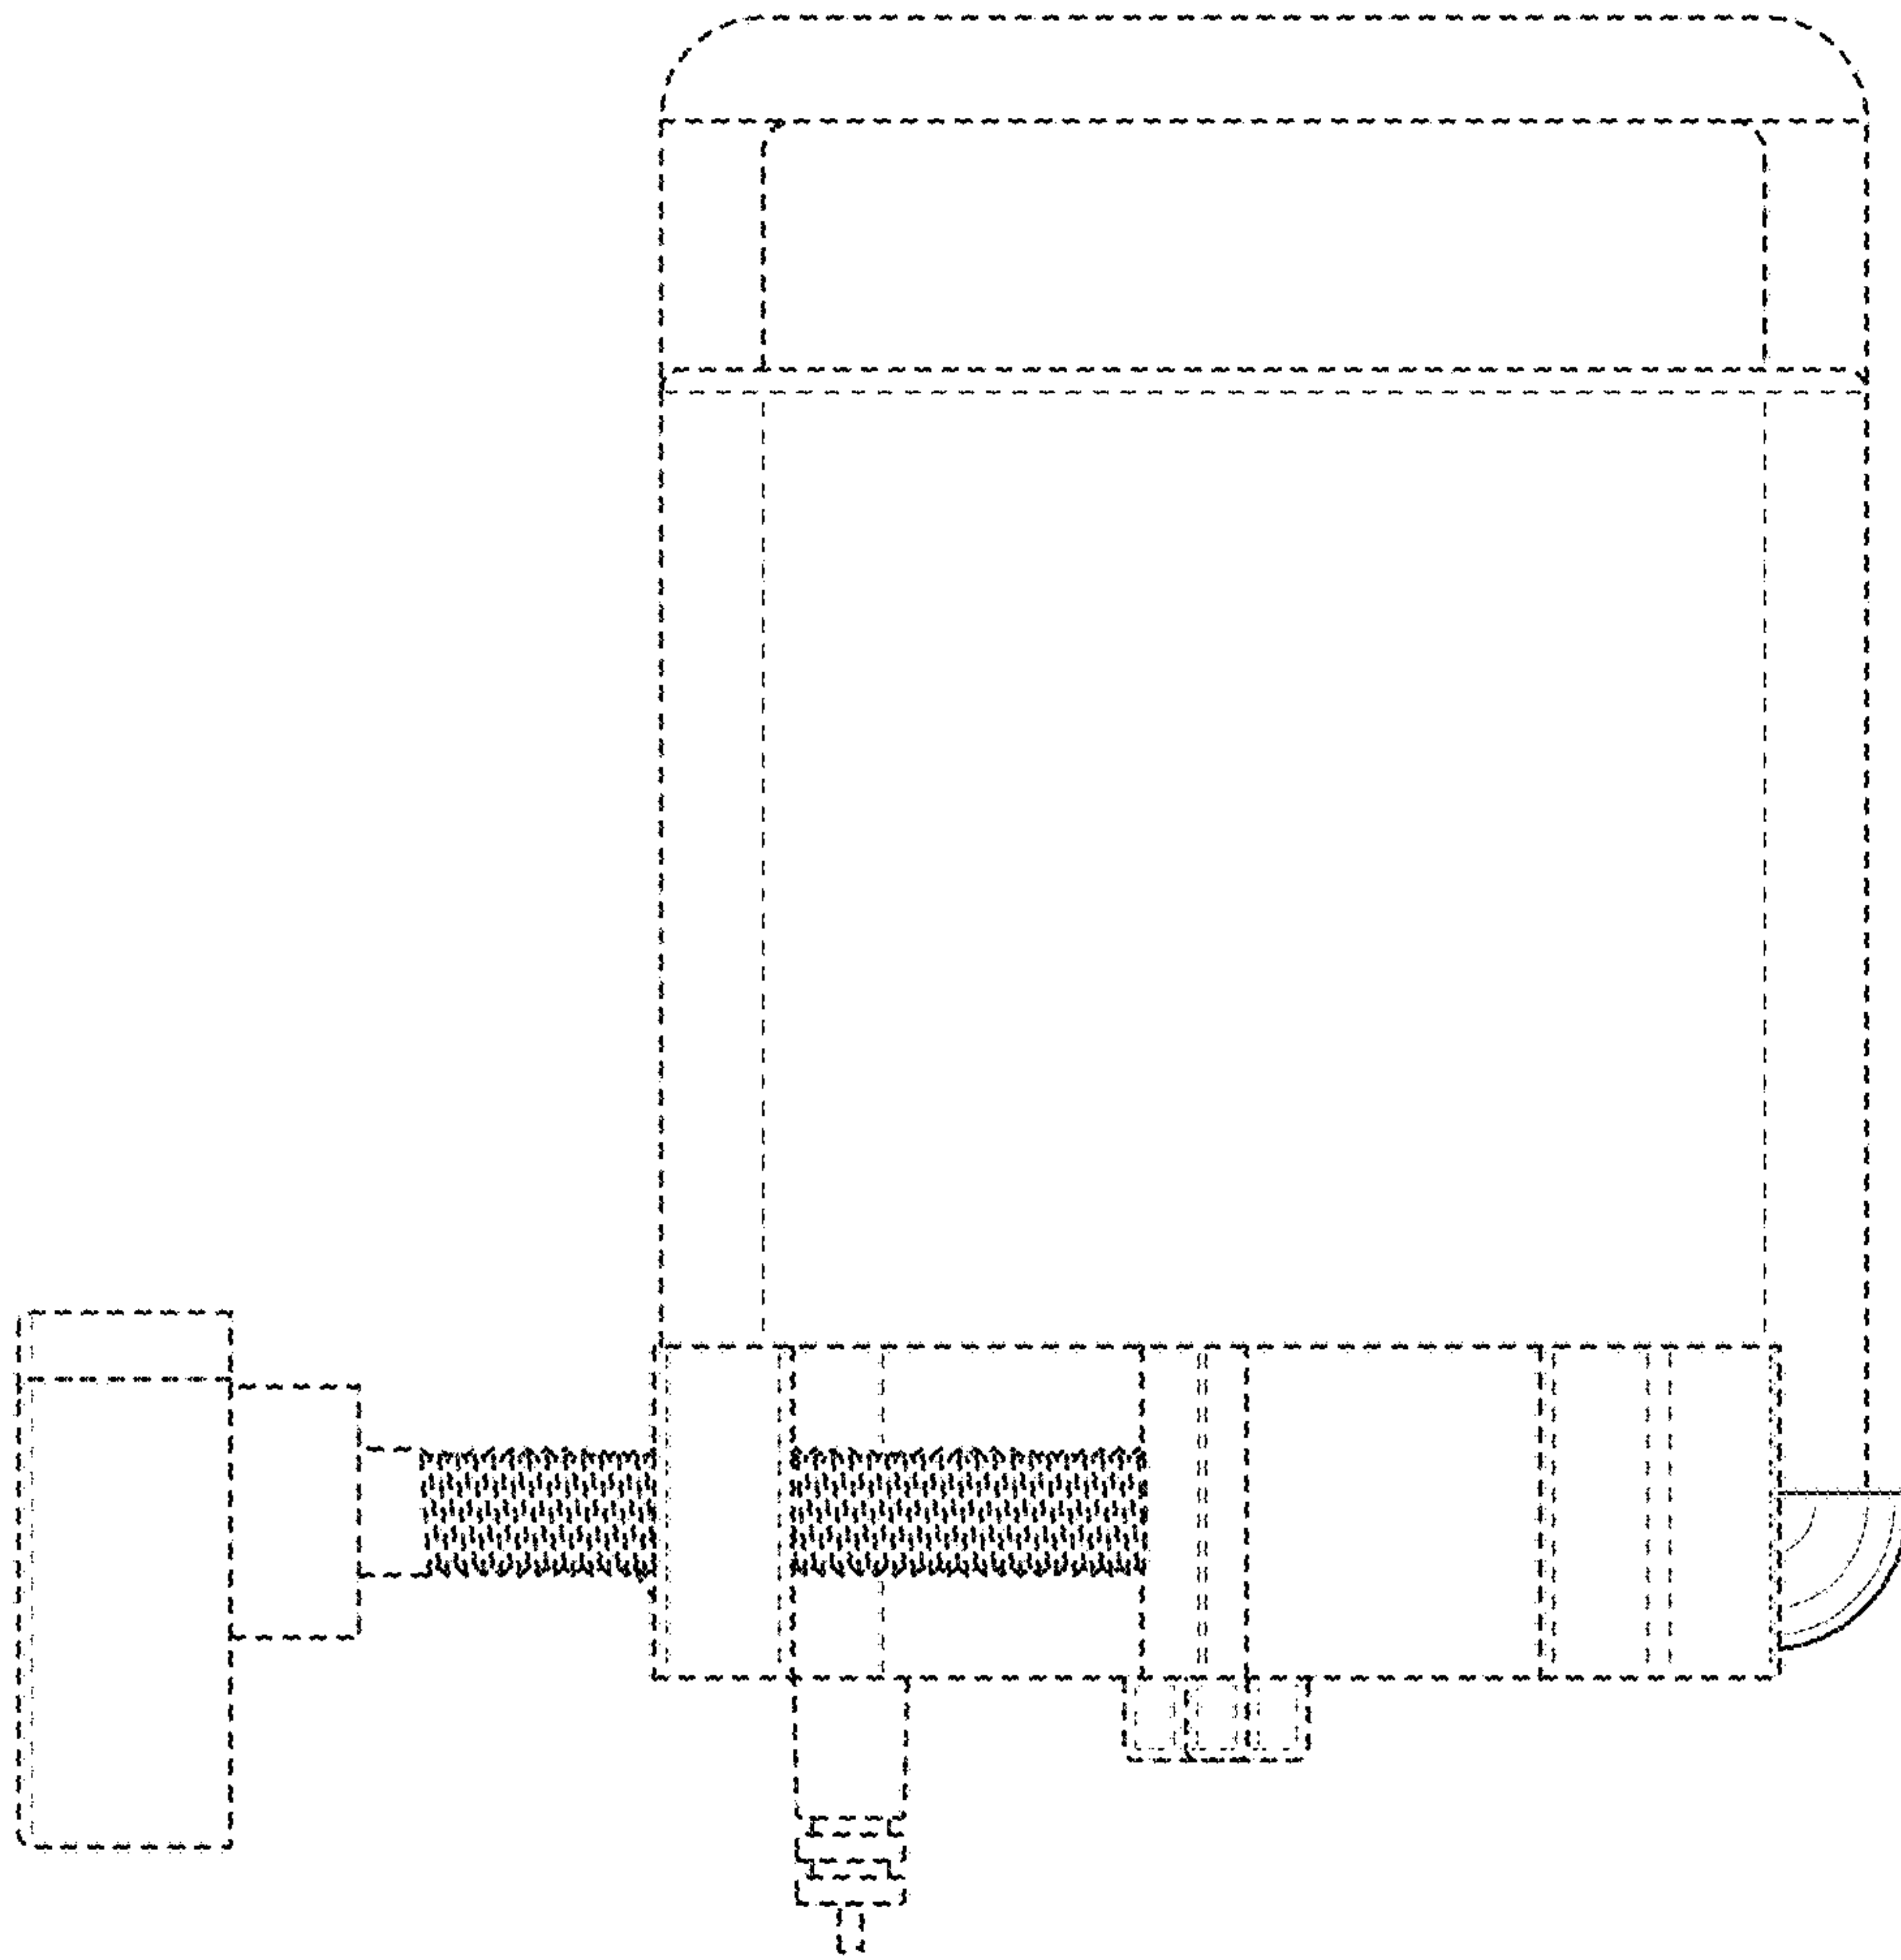


FIG. 3

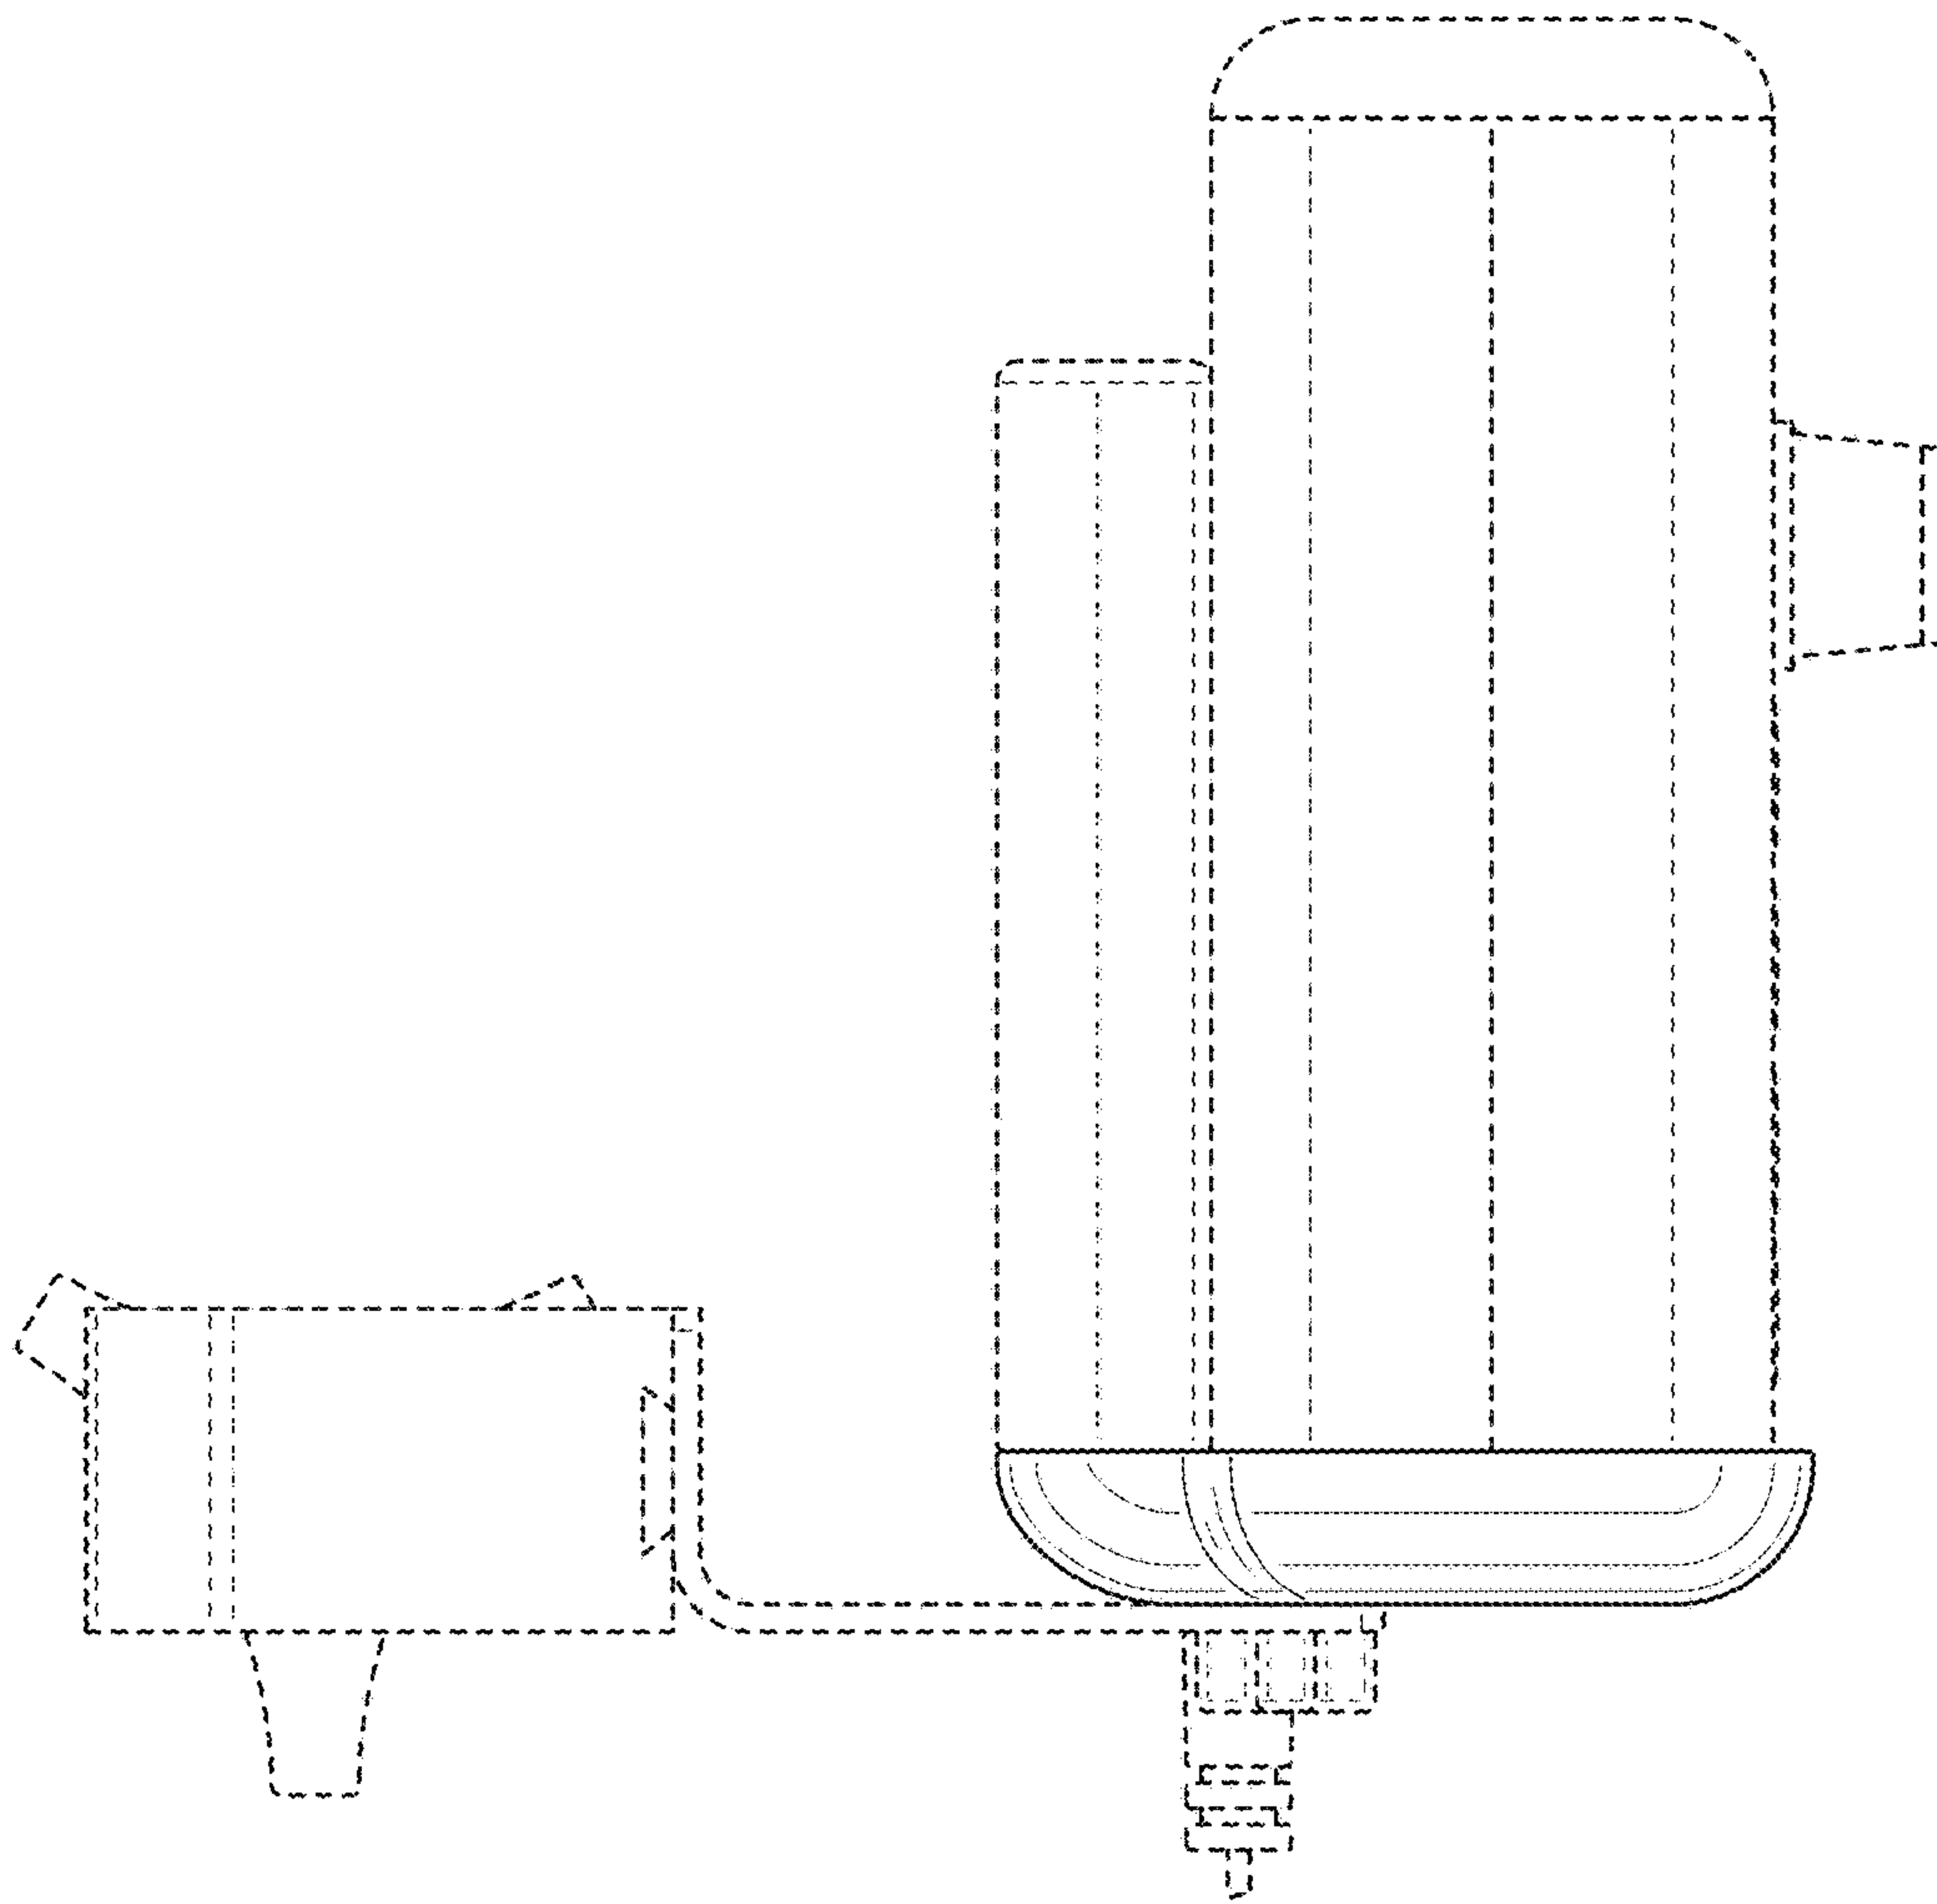


FIG. 4

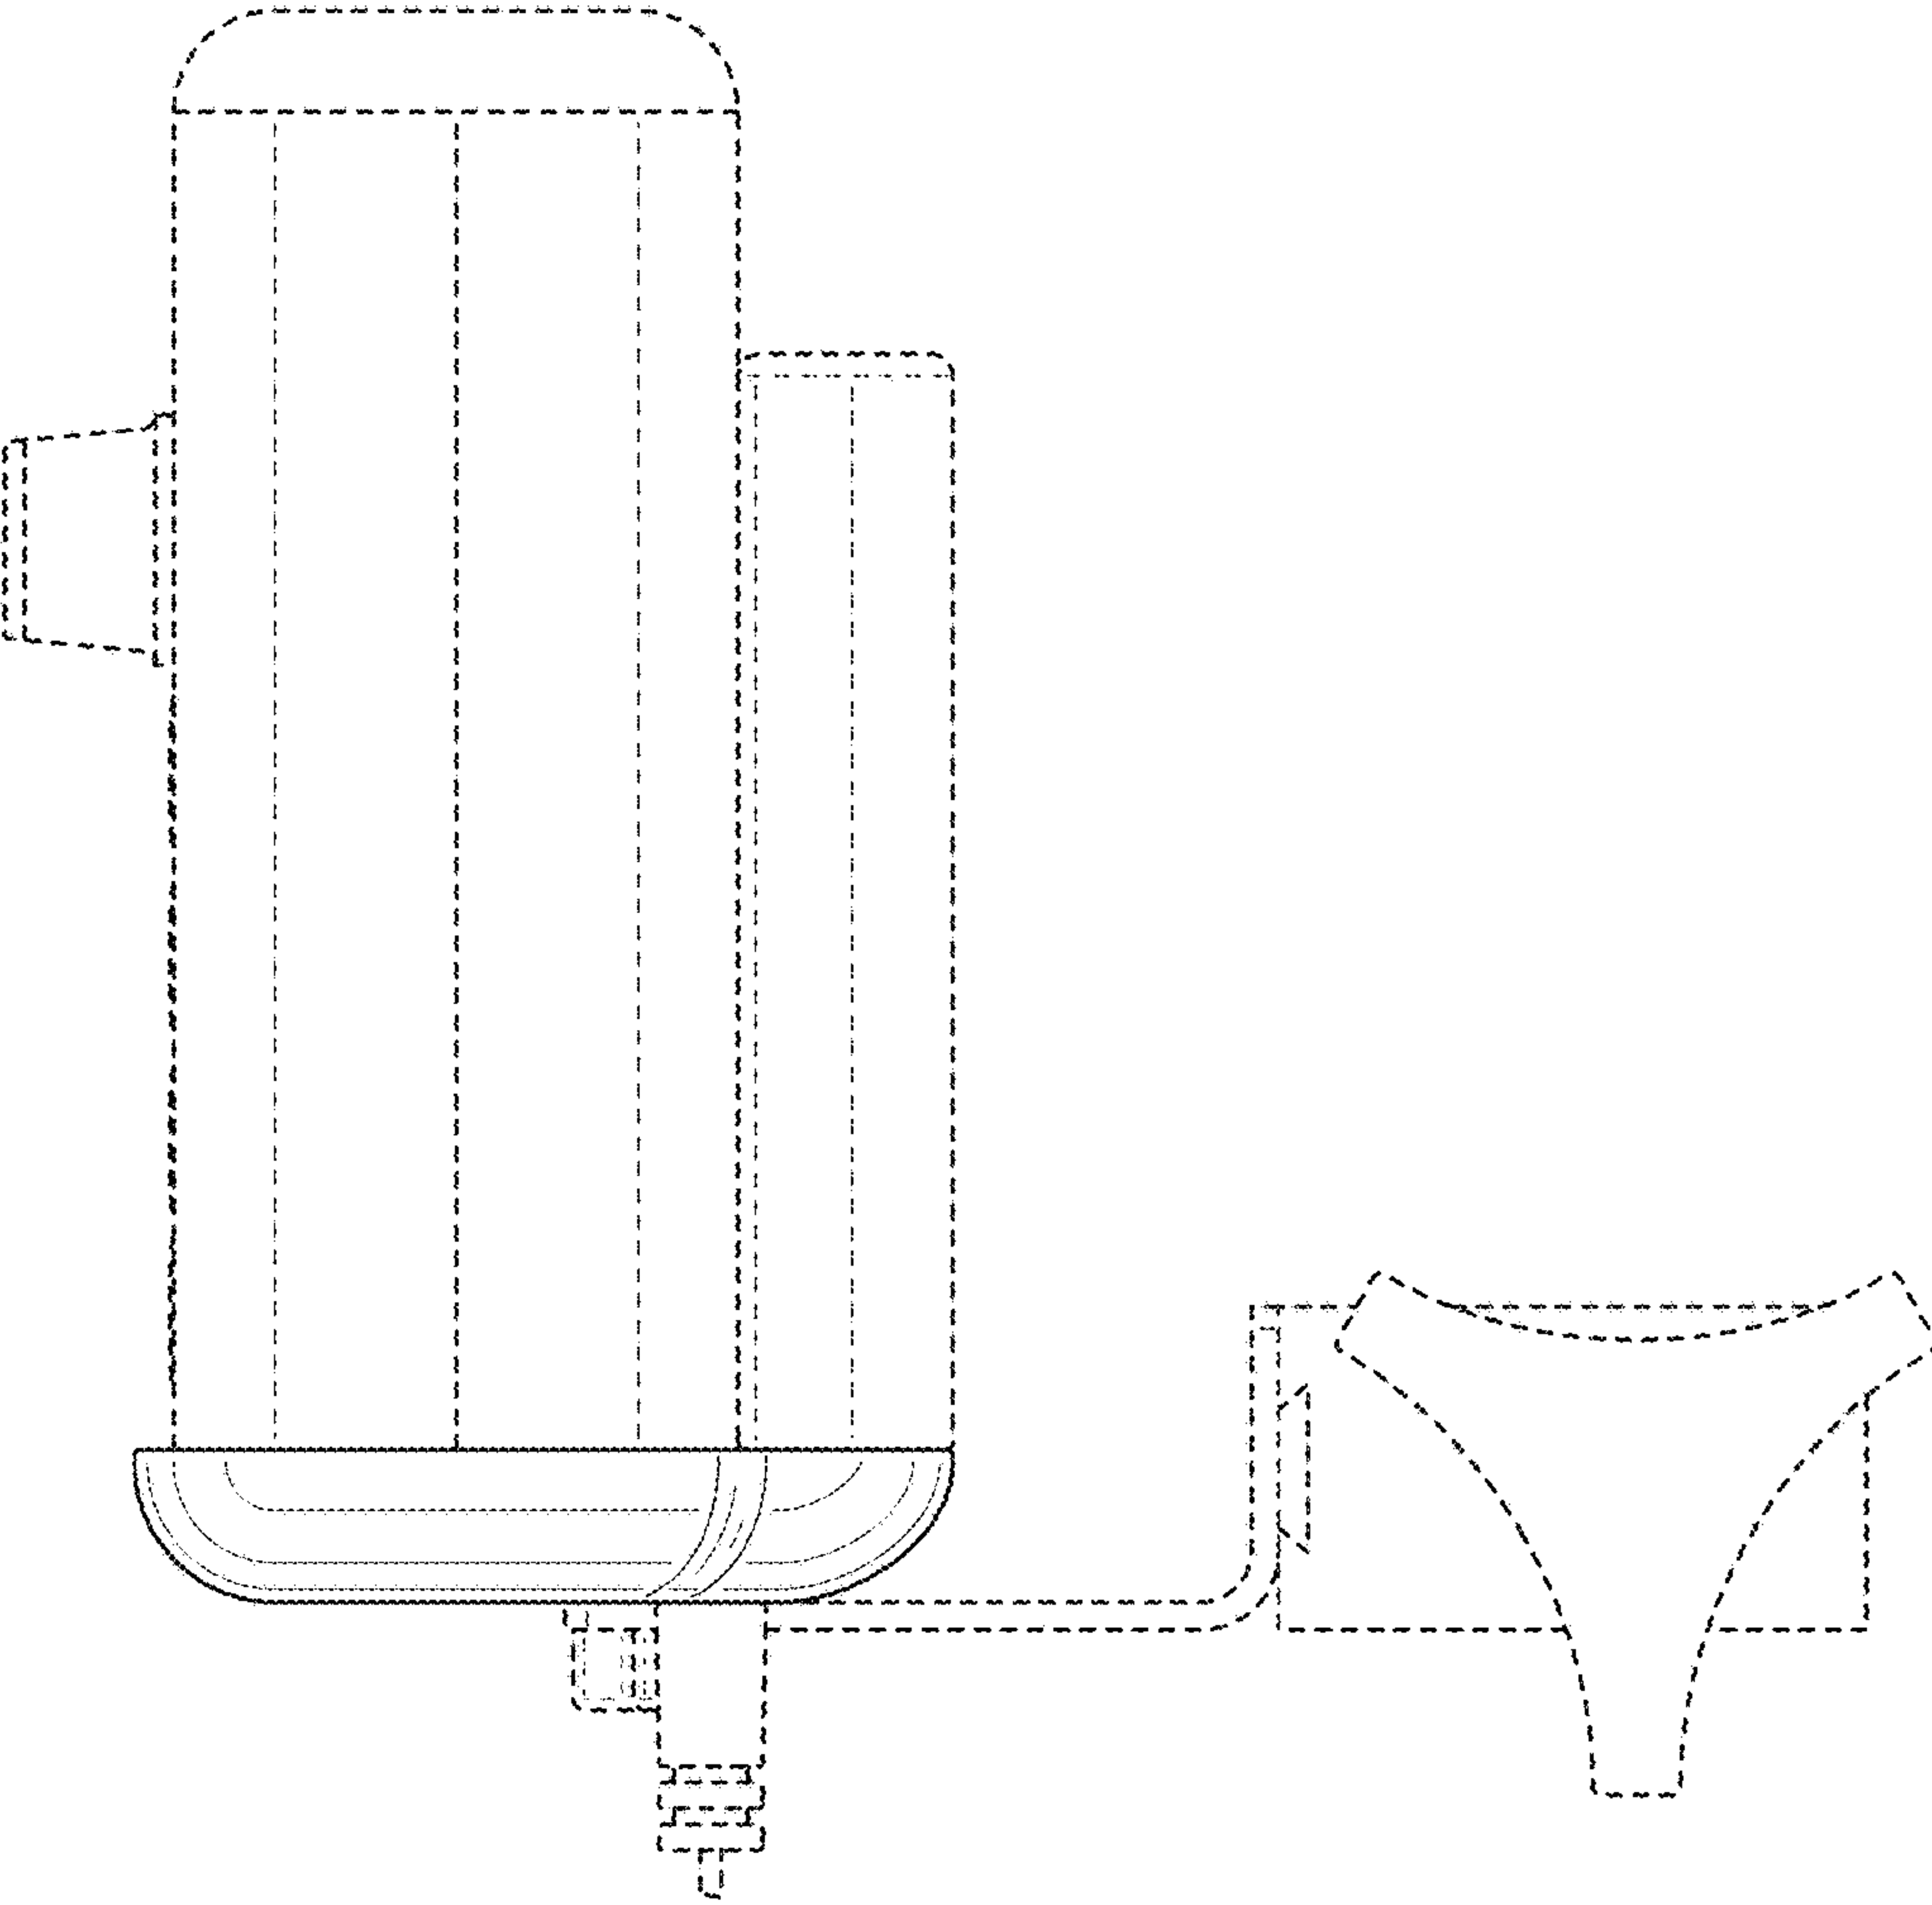


FIG. 5

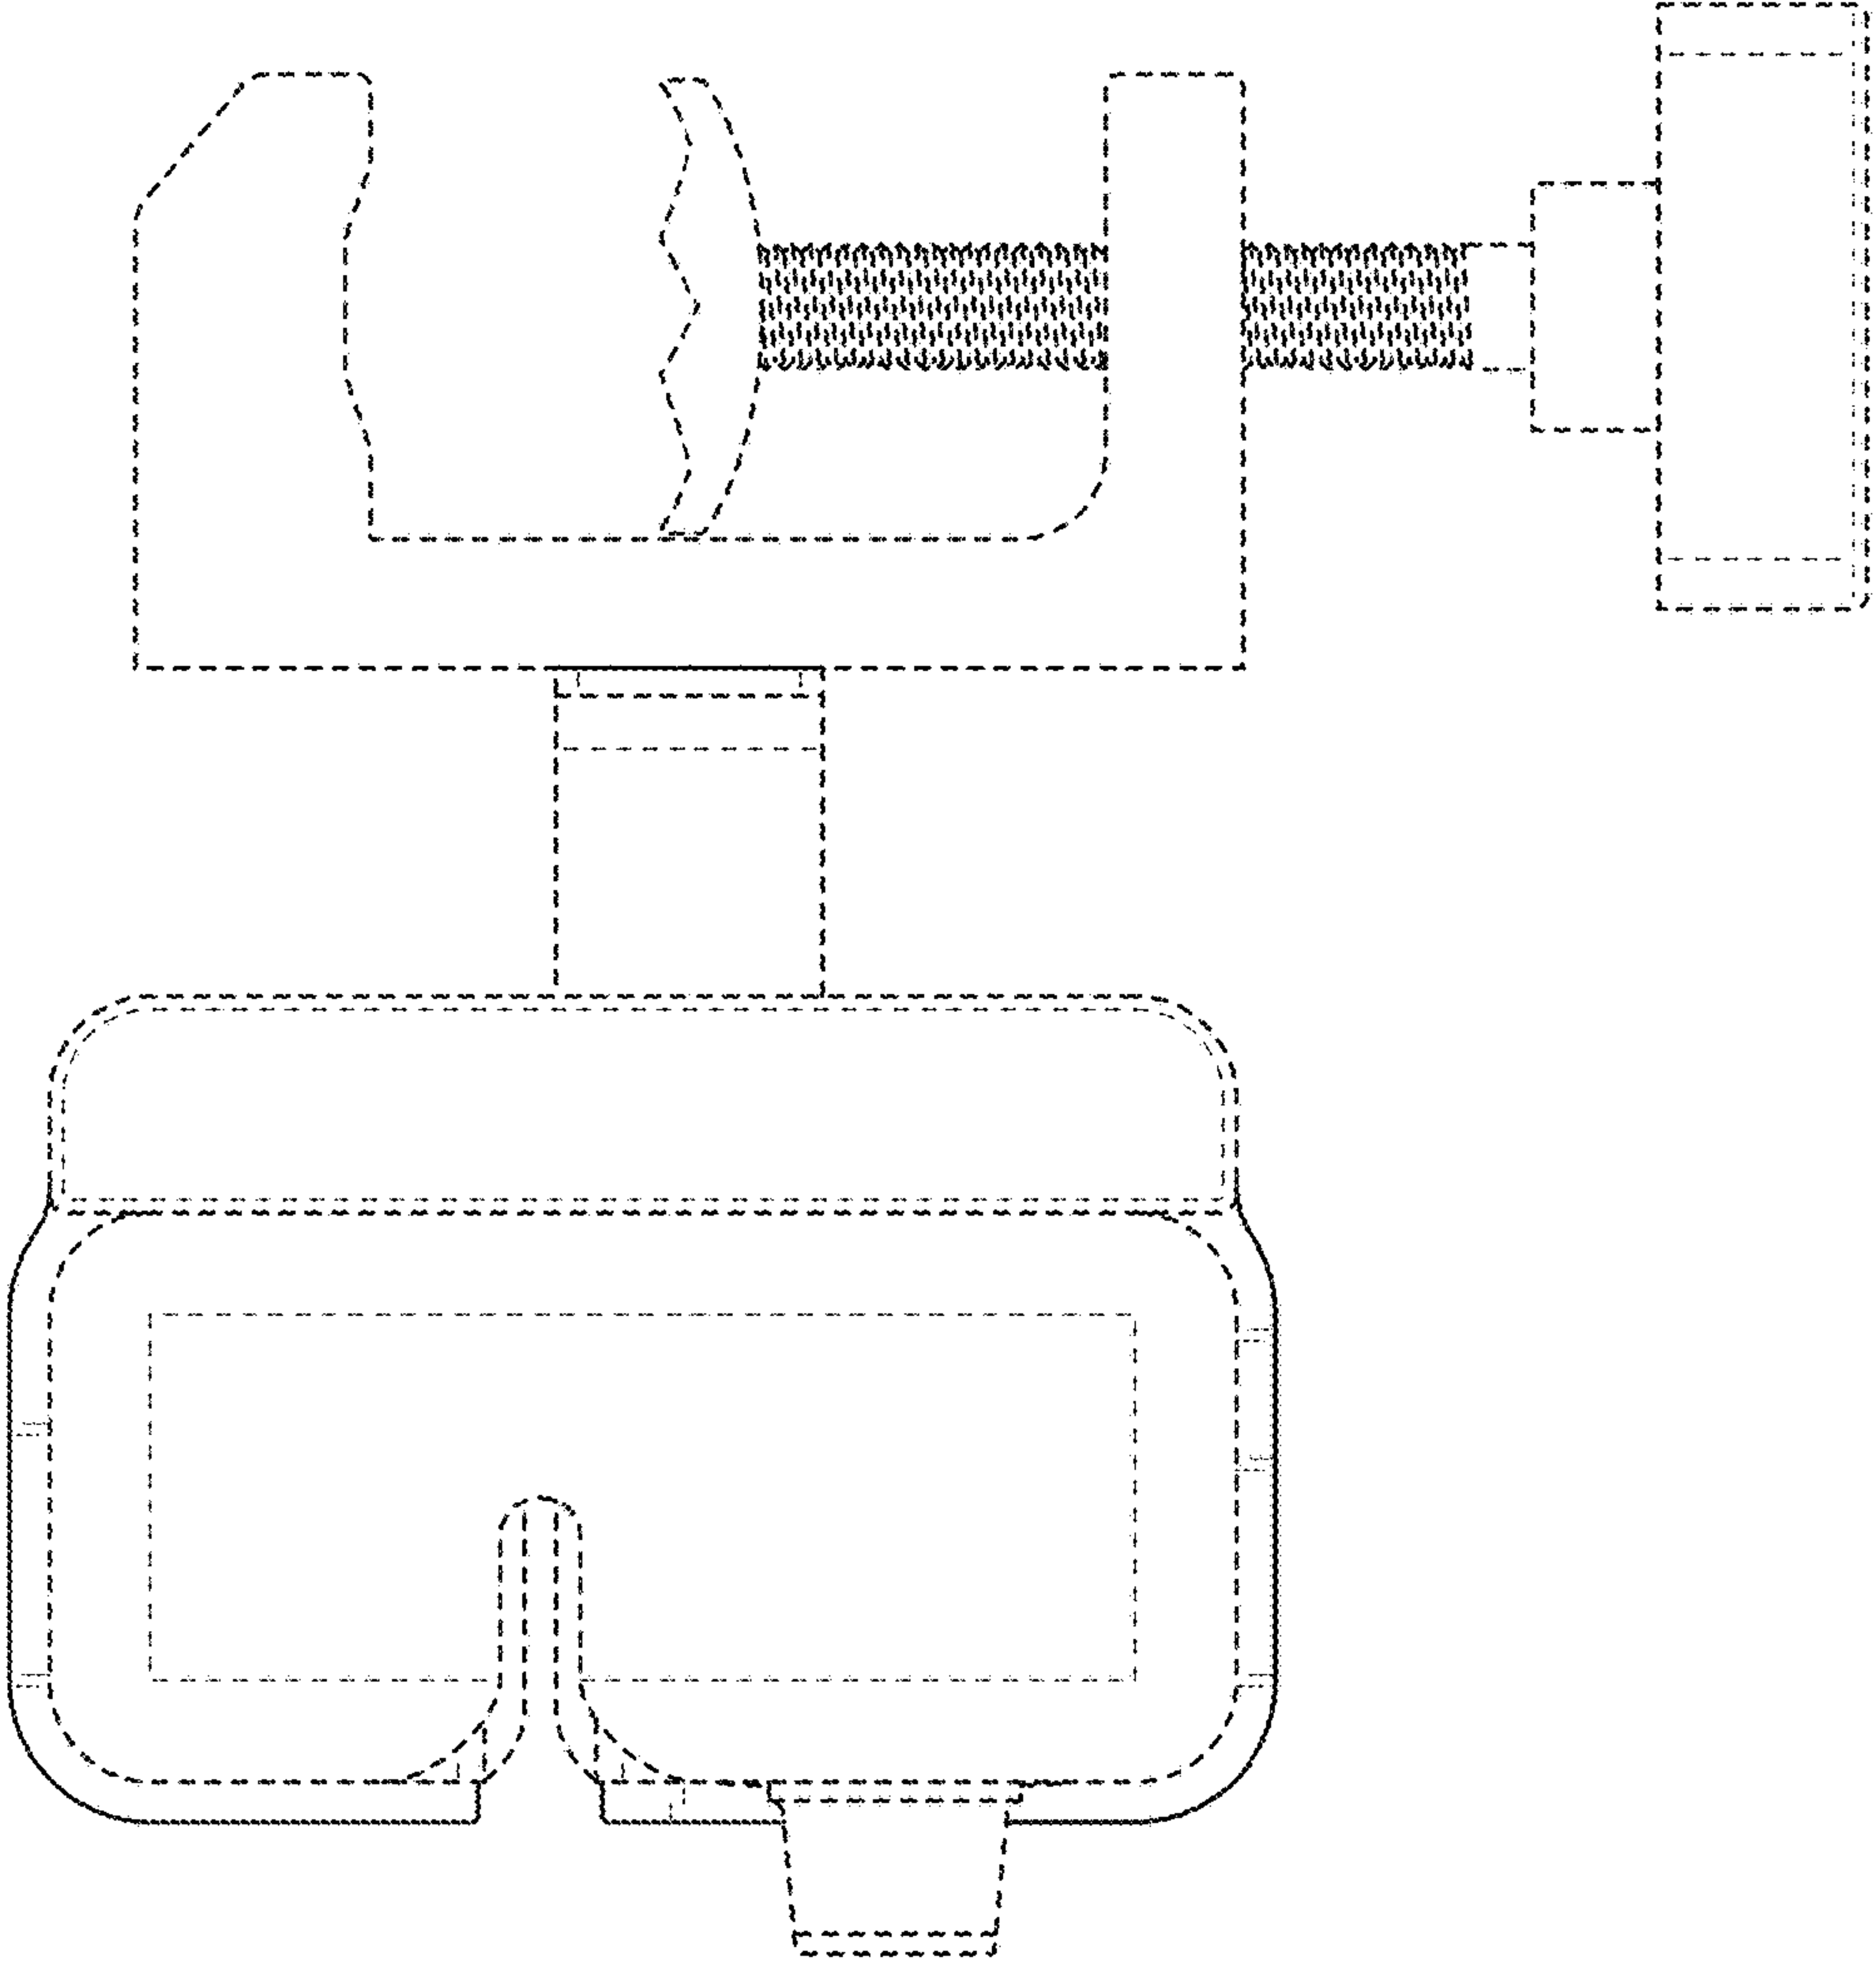


FIG. 6

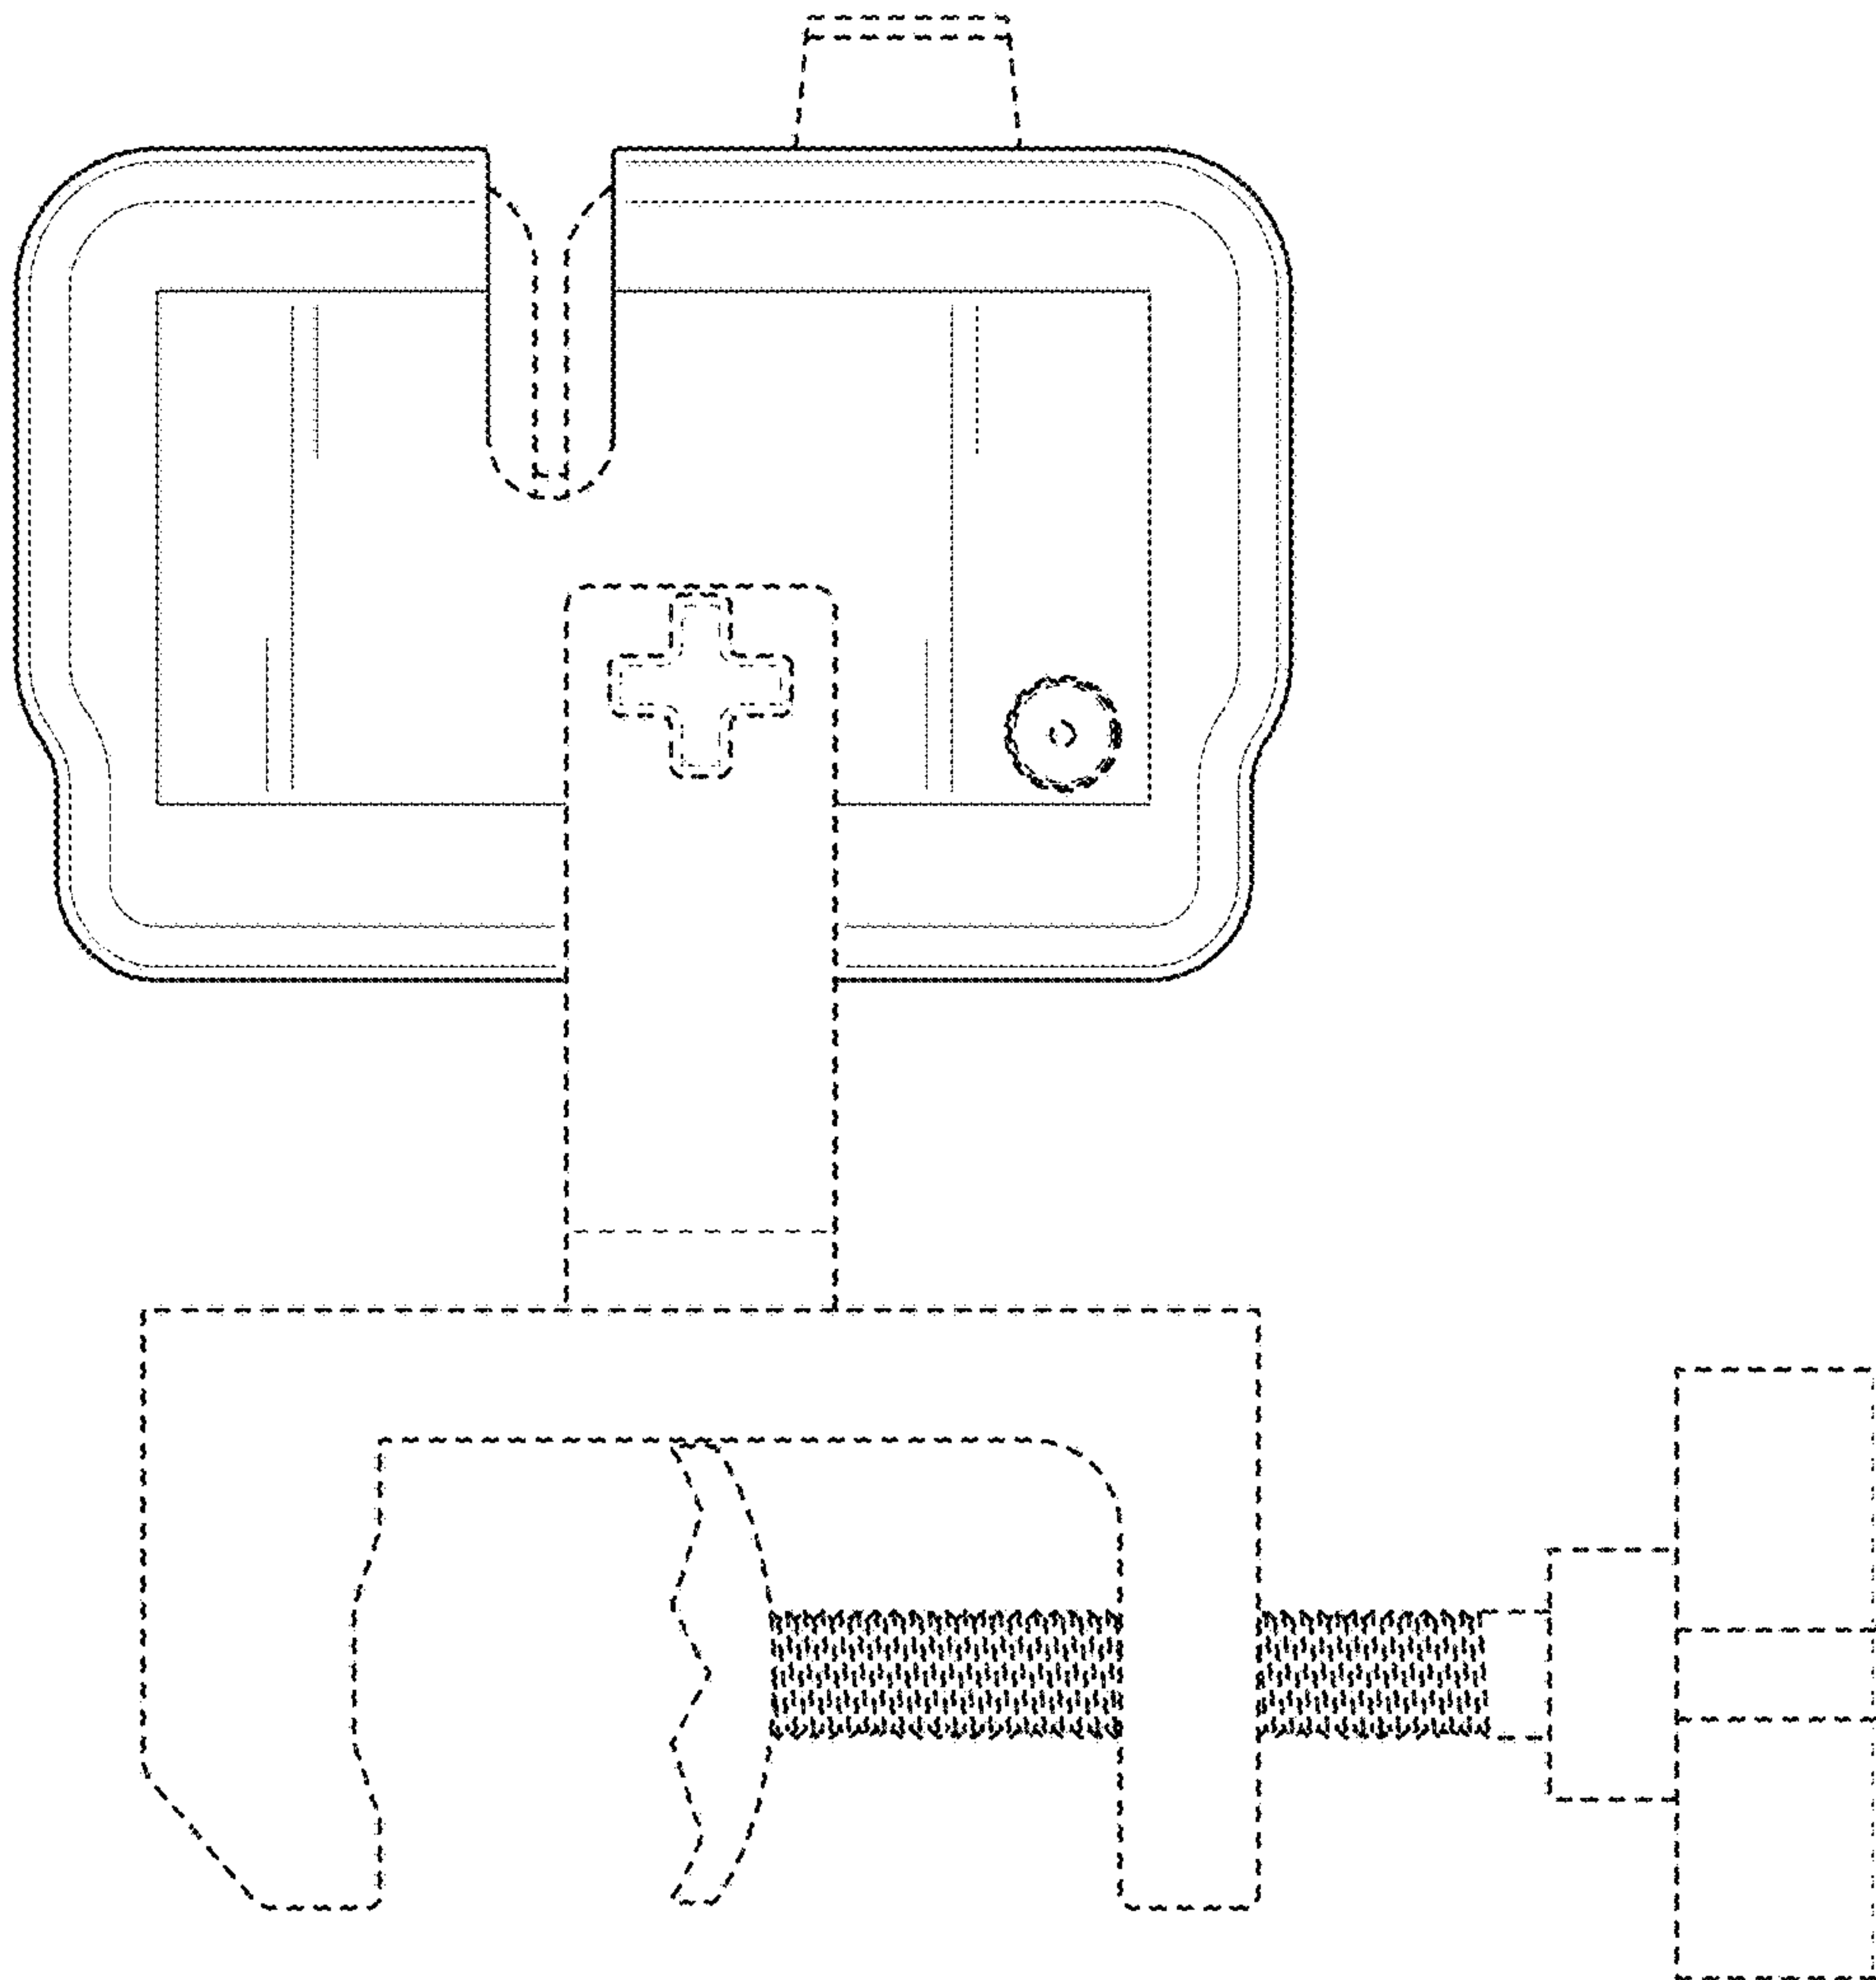


FIG. 7