



US00D861852S

(12) **United States Design Patent**
Sutherland et al.

(10) **Patent No.:** **US D861,852 S**

(45) **Date of Patent:** **** Oct. 1, 2019**

(54) **COMPLIANCE MONITOR FOR A
MEDICAMENT INHALER**

(71) Applicant: **Adherium (NZ) Limited**, Auckland
(NZ)

(72) Inventors: **Garth Campbell Sutherland**, Auckland
(NZ); **Michael James Gormack**,
Auckland (NZ); **Edward Scholten**,
Auckland (NZ); **Benjamin Lance Catt**,
Auckland (NZ); **Craig David Shannon**,
Auckland (NZ)

(73) Assignee: **ADHERIUM (NZ) LIMITED**,
Auckland (NZ)

(**) Term: **15 Years**

(21) Appl. No.: **29/554,754**

(22) Filed: **Feb. 15, 2016**

(30) **Foreign Application Priority Data**

Aug. 13, 2015 (NZ) 420537
Aug. 13, 2015 (NZ) 420540
Aug. 13, 2015 (NZ) 450538
Aug. 13, 2015 (NZ) 450541

(51) **LOC (12) Cl.** **29-02**

(52) **U.S. Cl.**
USPC **D24/110**

(58) **Field of Classification Search**
USPC D24/107, 108, 110, 111, 127, 164, 188
CPC A61M 15/00; A61M 15/0065; A61M
15/0091; A61M 15/0021; A61M 15/0026;
A61M 11/00; A61M 11/02; A61M 11/04;
A61M 15/0001; A61M 15/0068; A61M
15/008; A61M 15/0083; A61M 15/0025

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D560,793 S *	1/2008	Pearl	D24/110
D569,967 S *	5/2008	Pearl	D24/110
D613,848 S *	4/2010	Harvey	D24/110
D614,024 S *	4/2010	Eason	D24/110
D623,054 S *	9/2010	Eason	D24/110
D635,659 S *	4/2011	White	D24/110
D635,660 S *	4/2011	White	D24/110
D636,073 S *	4/2011	White	D24/110
D636,485 S *	4/2011	White	D24/110
D637,280 S *	5/2011	Harvey	D24/110
D637,281 S *	5/2011	Harvey	D24/110
D637,282 S *	5/2011	Harvey	D24/110
D645,734 S *	9/2011	Eason	D24/110
D673,260 S *	12/2012	White	D24/110

(Continued)

Primary Examiner — Karen E Kearney

Assistant Examiner — Lilyana Bekic

(74) *Attorney, Agent, or Firm* — Kenealy Vaidya LLP



(57) **CLAIM**

The ornamental design for a compliance monitor for a medicament inhaler, as shown and described.

DESCRIPTION

FIG. 1 is a top view of a compliance monitor for a medicament inhaler showing our new design.
FIG. 2 is a front view of the compliance monitor for a medicament inhaler of FIG. 1.
FIG. 3 is a right side view of the compliance monitor for a medicament inhaler of FIG. 1.
FIG. 4 is a rear view of the compliance monitor for a medicament inhaler of FIG. 1.
FIG. 5 is a left side view of the compliance monitor for a medicament inhaler of FIG. 1.
FIG. 6 is a perspective view of the compliance monitor for a medicament inhaler of FIG. 1; and,
FIG. 7 is a bottom view of the compliance monitor for a medicament inhaler of FIG. 1.

1 Claim, 7 Drawing Sheets

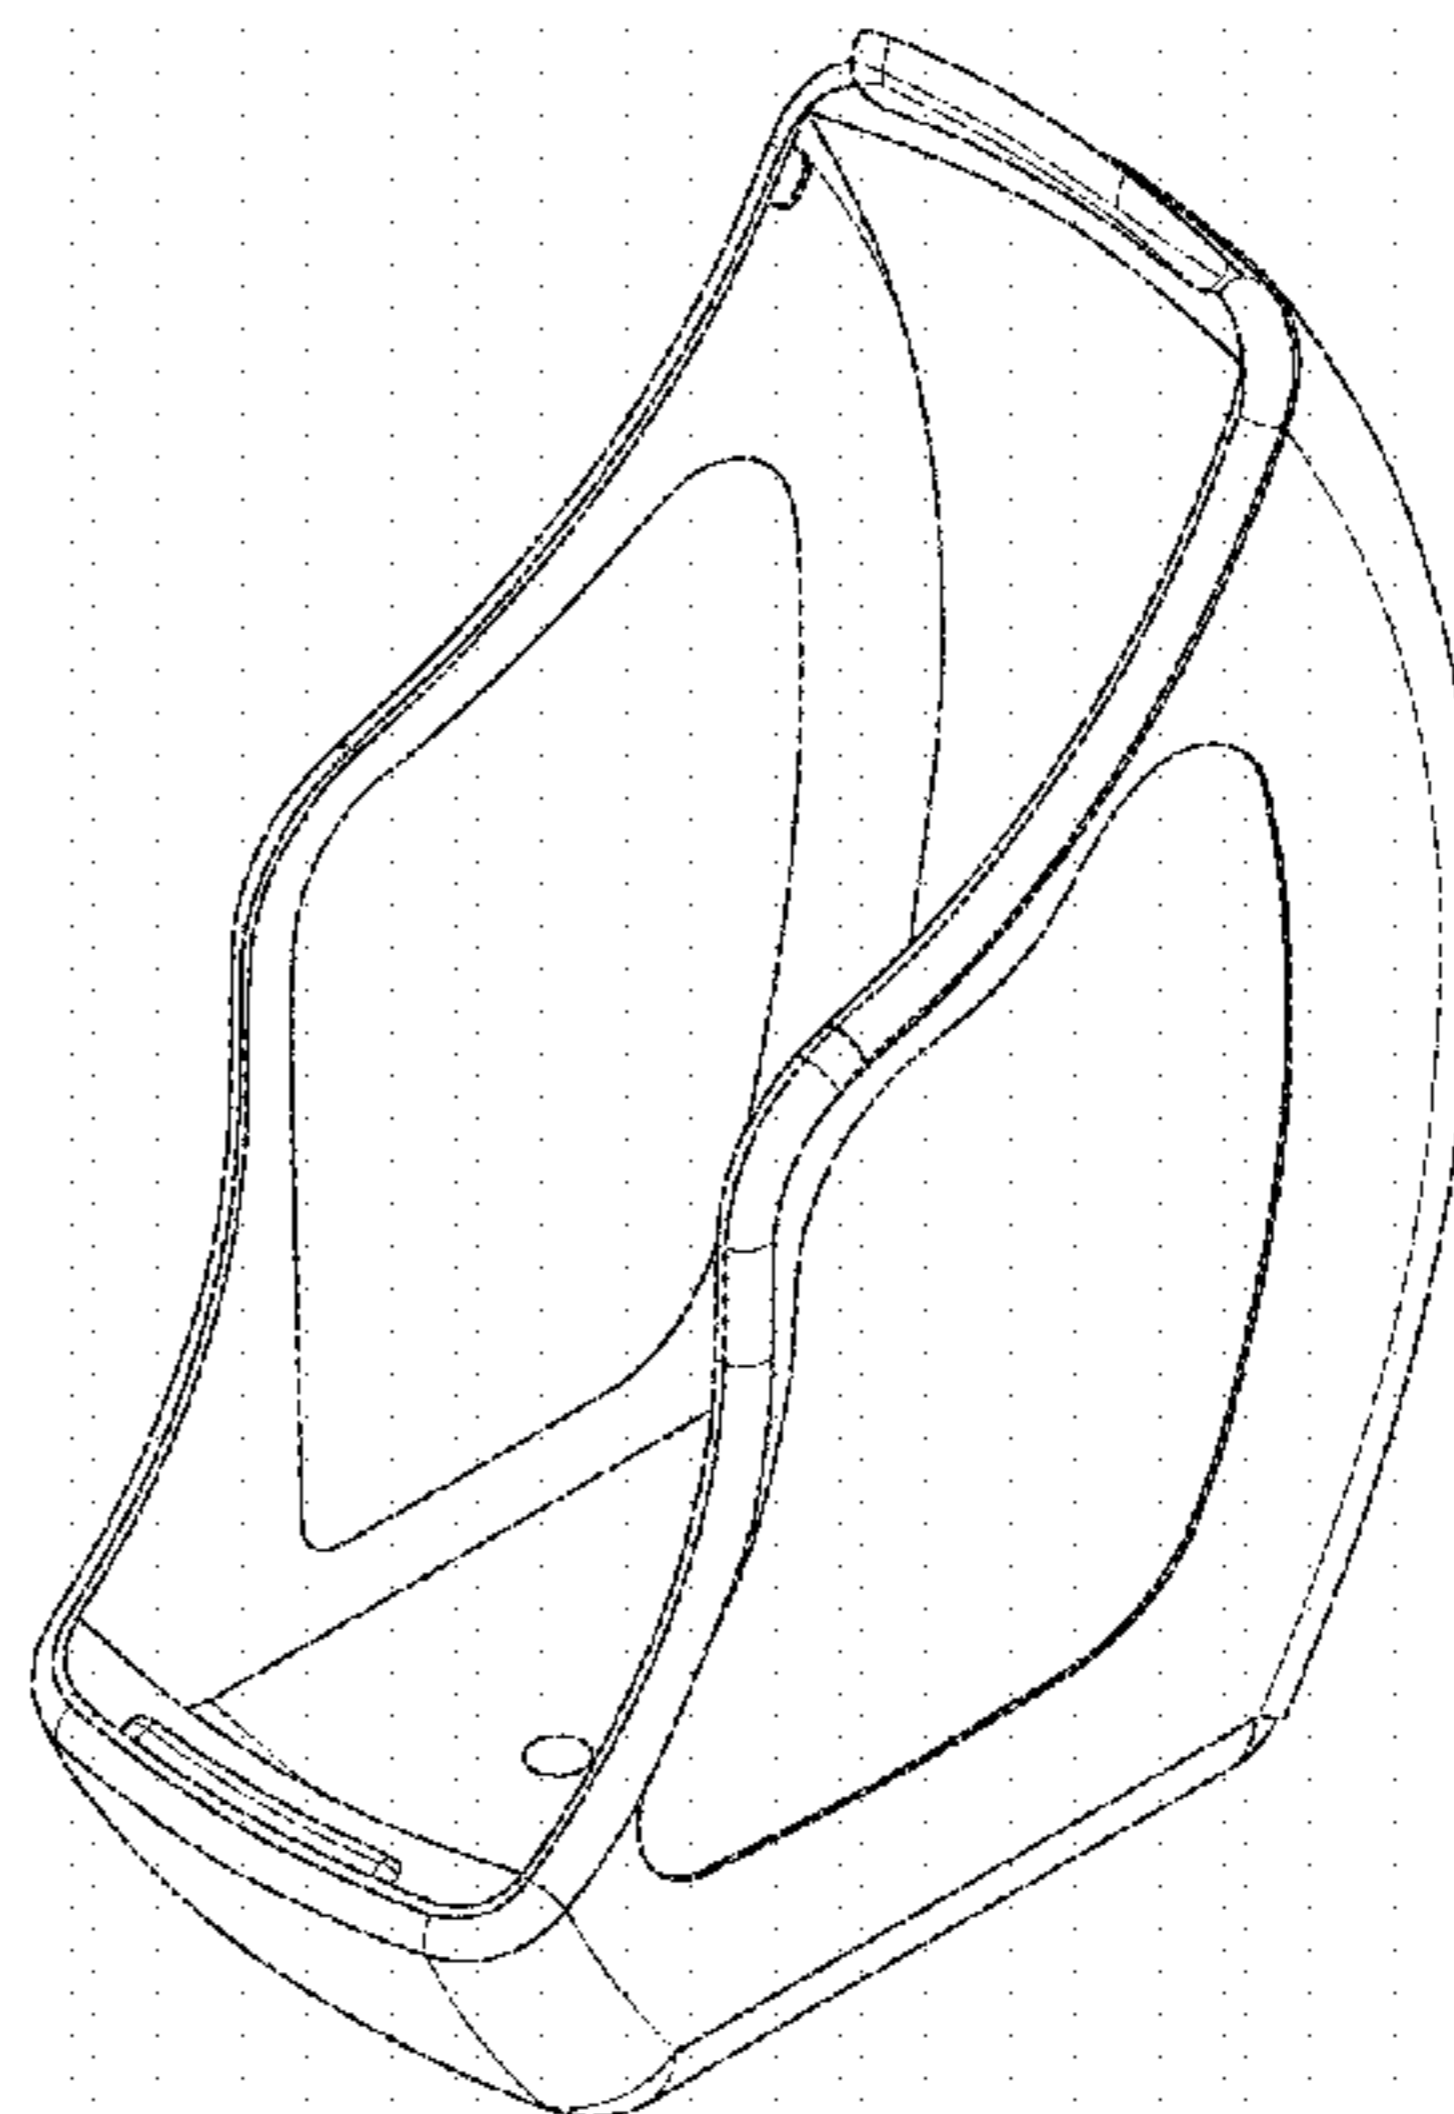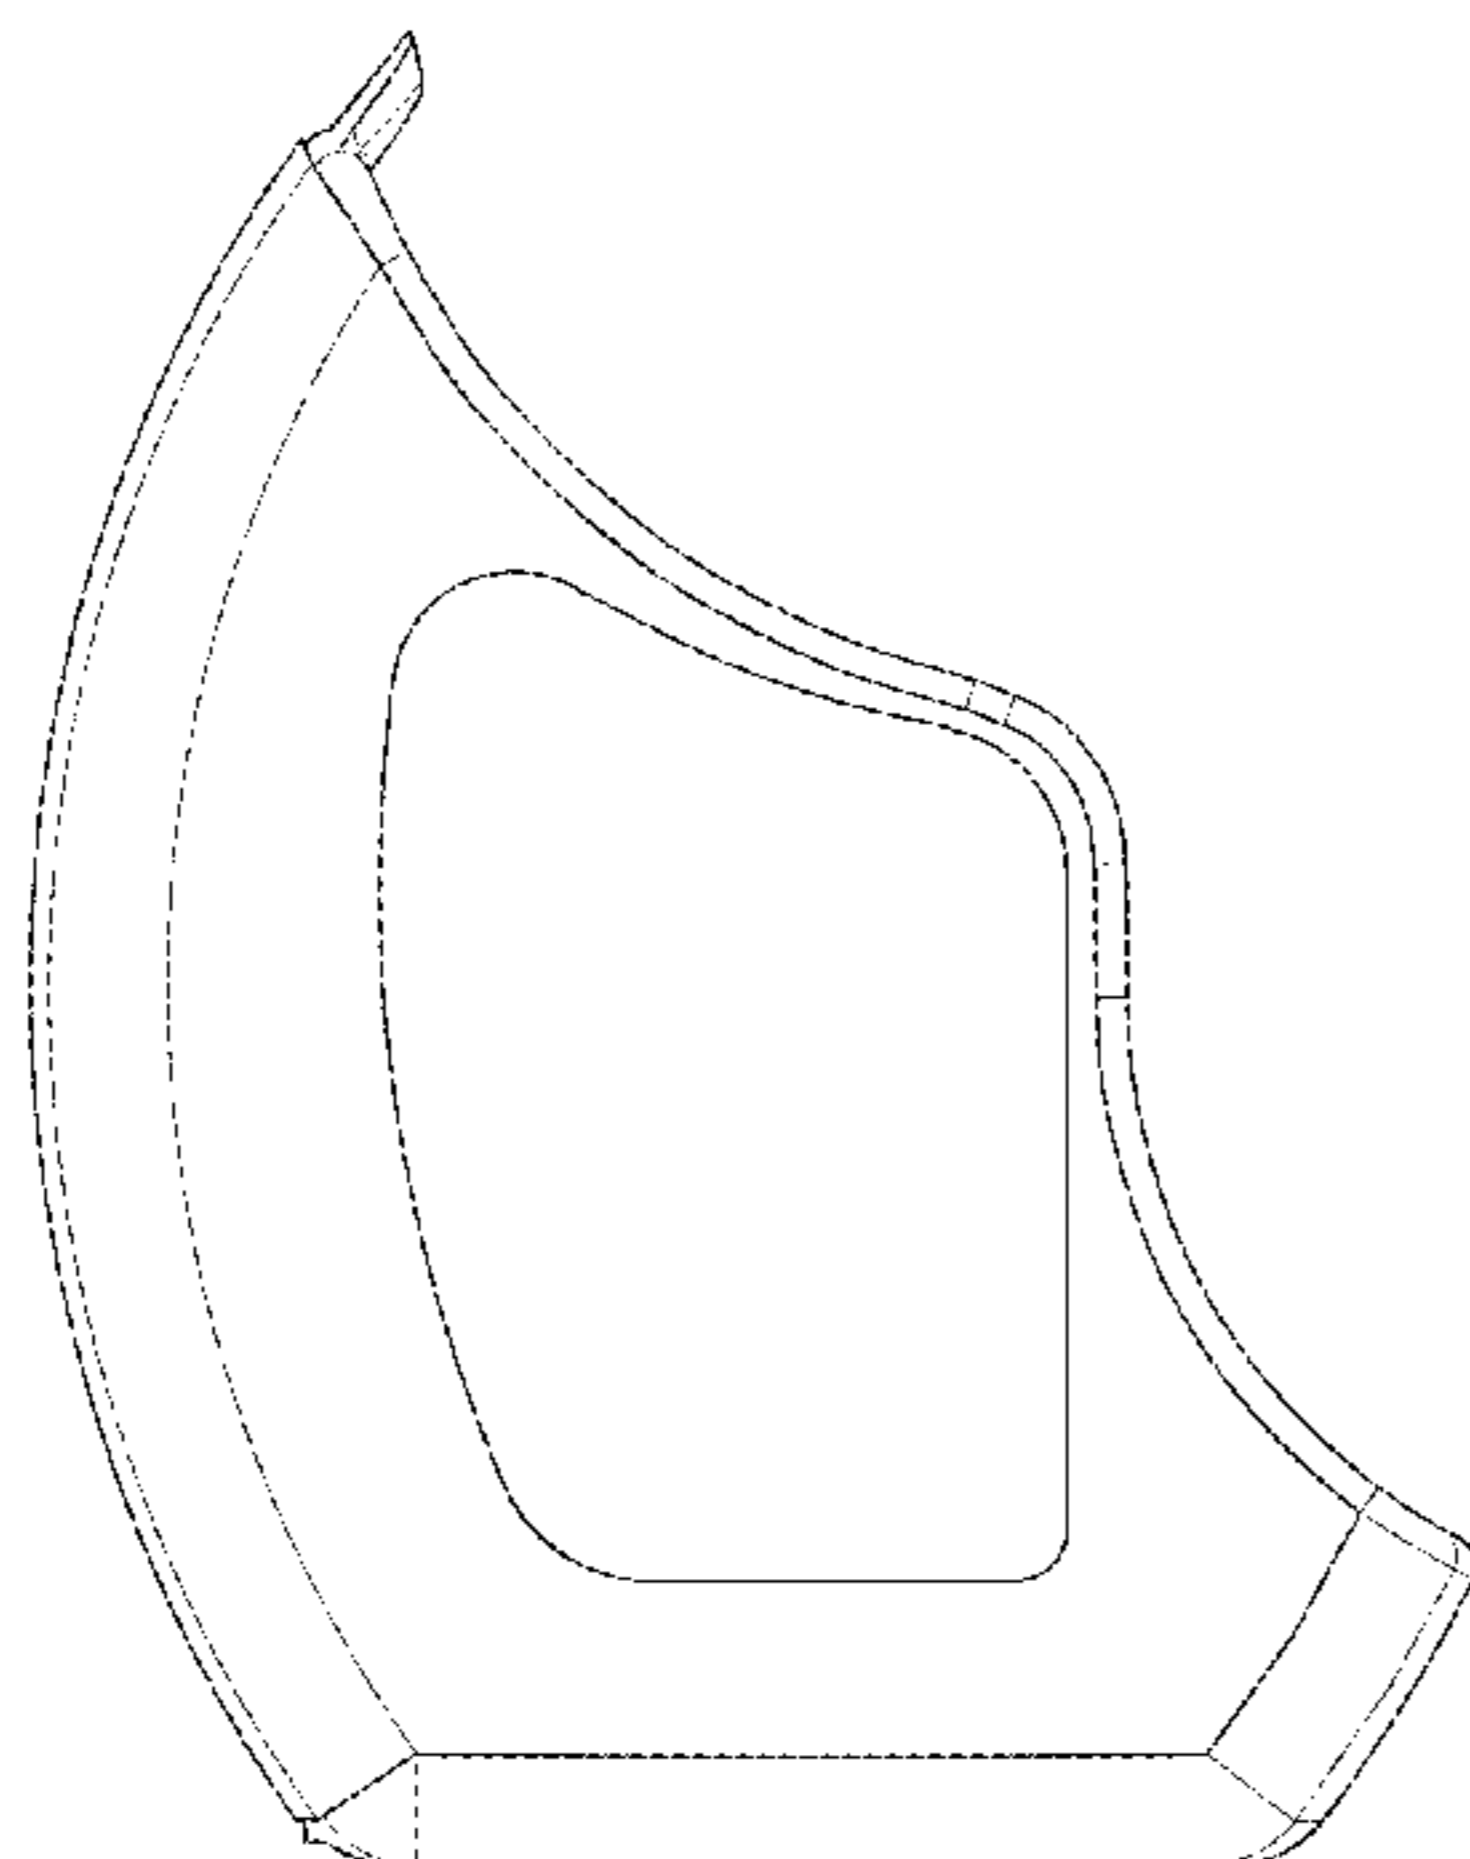

(56)

References Cited

U.S. PATENT DOCUMENTS

D677,377 S * 3/2013 White D24/110
D774,178 S * 12/2016 Van Sickle D24/110
D777,904 S * 1/2017 Van Sickle D24/110
D818,112 S * 5/2018 Van Sickle D24/110
2005/0174216 A1* 8/2005 Lintell A61M 15/0083
340/309.16
2005/0177275 A1* 8/2005 Harvey G04F 1/005
700/244
2007/0052544 A1* 3/2007 Lintell A61J 7/0481
340/815.4
2007/0125372 A1* 6/2007 Chen A61M 15/0065
128/200.23
2007/0181123 A1* 8/2007 Houzego A61M 15/0045
128/203.15
2008/0196718 A1* 8/2008 Connell A61M 15/0045
128/203.15
2008/0308102 A1* 12/2008 Davies A61M 15/0045
128/203.15

* cited by examiner

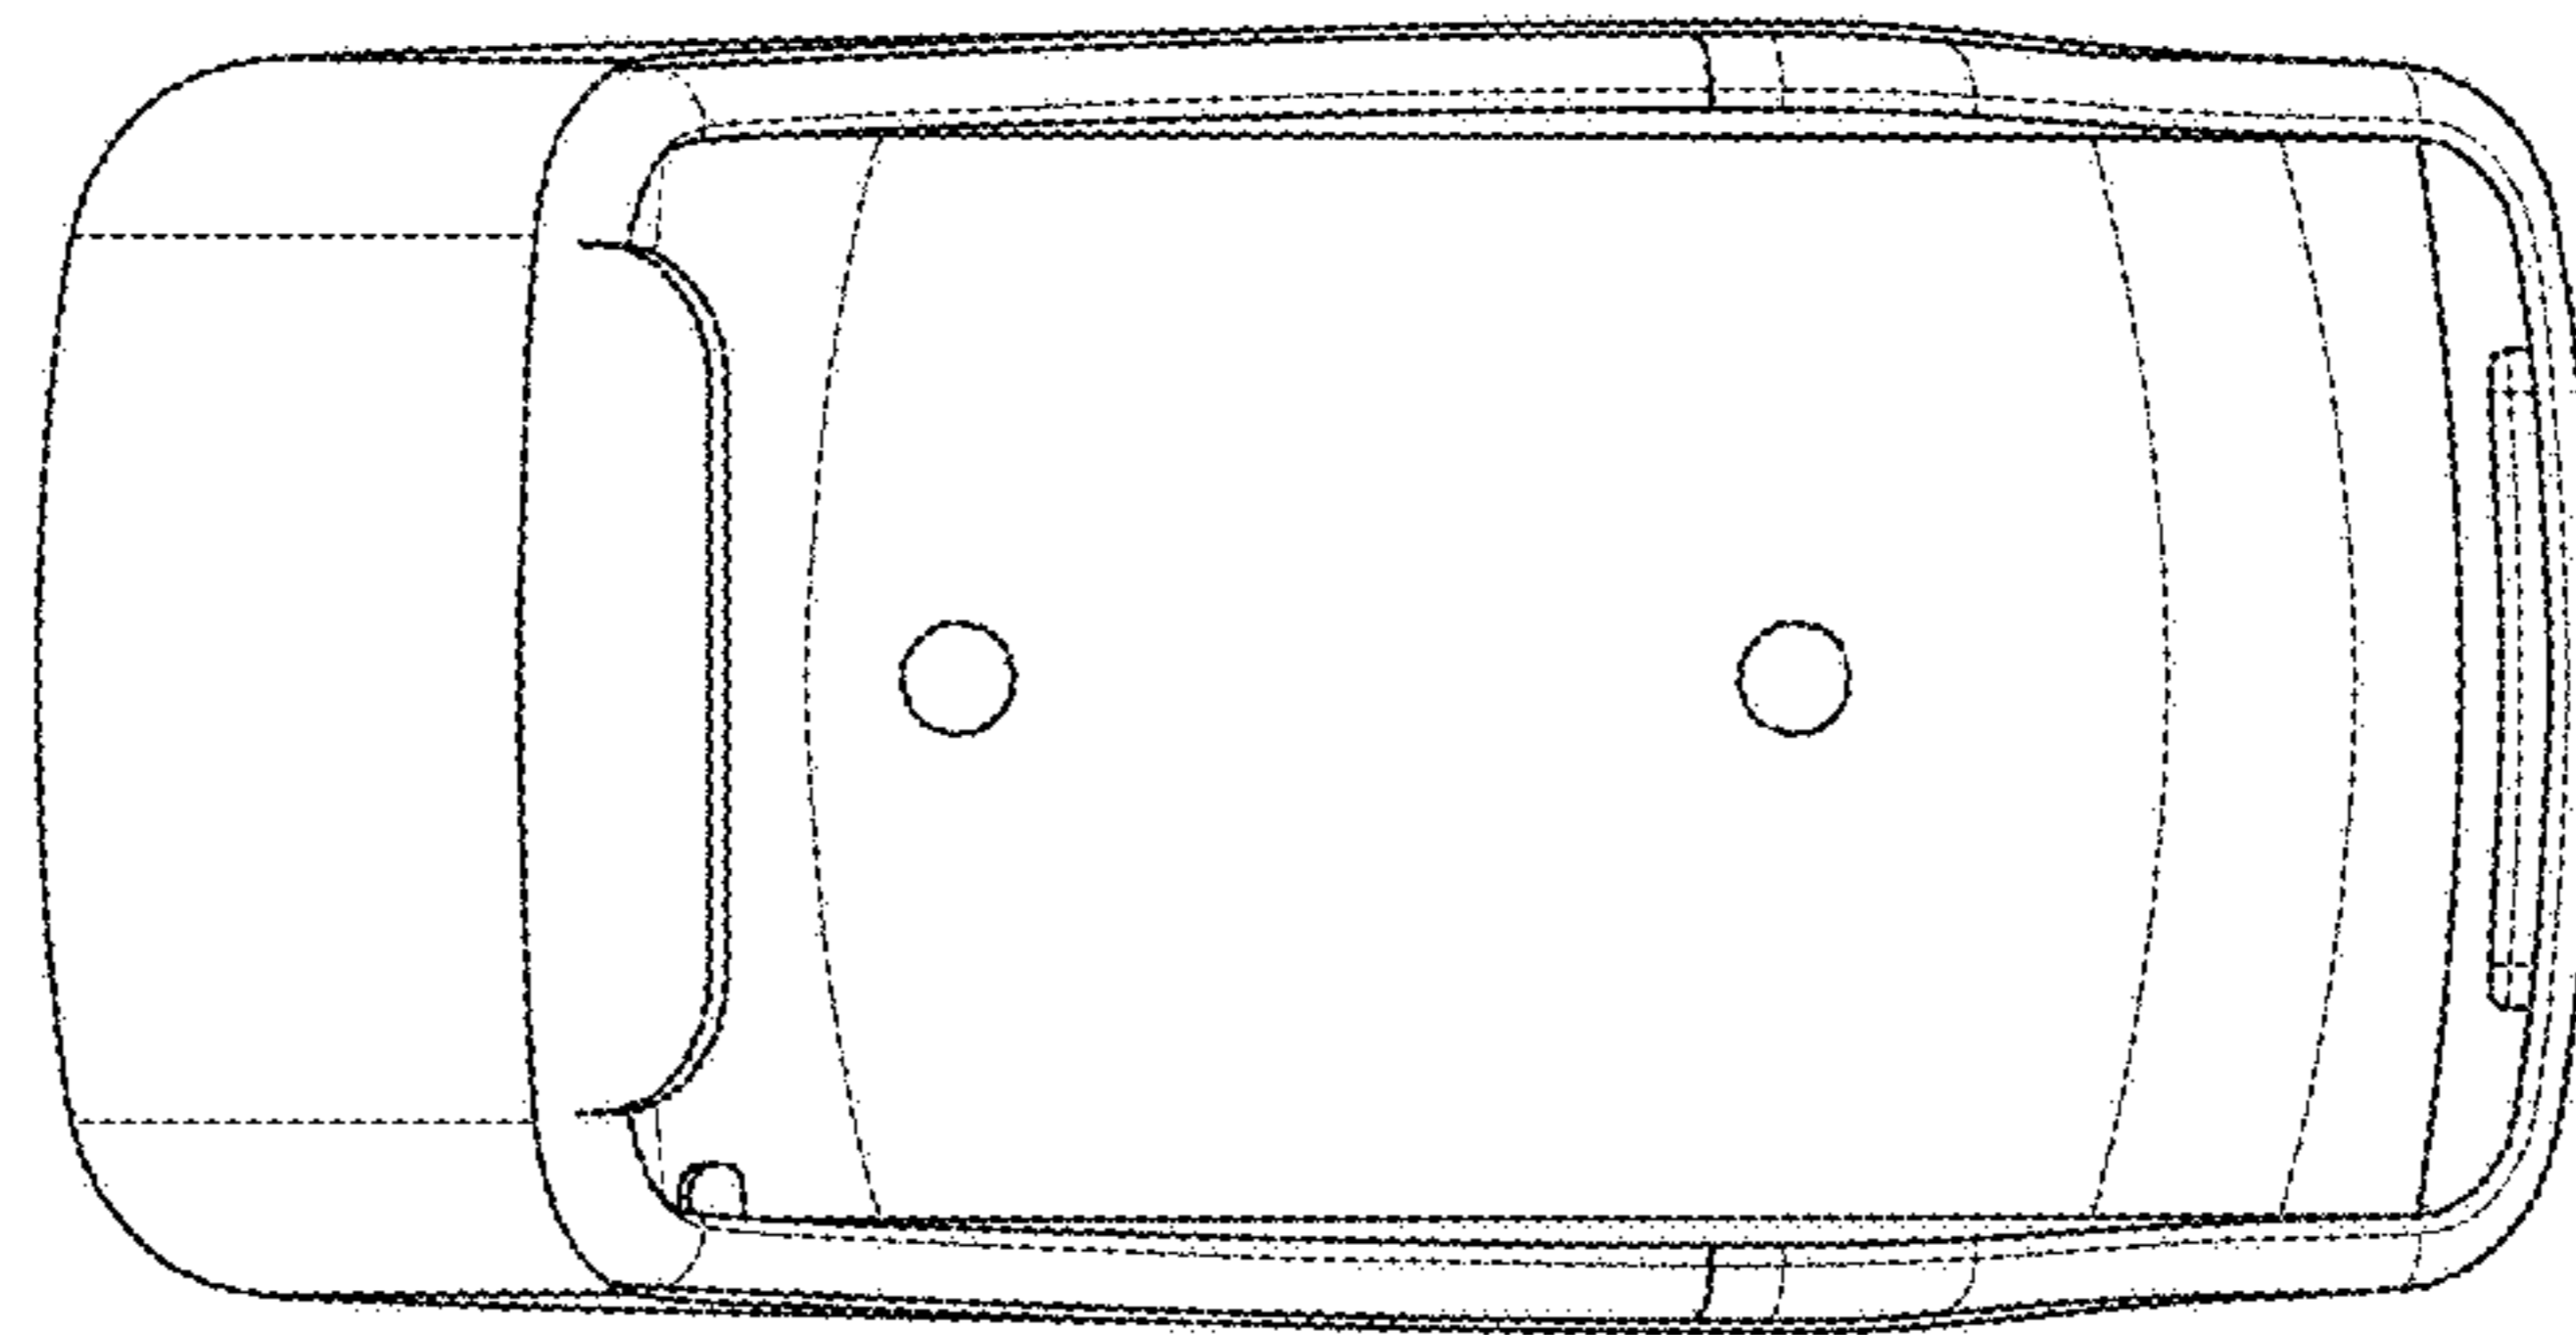


FIG. 1

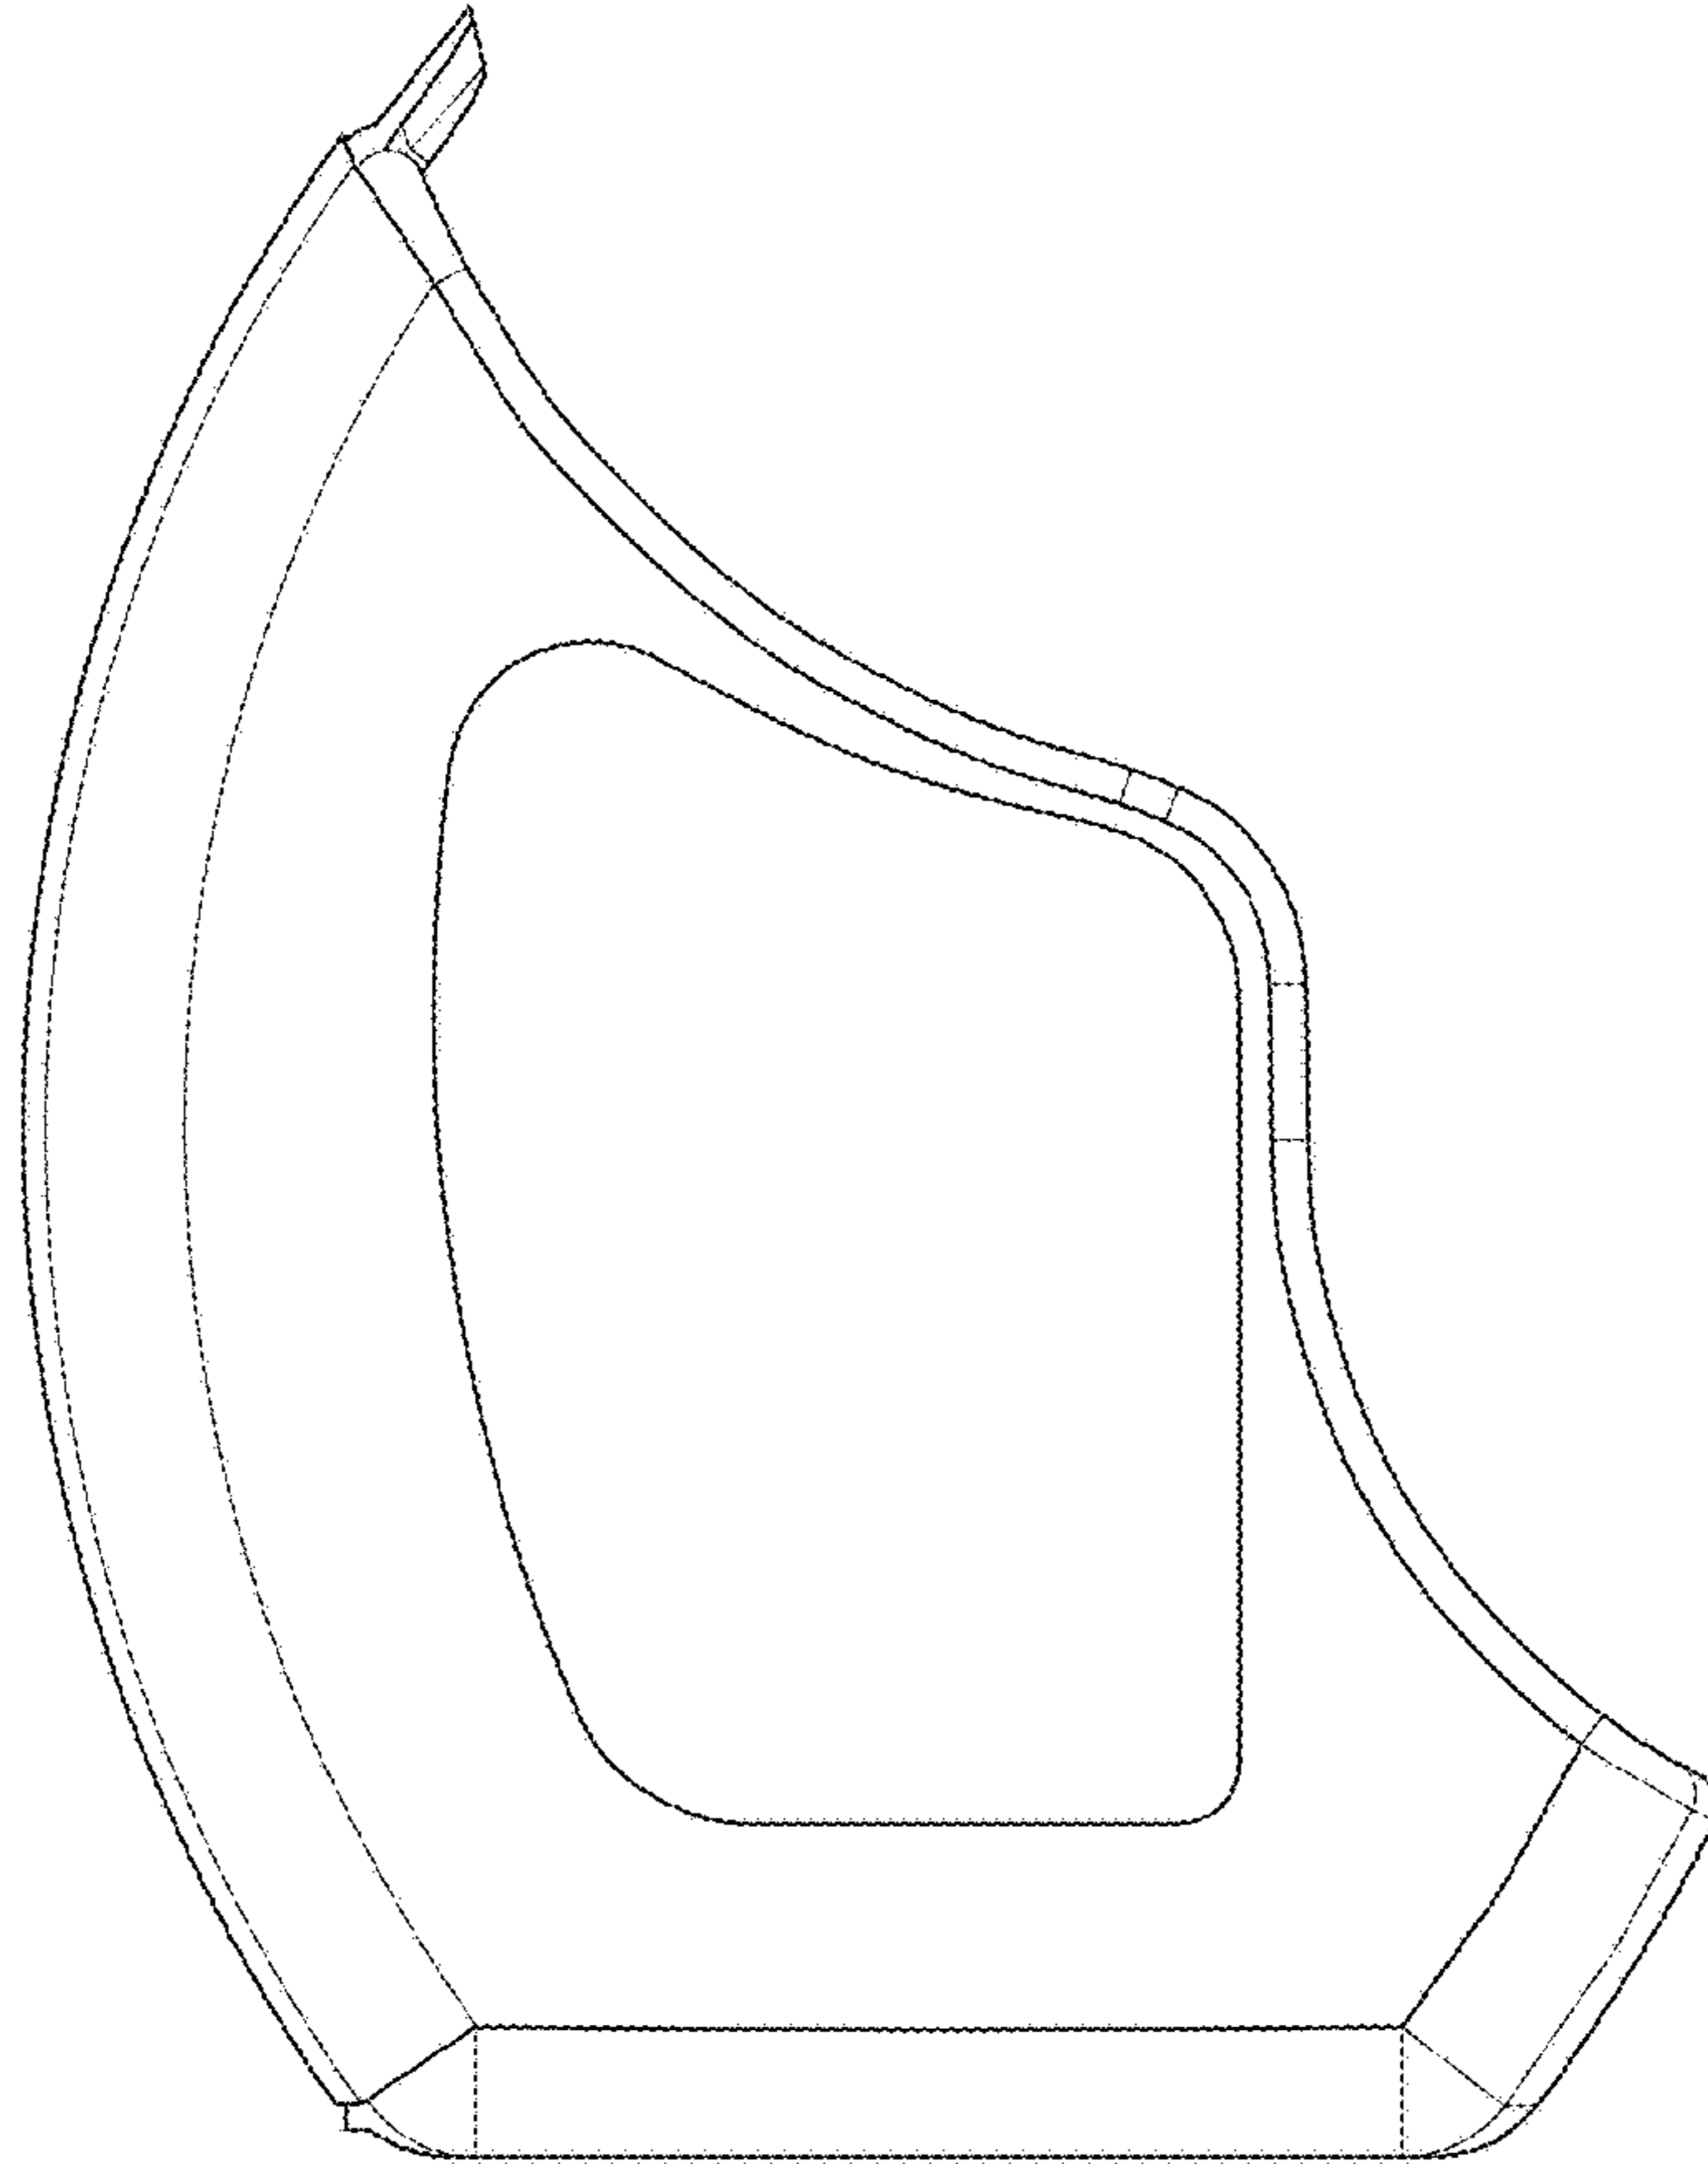


FIG. 2

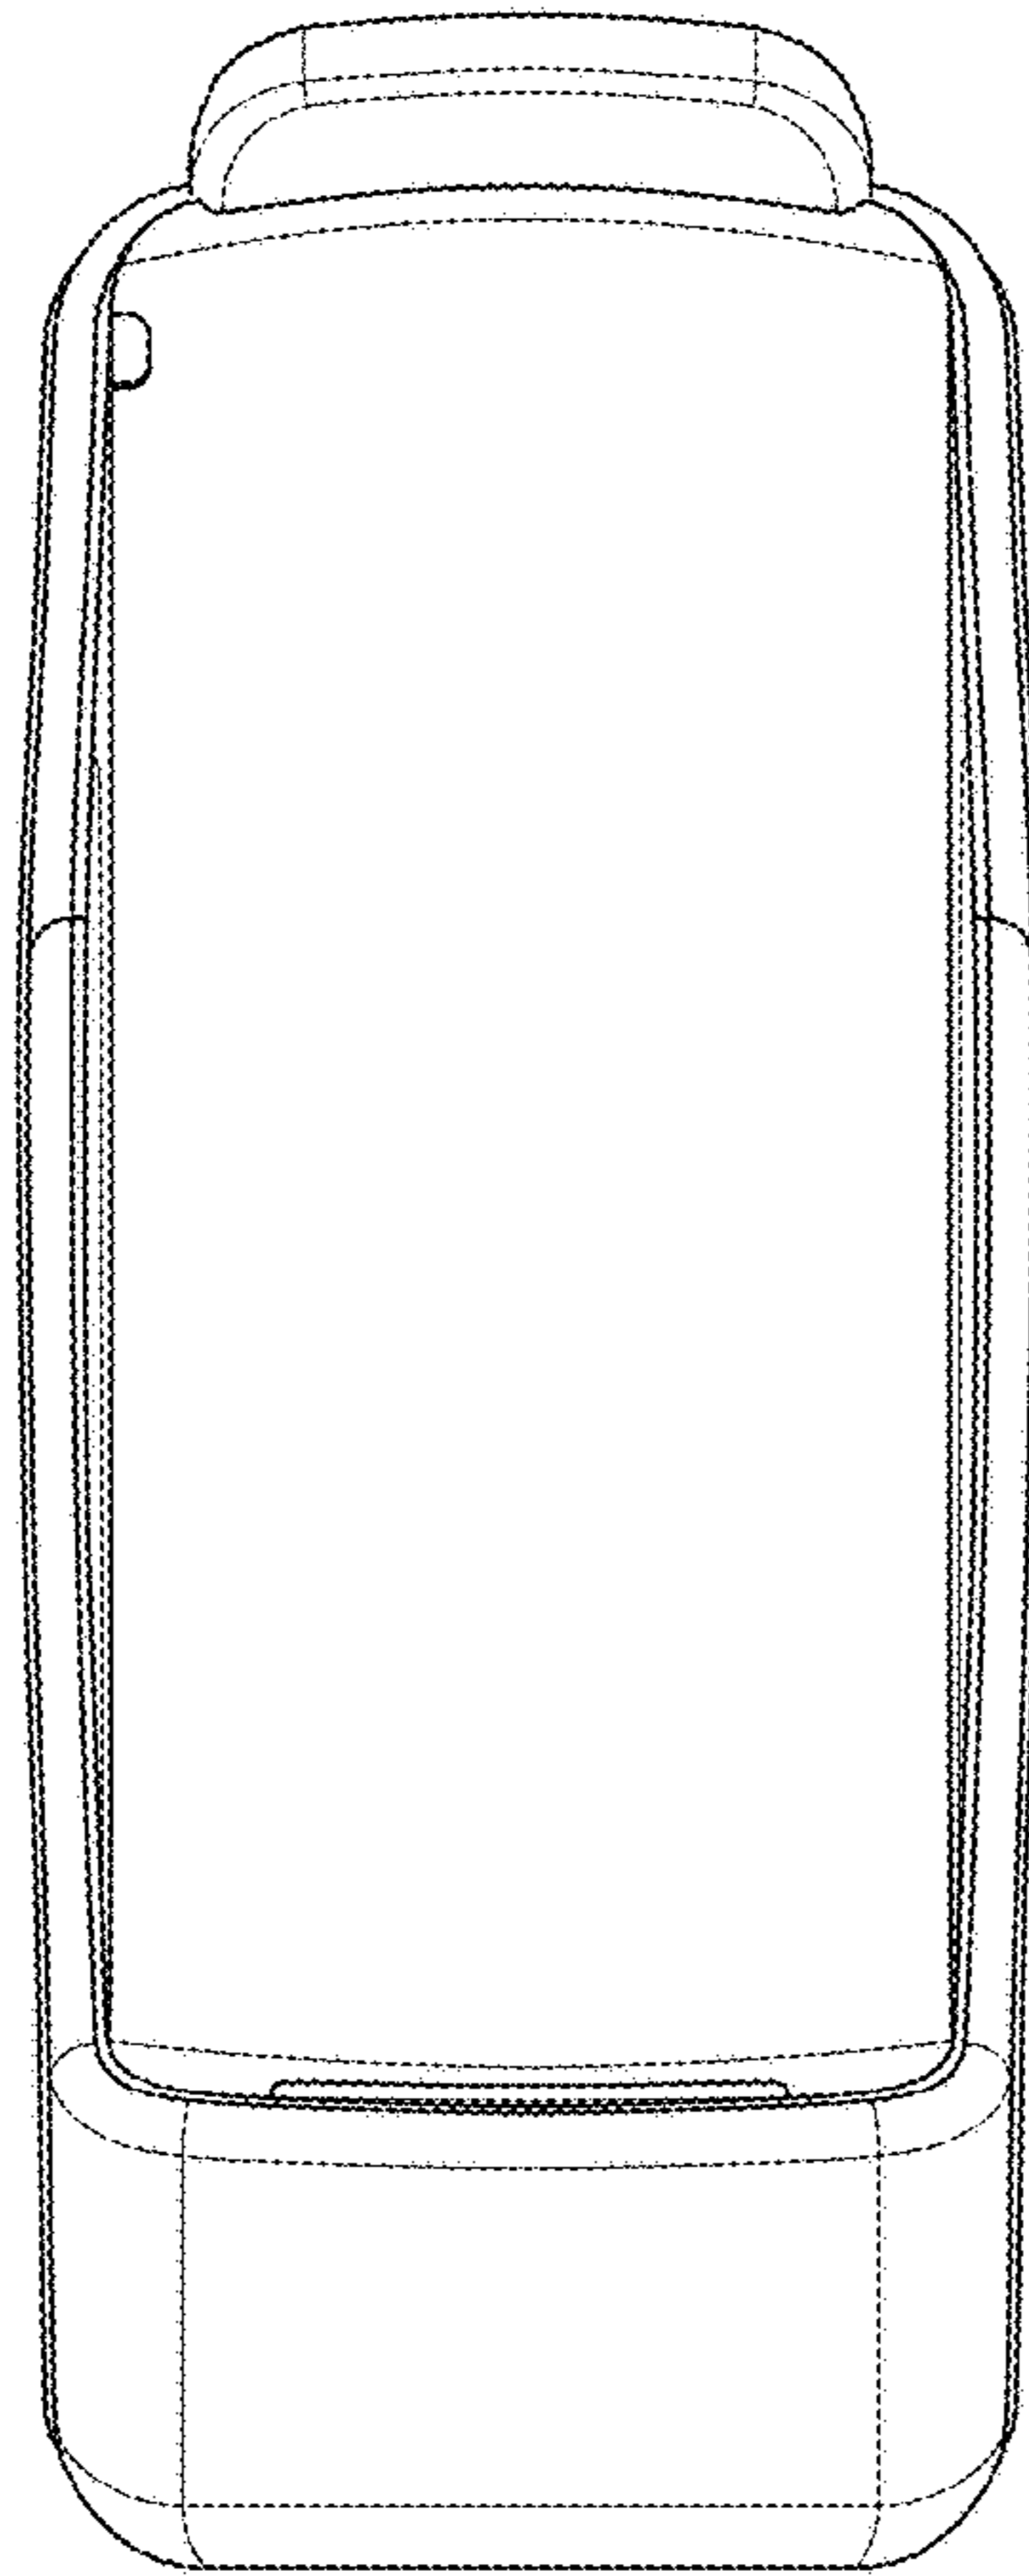


FIG. 3

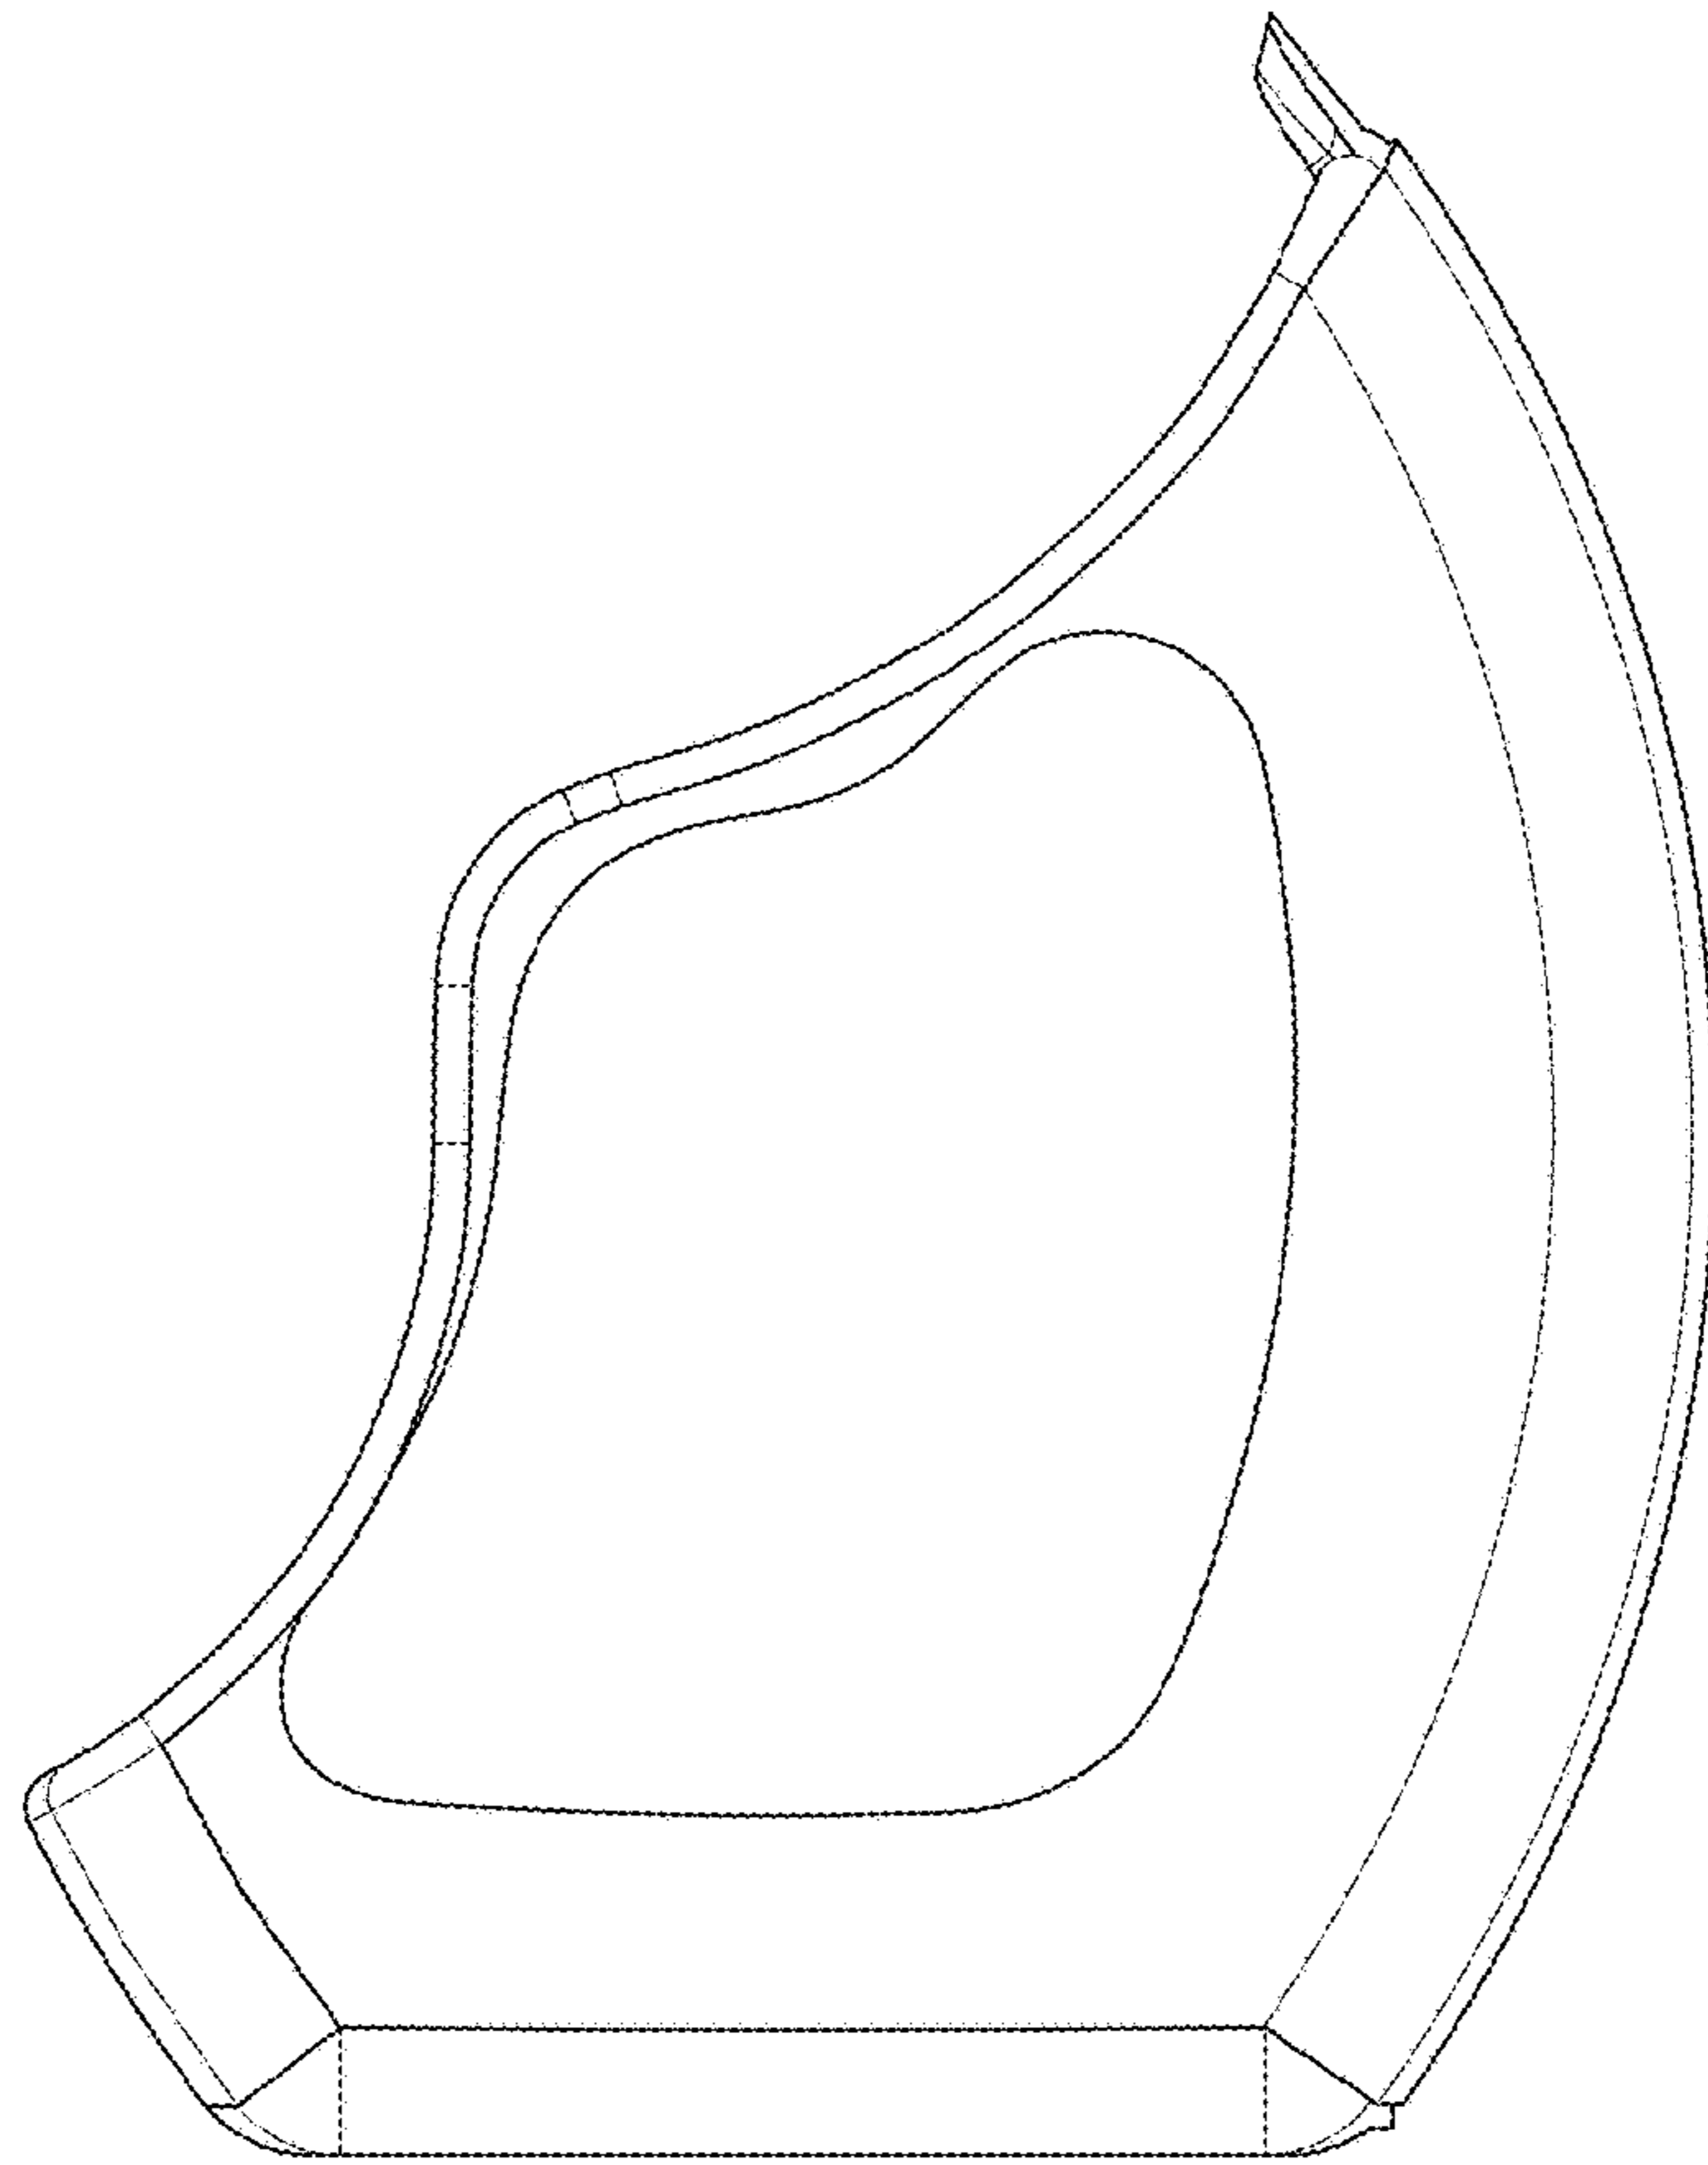


FIG. 4

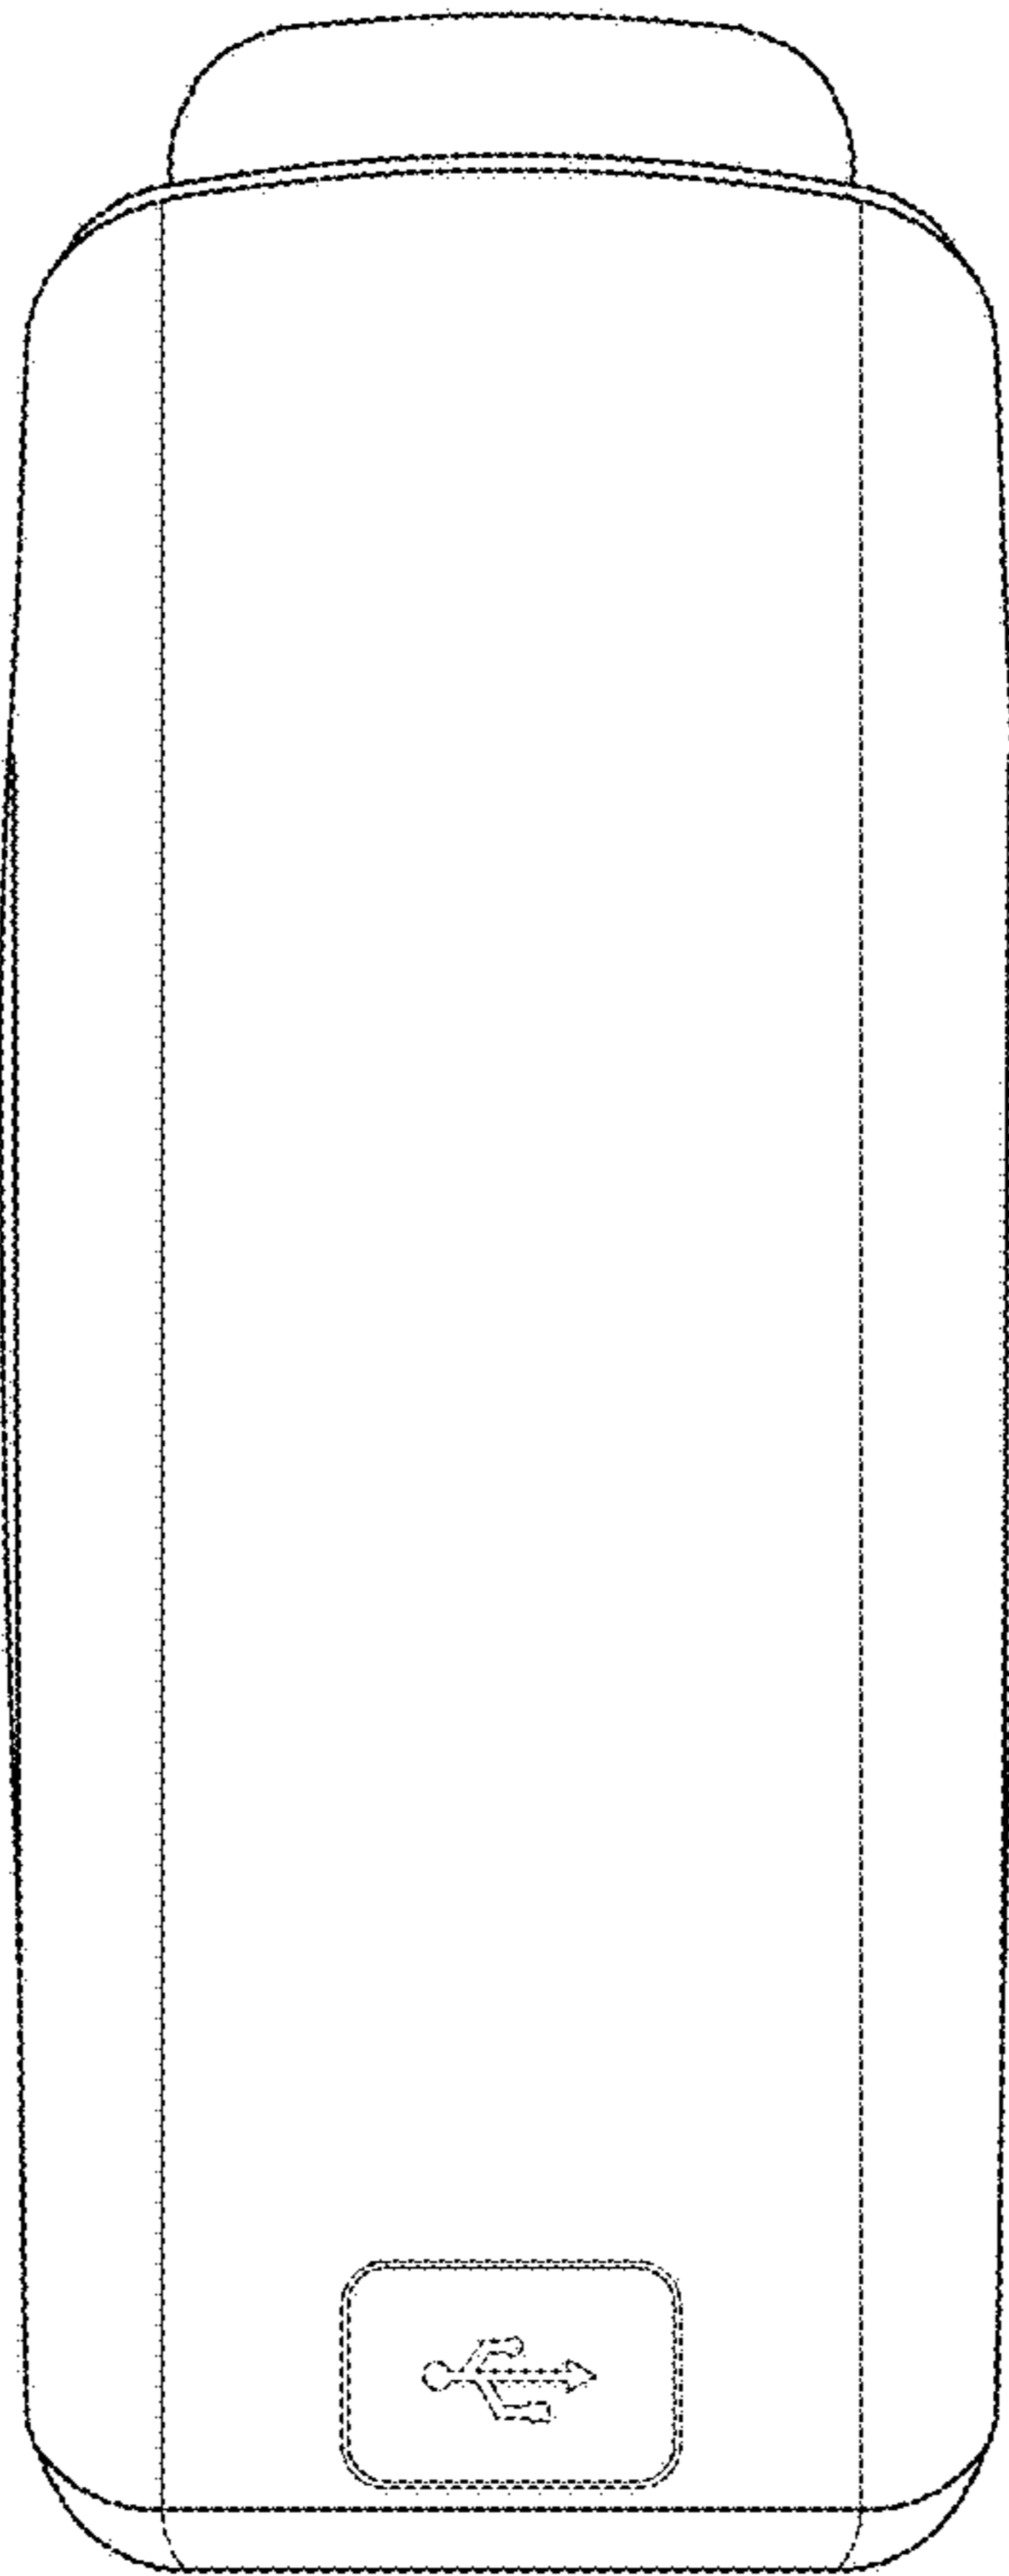


FIG. 5

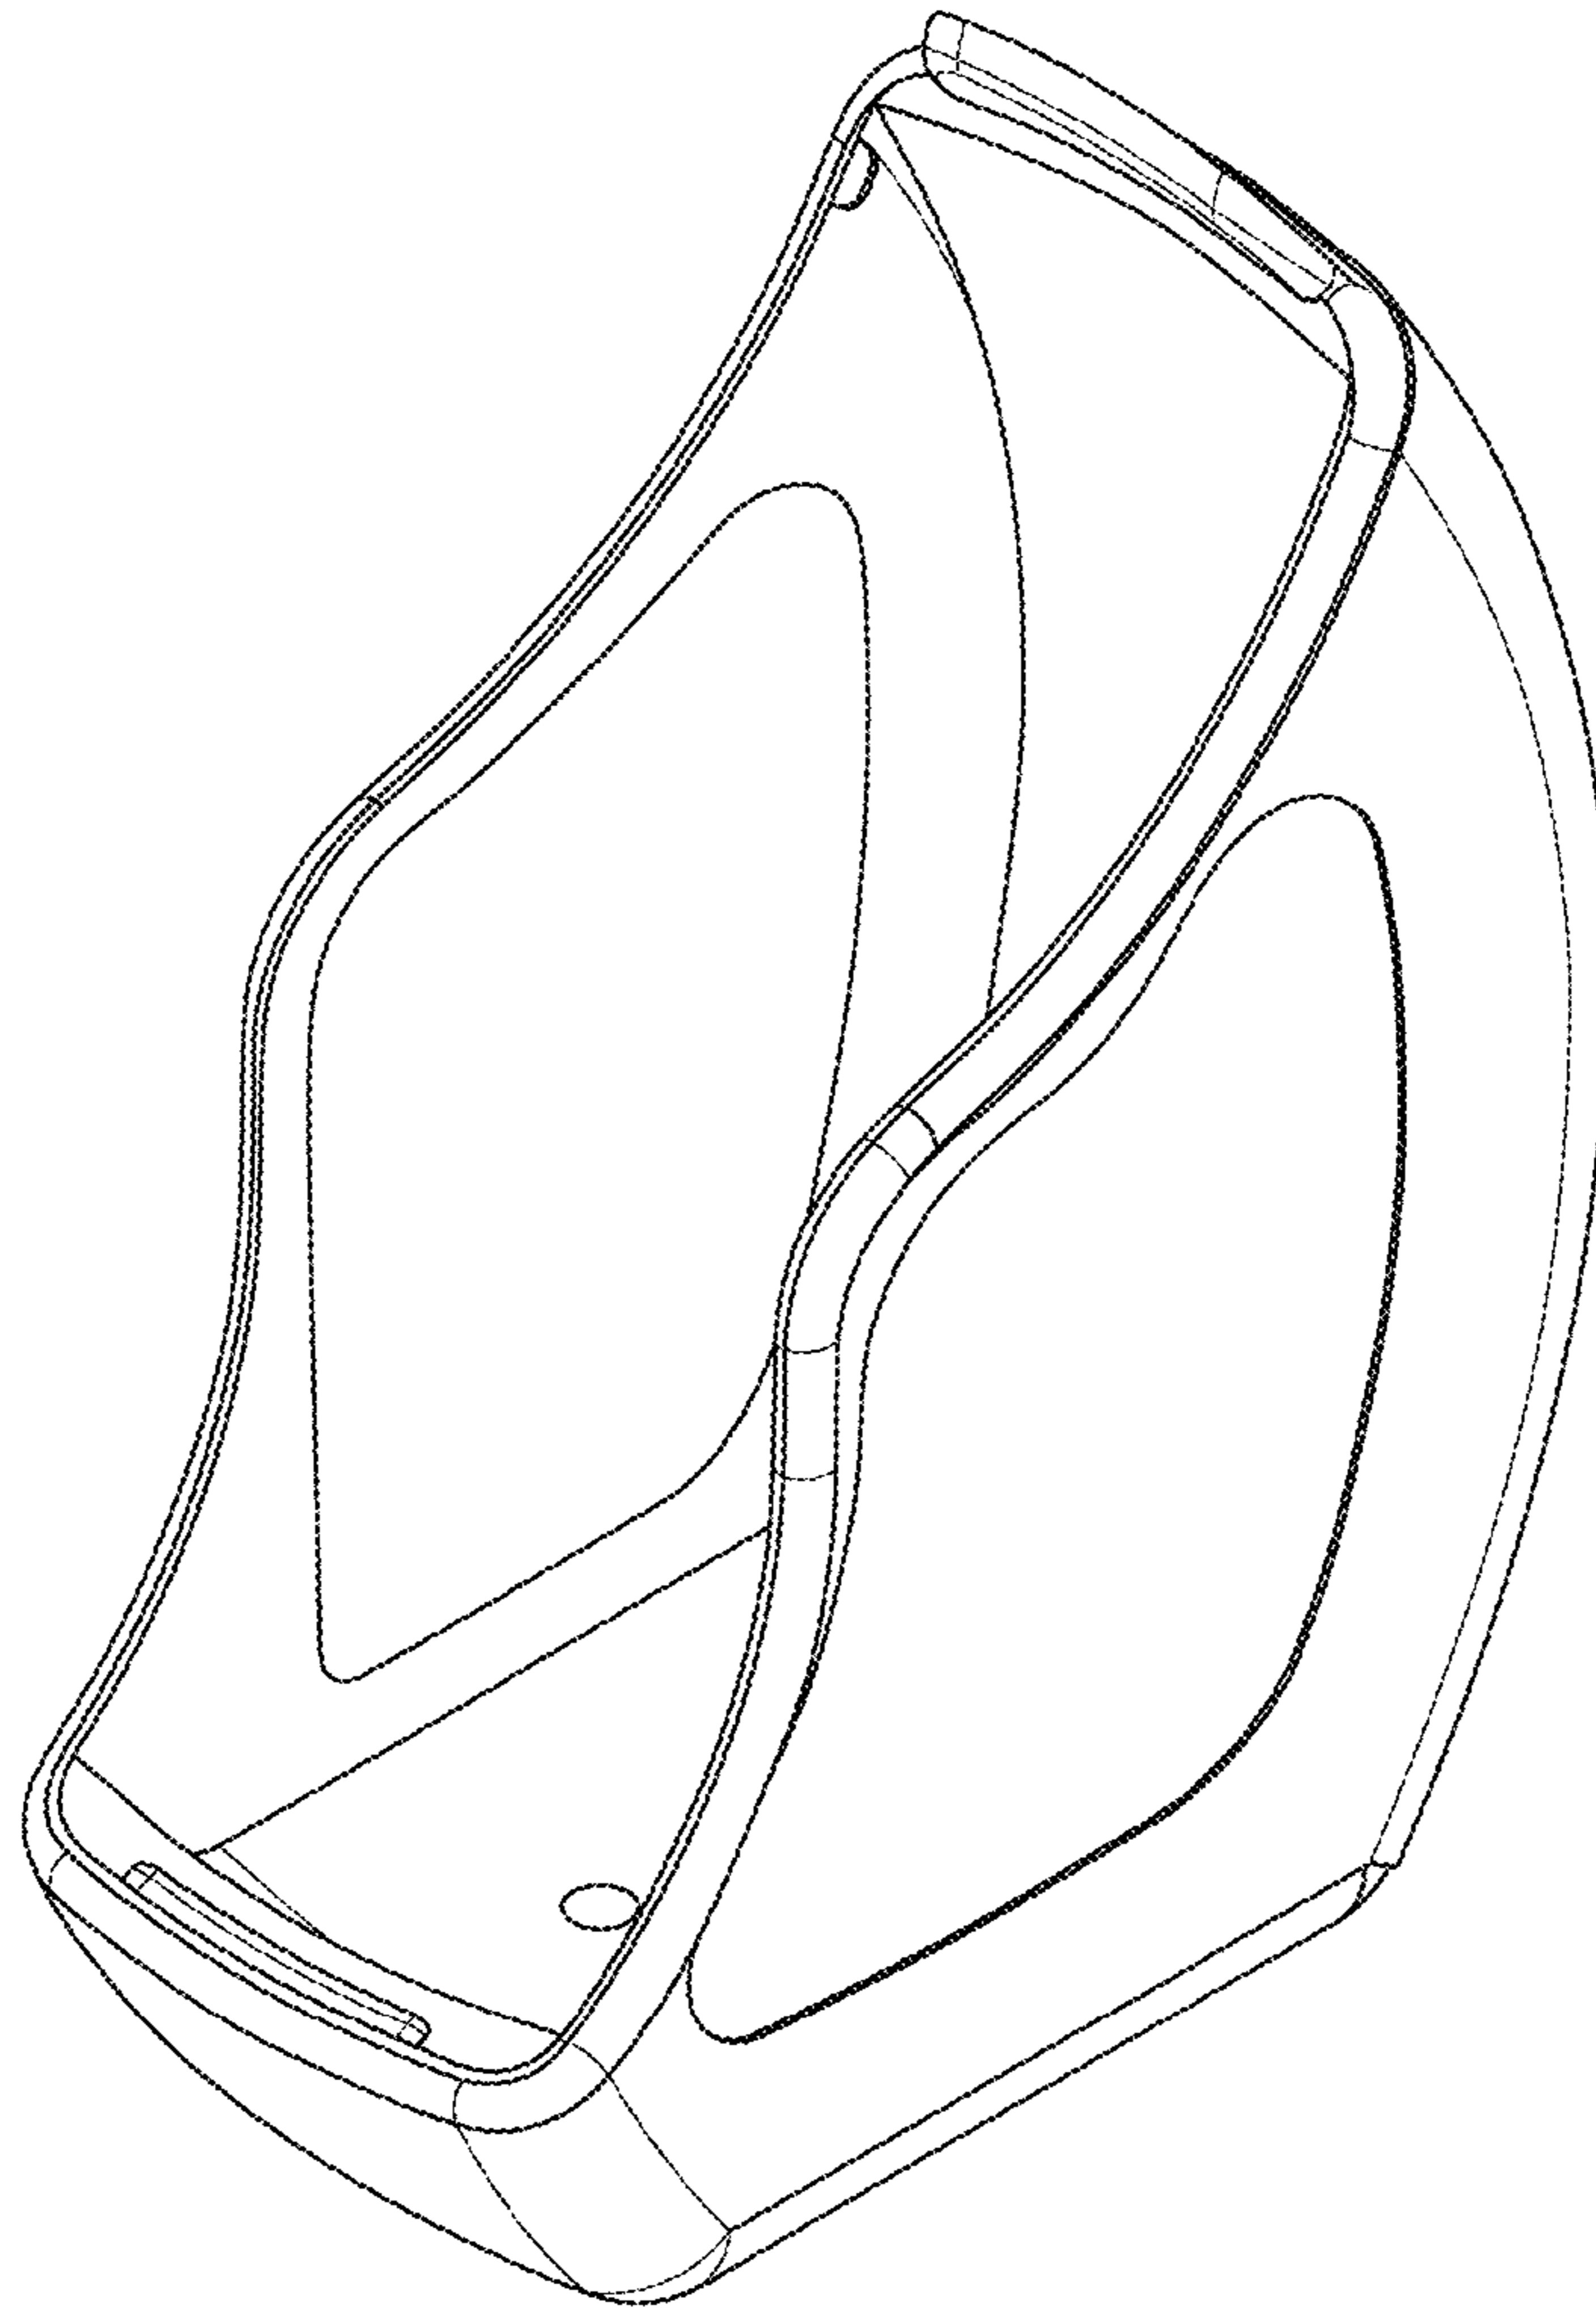


FIG. 6

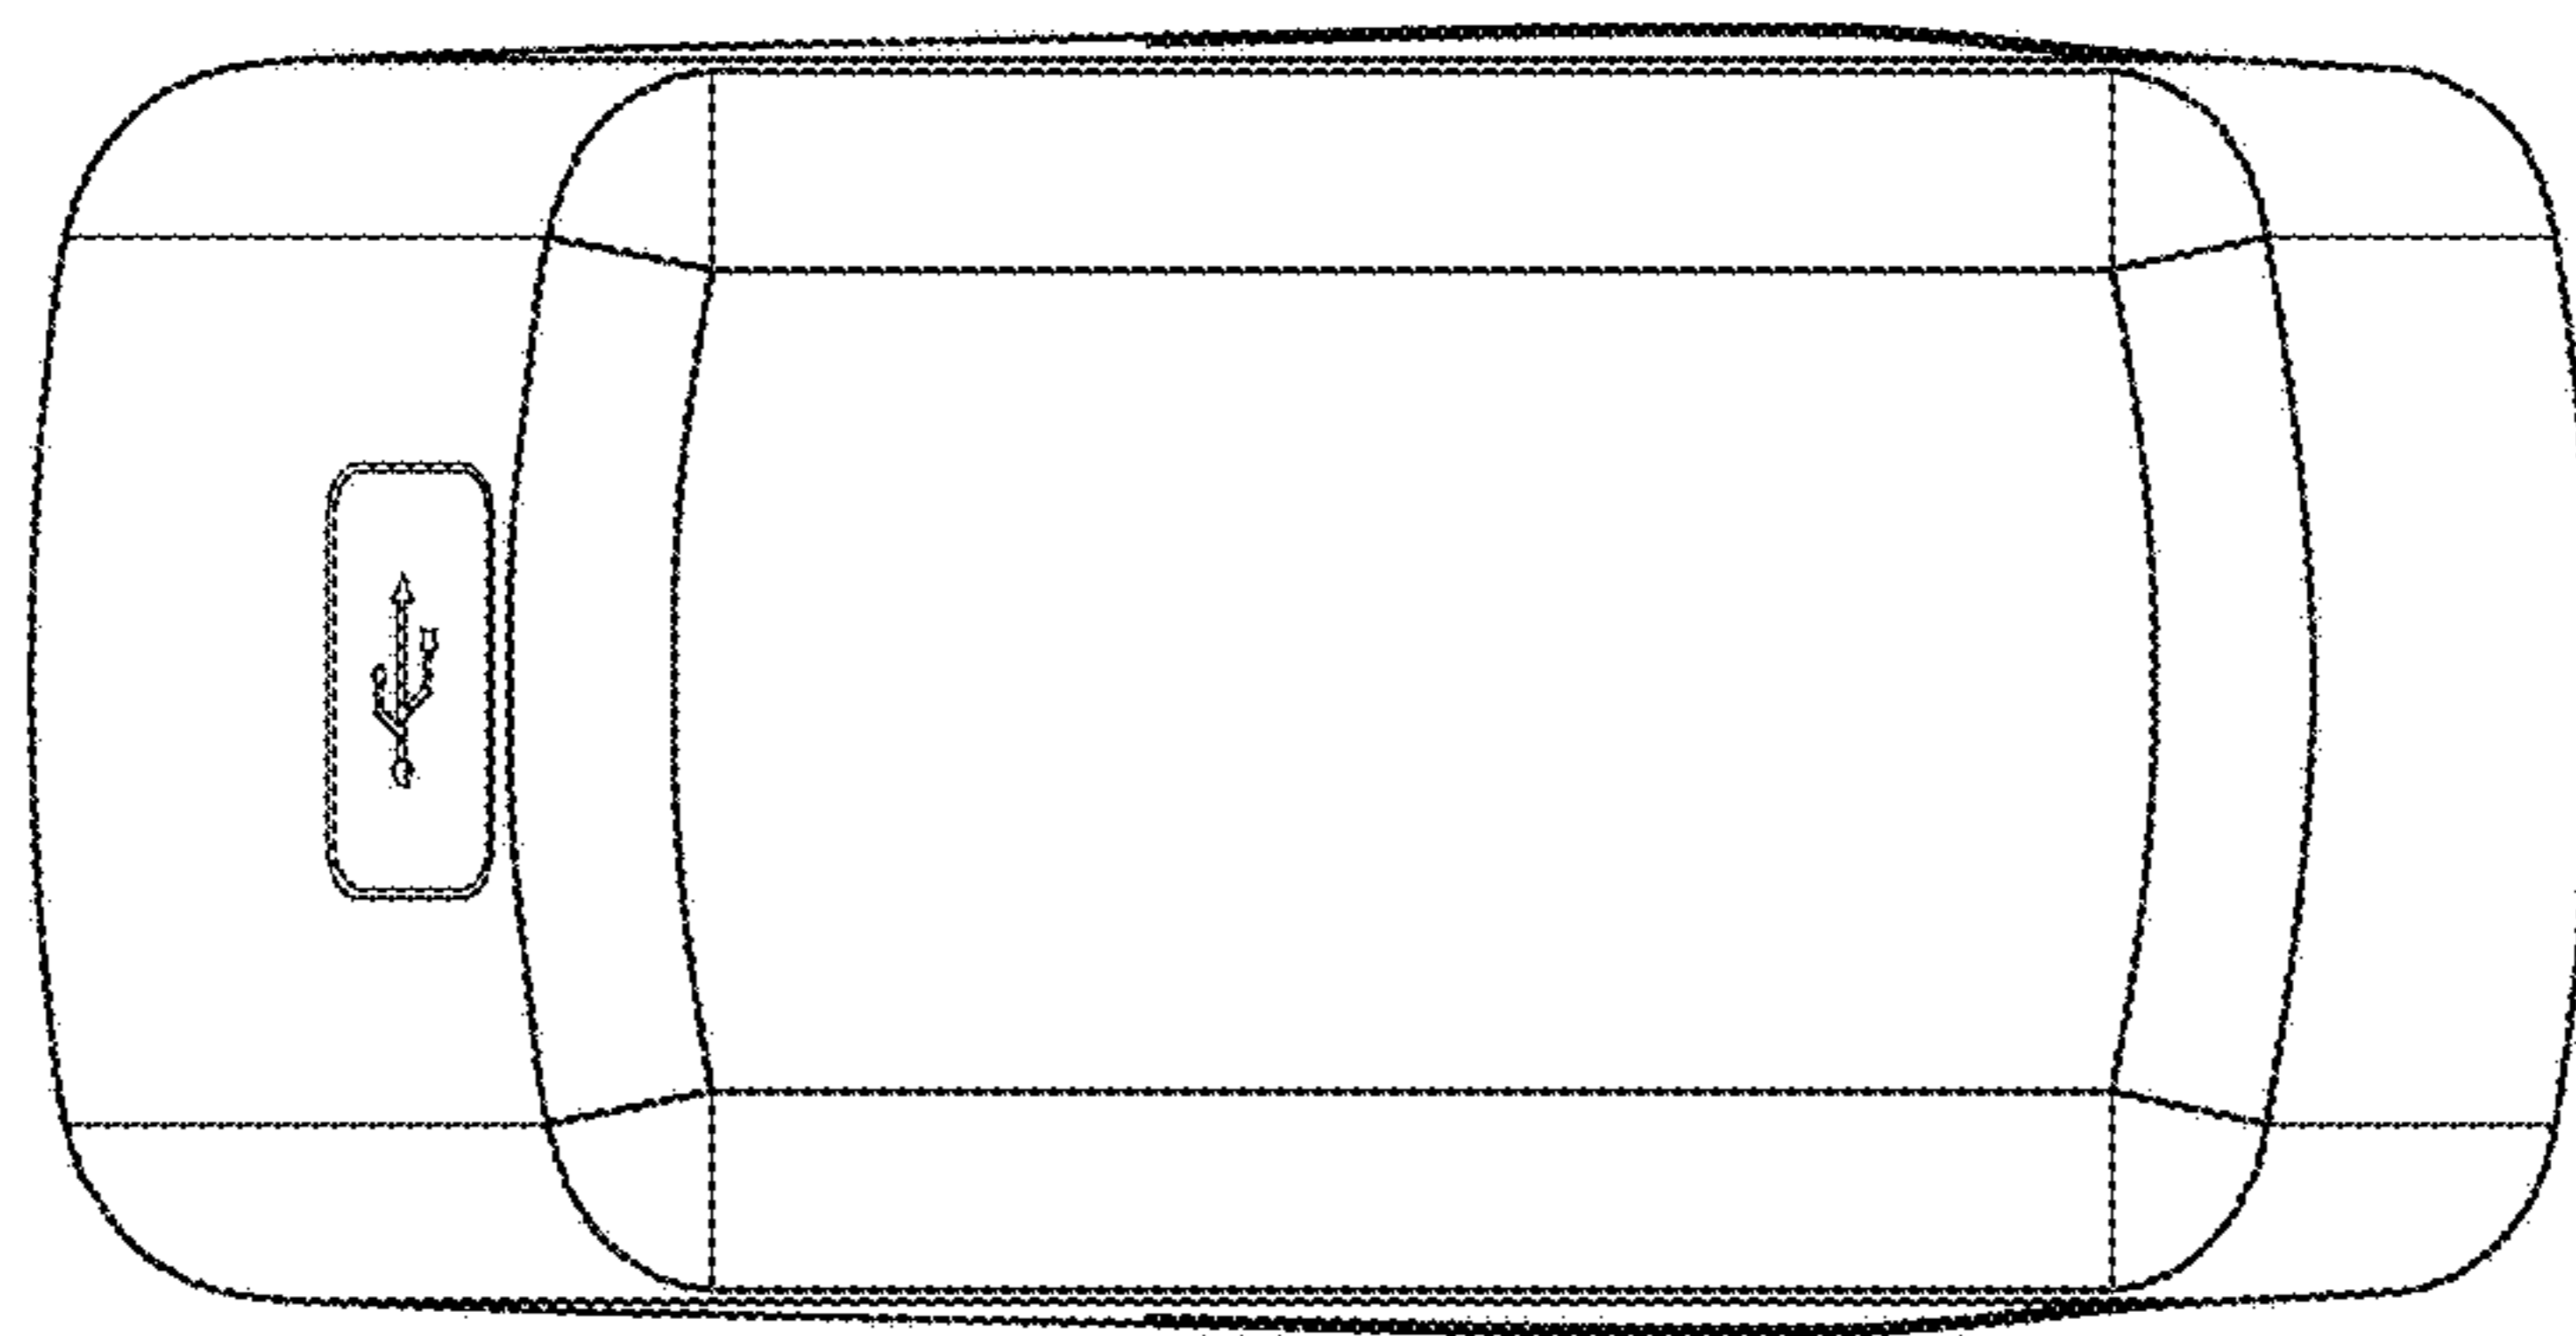


FIG. 7