



US00D862695S

(12) **United States Design Patent** (10) **Patent No.:** **US D862,695 S**
Eaves, III et al. (45) **Date of Patent:** **** Oct. 8, 2019**

(54) **MEDICAL TOOL FOR USE IN APPLYING MEDICAL ARTICLE**

(71) Applicant: **EMRGE, LLC**, Atlanta, GA (US)
(72) Inventors: **Felmont F. Eaves, III**, Atlanta, GA (US); **David O. Kazmer**, Georgetown, MA (US); **Gary W. Knight**, Lebanon, OH (US); **Timothy G. Dietz**, Reading, MA (US); **William Eugene Clem**, Bozeman, MT (US)
(73) Assignee: **EMRGE, LLC**, Atlanta, GA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/622,941**

(22) Filed: **Oct. 20, 2017**

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/143**

(58) **Field of Classification Search**
USPC D24/143, 145, 147, 148, 149, 133
CPC A61B 17/08; A61B 17/081; A61B 17/083;
A61B 17/085; A61B 17/086; A61B 17/088; A61B 17/10
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,254,620 A 9/1941 Miller
3,487,836 A 1/1970 Niebel et al.
4,702,251 A 10/1987 Sheehan

(Continued)

FOREIGN PATENT DOCUMENTS

AU 2012236205 B2 8/2016
AU 2016262734 12/2016

(Continued)

OTHER PUBLICATIONS

International Federation of Red Cross and Red Crescent Societies.
Link: <https://itemscatalogue.redcross.int/detail.aspx?itemcode=XSINMEDI173682&from=kit>. Dec. 31, 2018. Forceps, soft tissue, Duval—Standard products catalogue IFRC ICRC. (Year: 2018).*

(Continued)

Primary Examiner — Susan Bennett Hattan
Assistant Examiner — Lauren D McVey
(74) *Attorney, Agent, or Firm* — Additon, Higgins & Pendleton, P.A.


(57) **CLAIM**

The ornamental design for a medical tool for use in applying medical article, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a medical tool for use in applying a medical article, in accordance with the present invention;
FIG. 2 is a front elevation view of the medical tool of FIG. 1;
FIG. 3 is a rear elevation view of the medical tool of FIG. 1;
FIG. 4 is a right elevation view of the medical tool of FIG. 1;
FIG. 5 is a left elevation view of the medical tool of FIG. 1;
FIG. 6 is a top plan view of the medical tool of FIG. 1; and,
FIG. 7 is a bottom plan view of the medical tool of FIG. 1.
The dot-dash and evenly spaced broken lines immediately adjacent to the shaded areas depict the bounds of the claimed design, while all other broken lines are directed to environment. The broken lines form no part of the claimed design.

1 Claim, 5 Drawing Sheets

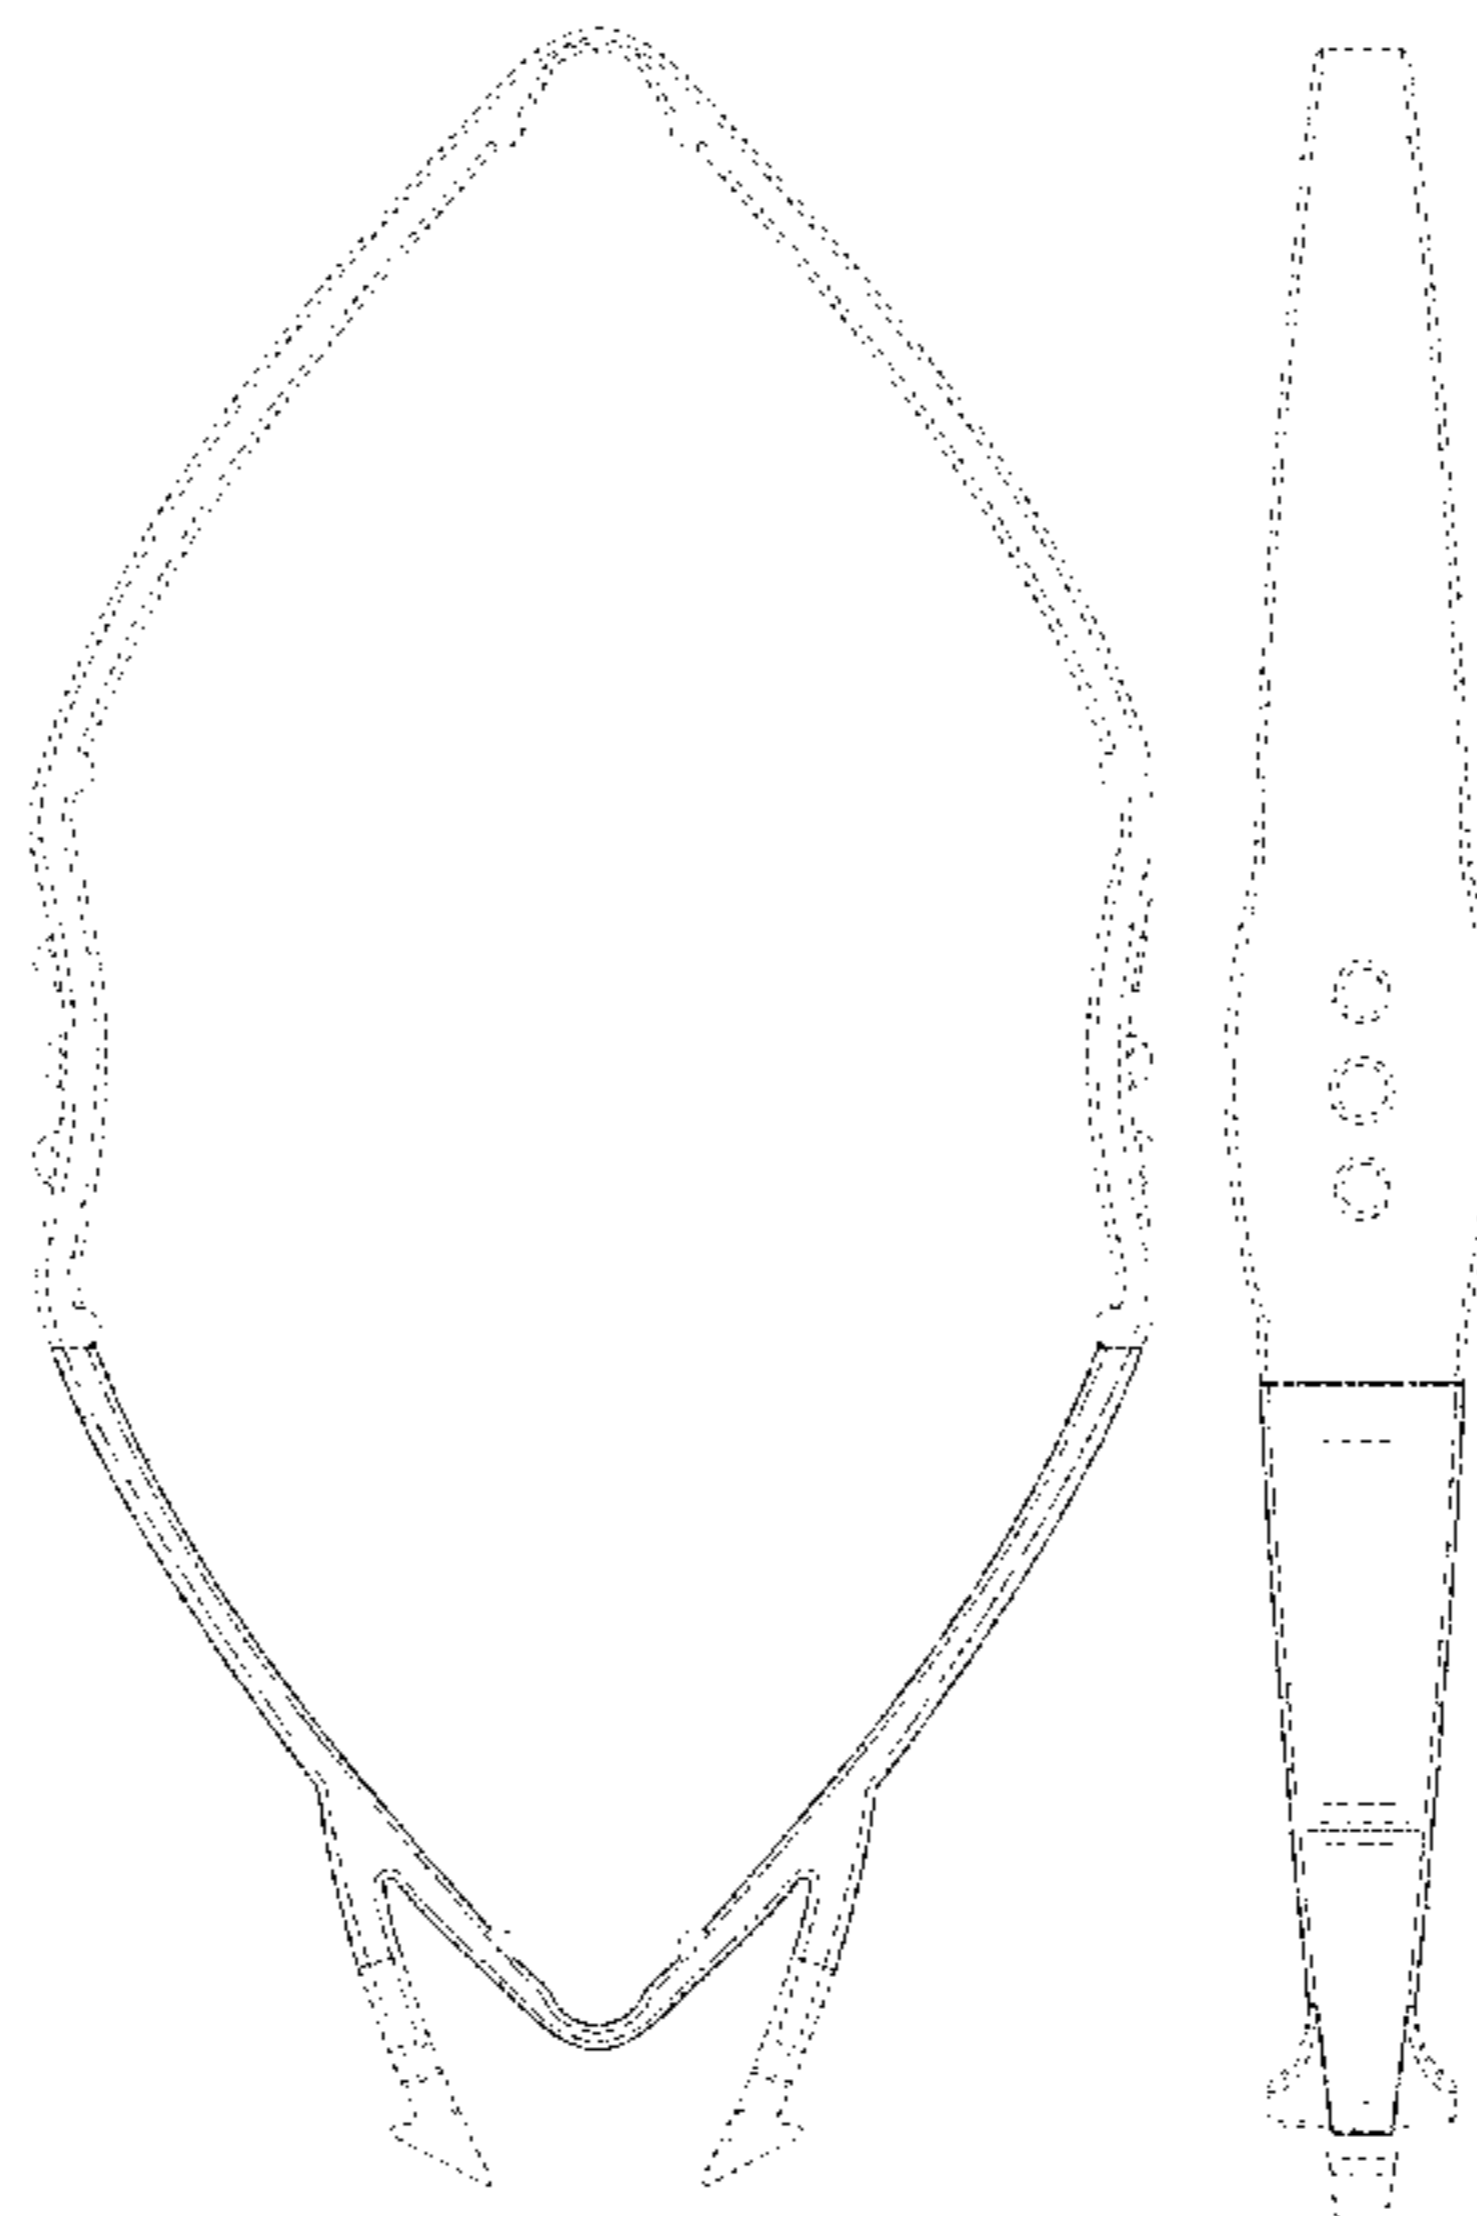

(56)

References Cited

U.S. PATENT DOCUMENTS

D331,527 S * 12/1992 Feng D8/52
 5,230,701 A 7/1993 Meyer et al.
 6,056,342 A * 5/2000 Chan A47G 21/10
 294/33
 6,176,868 B1 1/2001 Detour
 6,210,419 B1 * 4/2001 Mayenberger A61B 17/122
 606/120
 6,261,303 B1 * 7/2001 Mayenberger A61B 17/122
 606/151
 D450,571 S * 11/2001 Chen D8/395
 7,332,641 B2 2/2008 Lebner et al.
 D566,271 S * 4/2008 Gao D24/143
 D610,684 S * 2/2010 Gaydos D24/143
 D610,685 S * 2/2010 Gaydos D24/143
 D617,002 S * 6/2010 Lundkvist D24/227
 8,157,839 B2 4/2012 Riskin et al.
 8,246,590 B2 8/2012 Hu et al.
 8,435,221 B2 5/2013 Hu et al.
 8,562,576 B2 10/2013 Hu et al.
 D709,195 S * 7/2014 Peck D24/143
 8,834,434 B2 9/2014 Hu et al.
 9,028,529 B2 5/2015 Riskin et al.
 9,301,760 B2 4/2016 Fox
 D764,057 S * 8/2016 Schaffner D24/143
 9,421,133 B2 8/2016 Hu et al.
 D767,761 S * 9/2016 Babb D24/143
 9,603,596 B2 3/2017 Riskin et al.
 D828,552 S * 9/2018 Eippert D24/135
 2002/0111641 A1 8/2002 Peterson et al.
 2005/0080453 A1 4/2005 Lebner
 2009/0240186 A1 9/2009 Frang
 2009/0259203 A1 10/2009 Hu et al.
 2010/0081983 A1 4/2010 Zocher
 2010/0228287 A1 9/2010 Jeekel
 2010/0262126 A1 10/2010 Hu et al.
 2011/0004173 A1 1/2011 Hu et al.
 2011/0040325 A1 2/2011 Moehrl
 2011/0105963 A1 5/2011 Hu et al.
 2013/0178897 A1 7/2013 Wu et al.
 2014/0107597 A1 4/2014 Hu et al.
 2014/0128819 A1 5/2014 Eaves
 2014/0227483 A1 8/2014 Eaves
 2015/0005722 A1 1/2015 Hu et al.
 2015/0305739 A1 10/2015 Rolandi et al.
 2016/0324693 A1 11/2016 Hu et al.
 2018/0125492 A1 5/2018 Eaves

FOREIGN PATENT DOCUMENTS

CA 2830918 A1 10/2012
 CN 1889903 A 1/2007
 CN 103533900 B 12/2016
 CN 304947300 * 12/2018
 EP 2691029 * 6/2015 A61B 17/00
 FR 419096 10/1910
 JP 2011-500170 A 1/2011
 JP 2014-516288 7/2014
 KR 10-2014-0020993 2/2014
 TW M340039 U 9/2008
 WO 2009049232 A1 4/2009
 WO 2011019859 A2 2/2011
 WO 2013188884 A1 6/2012
 WO 2012/135735 A2 10/2012
 WO 2013/059600 A1 4/2013
 WO 2018/075879 A1 4/2018

OTHER PUBLICATIONS

Commonly owned U.S. Appl. No. 16/153,340, filed Oct. 5, 2018, pp. 1-111.
 Commonly owned U.S. Appl. No. 16/242,064, filed Jan. 8, 2019, pp. 1-184.
 Japanese Notice of Reasons for Rejection in related JP Application No. 2014-502866, dated Oct. 3, 2016; 9 pages.
 Supplementary Partial European Search Report for EP Application No. 12762897, dated Dec. 23, 2014, 7 pages.
 International Search Report and Written Opinion issued in PCT/US2012/031638 dated Nov. 29, 2012; 10 pages.
 Extended Search Report for related EP Application 12762897.2, dated May 27, 2015, 11 pages.
 Japanese Office Action for related JP Application No. 2014-502866, dated Dec. 10, 2015, Translation provided, 11 pages.
 Australian Patent Examination Report No. 1 in related Australian Patent Application No. 201226205, dated Aug. 28, 2015, 5 pages.
 Chinese First Office Action for related CN Application No. 201280017051.4, dated Jun. 1, 2015, Translation provided, 13 pages.
 Chinese Second Office Action for related CN Application No. 201280017051.4, dated Dec. 31, 2015, Translation provided, 8 pages.

* cited by examiner

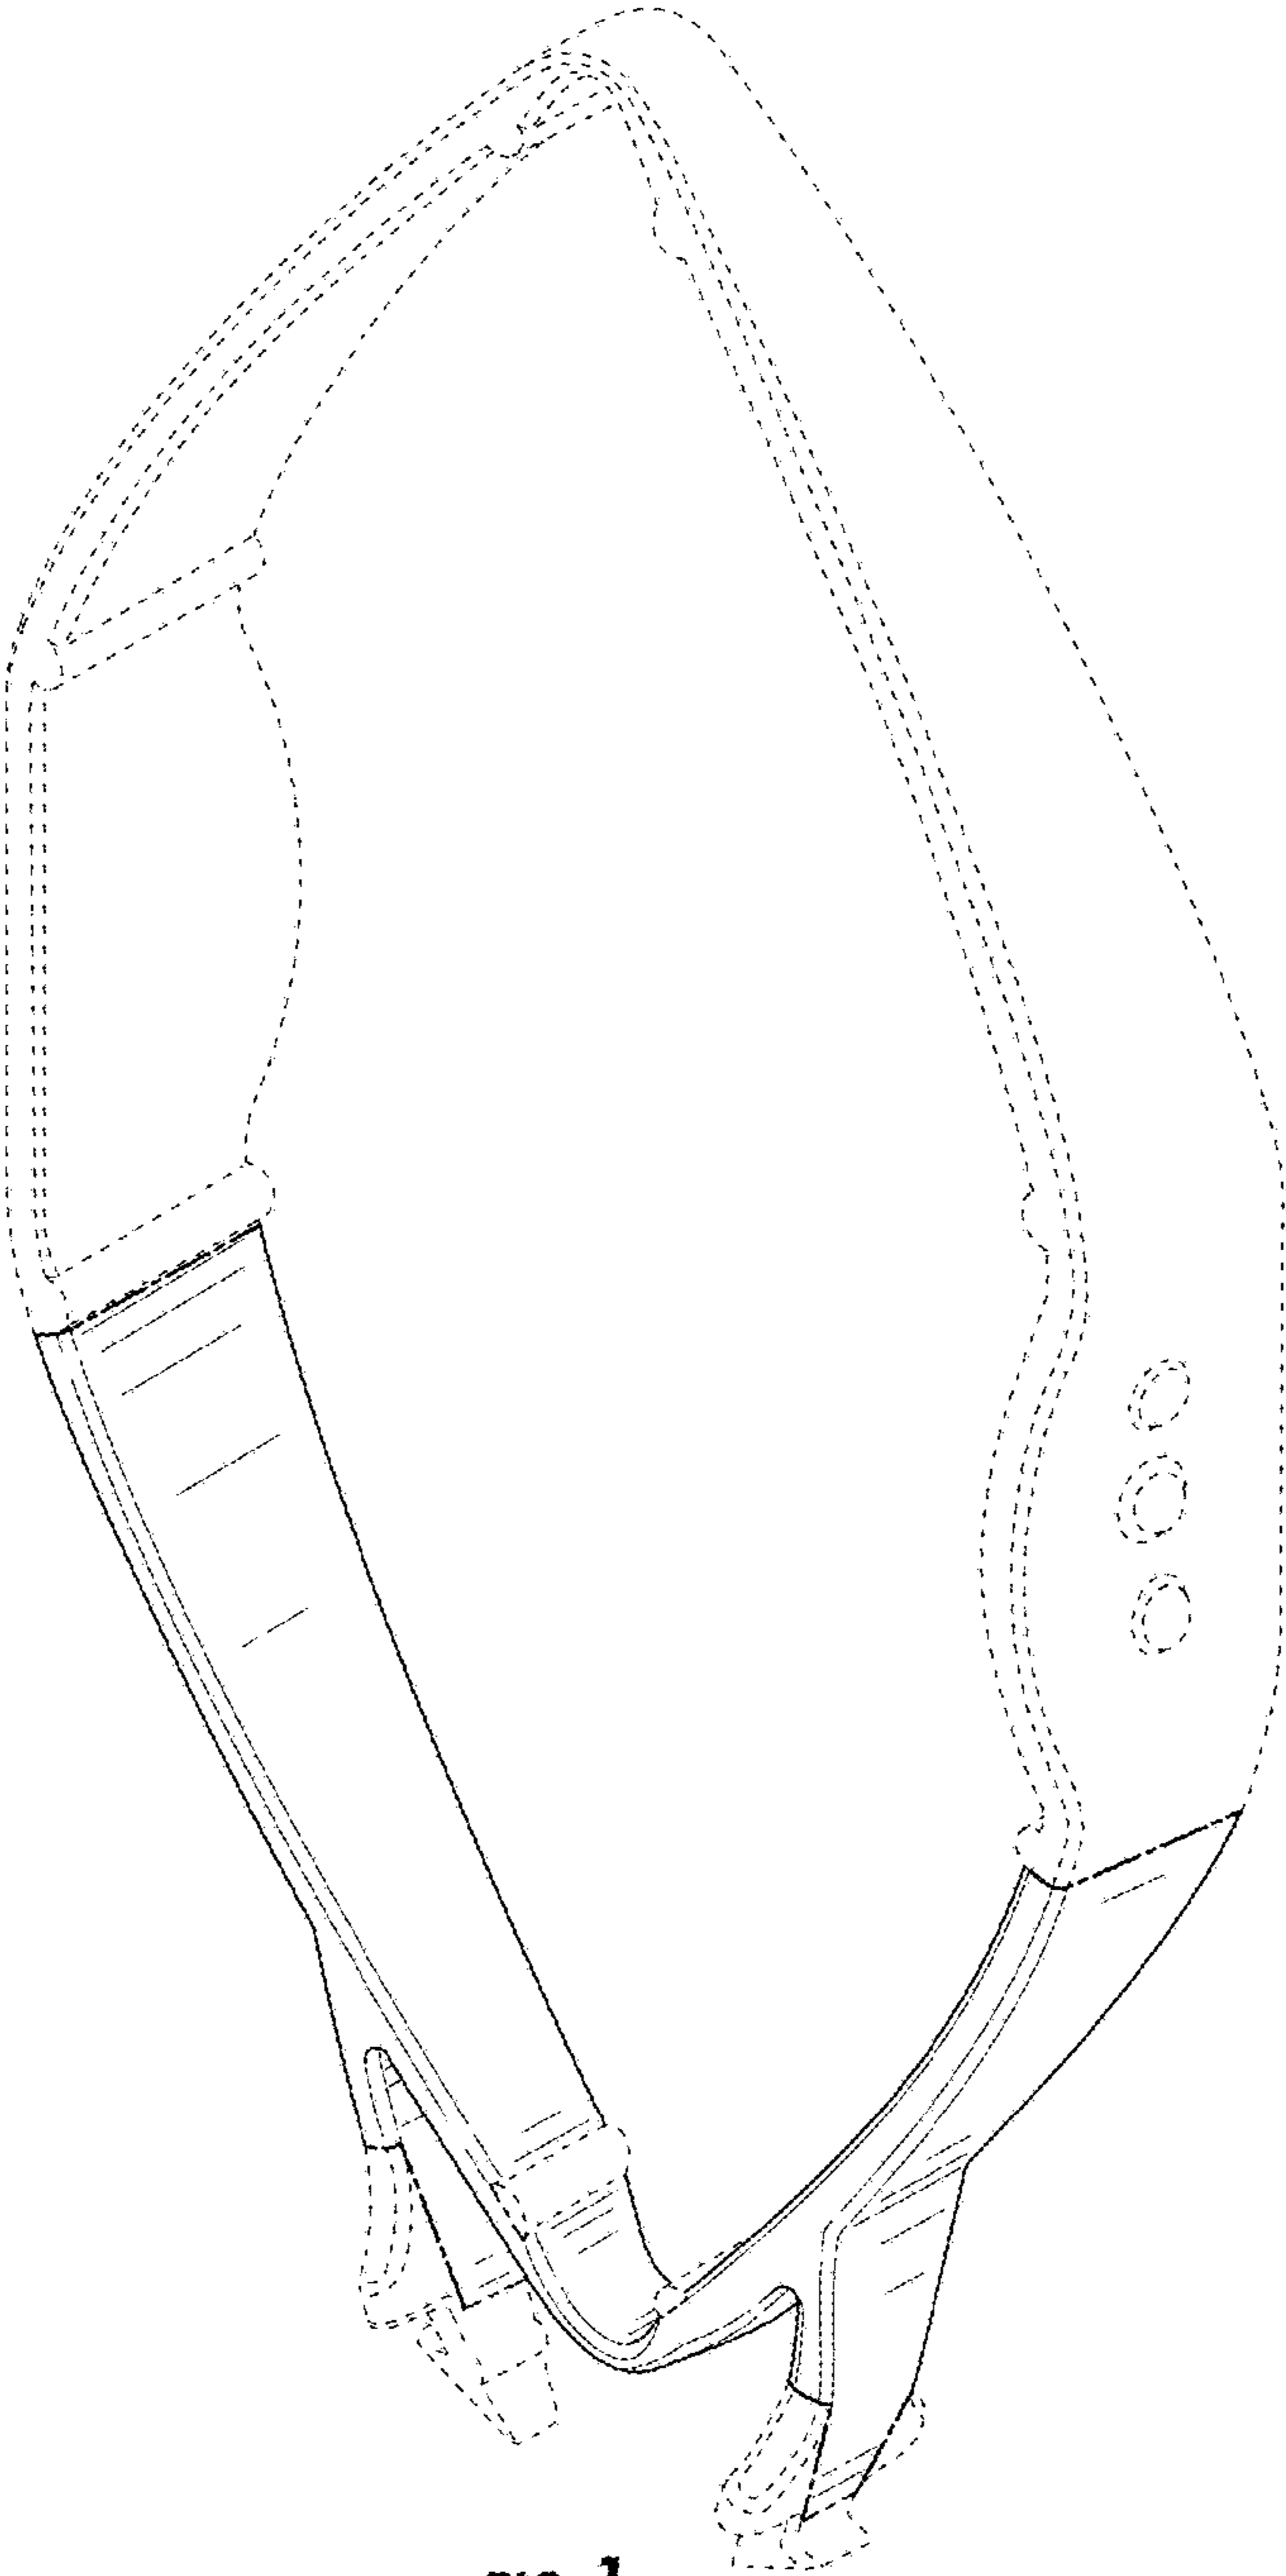


FIG. 1

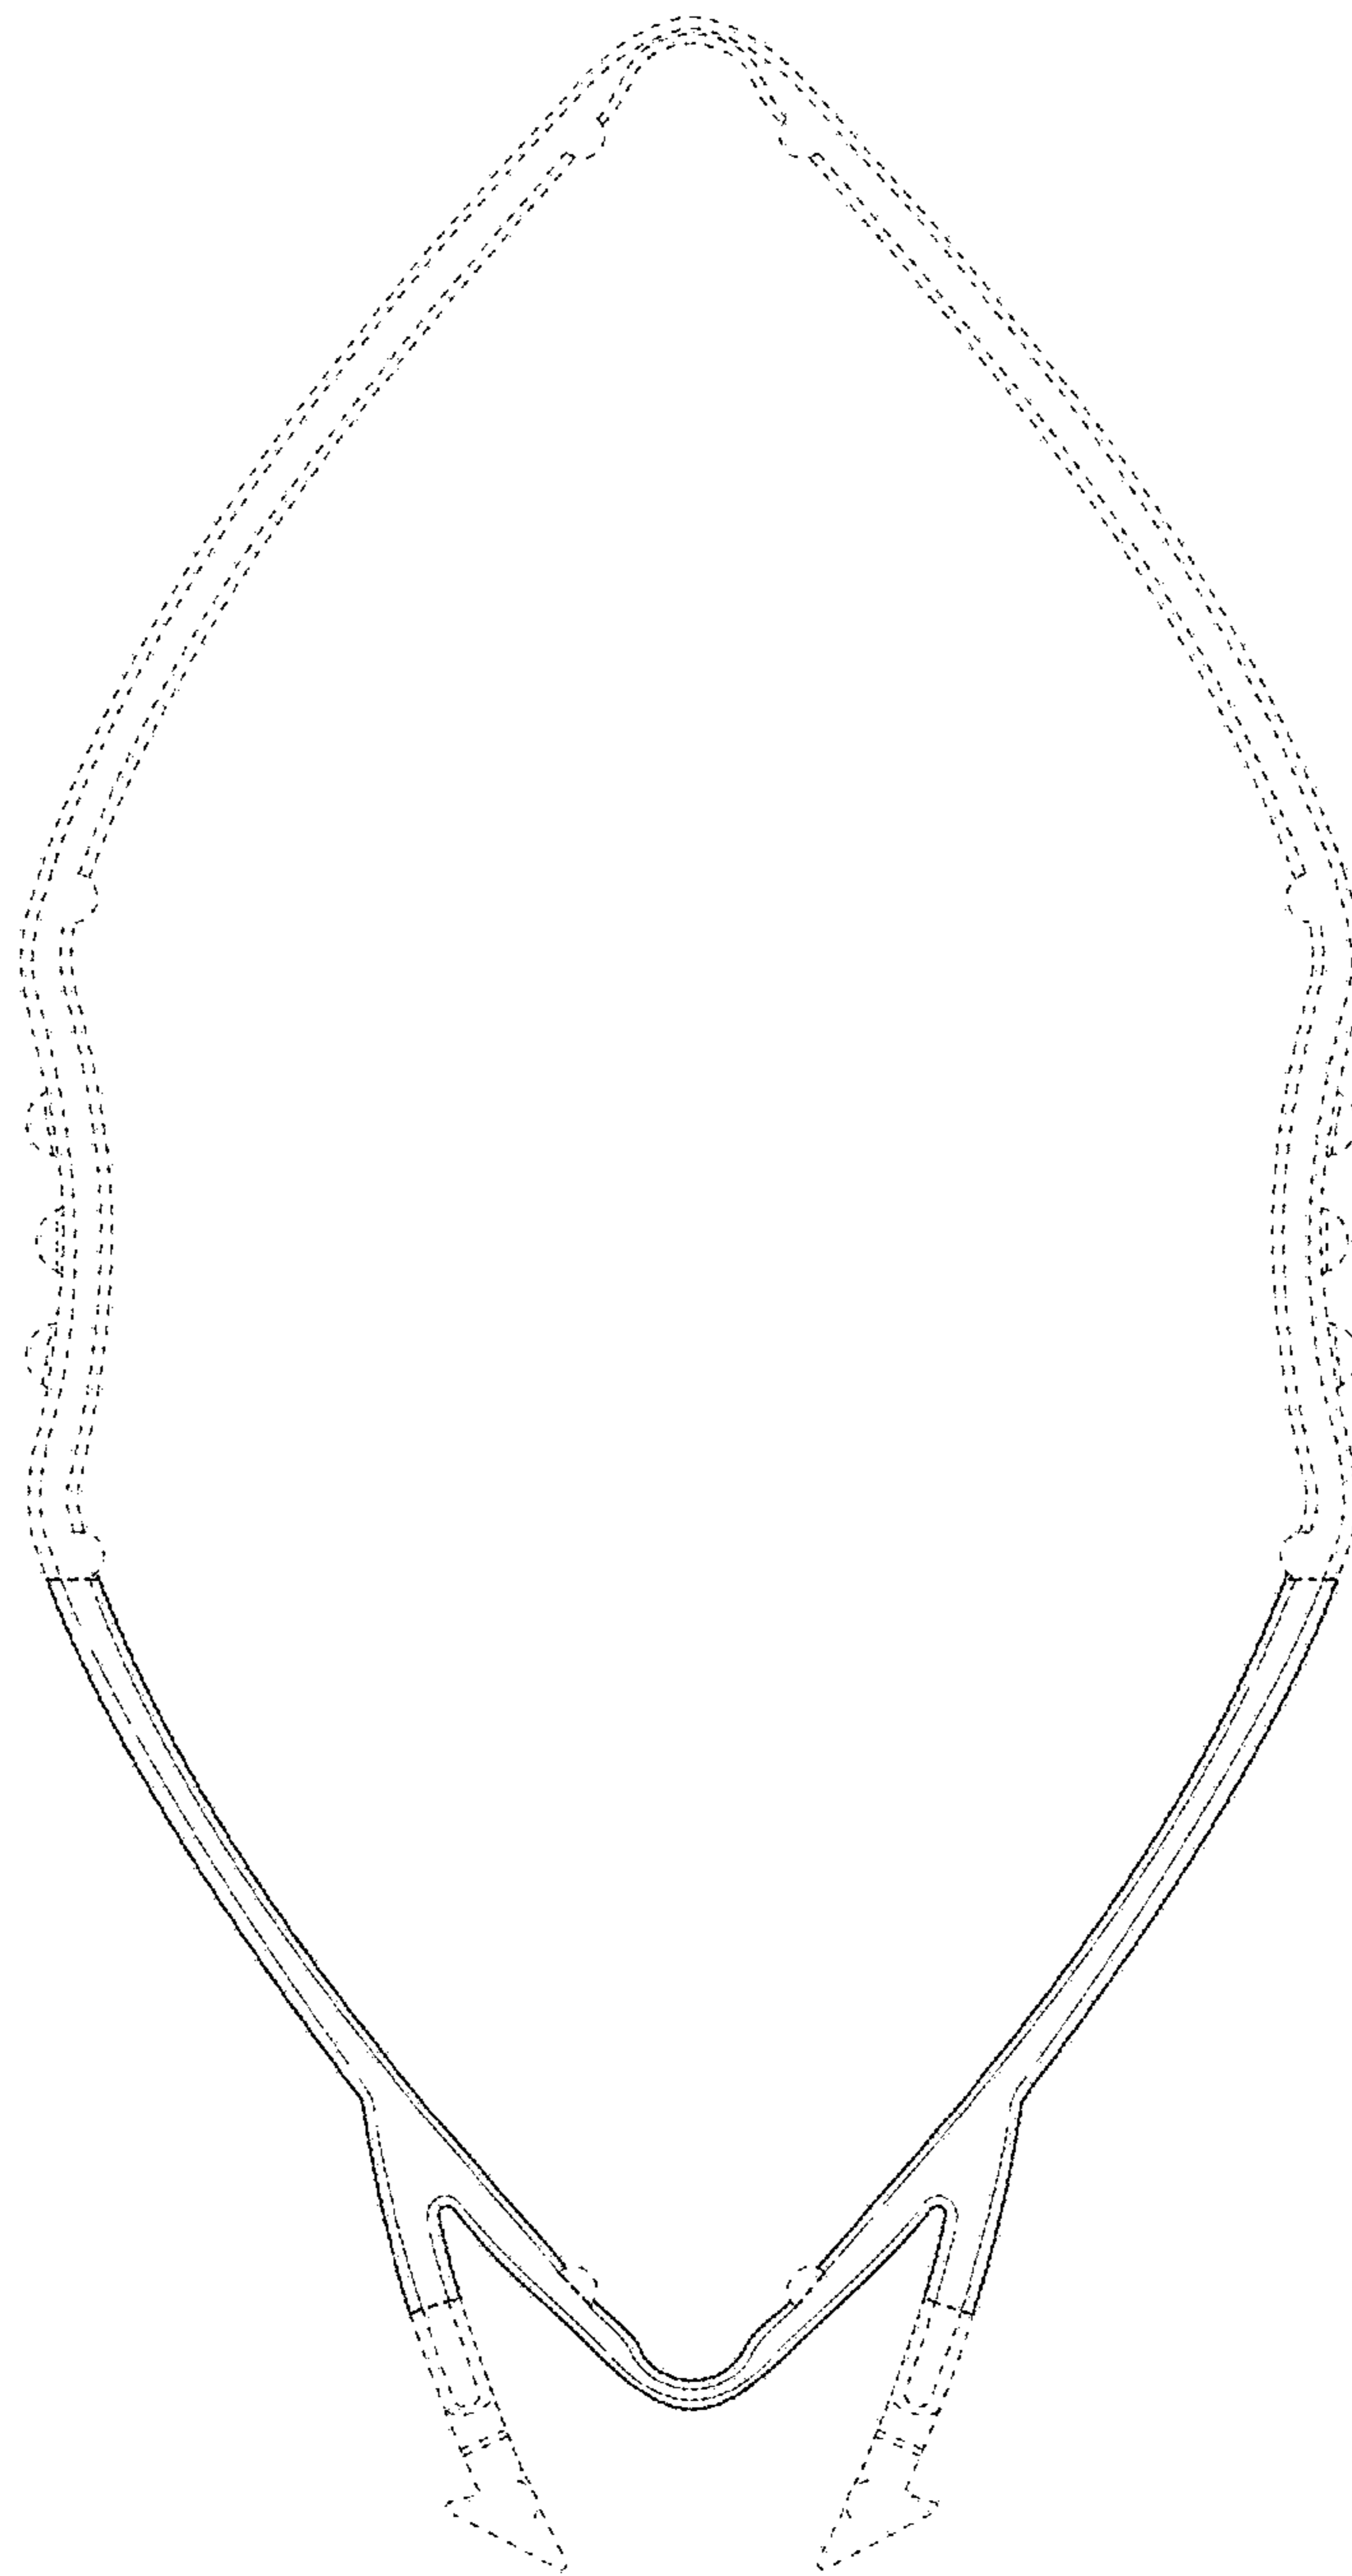


FIG. 2

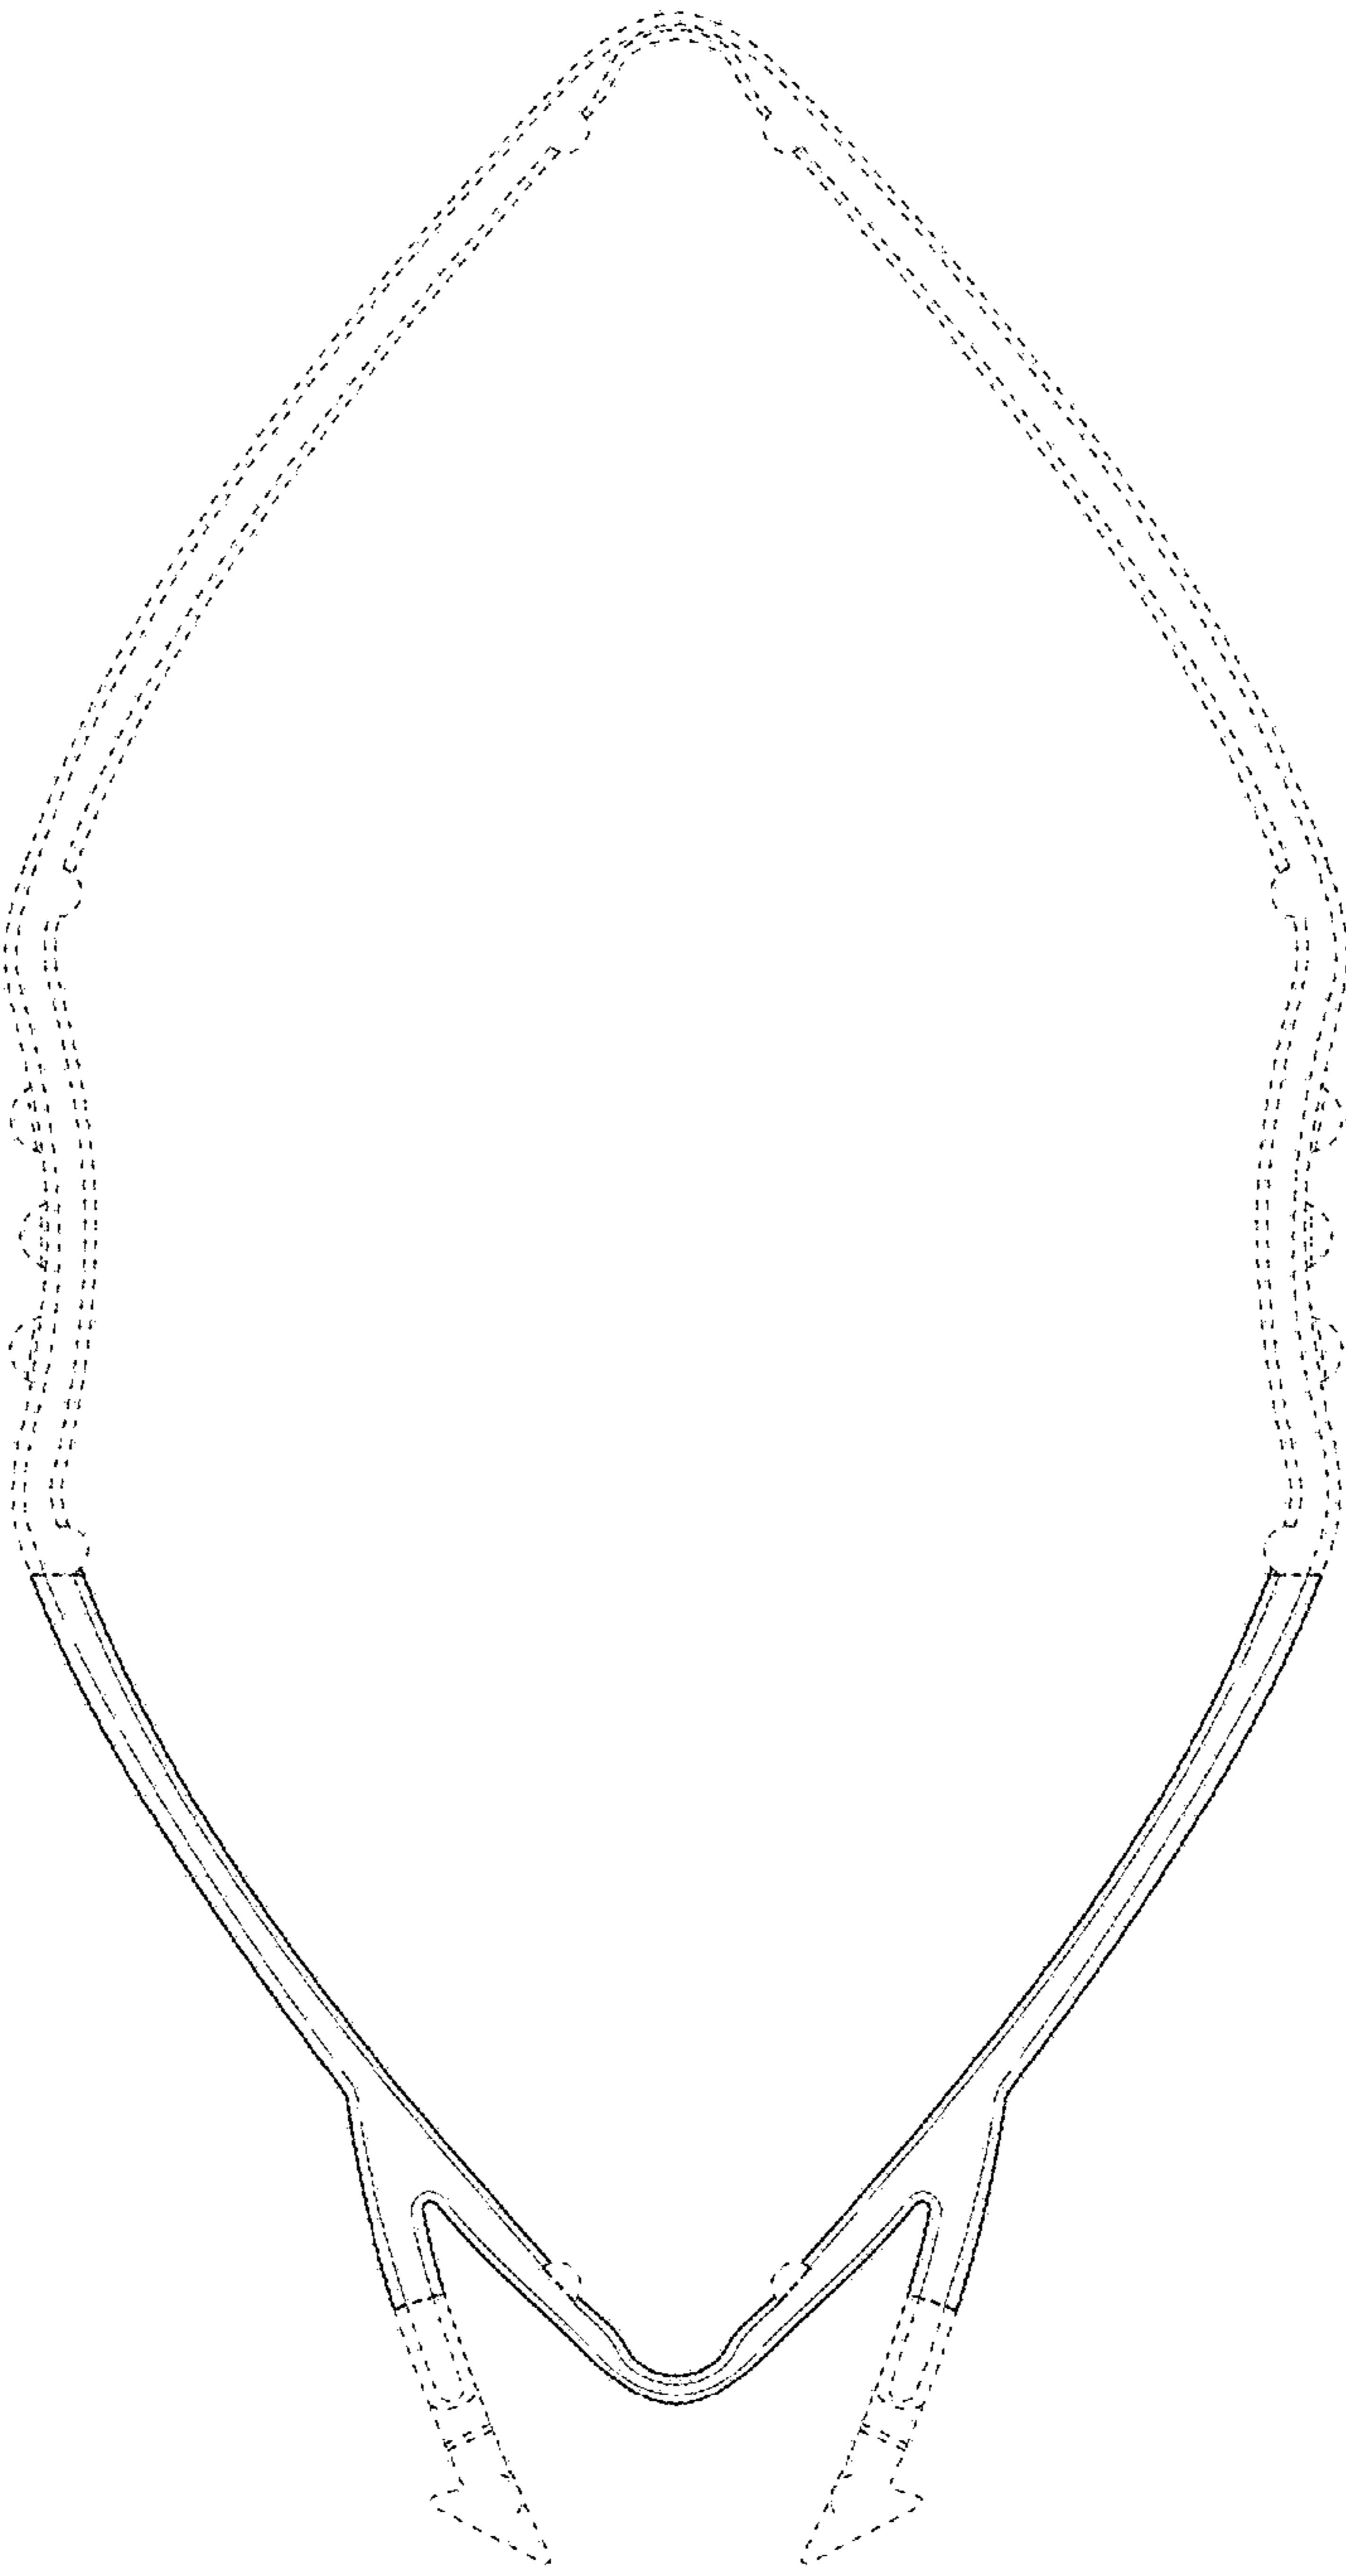


FIG. 3

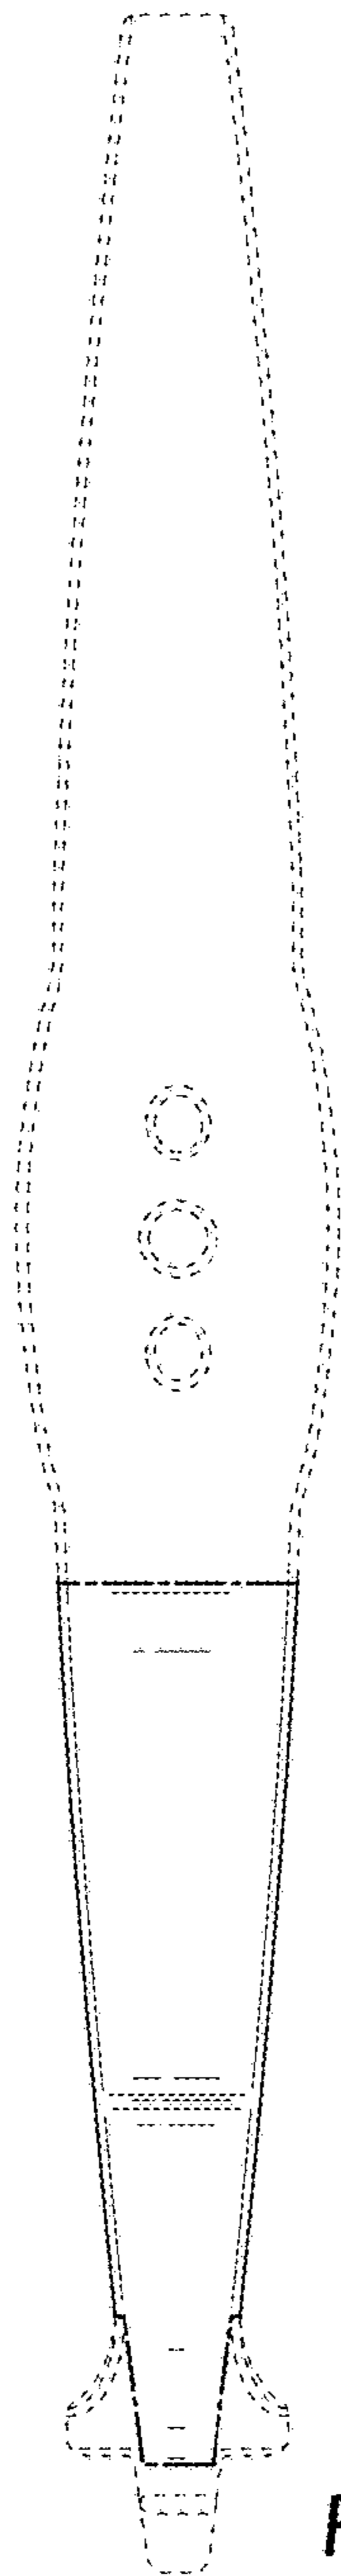


FIG. 4

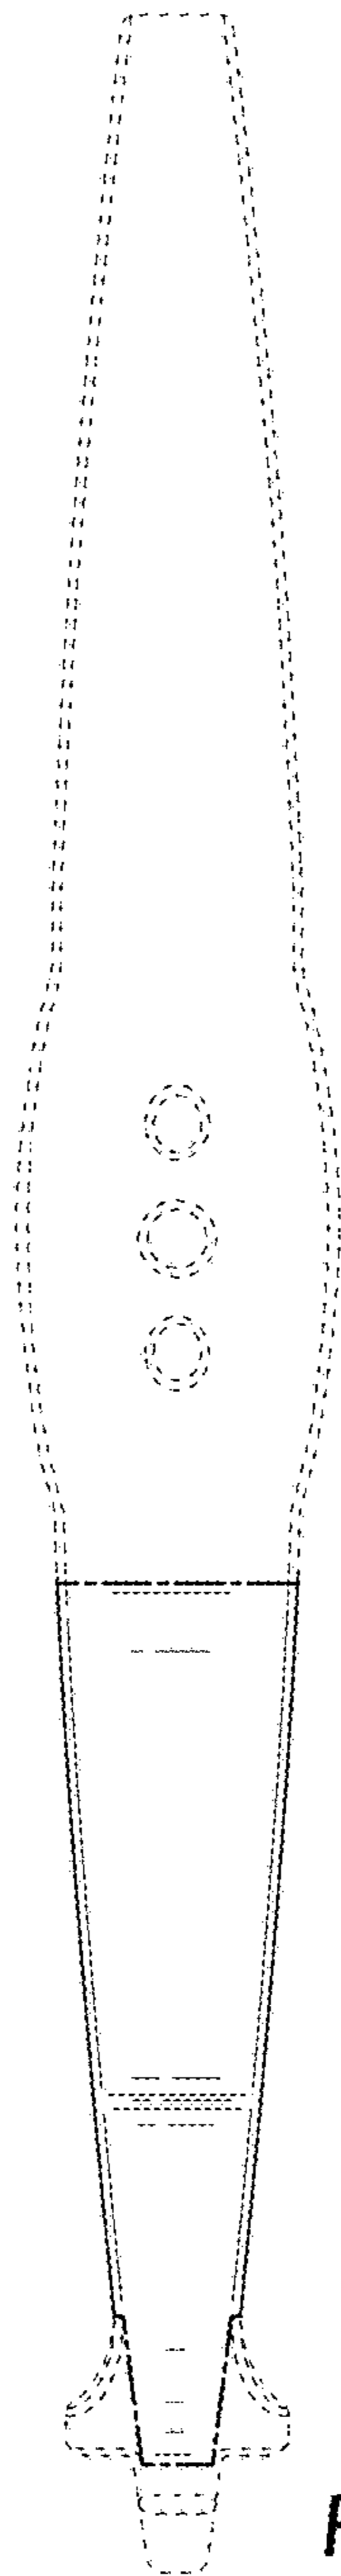


FIG. 5

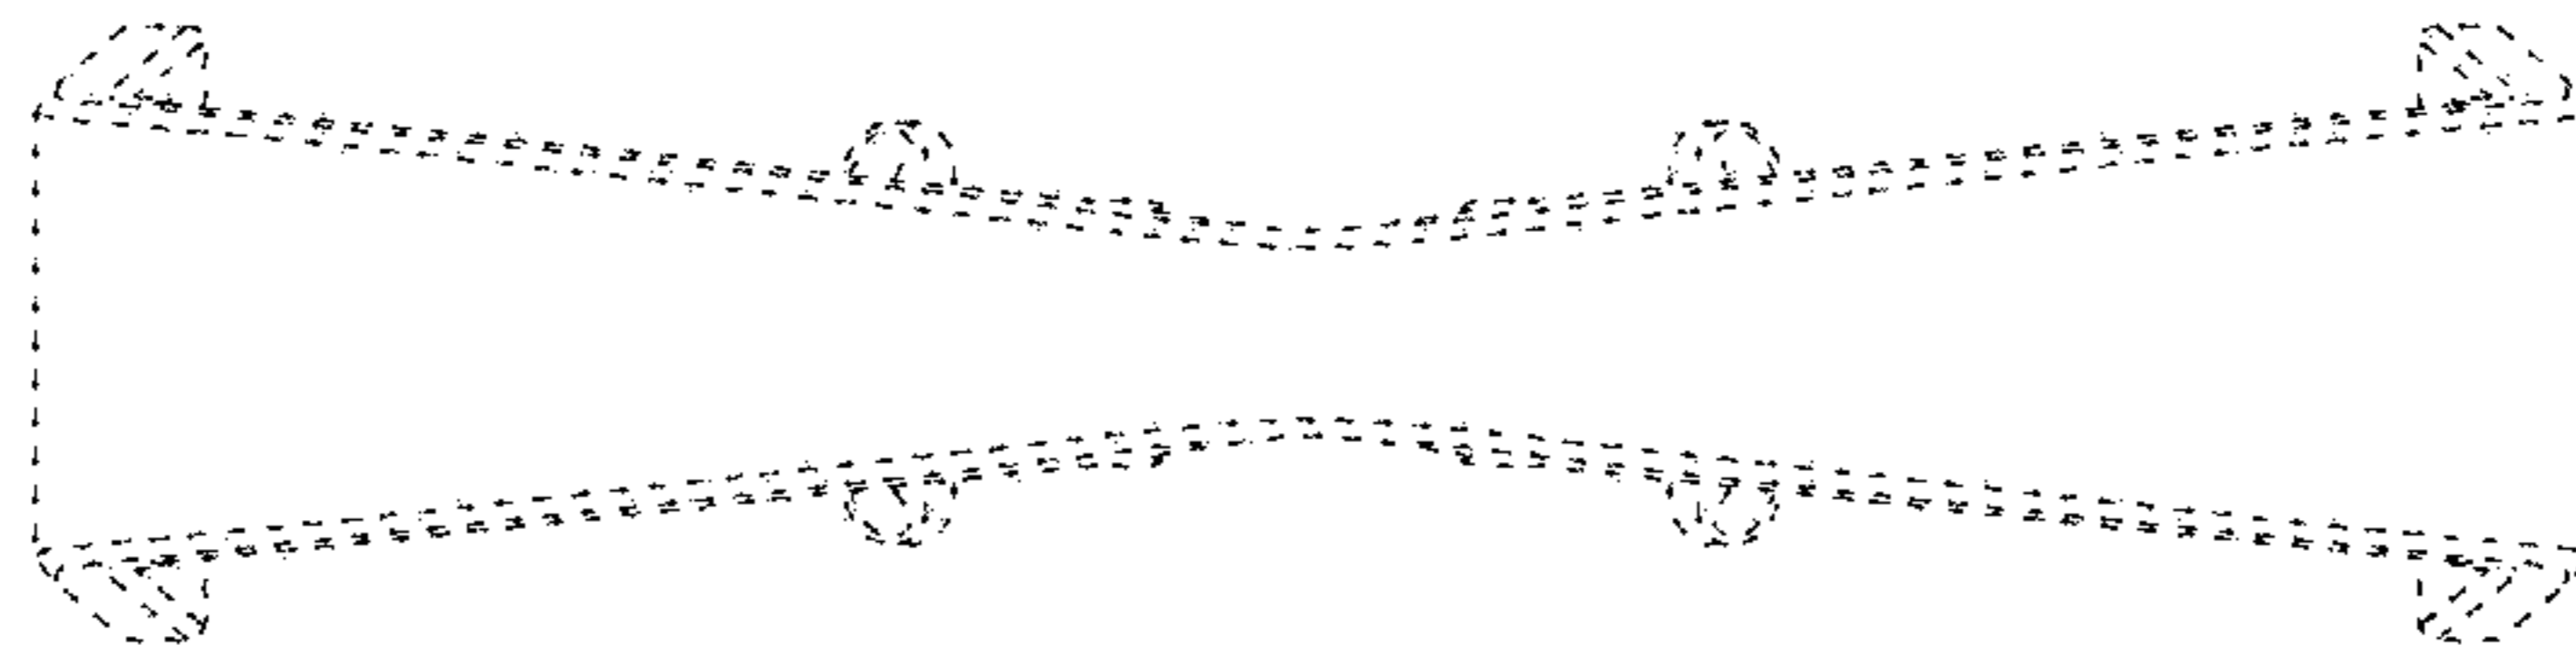


FIG. 6

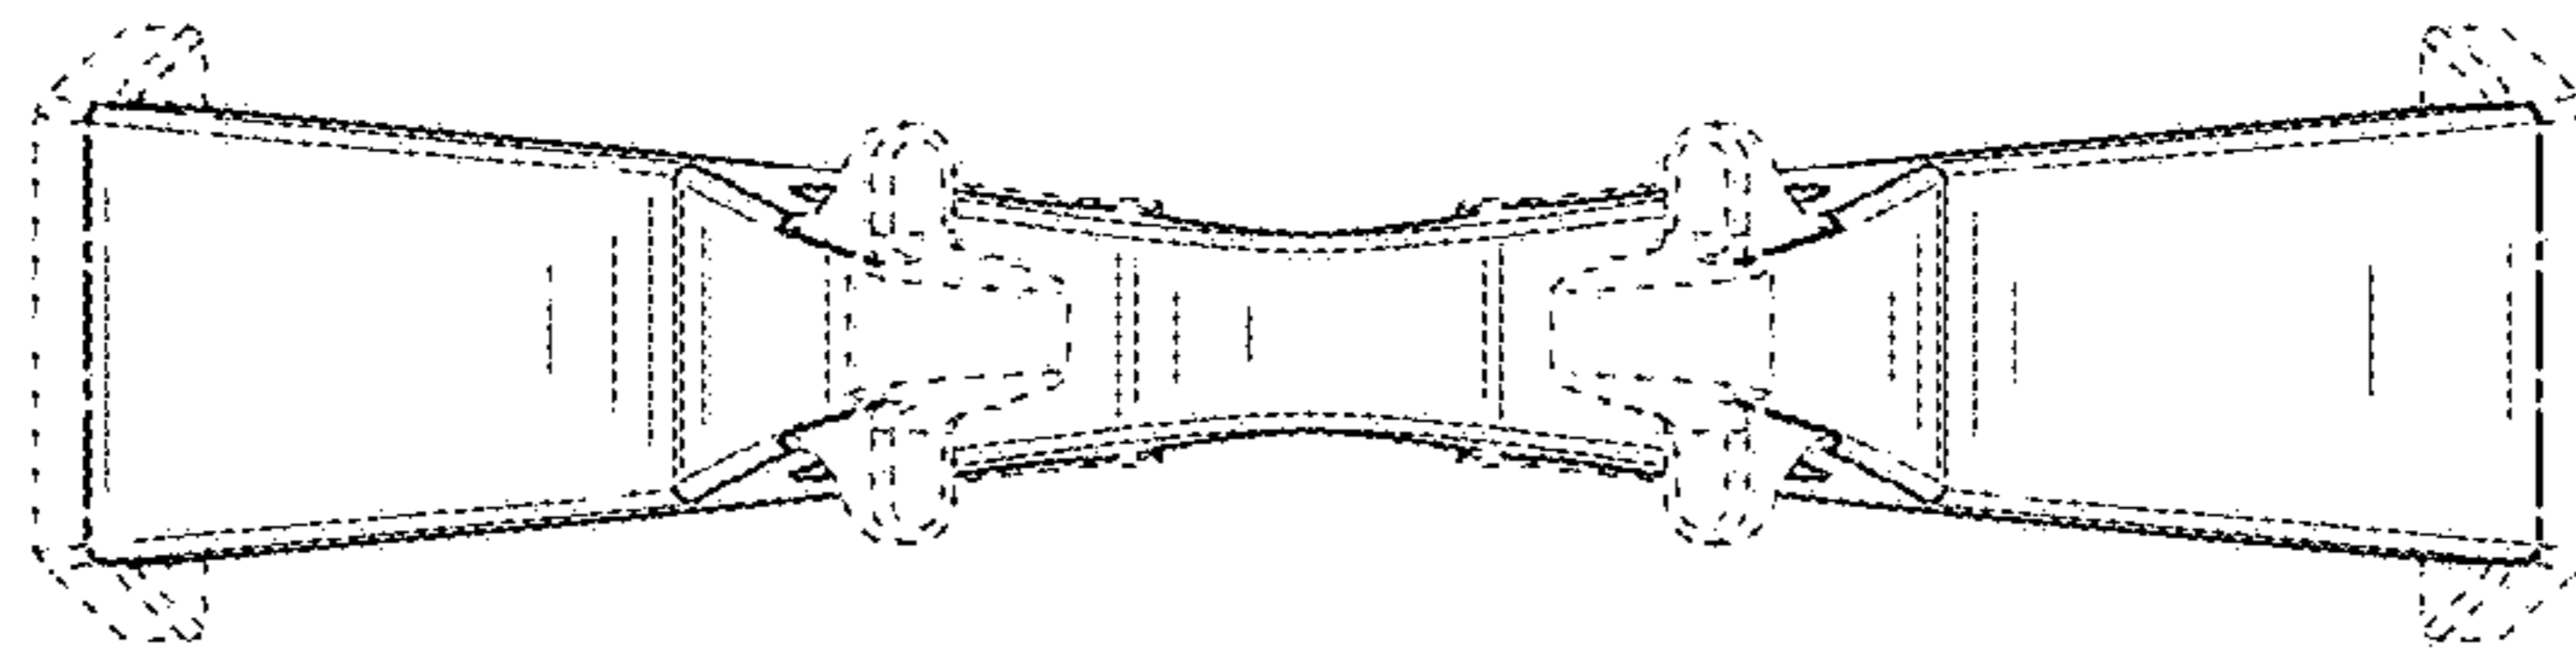


FIG. 7