



US00D862715S

(12) **United States Design Patent**
Wang

(10) **Patent No.:** **US D862,715 S**
(45) **Date of Patent:** **** Oct. 8, 2019**

- (54) **HEALTH-REGAIN DEVICE**
- (71) Applicant: **Jiangsu Alphay Medical Device Co., Ltd.**, Nantong, Jiangsu (CN)
- (72) Inventor: **Jiang Wang**, Nantong (CN)
- (73) Assignee: **Jiangsu Alphay Medical Device Co., Ltd.**, Nantong, Jiangsu (CN)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/606,661**
- (22) Filed: **Jun. 6, 2017**
- (51) **LOC (12) Cl.** **24-01**
- (52) **U.S. Cl.**
USPC **D24/200; D24/206; D24/215**
- (58) **Field of Classification Search**
USPC D24/189–192, 200, 206, 215, 231, 188;
D6/601
CPC A61F 5/028; A61F 5/055; A61F 5/3738;
A61F 13/108; A61F 13/062; A61H
15/0085; A61H 2007/009; A61H
2201/0134; A61H 7/007; A61N 1/0492;
A61N 1/36014; A61N 1/36021; A61N
1/32; A61N 1/3625; A61N 1/36146;
A61N 1/3606; A61N 1/36071; A61N
1/36017; A61N 1/39625; A61N 1/0502
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D504,954 S *	5/2005	Park	D24/200
D545,443 S *	6/2007	Ng	D24/200
D605,305 S *	12/2009	Carter	D24/231
D628,705 S *	12/2010	Usui	D24/206
D790,073 S *	6/2017	Mason	D24/215
D793,768 S *	8/2017	Goddard	D6/601
D793,770 S *	8/2017	Krishtul	D6/601
D808,901 S *	1/2018	Kelly	D13/107
D820,465 S *	6/2018	Chen	D24/215
D821,593 S *	6/2018	Perez	D24/200

D825,356 S *	8/2018	Yu	D10/70
2017/0348175 A1 *	12/2017	Emmel	A61H 7/001
2018/0184939 A1 *	7/2018	Christiansen	A61B 5/6833

FOREIGN PATENT DOCUMENTS

CN 304850089 * 10/2018

OTHER PUBLICATIONS

Hangsun Electric Lumbar Traction Device . . . posted at amazon.com, no posting date available, online, URL:https://www.amazon.com/Hangsun-Electric-Traction-Stretcher-Vibration/dp/B07C1G5PJS (Year: 2018).*

* cited by examiner

Primary Examiner — Barbara Fox

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Raymond Y. Chan;
David and Raymond Patent Firm



(57) **CLAIM**

The ornamental design for a health-regain device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a health-regain device showing my new design;
FIG. 2 is another perspective view thereof;
FIG. 3 is front view thereof;
FIG. 4 is a rear view thereof;
FIG. 5 is a left view thereof;
FIG. 6 is a right view thereof;
FIG. 7 is a top view thereof;
FIG. 8 is a bottom view thereof; and,
FIG. 9 is a front view showing the health-regain device which is inflated.
The broken lines show portions of the health-regain device that form no part of the claimed design.

1 Claim, 9 Drawing Sheets

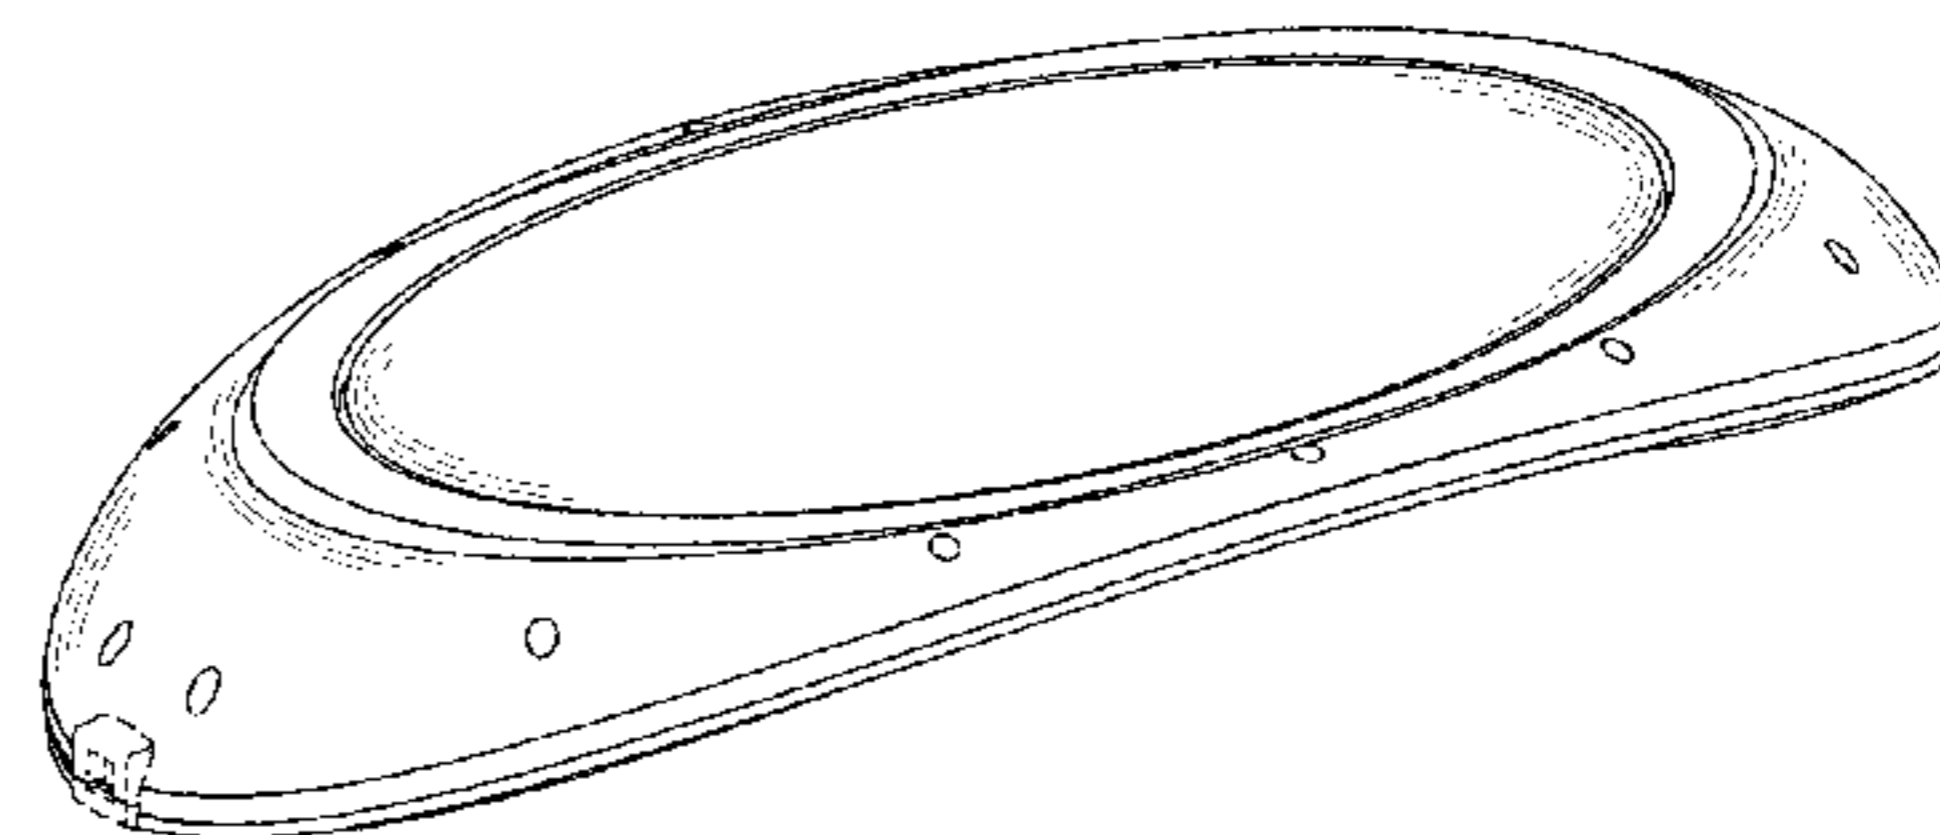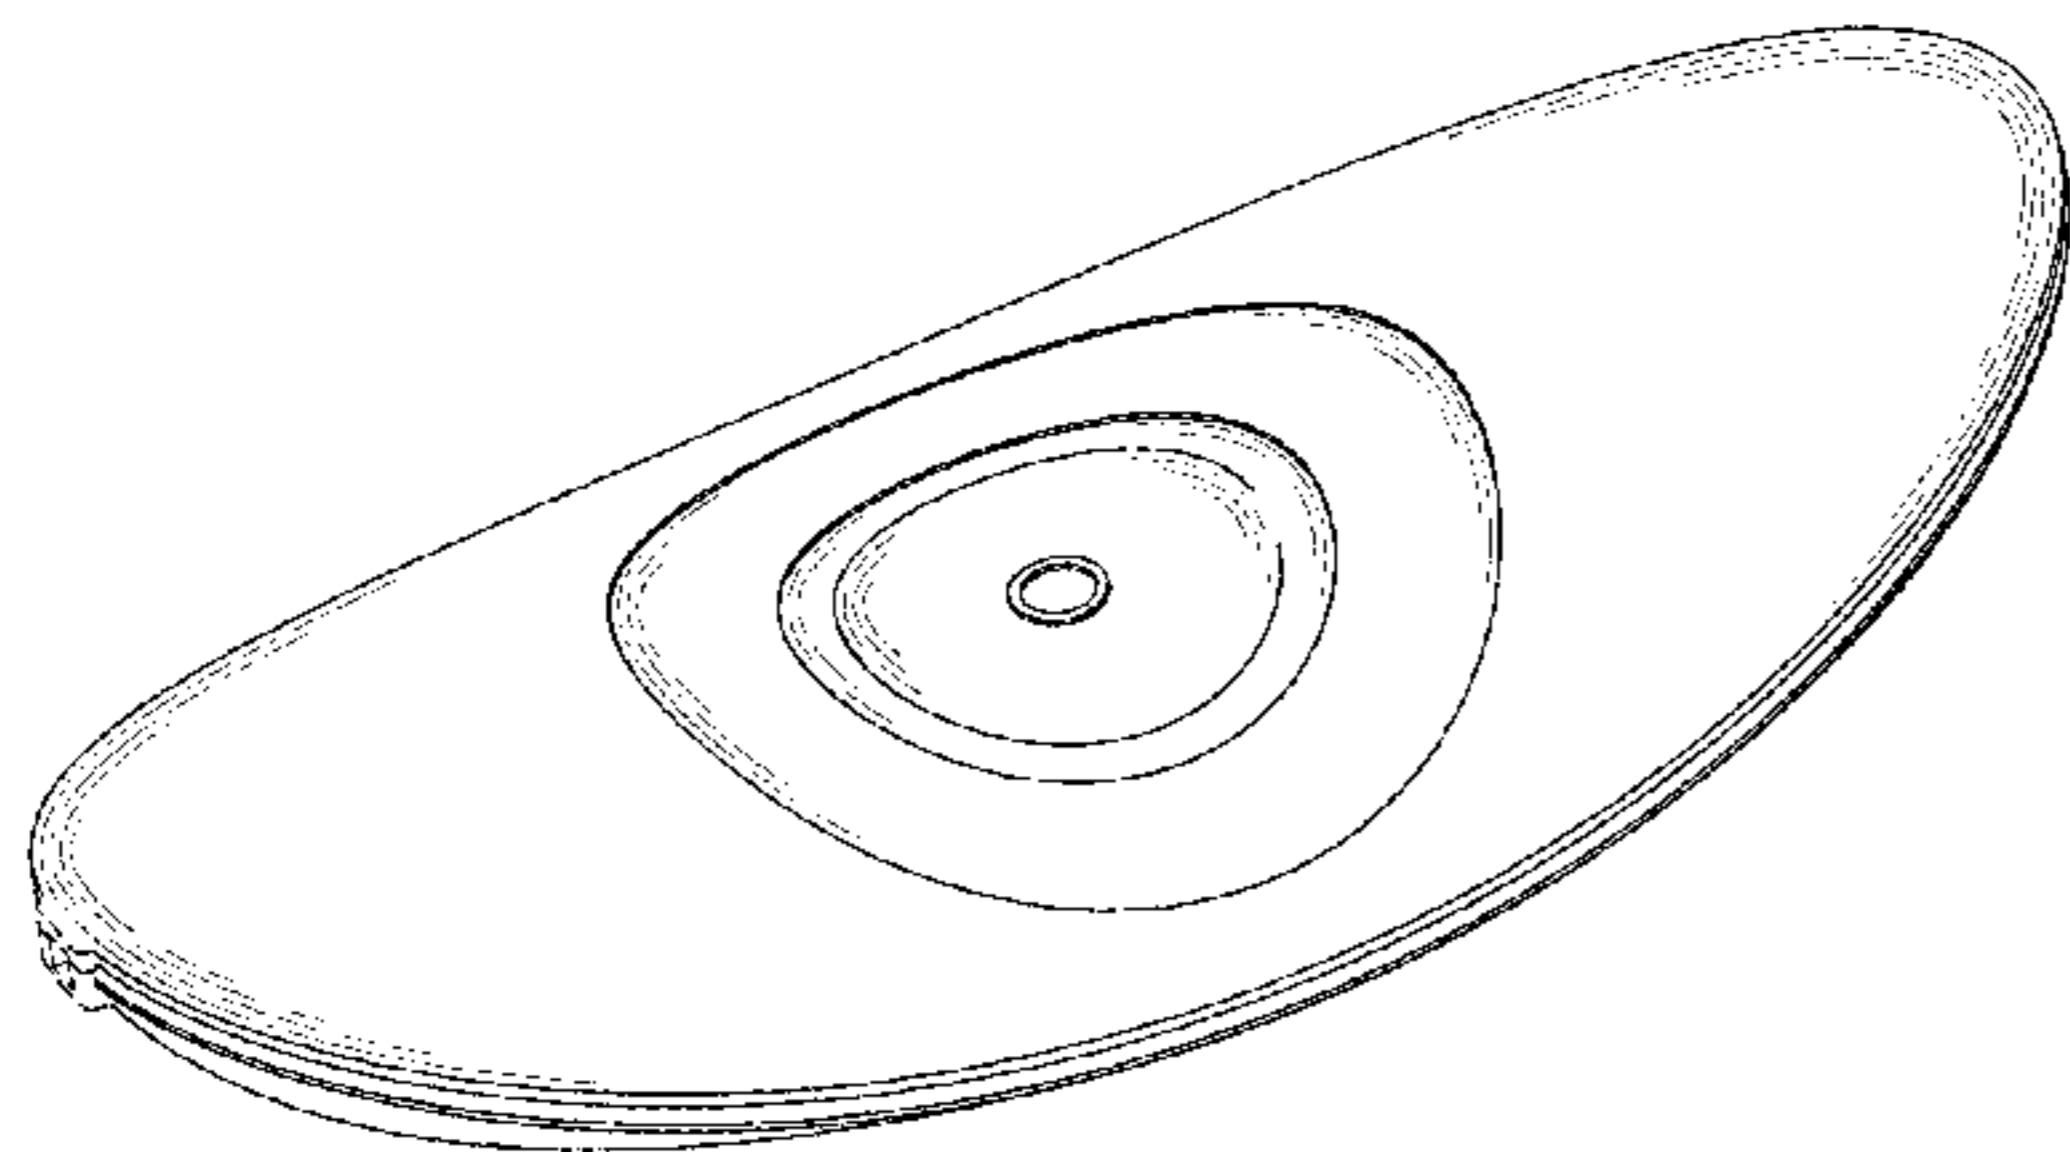

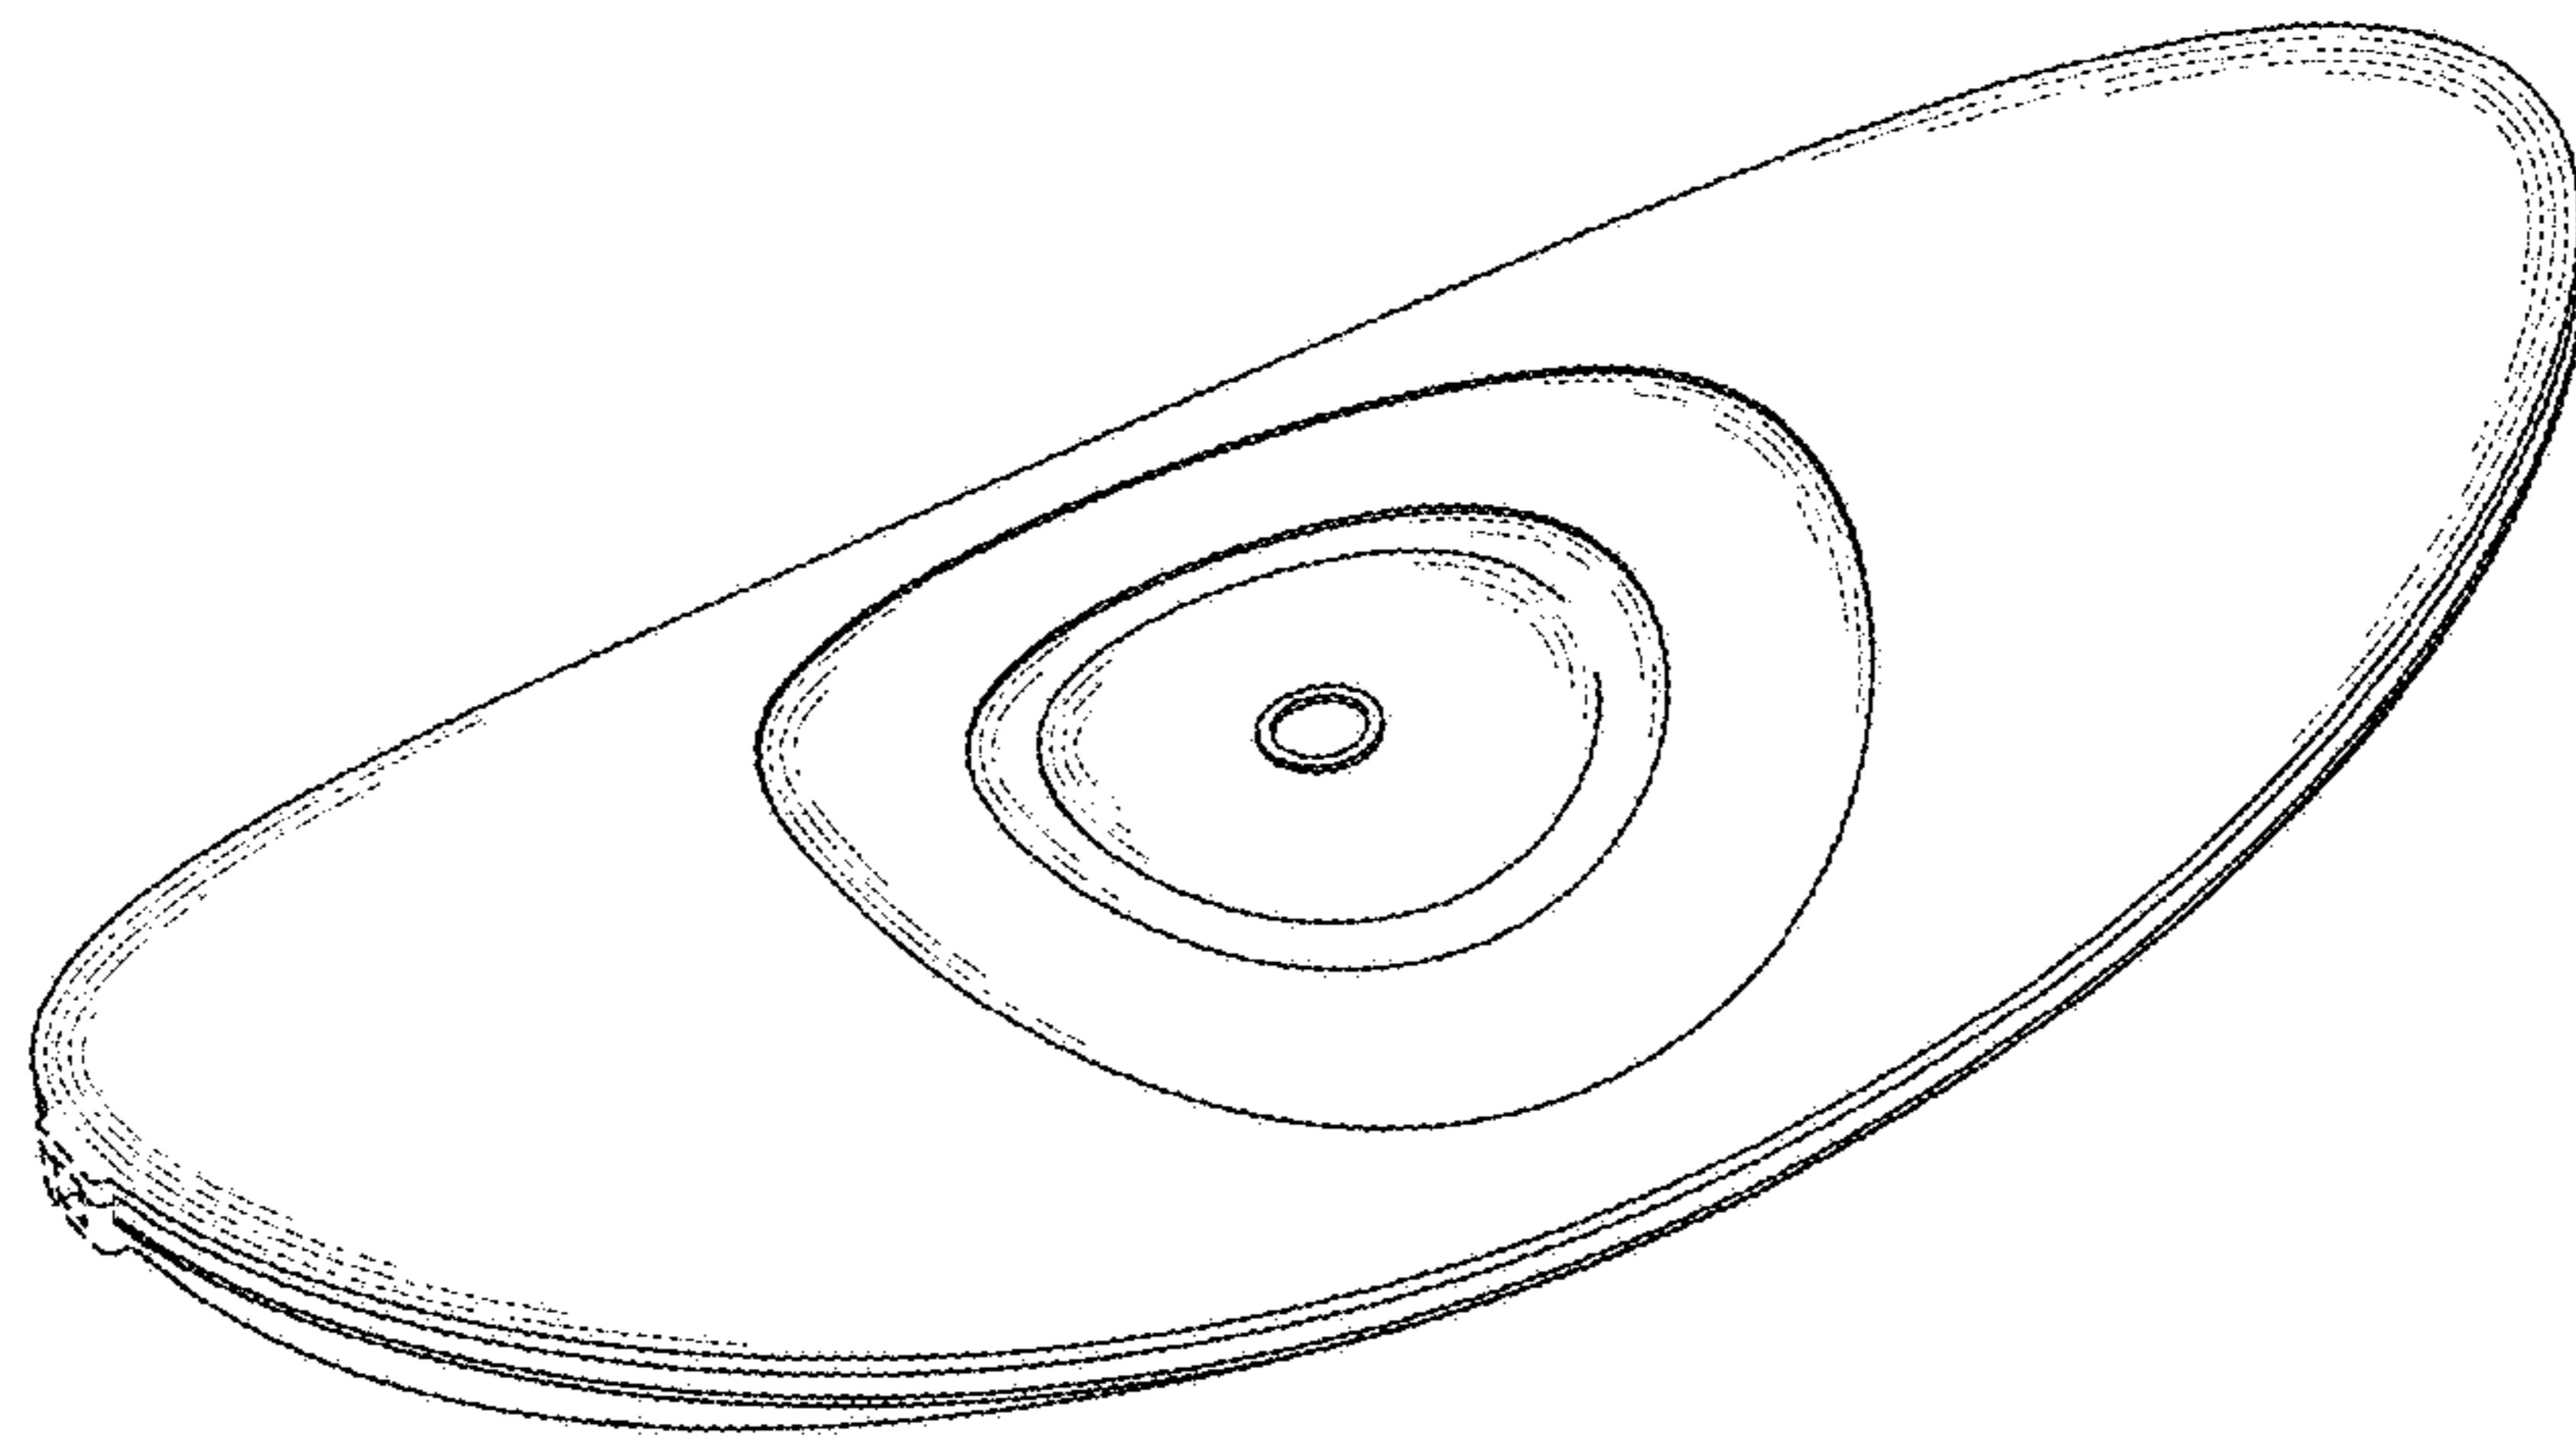


FIG.1

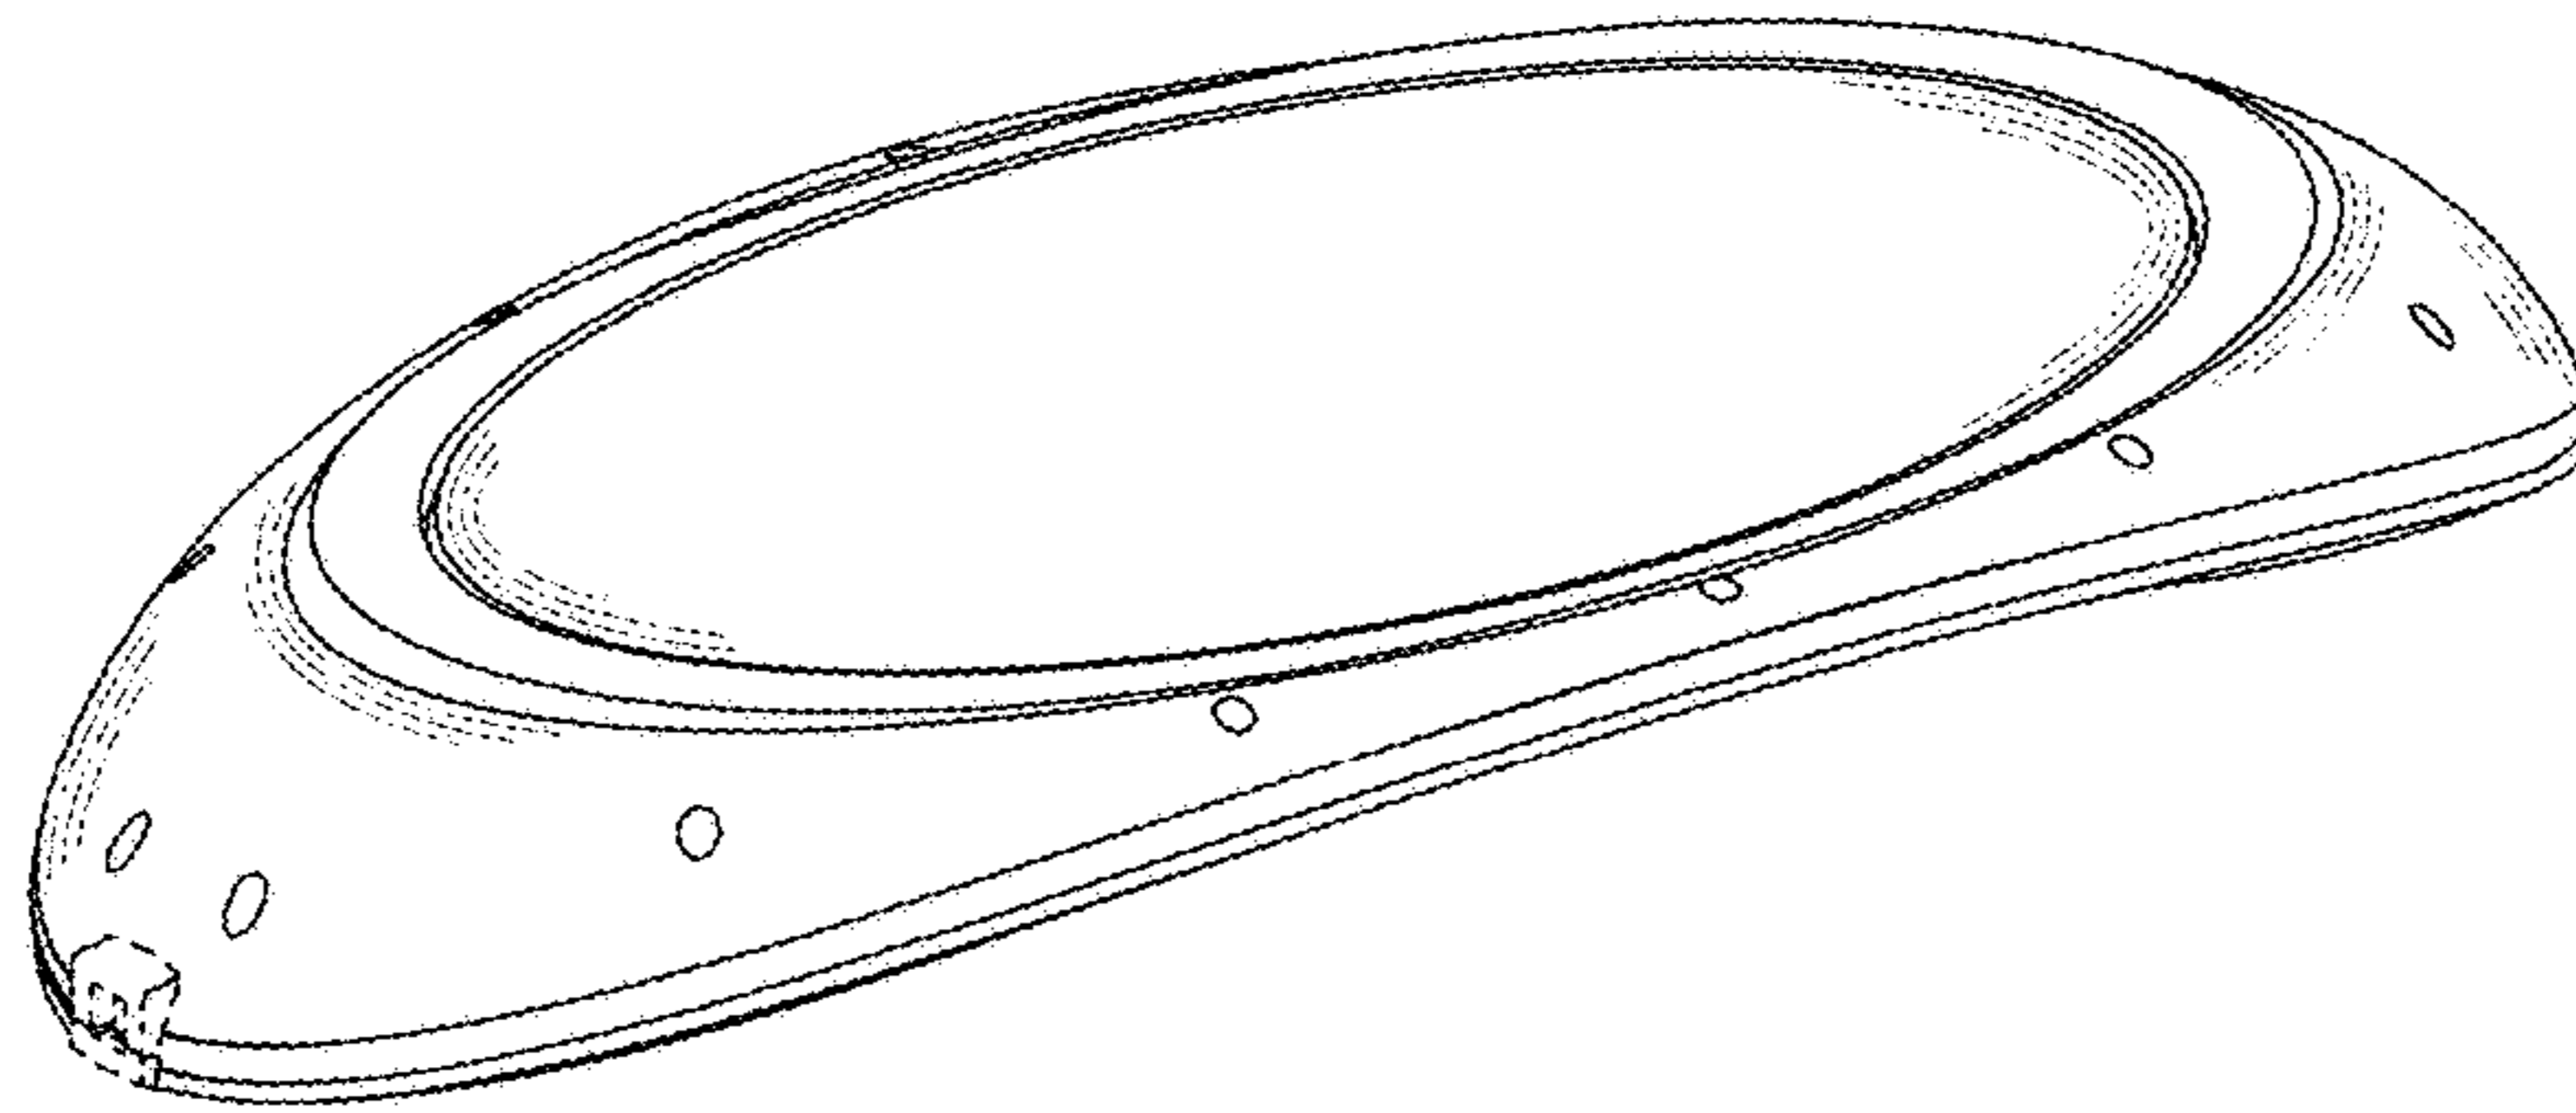


FIG.2



FIG.3

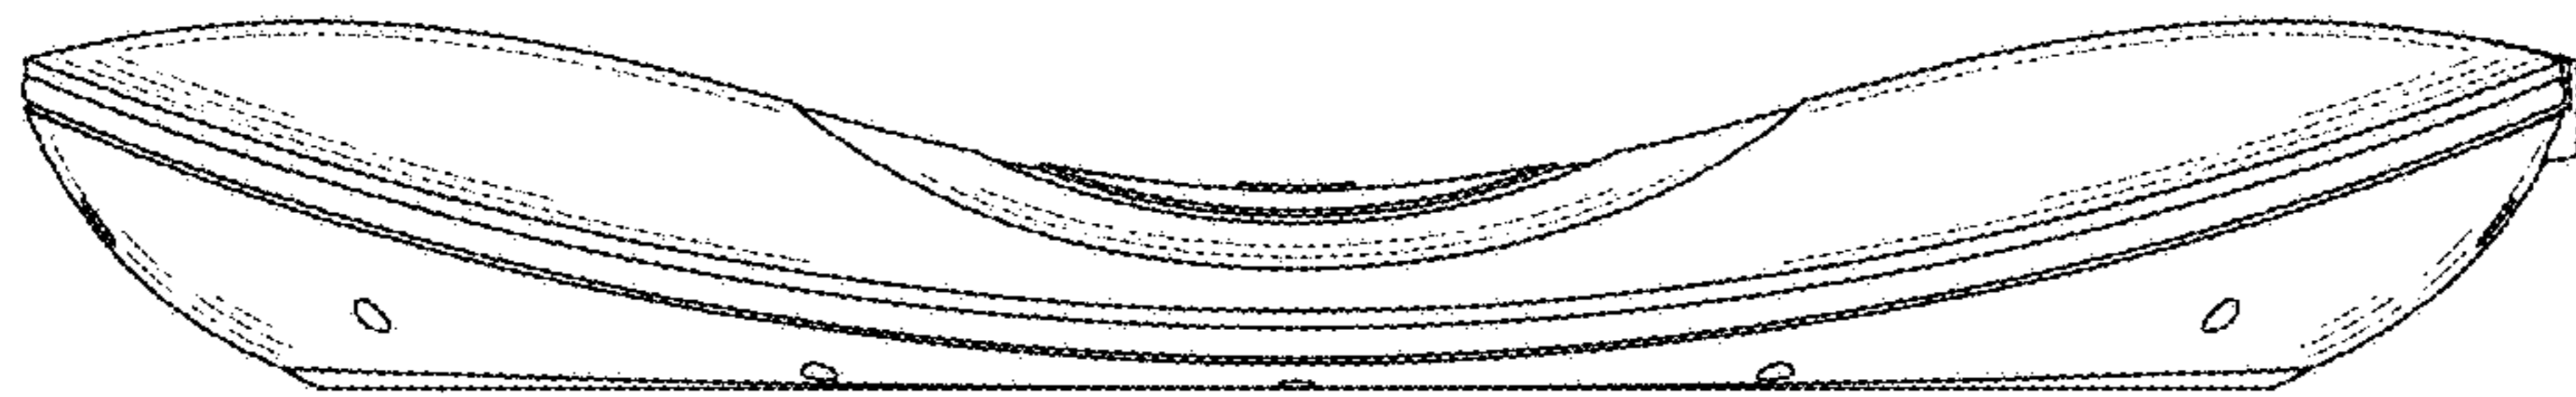


FIG.4

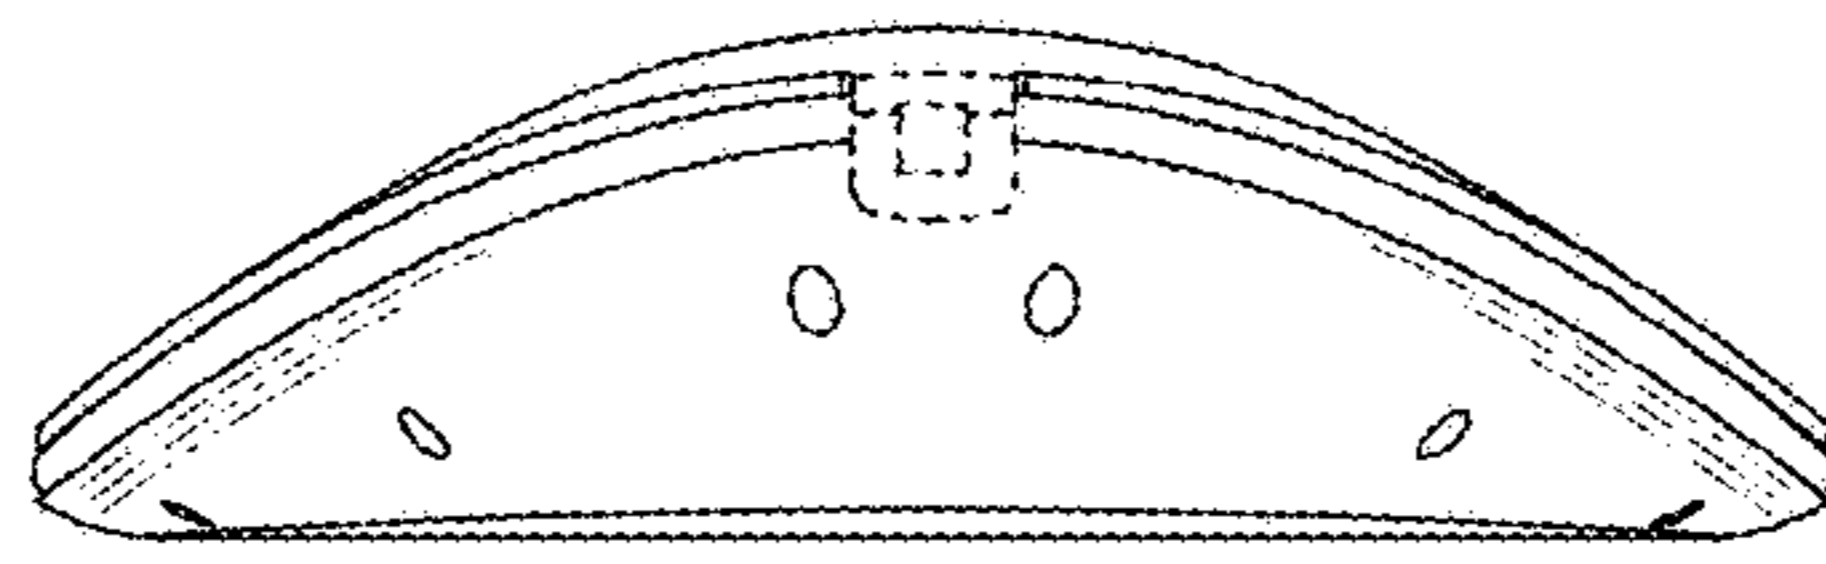


FIG.5

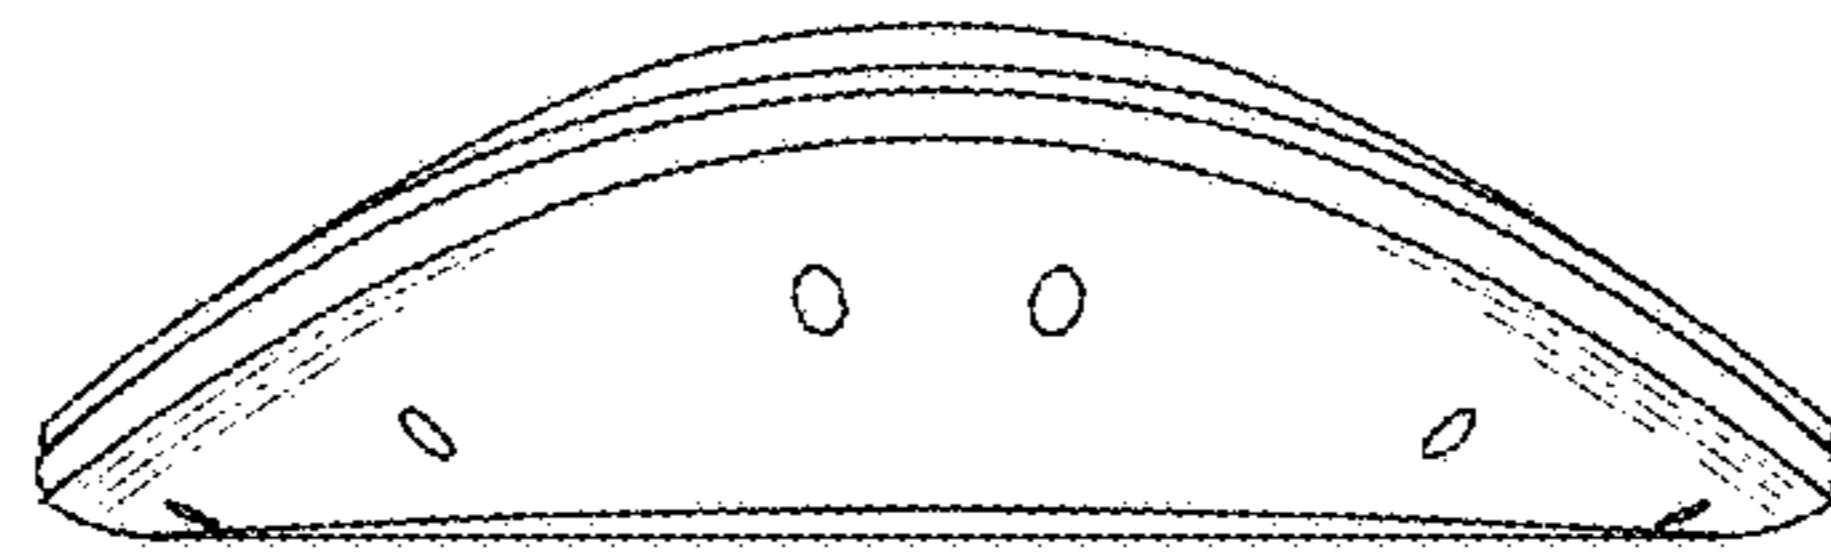


FIG.6

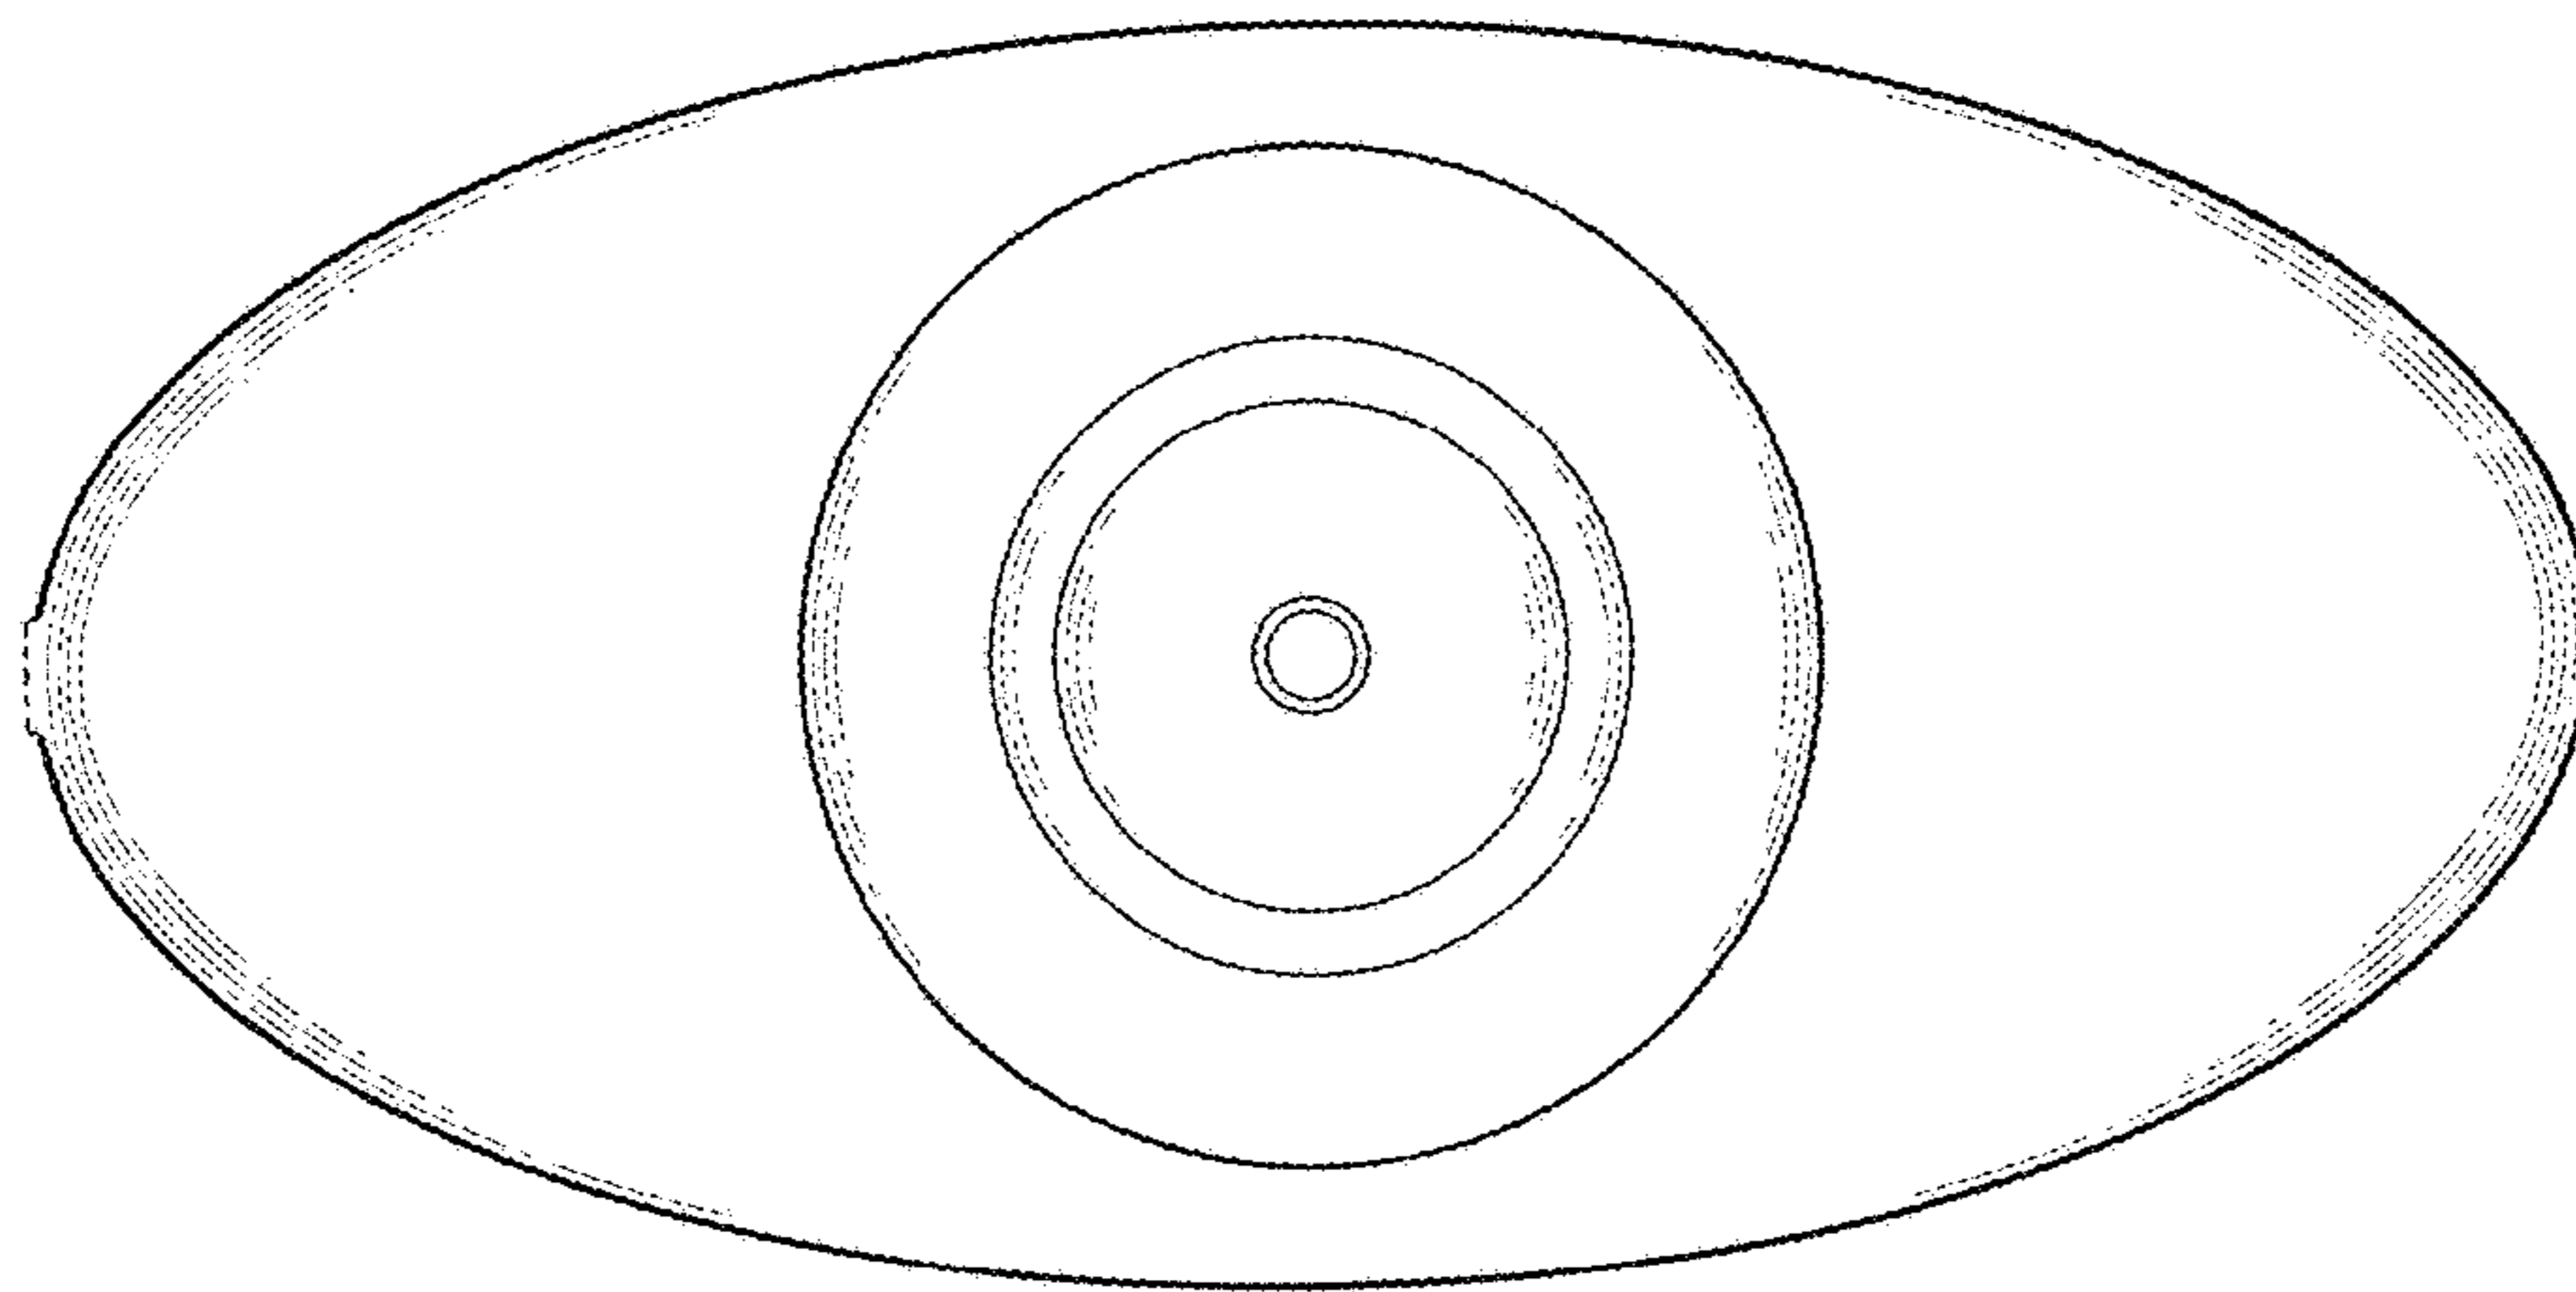


FIG.7

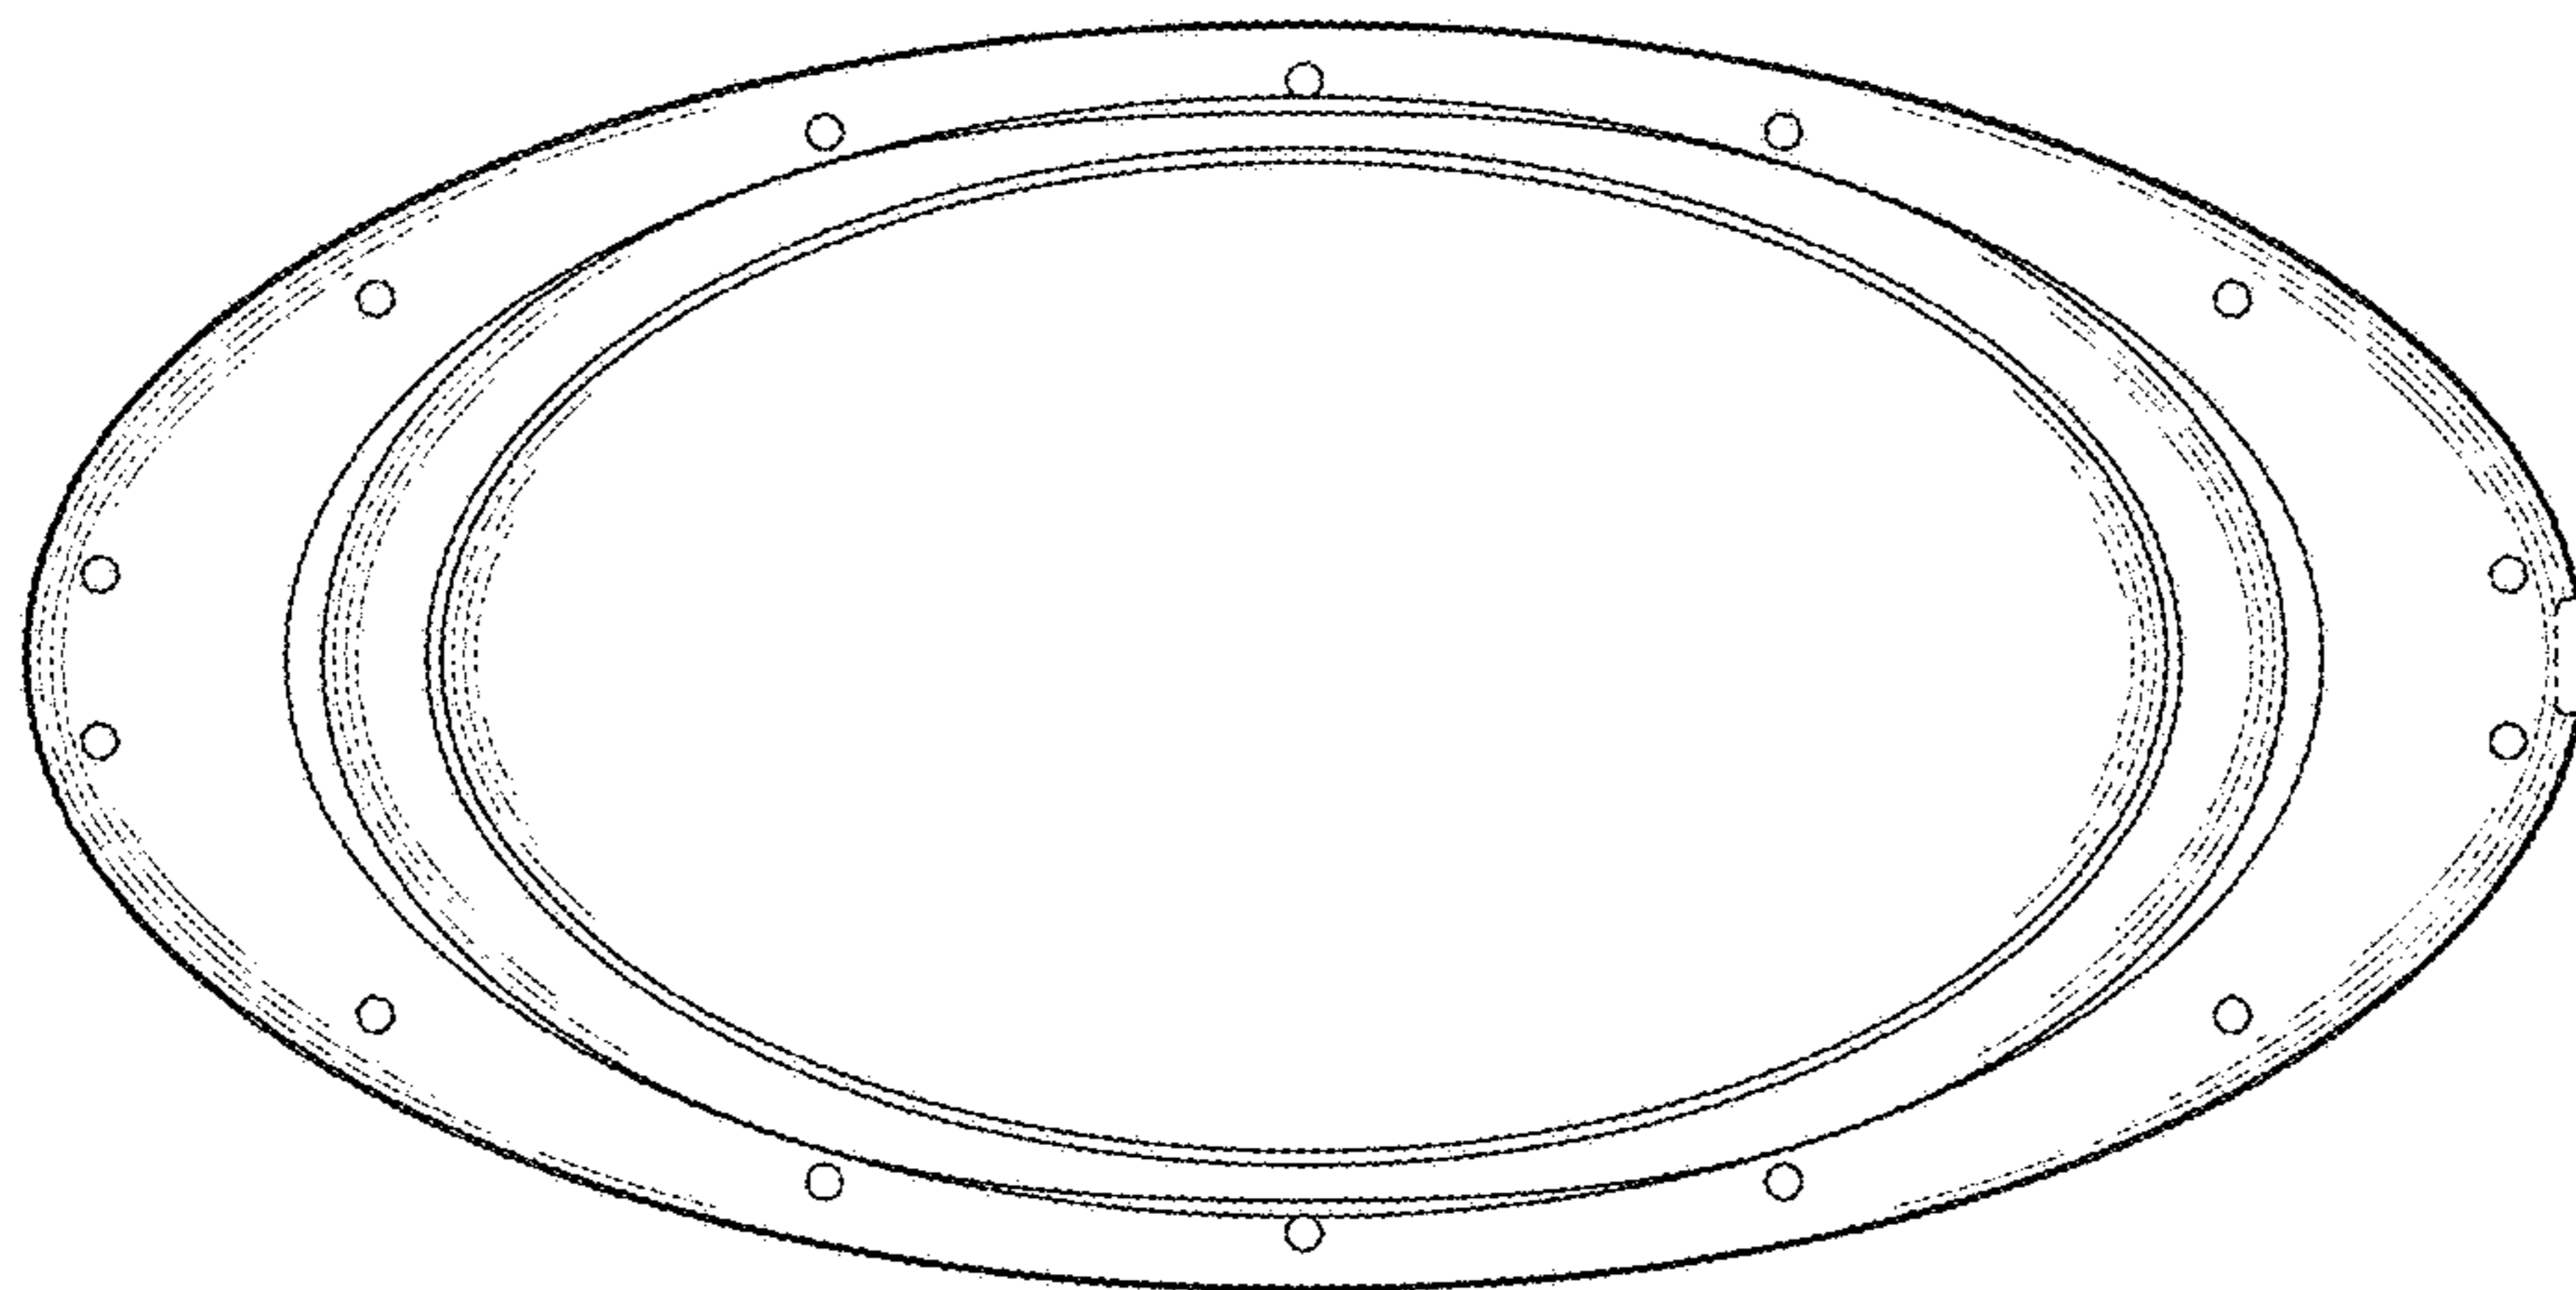


FIG.8

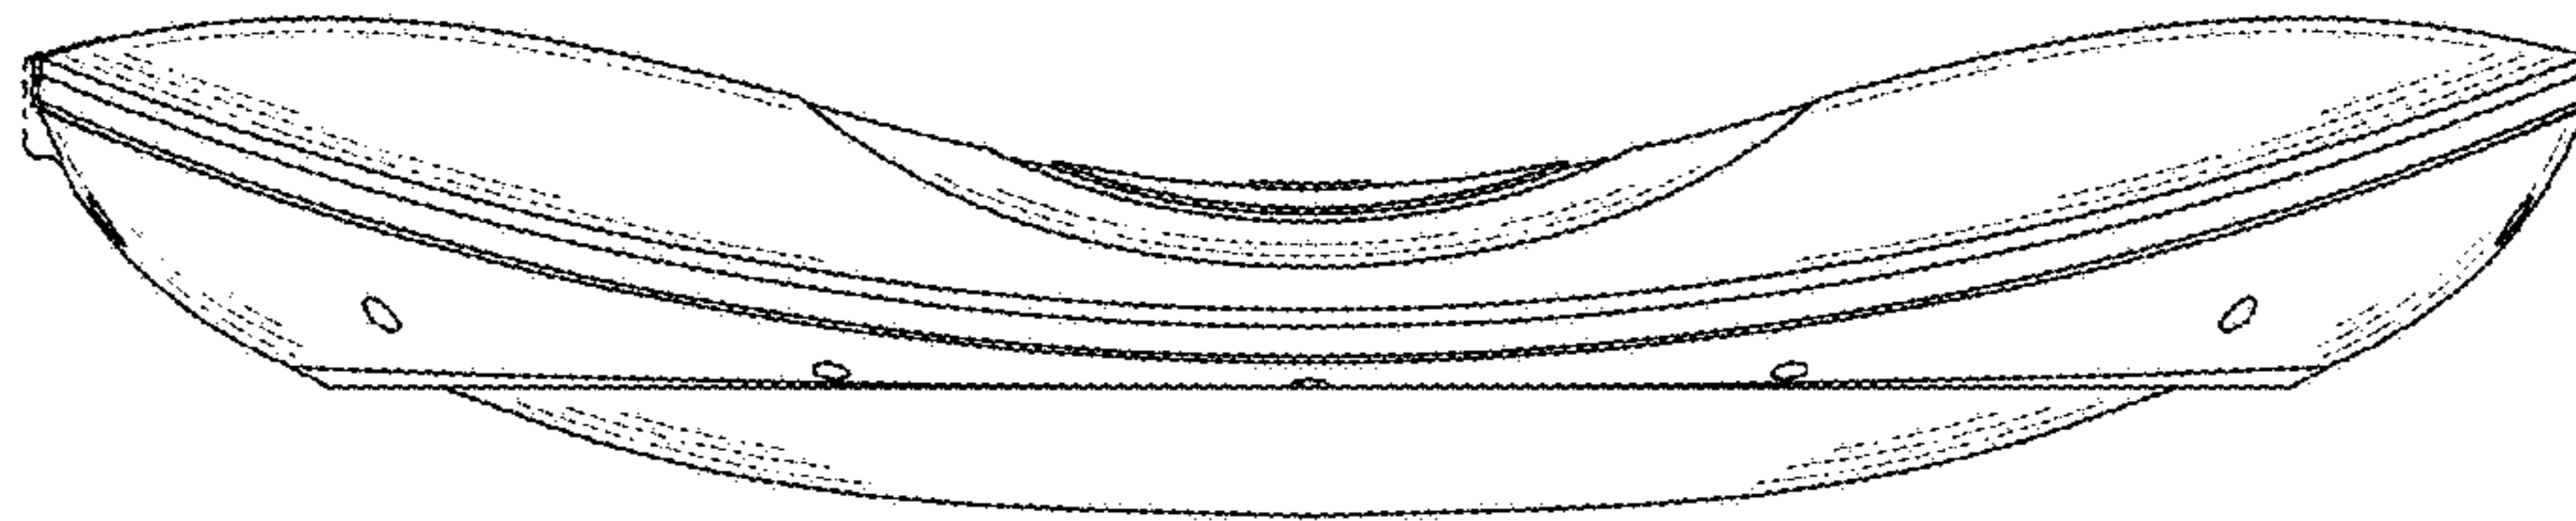


FIG.9