



US00D863532S

(12) **United States Design Patent** (10) **Patent No.:** **US D863,532 S**
Jackson et al. (45) **Date of Patent:** **** Oct. 15, 2019**

(54) **METERED-DOSE INHALER PUMP UNIT**

(71) Applicant: **Optimist Inhaler, LLC**, Buford, GA (US)

(72) Inventors: **David N. Jackson**, Buford, GA (US);
Russell M Smith, Buford, GA (US)

(73) Assignee: **Optimist Inhaler LLC**, Gainesville, GA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/675,656**

(22) Filed: **Jan. 4, 2019**

(51) **LOC (12) Cl.** **29-02**

(52) **U.S. Cl.**
USPC **D24/110**

(58) **Field of Classification Search**
USPC D24/108, 110, 110.5, 164, 127
CPC A61M 15/009; A61M 2202/064; A61M 15/0065; A61M 15/00; A61M 15/008; A61M 15/0068; A61M 15/0091; A61M 2205/3592; A61M 2205/3553; A61M 15/0021

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,834,083 A * 5/1989 Byram A61M 15/009 128/200.14
5,450,336 A * 9/1995 Rubsamen A61M 15/0091 341/120
D439,656 S * 3/2001 Andersson D24/110
D444,225 S * 6/2001 Andersson D24/110
D496,456 S * 9/2004 Harvey D24/110
D582,543 S * 12/2008 Lucking D24/110
D620,588 S * 7/2010 Nielsen D24/110

2010/0094099 A1 * 4/2010 Levy A61M 15/009 600/300
2013/0087142 A1 * 4/2013 Kane A61M 15/009 128/200.23
2016/0325058 A1 11/2016 Samson et al.
2017/0042215 A1 2/2017 Murison
2017/0319797 A1 11/2017 Germinario et al.

FOREIGN PATENT DOCUMENTS

WO WO2016187156 A1 11/2016
WO WO2017182975 A1 10/2017

OTHER PUBLICATIONS

Mhealthspot, <http://mhealthspot.com/2016/02/adherium-smart-inhalers-multicountry-study>, Mar. 18, 2017.
Vaporsmooth, <https://vaporsmooth.com/breeze-smart-inhaler-new-breeze-vaporizer-by-resolve-digital-health>, Jun. 24, 2017.

(Continued)

Primary Examiner — Lilyana Bekic
(74) *Attorney, Agent, or Firm* — Mehrman Law Office;
Michael J. Mehrman


(57) **CLAIM**

The ornamental design for a metered-dose inhaler pump unit, as shown and described.

DESCRIPTION

FIG. 1 is a left side, front, and top perspective view of a metered-dose inhaler pump unit, showing the new design. FIG. 2 is a front elevational view thereof. FIG. 3 is a left side elevational view thereof. FIG. 4 is a top plan view thereof; and, FIG. 5 is a bottom plan view thereof. The broken lines in the drawings depict portions of the metered-dose inhaler pump unit that form no part of the claimed design.

1 Claim, 2 Drawing Sheets

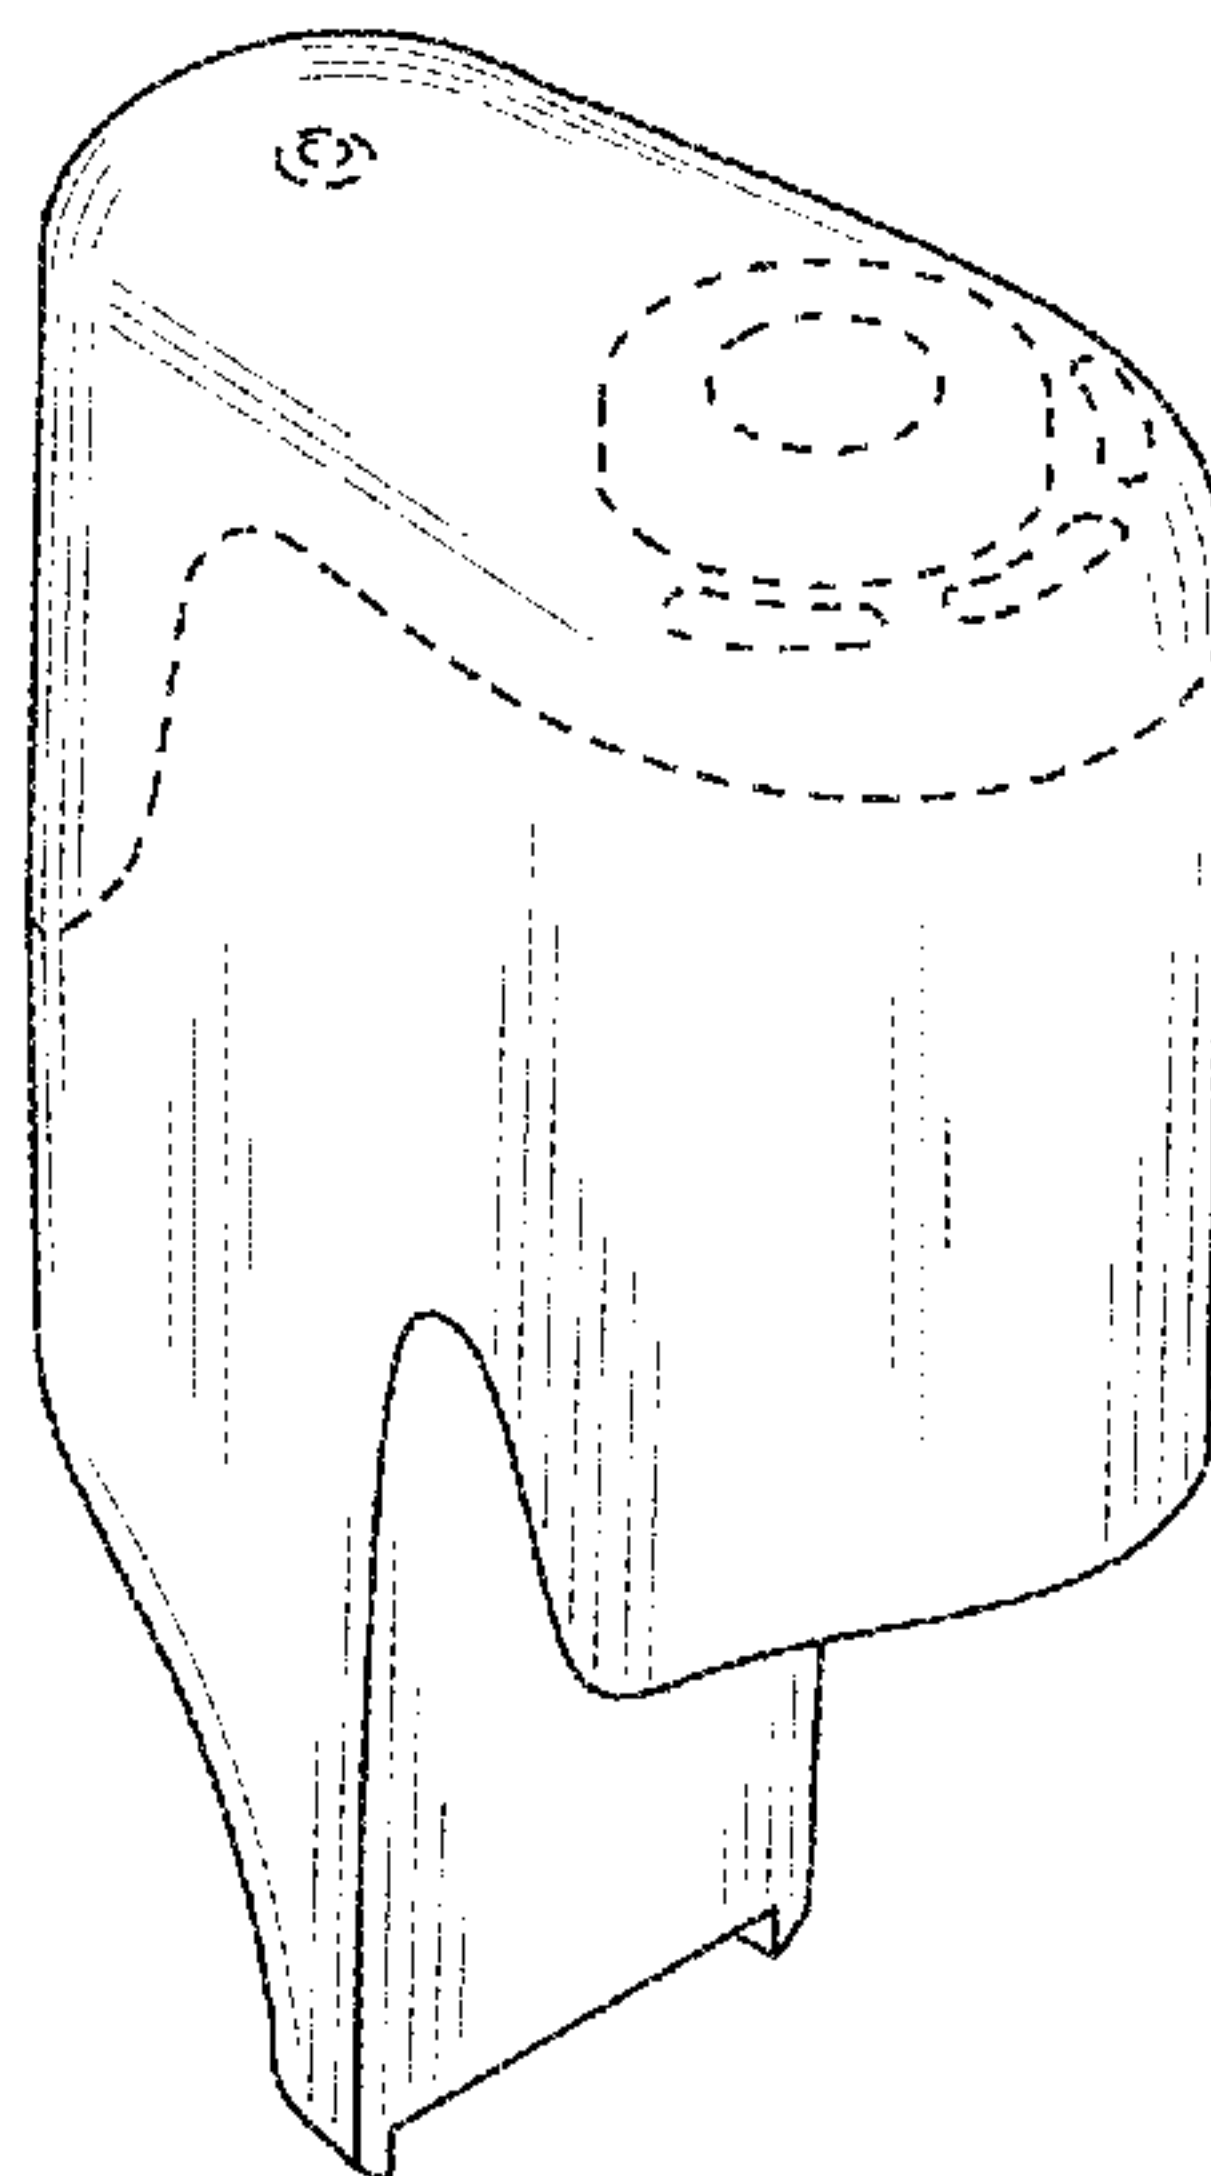

(56)

References Cited

OTHER PUBLICATIONS

www.3ders.org, <http://www.3ders.org/articles/20160314-3d-printed-smart-inhaler-could-help-doctors-better-understand-asthma.html>, Mar. 16, 2016.

Medgadget, <https://www.medgadget.com/2014/06/nexus6-smarttouch-inhaler-monitor-helps-patients-adhere-to-medication-regimens.html>, Jun. 6, 2014.

Syqemmedical, <https://www.syqemmedical.com>, Dec. 1, 2016.

www.vccny.com, <http://www.vmcny.com/blog/2016/12/01/albuterol-toxicity-in-pets-where-is-your-inhaler>, Dec. 1, 2016.

* cited by examiner

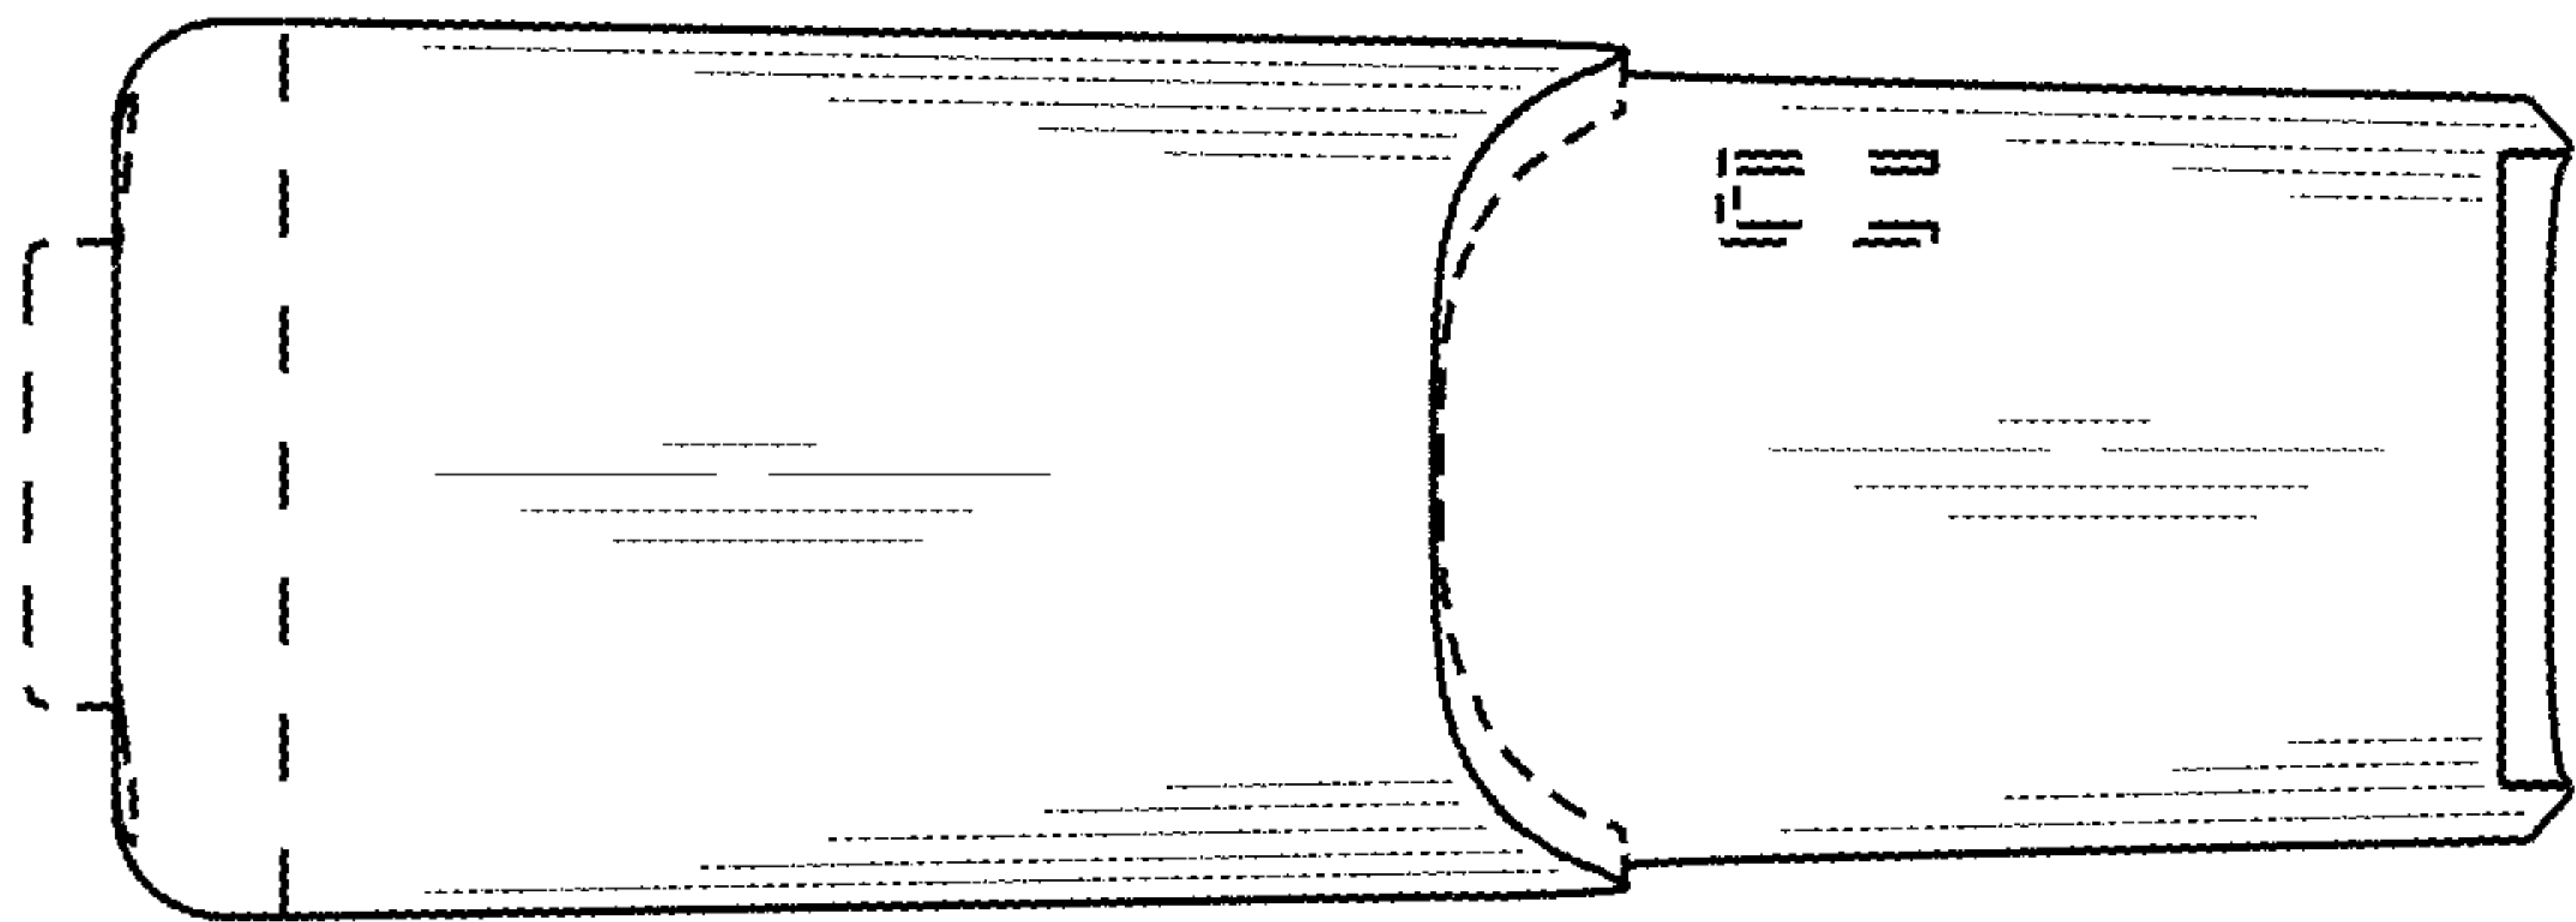


Fig. 2

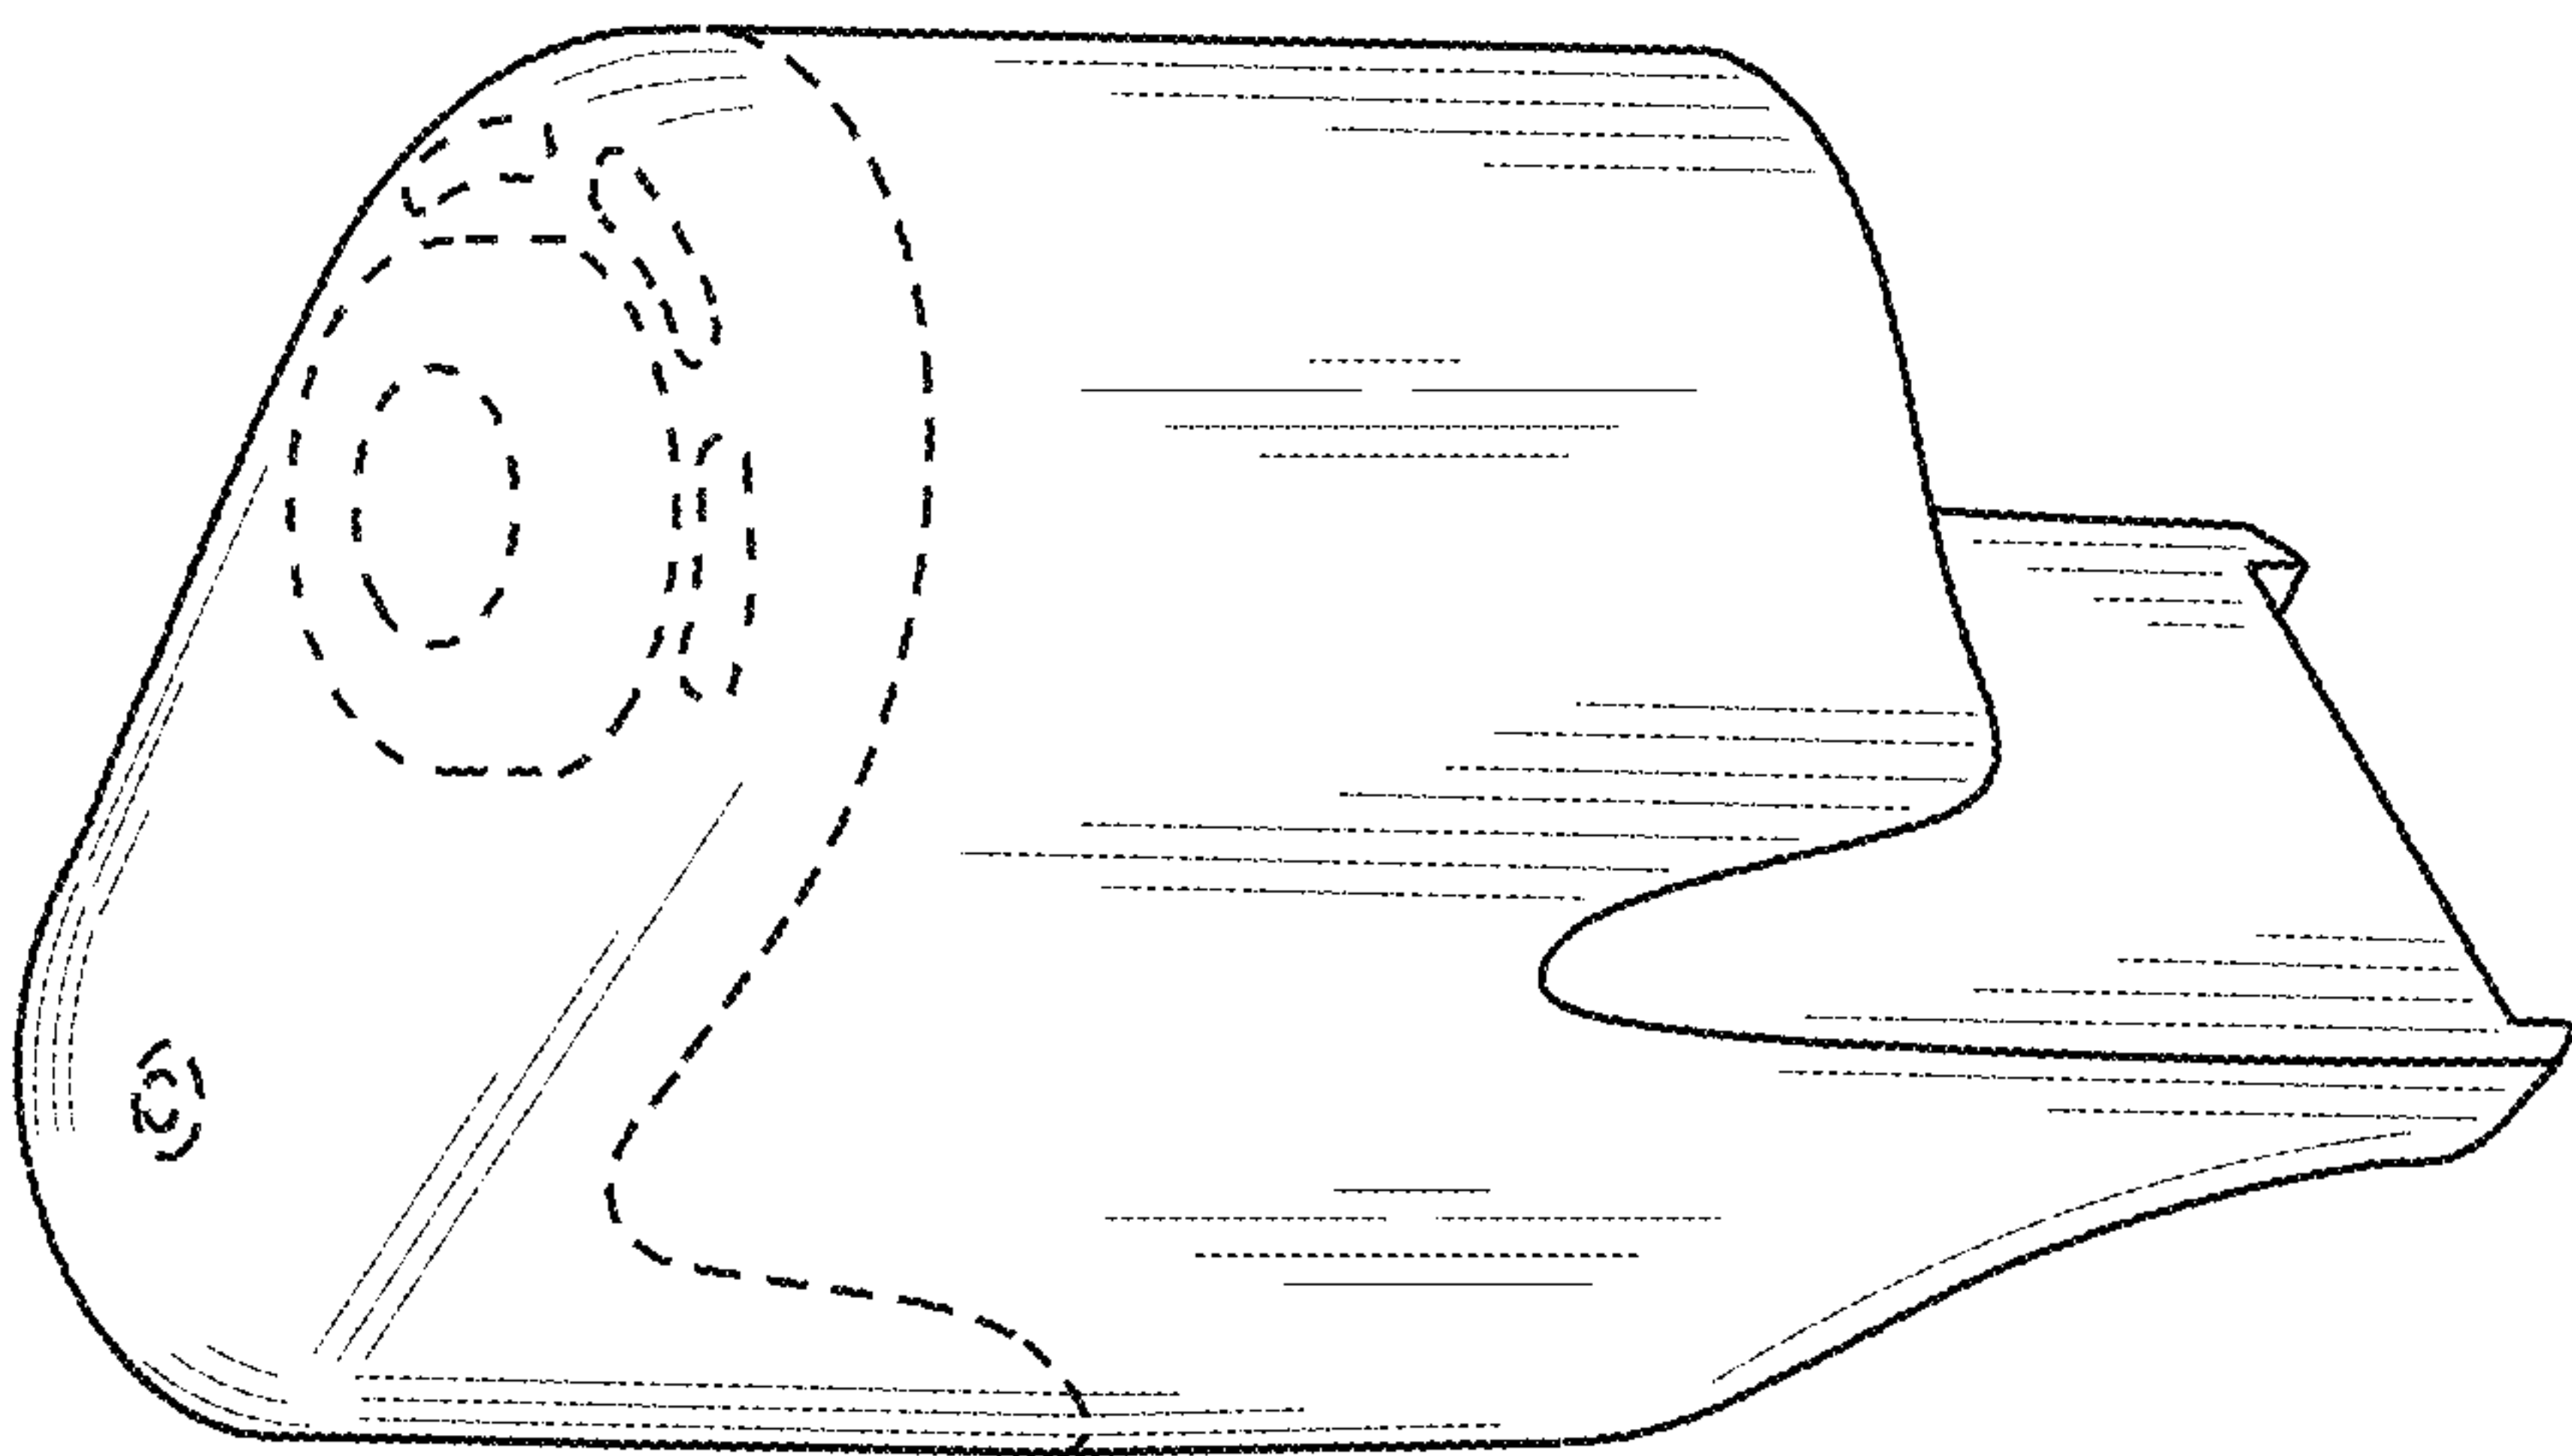


Fig. 1

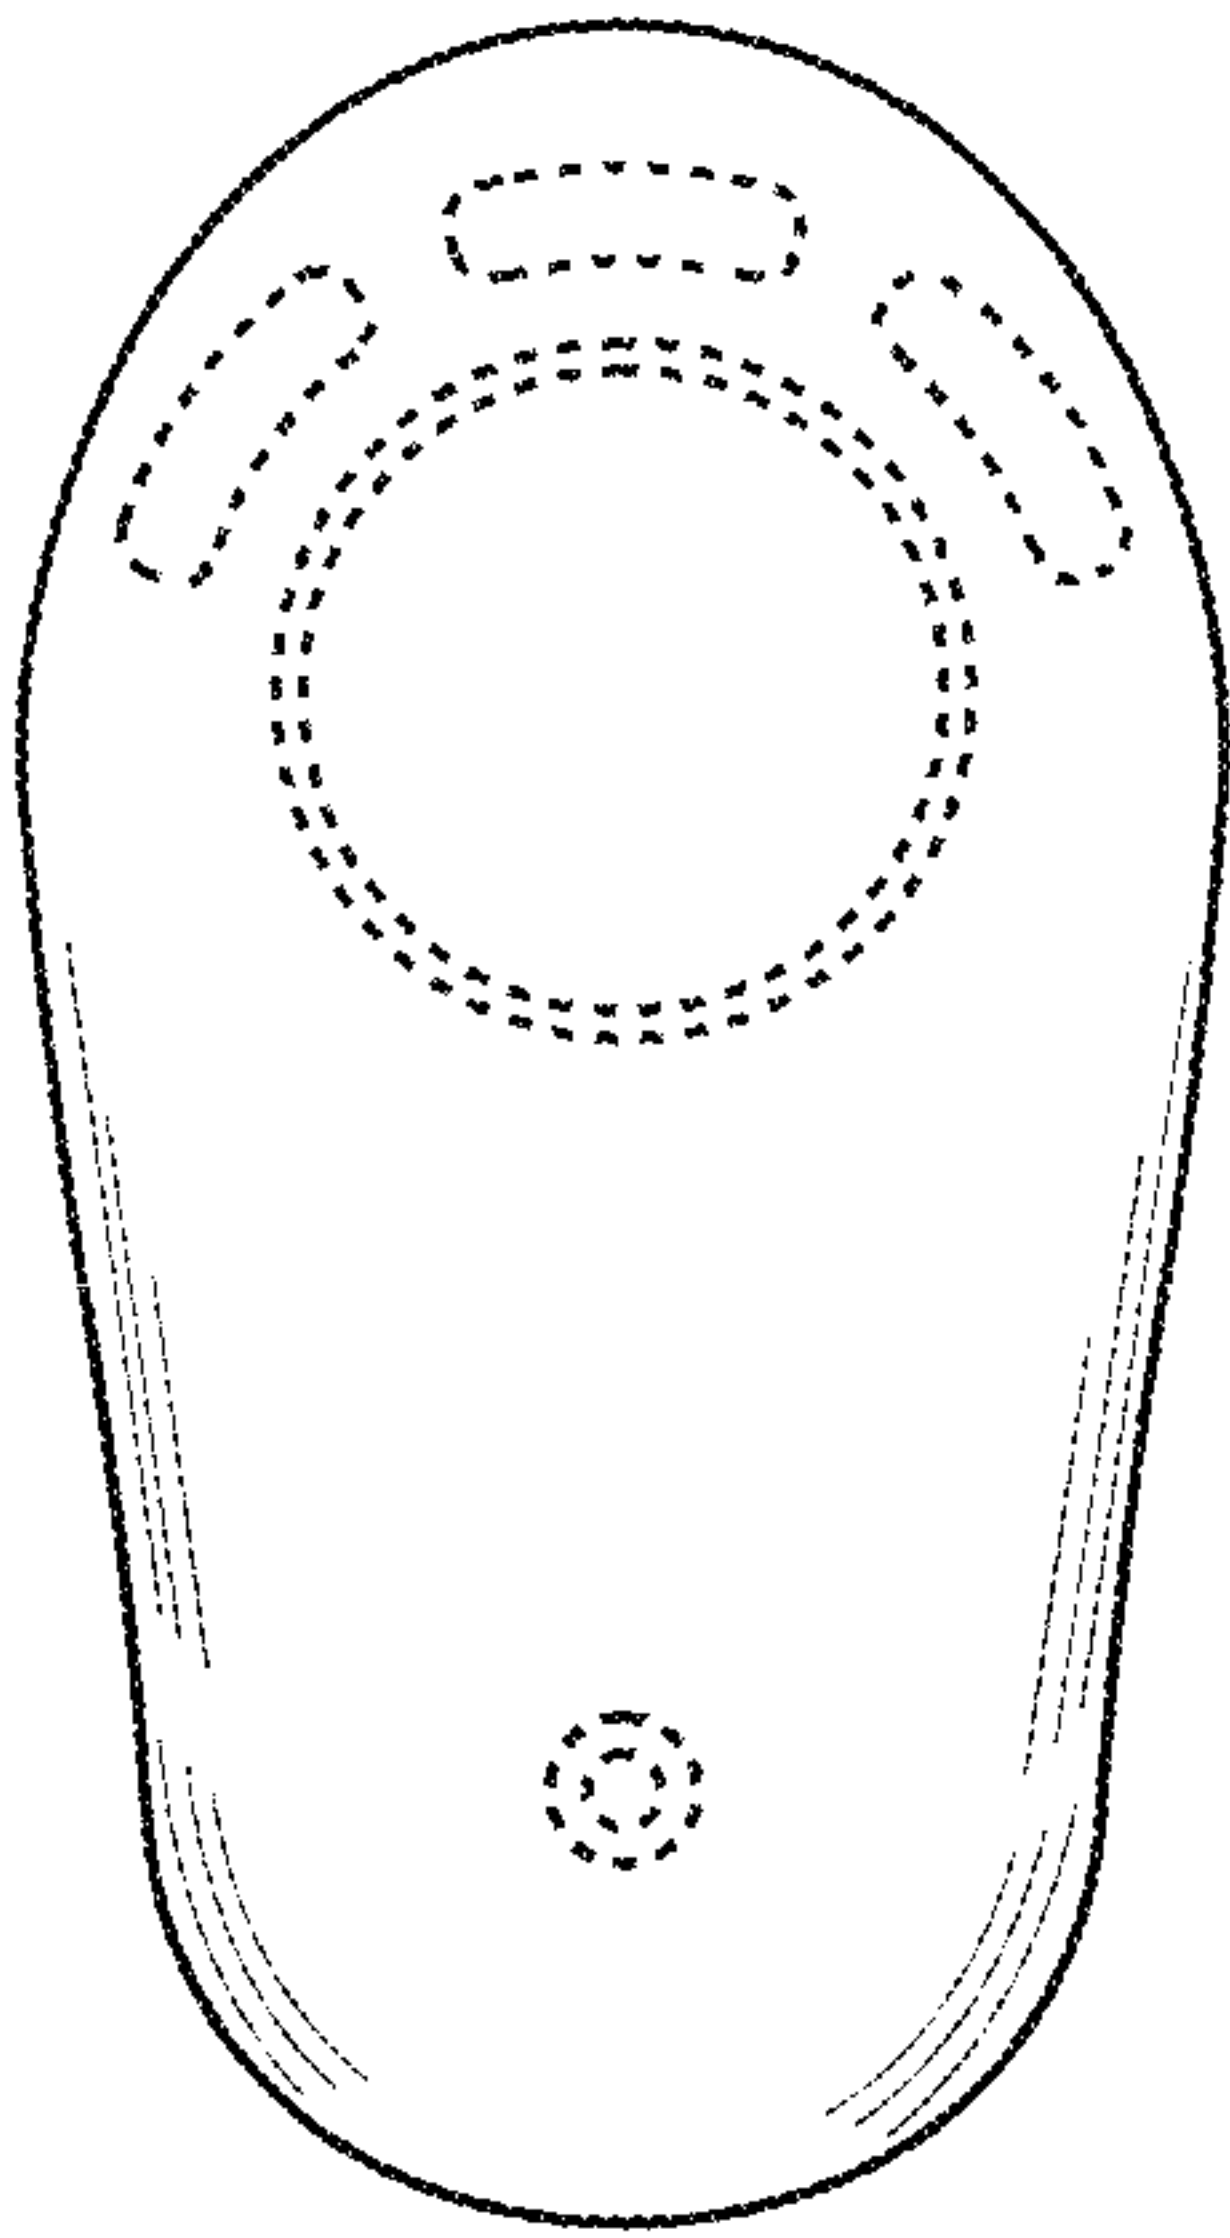


Fig. 4

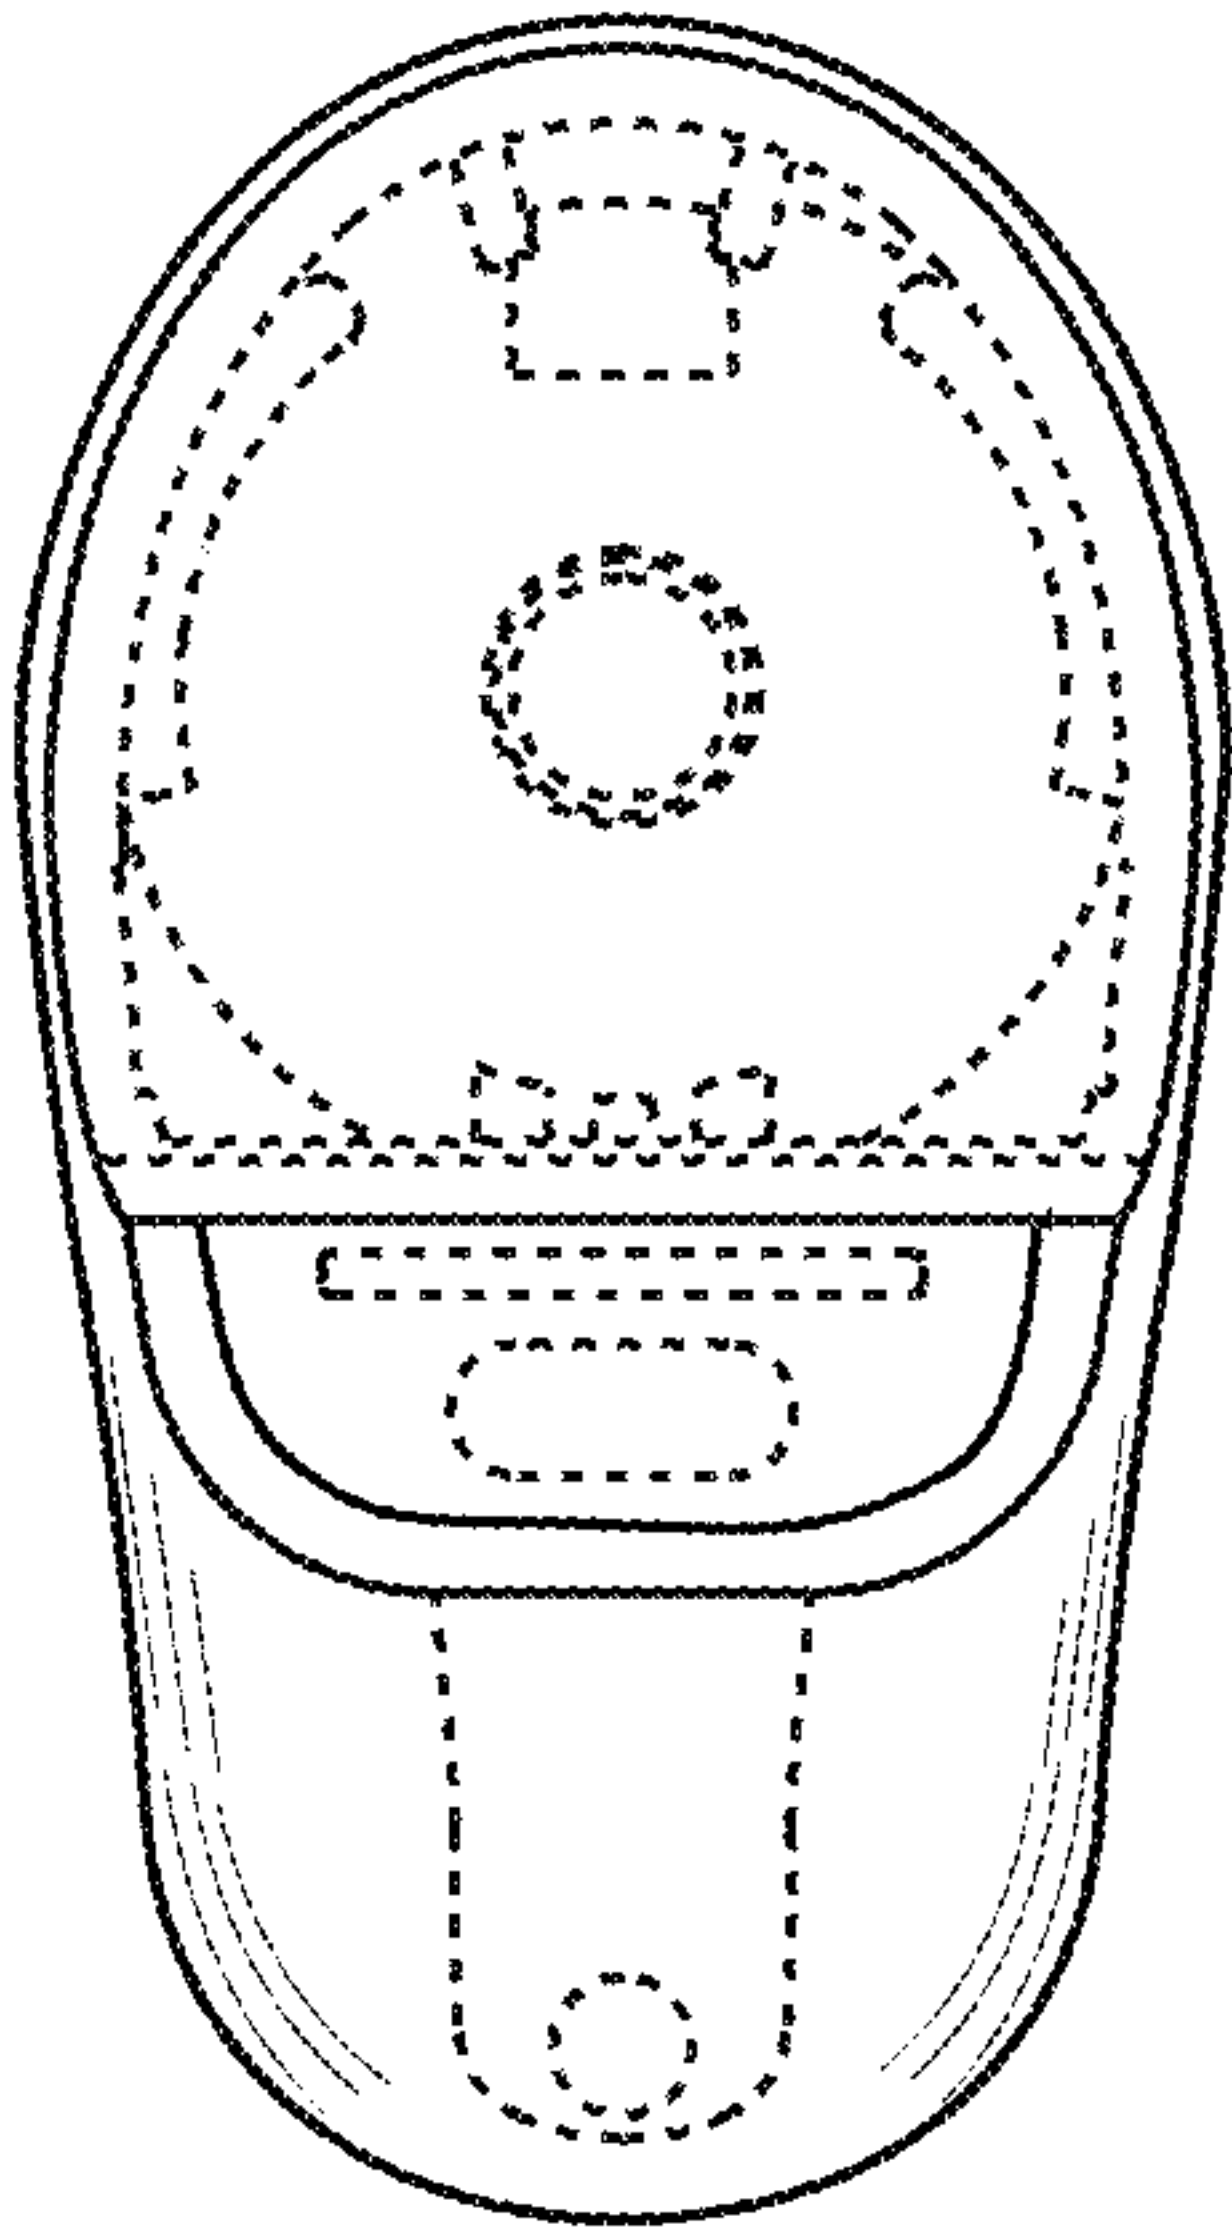


Fig. 5

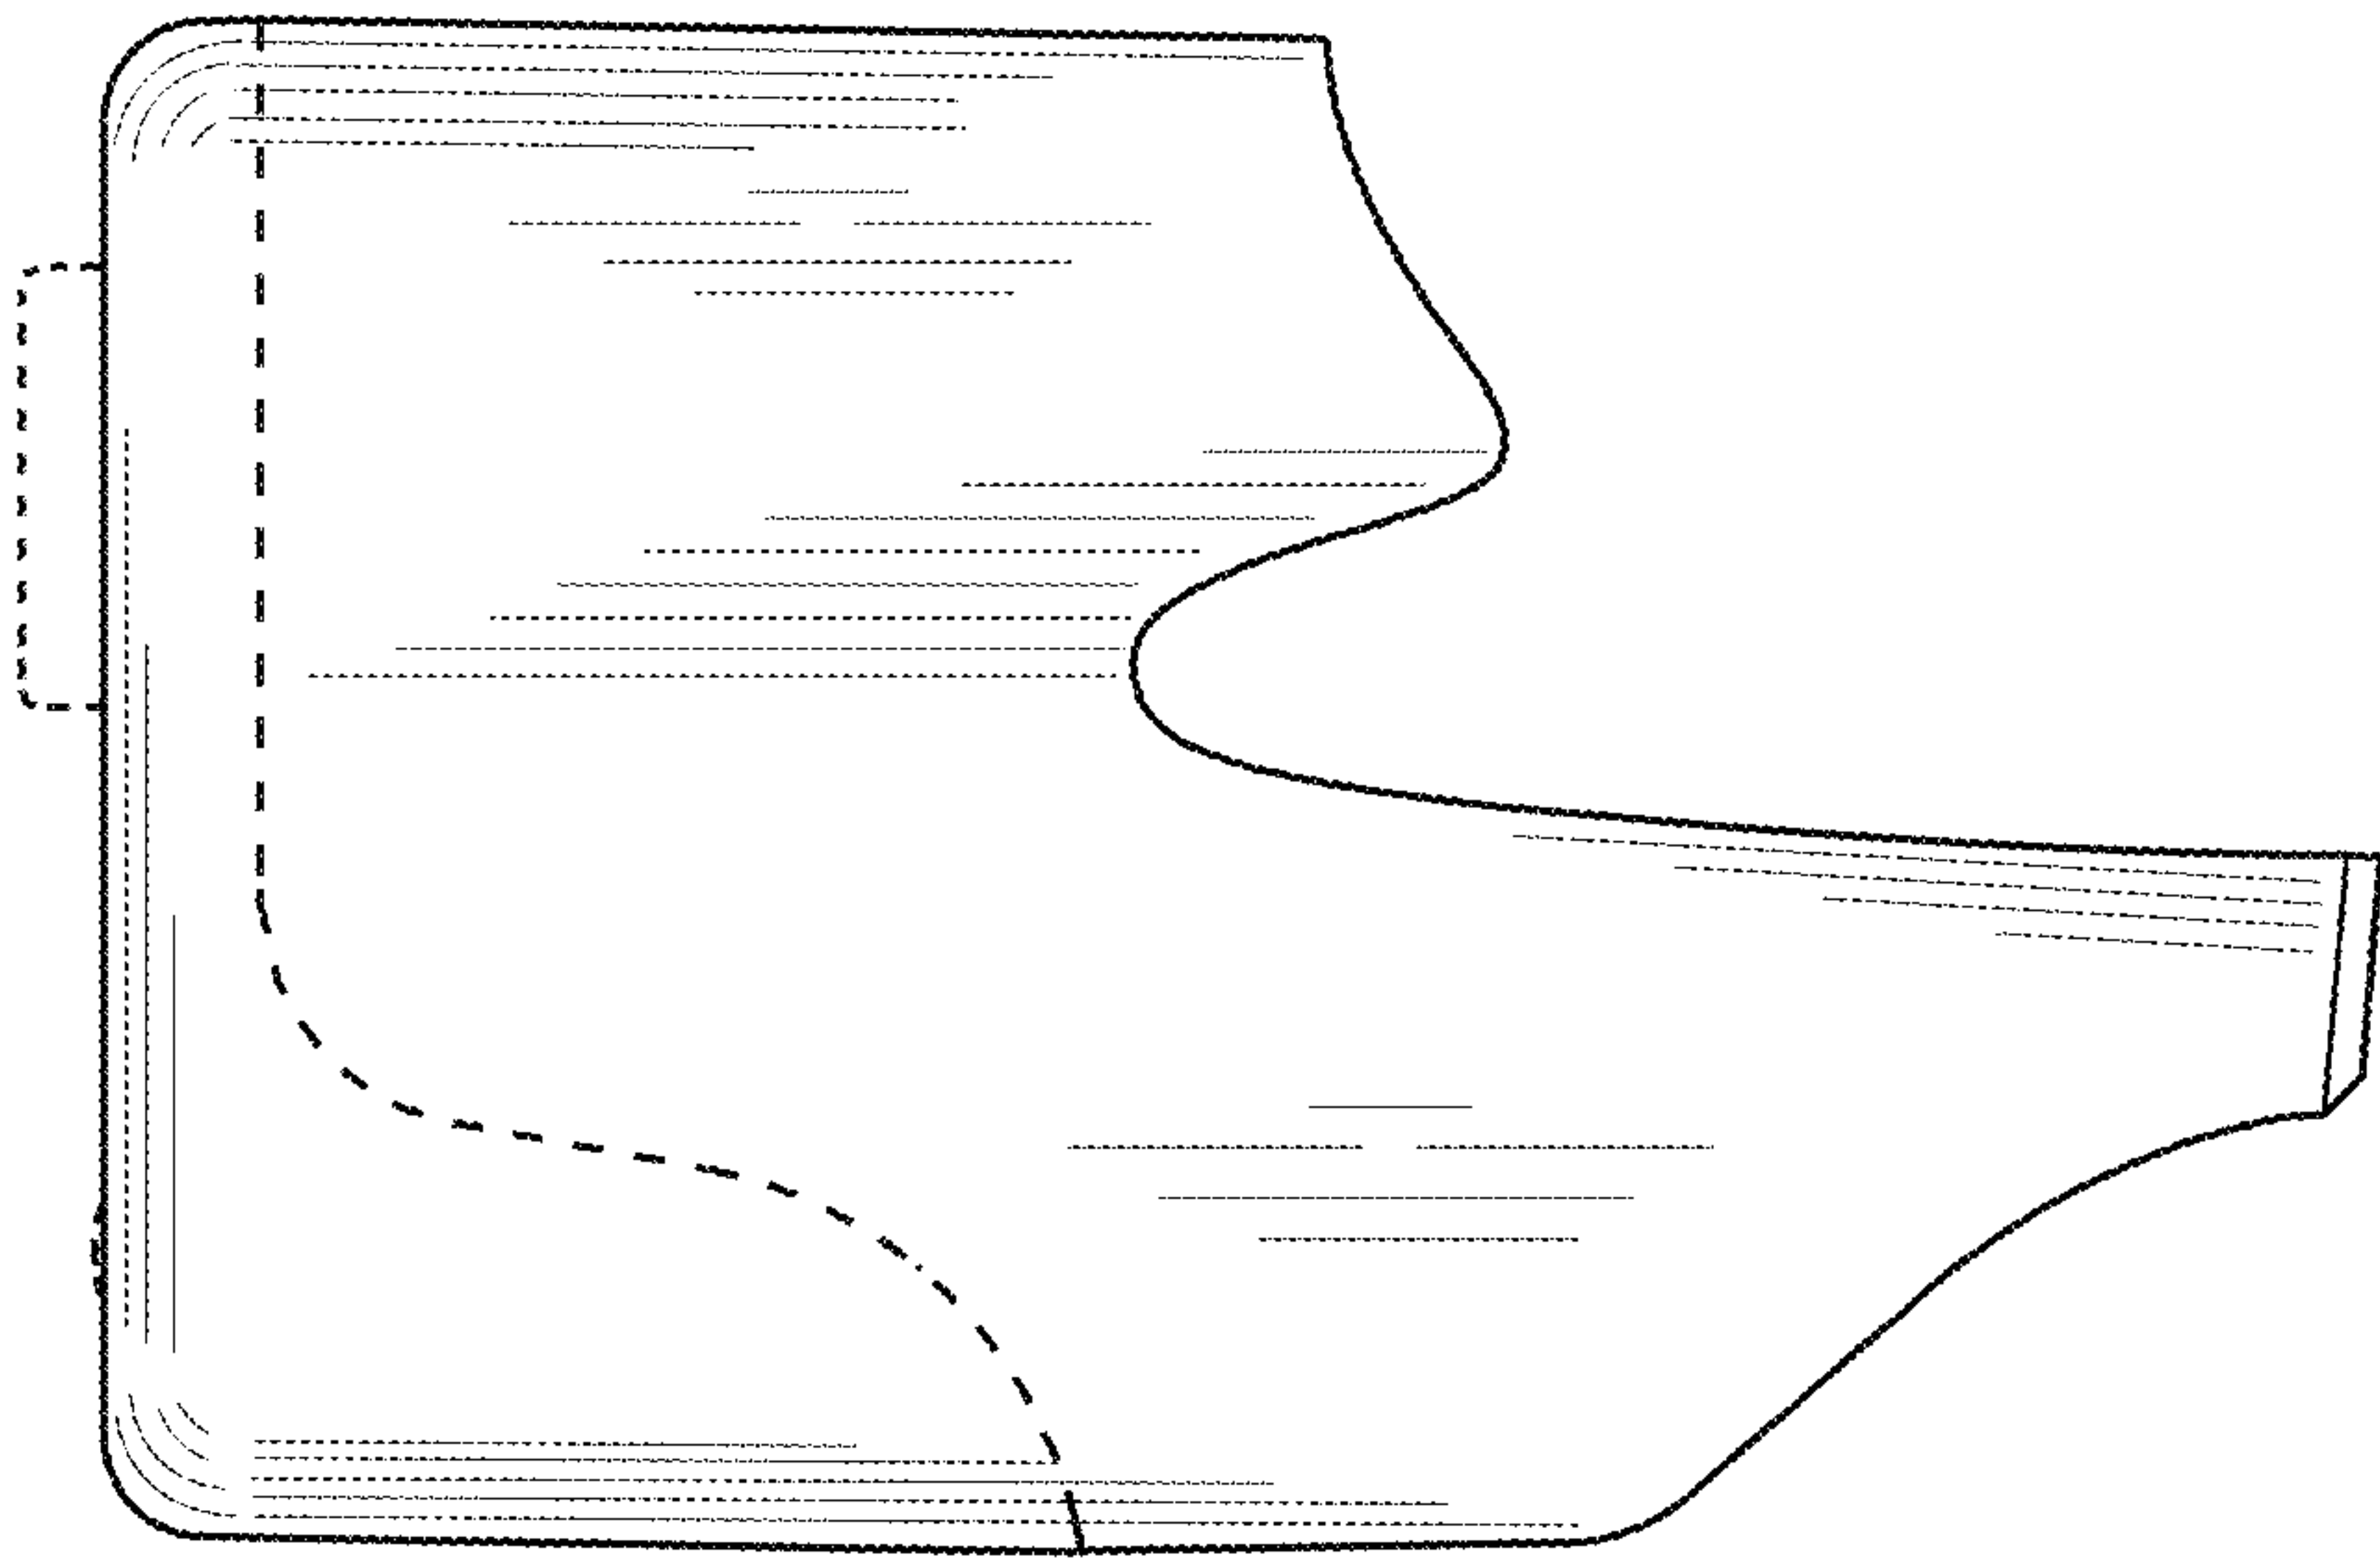


Fig. 3