



US00D863533S

(12) **United States Design Patent** (10) **Patent No.:** **US D863,533 S**  
**Jackson et al.** (45) **Date of Patent:** **\*\* Oct. 15, 2019**

(54) **METERED-DOSE INHALER**  
(71) Applicant: **Optimist Inhaler, LLC**, Buford, GA (US)  
(72) Inventors: **David N. Jackson**, Buford, GA (US); **Russell M Smith**, Buford, GA (US)  
(73) Assignee: **Optimist Inhaler LLC**, Gainesville, GA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/675,664**  
(22) Filed: **Jan. 4, 2019**  
(51) **LOC (12) Cl.** ..... **29-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/110**  
(58) **Field of Classification Search**  
USPC ..... D24/108, 110, 110.5, 164, 127  
CPC ..... A61M 15/009; A61M 2202/064; A61M 15/0065; A61M 15/00; A61M 15/008; A61M 15/0068; A61M 15/0091; A61M 2205/3592; A61M 2205/3553; A61M 15/0021

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,834,083 A \* 5/1989 Byram ..... A61M 15/009 128/200.14  
5,450,336 A \* 9/1995 Rubsamen ..... A61M 15/0091 341/120  
D439,656 S \* 3/2001 Andersson ..... D24/110  
D444,225 S \* 6/2001 Andersson ..... D24/110  
D496,456 S \* 9/2004 Harvey ..... D24/110  
D582,543 S \* 12/2008 Lucking ..... D24/110  
D620,588 S \* 7/2010 Nielsen ..... D24/110

2010/0094099 A1\* 4/2010 Levy ..... A61M 15/009 600/300  
2013/0087142 A1\* 4/2013 Kane ..... A61M 15/009 128/200.23  
2016/0325058 A1 11/2016 Samson et al.  
2017/0042215 A1 2/2017 Murison  
2017/0319797 A1 11/2017 Germinario et al.

**FOREIGN PATENT DOCUMENTS**

WO WO2016187156 A1 11/2016  
WO WO2017182975 A1 10/2017

**OTHER PUBLICATIONS**

Mhealthspot, <http://mhealthspot.com/2016/02/adherium-smart-inhalers-multicountry-study>, Mar. 18, 2017.  
Vaporsmooth, <https://vaporsmooth.com/breeze-smart-inhaler-new-breeze-vaporizer-by-resolve-digital-health>, Jun. 24, 2017.

(Continued)

*Primary Examiner* — Lilyana Bekic  
(74) *Attorney, Agent, or Firm* — Mehrman Law Office; Michael J. Mehrman


(57) **CLAIM**

The ornamental design for a metered-dose inhaler, as shown and described.

**DESCRIPTION**

FIG. 1 is a left side, front, and top perspective view of a metered-dose inhaler showing the new design.  
FIG. 2 is a front elevational view thereof.  
FIG. 3 is a left side elevational view thereof.  
FIG. 4 is a top plan view thereof; and,  
FIG. 5 is a bottom plan view thereof.  
The broken lines in the drawings depict portions of the metered-dose inhaler that form no part of the claimed design.

**1 Claim, 2 Drawing Sheets**

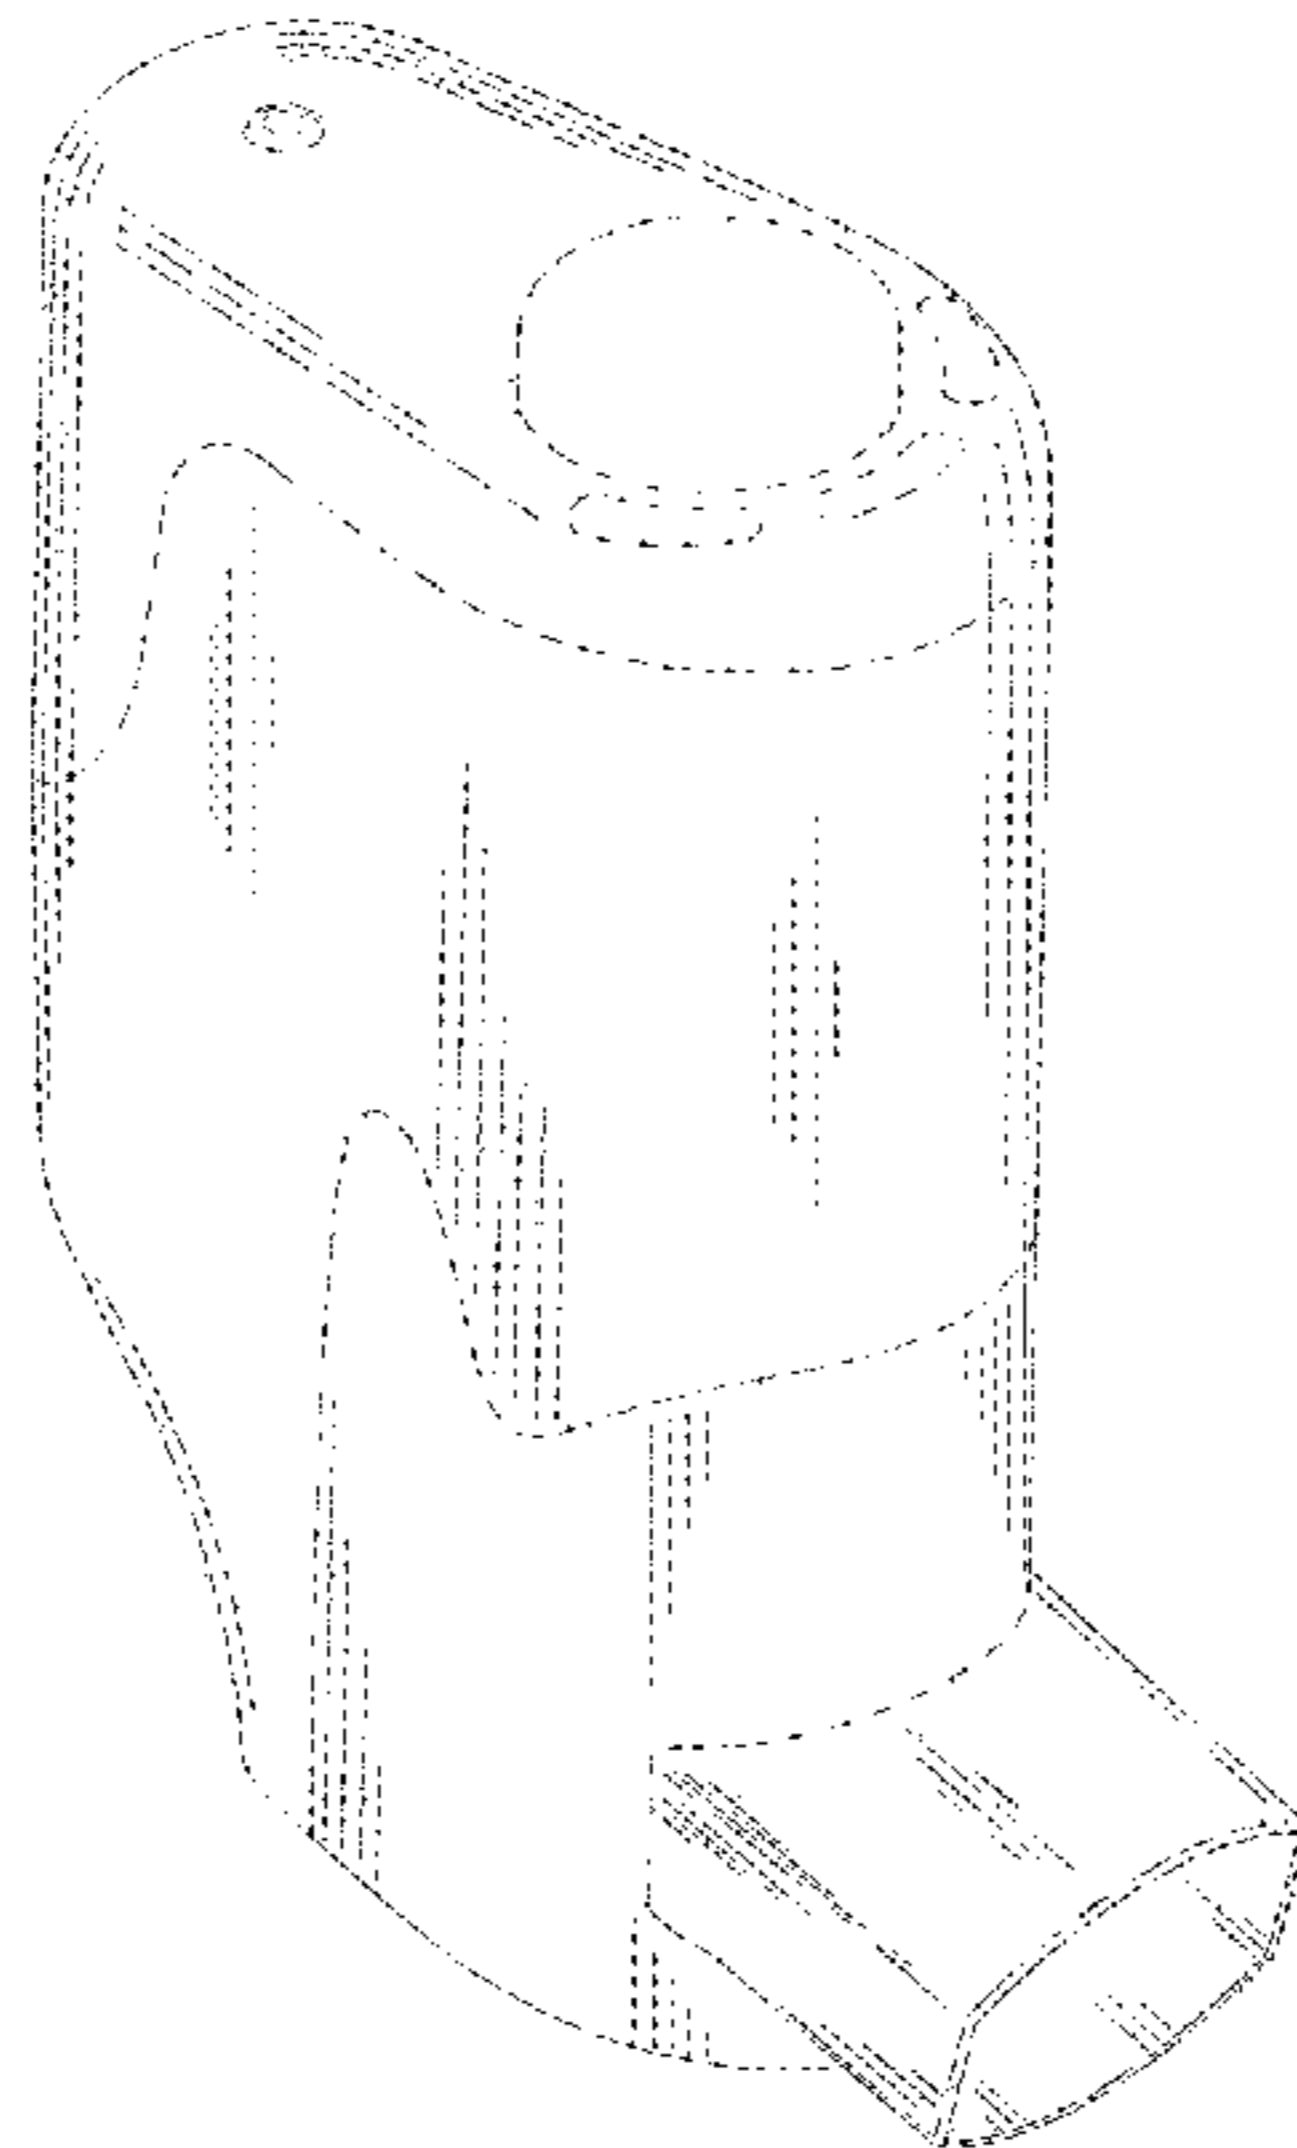

(56)

**References Cited**

OTHER PUBLICATIONS

www.3ders.org, <http://www.3ders.org/articles/20160314-3d-printed-smart-inhaler-could-help-doctors-better-understand-asthma.html>, Mar. 16, 2016.

Medgadget, <https://www.medgadget.com/2014/06/nexus6-smarttouch-inhaler-monitor-helps-patients-adhere-to-medication-regimens.html>, Jun. 6, 2014.

Syqemical, <https://www.syqemical.com>, Dec. 1, 2016.

www.vccny.com, <http://www.vccny.com/blog/2016/12/01/albuterol-toxicity-in-pets-where-is-your-inhaler>, Dec. 1, 2016.

\* cited by examiner

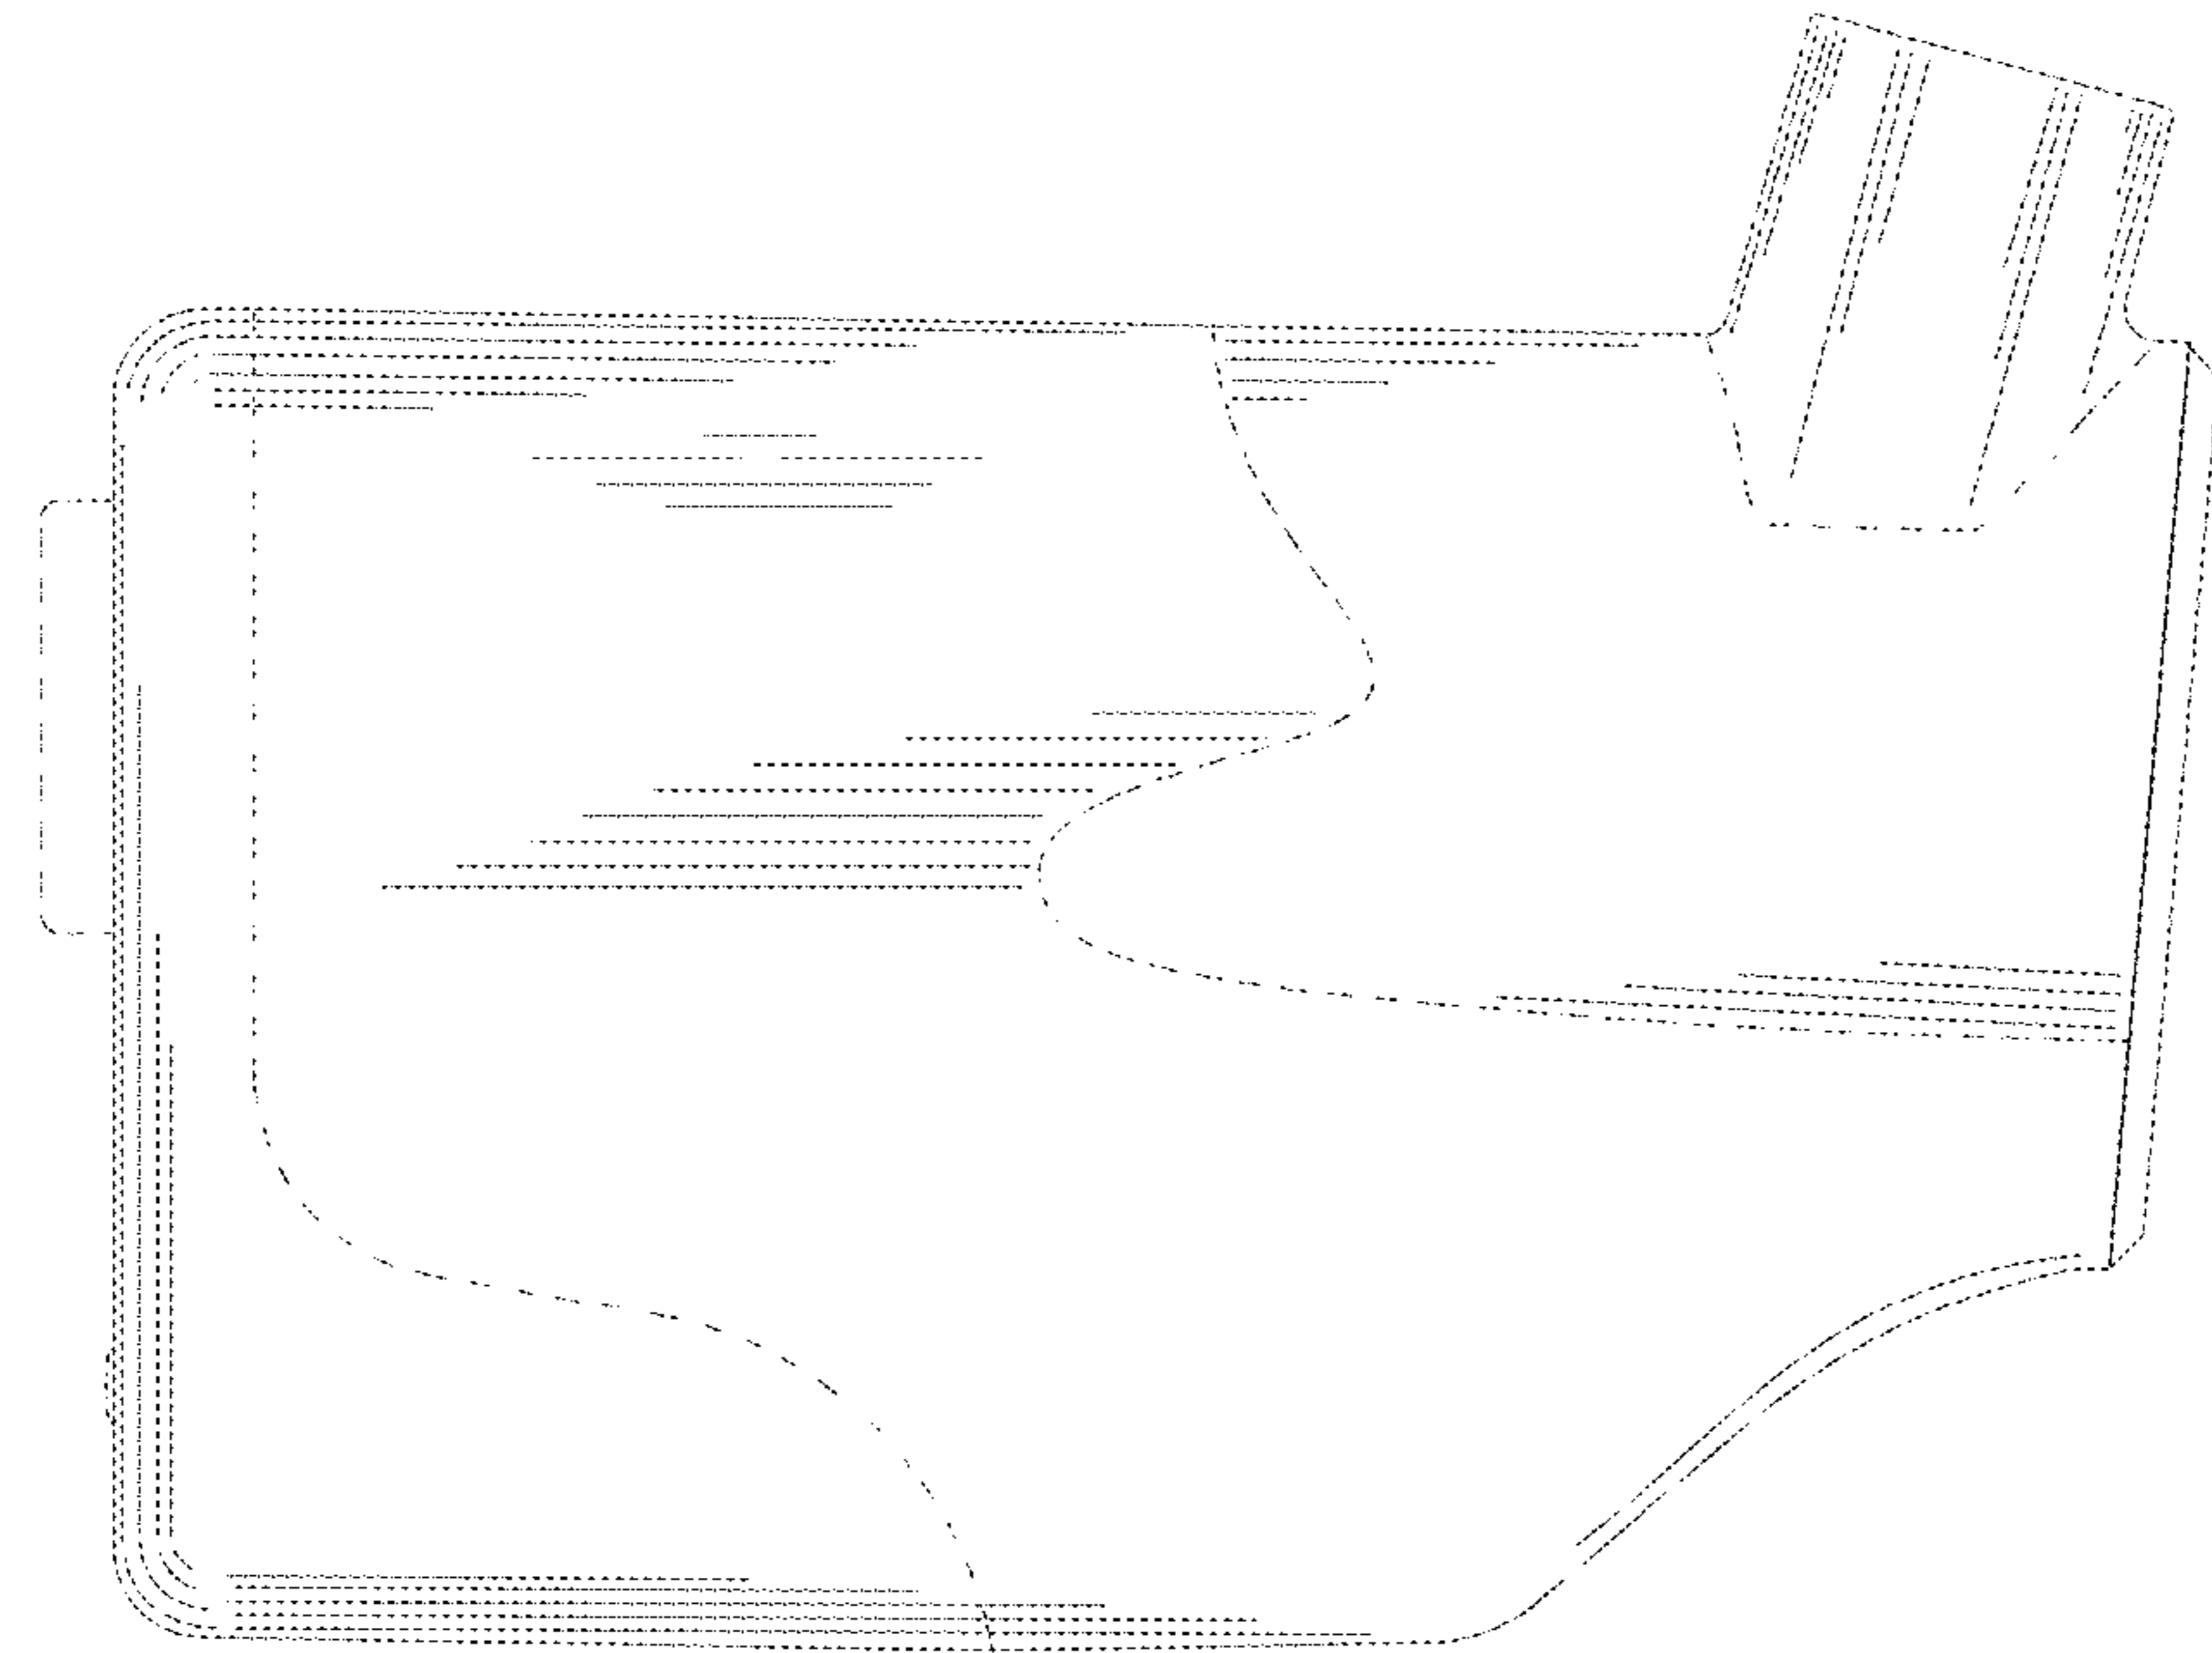


Fig. 1



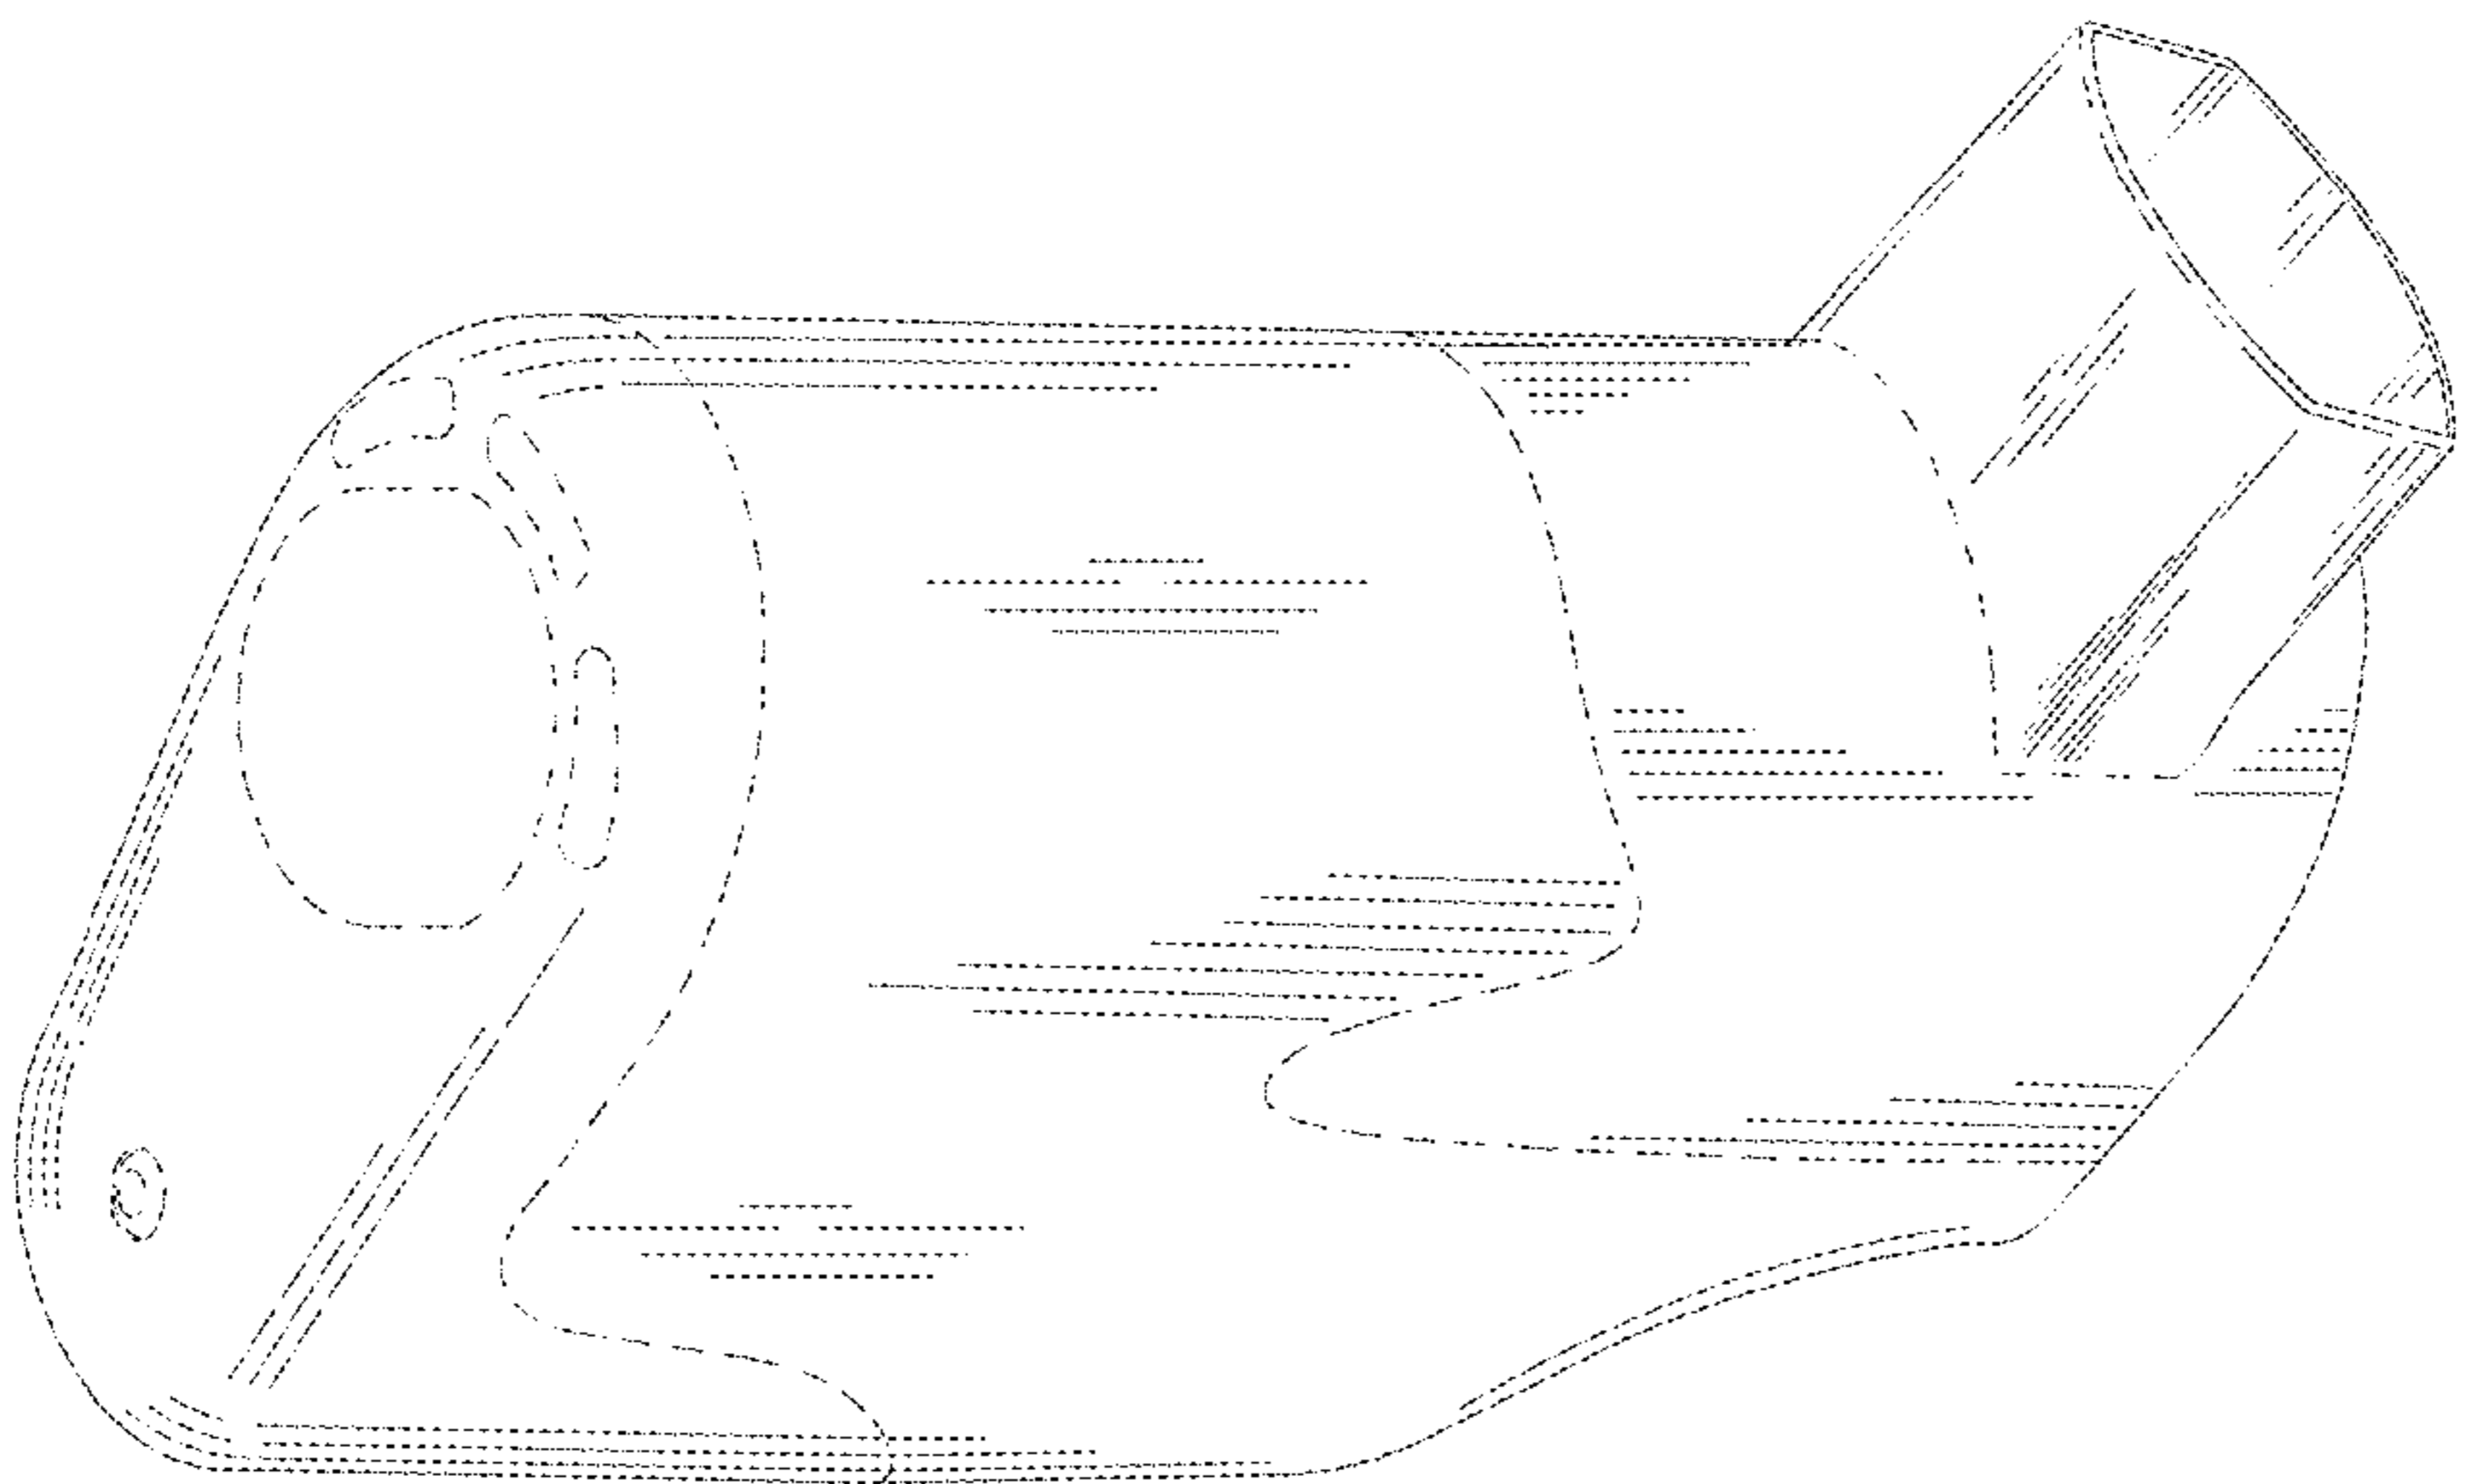



Fig. 2

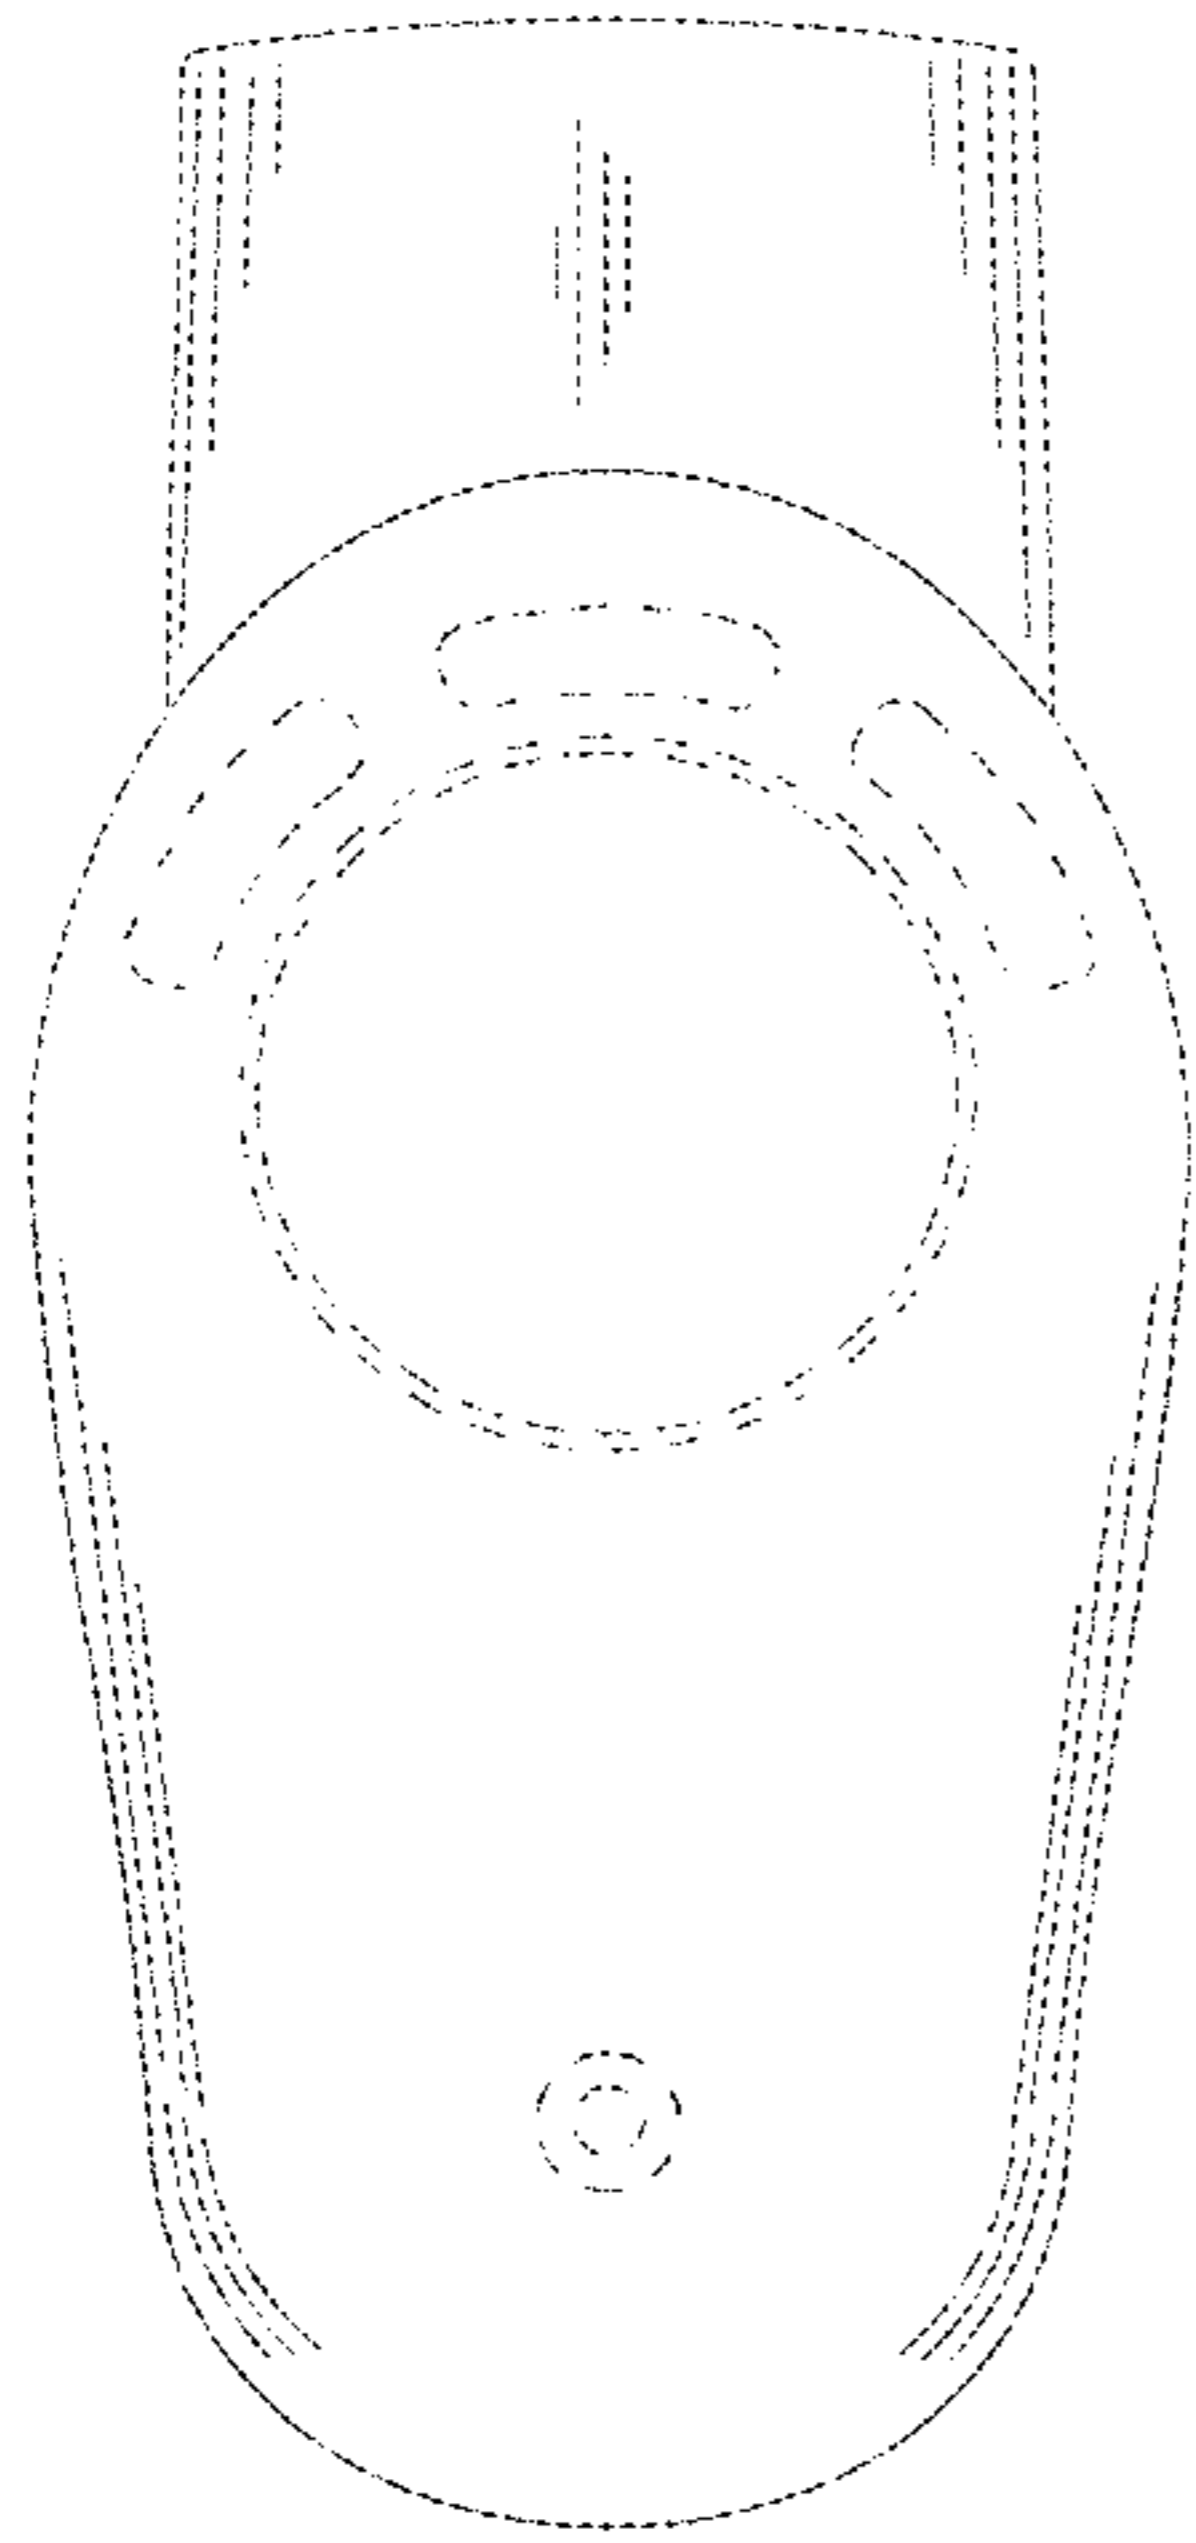

**Fig. 4**

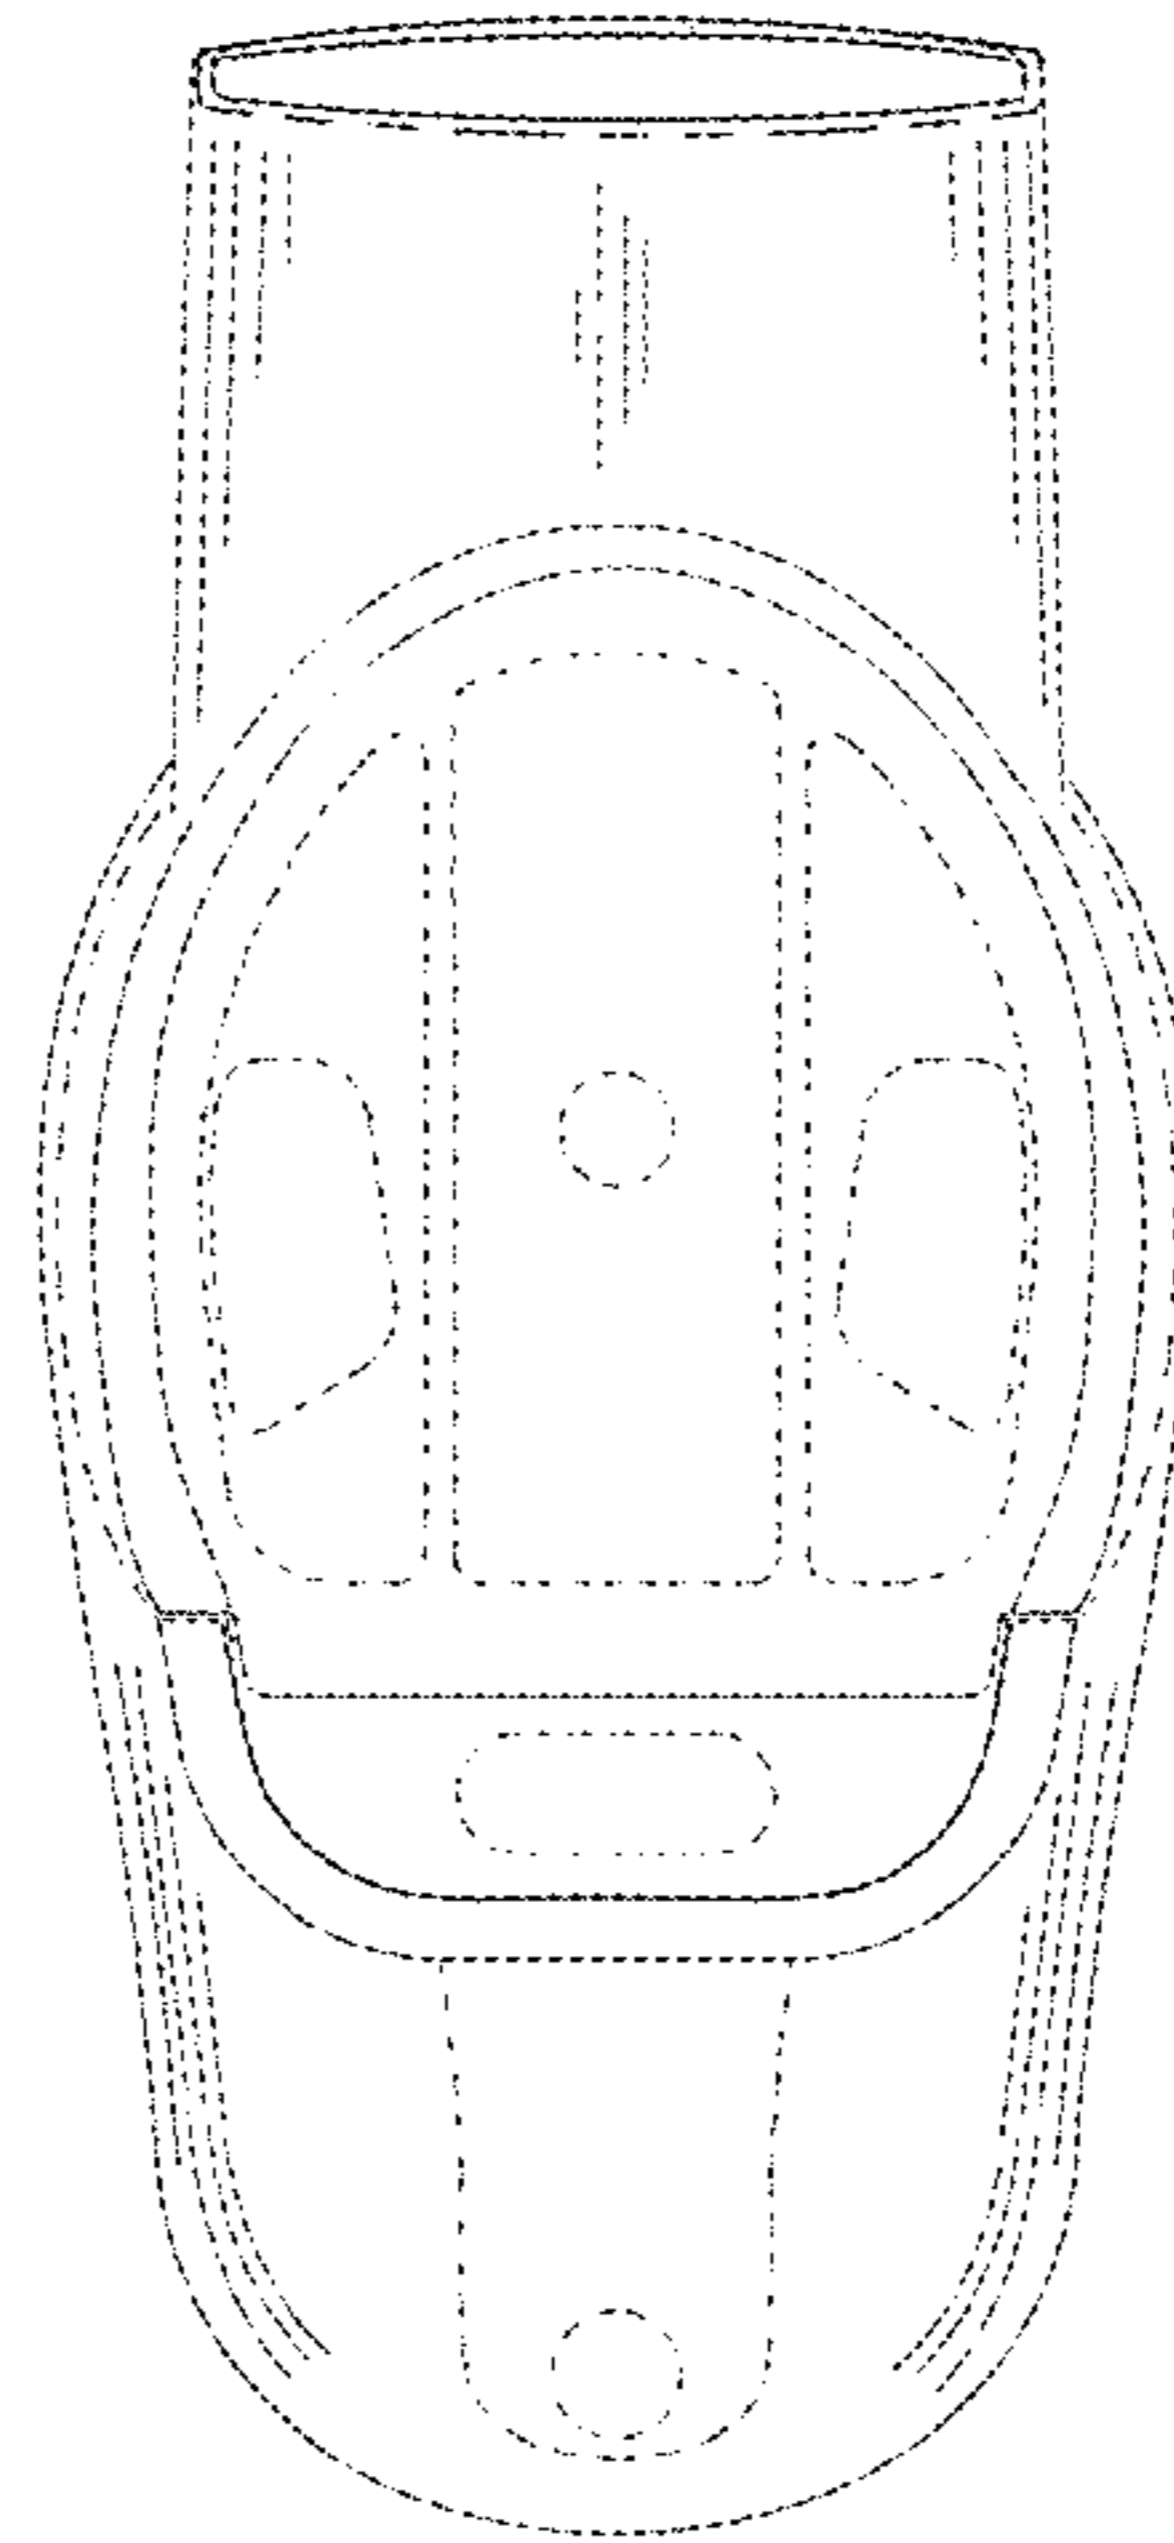

**Fig. 5**

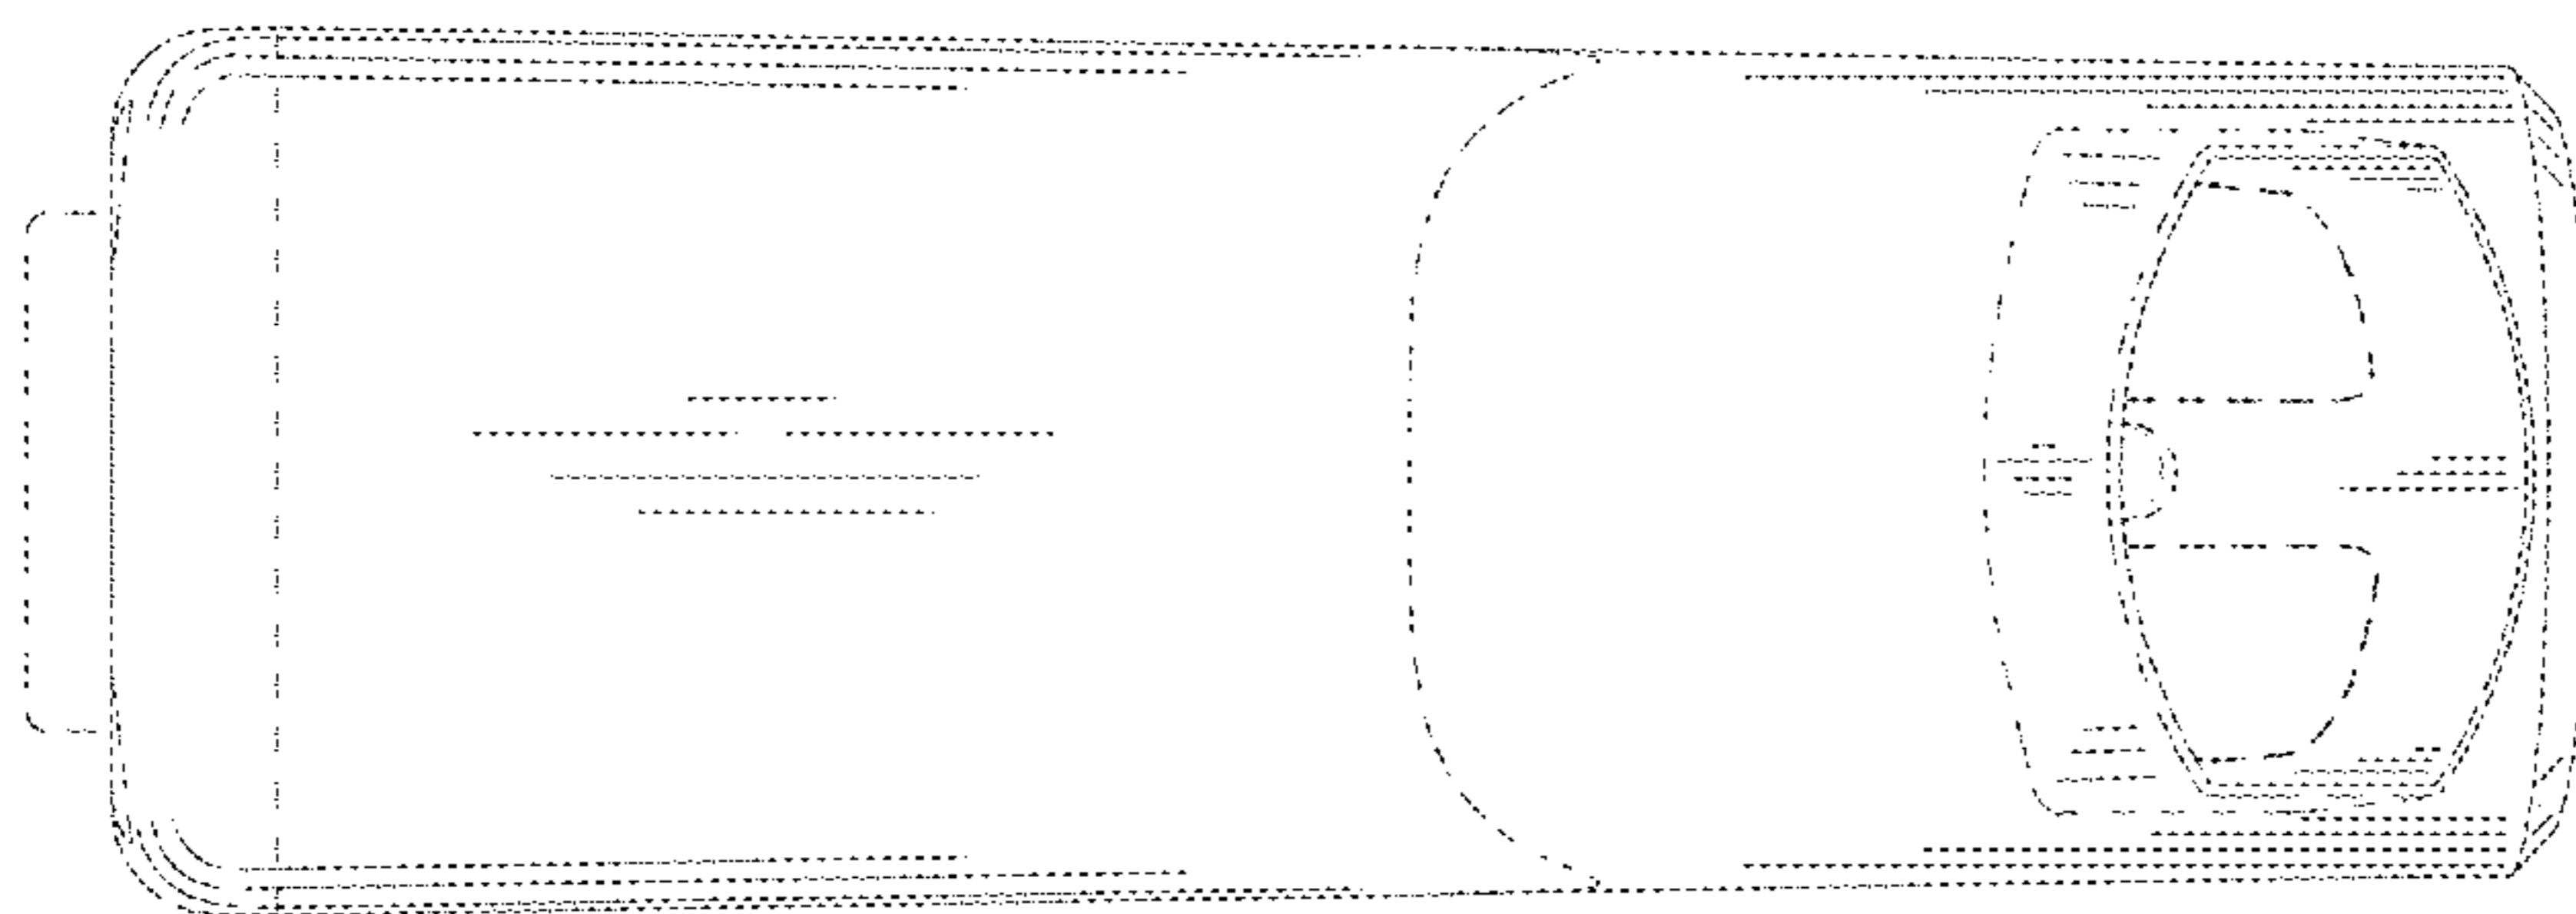

**Fig. 3**