

US00D865172S

(12)

United States Design Patent

Crawford et al.

(10) Patent No.:

US D865,172 S

(45) Date of Patent:

** *Oct. 29, 2019

(54) INSTRUMENT FOR USE WITH A SURGICAL ROBOTIC SYSTEM

(71) Applicant: GLOBUS MEDICAL, INC., Audubon, PA (US)

(72) Inventors: Neil Crawford, Chandler, AZ (US); Jeff Forsyth, Cranston, RI (US); Chris Major, Santa Clara, CA (US); Andrew Berkowitz, Philadelphia, PA (US); Norbert Johnson, North Andover, MA (US)

(73) Assignee: Globus Medical, Inc., Audubon, PA (US)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: 15 Years

(21) Appl. No.: 29/625,714

(22) Filed: Nov. 13, 2017

(51) LOC (12) Cl. 24-02

(52) U.S. Cl. D24/140

(58) Field of Classification Search
USPC D8/300, 307–310; D15/132, 142; D24/140, 108, 112, 128, 133, 137, 138, D24/155, 234
CPC .. A61F 2002/30471; A61F 2002/30565; A61F 2002/4615; A61F 2002/4623; A61F 2002/4627; A61F 2002/4632; A61F 2002/4635; A61F 2002/4668; A61F 2002/687; A61F 2002/4475; A61F 2002/4465; A61F 2250/0006; A61F 2/4611

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

7,547,307	B2 *	6/2009	Carson	A61B 17/154 606/87
7,643,862	B2 *	1/2010	Schoenefeld	A61B 90/36 600/407
9,161,799	B2 *	10/2015	Benson	A61B 17/1655
D761,428	S *	7/2016	Birkenbach	D24/140
D806,247	S *	12/2017	Kheradpir	D24/147
D816,838	S *	5/2018	Kheradpir	D24/140
D820,984	S *	6/2018	Kheradpir	D24/140
D828,561	S *	9/2018	Kheradpir	D24/147
2003/0069591	A1 *	4/2003	Carson	A61B 17/154 606/130

(Continued)

OTHER PUBLICATIONS

Globus Medical Excelsius Precruiting, Jan. 5, 2017, [online], [site visited Jan. 11, 2019]. Retrieved from url:https://www.youtube.com/watch?v=TDX6kbOFImM (Year: 2017).*

(Continued)

Primary Examiner — Jeffrey D Asch
Assistant Examiner — Tracey J Bell



(57) CLAIM

The ornamental design for an instrument for use with a surgical robotic system, as shown and described.

DESCRIPTION

FIG. 1 shows a perspective view of an instrument for use with a surgical robotic system showing our new design; FIG. 2 shows a front view thereof; FIG. 3 shows a rear view thereof; FIG. 4 shows a side view thereof; FIG. 5 shows another side view thereof; FIG. 6 shows a top view thereof; and, FIG. 7 shows a bottom view thereof.

(Continued)

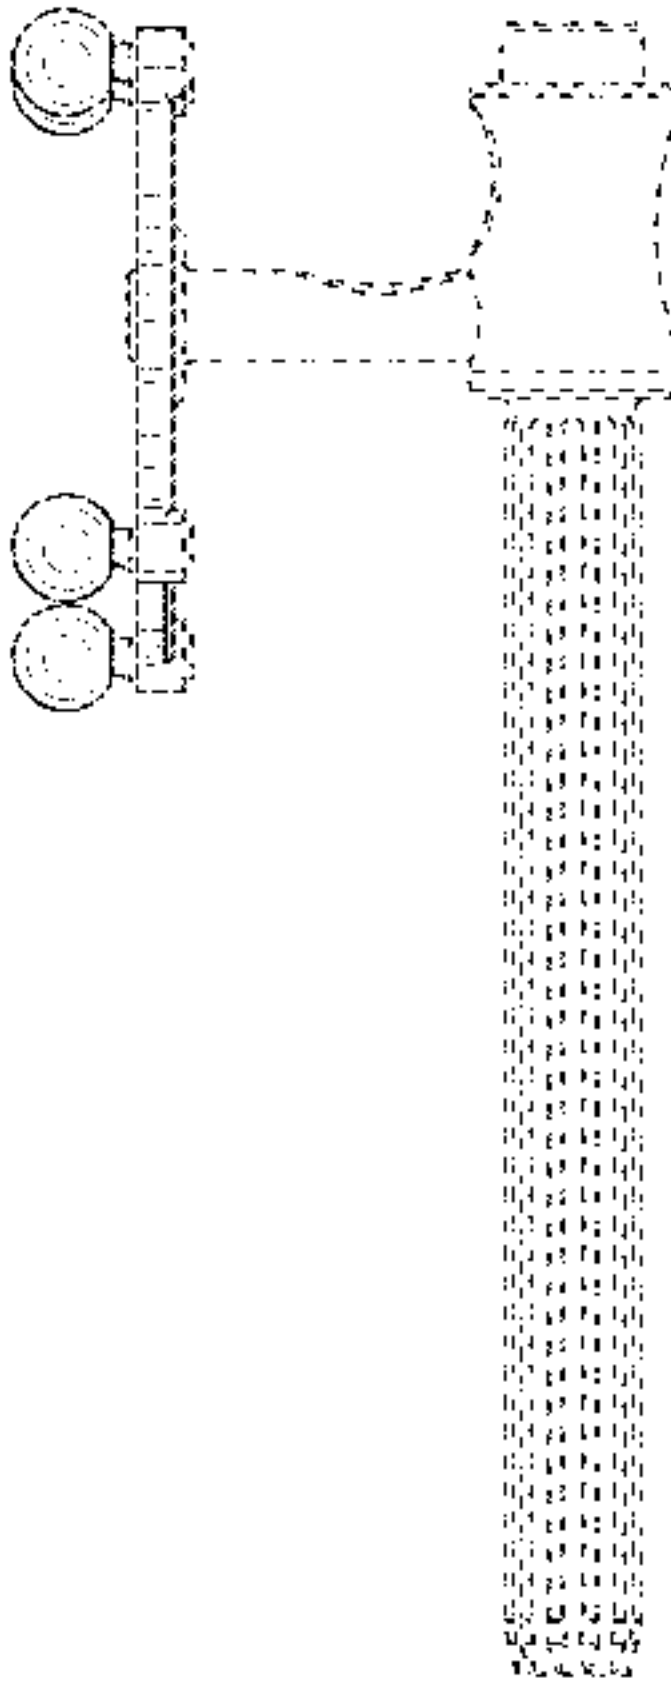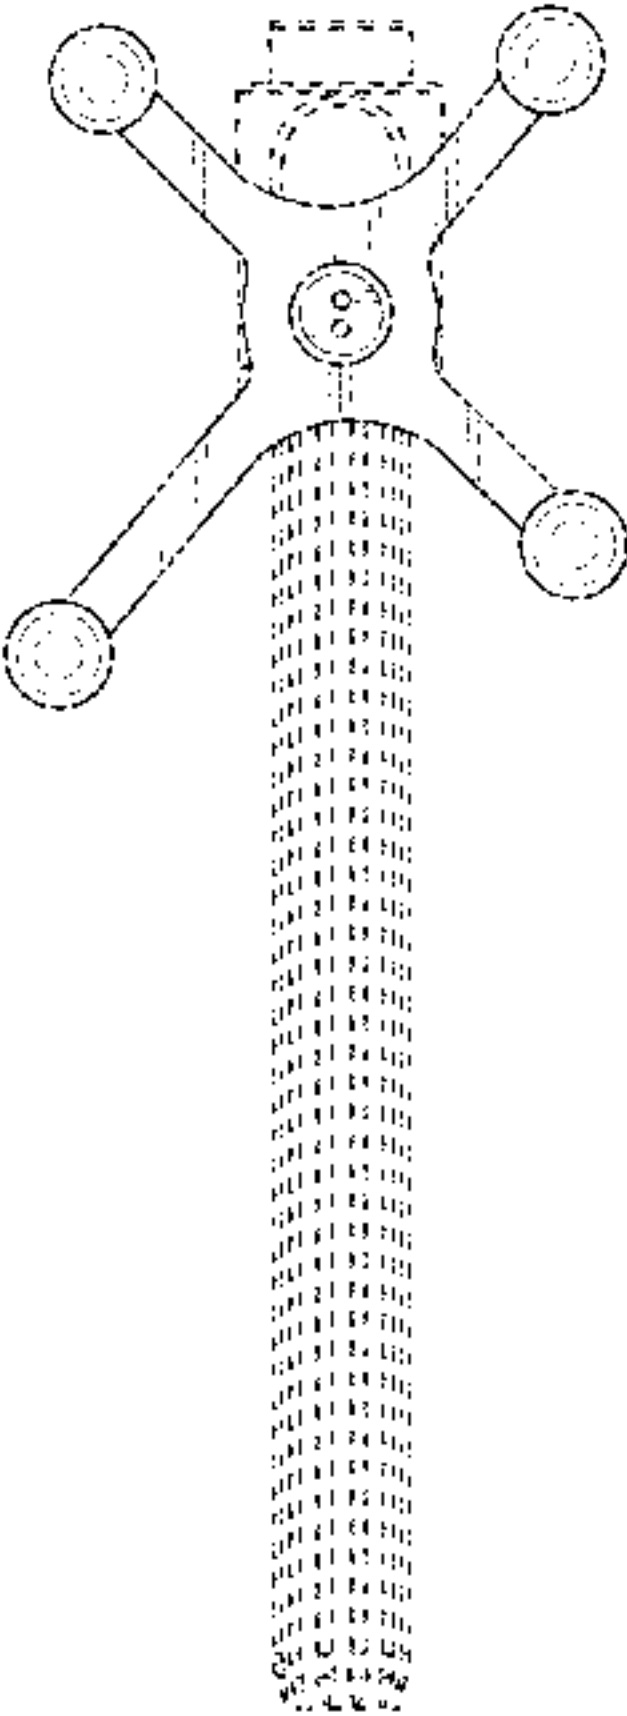

In the above drawings the broken lines and the areas within the broken lines form no part of the claimed design.

1 Claim, 7 Drawing Sheets

(56) References Cited

U.S. PATENT DOCUMENTS

2004/0167393 A1* 8/2004 Solar A61B 90/39
600/414
2005/0113846 A1* 5/2005 Carson A61F 2/461
606/130
2005/0124988 A1* 6/2005 Terrill-Grisoni
A61B 17/3403
606/53
2005/0137599 A1* 6/2005 Masini A61B 90/36
606/79
2006/0142657 A1* 6/2006 Quaid G06F 19/00
600/424
2015/0100129 A1* 4/2015 Waugh A61F 2/4455
623/17.16

2016/0081681 A1* 3/2016 Waugh A61B 17/0206
606/86 A
2017/0071691 A1* 3/2017 Crawford A61B 90/96
2017/0119339 A1* 5/2017 Johnson A61B 6/58
2017/0172669 A1* 6/2017 Berkowitz A61B 34/20
2017/0209286 A1* 7/2017 Palmatier A61F 2/4611
2017/0252114 A1* 9/2017 Crawford A61B 17/17
2017/0360521 A1* 12/2017 Johnson A61B 34/74
2018/0085233 A1* 3/2018 Palmatier A61F 2/80
2018/0311051 A1* 11/2018 Donaldson A61F 2/4611
2019/0000571 A1* 1/2019 Johnson A61B 34/30

OTHER PUBLICATIONS

Medtronic revises indications for use of Navlock trackers following patient deaths, May 8, 2017, [online], [site visited Jan. 11, 2019]. Retrieved from url:<https://spinalnewsinternational.com/medtronic-revises-indications-for-use-of-navlock-trackers-following-patient-deaths/> (Year: 2017).*

A Hands-on-Robot for Accurate Placement of Pedicle Screws, Ortmaier, Tobias, May 2006, [online], [site visited Jan. 11, 2019]. Retrieved from url:https://www.researchgate.net/publication/224998353_A_Hands-on-Robot_for_Accurate_Placement_of_Pedicle_Screws (Year: 2006).*

* cited by examiner

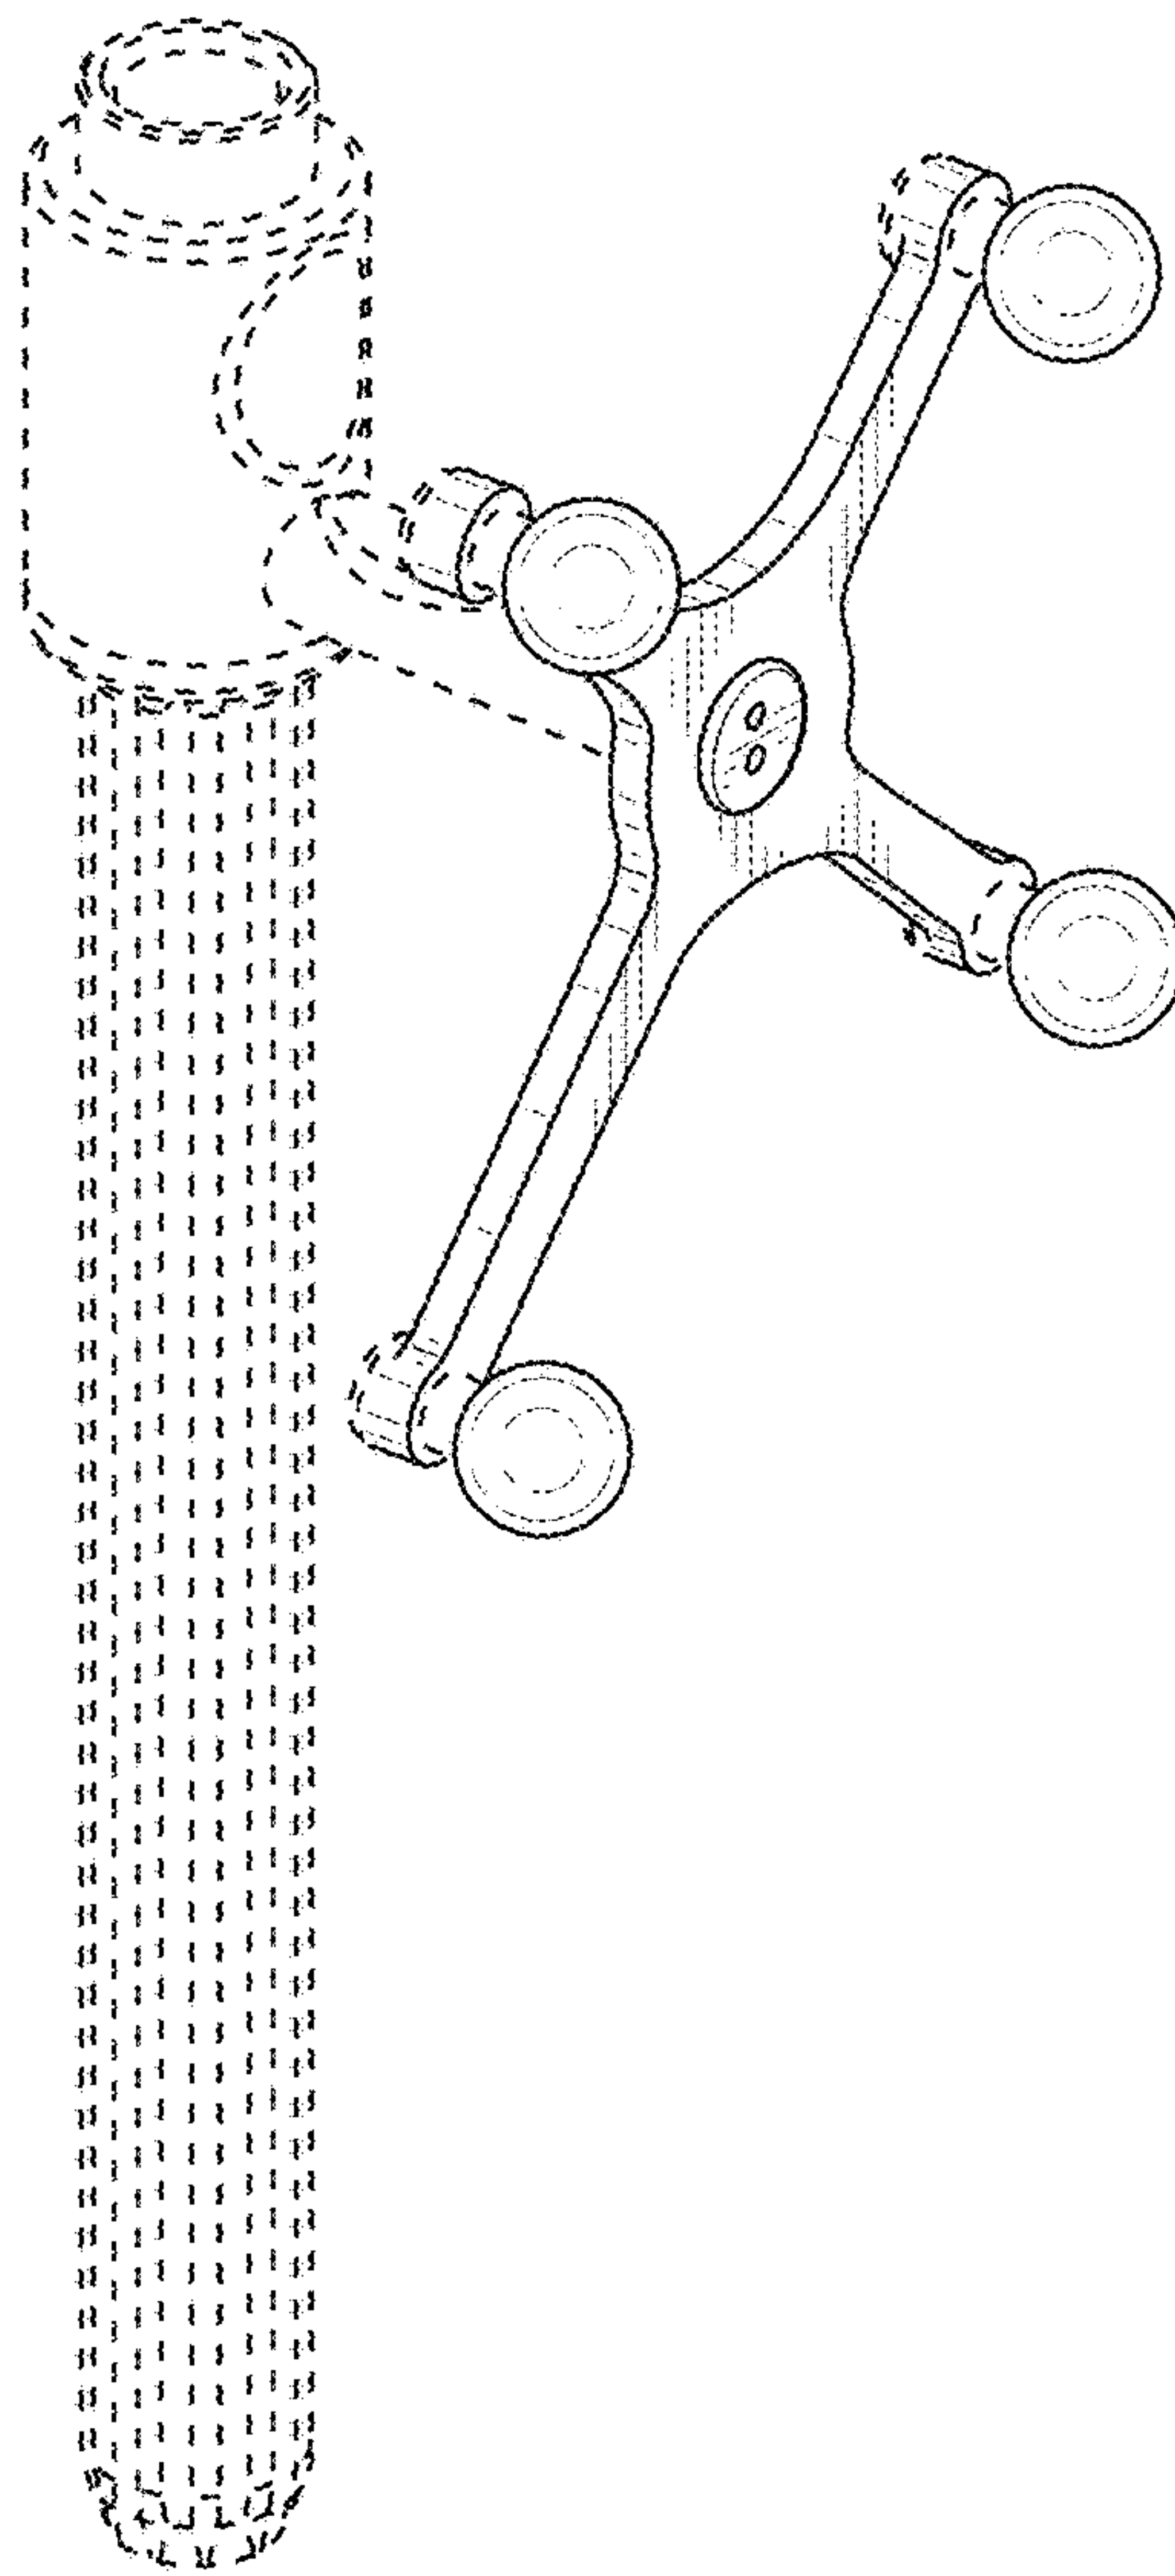


FIG. 1

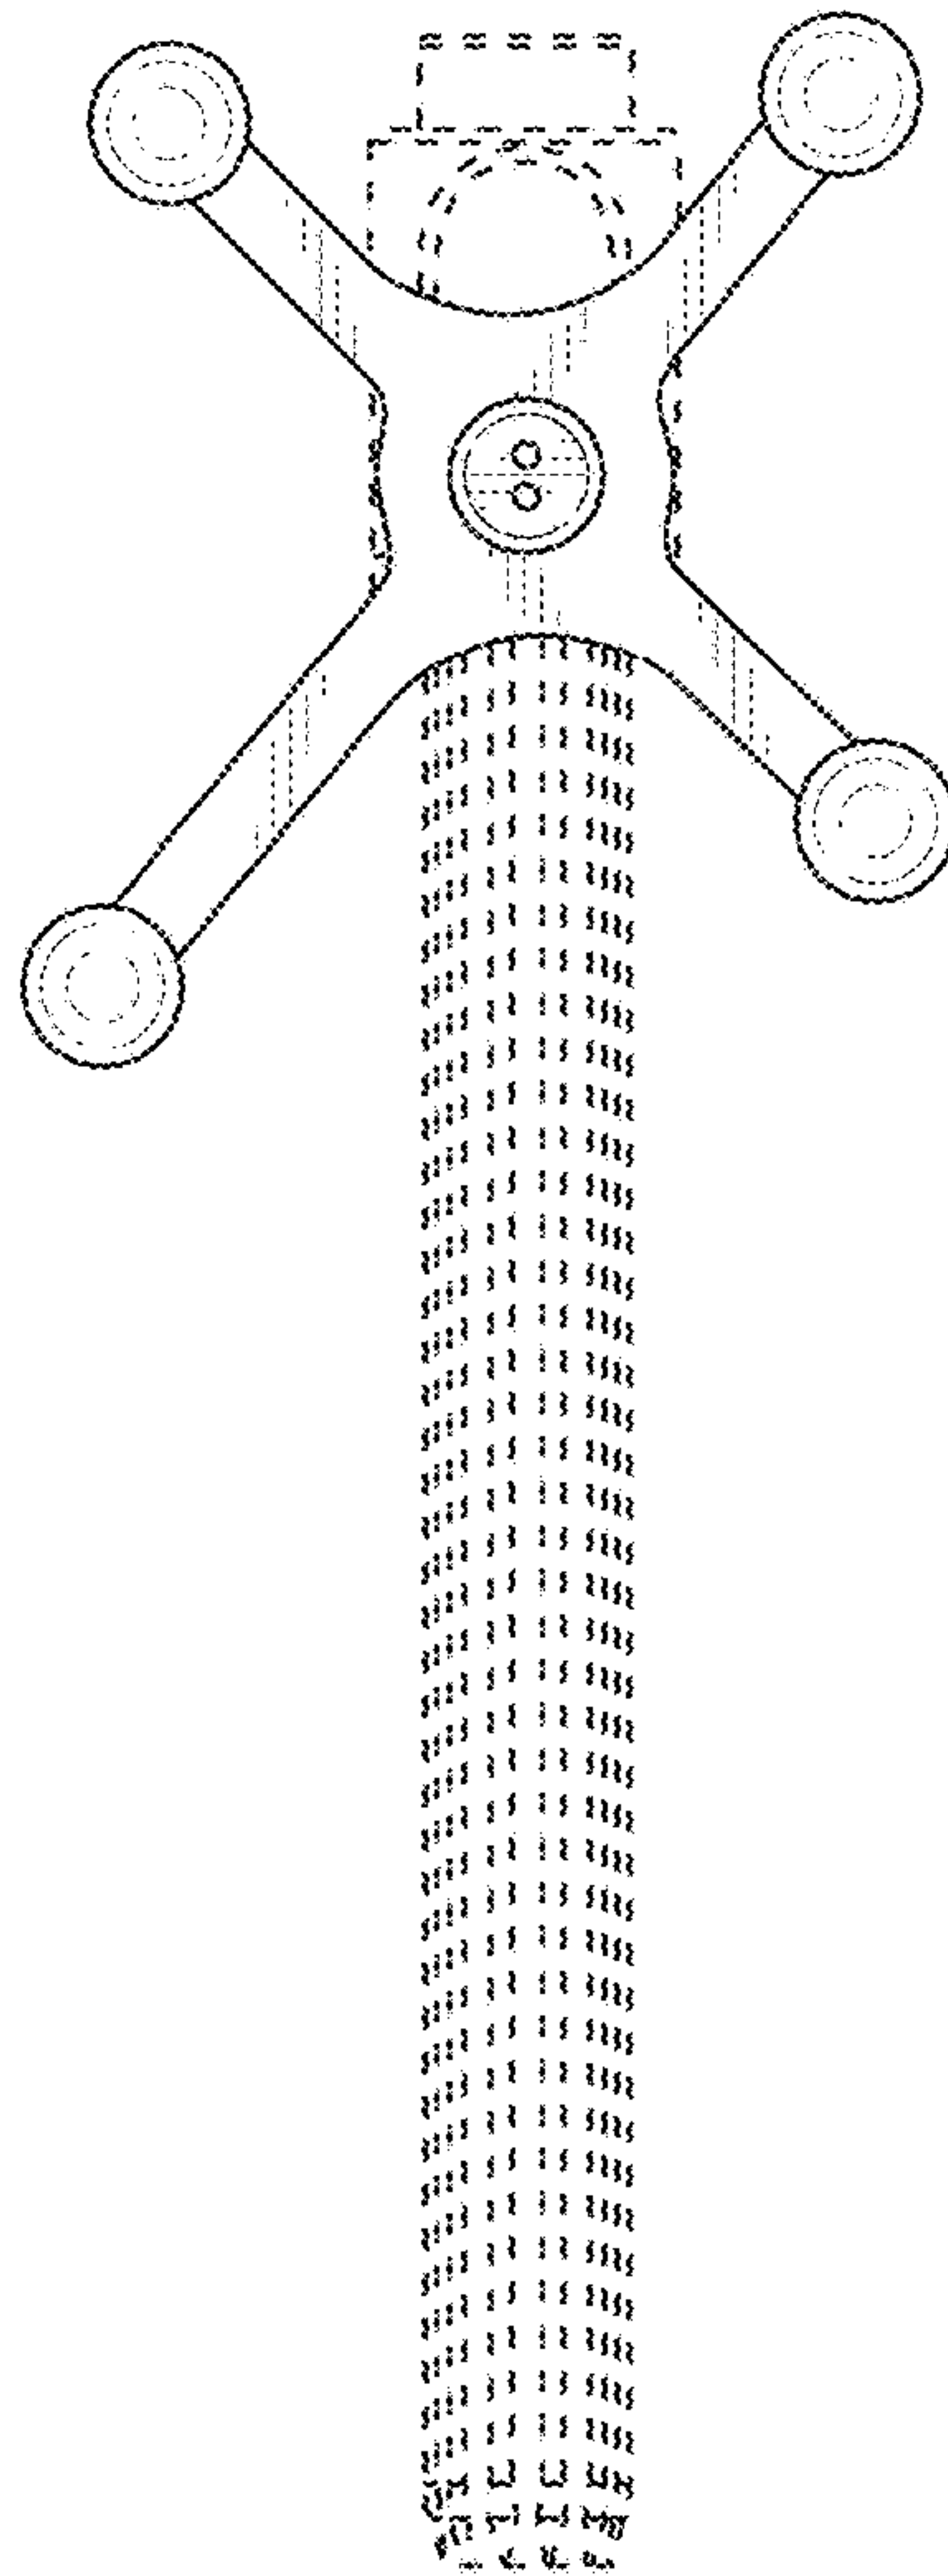


FIG. 2

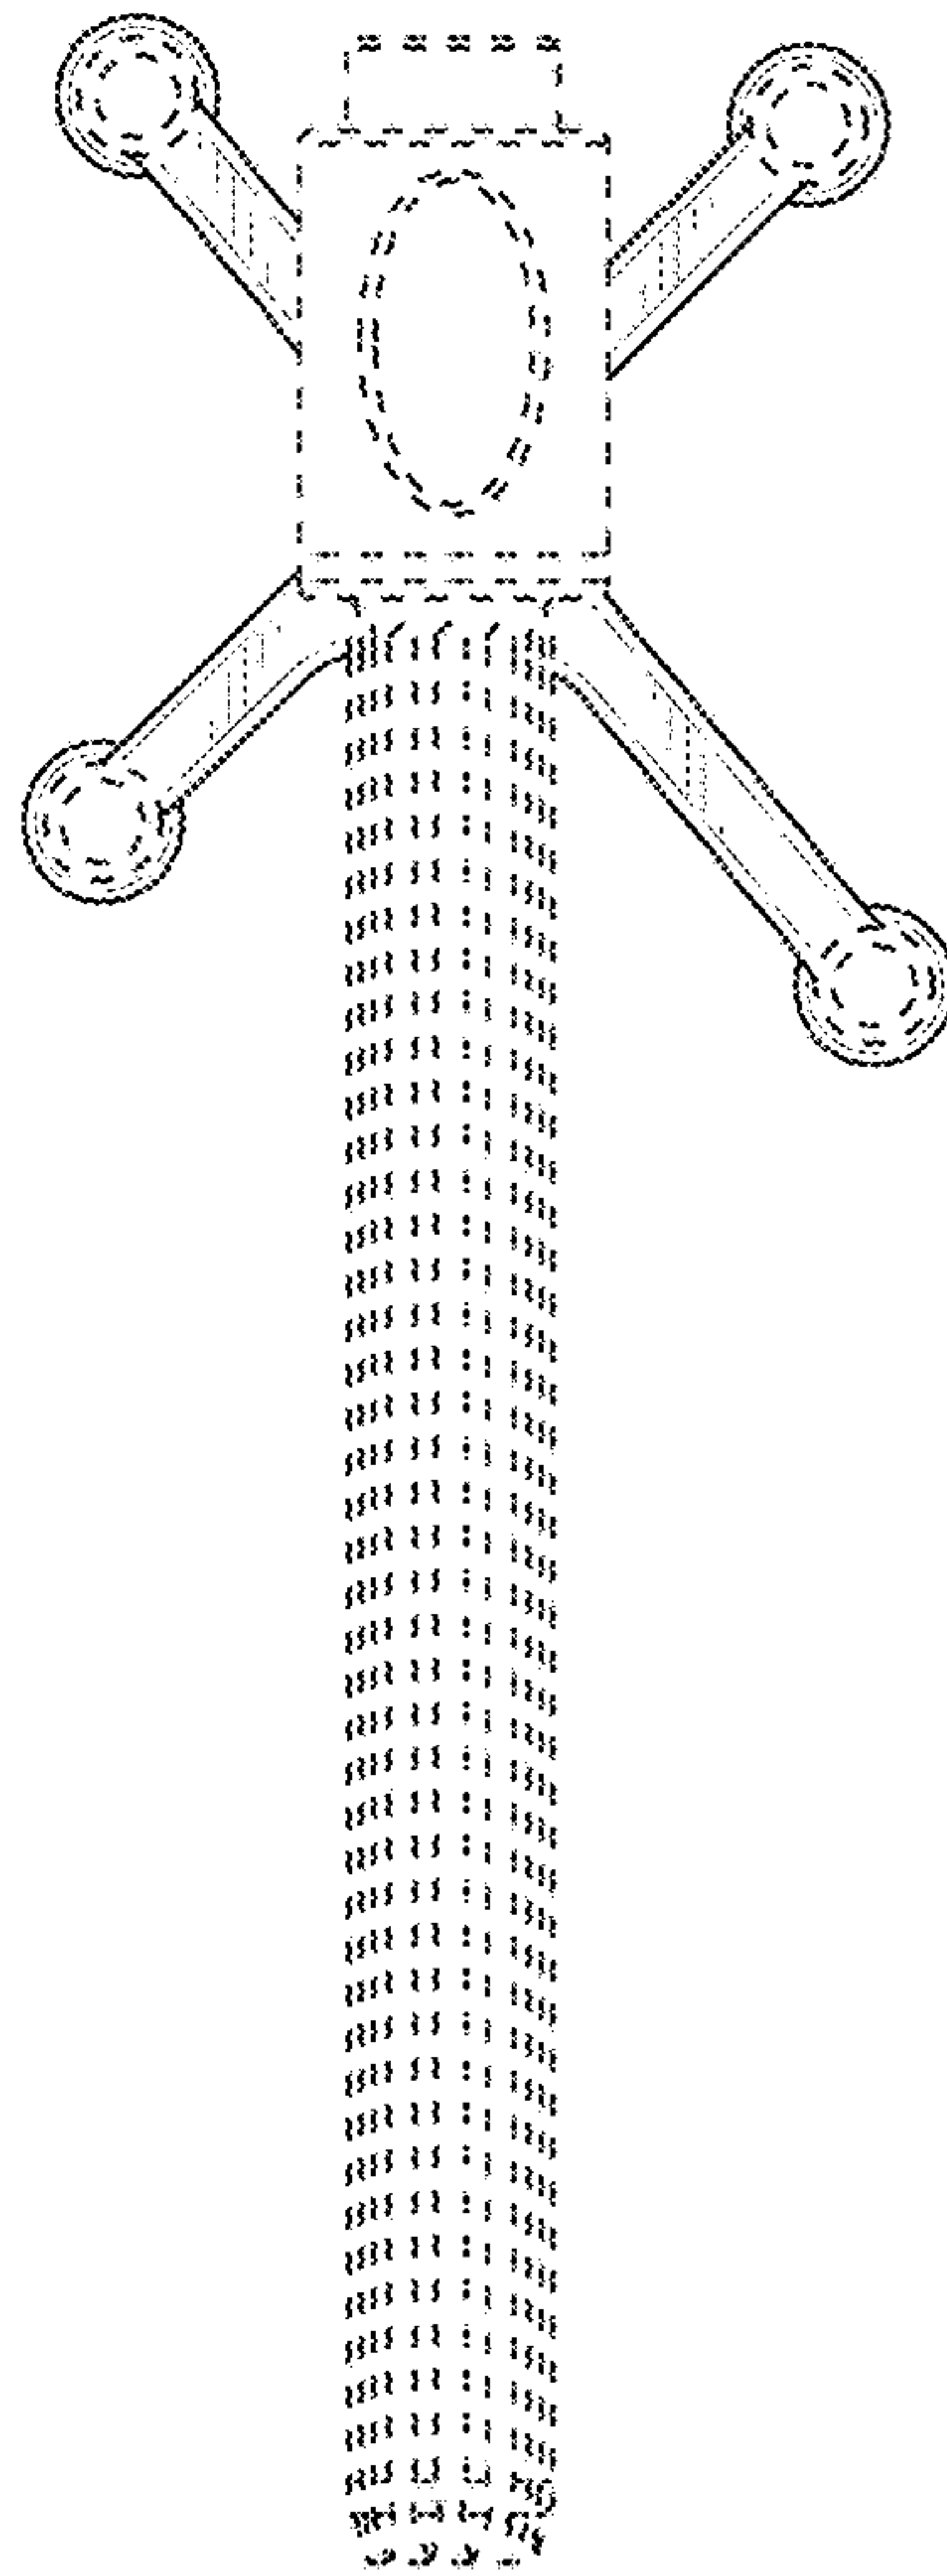


FIG. 3

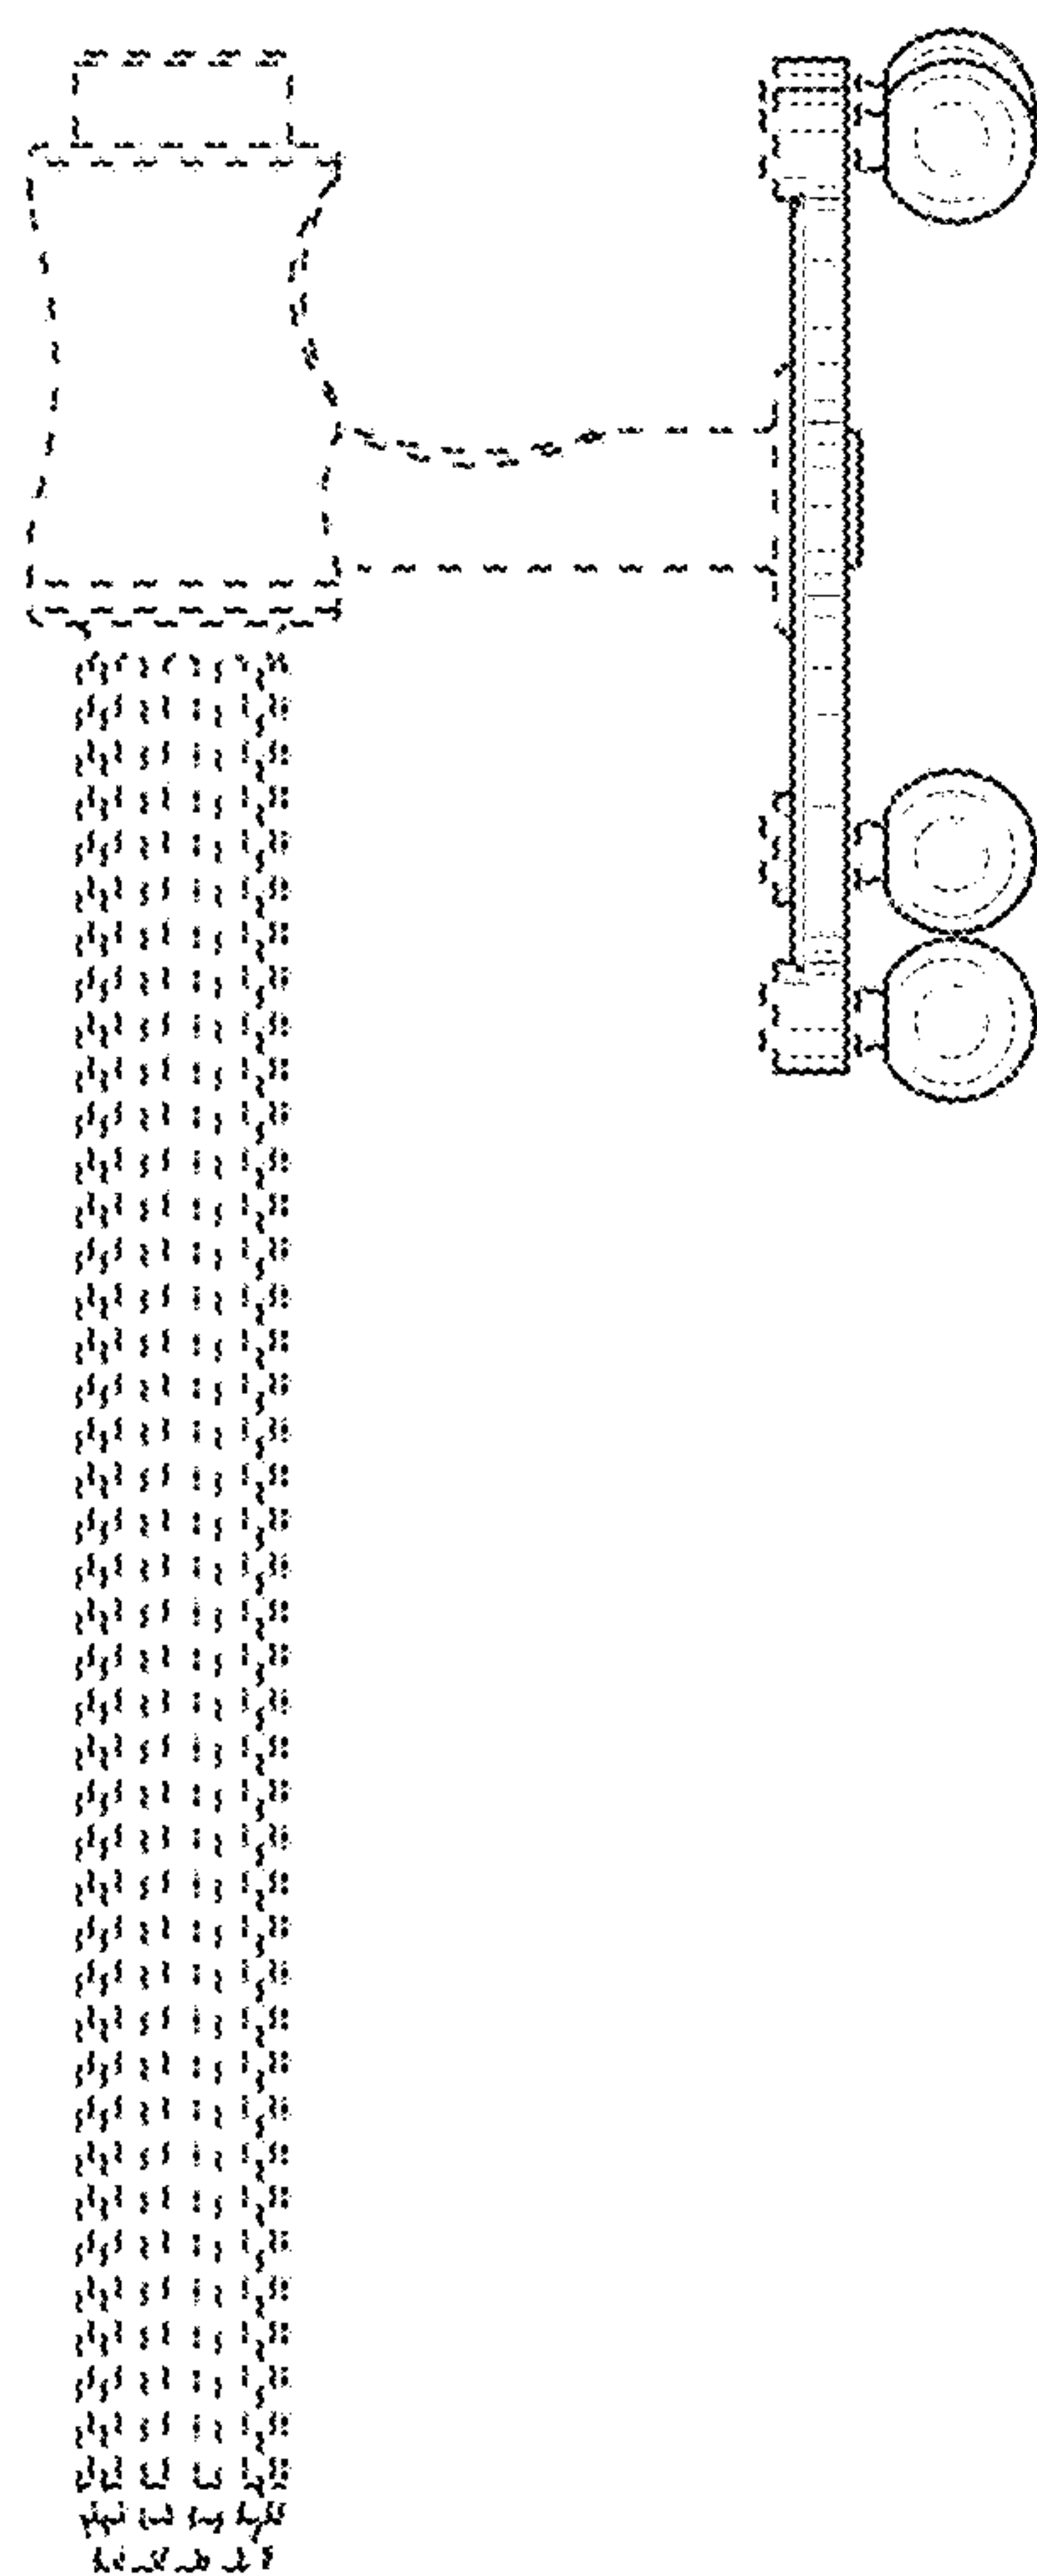


FIG. 4

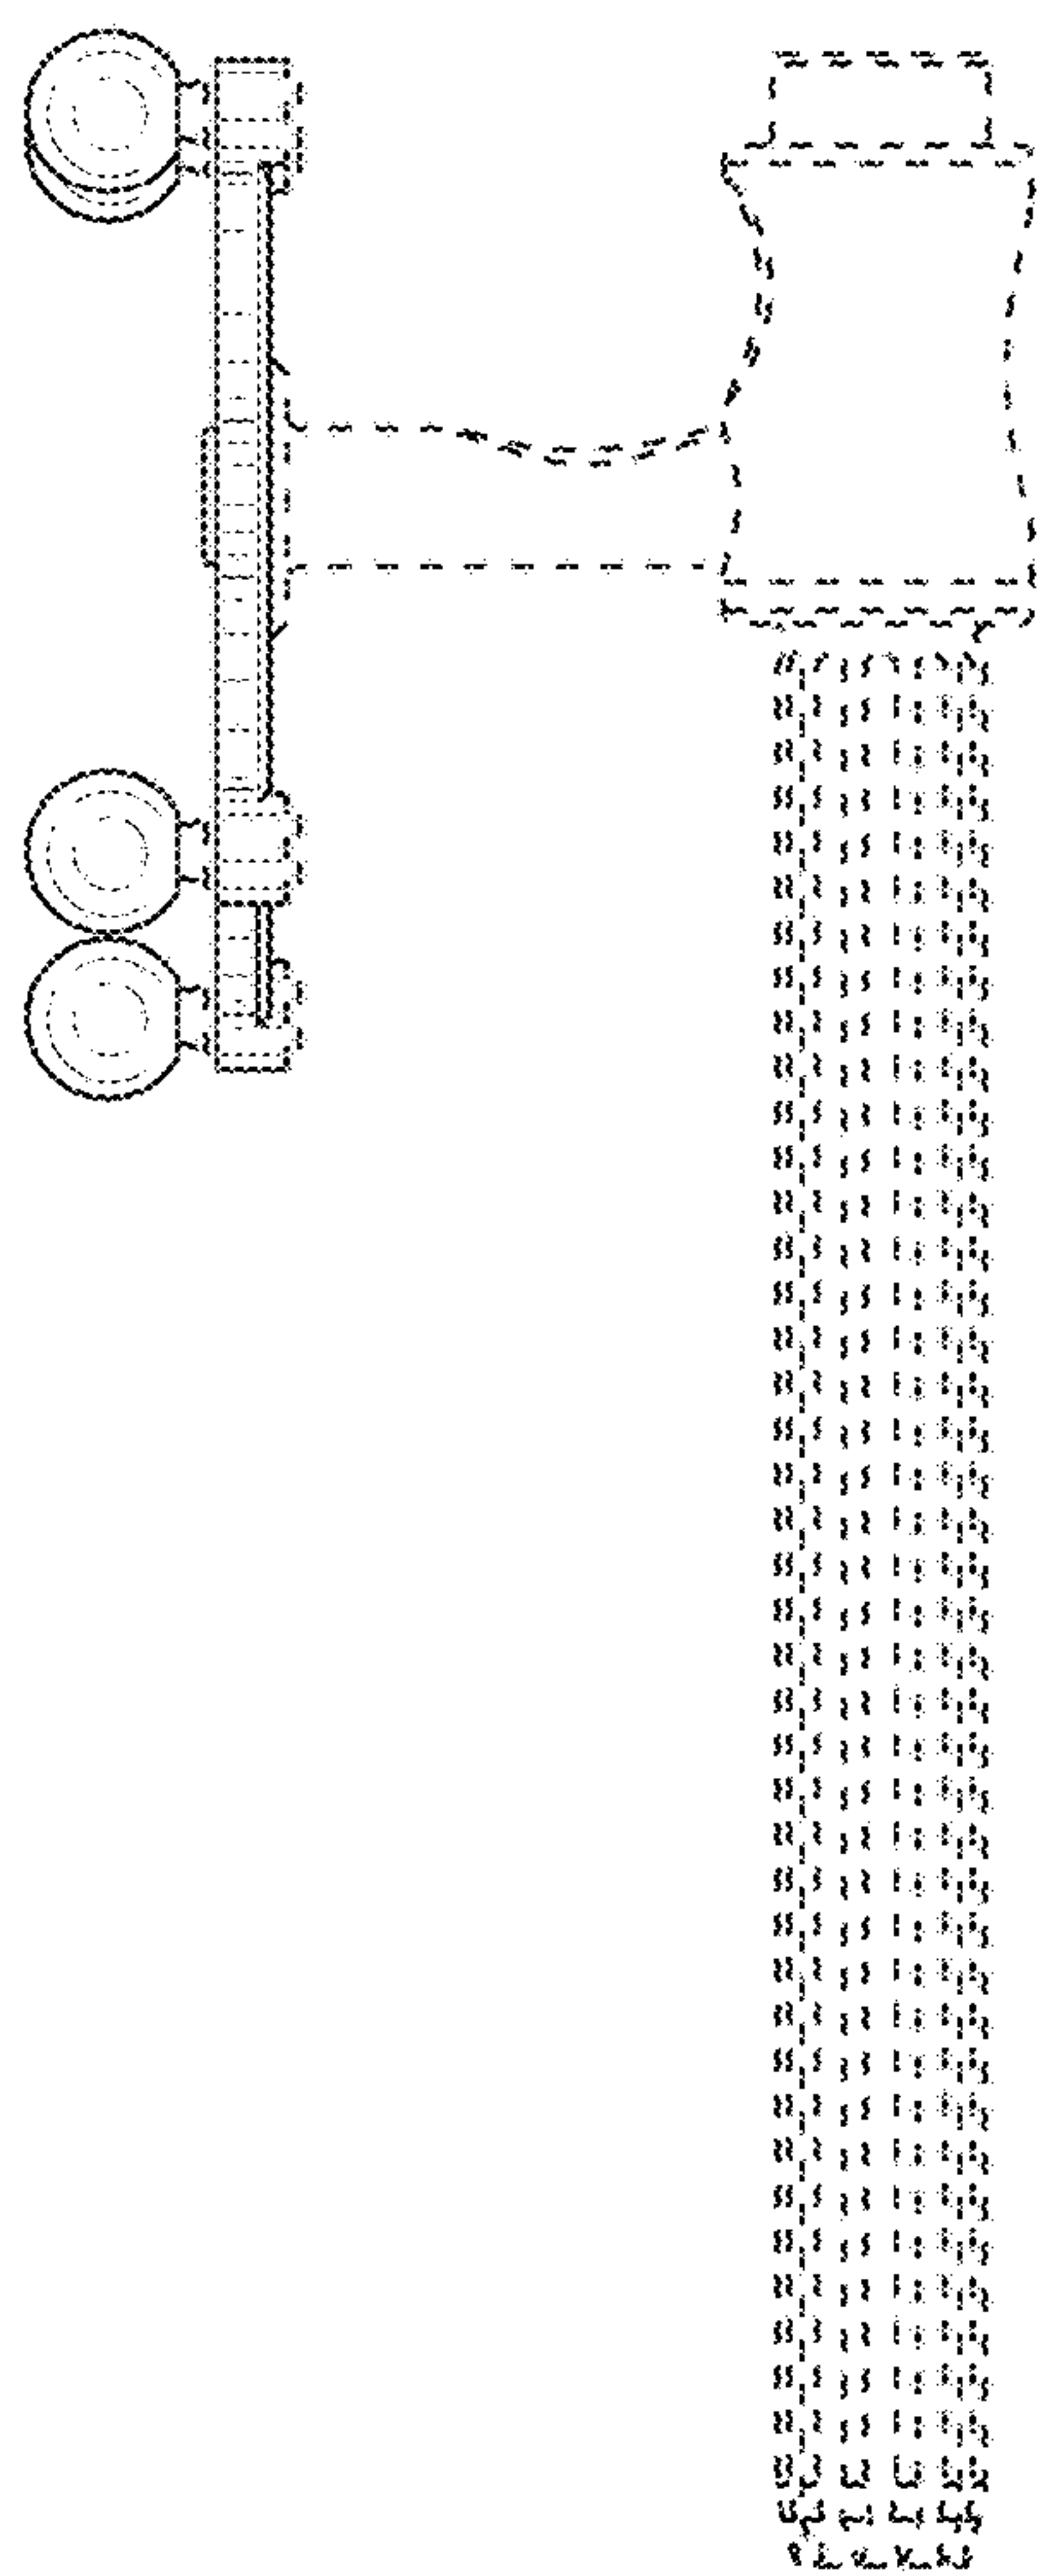


FIG. 5

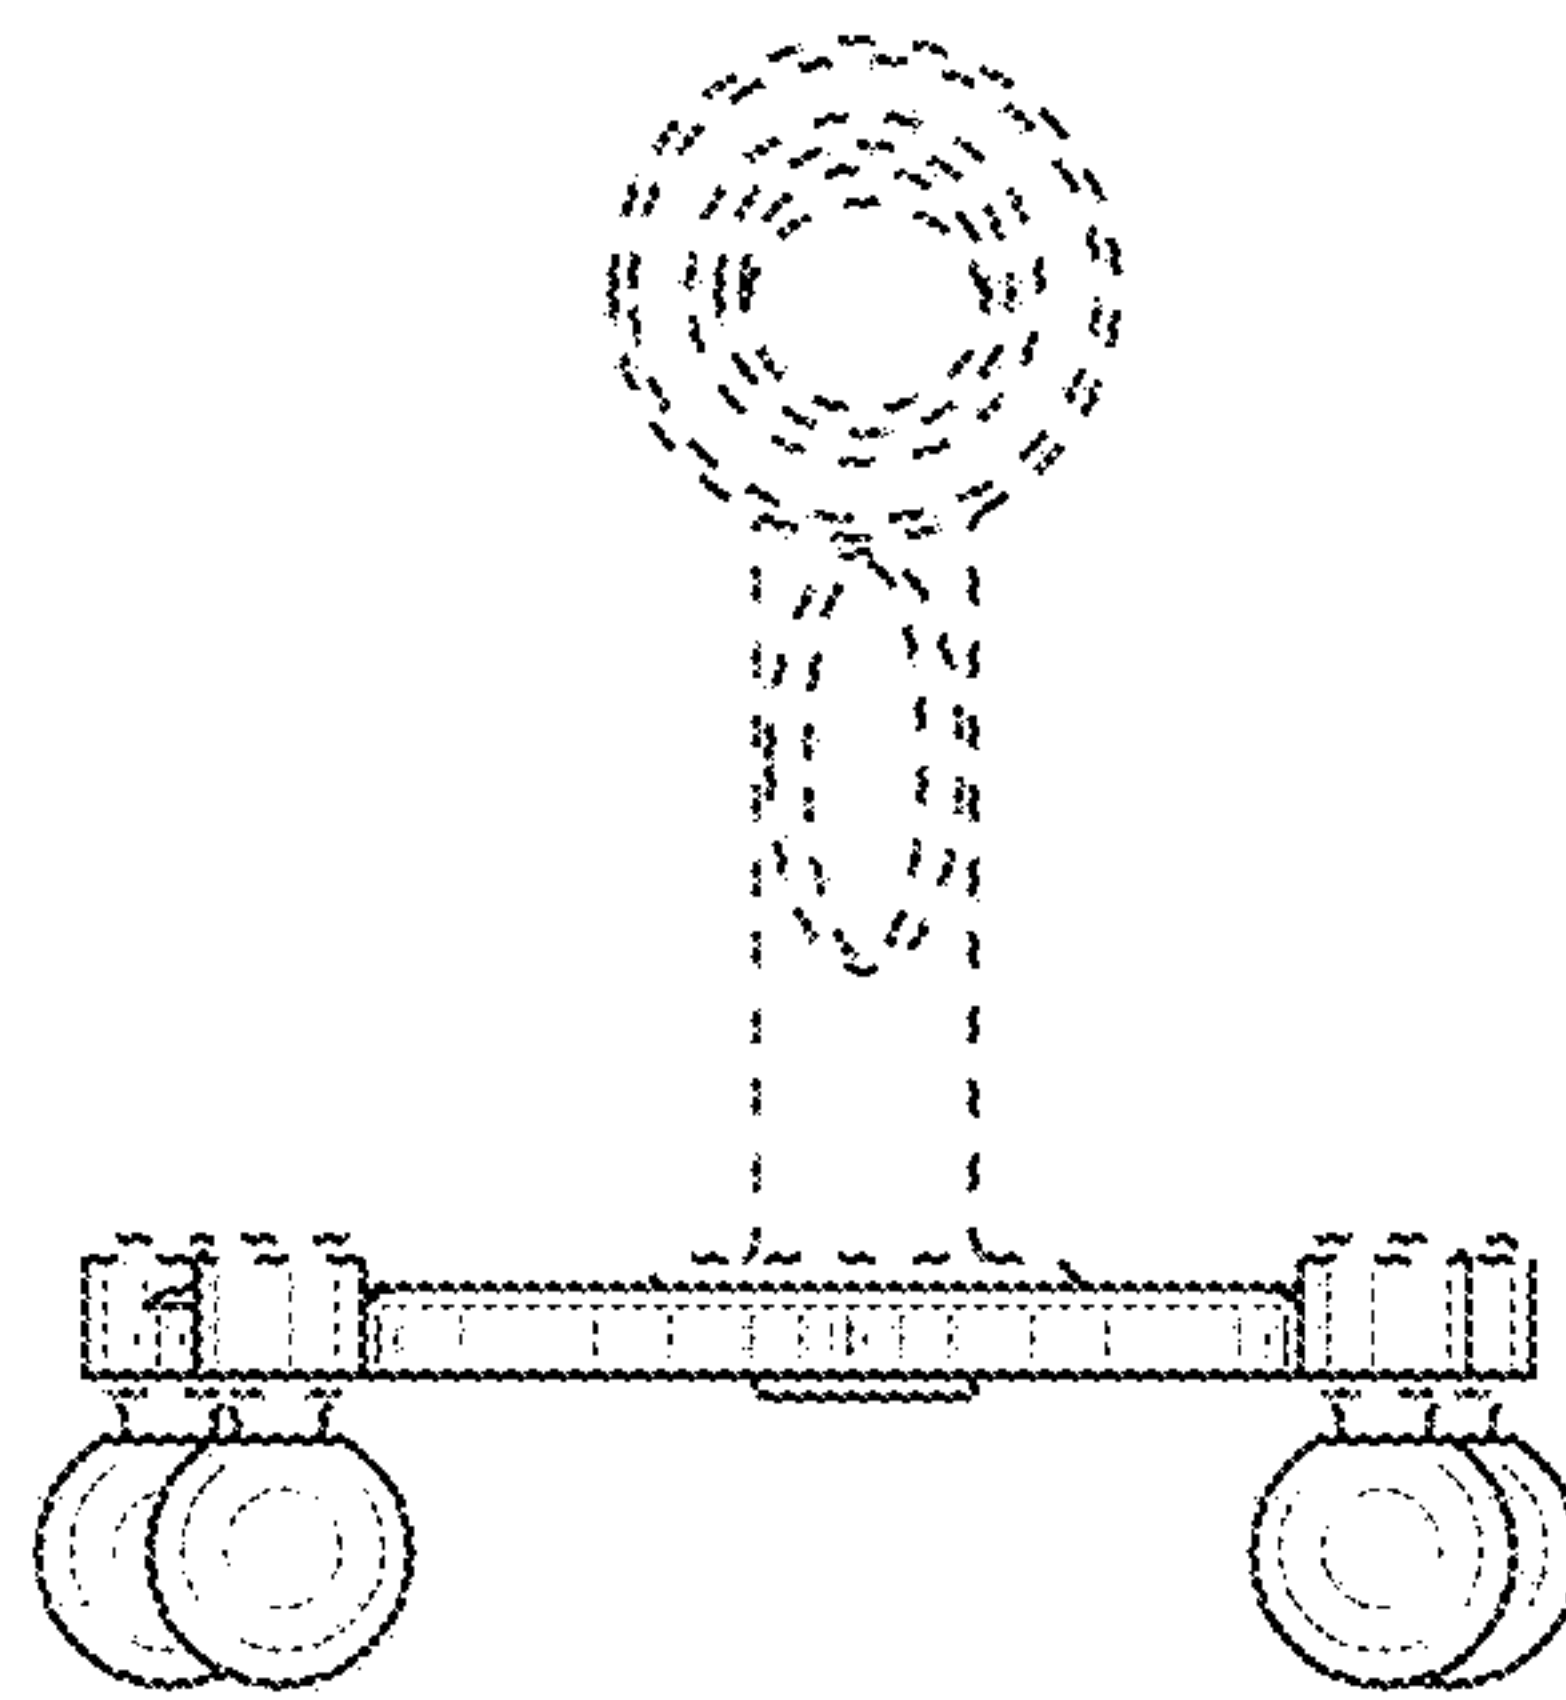


FIG. 6

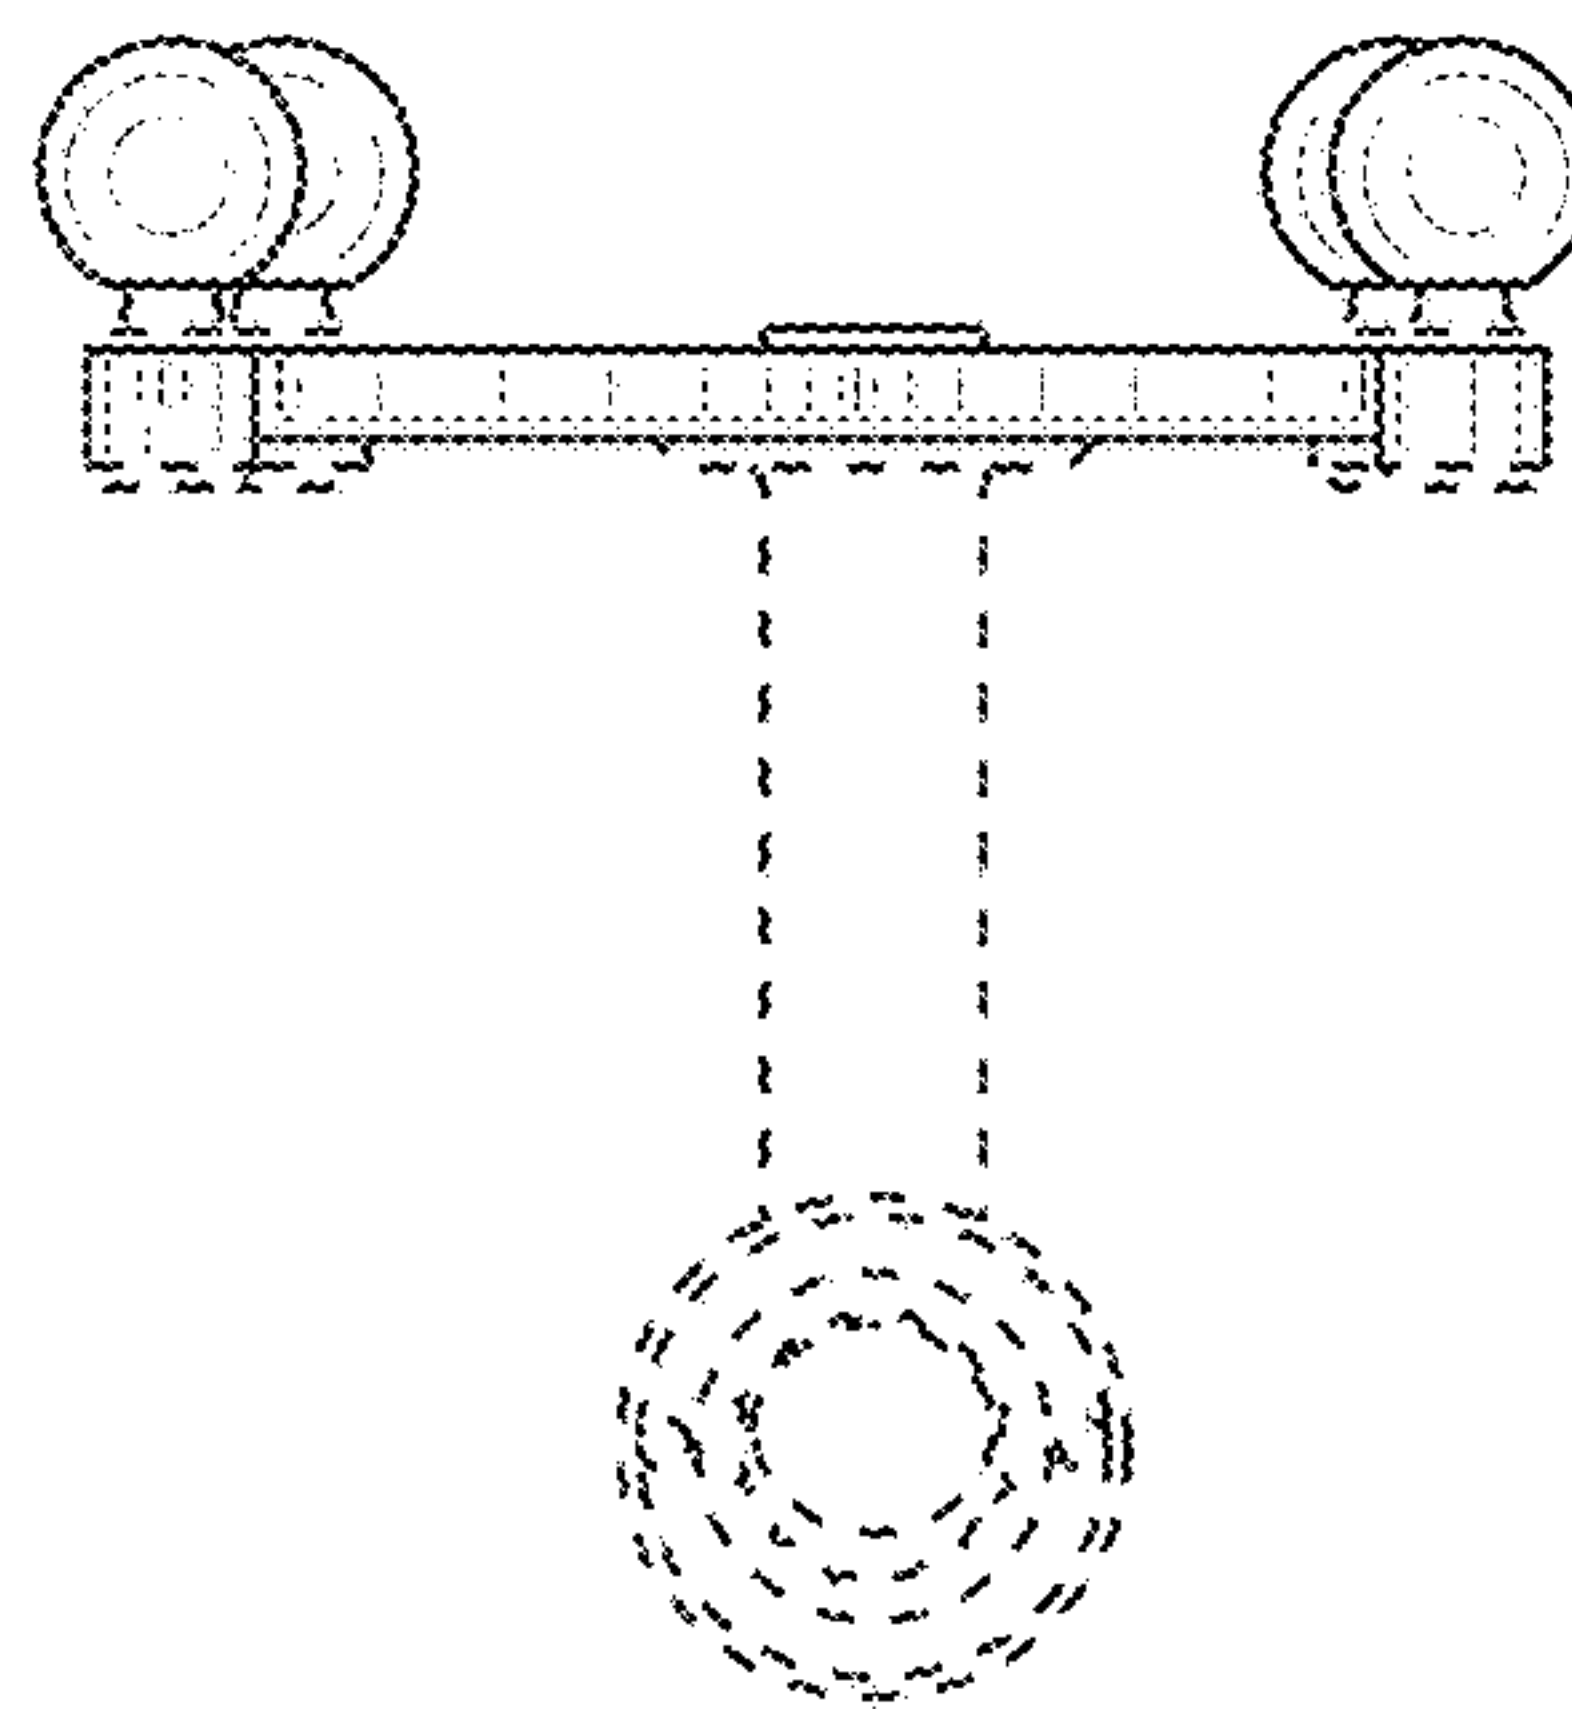


FIG. 7