



US00D865196S

(12) **United States Design Patent** (10) **Patent No.:** **US D865,196 S**  
**Godfrey** (45) **Date of Patent:** **\*\* \*Oct. 29, 2019**

(54) **TEMPERATURE THERAPY DEVICE**  
(71) Applicant: **Daniel H. Godfrey**, Portland, OR (US)  
(72) Inventor: **Daniel H. Godfrey**, Portland, OR (US)  
(\* ) Notice: This patent is subject to a terminal disclaimer.

8,357,189 B2 \* 1/2013 Ugajin ..... A61F 7/034  
607/108  
D683,040 S \* 5/2013 Arsenault ..... D24/206  
D690,022 S \* 9/2013 Sonoda ..... D24/206  
D702,847 S \* 4/2014 Arsenault ..... D24/206  
9,671,133 B2 \* 6/2017 Sonoda ..... A61F 7/034  
2010/0161014 A1 \* 6/2010 Lynch ..... A61F 7/02  
607/108

(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/601,069**  
(22) Filed: **Apr. 18, 2017**  
(51) **LOC (12) Cl.** ..... **24-04**  
(52) **U.S. Cl.**  
USPC ..... **D24/206**  
(58) **Field of Classification Search**  
USPC ..... D24/206-207, 200, 189; D6/582-583,  
D6/596, 601; 602/7, 41, 48, 54, 56;  
607/102, 108, 114, 96  
CPC ..... A61F 7/00; A61F 7/02; A61F 7/03; A61F  
7/034; A61F 7/106; A61F 2007/0001;  
A61F 2007/0056; A61F 2007/0063; A61F  
2007/026  
See application file for complete search history.

**OTHER PUBLICATIONS**

TempTraq 48-Hour Intelligent Baby Fever Monitor with Wireless Alerts (iOS & Android). Dated Dec. 22, 2017. Retrieved Jul. 10, 2019. Retrieved from Internet: <https://www.amazon.com/TempTraq-48-Hour-Intelligent-Monitor-Wireless/dp/B06XWG6F98>.\*

\* cited by examiner

*Primary Examiner* — Wan Laymon  
(74) *Attorney, Agent, or Firm* — Mohr Intellectual Property Law Solutions, PC


(56) **References Cited**  
**U.S. PATENT DOCUMENTS**  
4,095,583 A \* 6/1978 Petersen ..... A61F 7/03  
126/263.07  
5,720,391 A \* 2/1998 Dohm ..... A61F 2/0095  
206/363  
D490,103 S \* 5/2004 Rangel ..... D19/10  
D511,355 S \* 11/2005 Hunter, Jr. .... D19/10  
7,652,228 B2 \* 1/2010 Igaki ..... A61F 7/034  
219/401  
D669,994 S \* 10/2012 Bembridge ..... D24/200

(57) **CLAIM**  
The ornamental design for a temperature therapy device, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, front, isometric view of the temperature therapy device;  
FIG. 2 is a front plan view thereof; the back view being a mirror image thereof;  
FIG. 3 is a top plan view thereof;  
FIG. 4 is a bottom plan view thereof; and,  
FIG. 5 is a side plan view thereof.

**1 Claim, 2 Drawing Sheets**

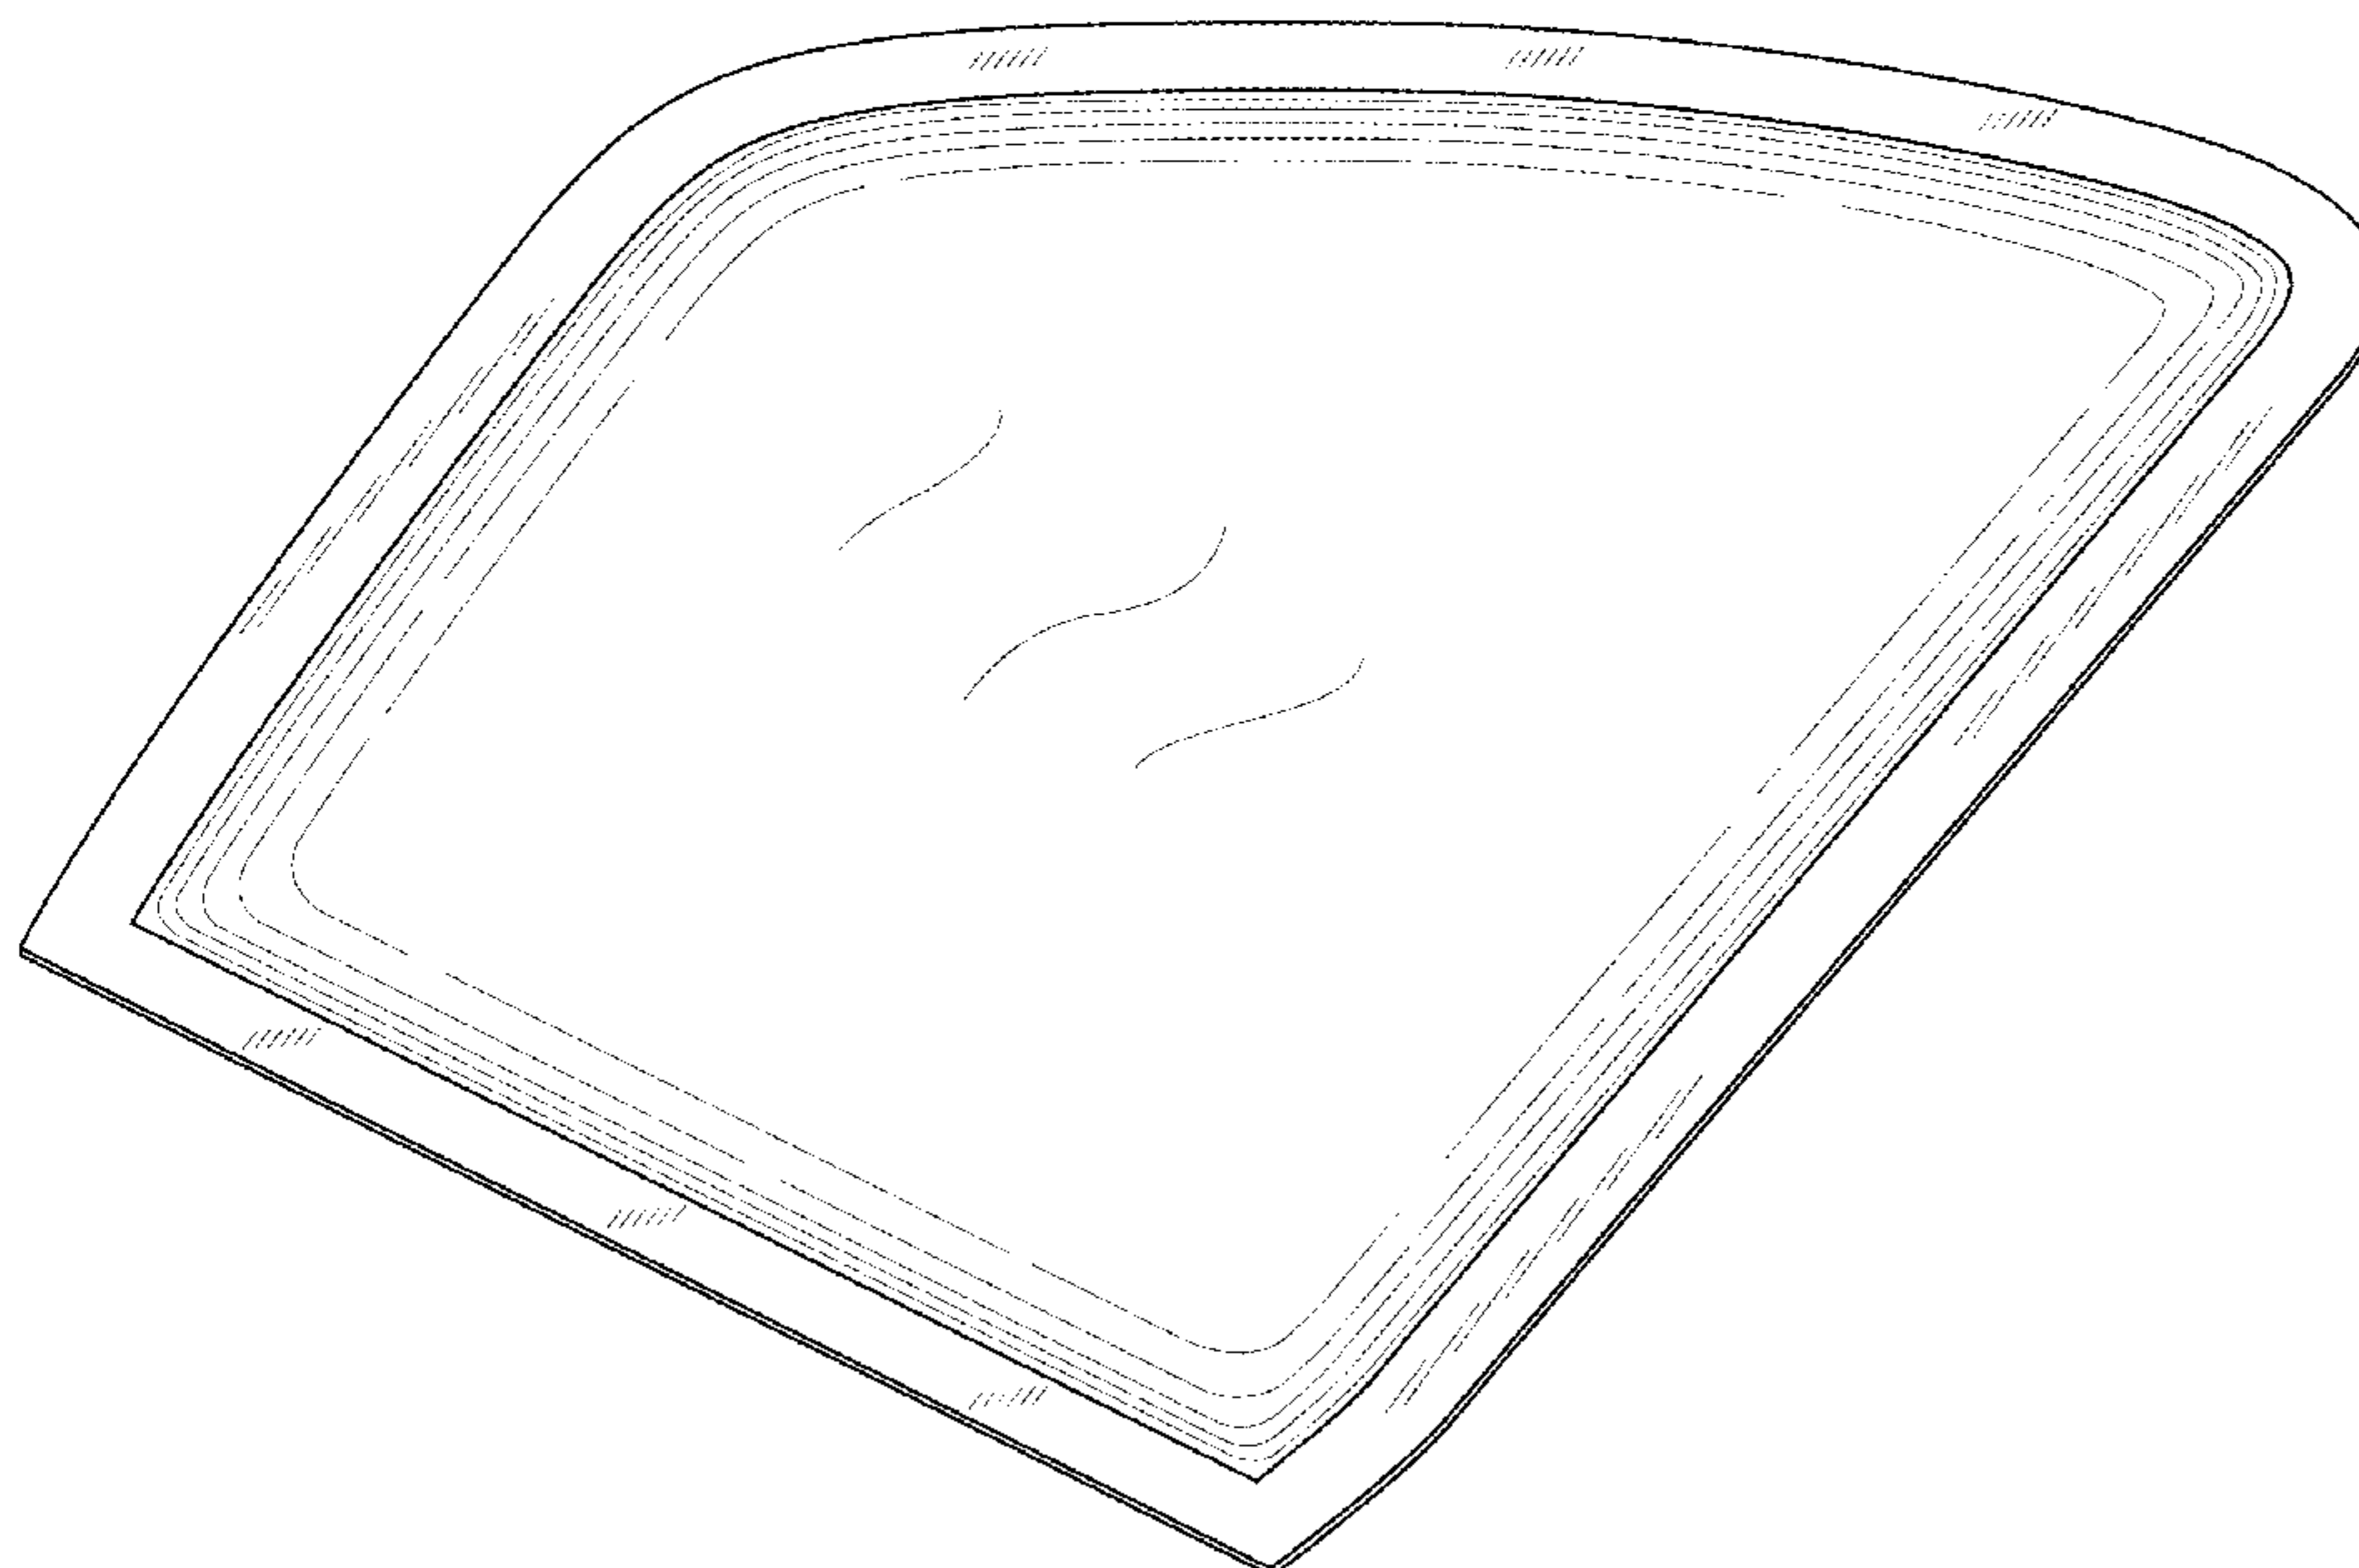

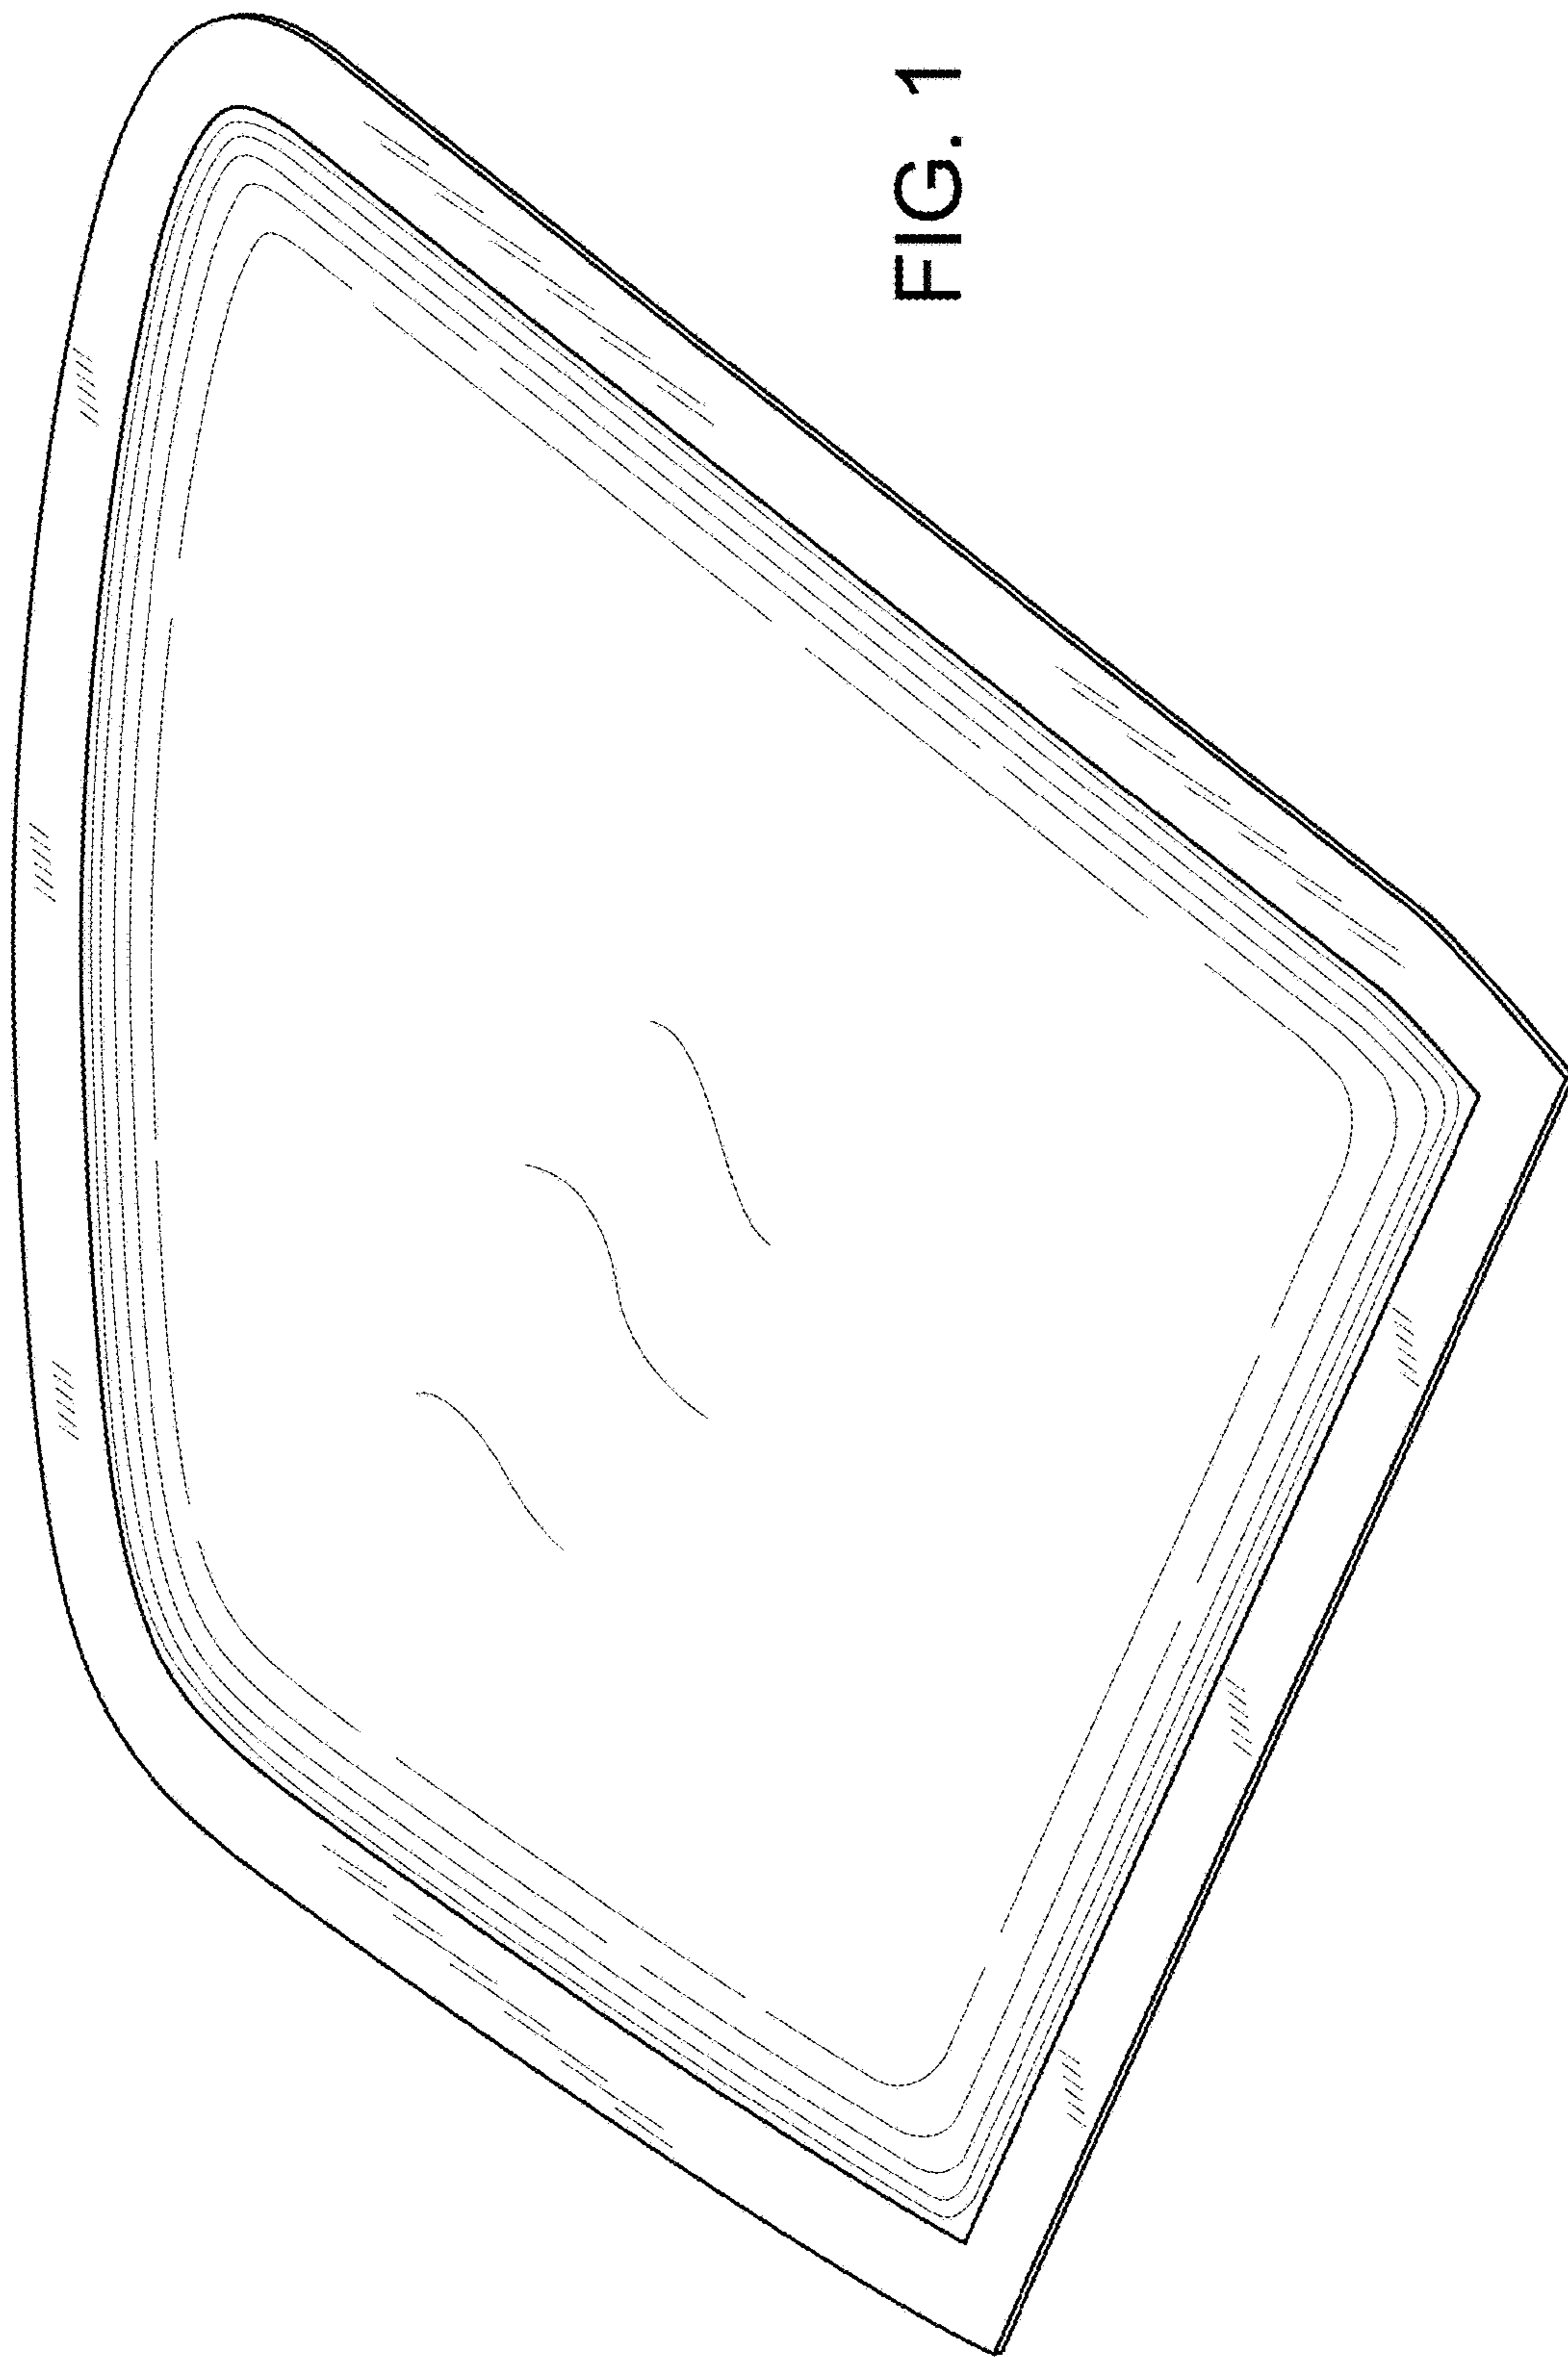


FIG. 1

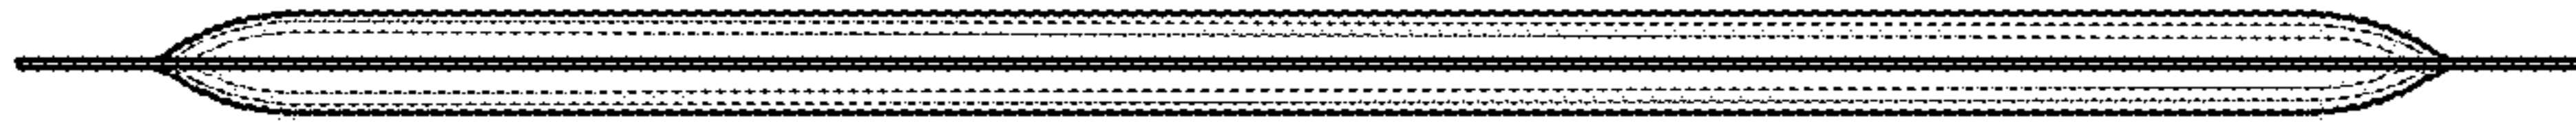


FIG. 3

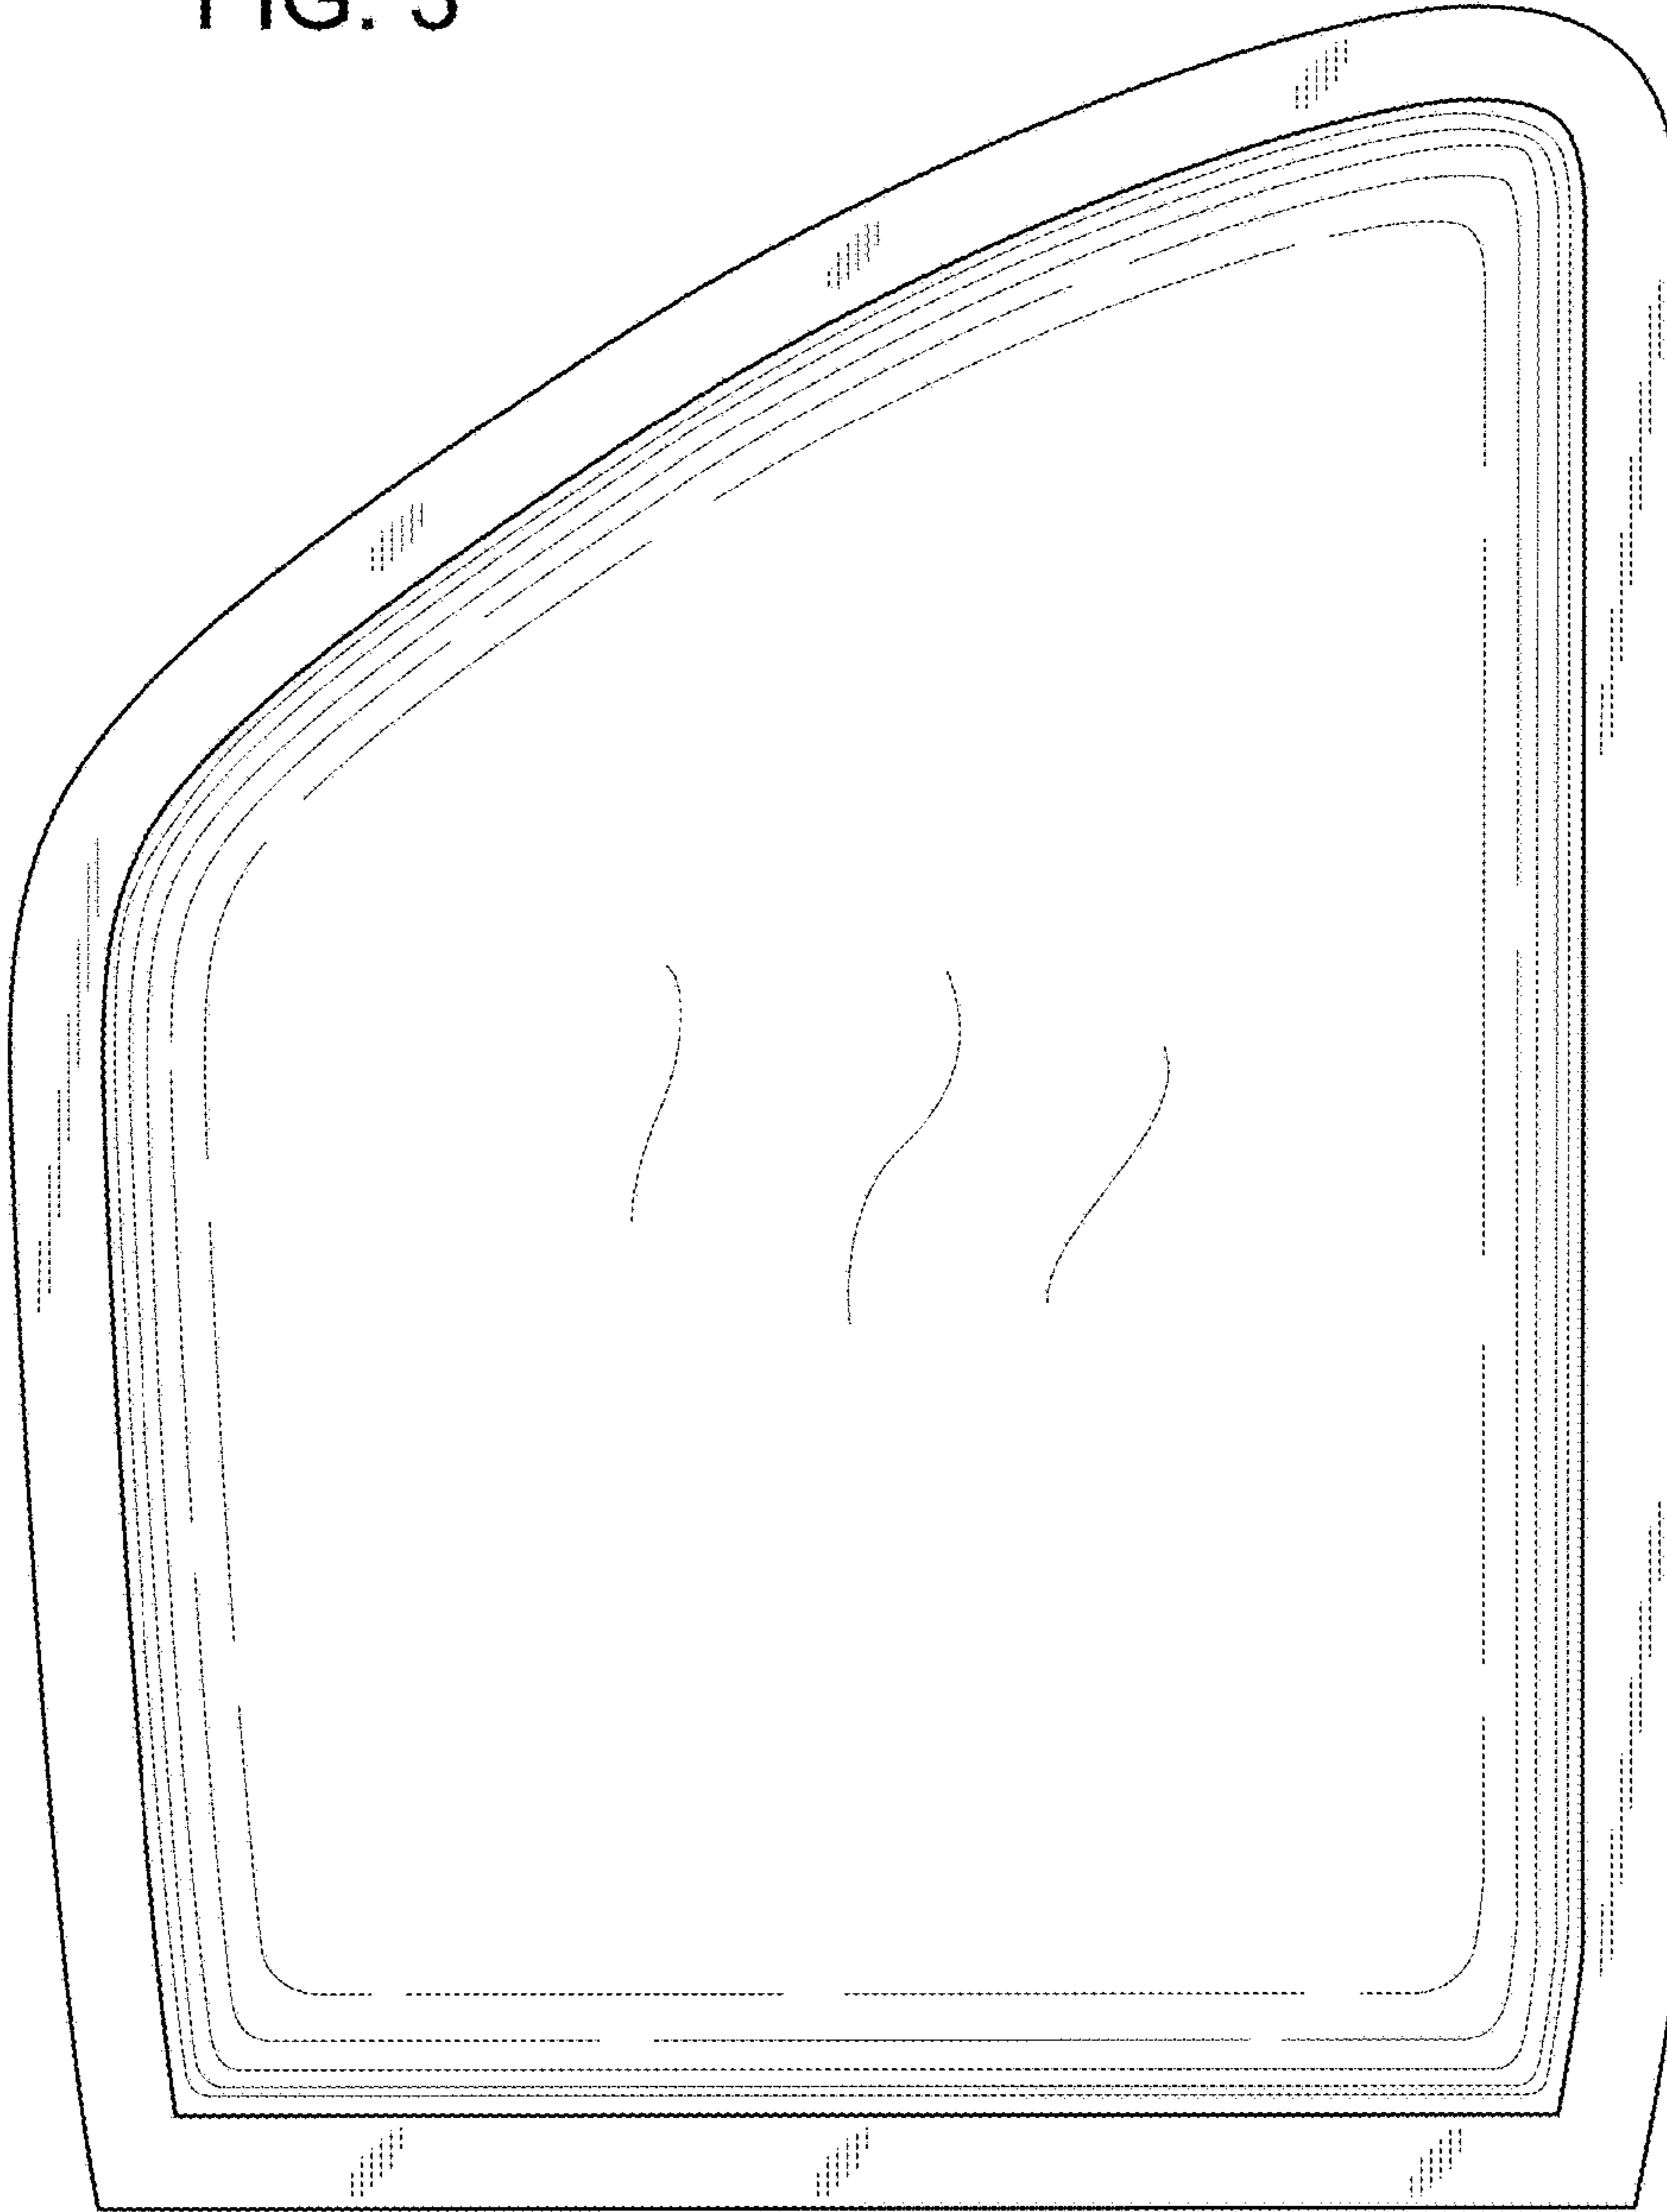


FIG. 2



FIG. 5

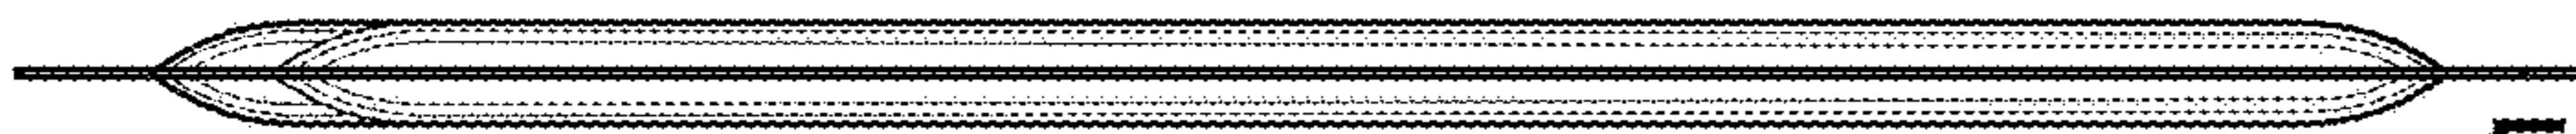


FIG. 4