

US00D865997S

(12) **United States Design Patent** (10) **Patent No.:** **US D865,997 S**
Mellett et al. (45) **Date of Patent:** **** Nov. 5, 2019**

(54) **USER INTERFACE FOR MEDICAL WORKSTATION**

(71) Applicant: **Hologic, Inc.**, Bedford, MA (US)

(72) Inventors: **Alyssa Mellett**, Kennesaw, GA (US);
Russell Kroll, Atlanta, GA (US)

(73) Assignee: **Hologic, Inc.**, Marlborough, MA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/585,525**

(22) Filed: **Nov. 25, 2016**

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/234**; D24/186

(58) **Field of Classification Search**
USPC D24/231, 185, 186, 169, 142, 158, 177,
D24/184, 216, 209, 108; D14/447, 344,
D14/486, 341, 346, 336; D10/15
CPC A61B 5/1071
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D352,463 S	11/1994	Kubo	
D361,129 S	8/1995	Collins	
D365,996 S	1/1996	Peterson	
D372,981 S	8/1996	McMahan, Jr.	
D415,834 S	10/1999	Barnes	
D426,833 S *	6/2000	Vanelli	D14/387
D461,895 S *	8/2002	Barnes	D24/158
6,792,801 B2	9/2004	Hoggan	
D504,516 S	4/2005	Yamazaki	
D507,832 S	7/2005	Yanniello	
D510,625 S *	10/2005	Widener	D24/186
D526,063 S *	8/2006	Widener	D24/186
D536,788 S	2/2007	Trifilio	
D538,243 S	3/2007	Seo	
D541,941 S	5/2007	Nakanishi	

D547,454 S	7/2007	Hsieh	
D547,873 S	7/2007	Hood	
D549,343 S *	8/2007	Schlagheck	D24/169
D550,364 S *	9/2007	Glover	D24/186
D551,350 S	9/2007	Lorimer	
D560,811 S *	1/2008	Powell	D24/216
D587,376 S *	2/2009	Takano	D24/169
D595,415 S *	6/2009	Fukuzawa	D24/186
D598,113 S	8/2009	Flaction	
D601,256 S *	9/2009	Takano	D24/169
D603,518 S	11/2009	Zafar	
D605,297 S	12/2009	Unsworth	
D605,771 S	12/2009	Unsworth	
D606,199 S *	12/2009	Vu	D13/162

(Continued)

Primary Examiner — Rhea Shields


(57) **CLAIM**

The ornamental design for a user interface for medical workstation, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an embodiment of a user interface for medical workstation showing our new design. FIG. 2 is a front view of the user interface for medical workstation of FIG. 1. FIG. 3 is a back view of the user interface for medical workstation of FIG. 1. FIG. 4 is a right-side view of the user interface for medical workstation of FIG. 1. FIG. 5 is a left-side view of the user interface for medical workstation of FIG. 1. FIG. 6 is a top view of the user interface for medical workstation of FIG. 1; and, FIG. 7 is a bottom view of the user interface for medical workstation of FIG. 1. In the drawings, the broken lines are for the purpose of illustrating environment only and form no part of the claimed design.

1 Claim, 5 Drawing Sheets

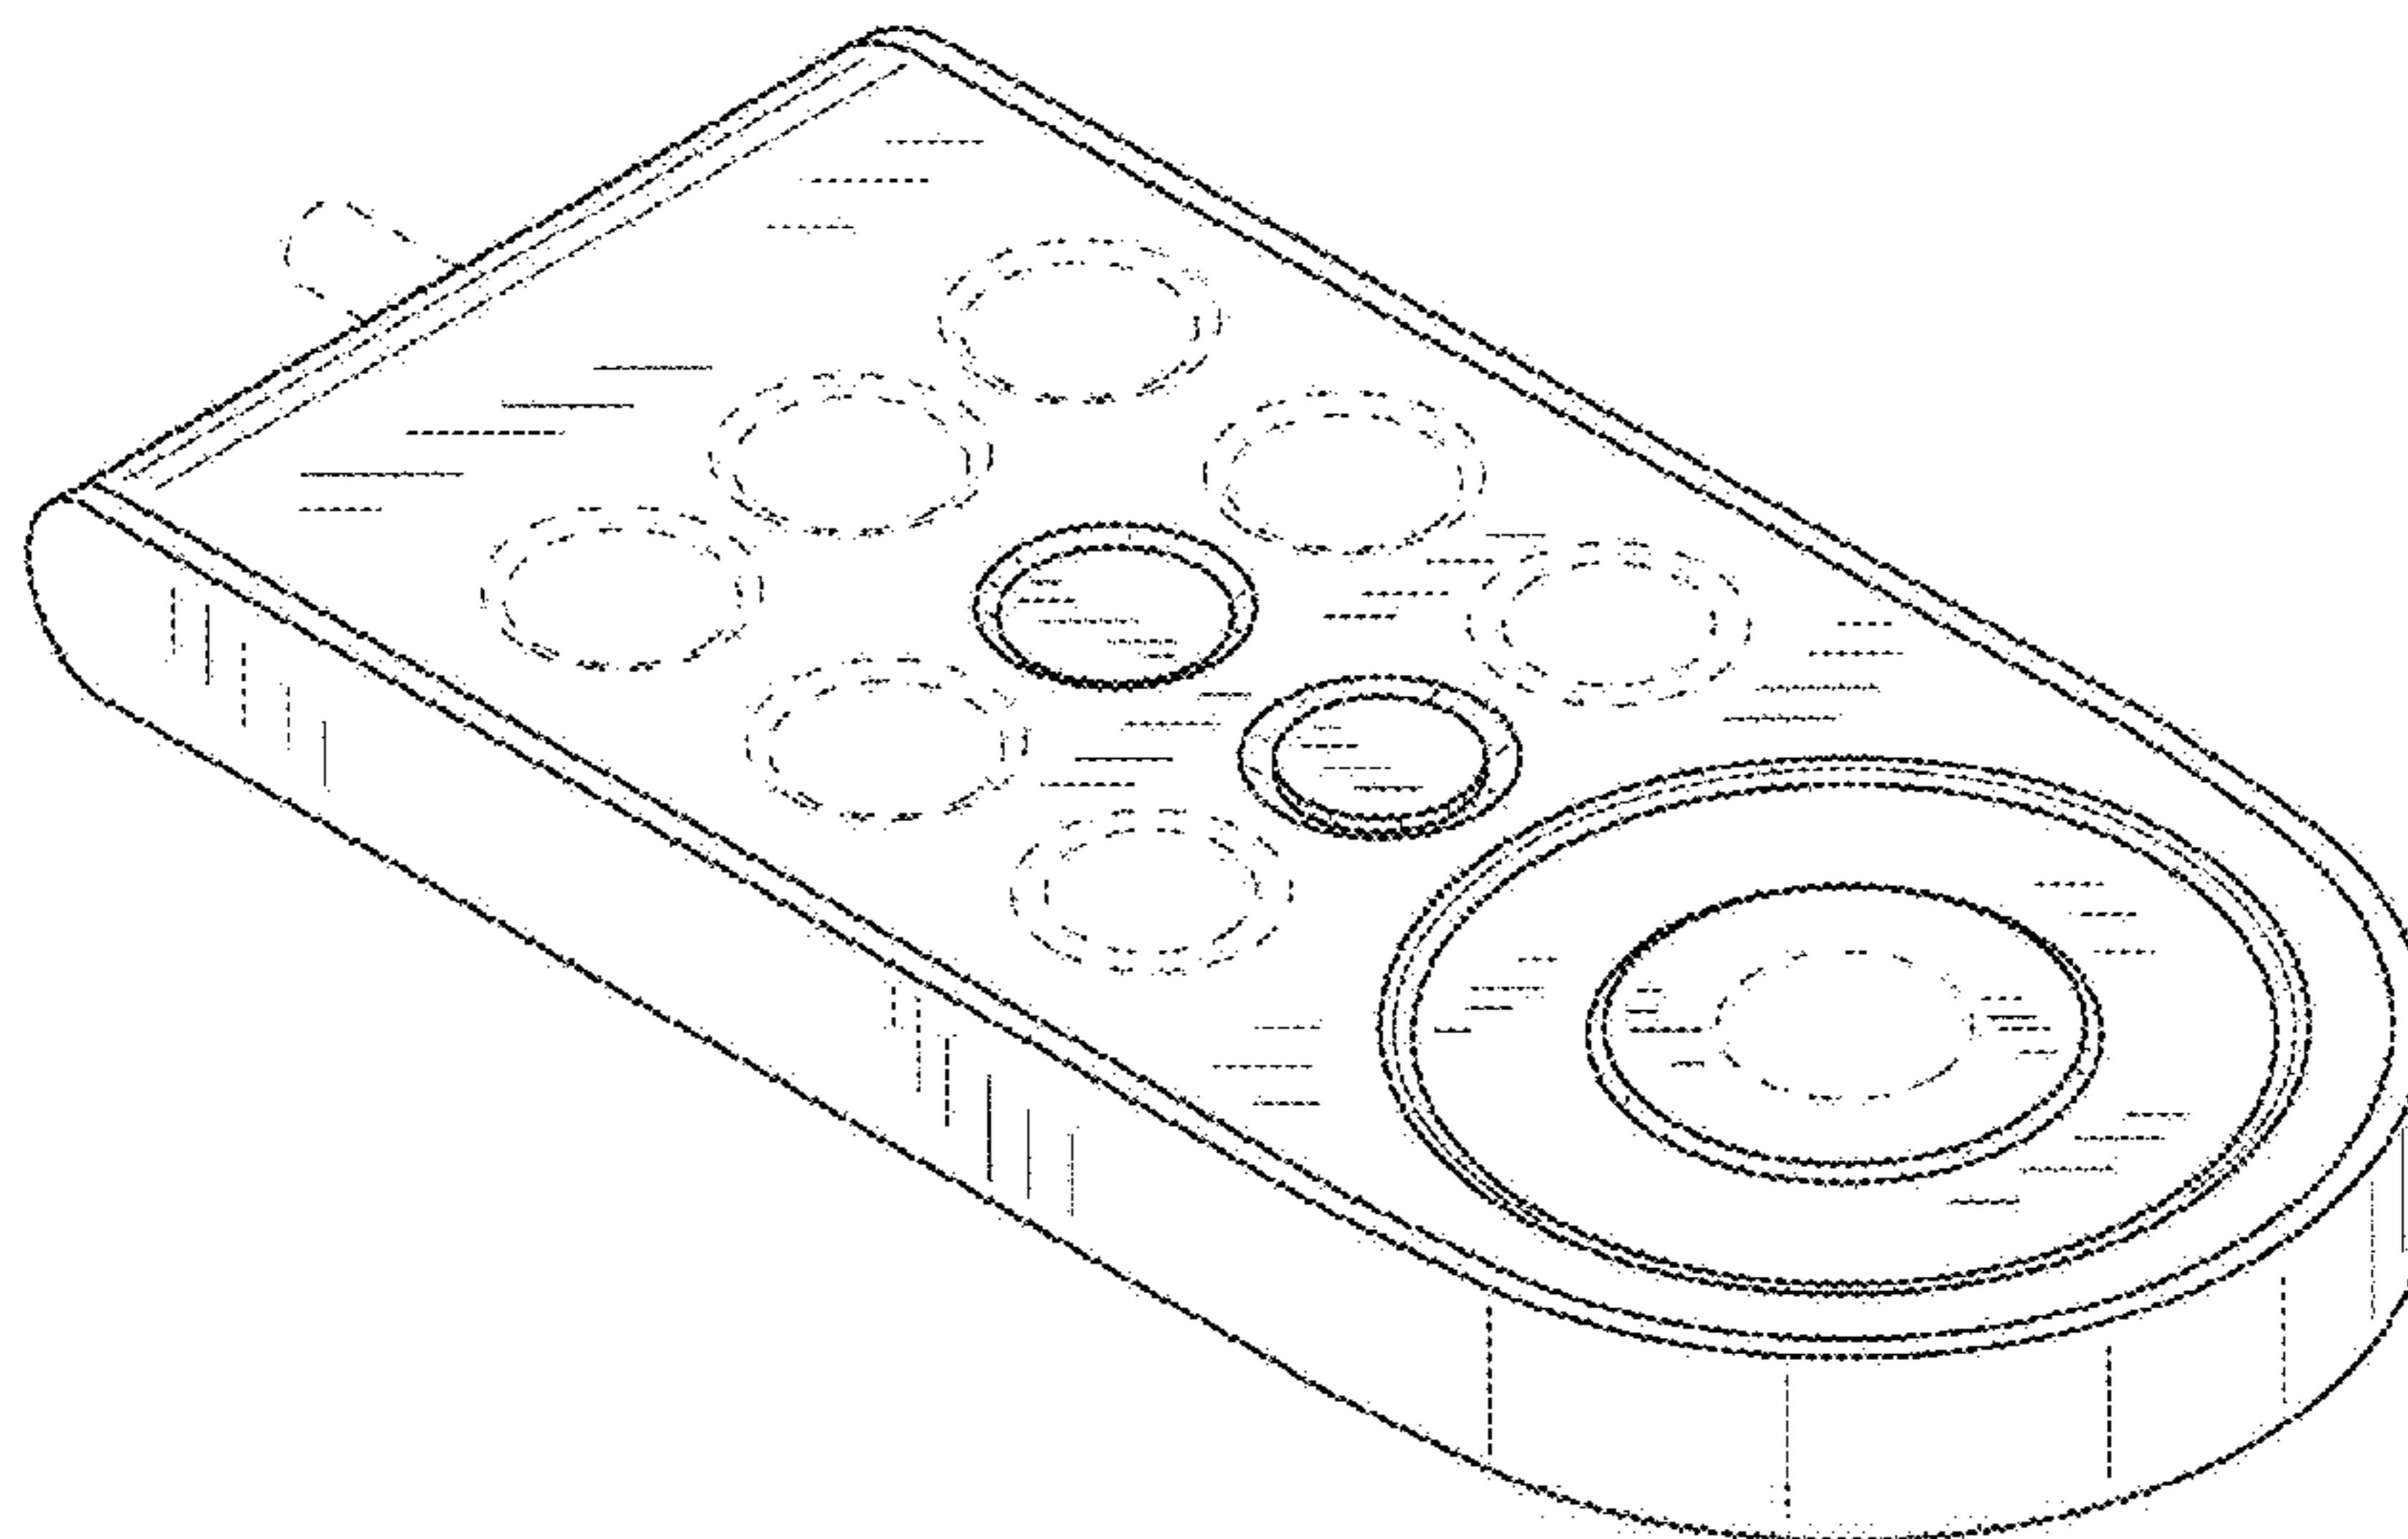

(56)

References Cited

U.S. PATENT DOCUMENTS

D606,203 S	*	12/2009	Husheer	D24/186
D609,197 S	*	2/2010	Koskela	D13/168
D609,349 S		2/2010	Pelissier		
D612,503 S		3/2010	Johnston		
D613,411 S		4/2010	Collins		
D616,993 S		6/2010	Muis		
D629,113 S		12/2010	Wodecki		
D634,435 S		3/2011	Chua		
D641,881 S		7/2011	Inami		
D670,810 S		11/2012	Fukuzawa		
D673,151 S		12/2012	Bousfield		
D673,153 S		12/2012	Bousfield		
D675,321 S		1/2013	Sanga		
D684,574 S		6/2013	Taunay da Graca Couto		
D687,540 S		8/2013	Nair		
D688,060 S	*	8/2013	Sizelove	D6/716.2
D696,403 S		12/2013	Noguchi		
D696,404 S		12/2013	Golnik		
D698,443 S	*	1/2014	Prais	D24/169
D700,702 S		3/2014	Kolb		
D705,190 S		5/2014	Shigeno		
D712,041 S		8/2014	Glaesker		
8,894,585 B2		11/2014	Hasbun		
D719,999 S		12/2014	Sohrabi		
D721,814 S		1/2015	Creed		
D732,729 S		6/2015	McKechnie		
D736,111 S		8/2015	Klein		
D738,507 S	*	9/2015	Prais	D24/169
D738,755 S		9/2015	Druce		
D739,938 S		9/2015	Schempp		
D742,371 S	*	11/2015	Bopp	D14/336
D743,035 S		11/2015	Uozumi		
D745,167 S		12/2015	Canas		
D748,271 S		1/2016	Clowry		
D749,073 S	*	2/2016	Navon	D14/346
D751,205 S		3/2016	Tan		
D755,977 S		5/2016	Winkelmann		
D766,442 S	*	9/2016	Prais	D24/169
D769,241 S	*	10/2016	Mazz	D14/341
D770,034 S	*	10/2016	McNall, III	D24/108
D770,052 S		10/2016	Abu-Tarif		
D774,057 S	*	12/2016	Anderson	D14/486
D779,677 S		2/2017	Chen		
D784,541 S		4/2017	Hilbig		
D791,336 S		7/2017	Lei		
D795,252 S		8/2017	Chung		
D799,484 S		10/2017	Tamillow		
D800,909 S		10/2017	Jones		
D800,912 S		10/2017	Uzri		
D801,538 S		10/2017	Rondoni		
D804,033 S	*	11/2017	Wightman	D24/169
D810,042 S		2/2018	Pazhoor		
D810,306 S		2/2018	Rondoni		
D810,947 S		2/2018	Larson		
D821,592 S	*	6/2018	Pham	D24/200
D822,216 S	*	7/2018	Barker	D24/186
D822,217 S		7/2018	Sebban		
D824,034 S		7/2018	Pushpala		
D829,337 S		9/2018	Klein		
D833,624 S		11/2018	DeJong		
D834,583 S		11/2018	Janzen		
D834,721 S	*	11/2018	Klein	D24/225
D835,798 S		12/2018	Ito		
D836,639 S	*	12/2018	Volta	D14/431
D836,769 S		12/2018	Kabel-Eckes		
D836,789 S	*	12/2018	Jiang	D24/200
D839,424 S		1/2019	Golosarsky		

* cited by examiner

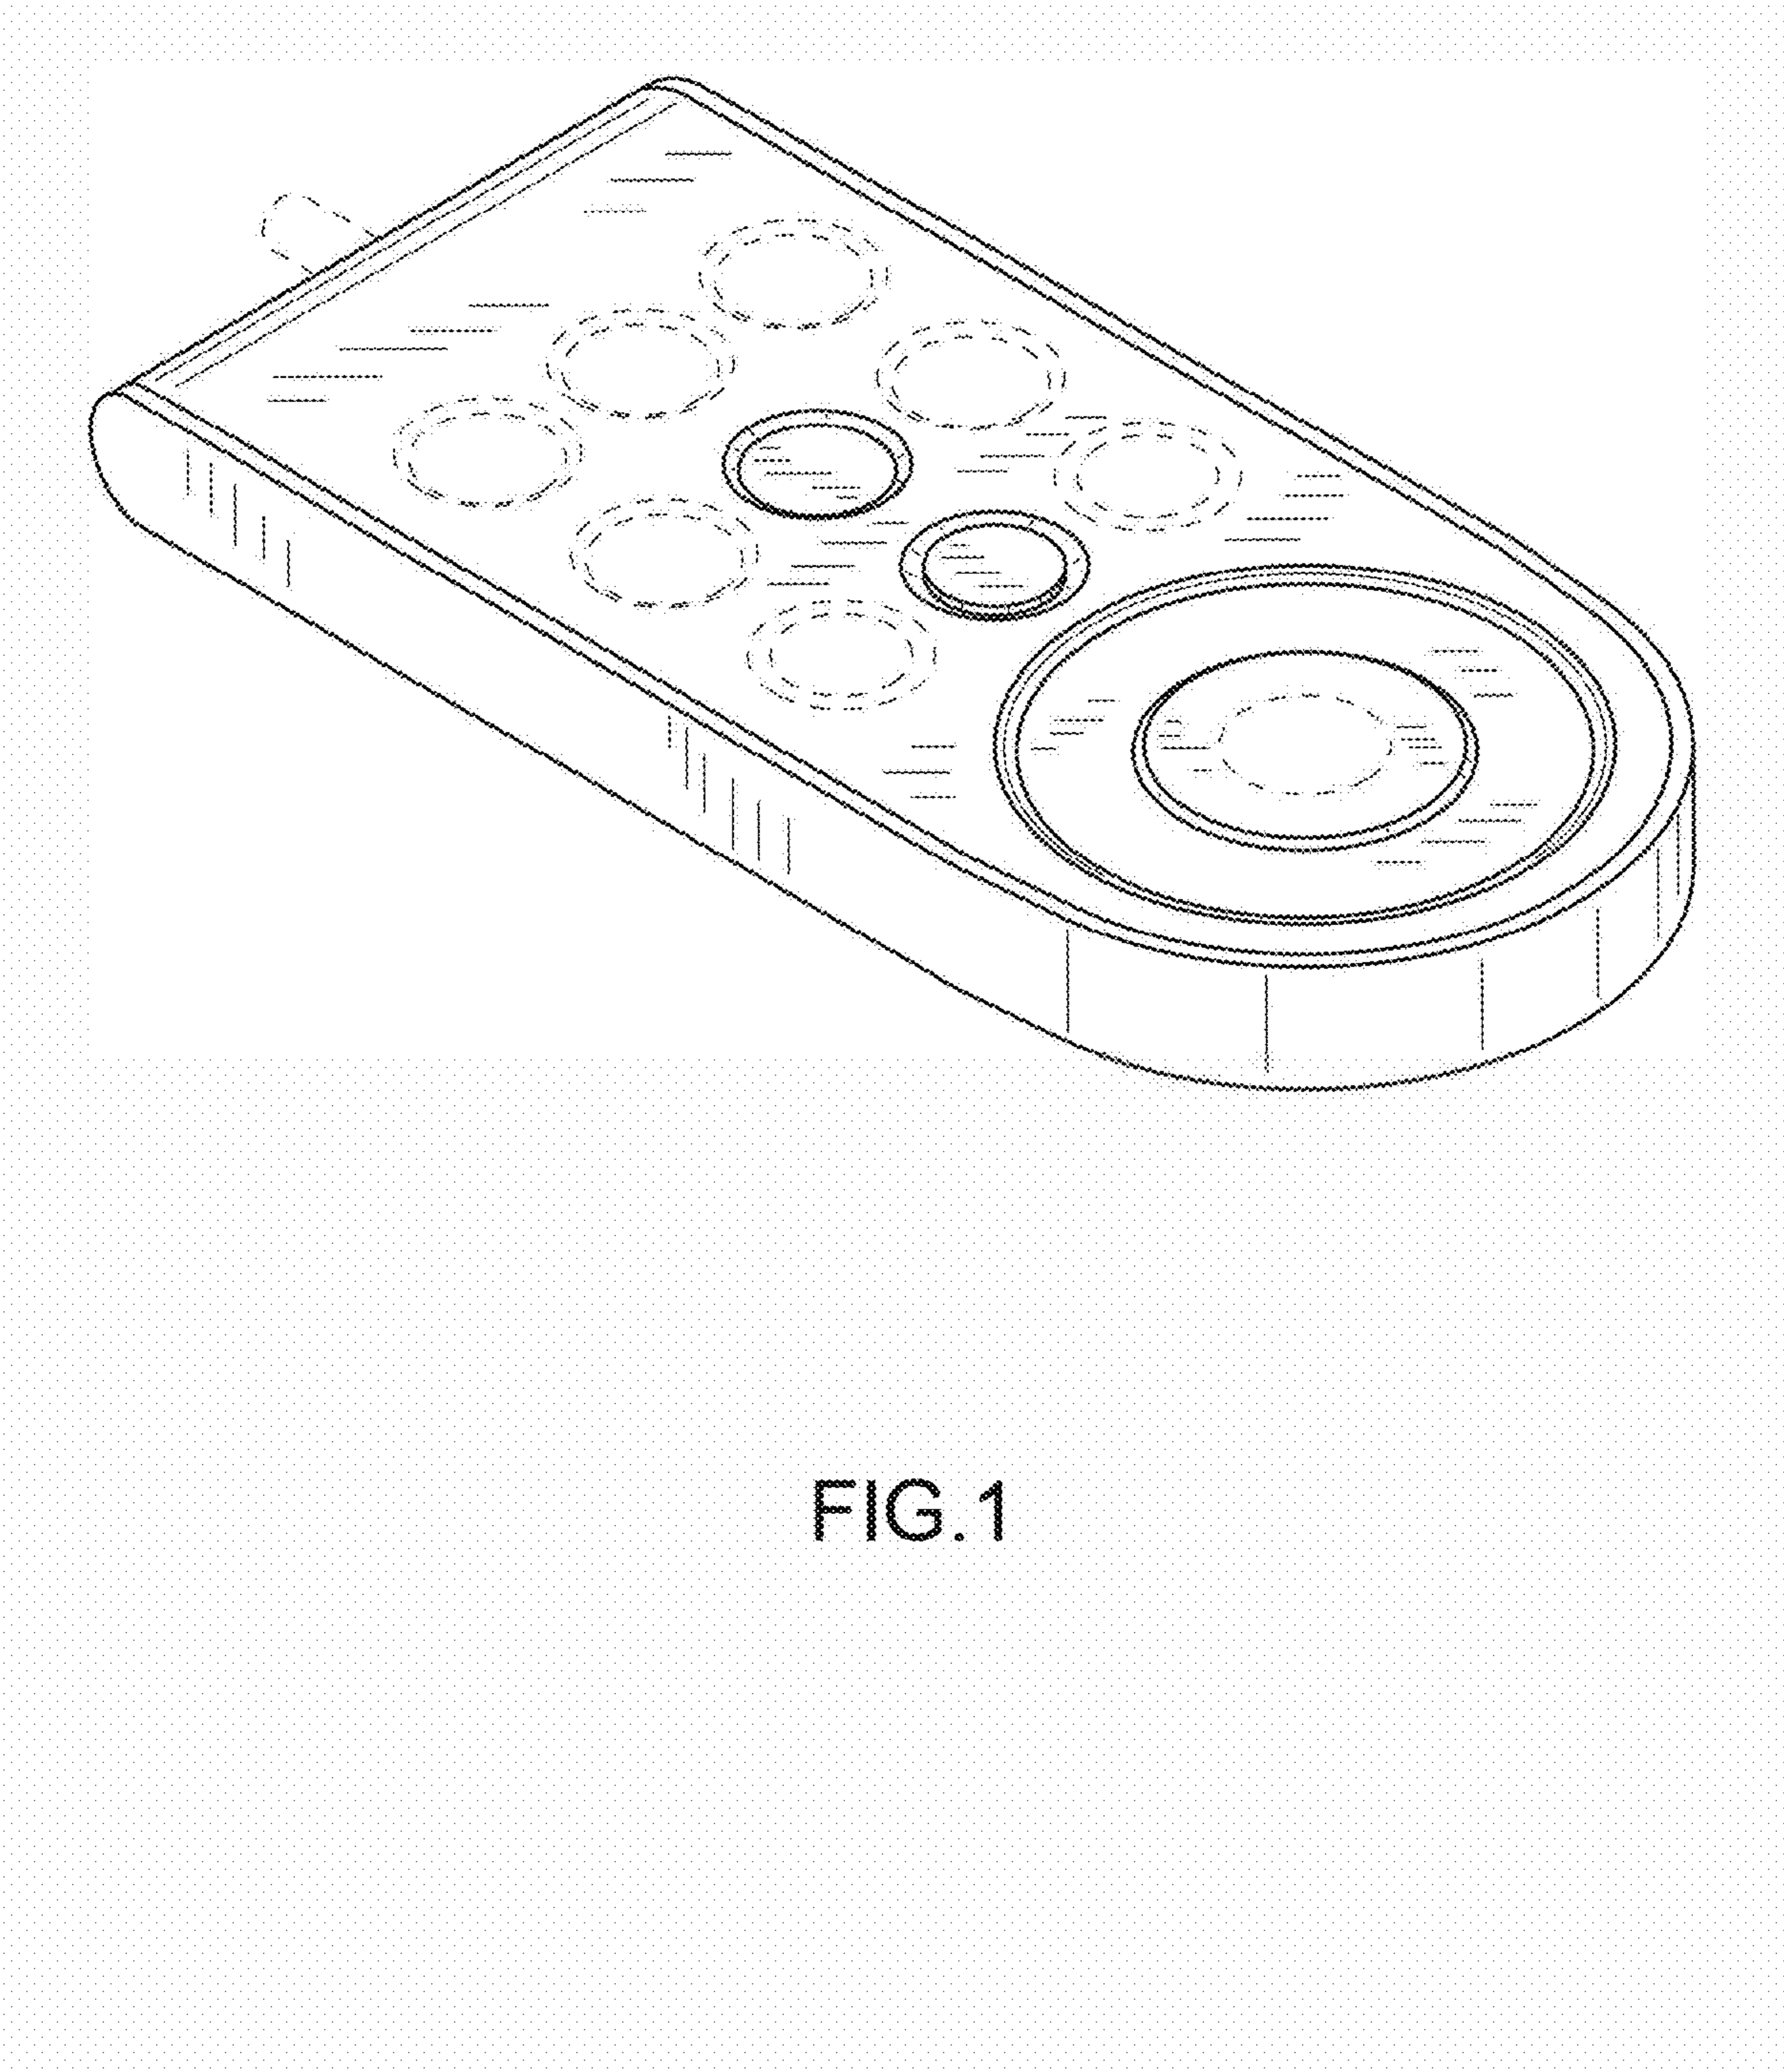


FIG. 1

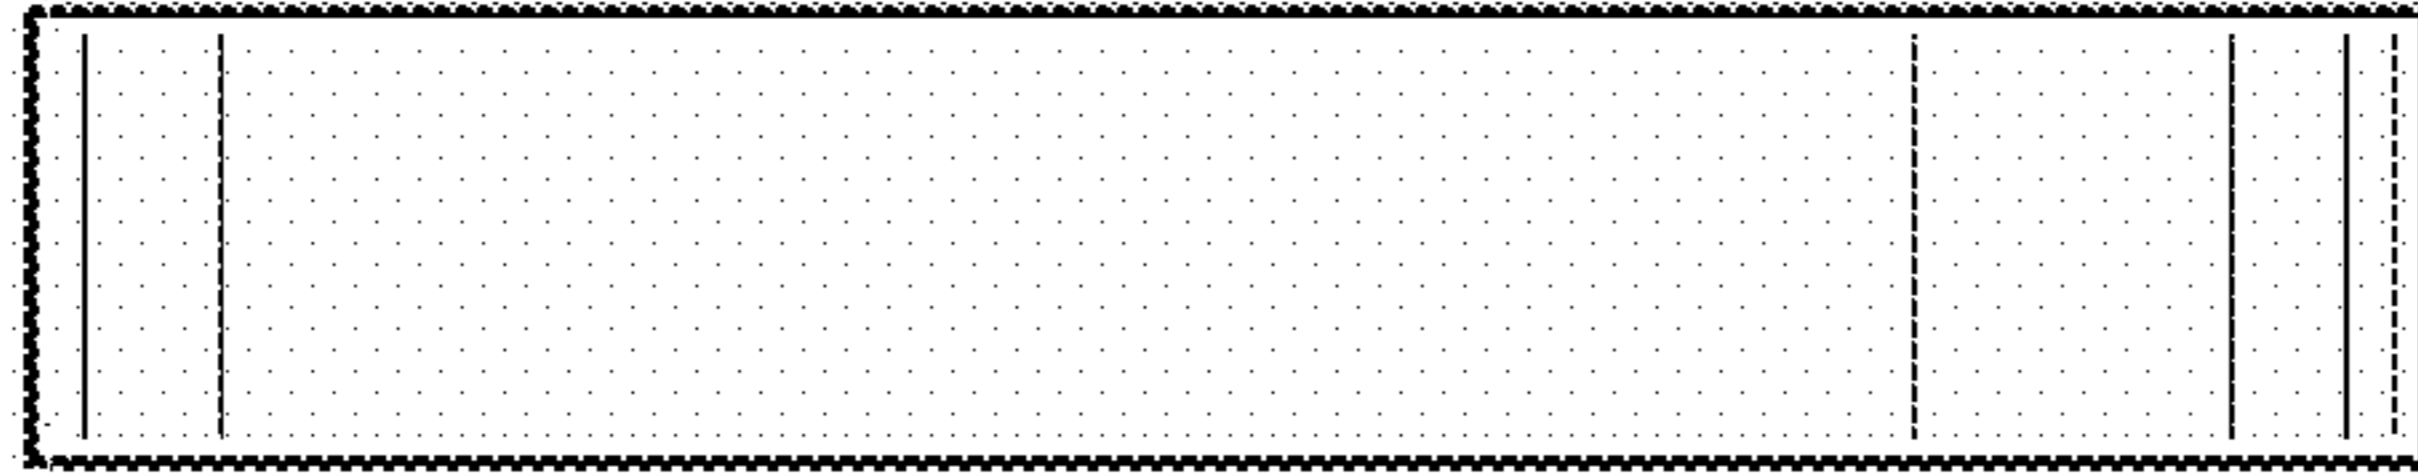


FIG. 2



FIG. 3

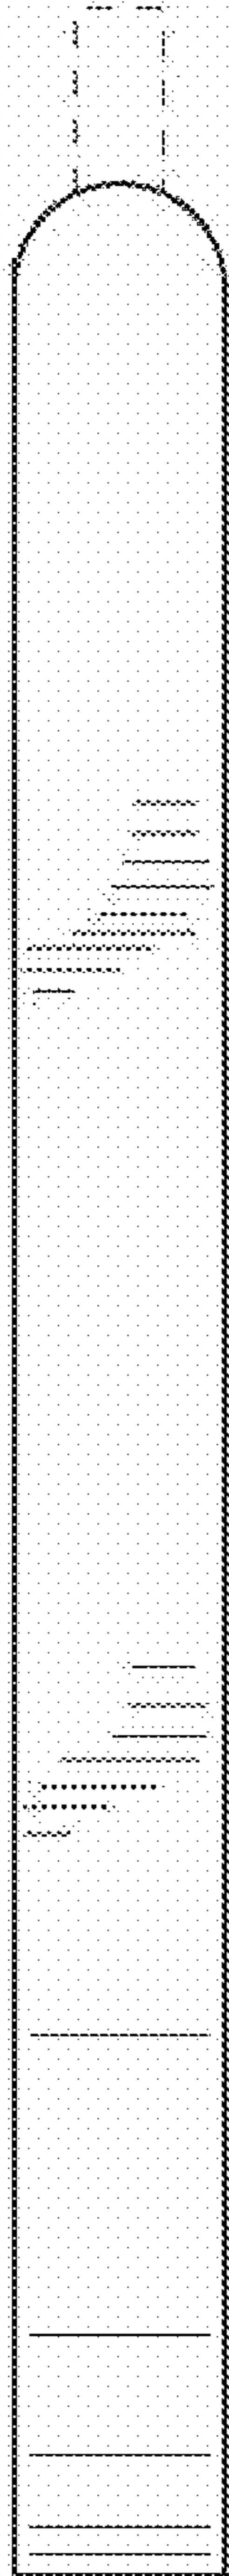


FIG. 4

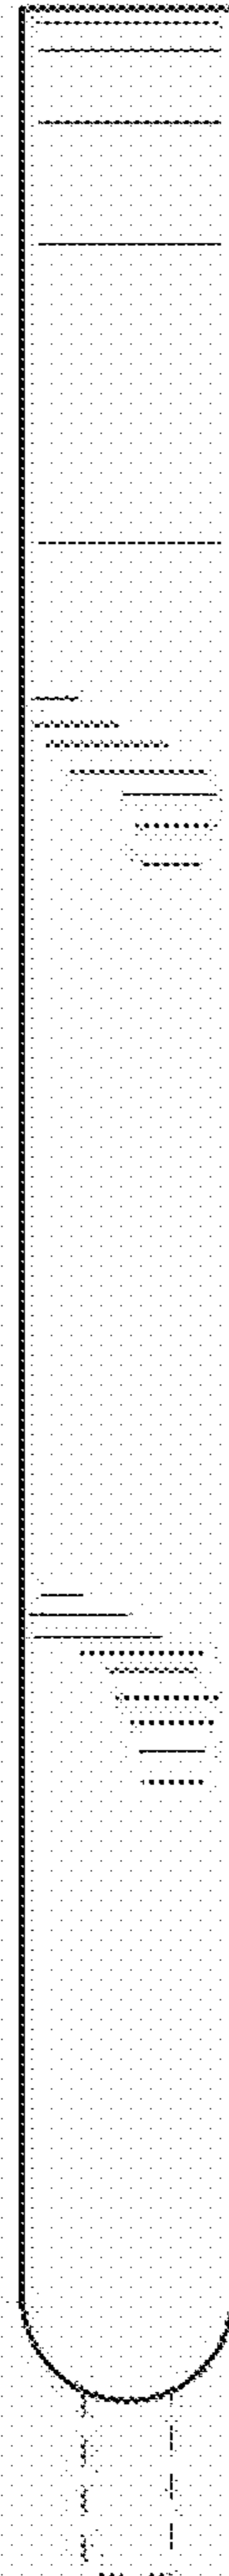


FIG. 5

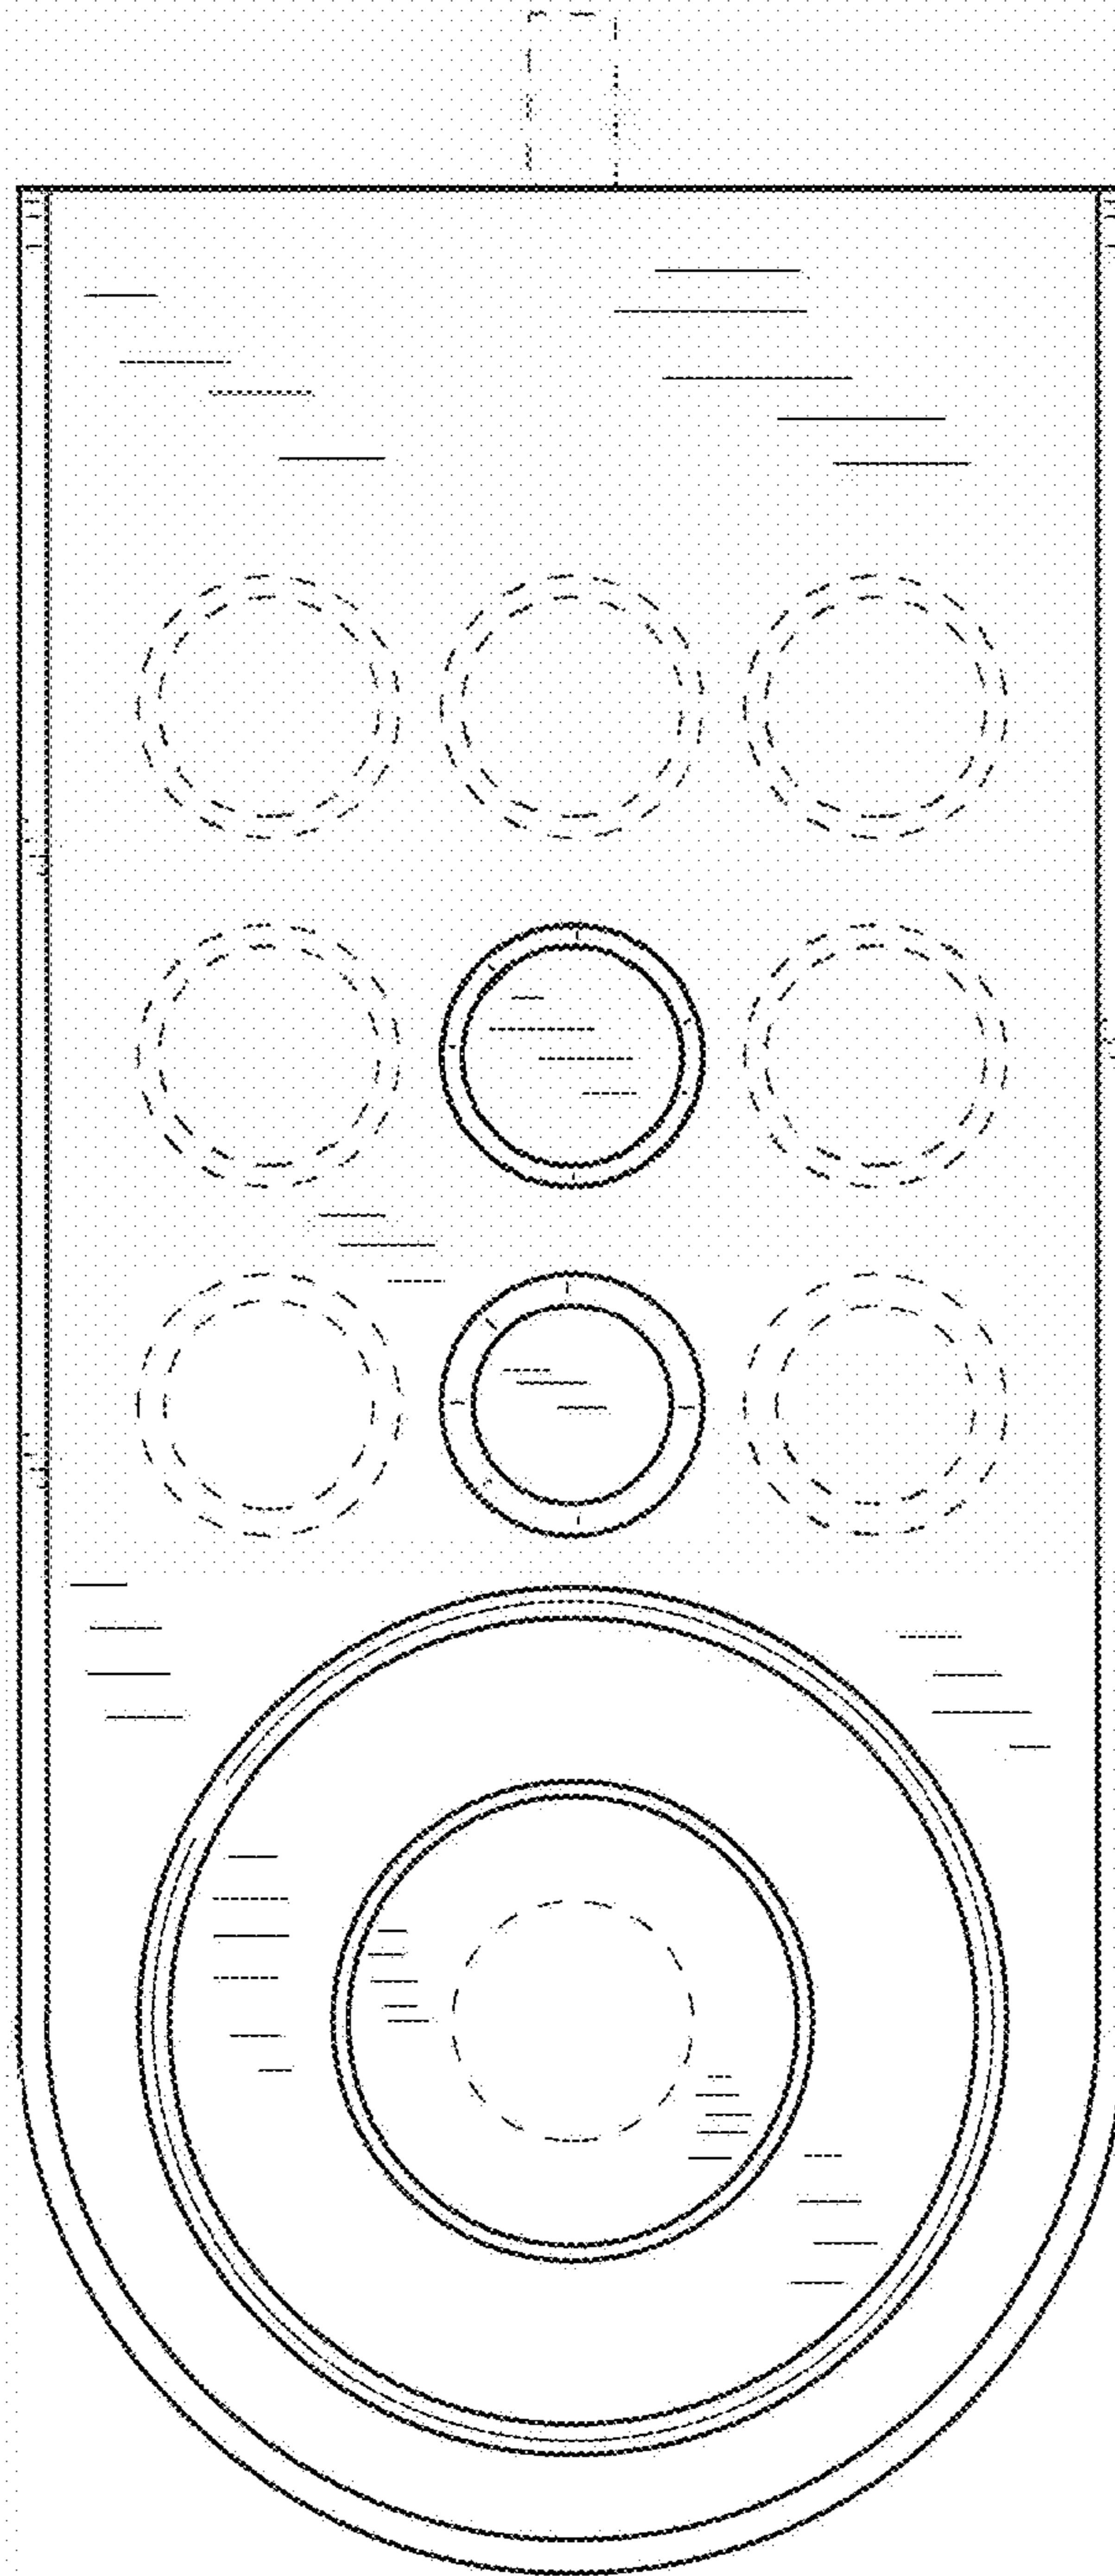


FIG. 6

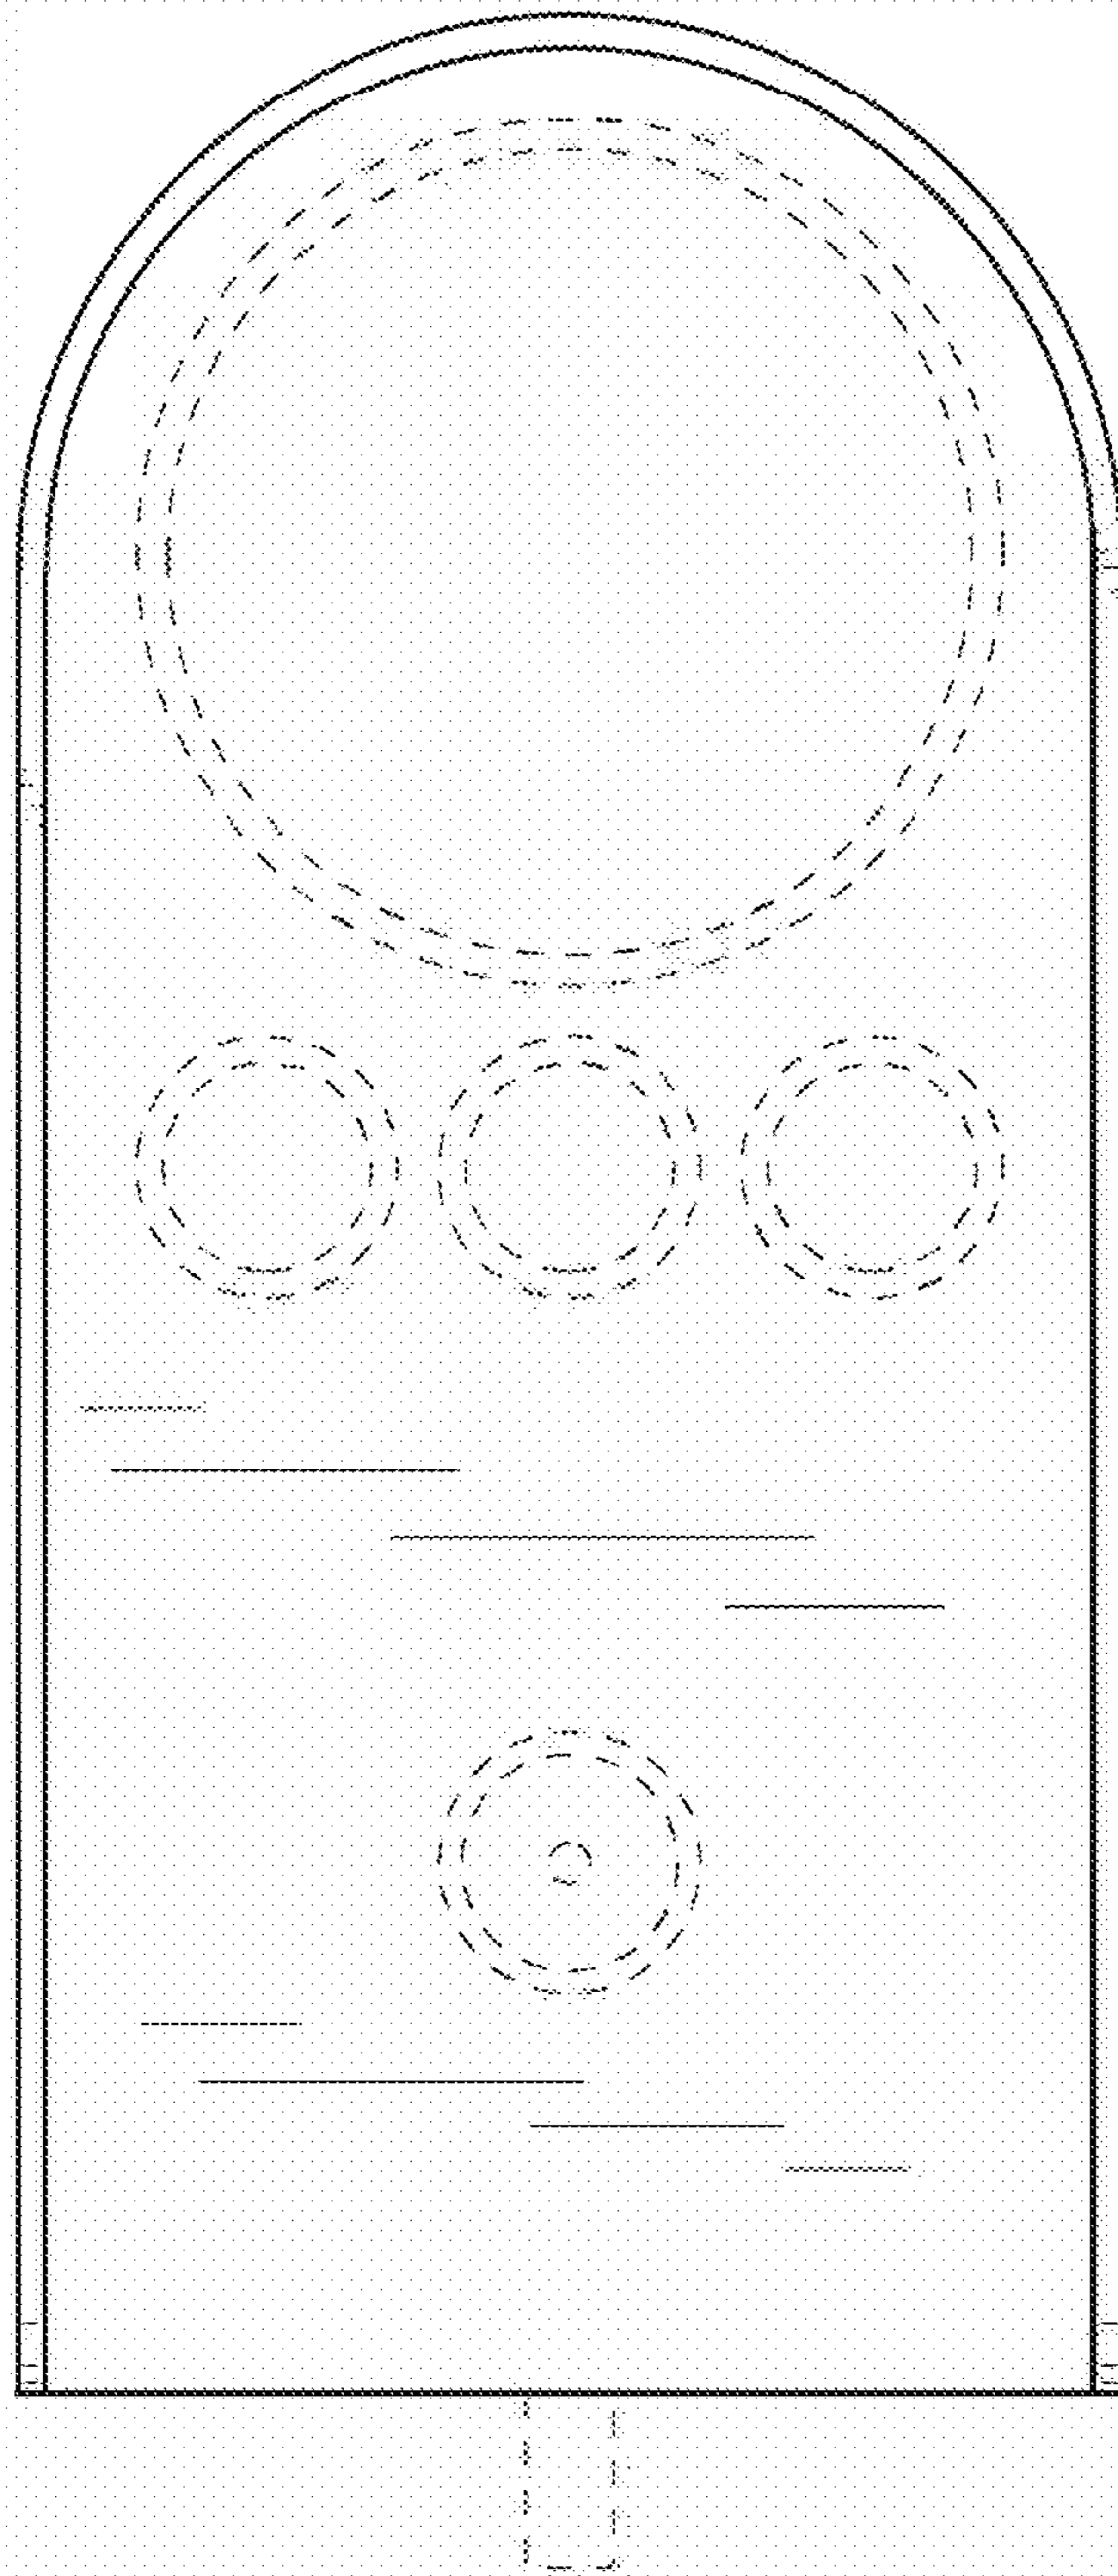


FIG.7